

1/6


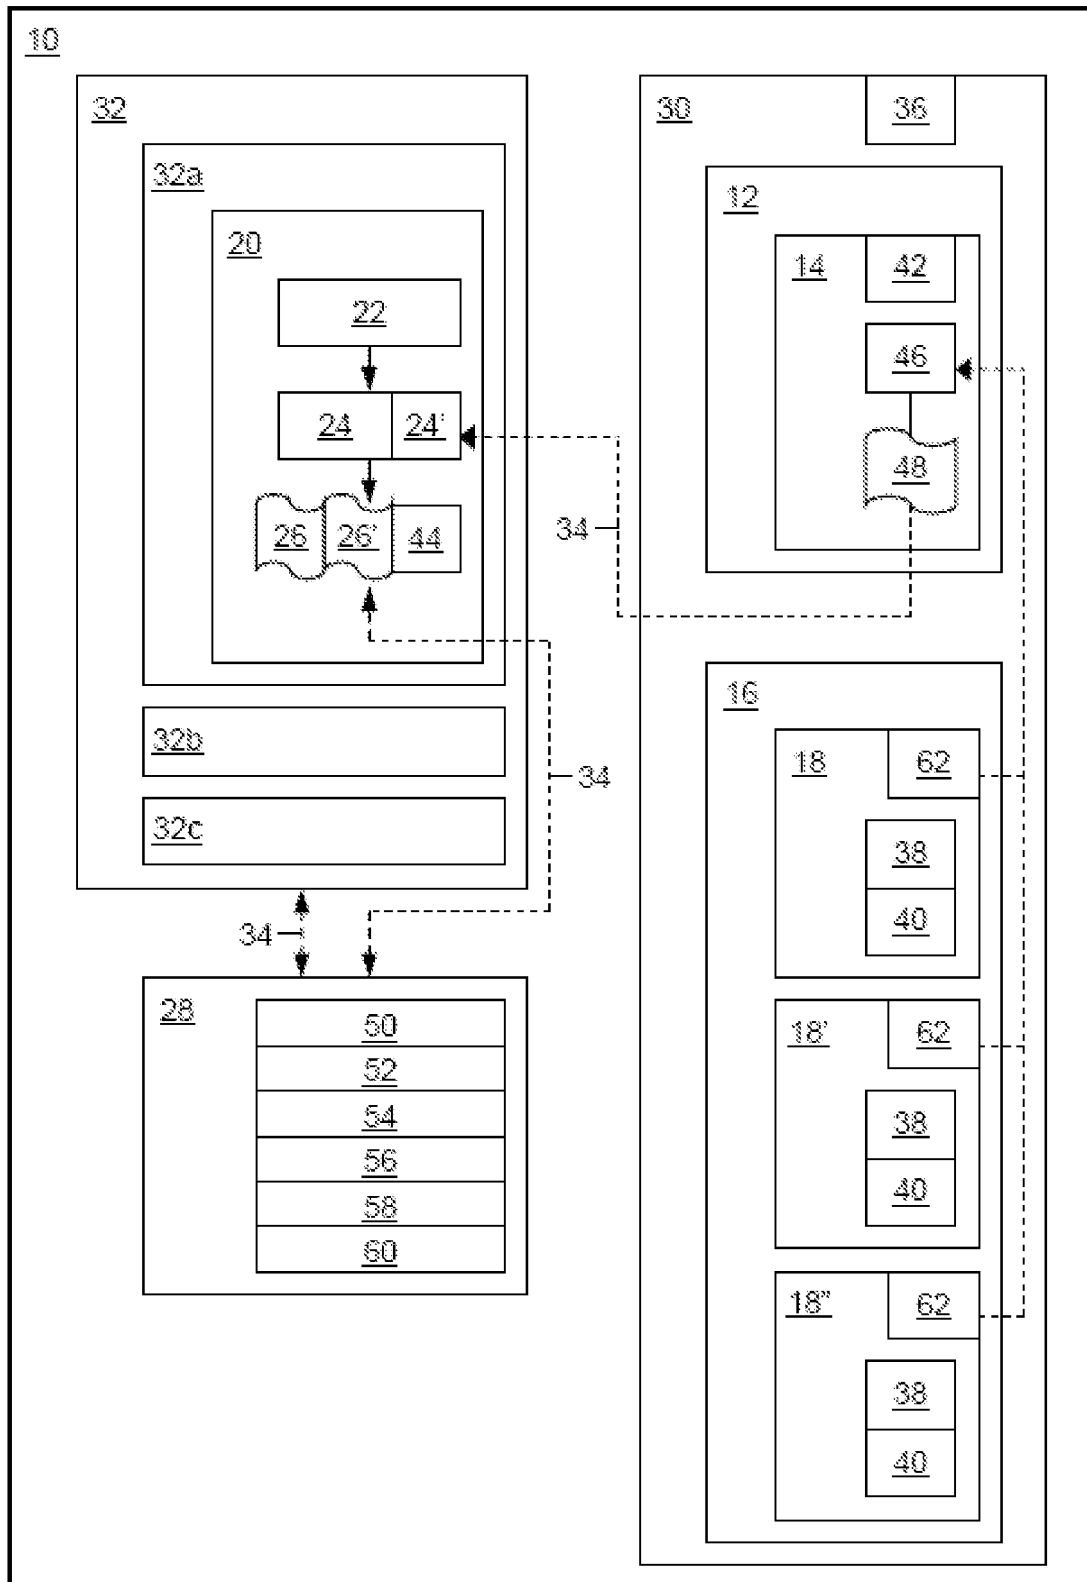


FIG. 1

Step 1 : Select Application

Select the chromatography application in which you are using the selected consumable(s)



☒ Gas Chromatography (GC)
Gas Chromatography (GC)

Detector Type:

- ☒ MS
- ☐ ECD
- ☐ ELCD
- ☐ NPD
- ☐ FID



☐ Liquid Chromatography (LC)
Liquid Chromatography (LC)

Detector Type:

- ☐ MS



☐ ICP
ICP

Detector Type:

- ☐ MS

[Previous](#) [Next](#)

FIG. 2

Step 2 : Application Usage

Please indicate the necessary details to calculate the lifetime of the selected consumable(s)

Gas Chromatography (GC) / MS

Carrier Gas

Helium

Source Gas Quality (%)

99.9999

Gas Delivery System

☒ Bottle ☐ Generator

Usage:

☒ Daily ☐ Weekly ☐ Monthly

Flow

2

L/Min.

pressure

5

☒ Bar ☐ Psi

Tubing & Fittings

Material: ☒ Stainless Steel ☐ Brass

Size: ☐ 1/4" ☒ 1/8"

5

Sample(s).

Runtime per sample:

30

Minutes

25

Seconds

Previous

Next

FIG. 3

4/6

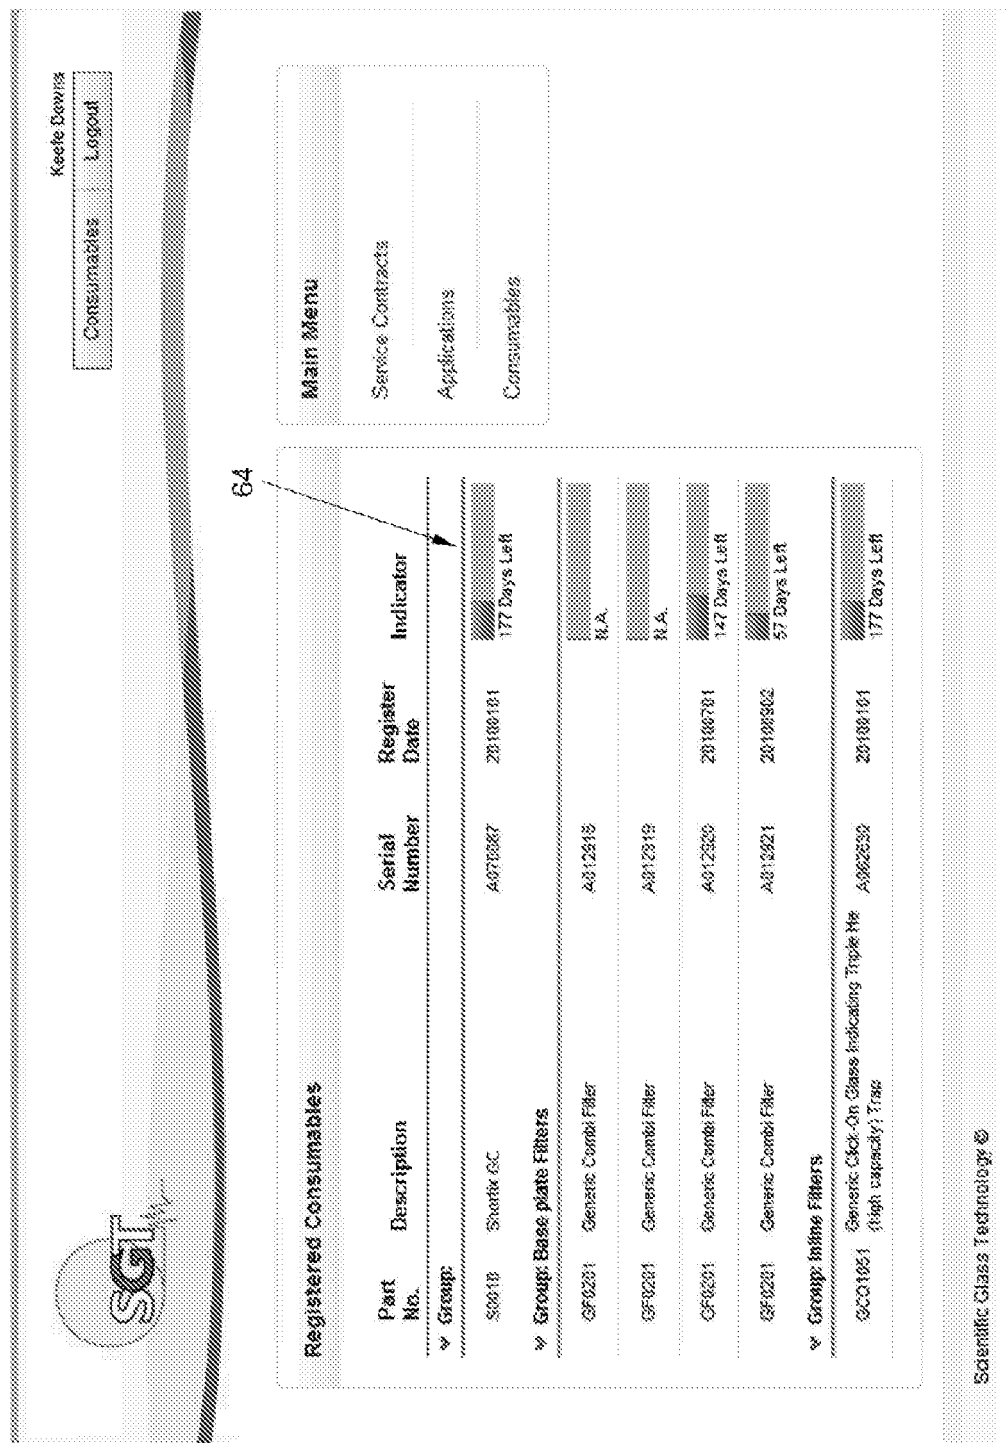


FIG. 4

5/6

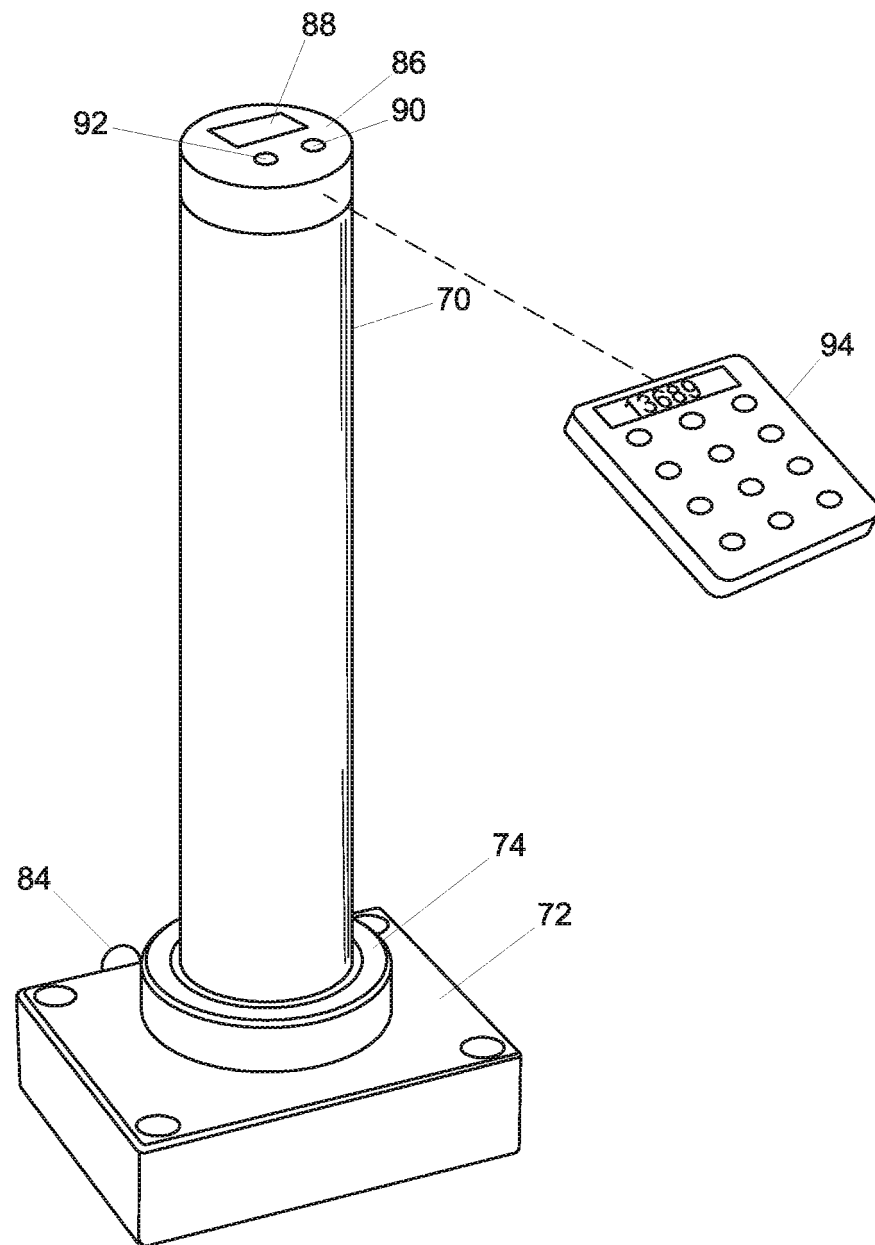


FIG. 5

6/6

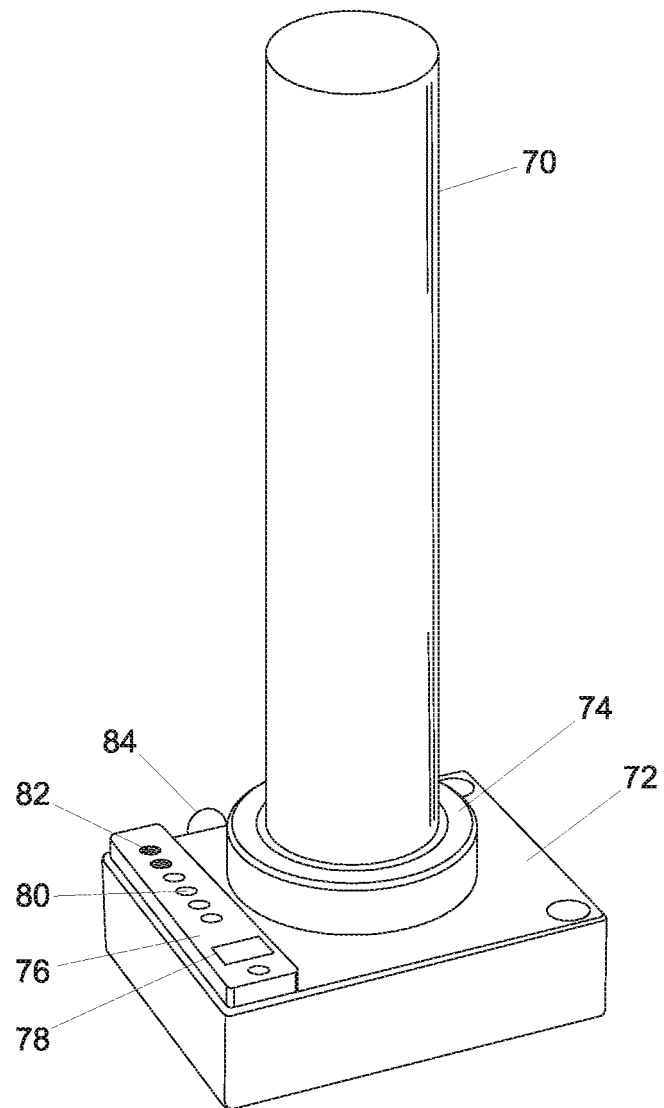


FIG. 6