

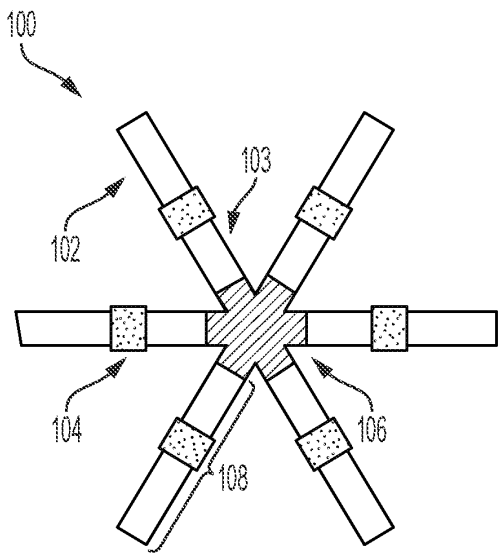


FIG. 1A

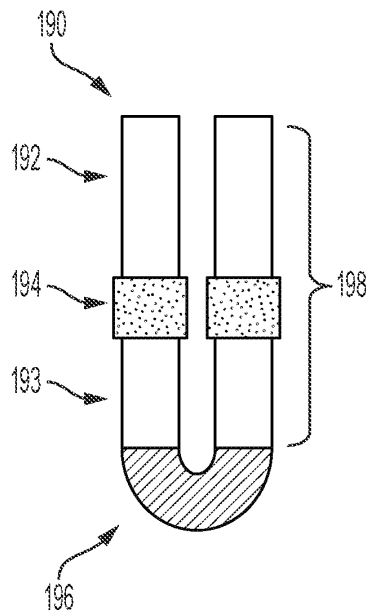


FIG. 1B

FIG. 2A


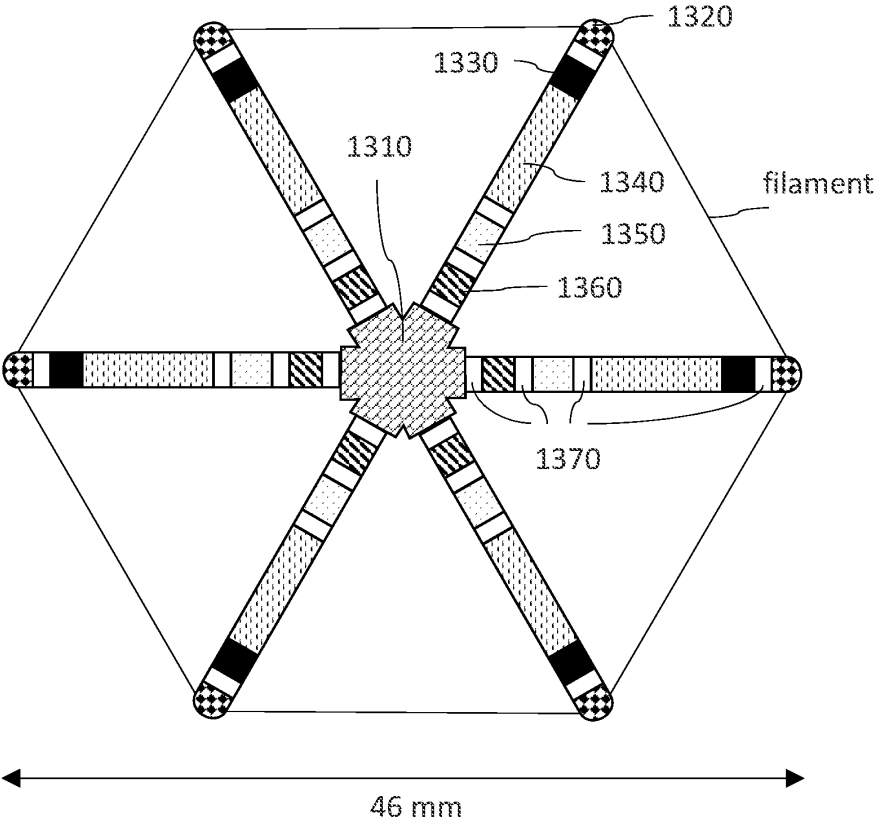


FIG. 2B

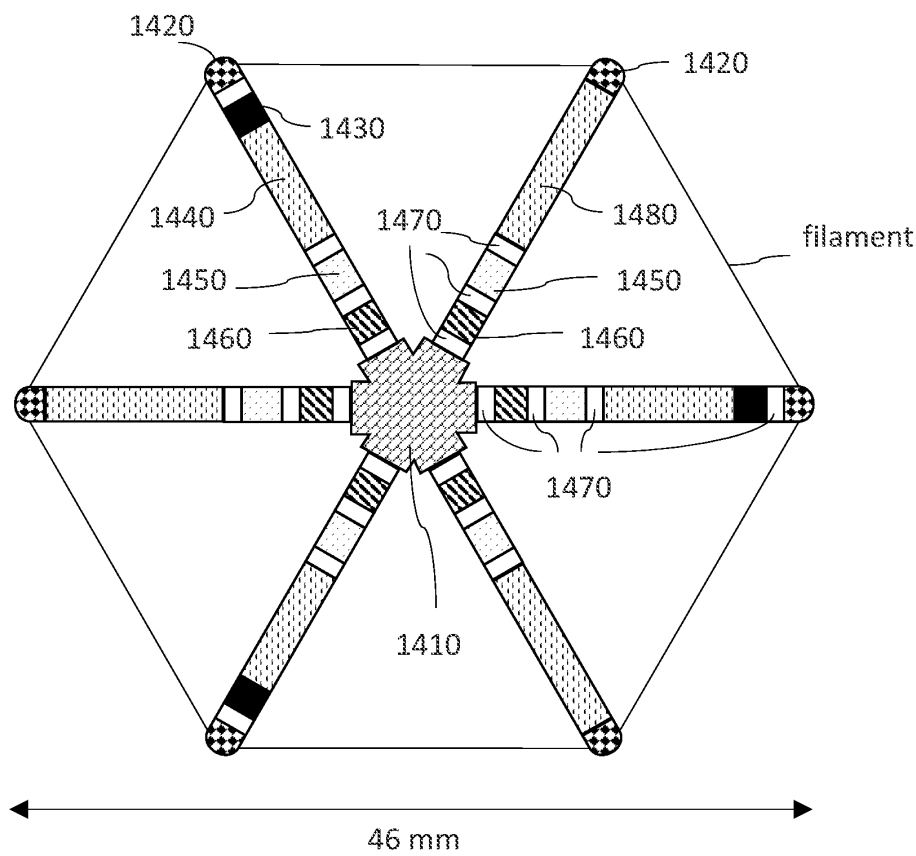

4/19

FIG. 3

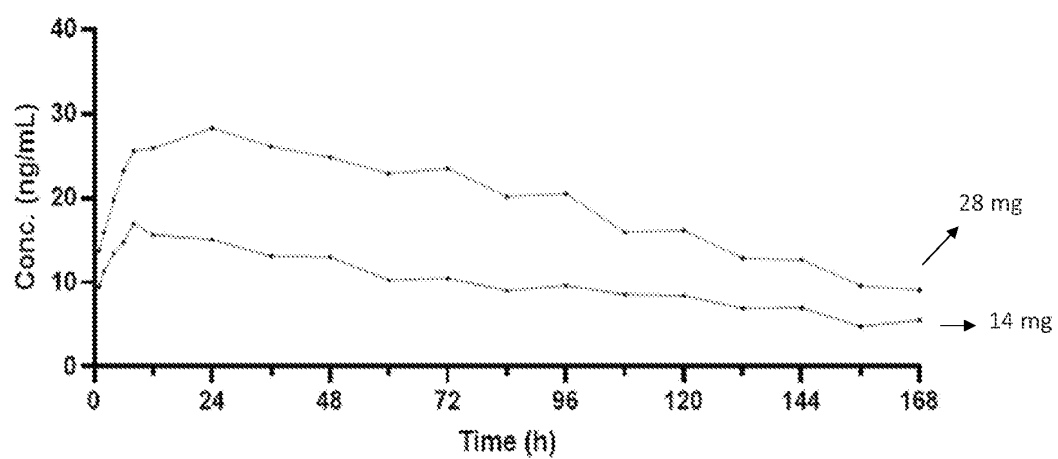
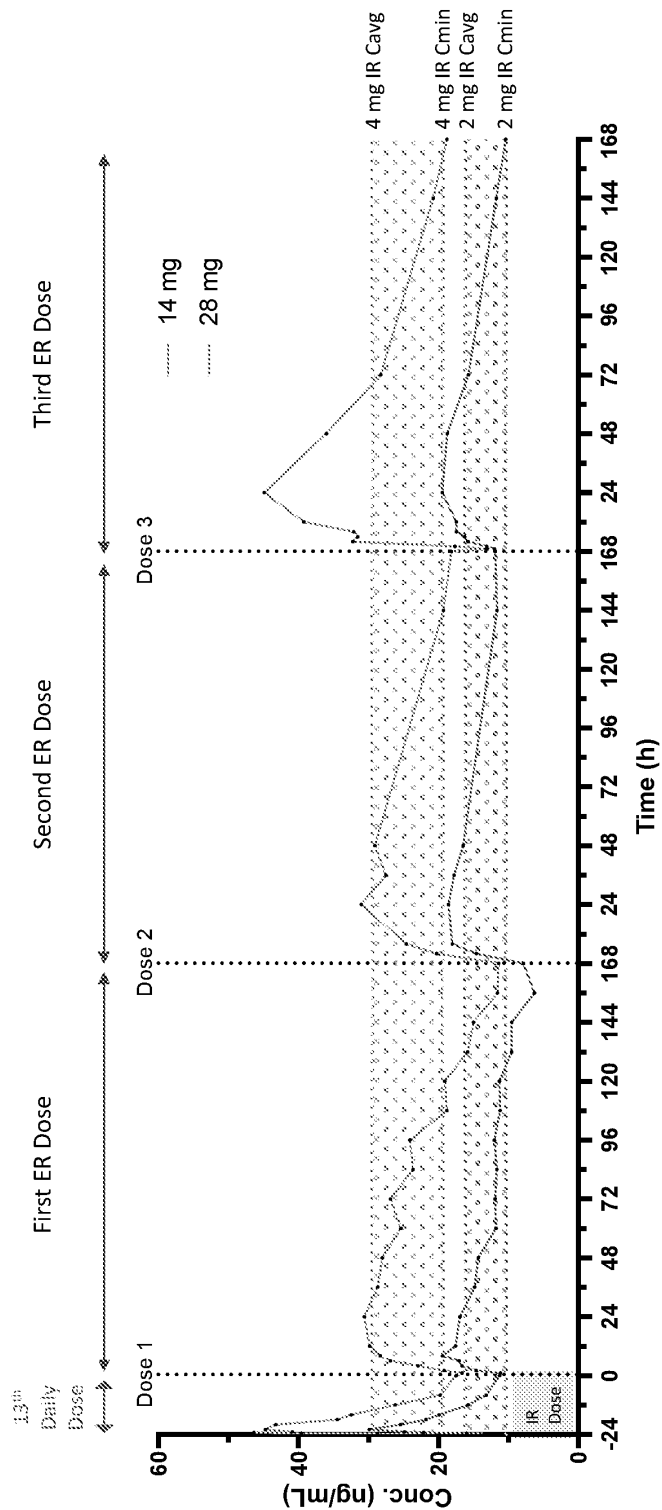


FIG. 4



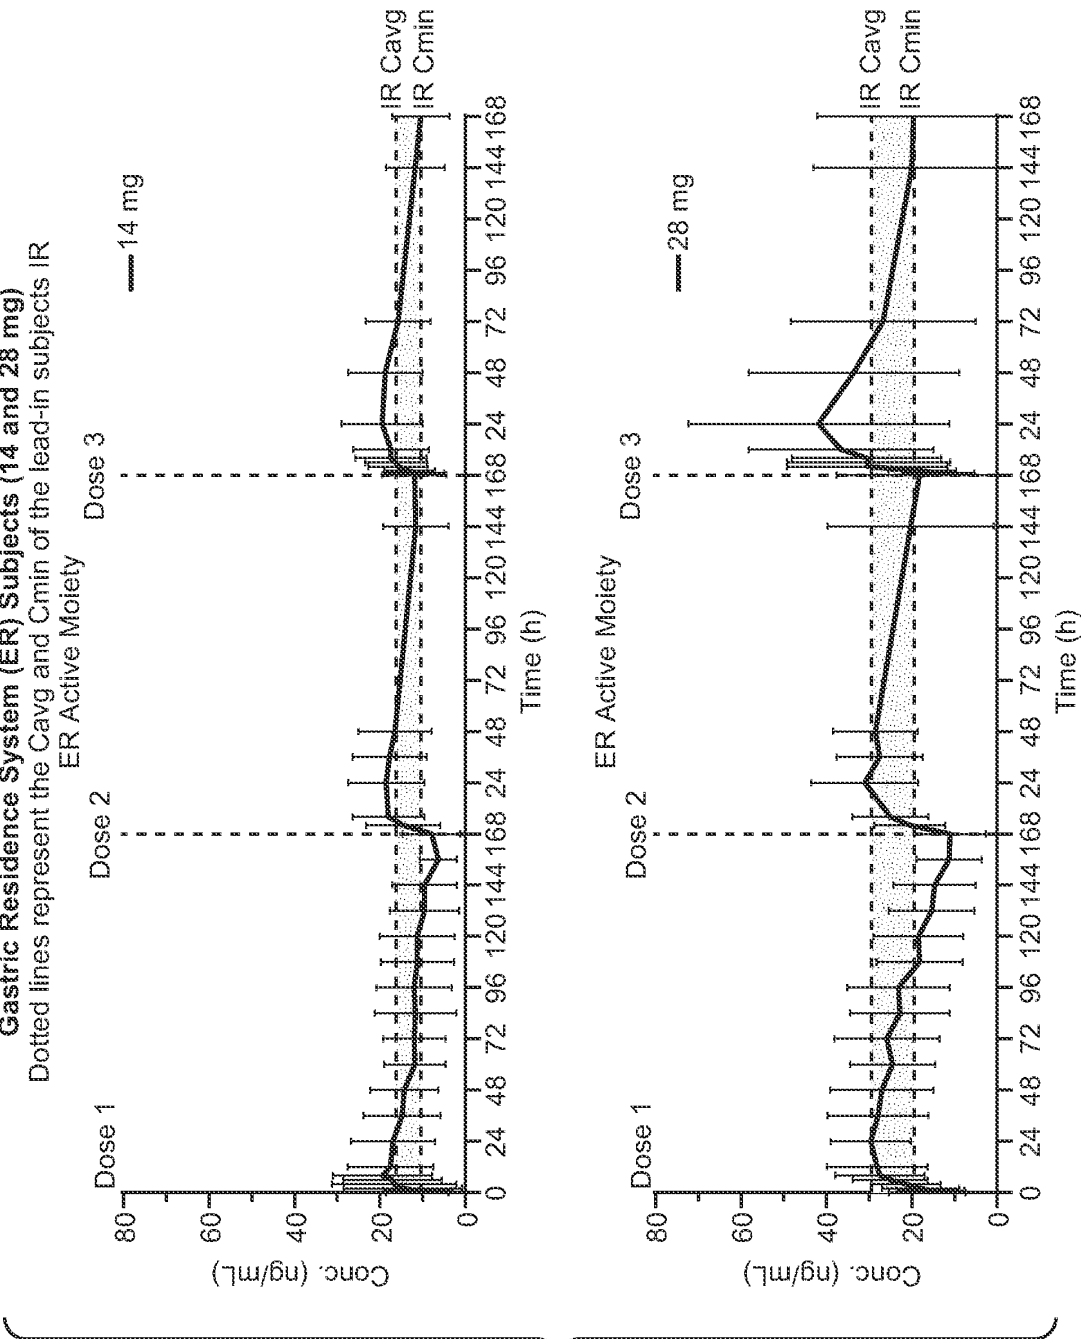


FIG. 5A

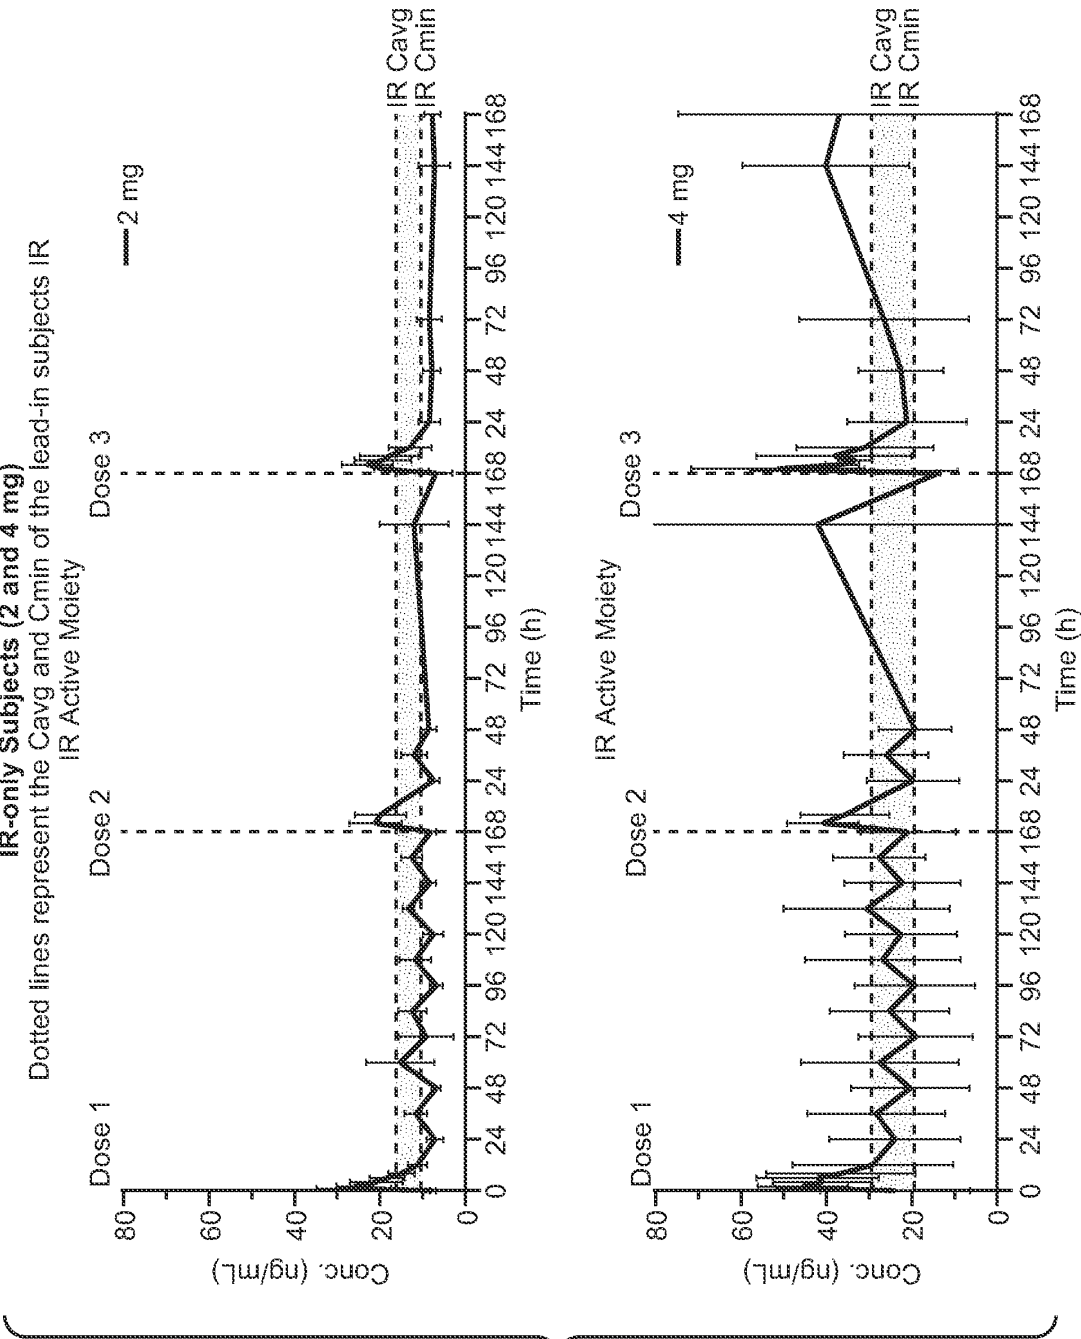


FIG. 5B

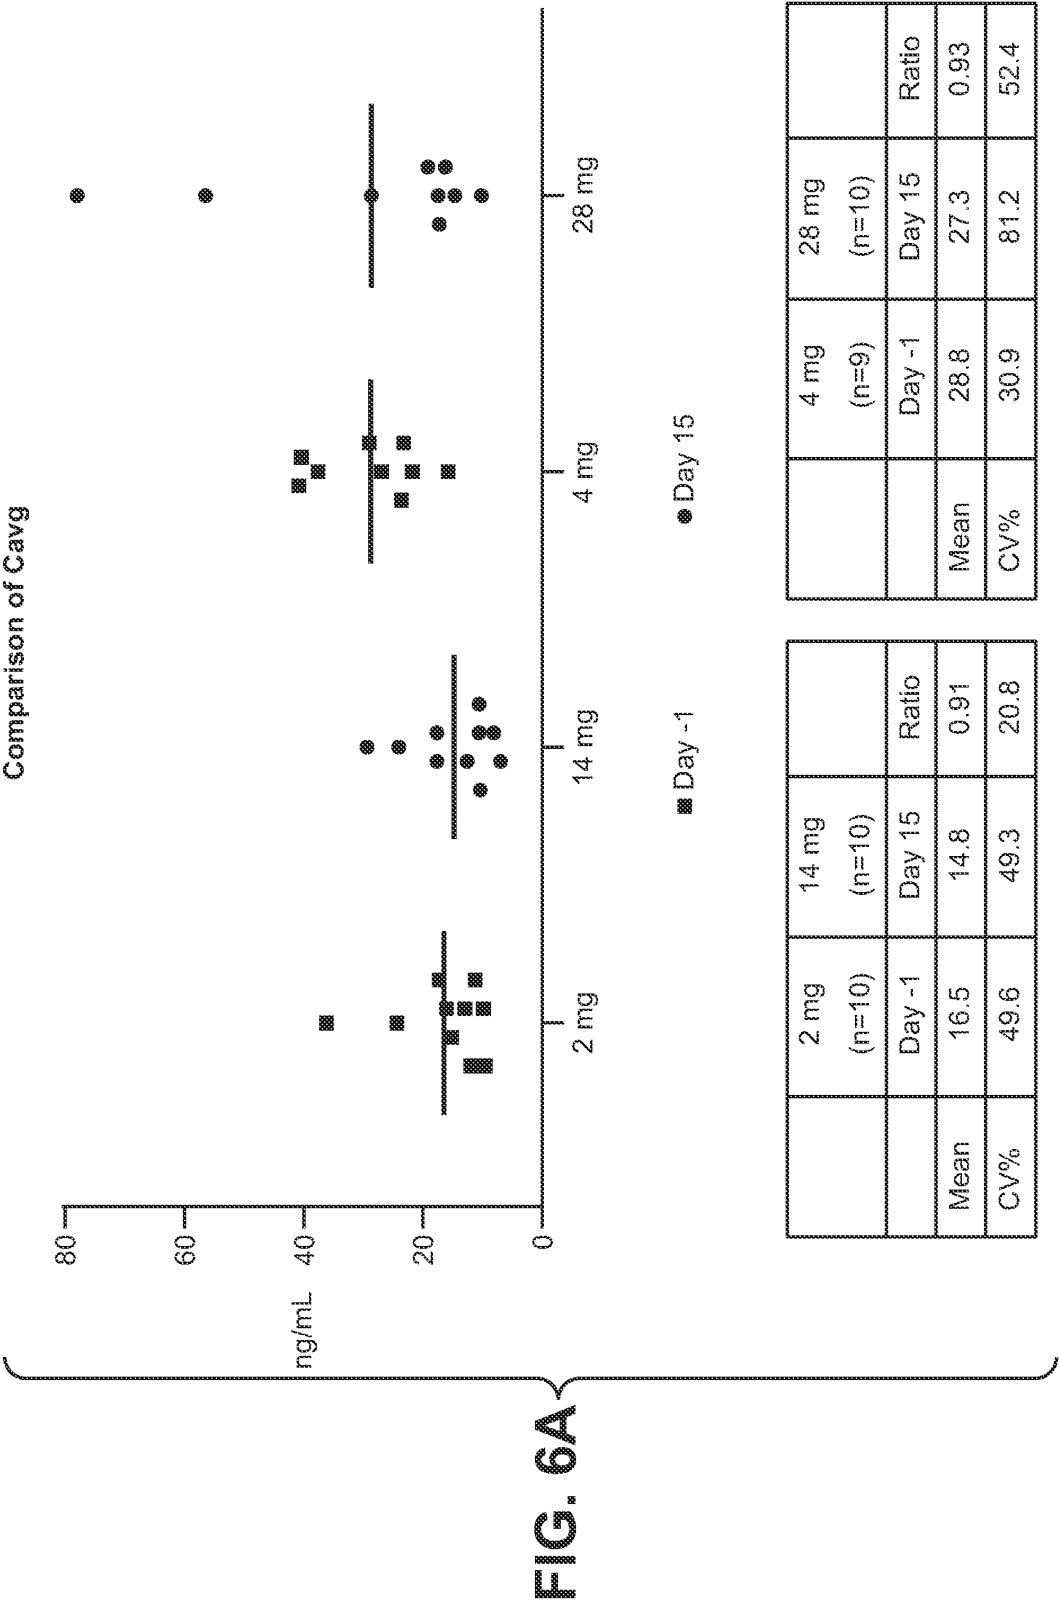


FIG. 6A

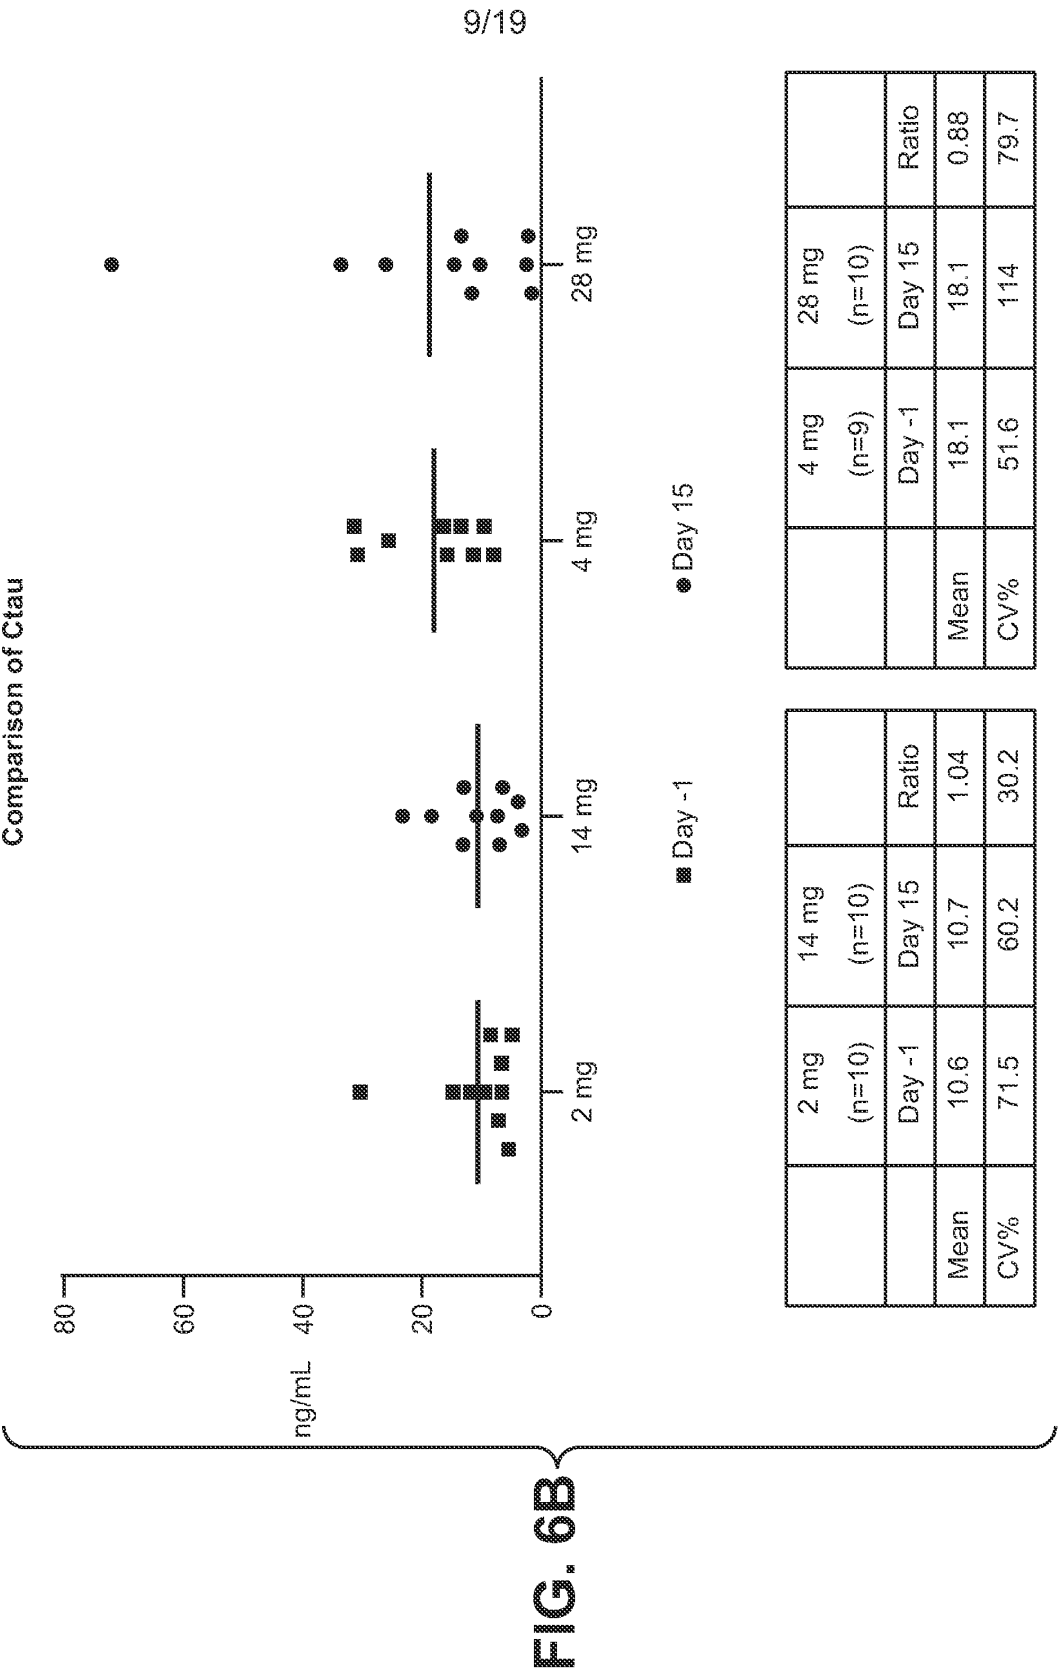


FIG. 6B

FIG. 7



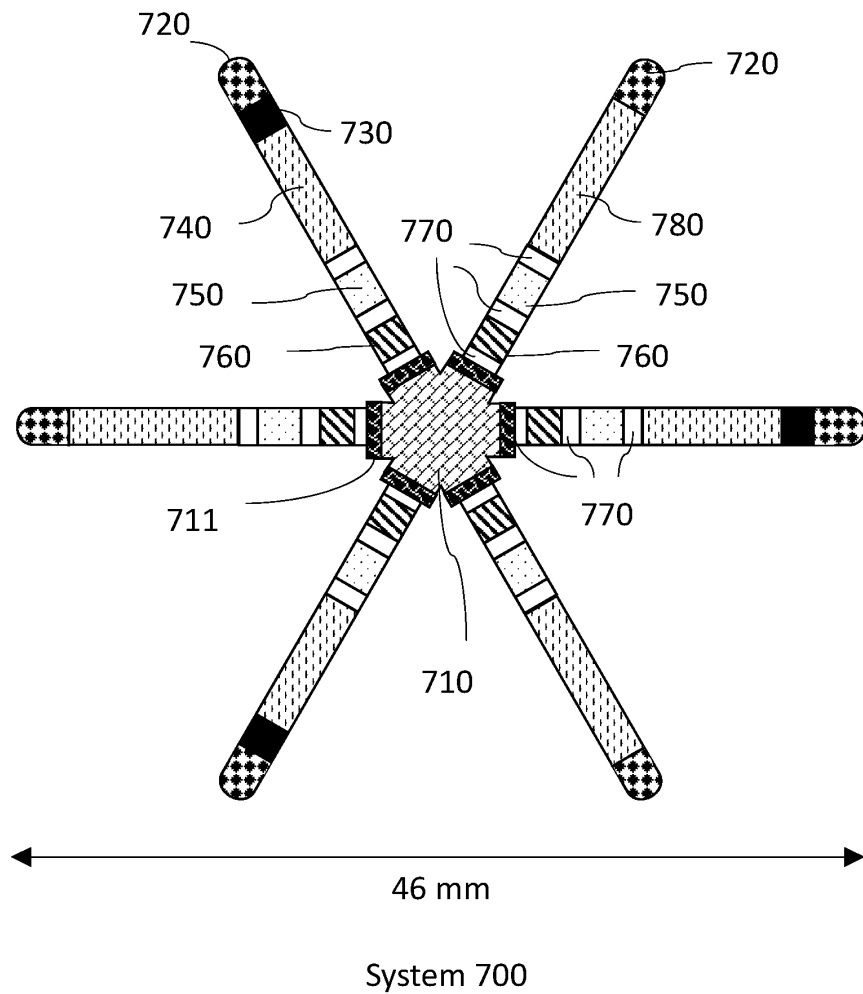


FIG. 8A

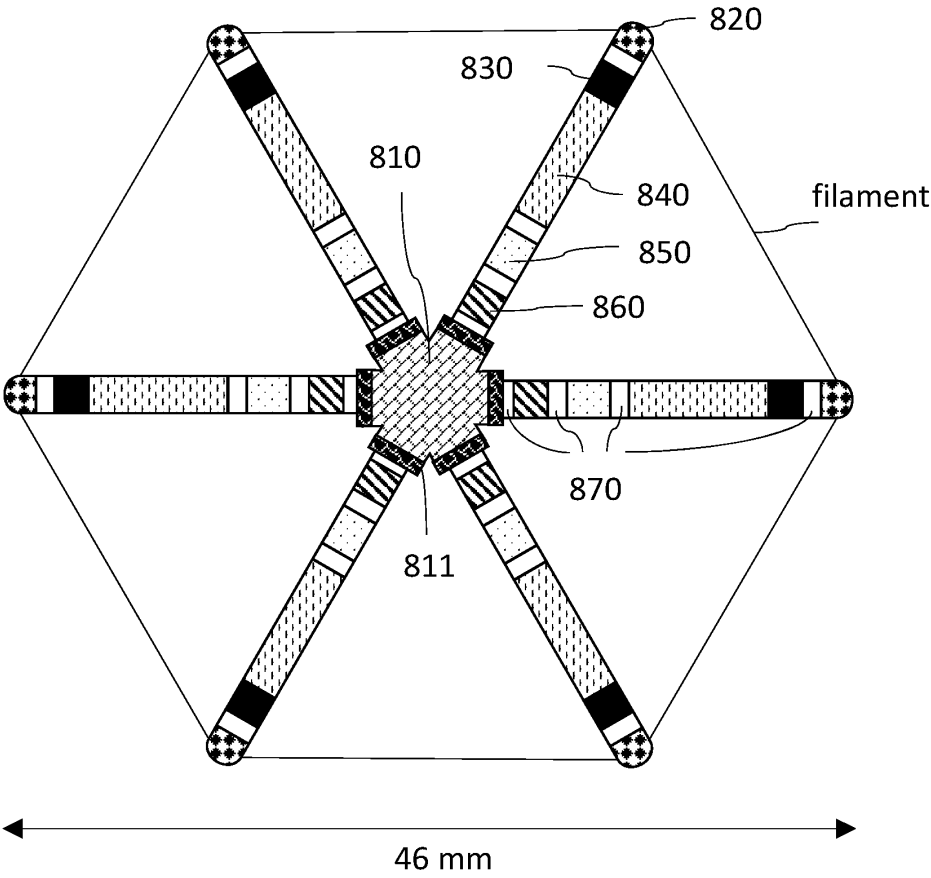

System 800.1

FIG. 8B

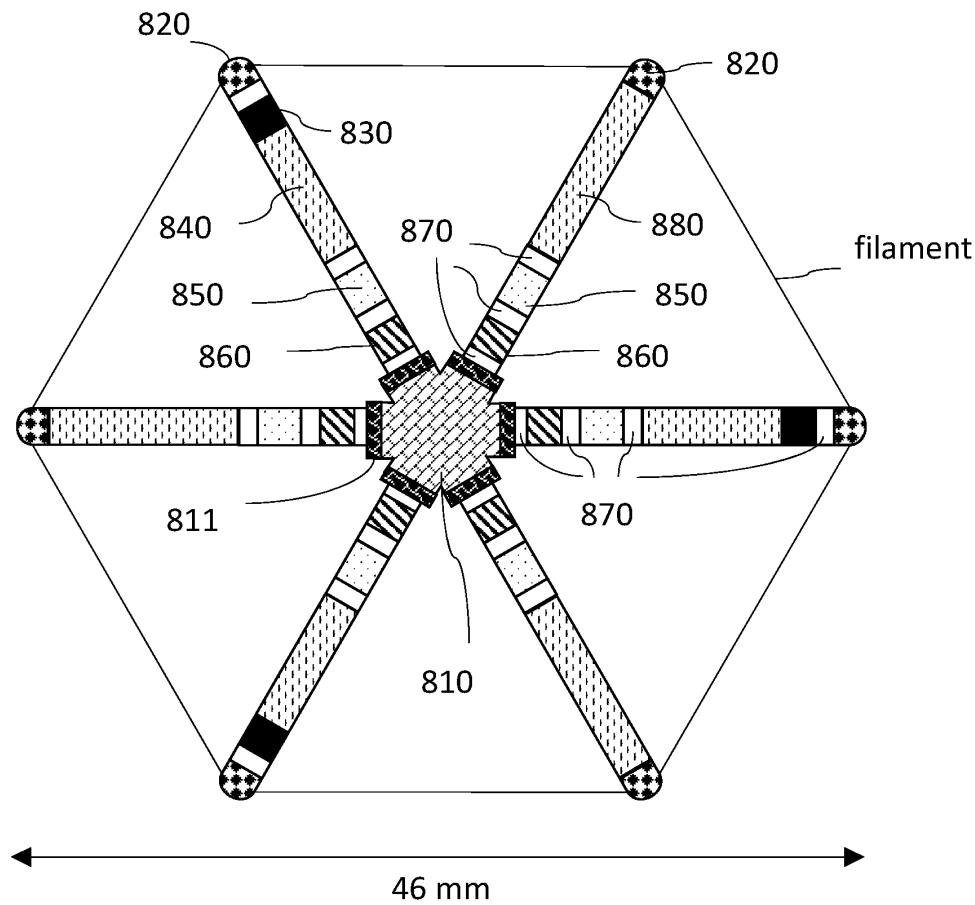

System 800.2

FIG. 8C



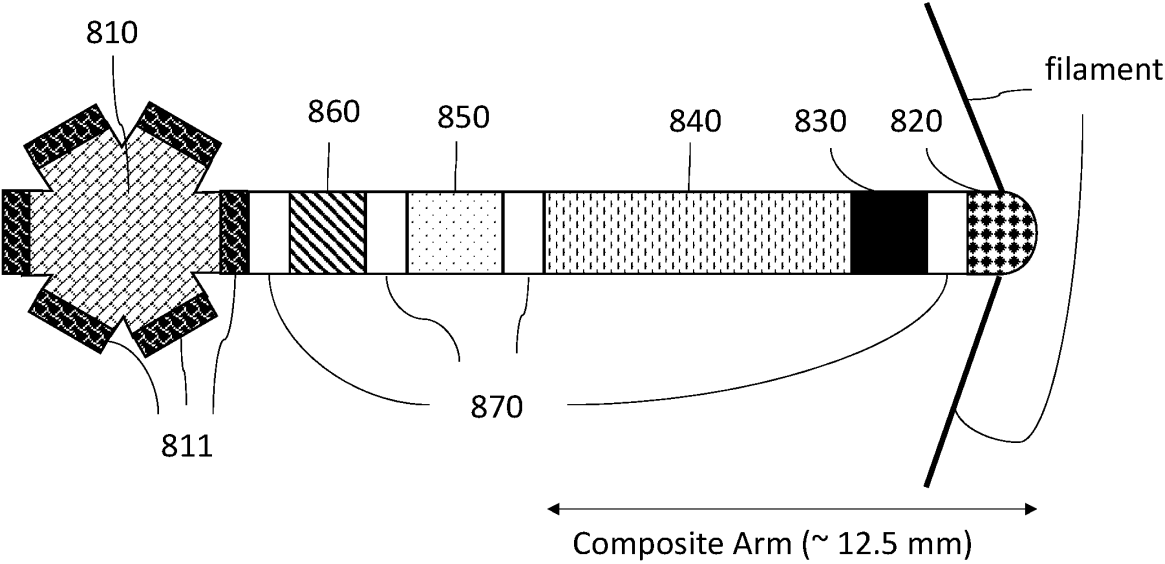


FIG. 8D

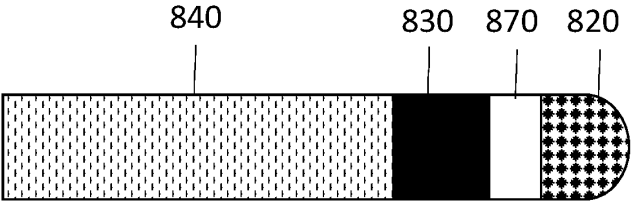

Active Composite Arm

FIG. 8E

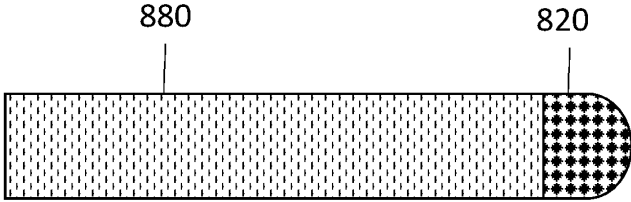

Inactive Composite Arm

FIG. 9A

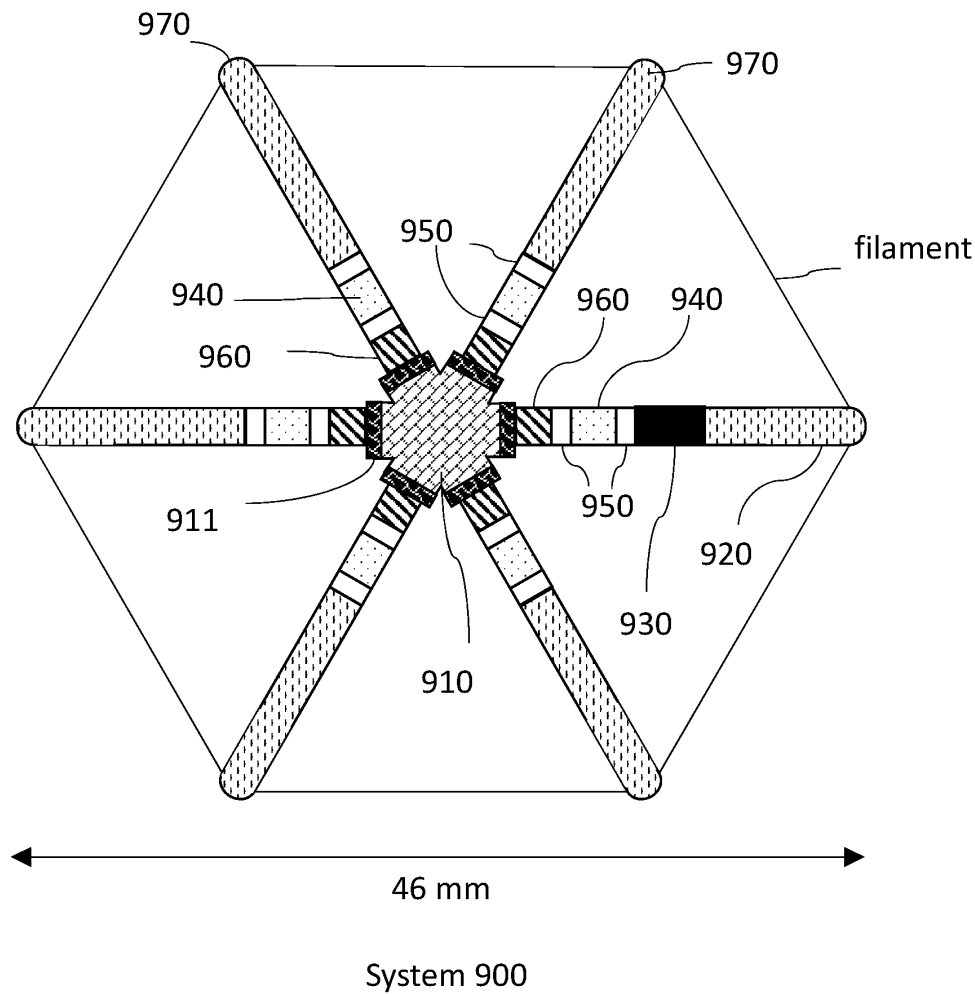


FIG. 9B

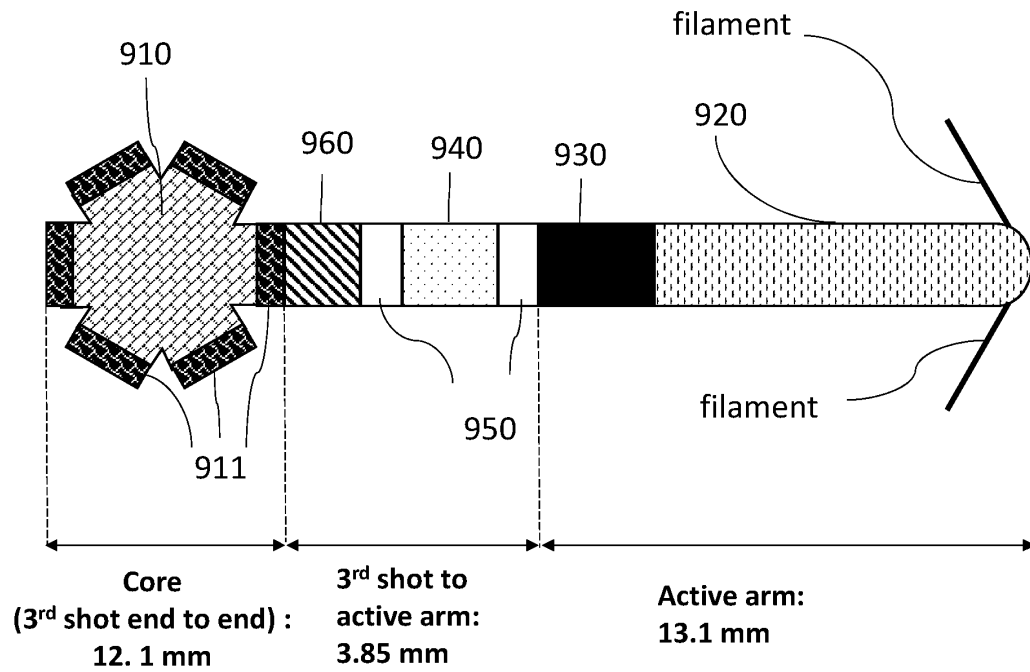


FIG. 9C


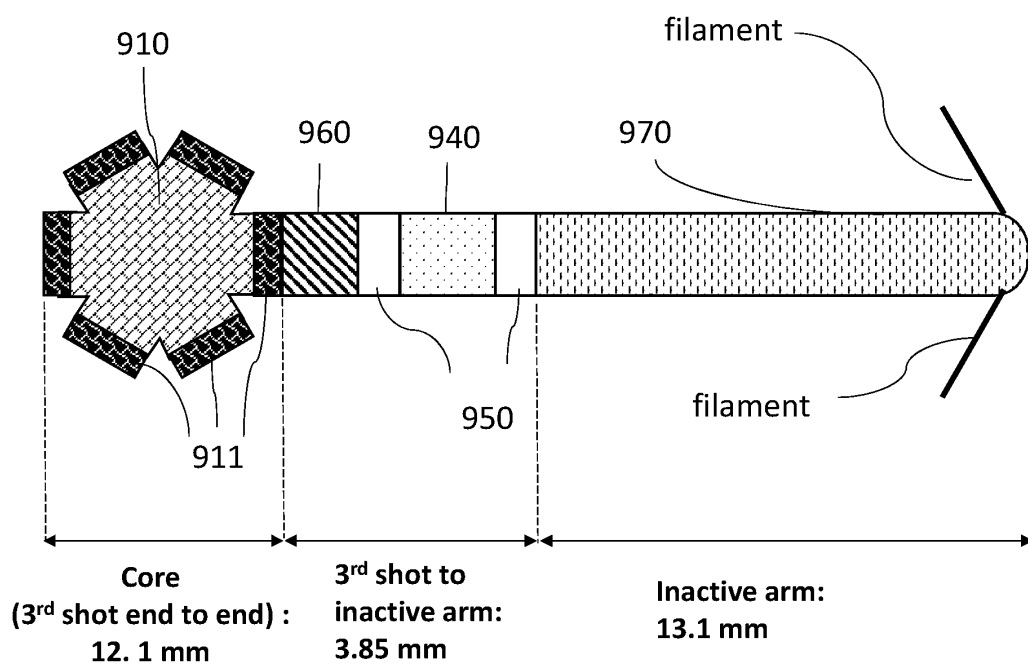


FIG. 10A

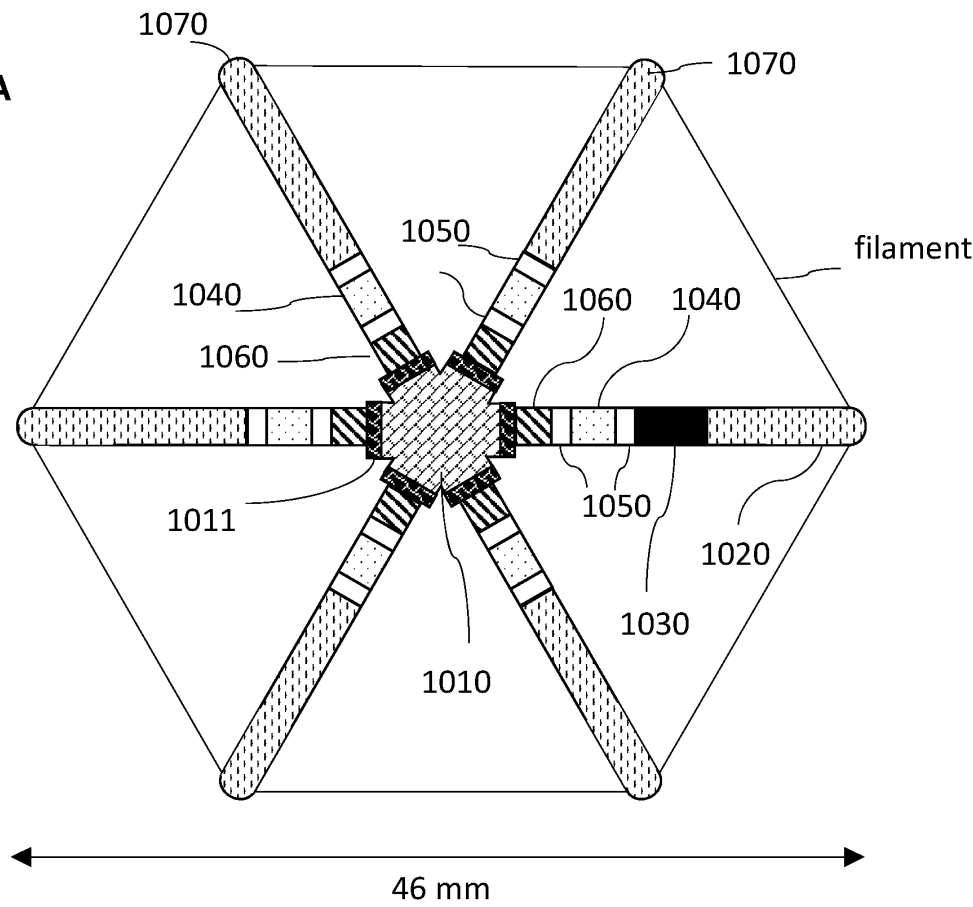

System 1000

FIG. 10B

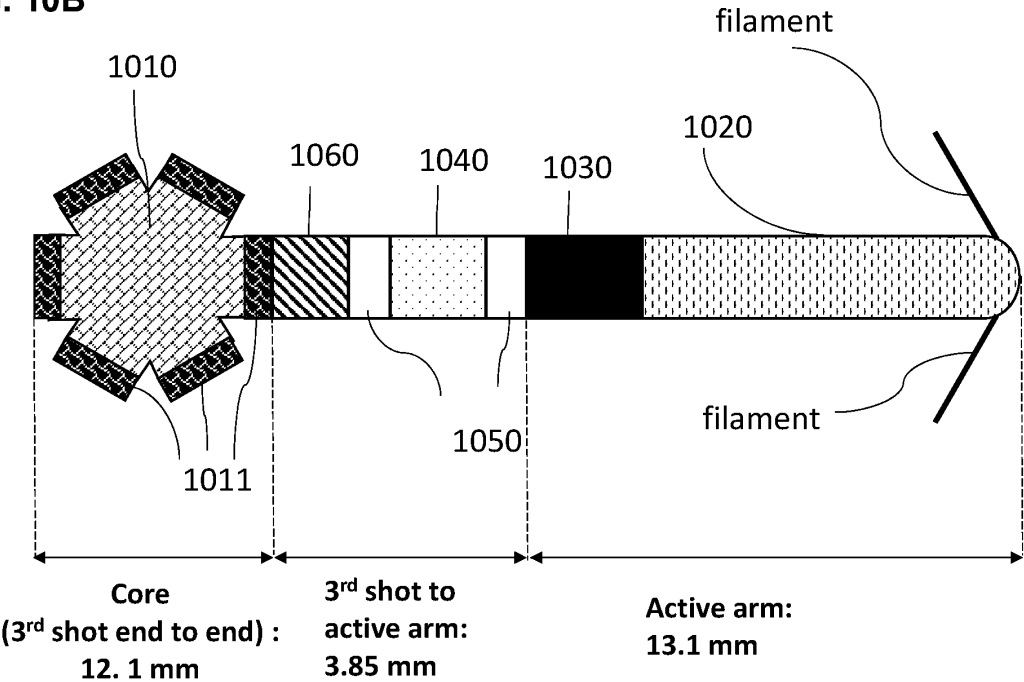


FIG. 10C



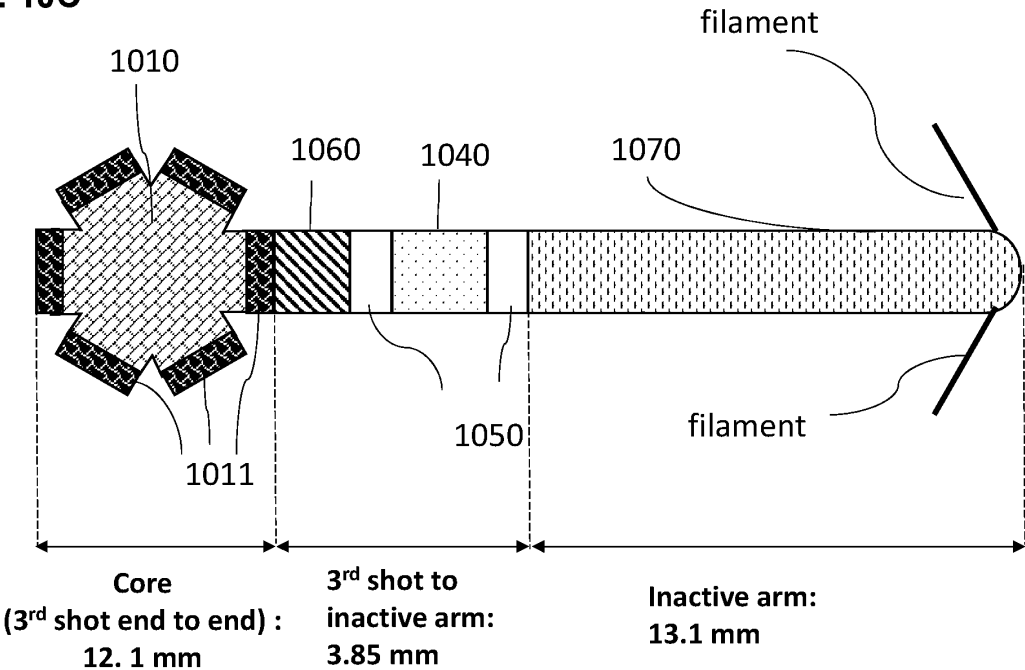



FIG. 11A

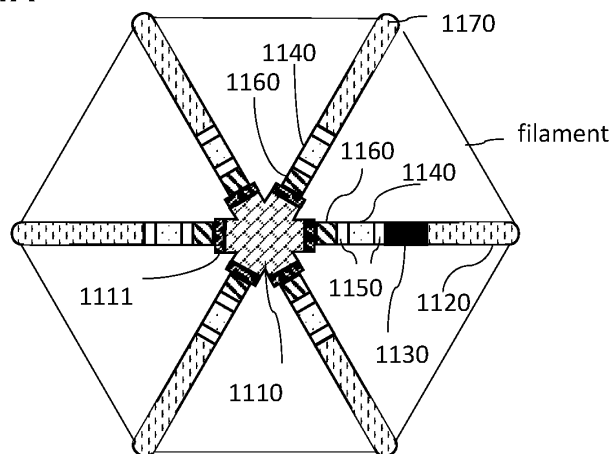

System 1100.1
16mg risperidone

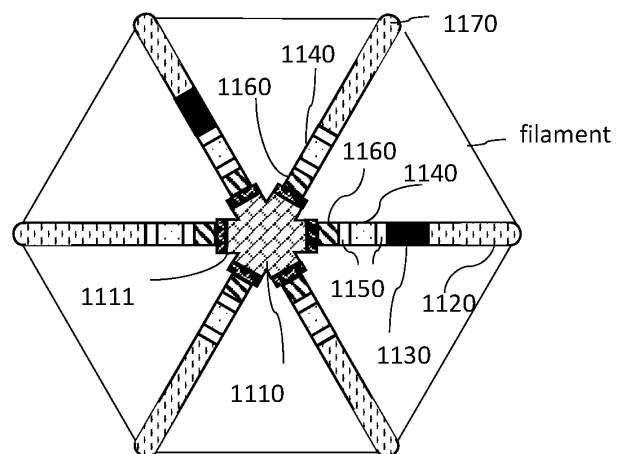

System 1100.2
32mg risperidone

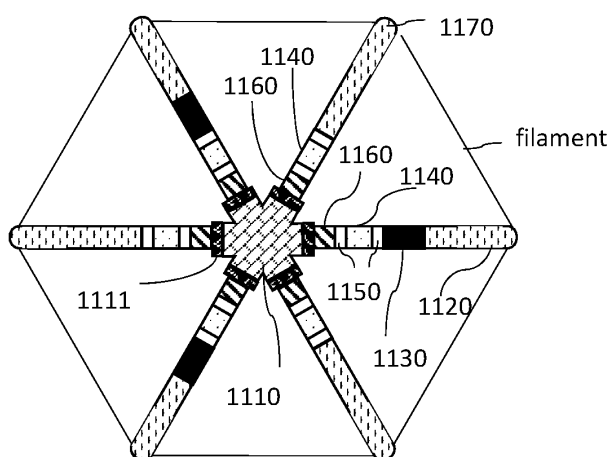

System 1100.3
48mg risperidone

FIG. 11B

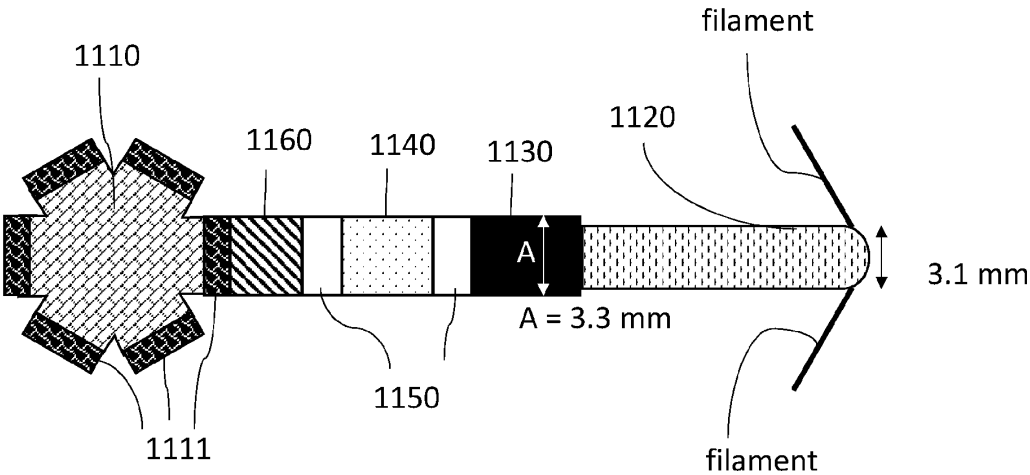


FIG. 11C

