

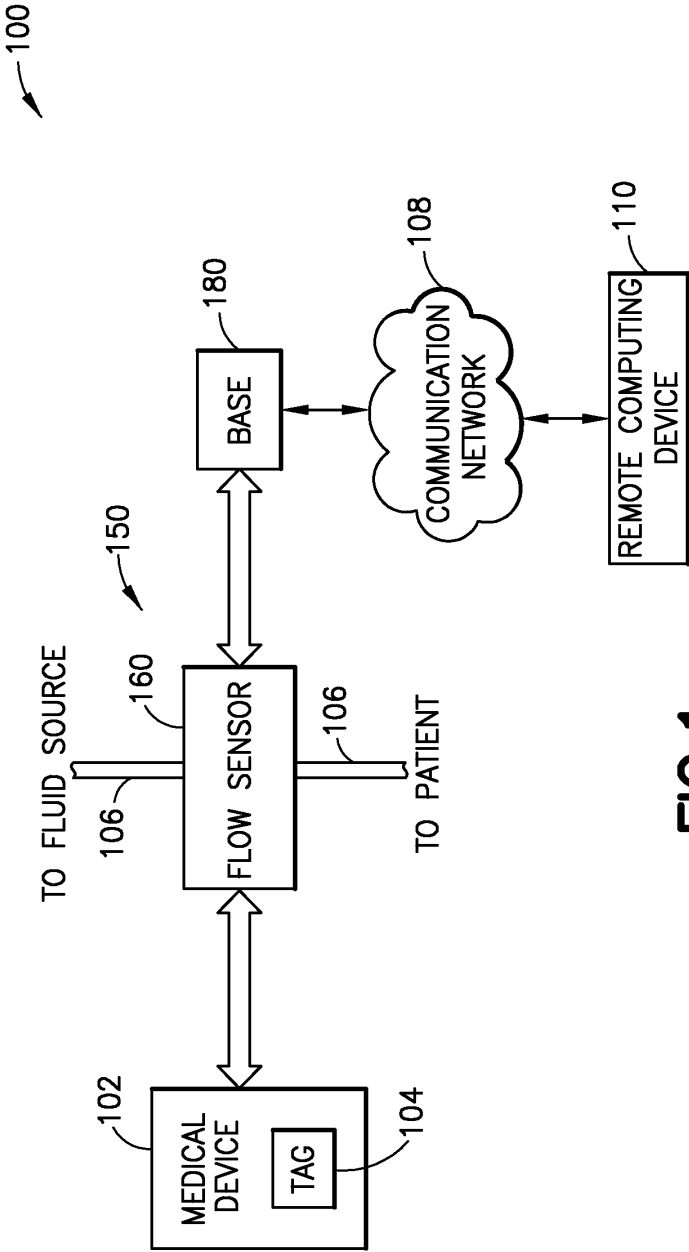


FIG.1

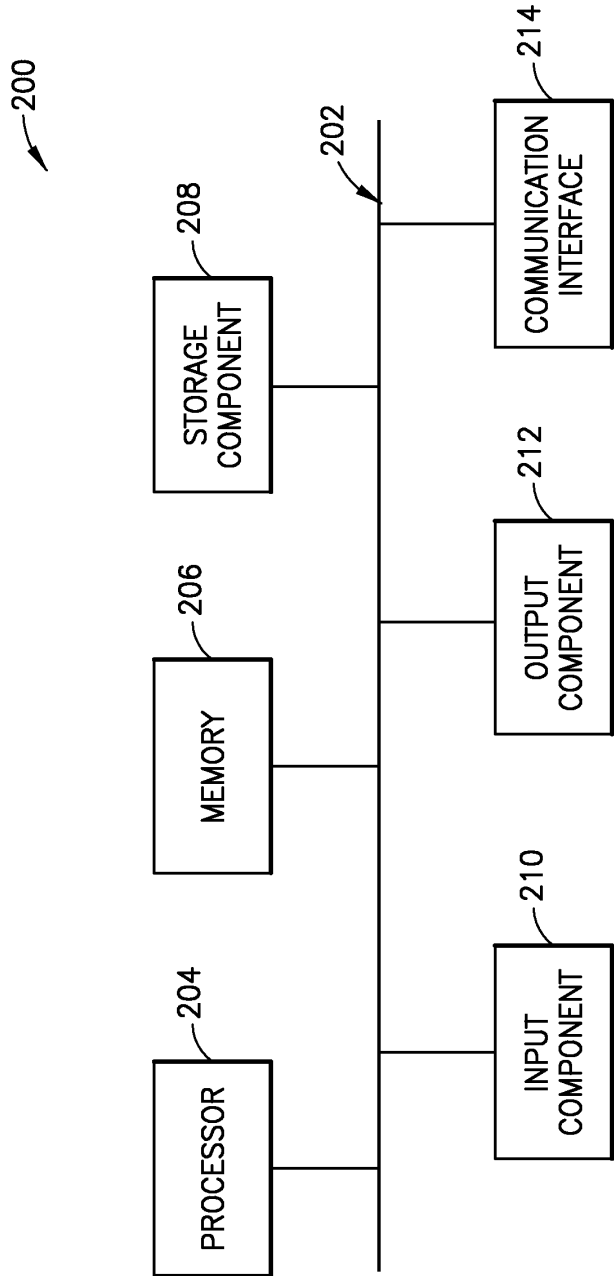


FIG.2

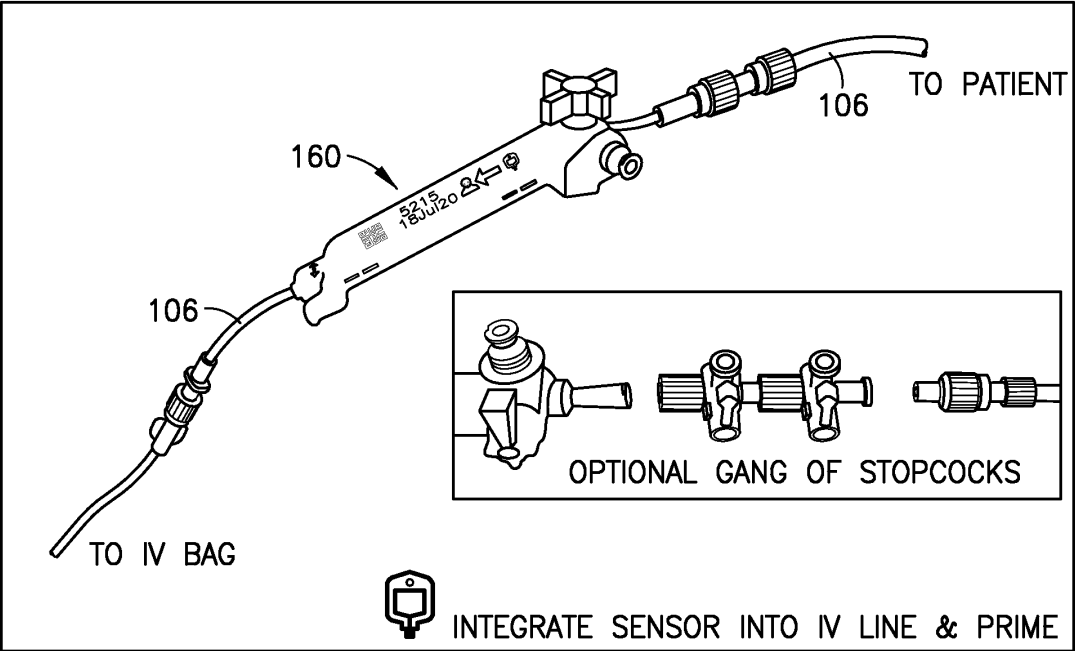


FIG.3A

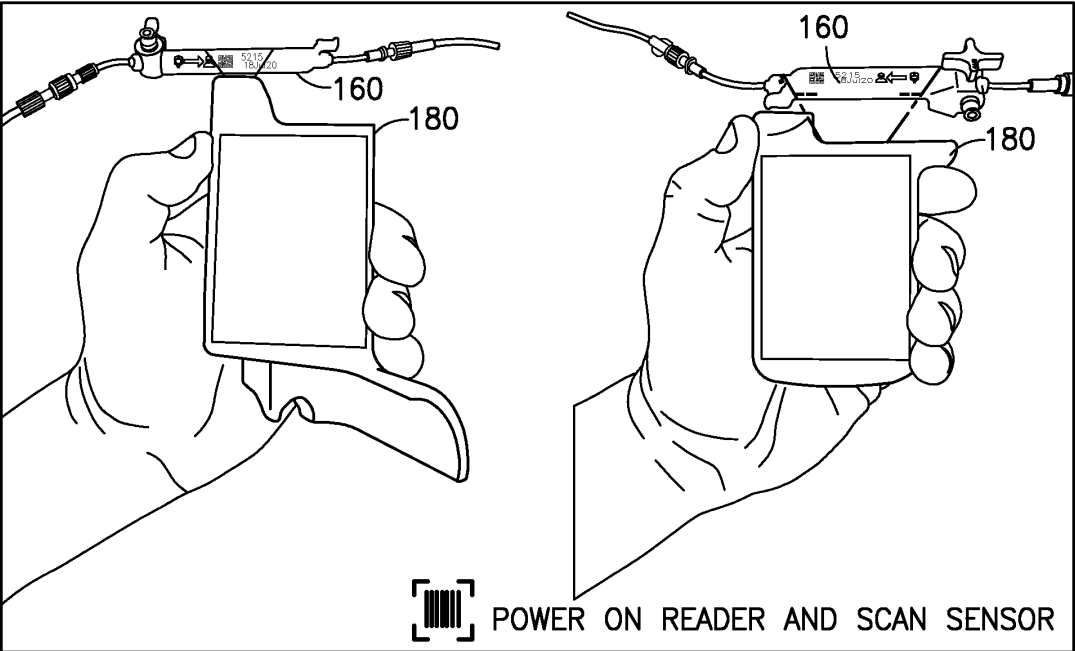
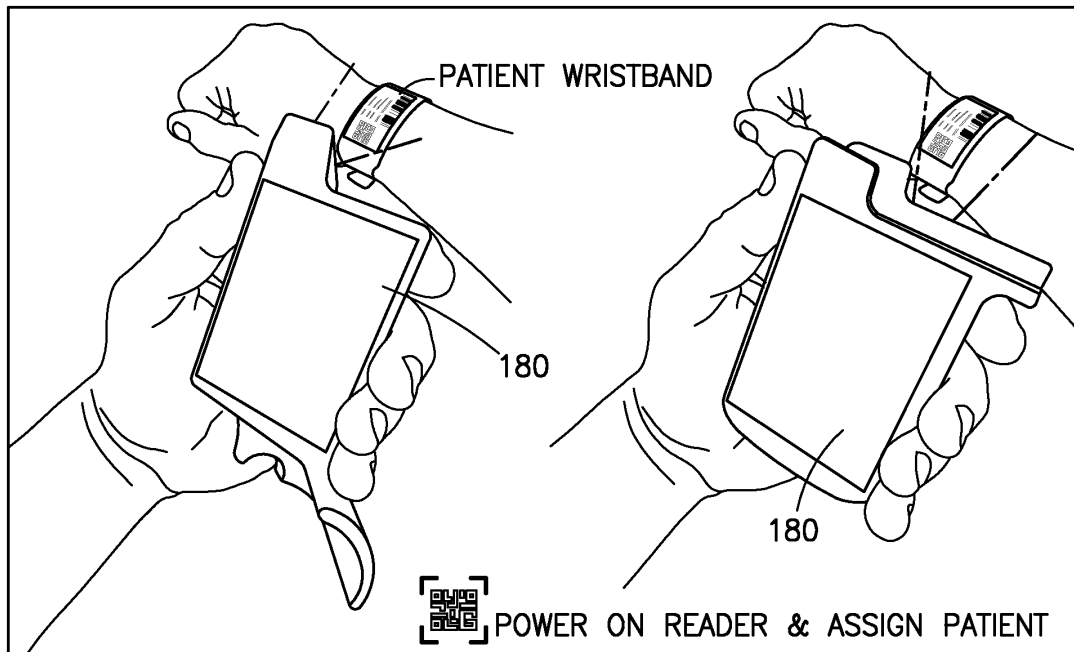
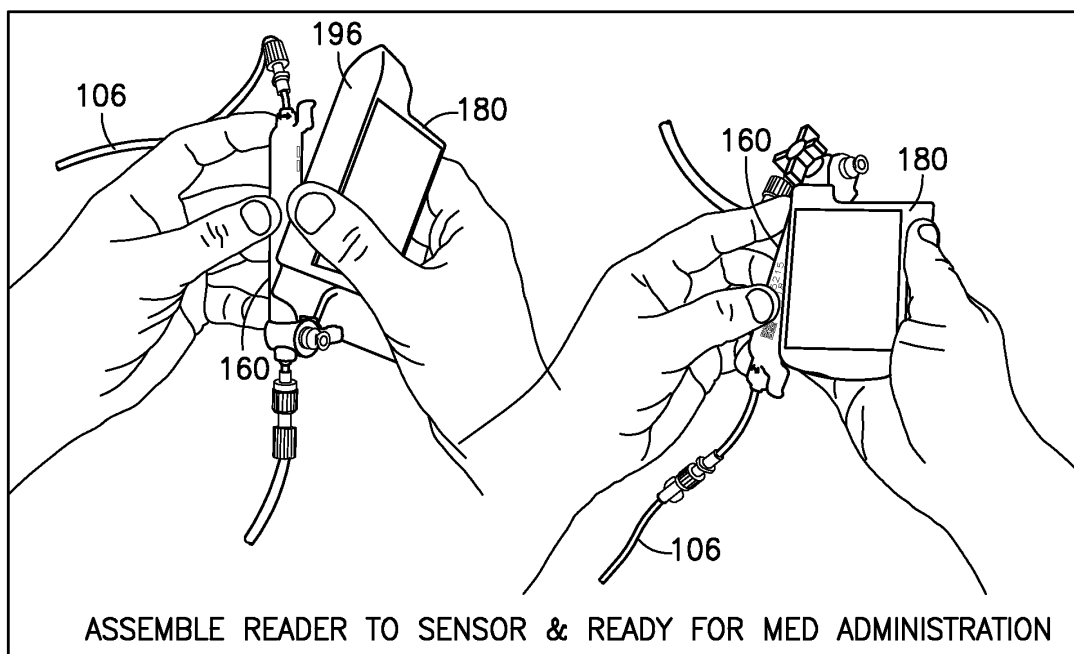


FIG.3B

**FIG. 3C****FIG. 3D**

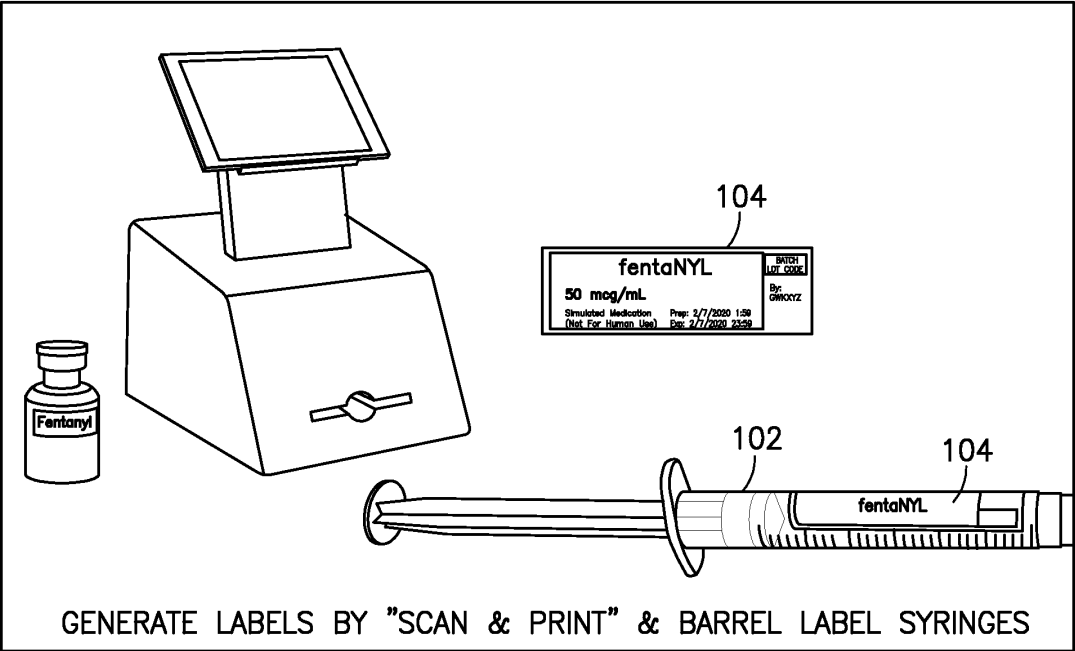


FIG.3E

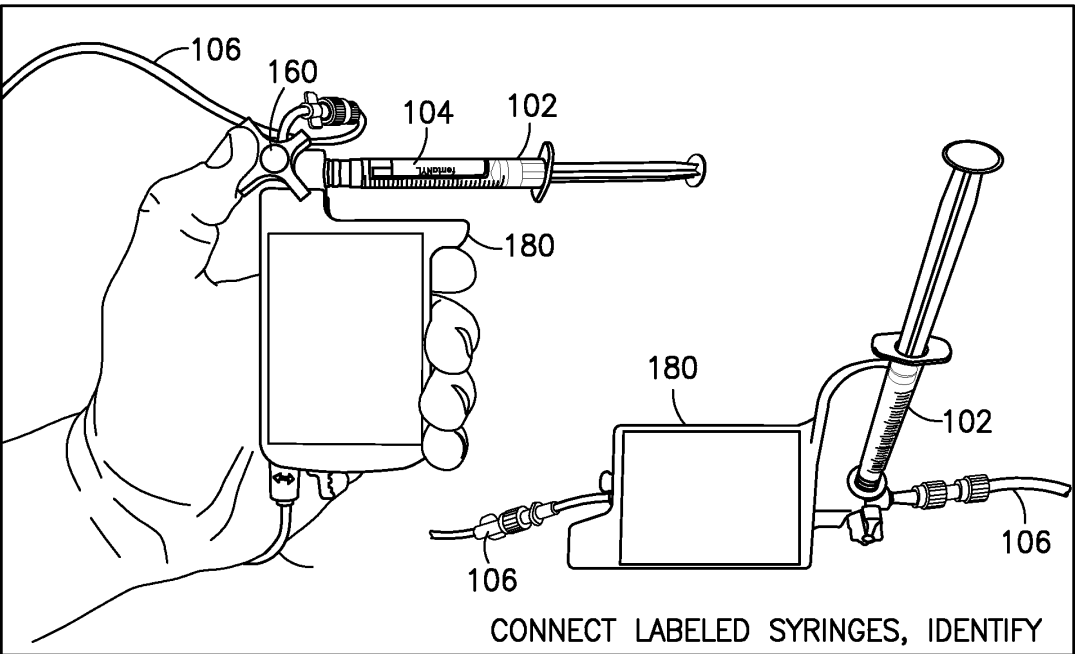
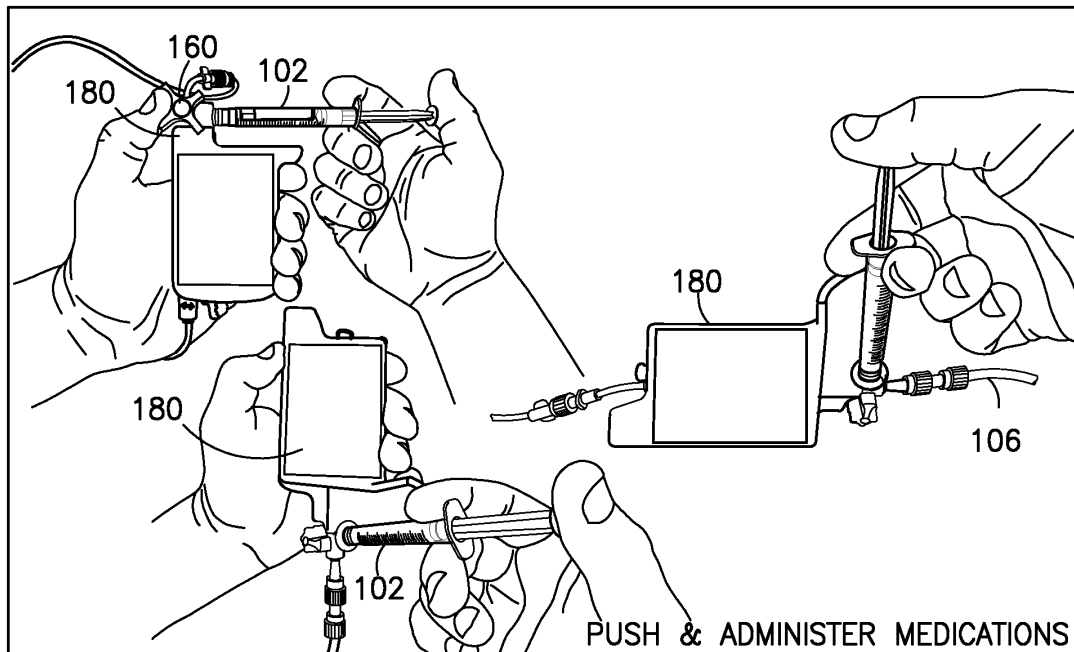
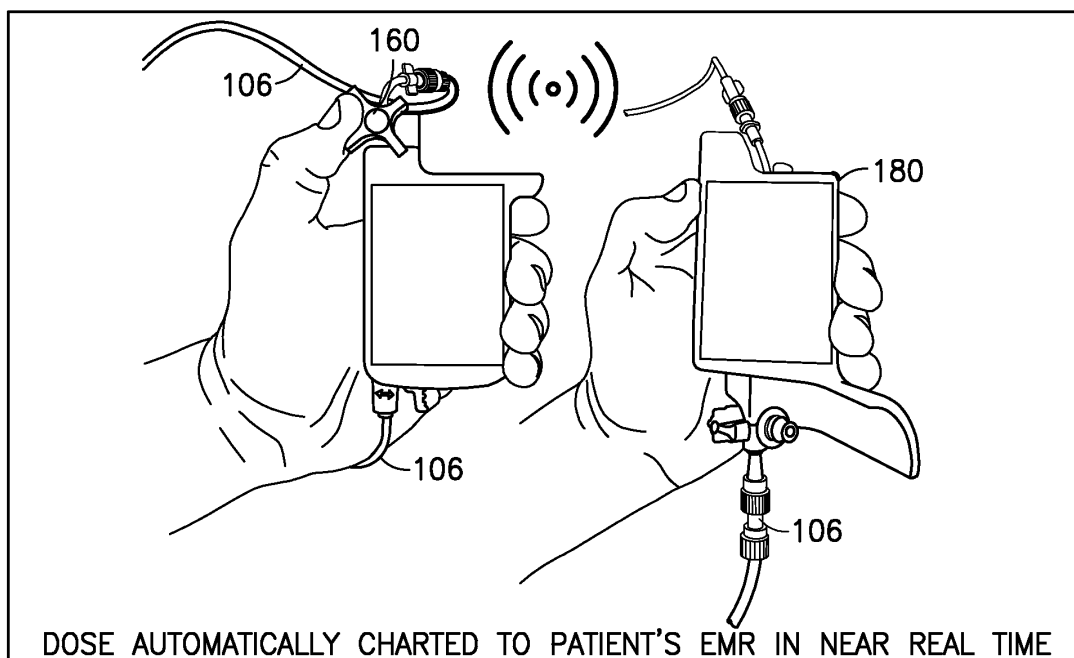


FIG.3F

**FIG.3G****FIG.3H**

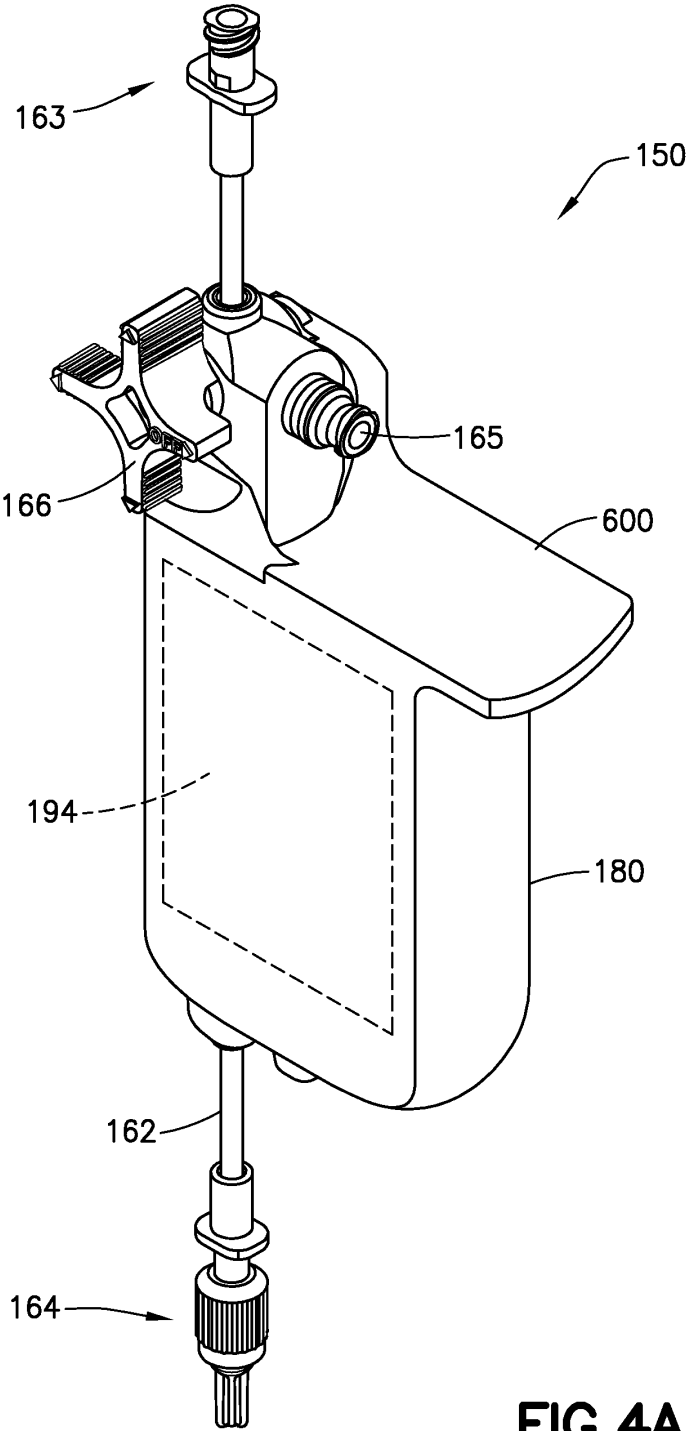


FIG. 4A

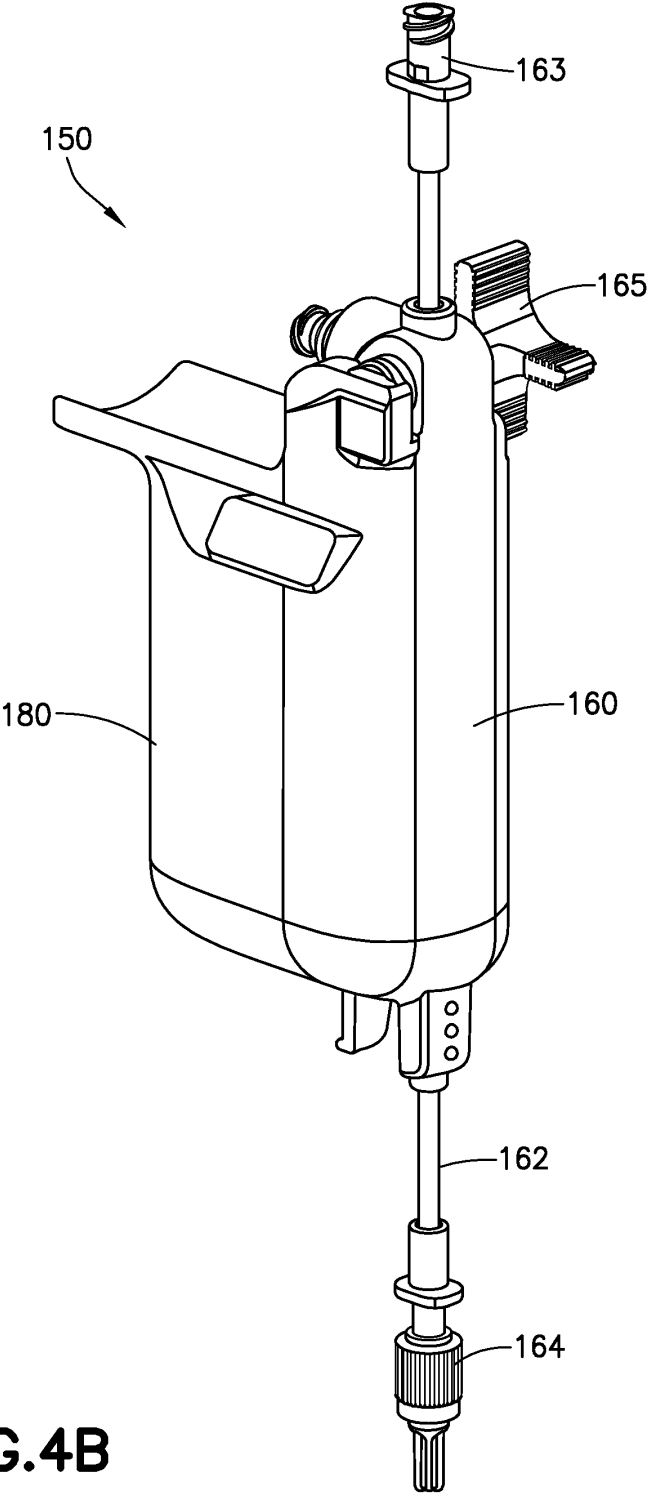
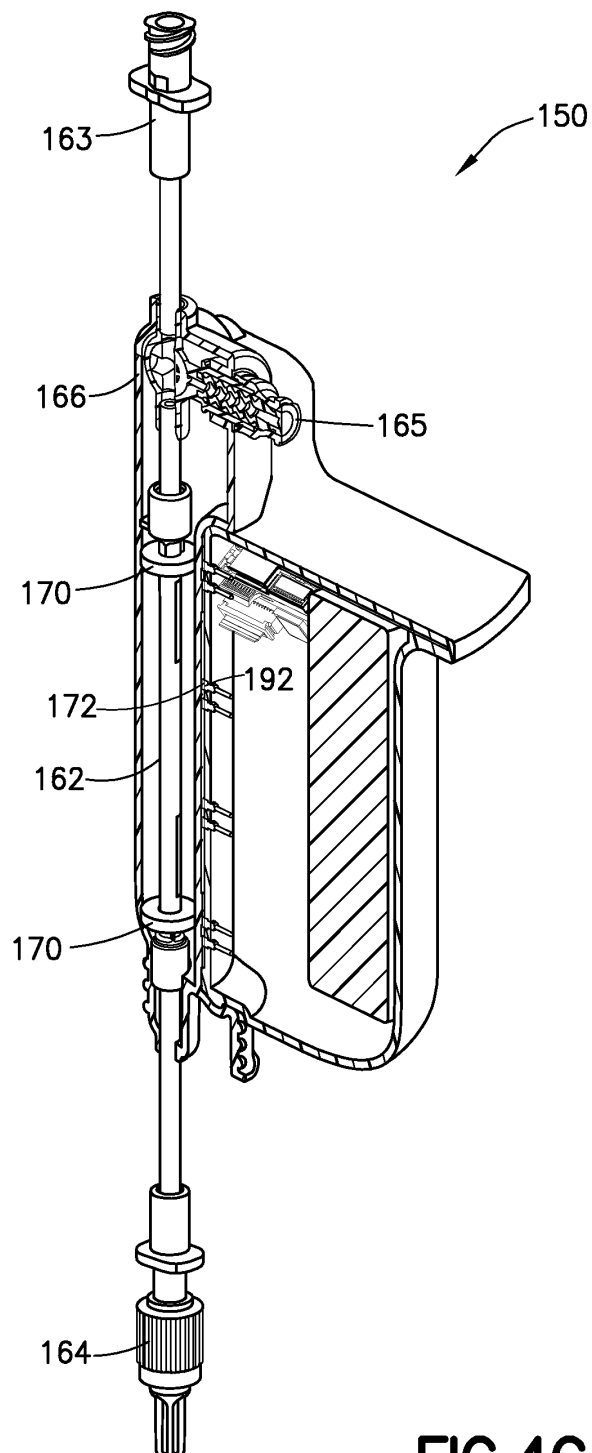


FIG. 4B

**FIG. 4C**

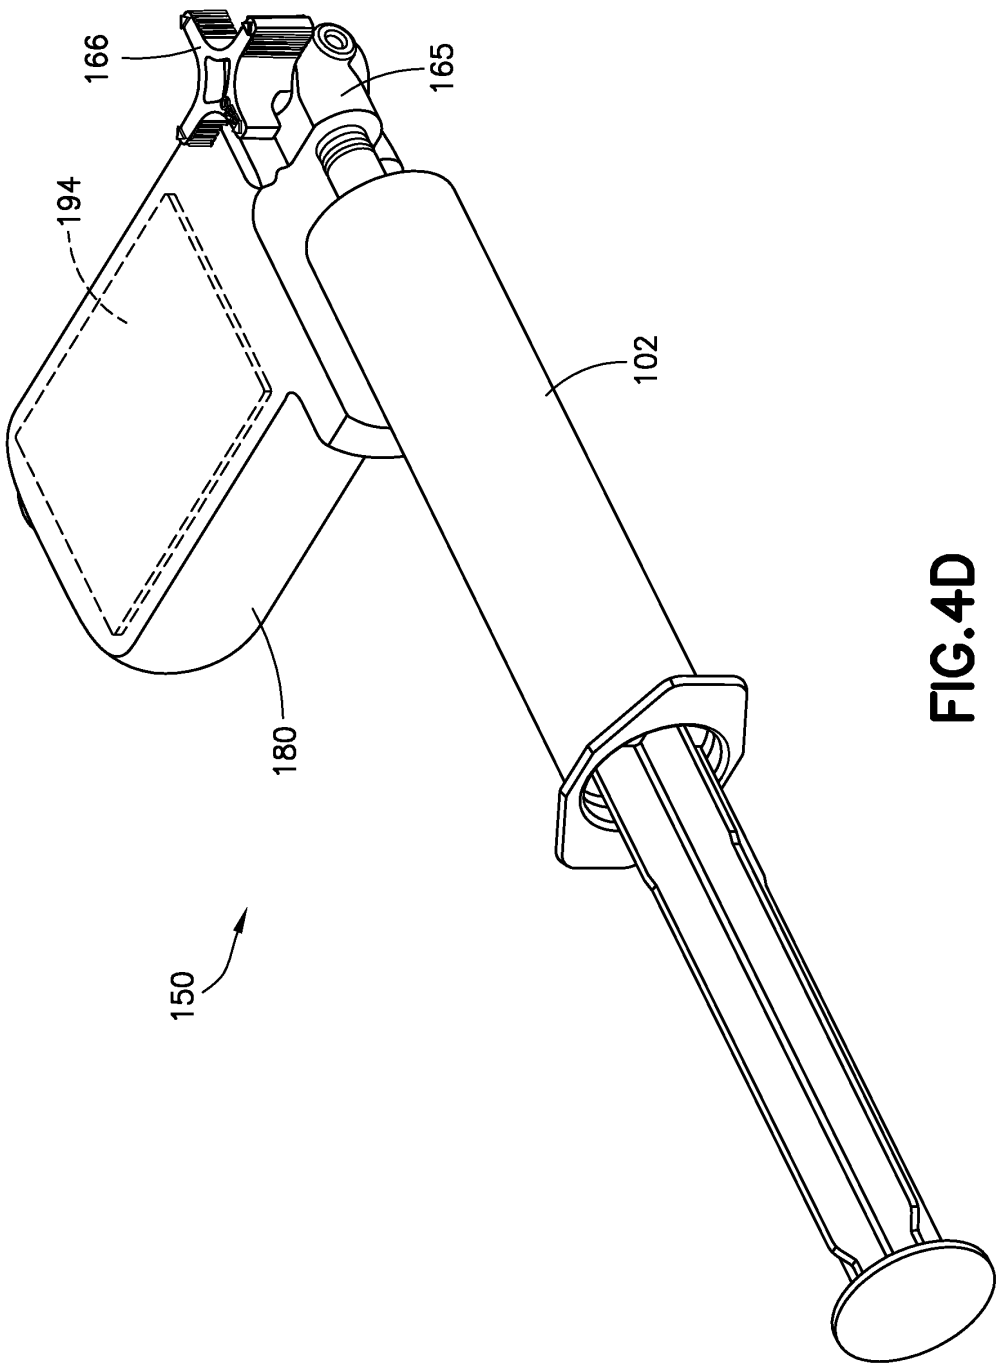


FIG. 4D

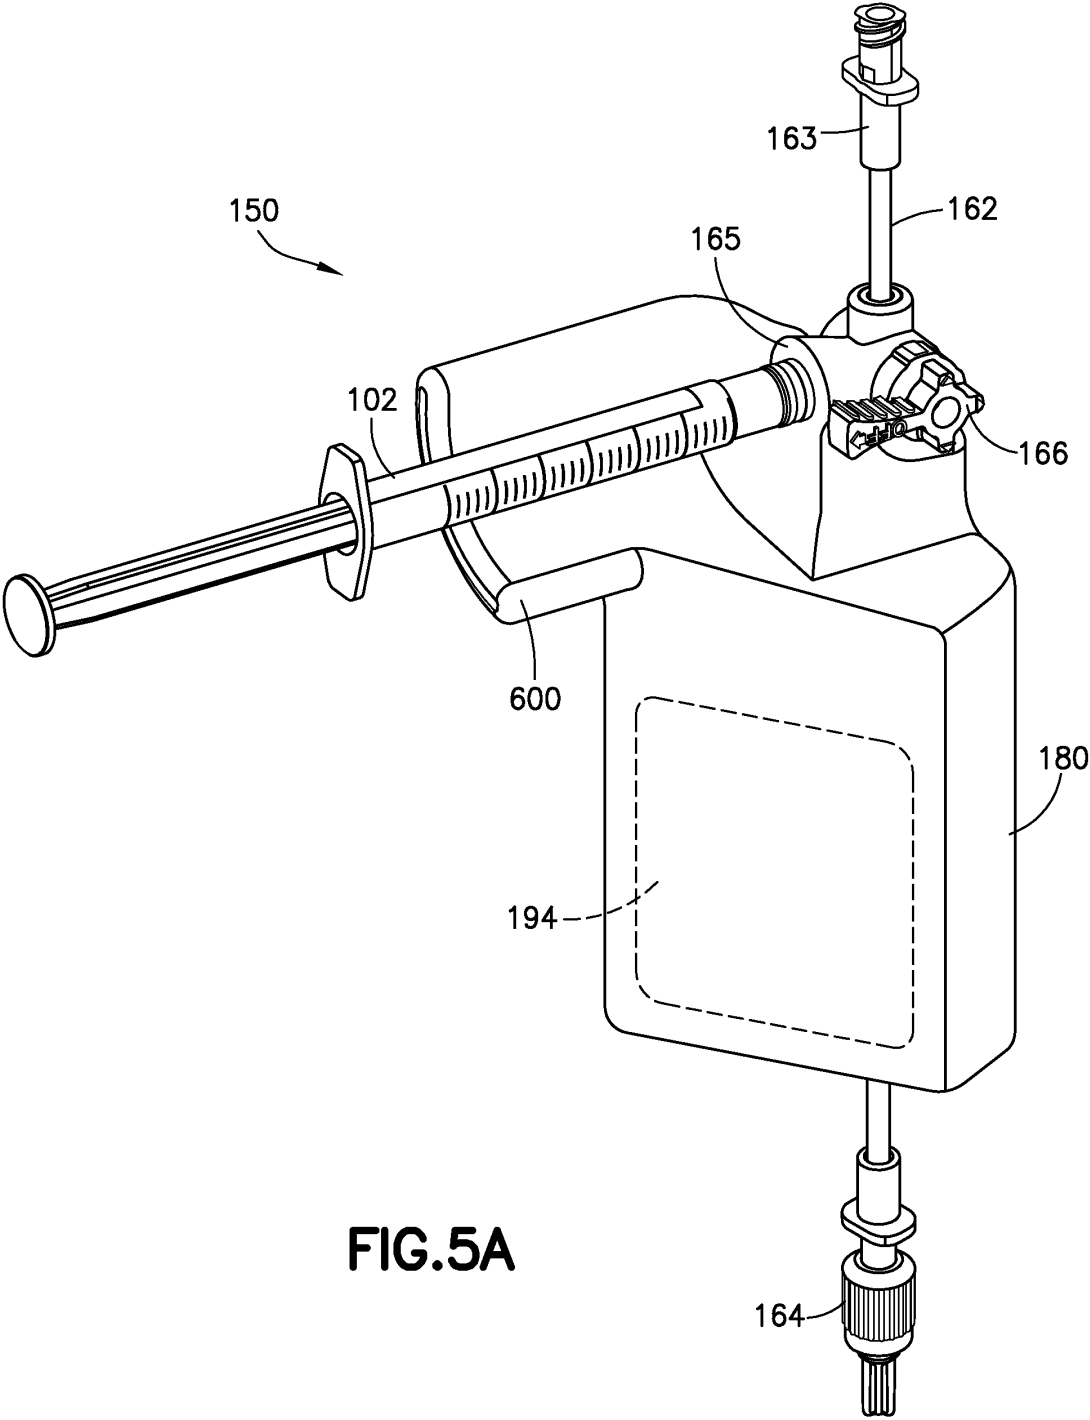


FIG.5A

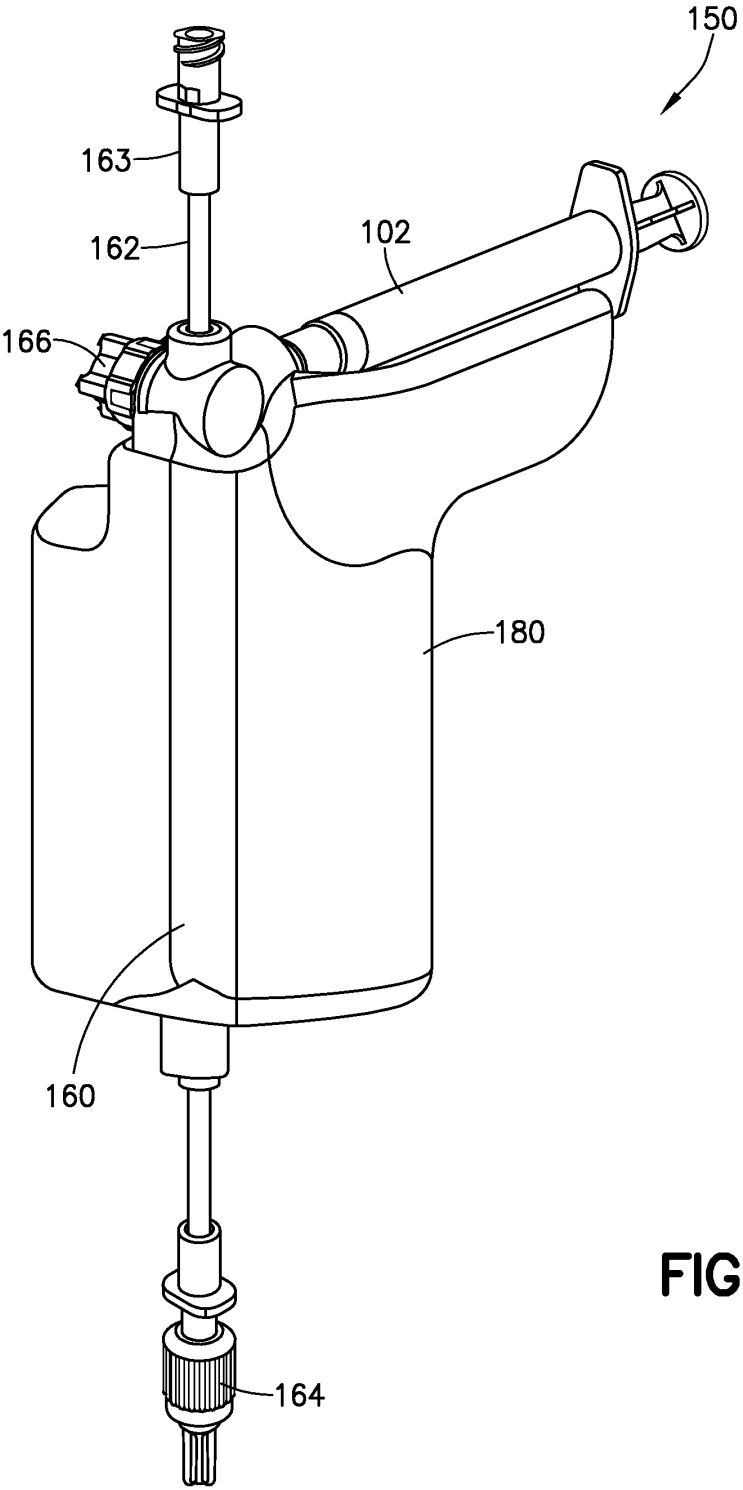


FIG.5B

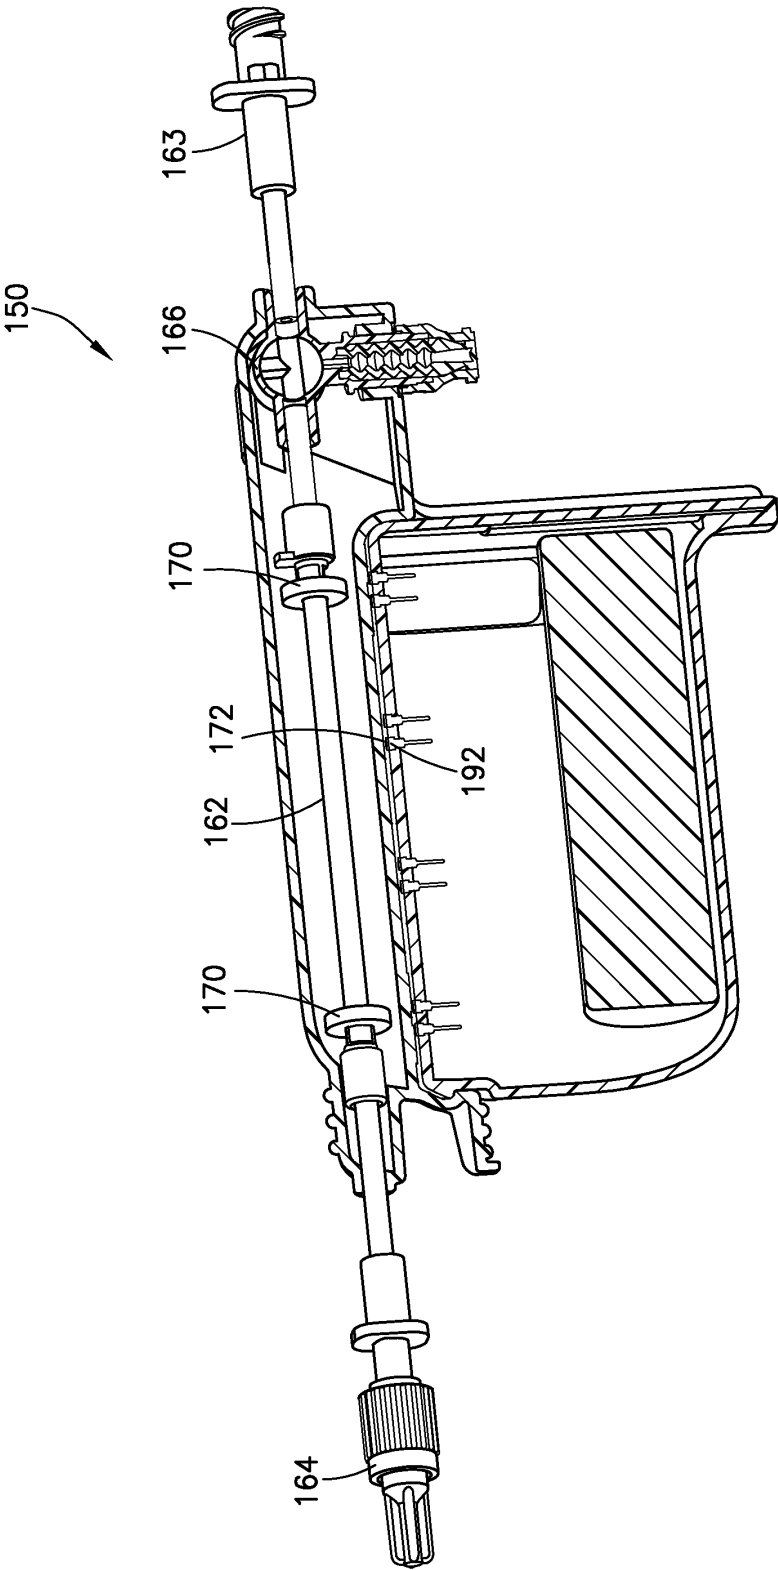
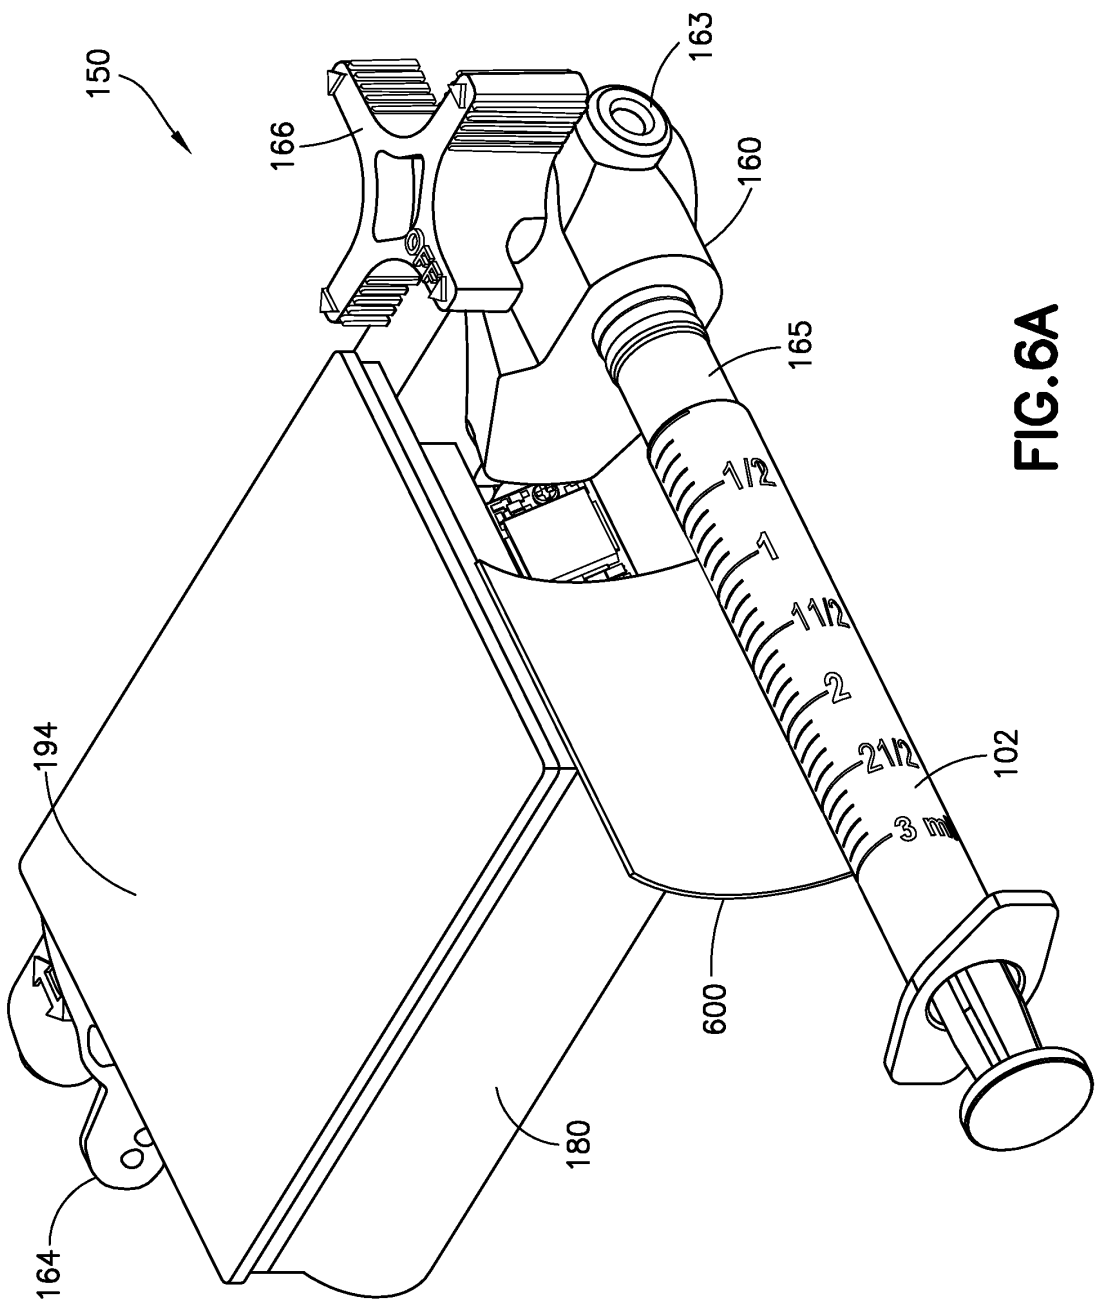


FIG.5C



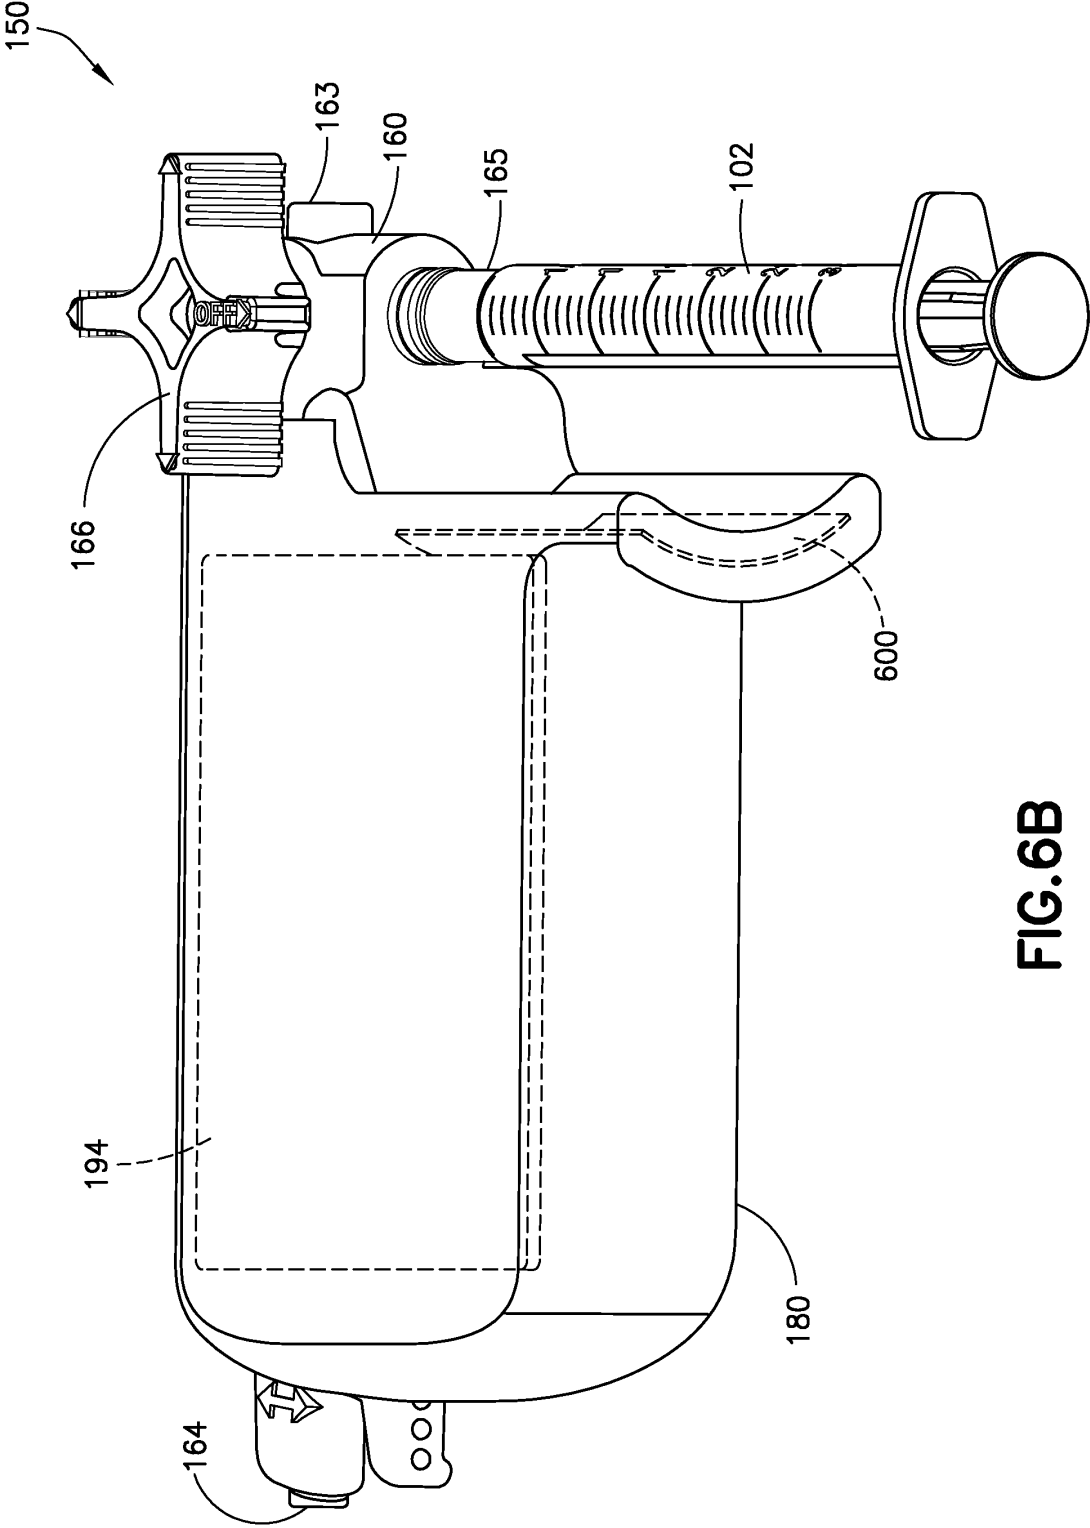


FIG. 6B

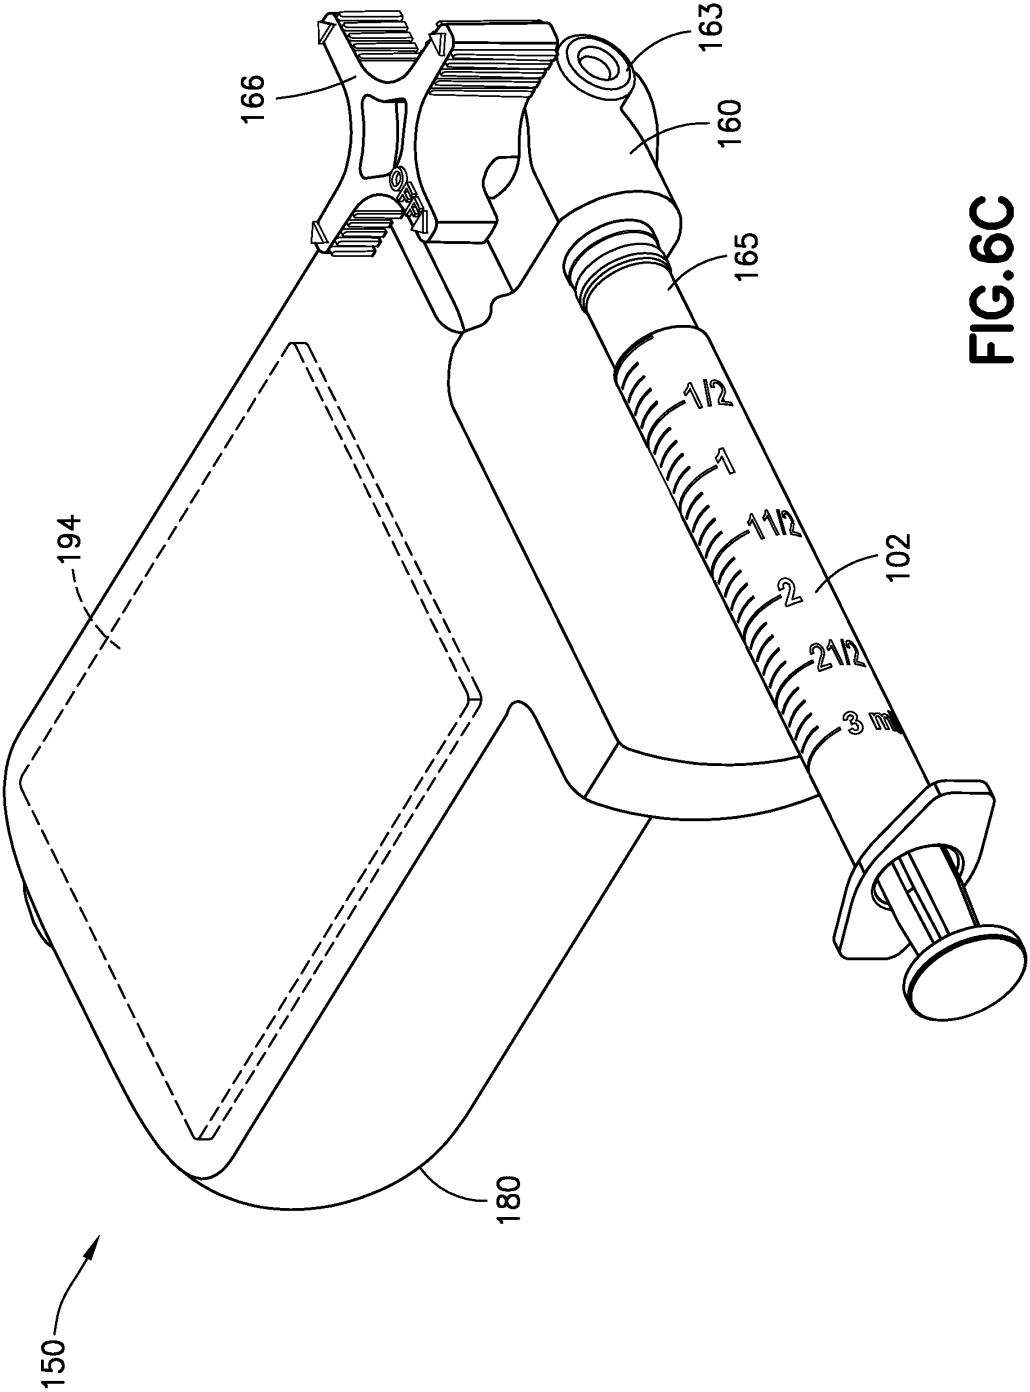


FIG. 6C

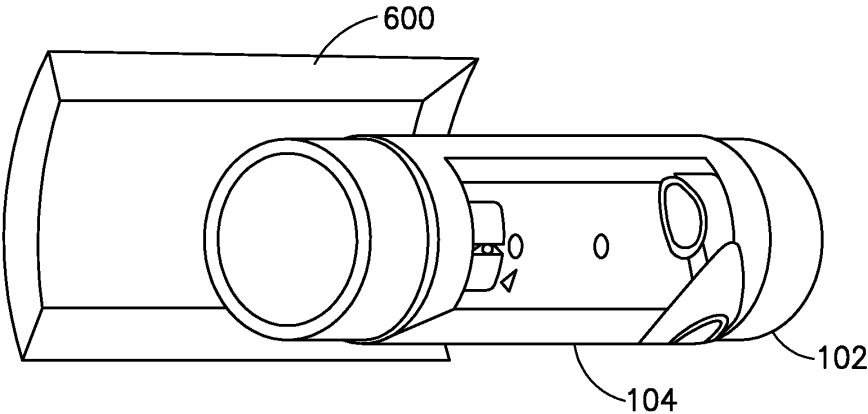


FIG. 7A

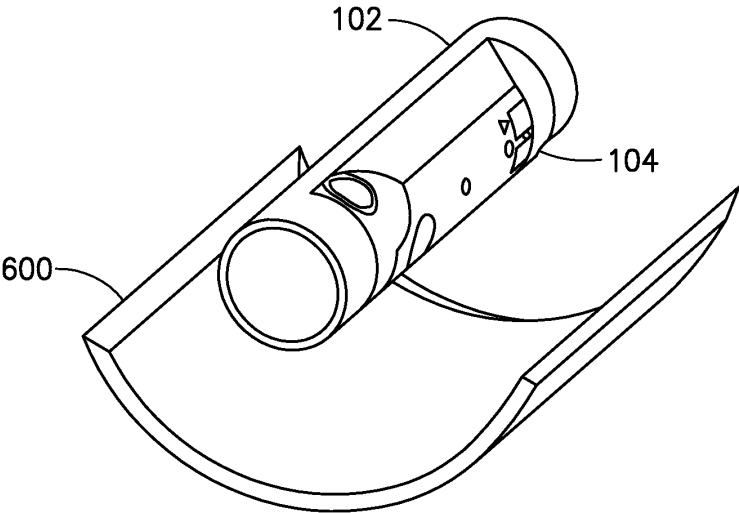


FIG. 7B


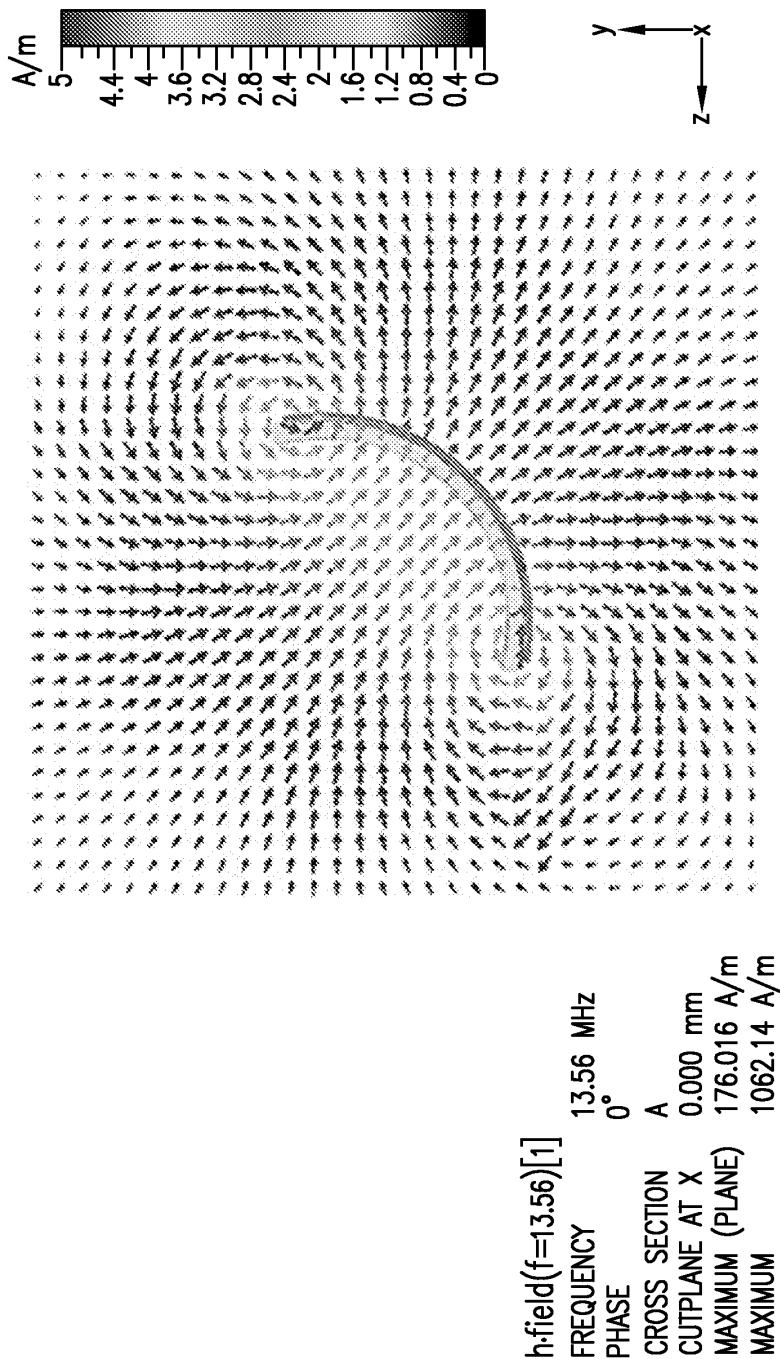


FIG.8

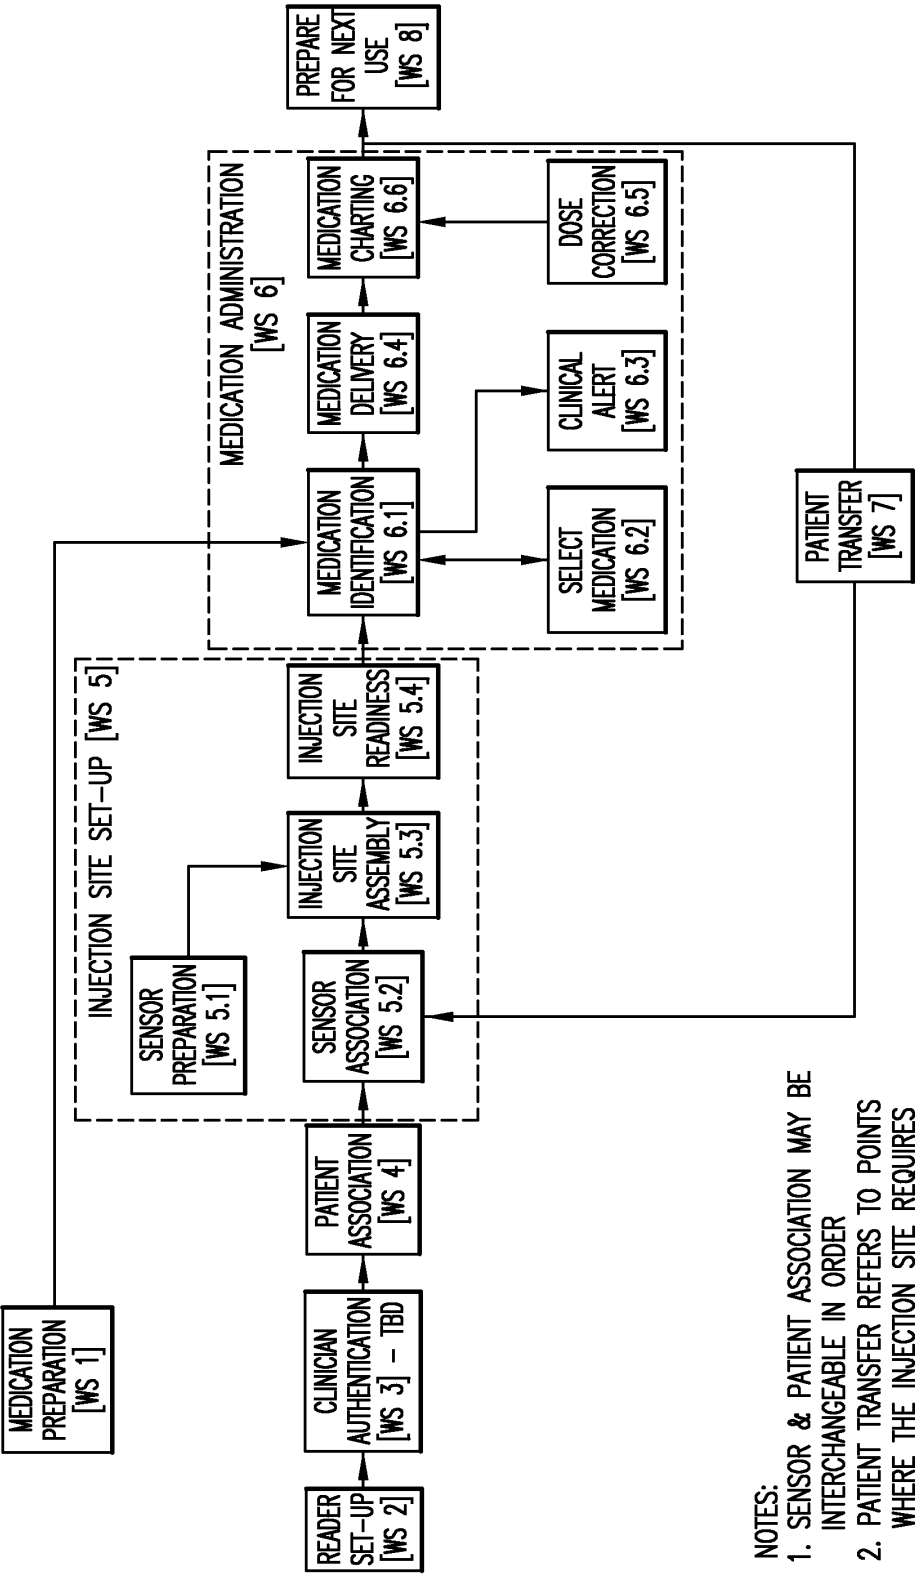

- NOTES:
1. SENSOR & PATIENT ASSOCIATION MAY BE INTERCHANGEABLE IN ORDER
 2. PATIENT TRANSFER REFERS TO POINTS WHERE THE INJECTION SITE REQUIRES DISSASSEMBLY AFTER ASSOCIATION

FIG.9A

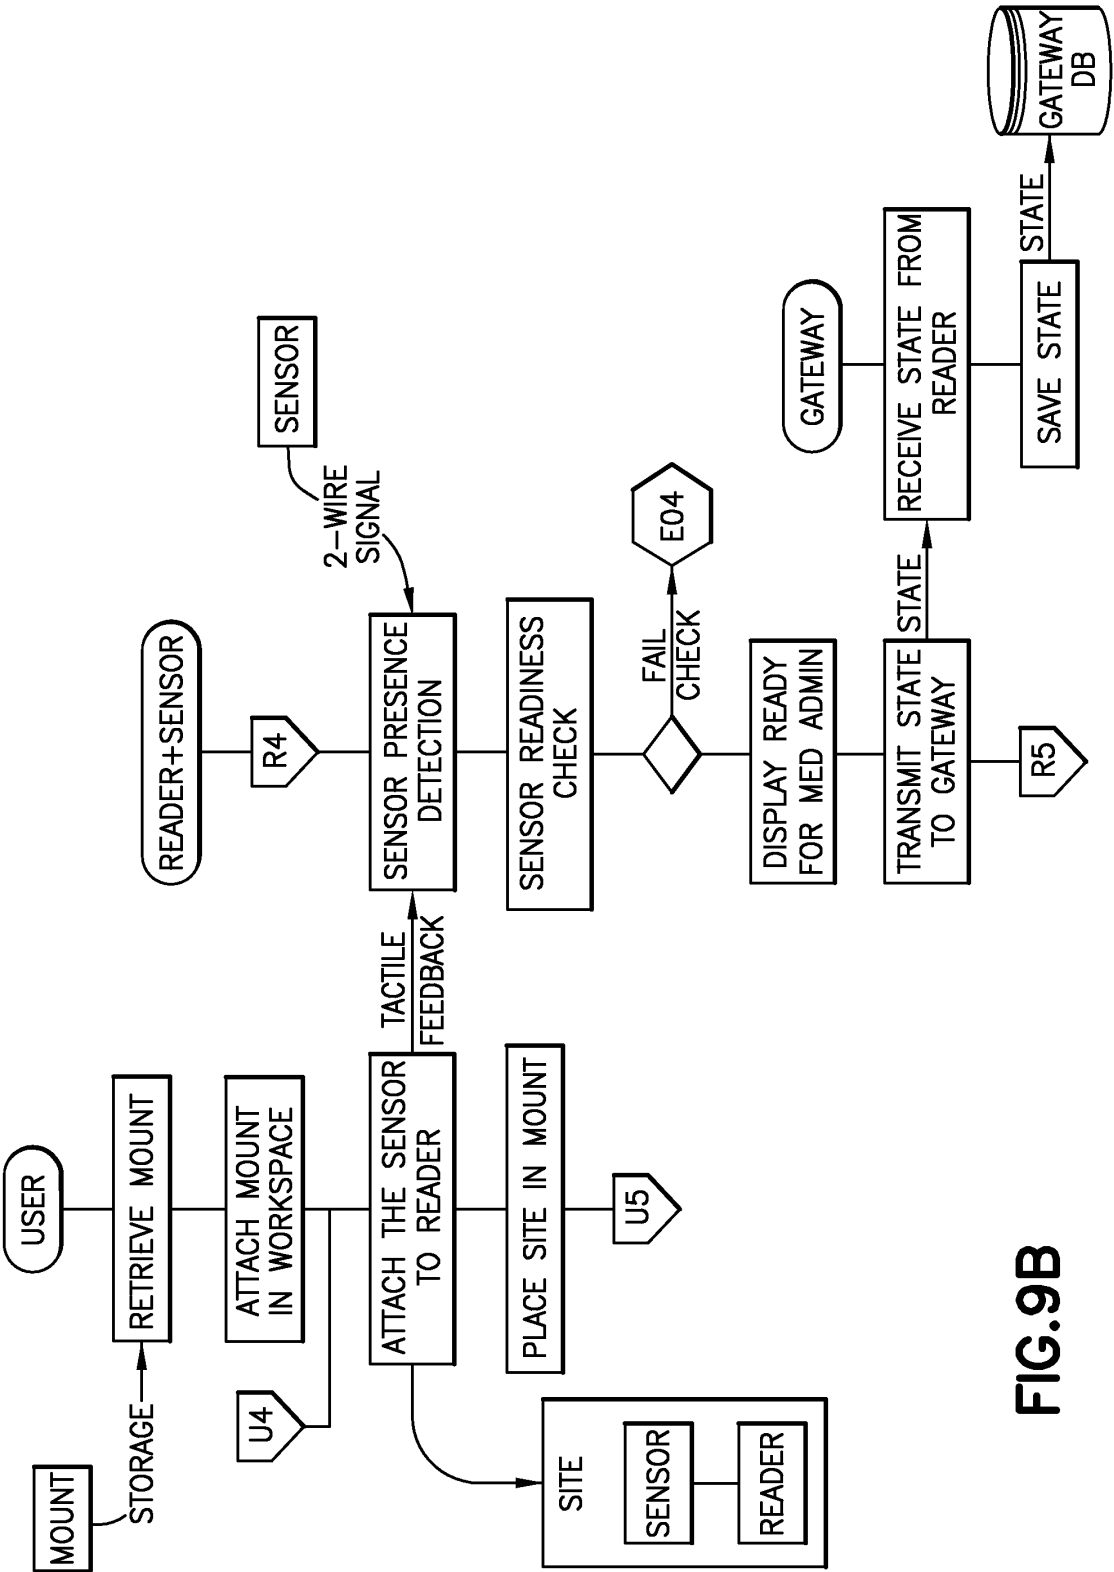
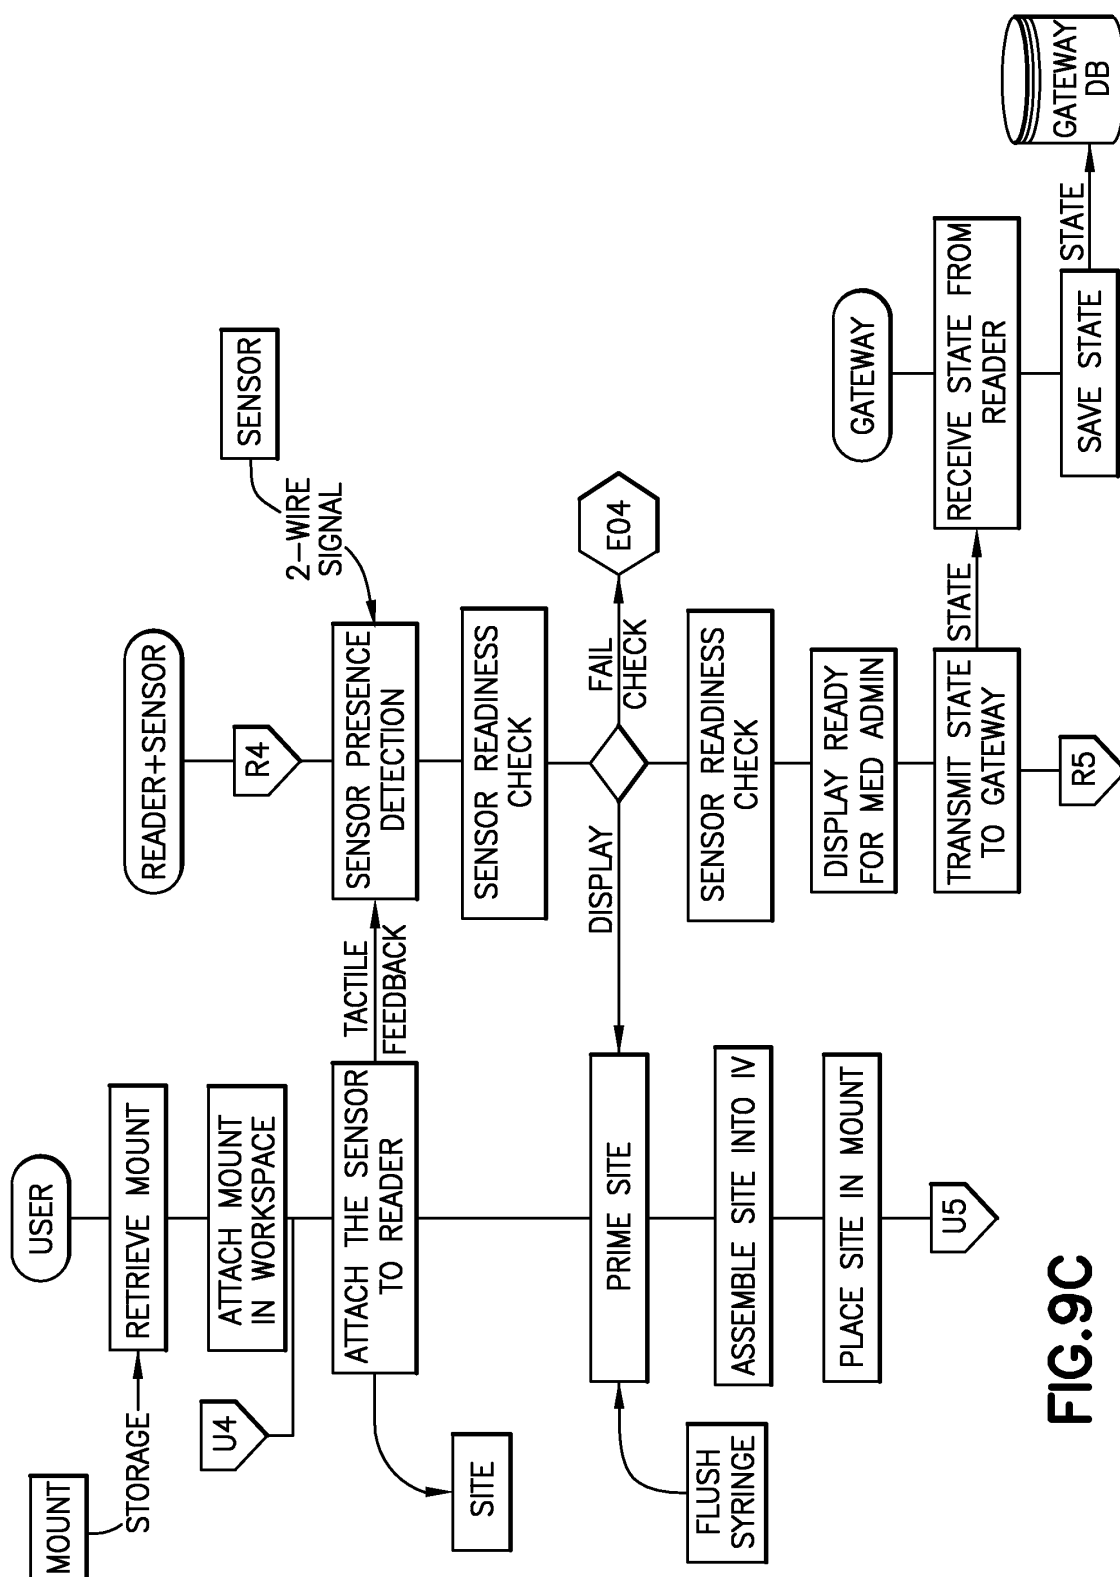


FIG.9B



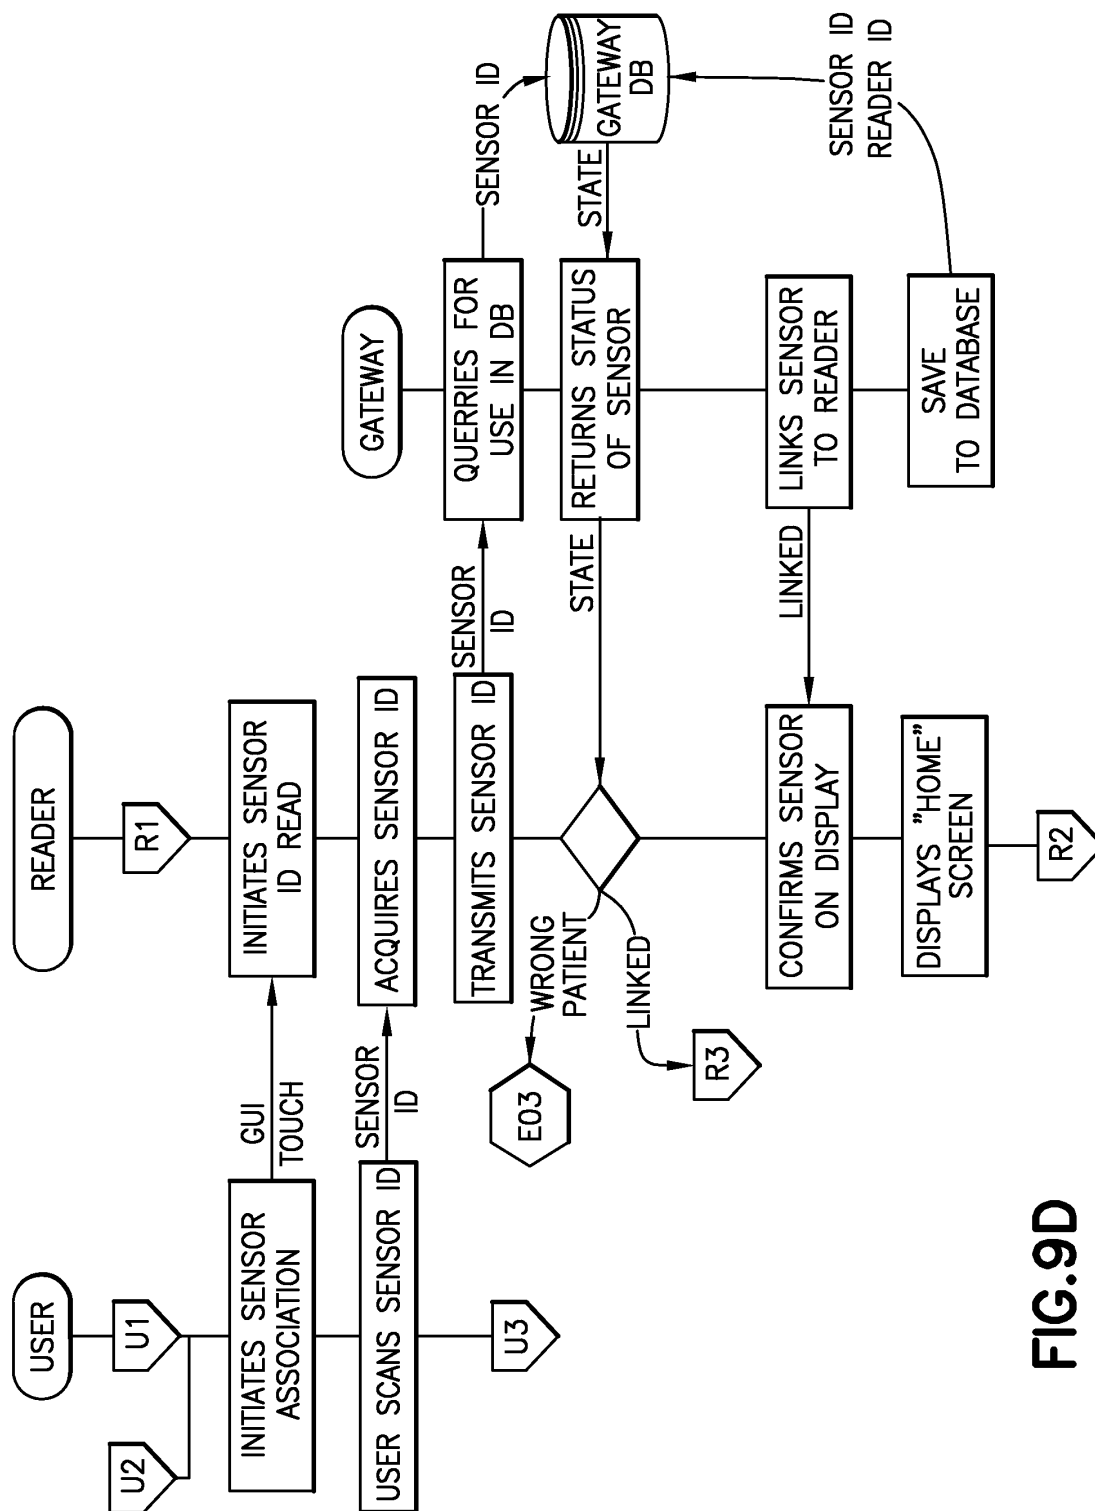


FIG. 9D

