

Figure 1

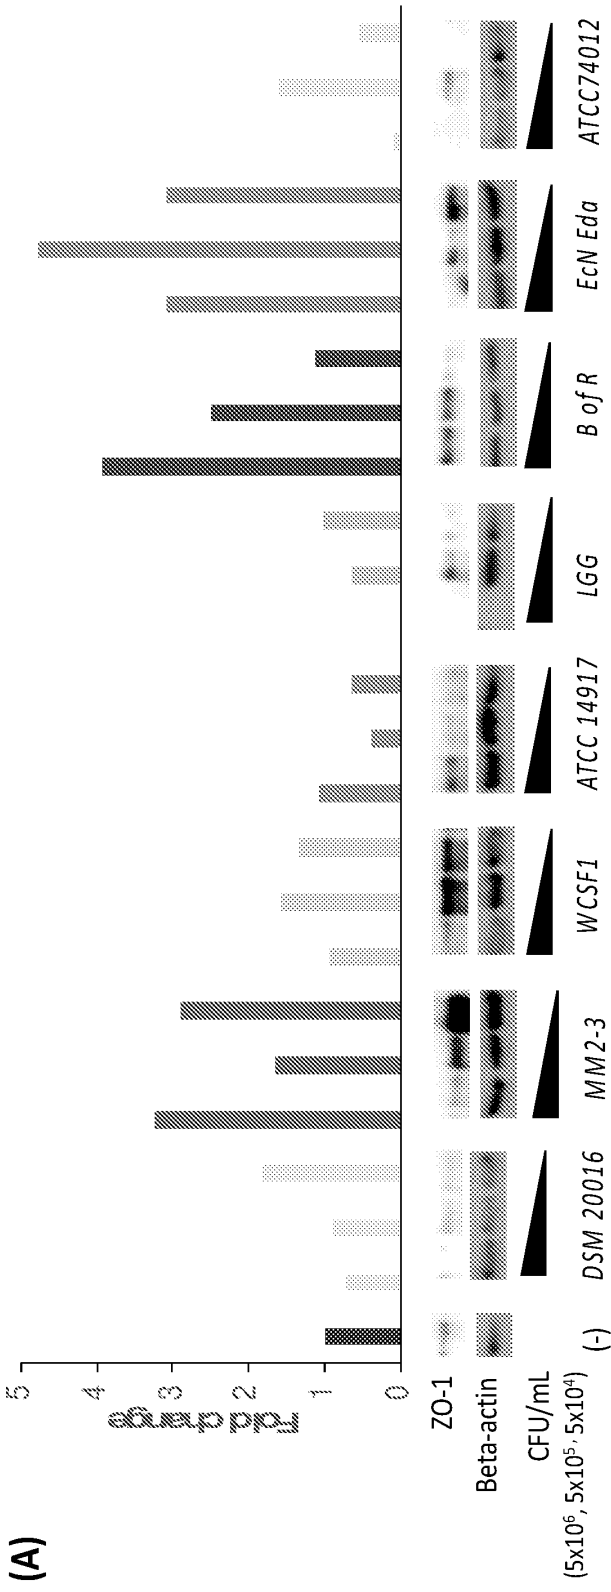


Figure 1 (continued)
(B)

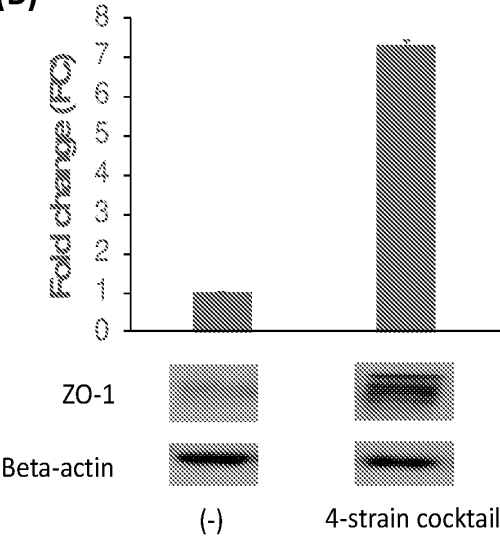


Figure 2



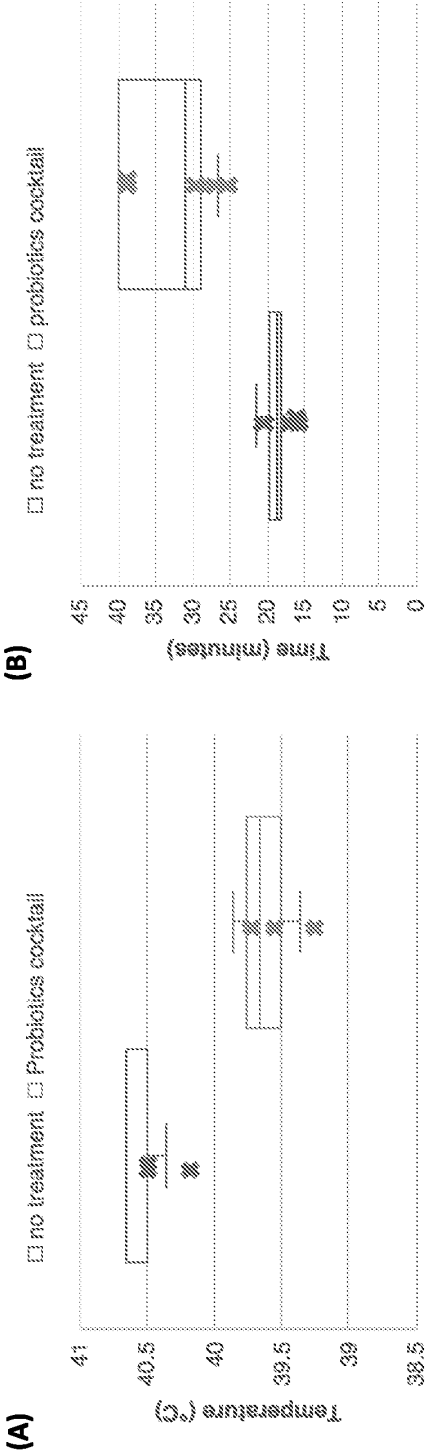


Figure 3

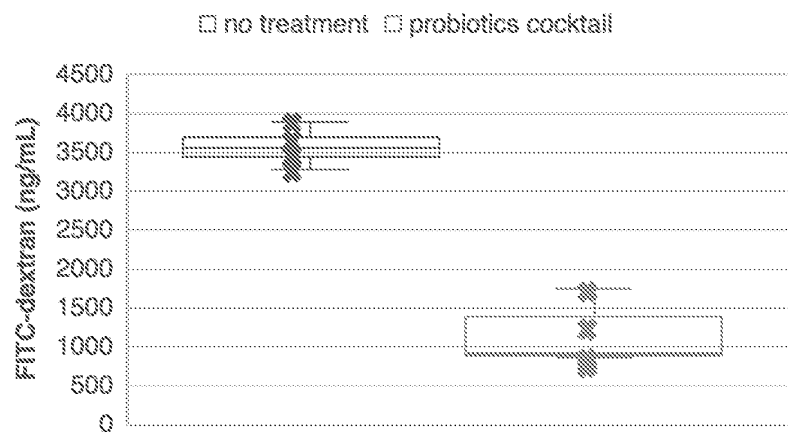

DSS treatment

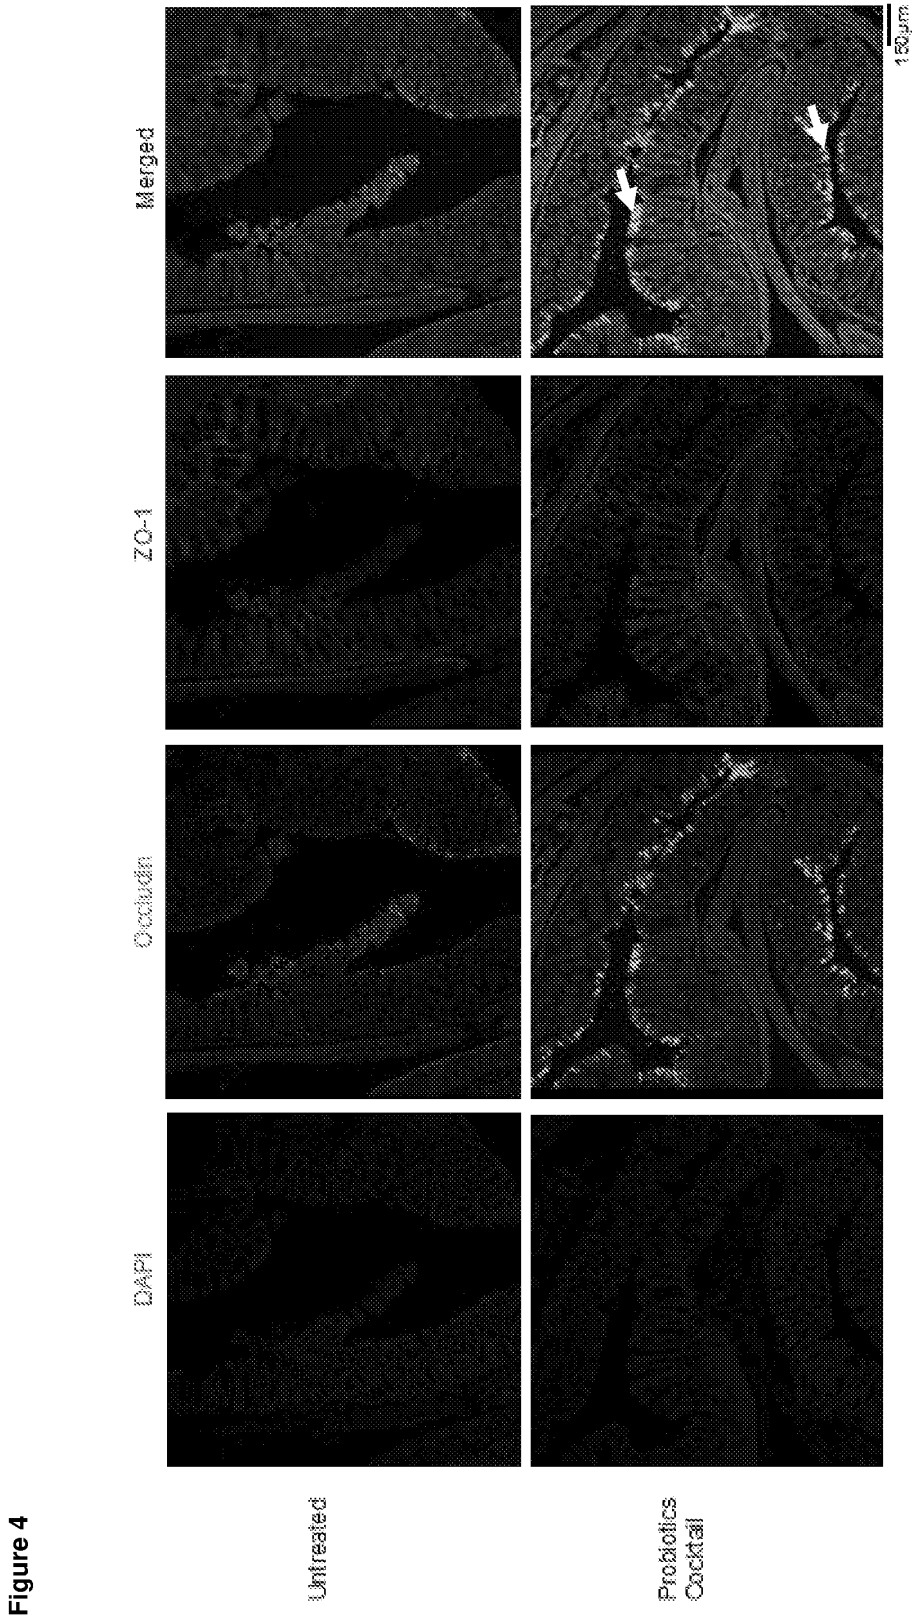

Control



Figure 5

Figure 6

