

1/13

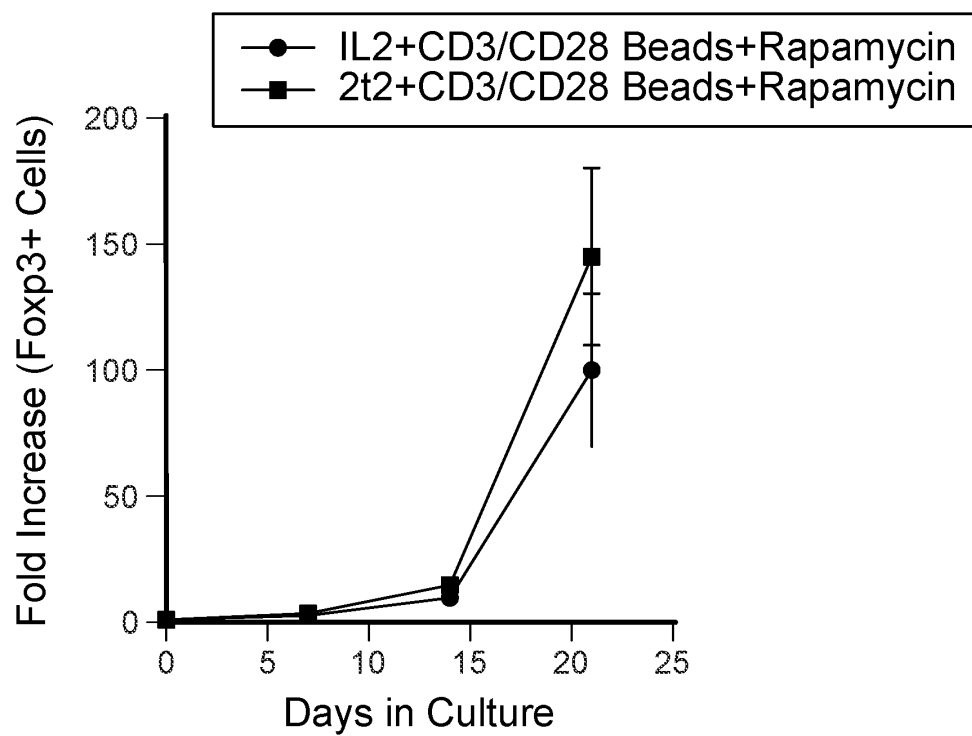

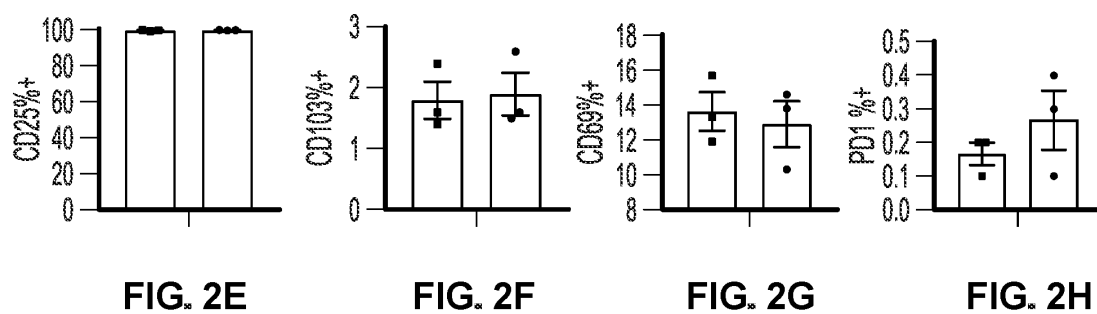
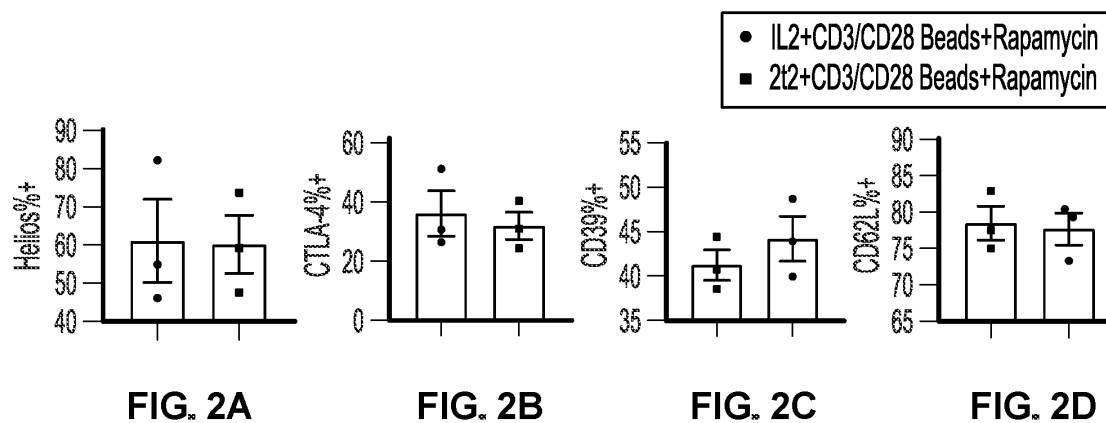


FIG. 1

2/13



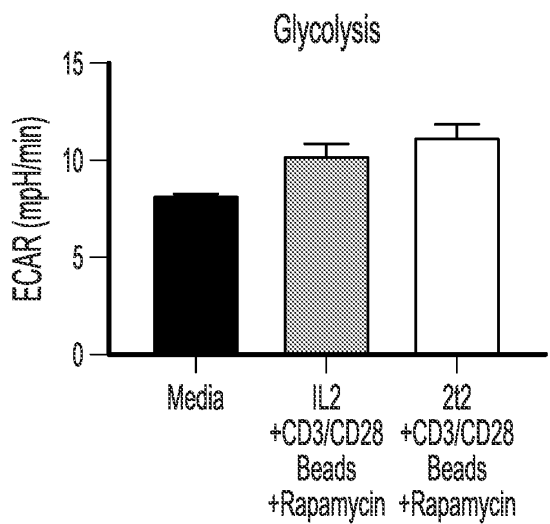


FIG. 3A

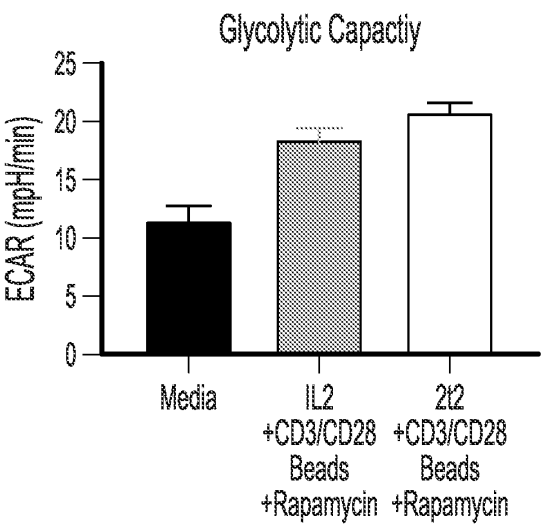


FIG. 3B

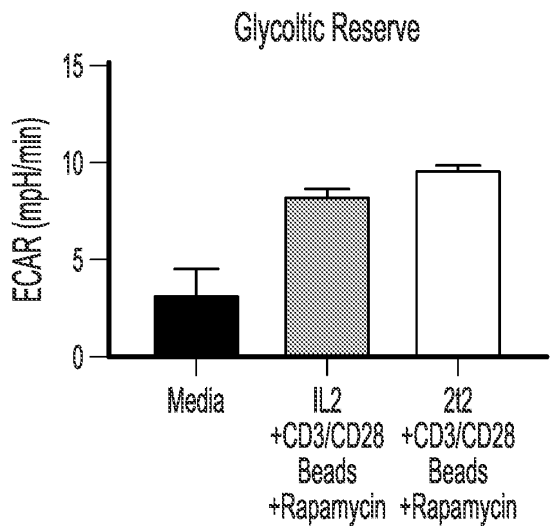


FIG. 3C

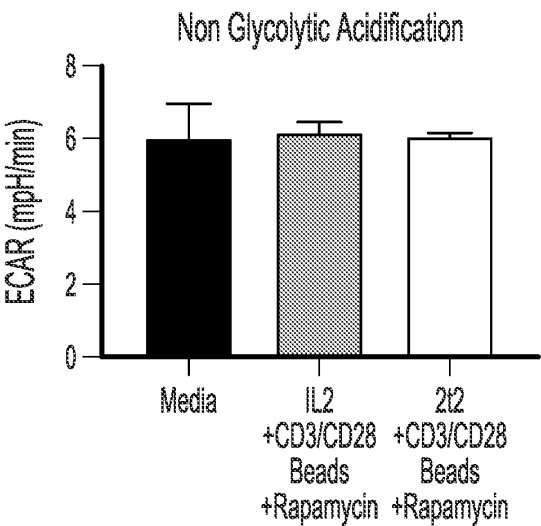


FIG. 3D

4/13

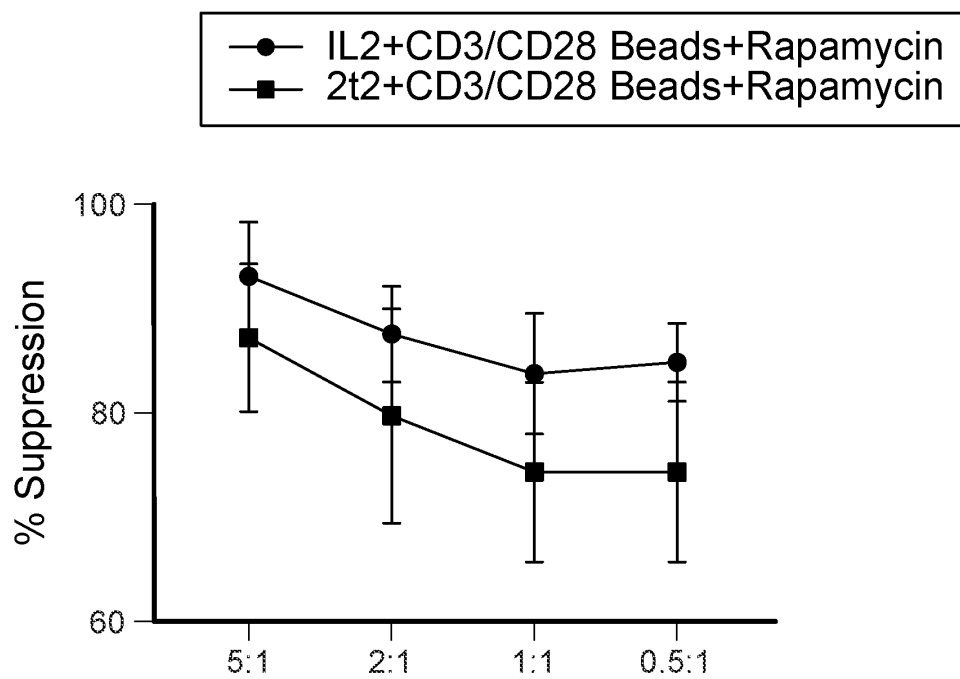


FIG. 4

5/13

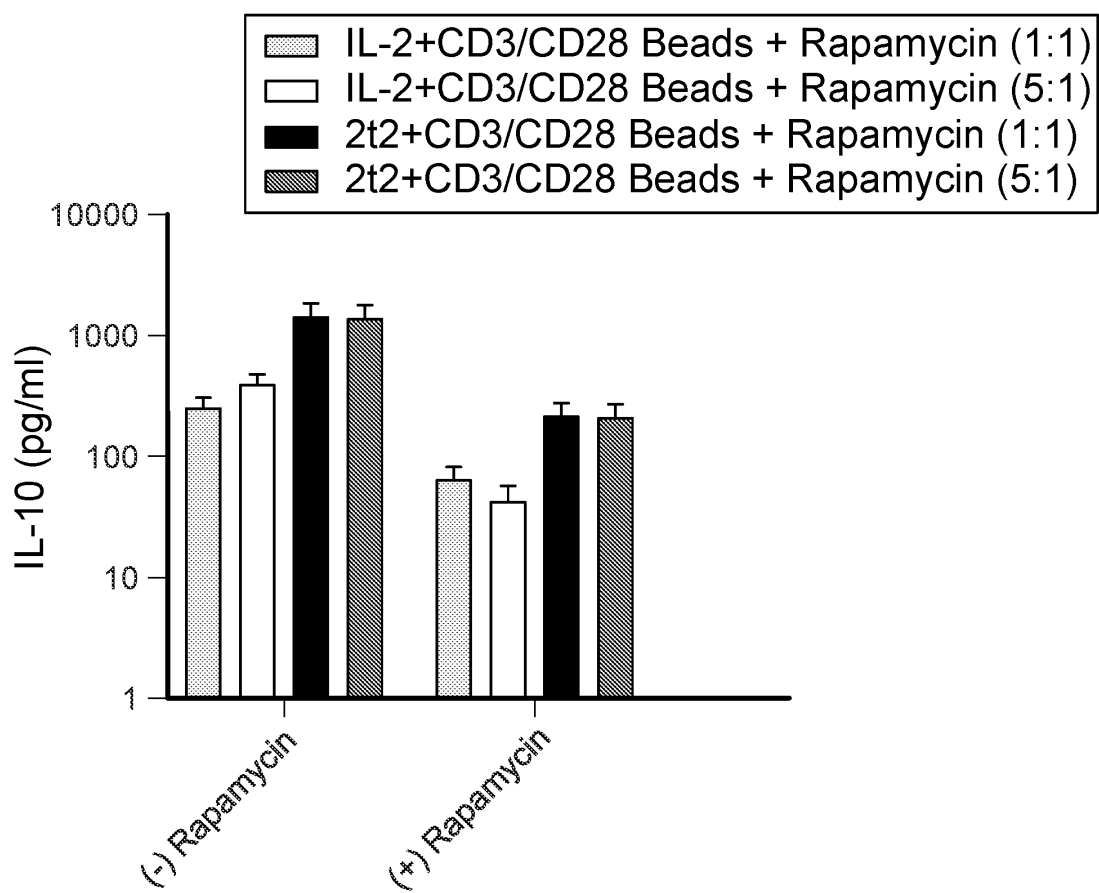


FIG. 5

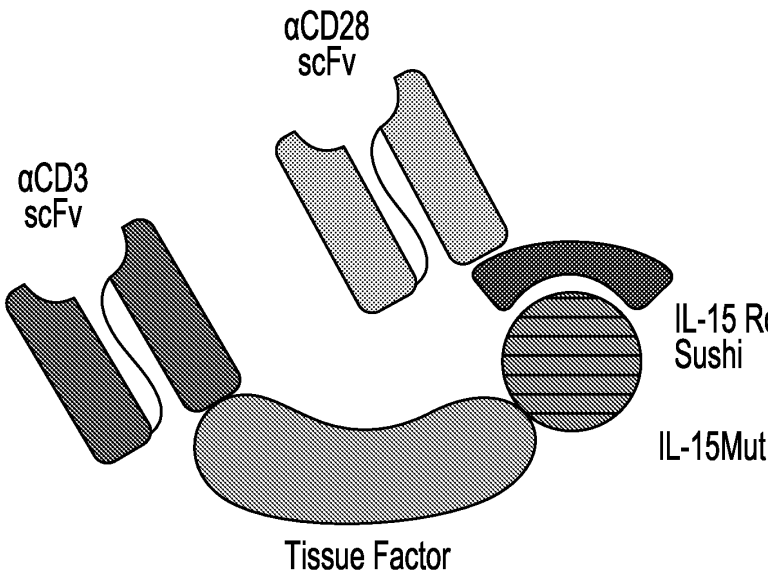


FIG. 6A

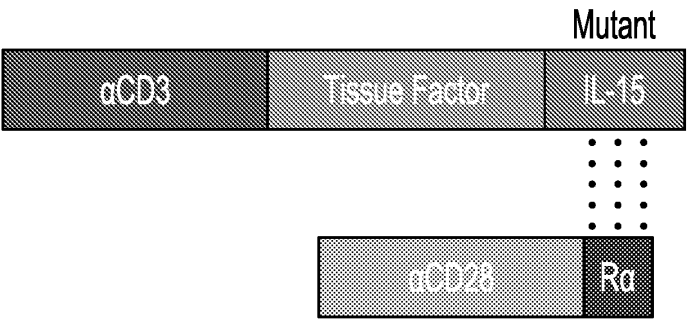


FIG. 6B

7/13


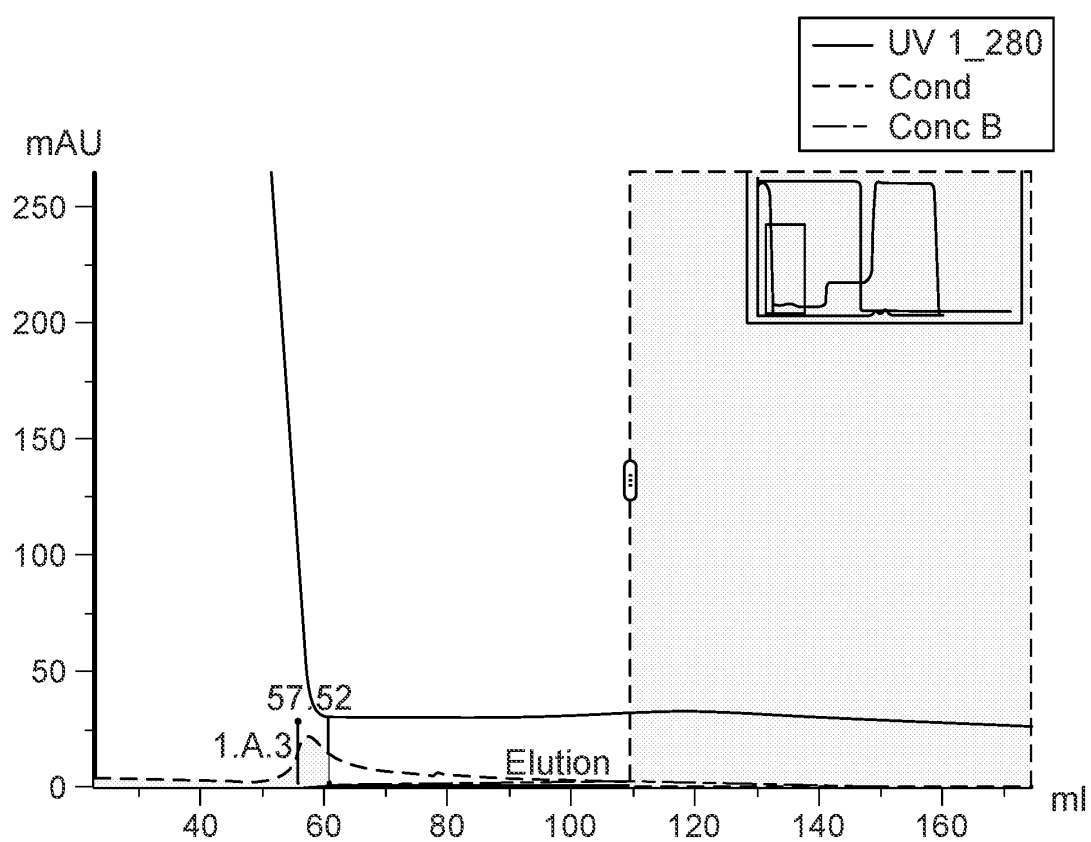


FIG. 7

8/13

Injection Name:	58-77 9213	Run Time (min):	15.00
Vial Number:	RB2	Injection Volume:	50.00
Injection Type:	Unknown	Channel:	UV_VIS_1
Calibration Method:		Wavelength:	280
Instrument Method:	Agilent AdvanceBioSEC 4.6 x 300 with Guard	Bandwidth:	n.a.
Processing Method:	HCW9218 SEC Processing Method	Dilution Factor:	1.0000
Injection Date/Time:	01/Oct/20 19:14	Sample Weight:	1.0000

Chromatogram

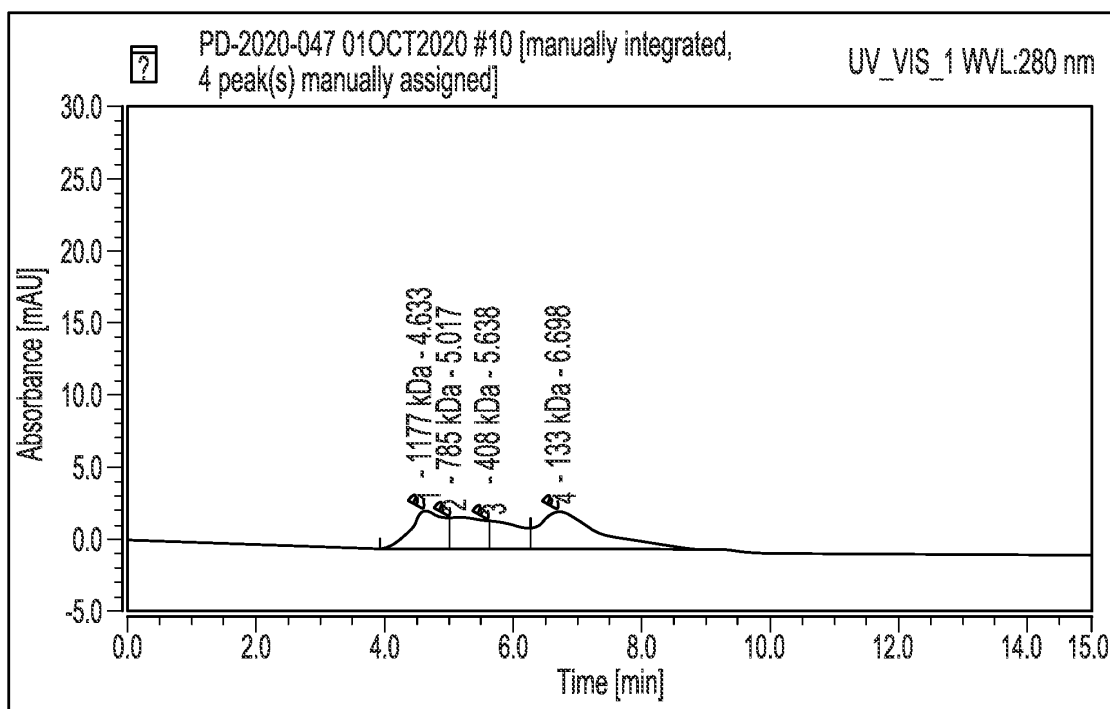

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount n.a.
1	1177 kDa	4.633	1.587	2.681	22.89	28.14	n.a.
2	785 kDa	5.017	1.312	2.201	18.92	23.10	n.a.
3	408 kDa	5.638	1.107	1.985	15.96	20.84	n.a.
4	133 kDa	6.698	2.928	2.661	42.23	27.92	n.a.
Total:			6.934	9.529	100.00	100.00	

FIG. 8

SUBSTITUTE SHEET (RULE 26)

9/13

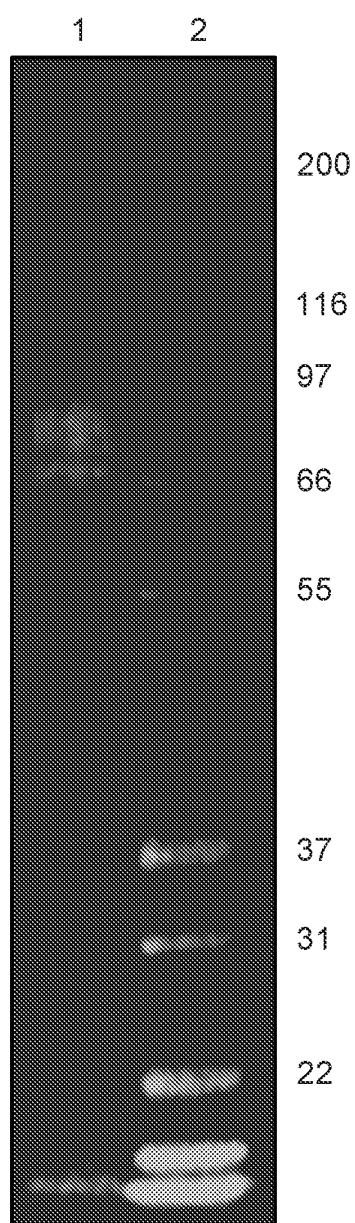


FIG. 9

10/13

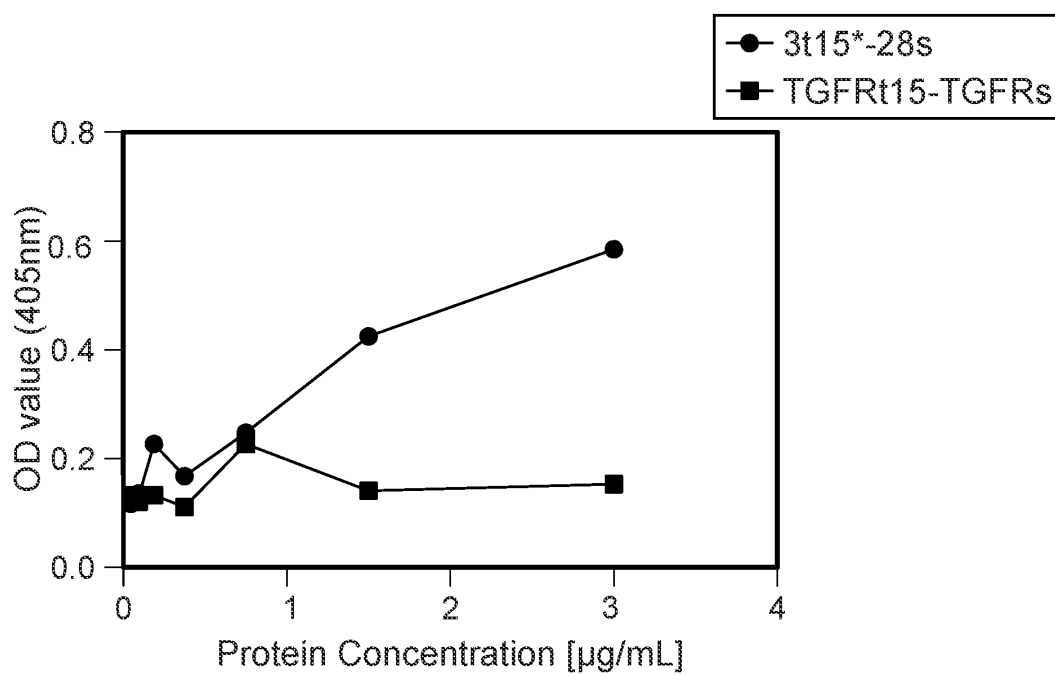


FIG. 10A

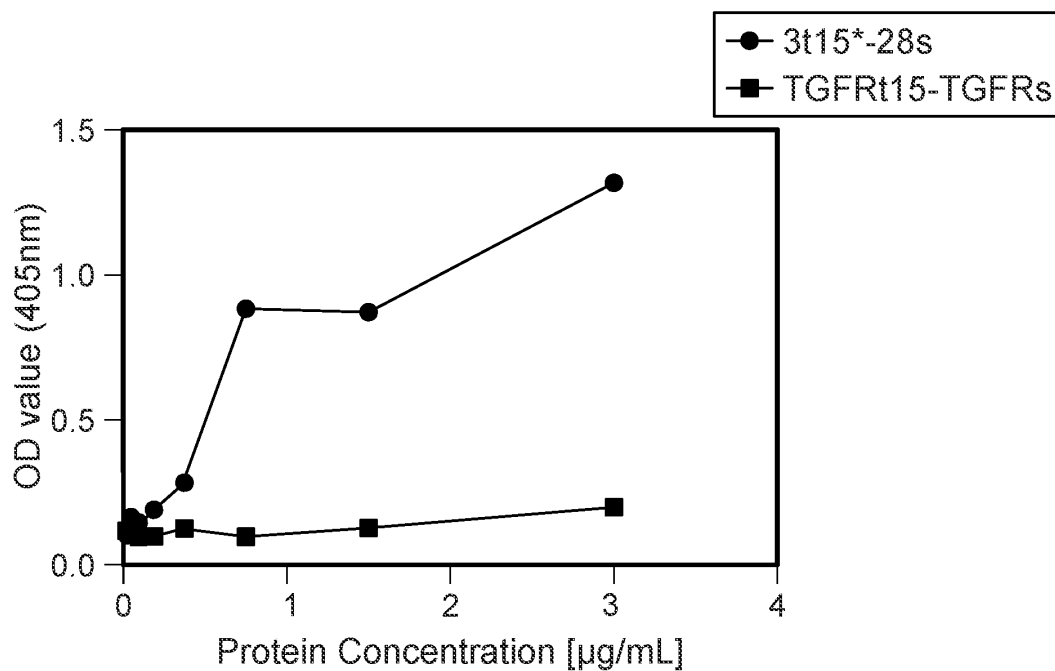


FIG. 10B

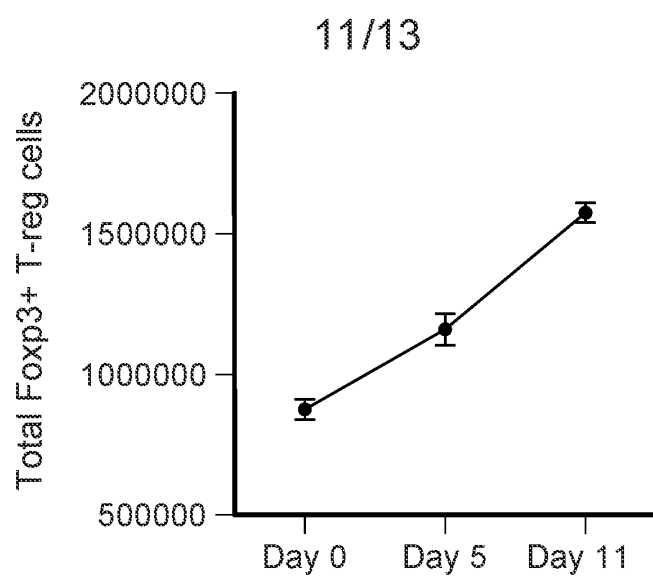


FIG. 11

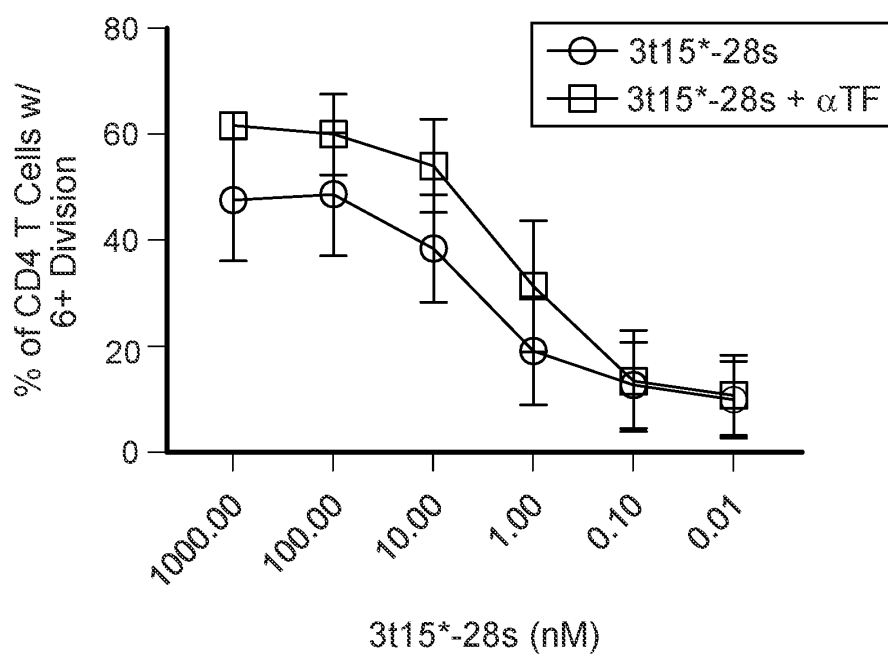


FIG. 12

SUBSTITUTE SHEET (RULE 26)

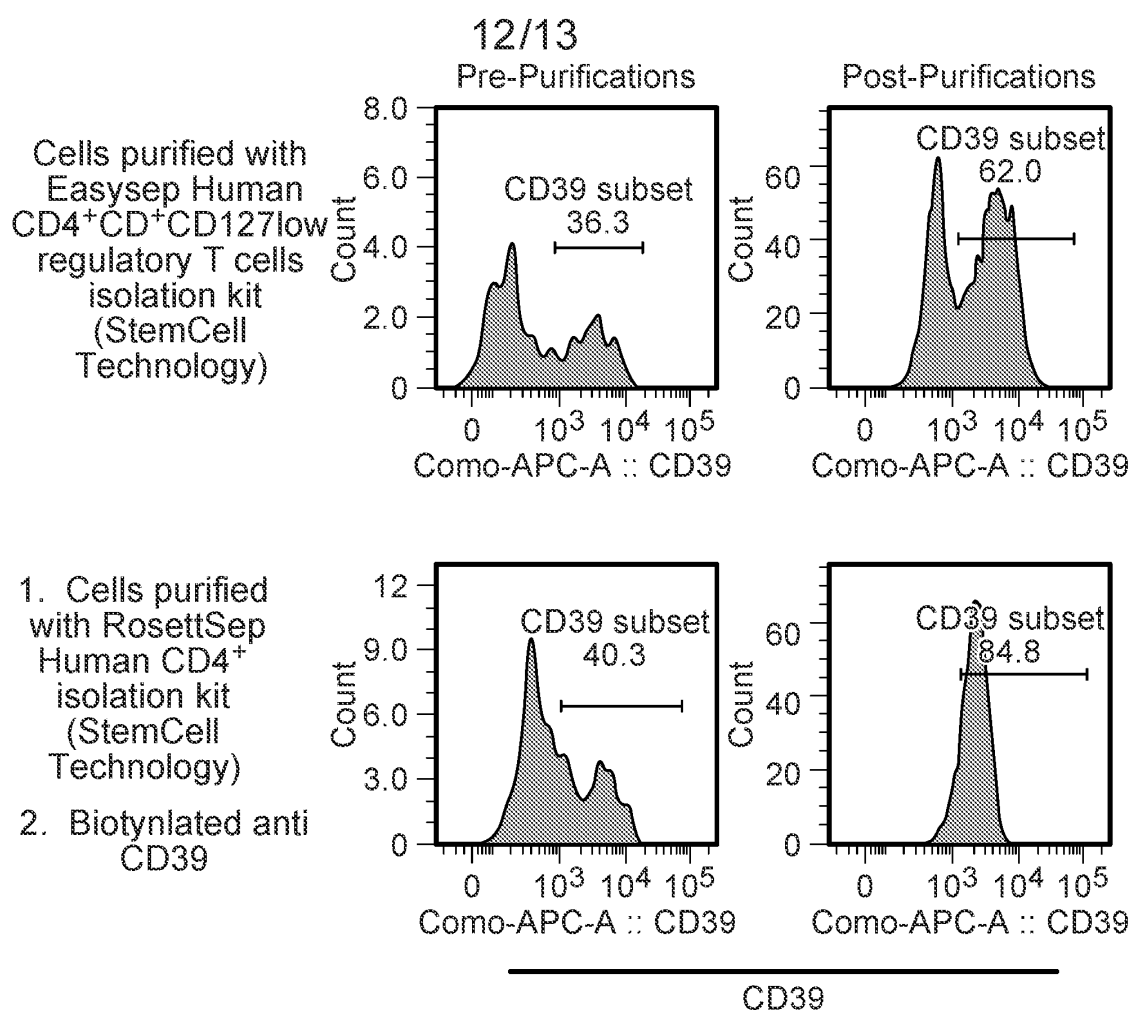


FIG. 13A

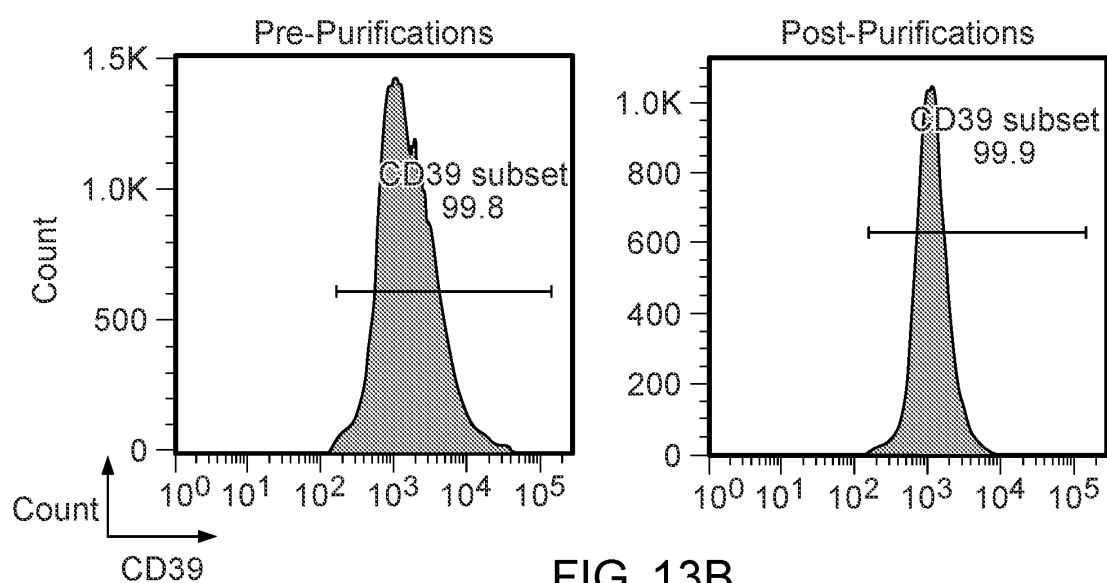


FIG. 13B

13/13

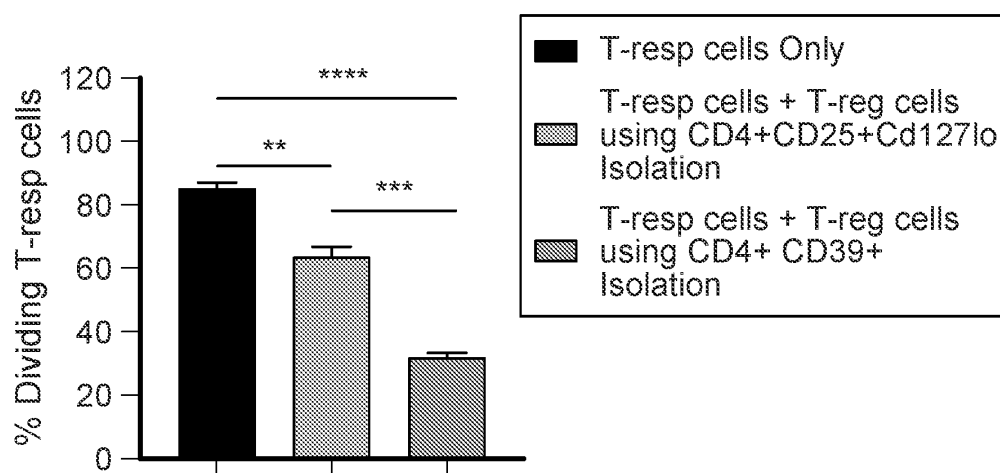


FIG. 14

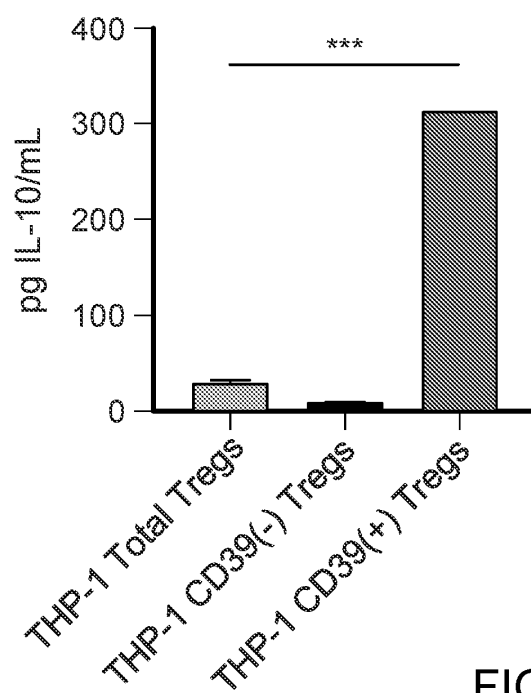


FIG. 15