
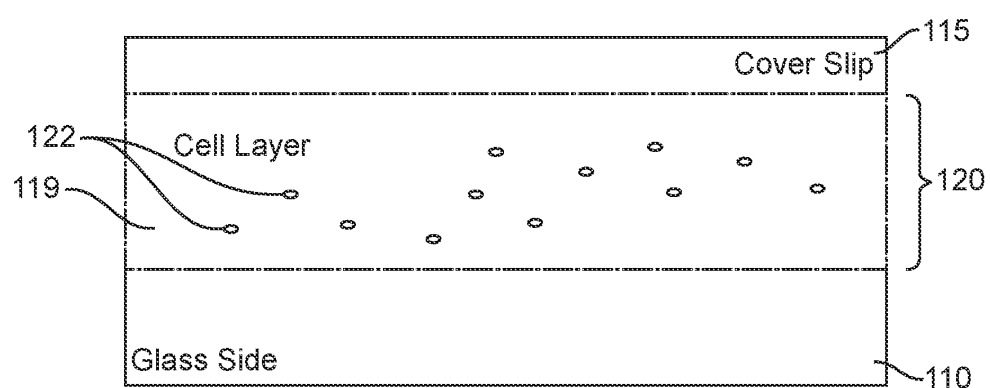


1 / 12

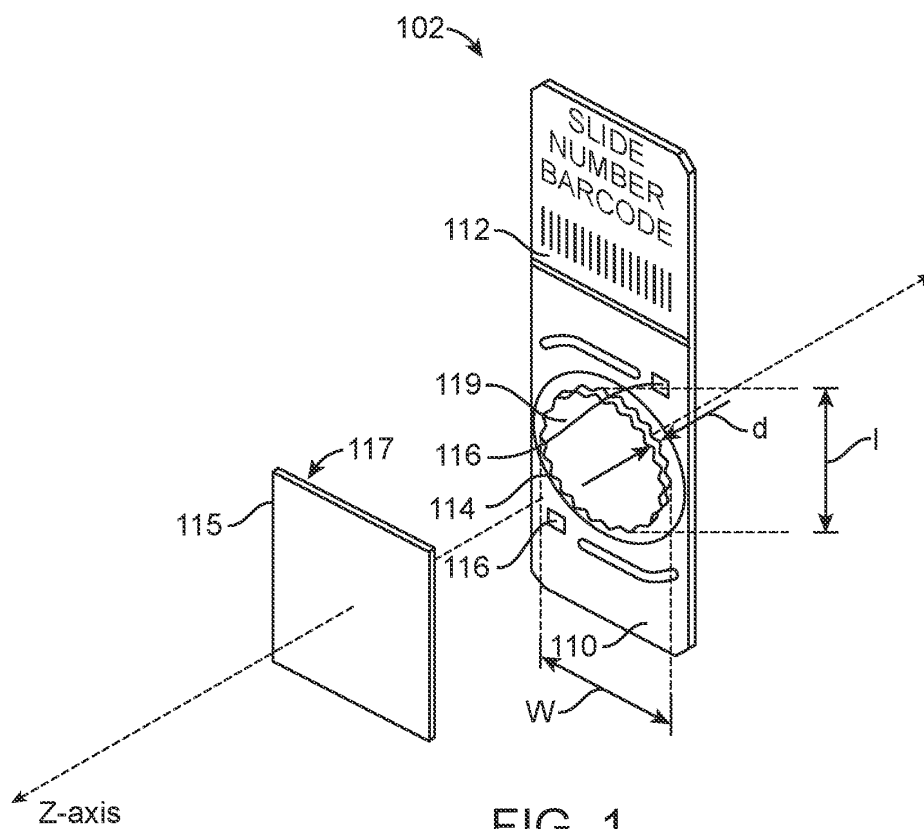

2 / 12

Slide Number (Glass Cover Slip)	ΔZ Focus Depth (in μ)
1	8.4
2	11.3
3	11
4	13.7
5	9
6	8.8
7	13.2
8	11.85
9	12.6
MEAN $\pm$ STD	11.09 $\pm$ 1.969

Slide Number (Plastic Cover Slip)	ΔZ Focus Depth (in μ)
1	11.8
2	22
3	14.38
4	24.2
5	15
6	22.86
7	47
8	28
9	15.7
10	27
11	24.48
12	23.68
13	19.9
14	29.6
MEAN $\pm$ STD	23.6 $\pm$ 8.96

FIG. 3

Patient Whole Slide Focus Map

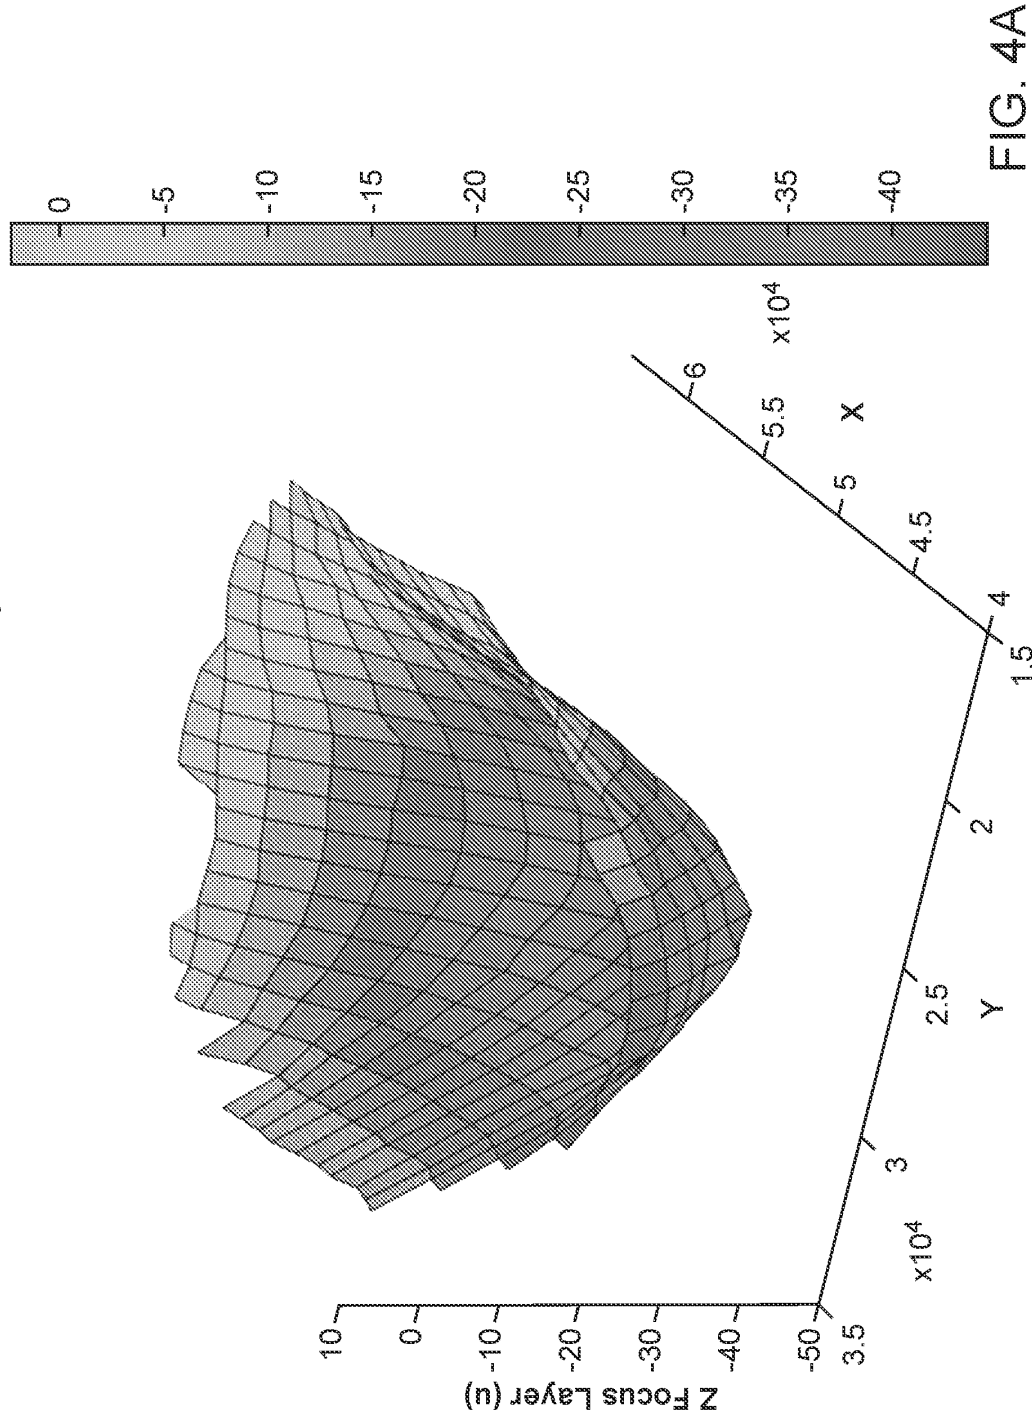


FIG. 4A

4 / 12

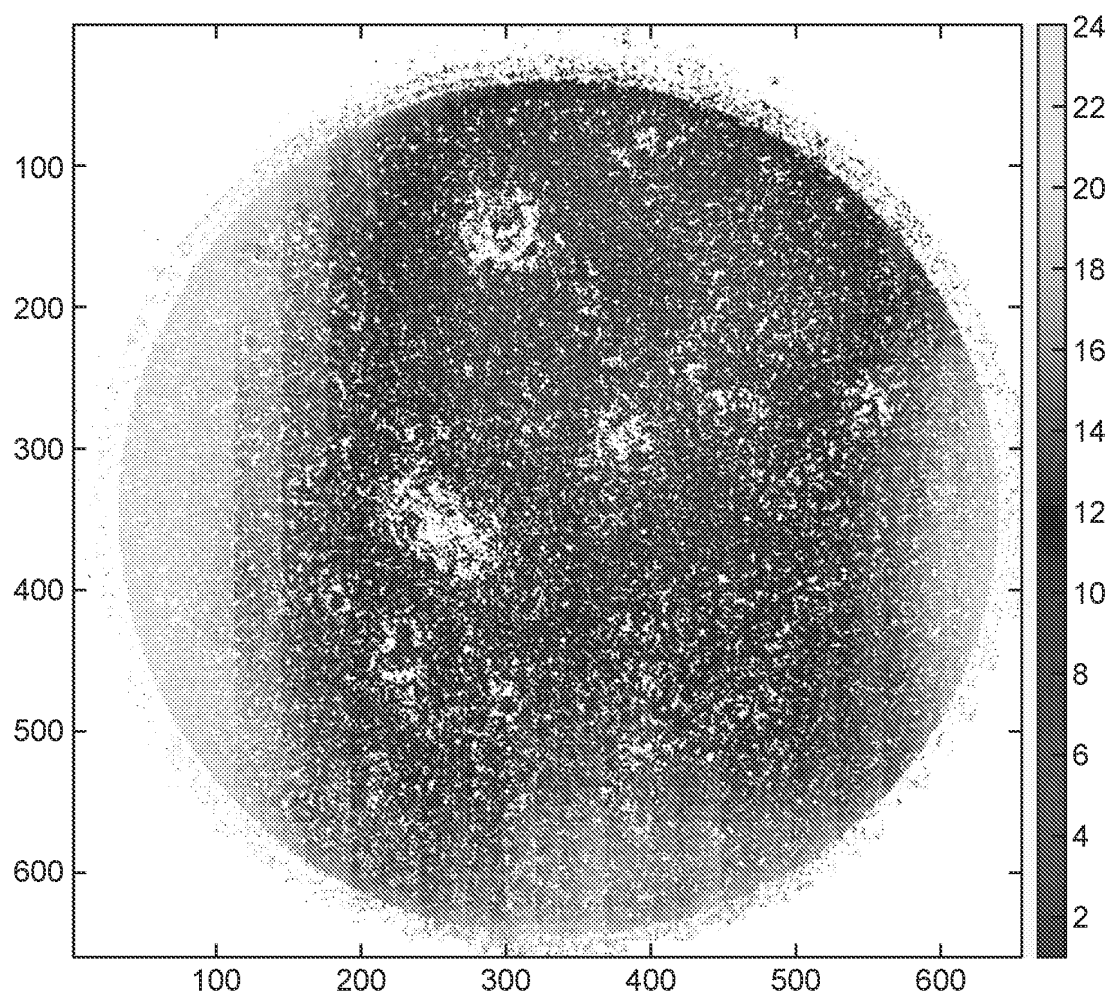


FIG. 4B

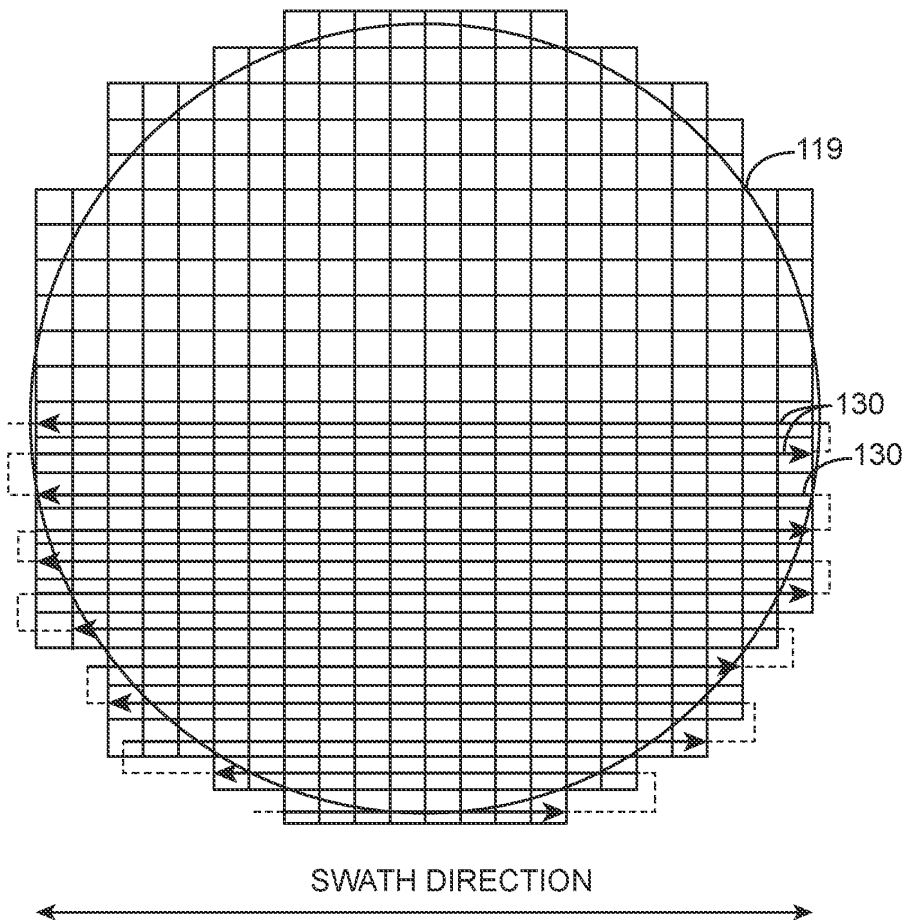


FIG. 5

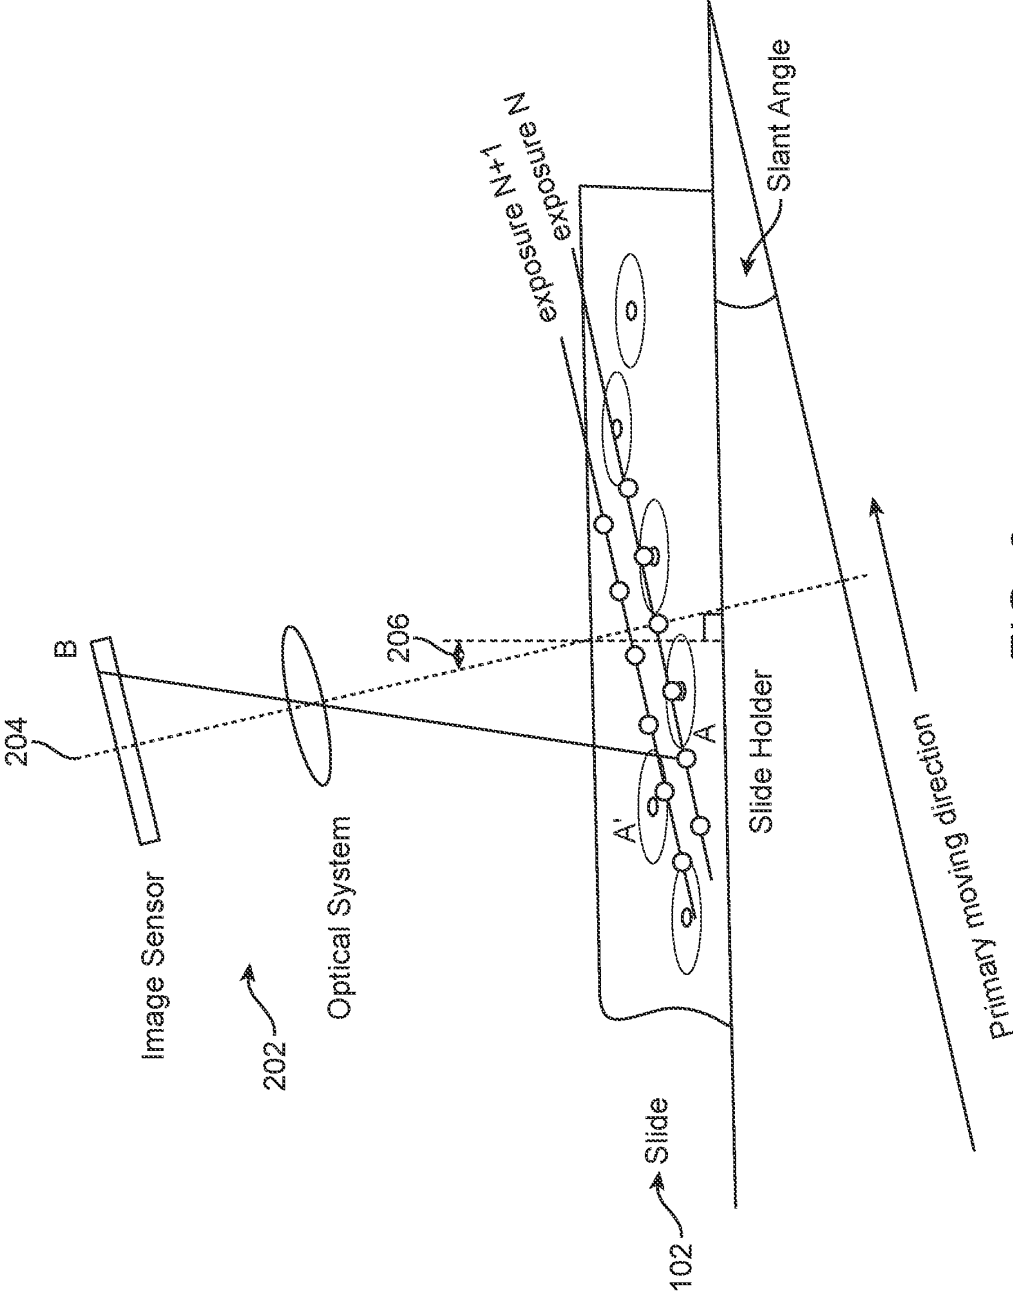


FIG. 6

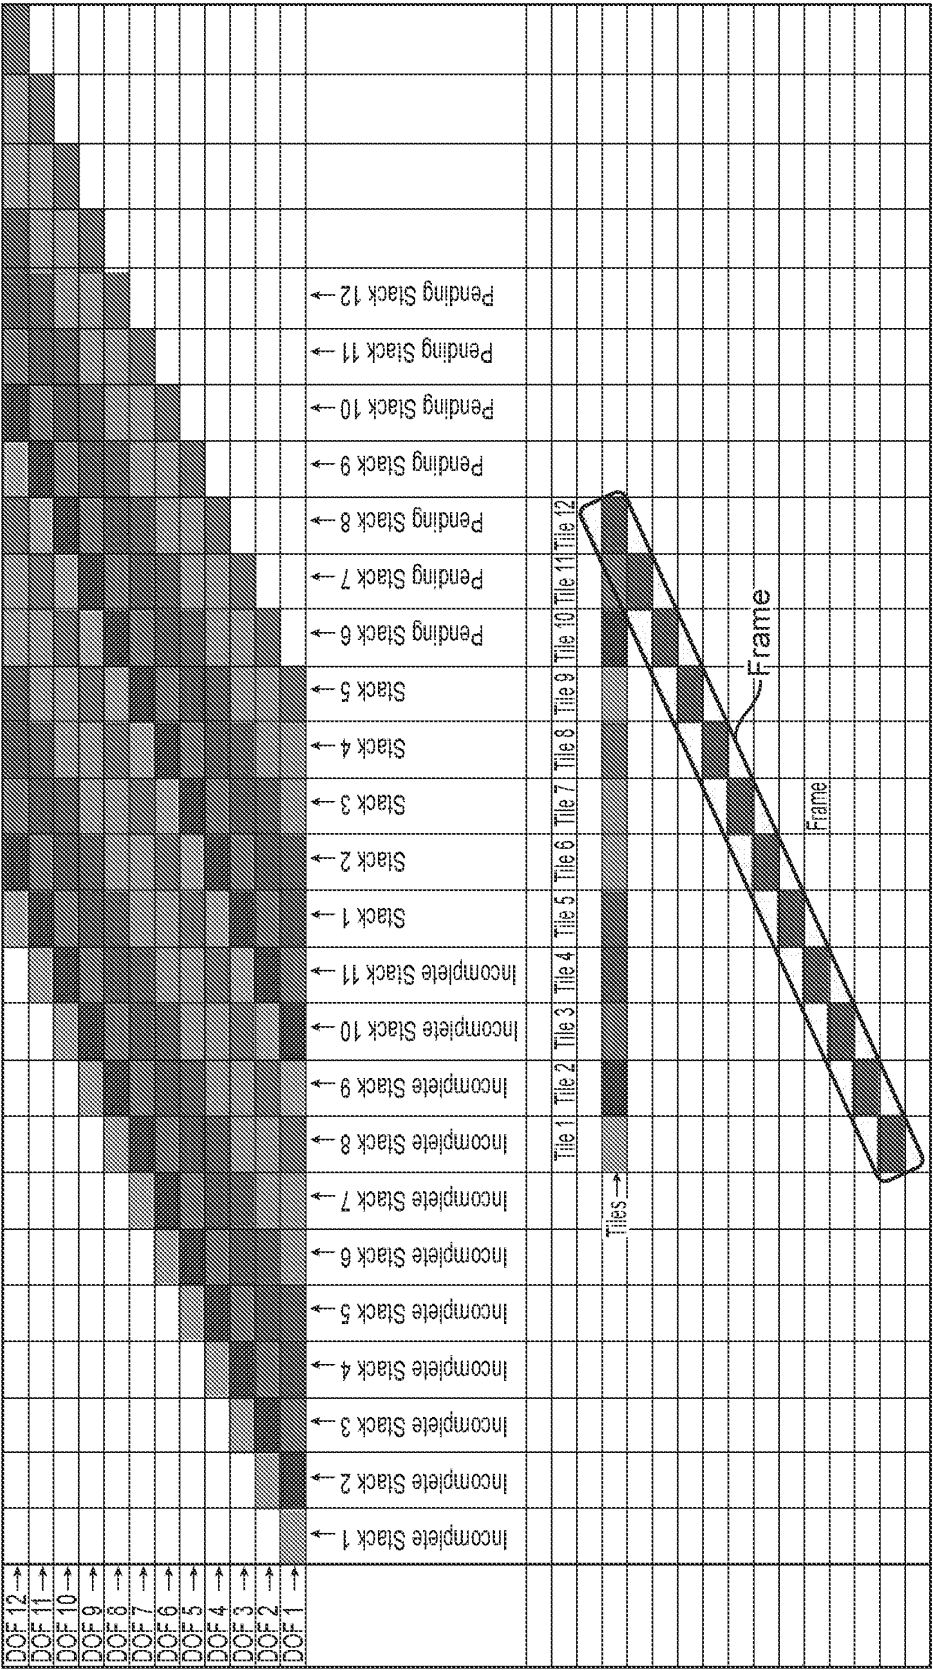


FIG. 7

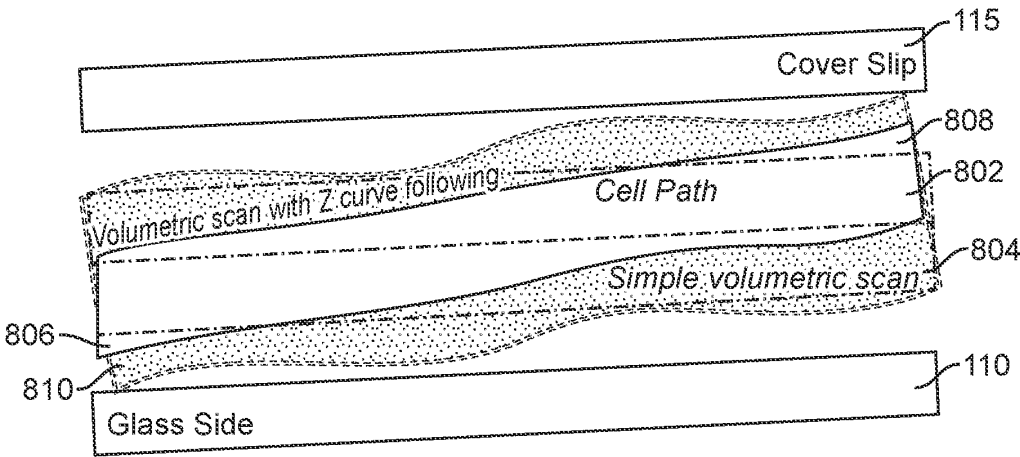


FIG. 8A

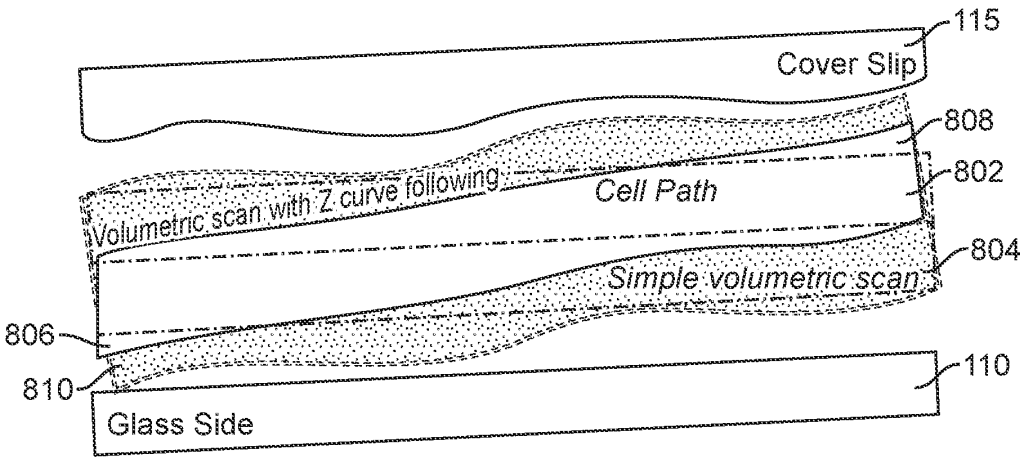


FIG. 8B

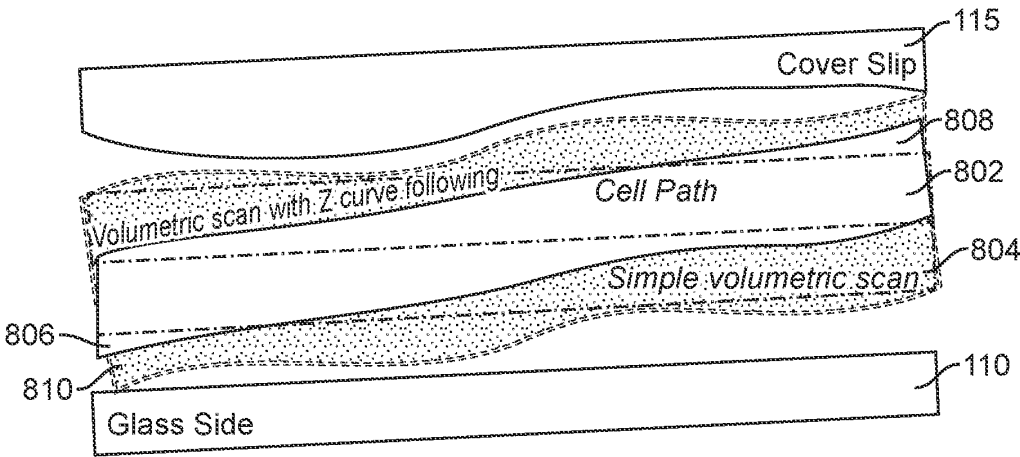


FIG. 8C

11 / 12

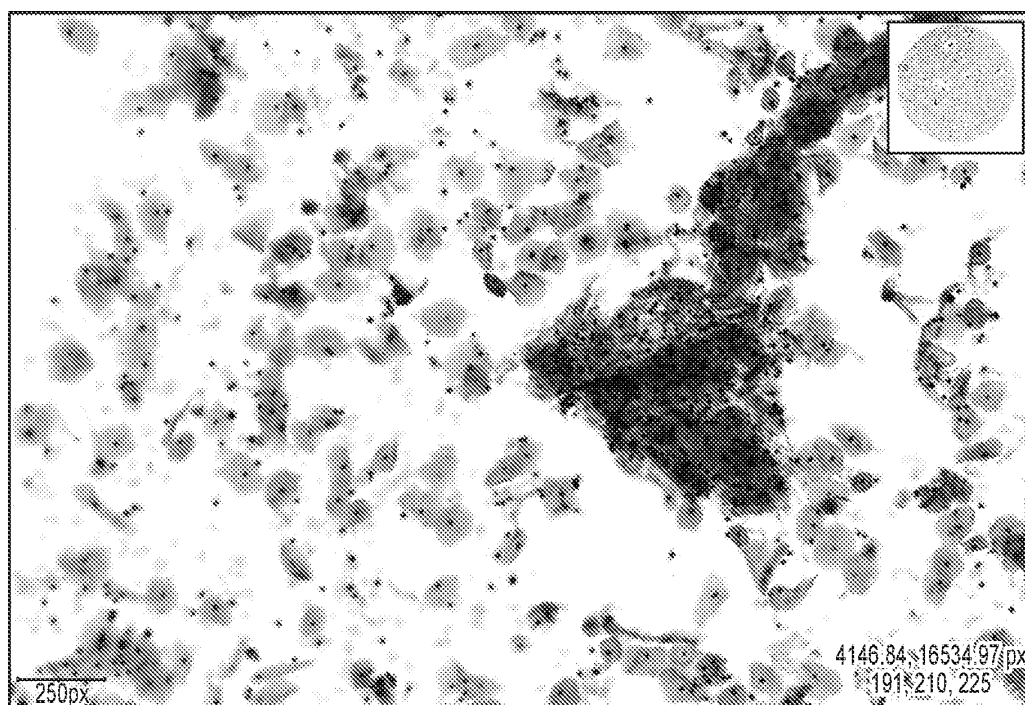


FIG. 9A

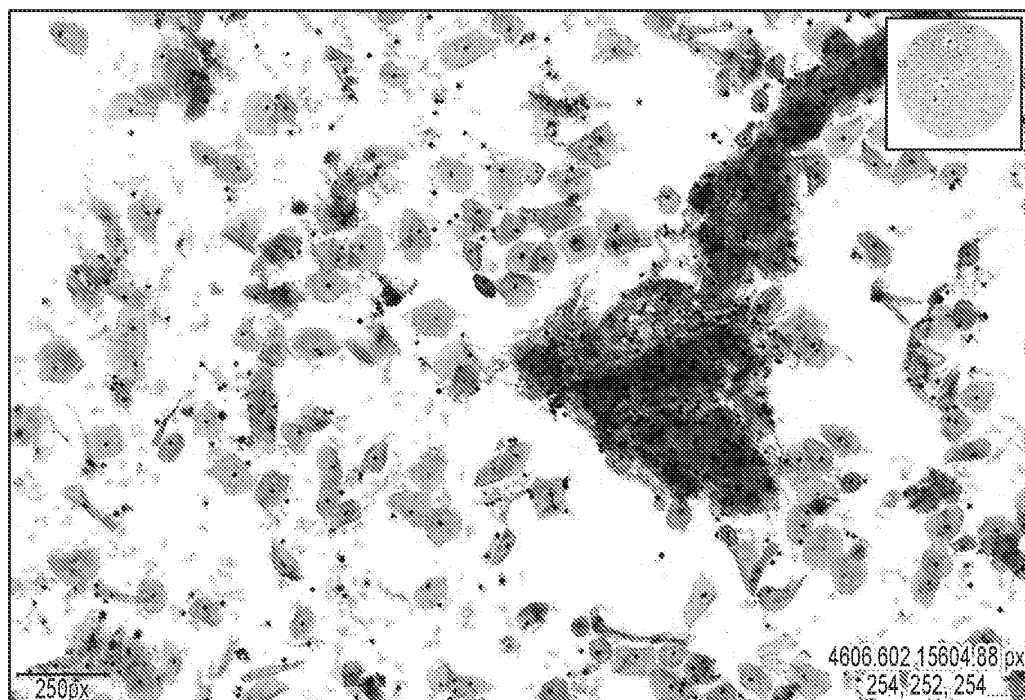


FIG. 9B

12 / 12

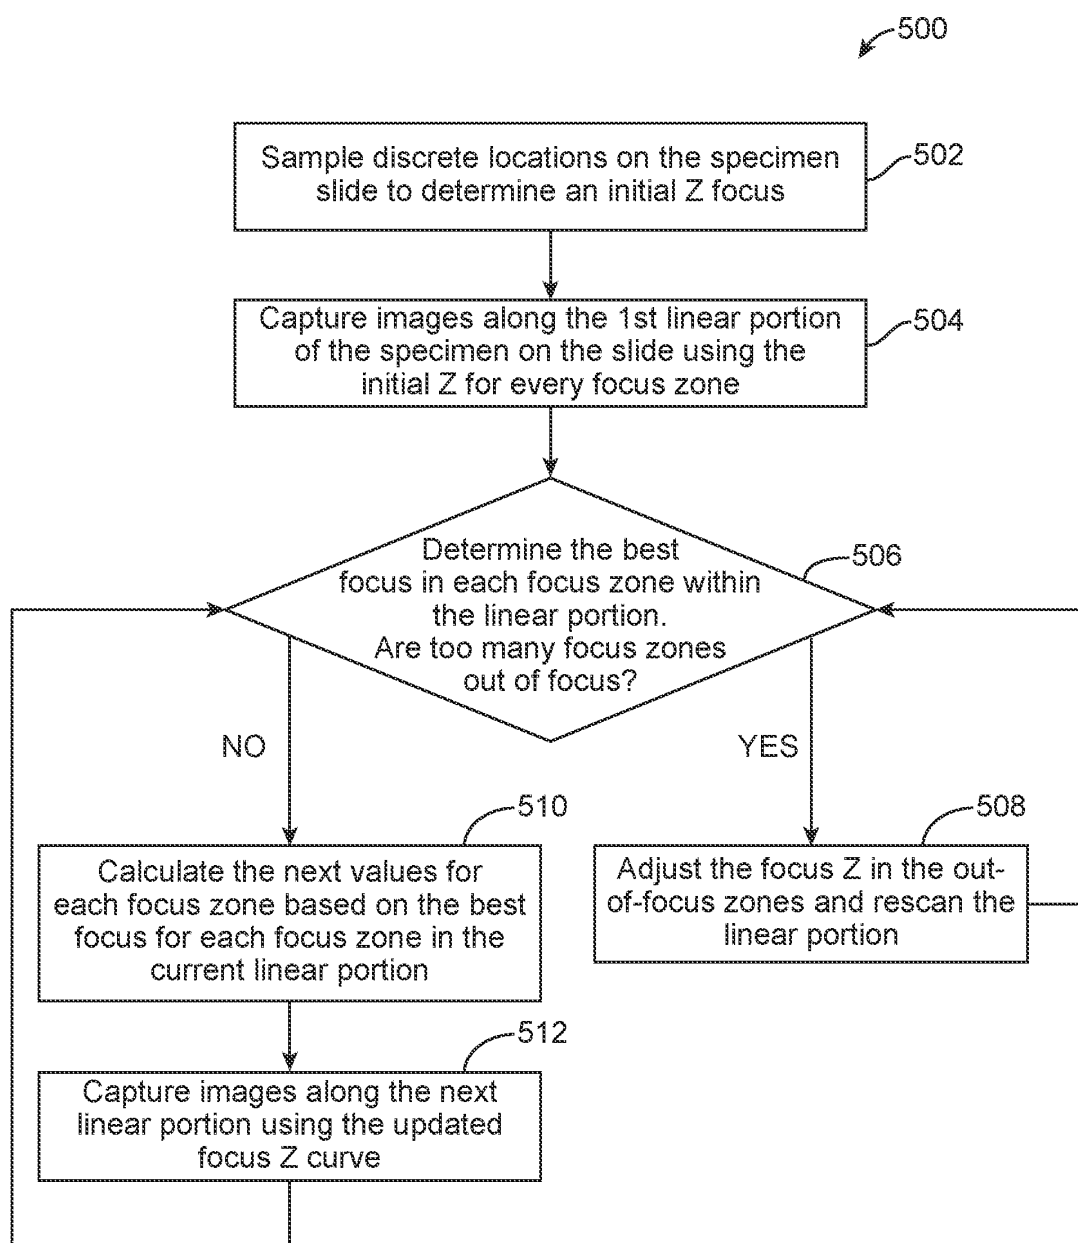


FIG. 10