



[Fig. 1]

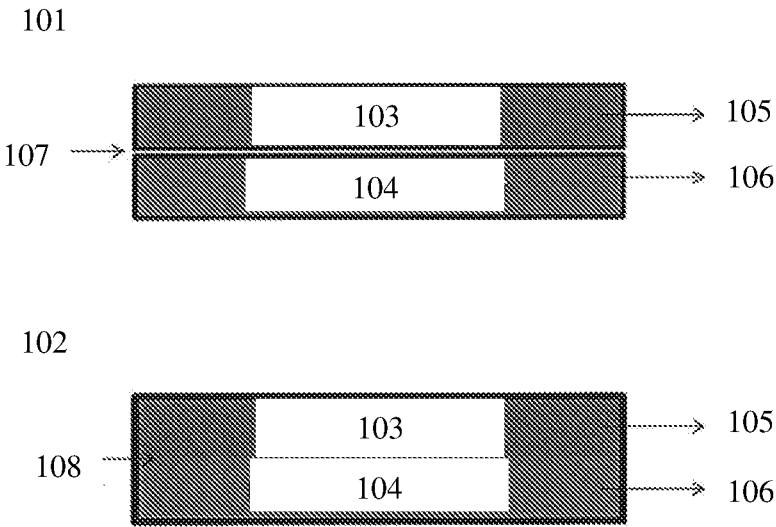

[Fig. 2]

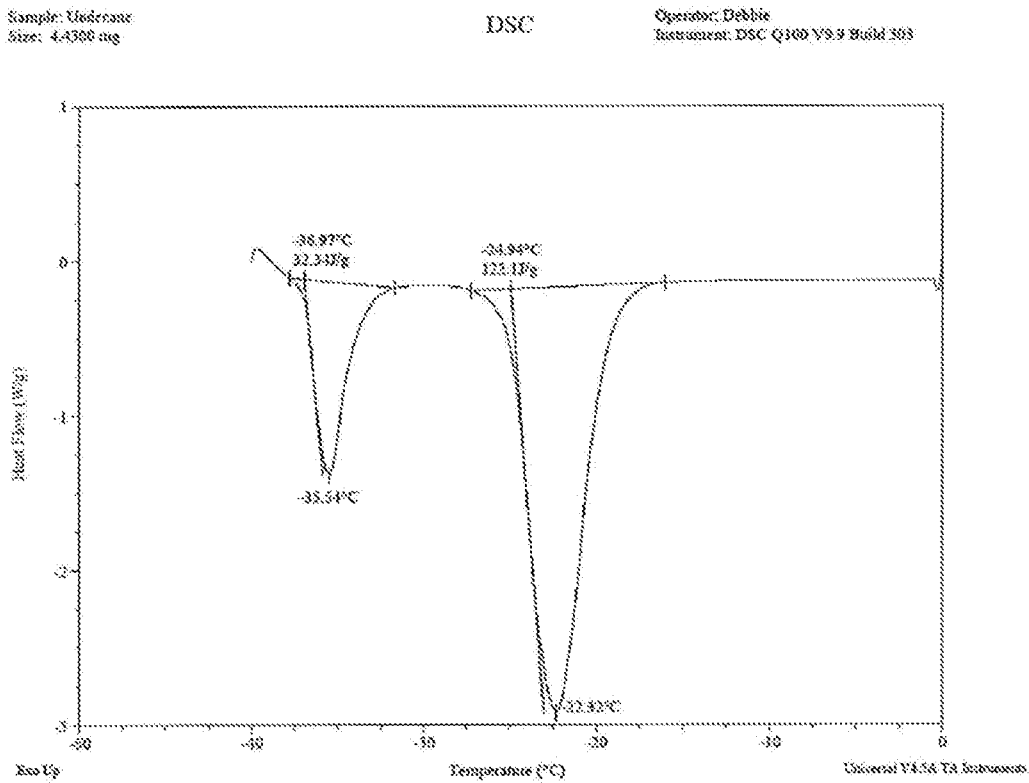


[Fig. 3]

Sample: DSC-1
Size: 4.8290 mg

DSC

Operator: Debbie
Instrument: DSC Q100 V9.9 Build 363

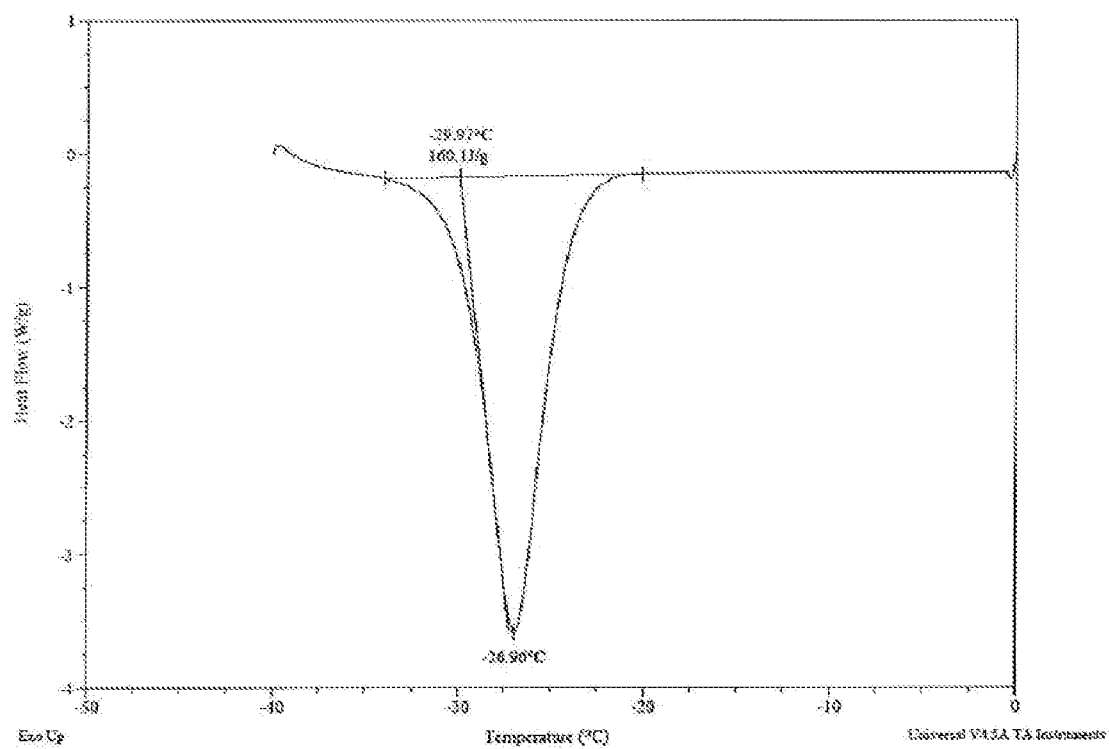


[Fig. 4]


Sample: 26.6% CaCl₂
Size: 4.2900 mg

DSC


Operator: Debbie
Instrument: DSC Q108 V9.9 Build 303

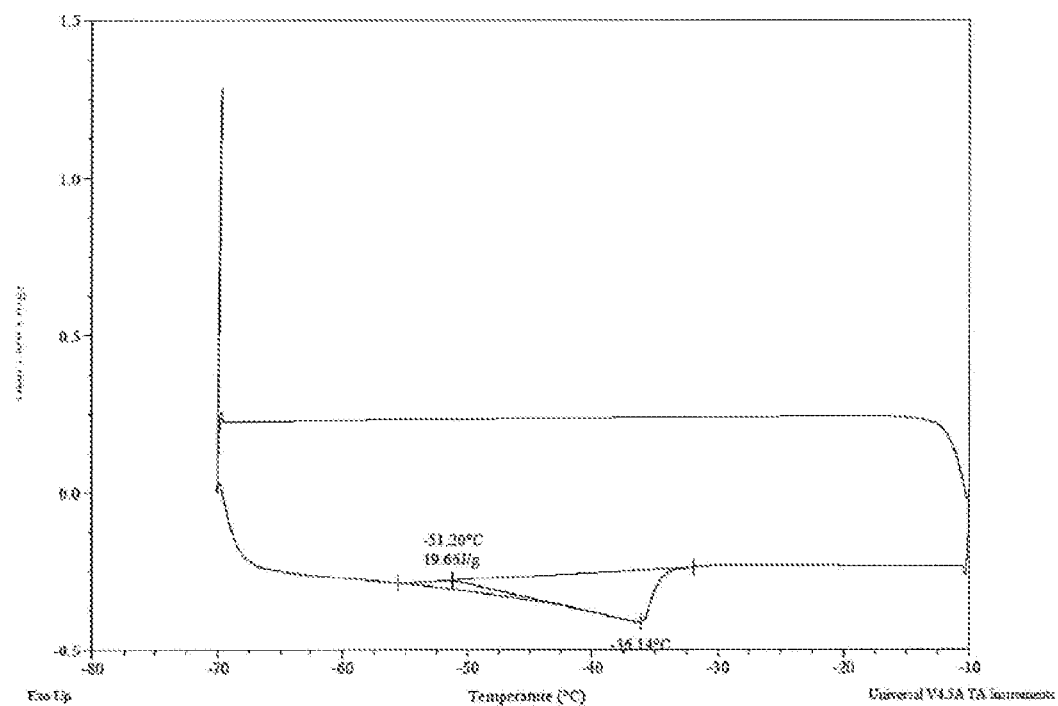


[Fig. 5]

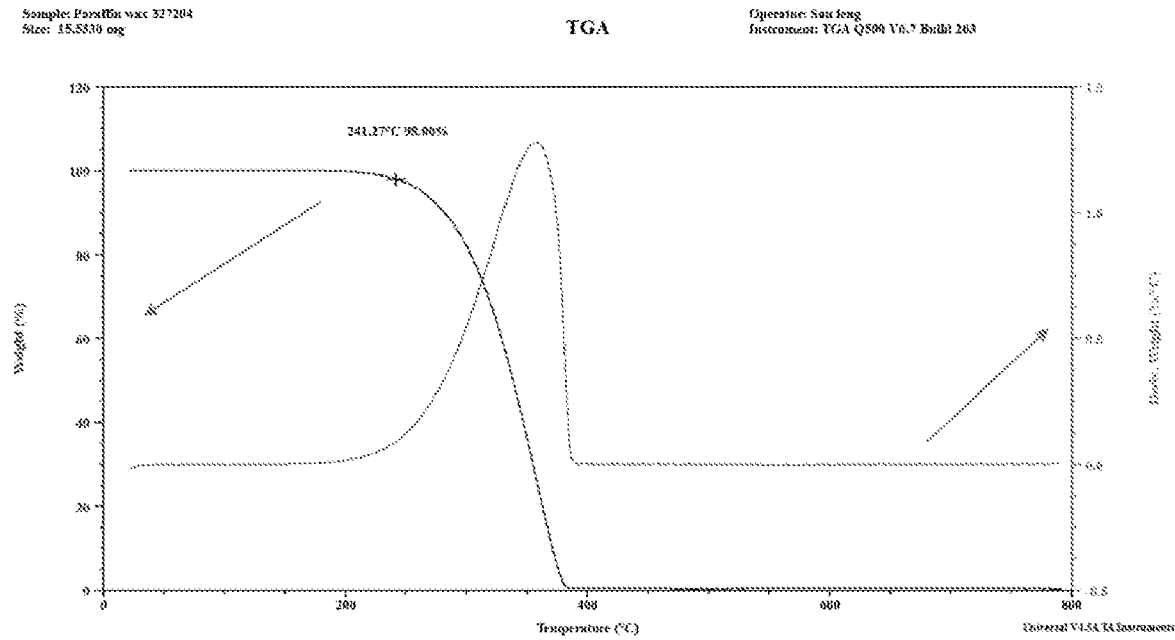


[Fig. 6]

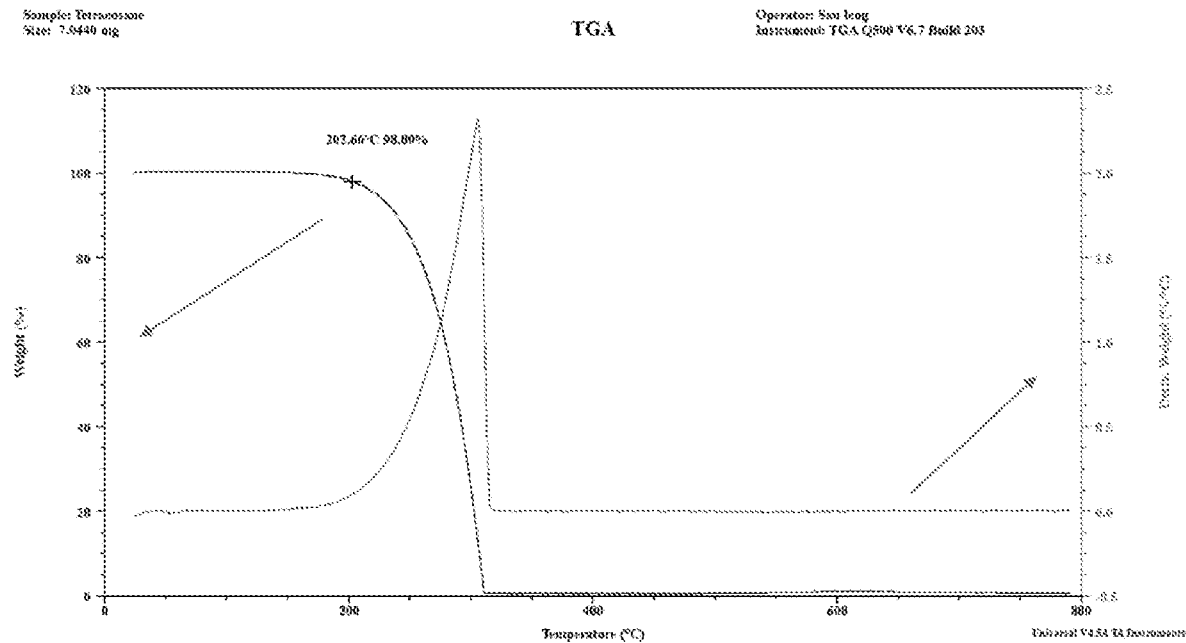


[Fig. 7]

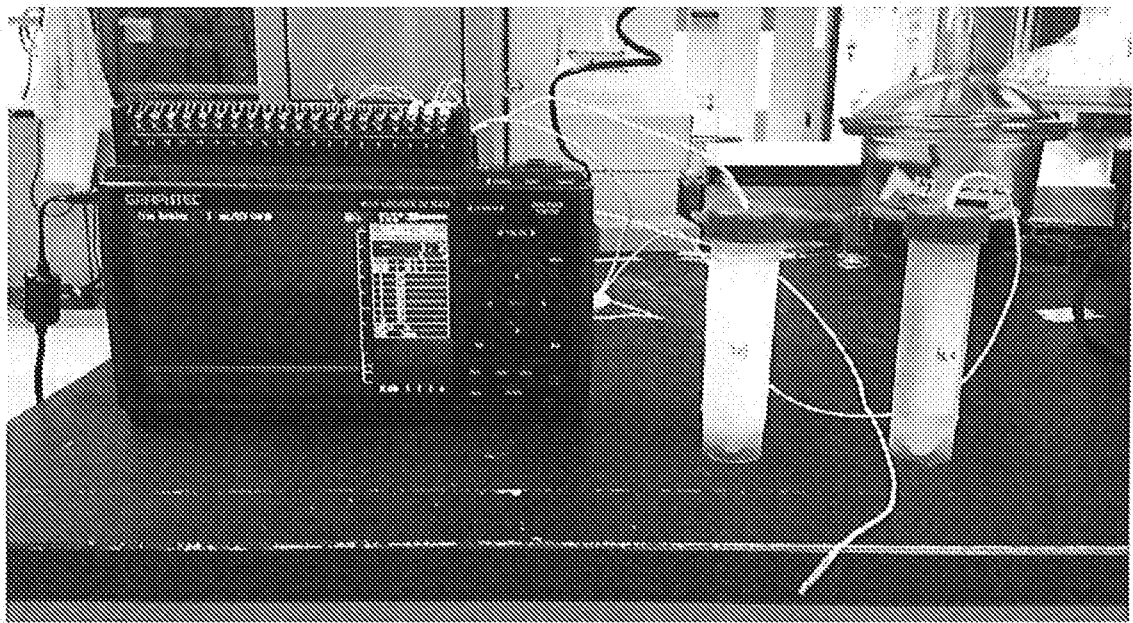


[Fig. 8]

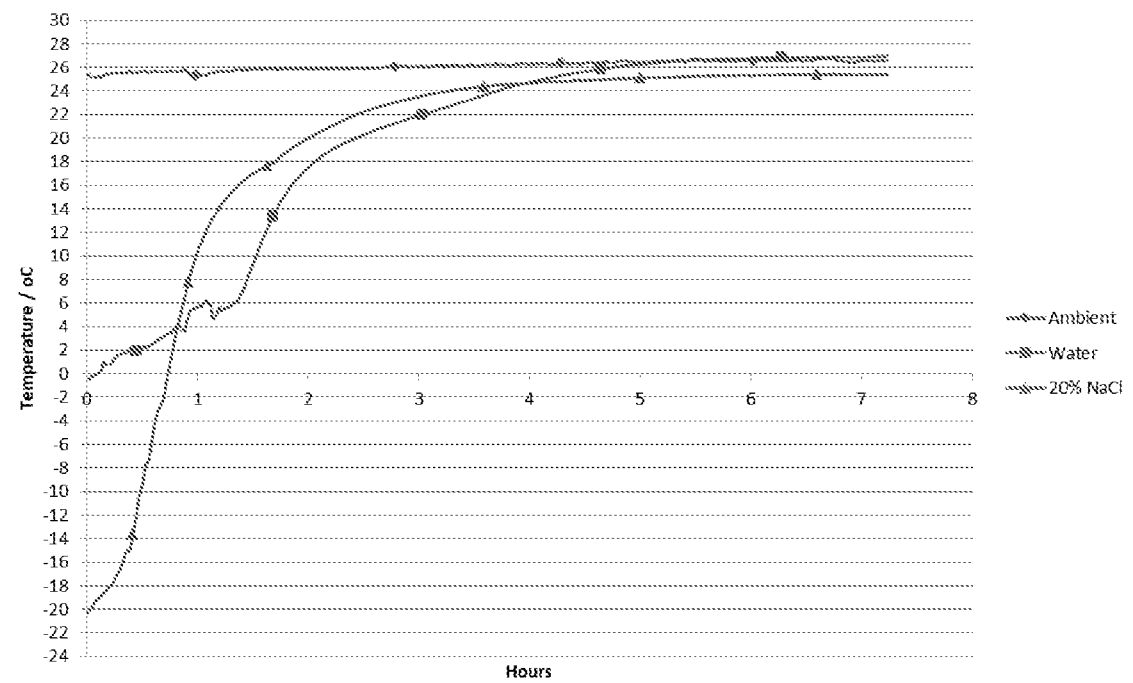


[Fig. 9]

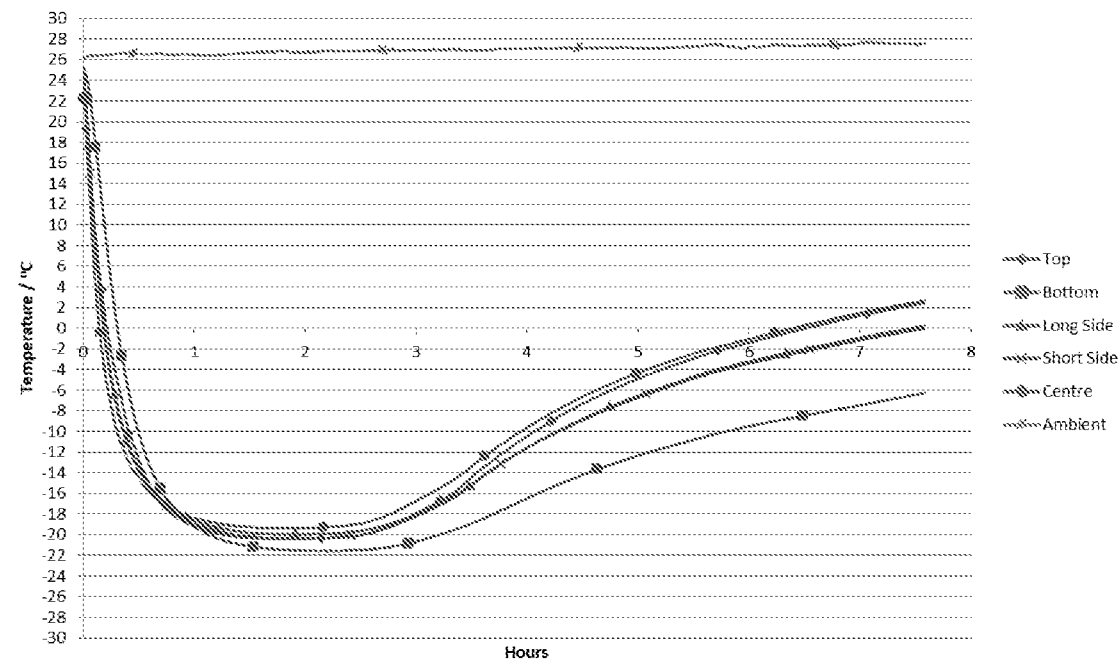


[Fig. 10]

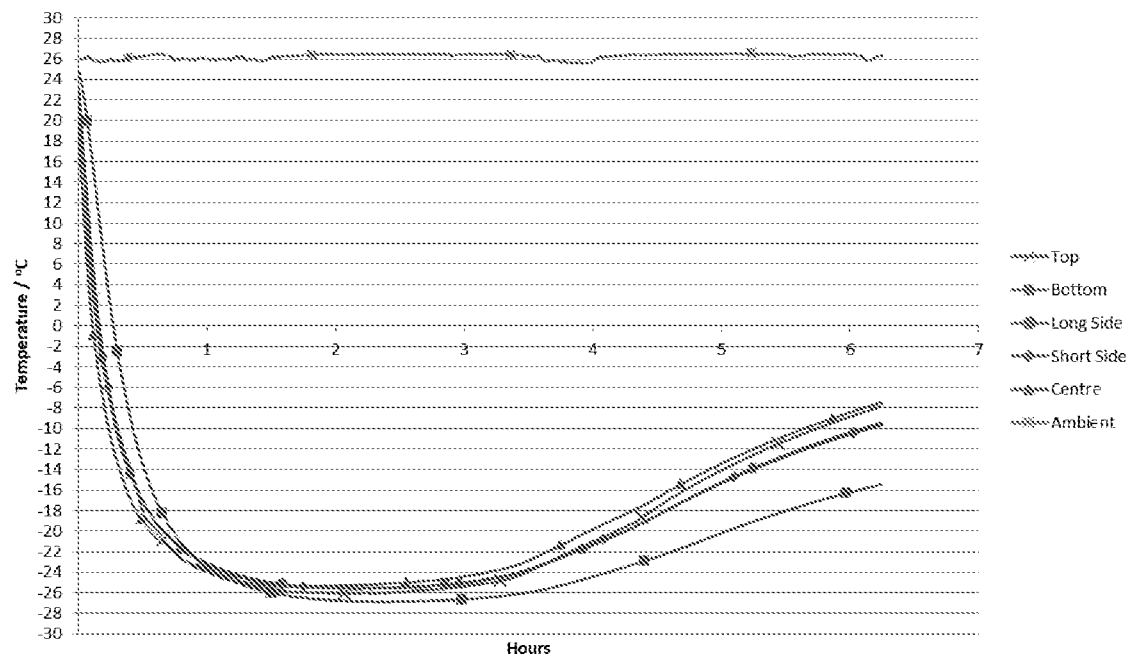

[Fig. 11]

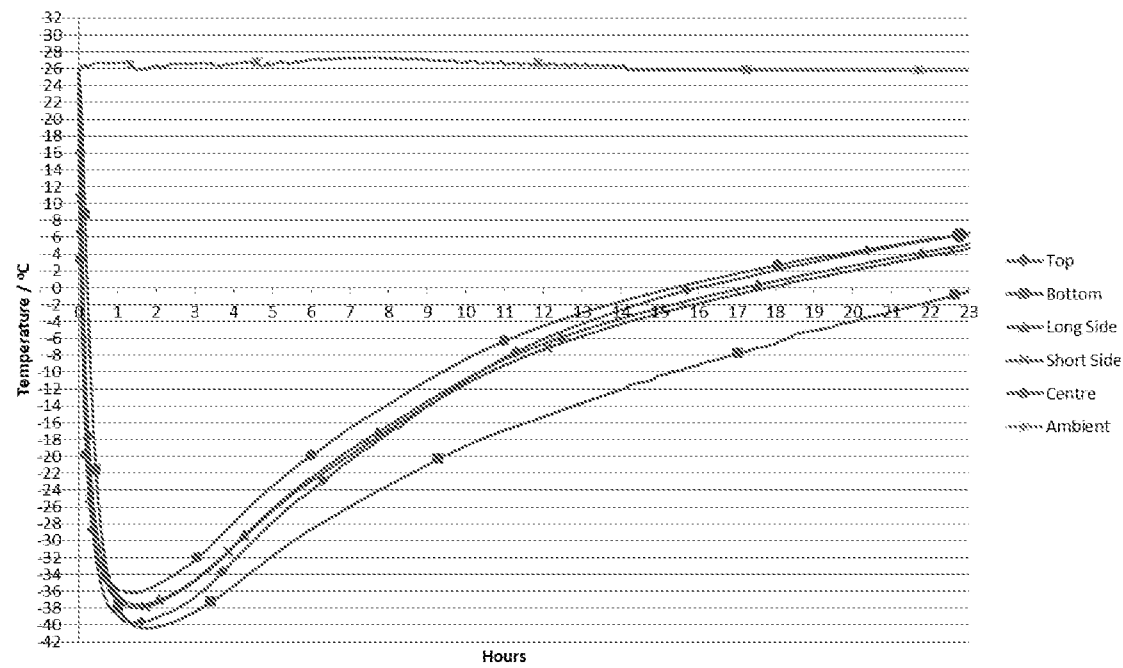

[Fig. 12]

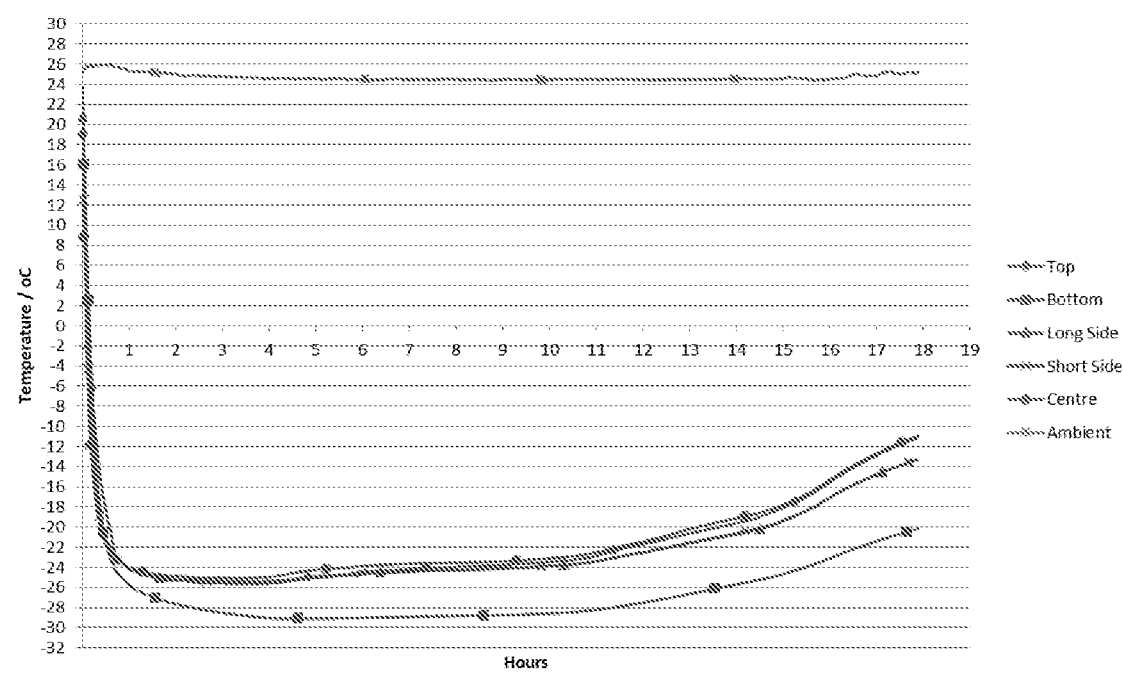

[Fig. 13]

