

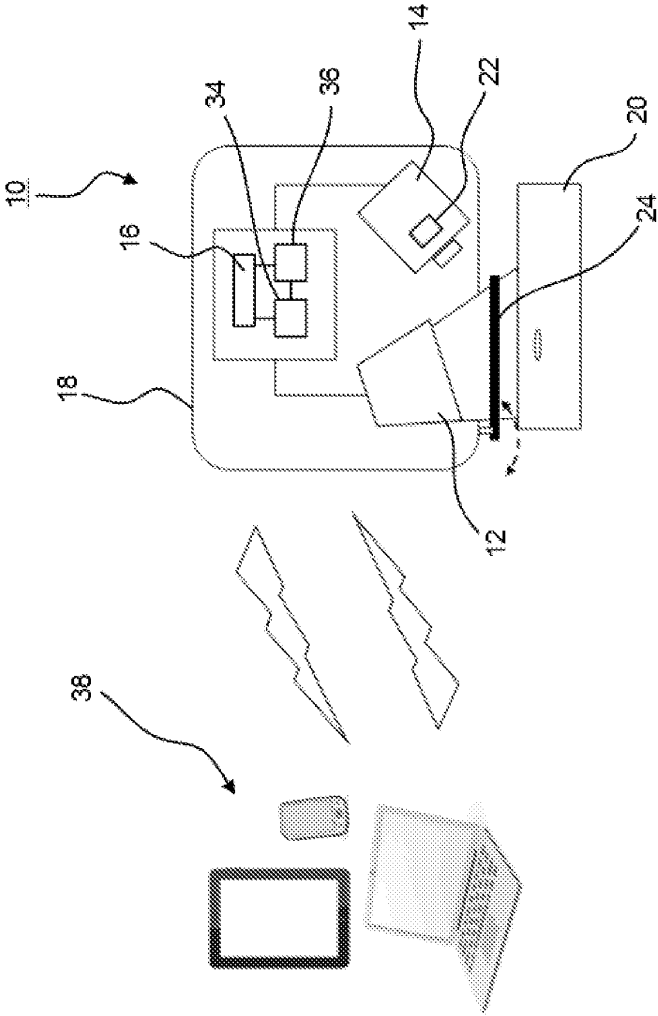


FIG. 1

2/17

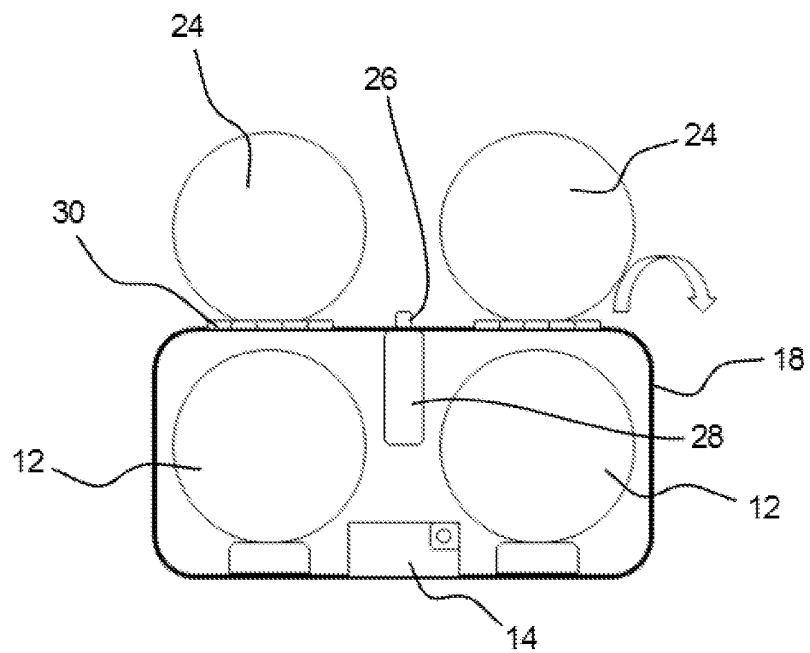


FIG. 2A

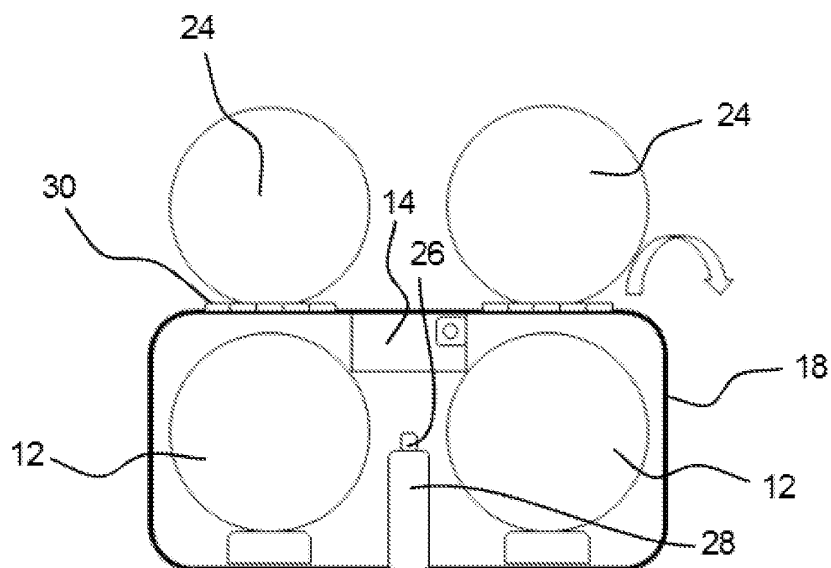


FIG. 2B

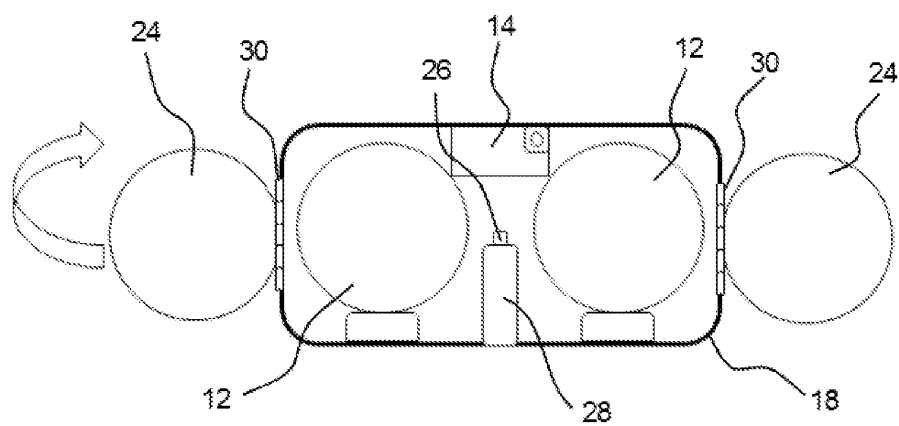


FIG. 2C

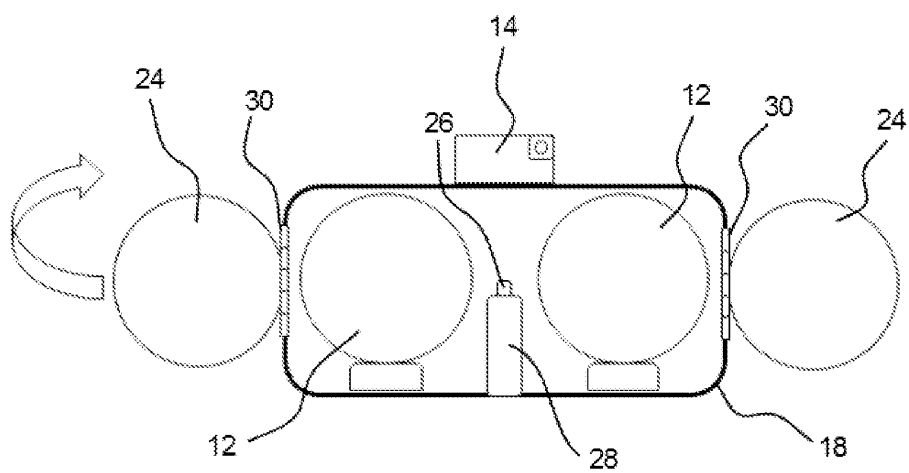


FIG. 2D

4/17

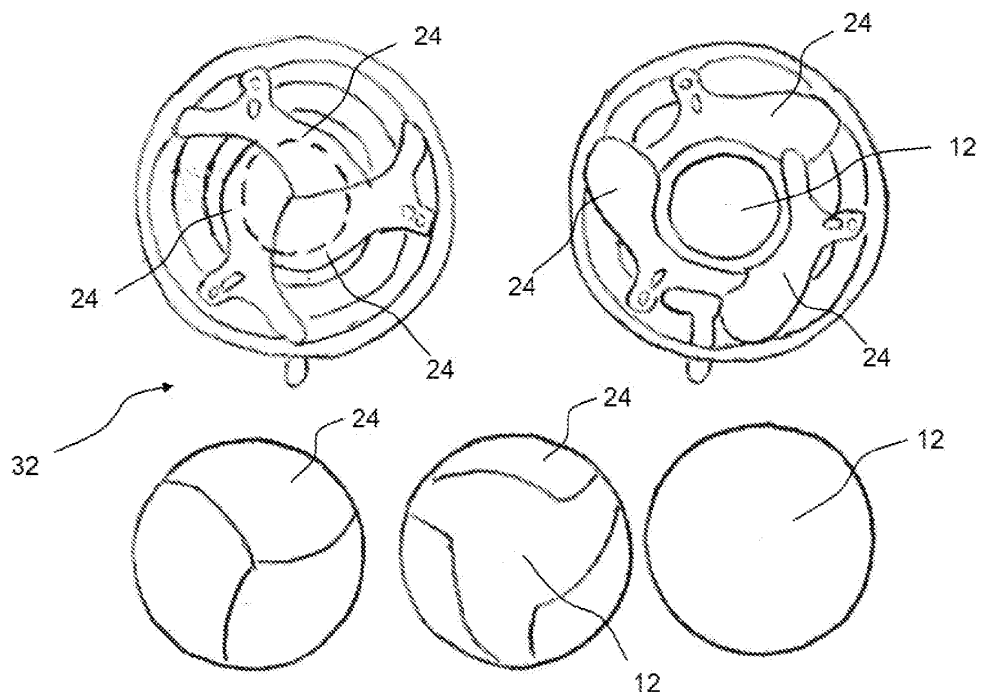


FIG. 2E

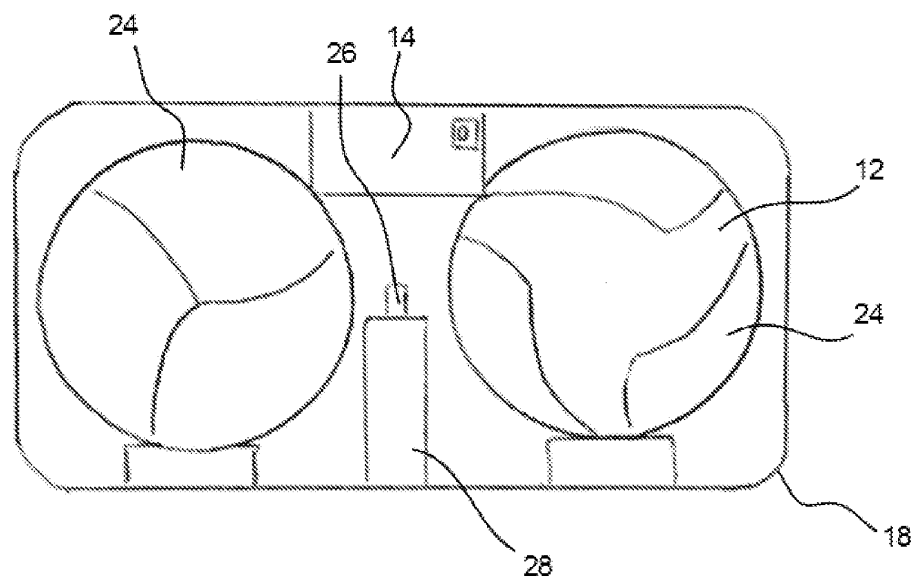


FIG. 2F

5/17

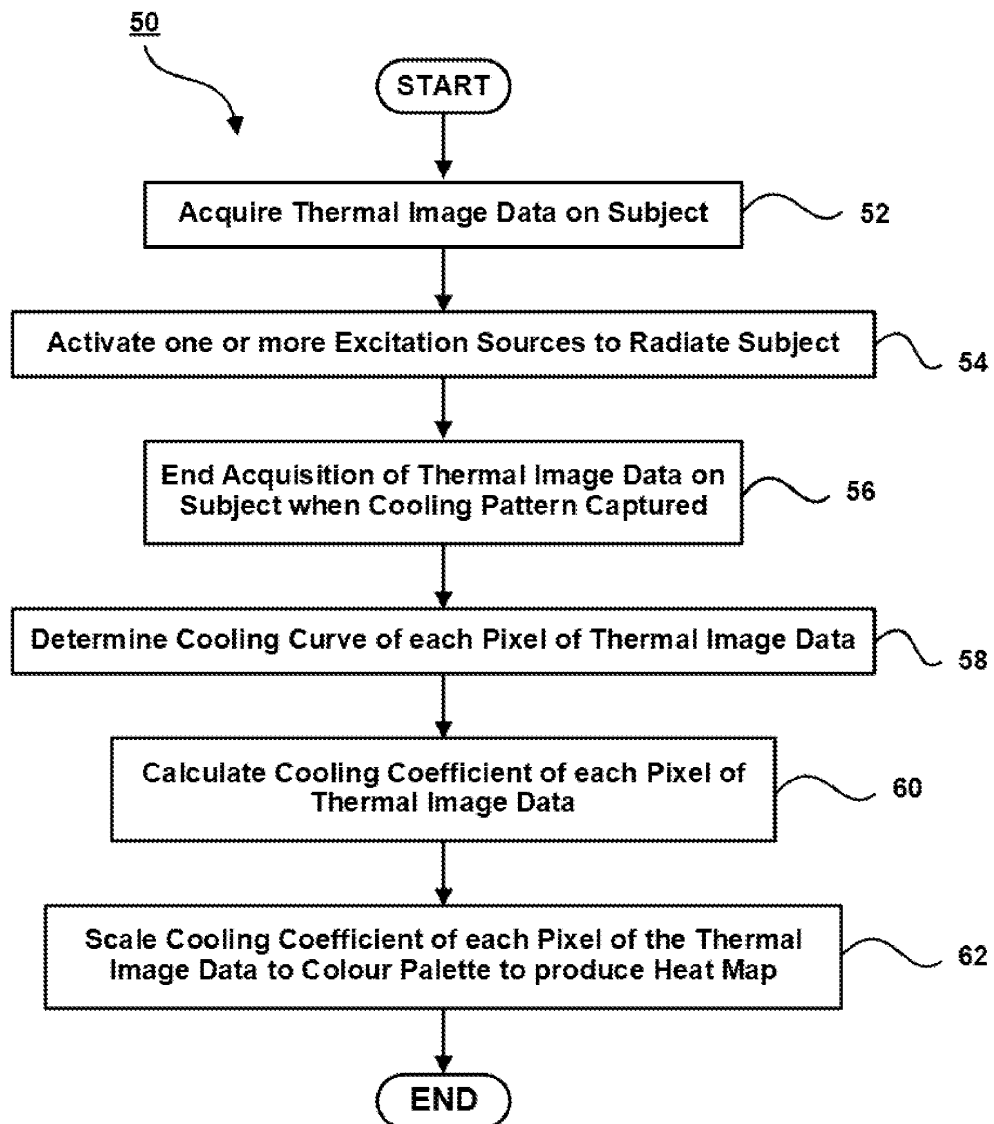


FIG. 3

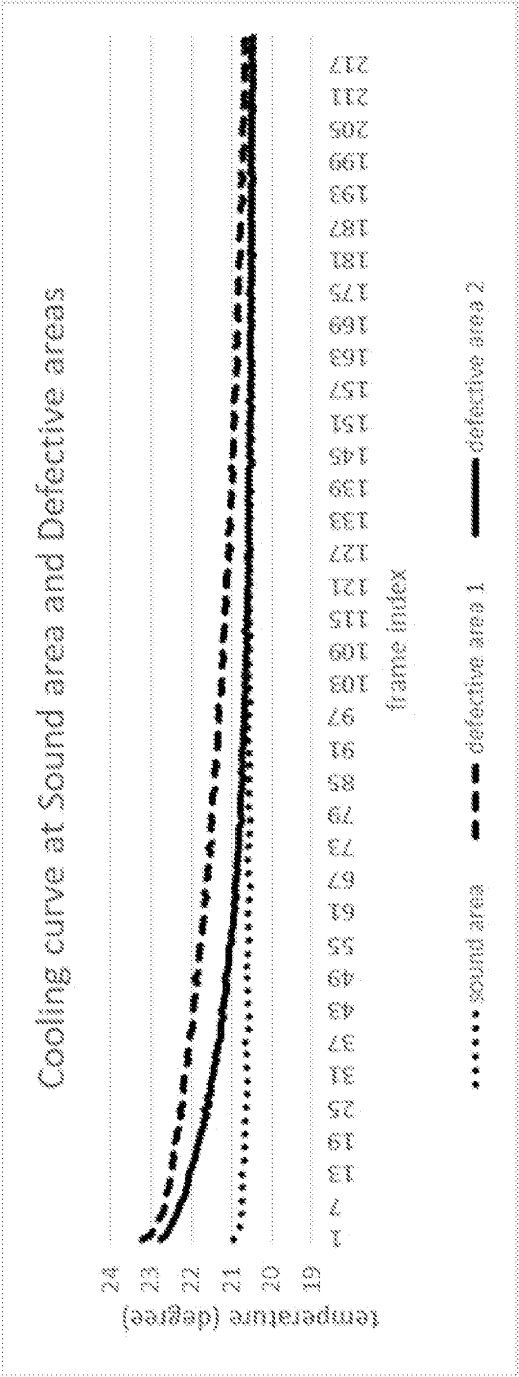


FIG. 4

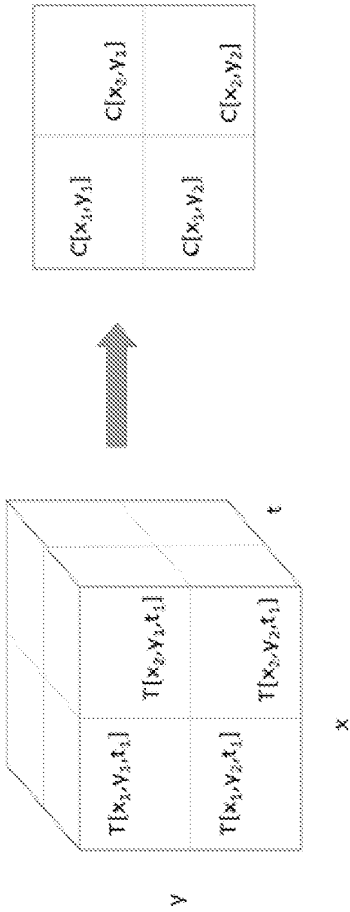


FIG. 5







	"Best" frame chosen by experienced thermographer	Reconstructed image from Embodiments of Present Invention
(1)		
(2)		
(3)		

FIG. 6

9/17







FIG. 7

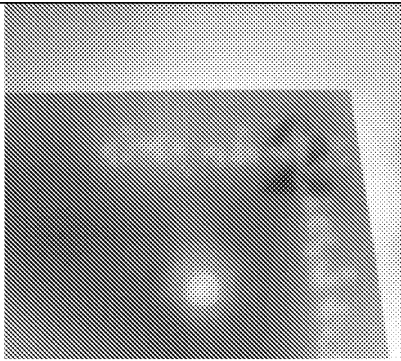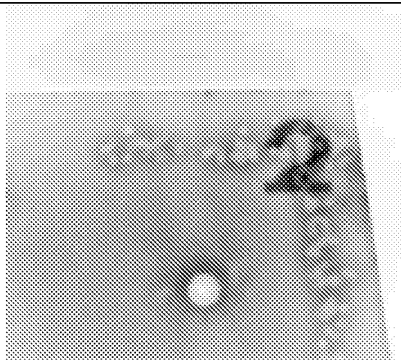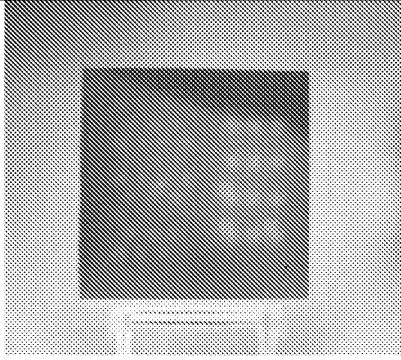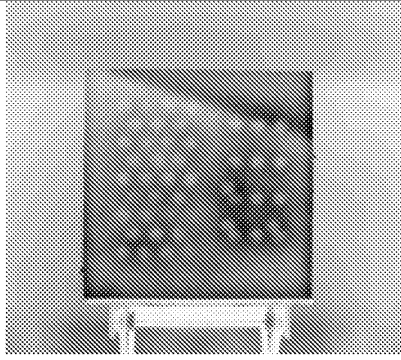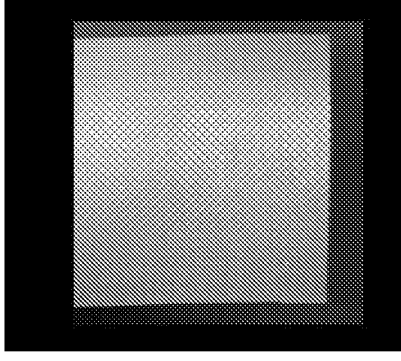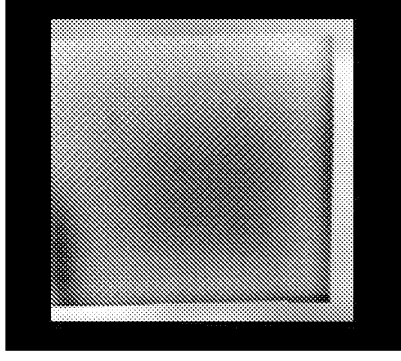

+

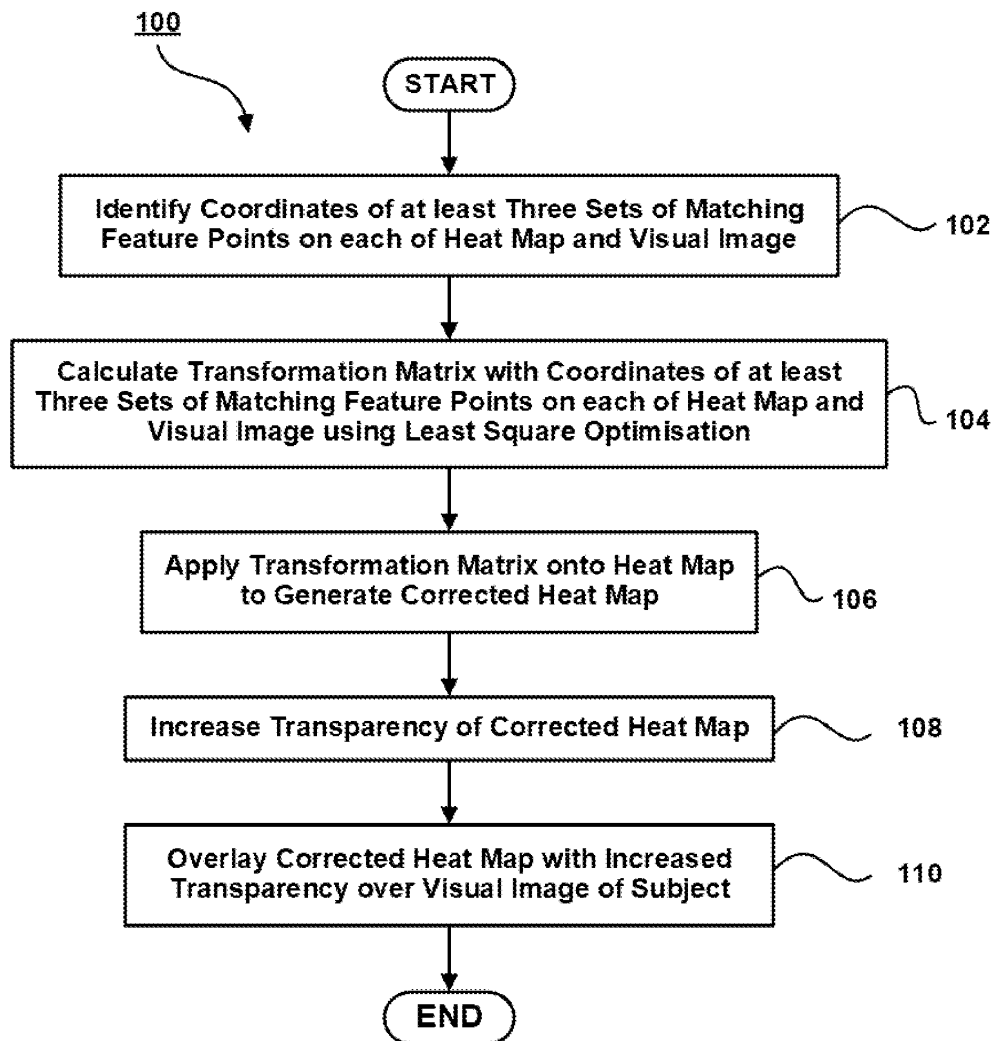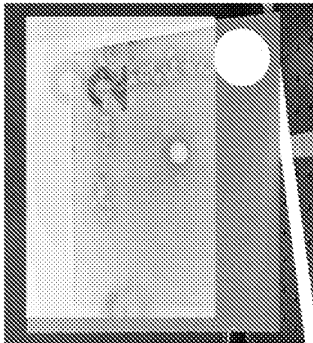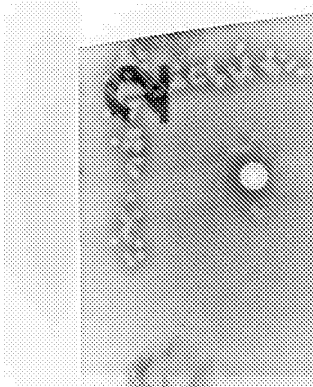

+

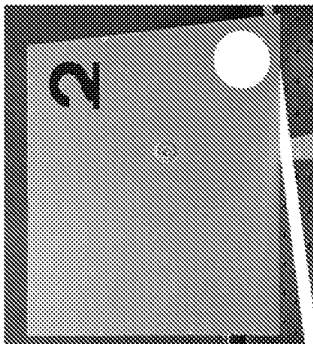


+


FIG. 8A

FIG. 8B


FIG. 8C

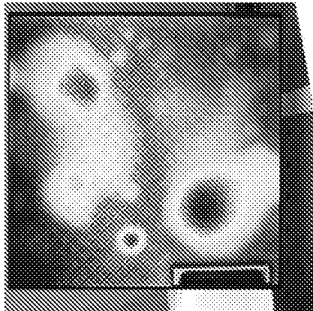

+

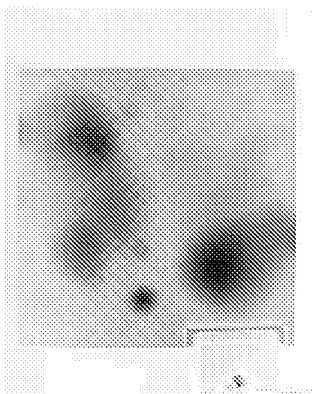

+

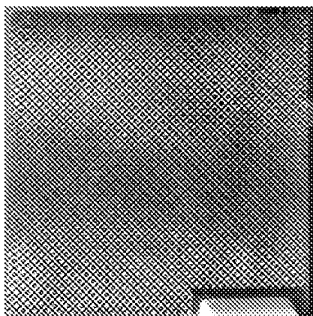

+

FIG. 9A

FIG. 9B

FIG. 9C

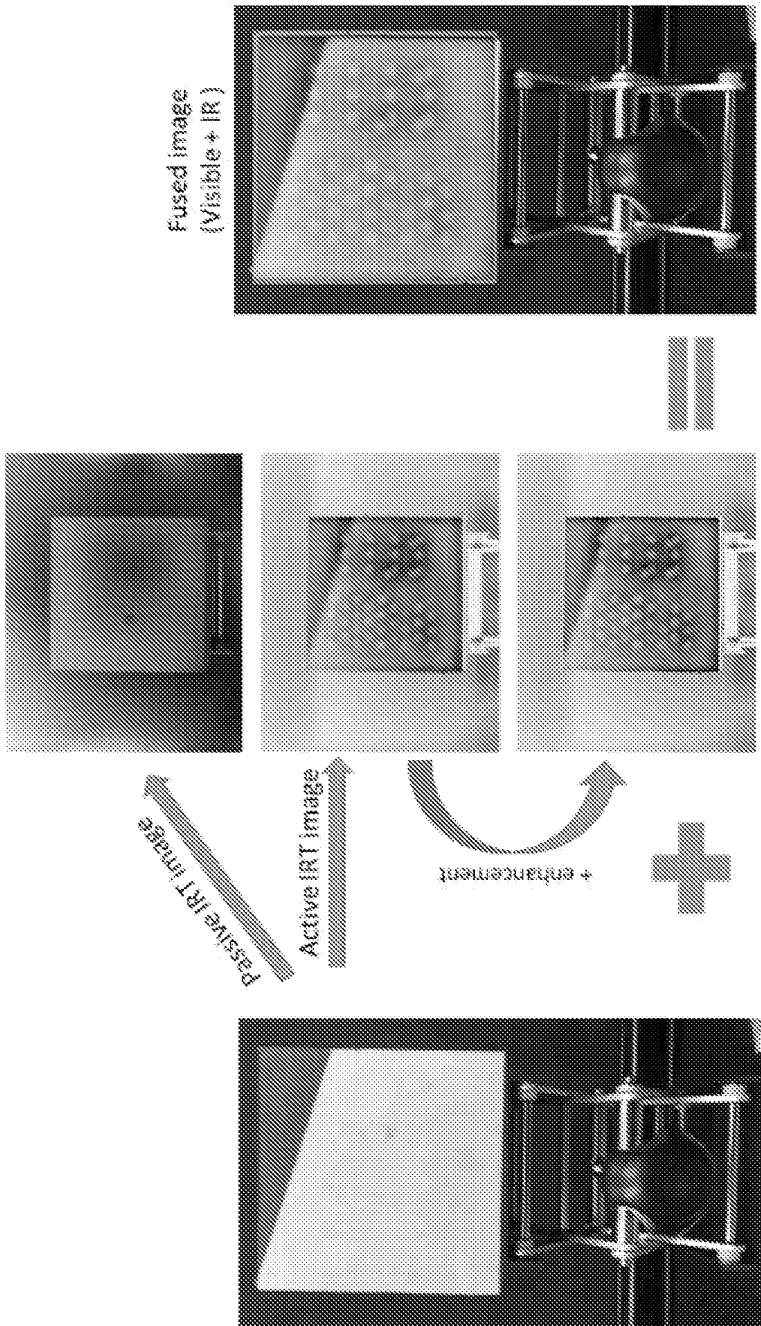


FIG. 10A

12/17

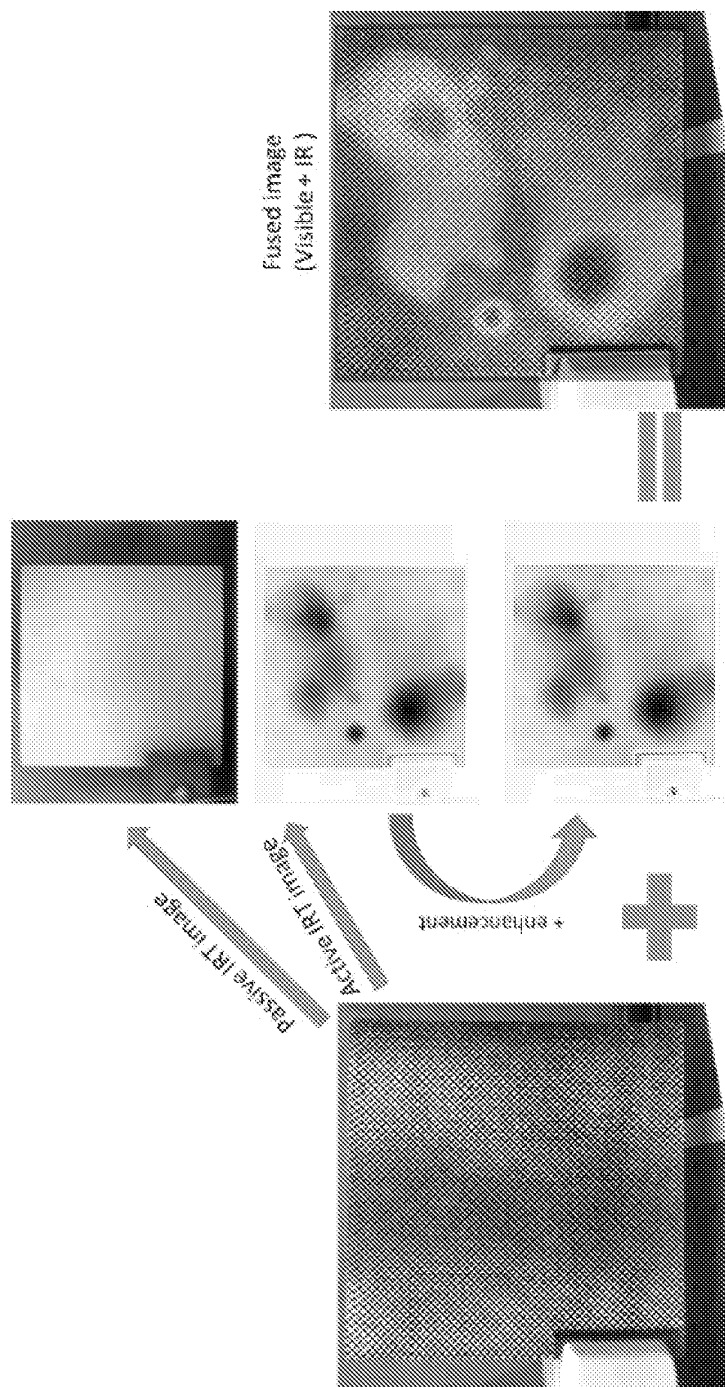
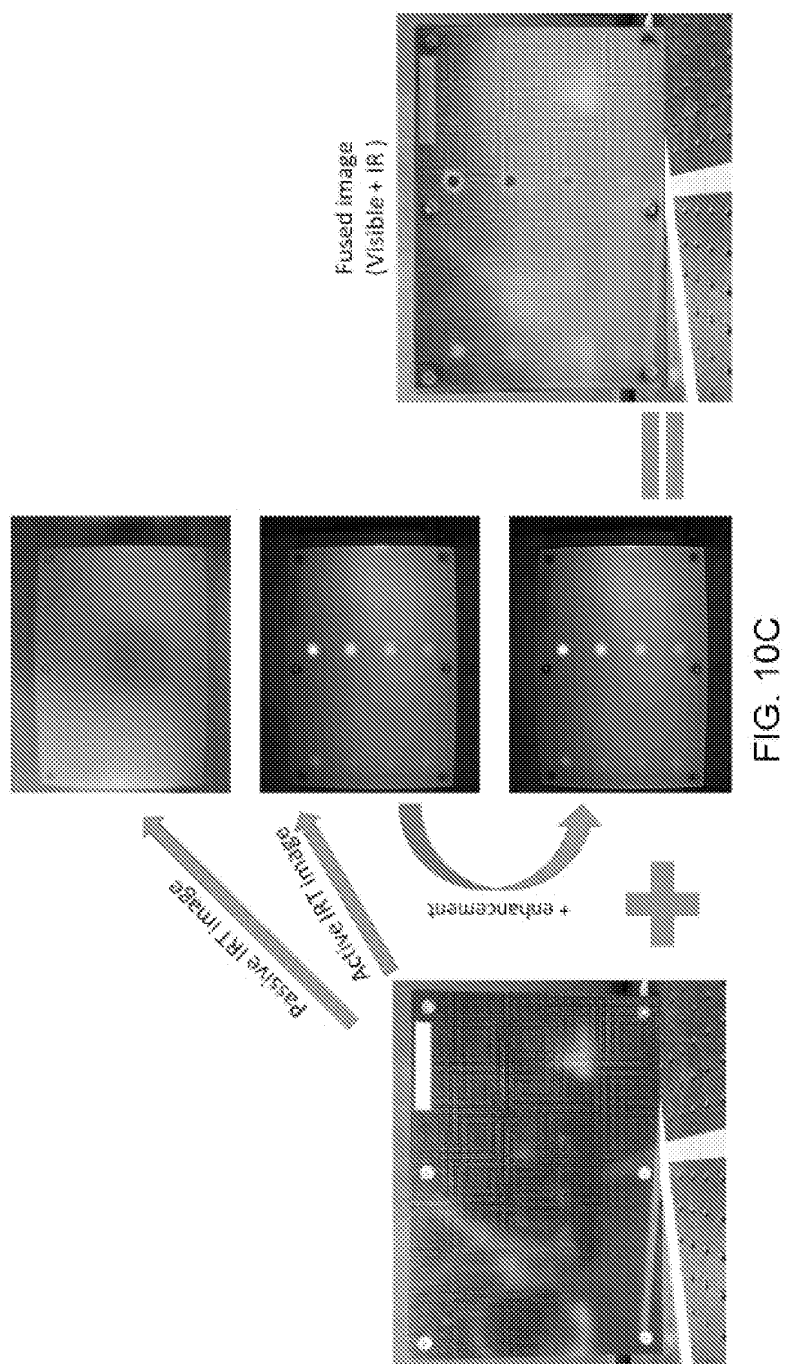
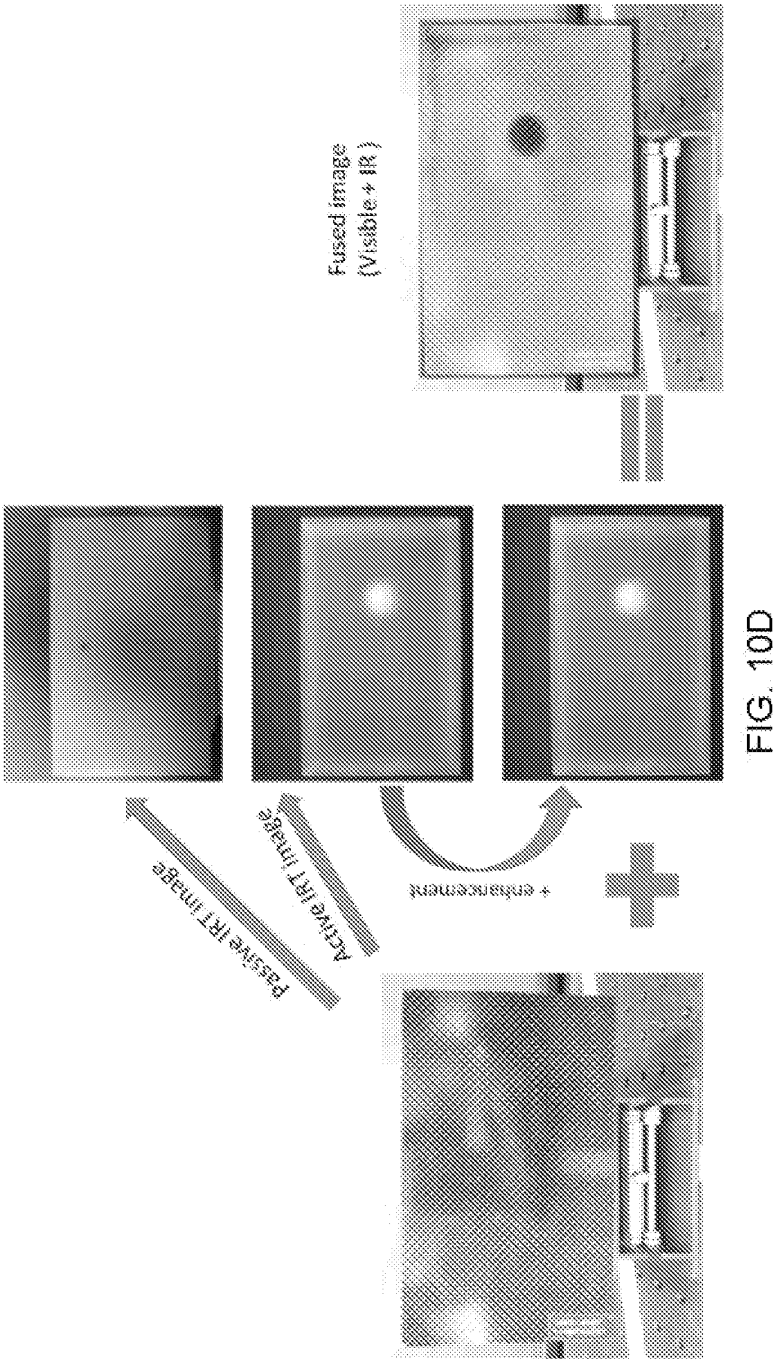
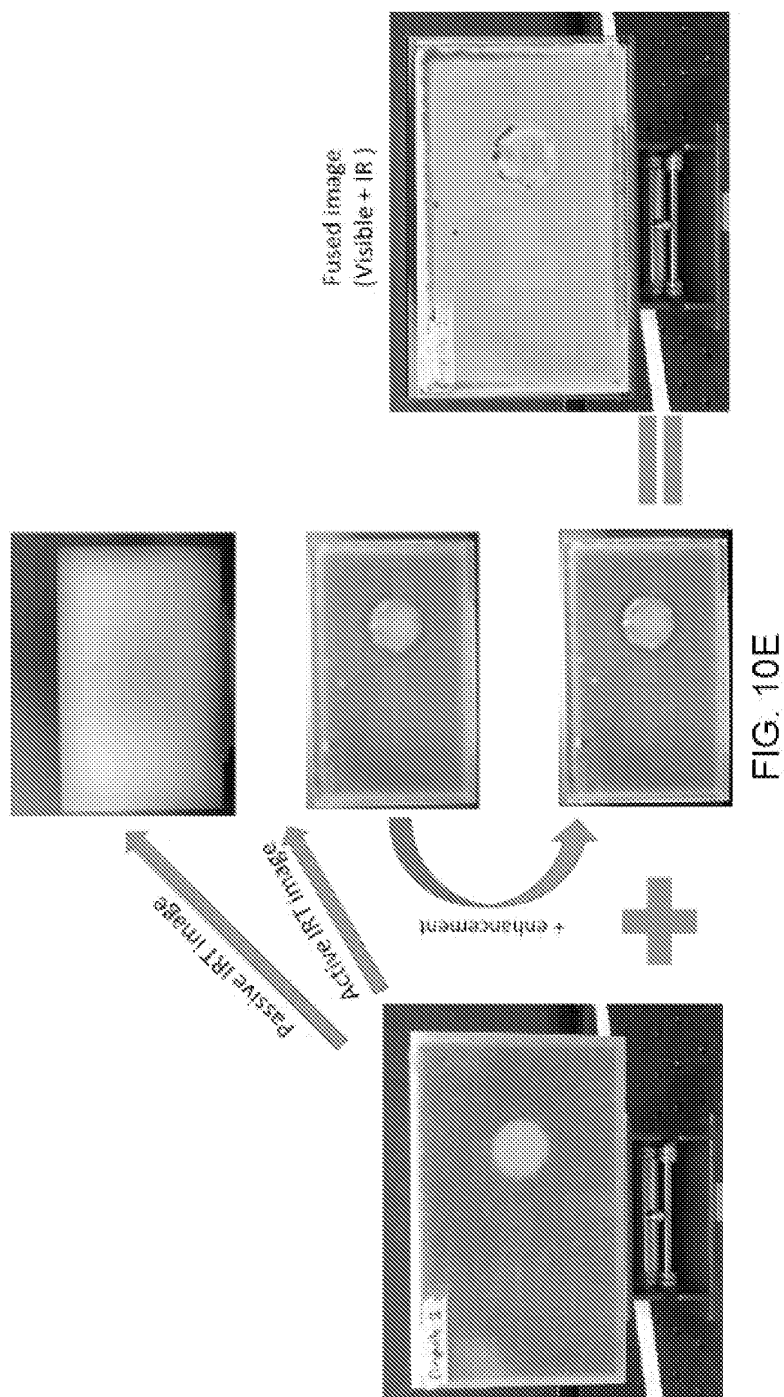


FIG. 10B







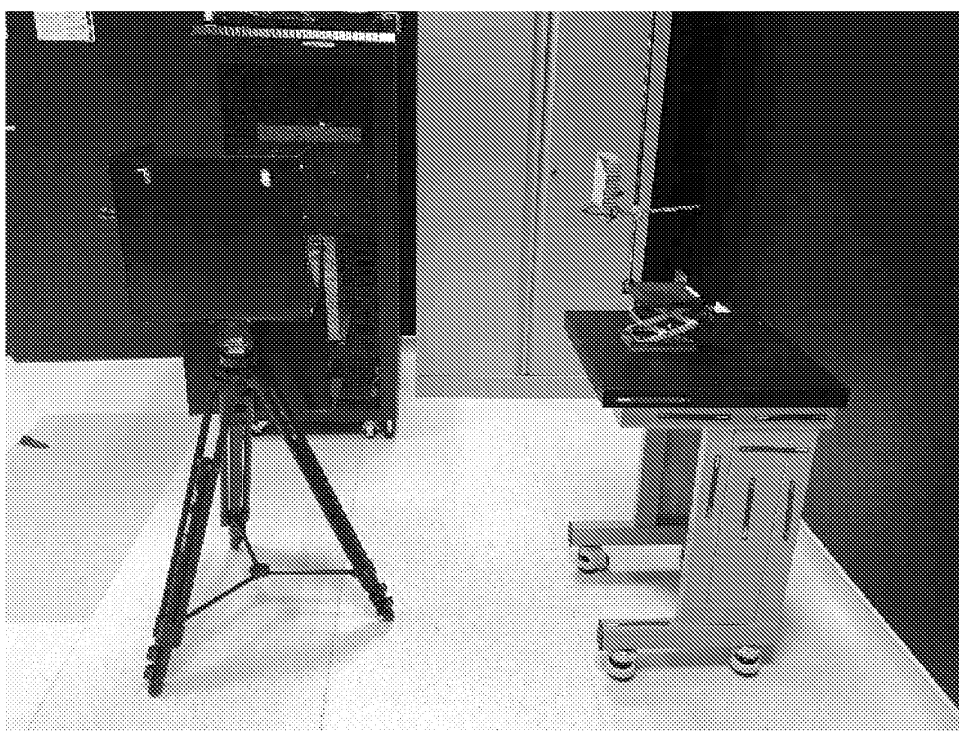


FIG. 11A

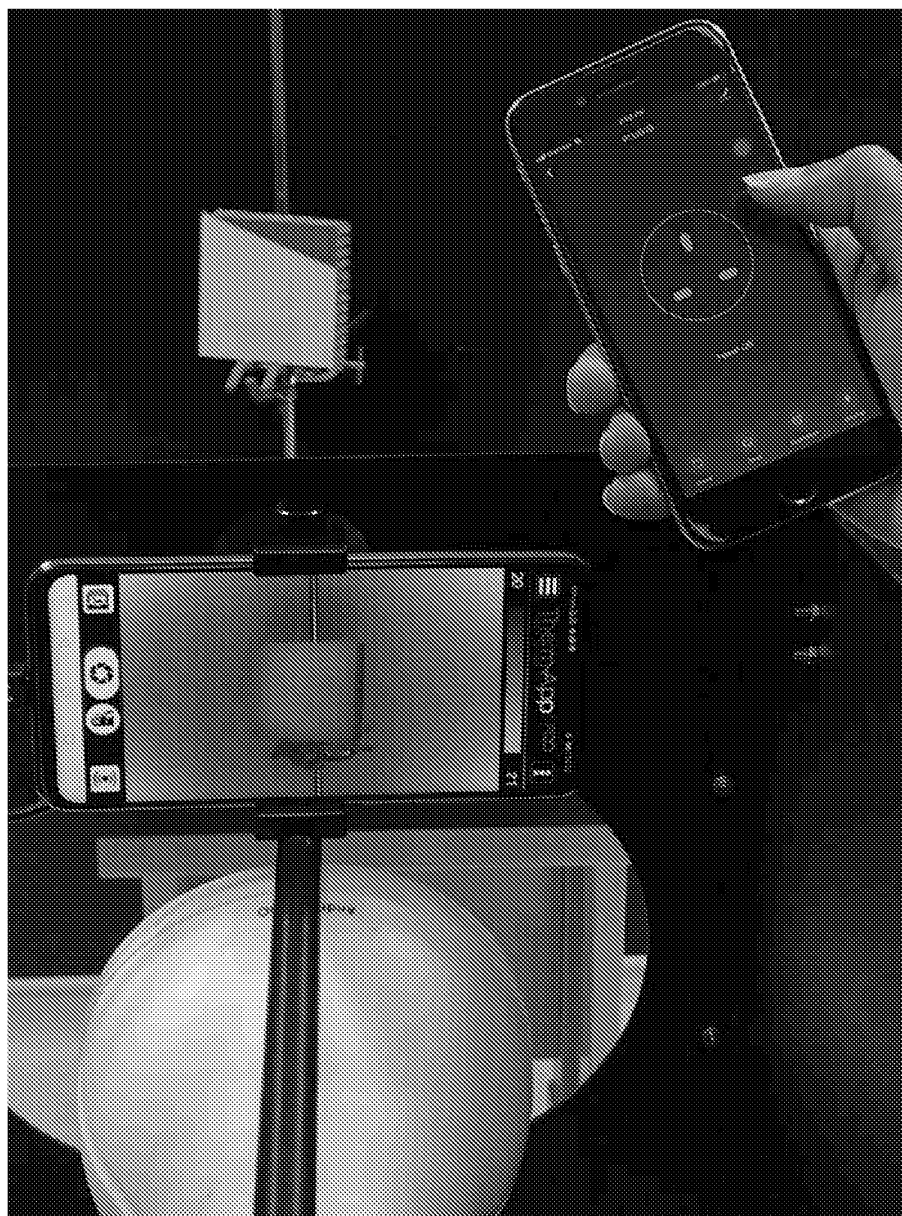


FIG. 11B