

Fig. 1

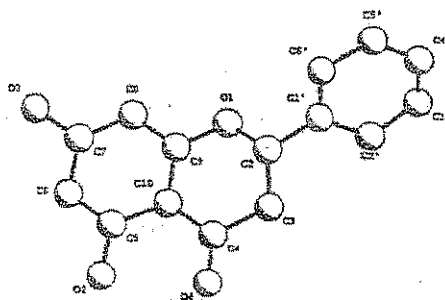


Fig. 2

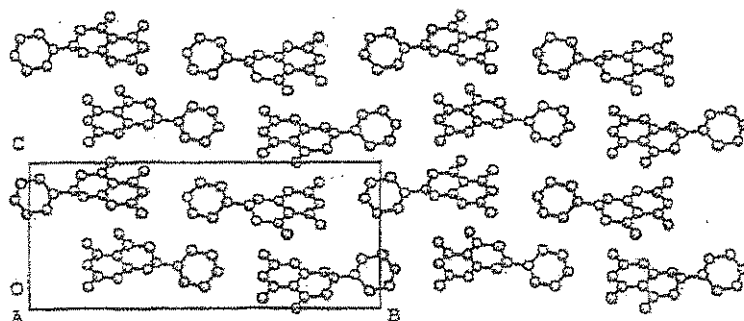


Fig. 3


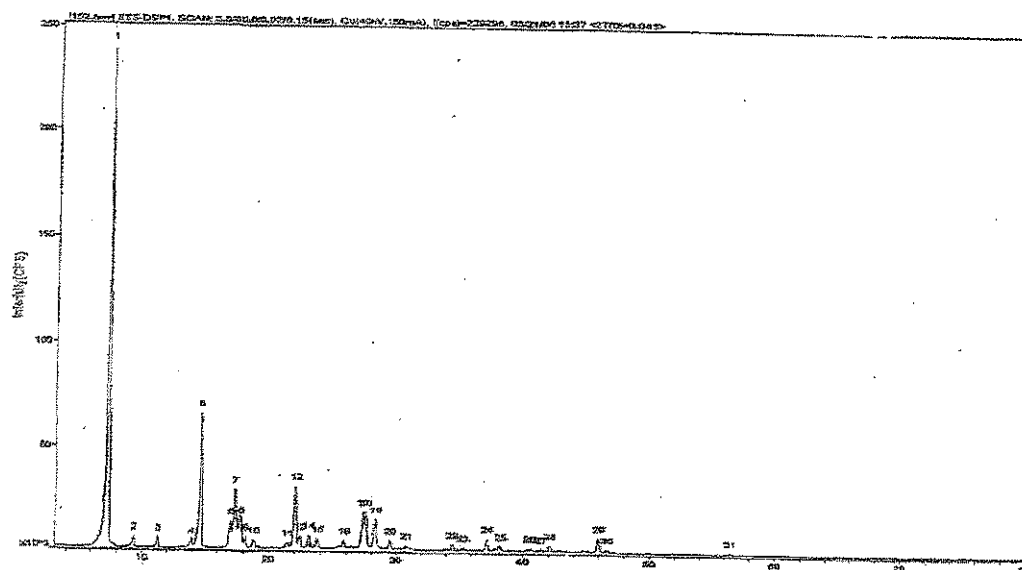


Fig. 4

<< DSC >>
 Data Name: SSS-DSP
 Date: 7/3/22 16:03
 Sample: SSS-DSP
 Reference: 0

Temperature Program:
 1 15 - 200 10 0 0.5

Comments:
 Operator: Wang
 N2=60ml/min

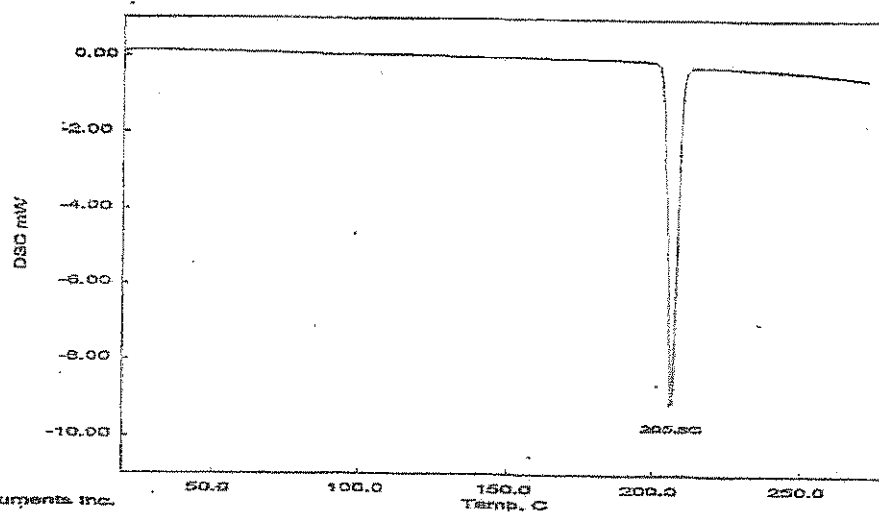

Seiko Instruments Inc.

Fig. 5

<< DSC >>
 Data Name: SSS-DY
 Date: 7/3/22 15:19
 Sample: SSS-DY
 Reference: Q
 3 mg
 0 mg

Temperature Program:
 [C] [Rate] [min] [Sec]
 1* 15 - 250 10 0 0.5

Comments:
 Operator Wang
 N2=50ml/min

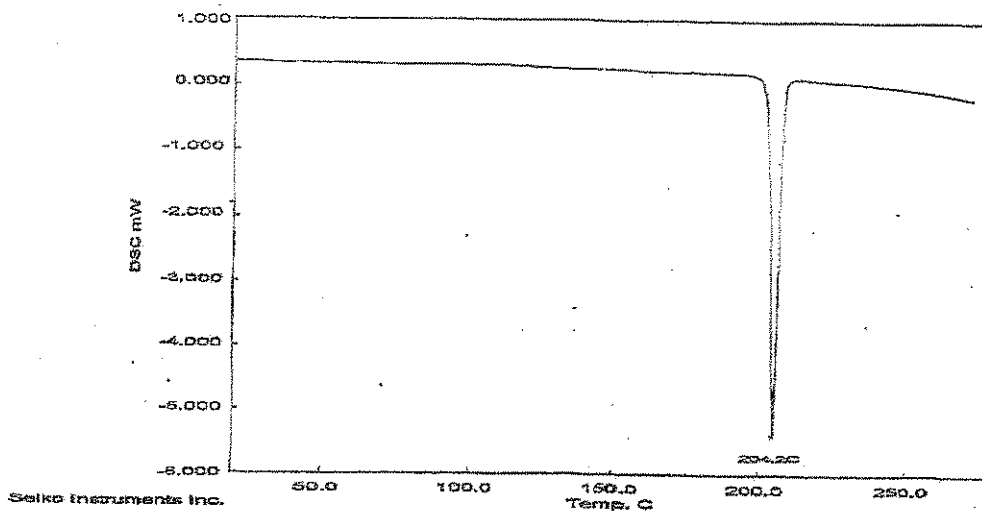


Fig. 8

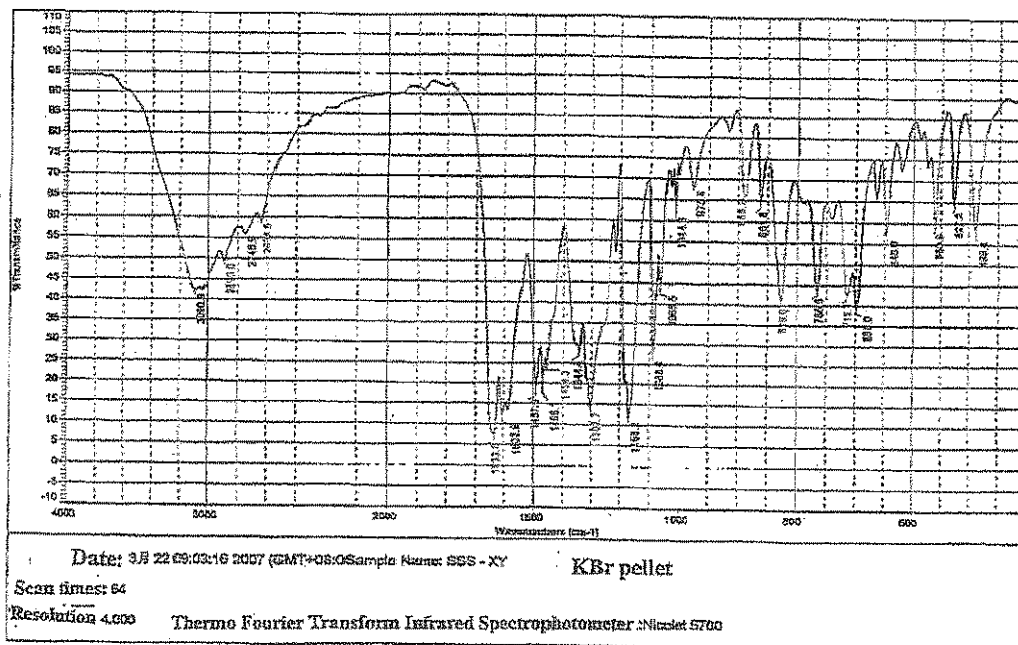


Fig. 9