



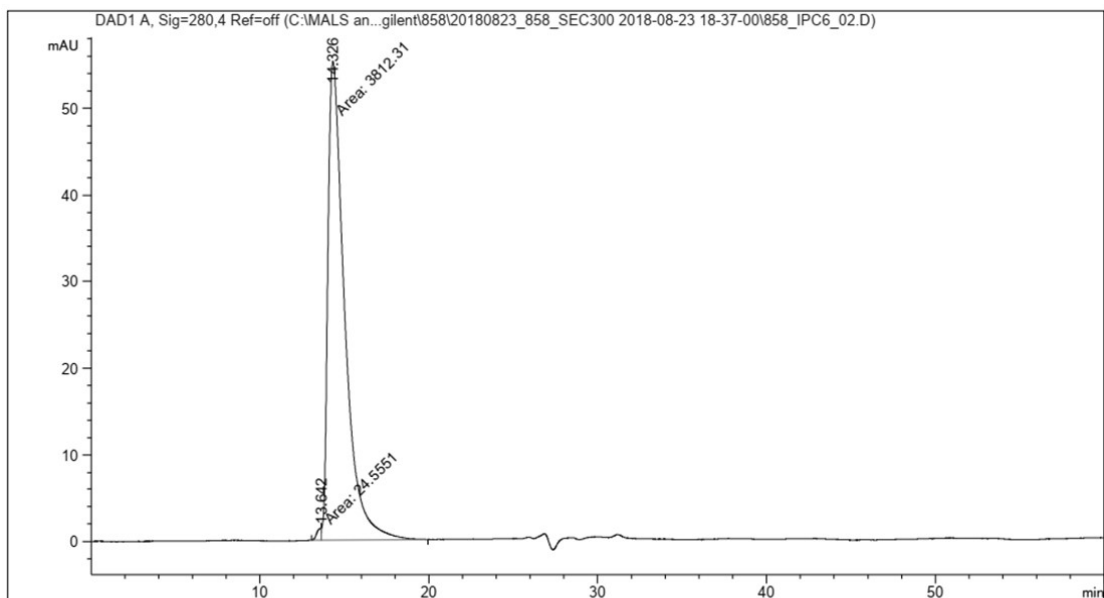

Retention Time (min)	Width (min)	Height (mAU)	Peak Area	Percentage (%)
13.642	0.2978	1.3745	24.5551	0.64
14.326	1.1506	55.2221	3812.31	99.36

Fig. 1

Fitting Result

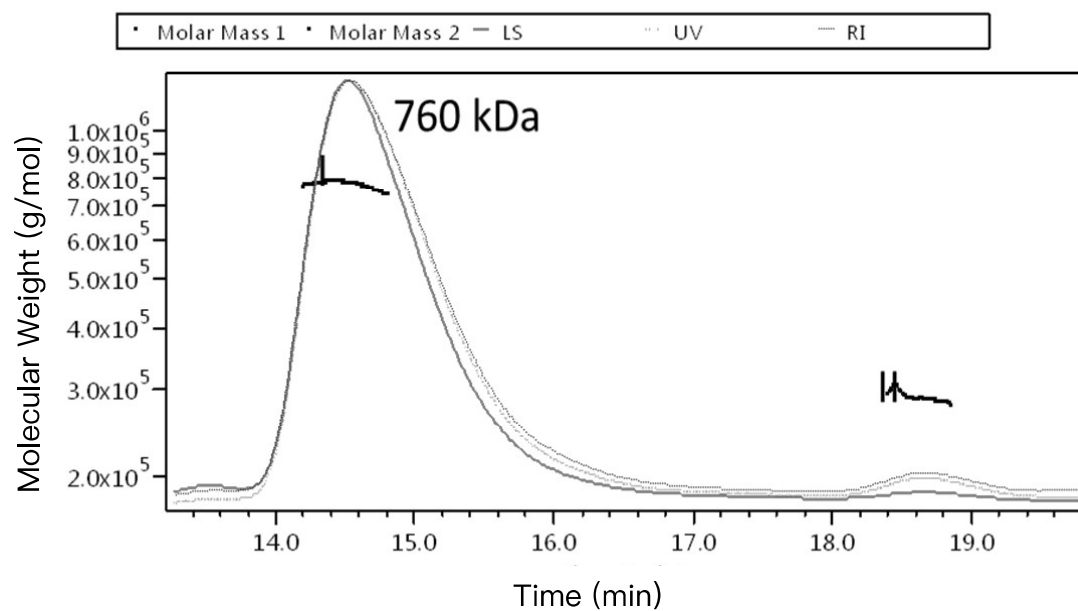

	RI (dn/dc=0.185)	UV (EC=1.49)
Average Value	779	759

Fig. 2

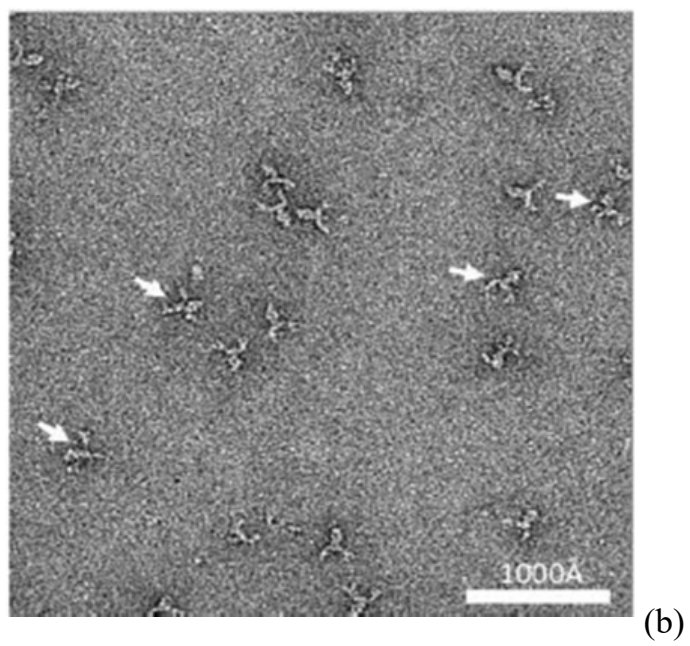
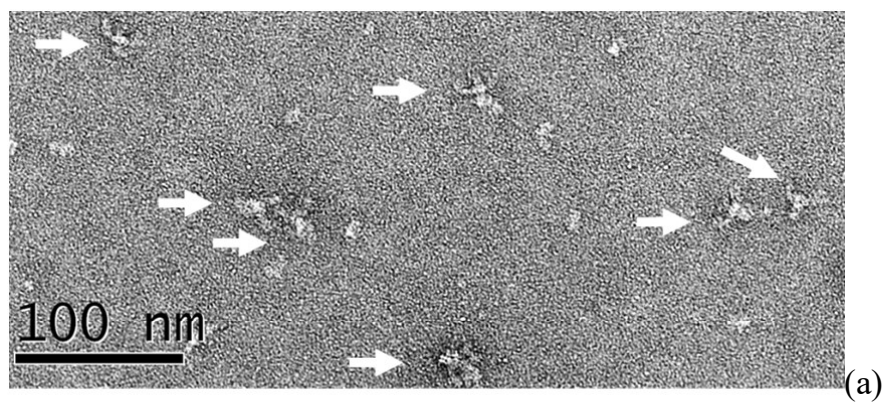


Fig. 3

DAS Assay Scoring

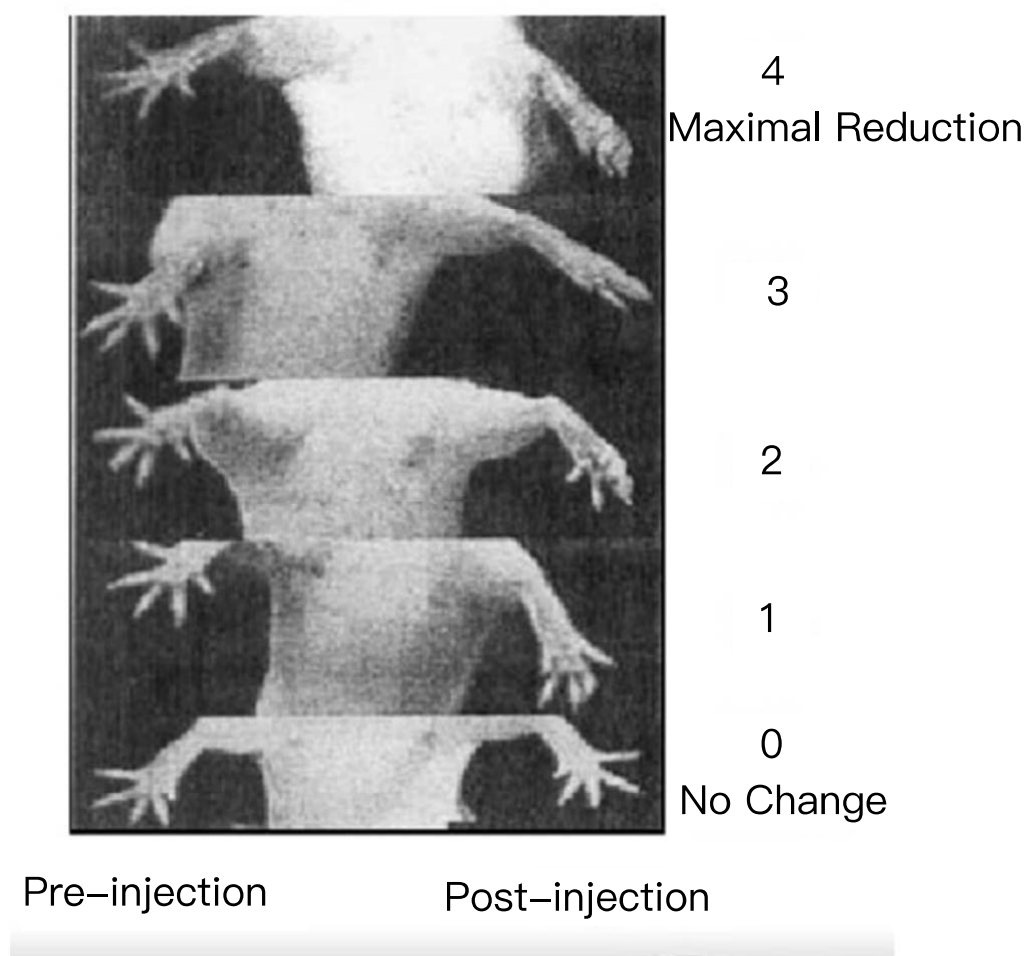


Fig. 4