

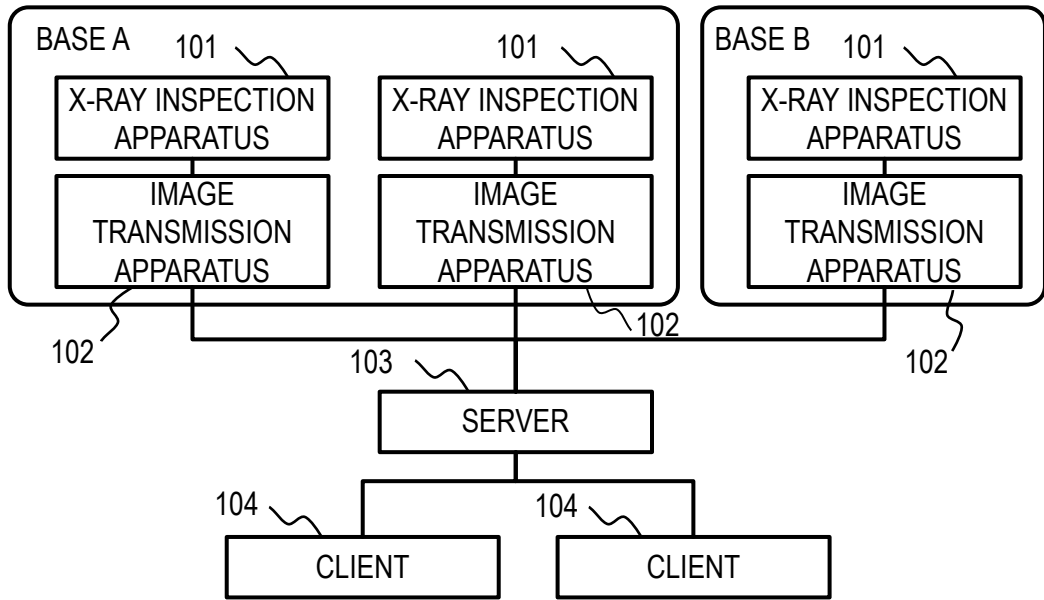


FIG. 1

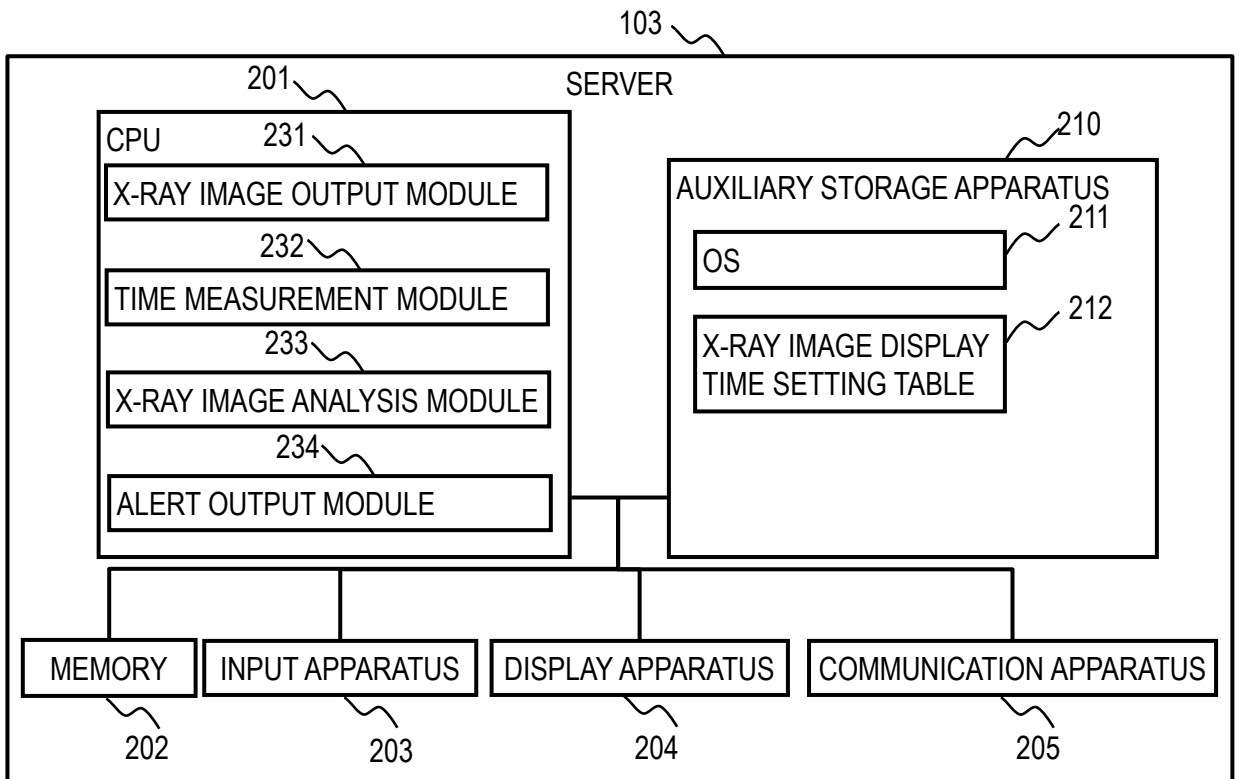


FIG. 2

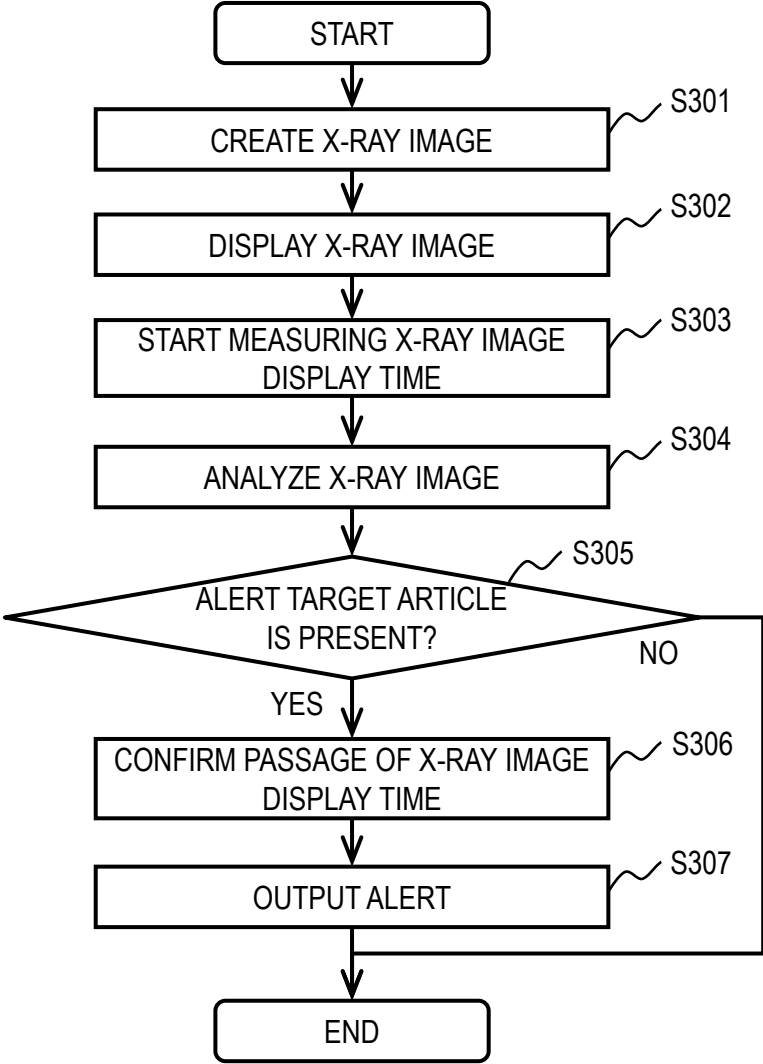


FIG. 3

X-RAY IMAGE DISPLAY TIME SETTING TABLE		
INSPECTOR ID	SKILL	X-RAY IMAGE DISPLAY TIME
INSPECTOR 1	SKILLED	2 SECONDS
INSPECTOR 2	ORDINARY	3 SECONDS
INSPECTOR 3	ORDINARY	3 SECONDS
INSPECTOR 4	ORDINARY	3 SECONDS
INSPECTOR 5	NOVICE	4 SECONDS

212

FIG. 4

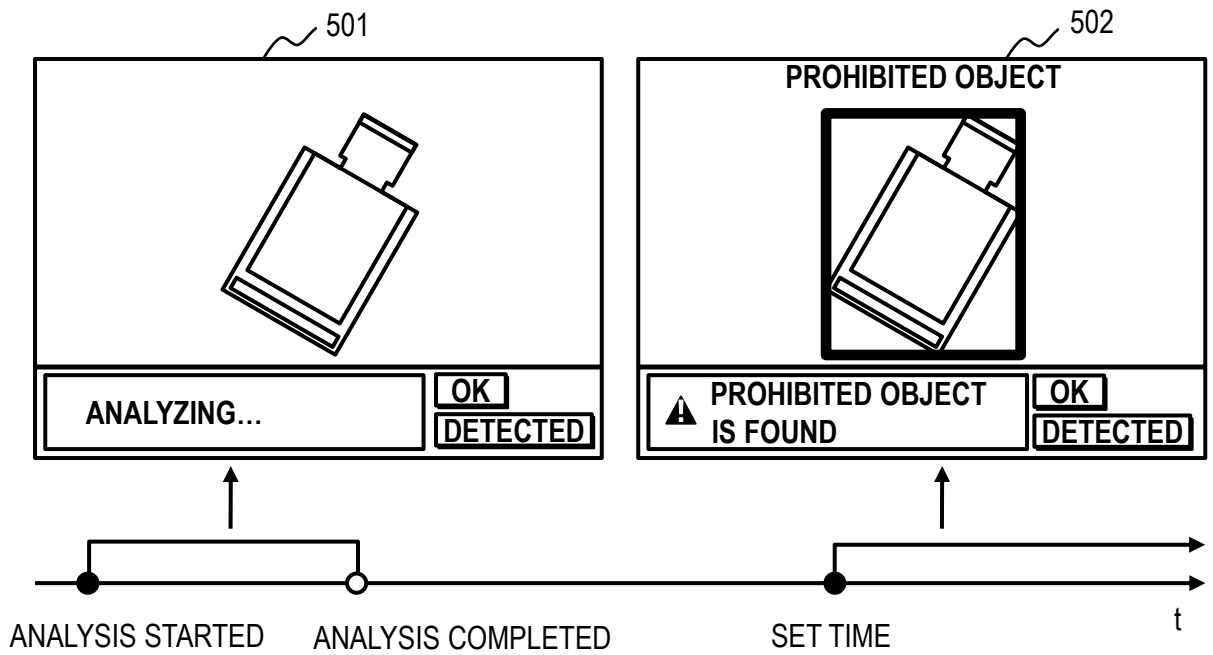


FIG. 5

FIG. 6 illustrates a form for setting inspector skills and X-ray image display times. The form is labeled 600.

INSPECTOR ID	SKILL
INSPECTOR 1	SKILLED ▼
INSPECTOR 2	SKILLED ▼
INSPECTOR 3	ORDINARY ▼
INSPECTOR 4	ORDINARY ▼
INSPECTOR 5	NOVICE ▼

SKILL	X-RAY IMAGE DISPLAY TIME
SKILLED	2 SECONDS
ORDINARY	3 SECONDS
NOVICE	4 SECONDS

SET

FIG. 6