

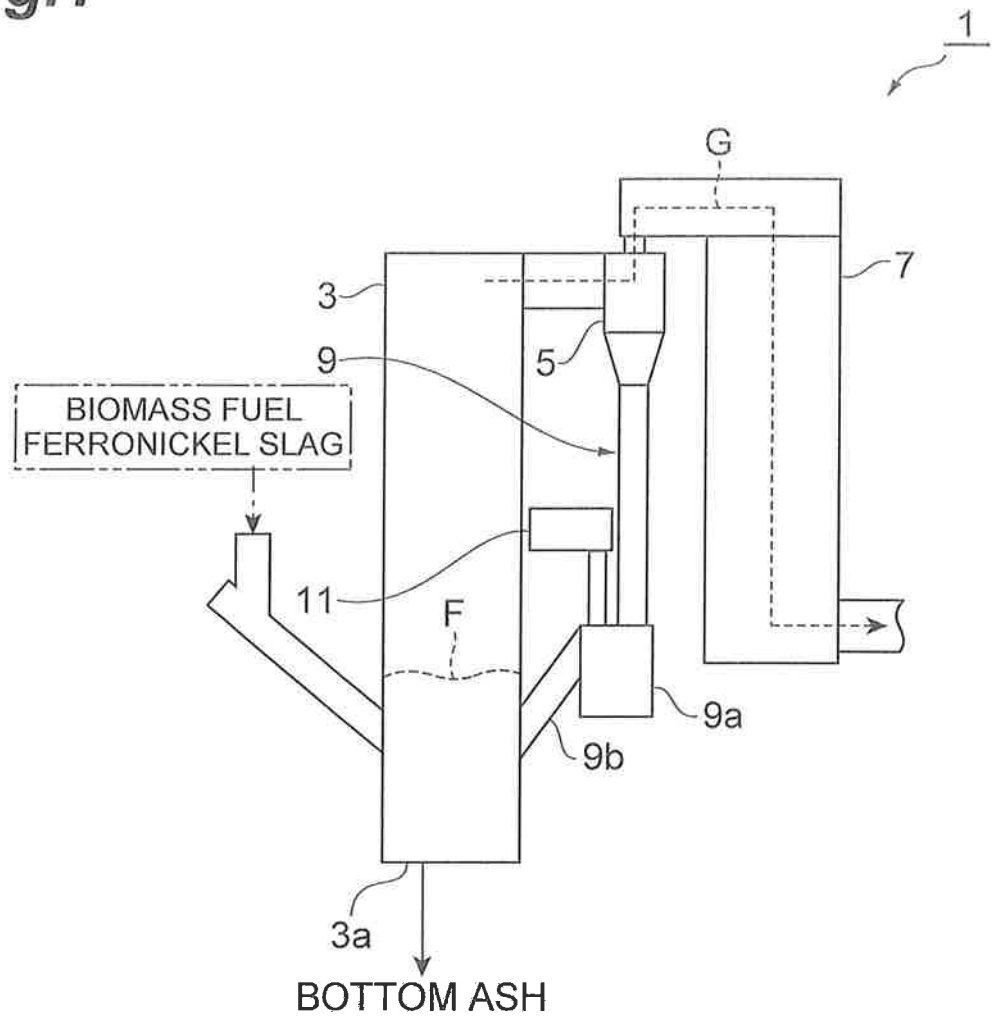
Fig.1


Fig.2


Fig.3


Fig.4

Fig.5

K_2O - MgO - SiO_2

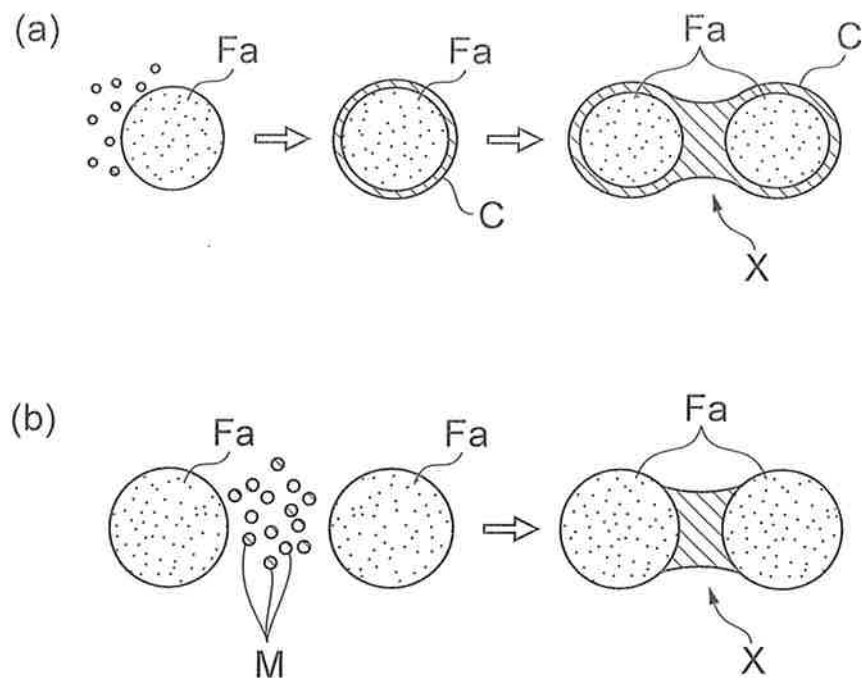


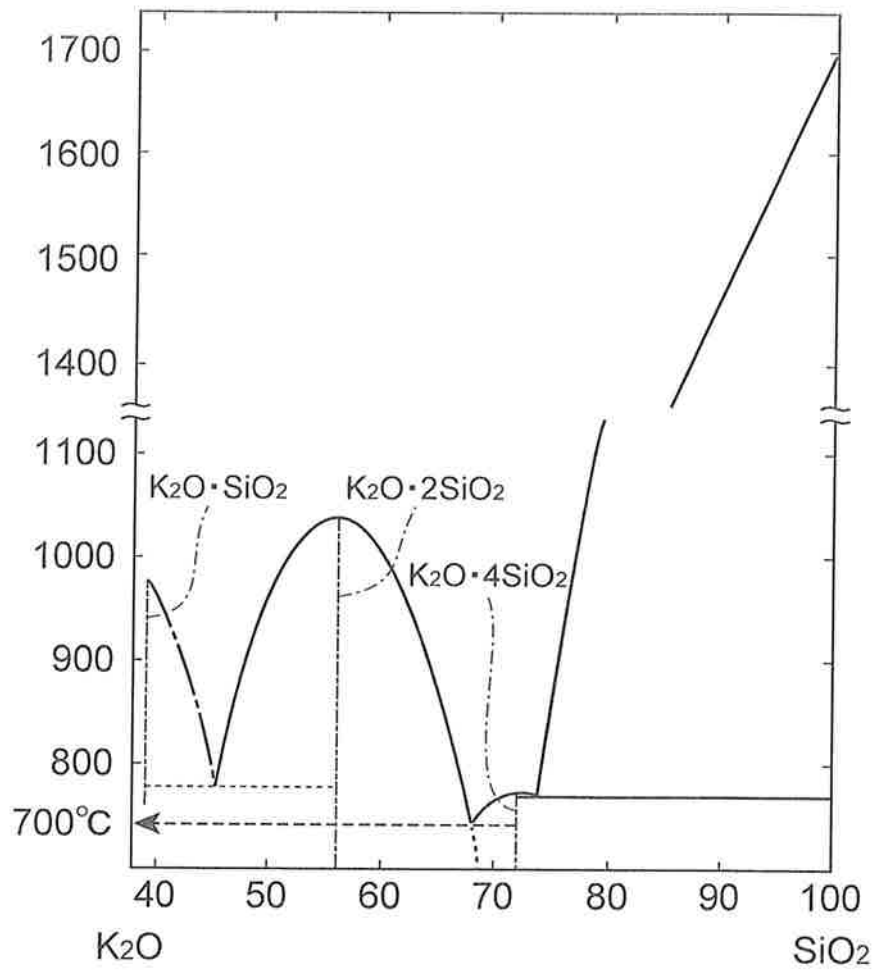
Fig.6

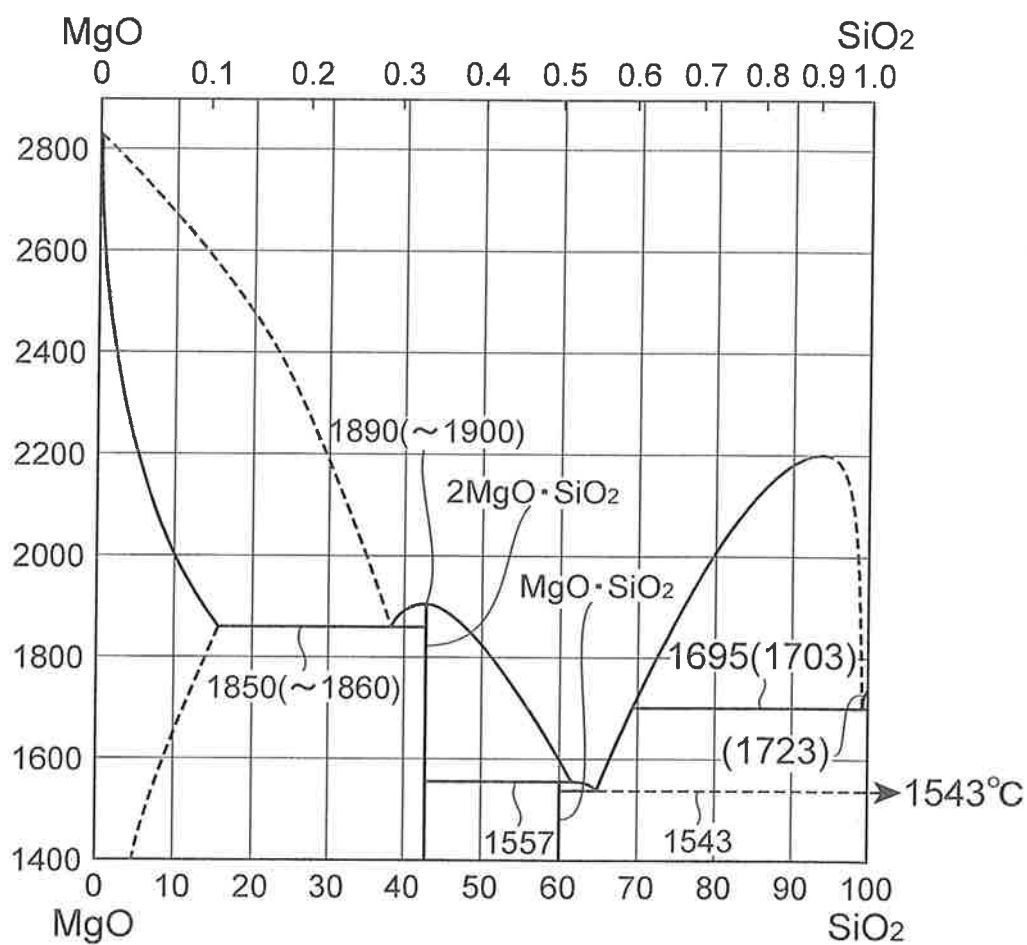Fig.7

UNIT: %

	SiO ₂	MgO	CaO	FeO	Al ₂ O ₃
SAMPLE A	56.0	28.1	4.7	8.0	1.9
SAMPLE B	53.5	35.5	0.7	4.5	1.5
SAMPLE C	50~55	32~34	0.5~1.0	5~10	1.5~2.0

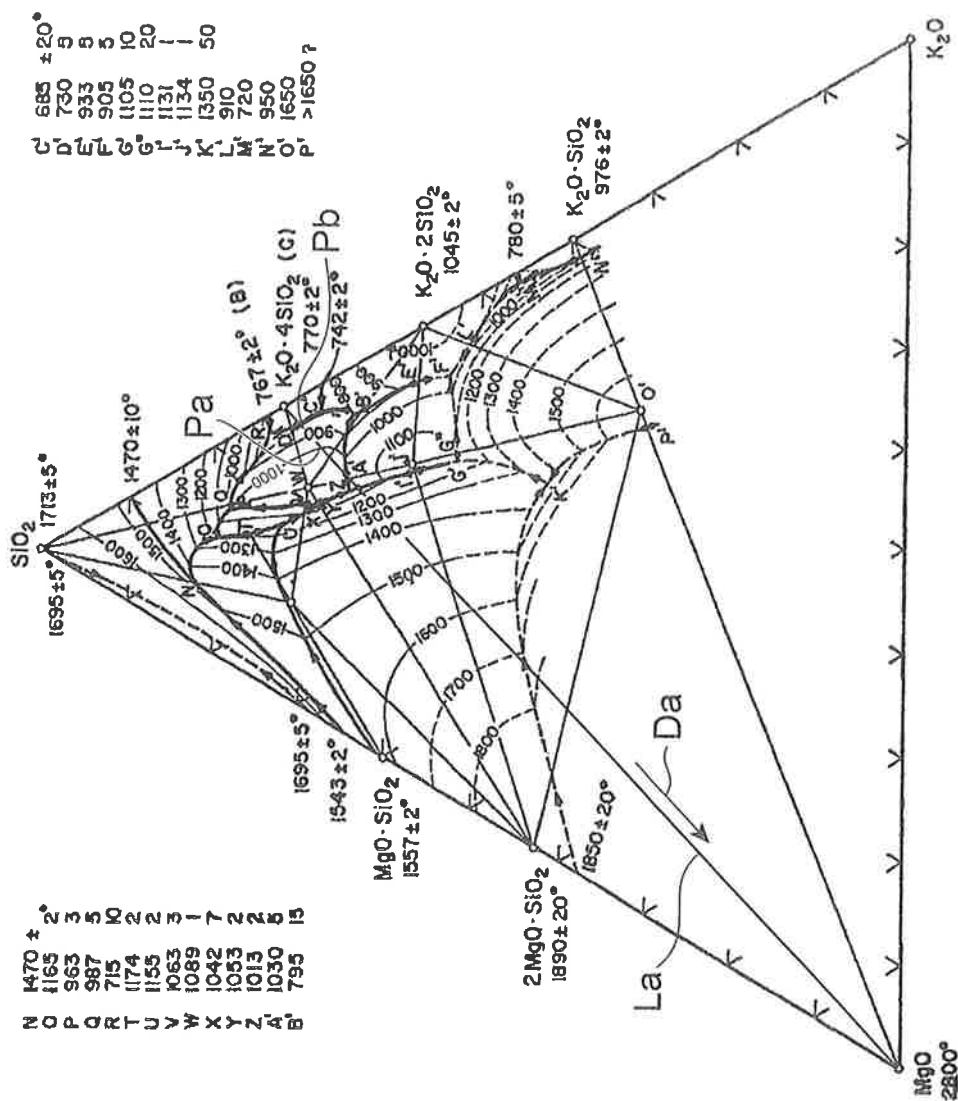Fig.8

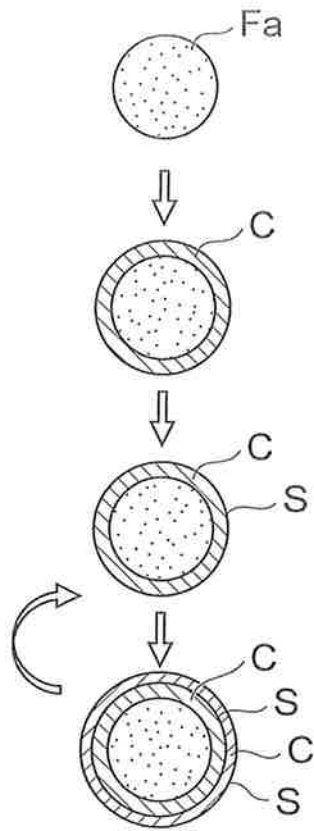