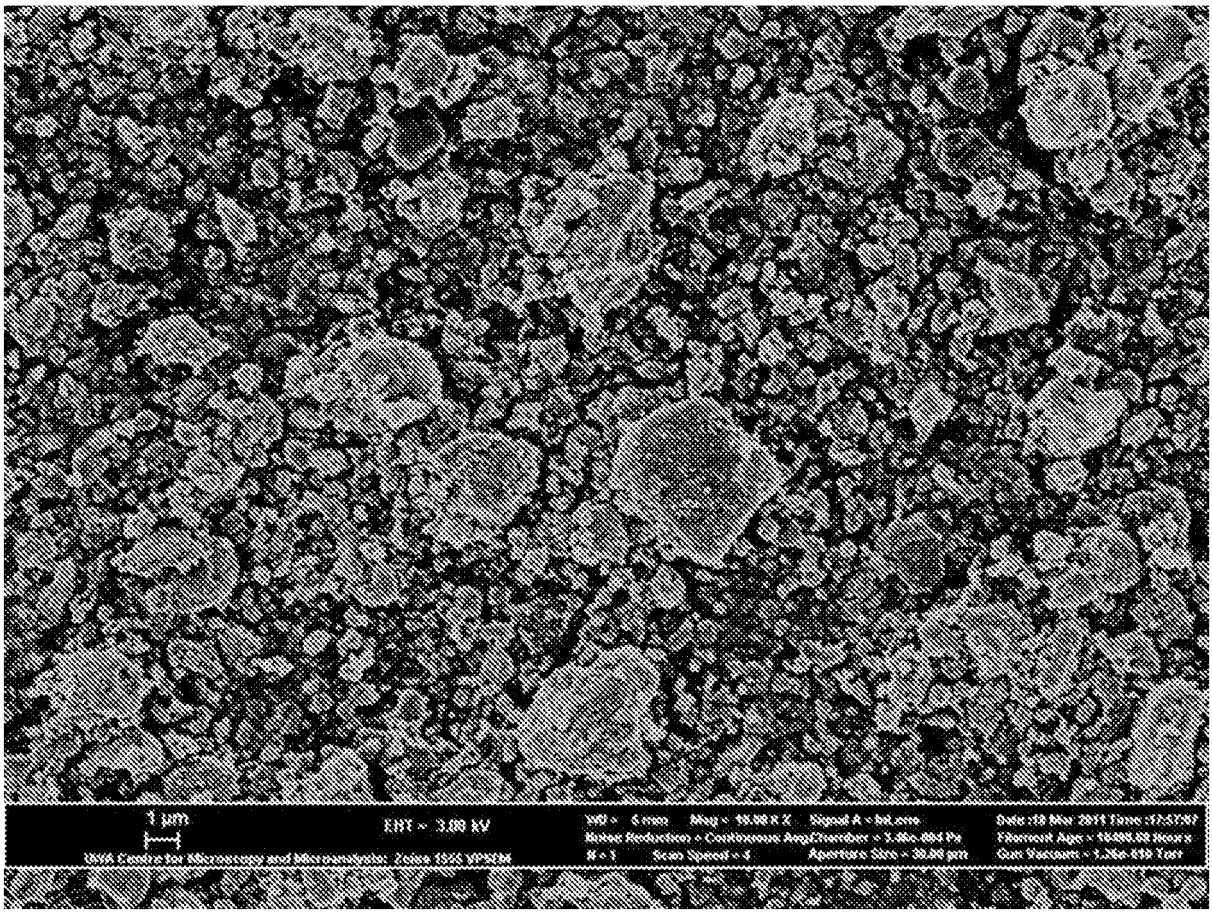


FIGURE 1

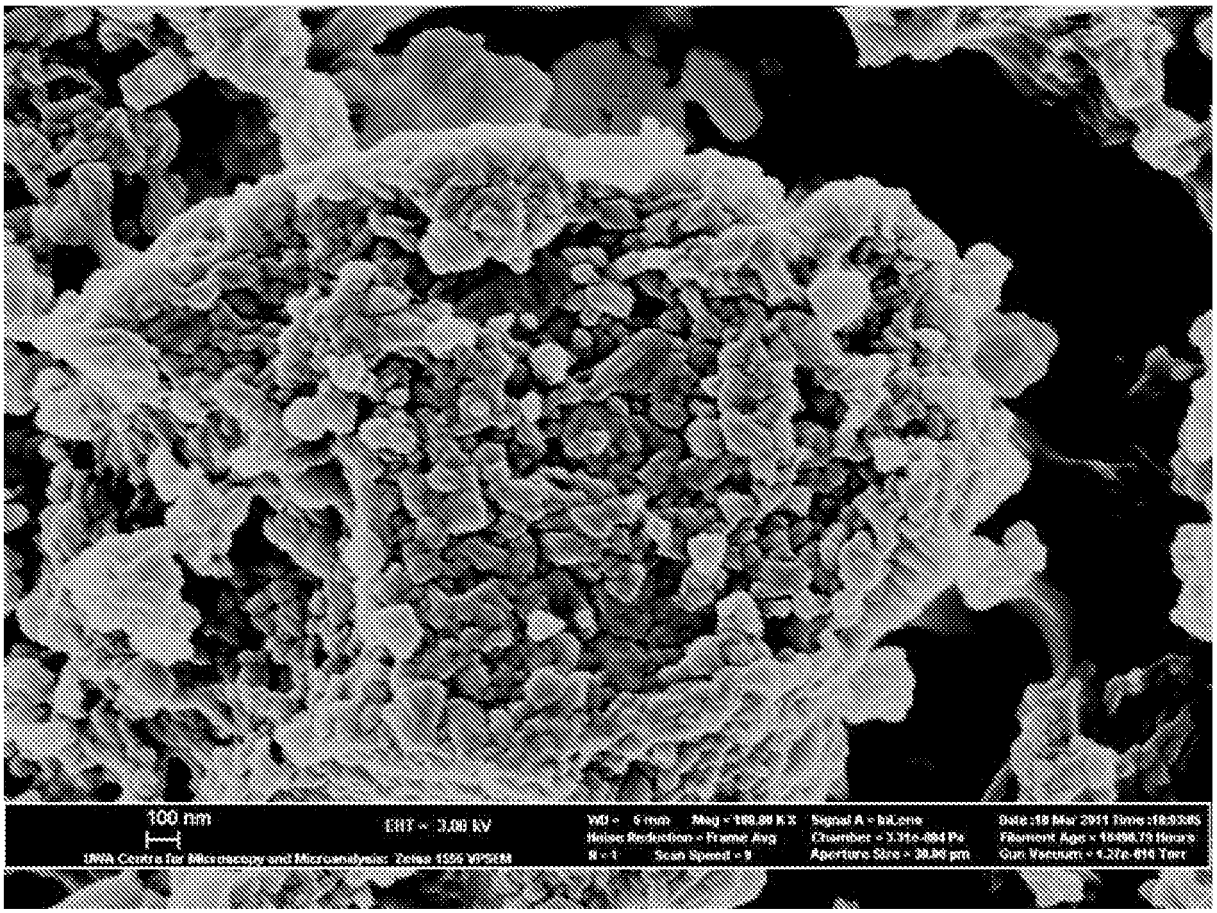

100 nm
EHT = 3.00 kV
WD = 6 mm Mag = 100.00 K X
Noise Reduction = Frame Avg
Scan Speed = 9
Signal A = InLens
Chamber = 3.31e-004 Pa
Aperture Size = 30.00 µm
Date :18 Mar 2011 Time :18:03:05
Gun Vacuum = 4.27e-010 Torr

FIGURE 2