
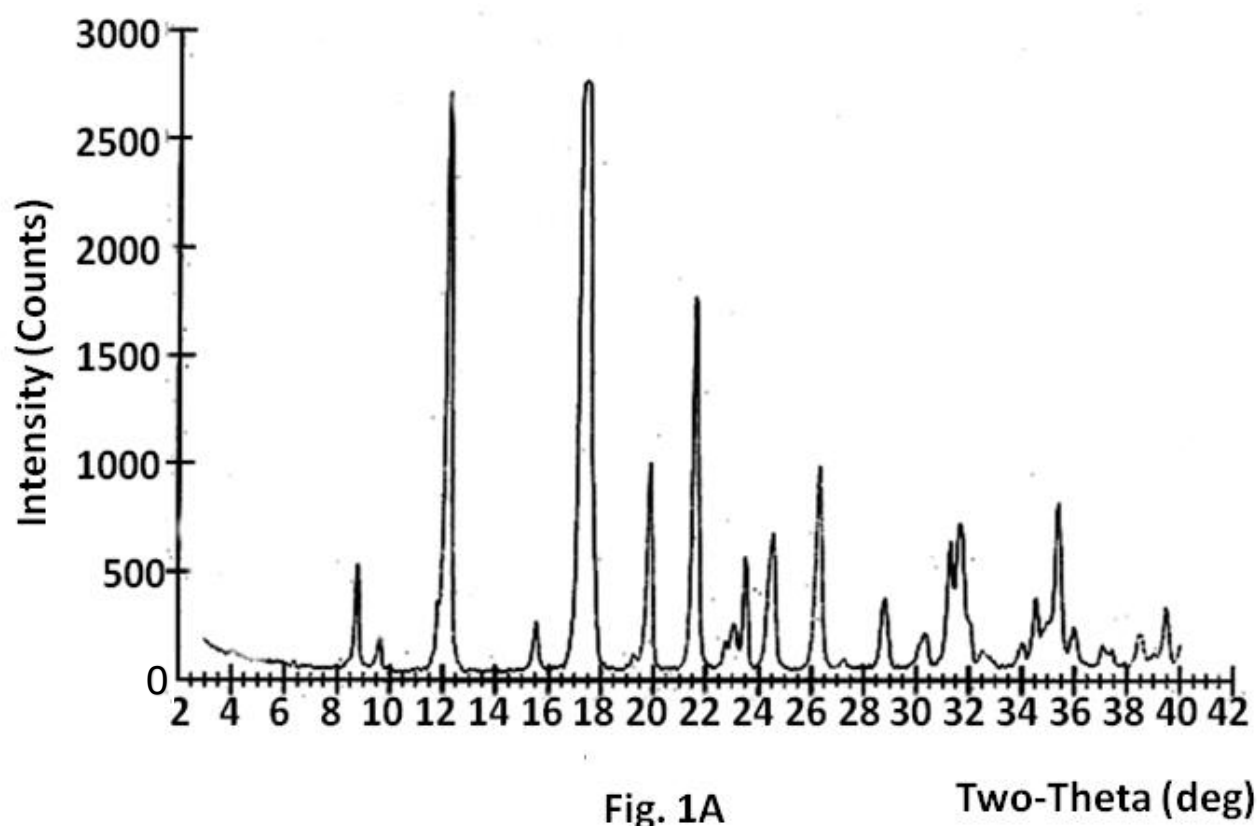
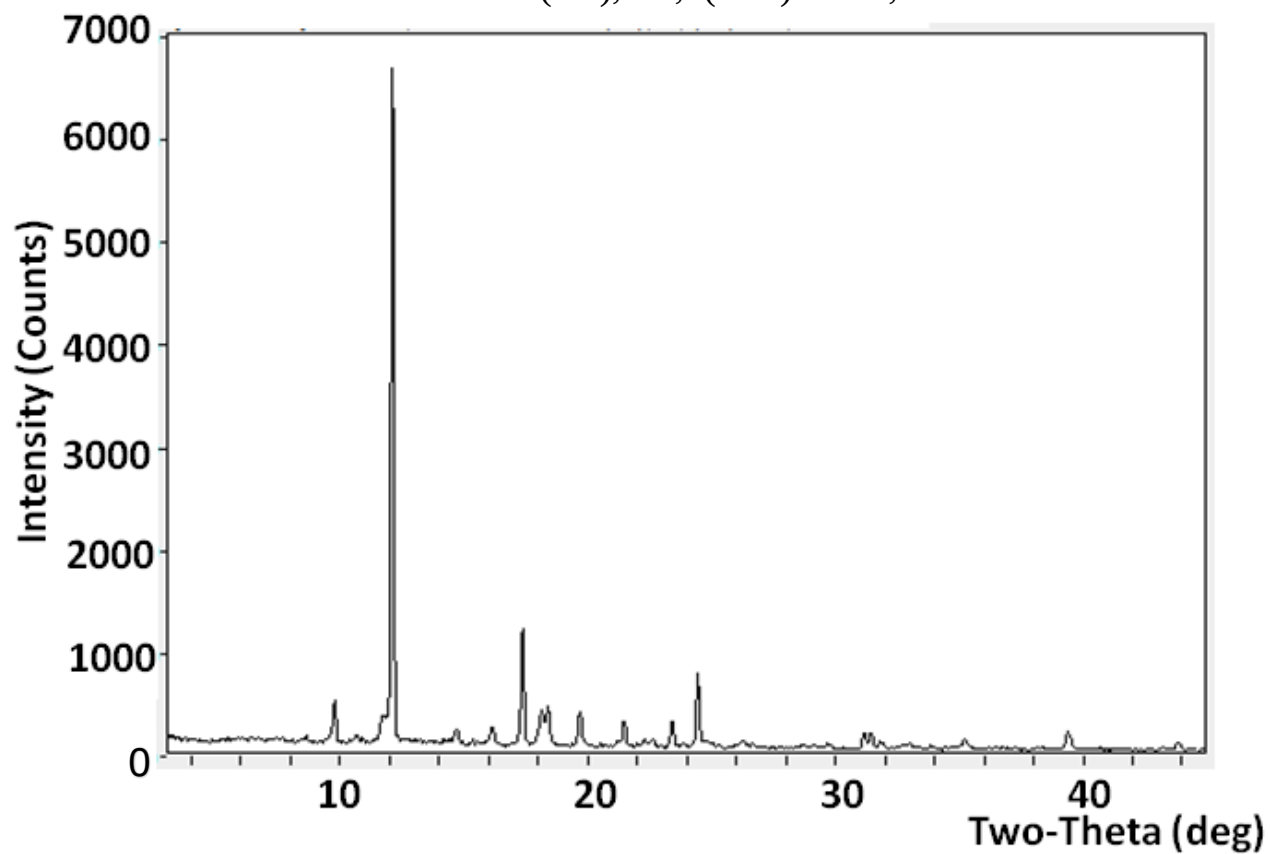


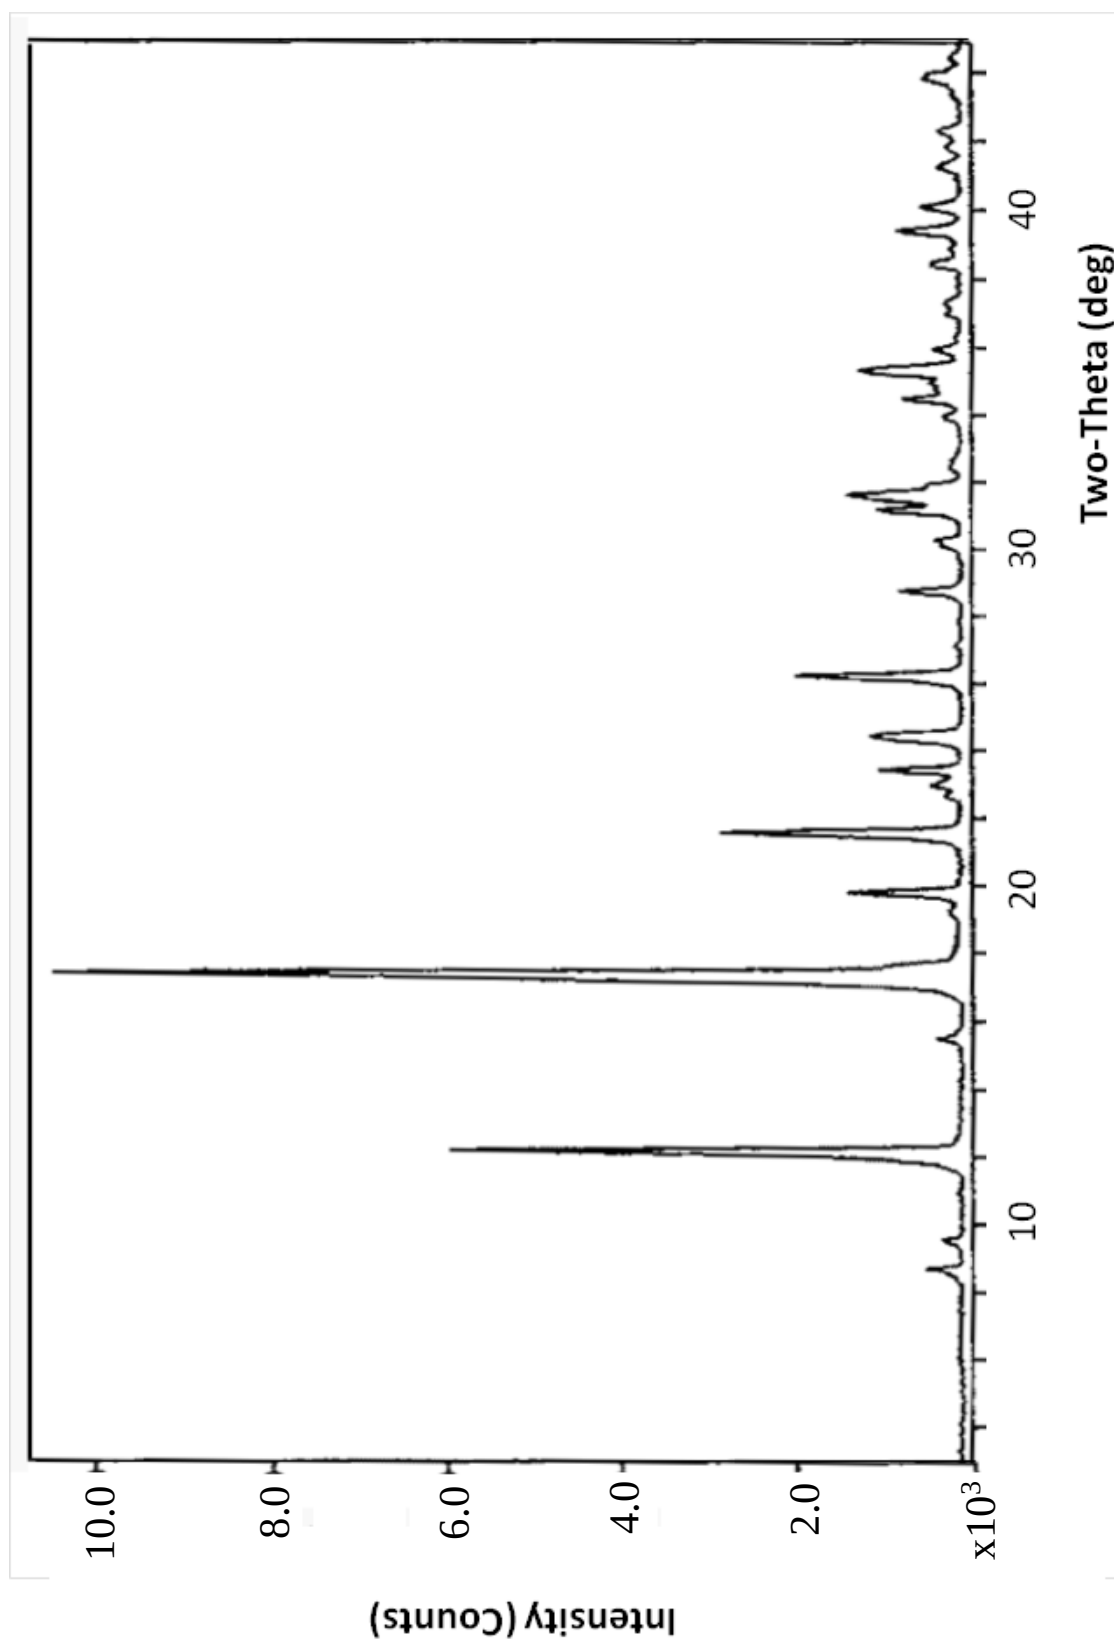

Scan: 3.0/45.0/0.02/0.6(sec), Cu, I(max)=6709, 10/03/05 10:38a



**Fig. 2**

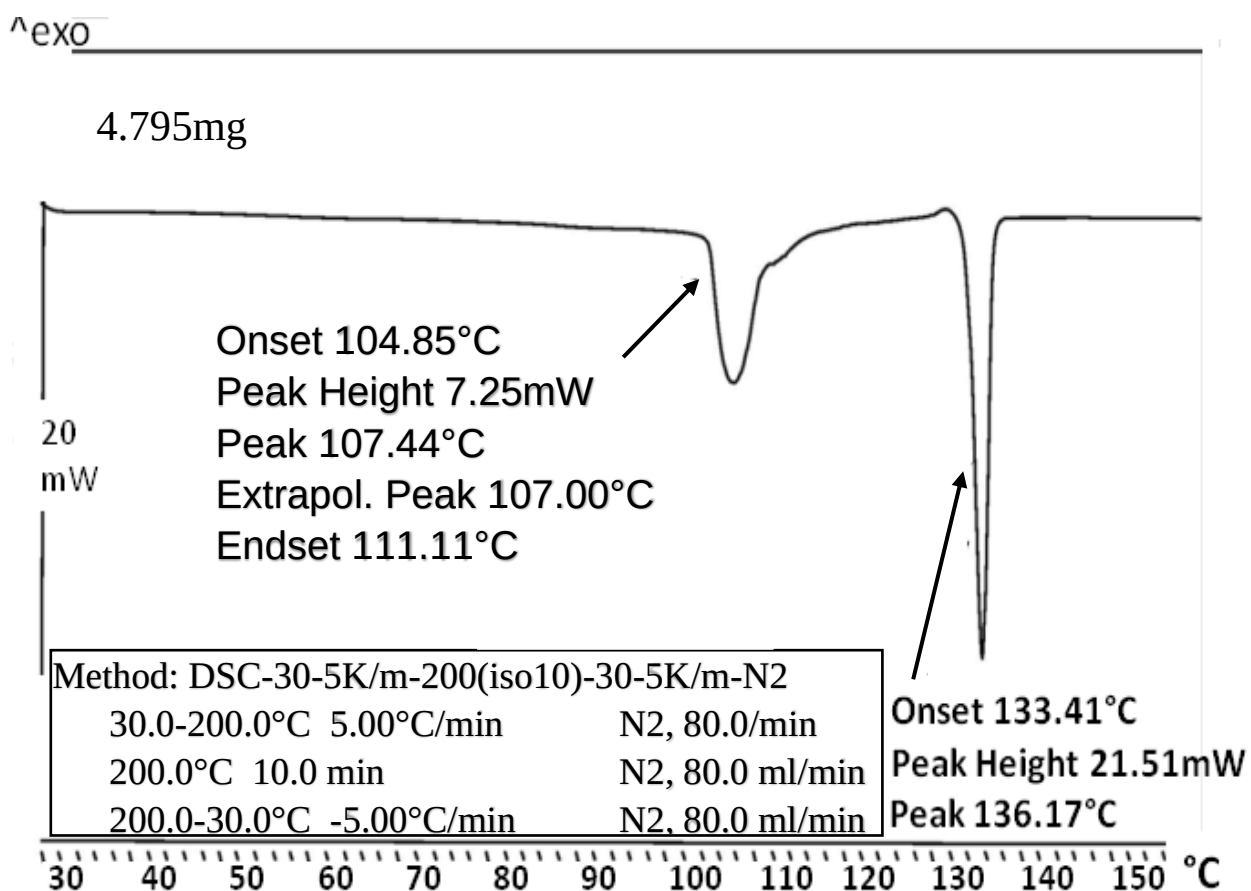


Fig. 3A


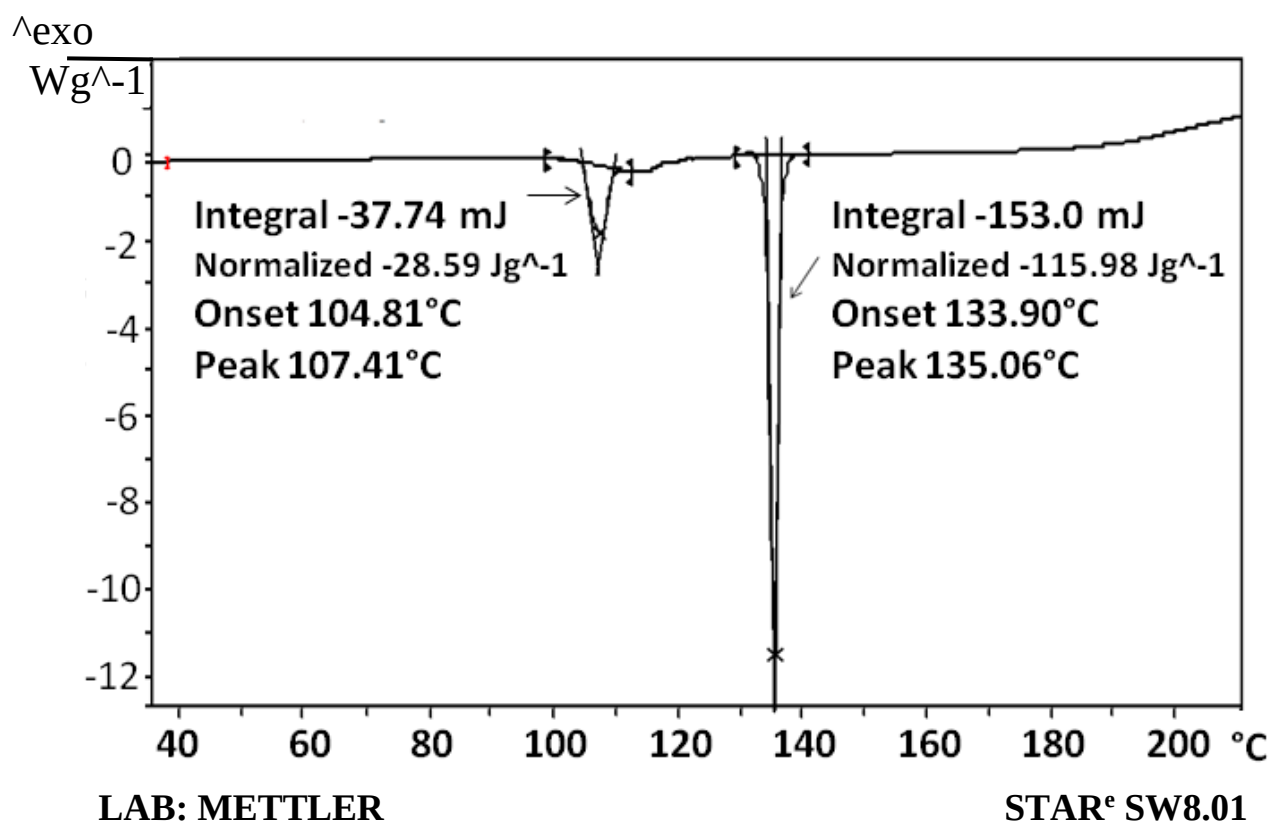


Fig. 3B

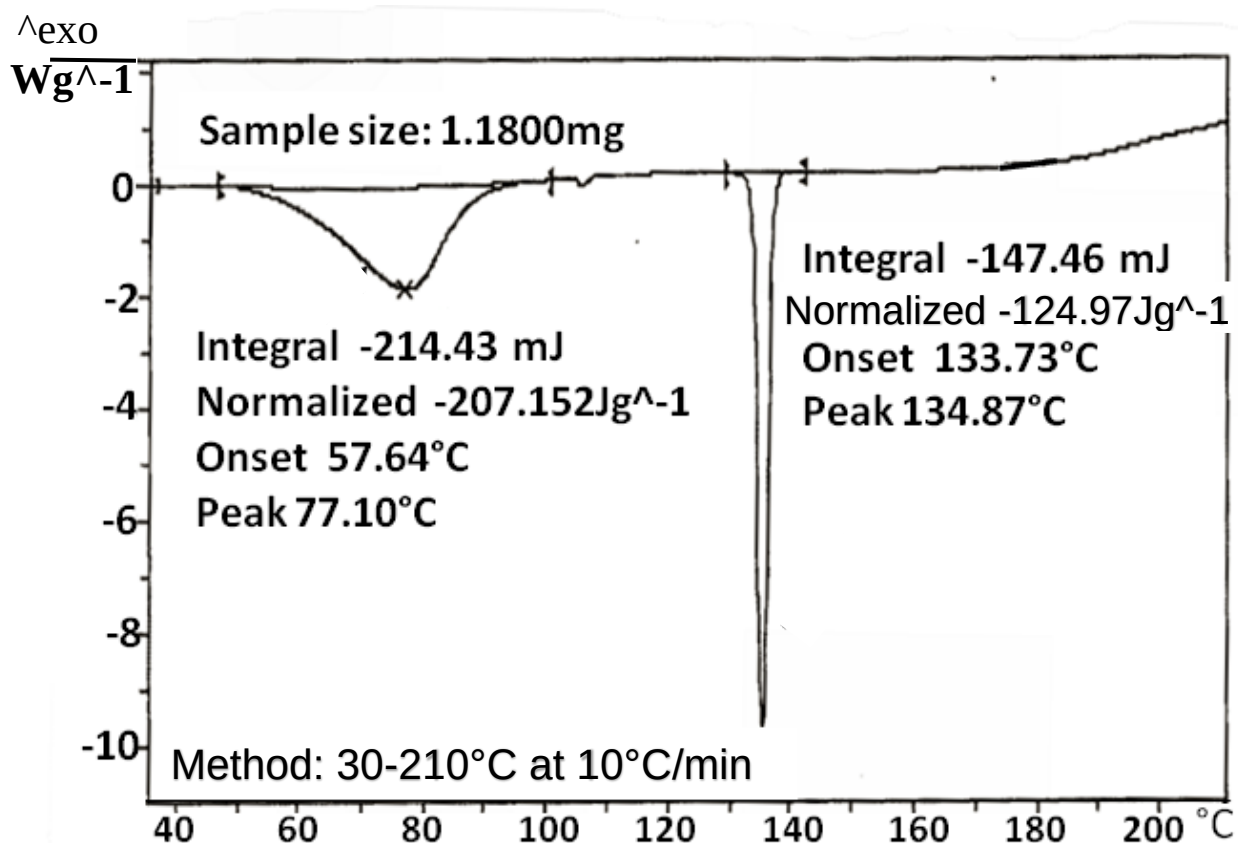

LAB: METTLER

STAR^e SW8.01

Fig. 4A

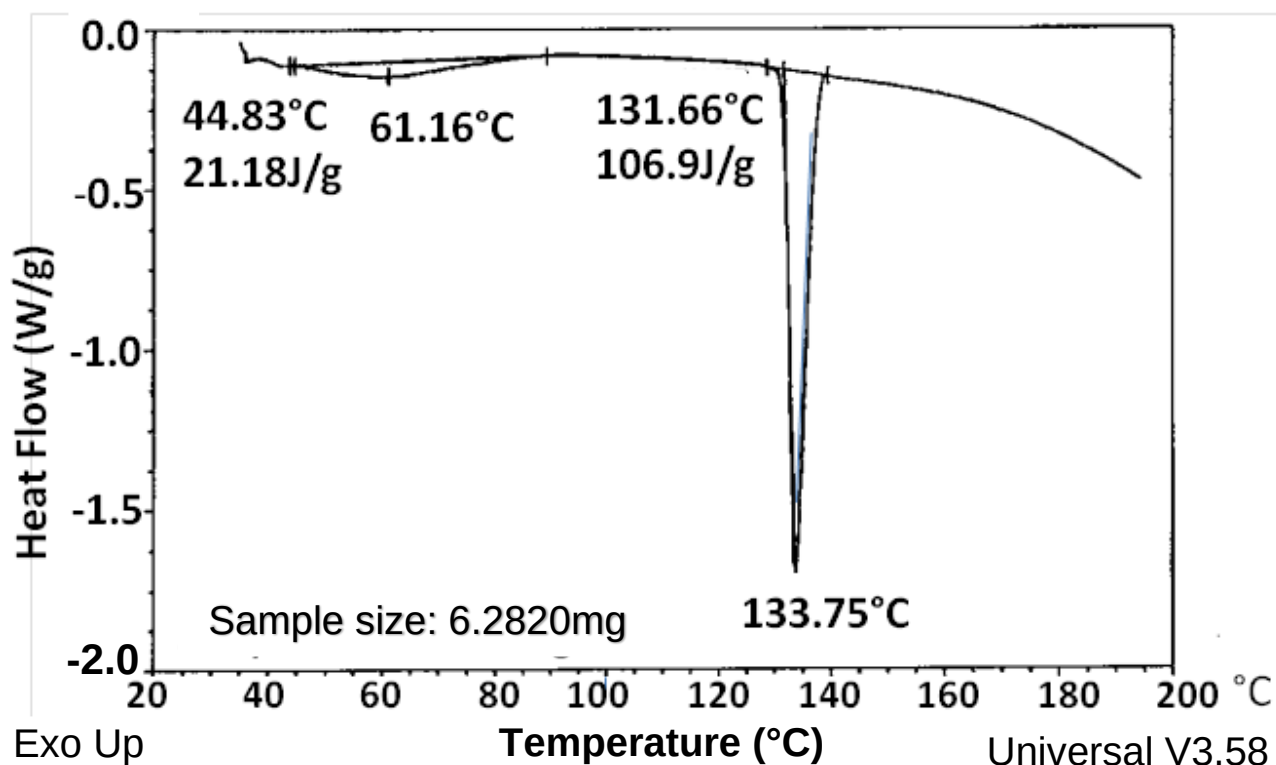
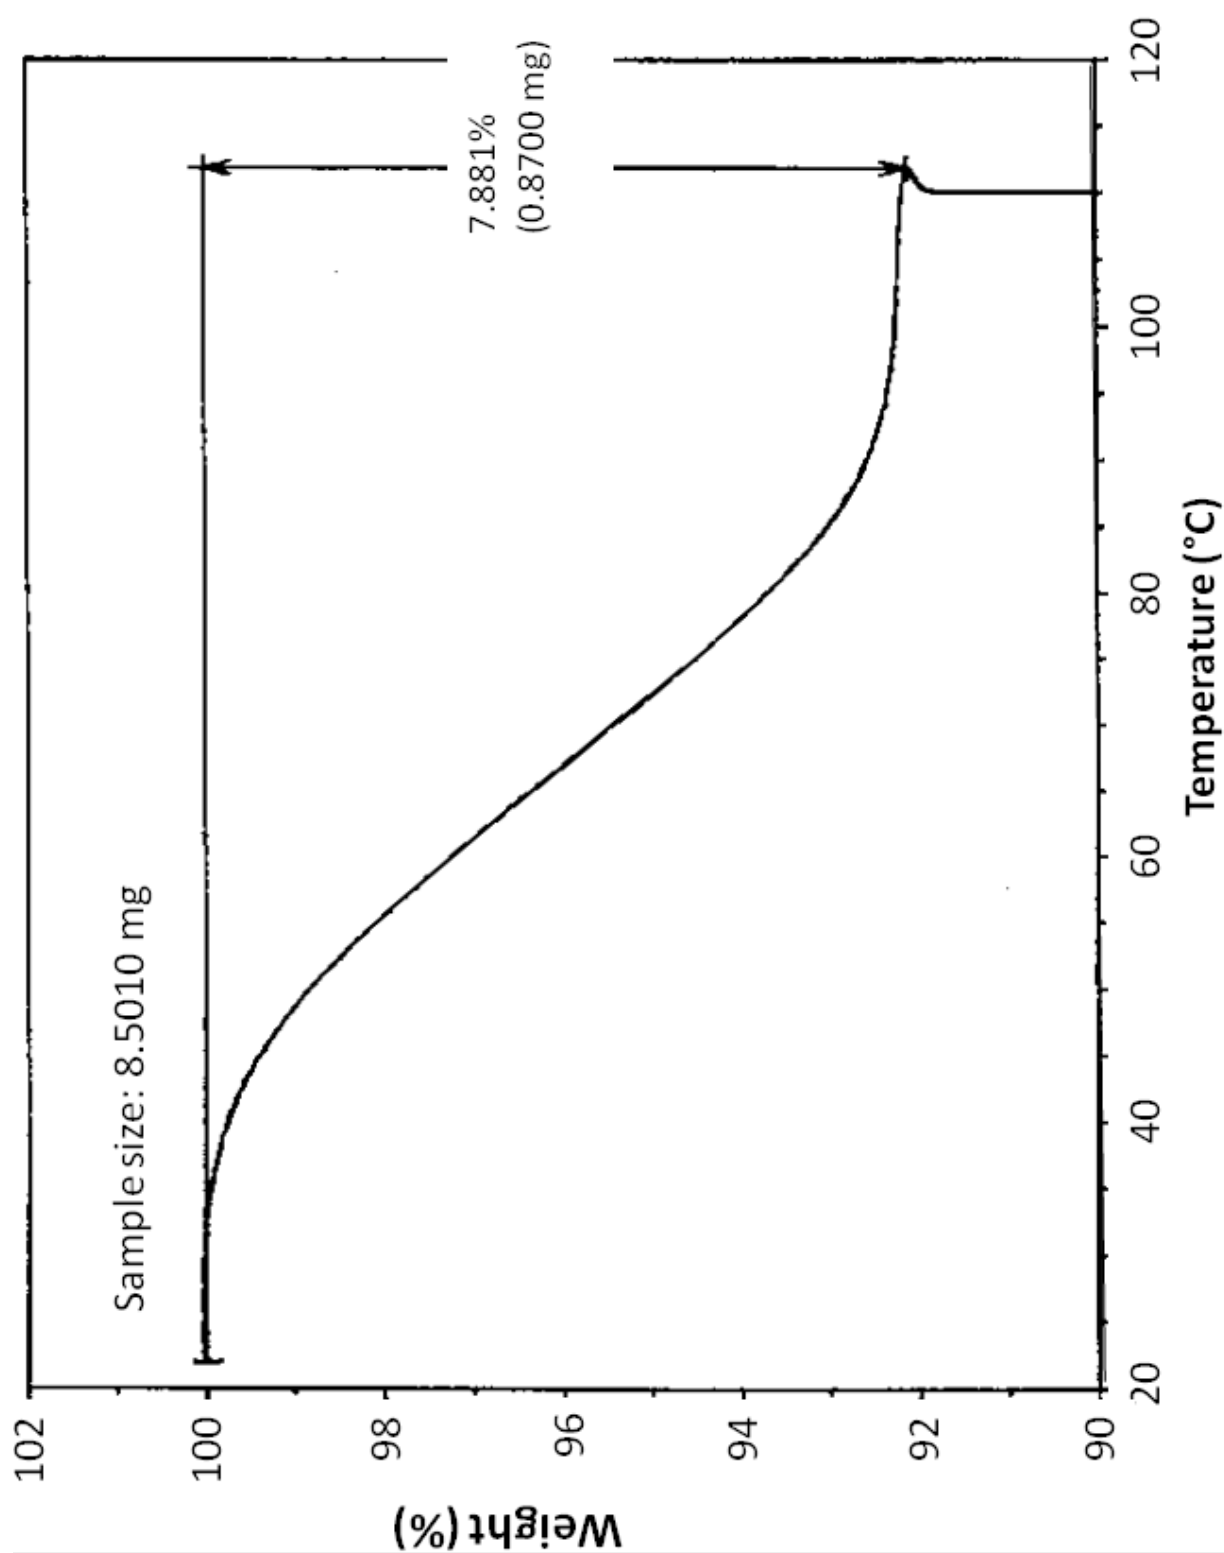


Fig. 4B

**Fig. 5**

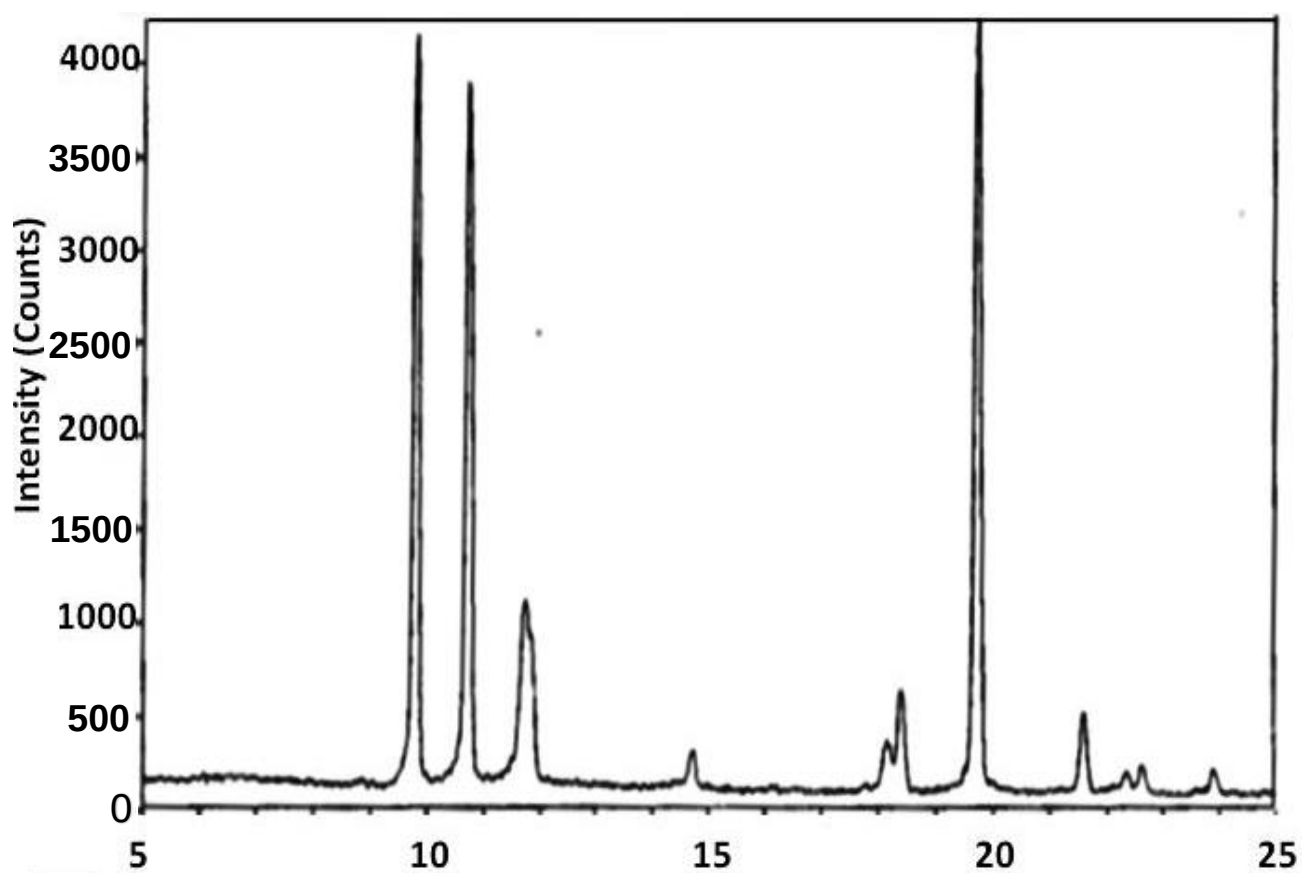


Fig. 6A

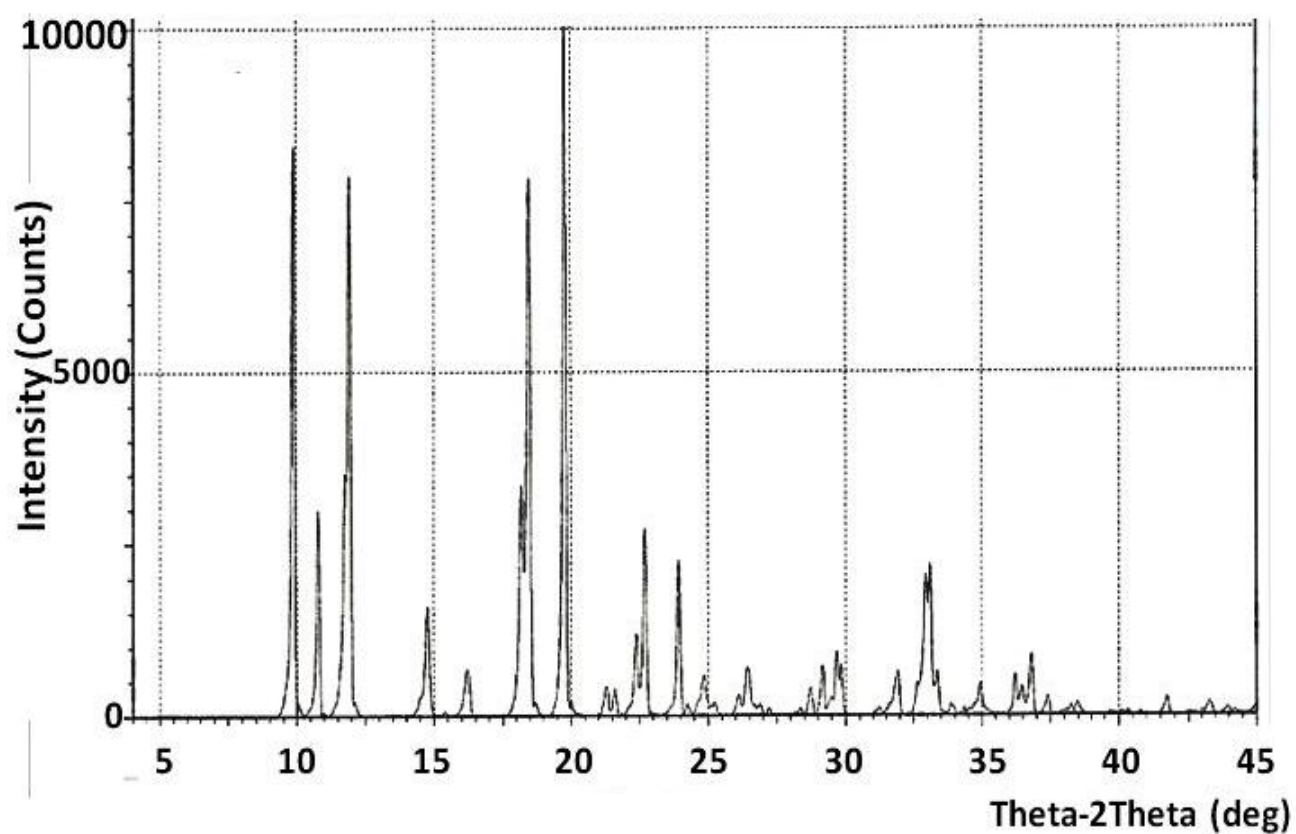


Fig. 6B


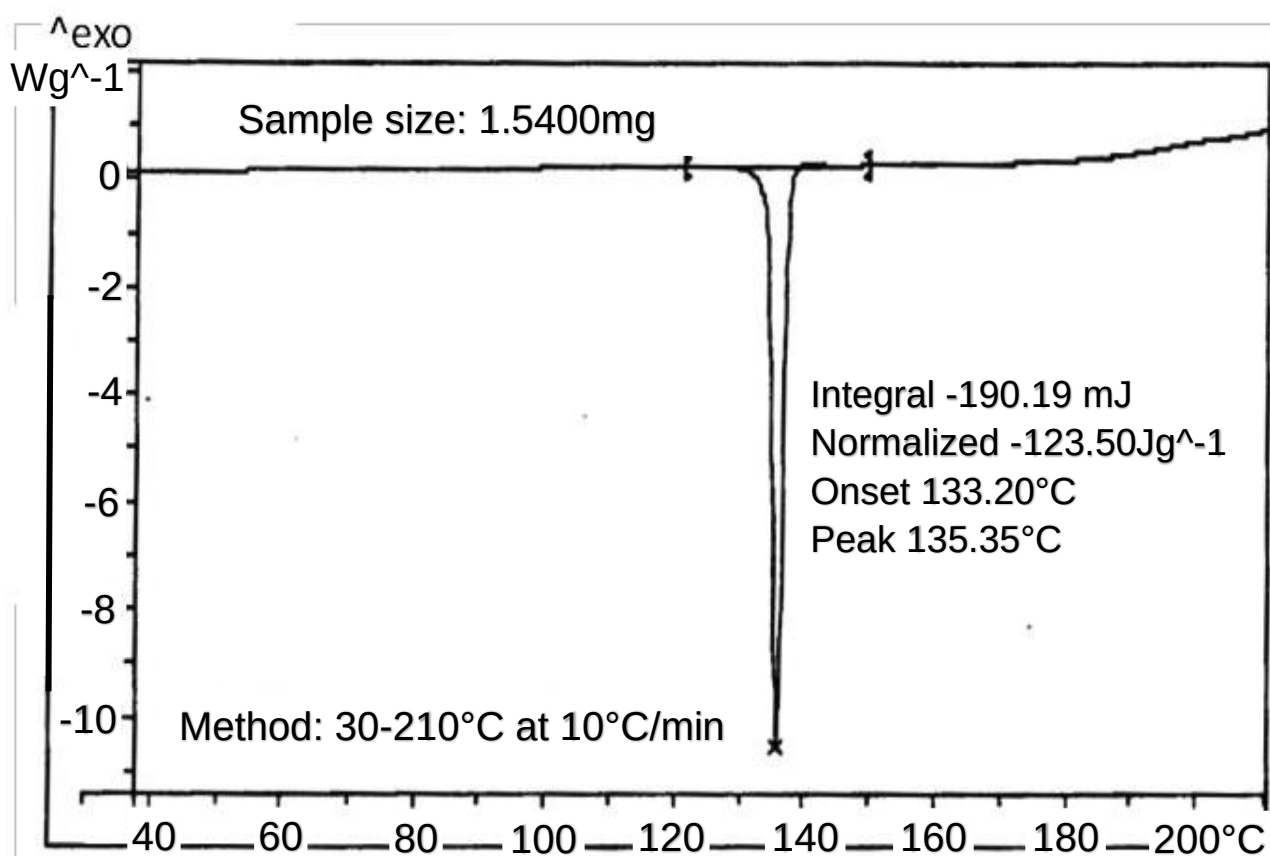


Fig. 7A

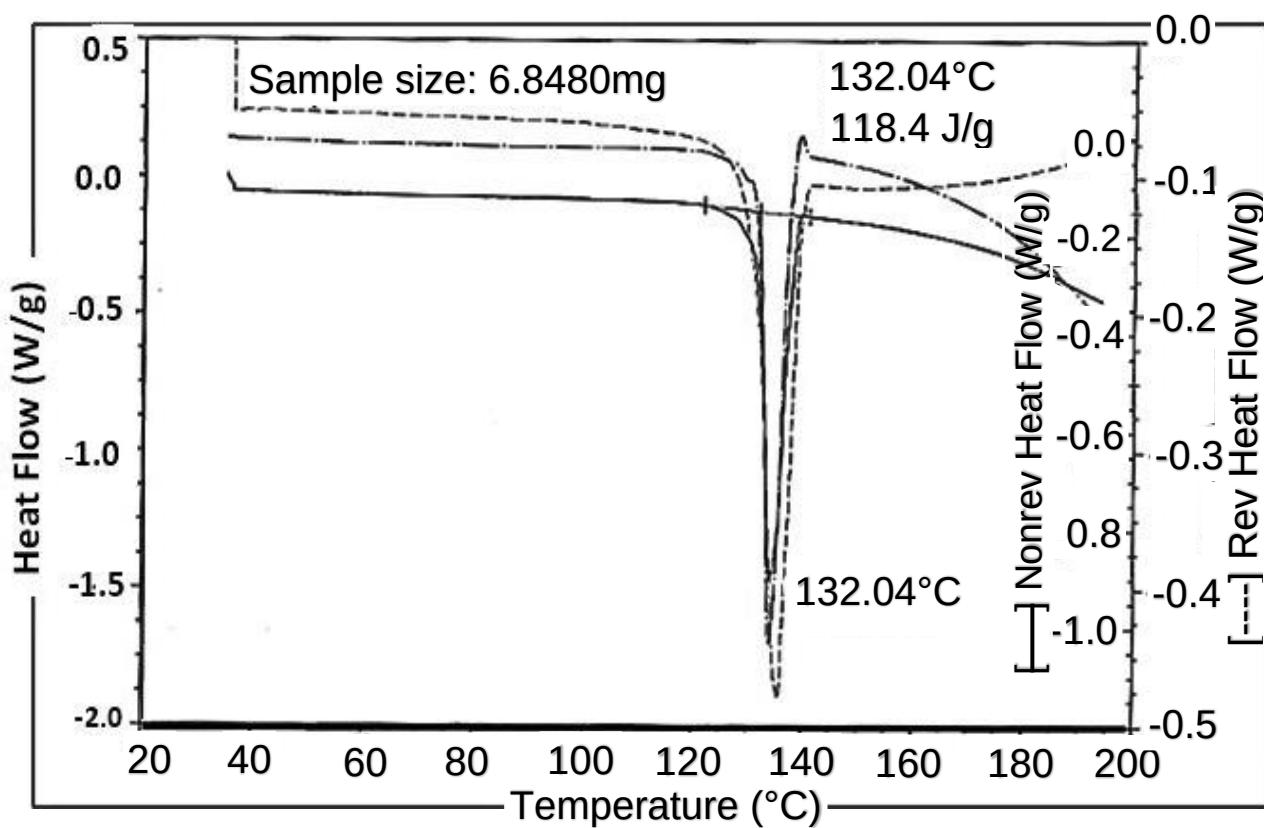

Exo Up

Universal V3.58
TA Instruments

Fig. 7B

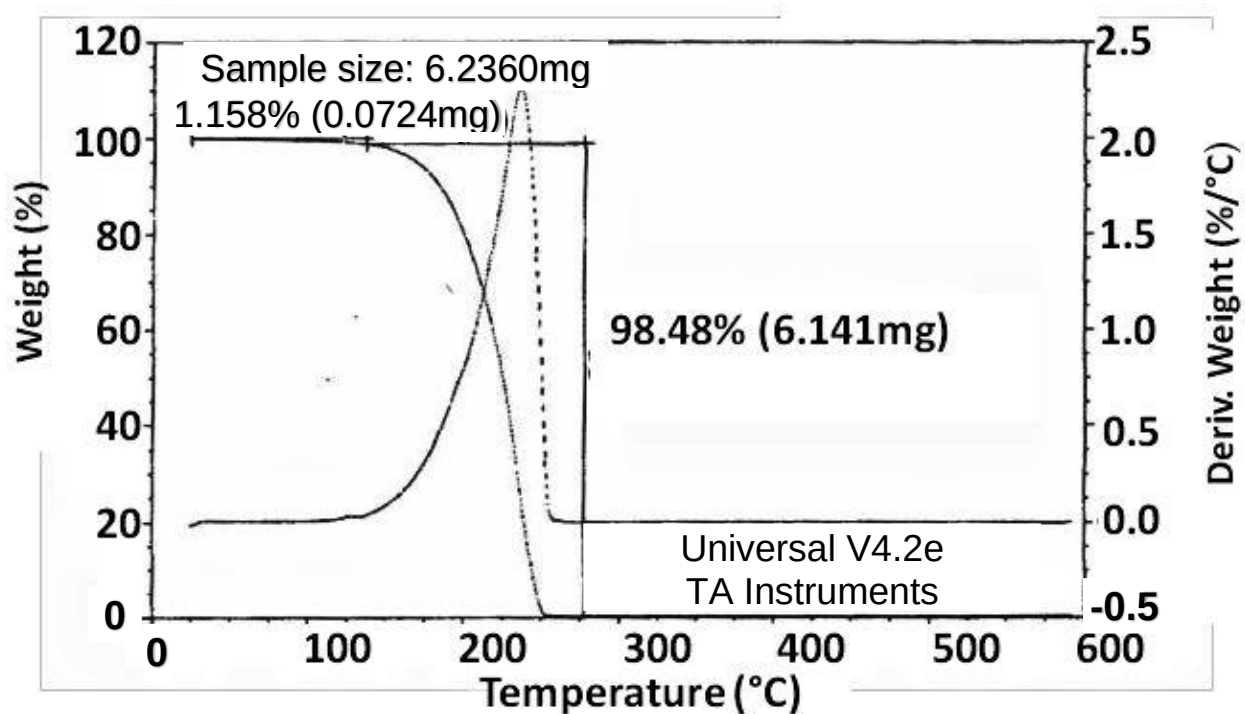


Fig. 8A

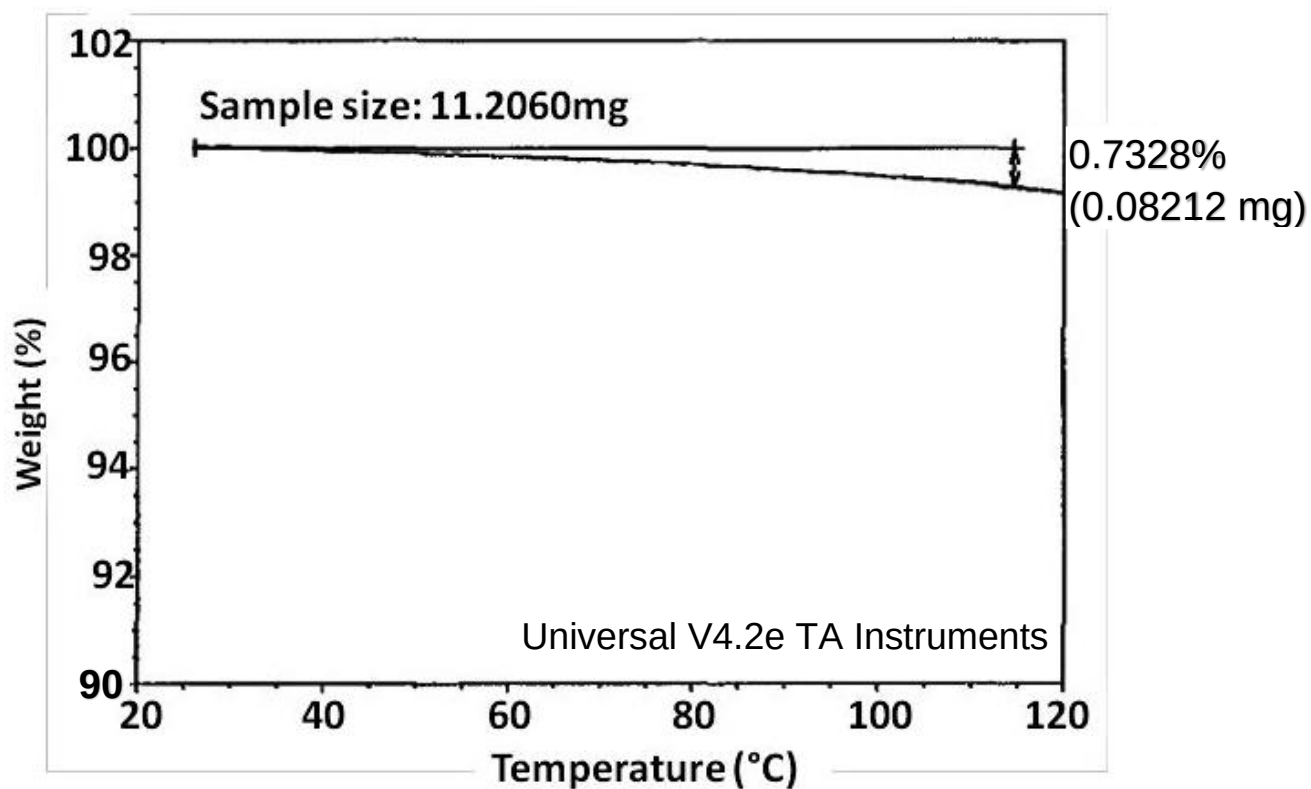
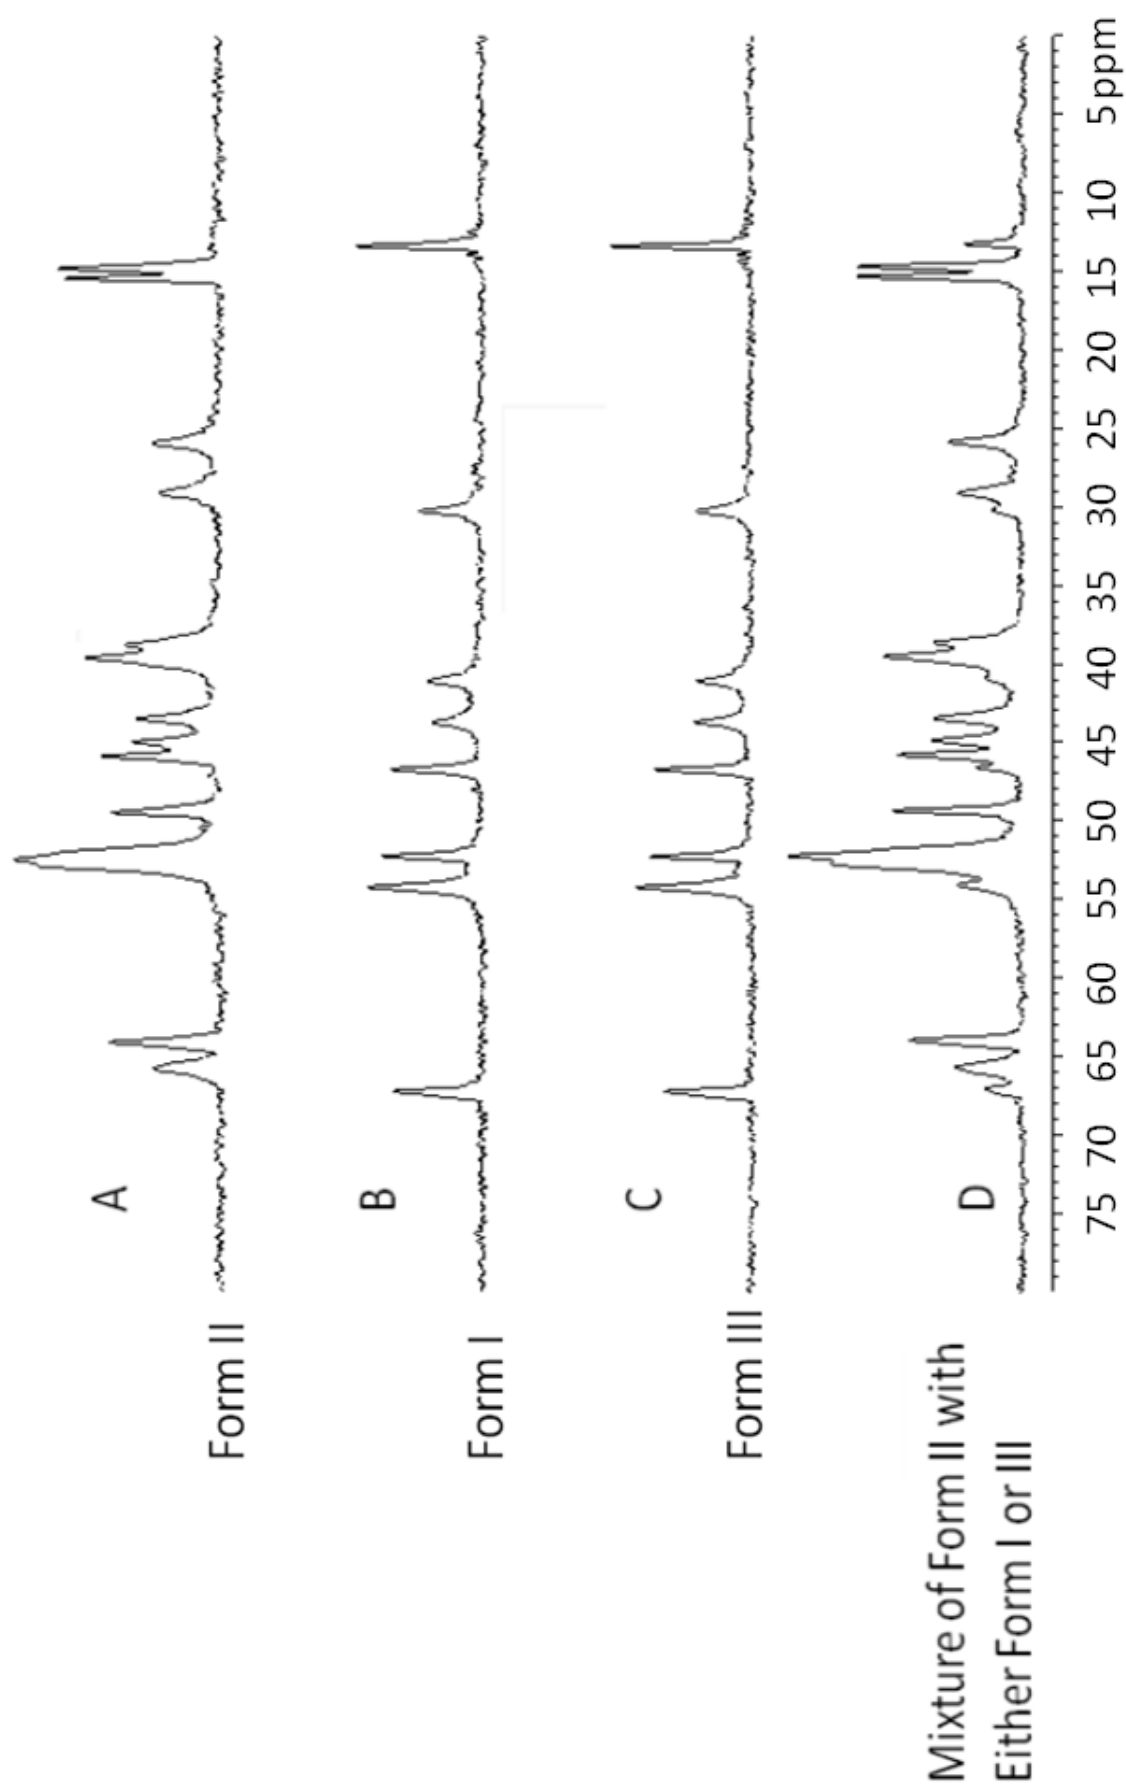


Fig. 8B

**Fig. 9**

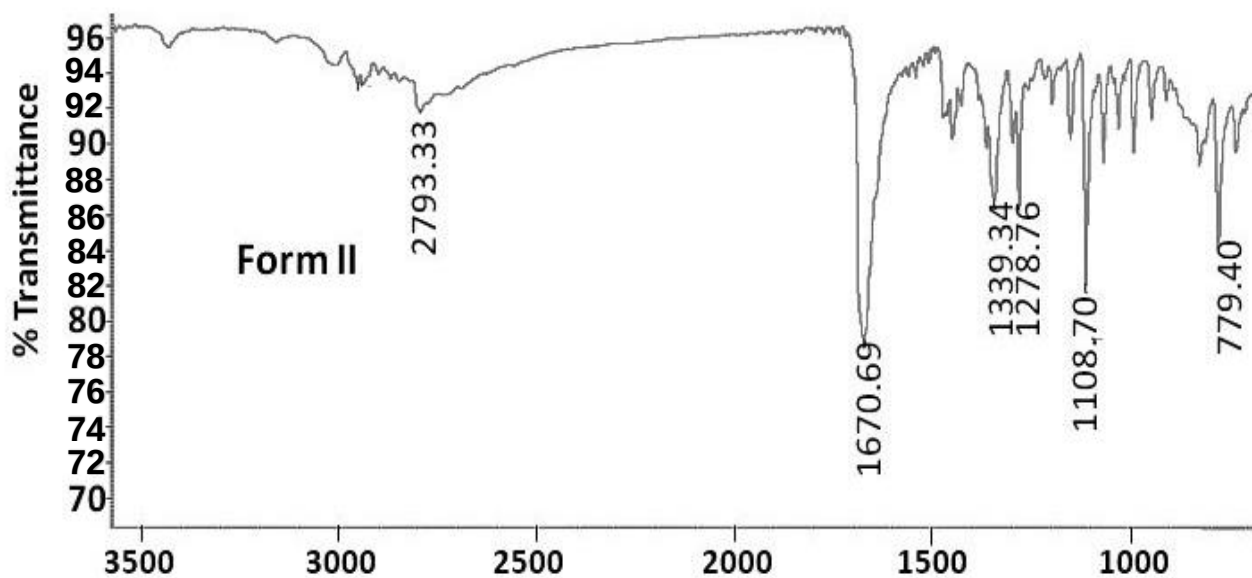
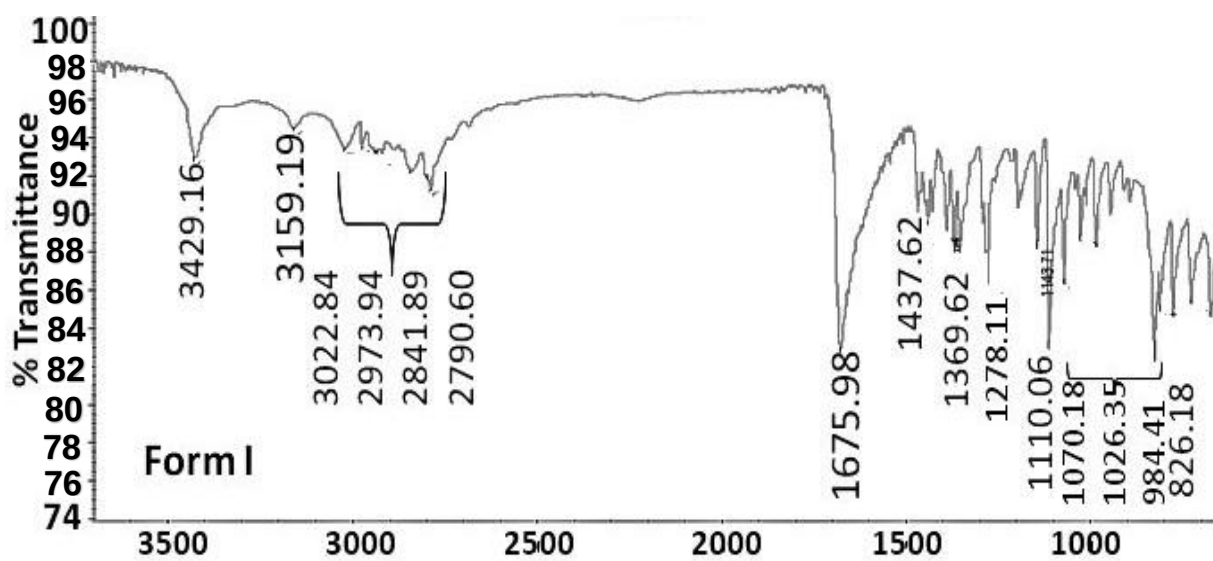


Fig. 10A

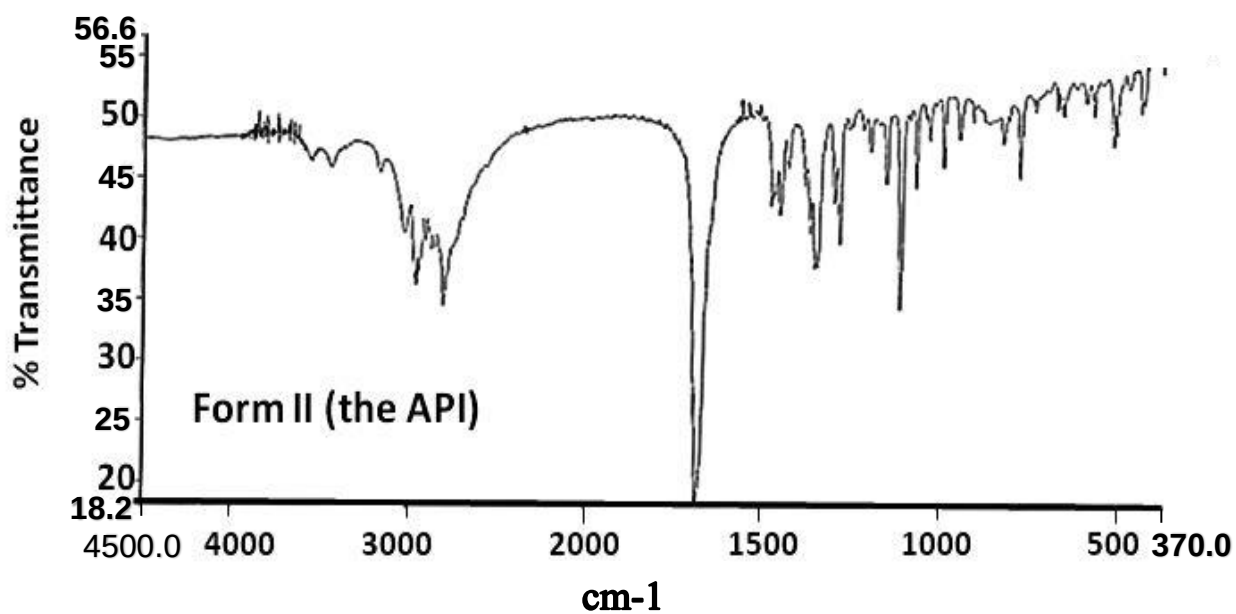


Fig. 10B

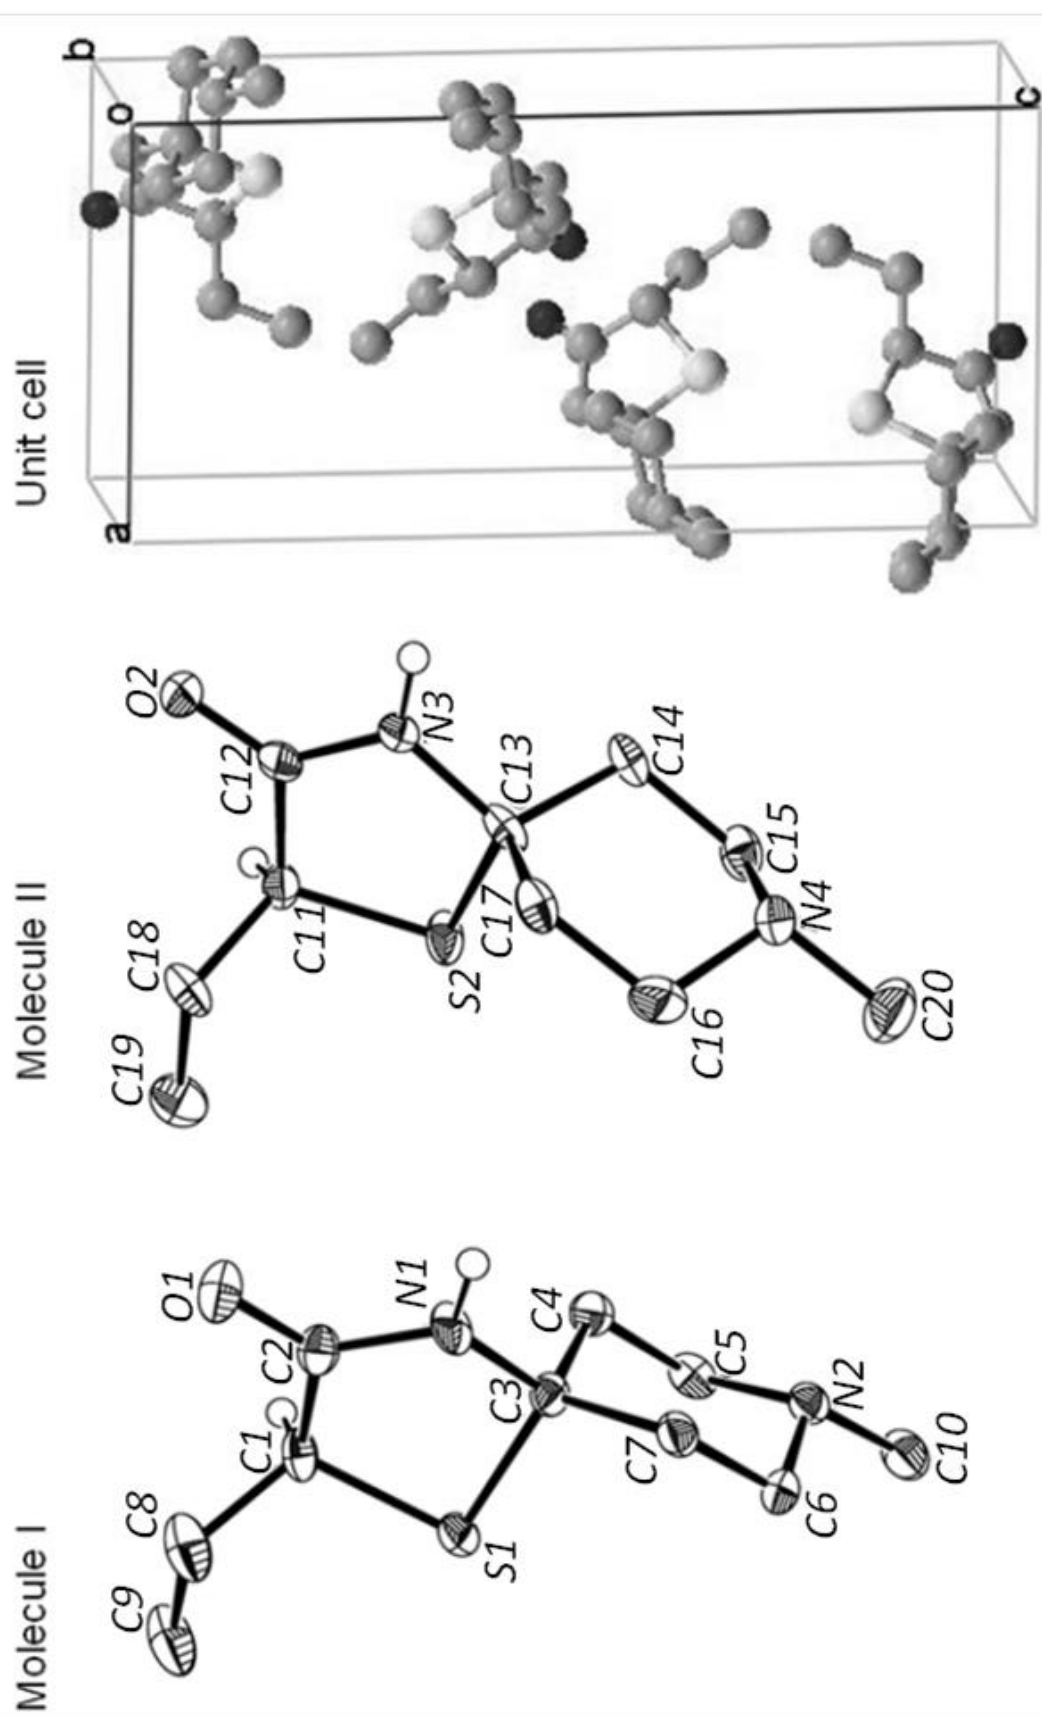


Fig. 11

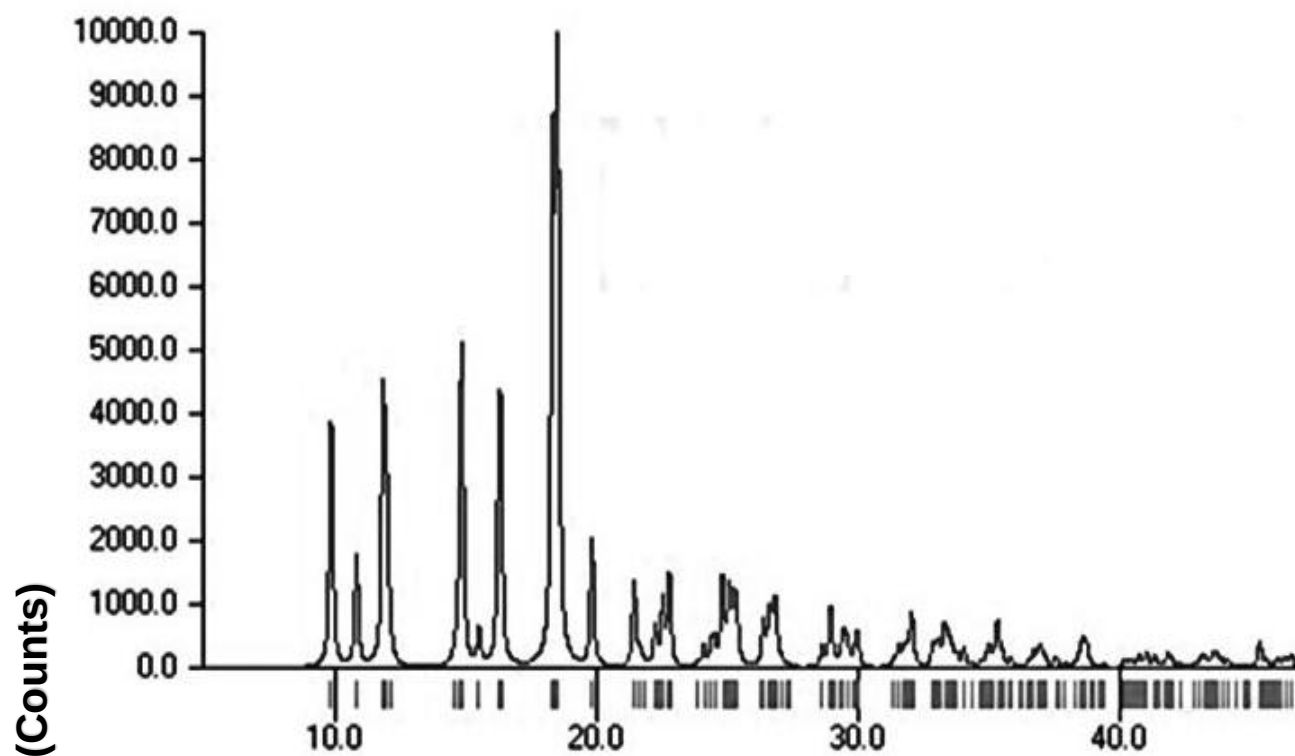


Fig. 12A

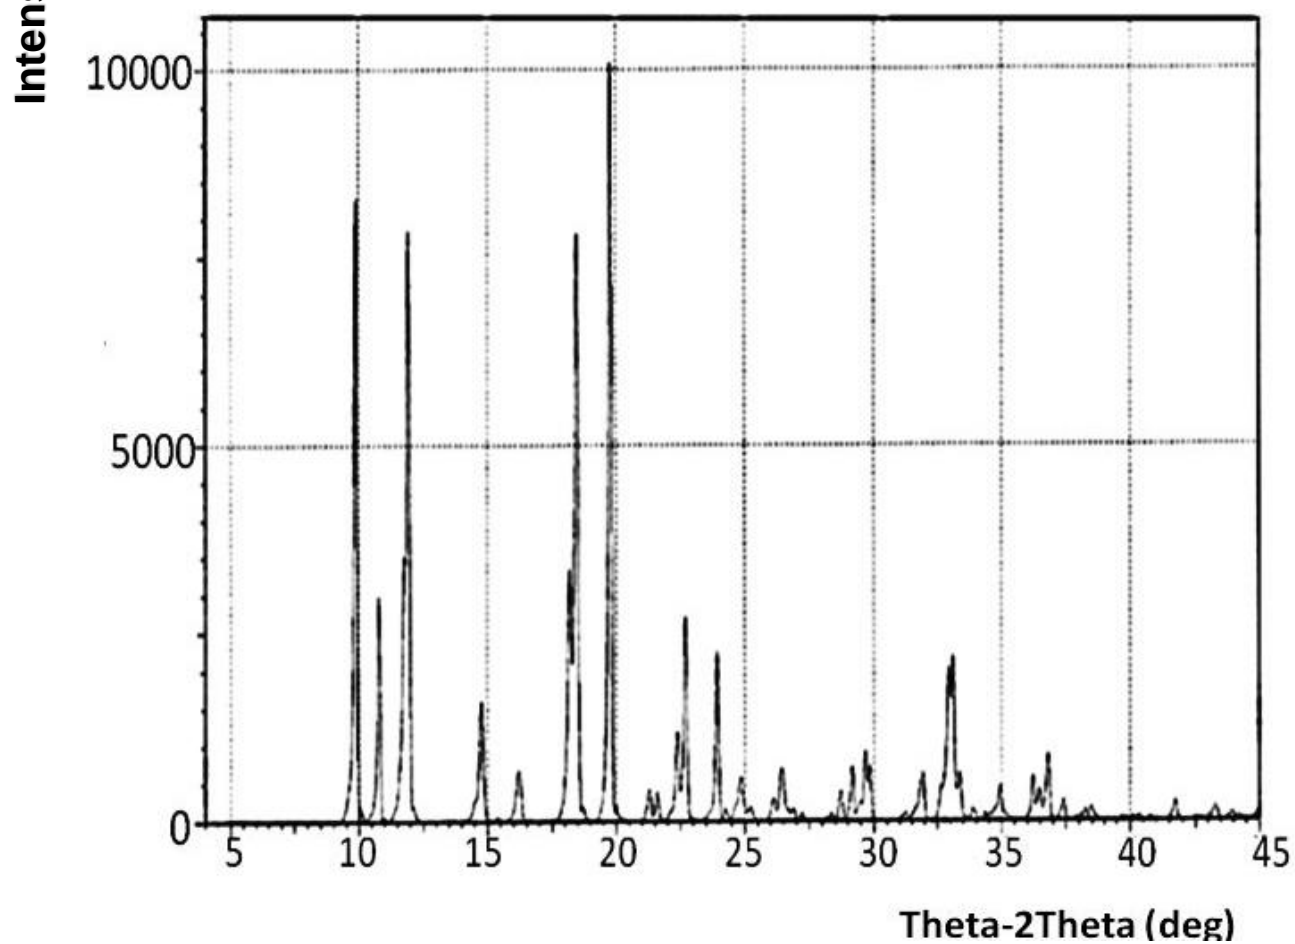


Fig. 12B

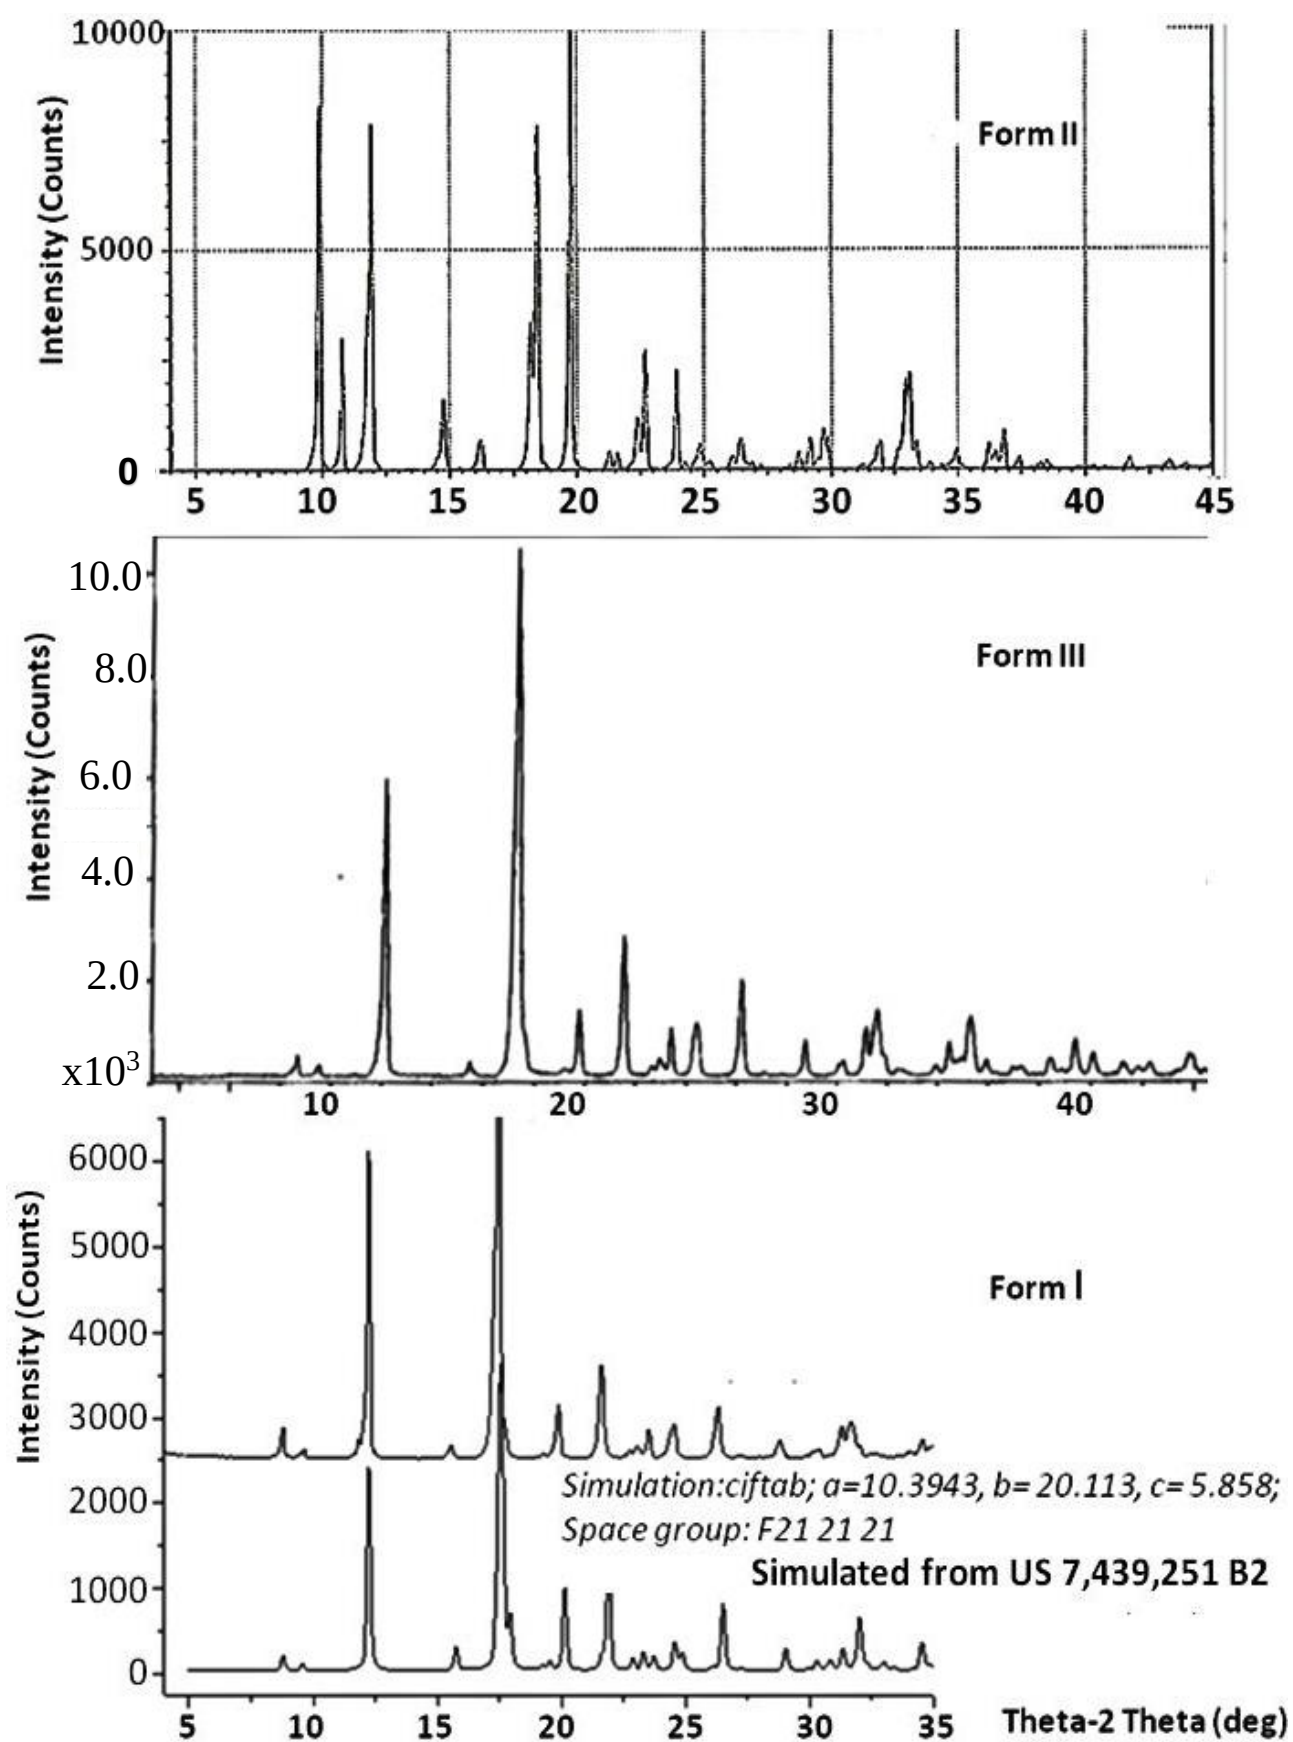


Fig. 13

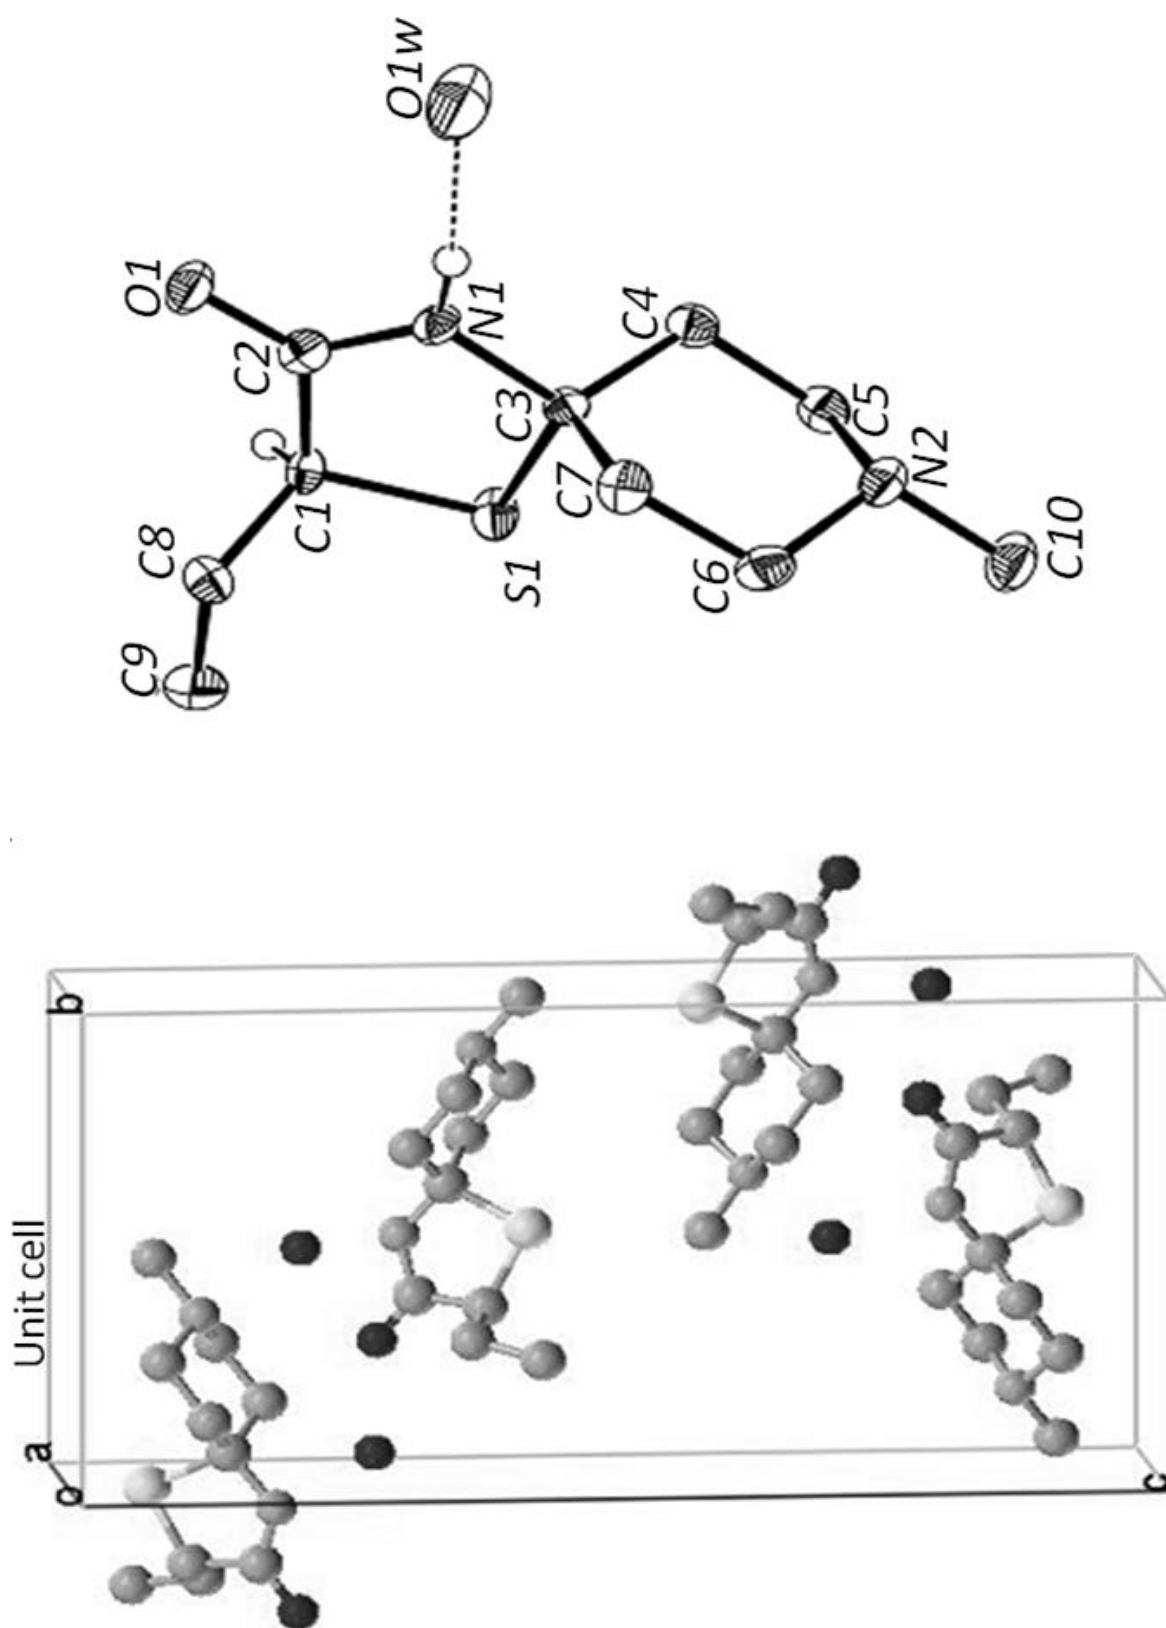
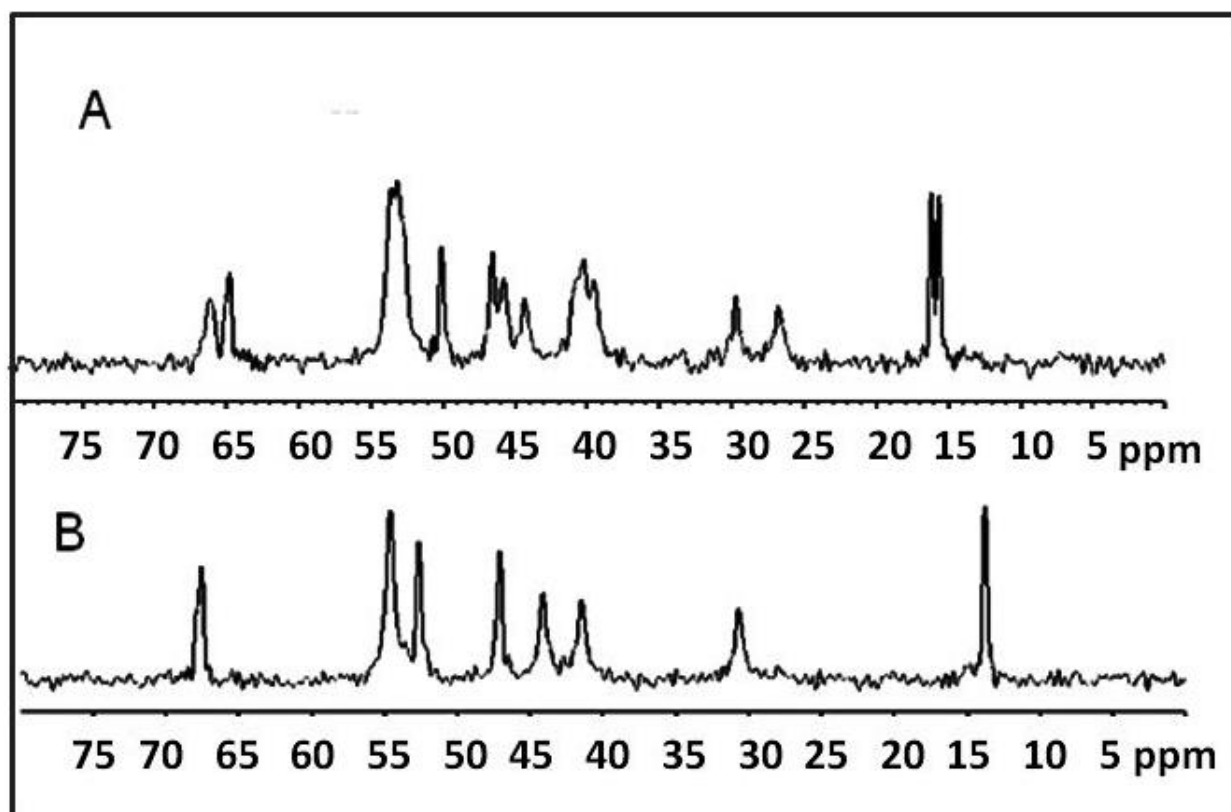


Fig. 14

**Fig. 15A**

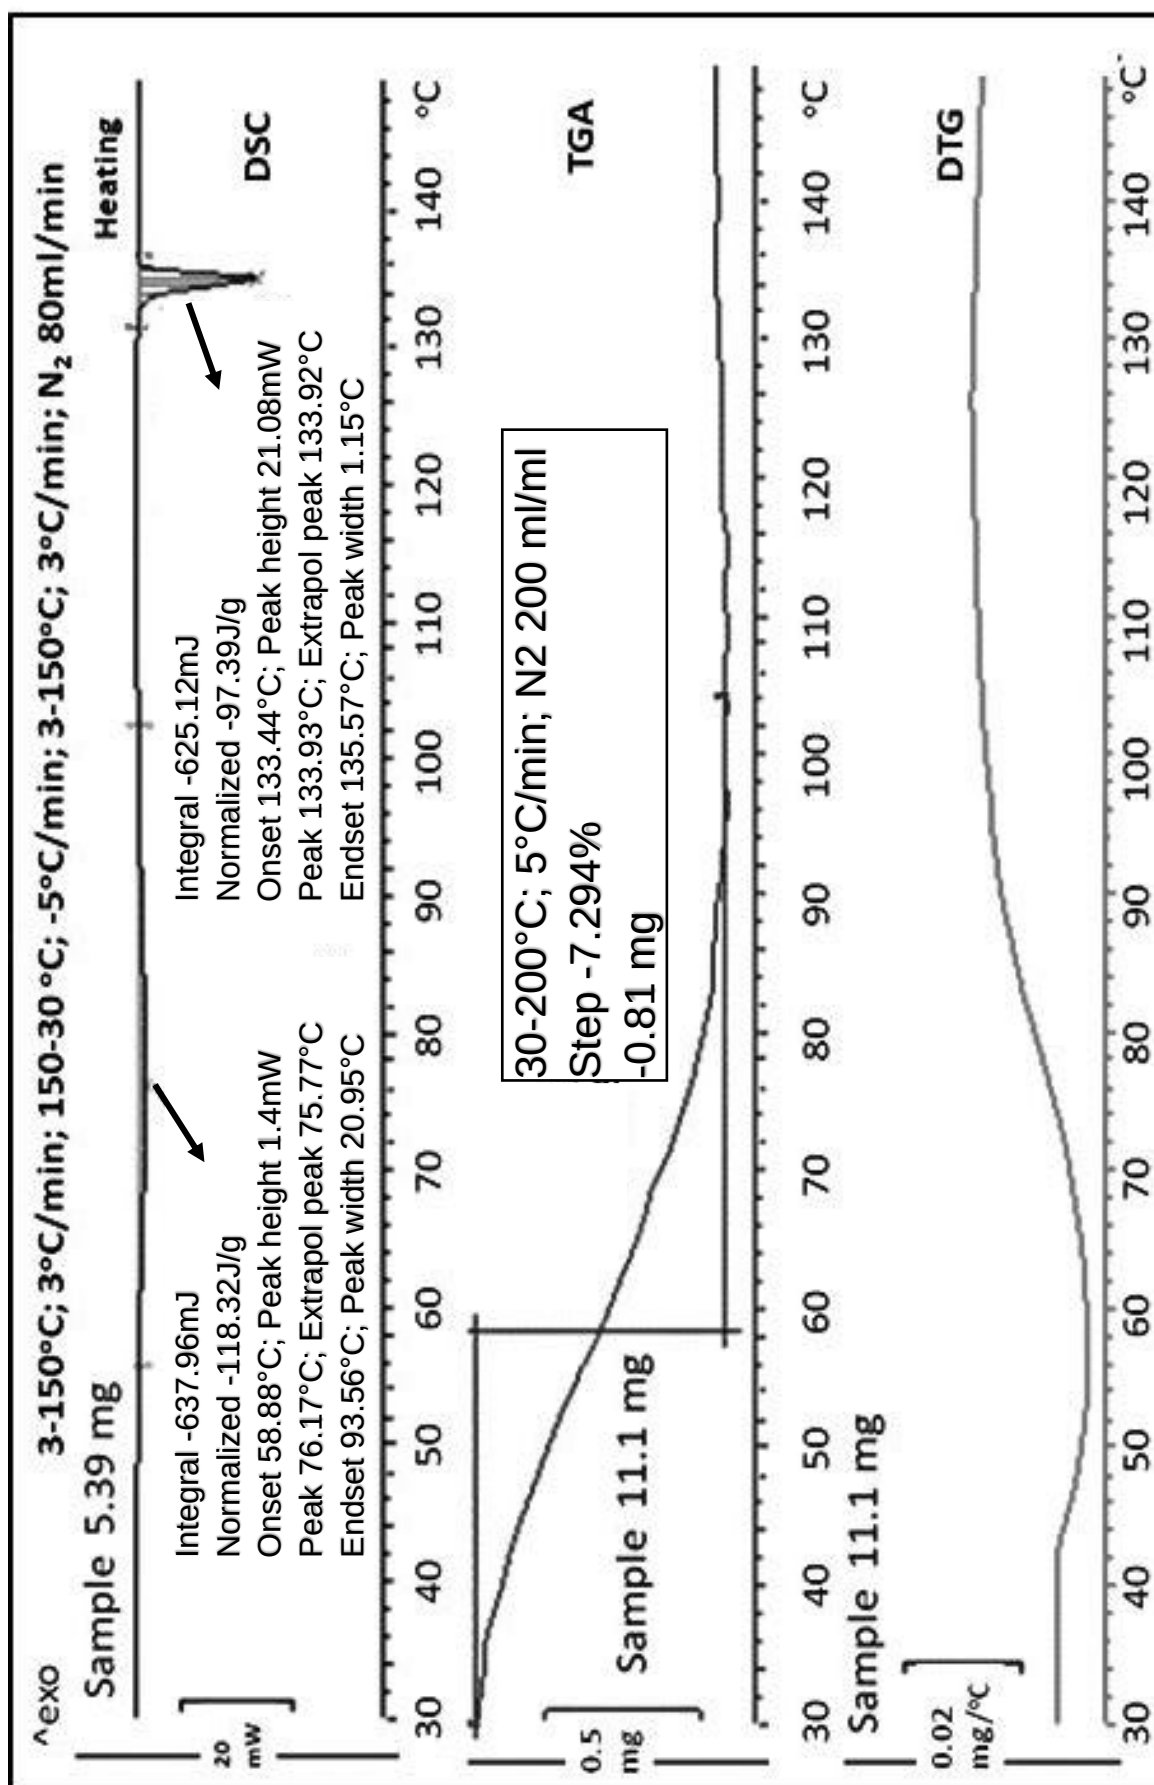


Fig. 15B

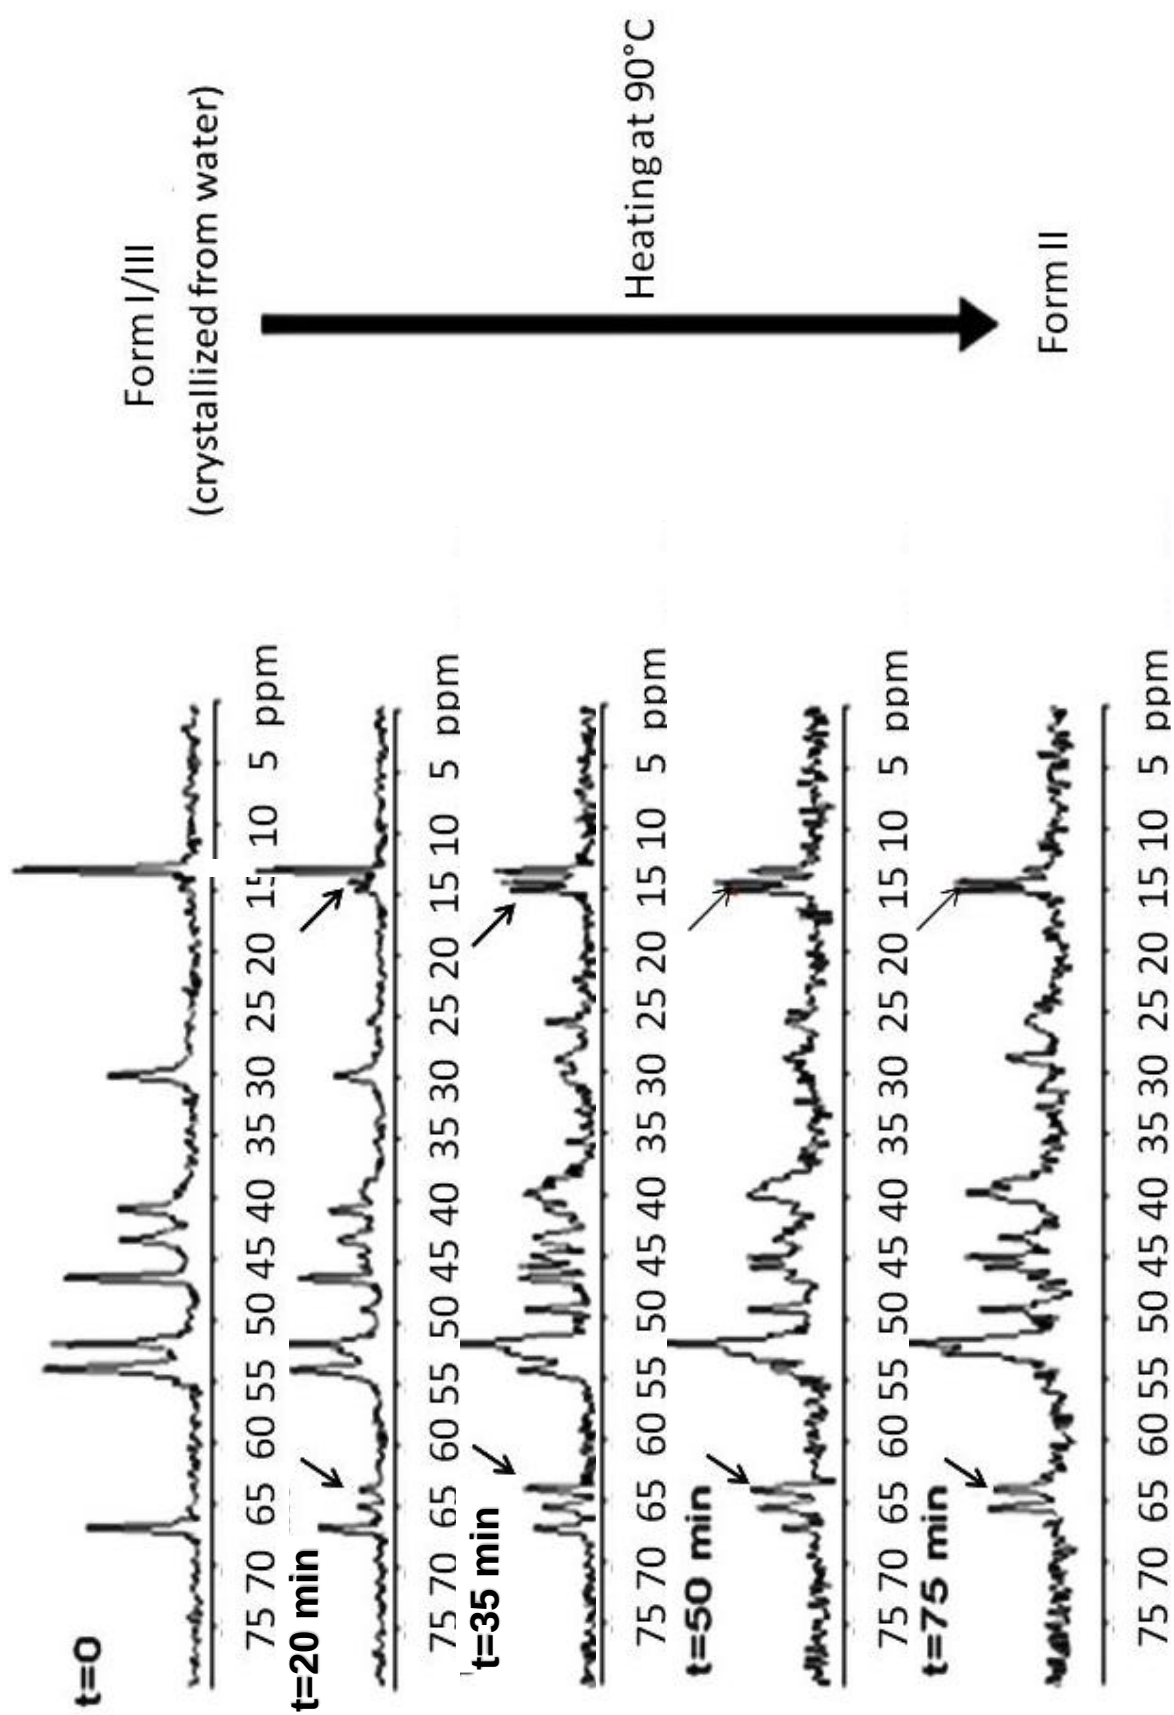


Fig. 16