

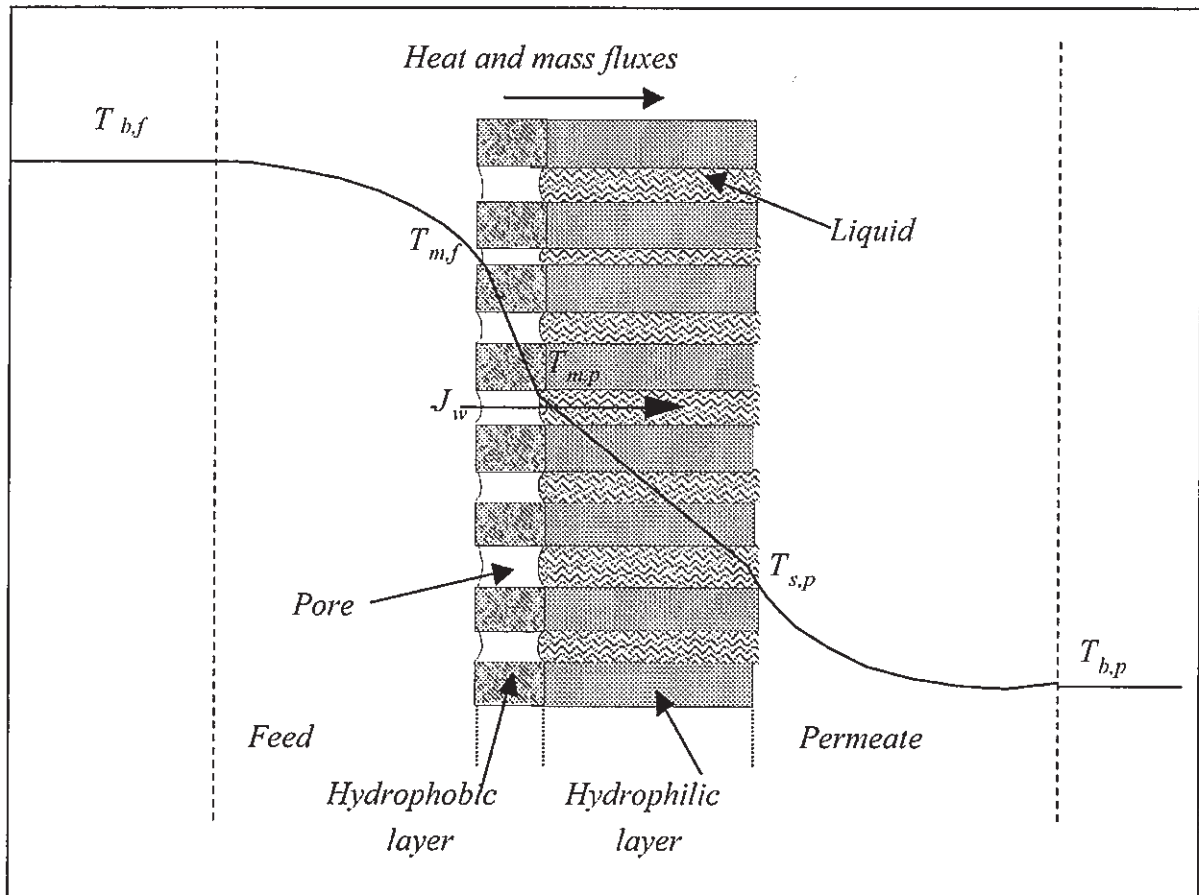


FIG. 1

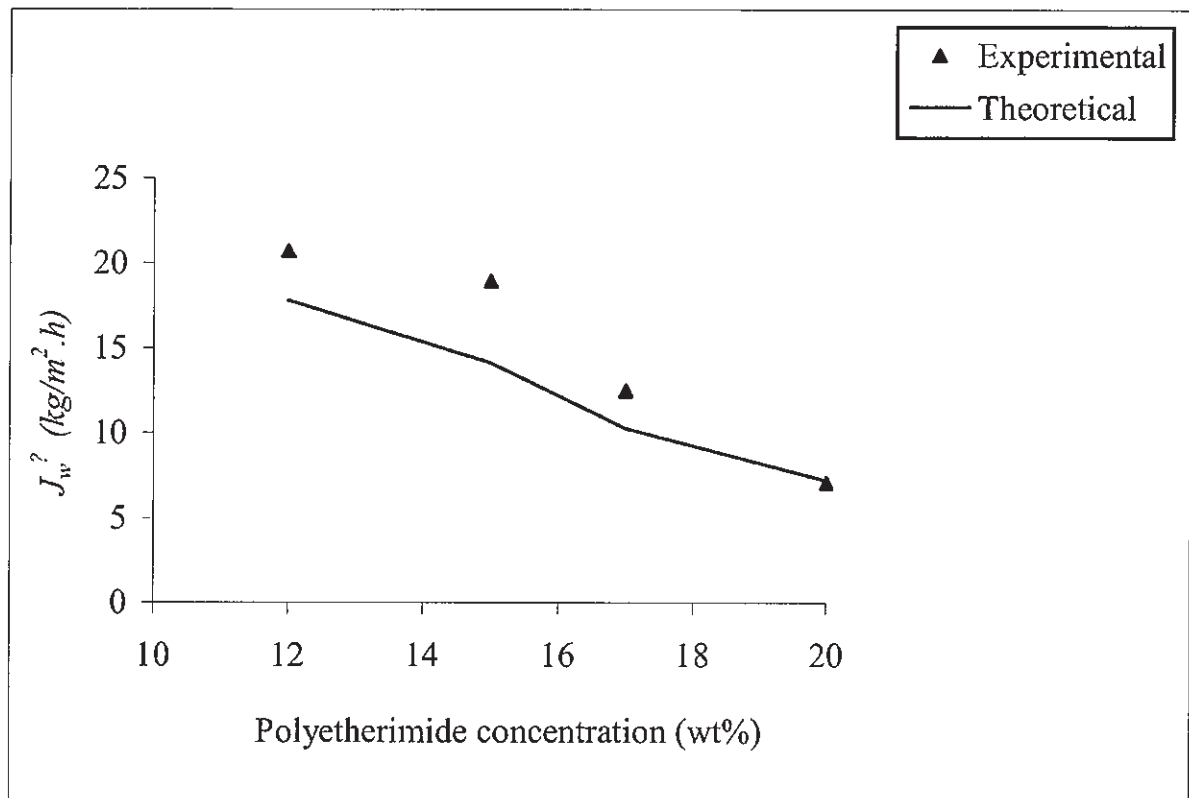


FIG. 2

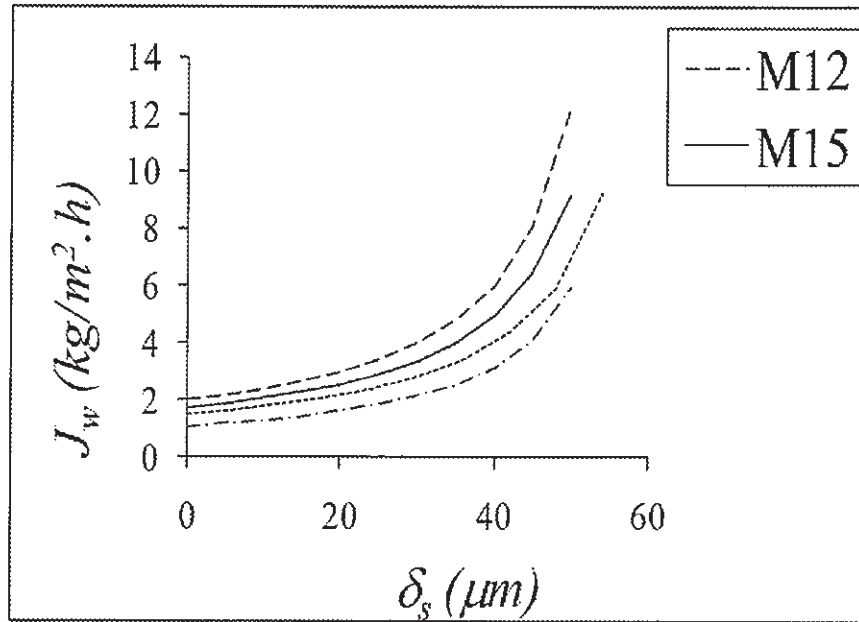


FIG. 3A

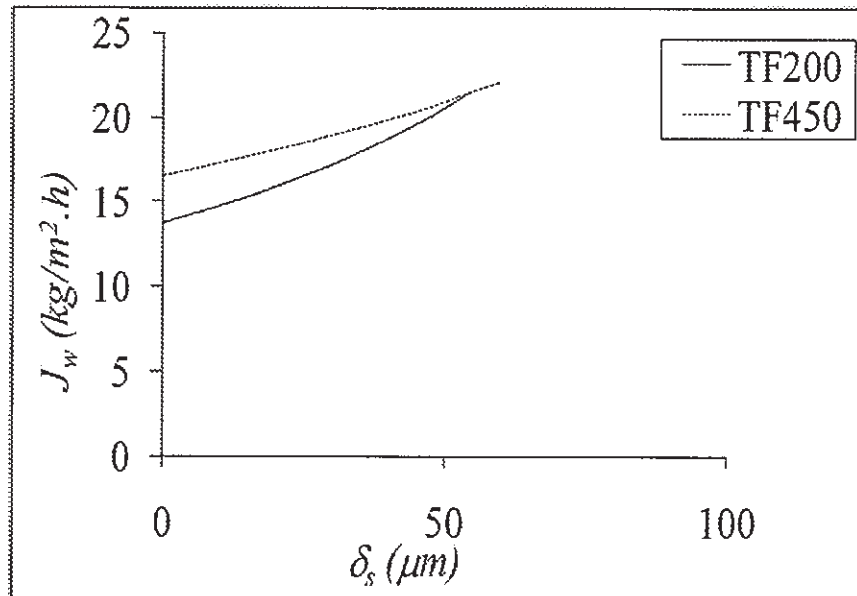


FIG. 3B

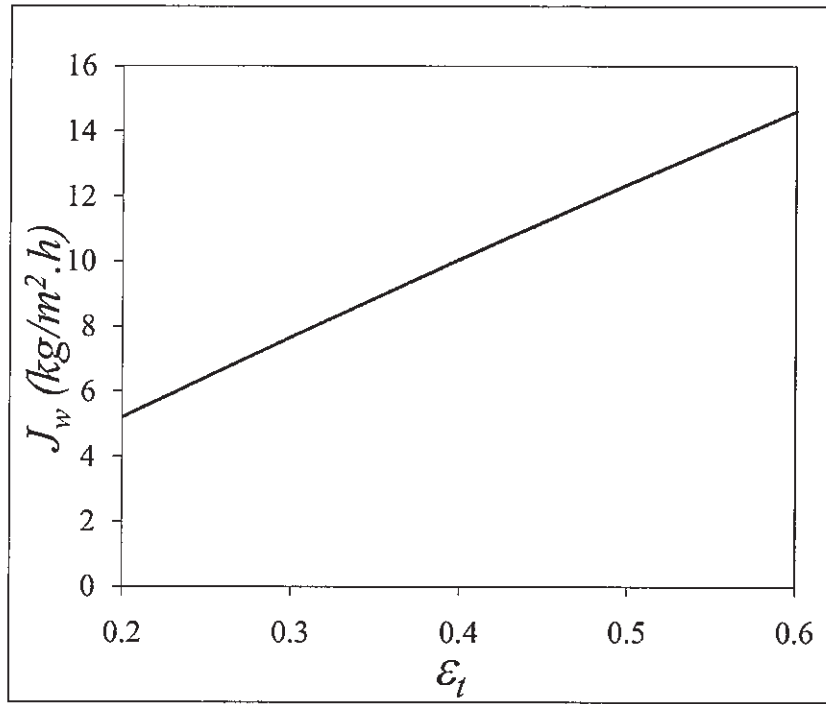


FIG. 4

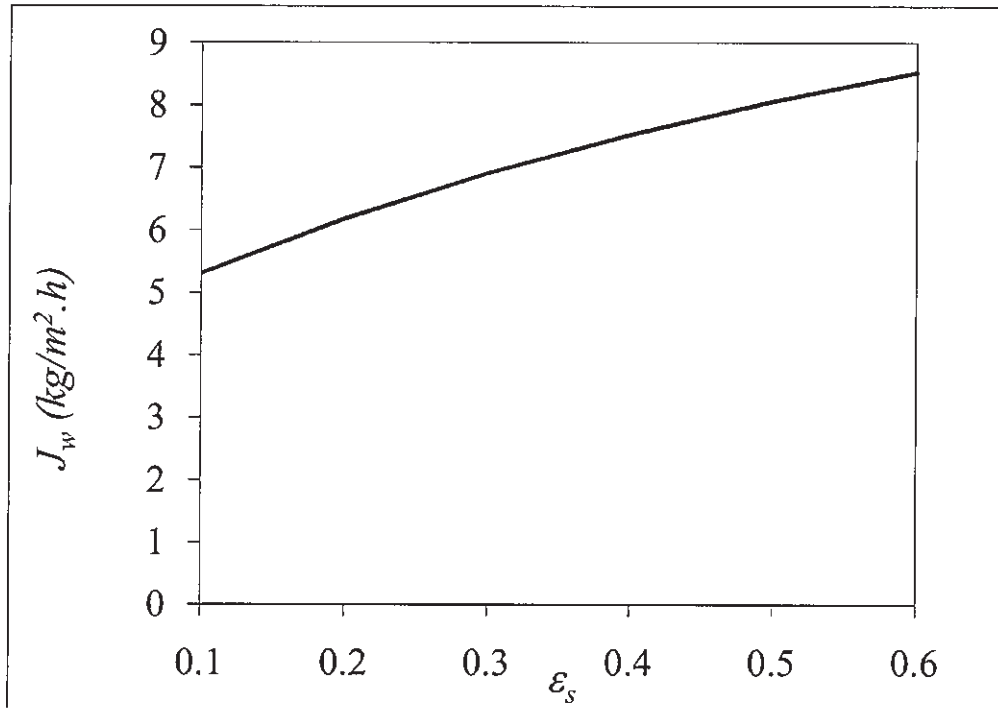


FIG. 5

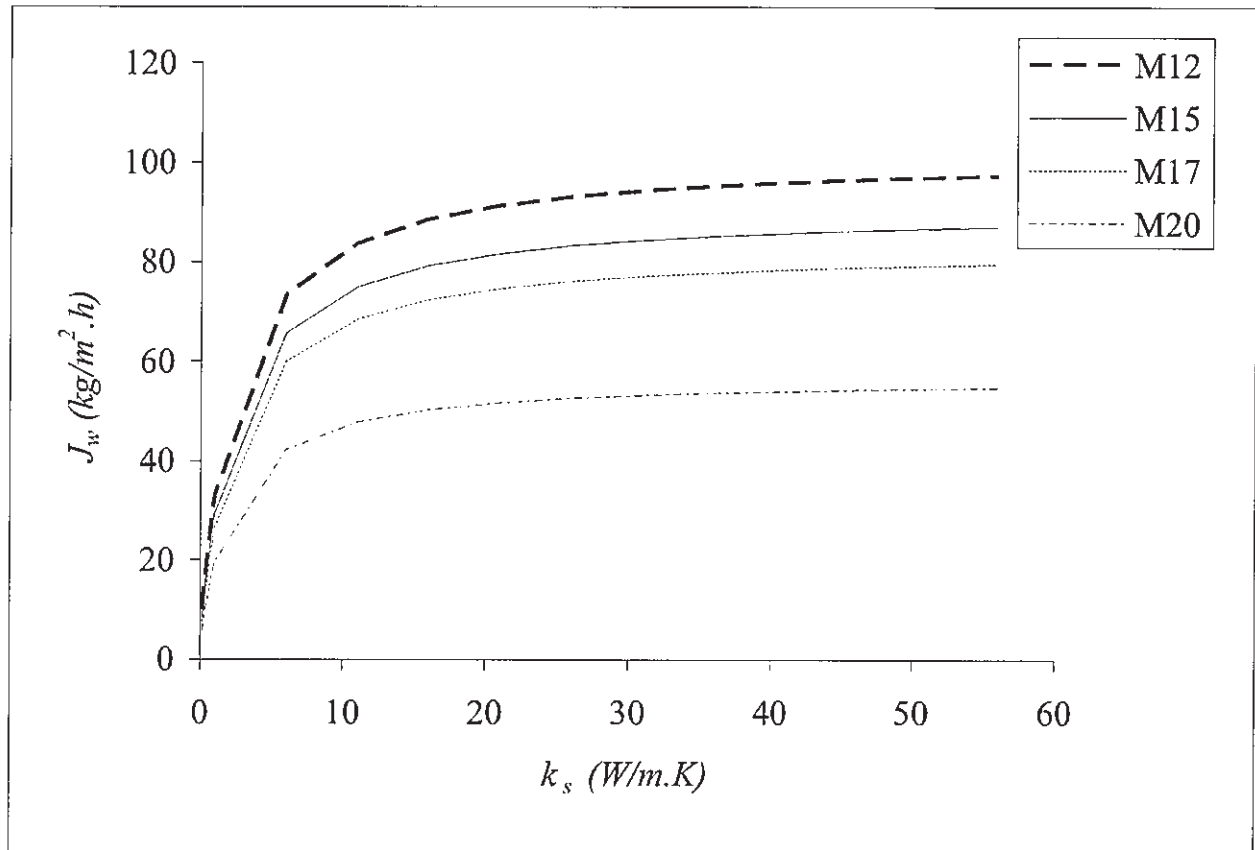


FIG. 6



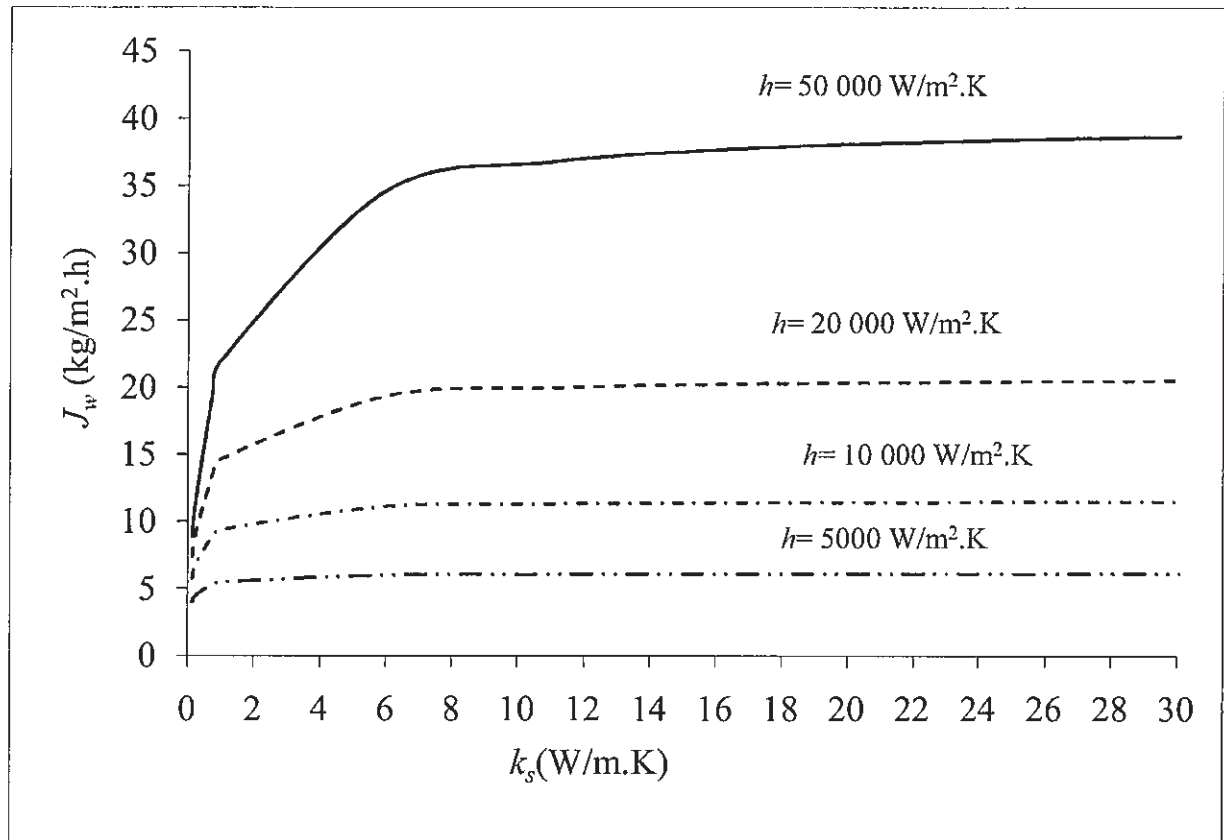


FIG. 7

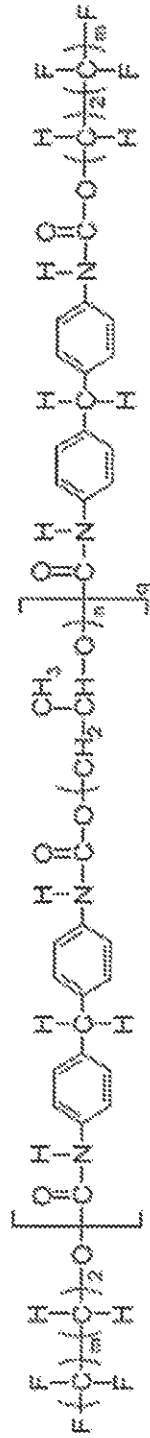


PUP

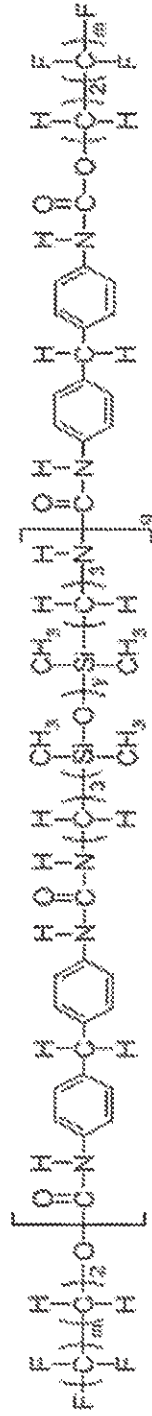


PUDU

FIG. 8

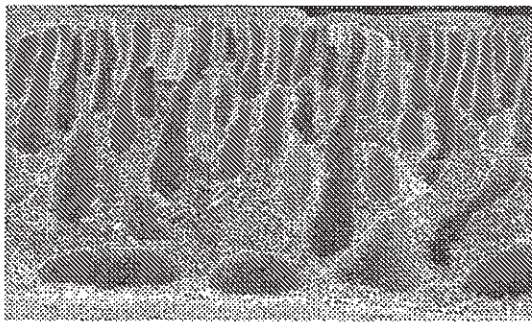


100 μm

FIG. 9A

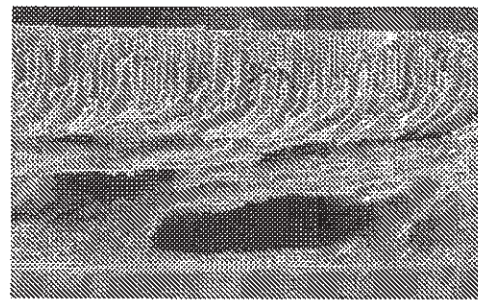


100 μm

FIG. 9B

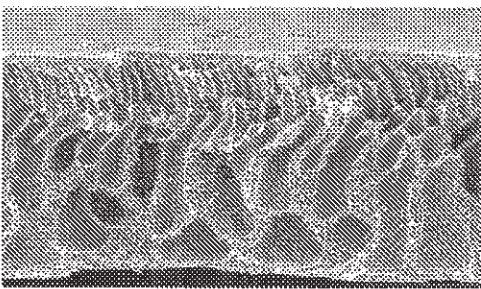

100 μm

FIG. 9C

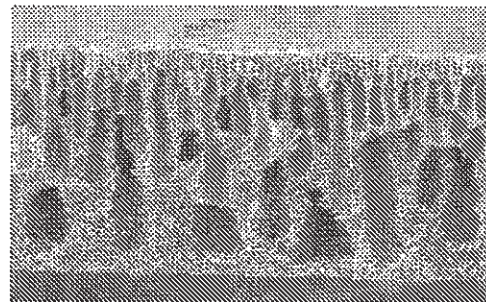

100 μm

FIG. 9D


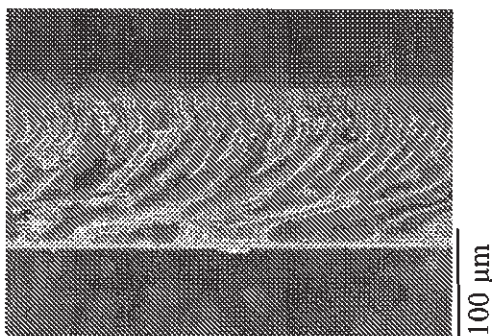


FIG. 9E

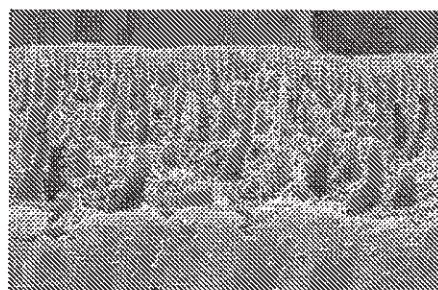

100 μm

FIG. 9F

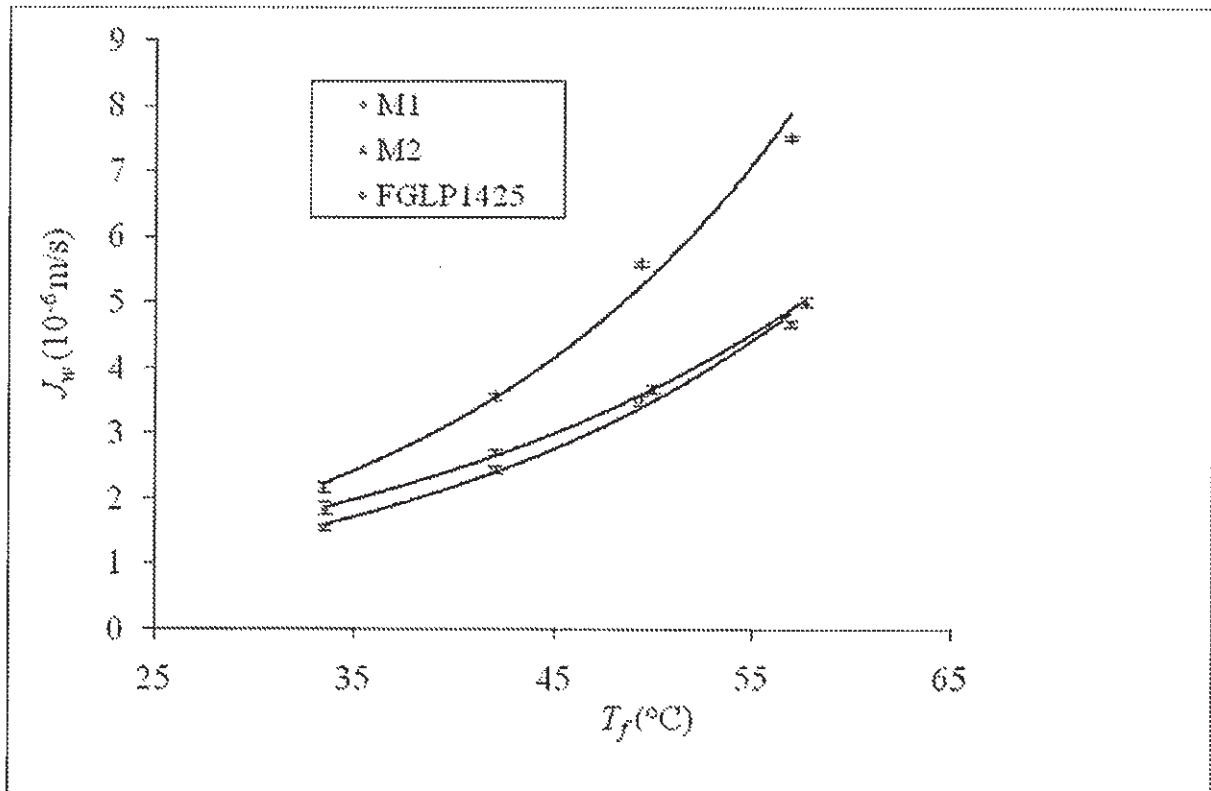


FIG. 10A

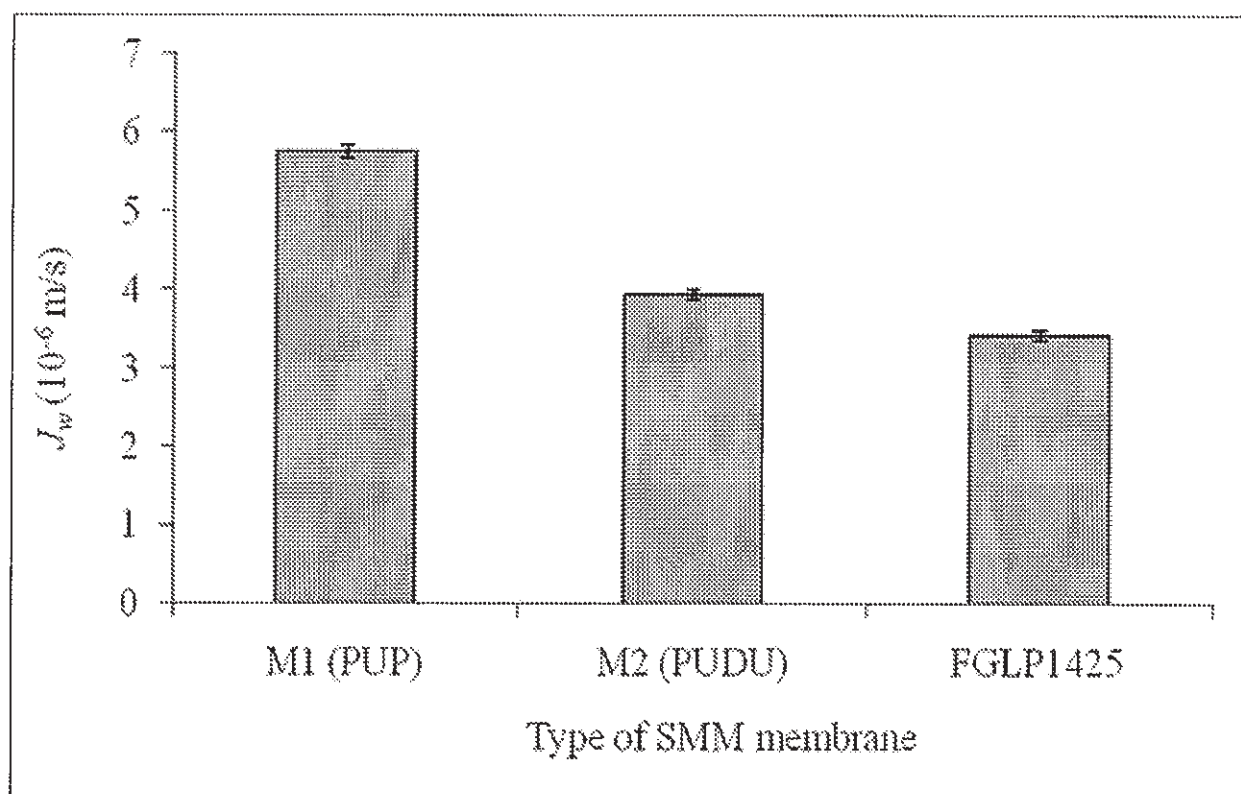


FIG. 10B

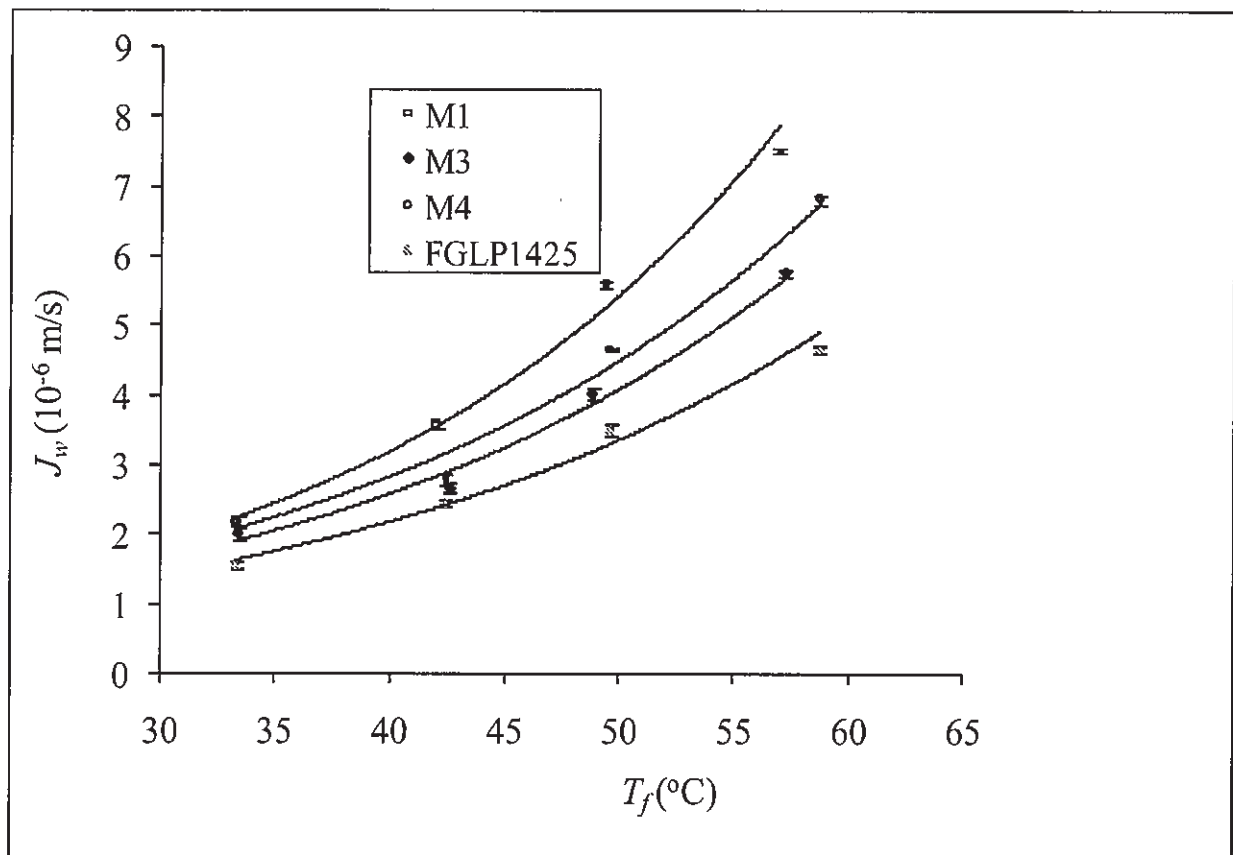


FIG. 11A

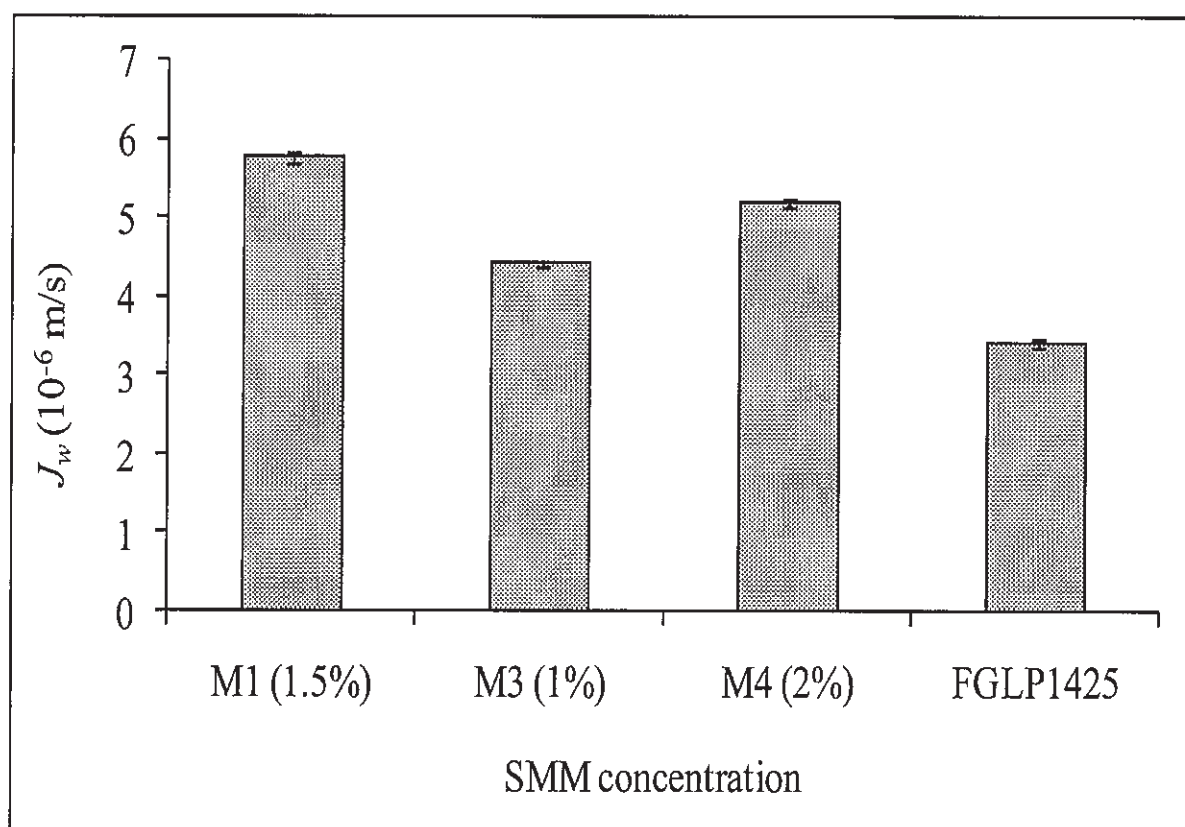


FIG. 11B

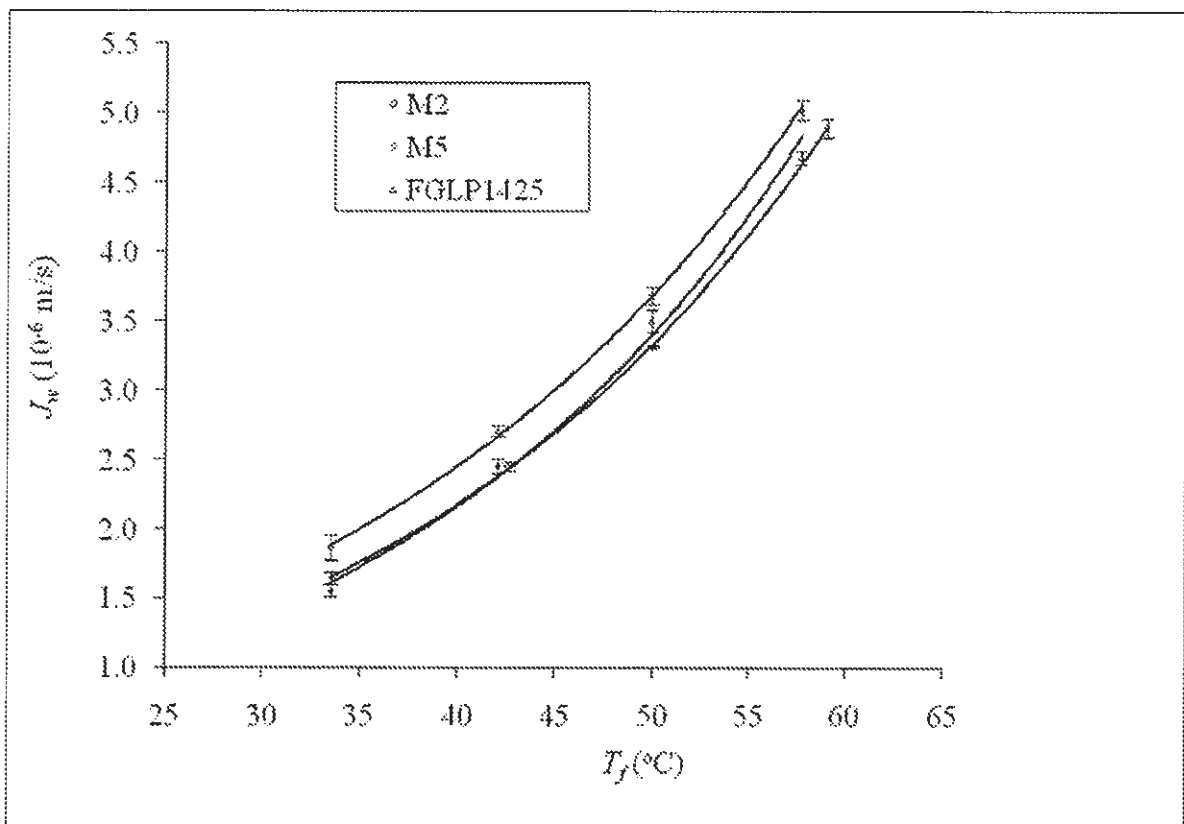


FIG. 12A

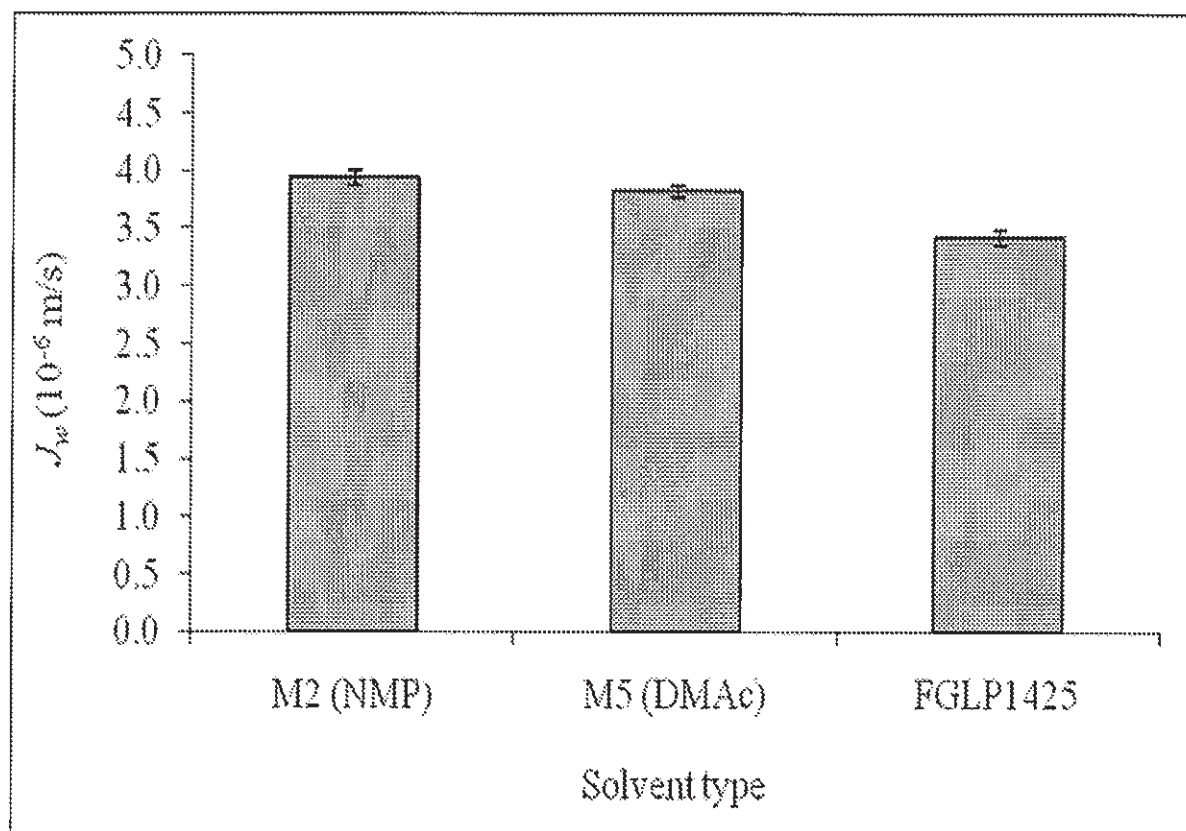


FIG. 12B

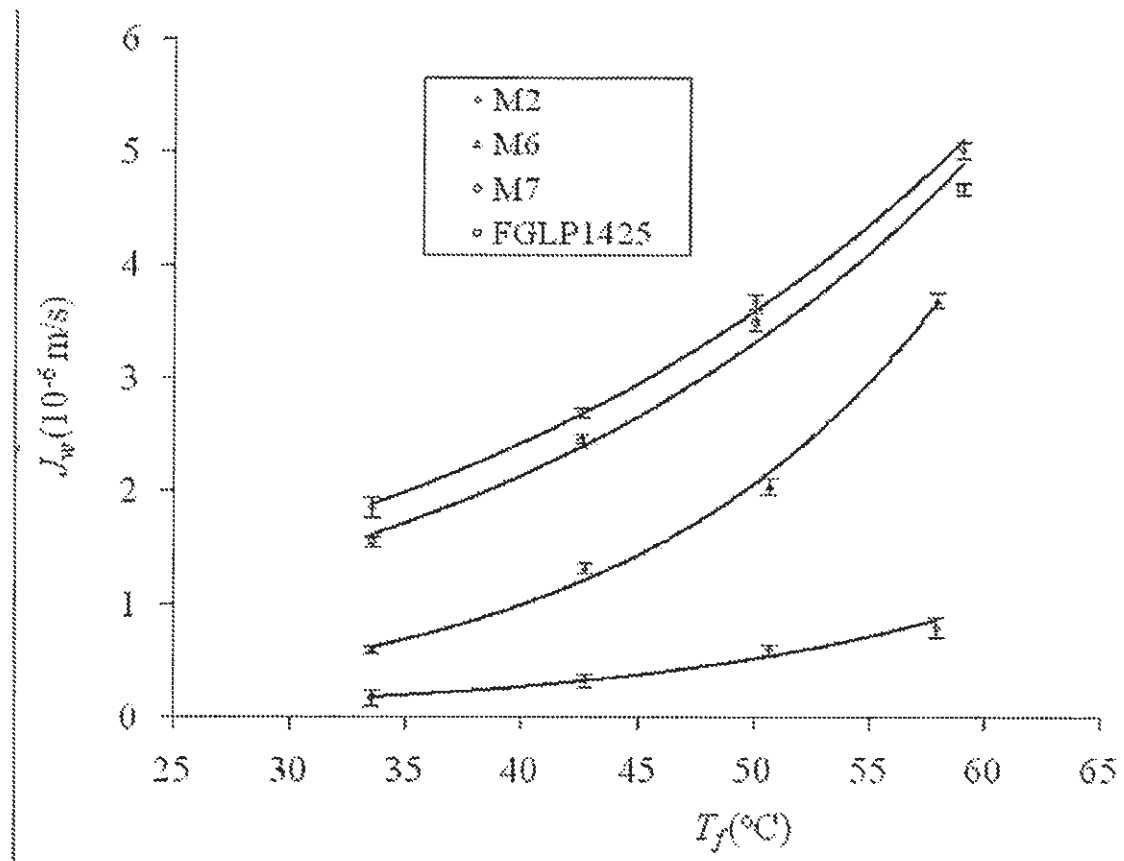


FIG. 13A

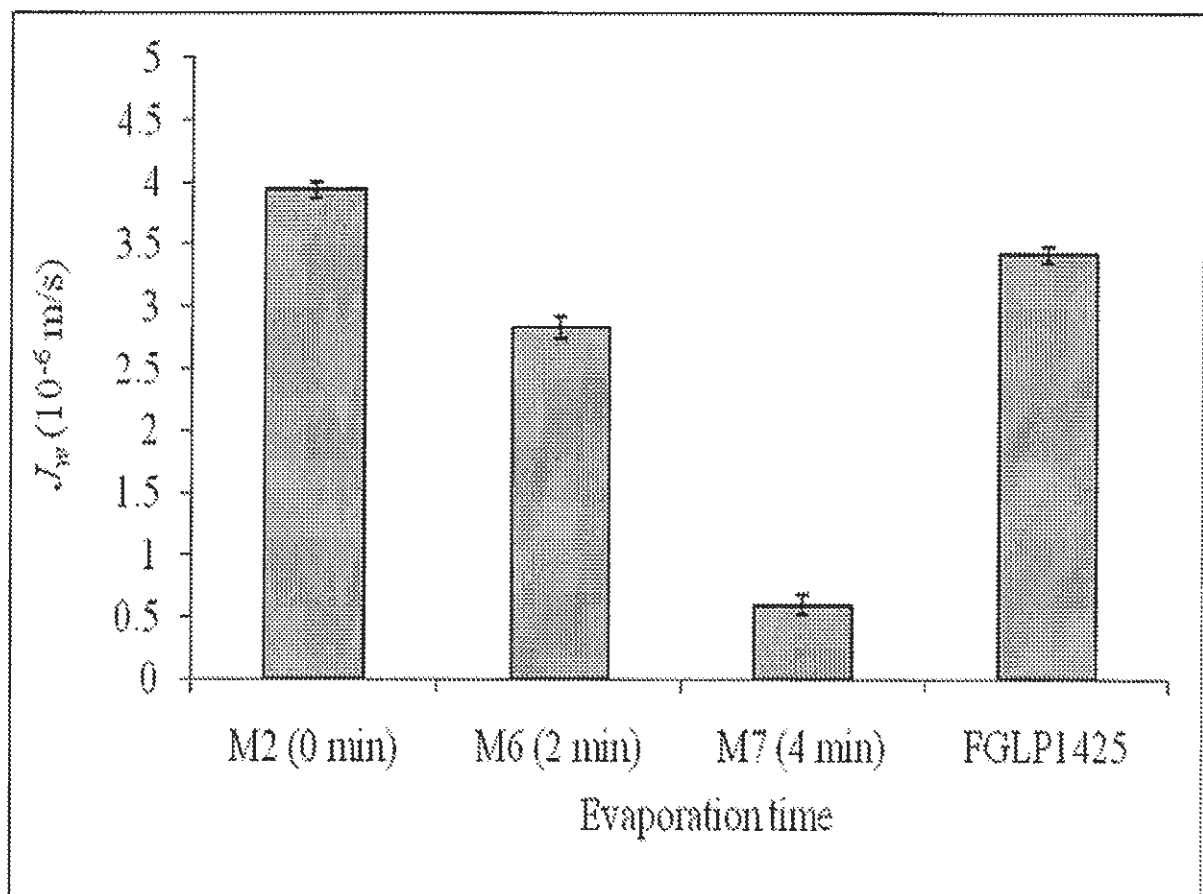


FIG. 13B

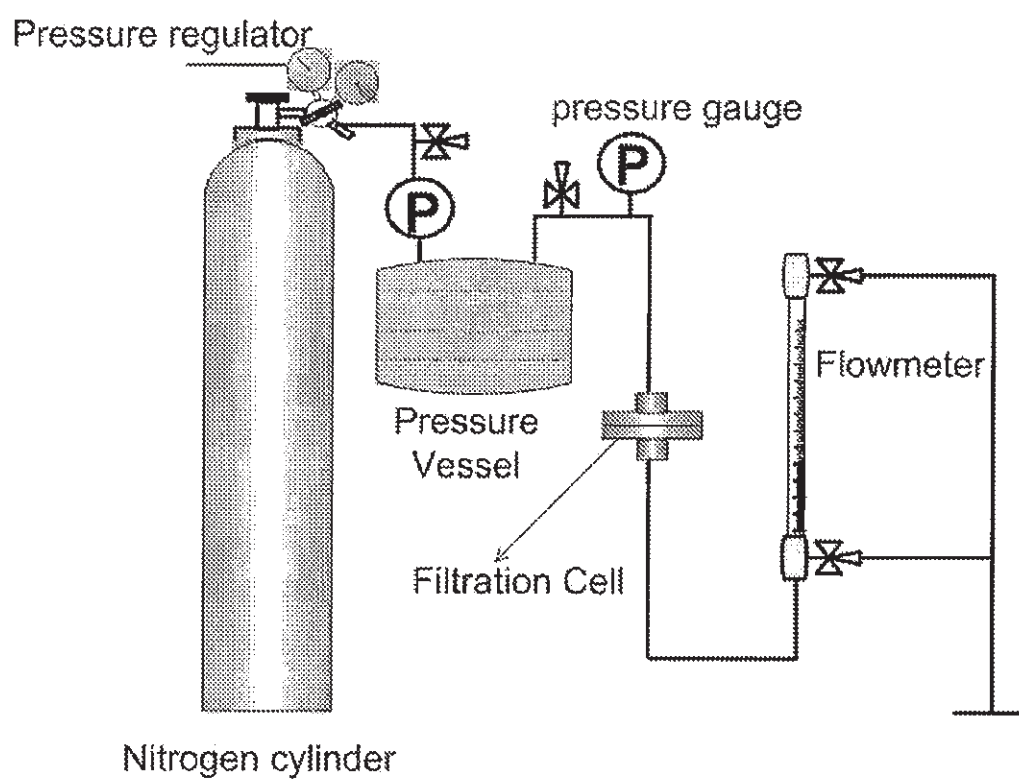


FIG. 14

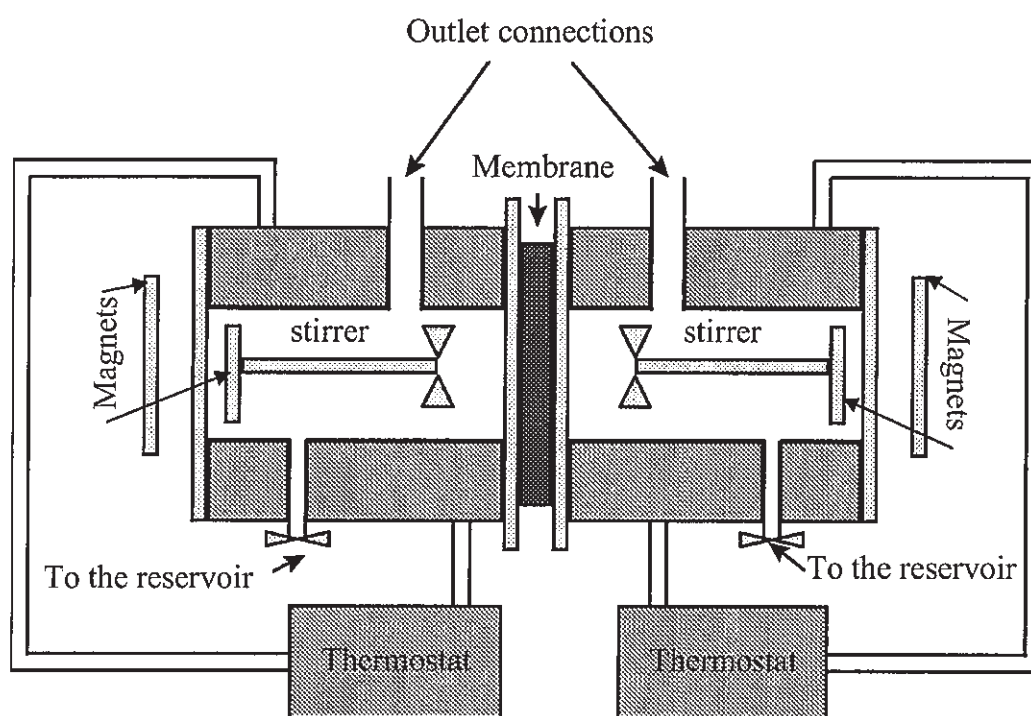


FIG. 15

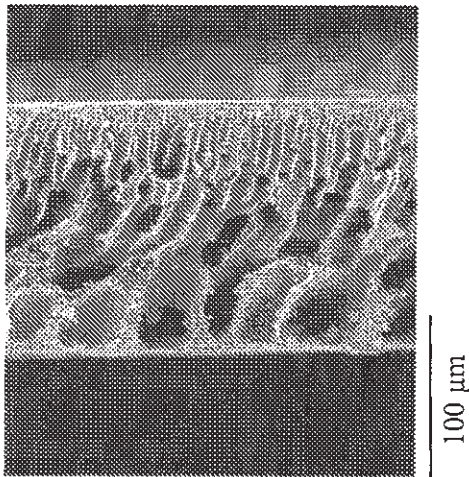


FIG. 16A

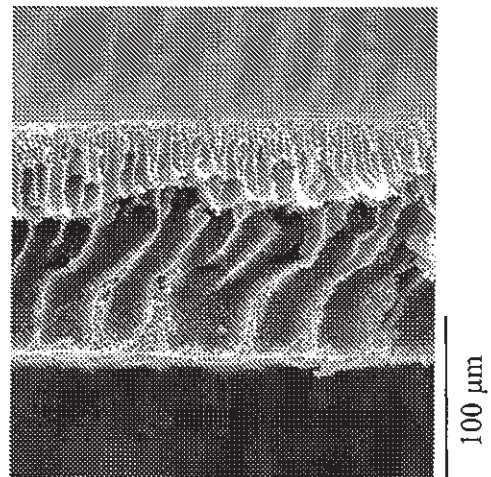


FIG. 16B

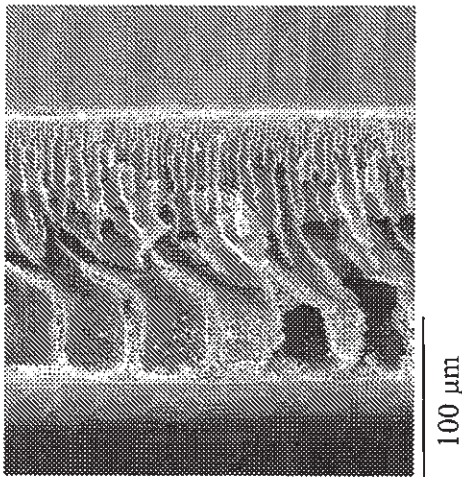


FIG. 16C

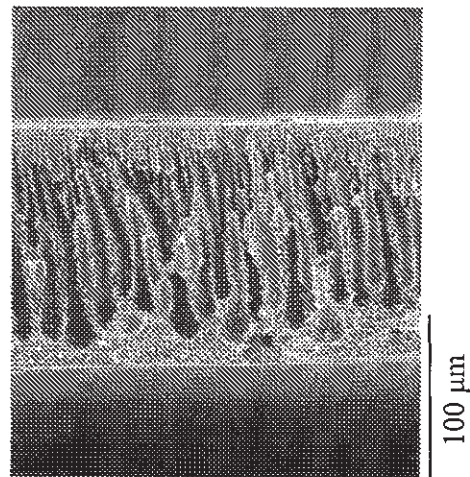


FIG. 16D

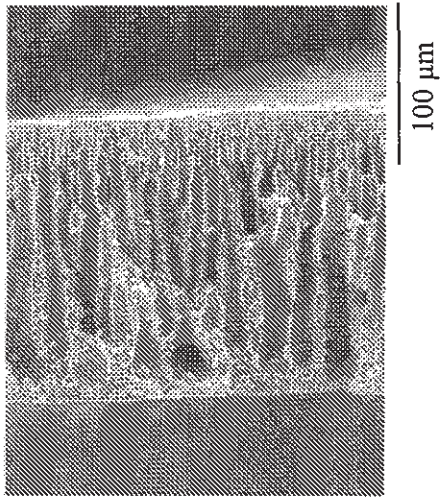


FIG. 16E

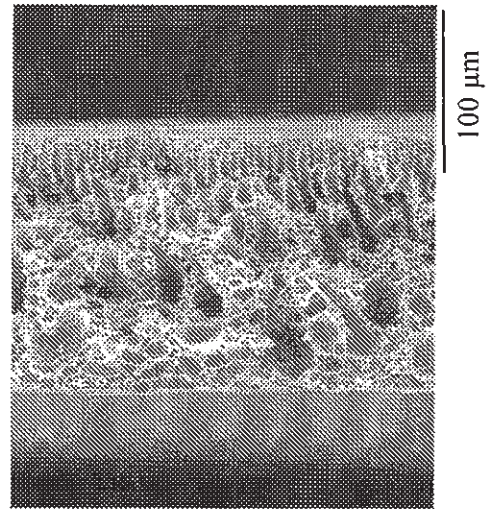


FIG. 16F

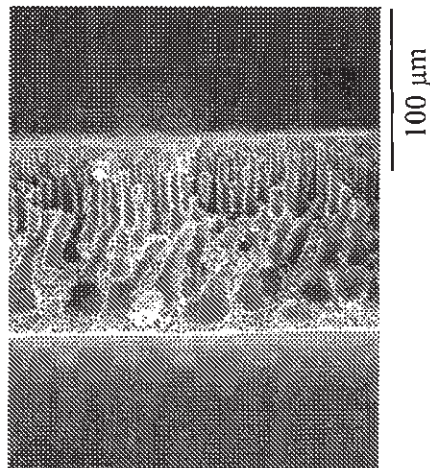


FIG. 16G

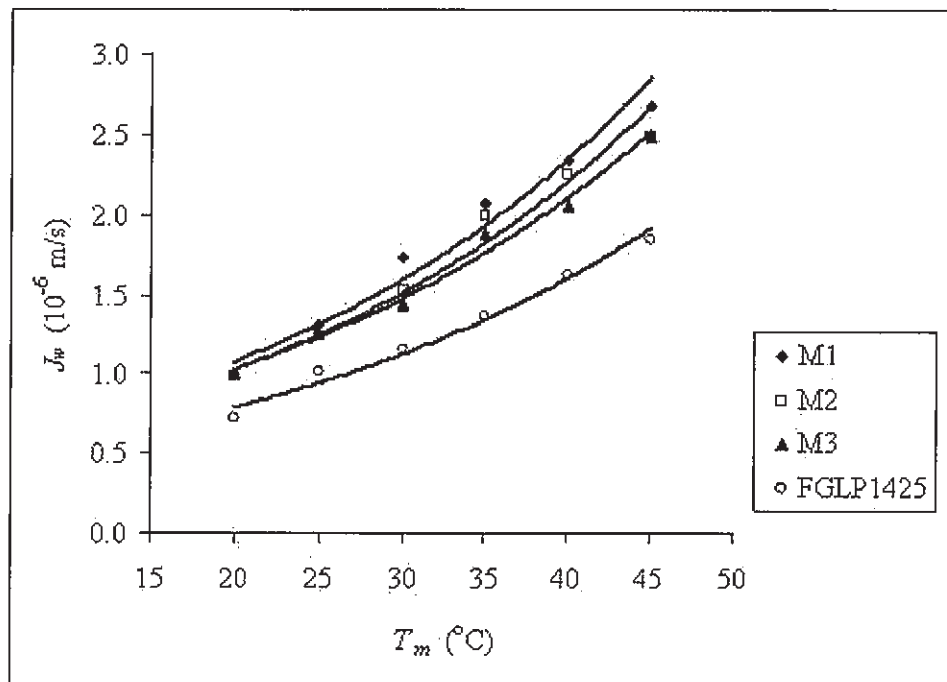


FIG. 17A

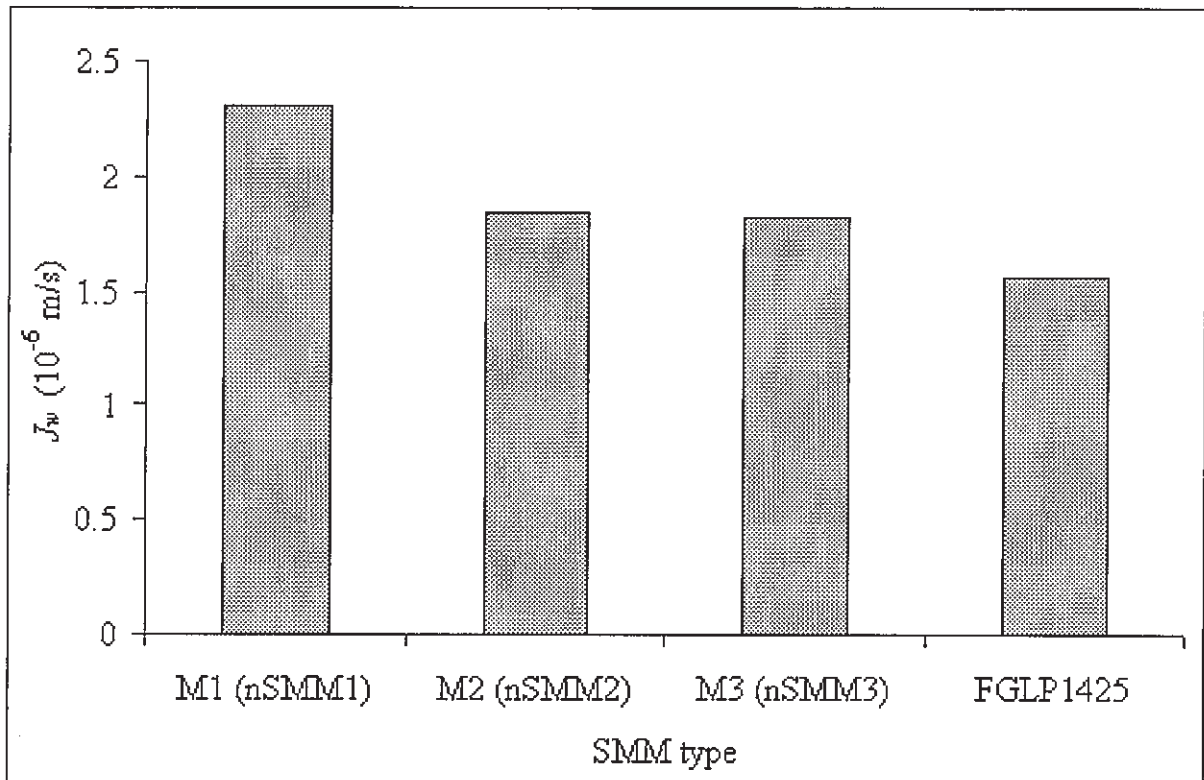


FIG. 17B

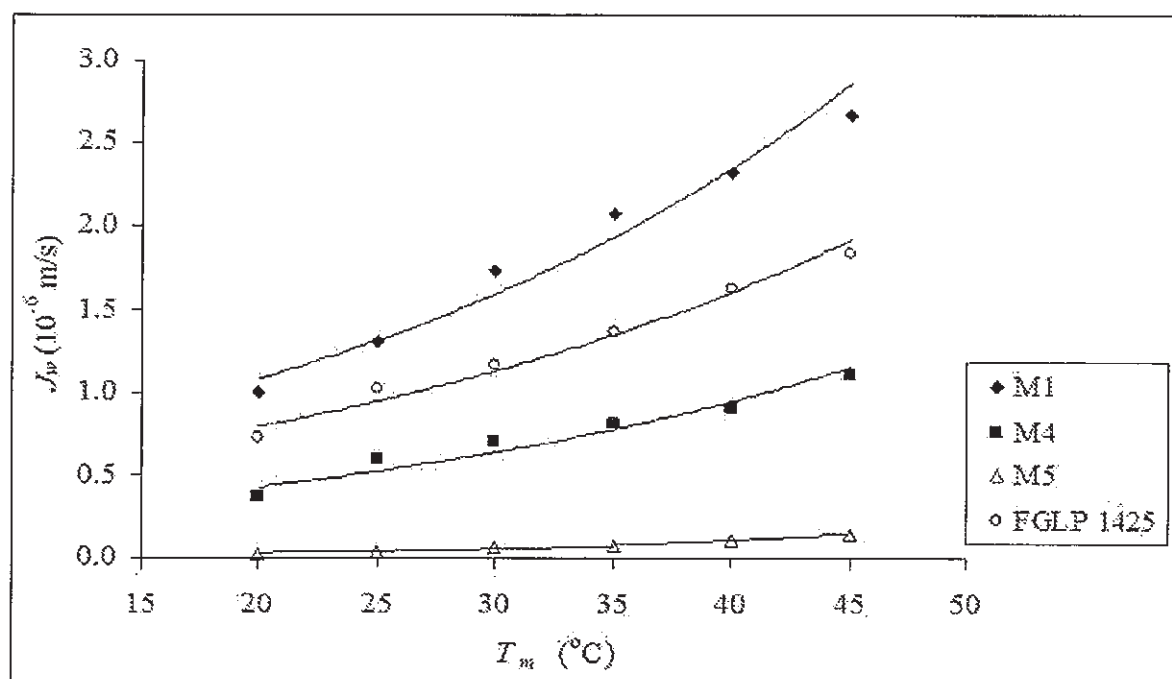


FIG. 18A

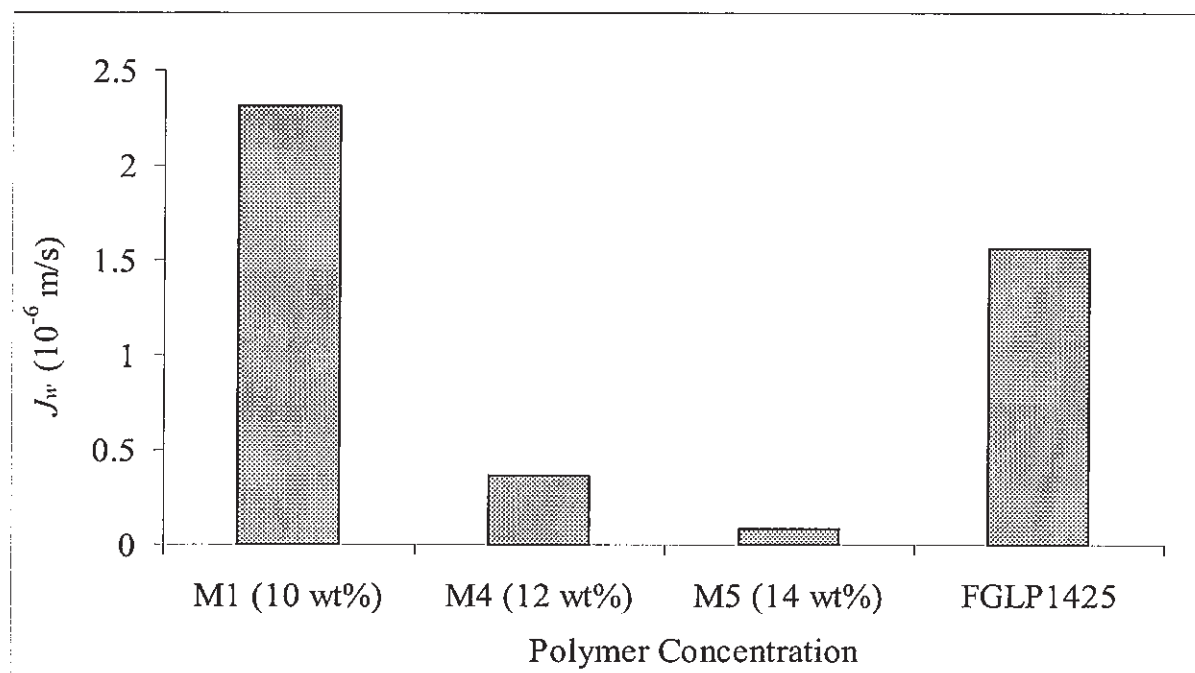


FIG. 18B

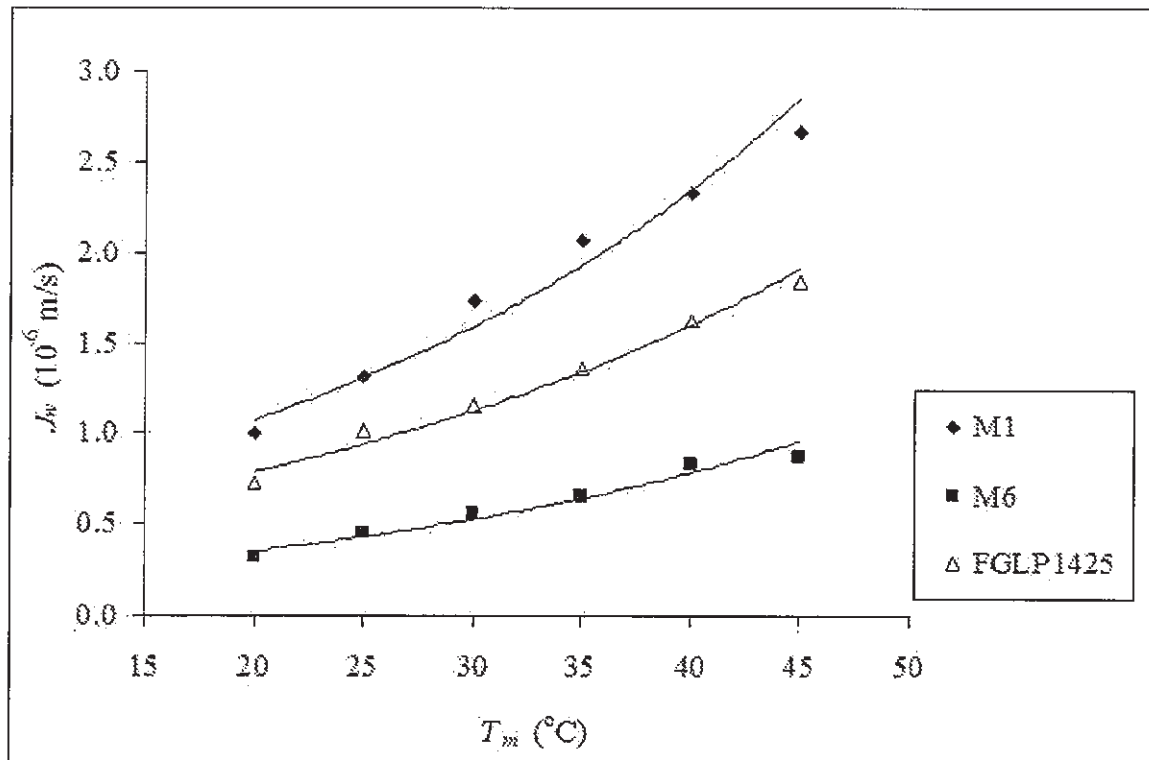


FIG. 19A

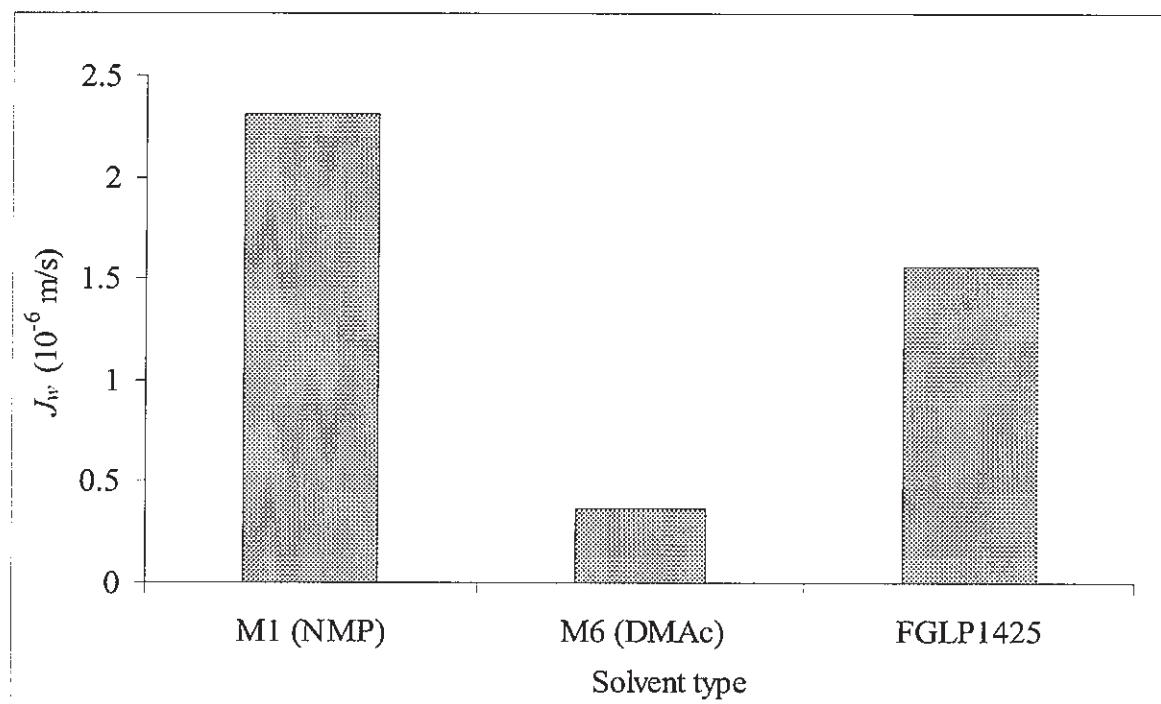


FIG. 19B

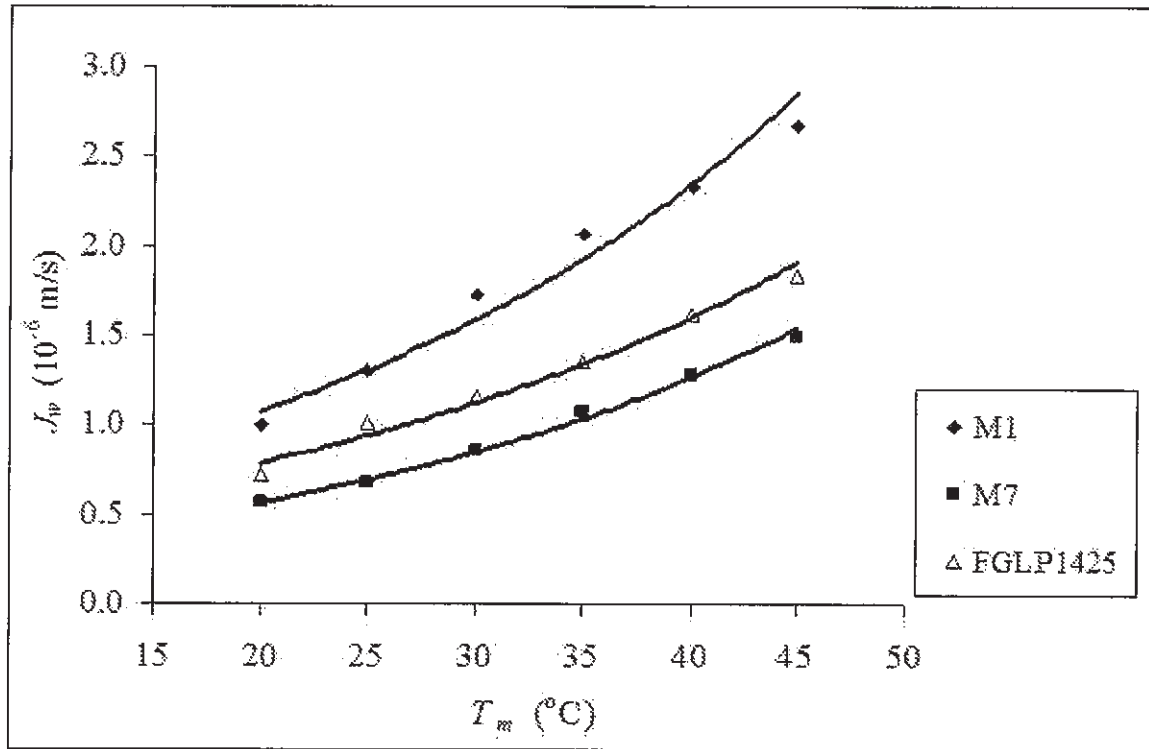


FIG. 20A

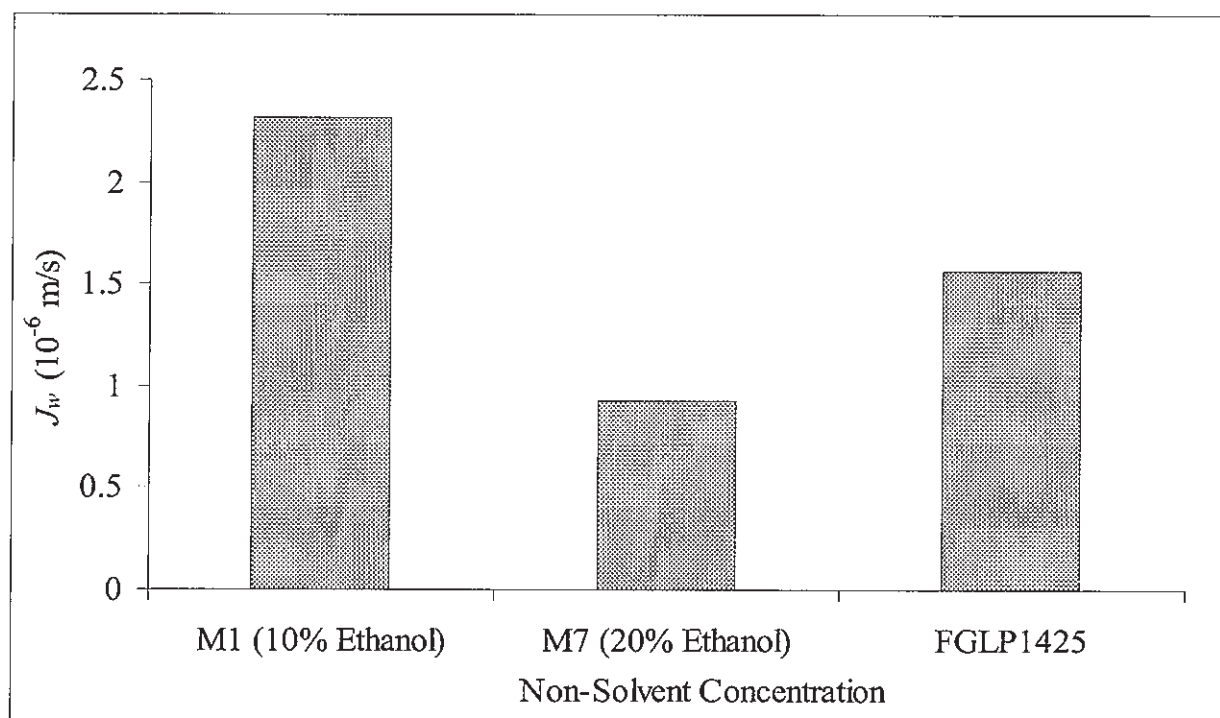


FIG. 20B

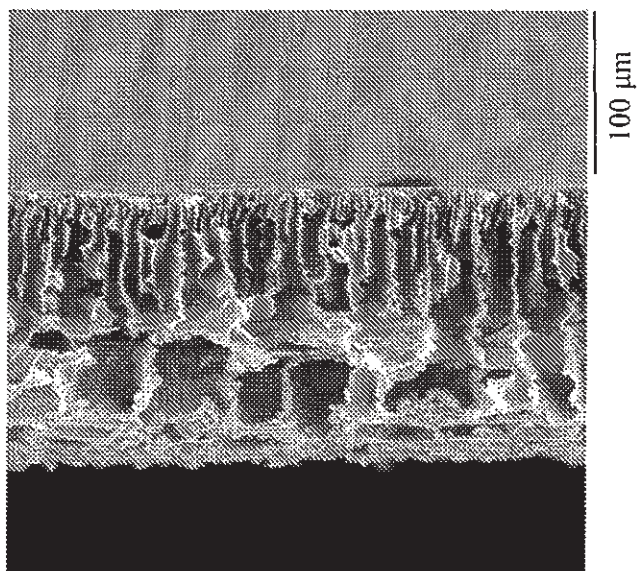


FIG. 21A

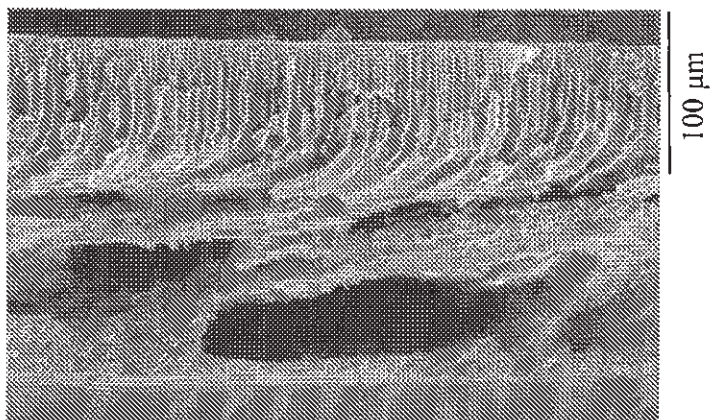


FIG. 21B

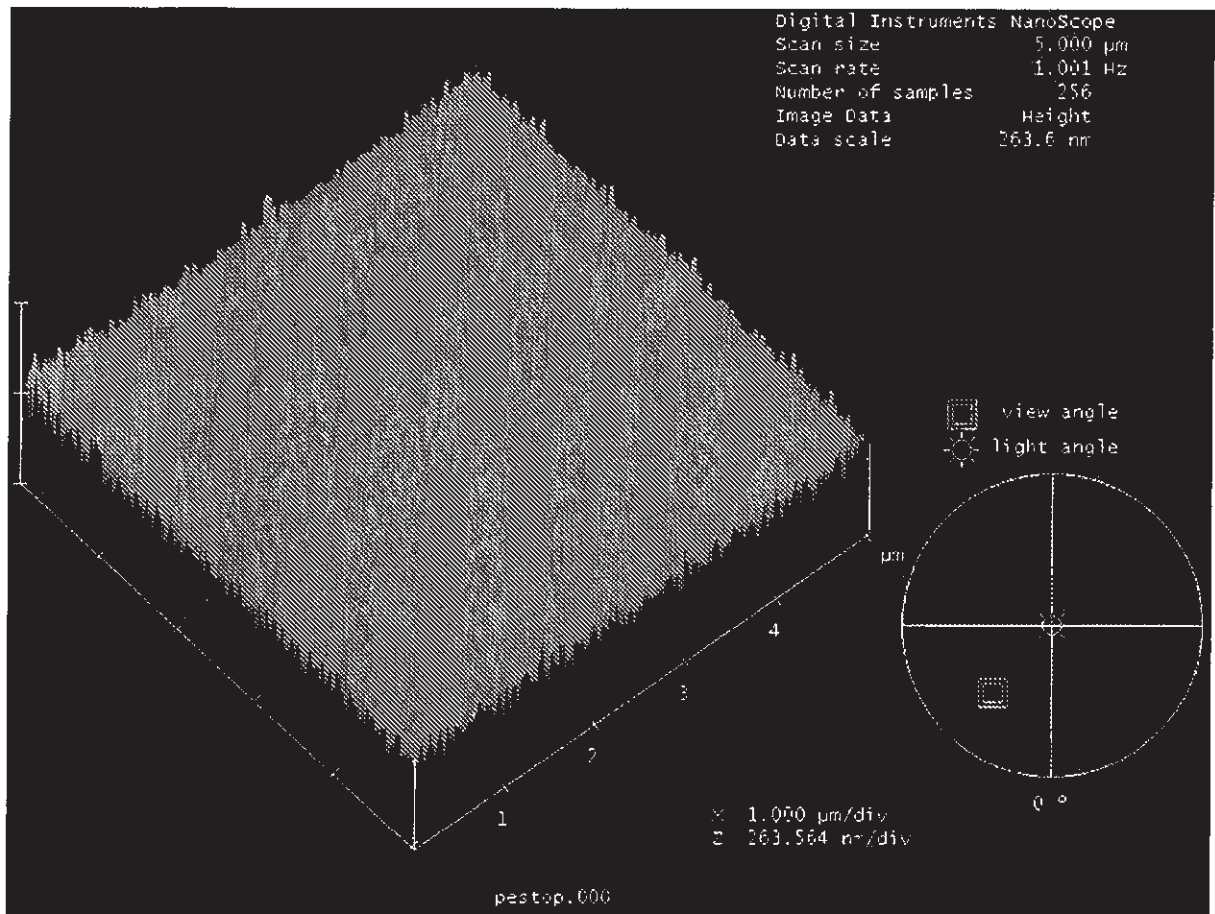


FIG. 22A

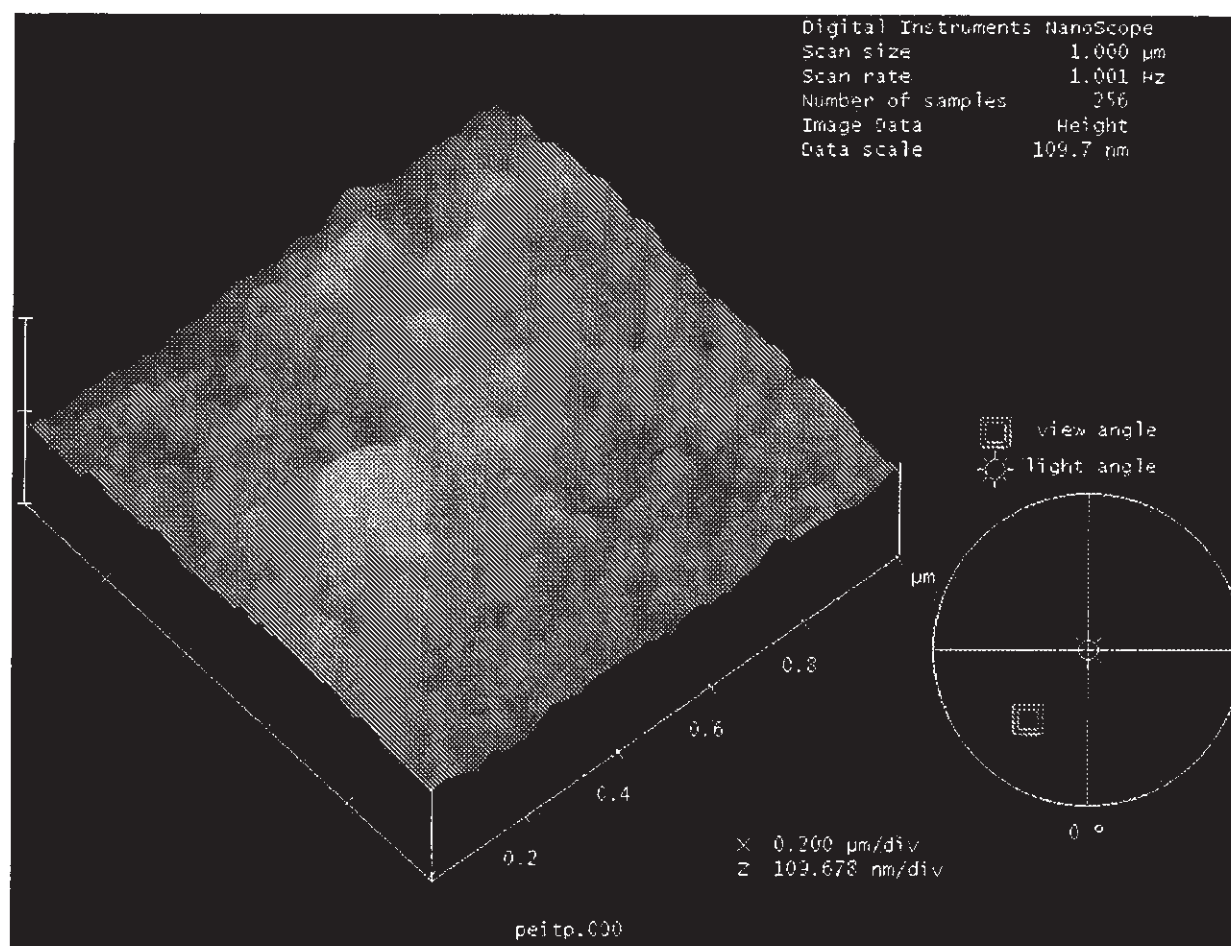


FIG. 22B

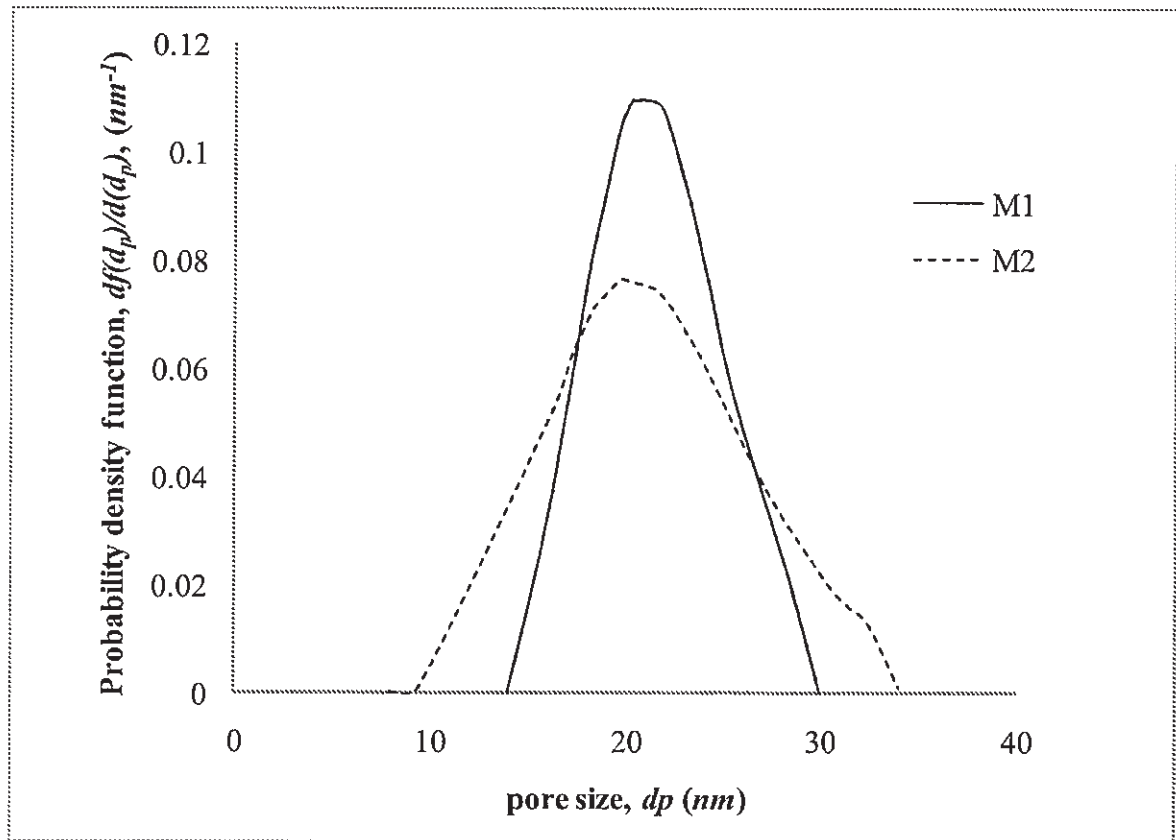


FIG. 23

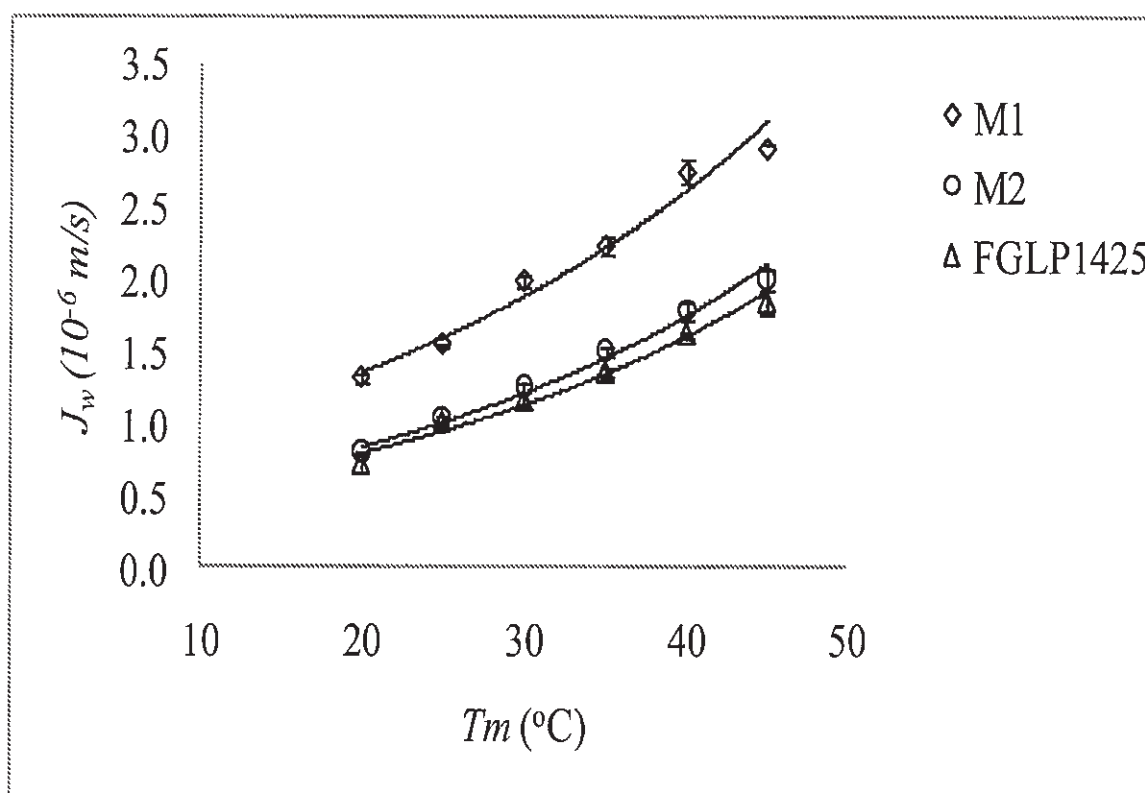


FIG. 24A

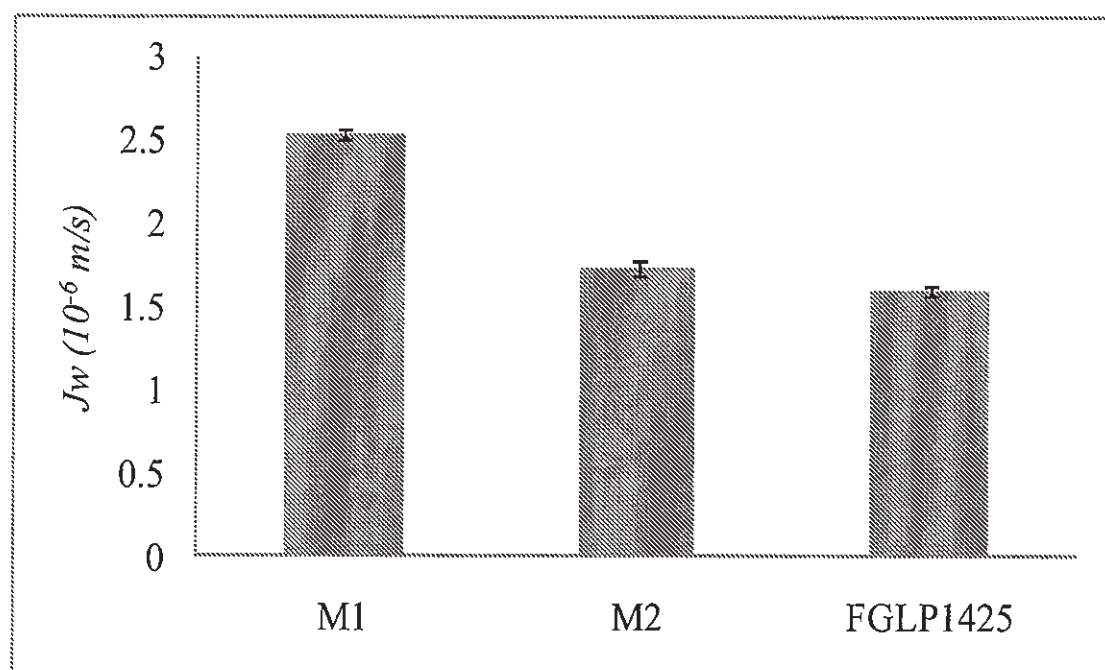


FIG. 24B

FIG. 25A

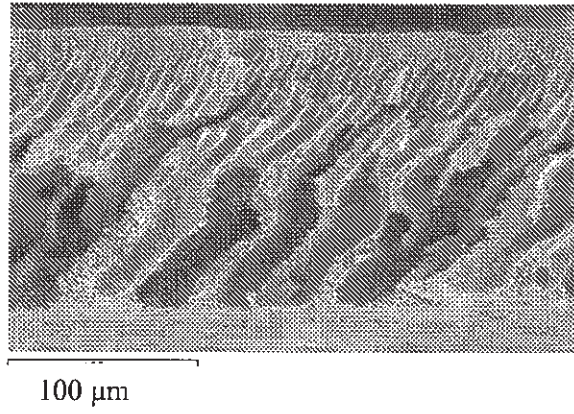


FIG. 25B

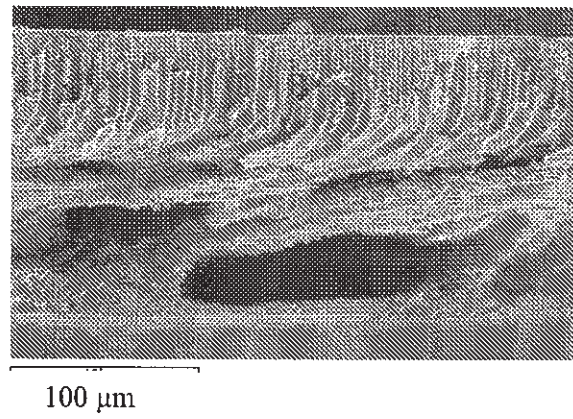
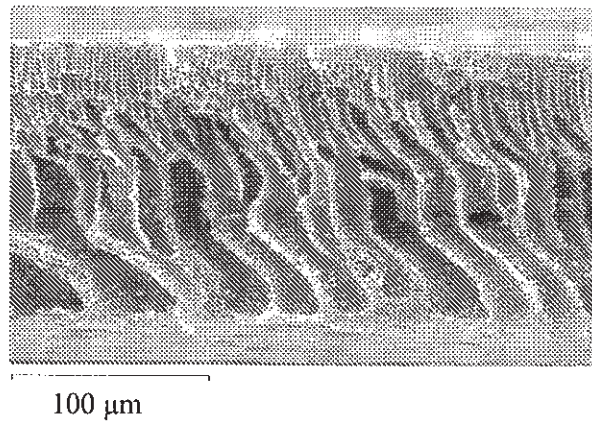


FIG. 25C



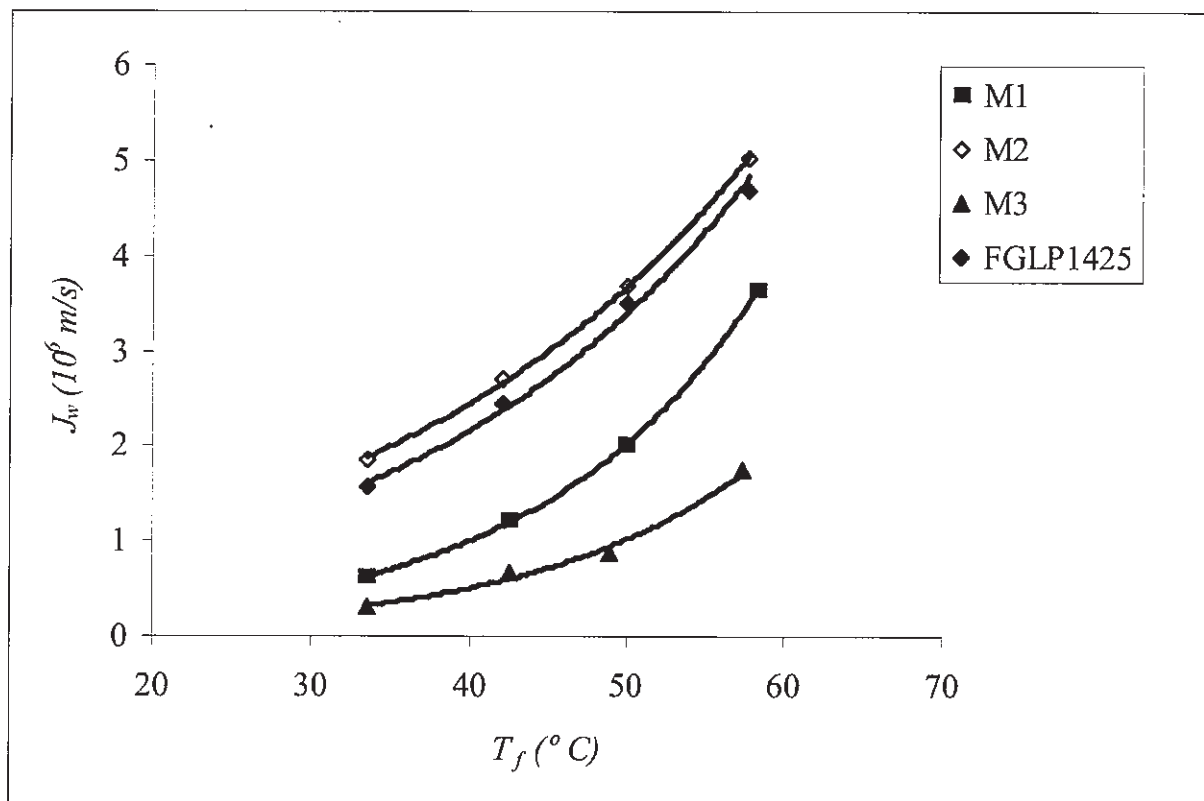


FIG. 26A

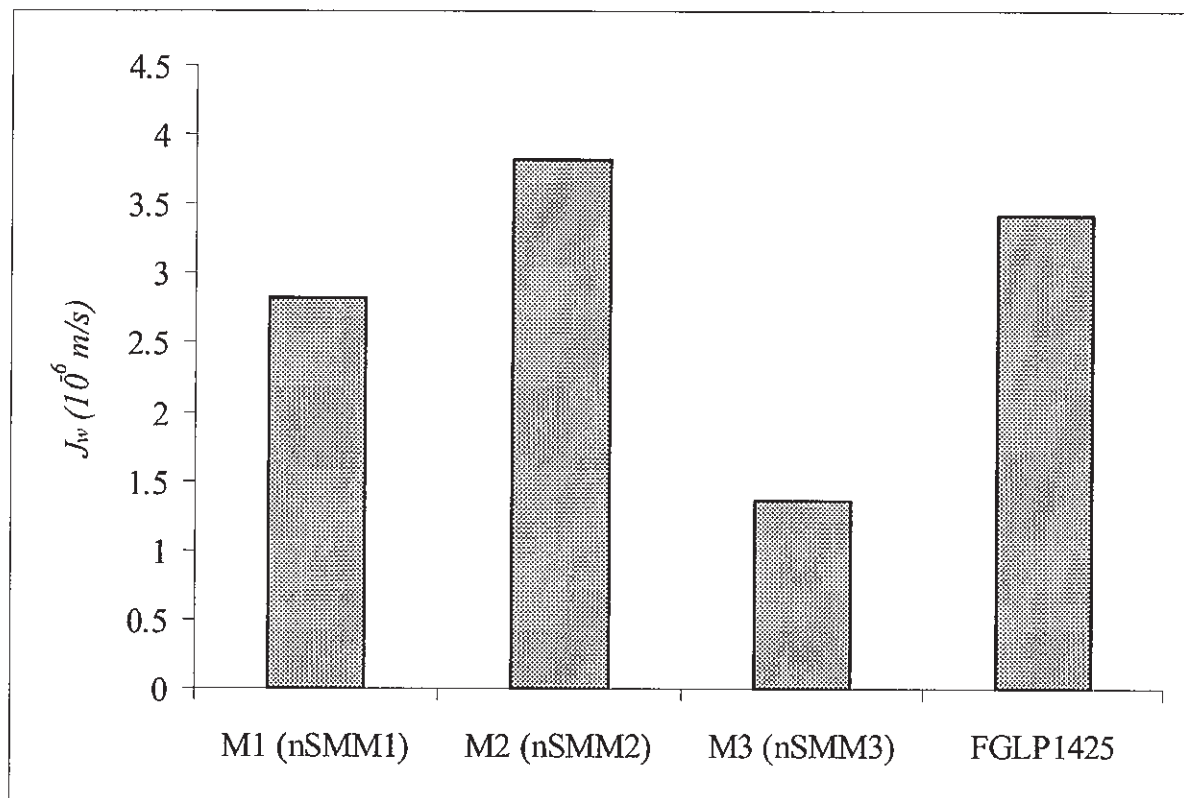


FIG. 26B