

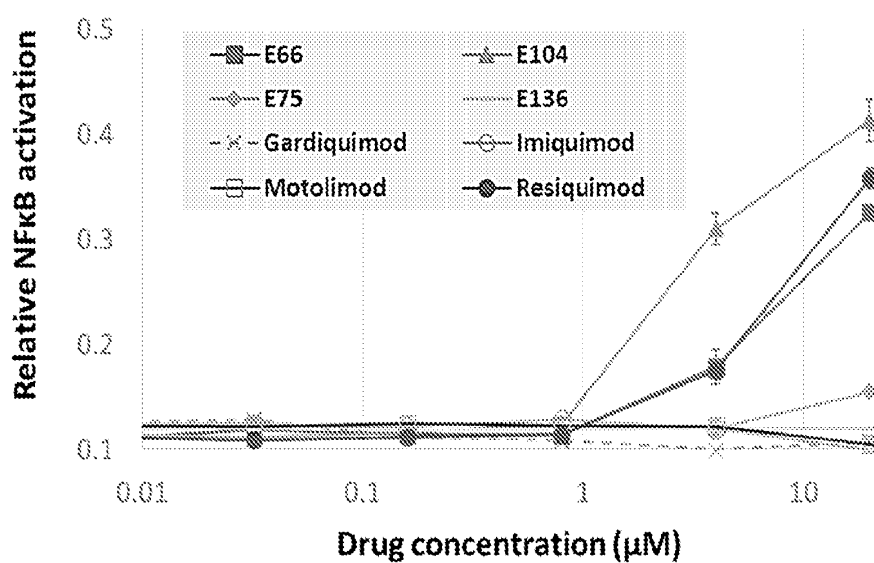
24h assay

FIG. 1A

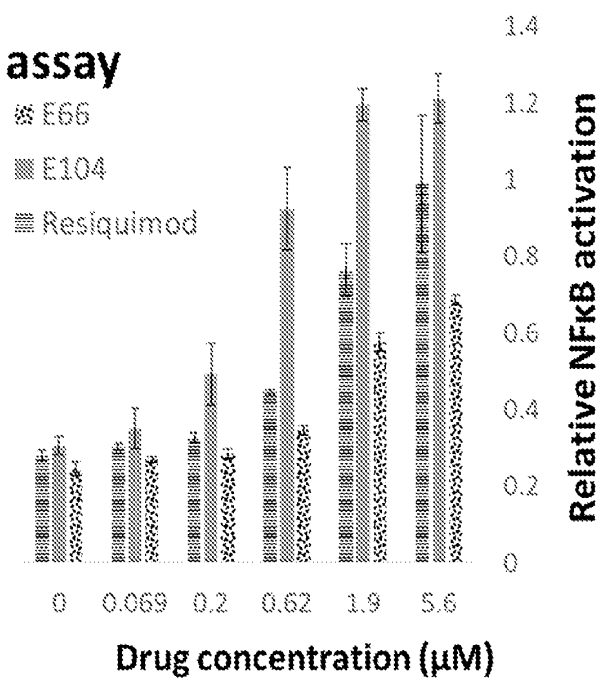
72h assay

FIG. 1B

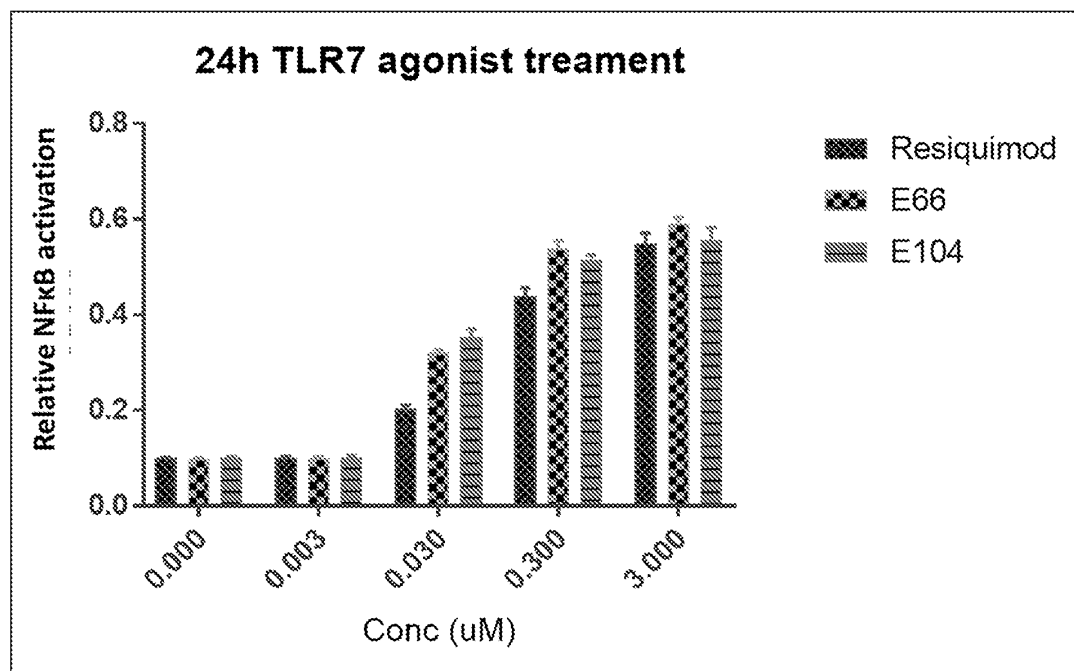


FIG. 2

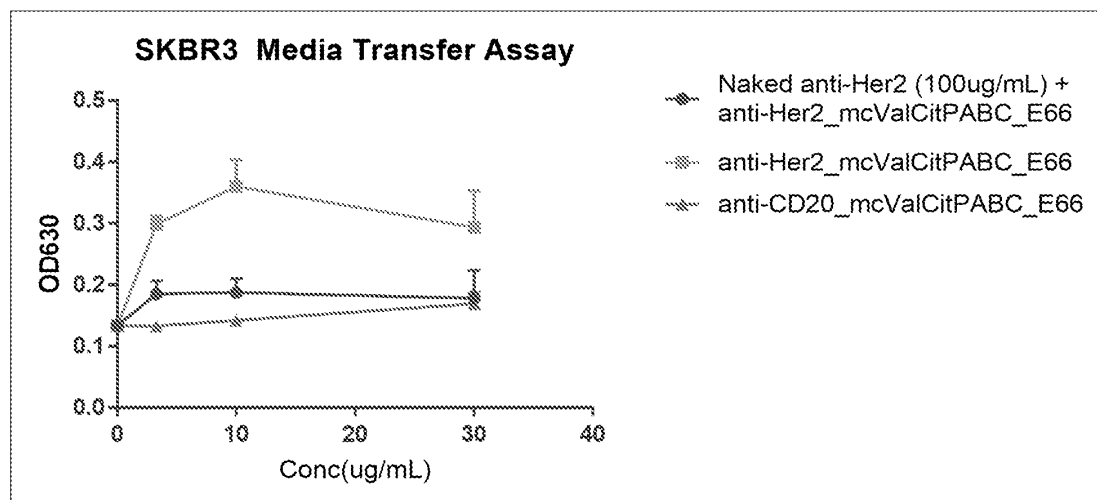


FIG. 3



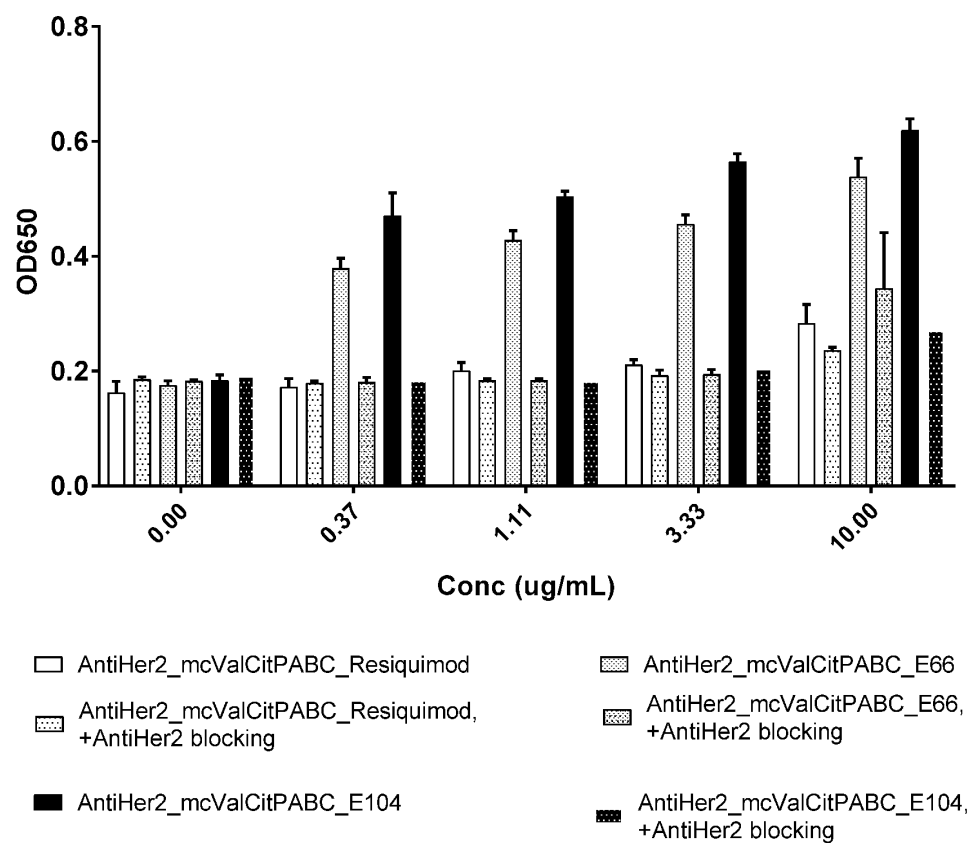


FIG. 4

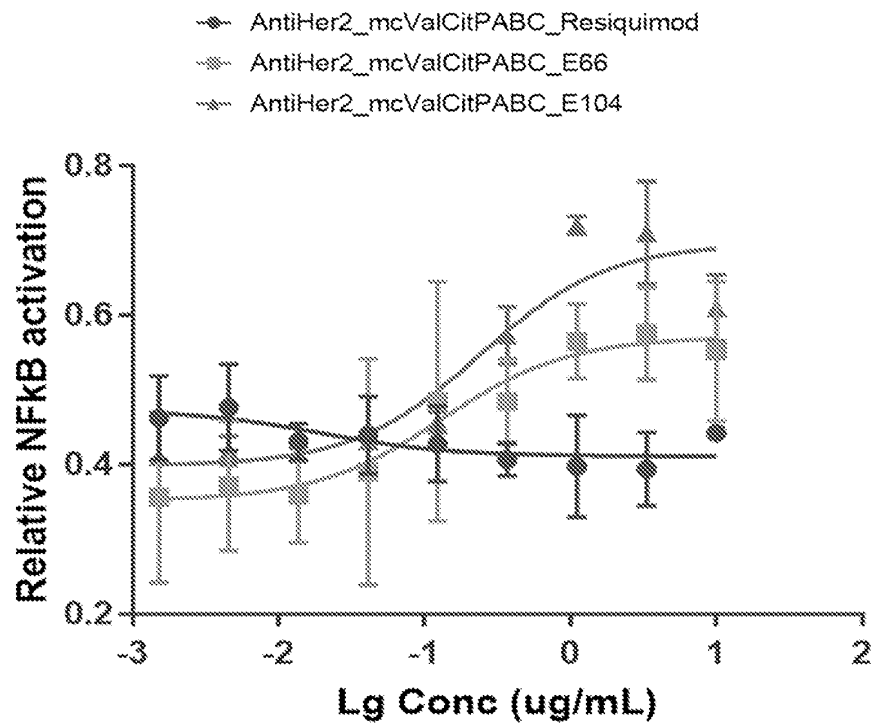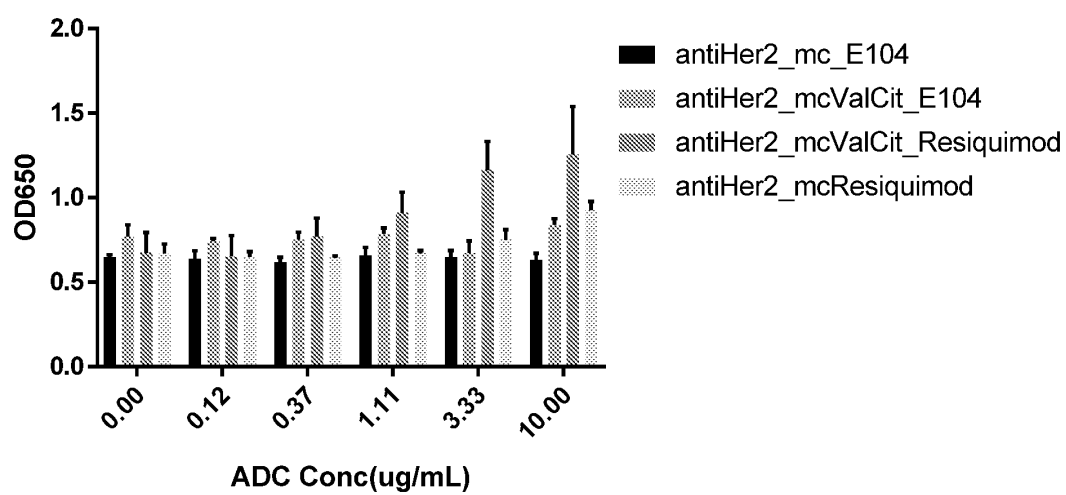

ABC	IC ₅₀
Anti-Her2_ValCitPABC_Resiquimod	>10 µg/mL
Anti-Her2_ValCitPABC_E66	0.13 µg/mL
Anti-Her2_ValCitPABC_E104	0.24 µg/mL

FIG. 5

Activity of ADCs without the PABC spacer**FIG. 6**


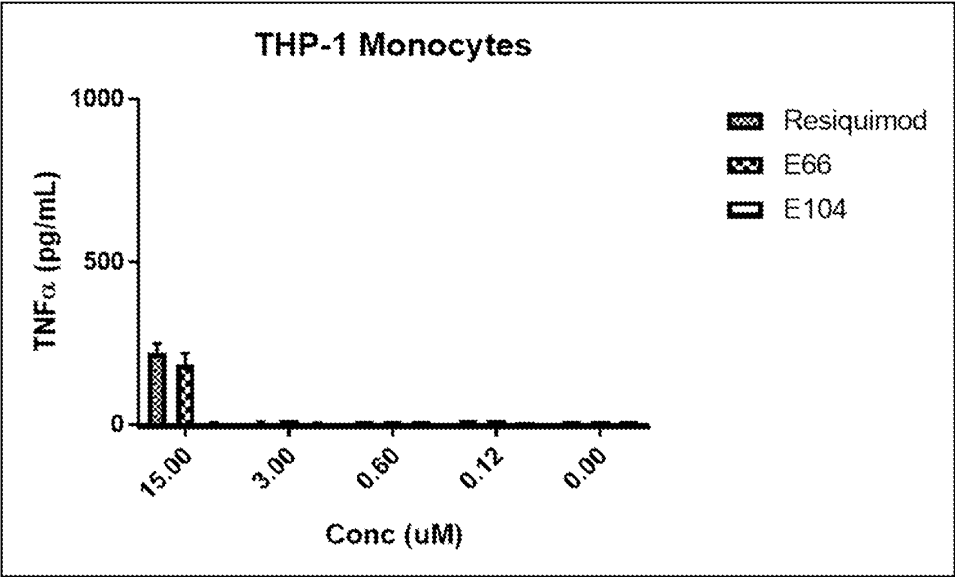


FIG. 7A

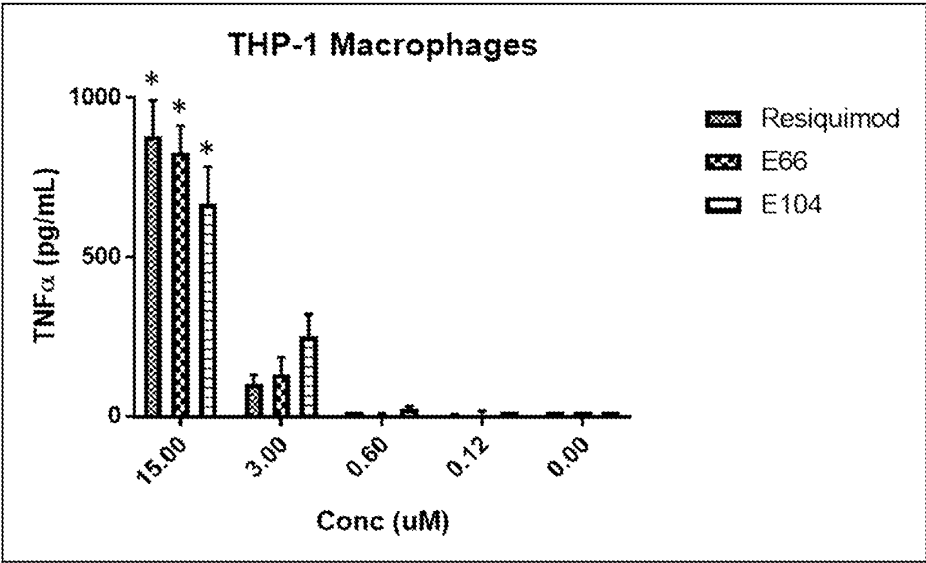

* Outside calibration range

FIG. 7B

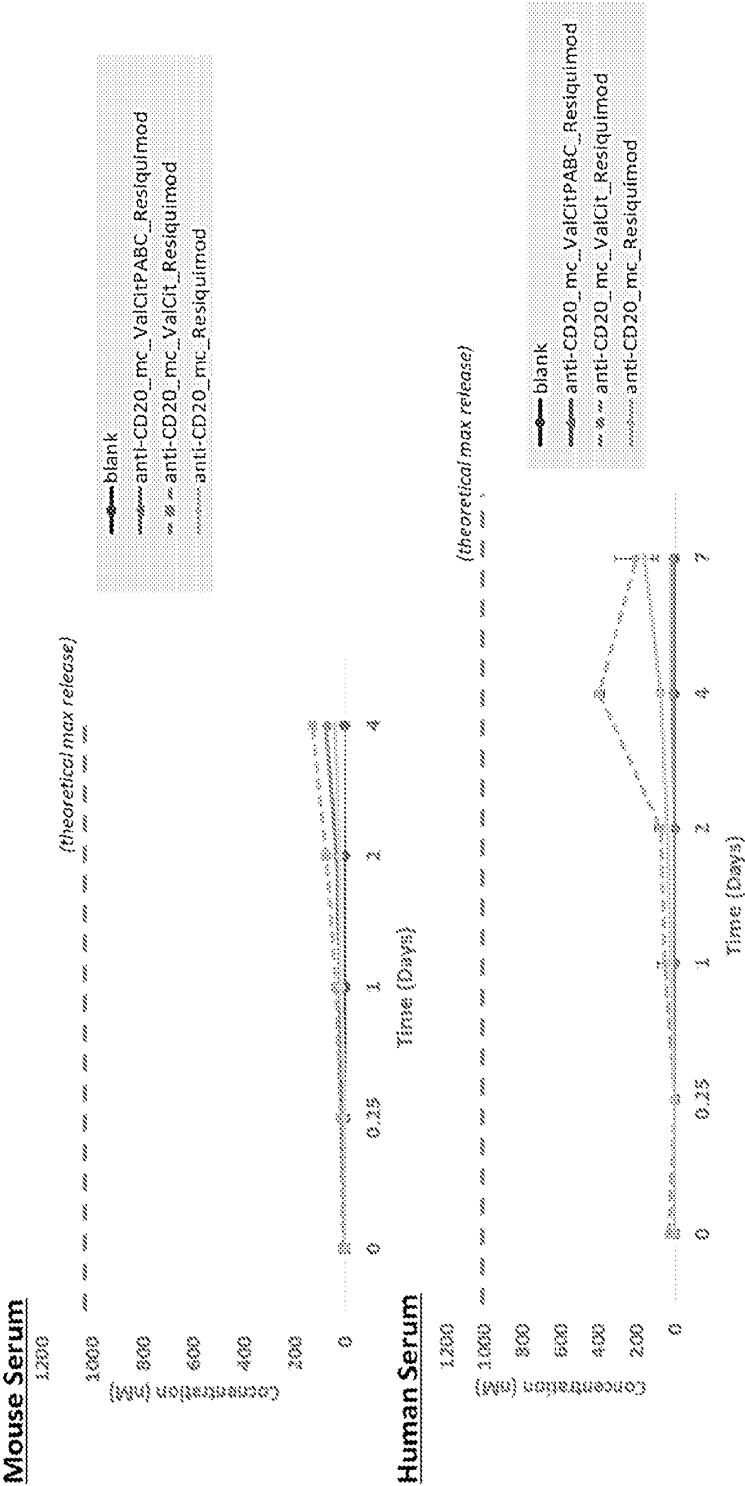
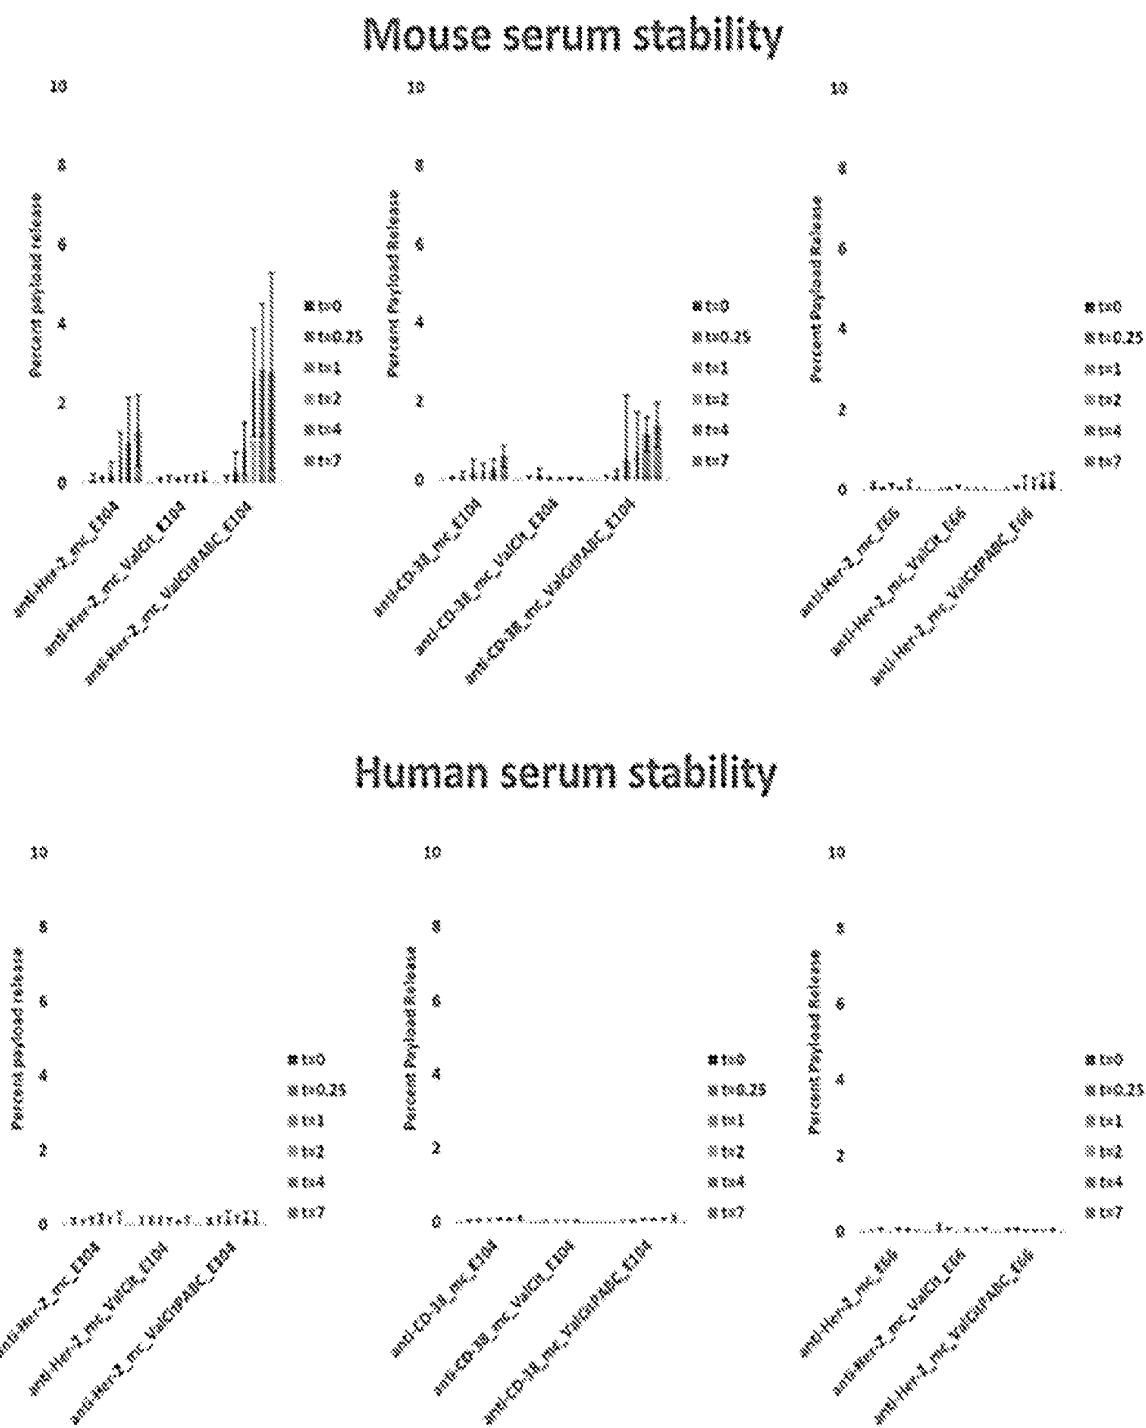


FIG. 8



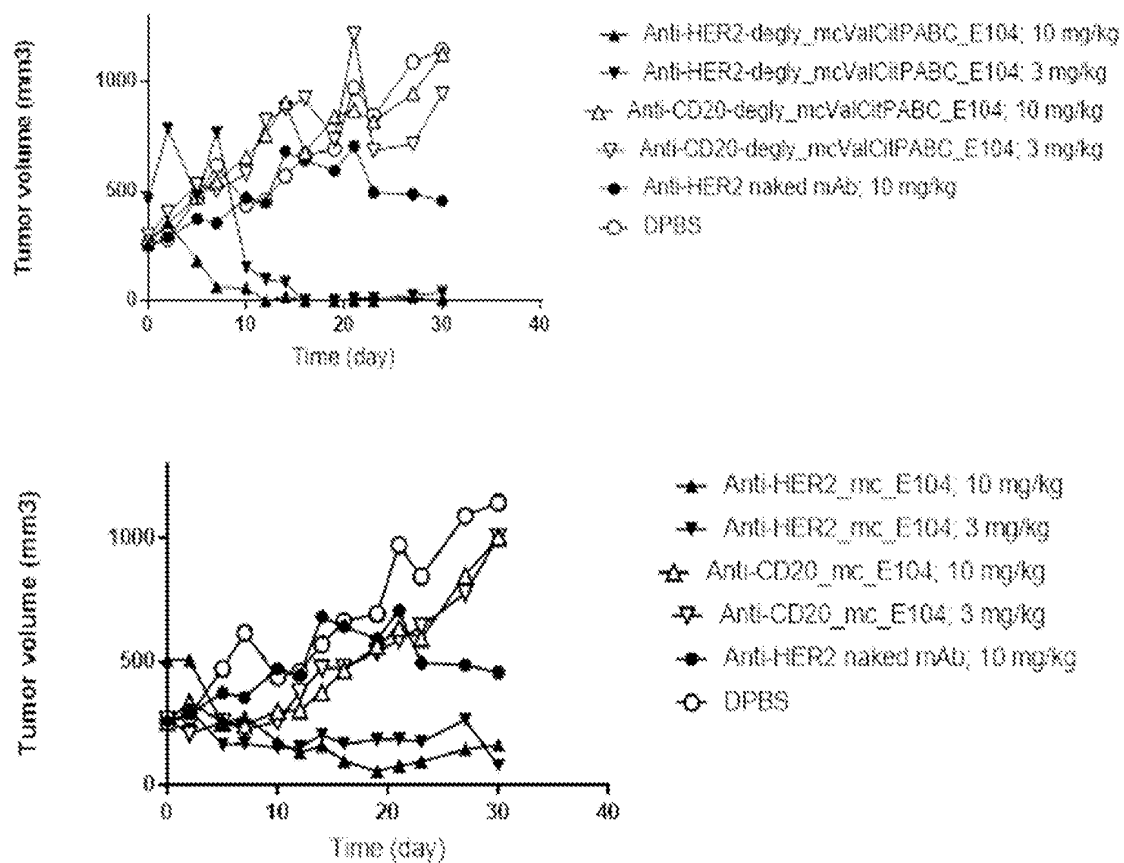


FIG. 10

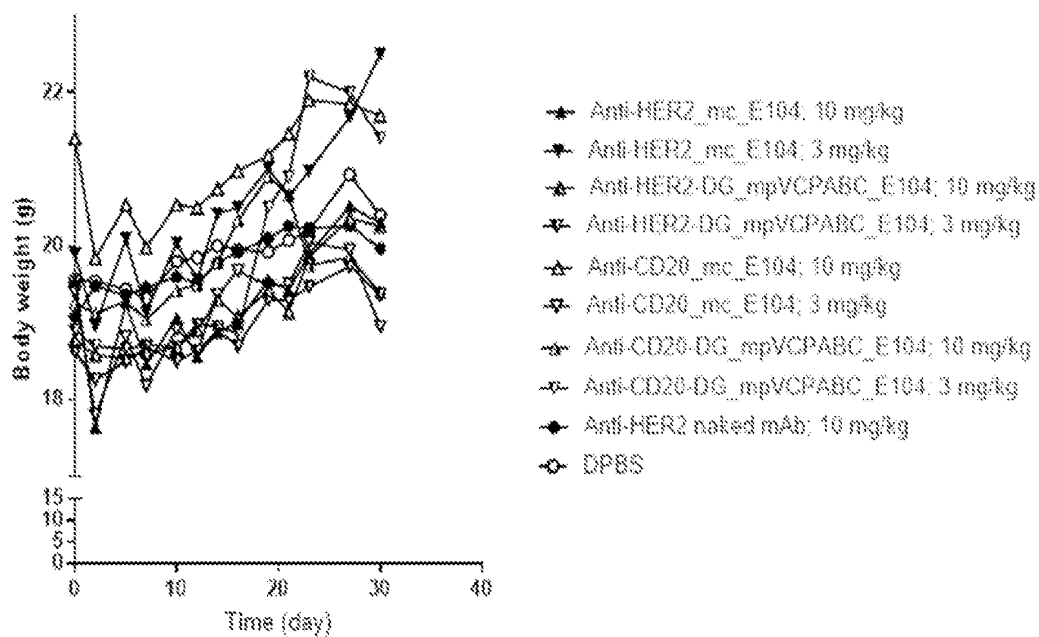


FIG. 11

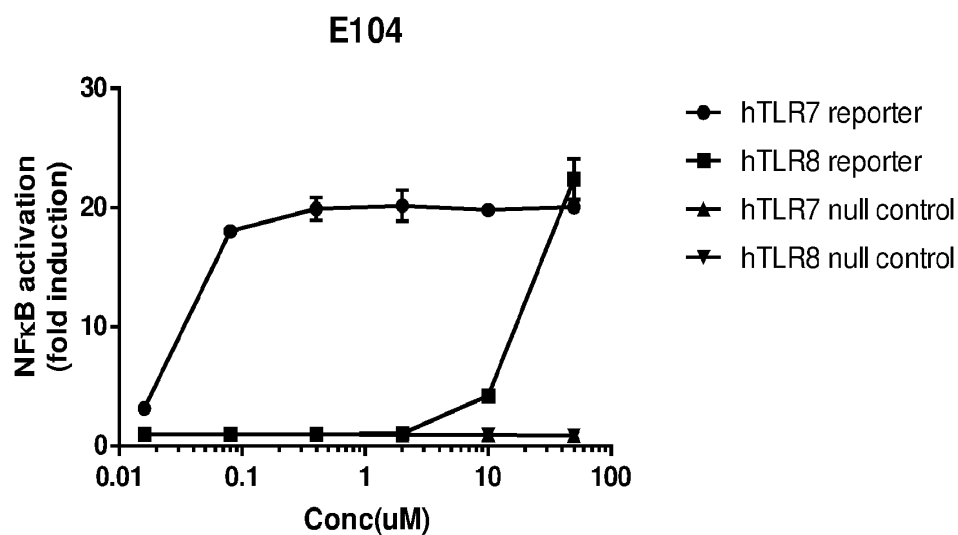


FIG. 12

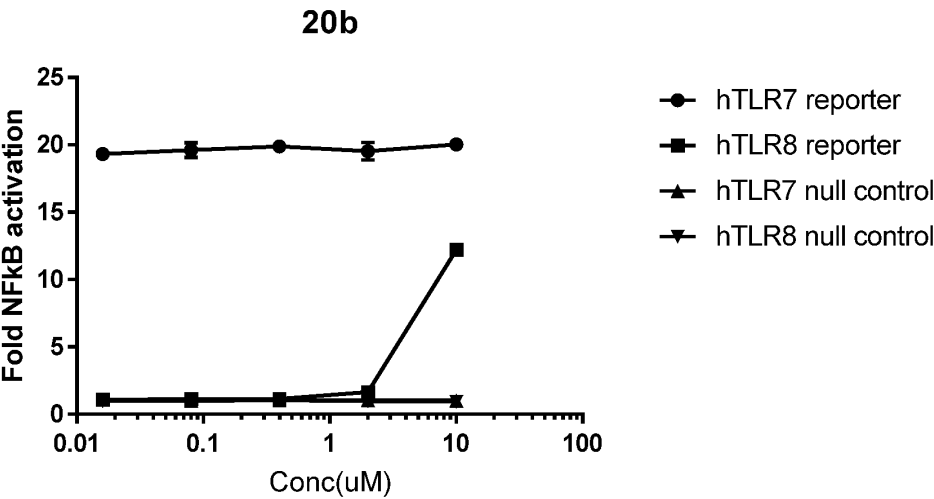


FIG. 13

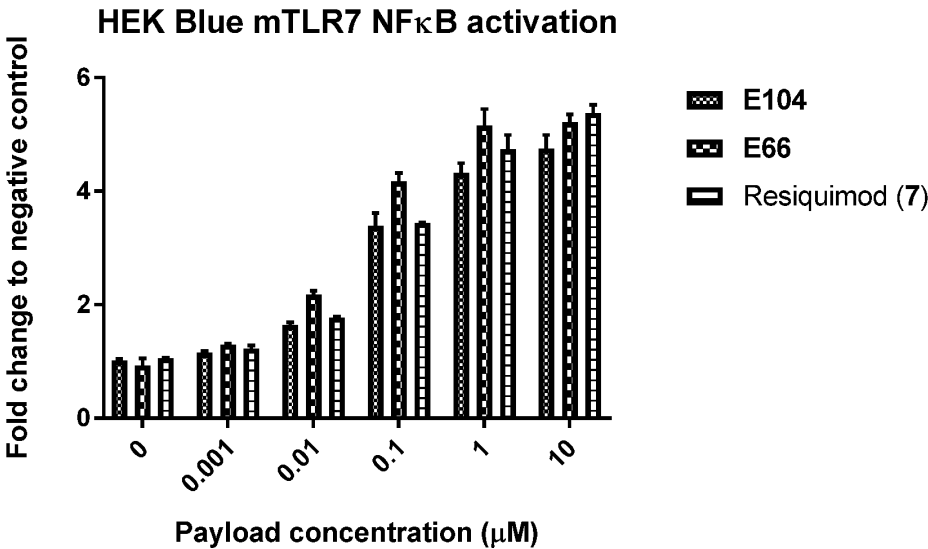


FIG. 14

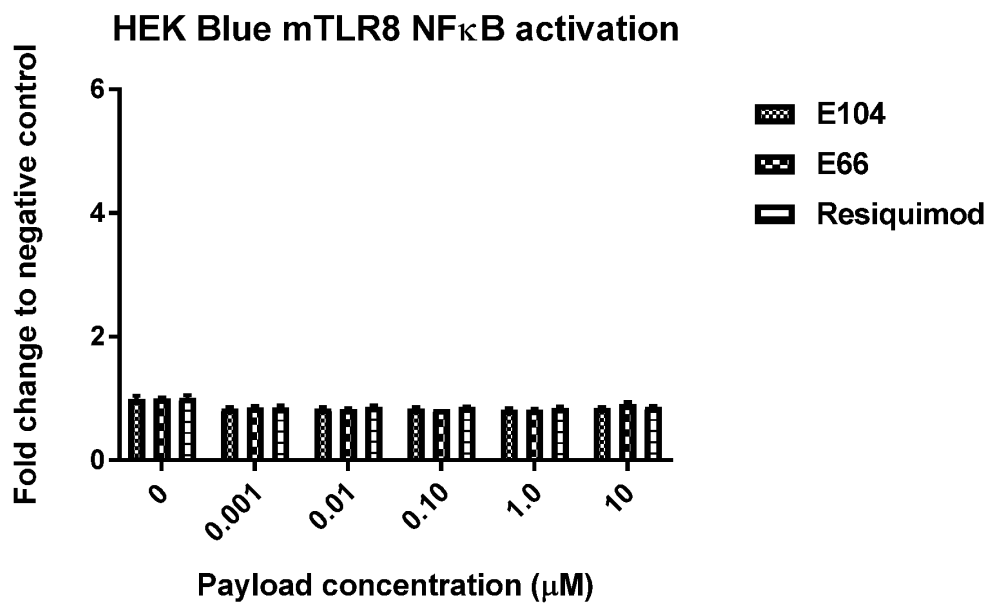


FIG. 15

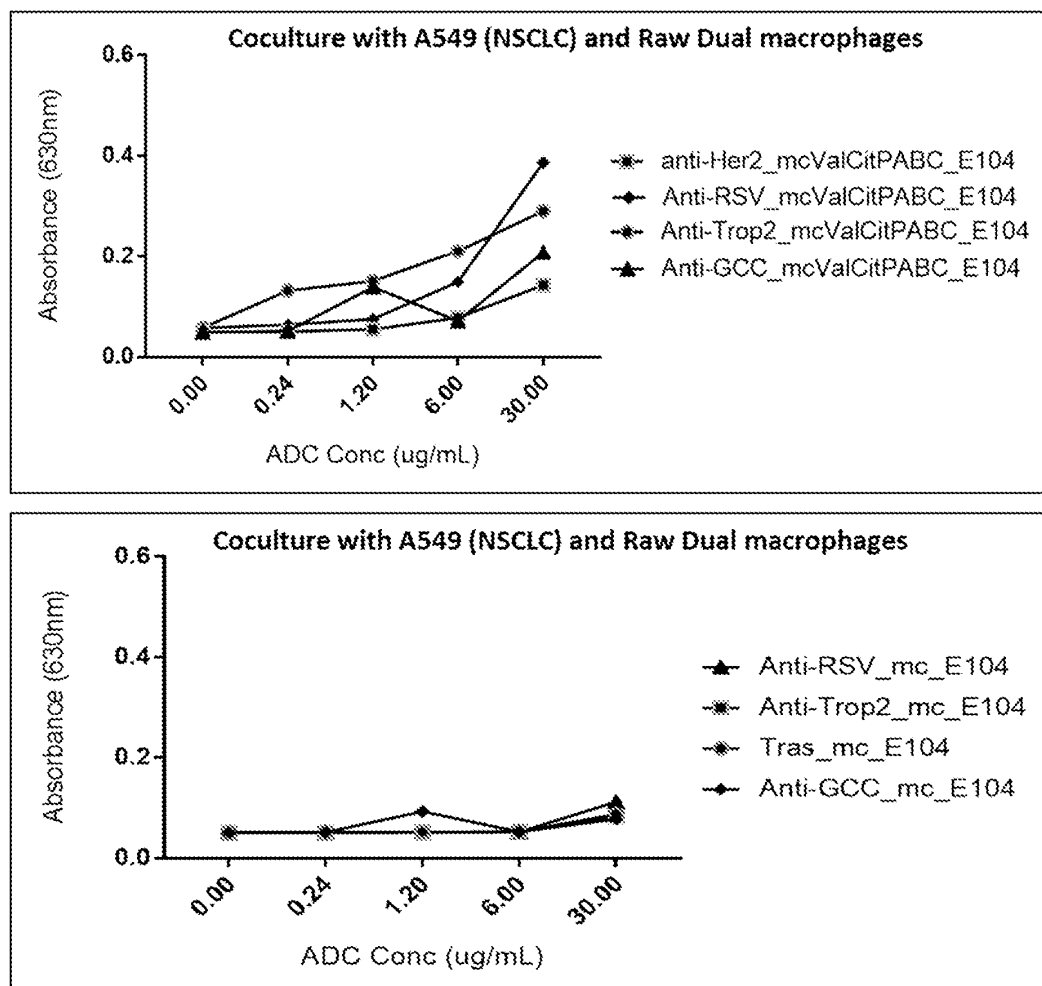


FIG. 16

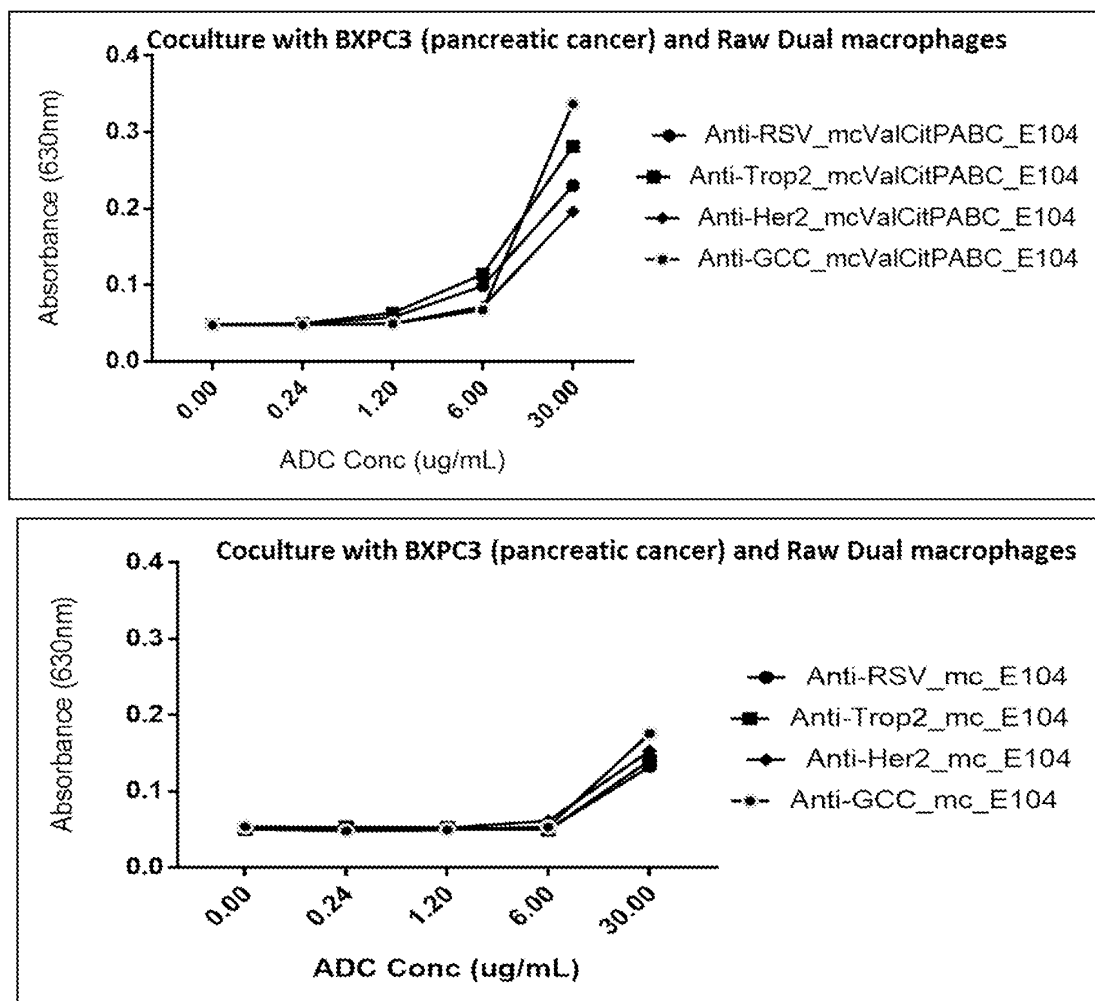


FIG. 17