

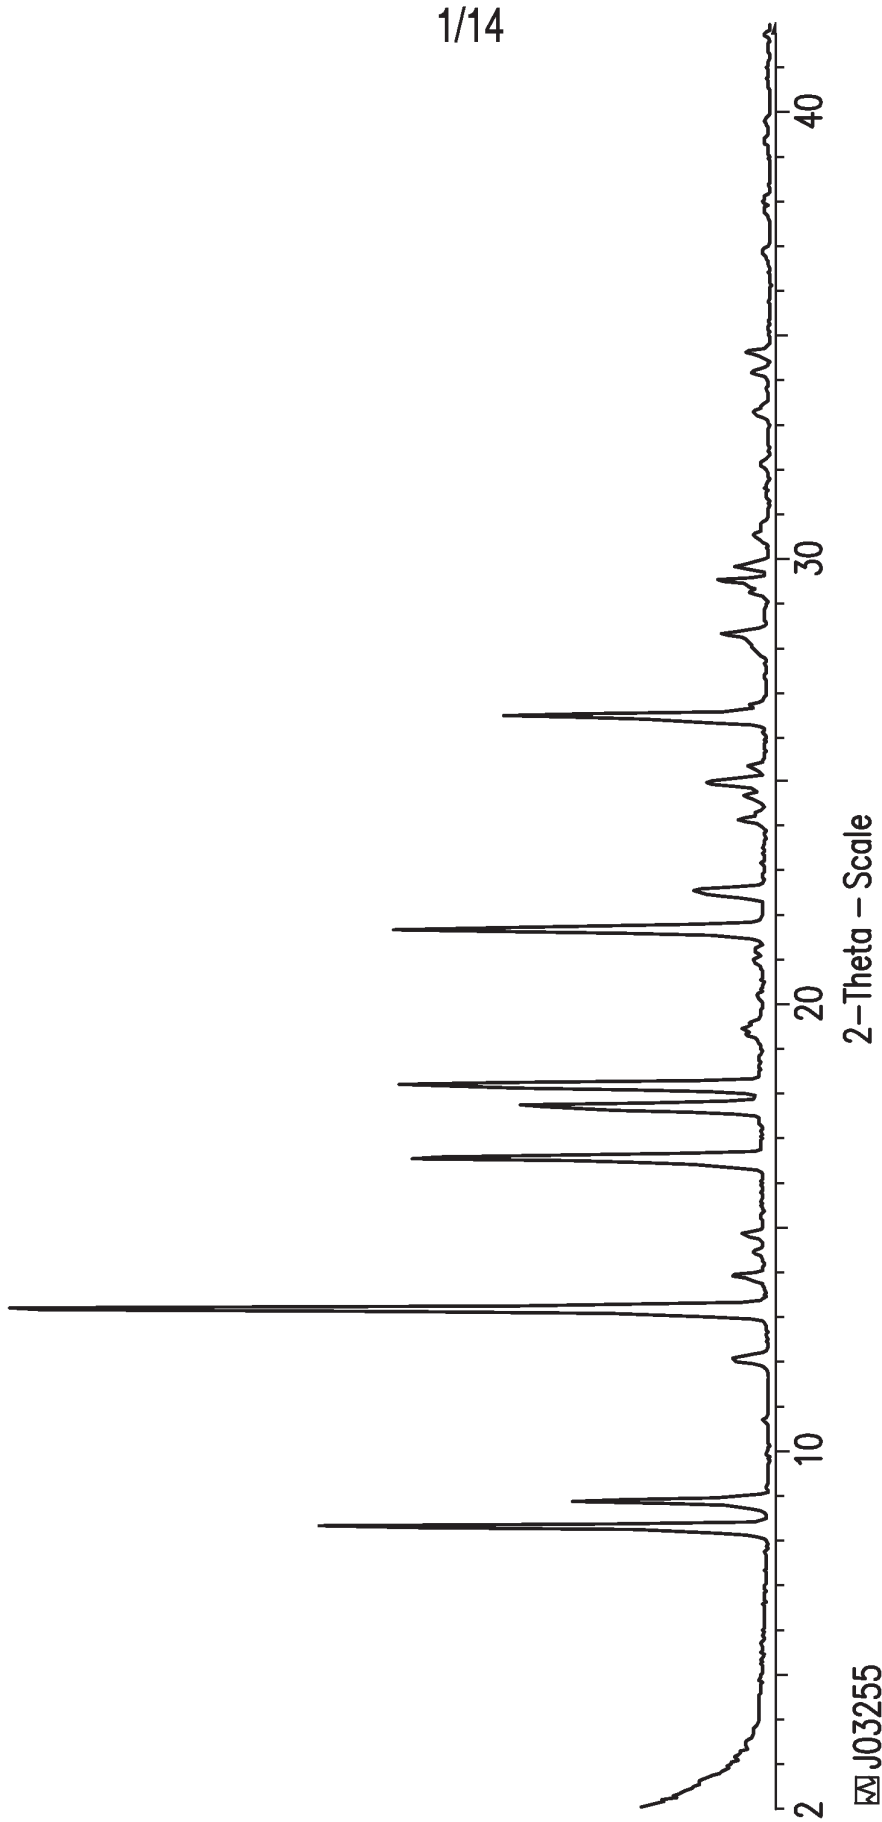


FIG. 1

2/14

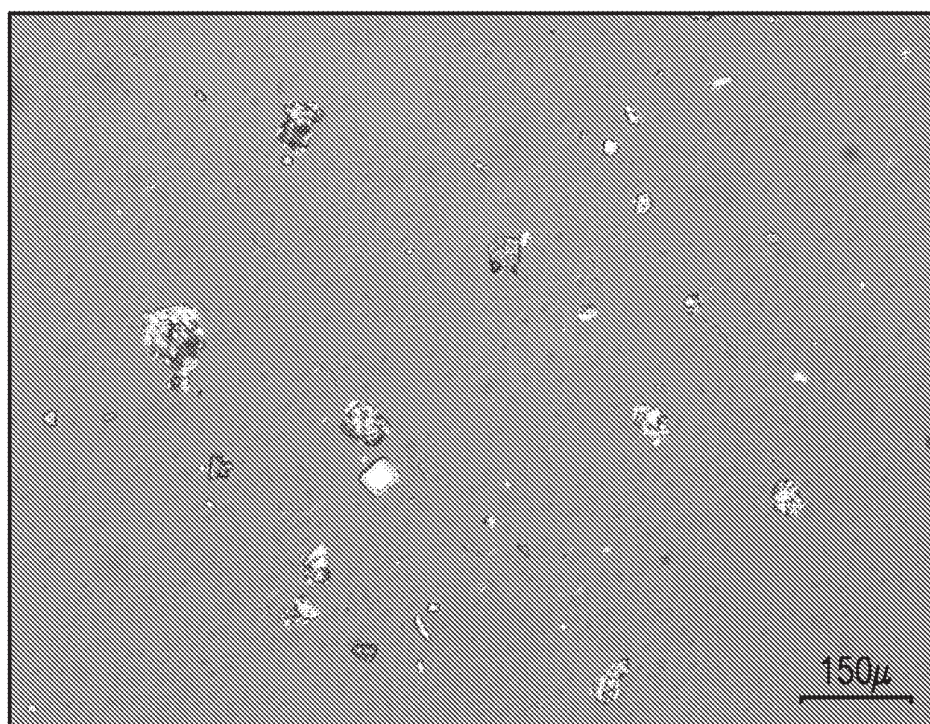


FIG. 2

3/14

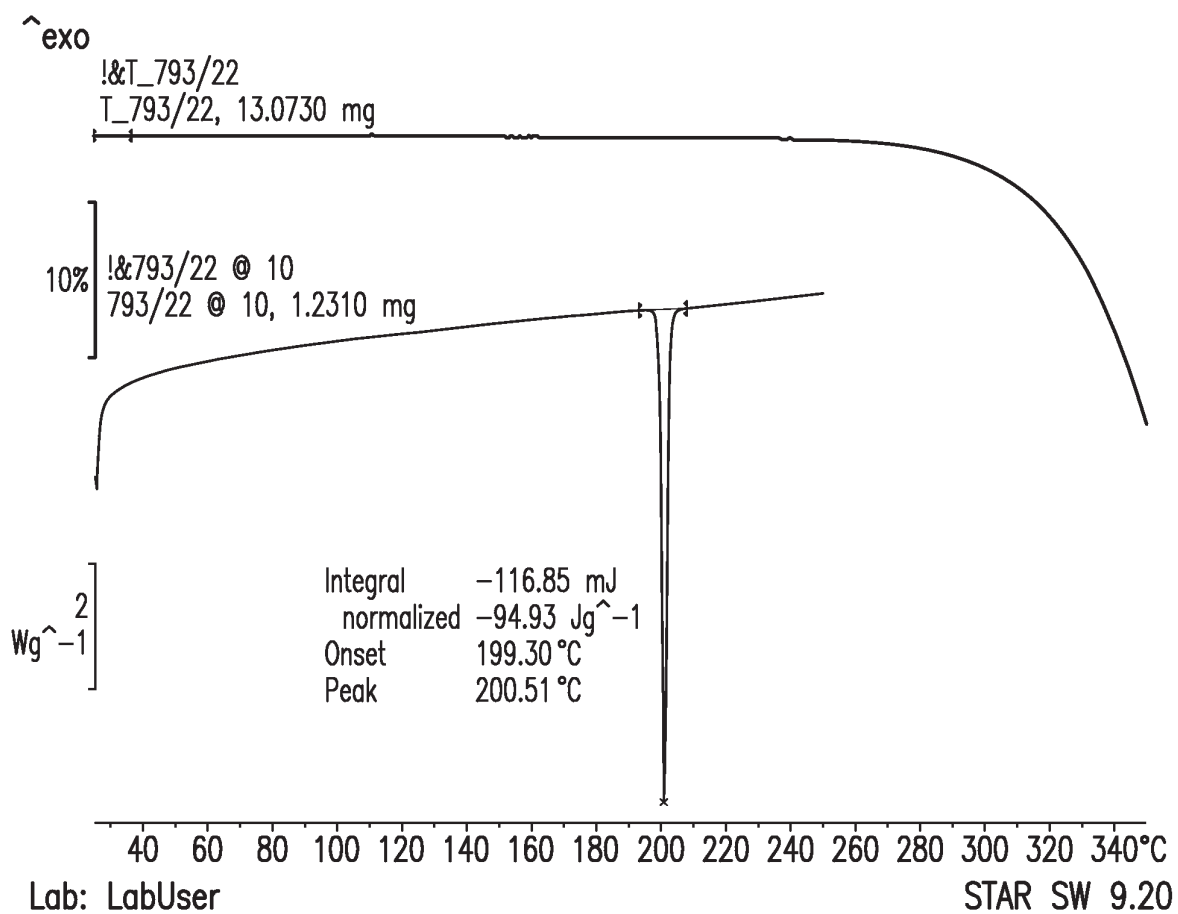


FIG. 3

4/14

Date: 17 Dec 2010

Time: 12:00am


File: J03255-Fri 17 Dec 2010 13-06-47.xls

Sample: J03255

Temp: 25.0°C

Meth: SingleCycle_LowMass.sao

MRef: 8.0191

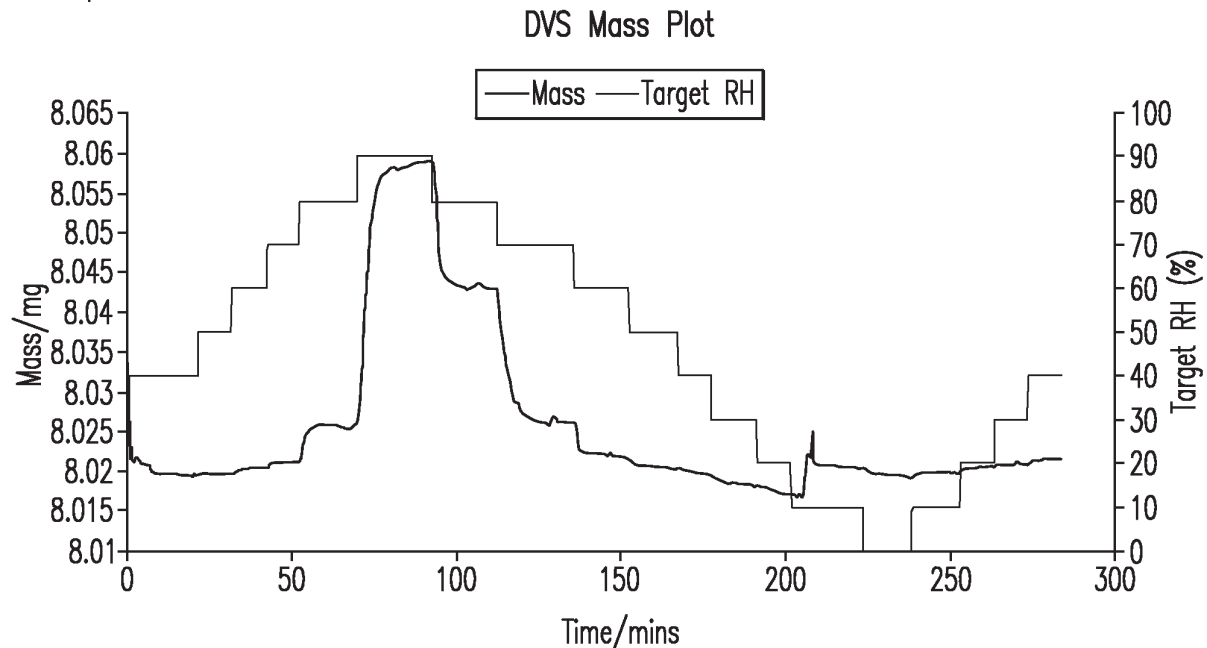

DVS-The Sorption Solution

©SurfaceMeasurementSystems Ltd UK 1996-2007

Date: 17 Dec 2010

Time: 12:00am


File: J03255-Fri 17 Dec 2010 13-06-47.xls

Sample: J03255

Temp: 25.0°C

Meth: SingleCycle_LowMass.sao

MRef: 8.0191

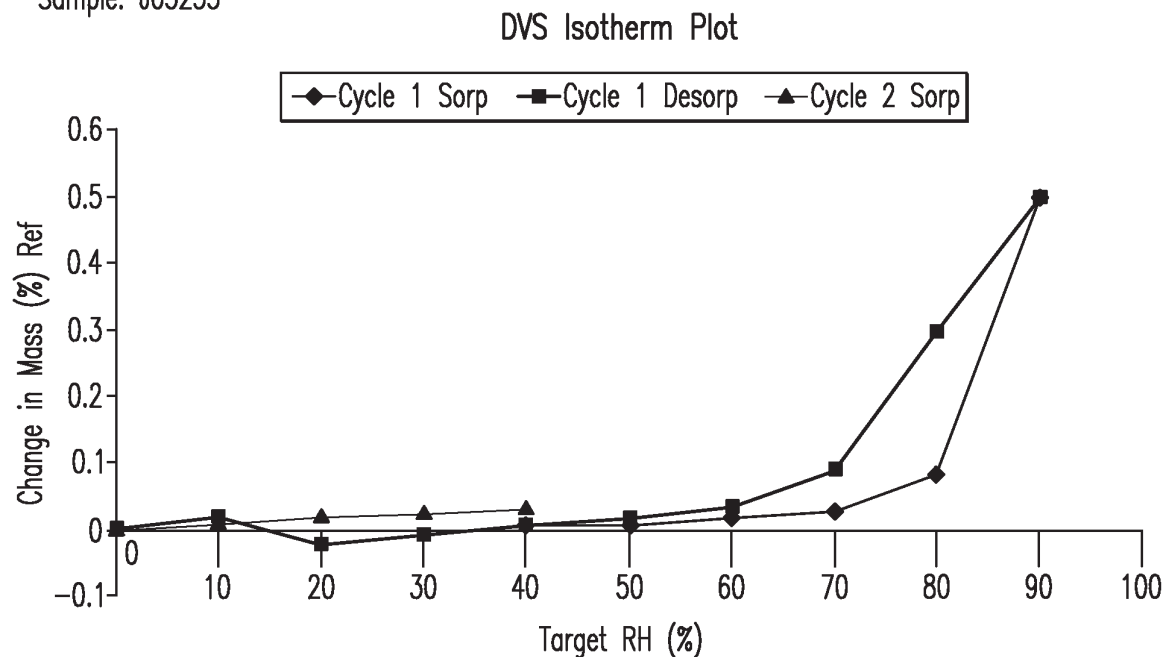

DVS-The Sorption Solution

©SurfaceMeasurementSystems Ltd UK 1996-2007

FIG. 4

SUBSTITUTE SHEET (RULE 26)

5/14

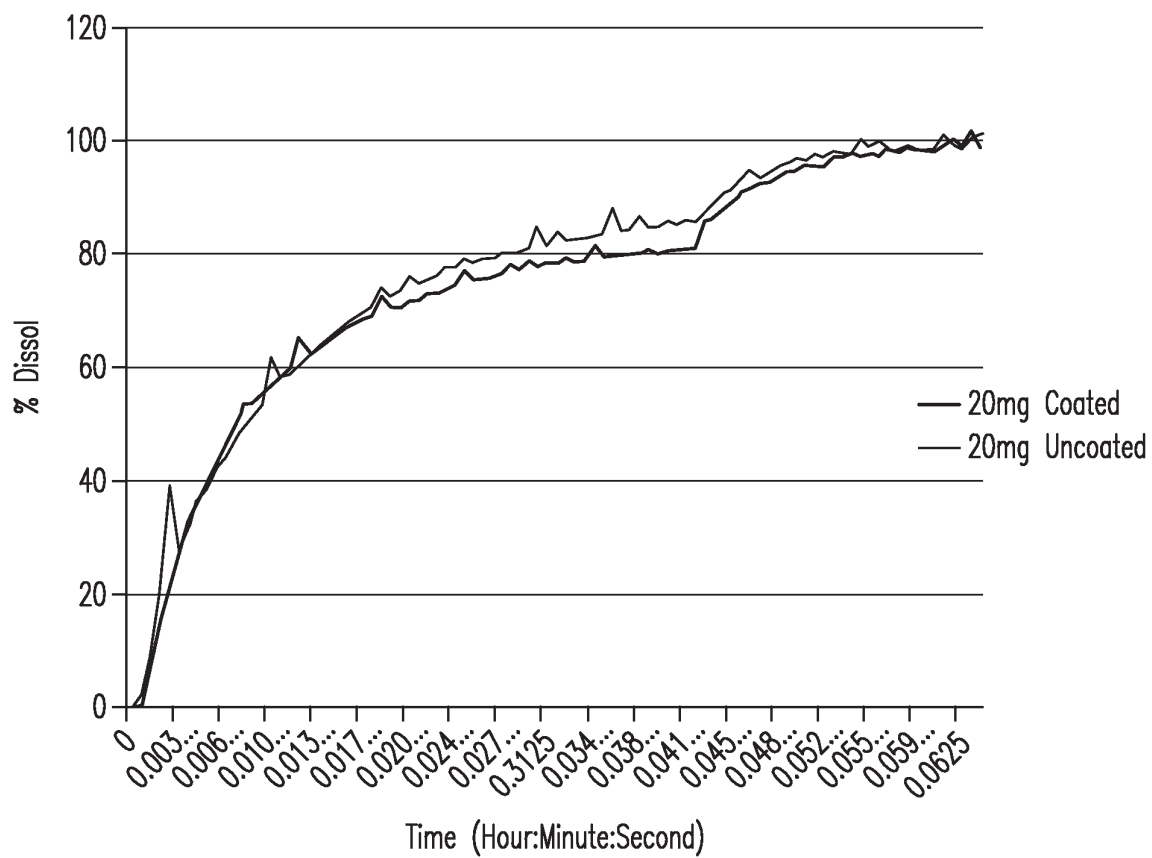


FIG. 5

6/14

Method: 20 to 300, 10 cpm

Run Date: 02-Mar-2012 11:01

Instrument: DSC Q2000 V24.9 Build 121

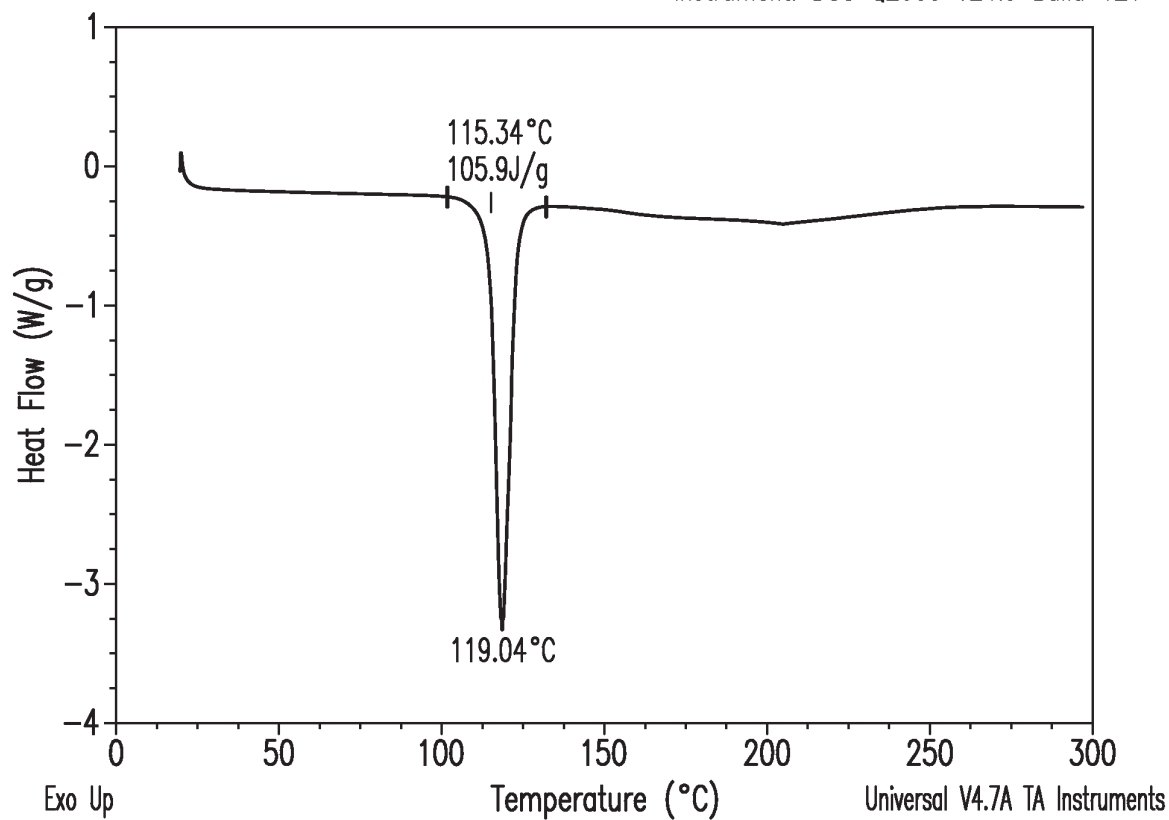


FIG. 6

7/14

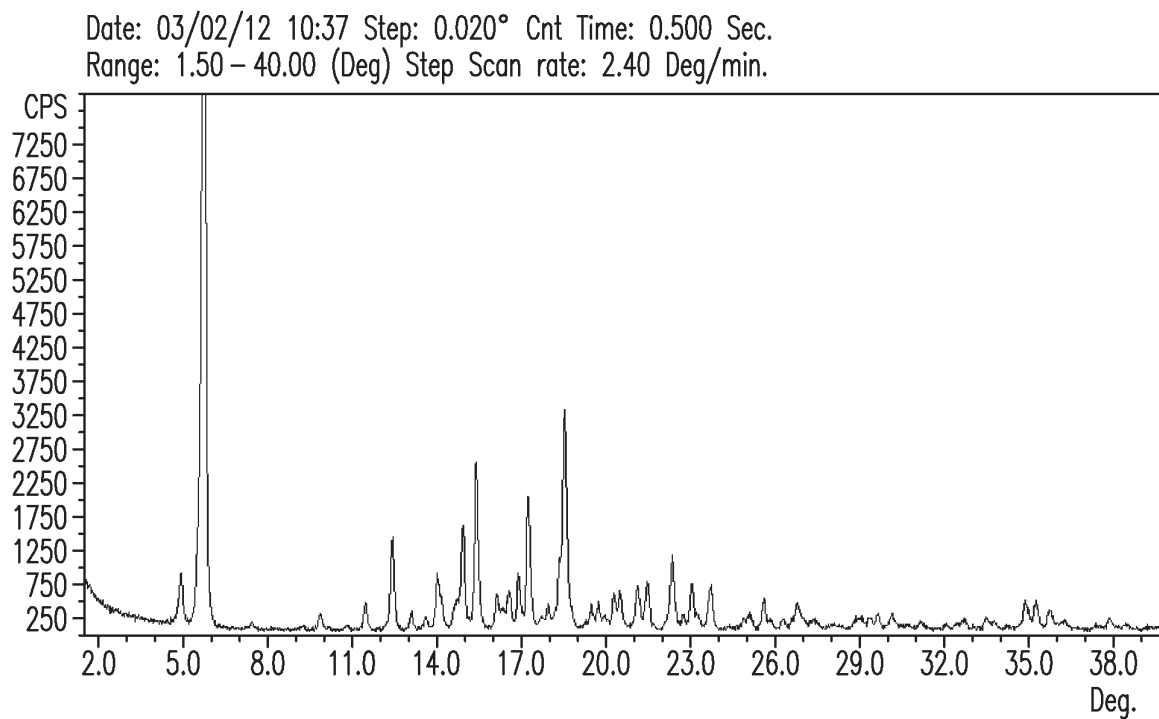


FIG. 7

8/14

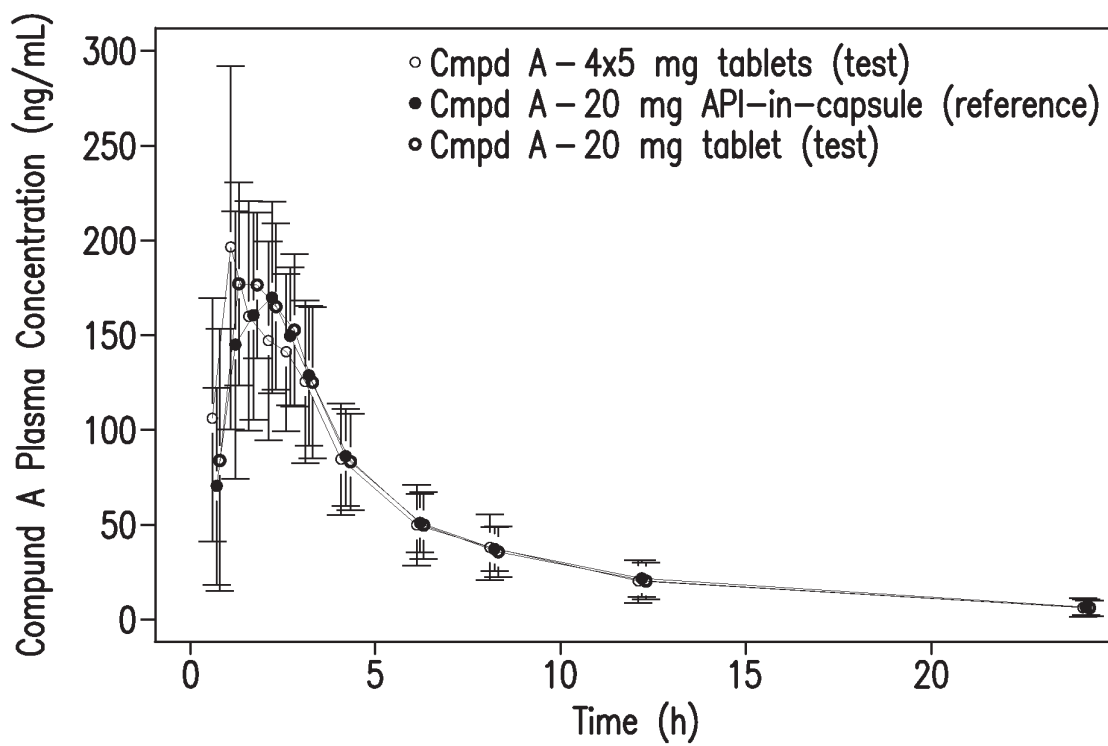


FIG. 8

9/14

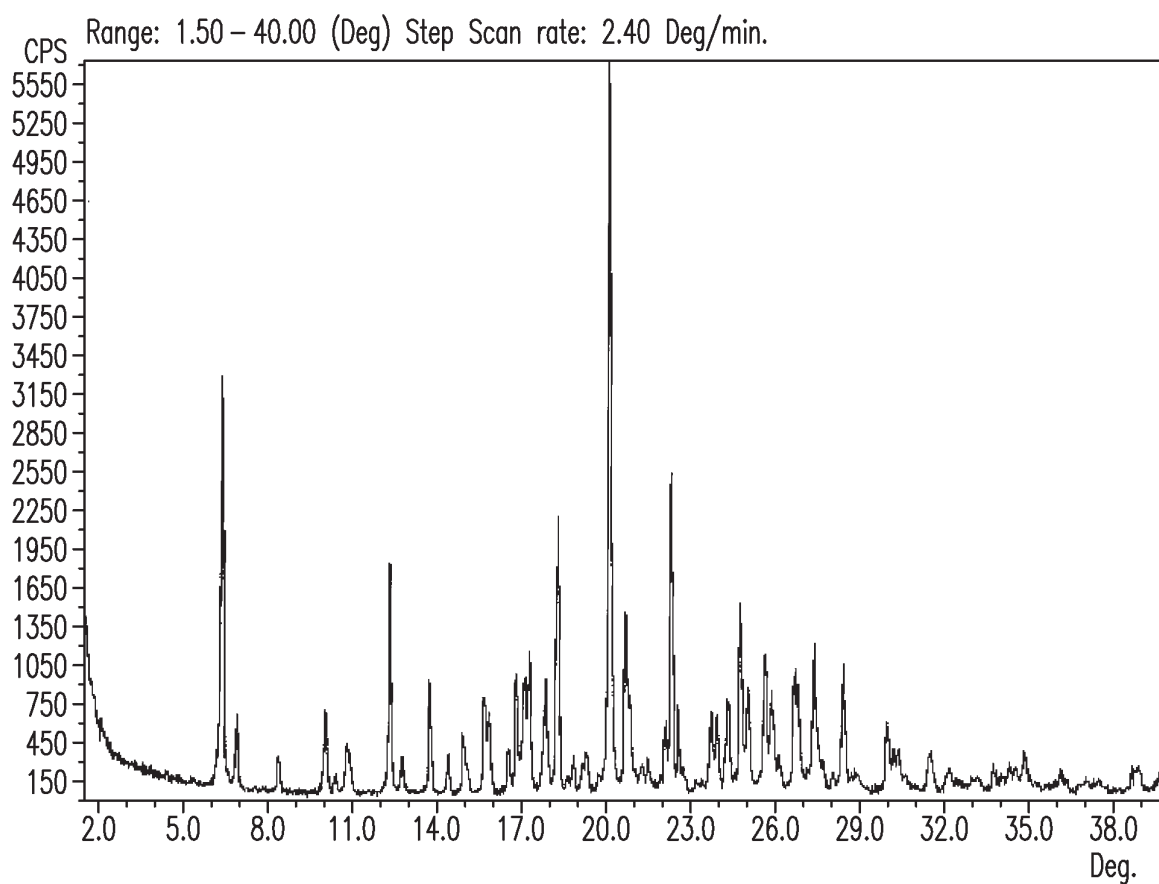


FIG. 9

10/14

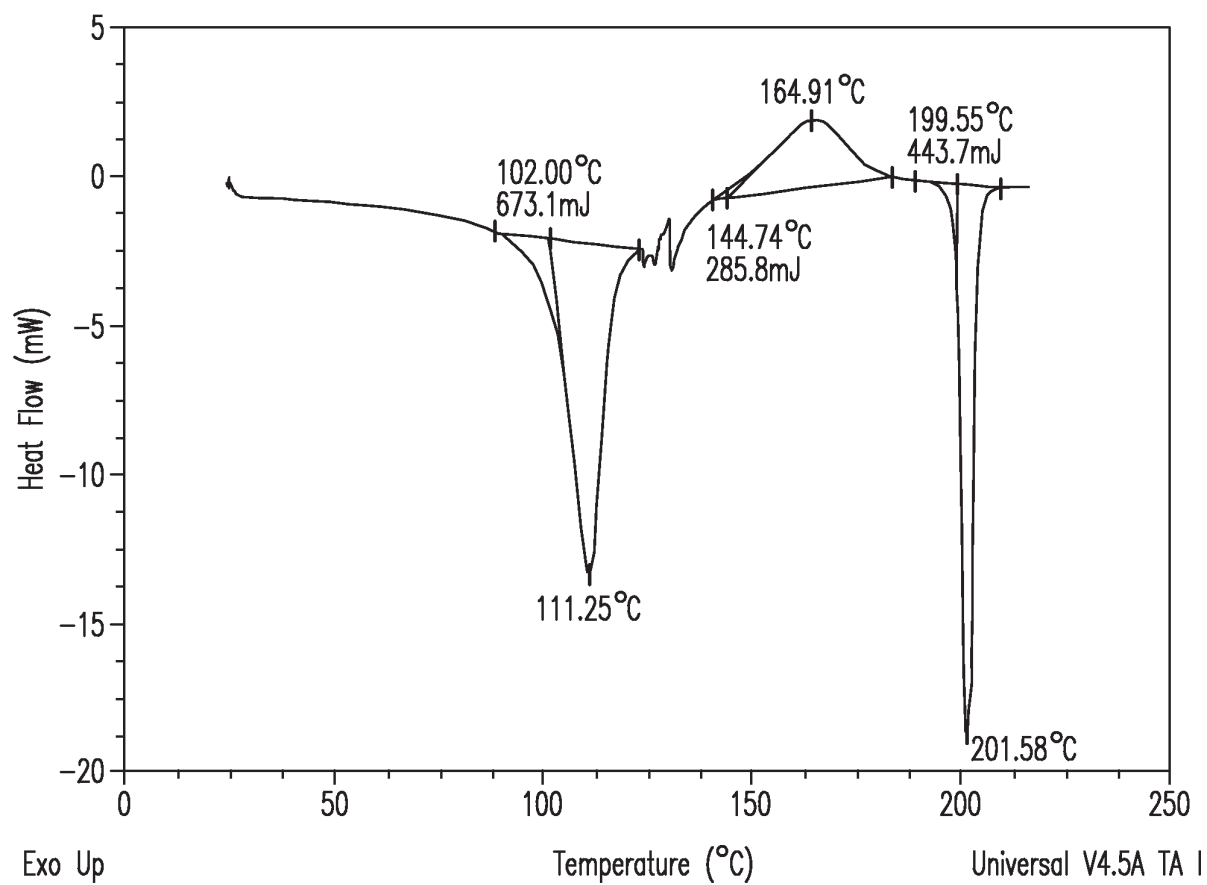


FIG. 10

11/14

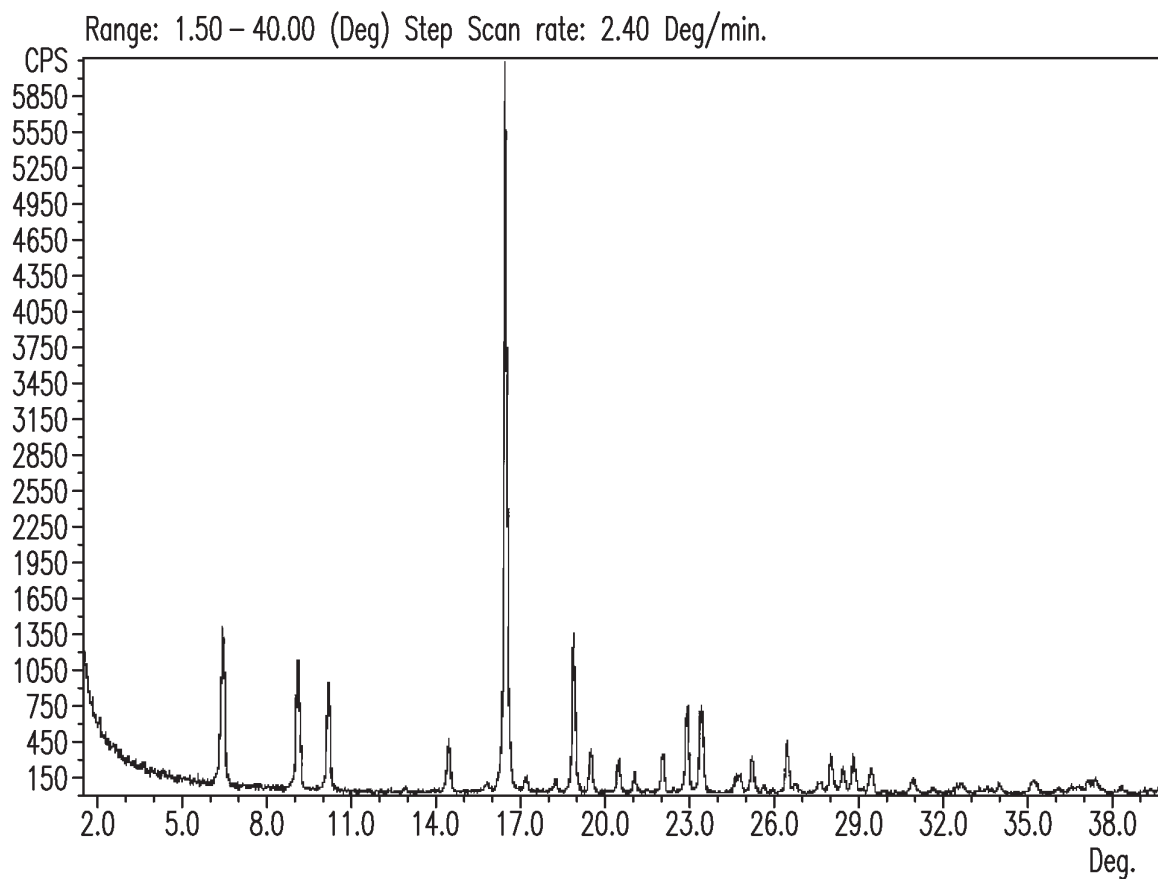


FIG. 11

12/14

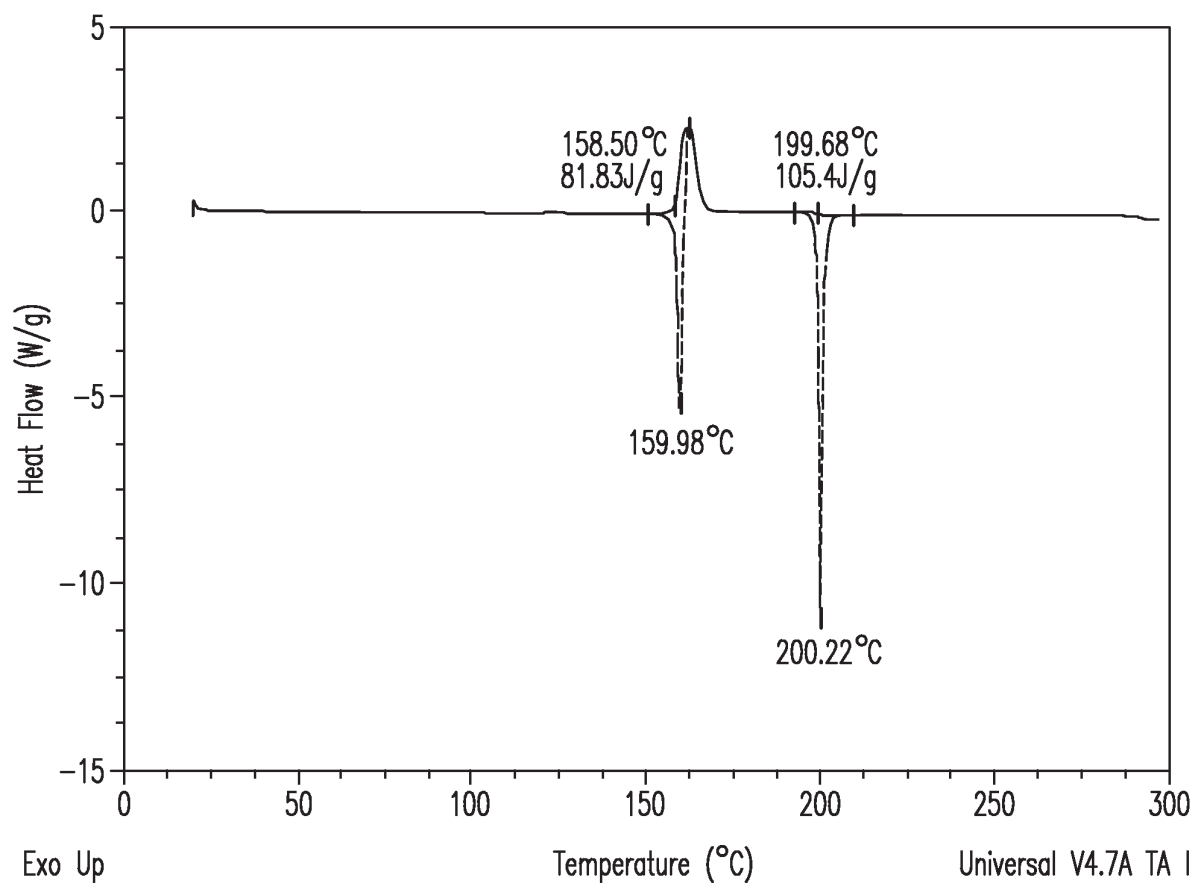


FIG. 12

13/14

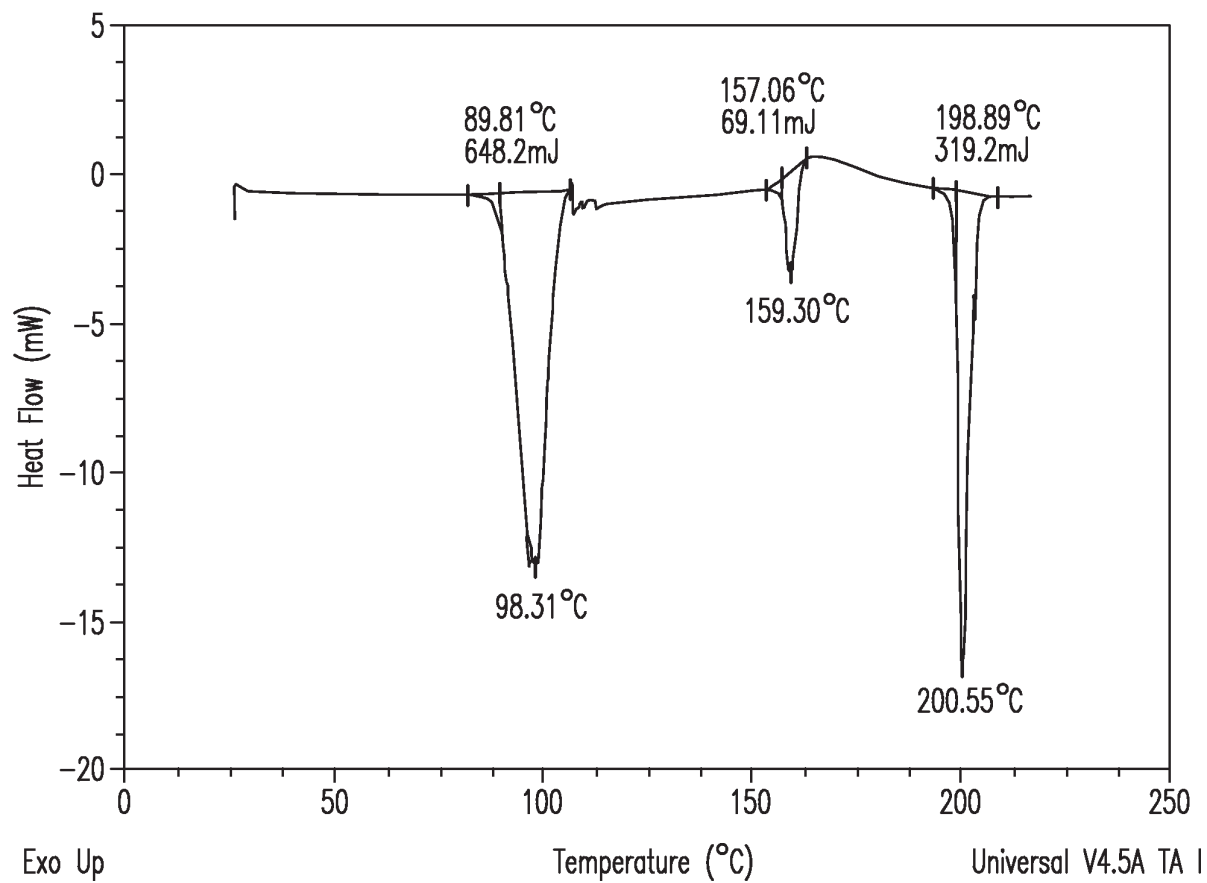


FIG. 13

14/14

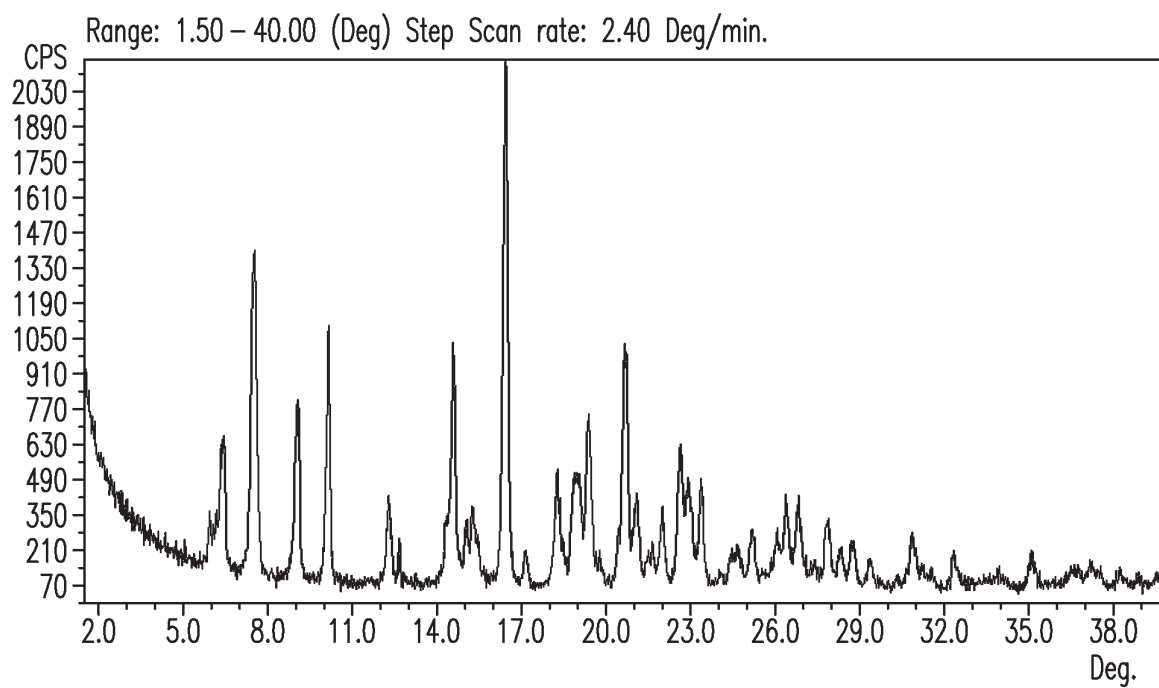


FIG. 14