

Sample Receipt and QC; DNA Isolation

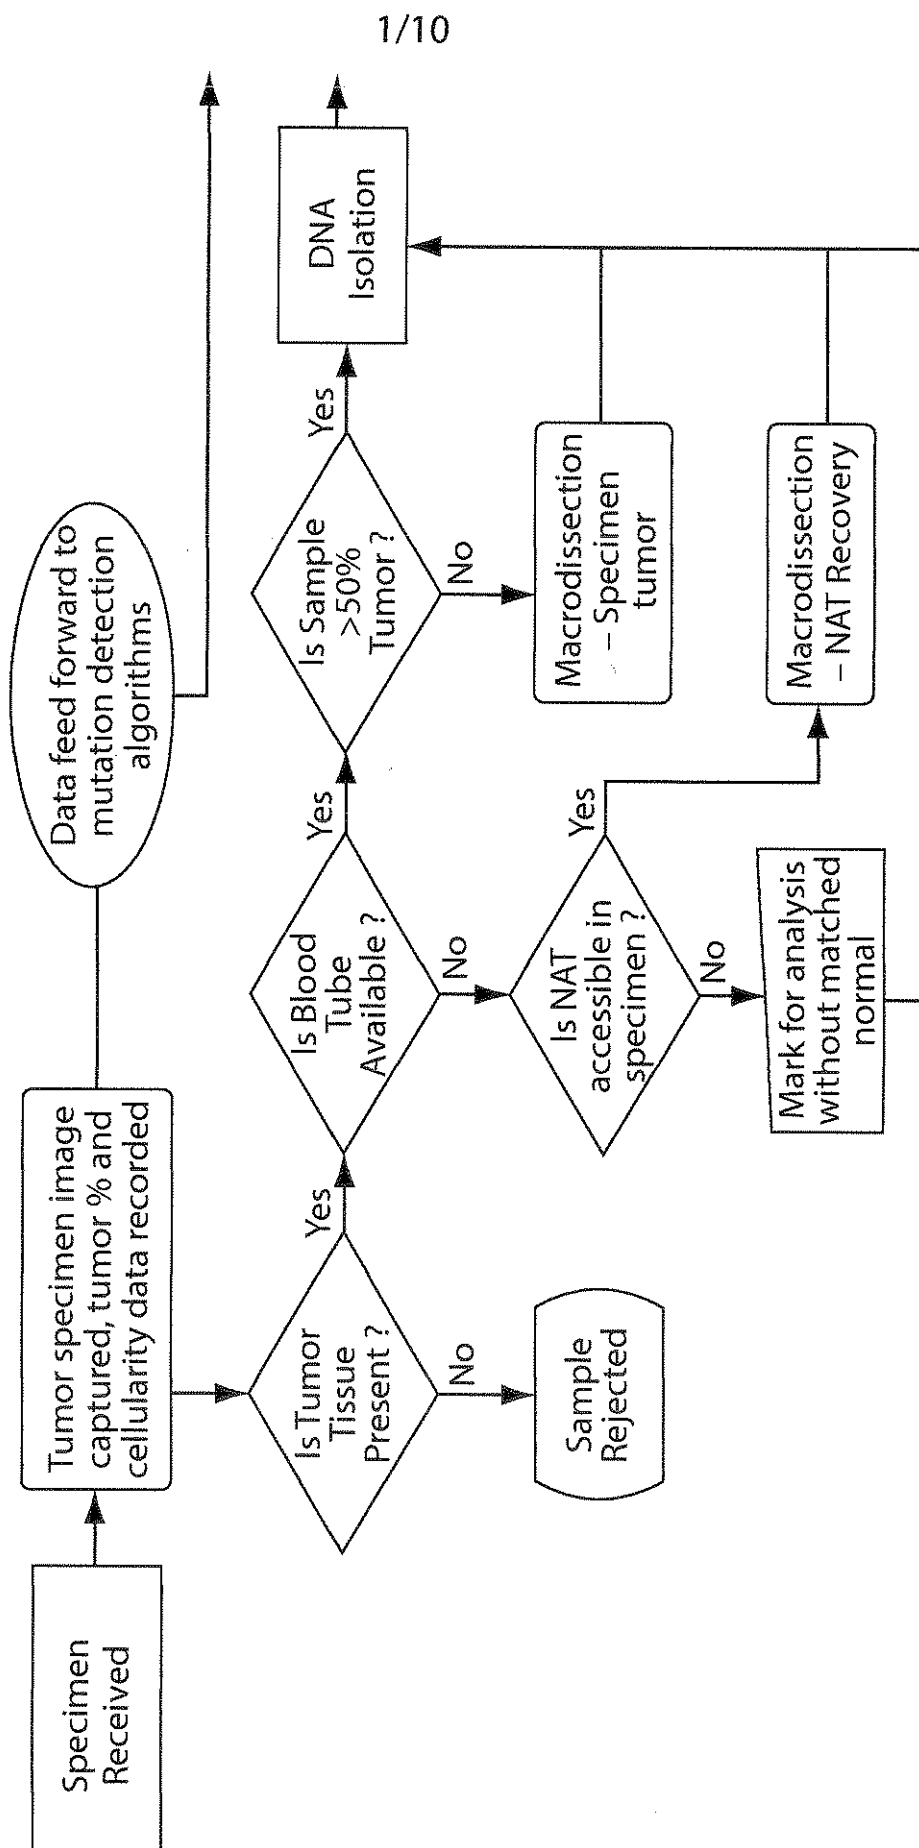


Fig. 1A

2/10

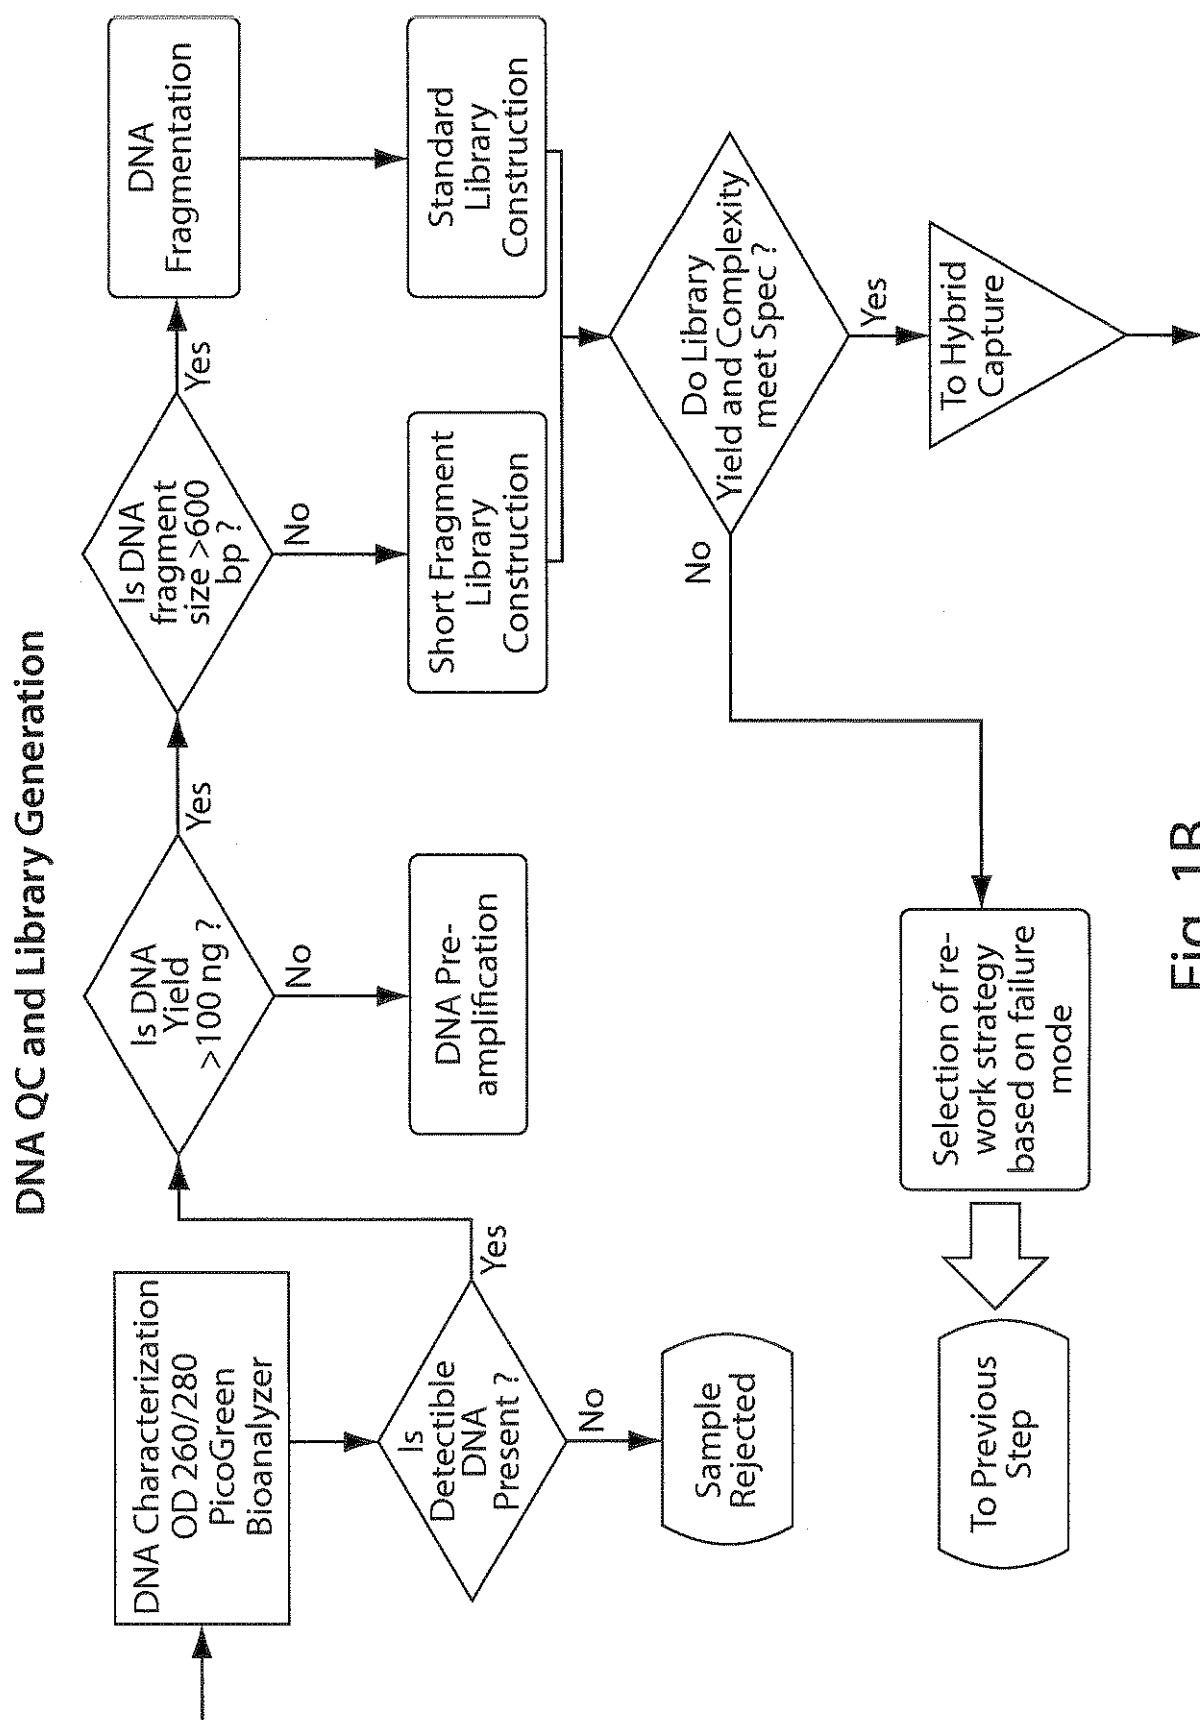


Fig. 1B

3/10

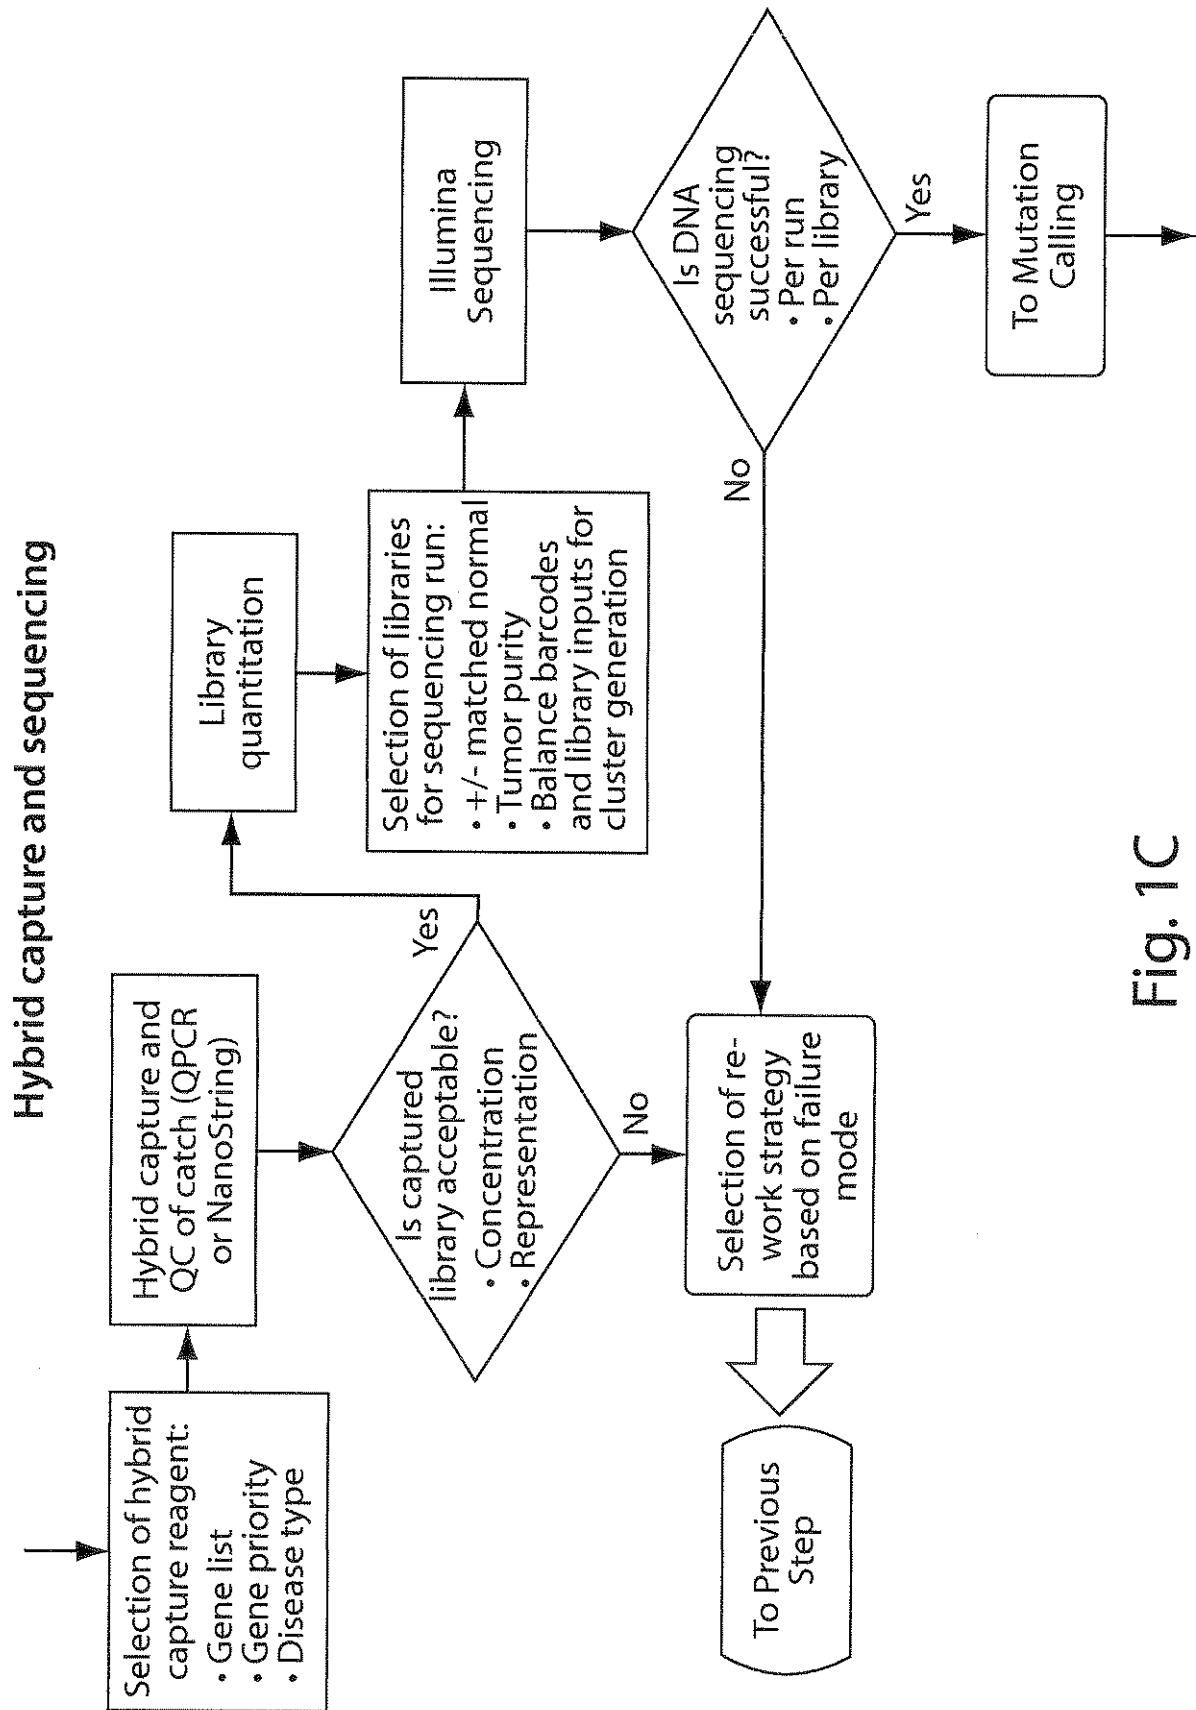


Fig. 1C

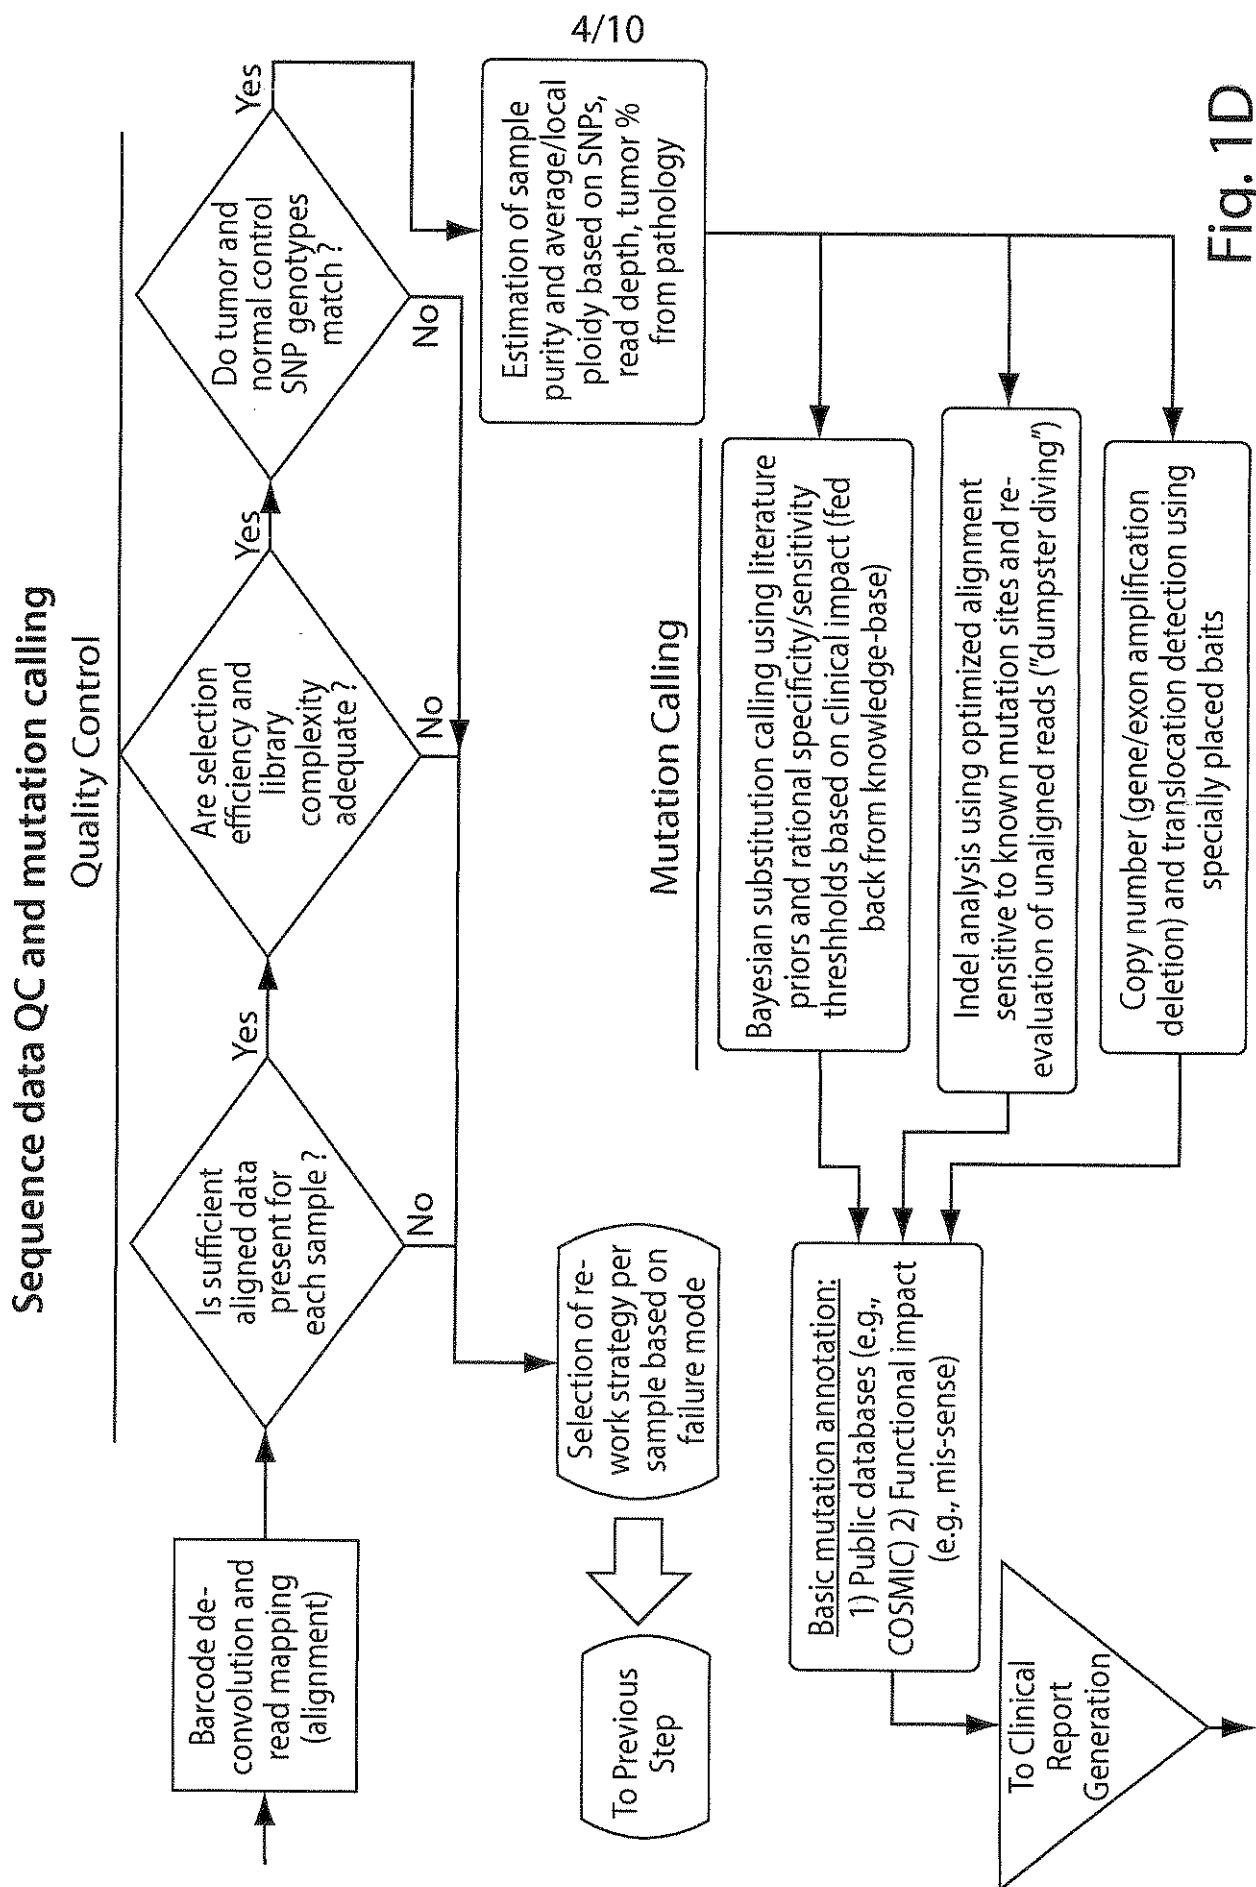


Fig. 1D

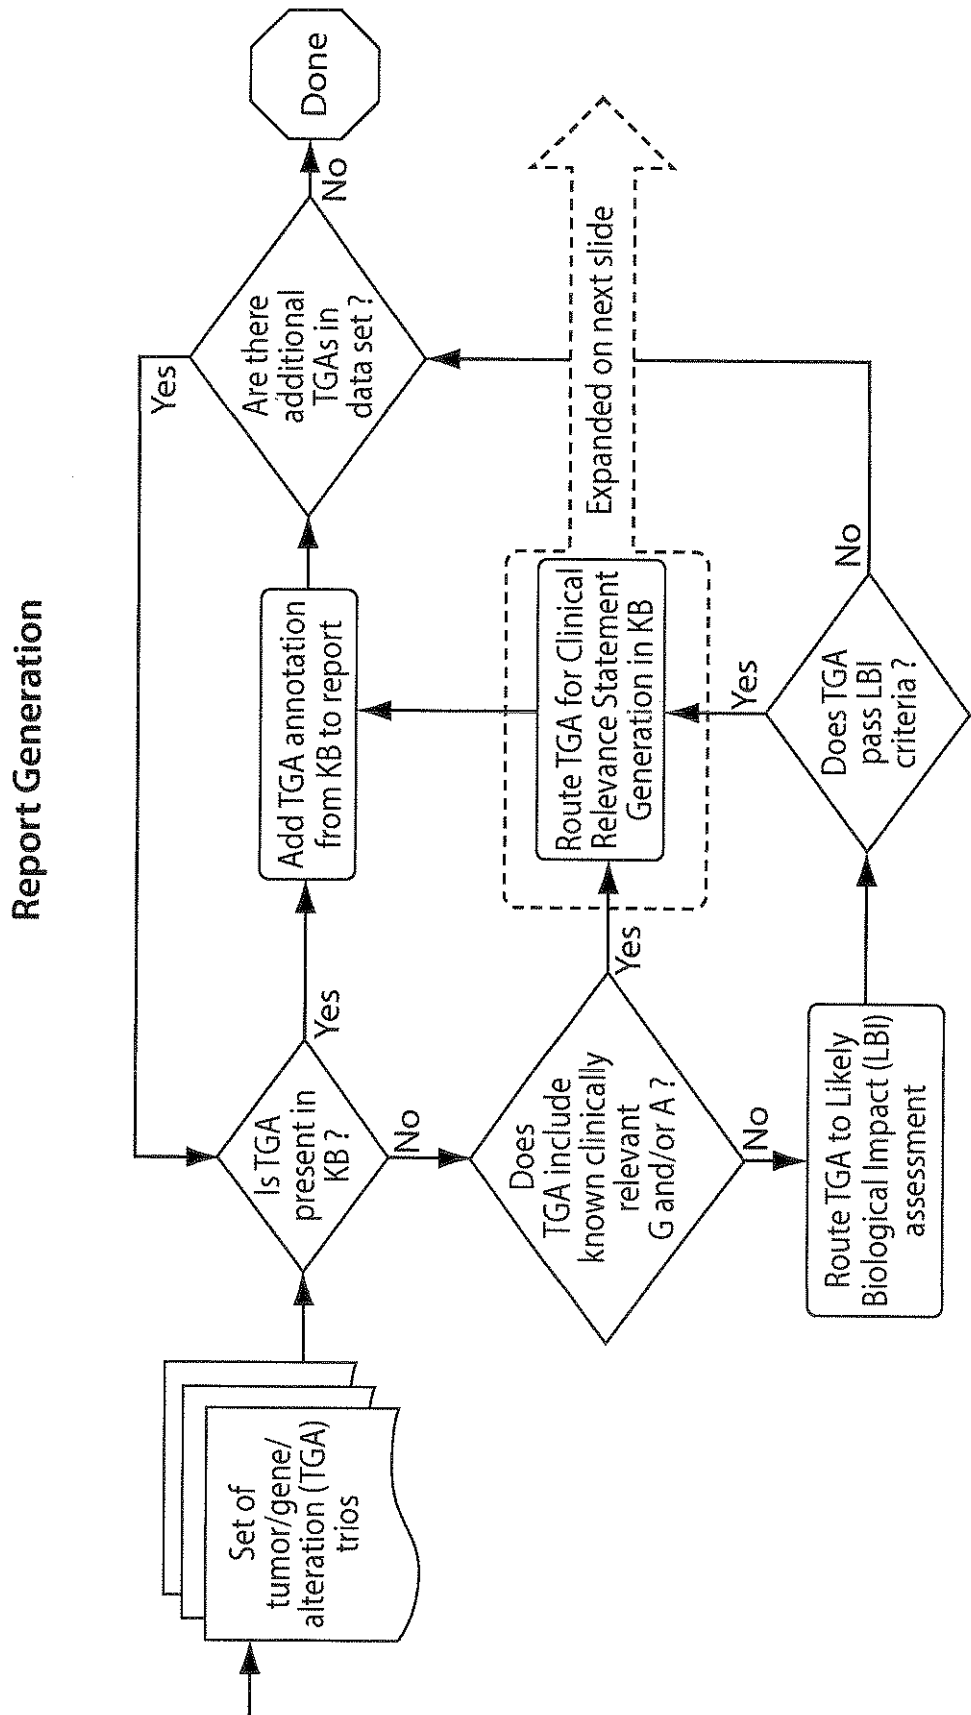


Fig. 1E

6/10

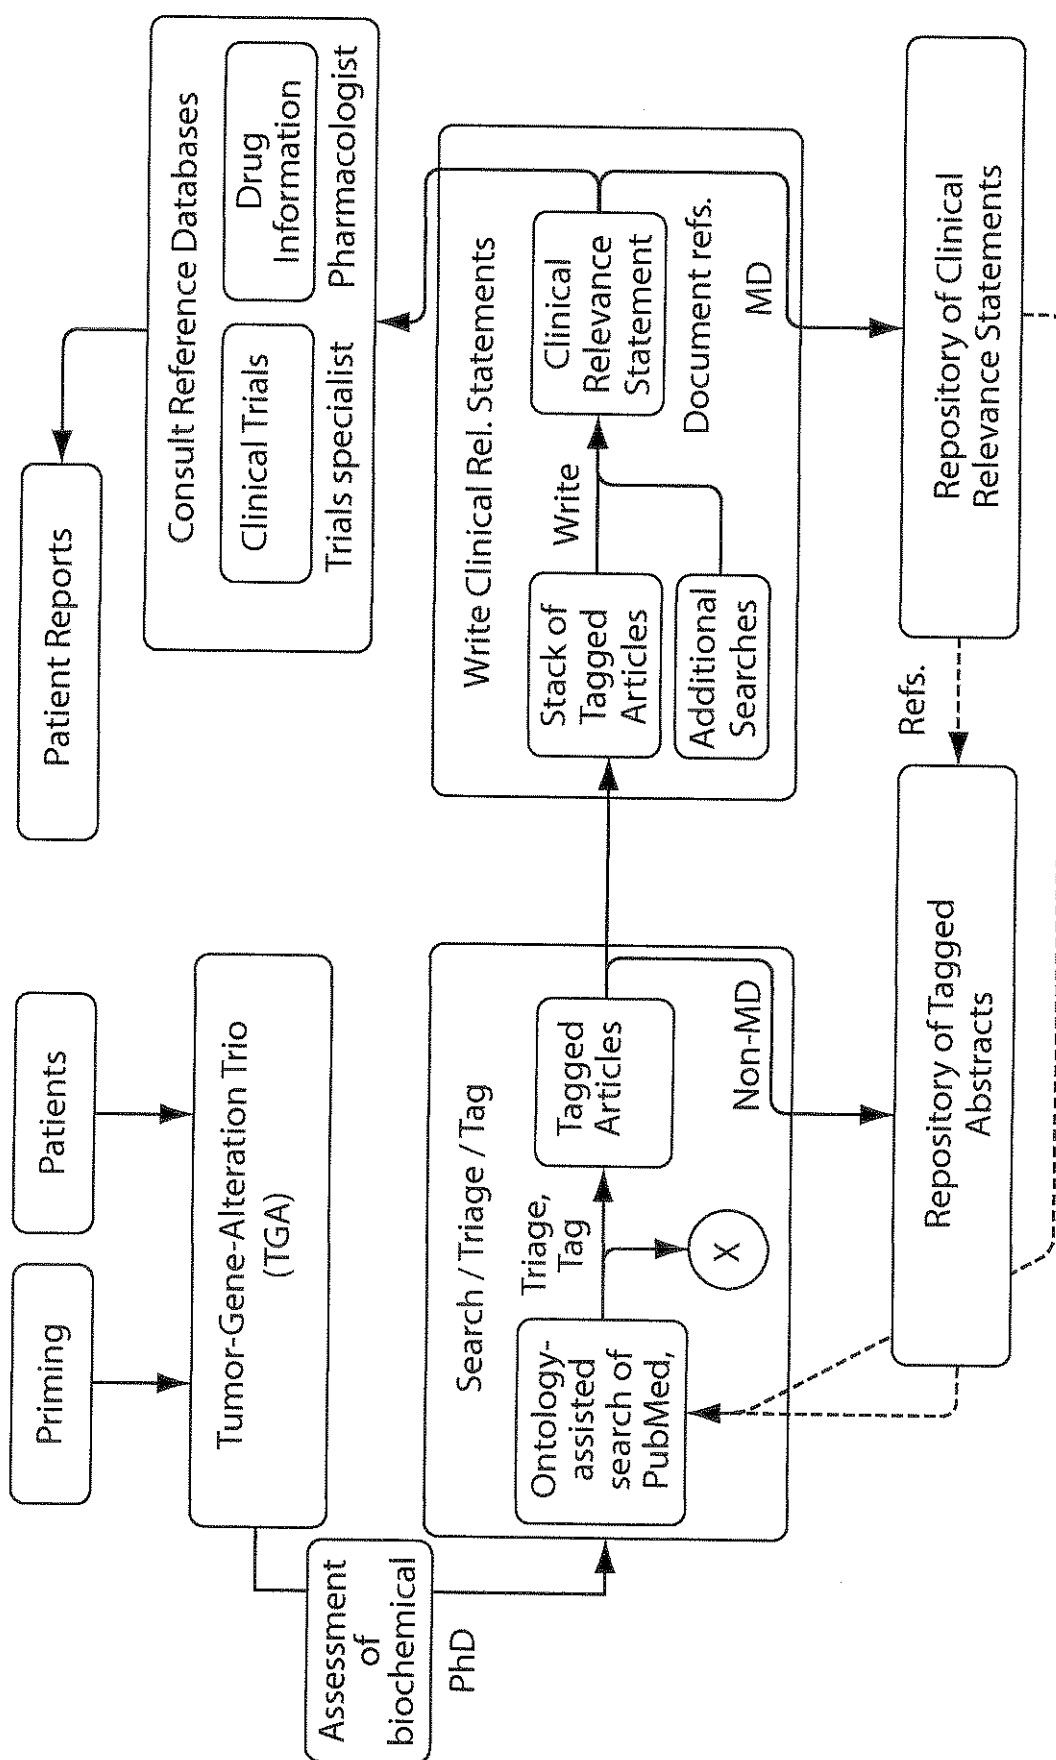


Fig. 1F

Impact of prior expectation and read depth on mutation detection

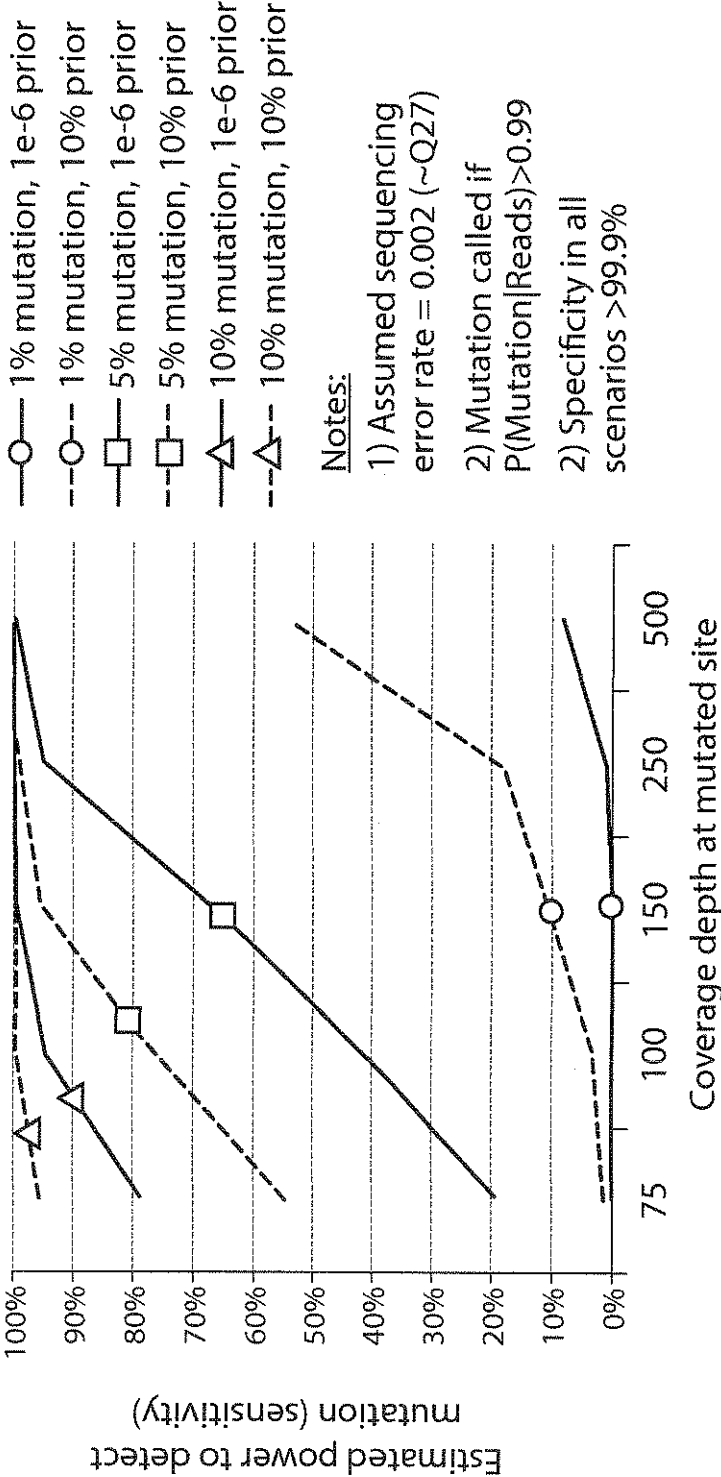
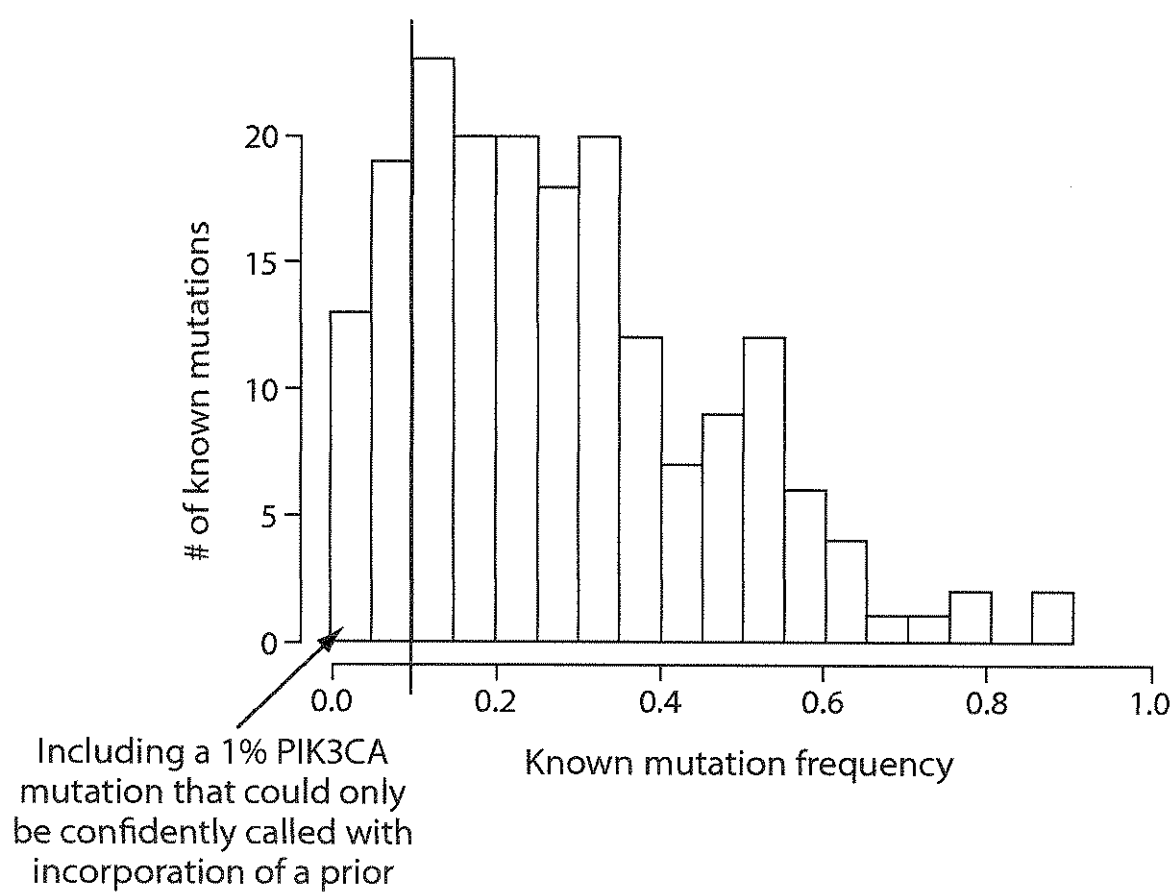


Fig. 2

8/10

Mutation frequencies in > 100 clinical cancer samples**Fig. 3**

9/10

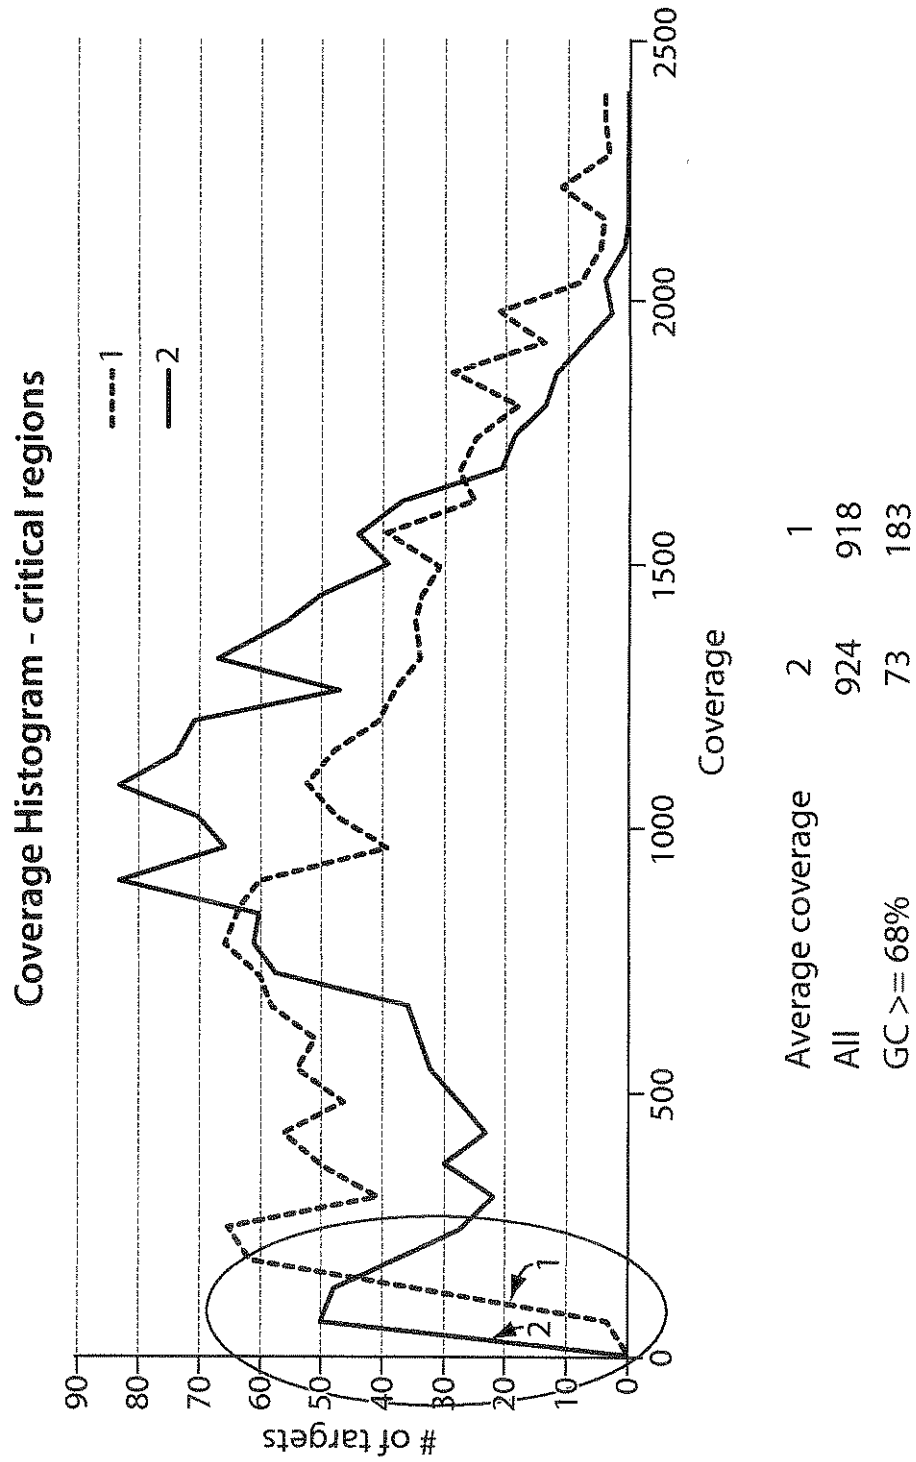


Fig. 4

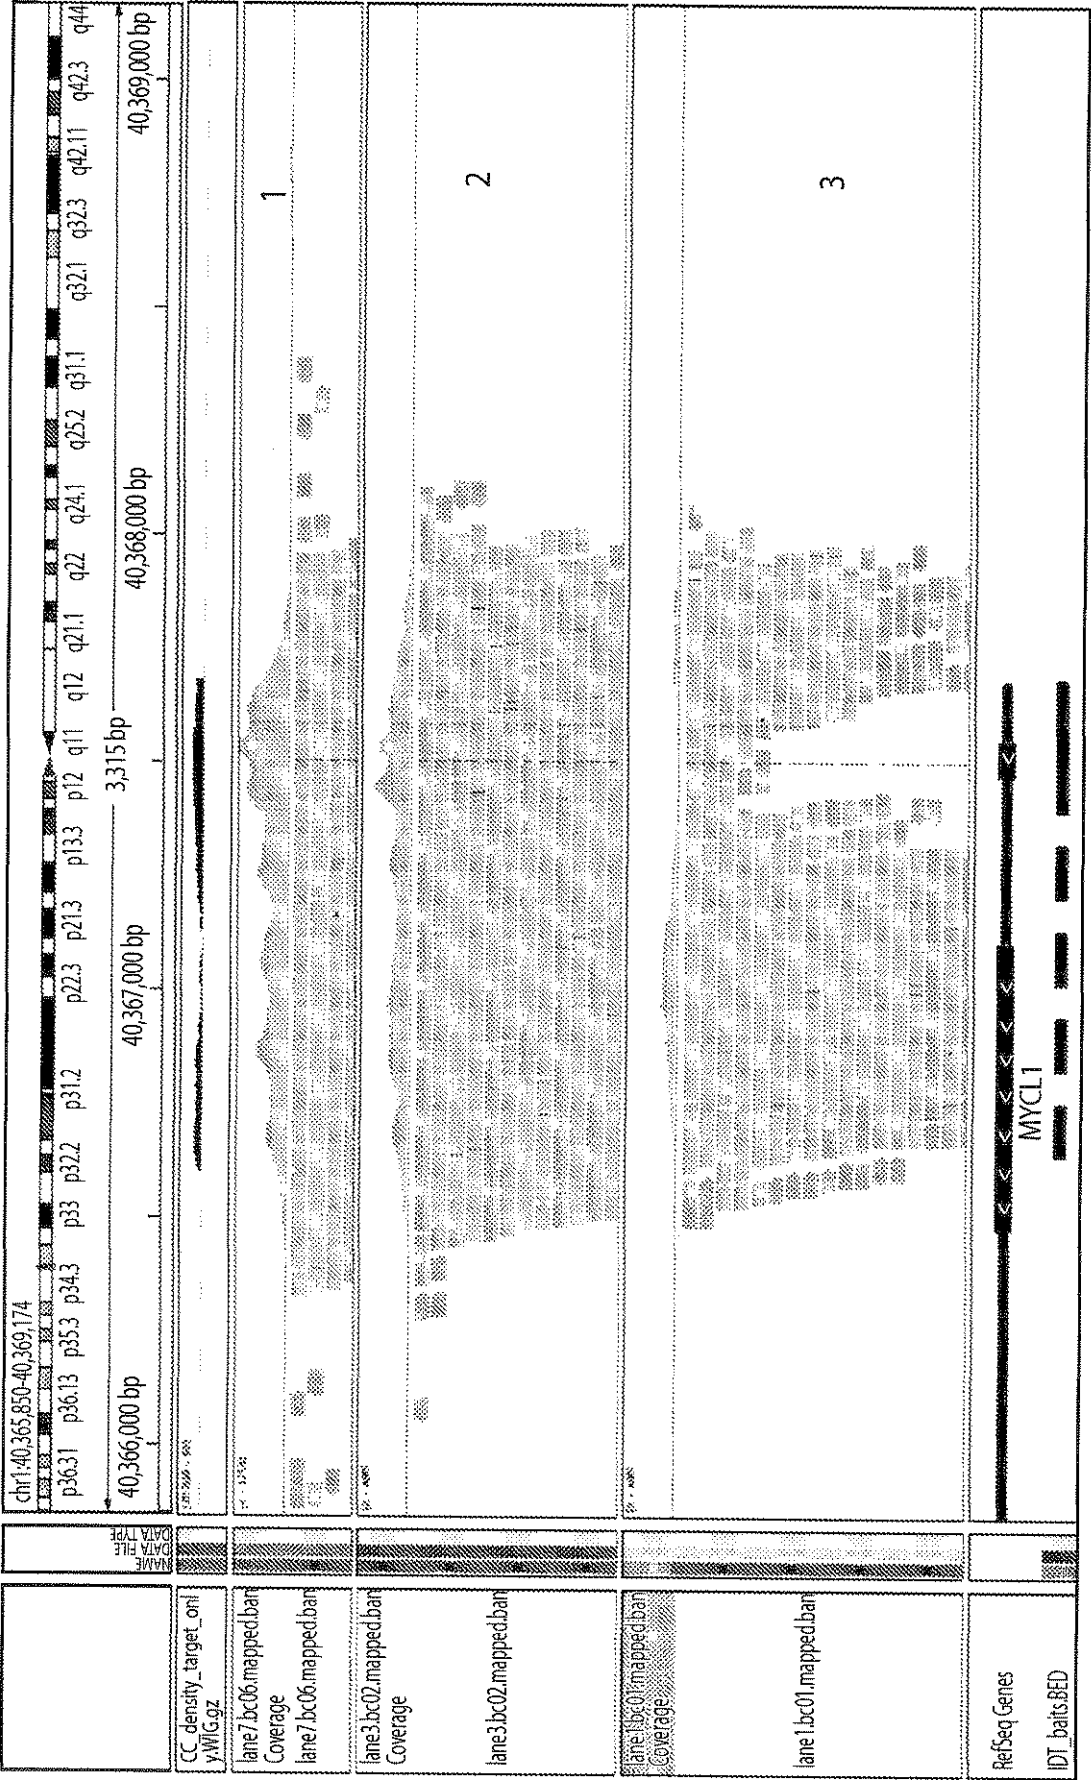


Fig. 5