

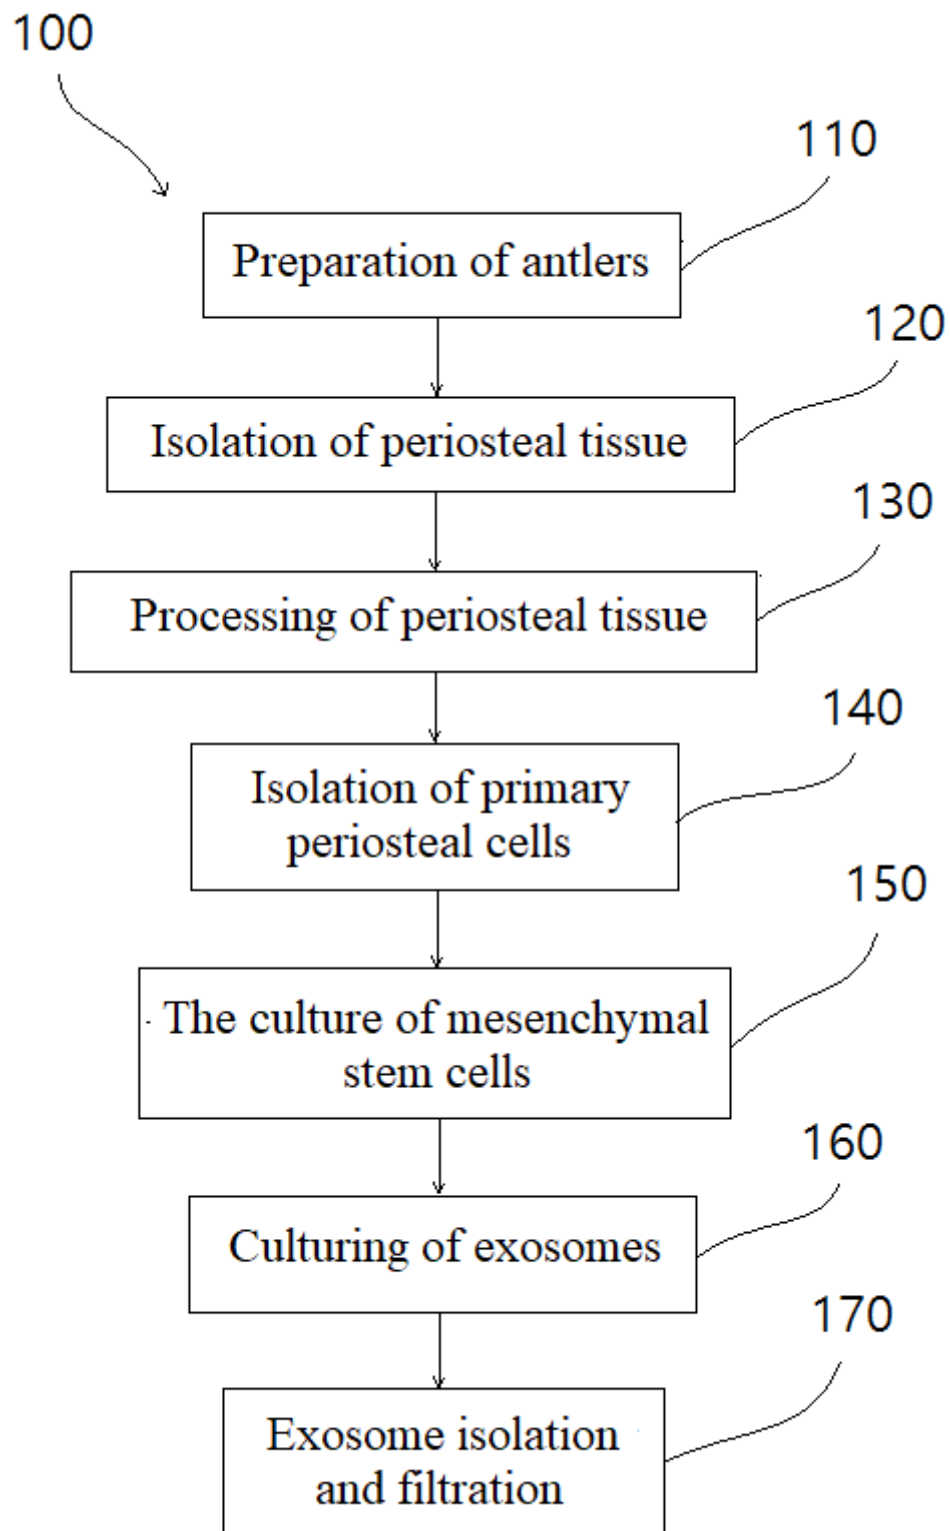


FIG. 1

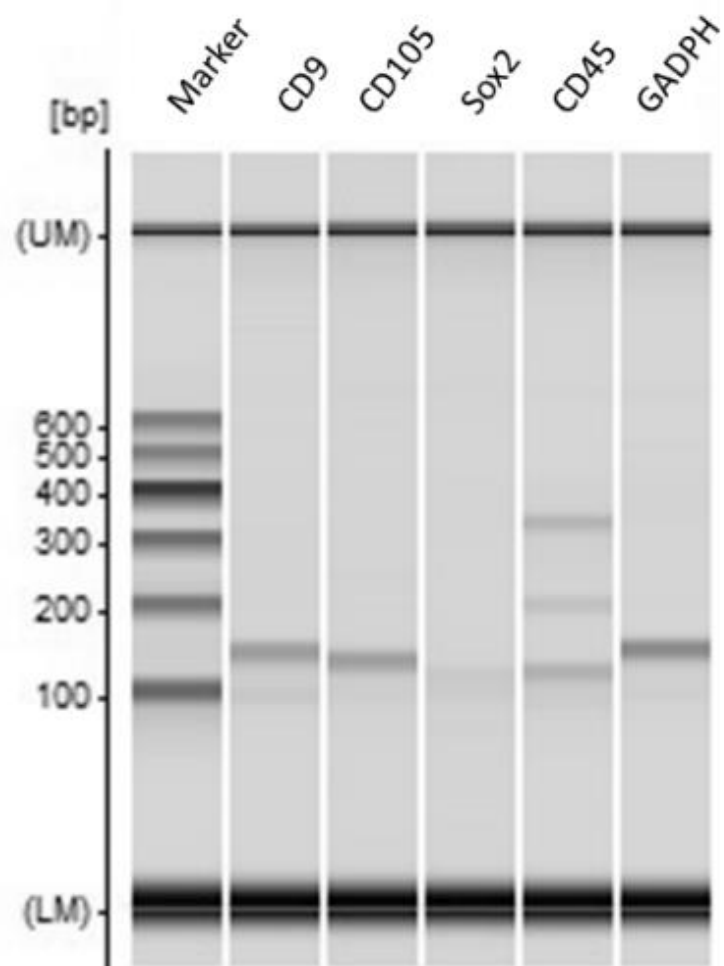


FIG. 2












FIG. 3

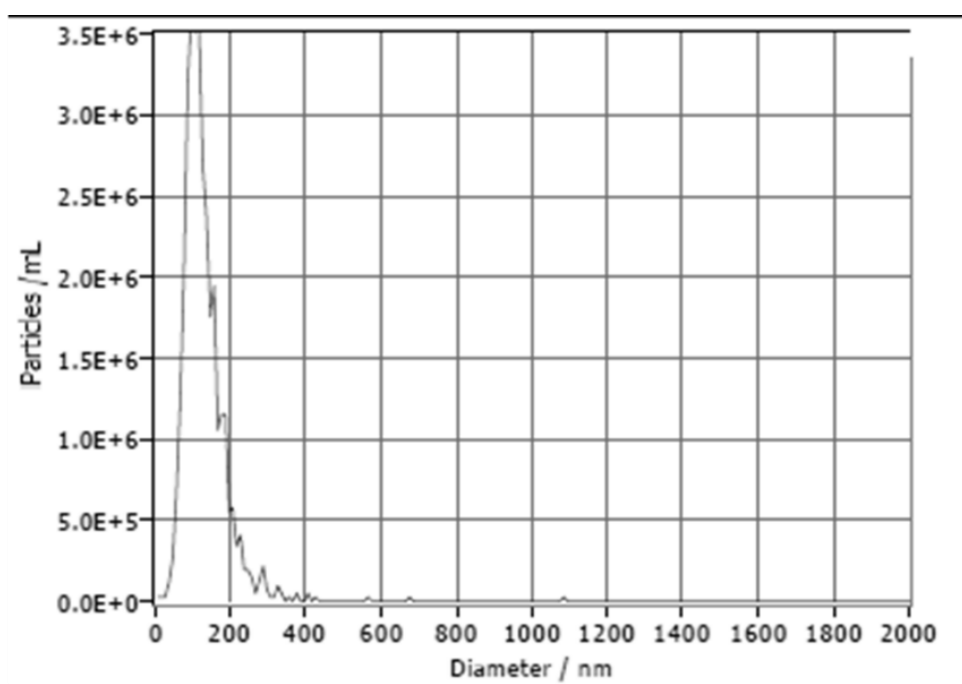

Peak Analysis (Concentration)

Diameter / nm	Particles/mL	FWHM / nm	Percentage
103.7	3.7E+6	76.7	100.0

FIG. 4






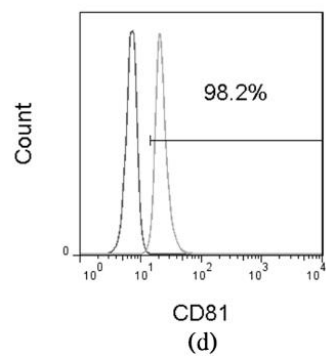


FIG. 5

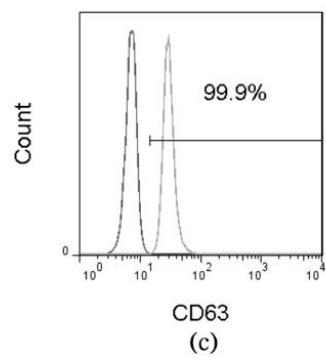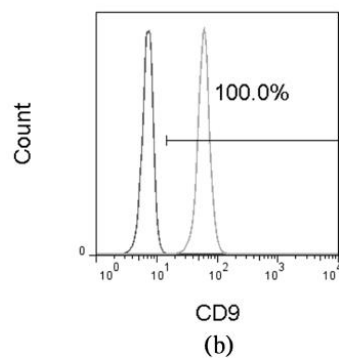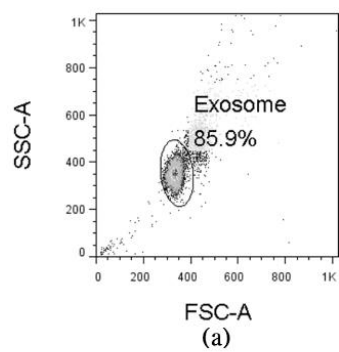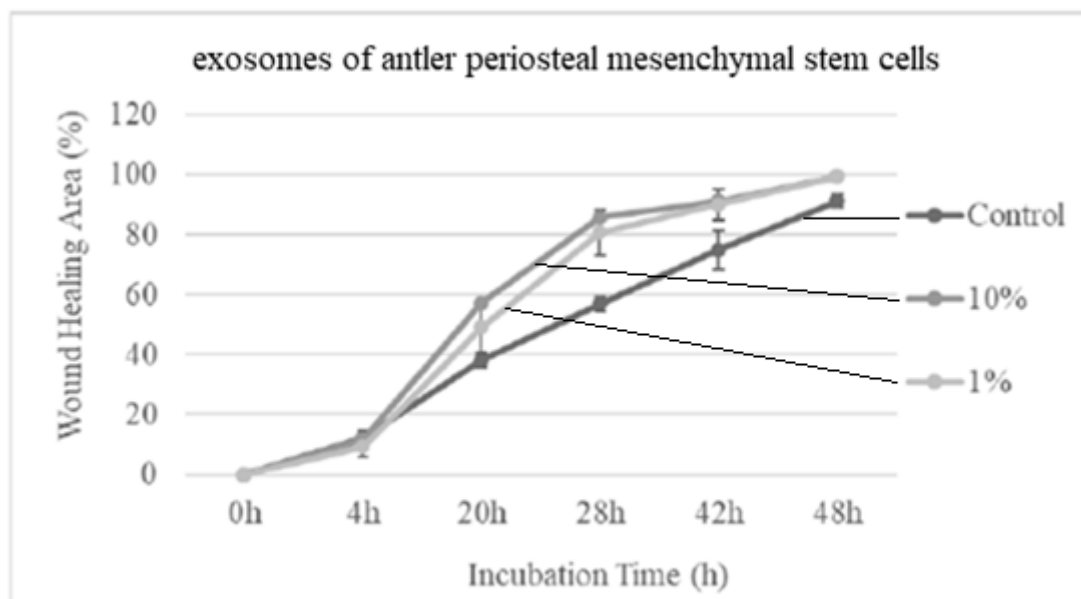

(a)

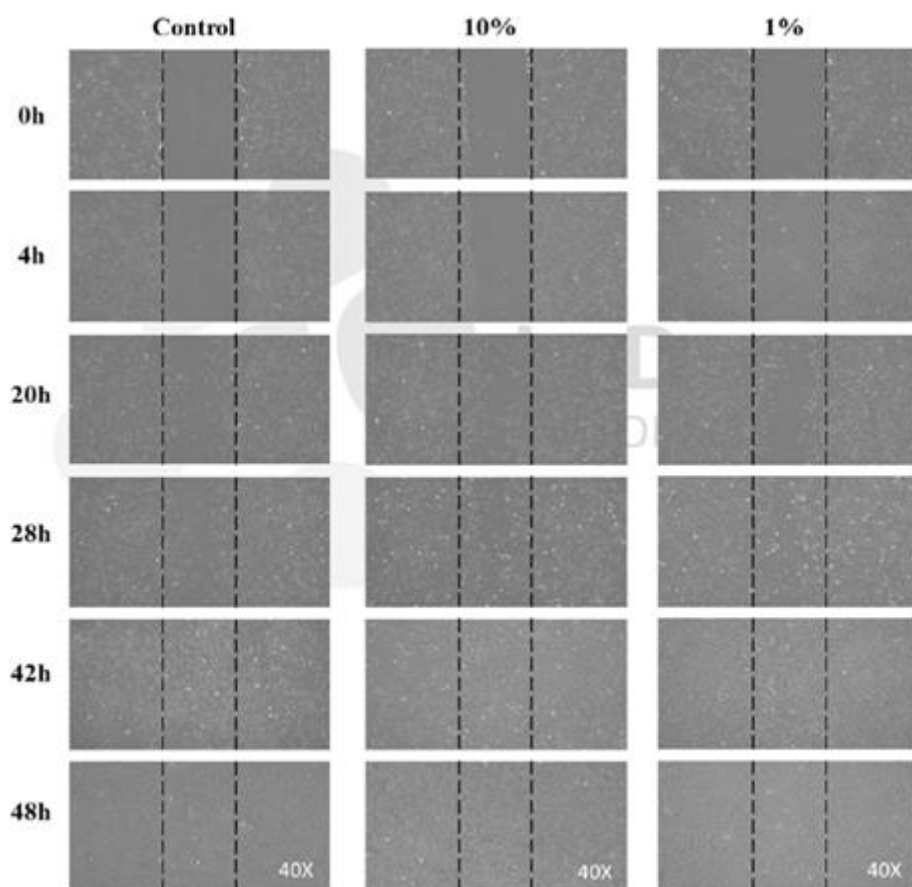

(b)

FIG. 6

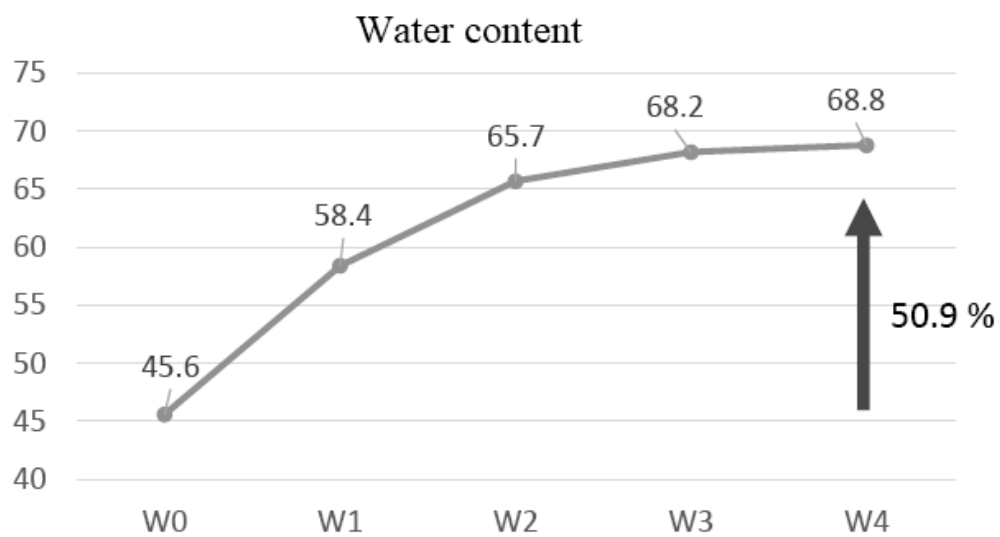


FIG. 7

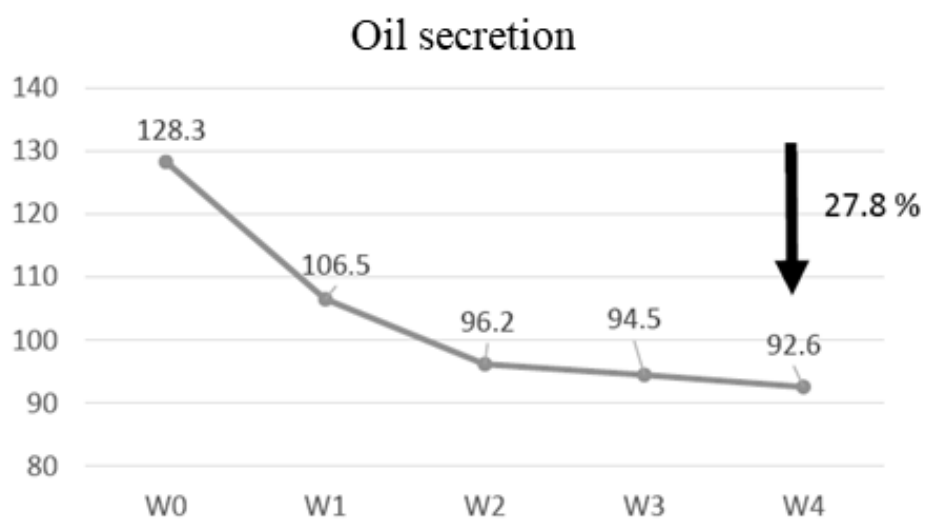


FIG. 8

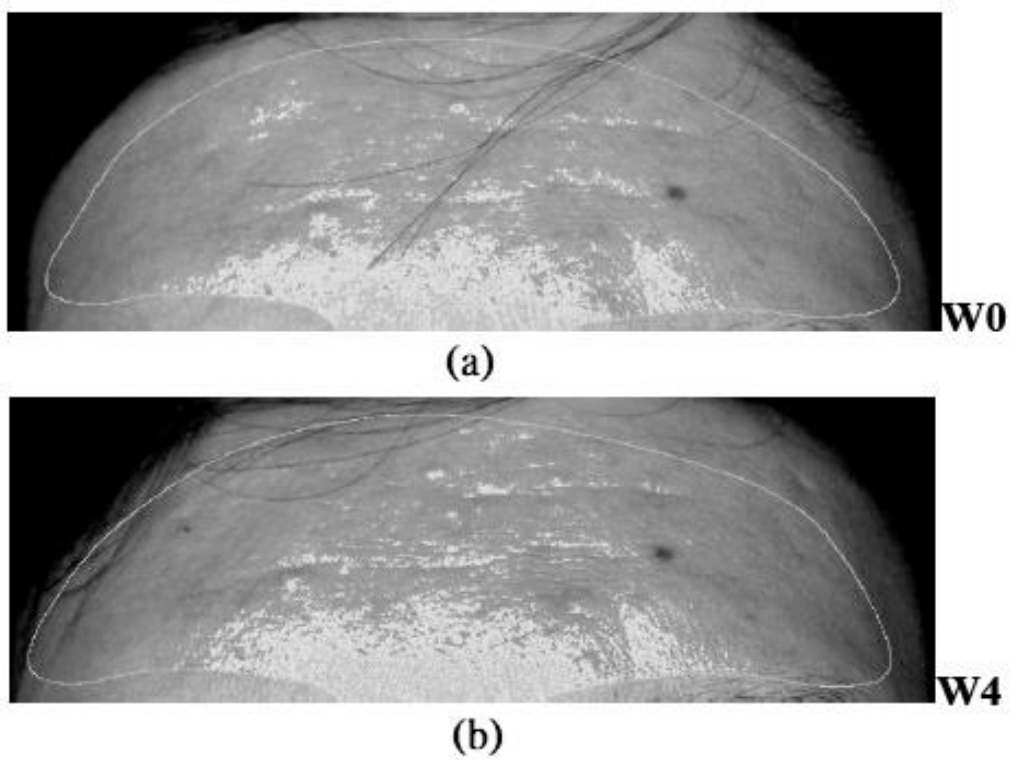


FIG. 9

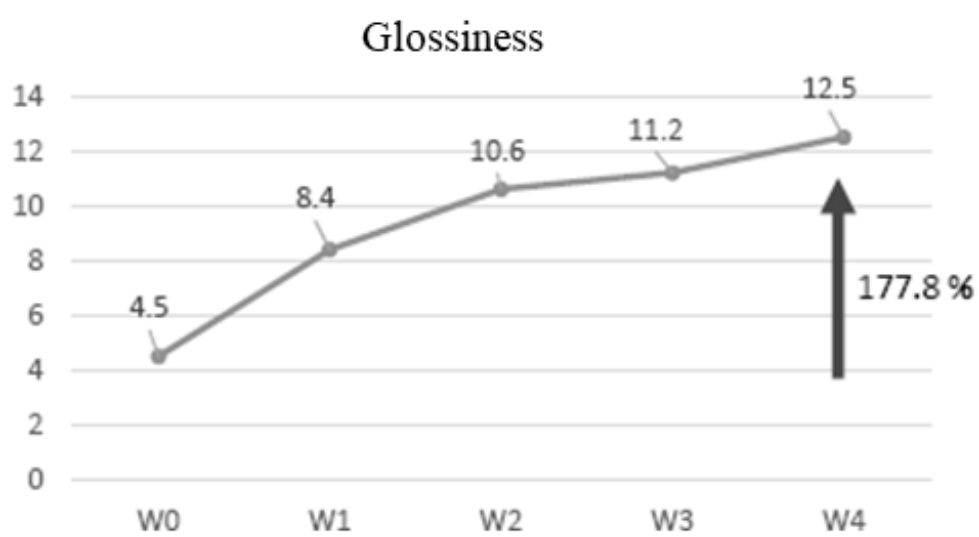


FIG.10

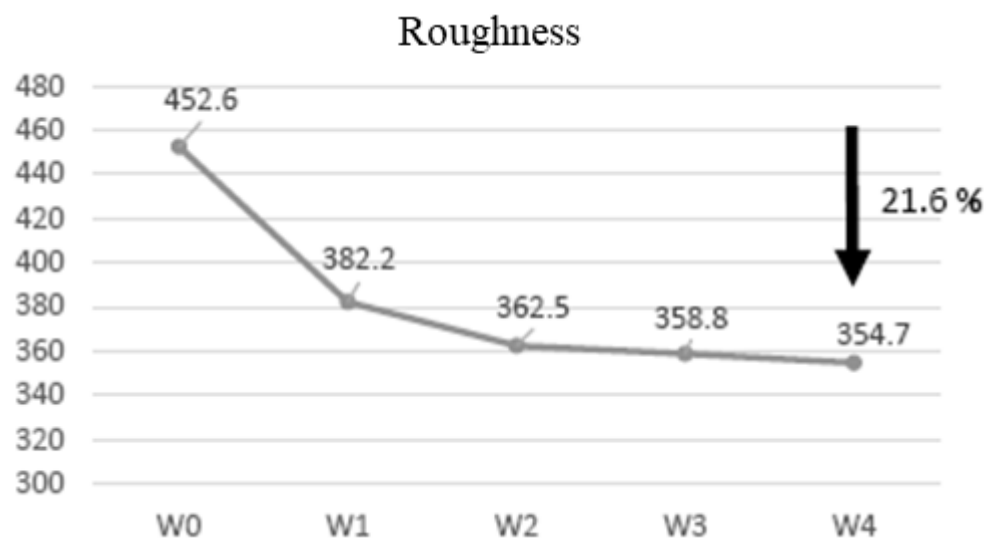


FIG.11



(a)



(b)

FIG.12

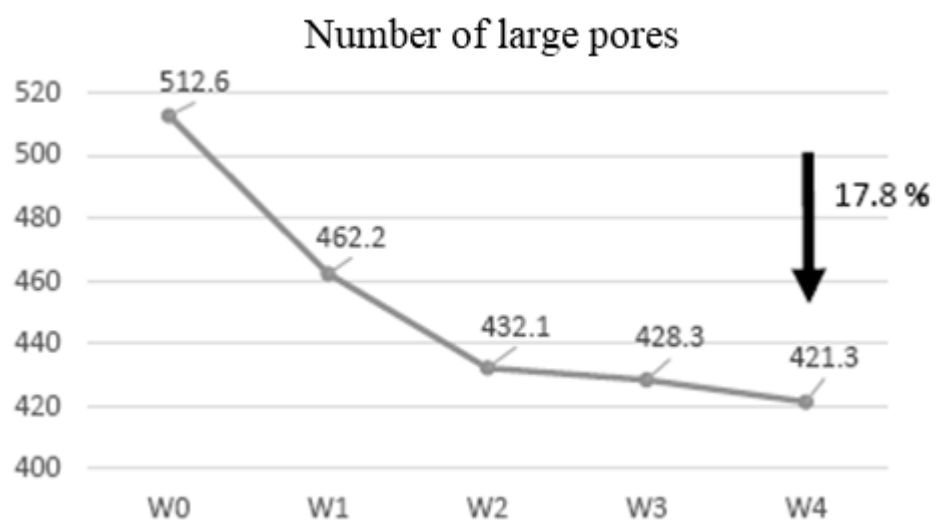


FIG.13

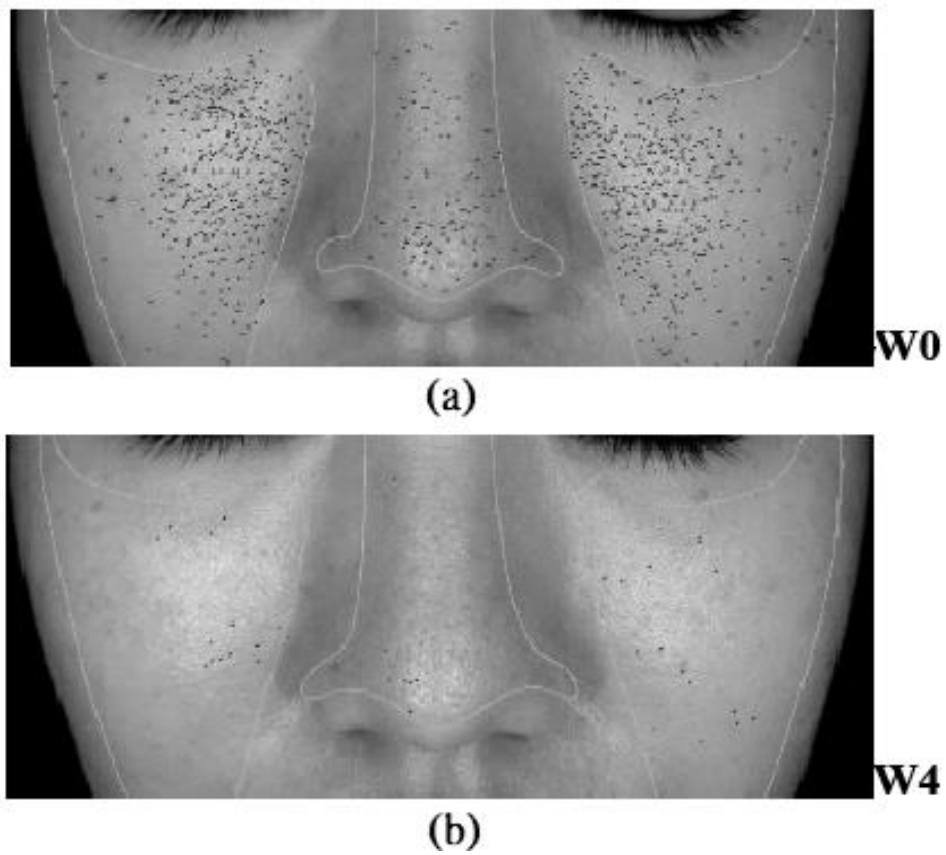


FIG.14

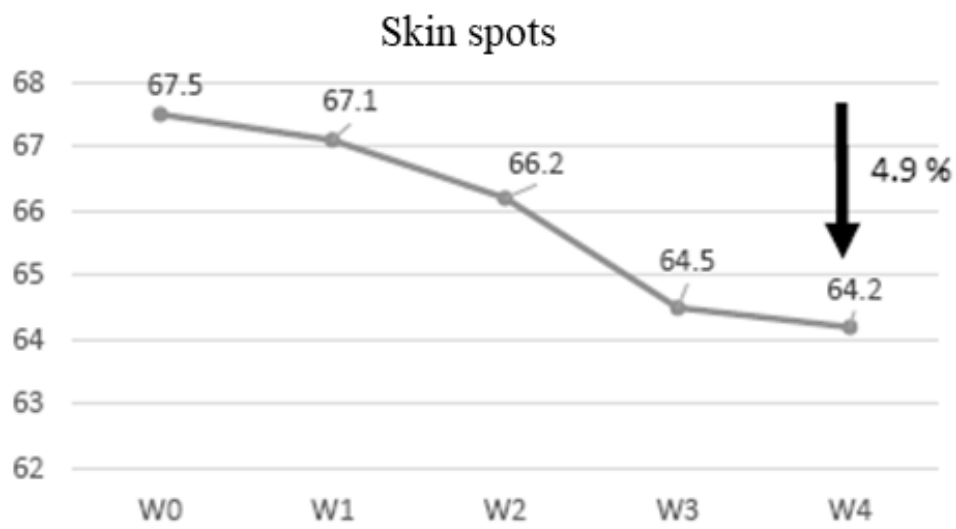


FIG.15

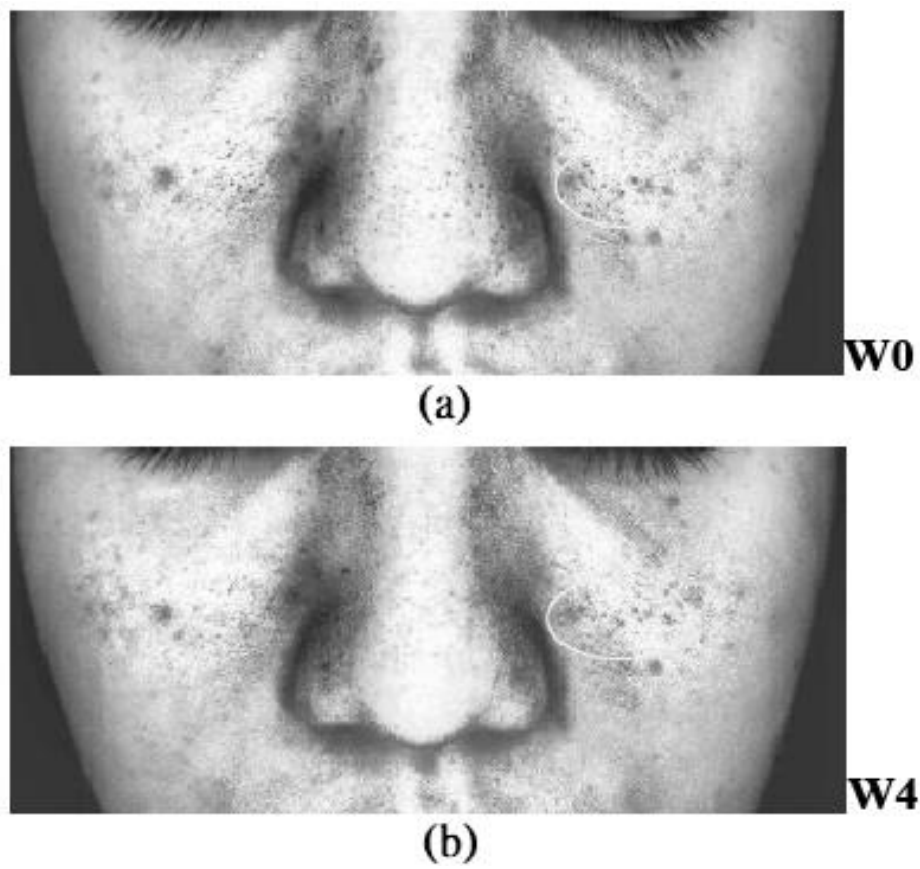


FIG.16

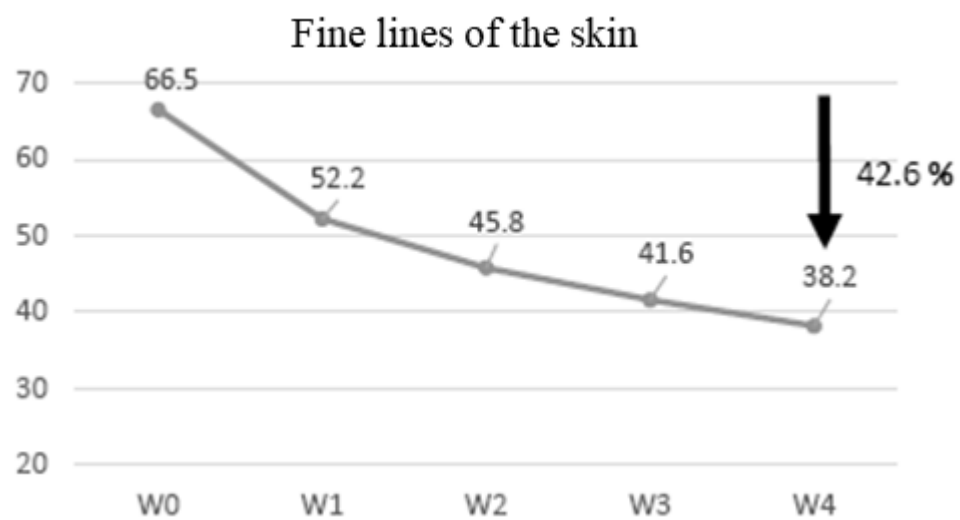


FIG.17

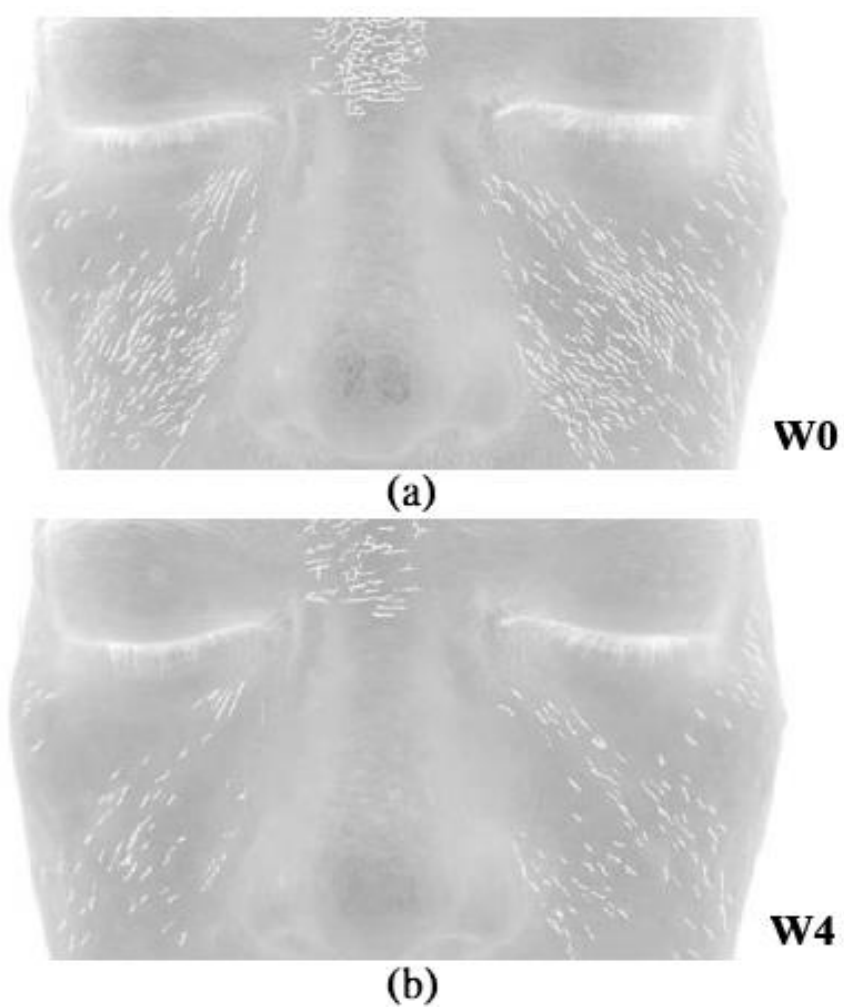


FIG.18

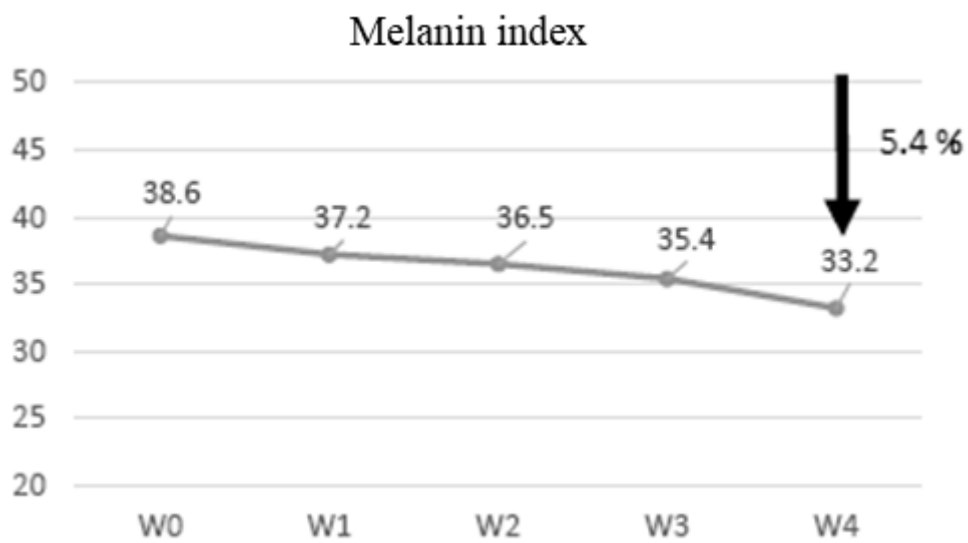


FIG.19

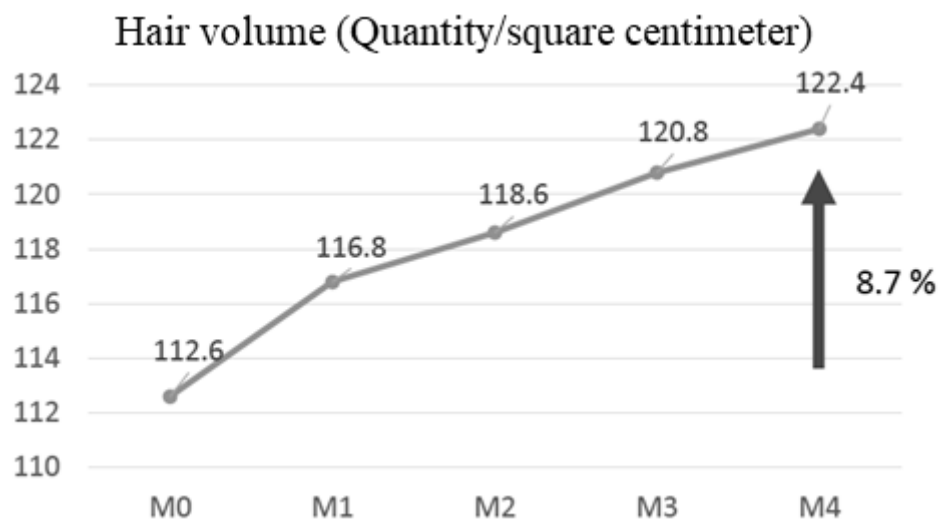


FIG.20

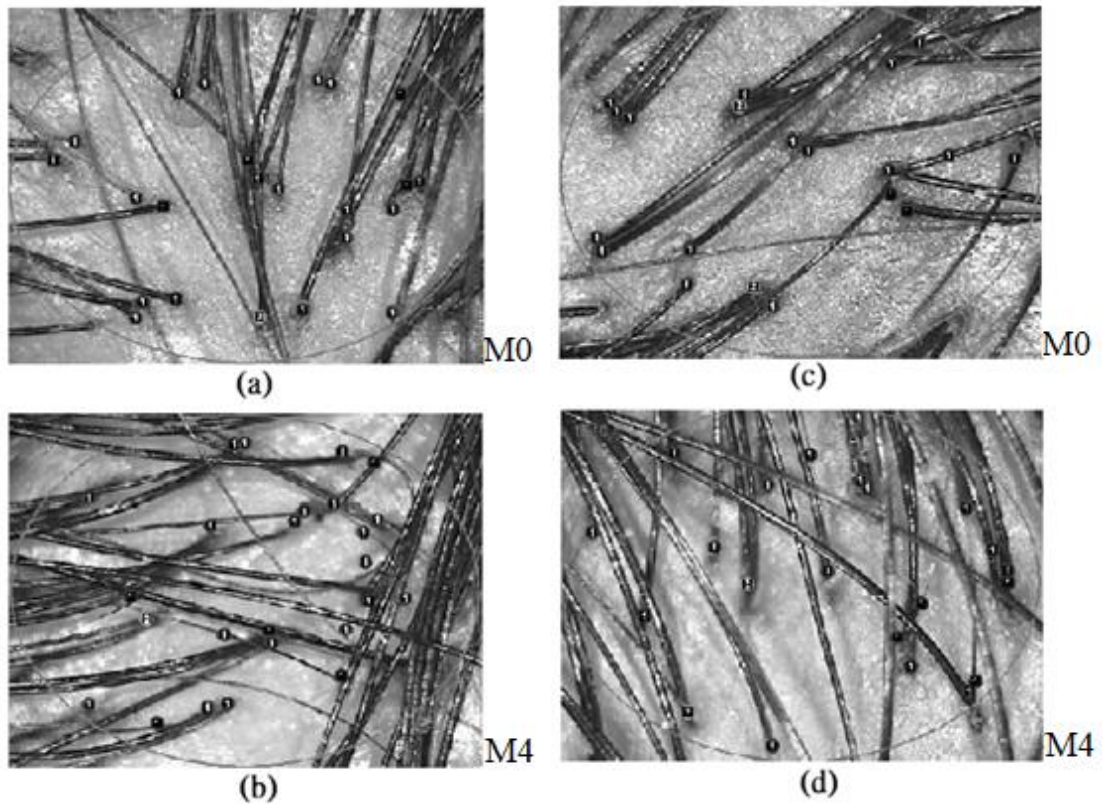


FIG.21

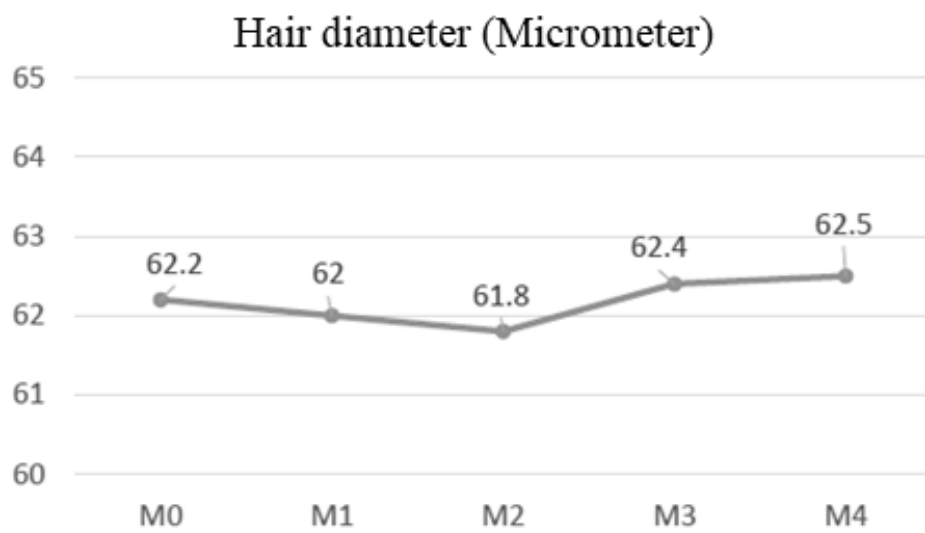


FIG.22

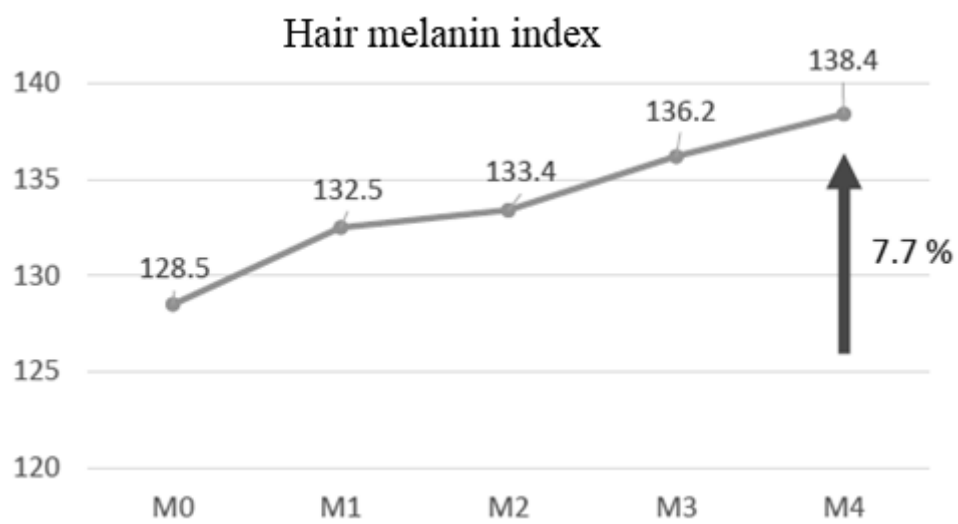


FIG.23

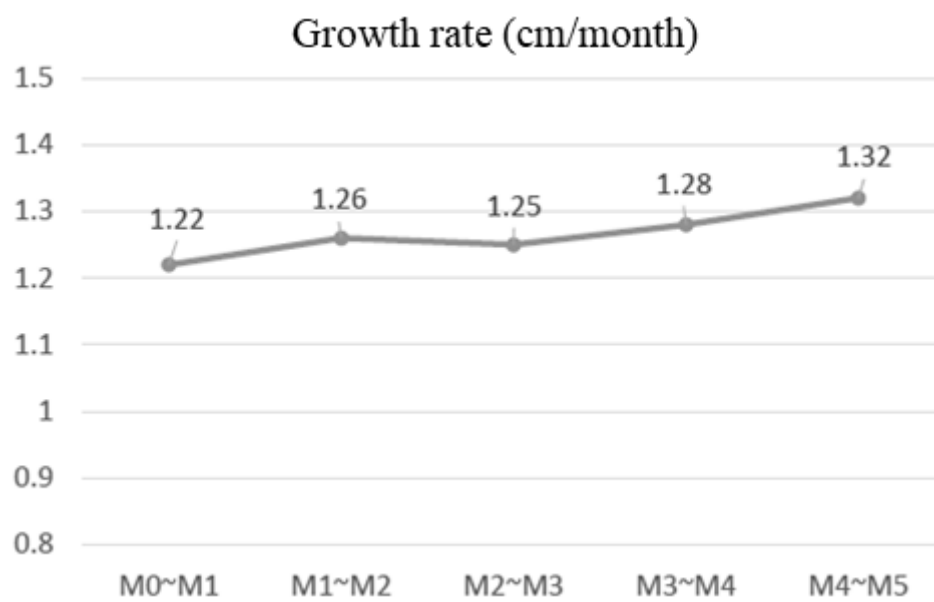


FIG.24