9801694-2
IPOS Copy

RECEIVED 02 Apr 98 Patent Office TRADE MARKS REGISTRY OF

PCT

WORLD INTELLECTUAL PROPERTY ORGANIZATION
International Bureau

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification 6 :
A61M 1/28

(11) International Publication Number: **WO 97/45149**

(43) International Publication Date: 4 December 1997 (04.12.97)

(21) International Application Number: PCT/US97/08896

(22) International Filing Date: 23 May 1997 (23.05.97)

(30) Priority Data:
08/657,832 31 May 1996 (31.05.96) US

(71) Applicant: BAXTER INTERNATIONAL INC. [US/US]; One Baxter Parkway, Deerfield, IL 60015 (US).


(72) Inventors: PELUSO, Francesco; Verbindubgslaan 70, B-3001 Heverlee (US). BALTEAU, Patrick, R.; Rue Louis Burteau 69, B-5032 Bothey (BE). HENAUT, Eric, J.; Rue de la Samme 11, B-7181 Arquennes (BE).

(74) Agents: BORECKI, Thomas, S. et al.; Baxter International Inc., One Baxter Parkway, DF3-3E, Deerfield, IL 60015 (US).

(81) Designated States: AU, BR, CA, CN, JP, KR, MX, SG, European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).

Published
With international search report.
Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.

(54) Title: SOLUTION DELIVERY SYSTEM WITH INDIVIDUAL INTEGRATED FINAL PACKAGING AND A METHOD FOR PACKAGING THE SAME

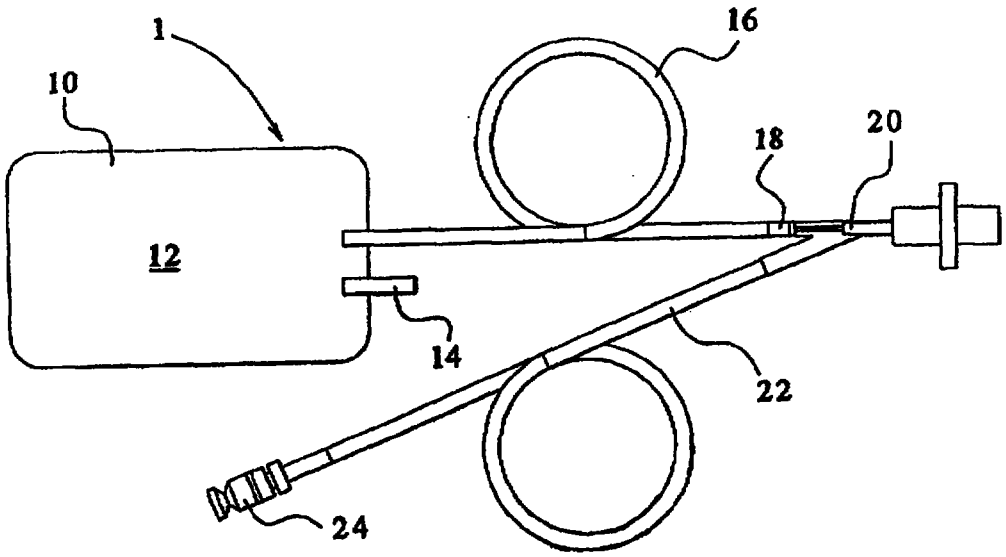

(57) Abstract

A system and a method are provided for packaging components required for conducting a dialysis procedure. To this end, a rigid container is designed such that other necessary components required for conducting a dialysis procedure may be contained therein prior to use. The rigid container is designed with a lid having a port in the lid such that a drainage line may be connected to the port and the rigid container may be used as a drainage container. The rigid container is constructed from a rigid material such that rigid containers may be stacked during transport and storage of the same. The rigid container may also be re-used for subsequent dialysis procedures.