(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property Organization
International Bureau

(43) International Publication Date
15 September 2005 (15.09.2005)

PCT

(10) International Publication Number
WO 2005/084530 A3

(51) International Patent Classification[7]: A61B 5/15

(21) International Application Number:
PCT/EP2005/002273

(22) International Filing Date: 4 March 2005 (04.03.2005)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
04005385.2 6 March 2004 (06.03.2004) EP

(71) Applicant *(for all designated States except DE, US)*: **F. HOFFMANN-LA ROCHE AG** [CH/CH]; Grenzacherstrasse 124, CH-4070 Basel (CH).

(71) Applicant *(for DE only)*: **ROCHE DIAGNOSTICS GMBH** [DE/DE]; Sandhofer Strasse 116, 68305 Mannheim (DE).

(72) Inventors; and


(75) Inventors/Applicants *(for US only)*: **CALASSO, Irio** [CH/CH]; Kronenhofweg 1, CH-6415 Arth (CH). **GRISS, Patrick** [CH/CH]; Elsastrasse 20, CH-8004 Zürich (CH). **JÄGGI, Rainer** [CH/CH]; Ringstrasse 5, CH-5610 Wohlen (CH). **SAROFIM, Emad** [CH/CH]; Loretostrasse 9, CH-6300 Zug (CH).


(74) Agents: **PFIZ, Thomas** et al.; Hauptmannsreute 93, 70193 Stuttgart (DE).

(81) Designated States *(unless otherwise indicated, for every kind of national protection available)*: AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SM, SY, TJ,

[Continued on next page]

(54) Title: BODY FLUID SAMPLING DEVICE

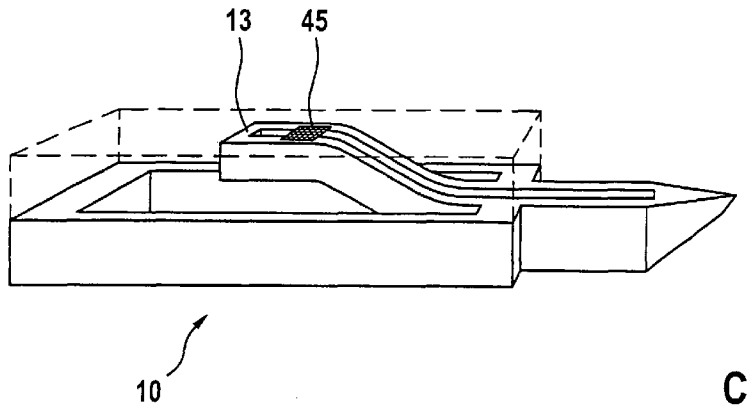

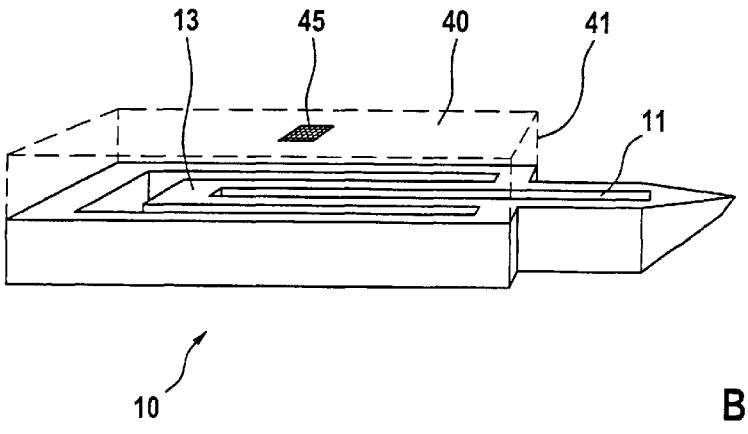

(57) Abstract: Body fluid sampling device comprising a skin-piercing element (10) having a fluid pathway (11) for receiving body fluid, at least a portion of said fluid pathway is open to the environment and further comprising a fluid receiving means (40) being spaced from said fluid pathway so that fluid in said pathway will not contact the fluid receiving means initially. Said fluid receiving means may have a test zone (45) for performing an analytical reaction. Fluid from said channel is contacted with said fluid receiving means either by bringing the fluid receiving means and the fluid into mechanical contact or by electrically transporting fluid from the channel onto the fluid receiving means.

WO 2005/084530 A3

TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(84) Designated States *(unless otherwise indicated, for every kind of regional protection available)*: ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— *with international search report*

— *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments*

(88) Date of publication of the international search report:
10 November 2005

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.