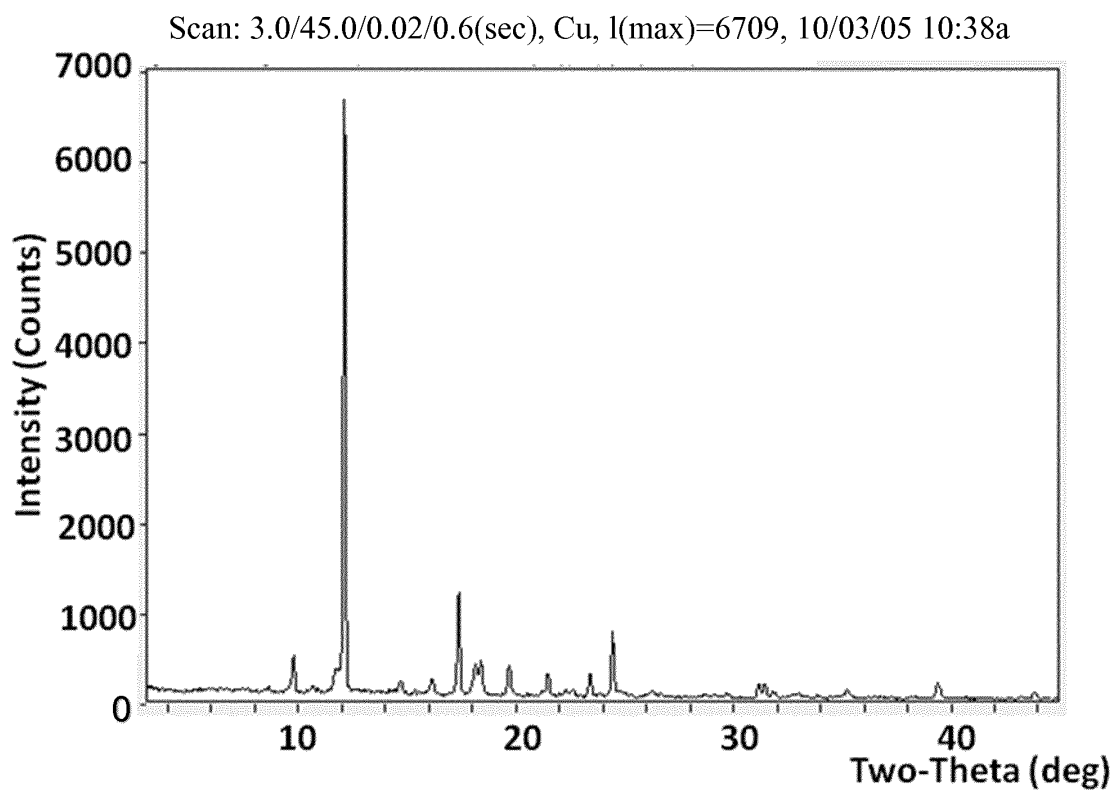
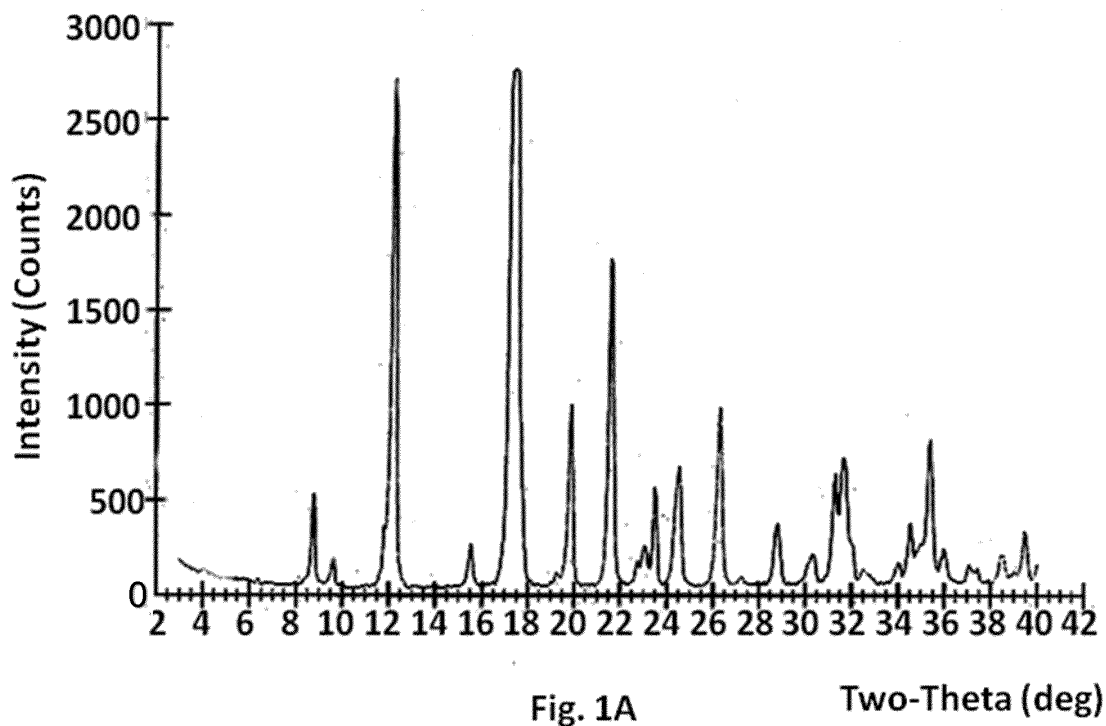


1/17



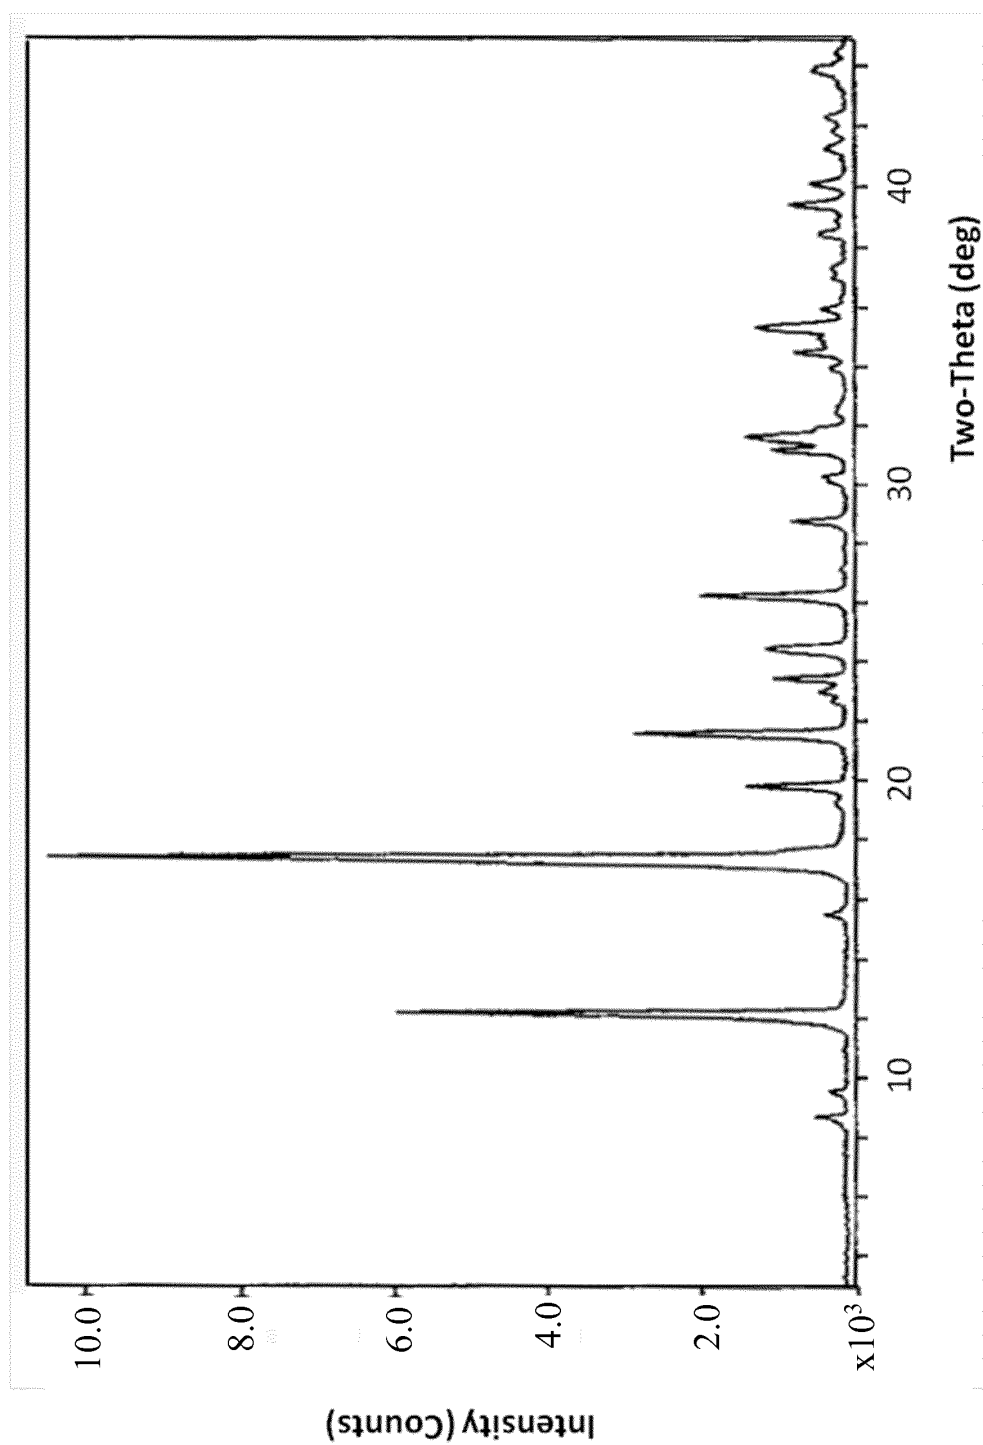


Fig. 2

3/17

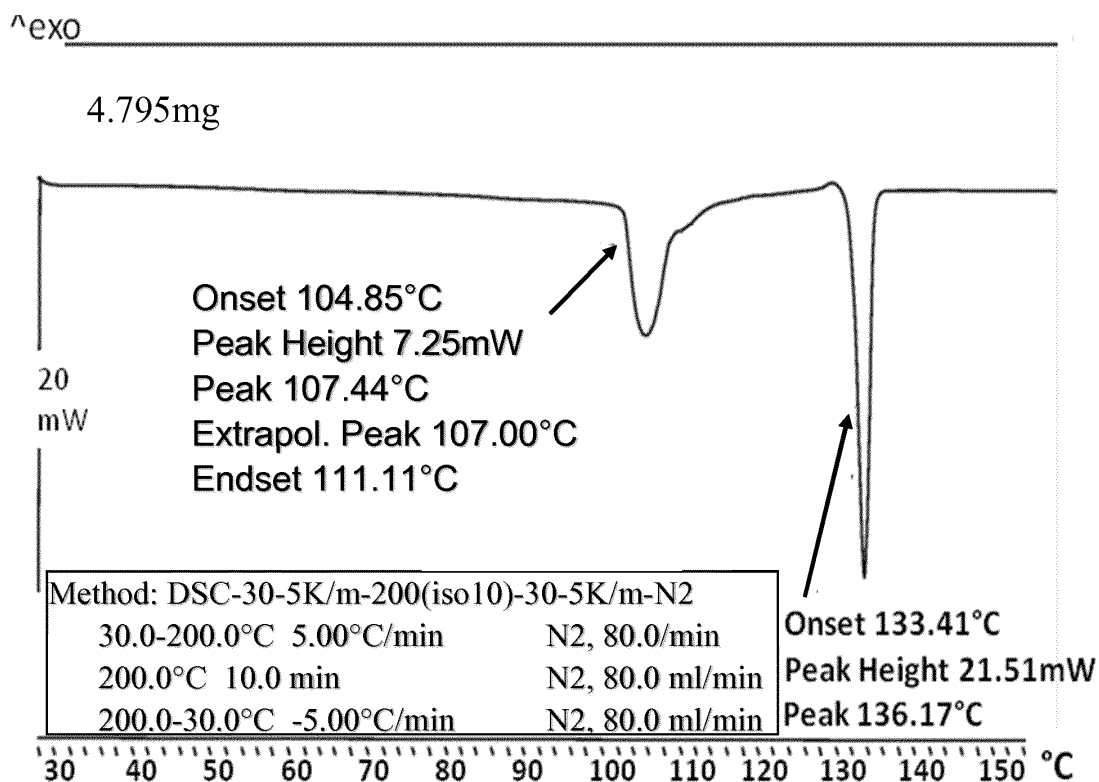


Fig. 3A

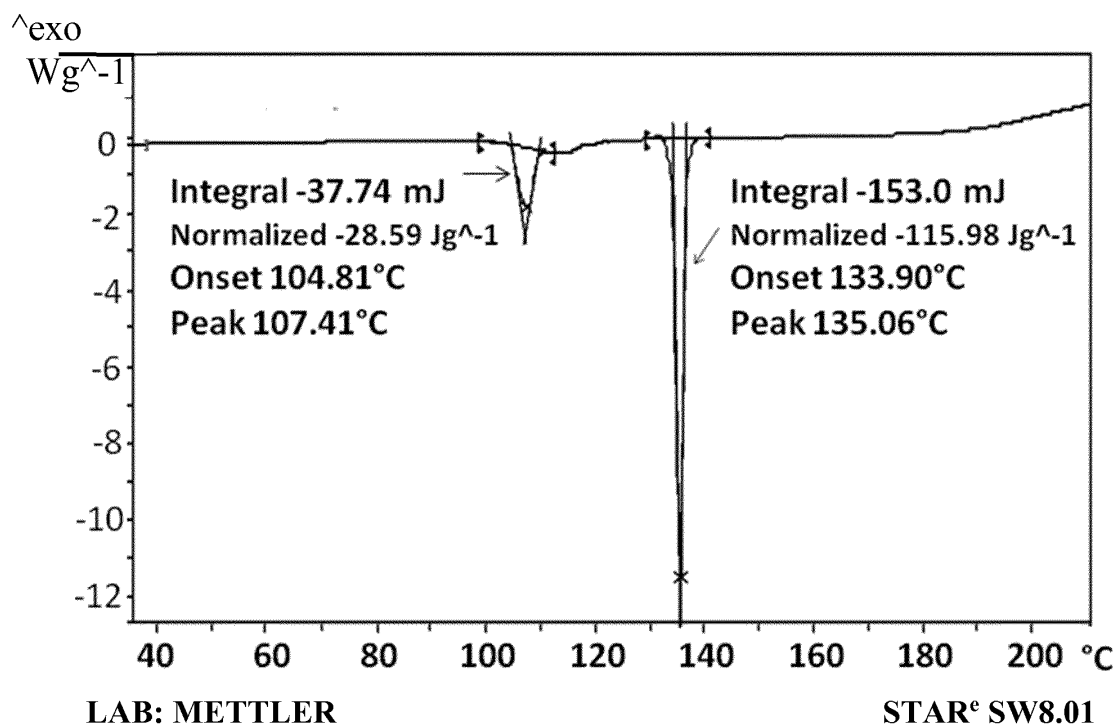


Fig. 3B

4/17

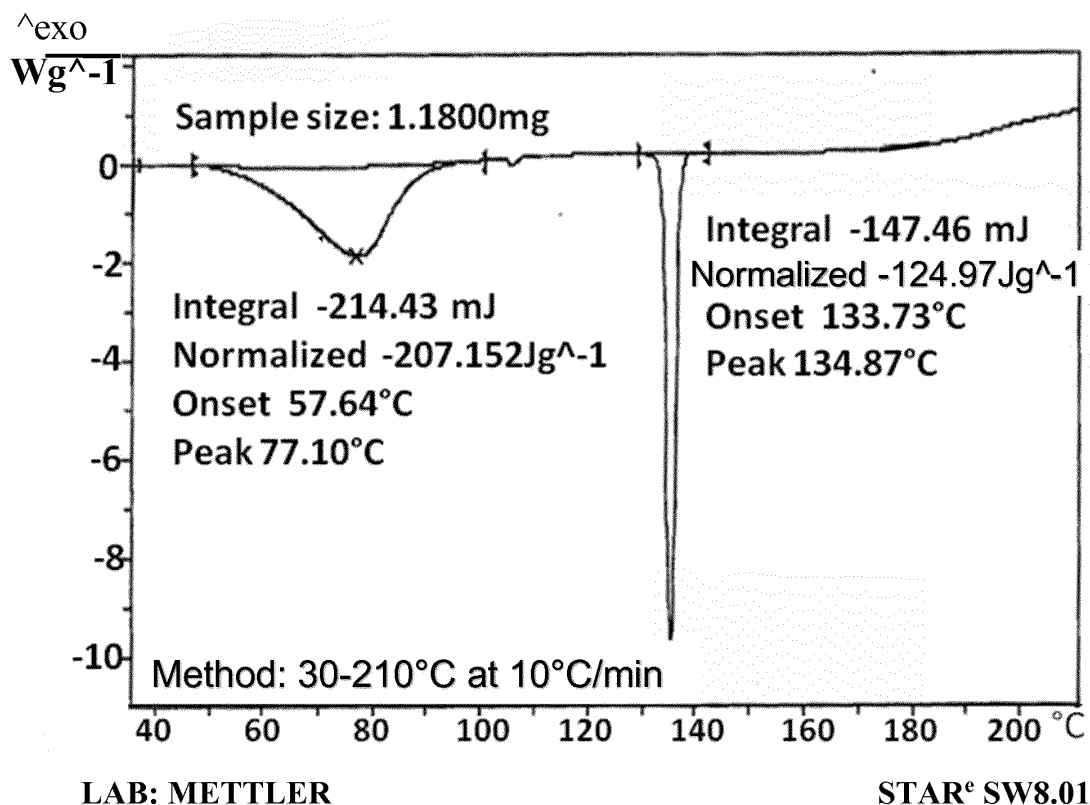


Fig. 4A

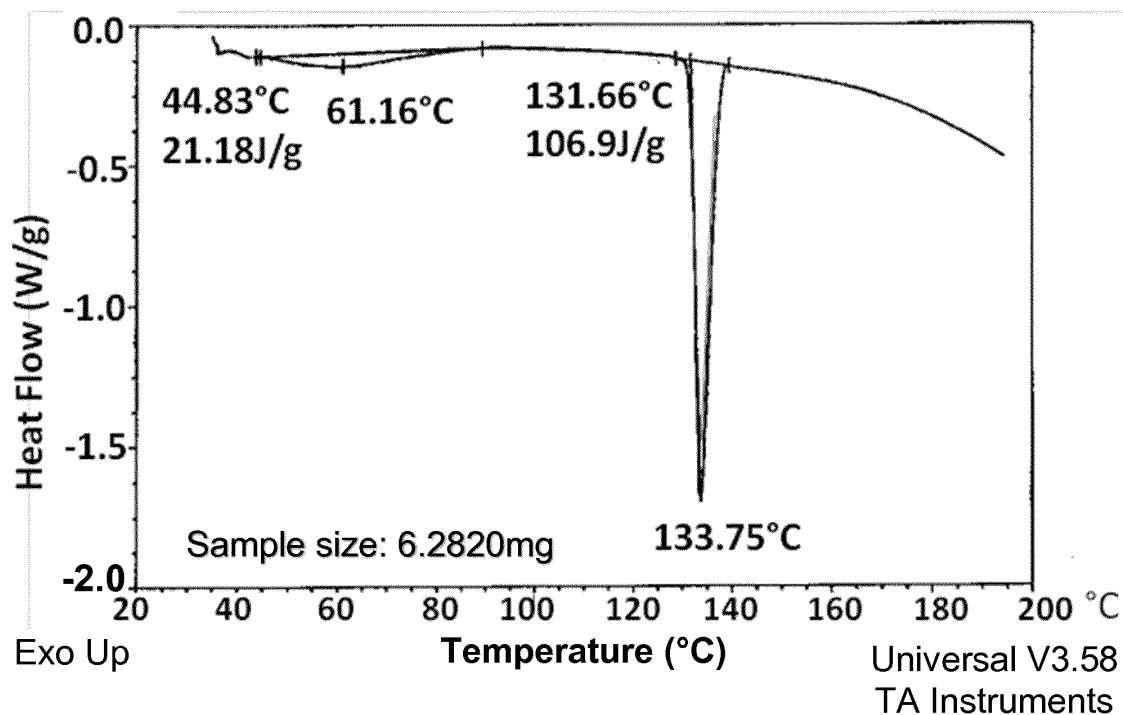


Fig. 4B

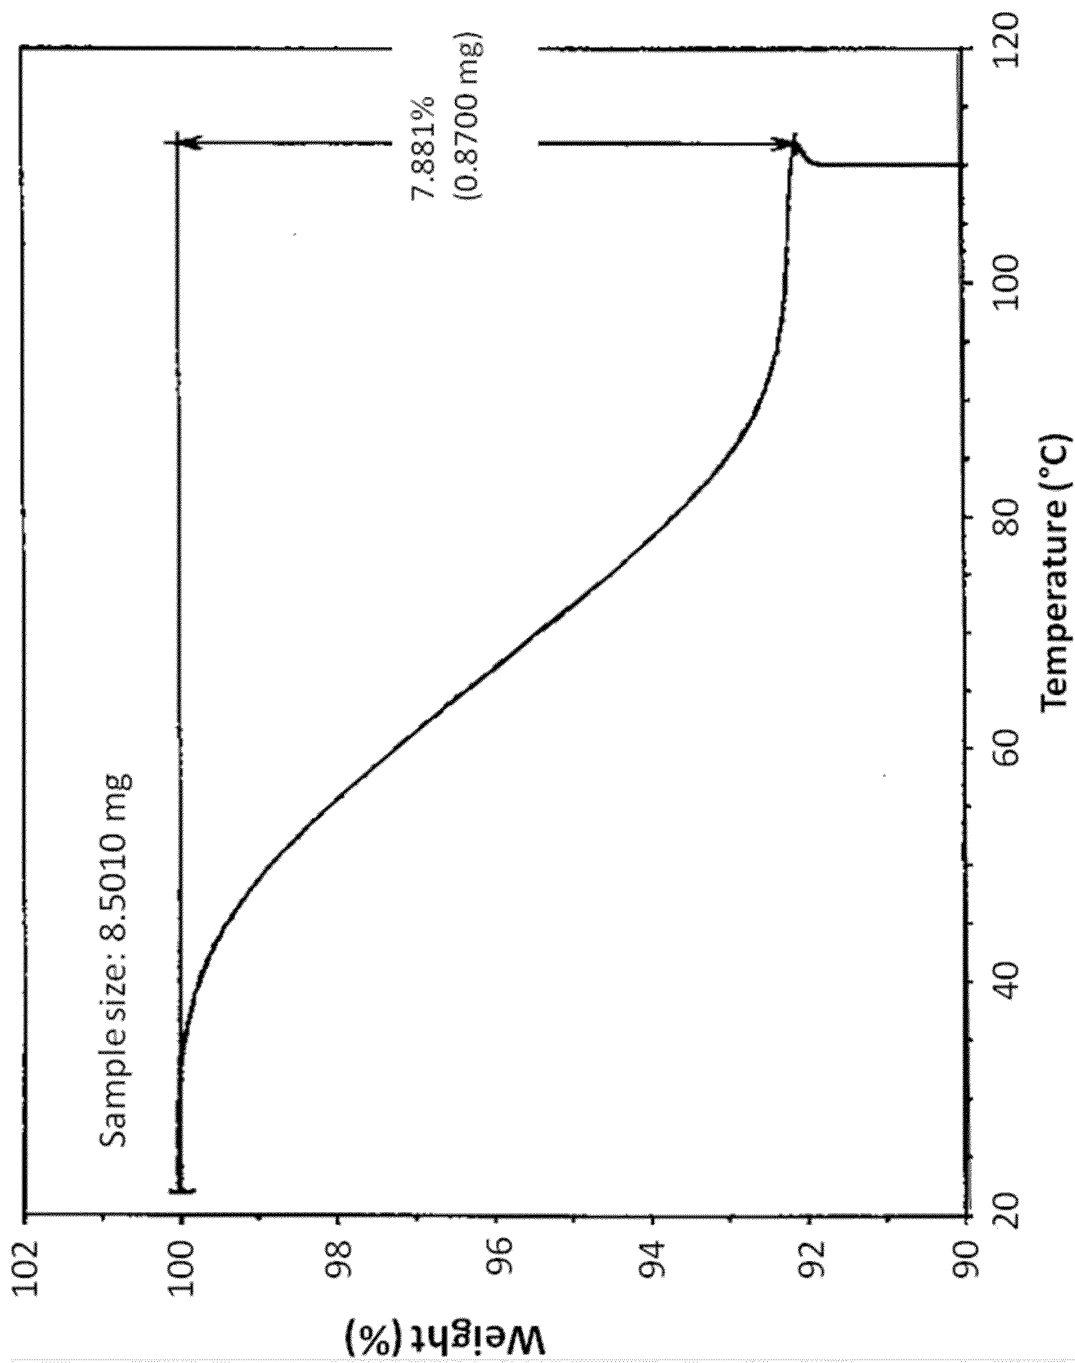


Fig. 5

6/17

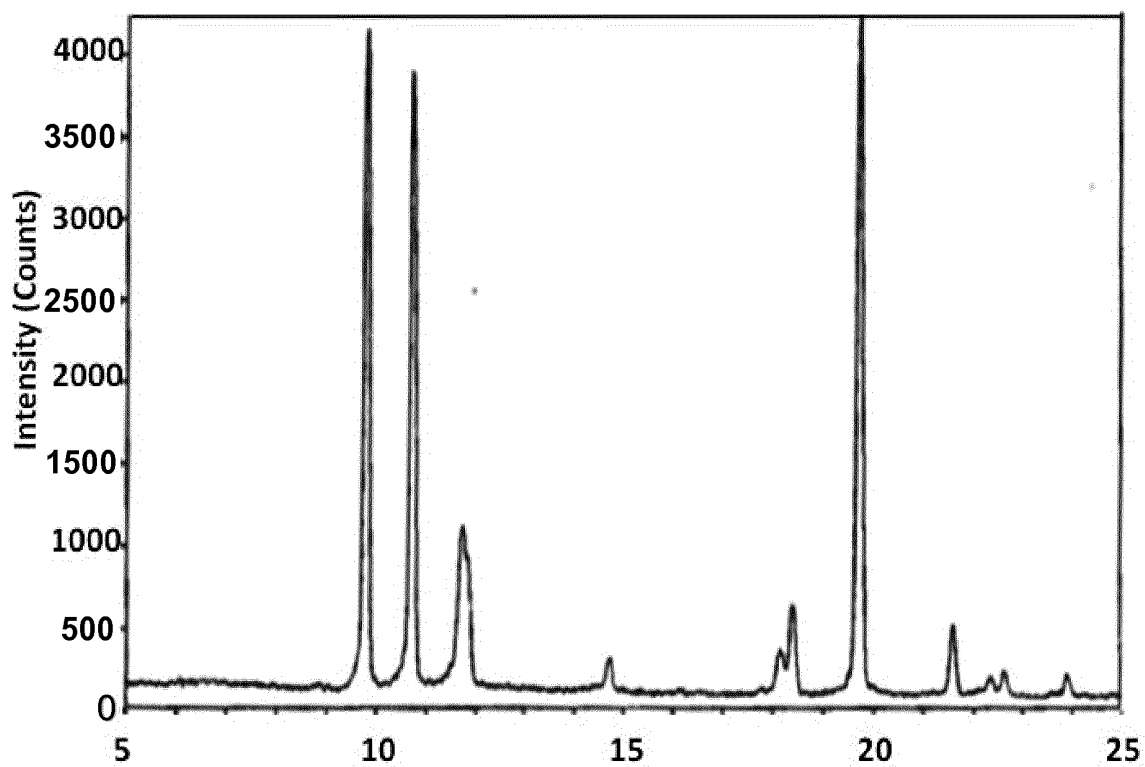


Fig. 6A

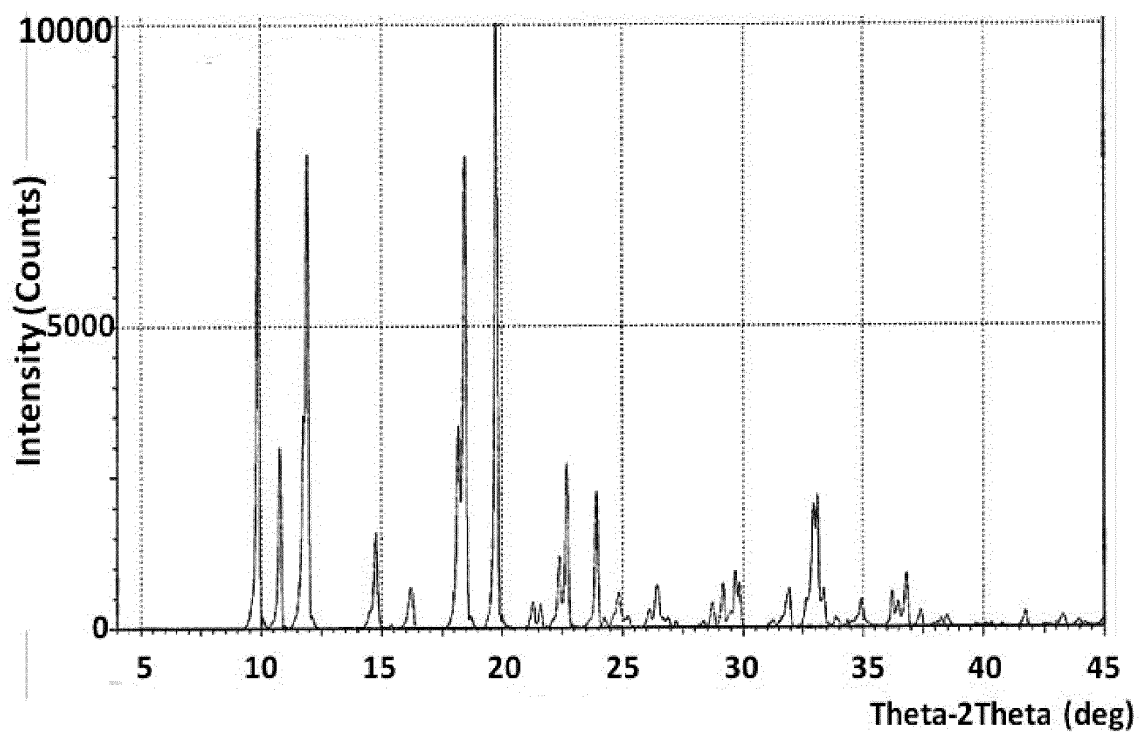


Fig. 6B

7/17


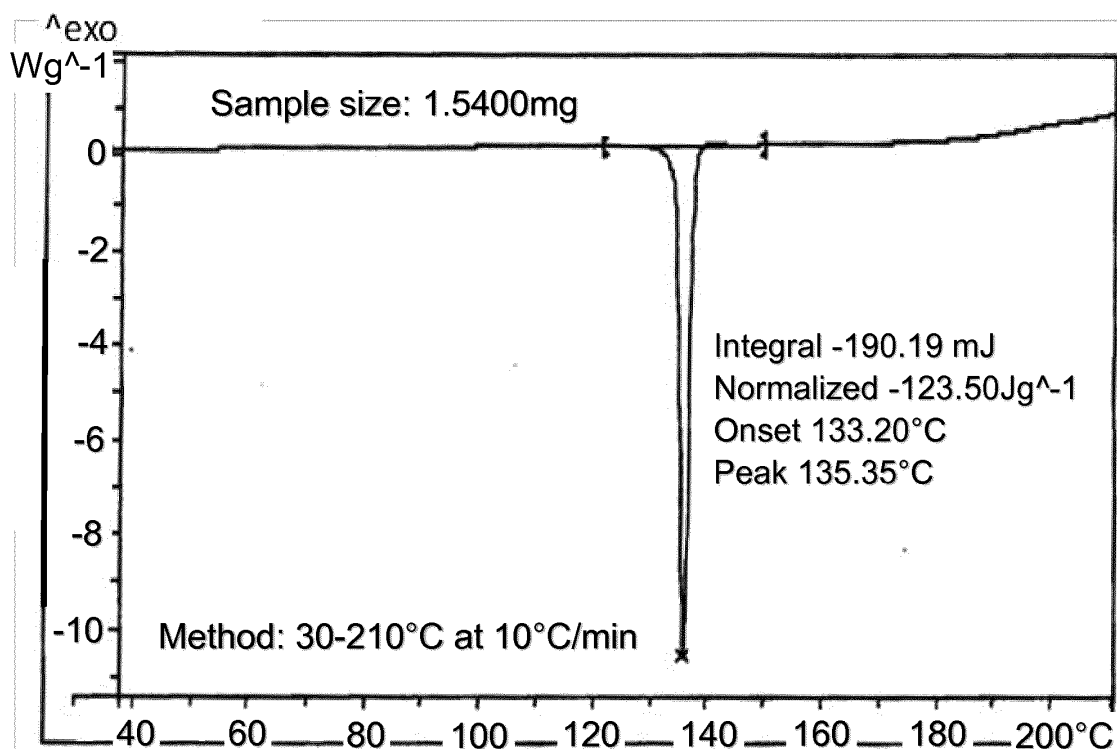


Fig. 7A

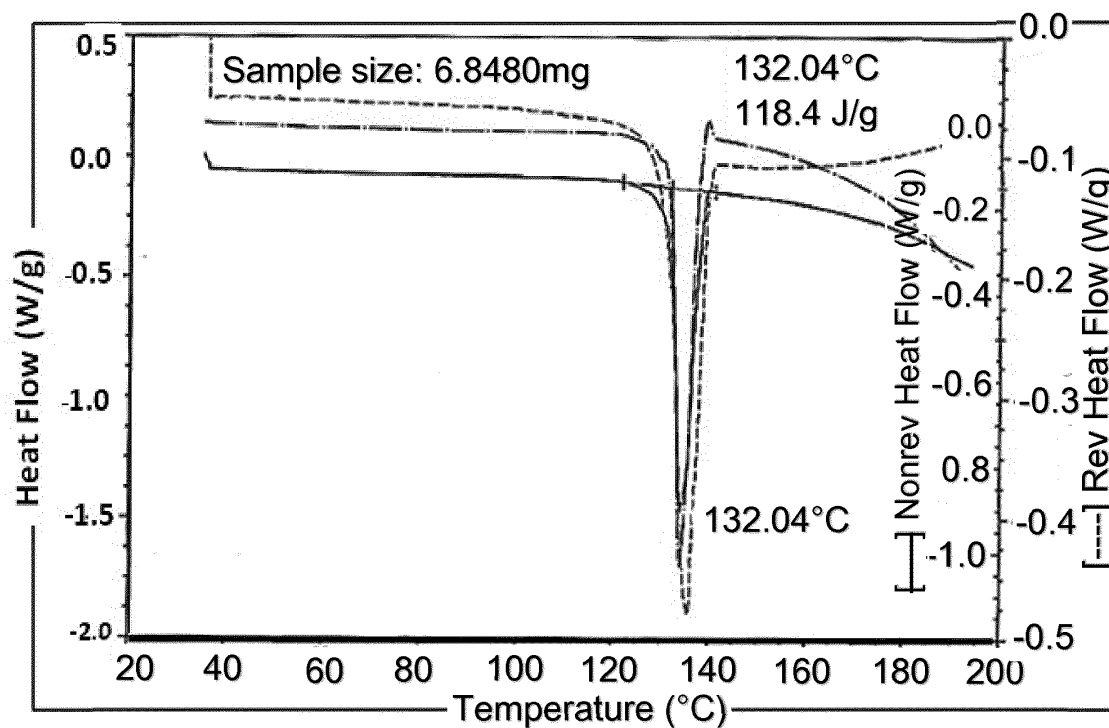

Exo Up

Universal V3.58
TA Instruments

Fig. 7B

8/17

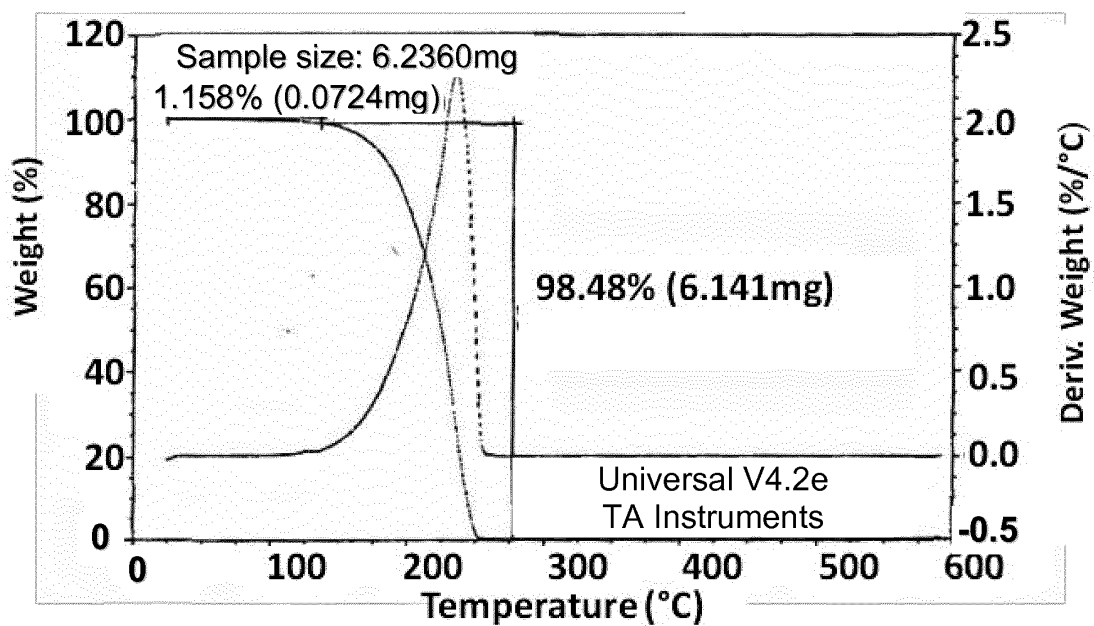


Fig. 8A

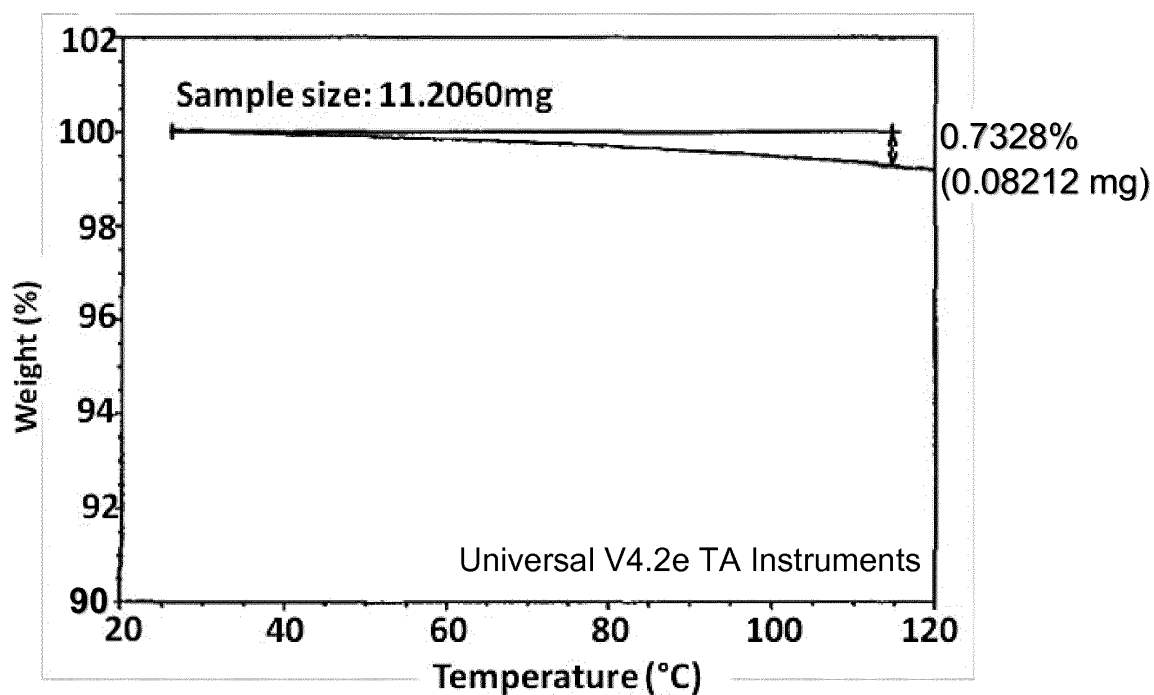


Fig. 8B

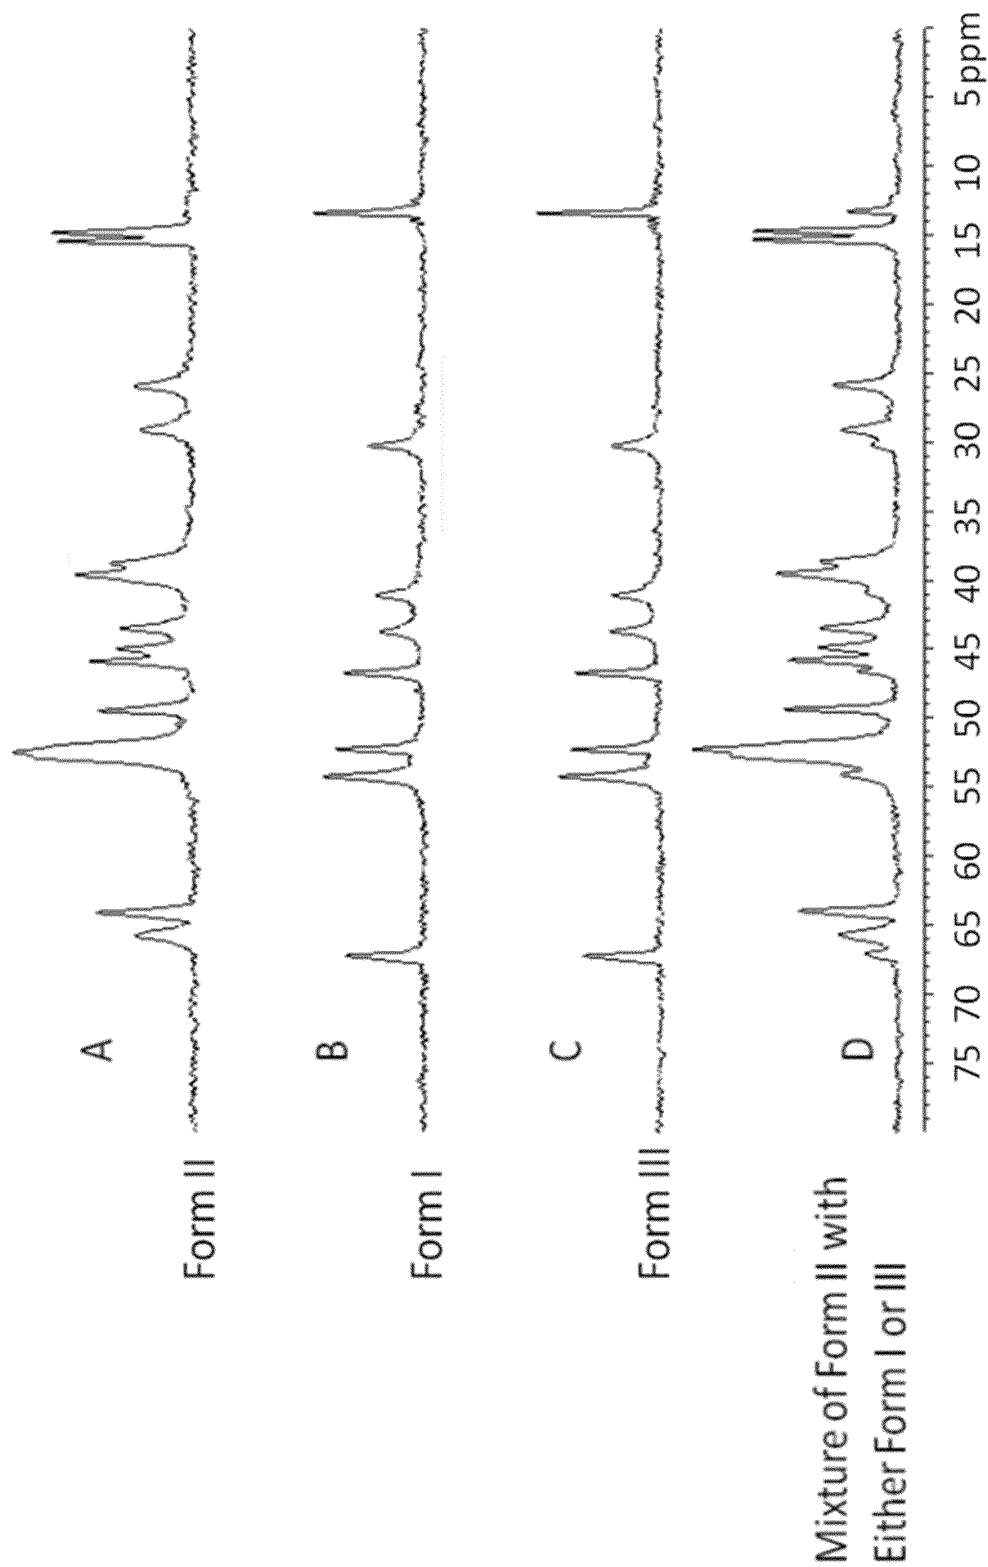


Fig. 9

10/17

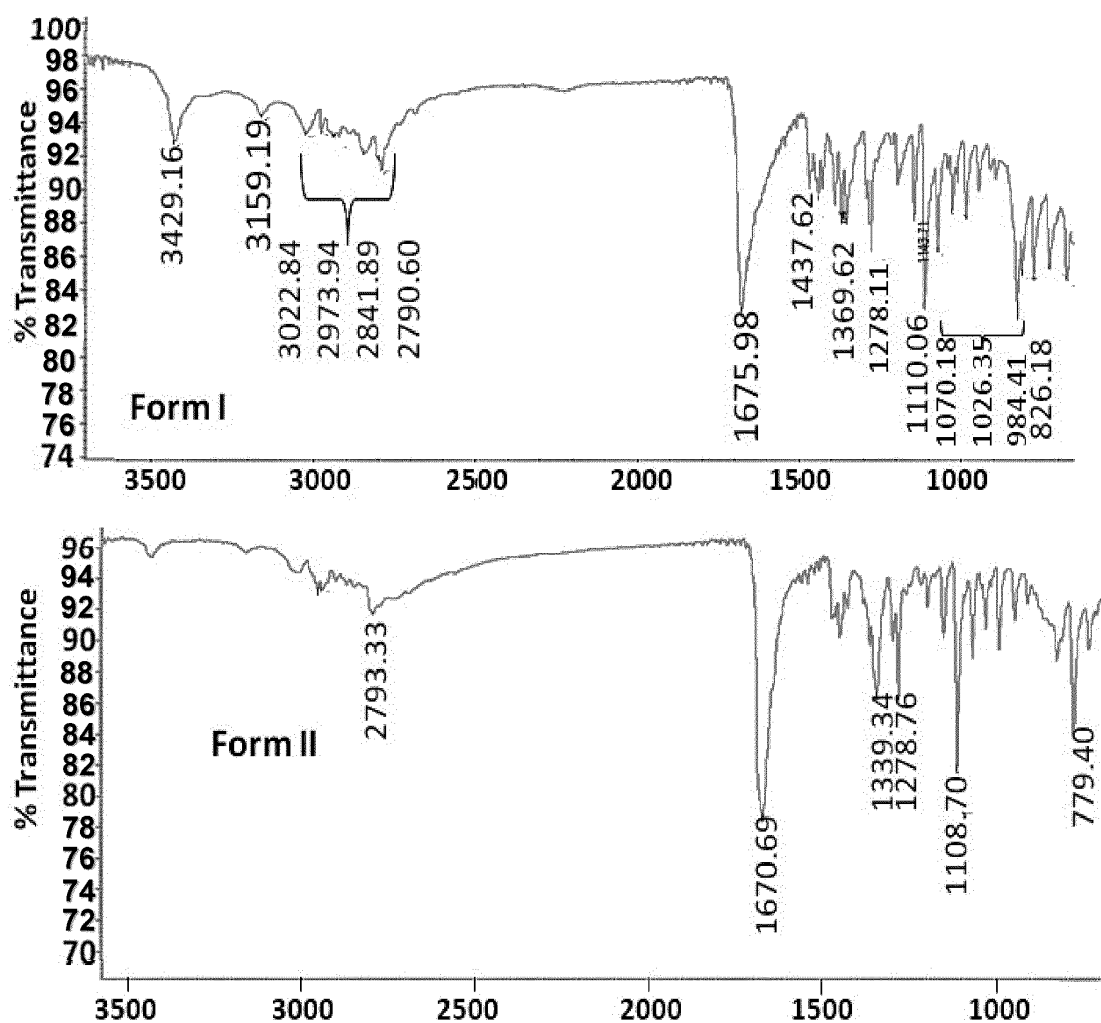


Fig. 10A

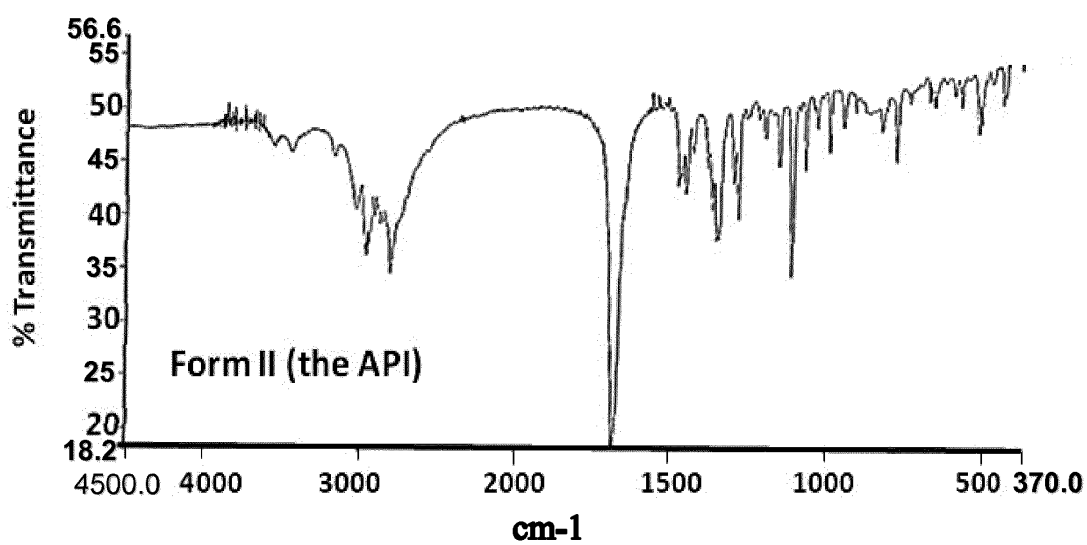


Fig. 10B

11/17

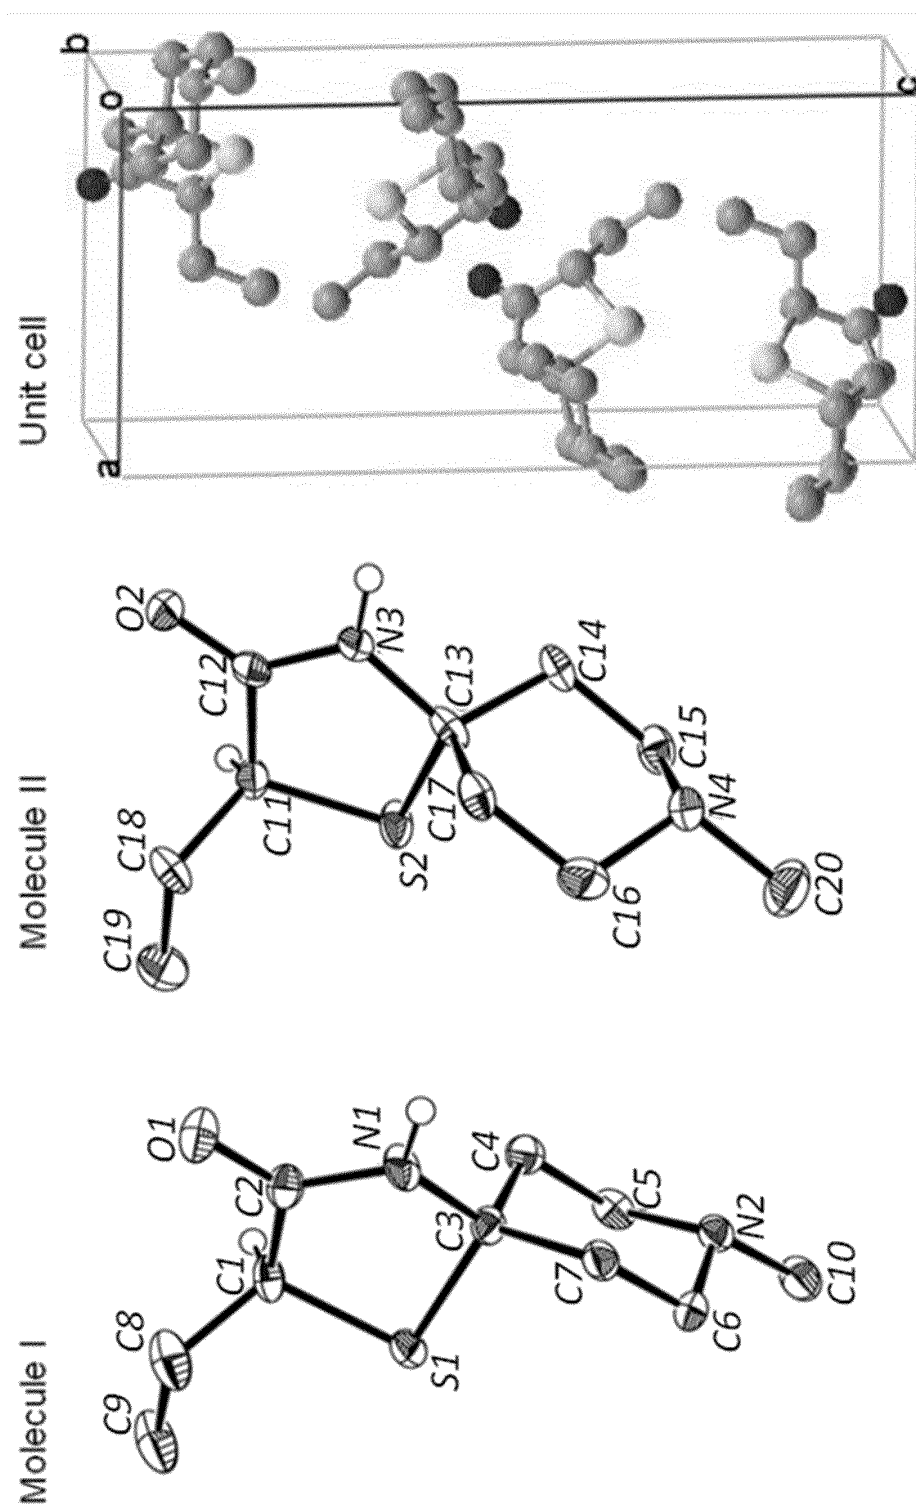


Fig. 11

12/17

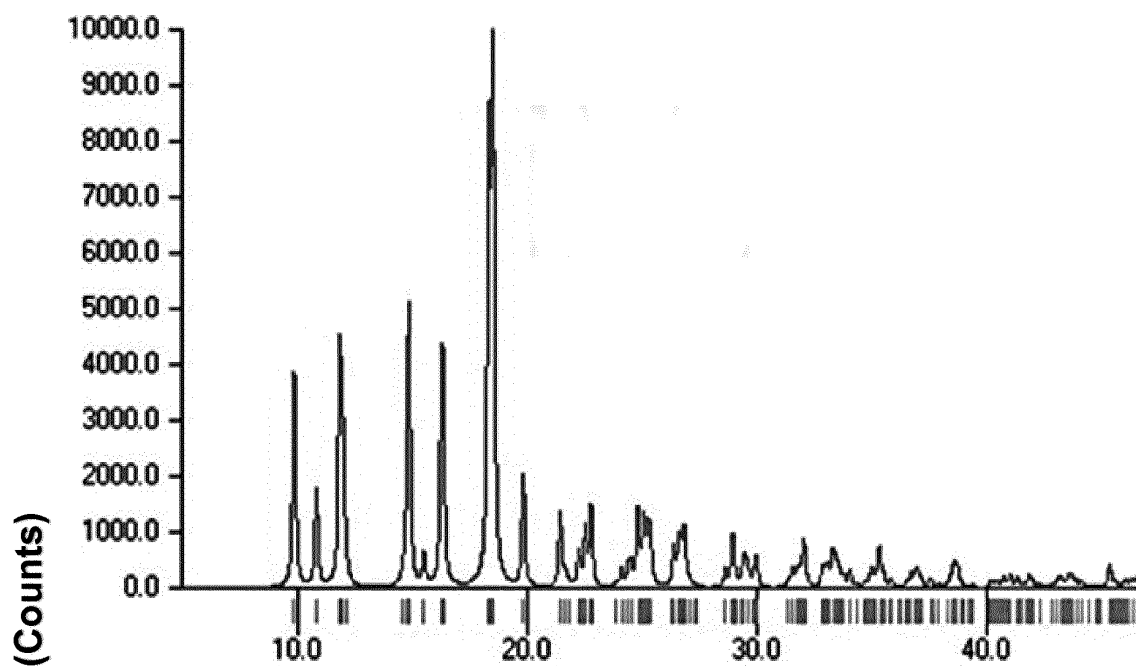


Fig. 12A

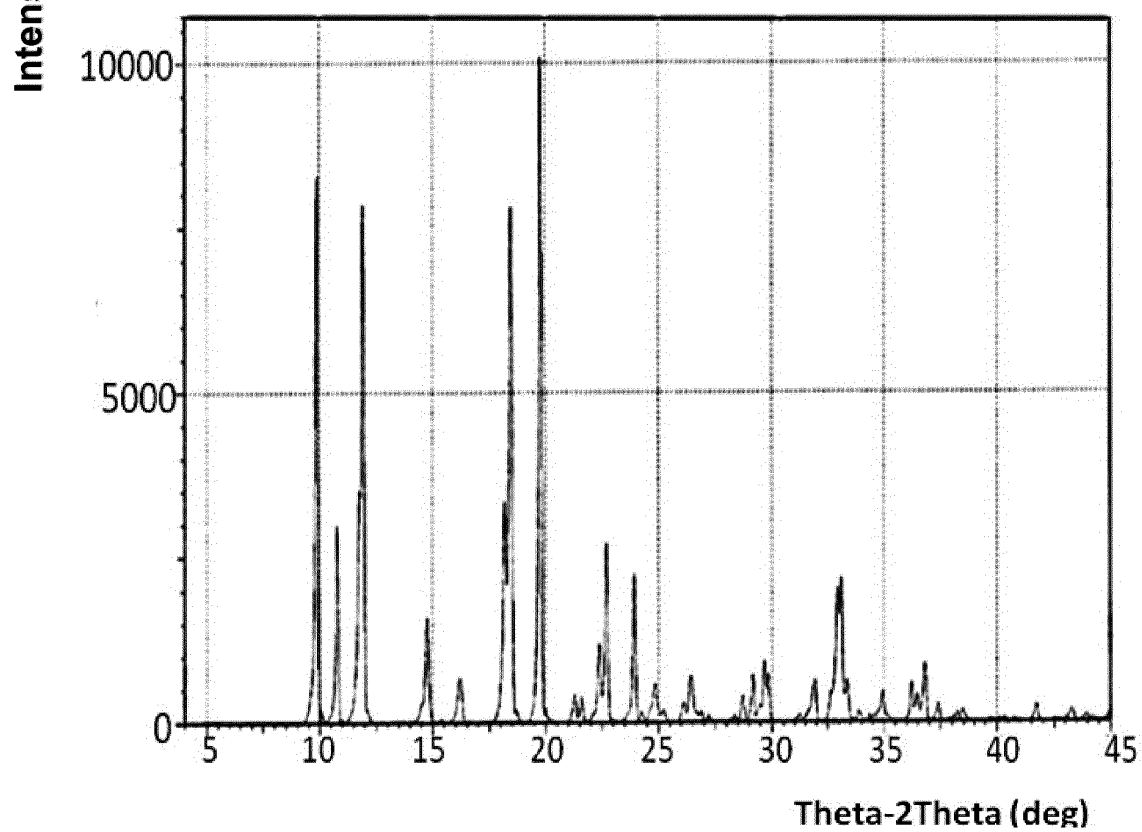


Fig. 12B

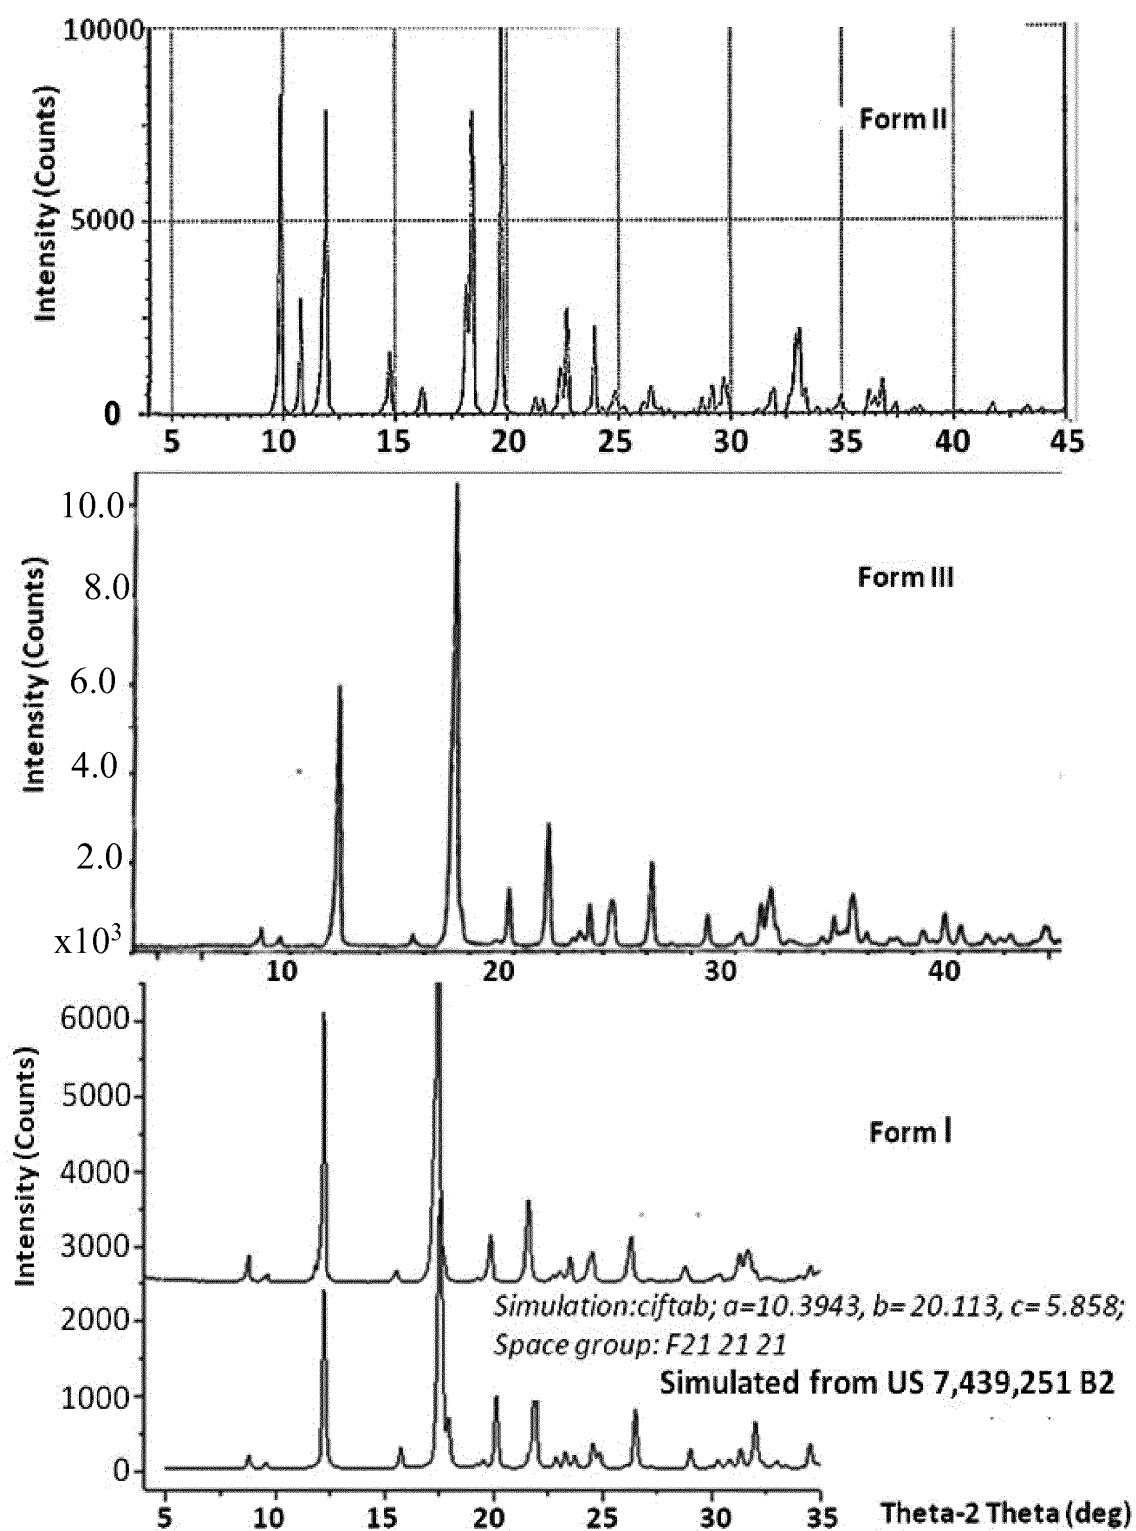


Fig. 13

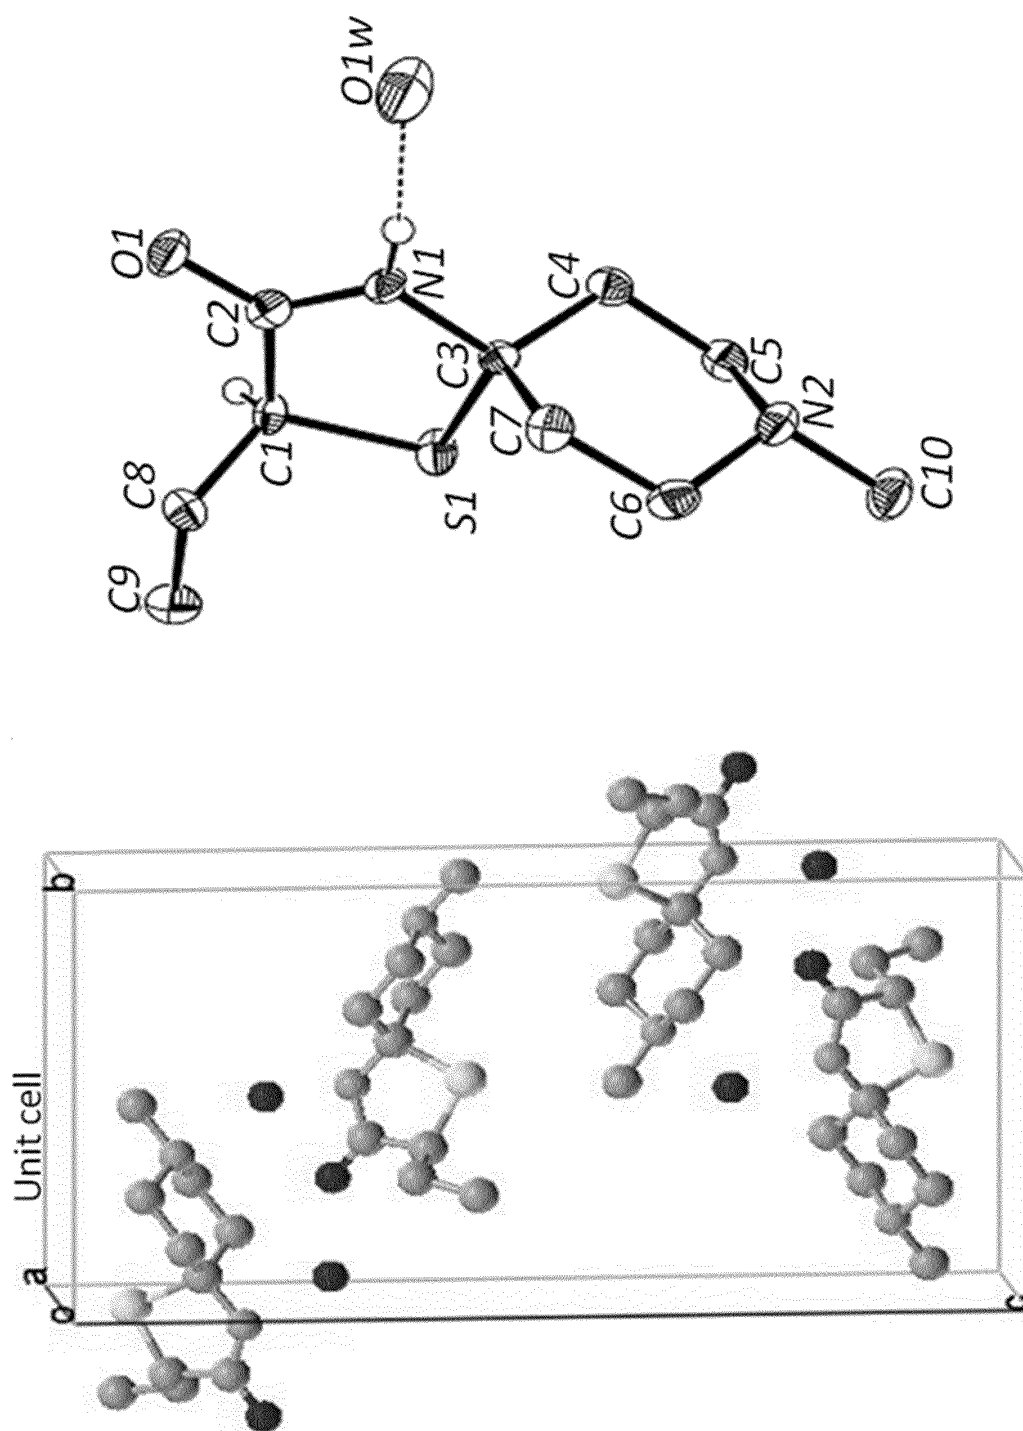


Fig. 14

15/17

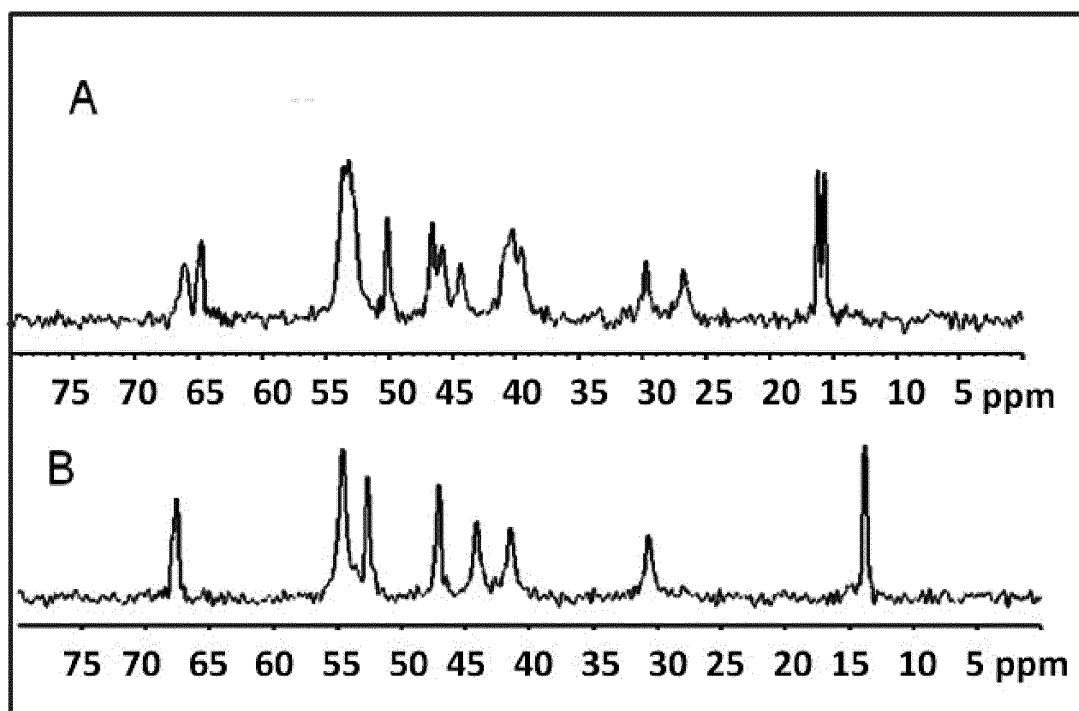


Fig. 15A

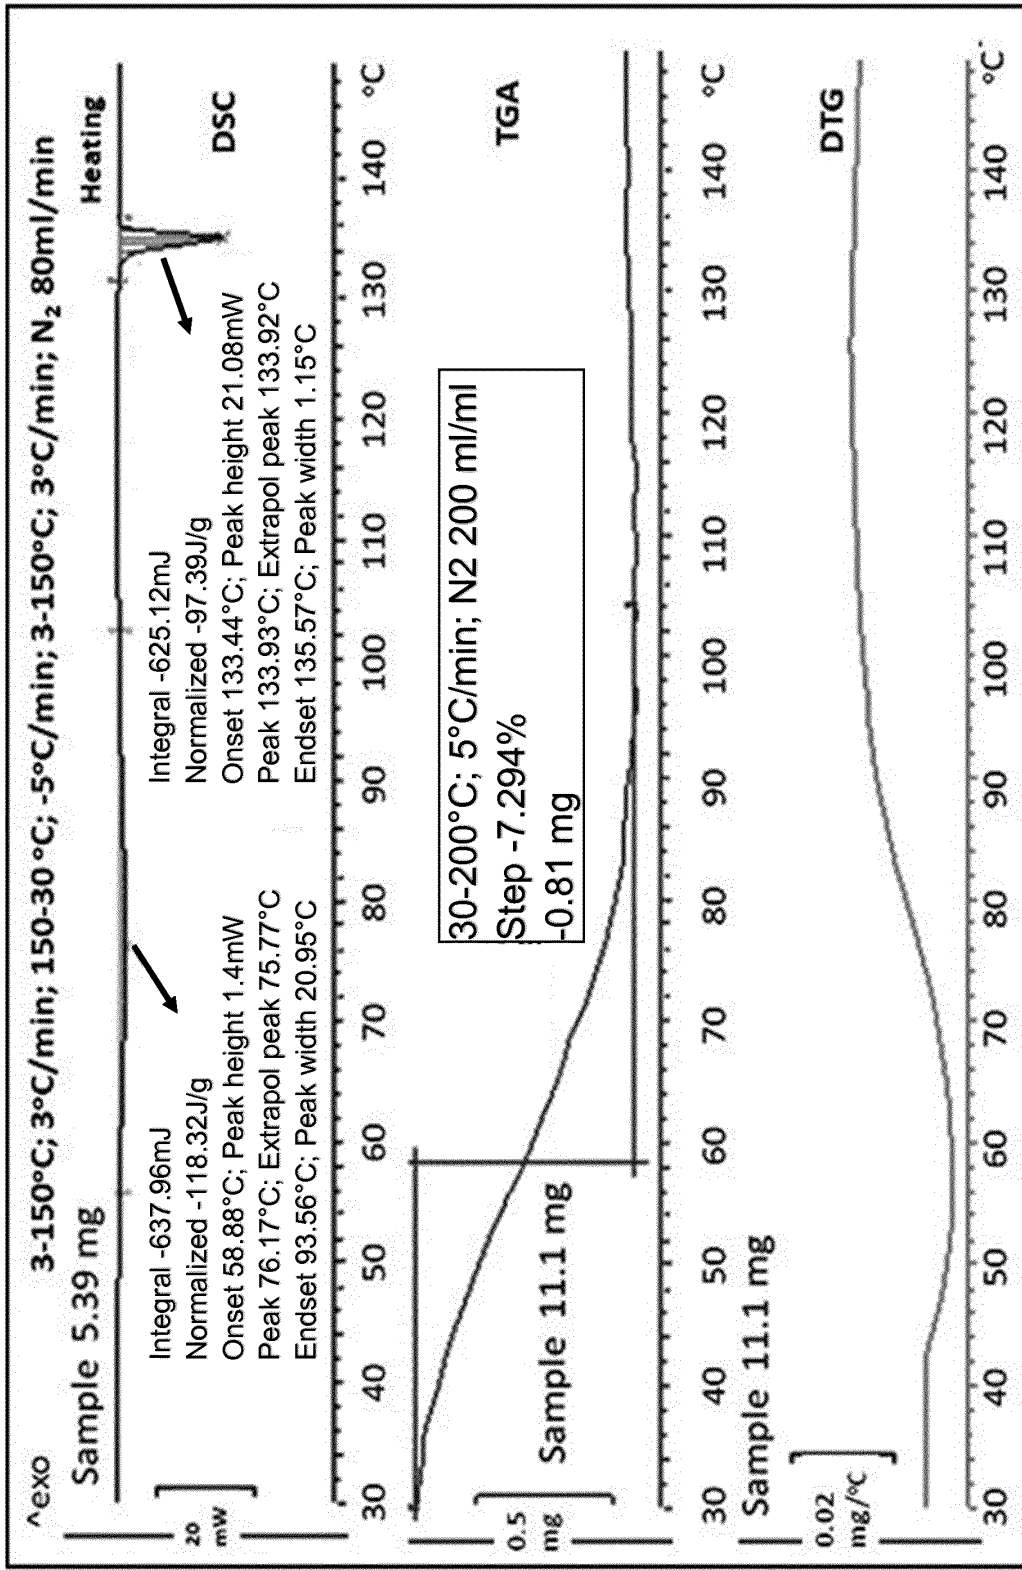


Fig. 15B

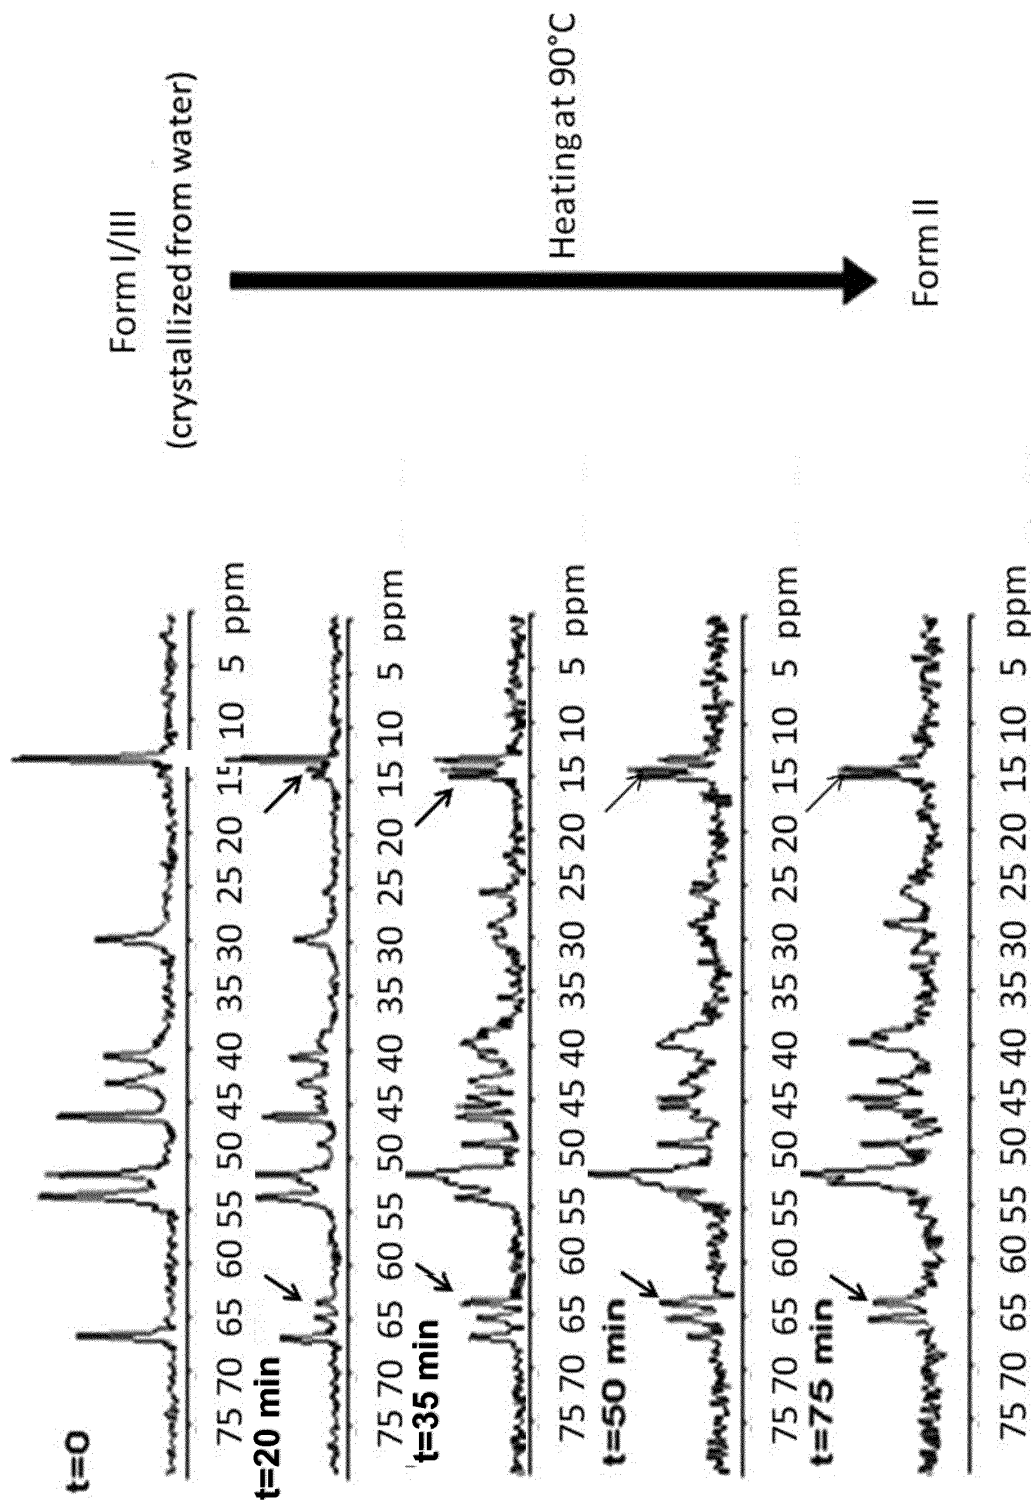


Fig. 16