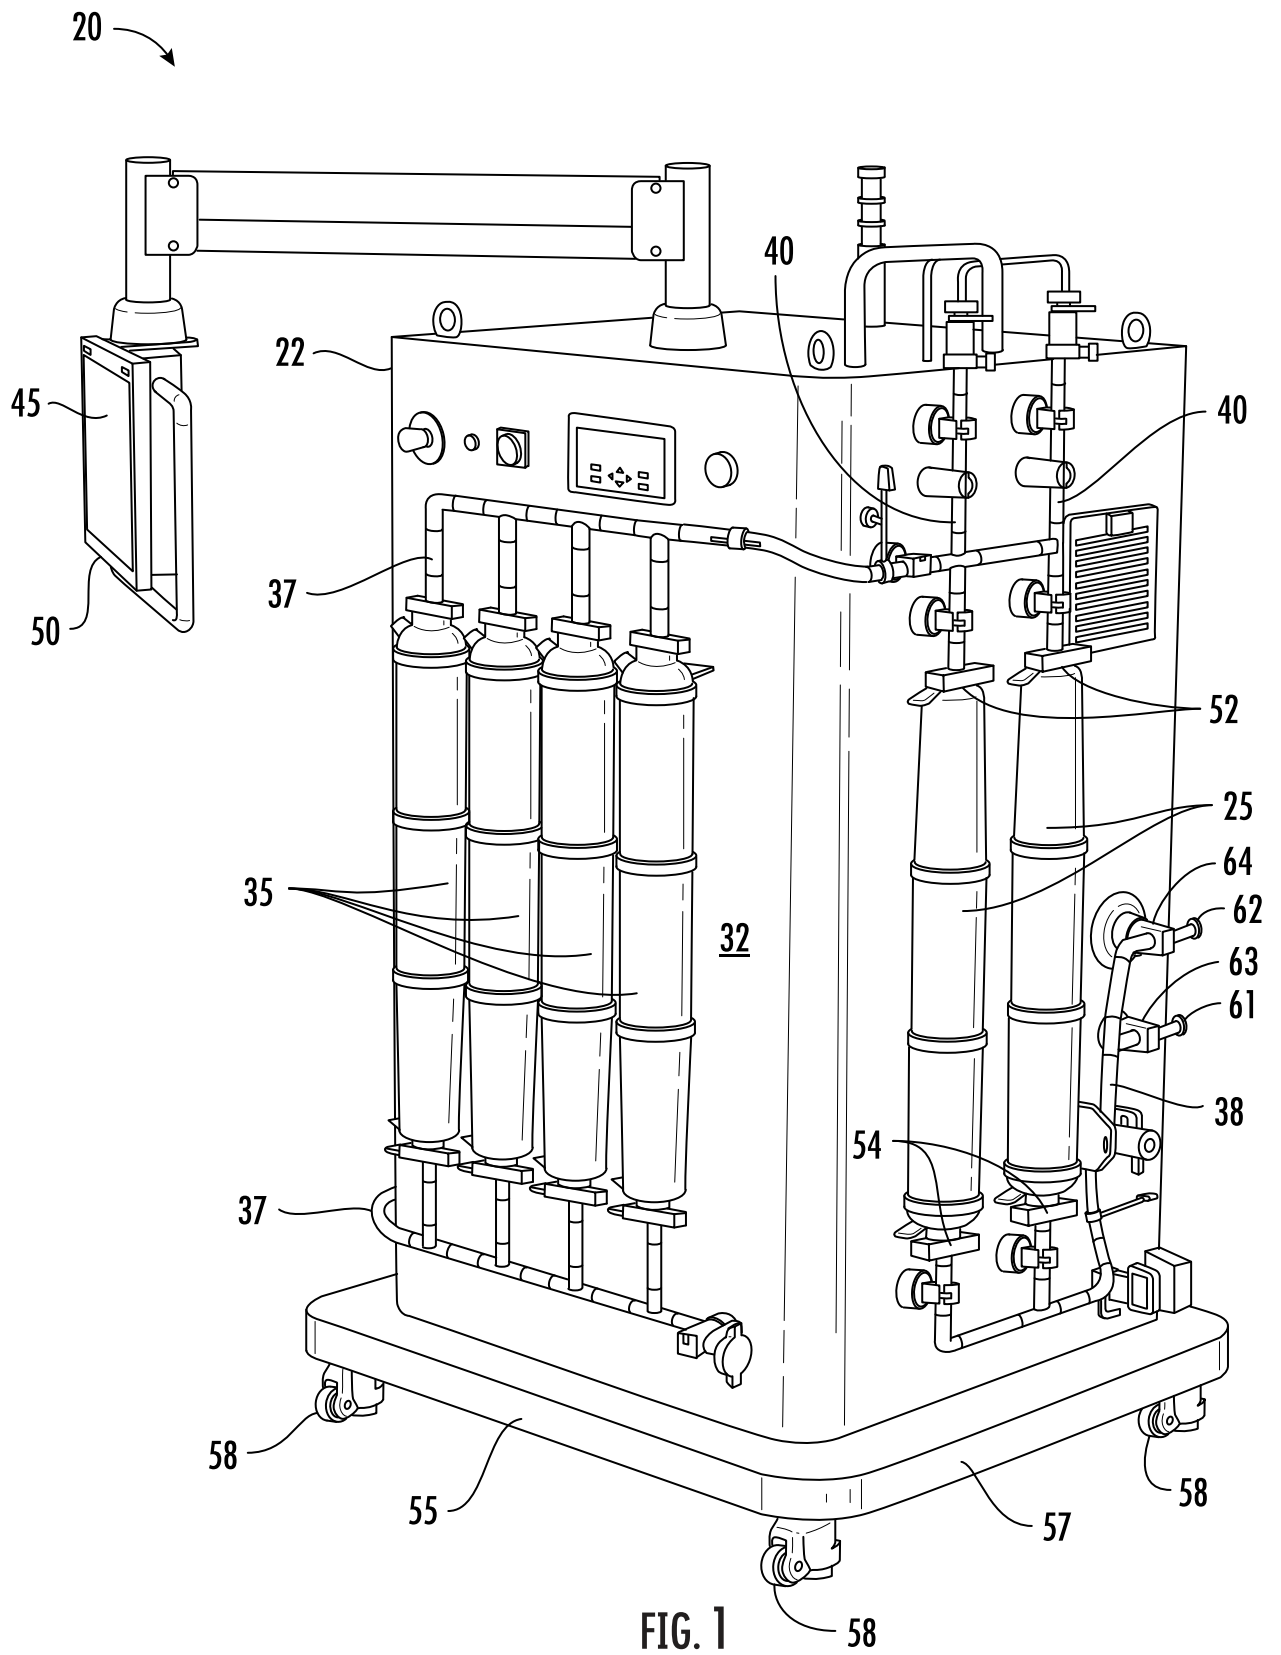




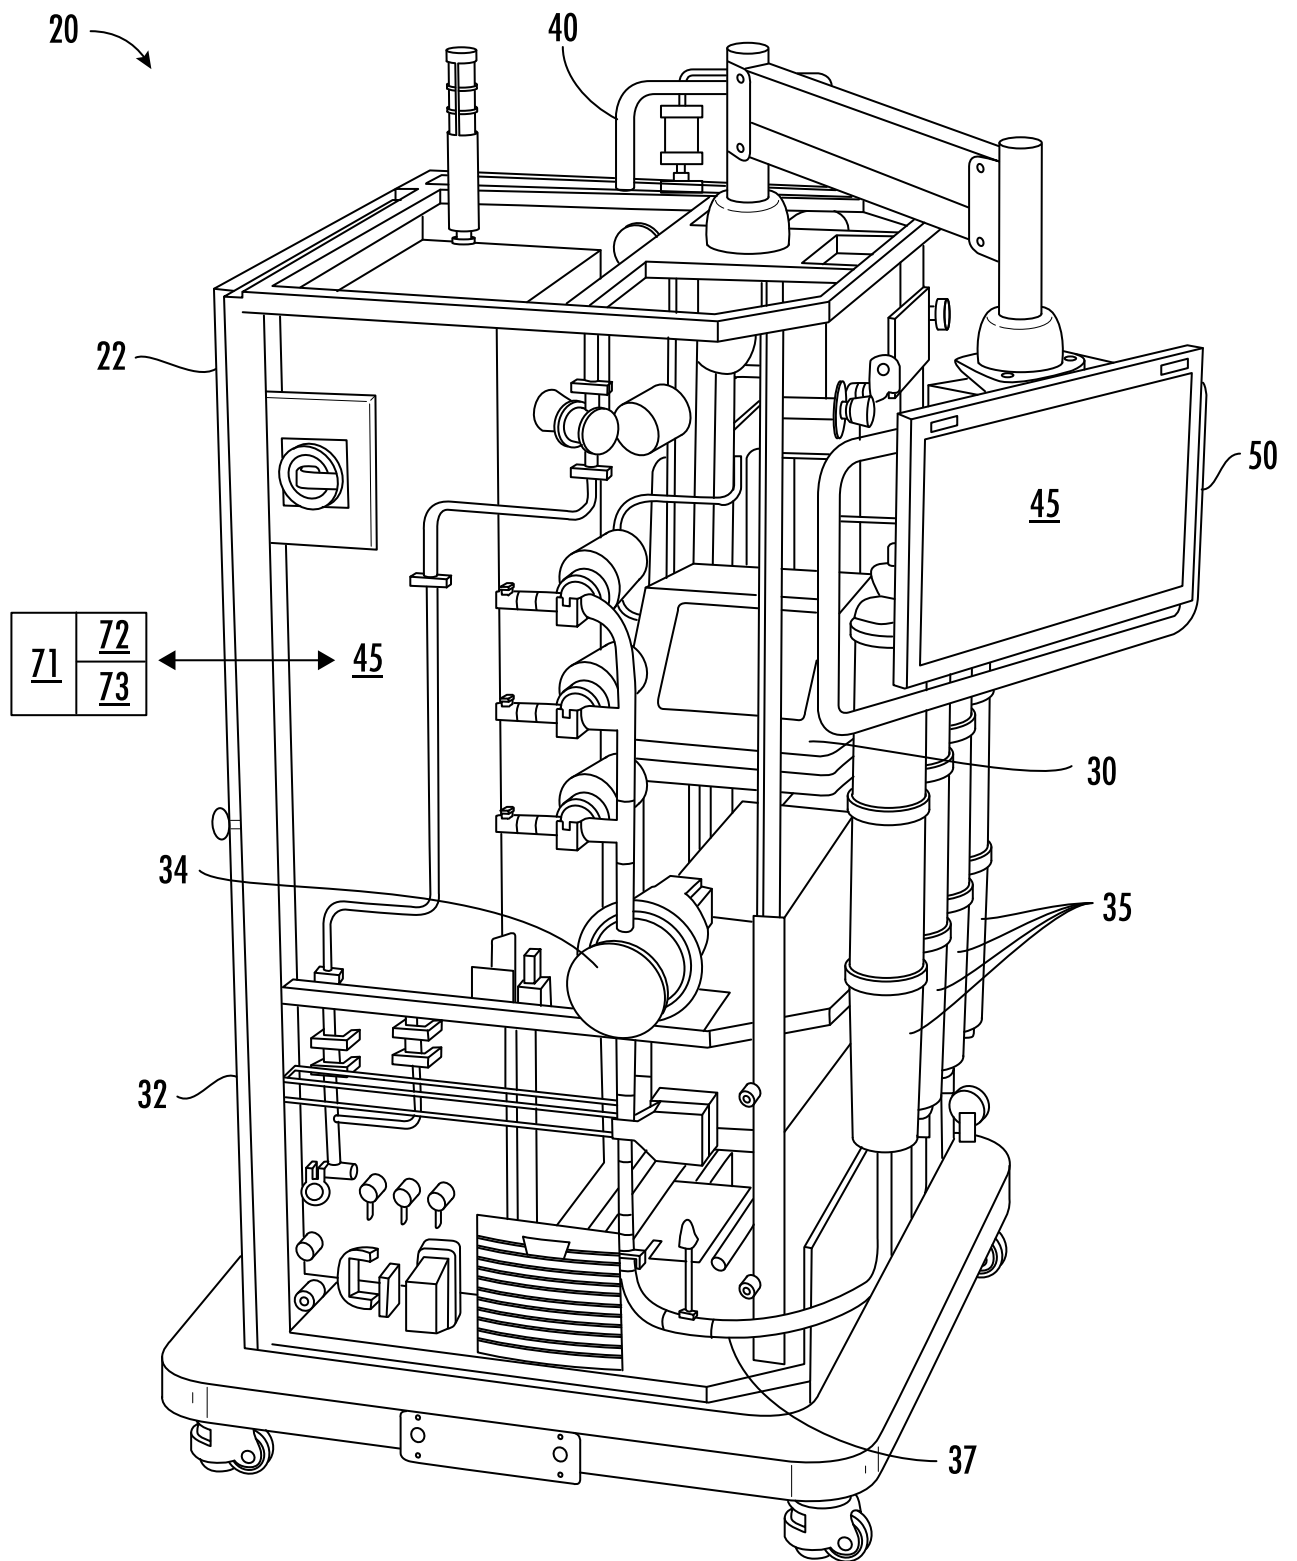


FIG. 2

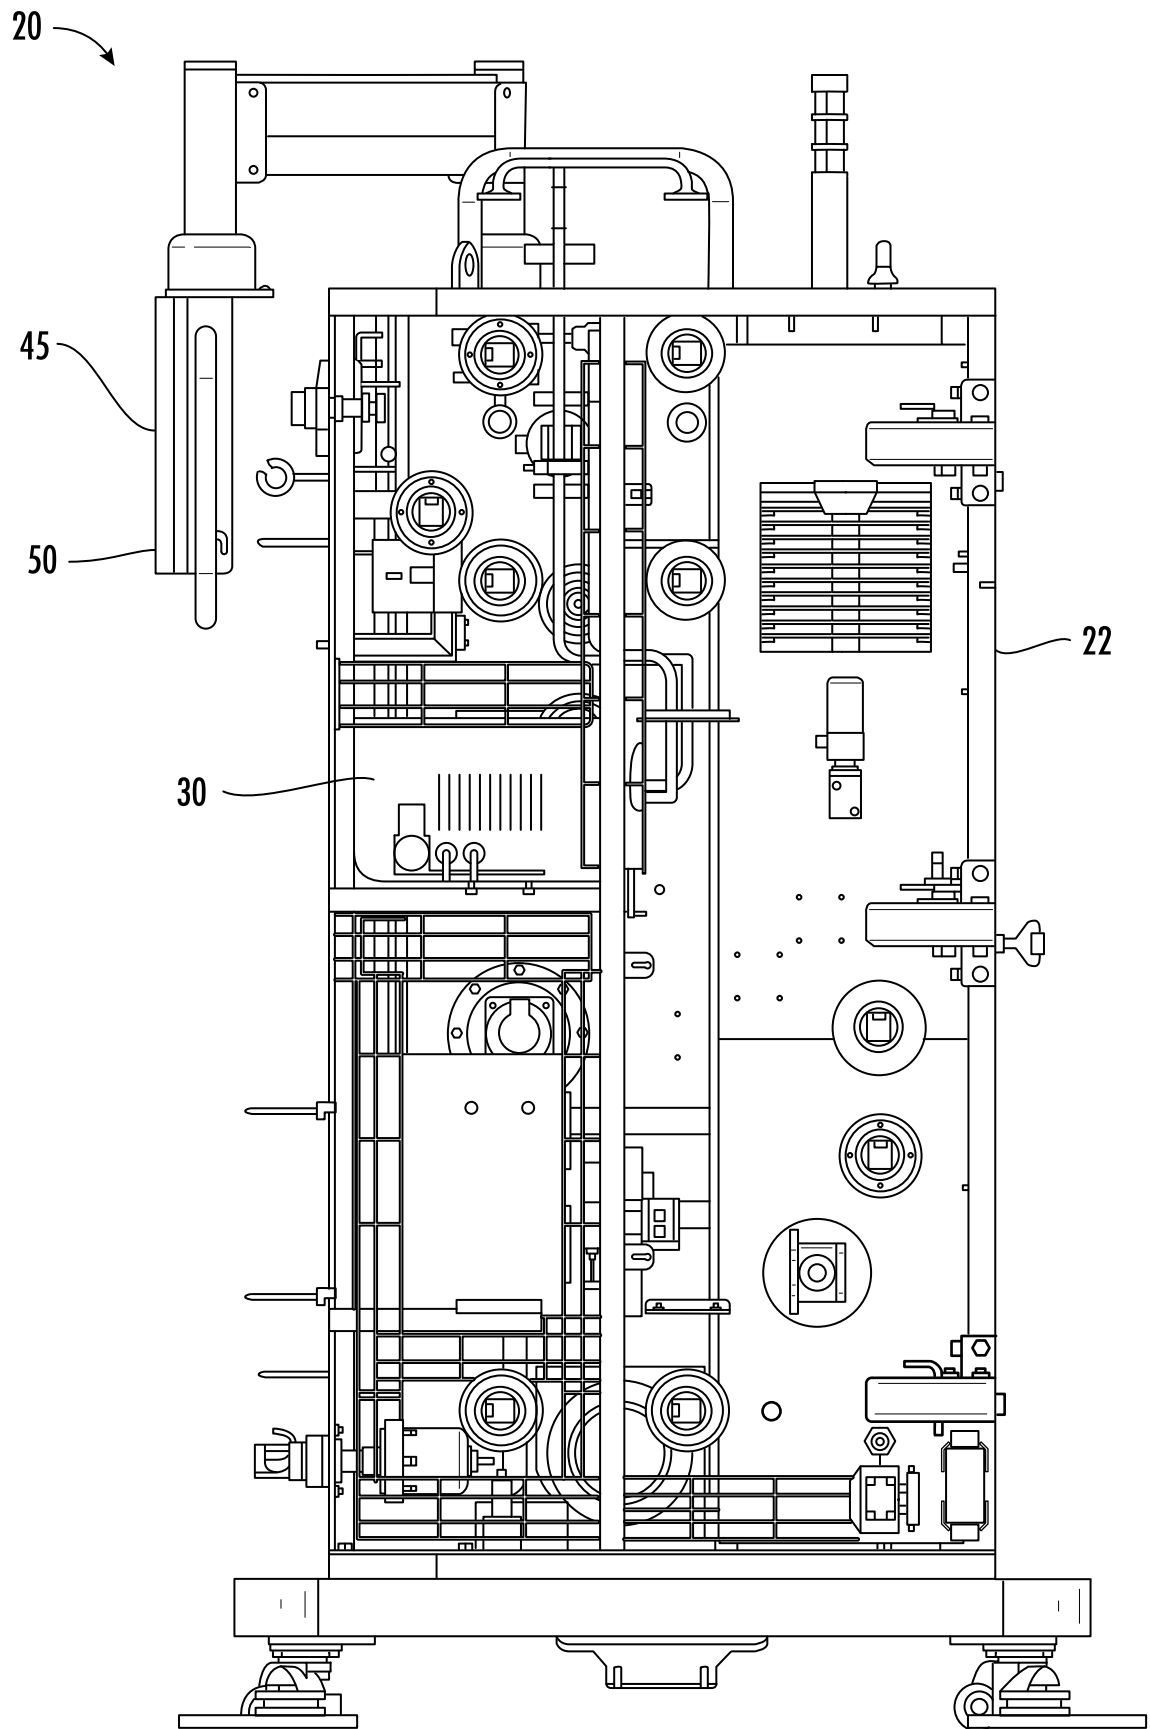
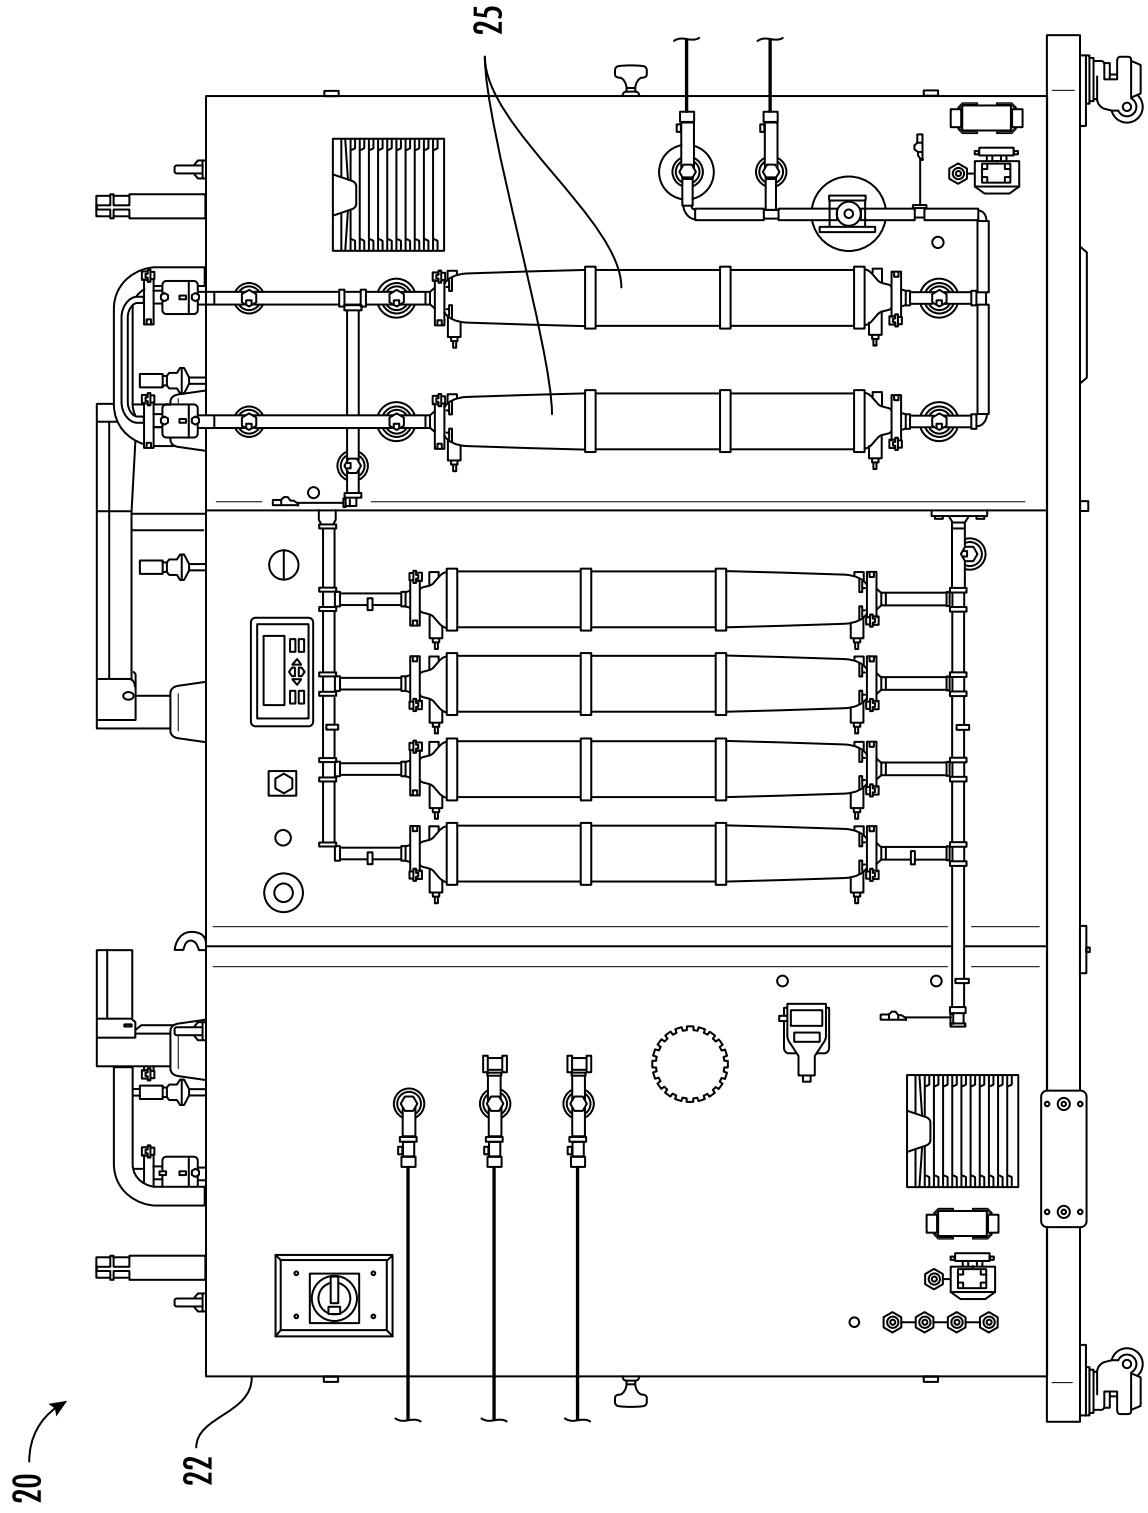
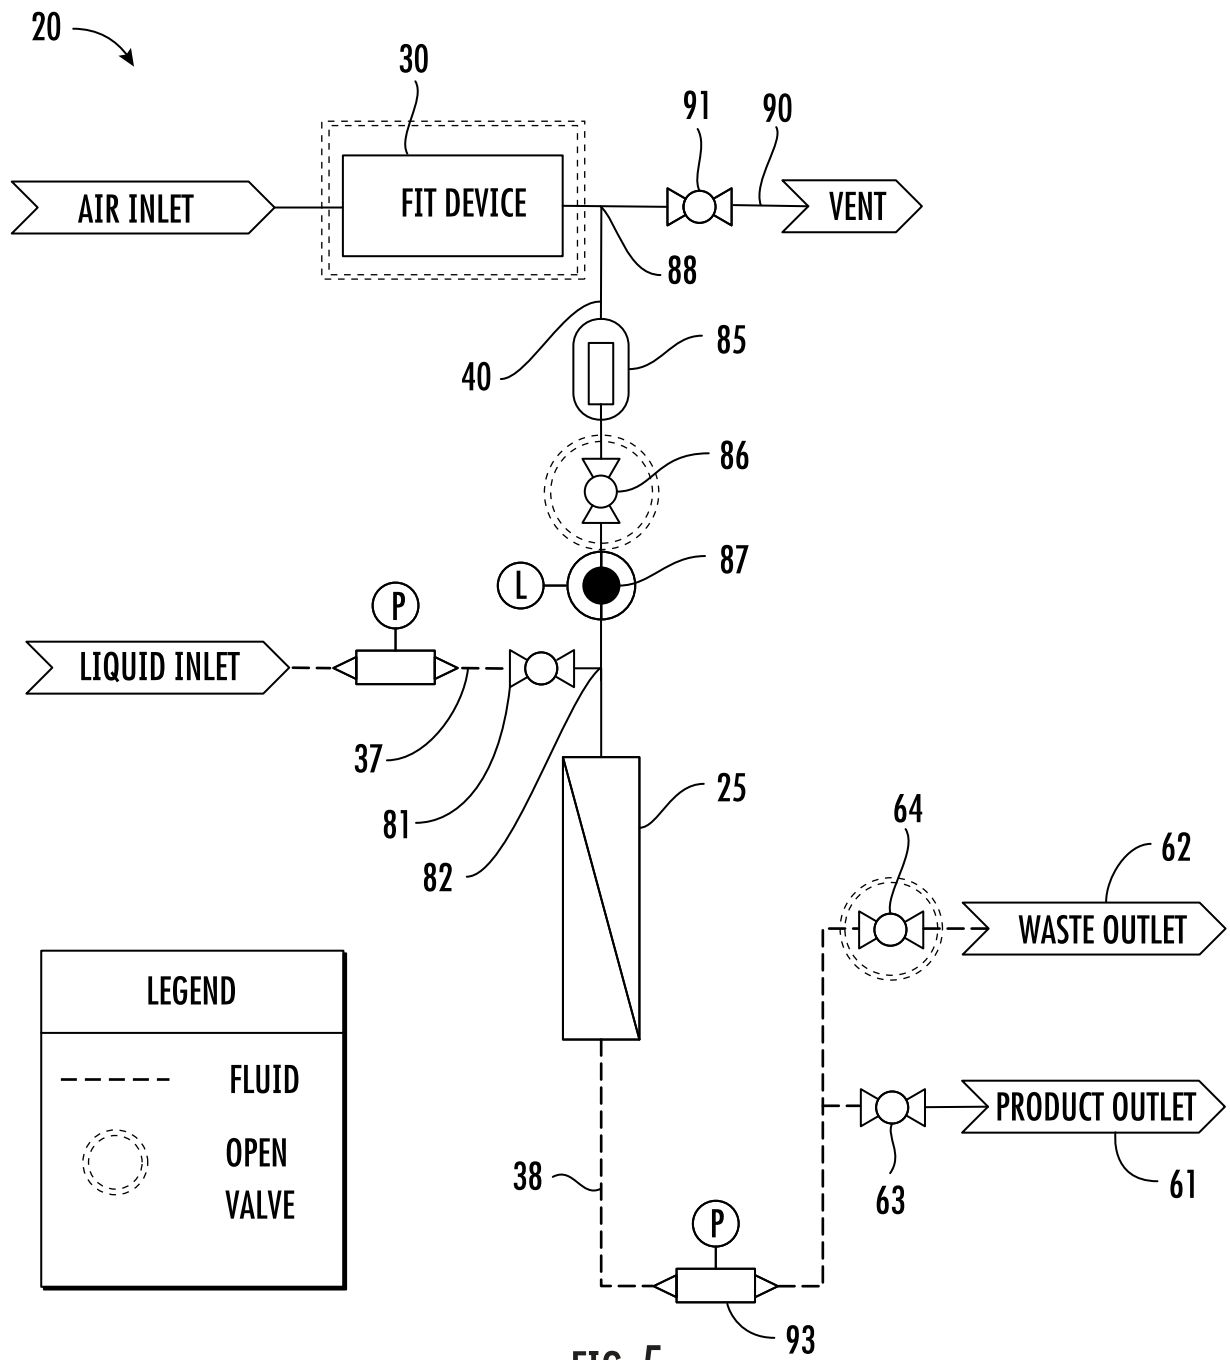


FIG. 3





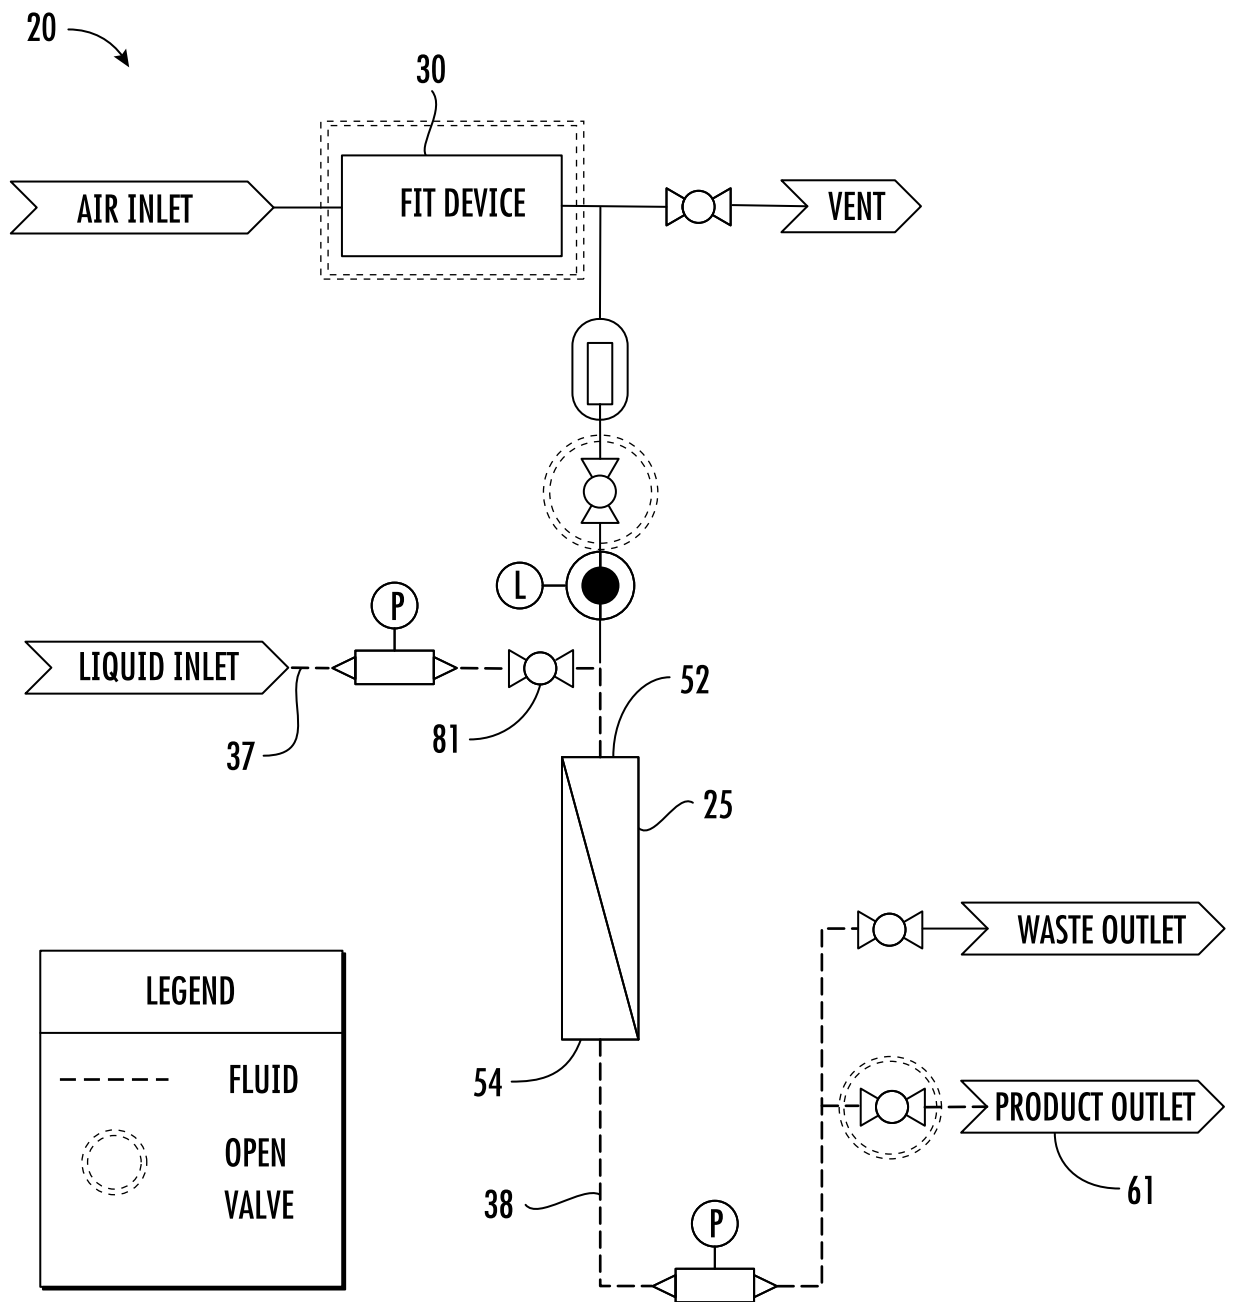


FIG. 6

95 →

BULK FILL

MBF01

23-MAR-2021

07:27:18

BATCH

RECIPE

UNIT OP

OPERATION

BATCH 283

TESTFILTERIT

UNITOP

TESTOP

OK

RPHPPOSTFILTERIT - RUN

EEENG

LOG OUT

FORWARD FLOW TEST: F2 (TO FLUSH)

PRESSURIZATION

STABILIZATION

VENTING

RESULTS

○

○

○

●

☑ PASSED

49.9 ML/MIN

ACCEPTABLE RANGE: 10.0-100.0 ML/MIN

PRE-STABL PRESSURE: 50 MBAR

PRE-STABL TIME: 0 S

TEST PRESSURE: 50 MBAR

TEST TIME: 100 S

SYSTEM VOLUME: N/A

FILTER HOUSING: N/A

WETTING LIQUID: WIT

TEST GAS: 02

TEST STARTED: 07:24:46 MAR-23

TEST COMPLETE: 07:26:09 MAR-23

COMMENT:

RE-TEST

CONTINUE

🏠

⚙️

📊

📅

📄

📋

📄

📄

⏏

⚙️

PROCESS

ALARMS


TRENDS

EVENT LOG

RECIPES

REPORTS

FIG. 7

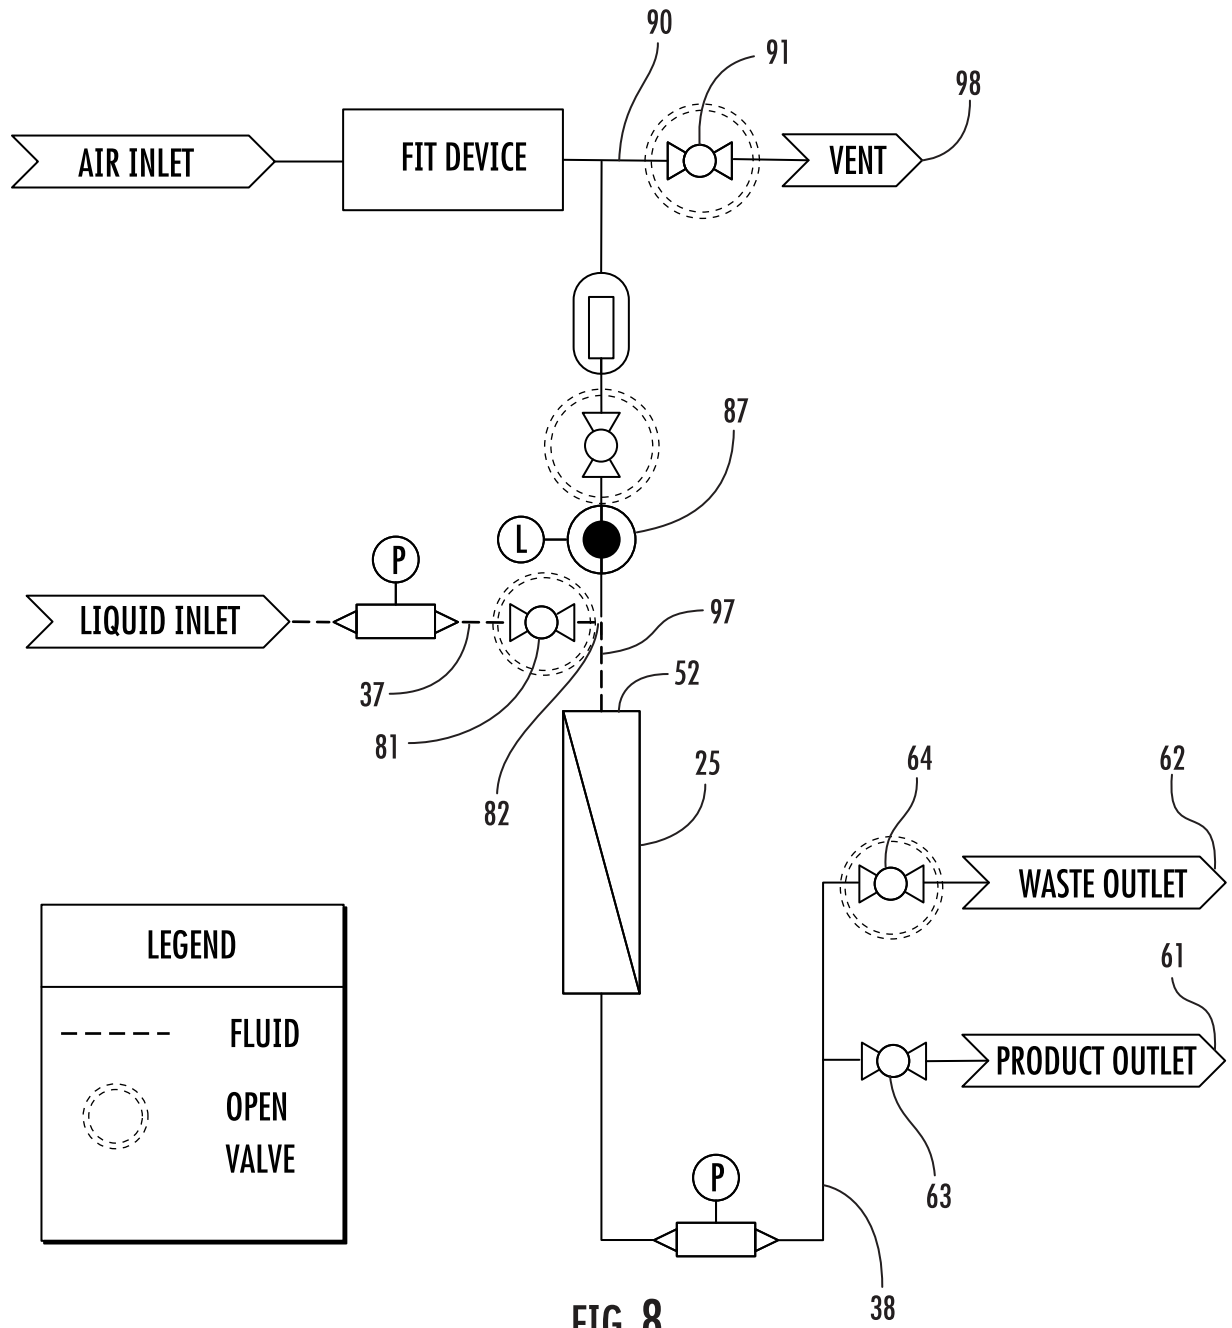

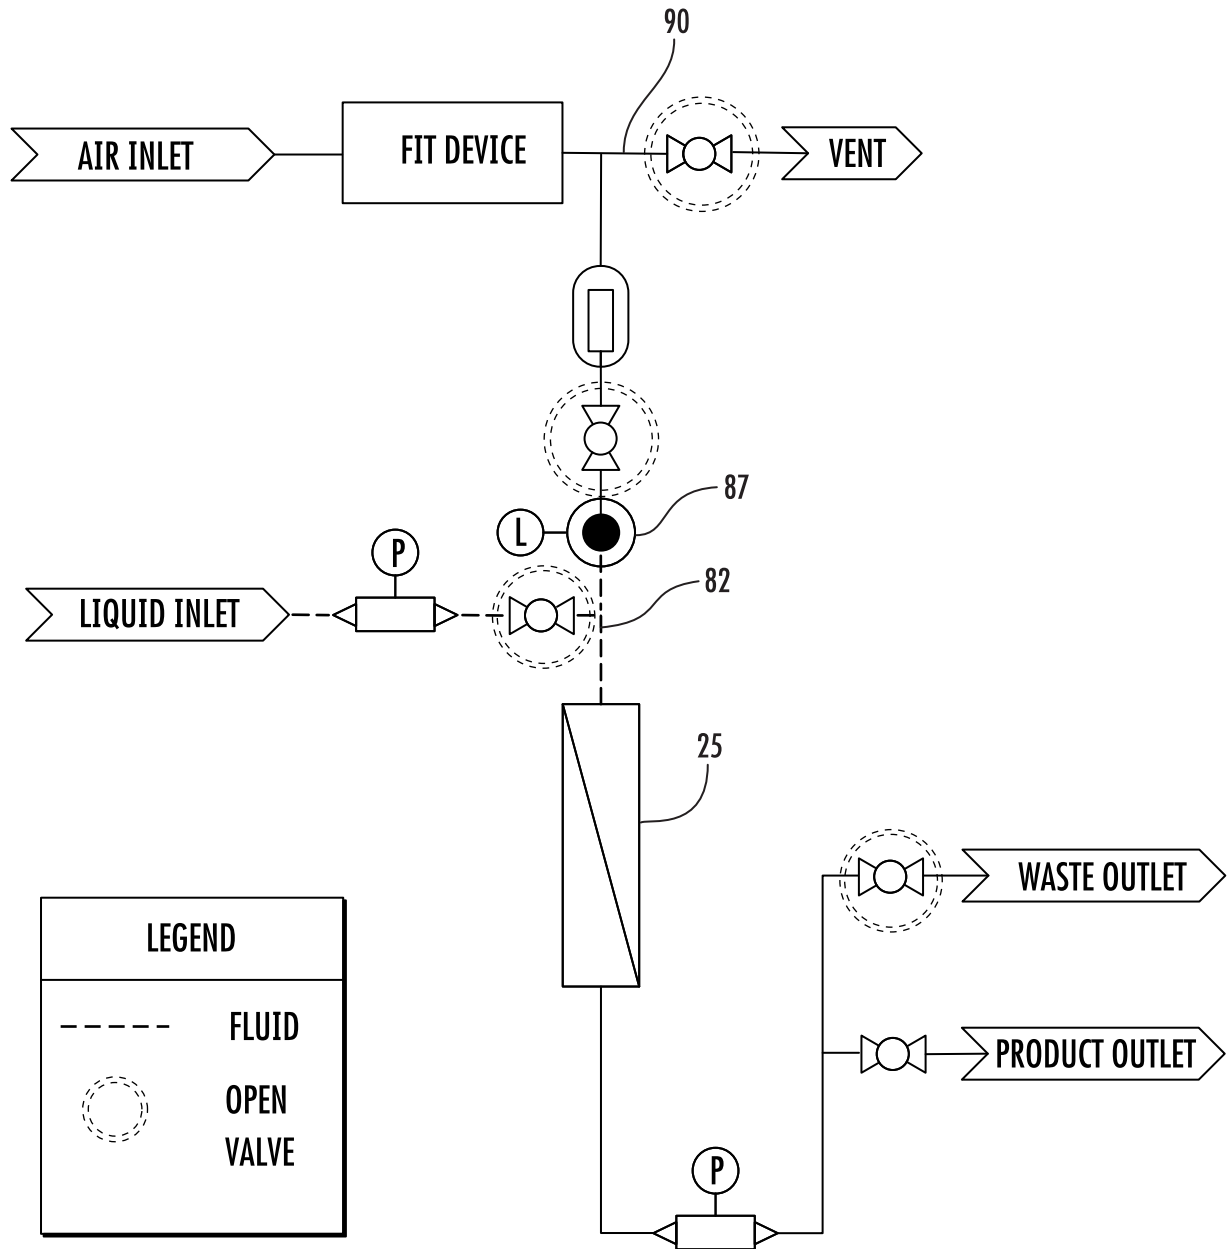
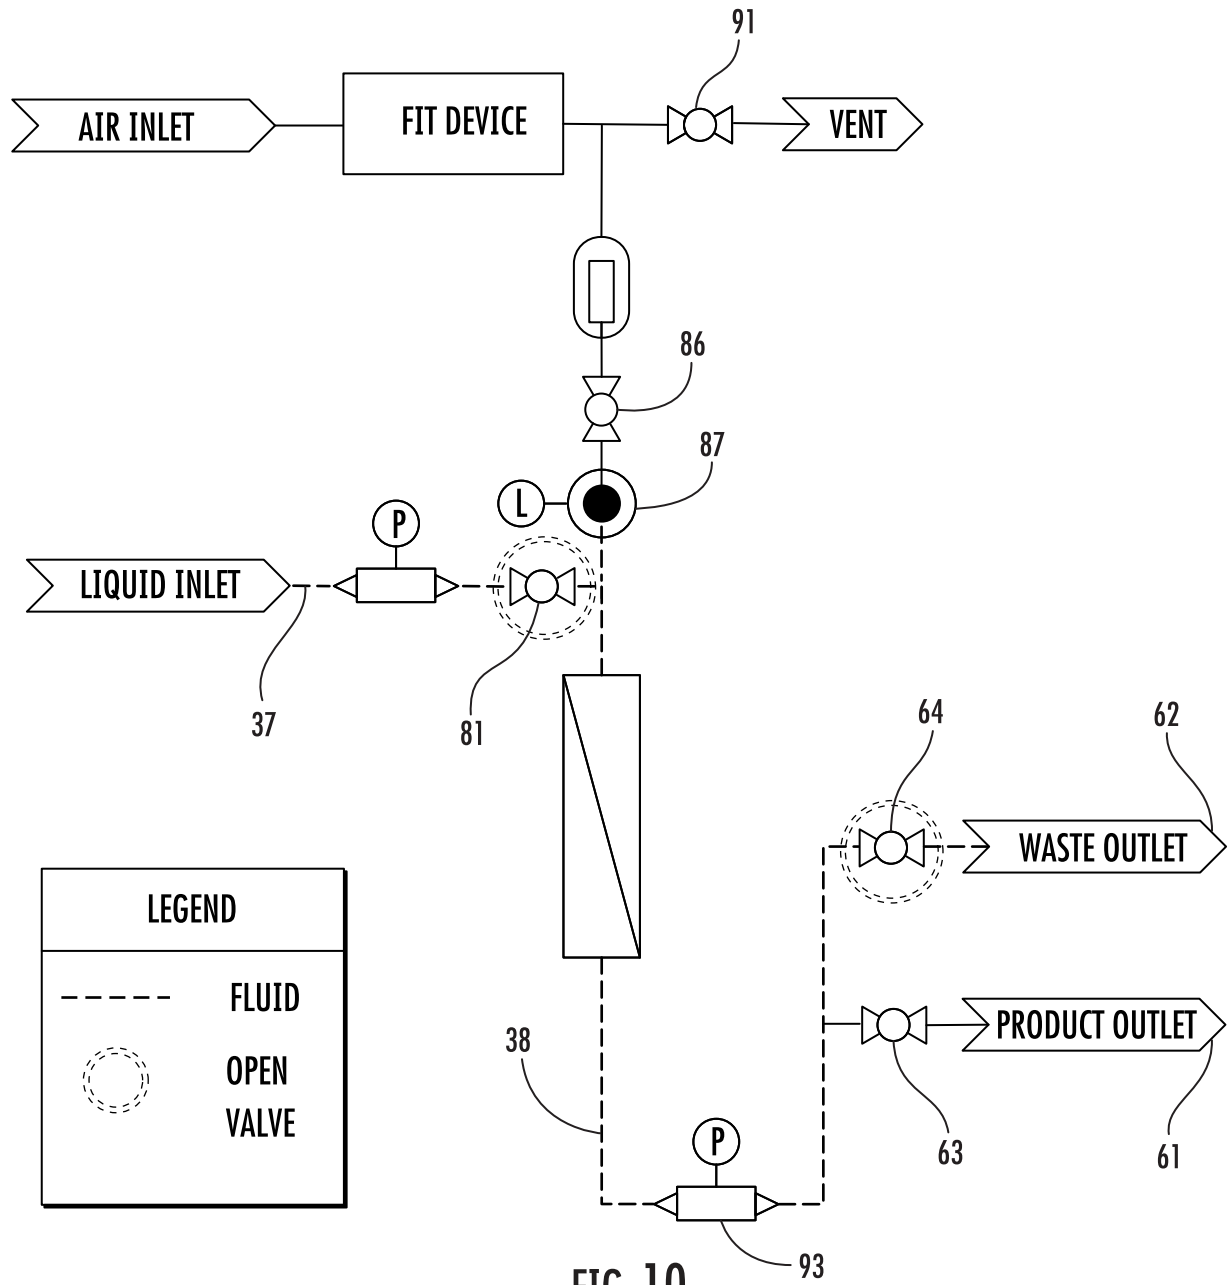
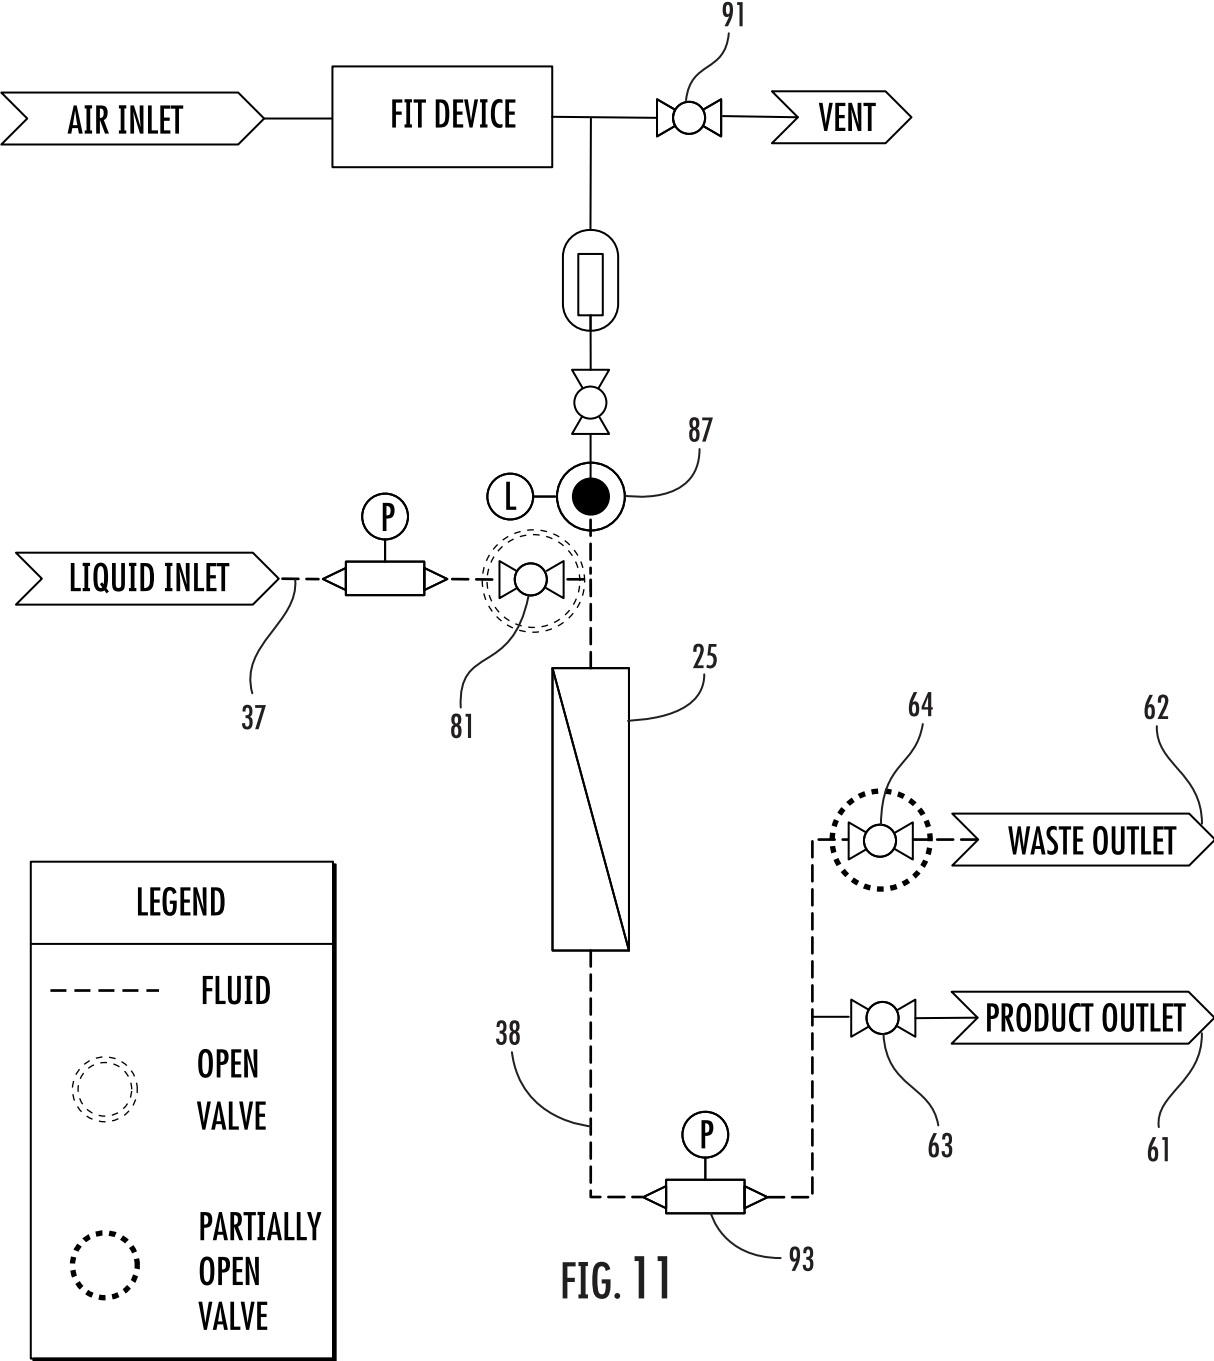


FIG. 9





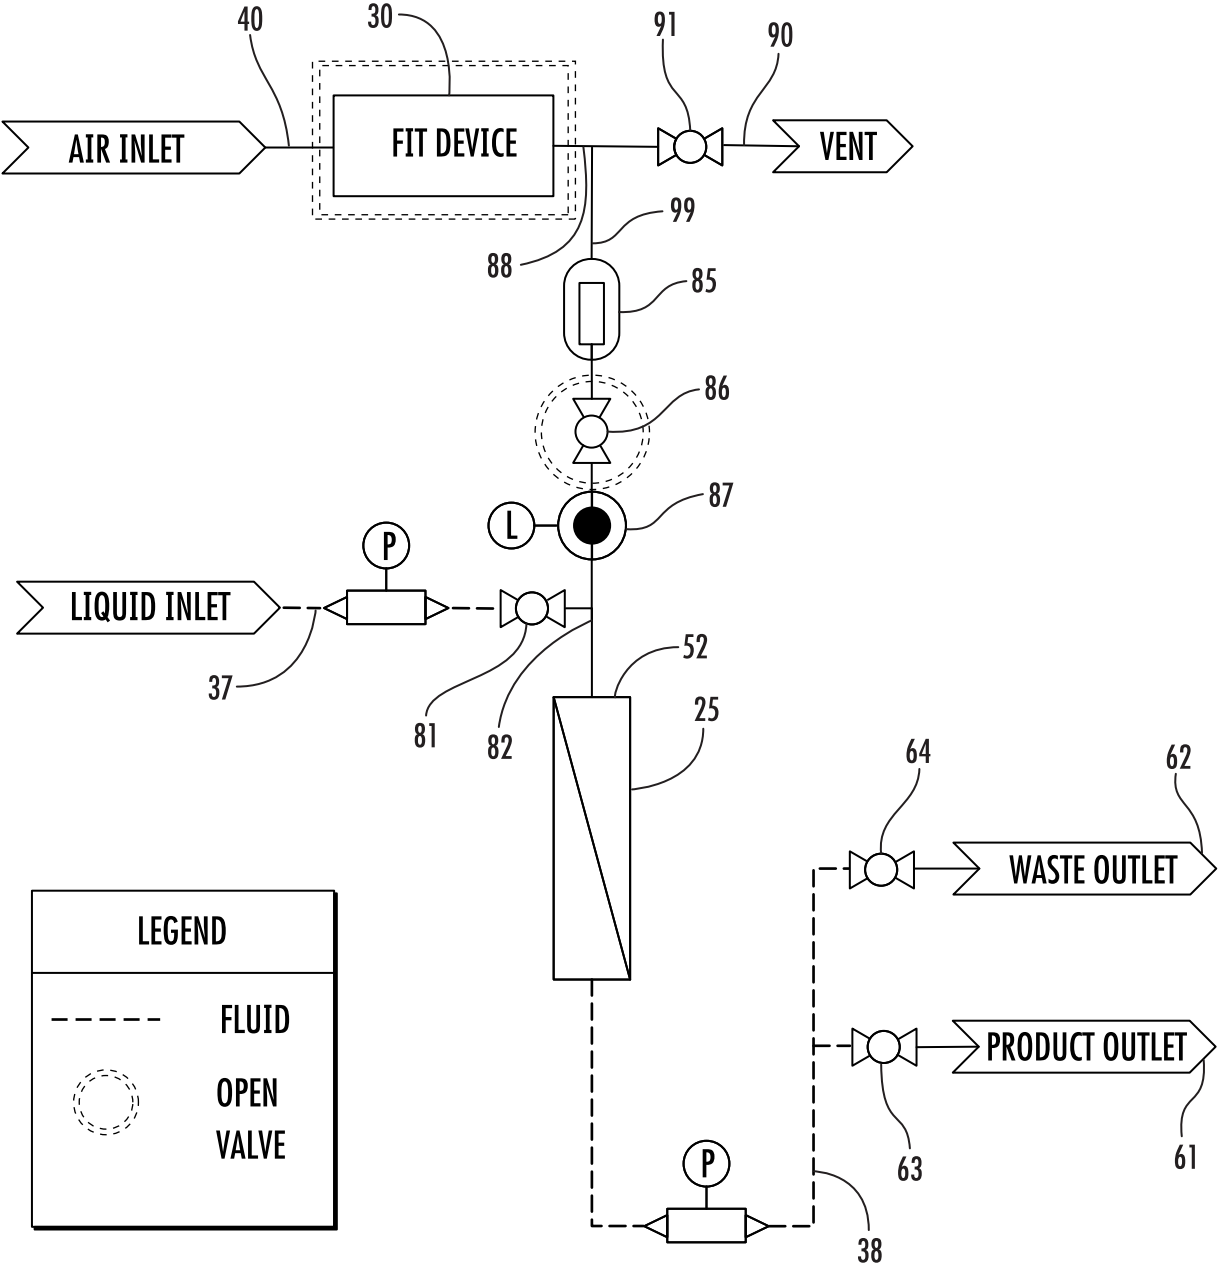


FIG. 12