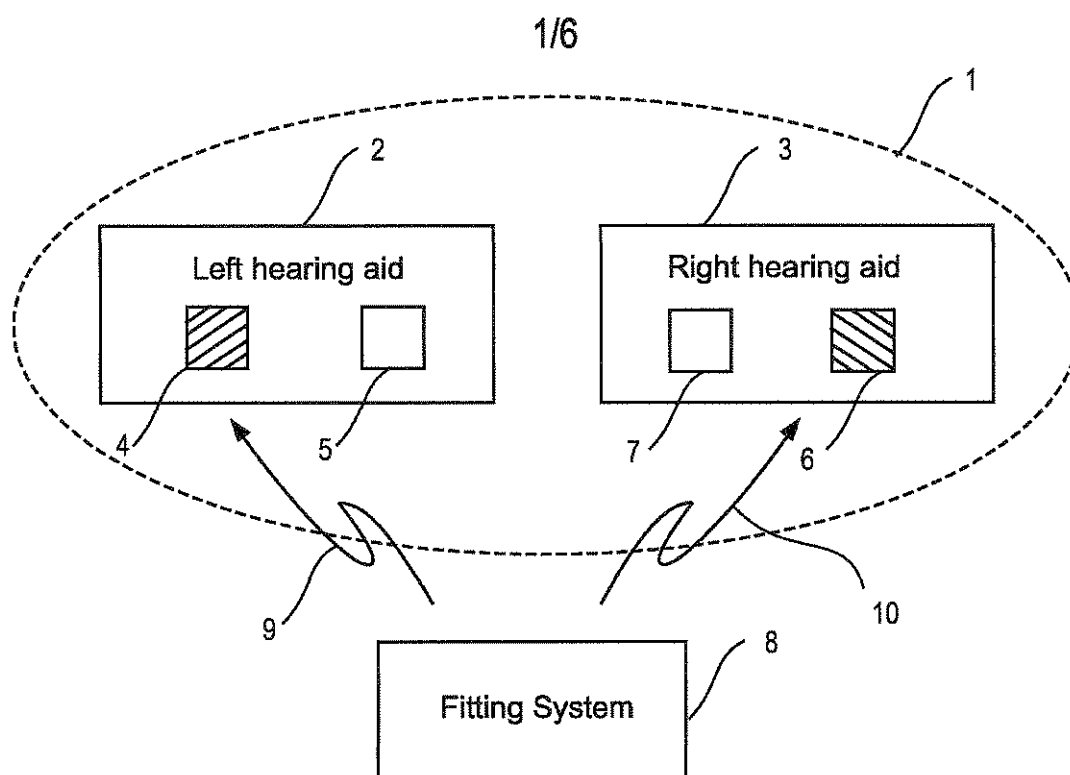
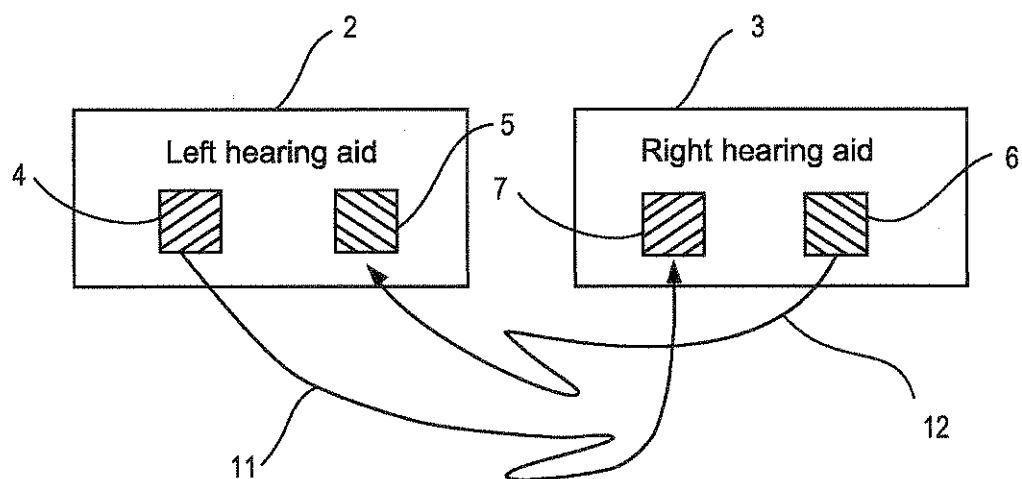
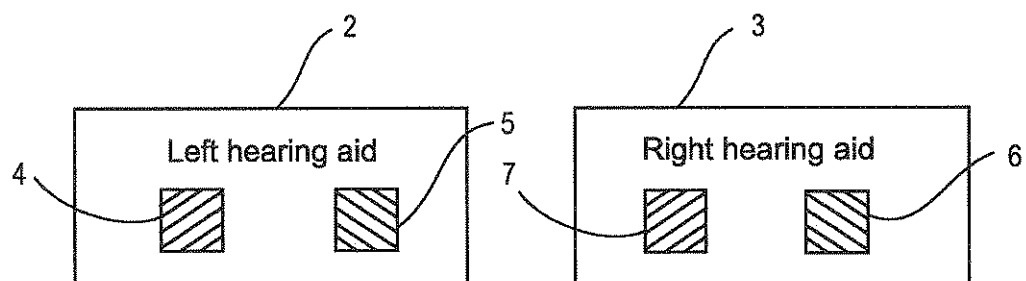
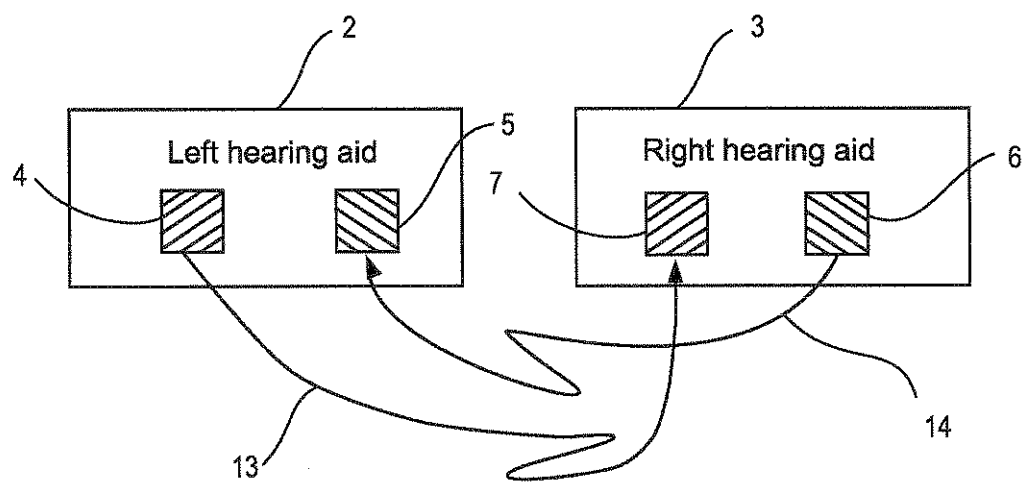
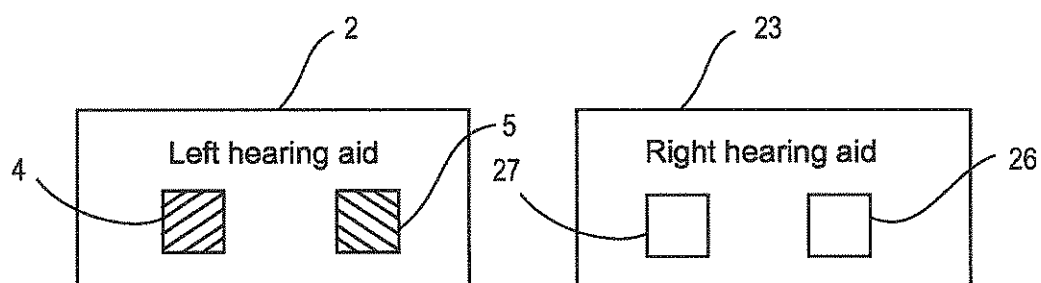
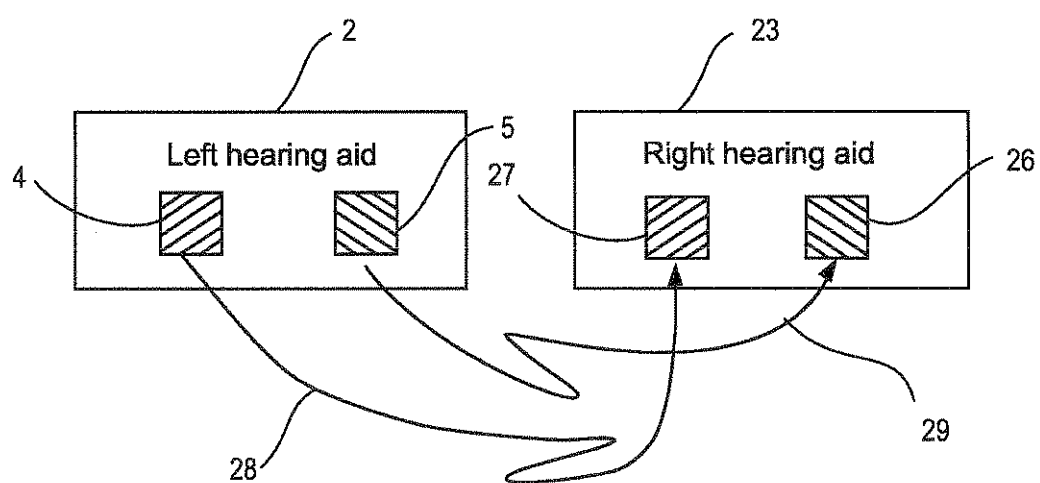



**Fig. 1****Fig. 2**

2/6


**Fig. 3****Fig. 4**

3/6

**Fig. 5****Fig. 6**

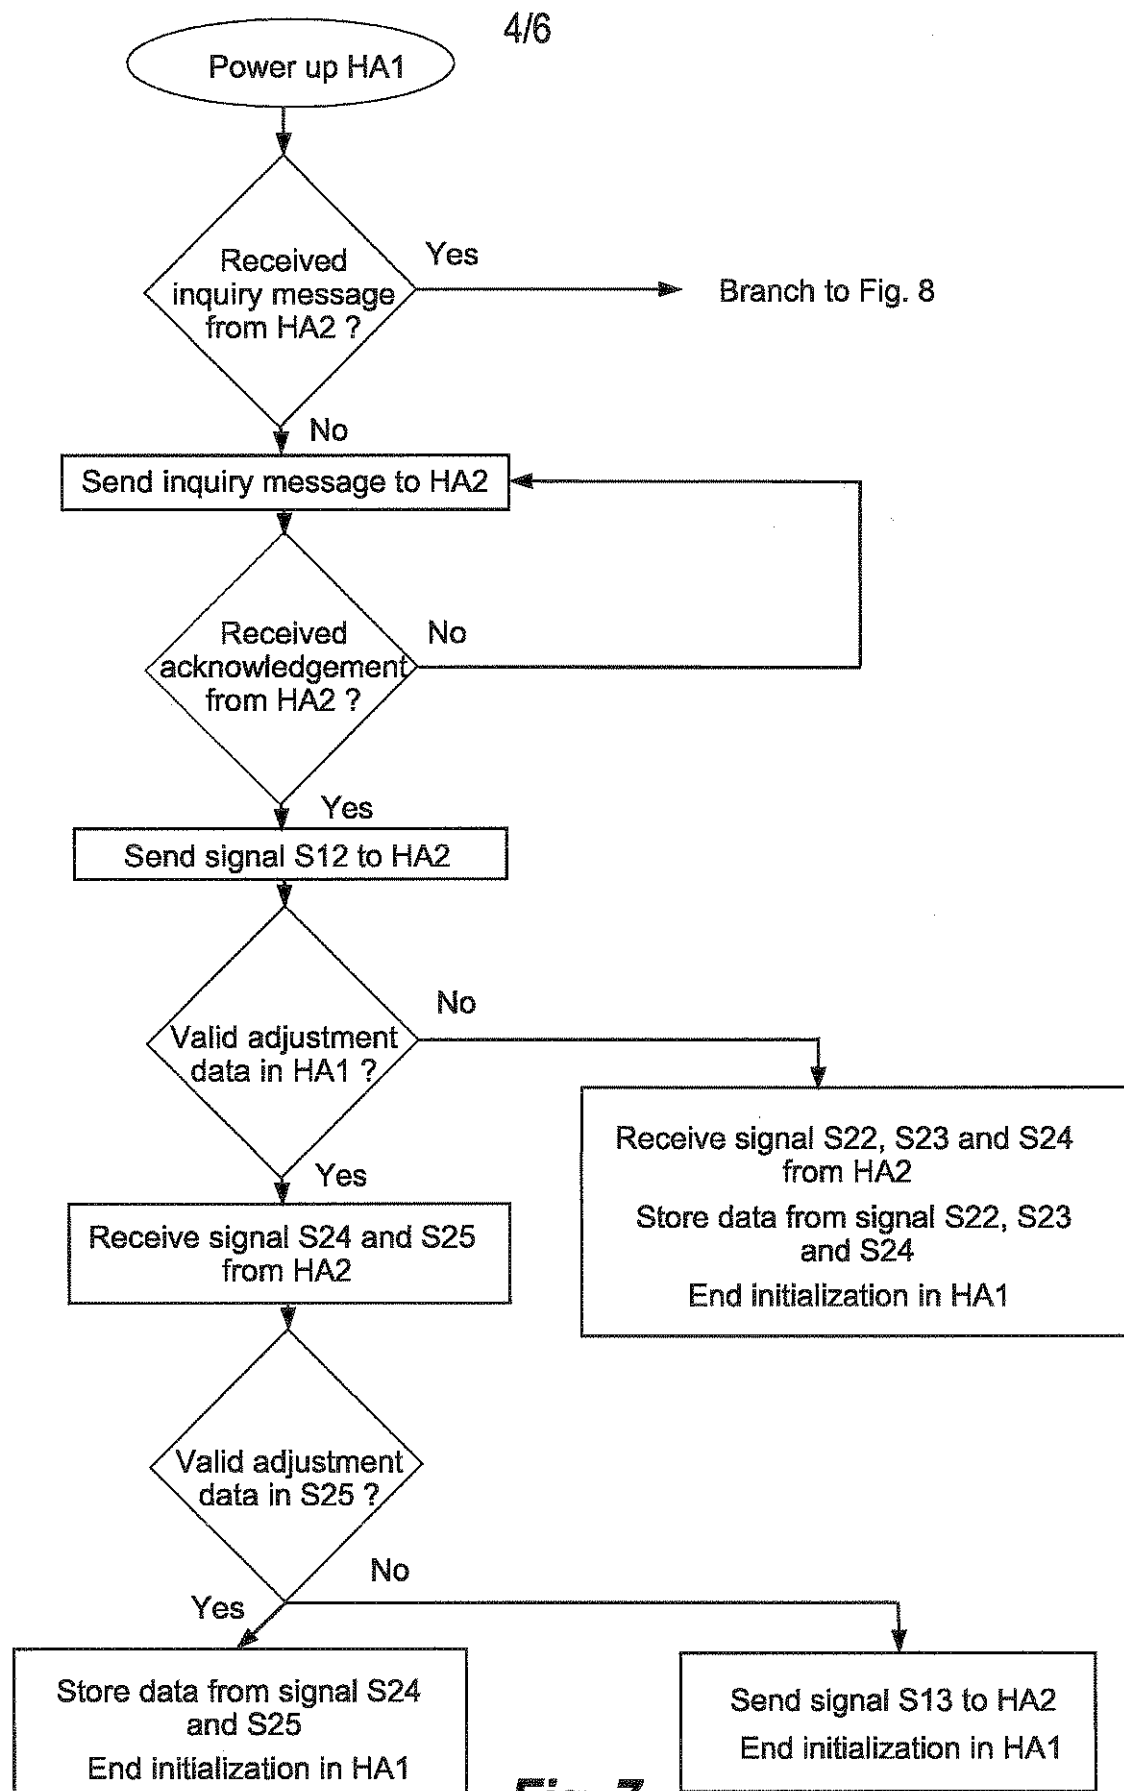**Fig. 7**

5/6

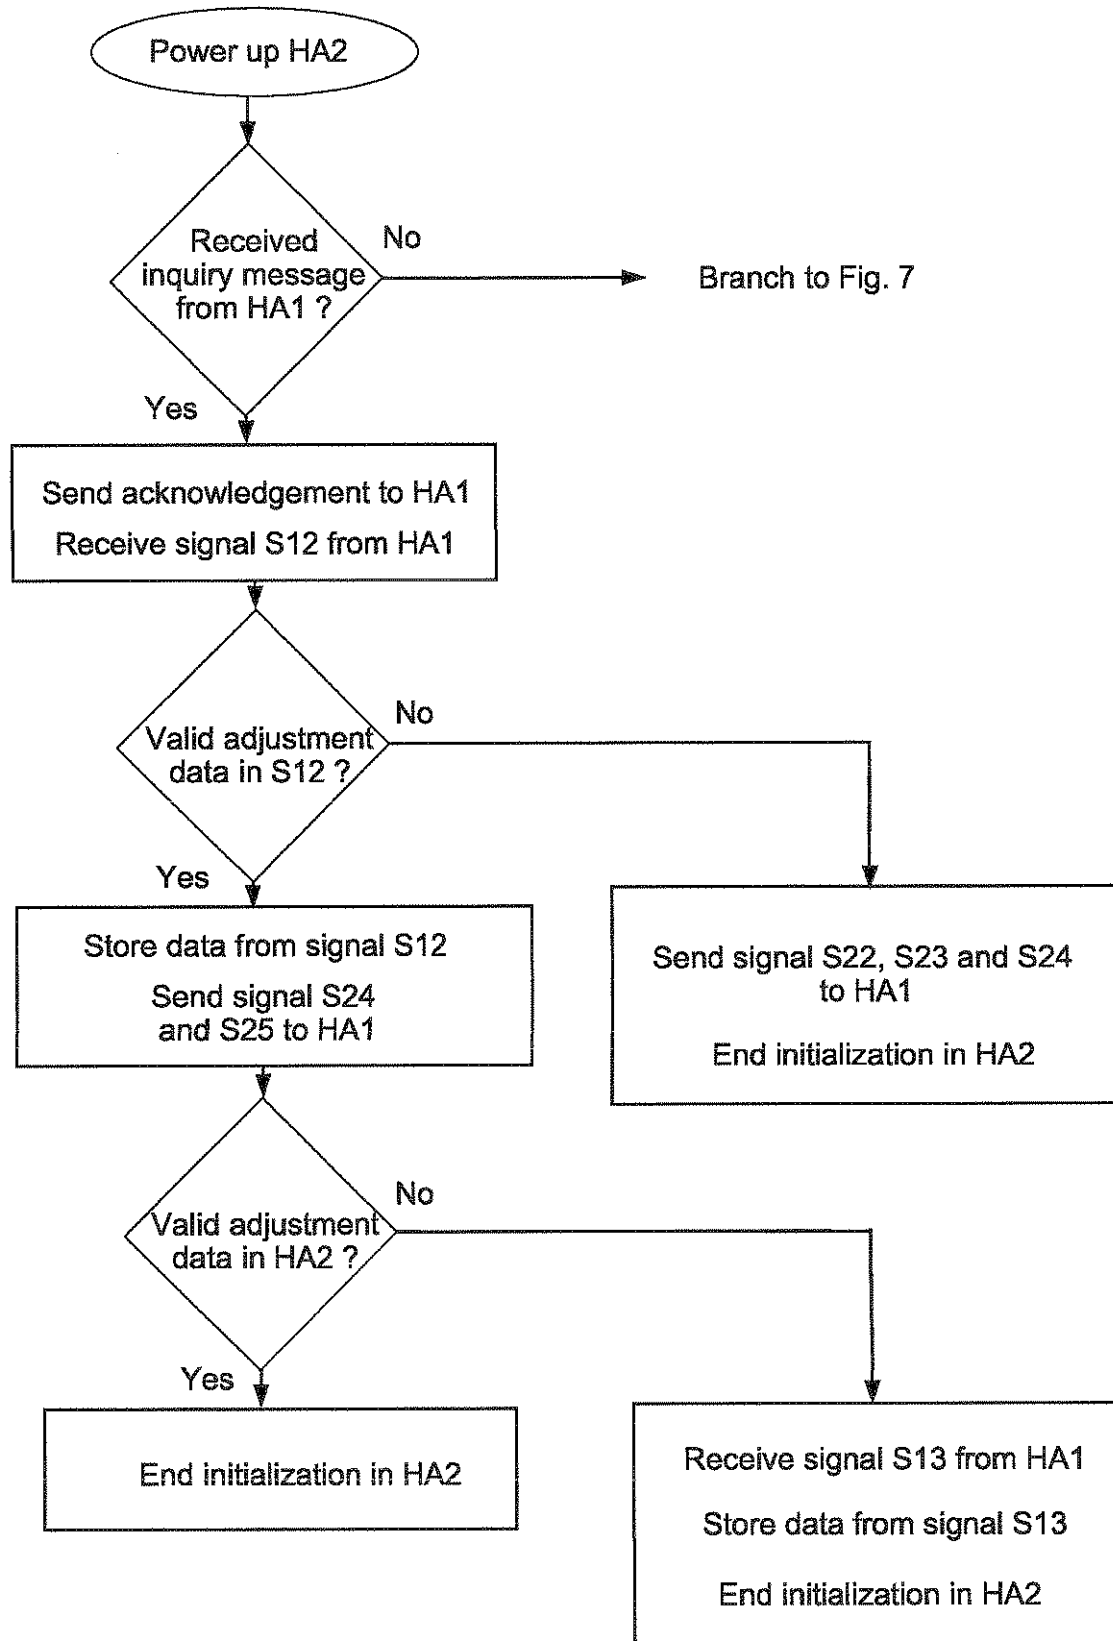**Fig. 8**

6/6

Right Hearing Aid

	Ipse-lateral data only	Ipse- and contra-lateral data	No data
Ipse-lateral data only	Exchange ipse-lateral data, then binaural operation	Exchange ipse-lateral data, then binaural operation	Monaural operation on left hearing aid
Ipse- and contra-lateral data	Exchange ipse-lateral data, then binaural operation	Exchange ipse-lateral data, then binaural operation	Transmit ipse- and contra-lateral data, then binaural operation
No data	Monaural operation on right hearing aid	Transmit ipse- and contra-lateral data, then binaural operation	No operation

Left Hearing Aid

Fig. 9