


1/12

FIG. 1

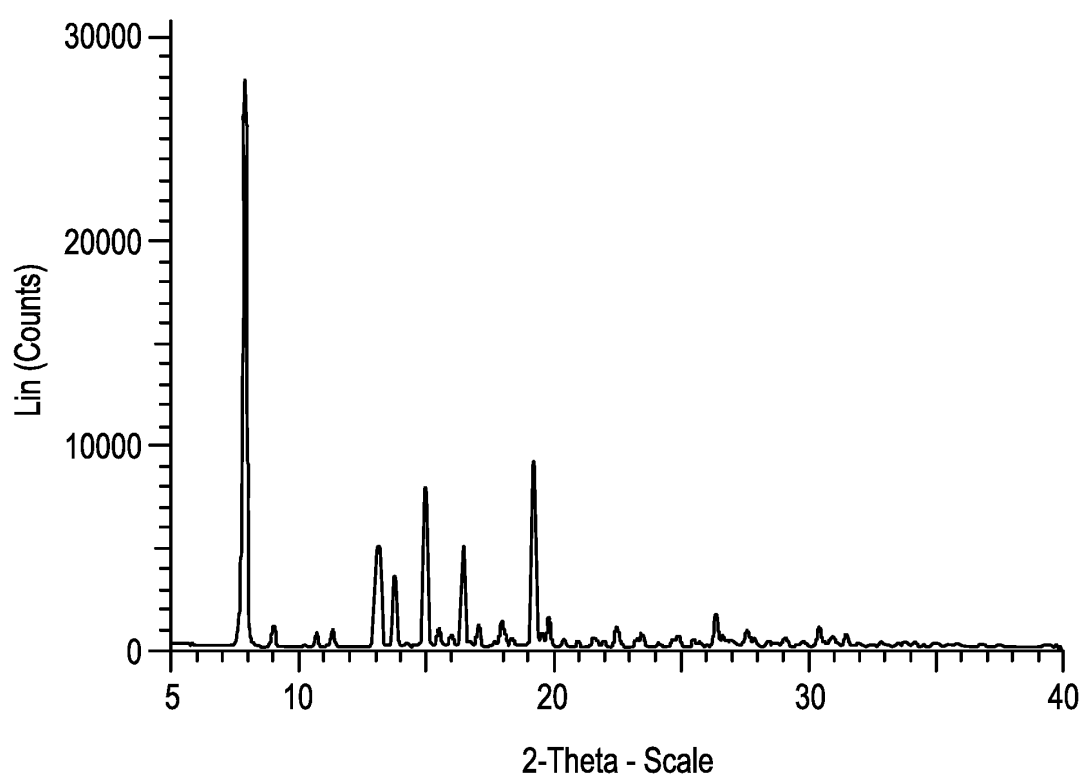

2/12

FIG. 2

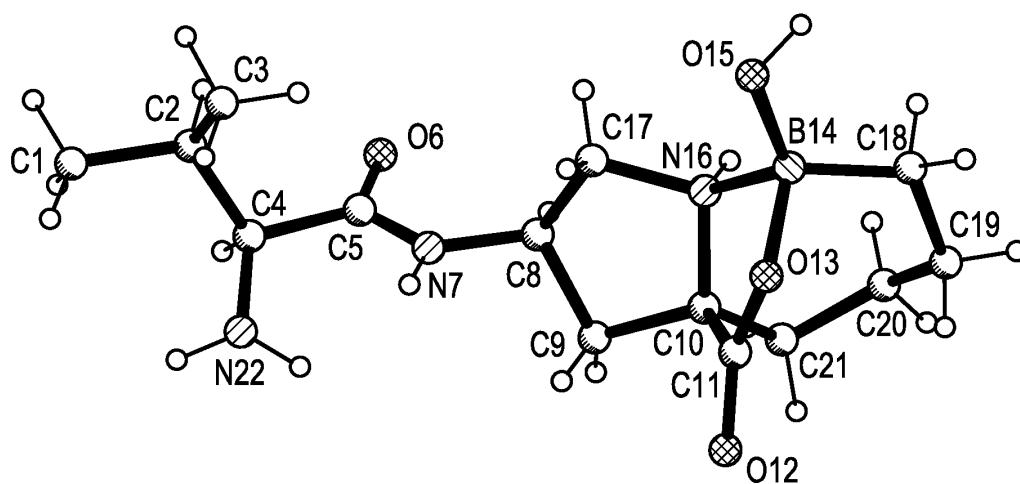


FIG. 3


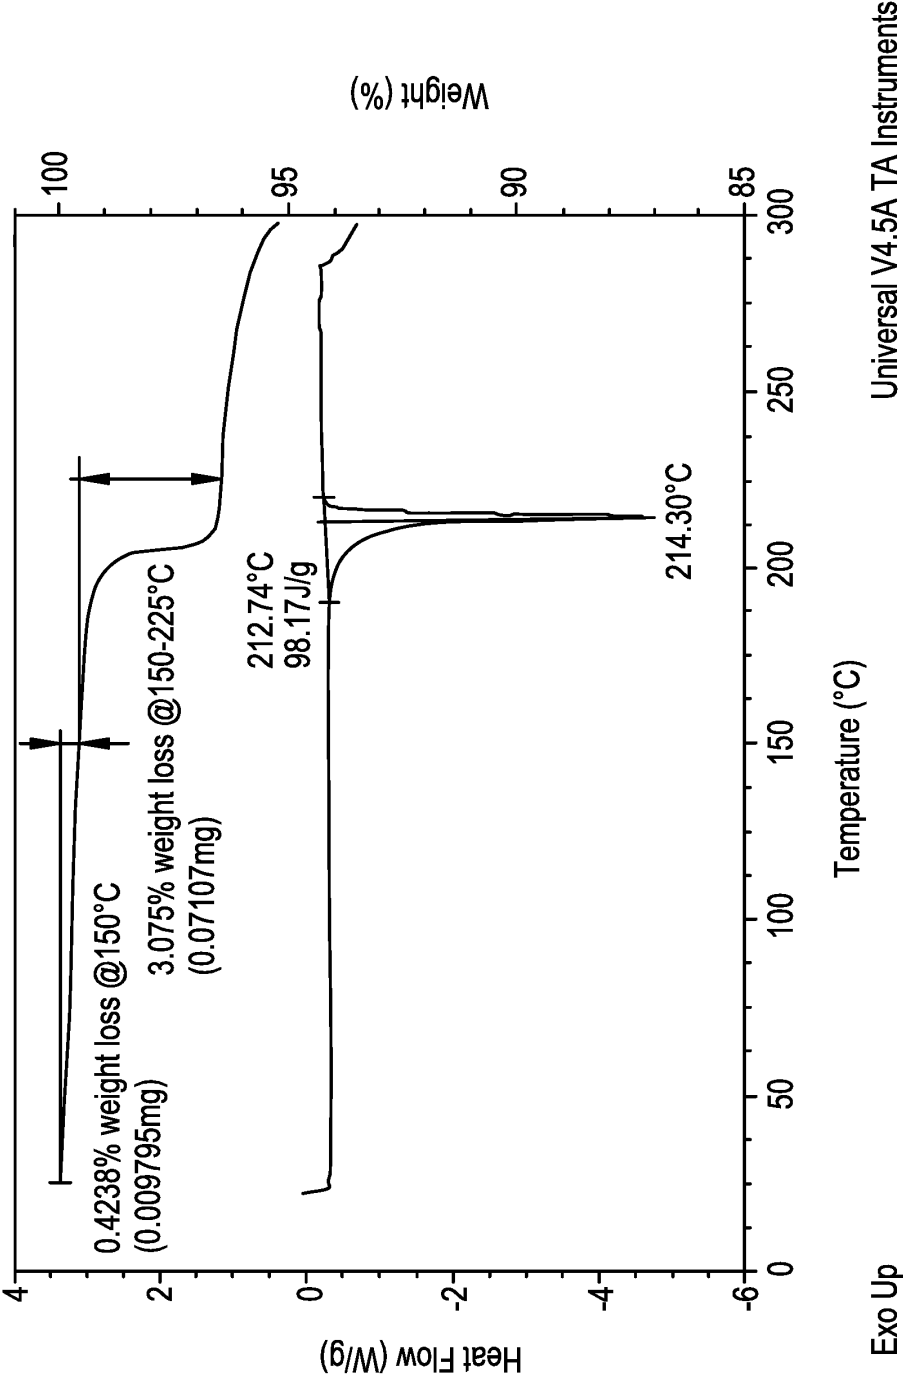



FIG. 4

Sorption Isotherm

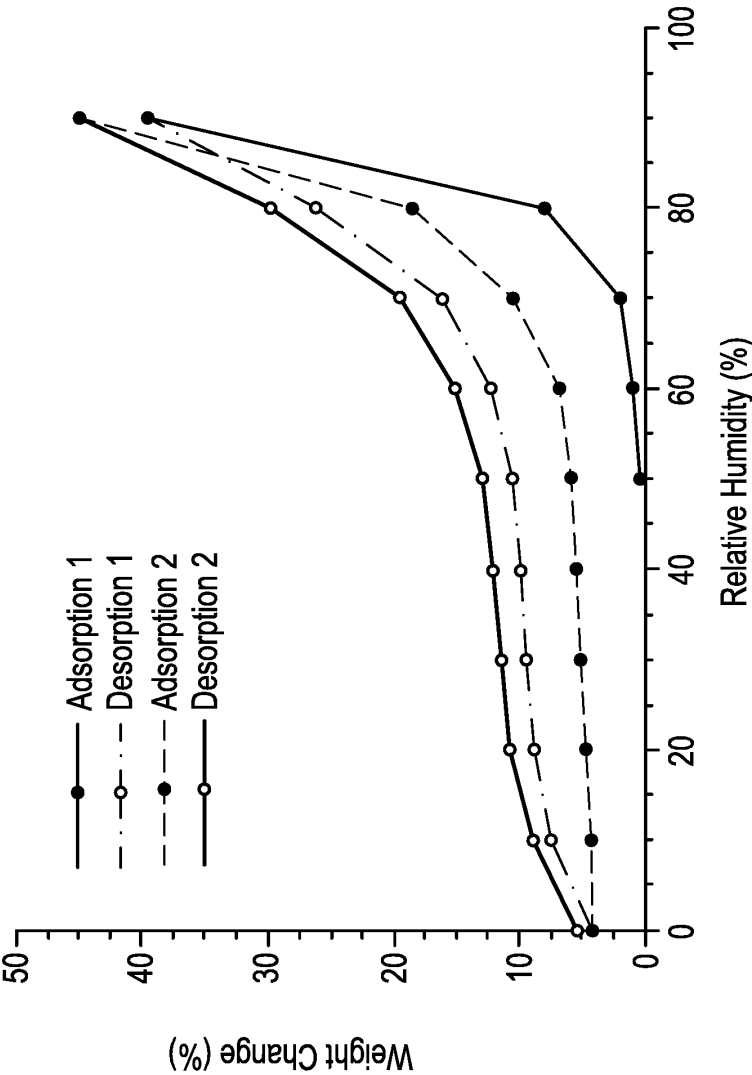

5/12

FIG. 5

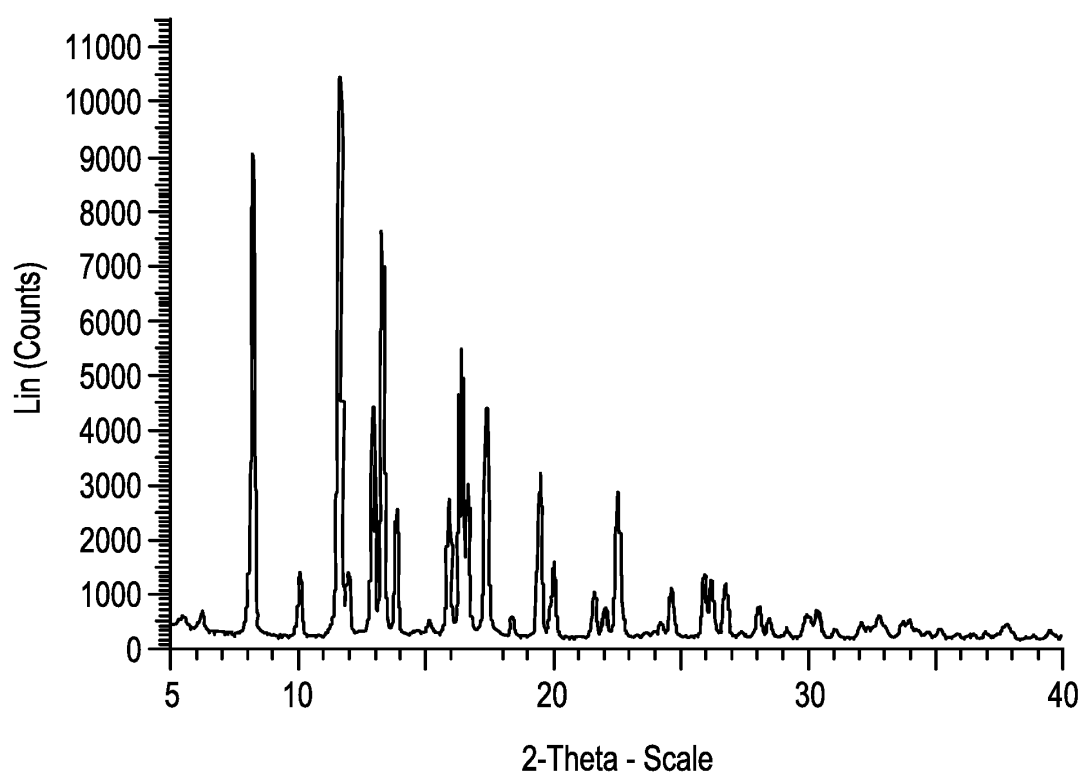

6/12

FIG. 6

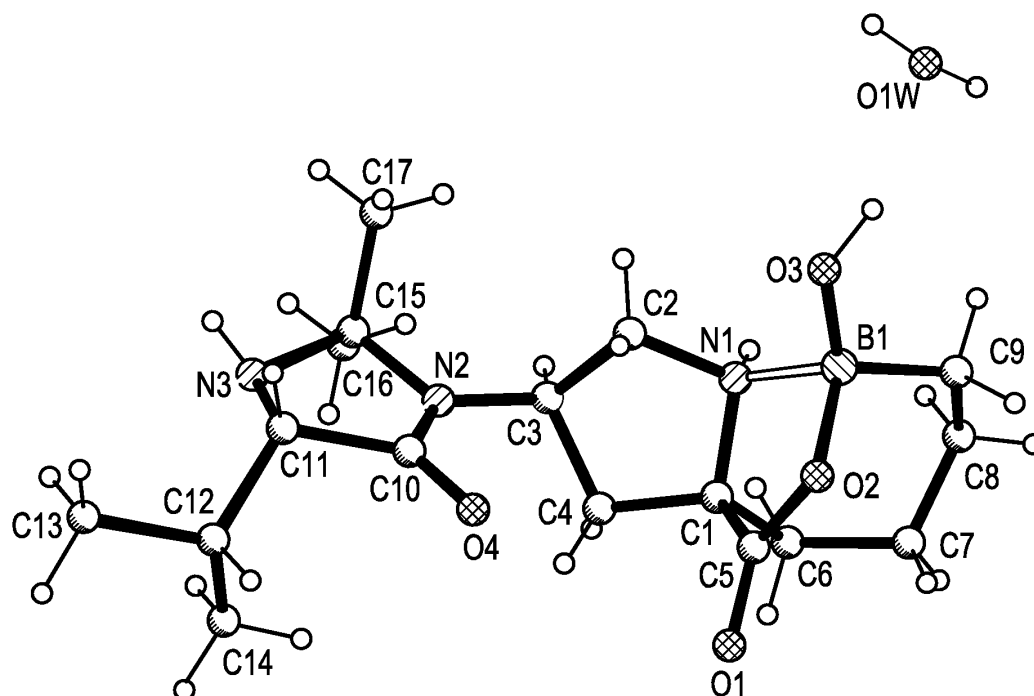


FIG. 7


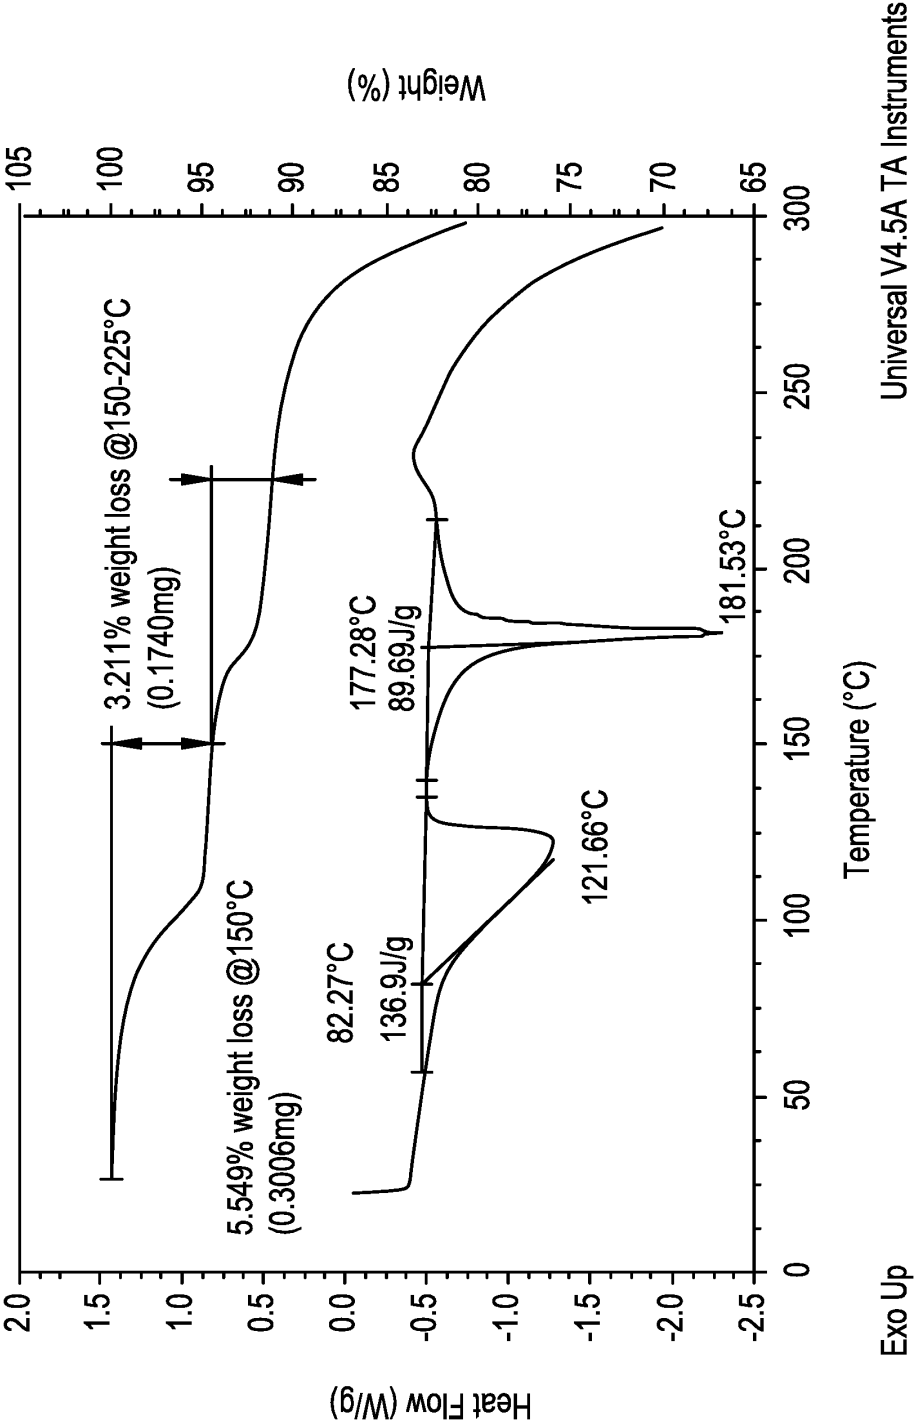



FIG. 8
Sorption Isotherm

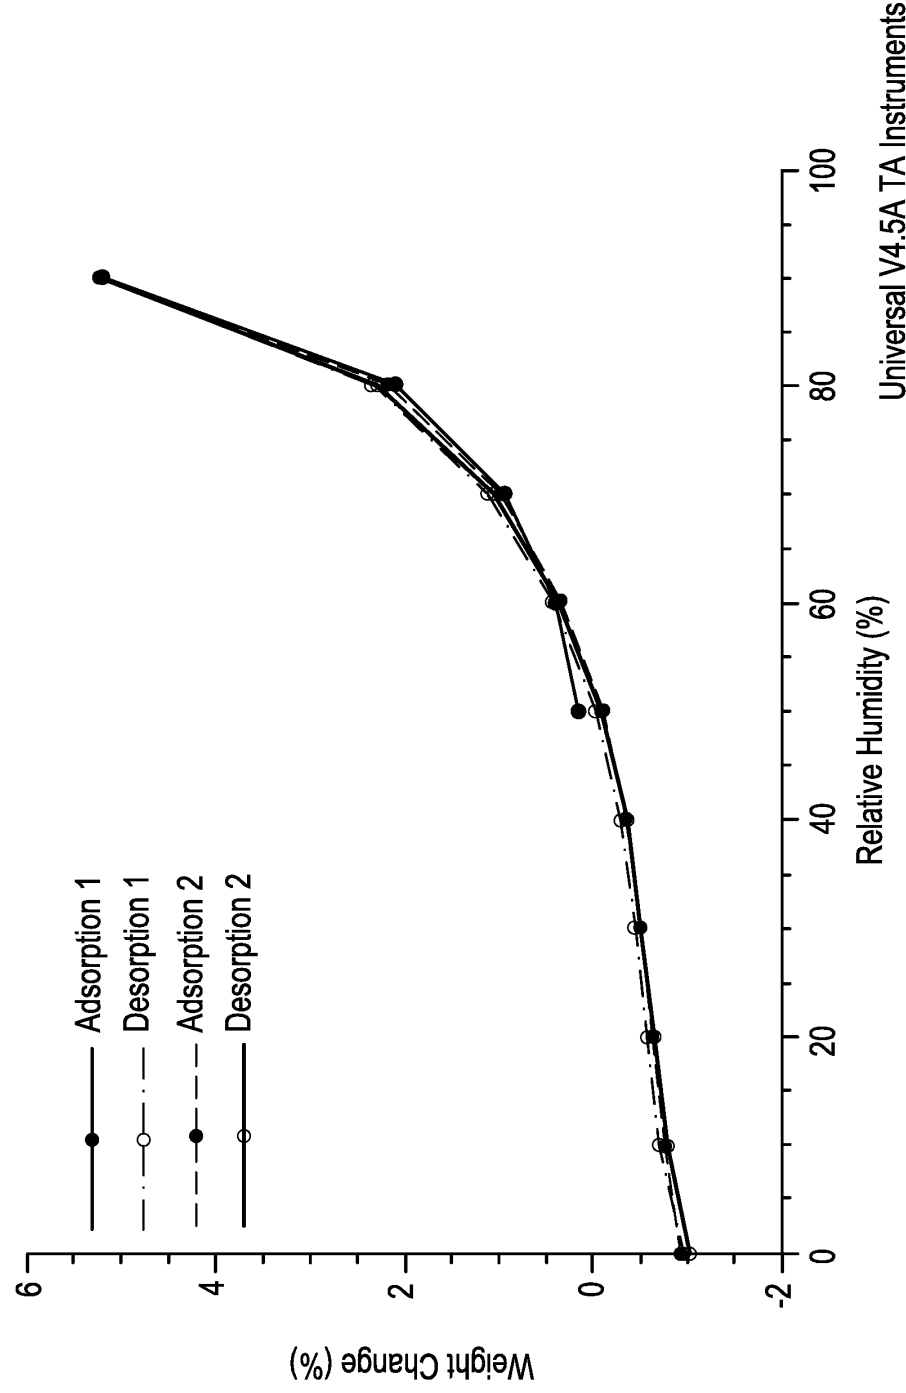

Universal V4.5A TA Instruments

9/12

FIG. 9

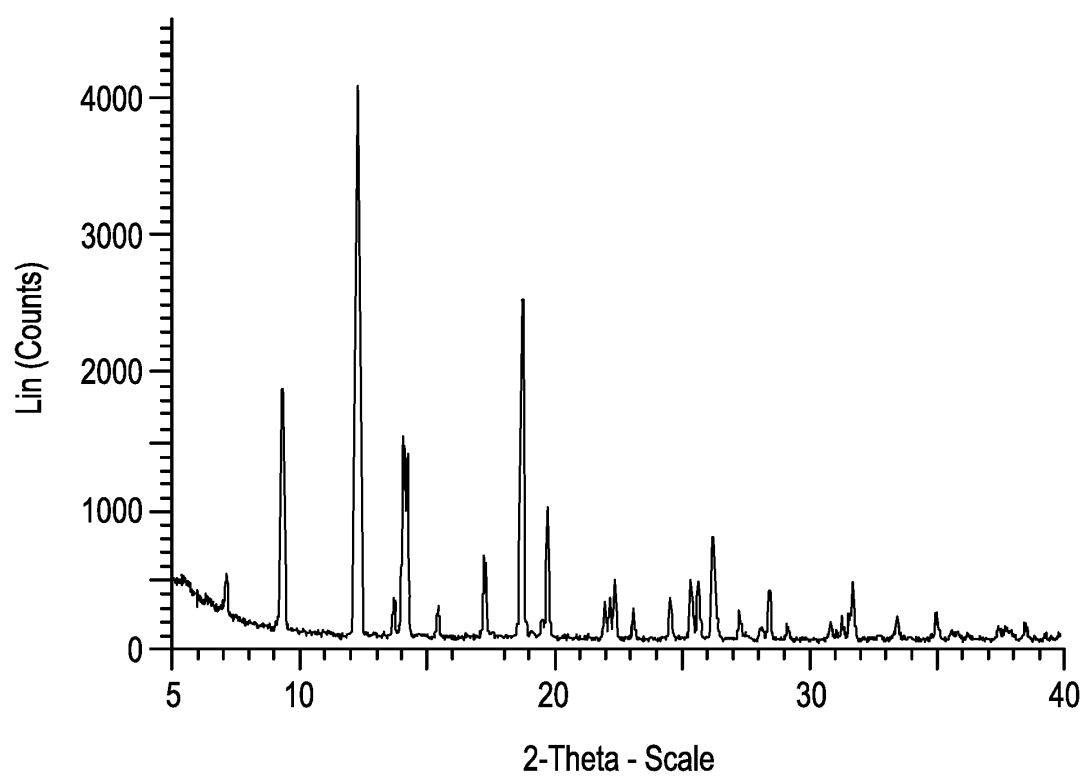

10/12

FIG. 10

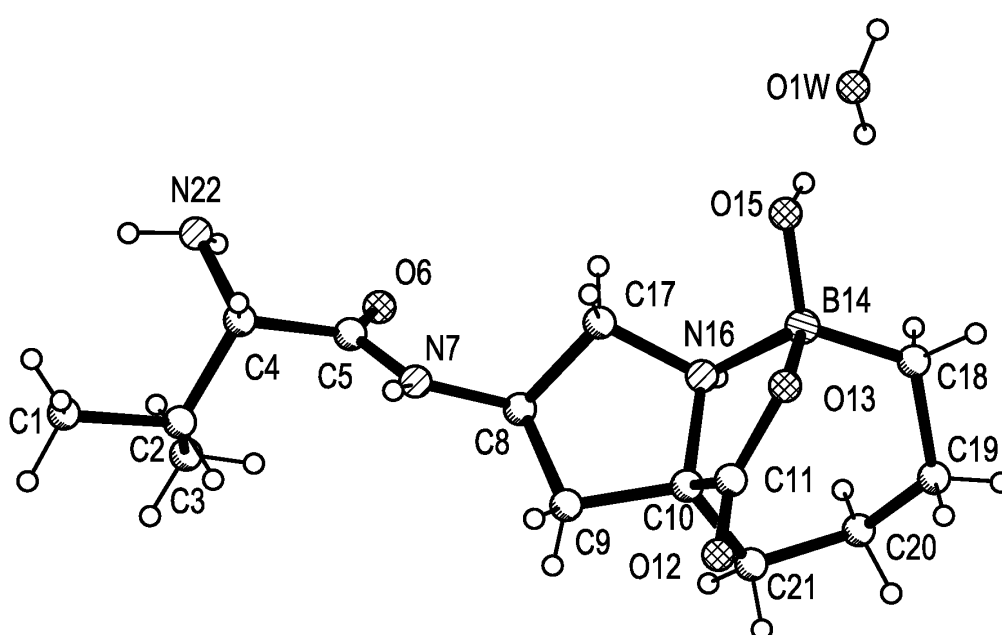


FIG. 11

