

FIG. 1

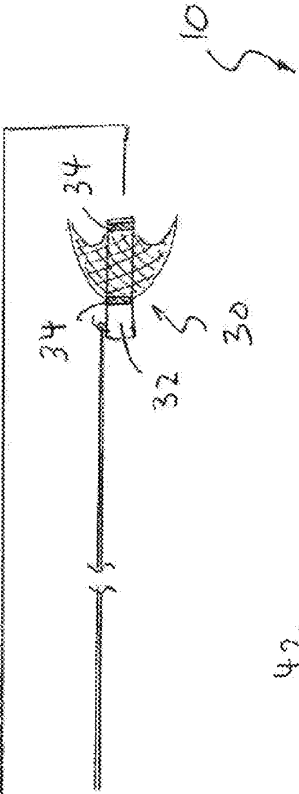


FIG. 2

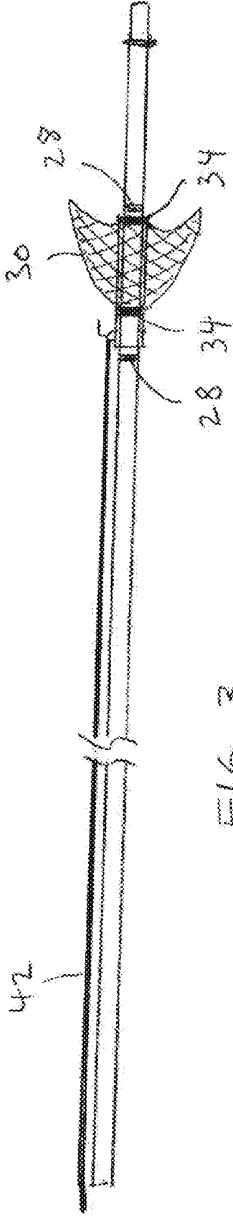
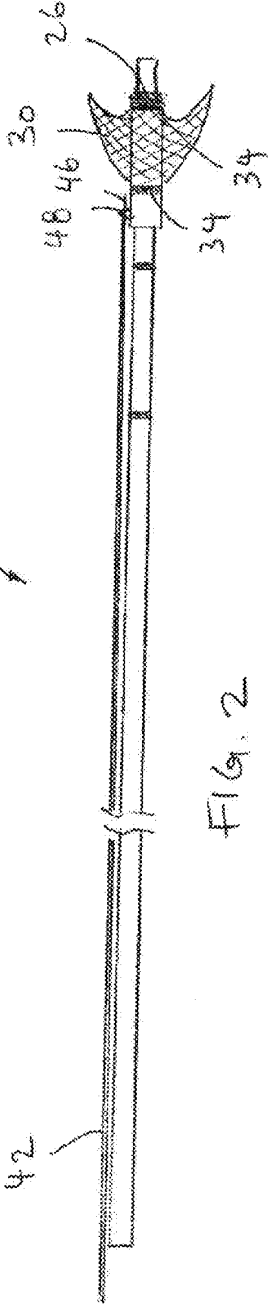


FIG. 3

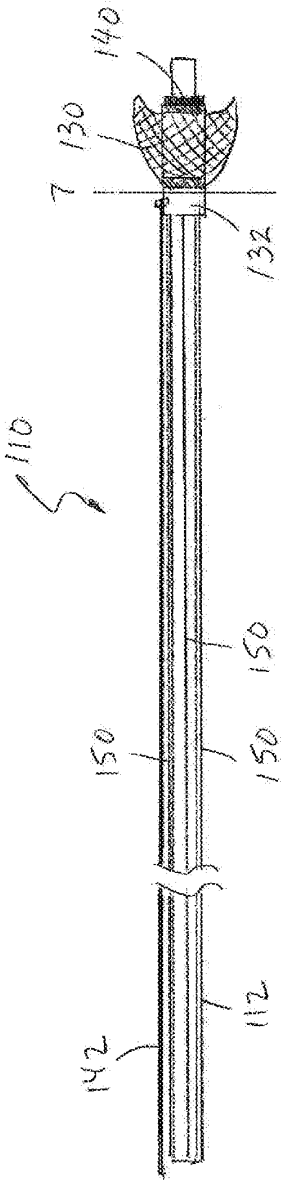


FIG. 4

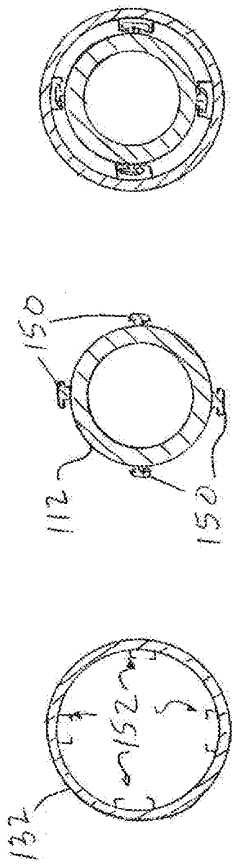


FIG. 5

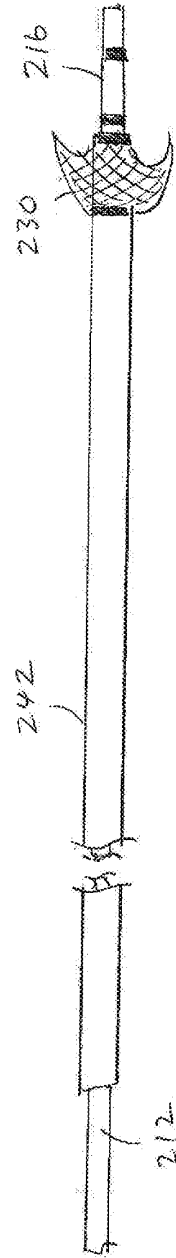
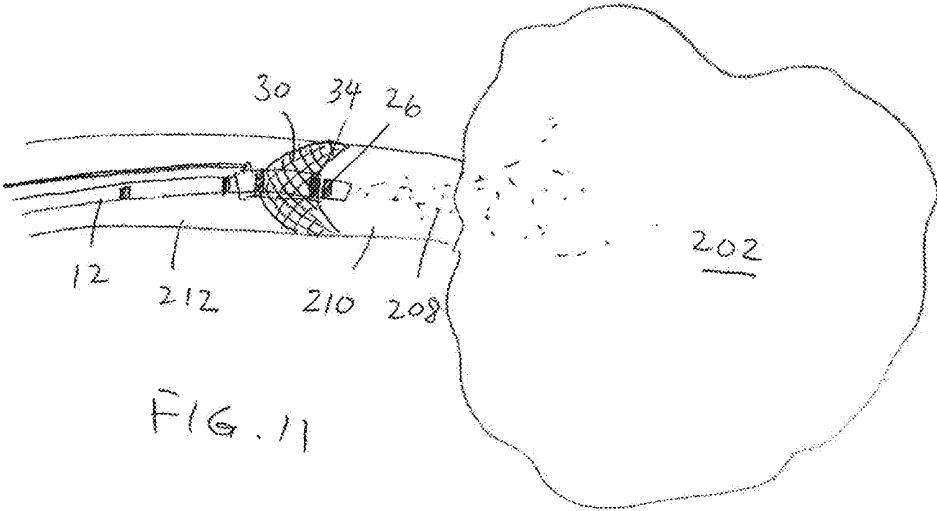
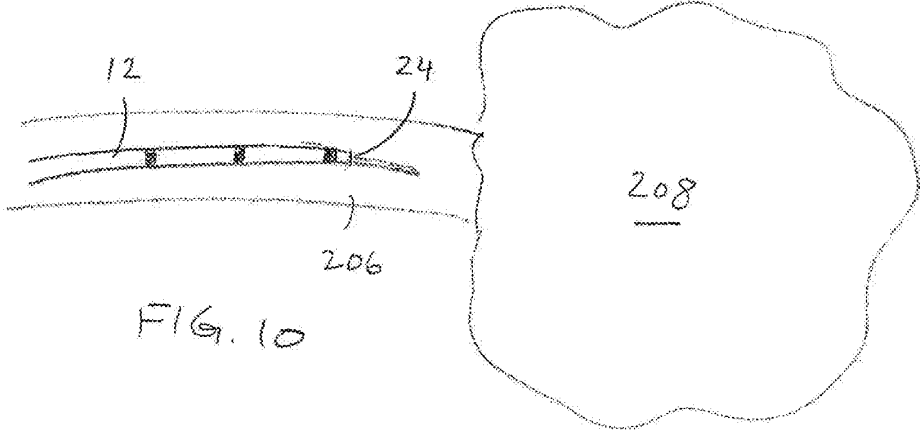
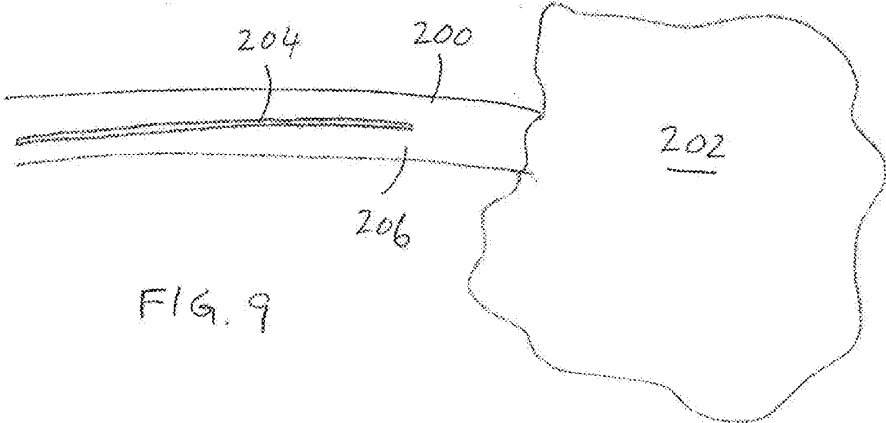


FIG. 6



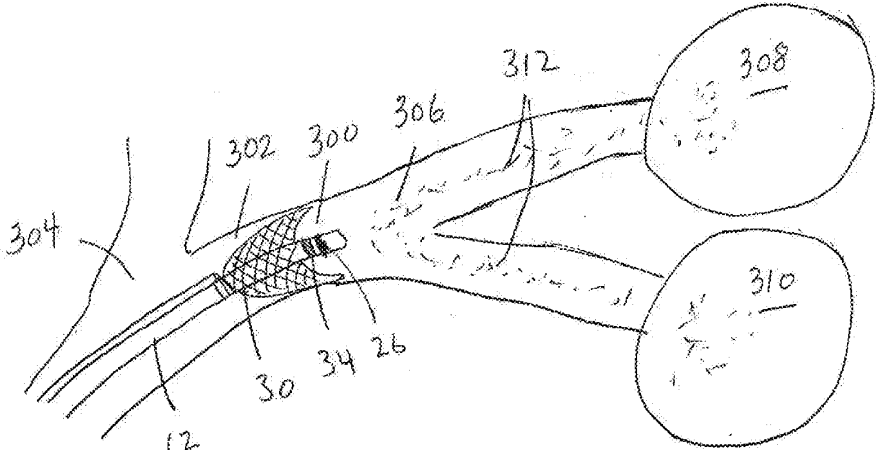


FIG. 12

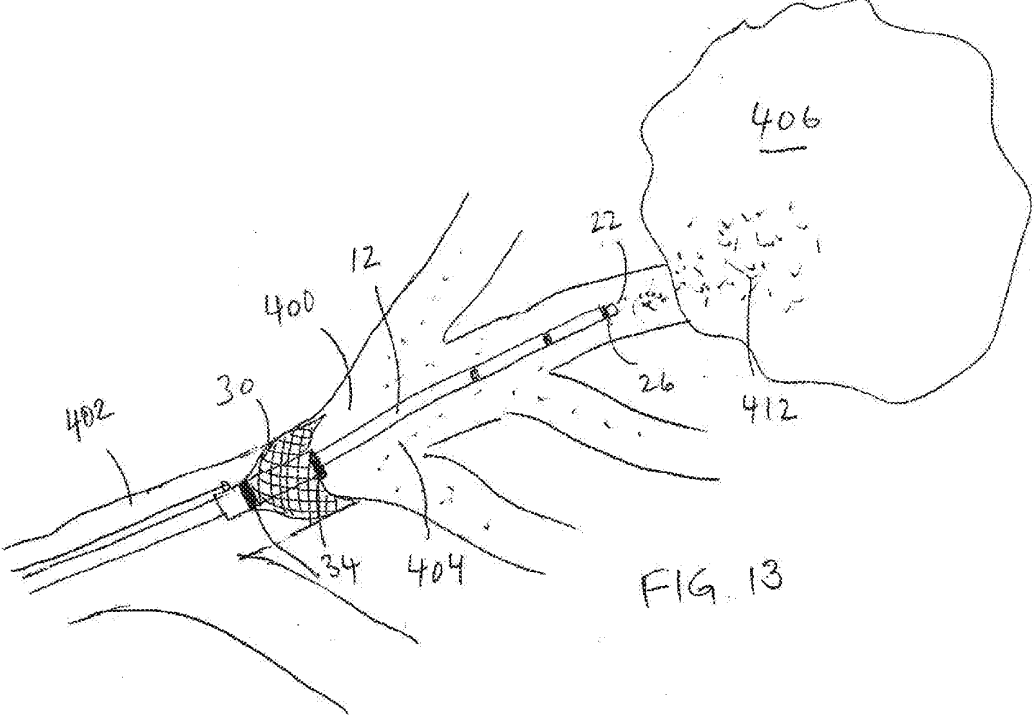
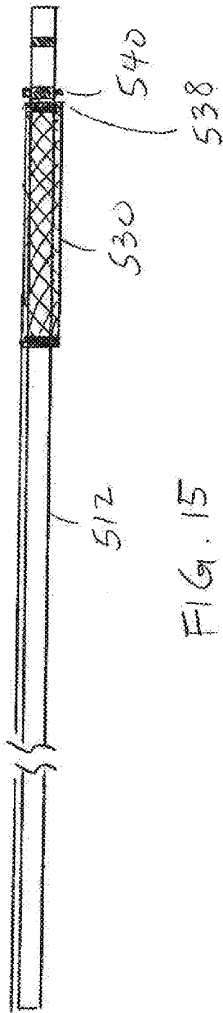
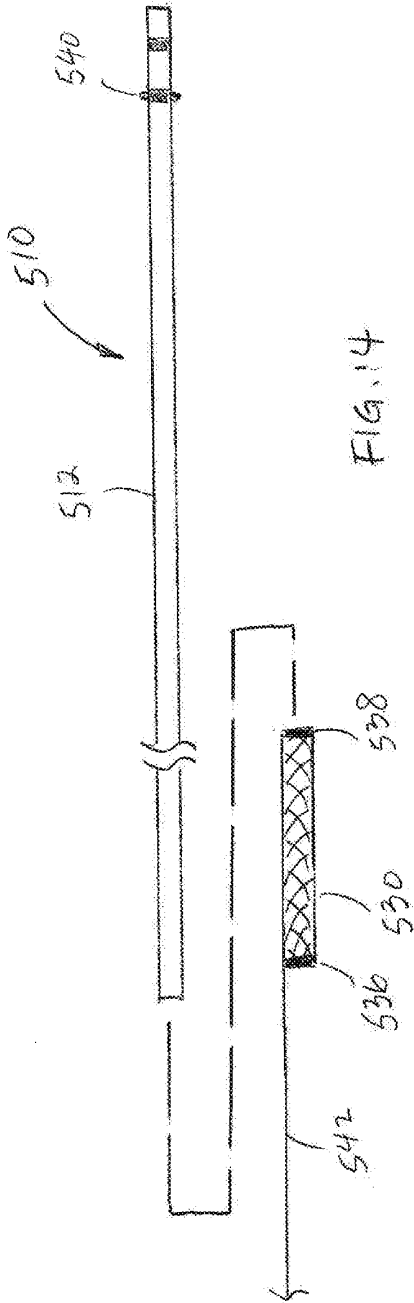


FIG. 13



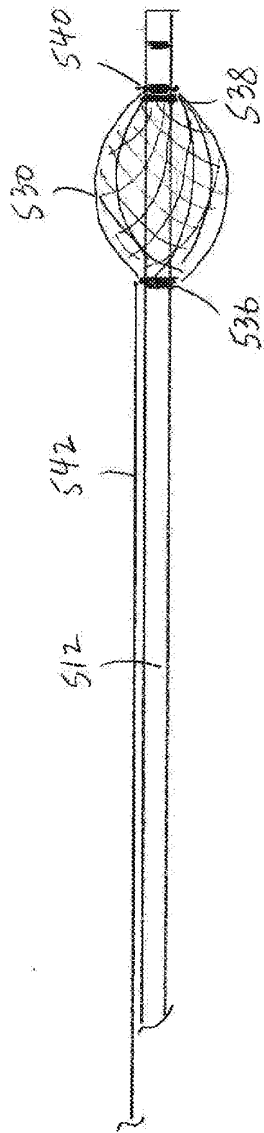


FIG. 16

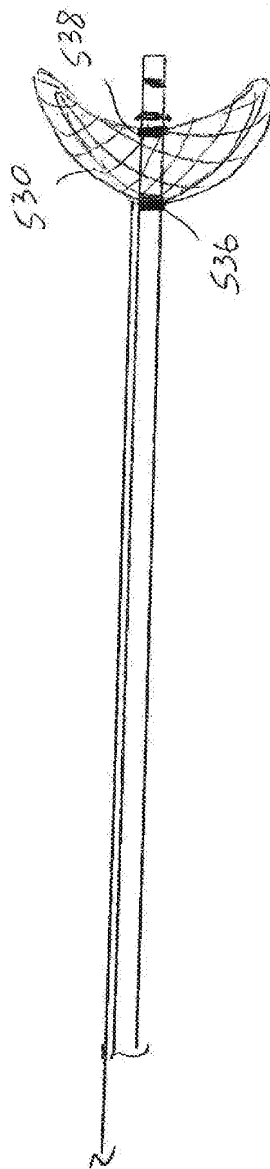


FIG. 17

7/28

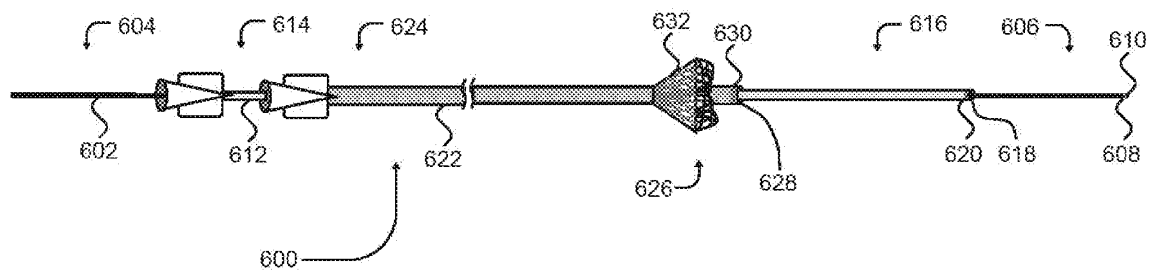


Fig. 18

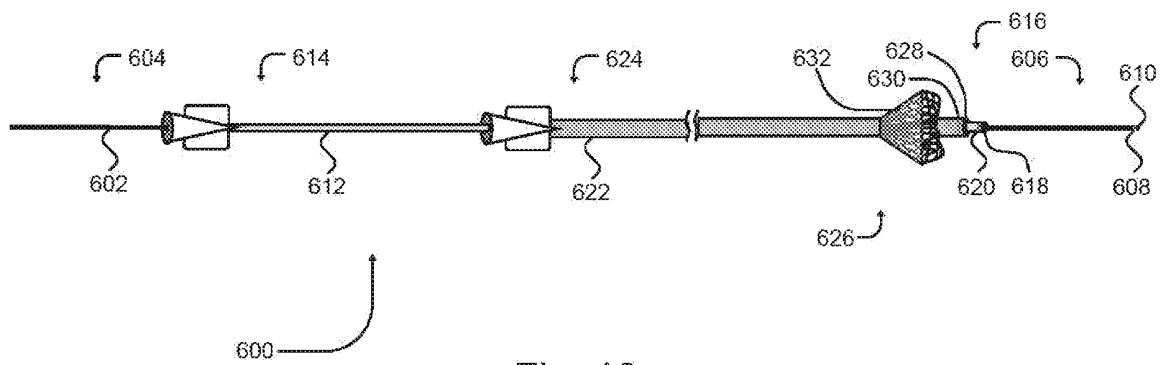


Fig. 19

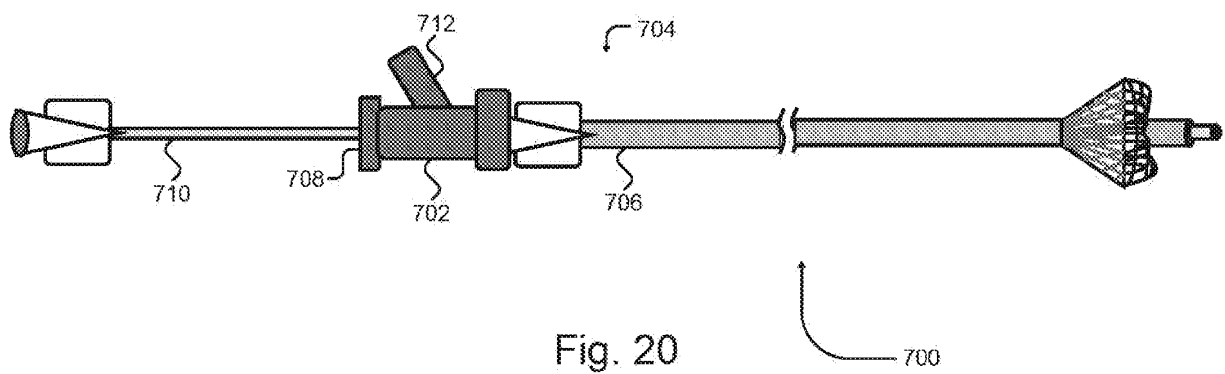


Fig. 20

8/28

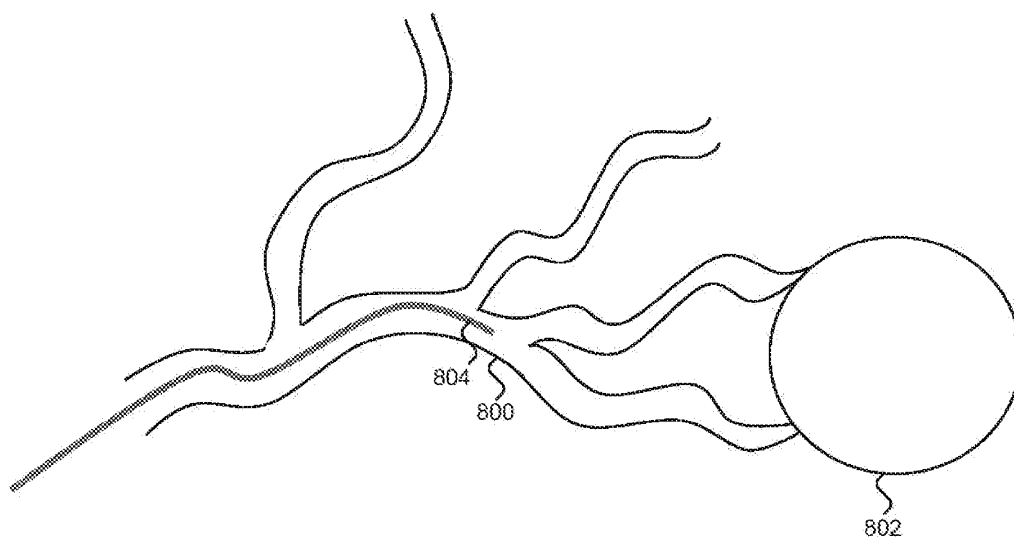


Fig. 21A

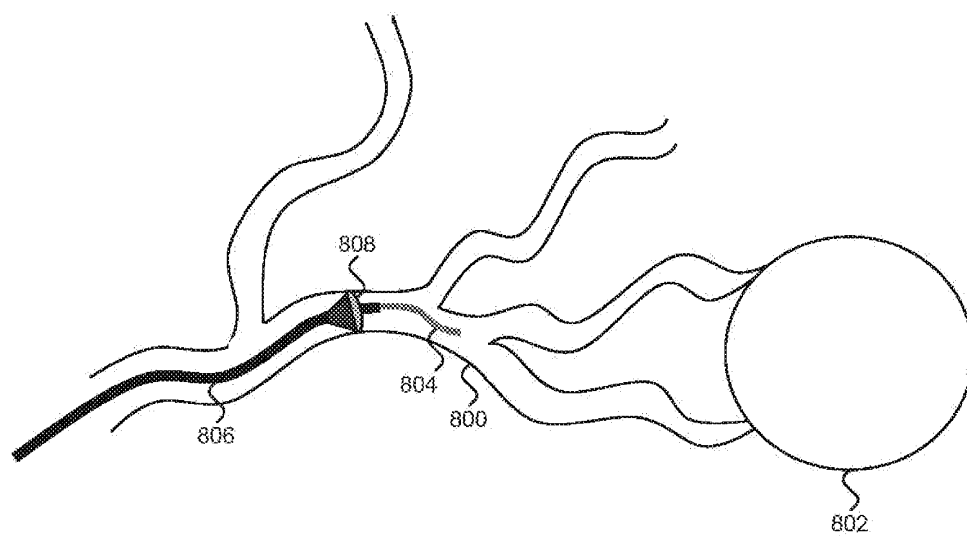


Fig. 21B

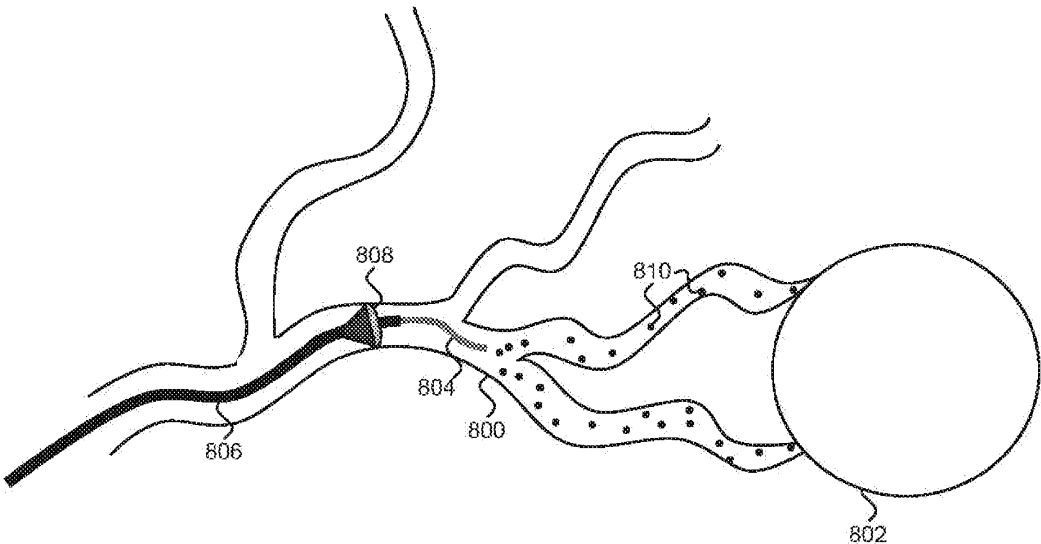


Fig. 21C

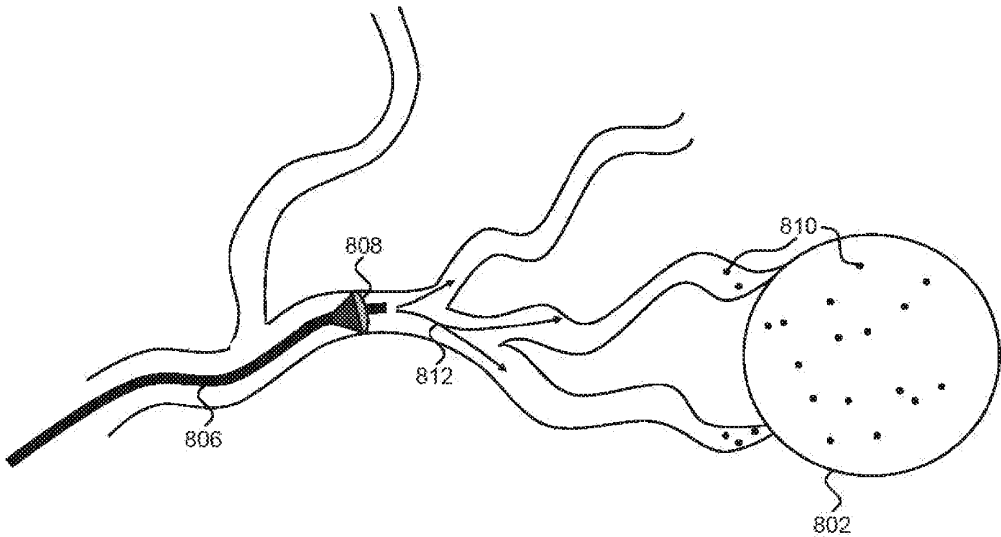


Fig. 21D

10/28

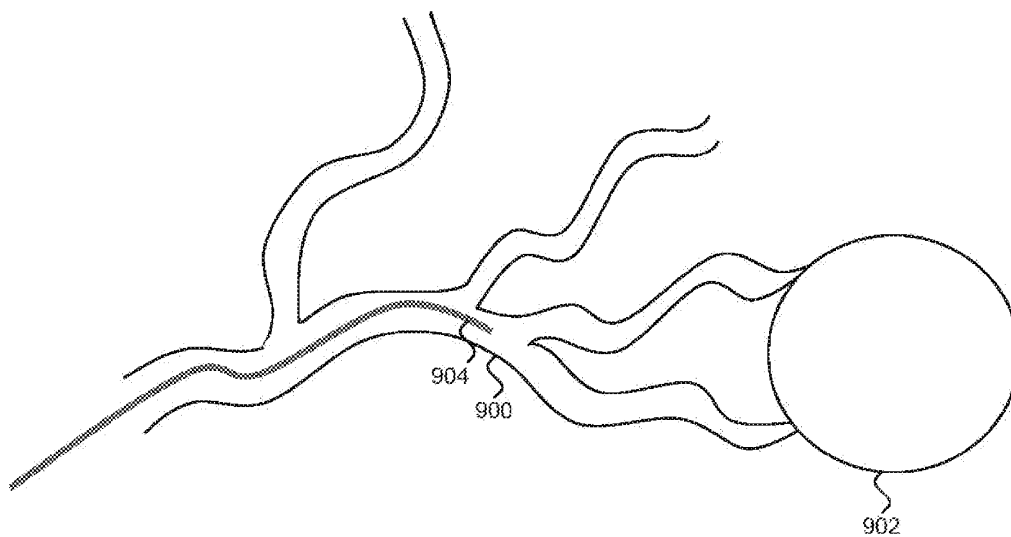


Fig. 22A

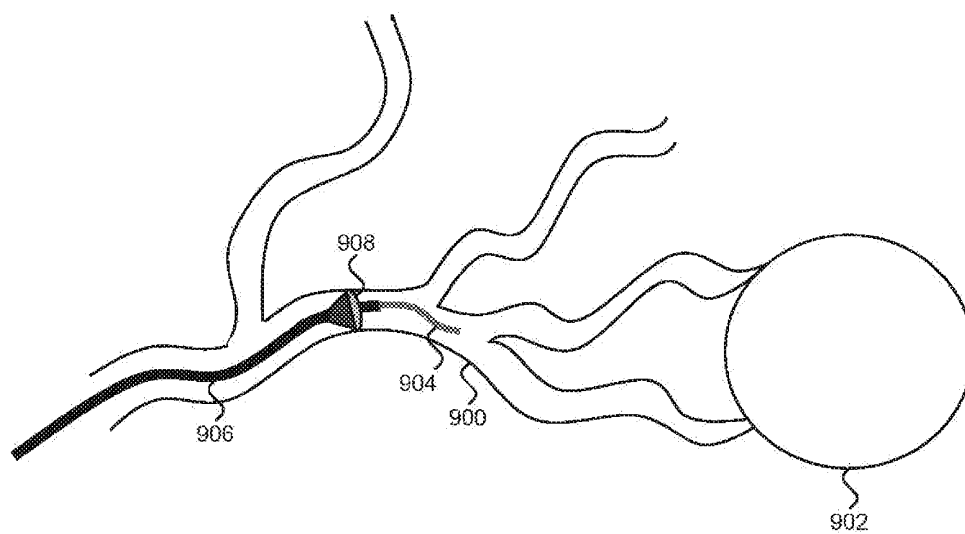


Fig. 22B

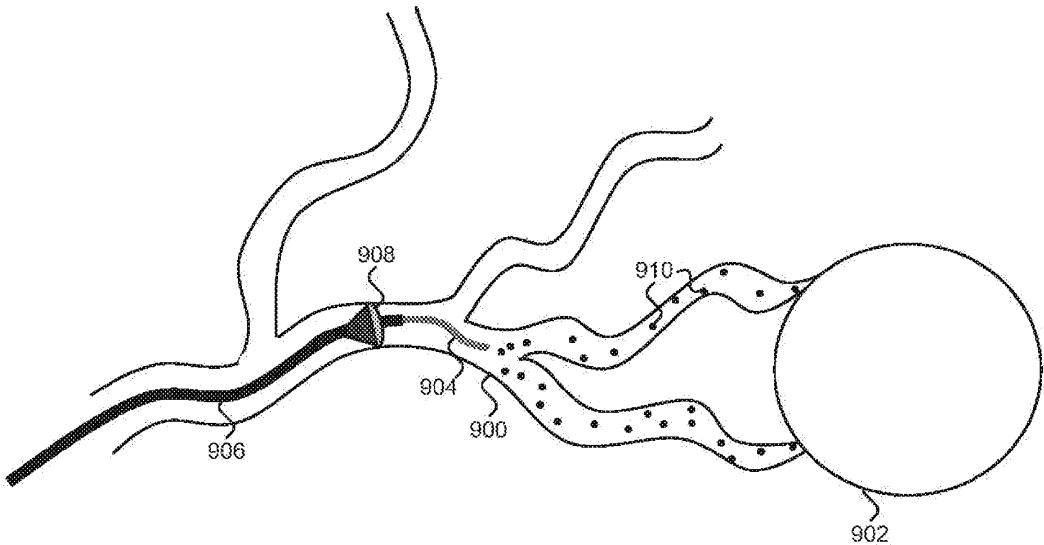


Fig. 22C

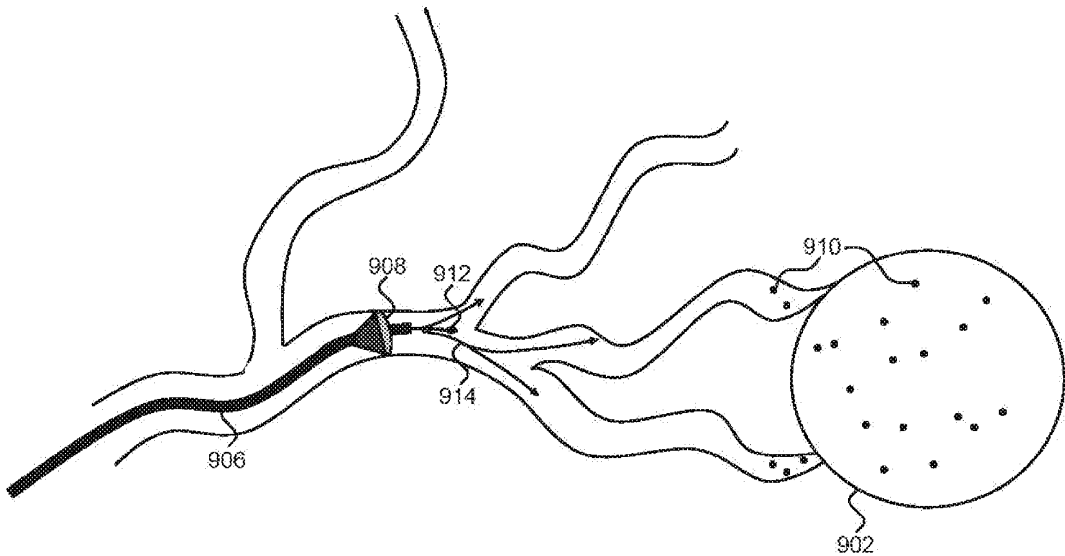


Fig. 22D

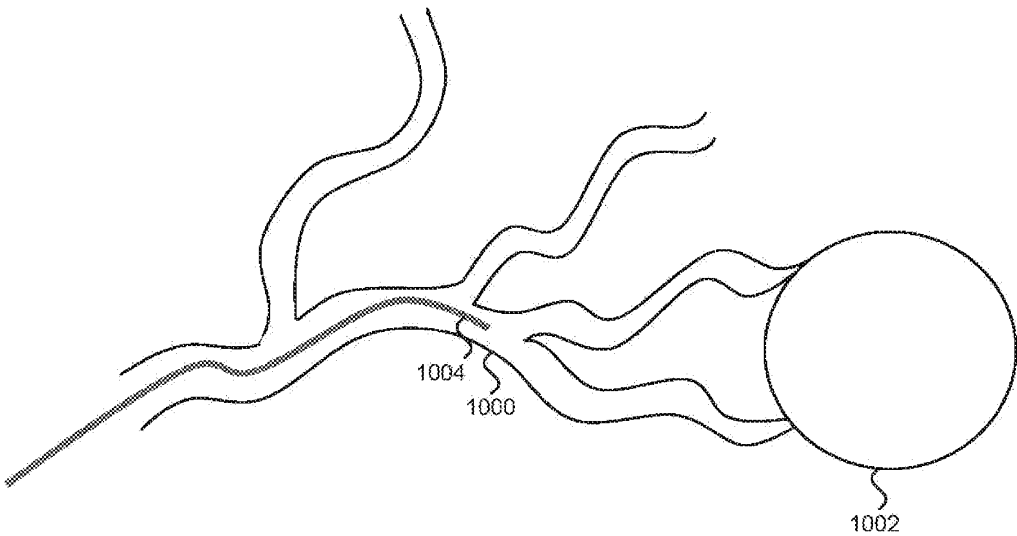


Fig. 23A

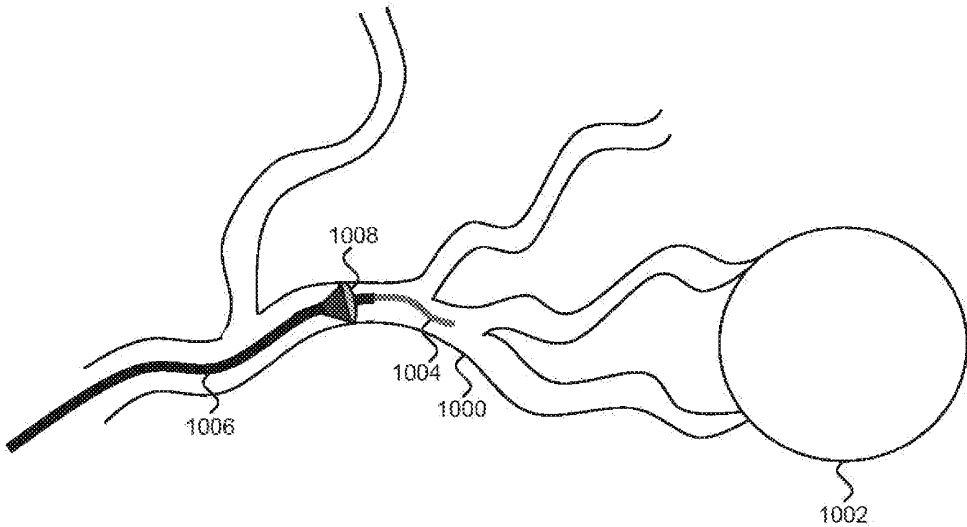


Fig. 23B

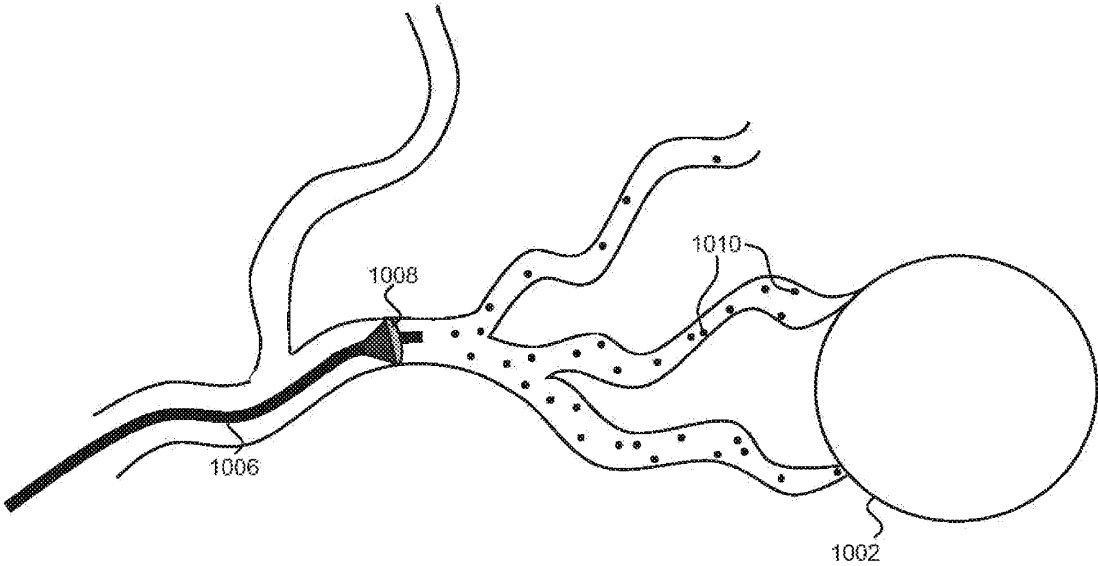


Fig. 23C

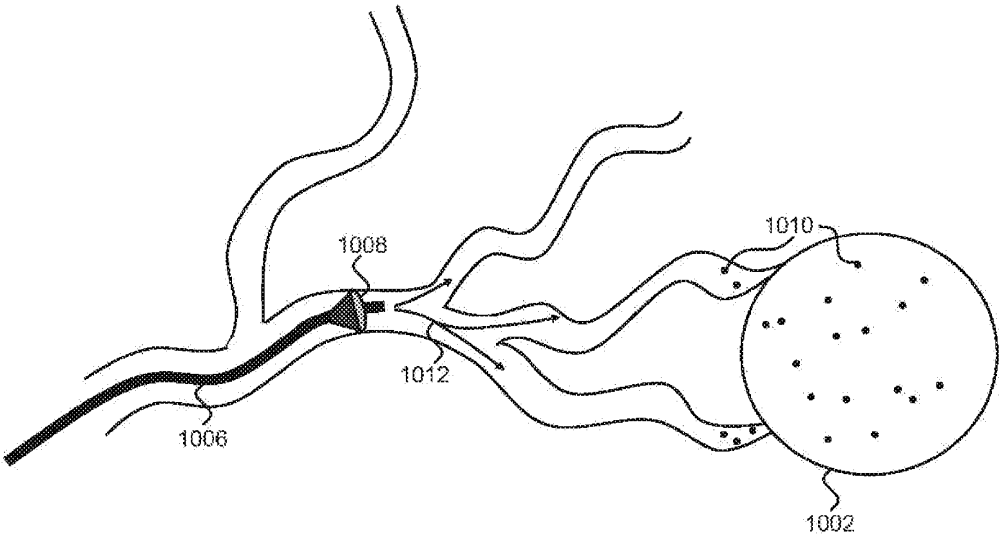


Fig. 23D

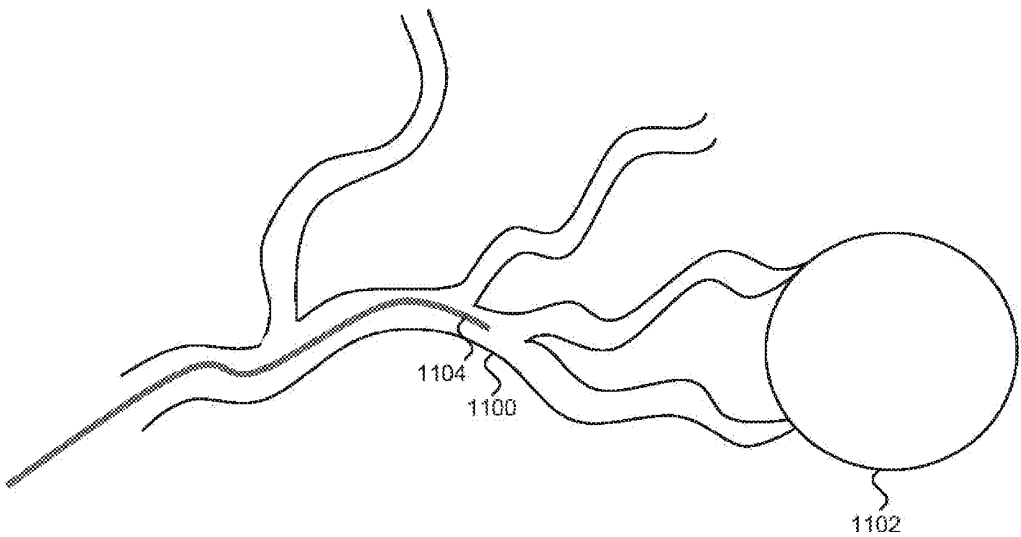


Fig. 24A

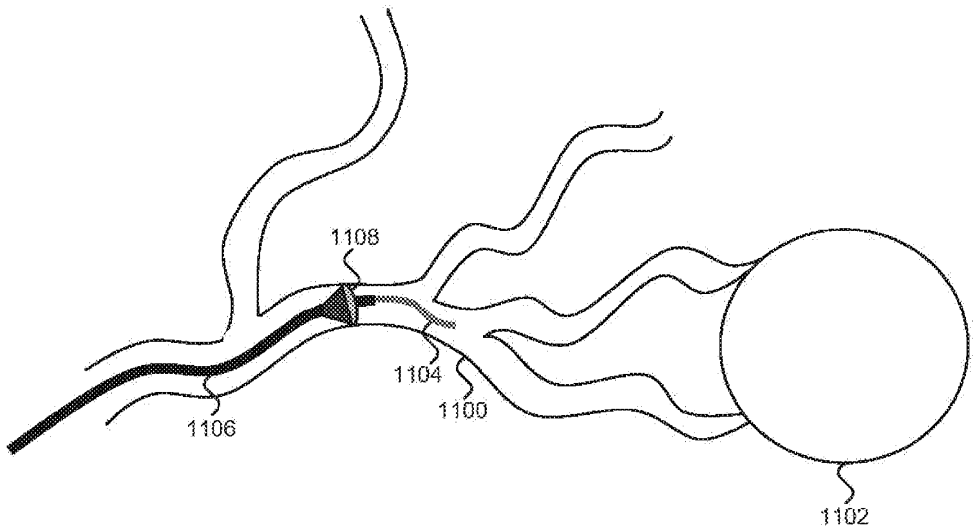


Fig. 24B

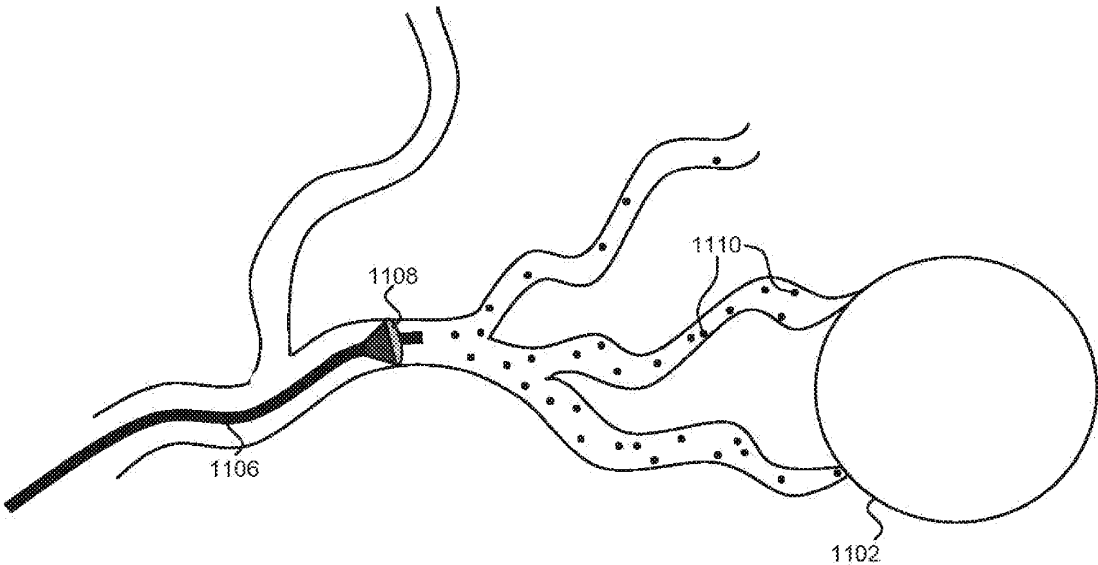


Fig. 24C

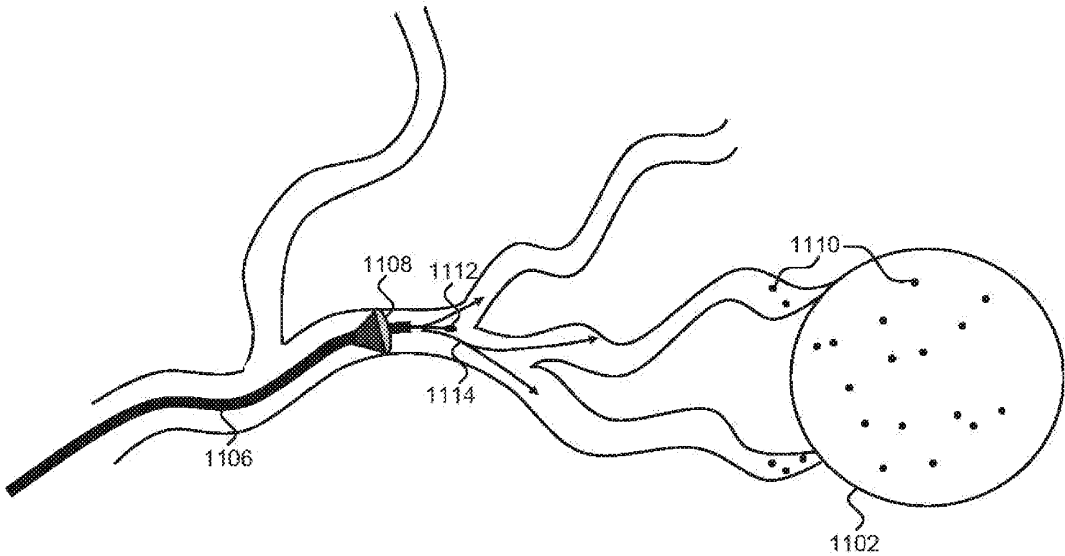


Fig. 24D

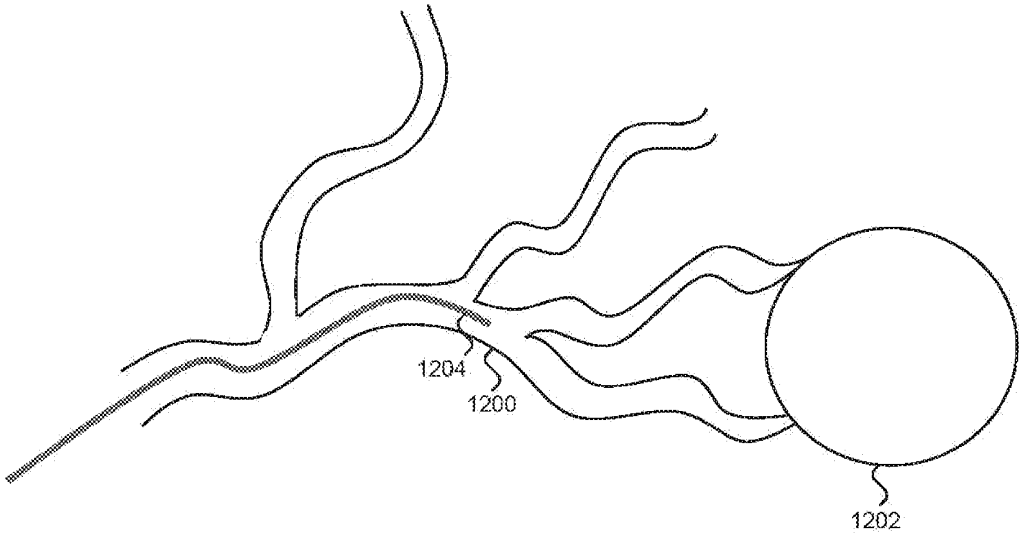


Fig. 25A

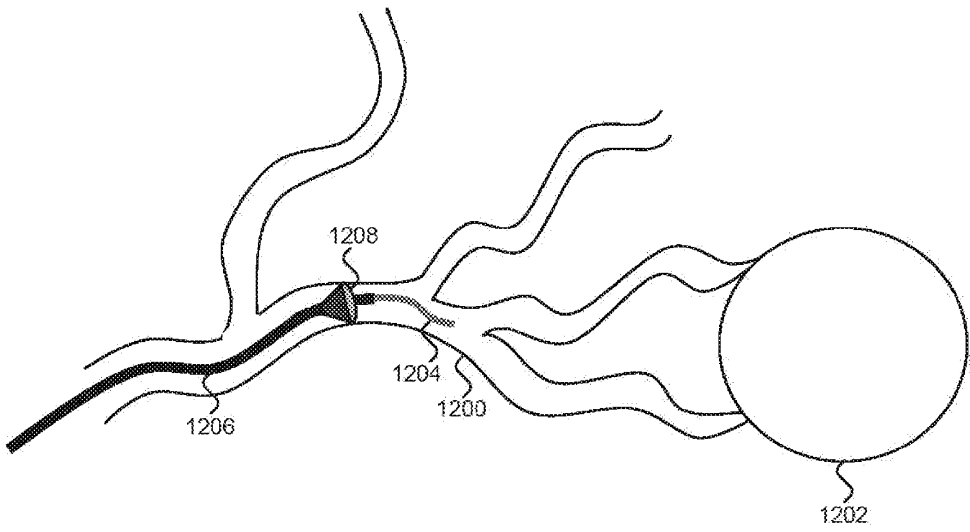


Fig. 25B

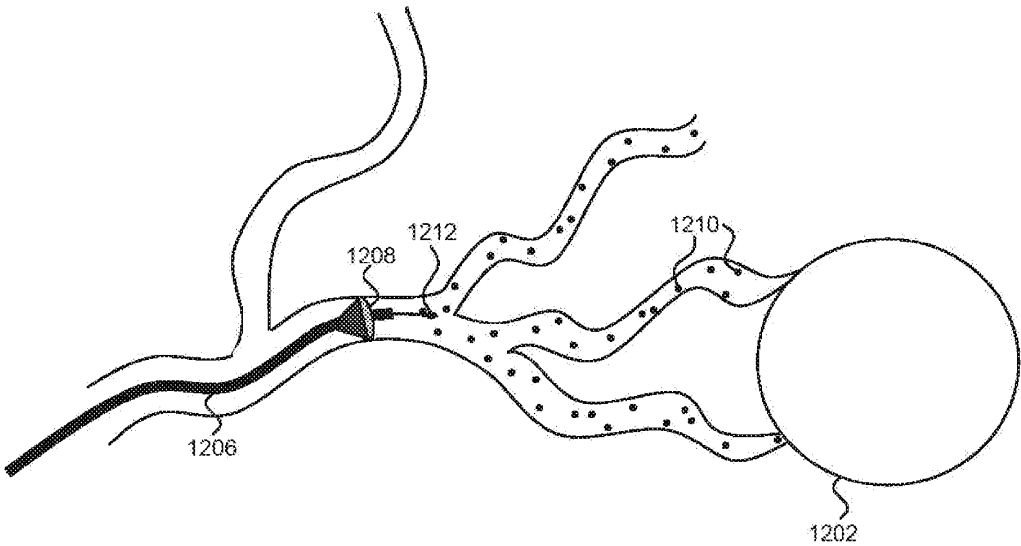


Fig. 25C

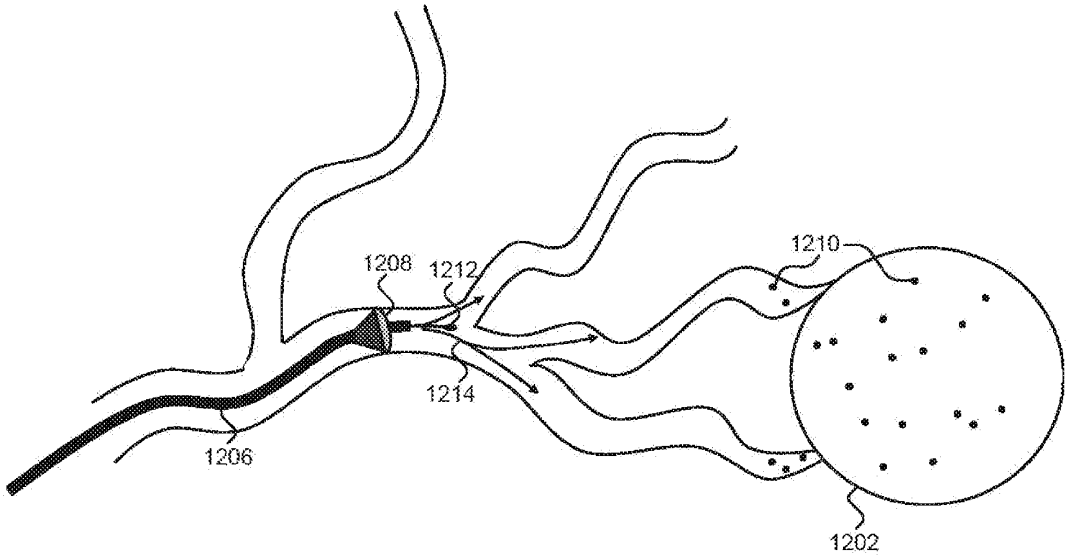
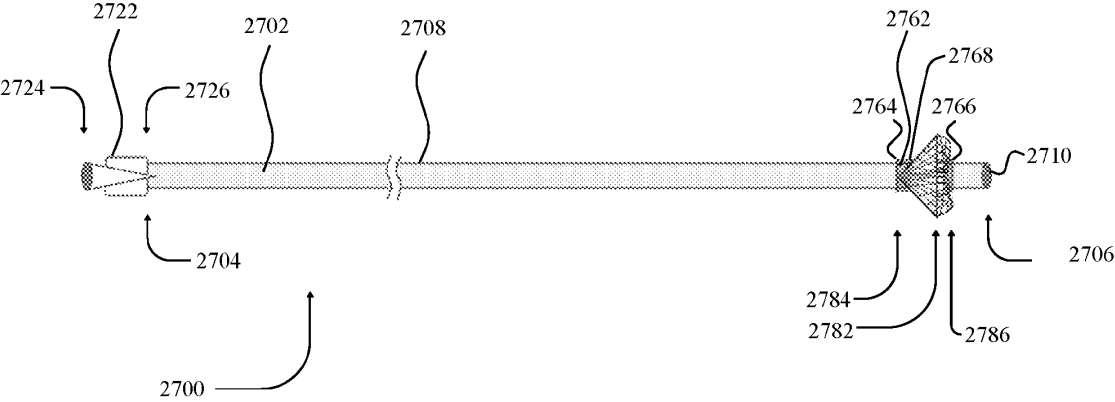
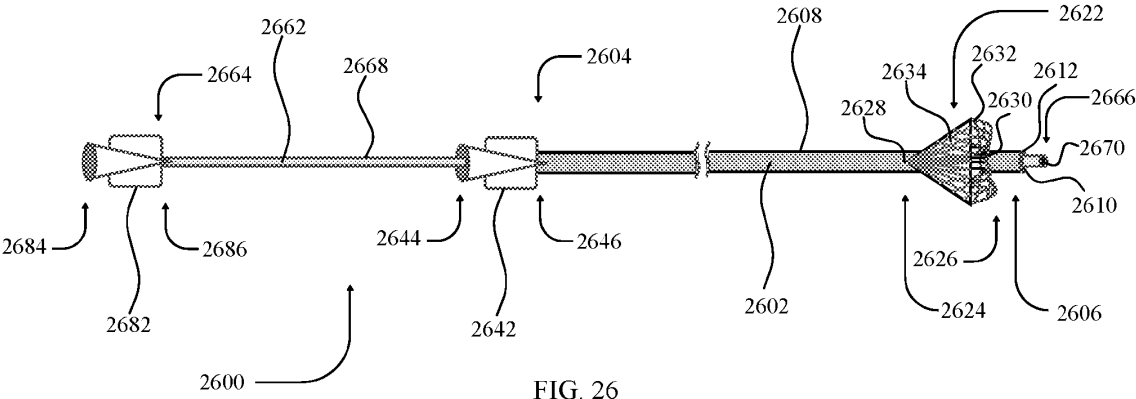


Fig. 25D



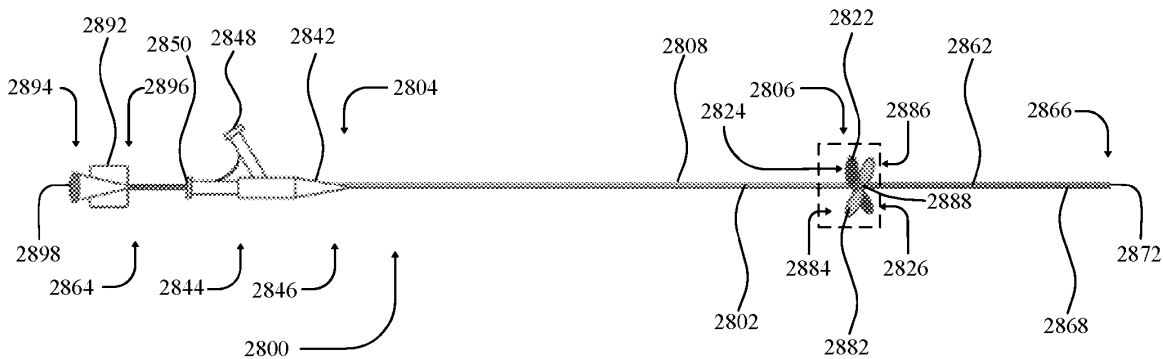


FIG. 28A

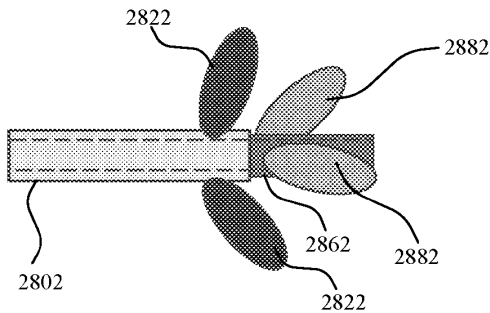


FIG. 28B

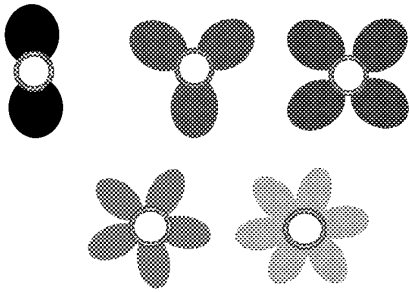


FIG. 28C

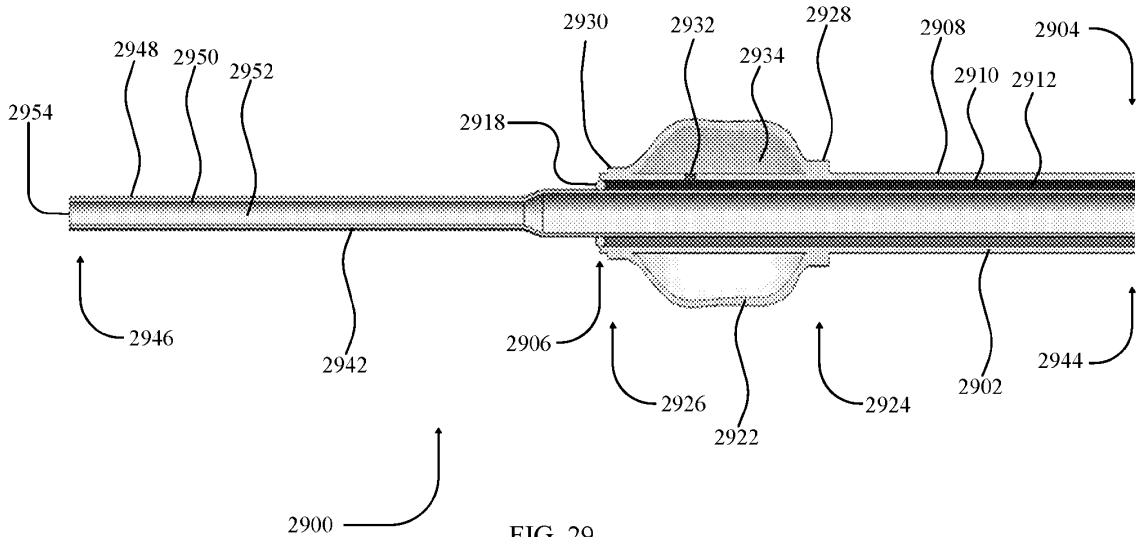


FIG. 29

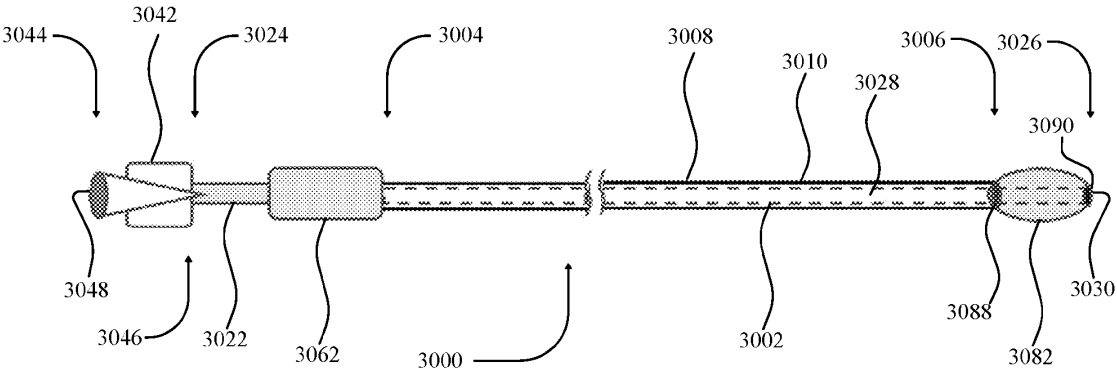


FIG. 30

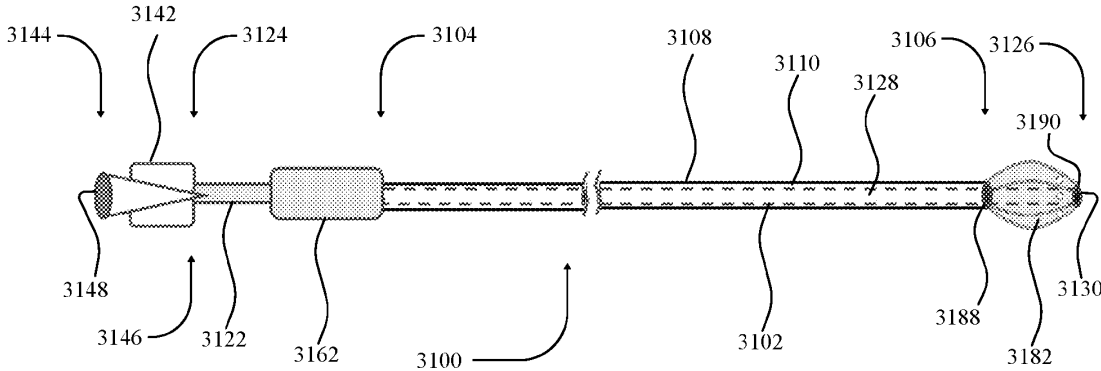


FIG. 31

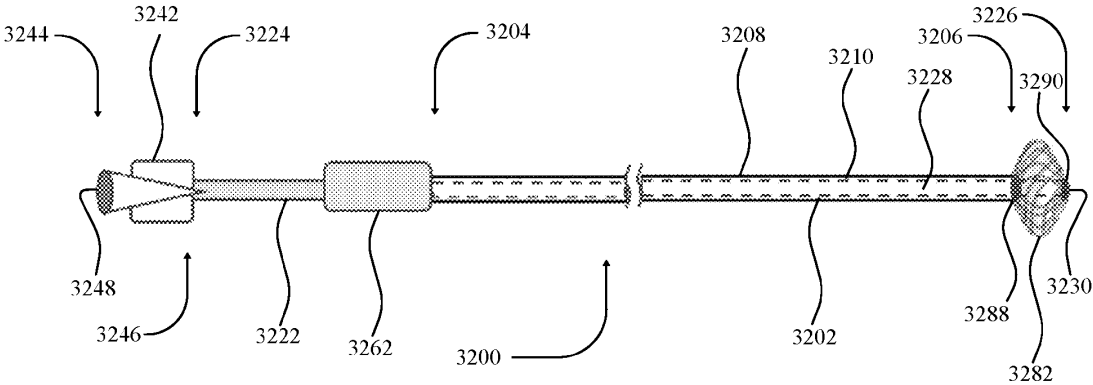
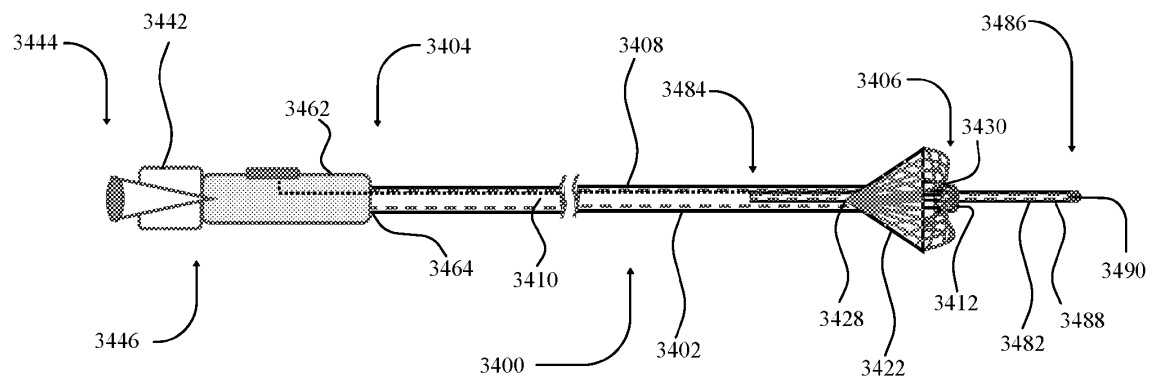
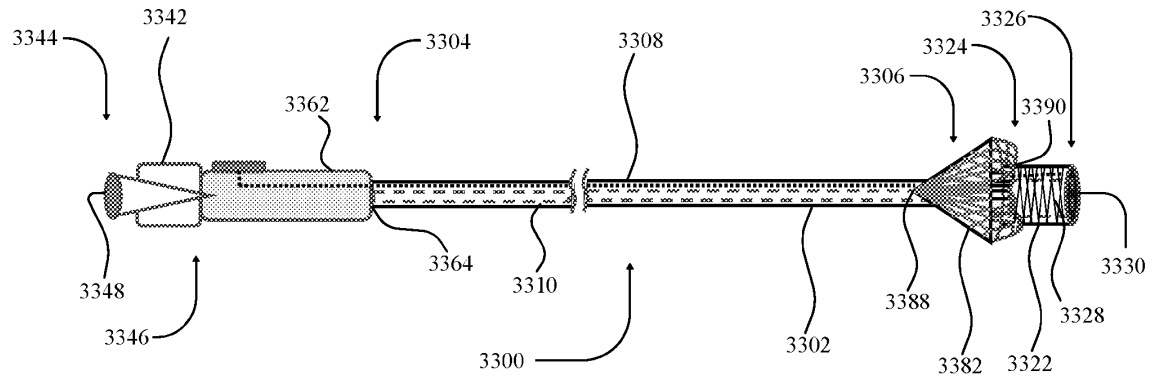


FIG. 32



22/28

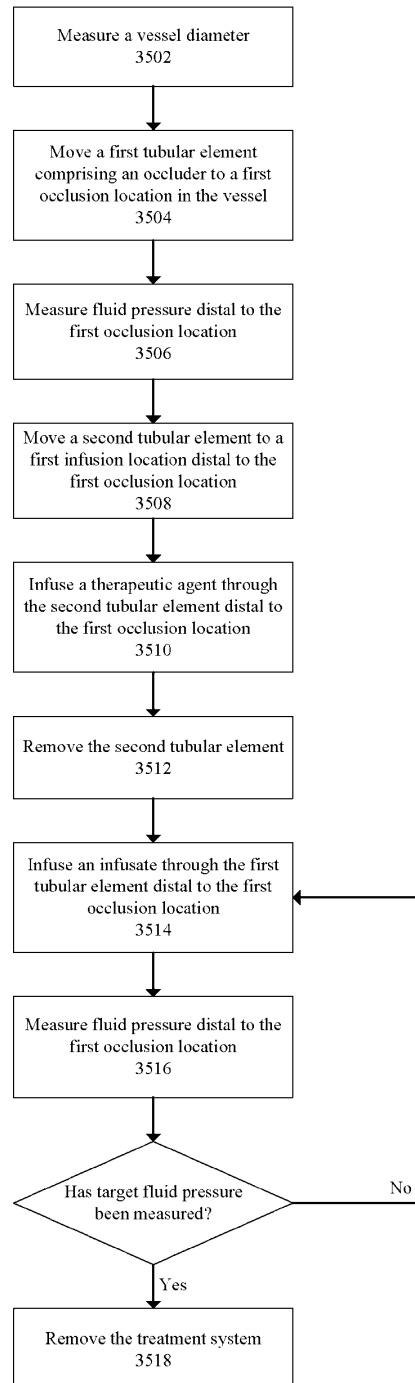
3500

FIG. 35

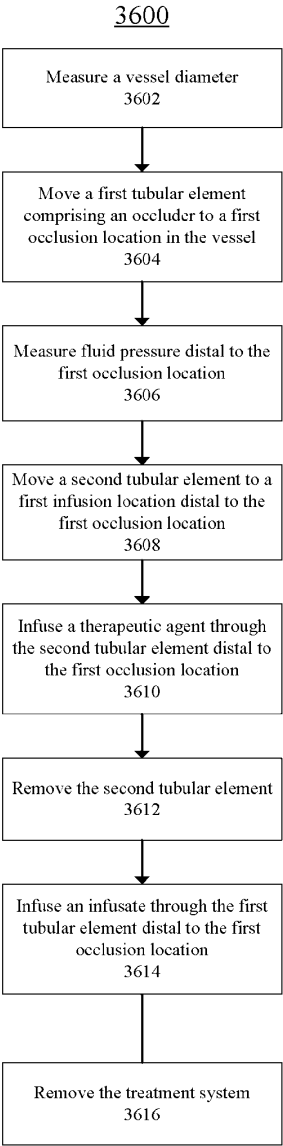


FIG. 36

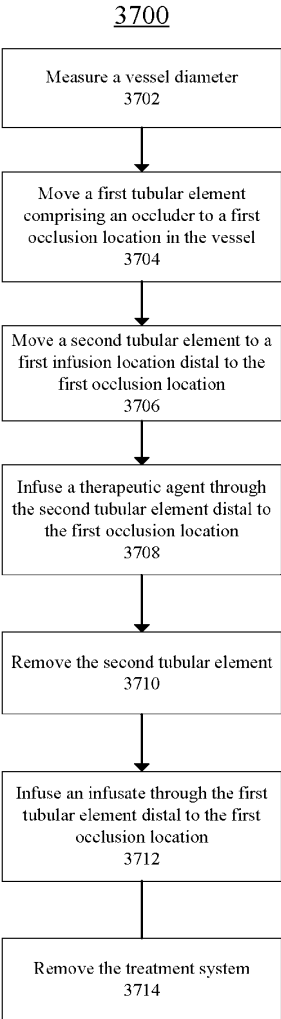


FIG. 37

24/28

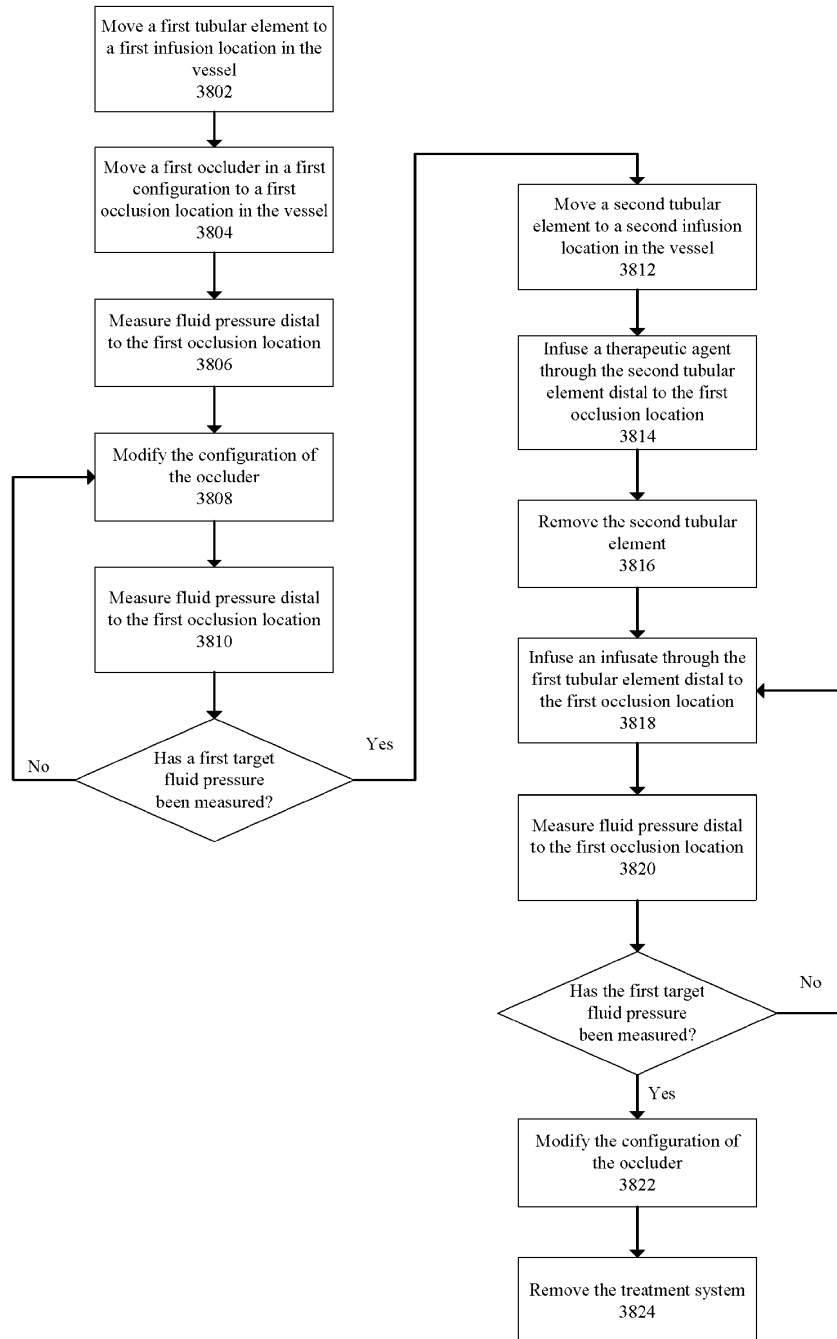
3800

FIG. 38

25/28

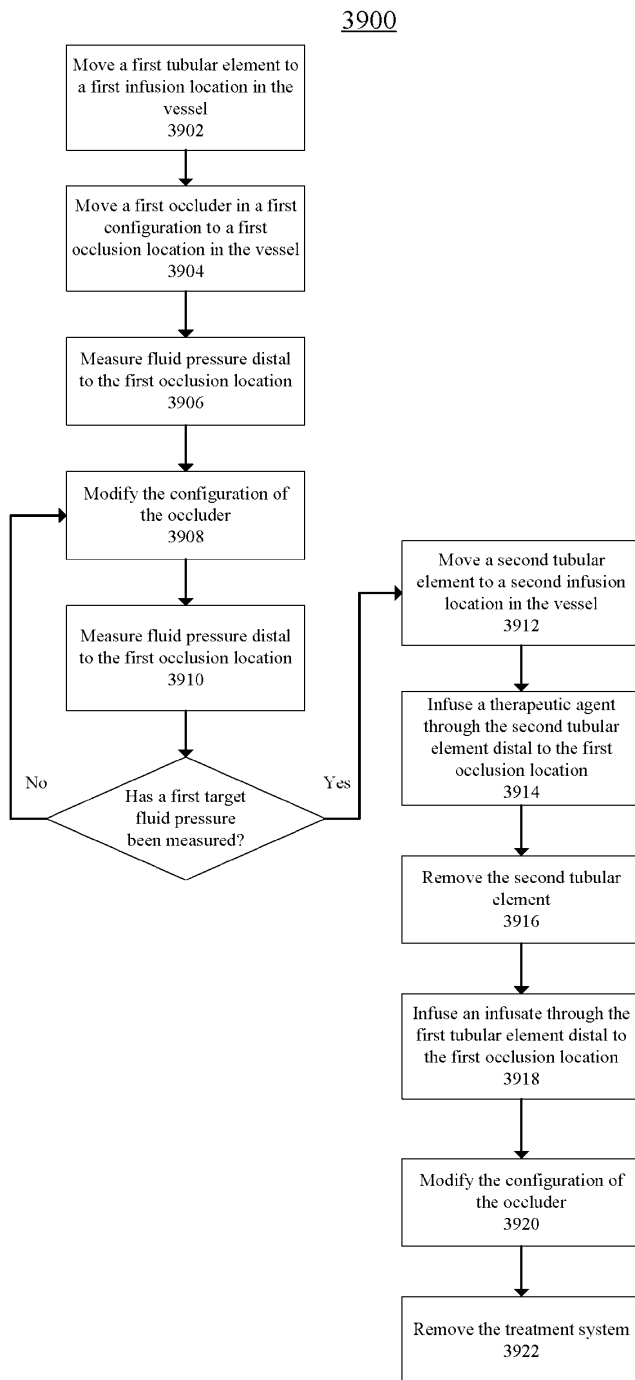


FIG. 39

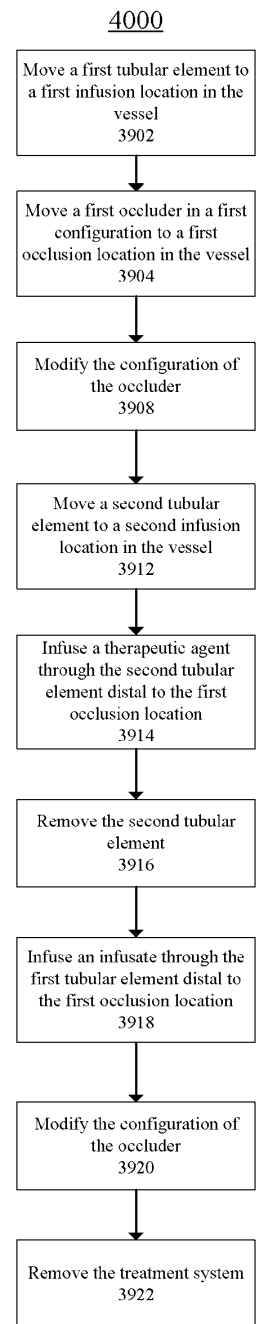


FIG. 40

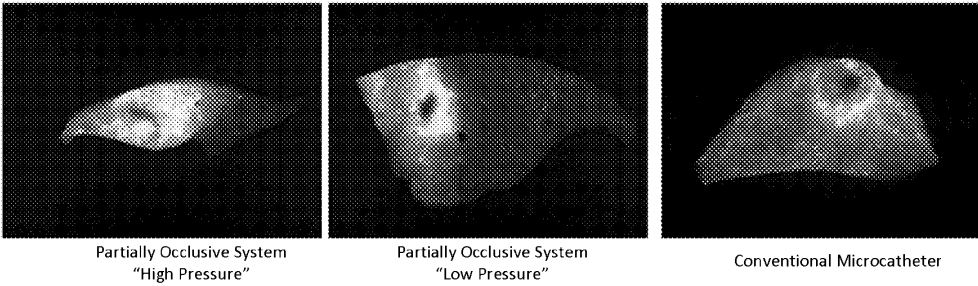


FIG. 41

	Tumor Diameter (mm)	Distal Vessel Diameter (mm)	Proximal Vessel Diameter (mm)	Secondary Catheter Displacement from Partial Occluder (mm)	Initial Vessel Pressure (mmHg)	Distal Pressure with Partially Occlusive System (mmHg)	Distal Pressure Decrease (%)
Average	2.01	1.39	2.47	35.04	100.89	55.63	45.66
Standard Deviation	0.49	0.25	0.43	18.14	6.31	12.15	13.61
Minimum	1.30	1.00	1.68	10.20	92.00	27.00	20.02
Maximum	3.00	1.80	3.22	83.00	111.00	76.00	71.74

FIG. 42

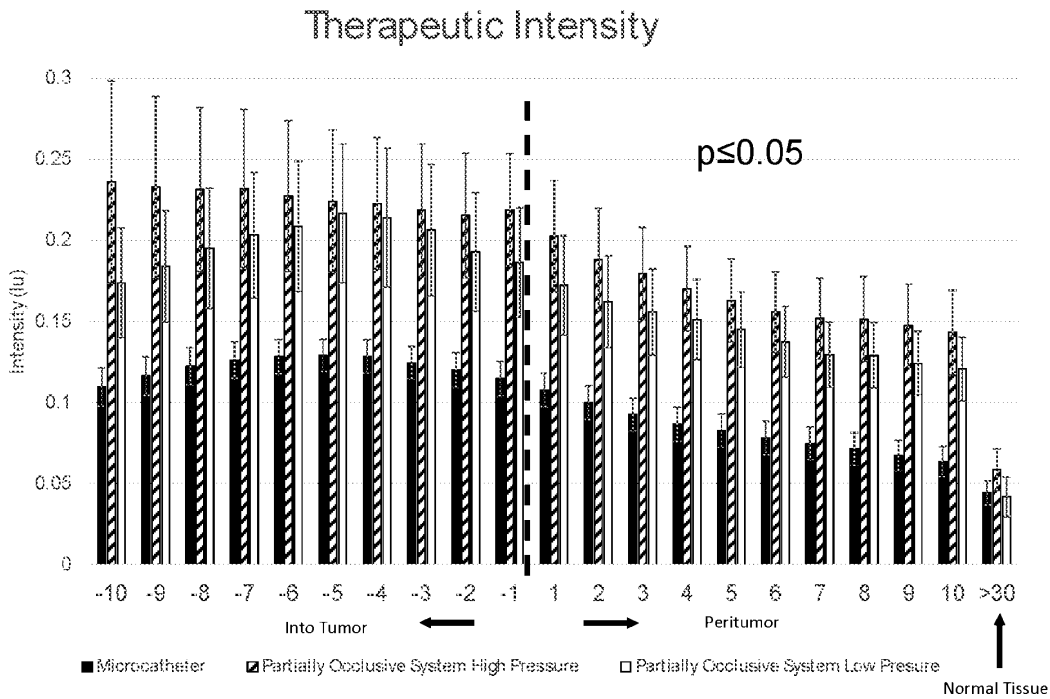


FIG. 43

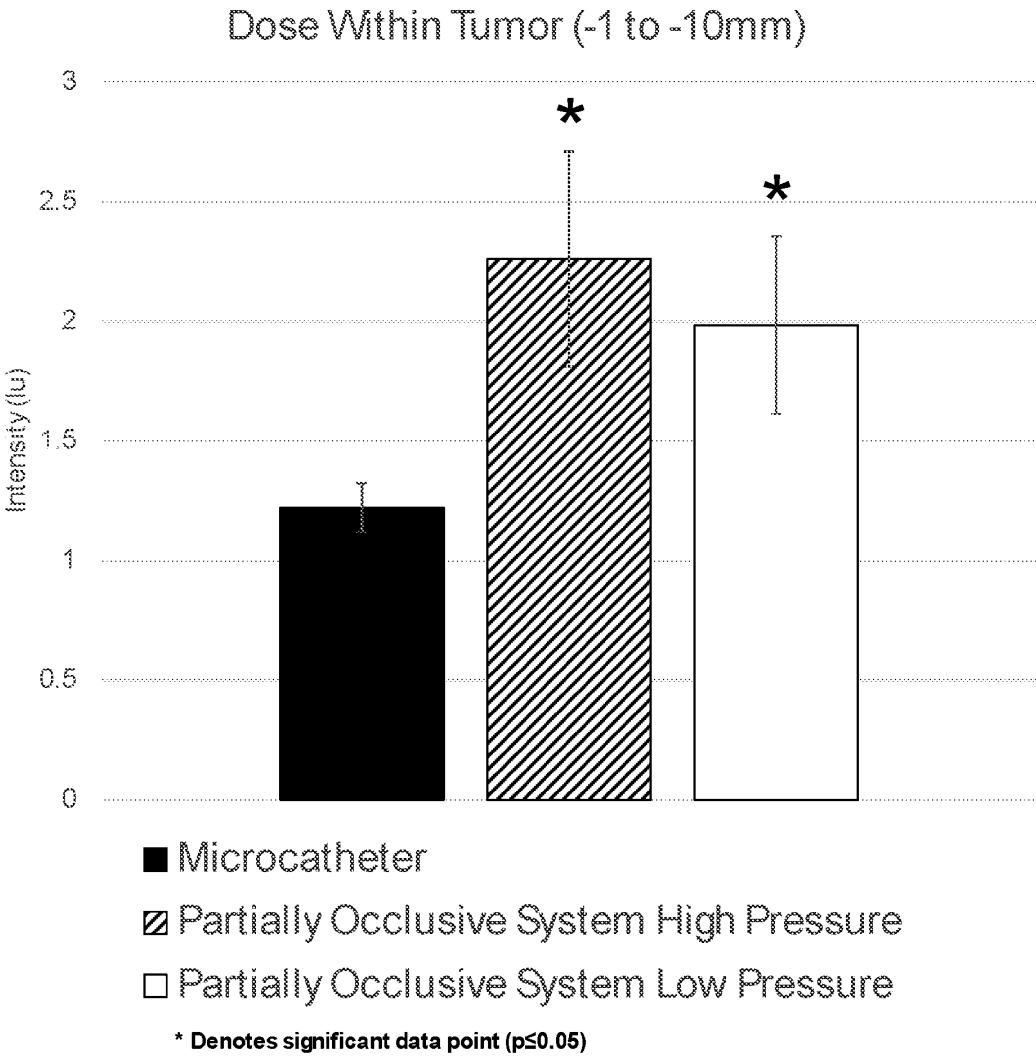


FIG. 44