


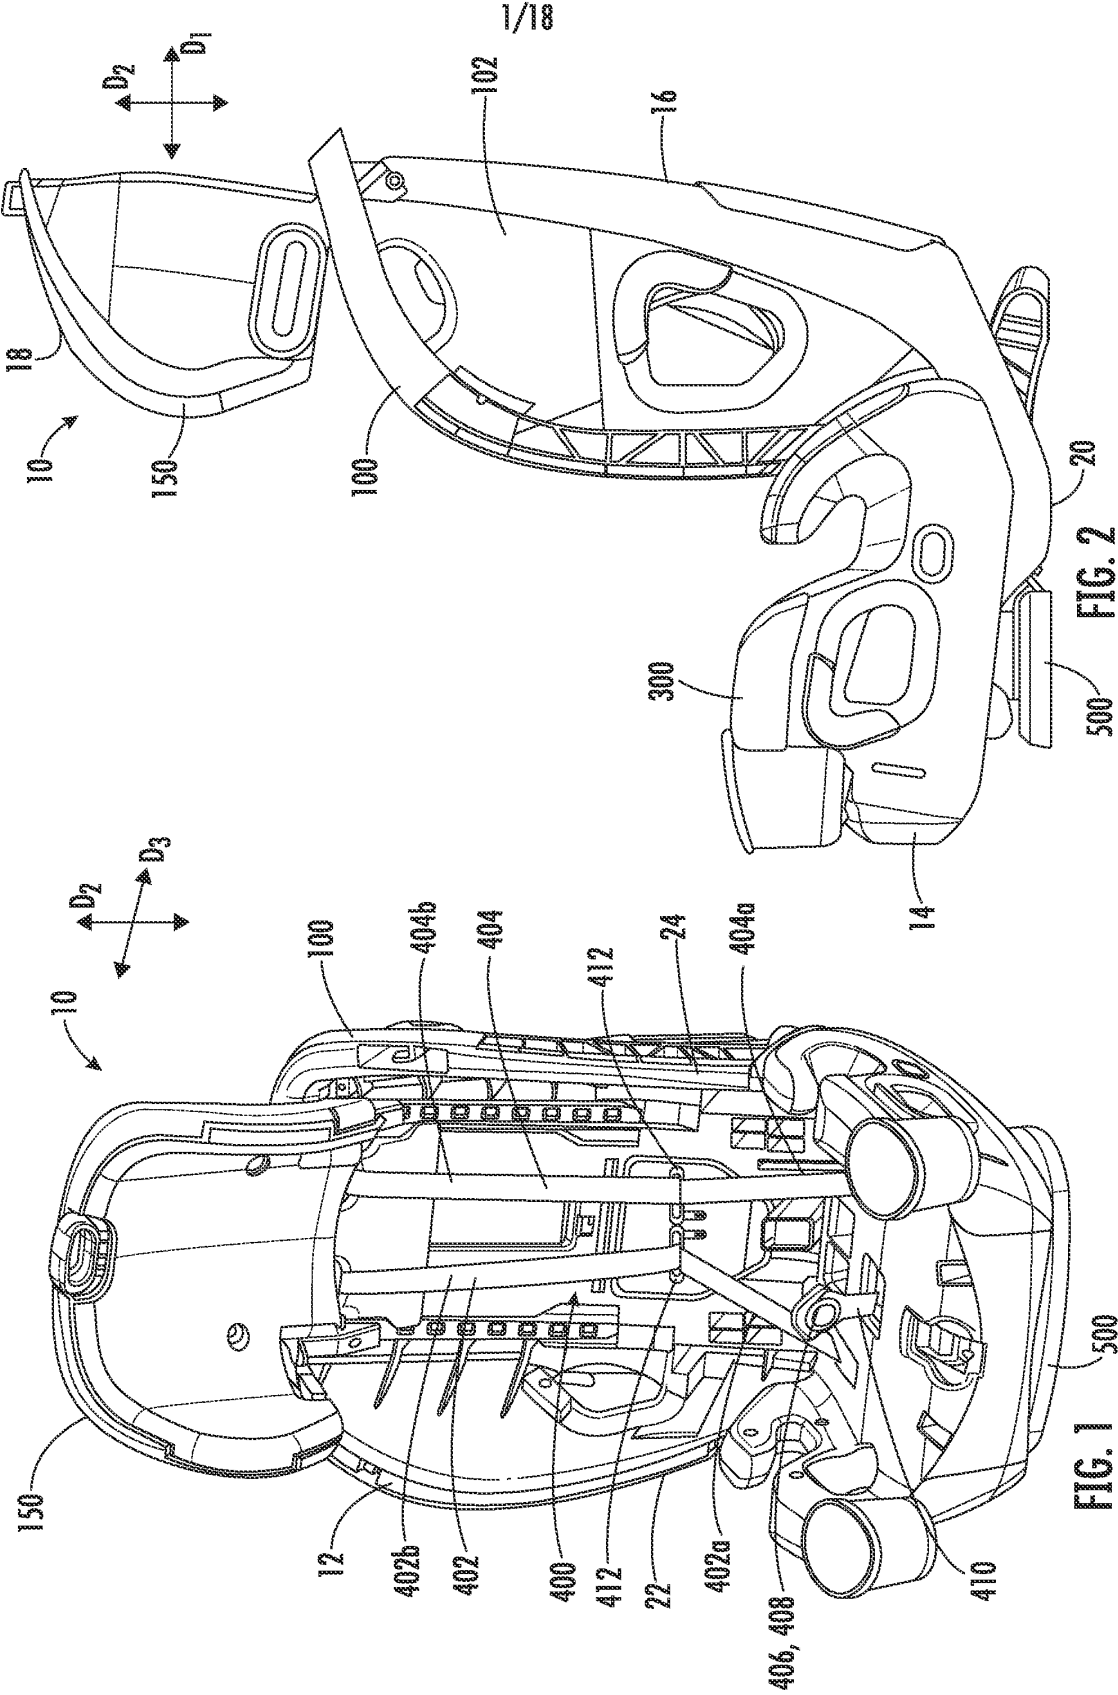

2/18


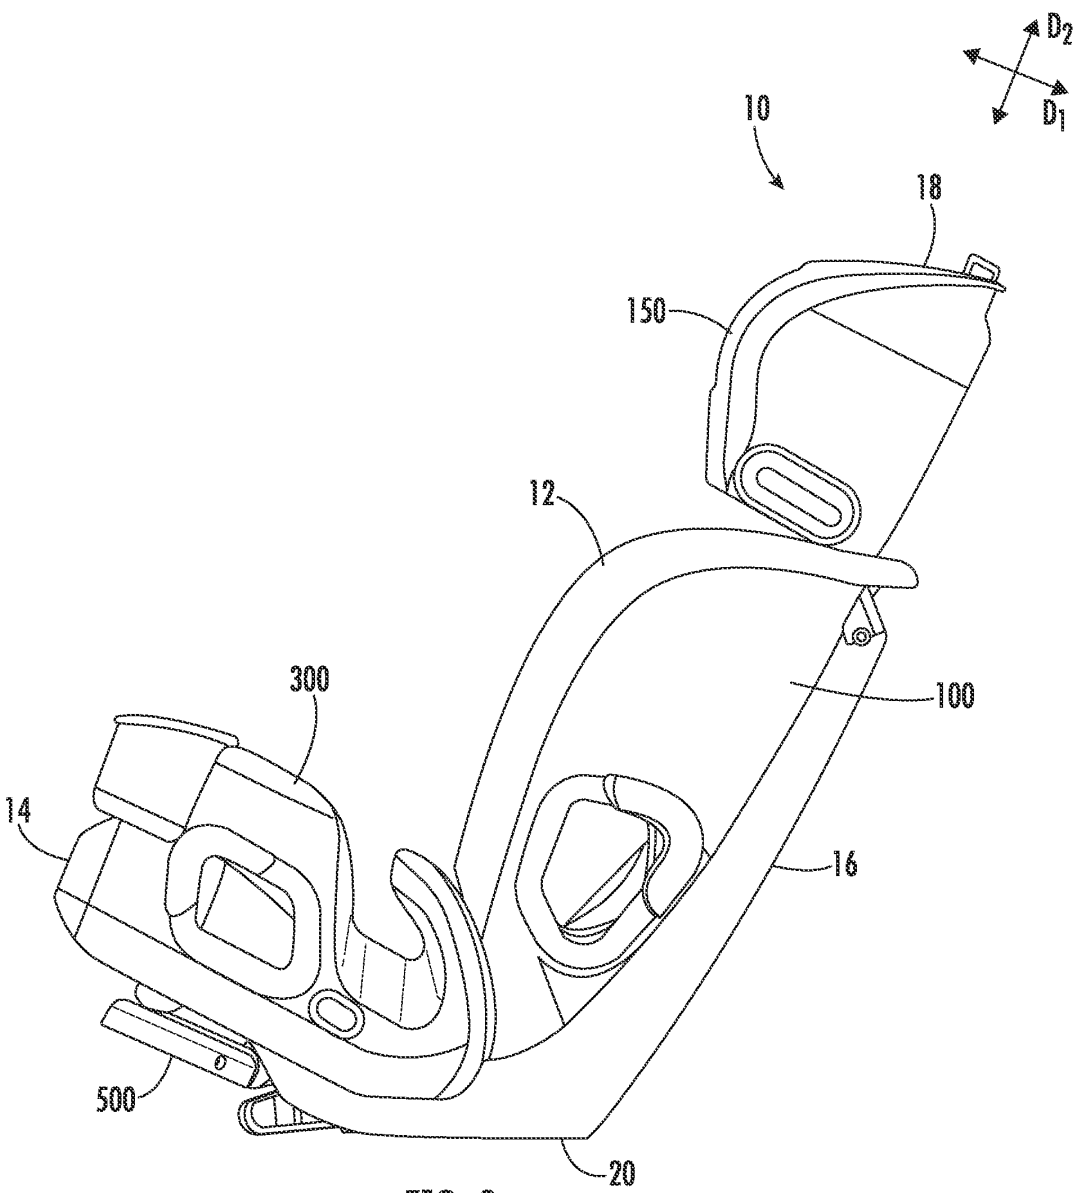


FIG. 3

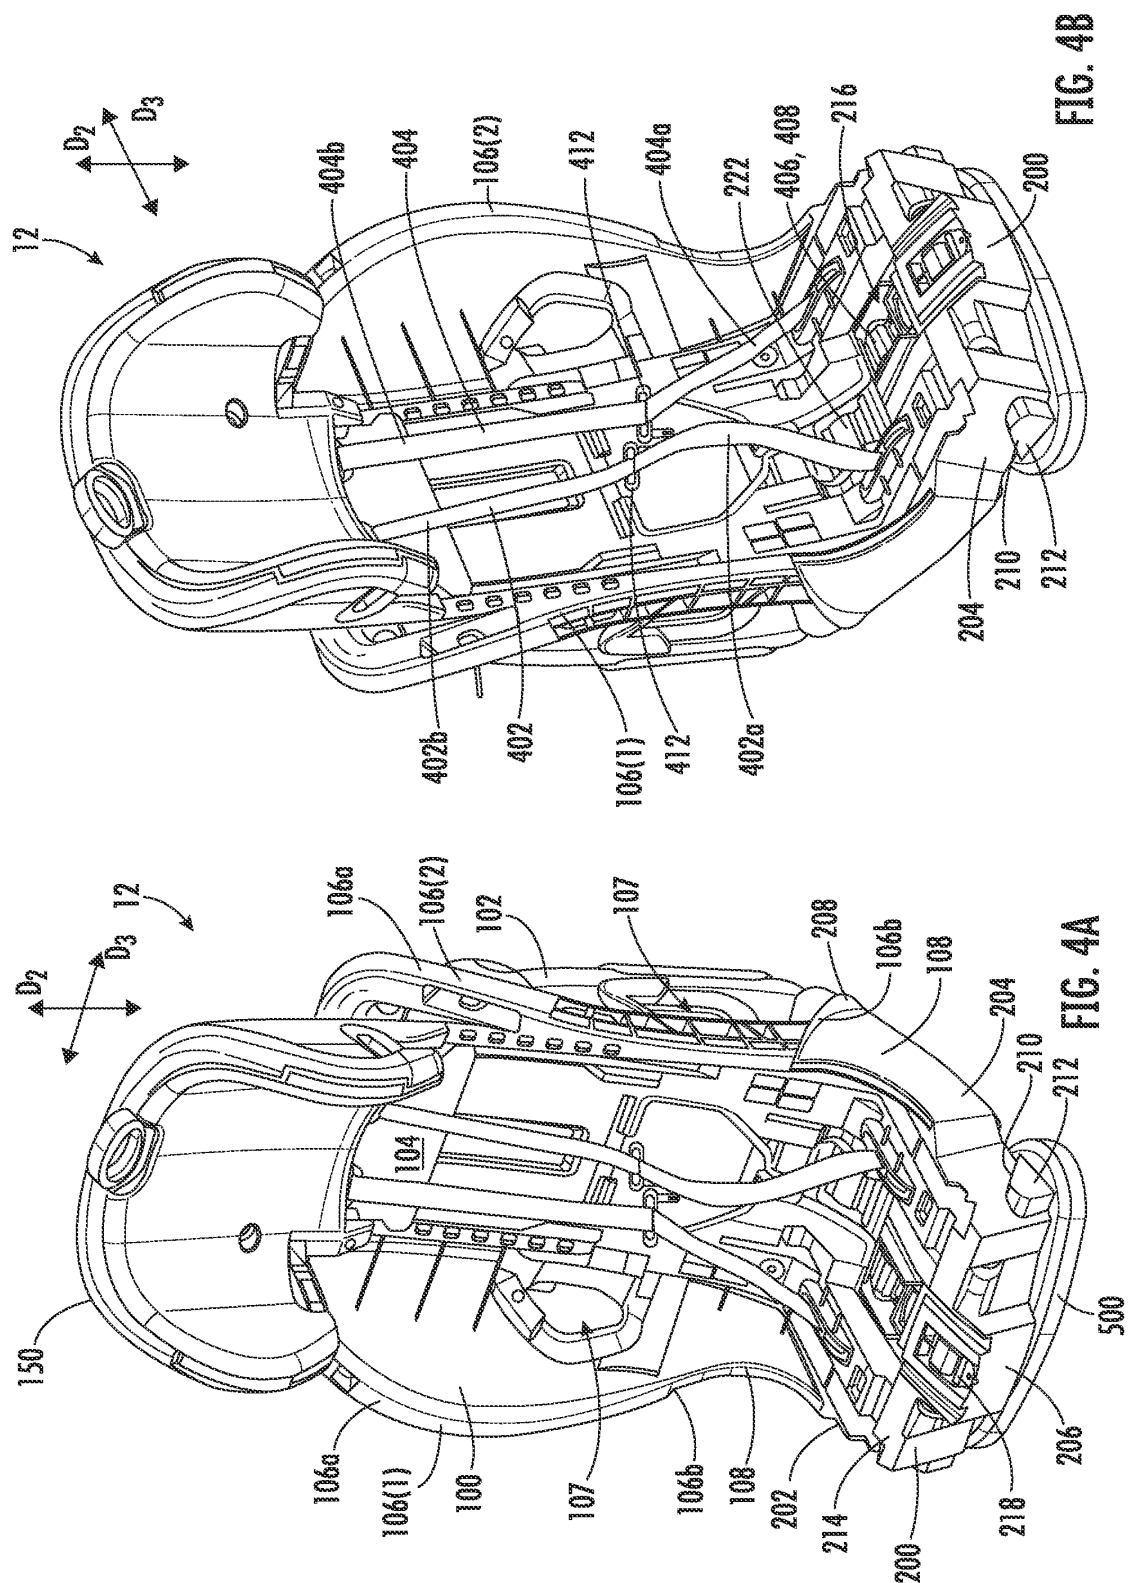

4/18

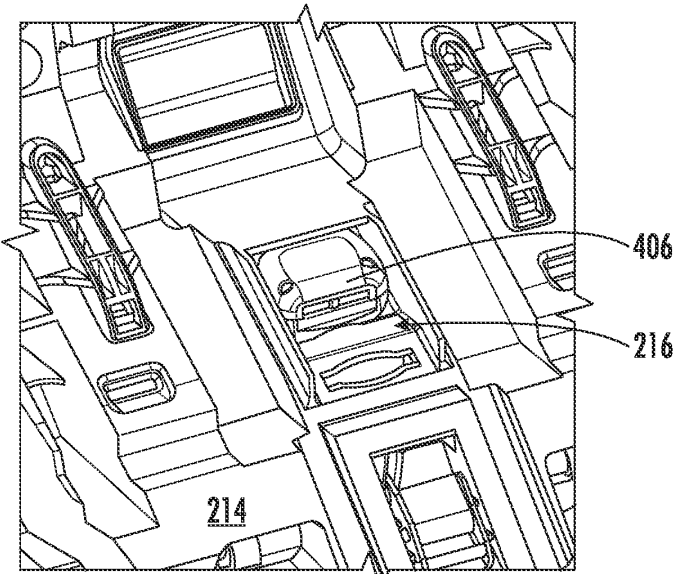


FIG. 4C

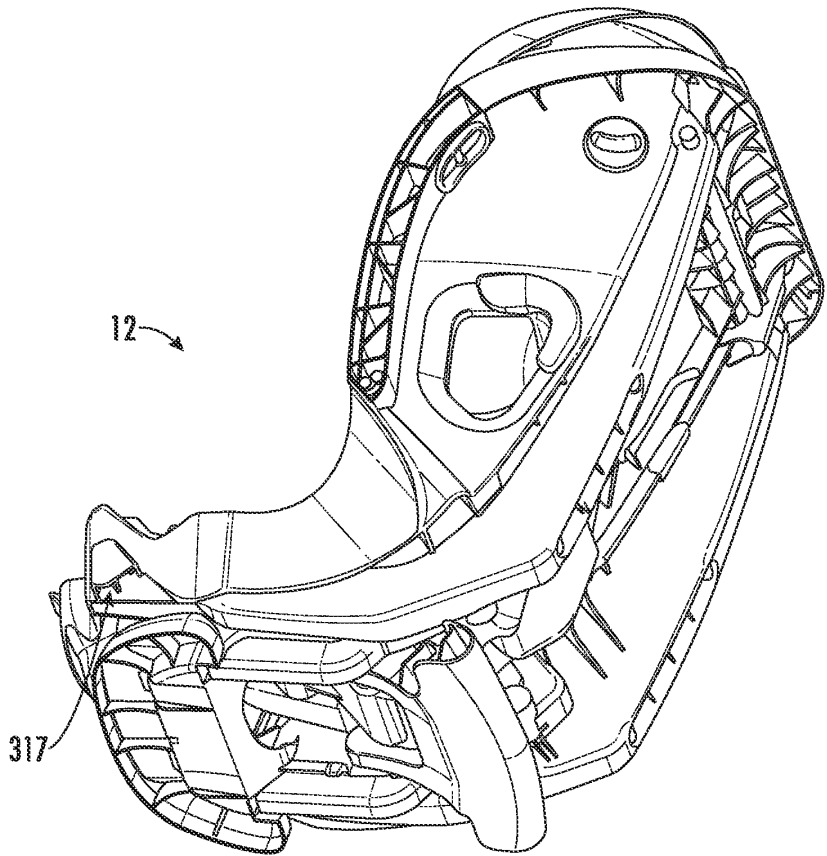


FIG. 4D

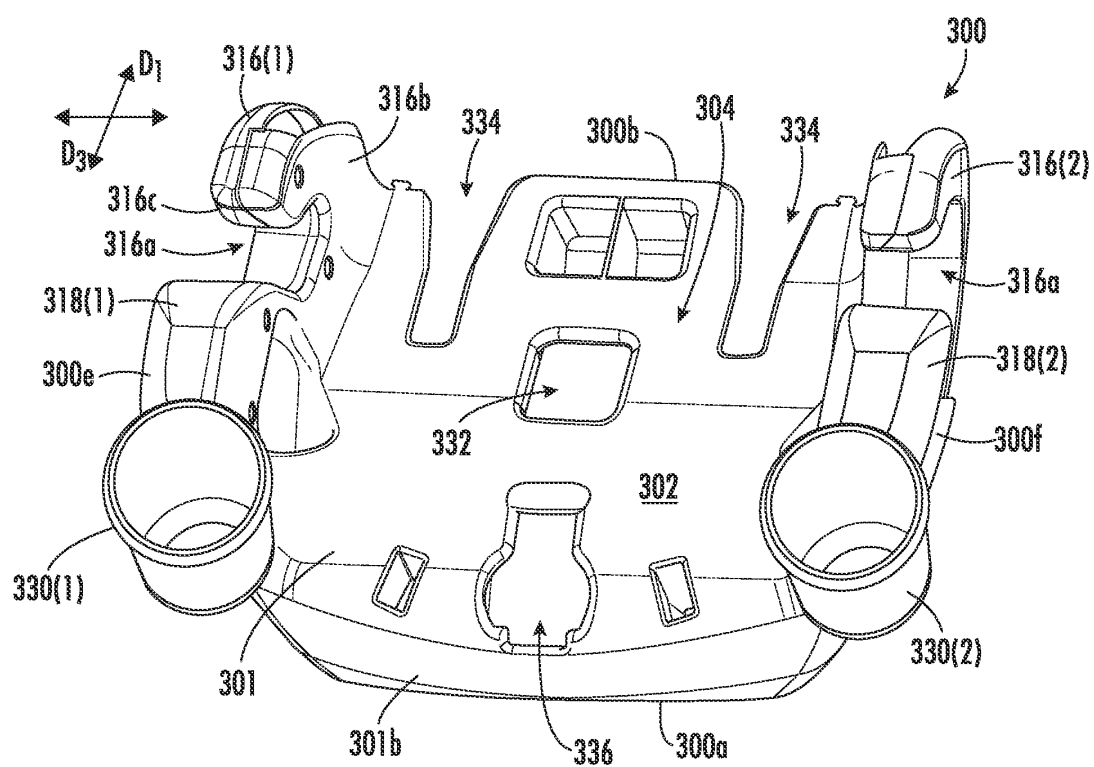
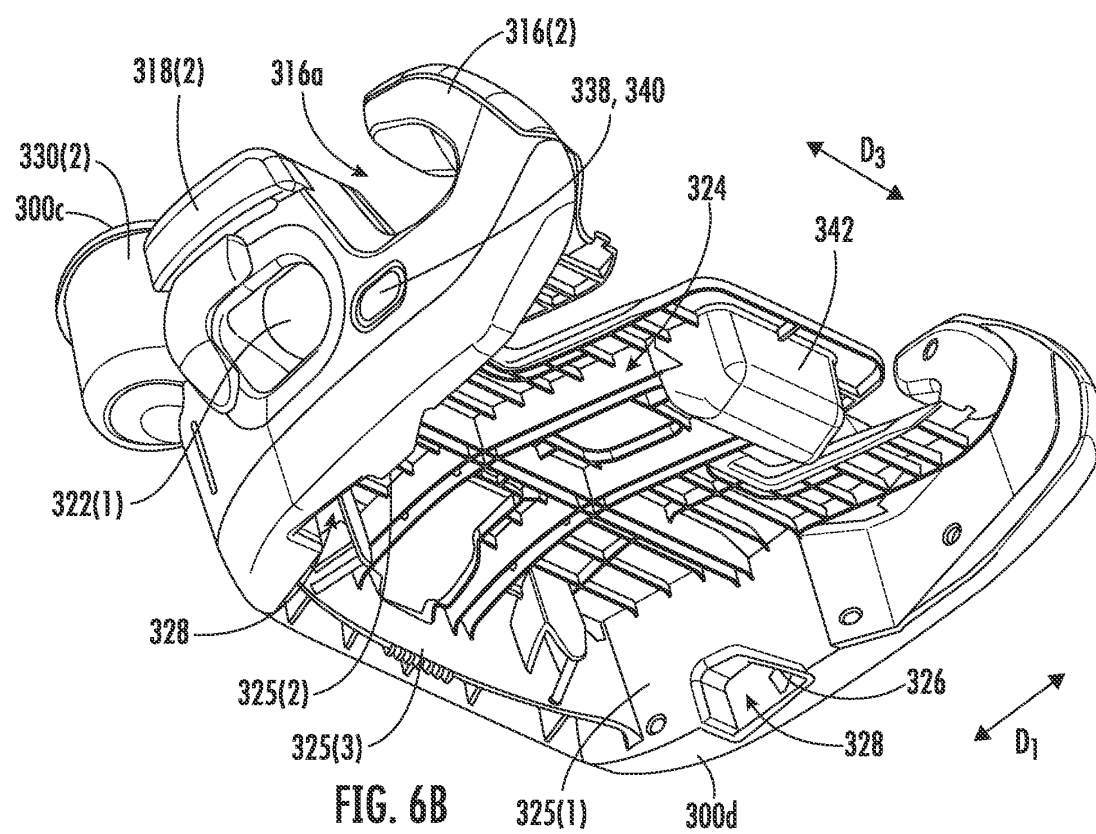
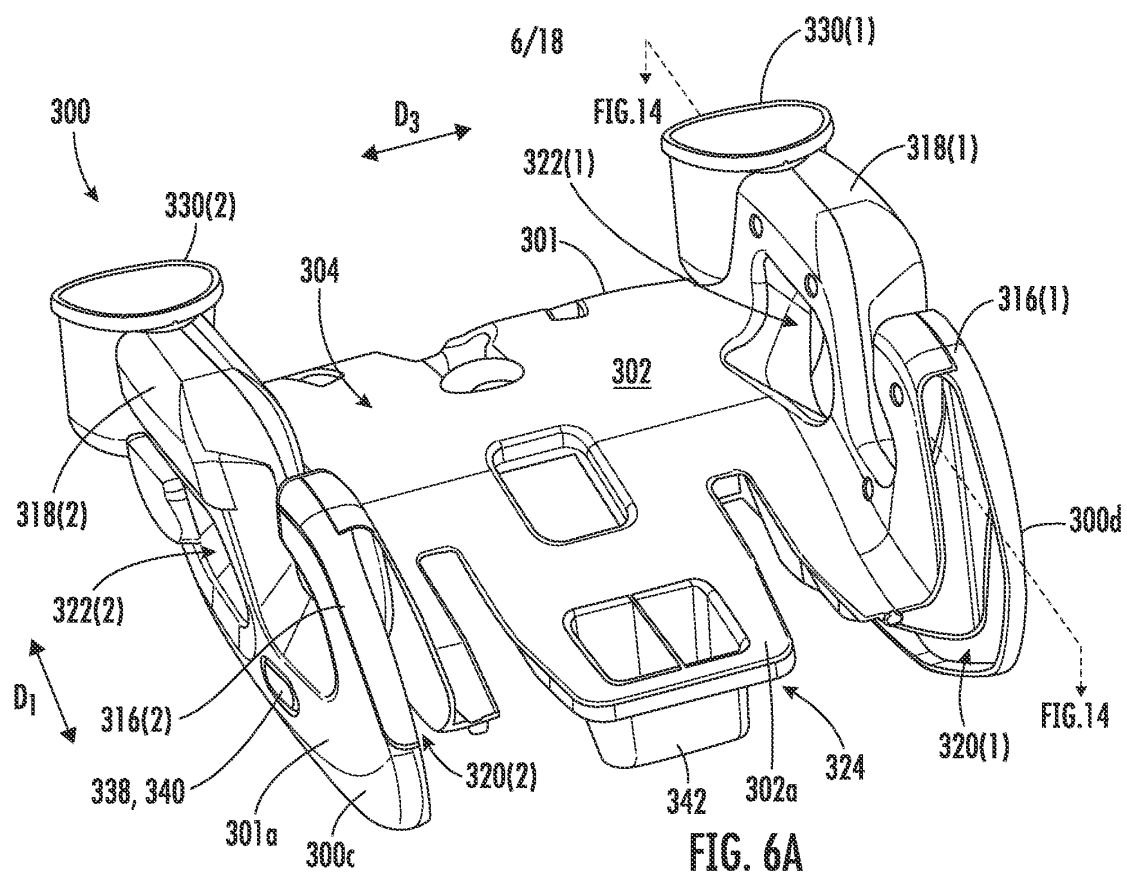
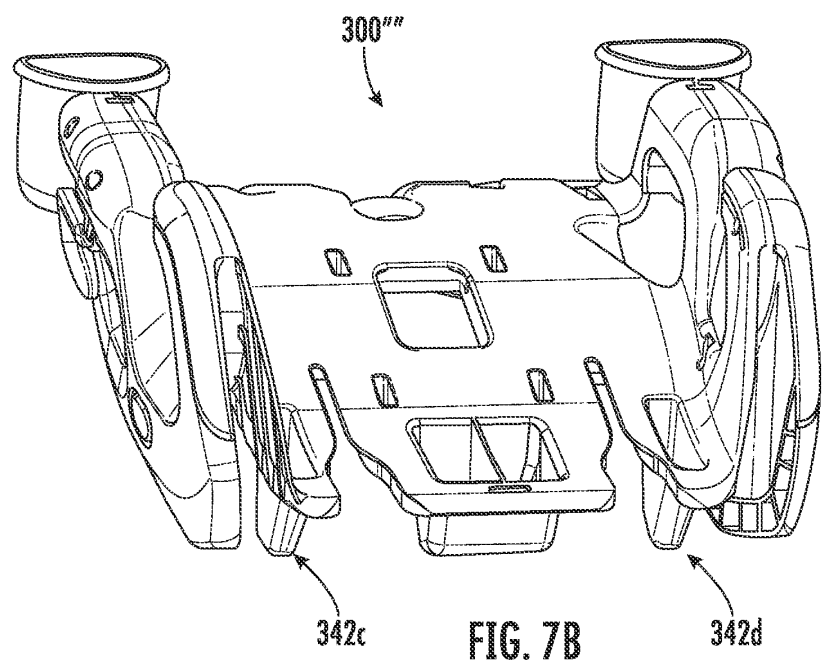
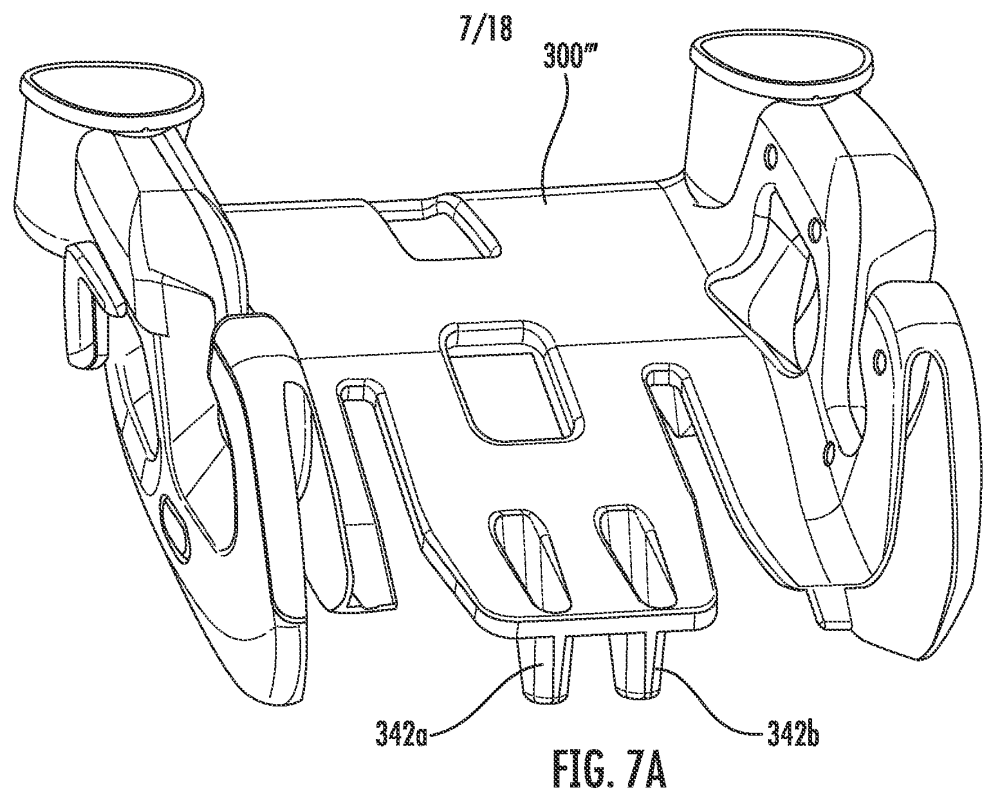
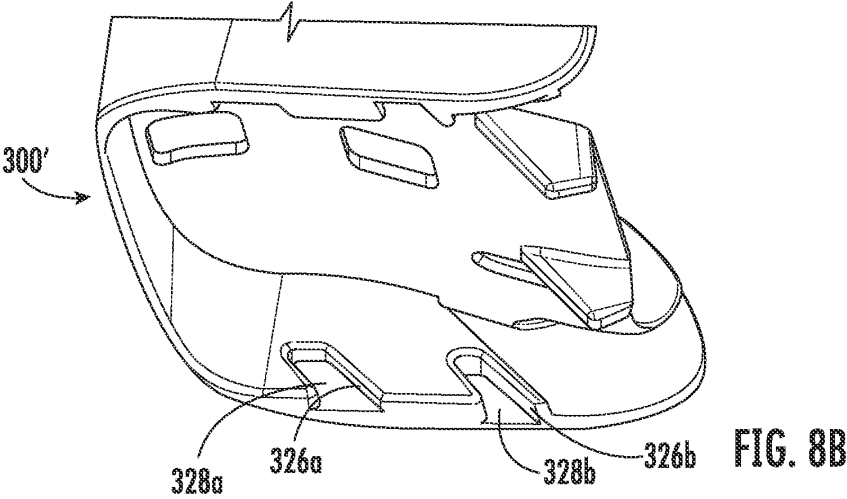
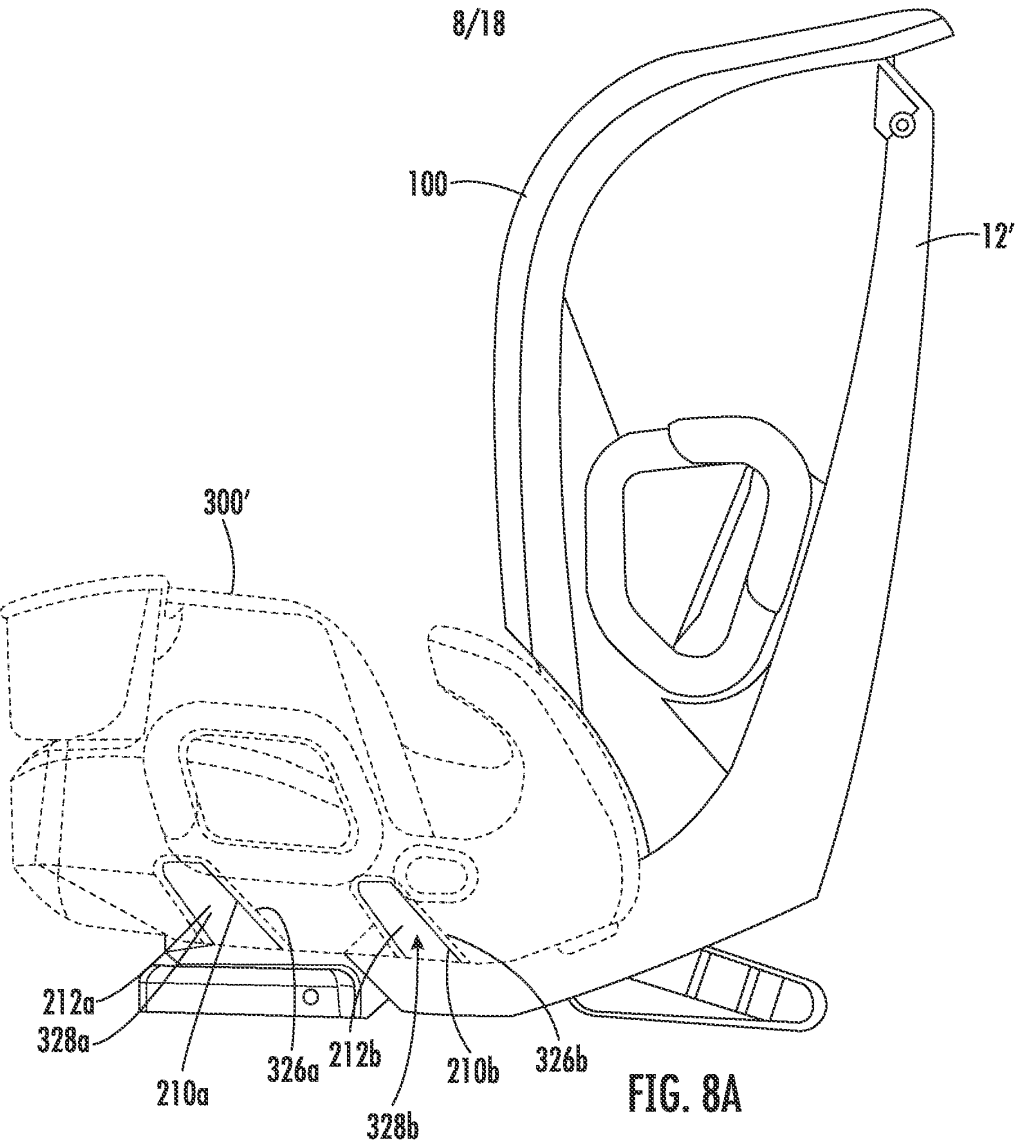


FIG. 5







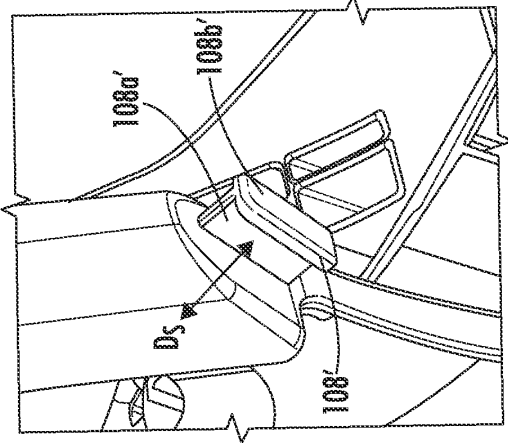


FIG. 10

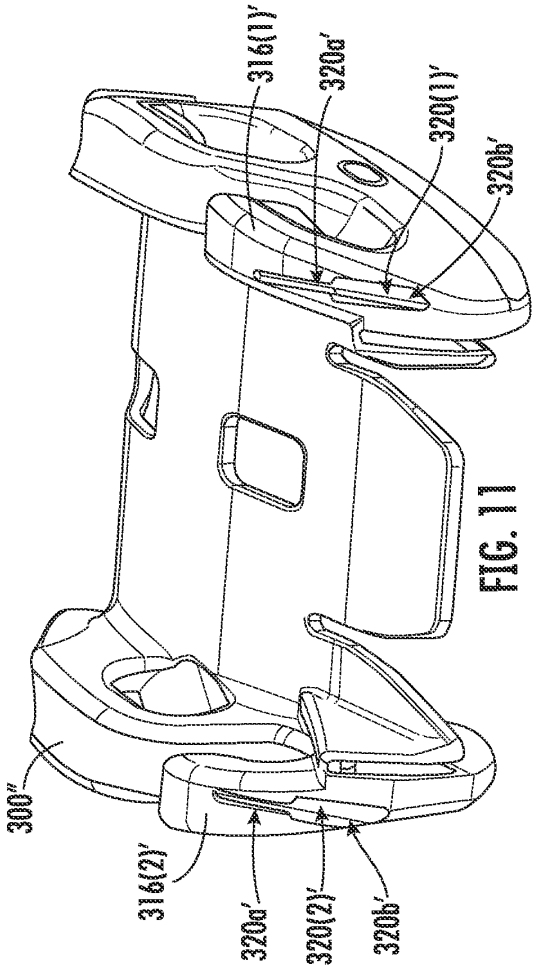


FIG. 11

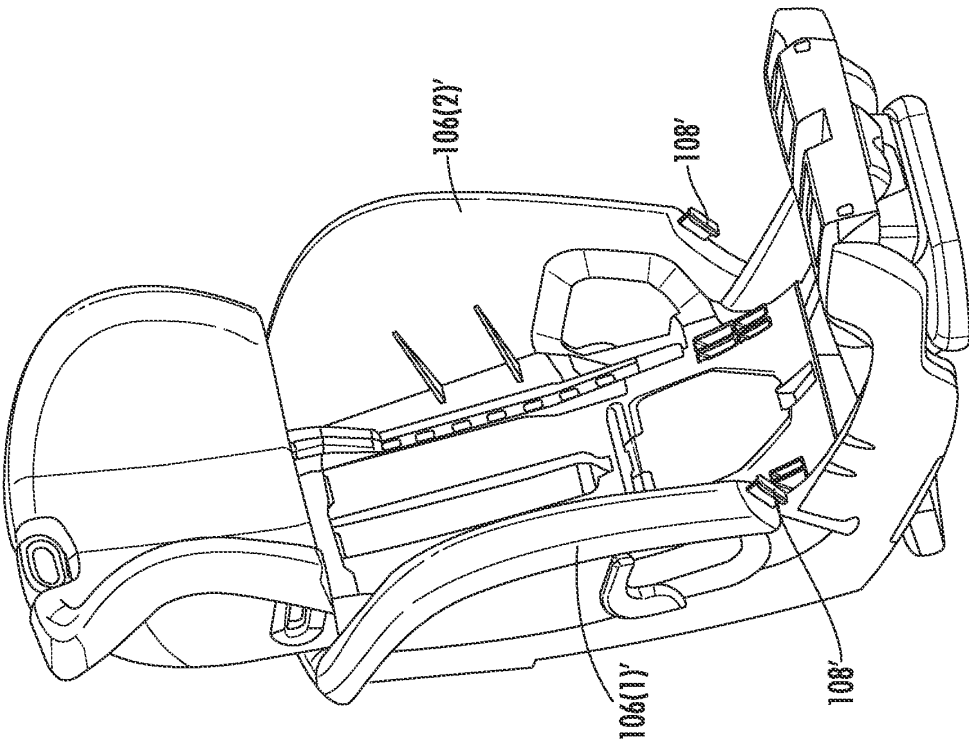
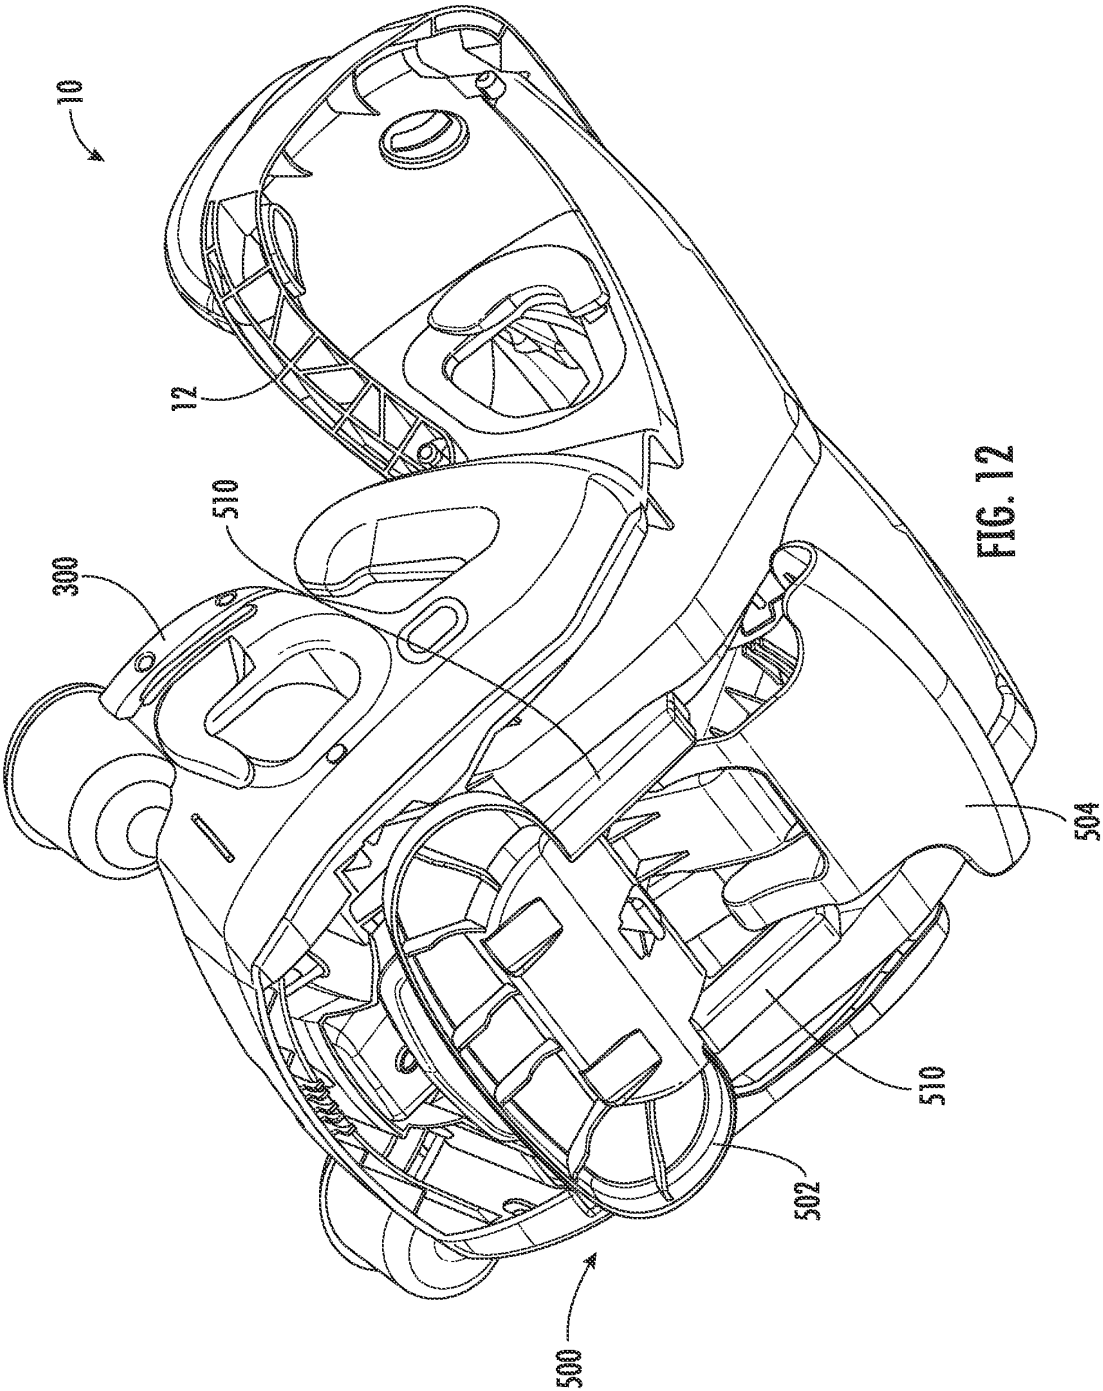


FIG. 9



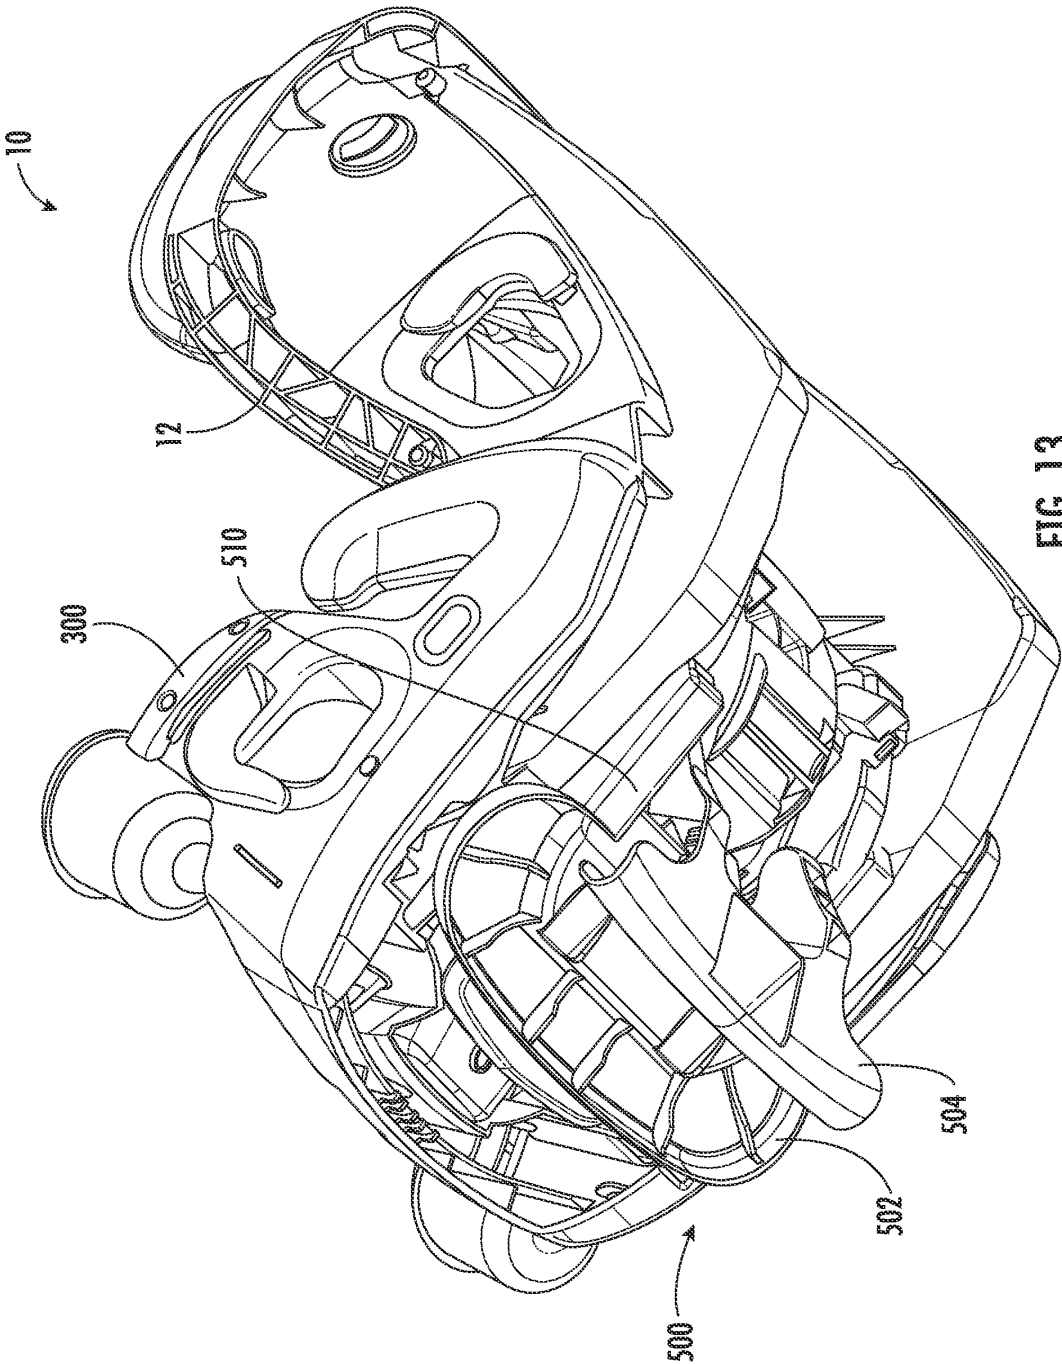


FIG. 13

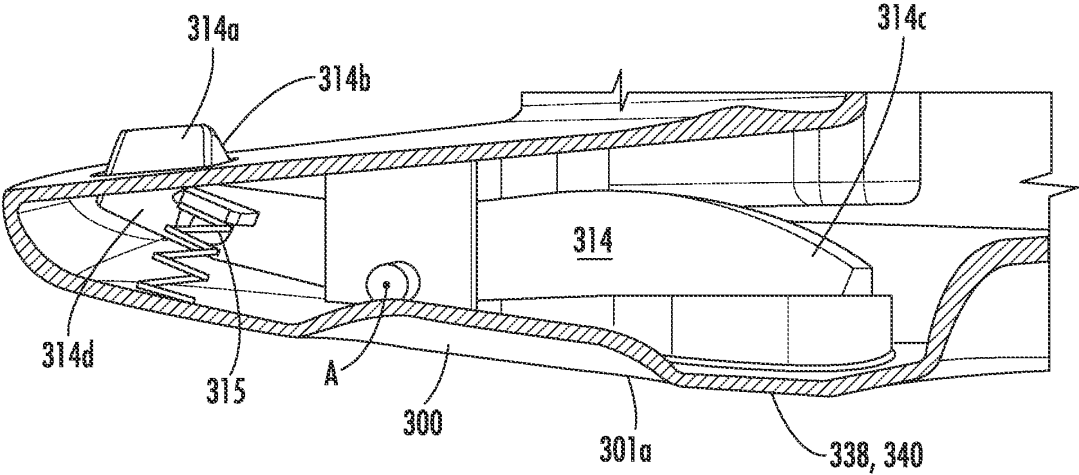


FIG. 14

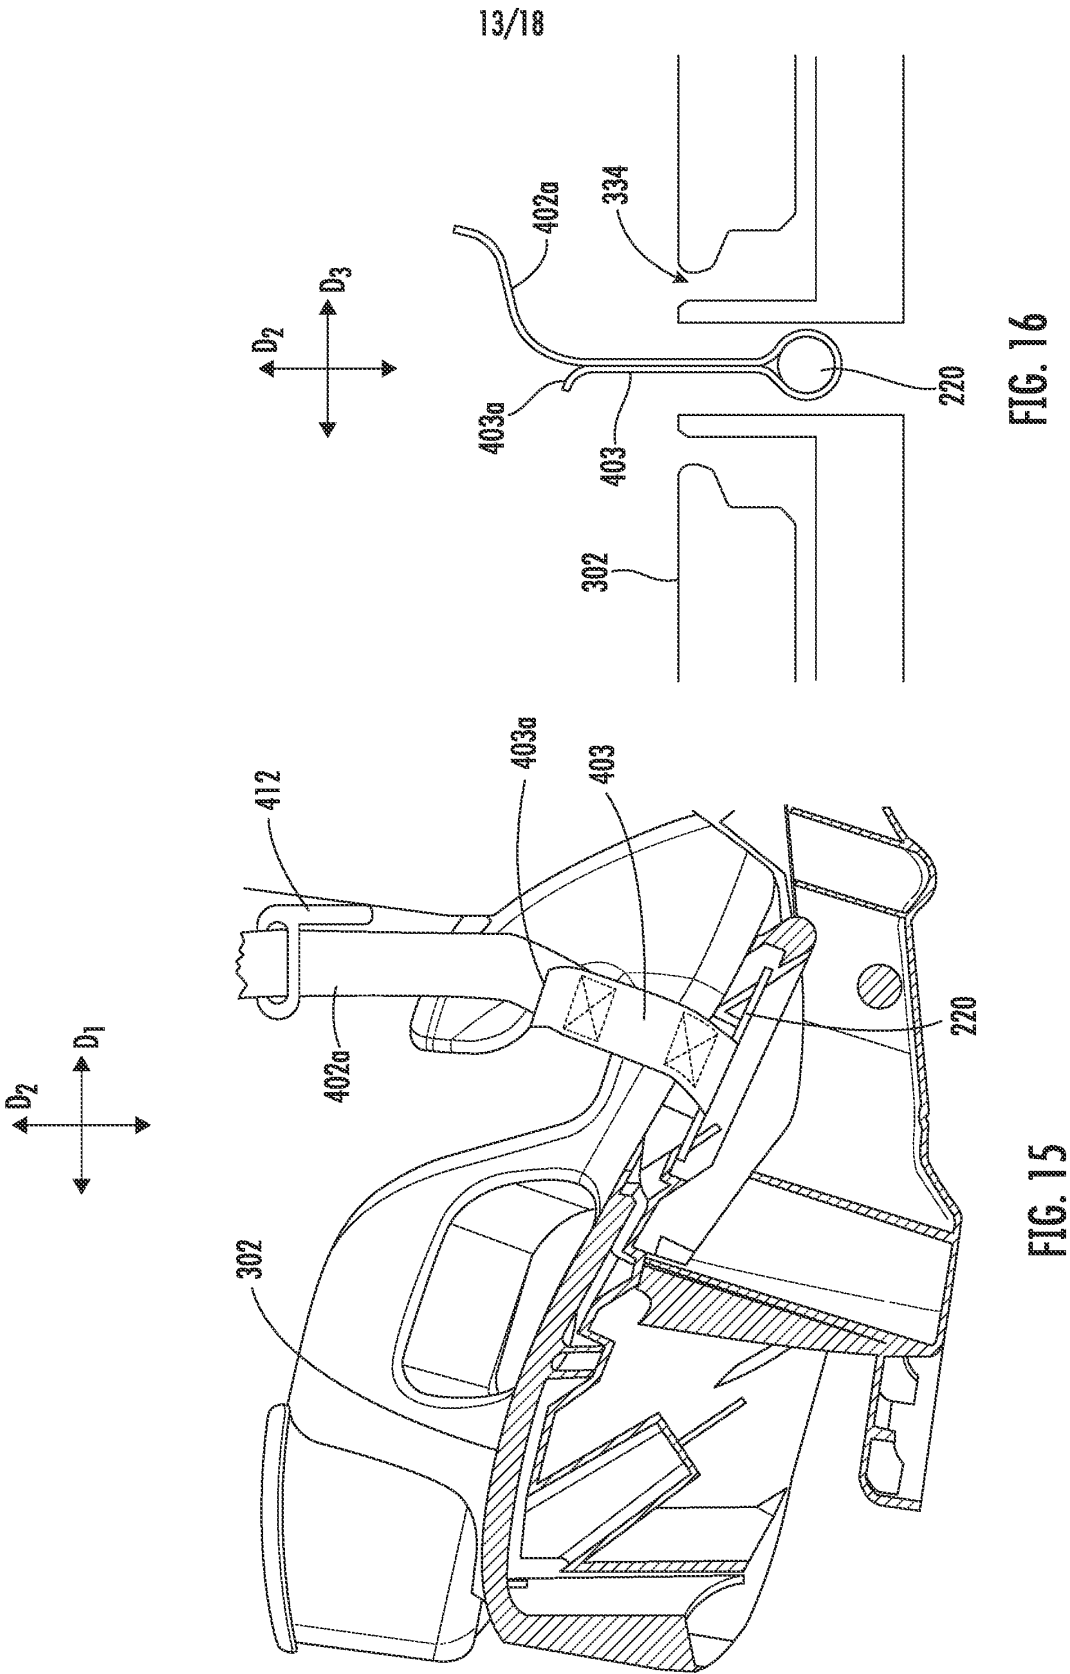


FIG. 16

FIG. 15

14/18

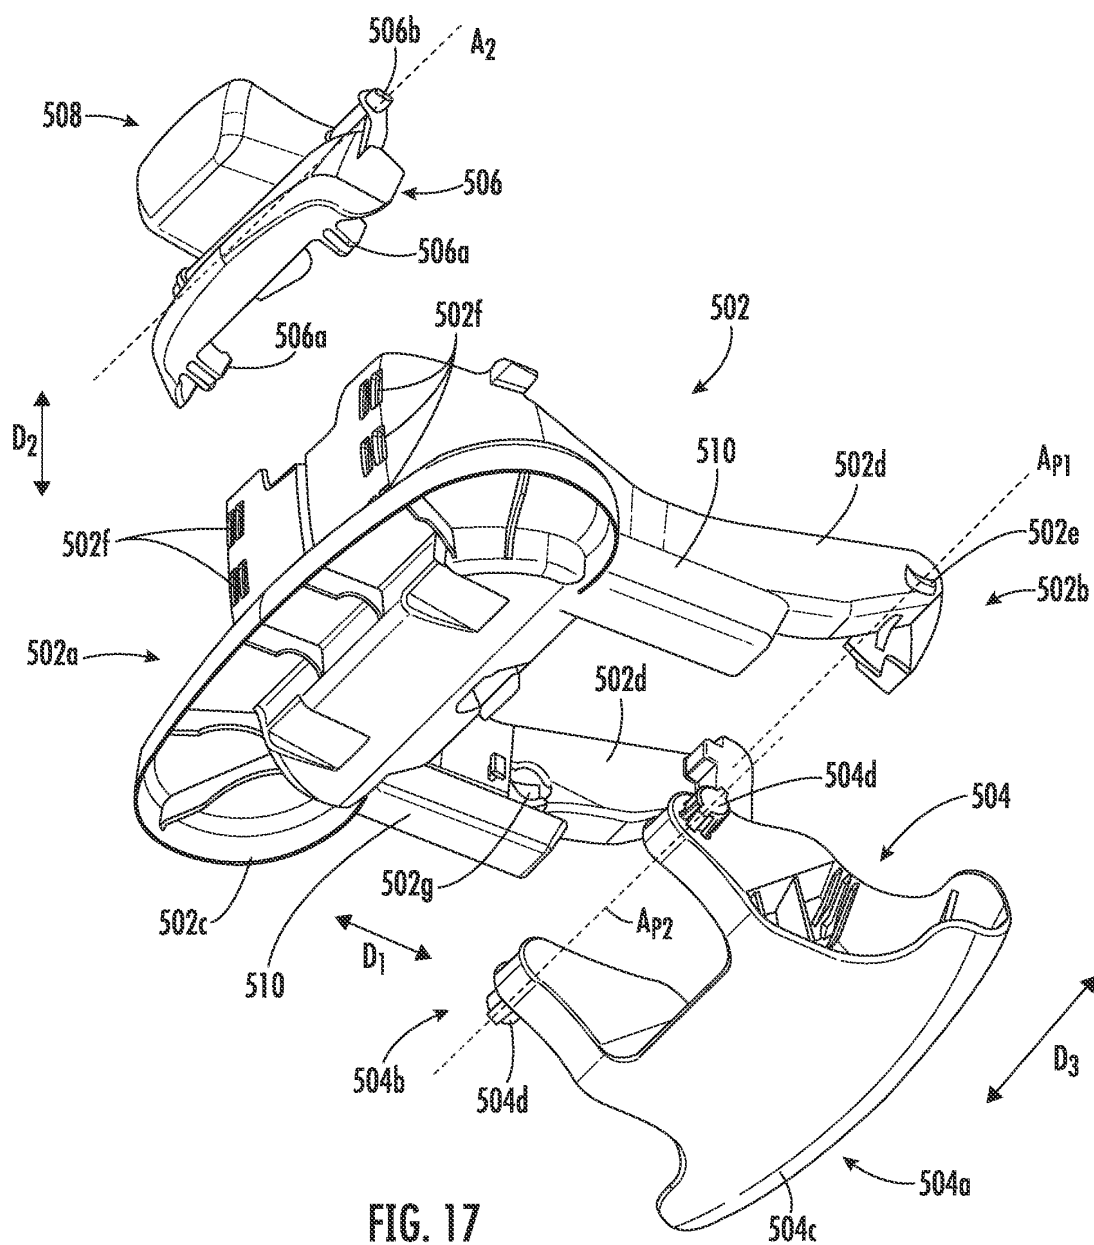


FIG. 17

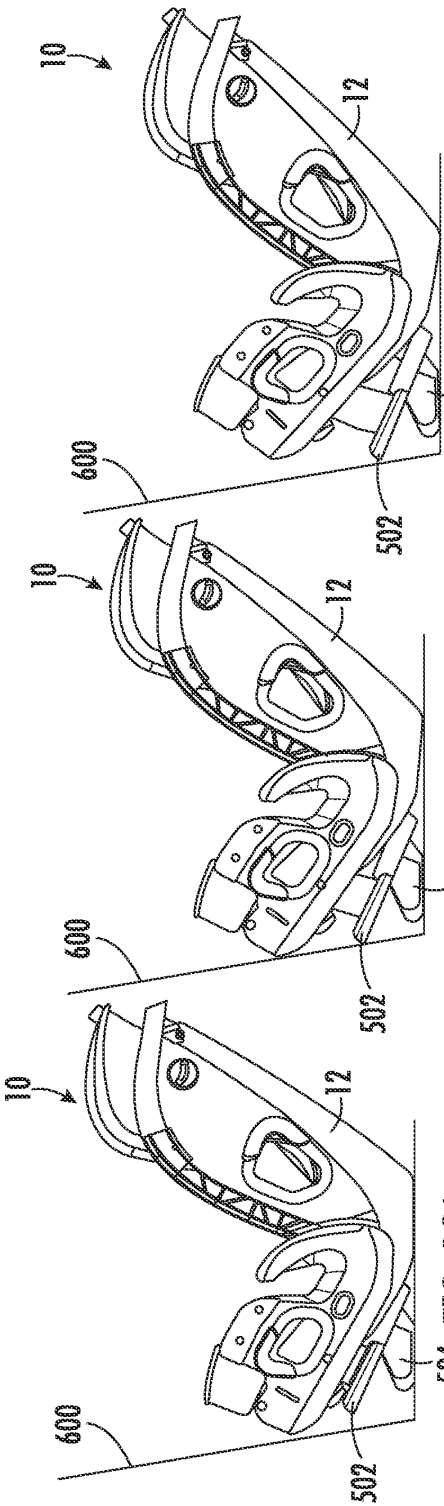


FIG. 18C

FIG. 18B

FIG. 18A

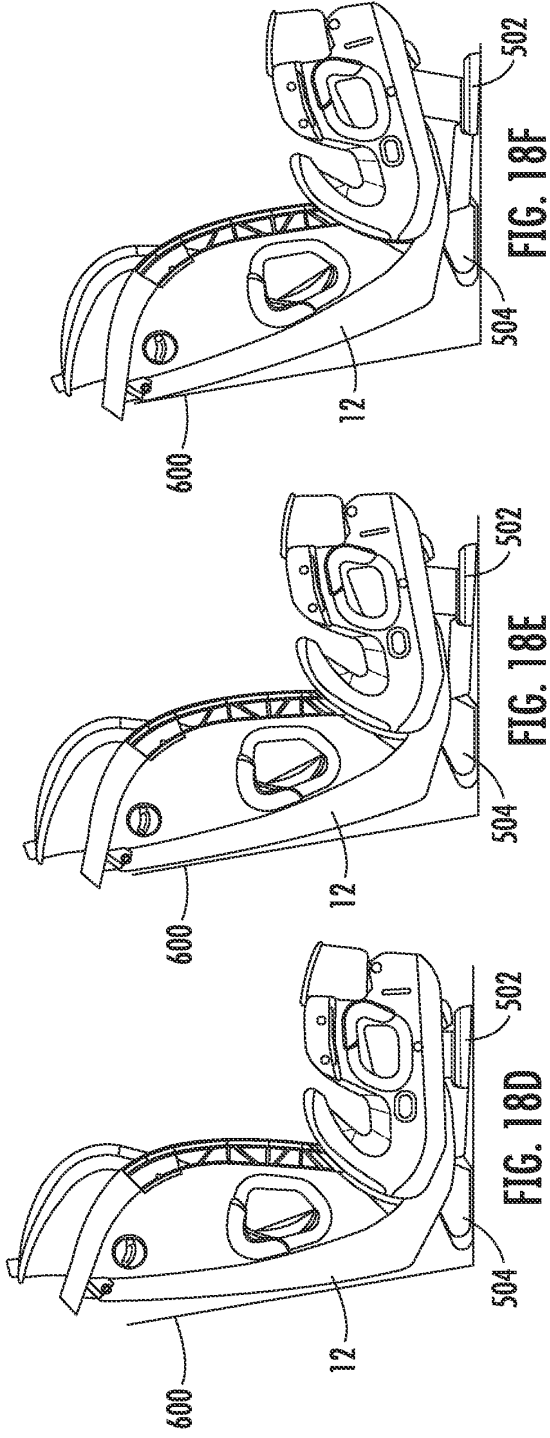


FIG. 18F

FIG. 18E

FIG. 18D

16/18

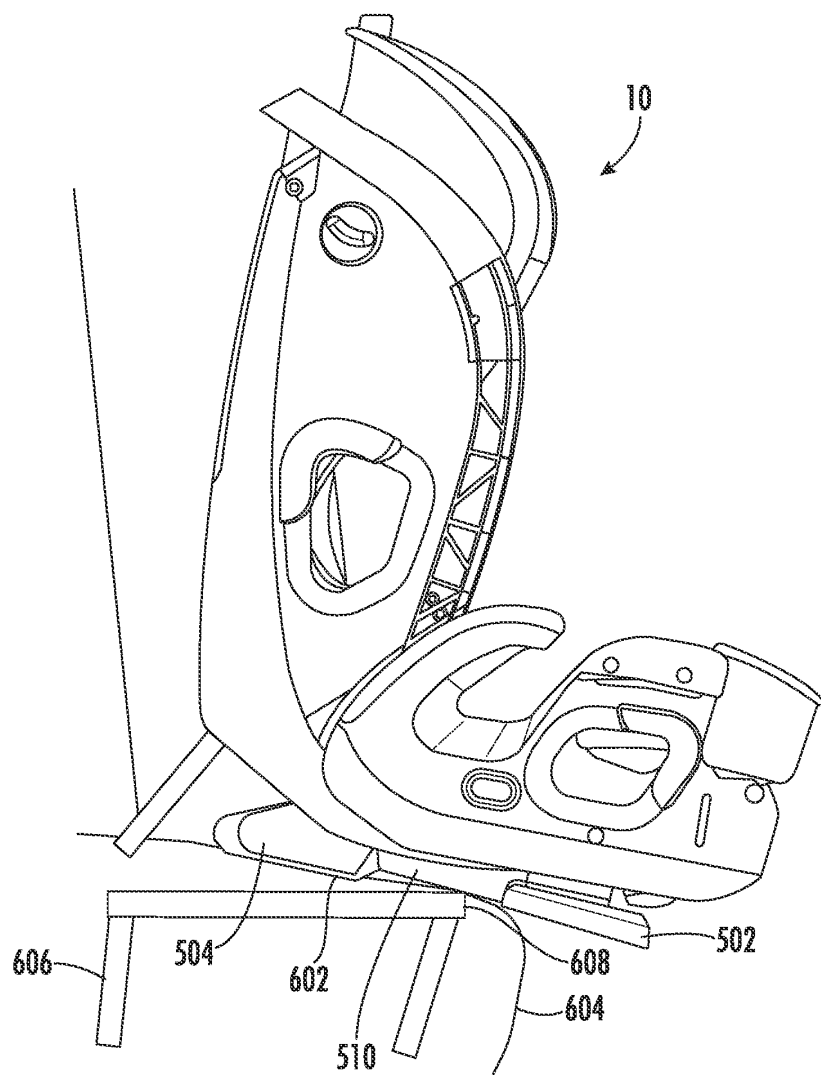


FIG. 19

17/18

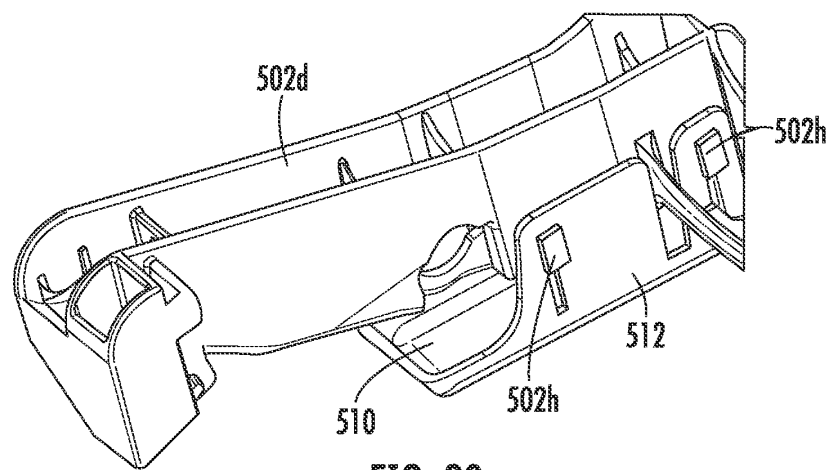


FIG. 20

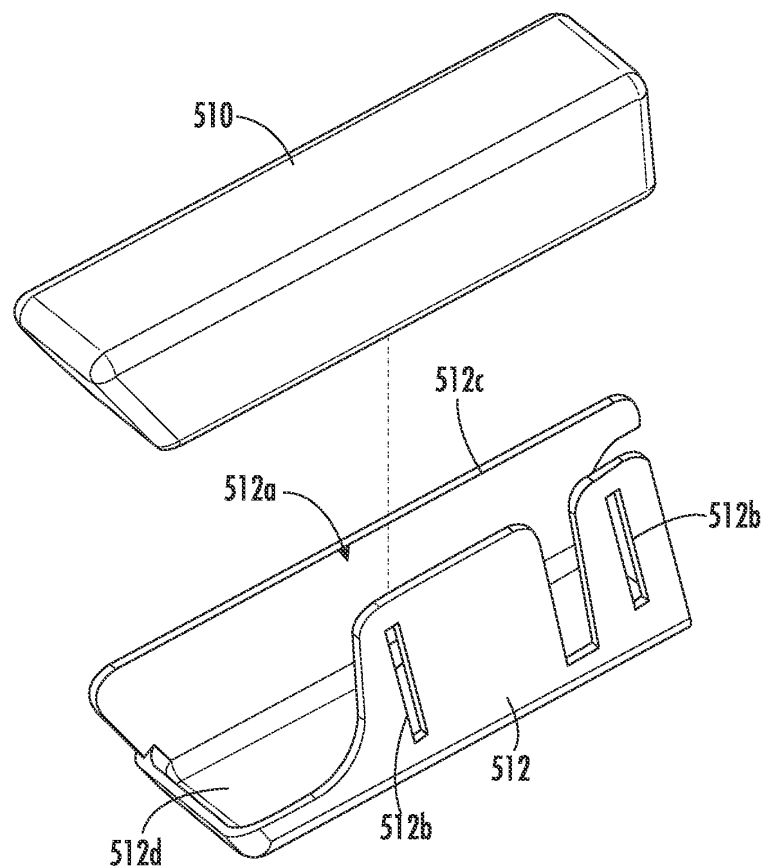


FIG. 21

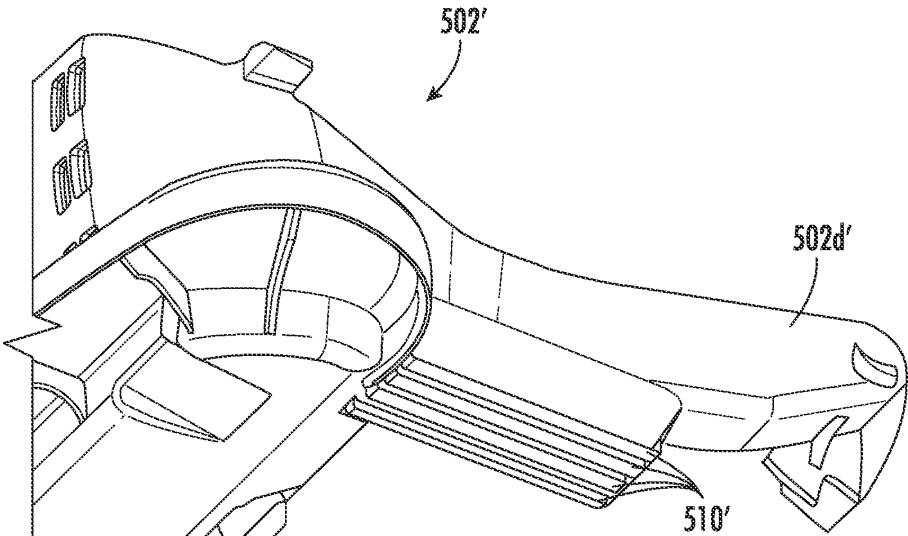


FIG. 22