

FIG. 1

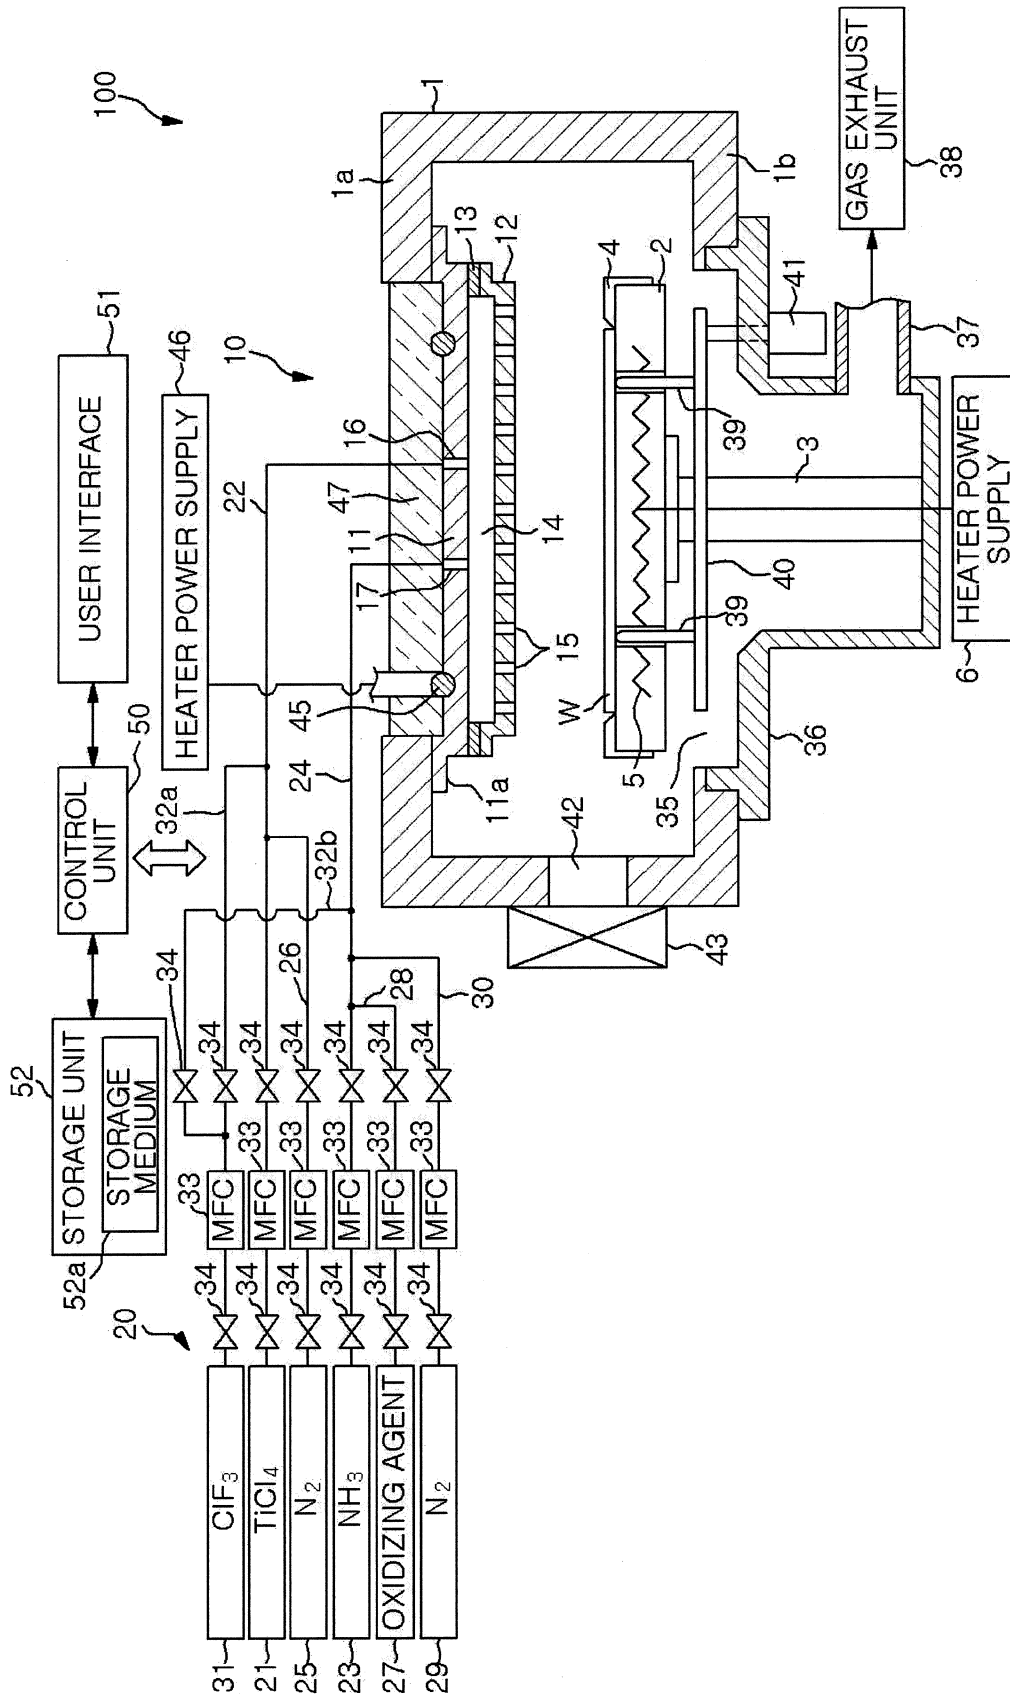


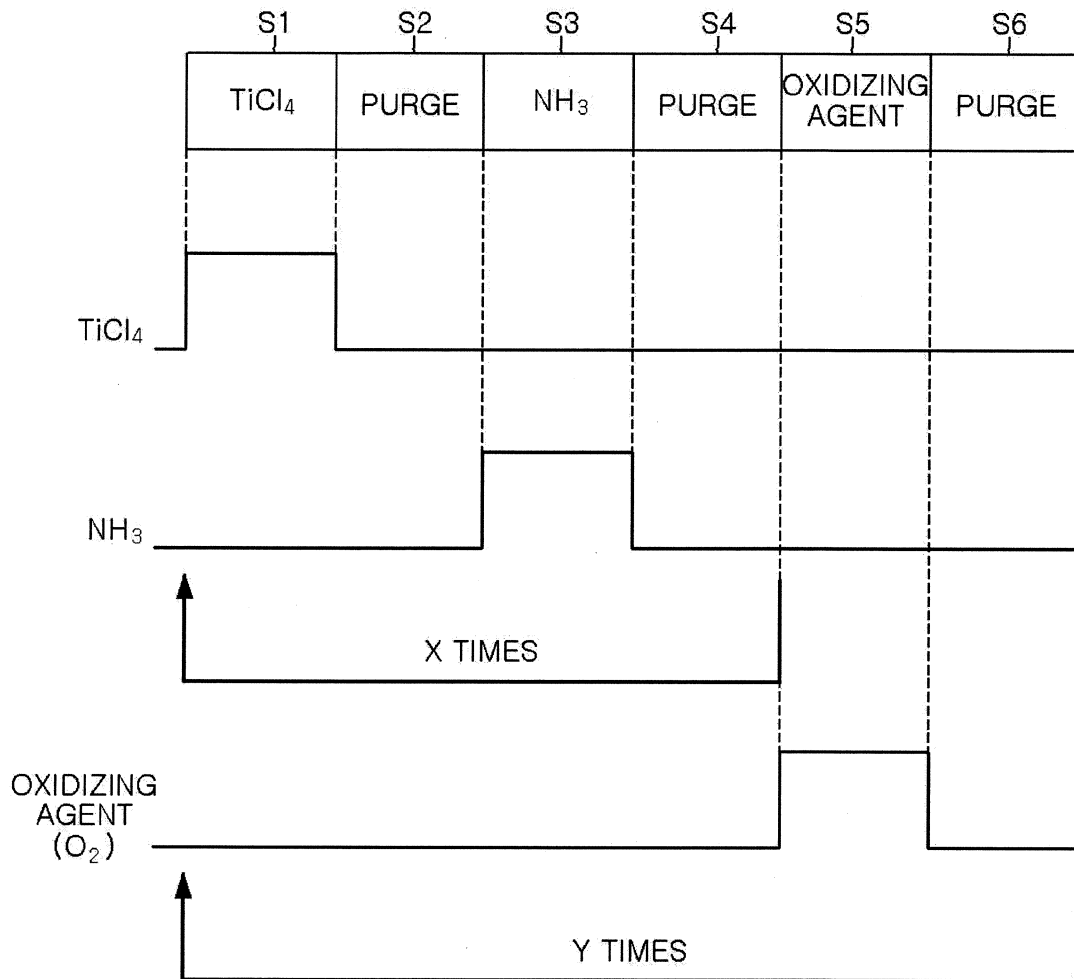
FIG. 2

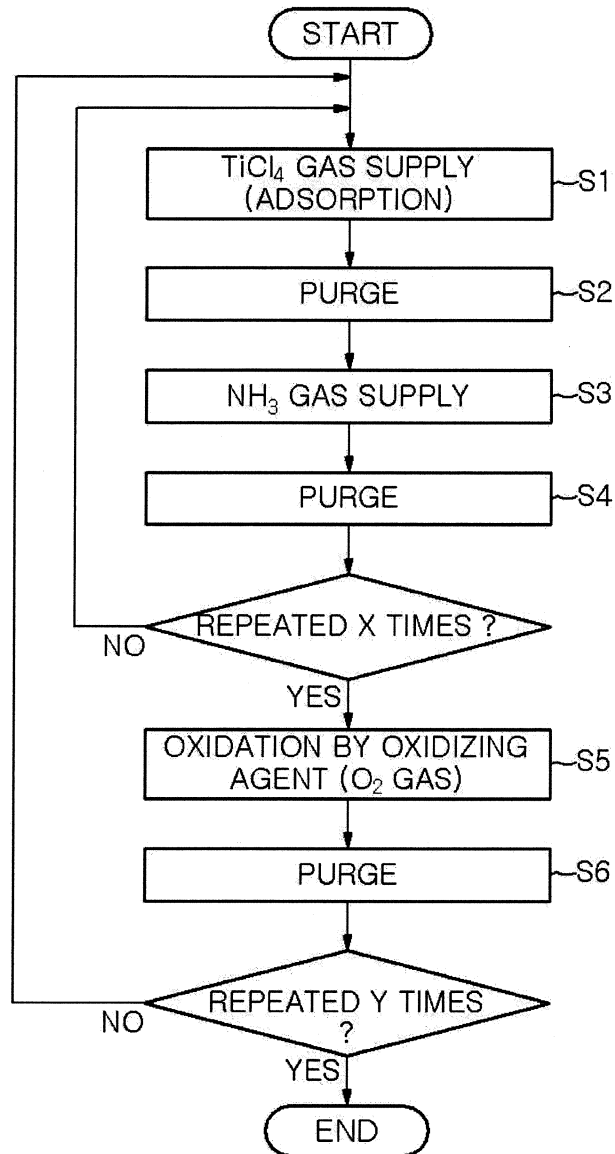
FIG. 3

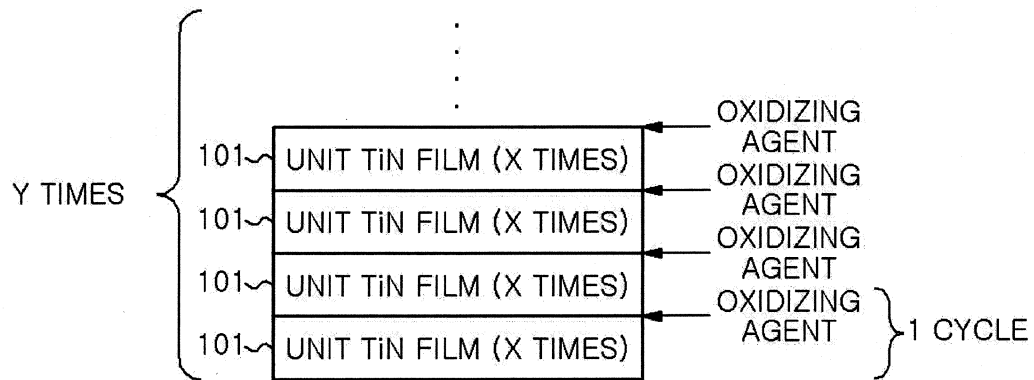
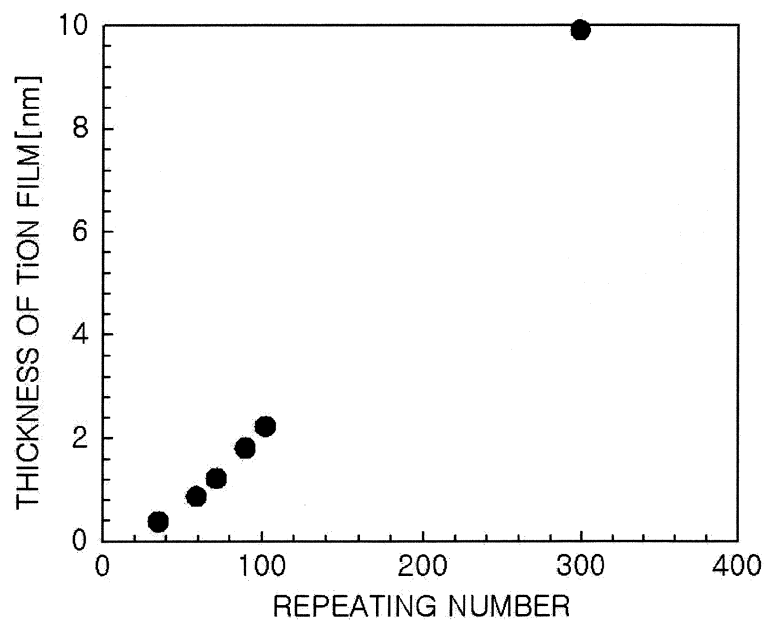
FIG. 4**FIG. 5**

FIG. 6

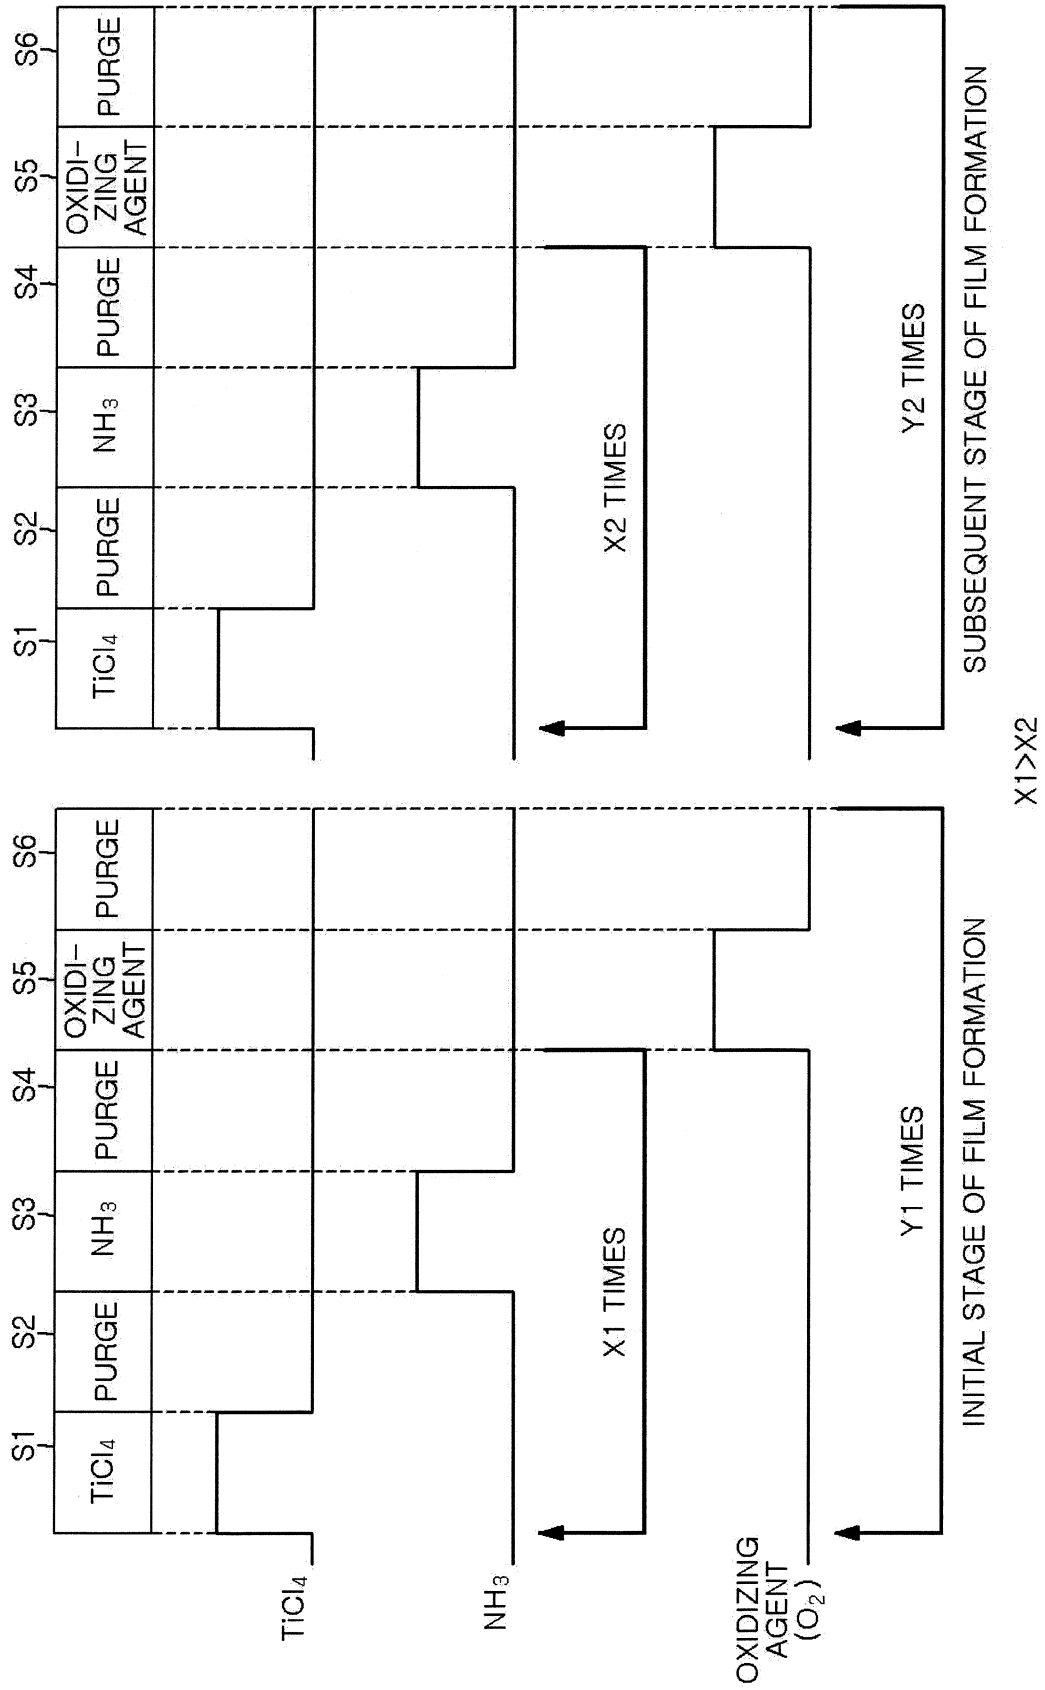


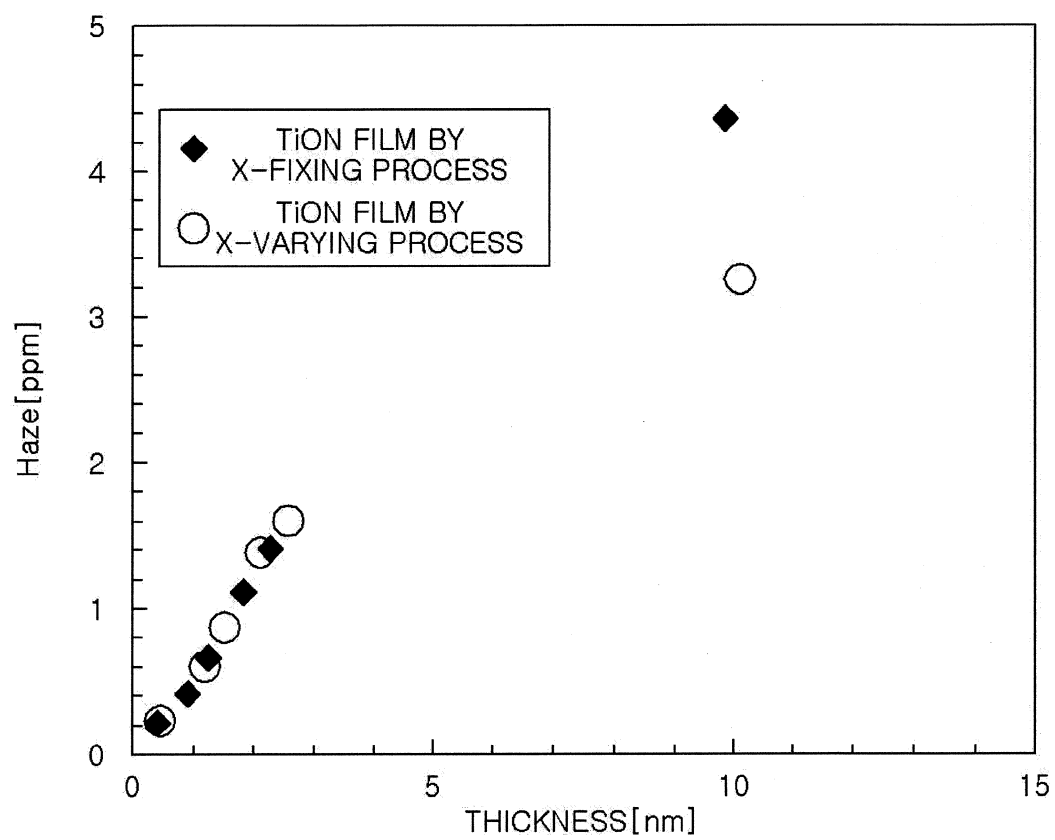
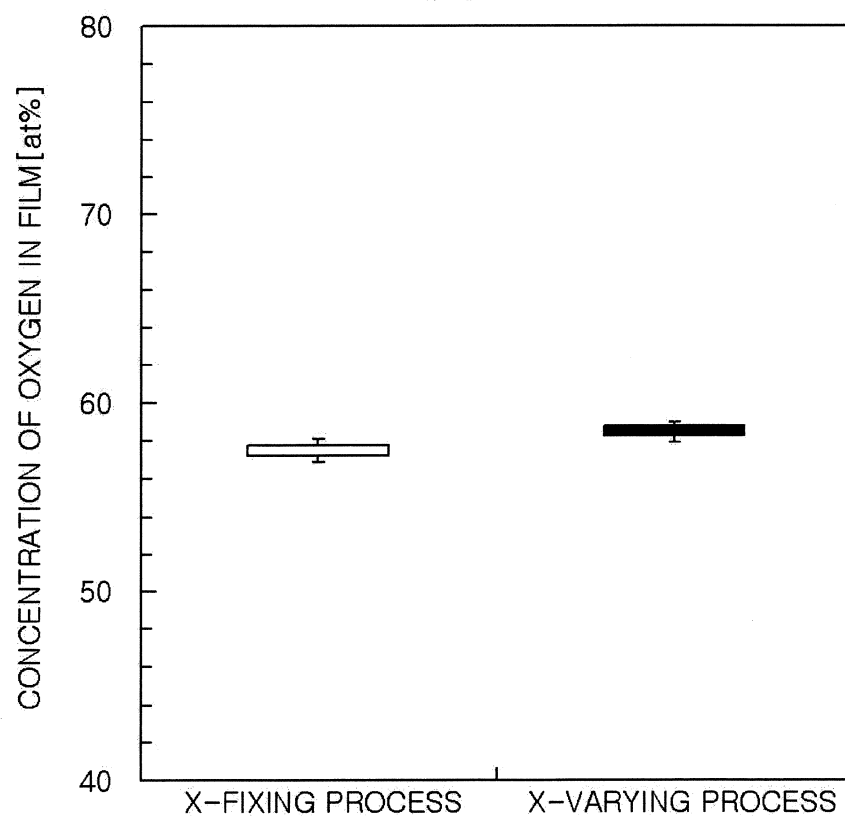
FIG. 7**FIG. 8**

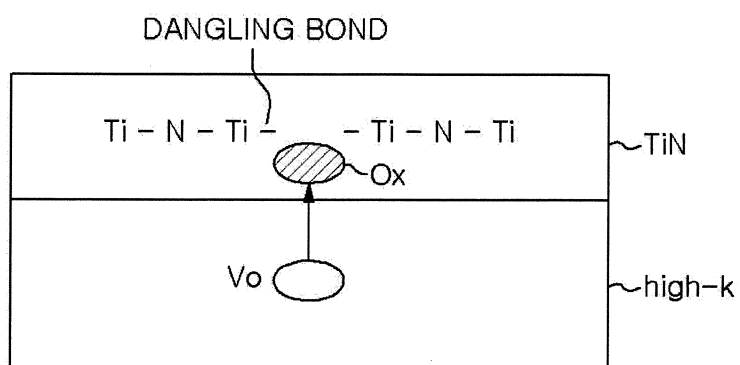
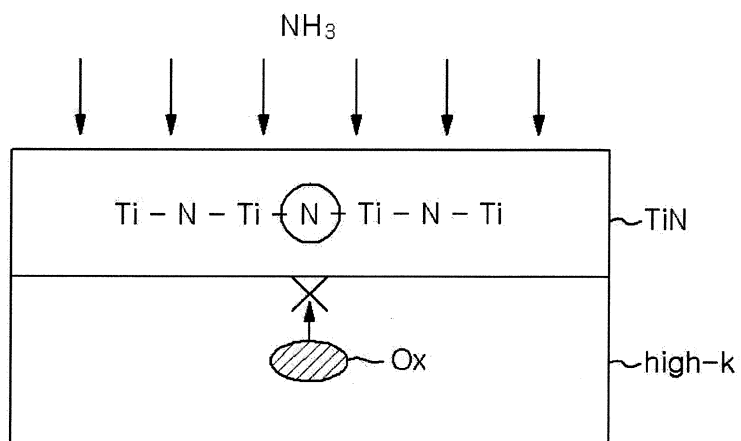
FIG. 9A**FIG. 9B**

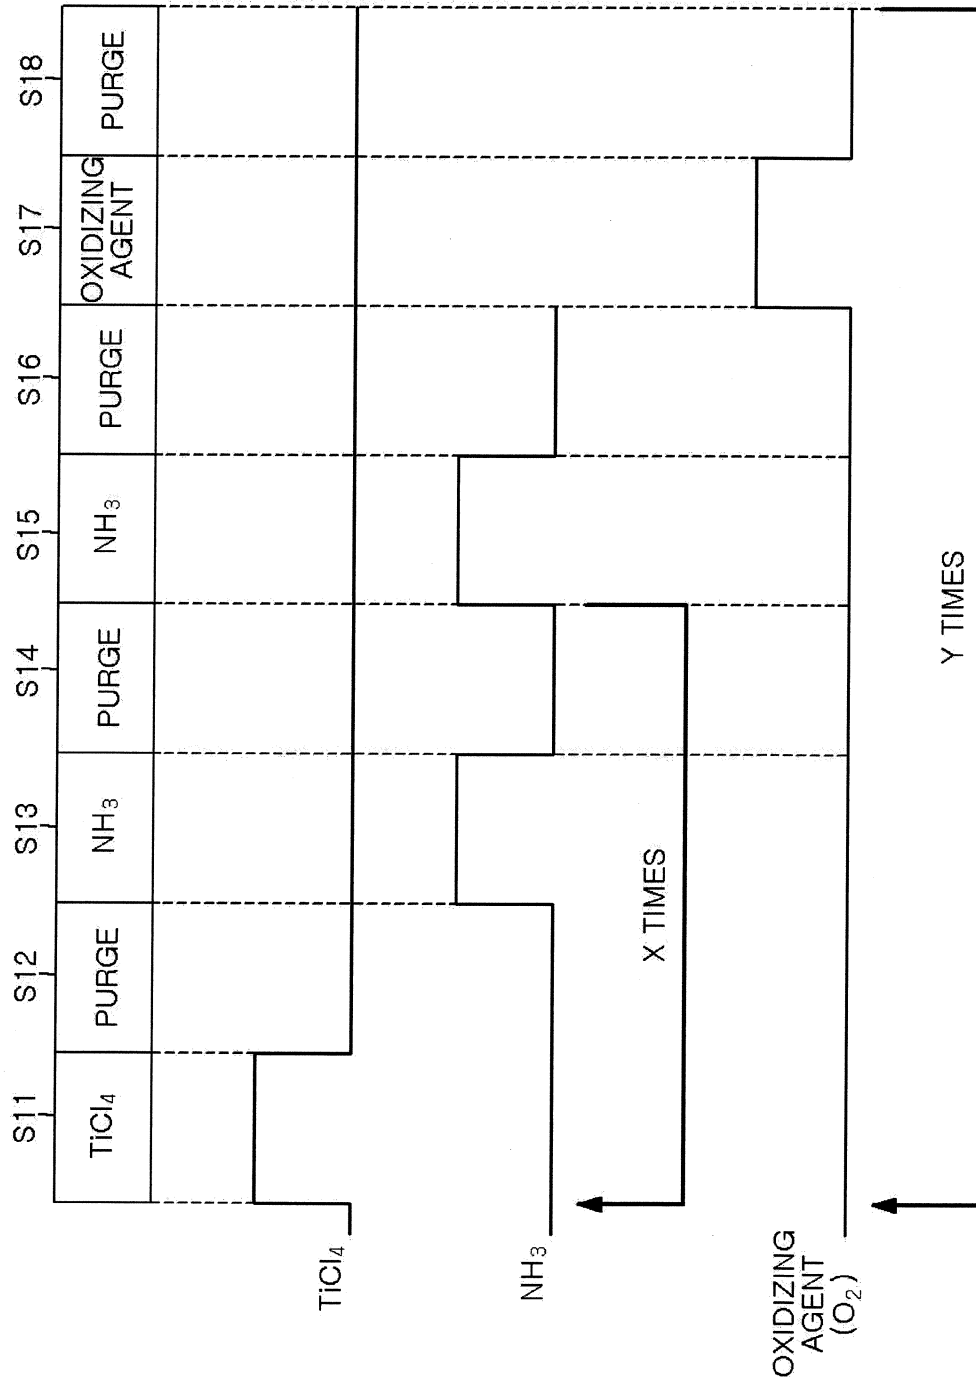
FIG. 10

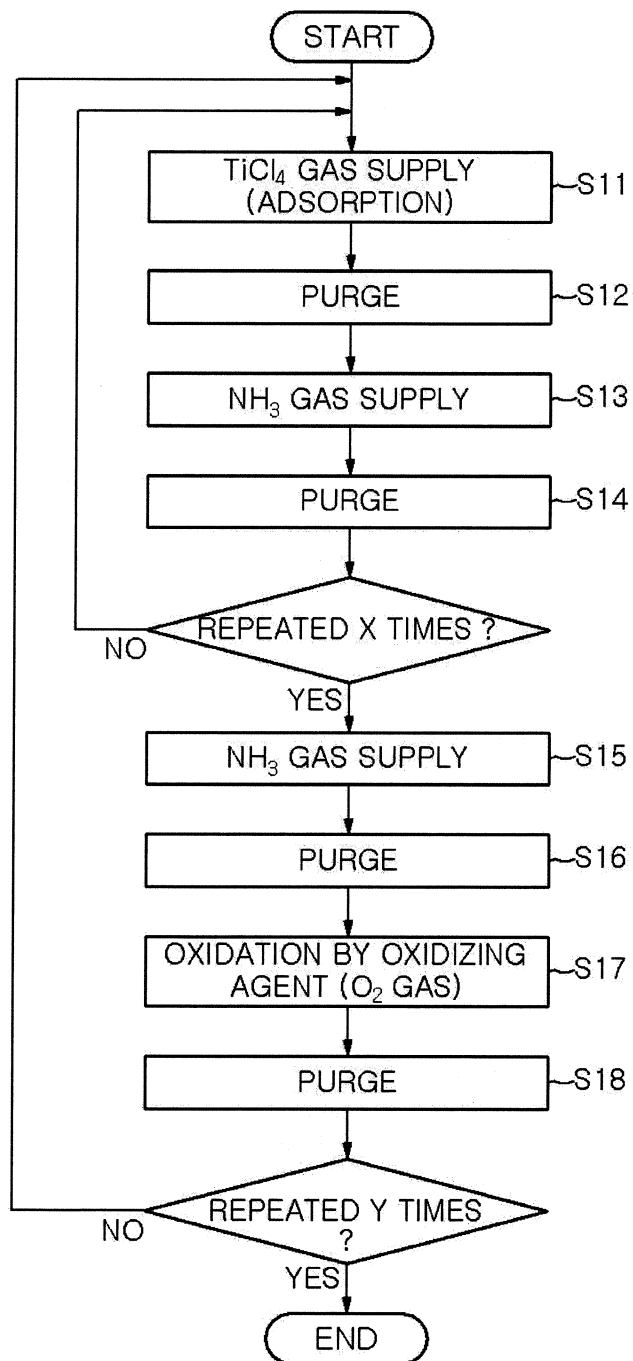
FIG. 11

FIG. 12

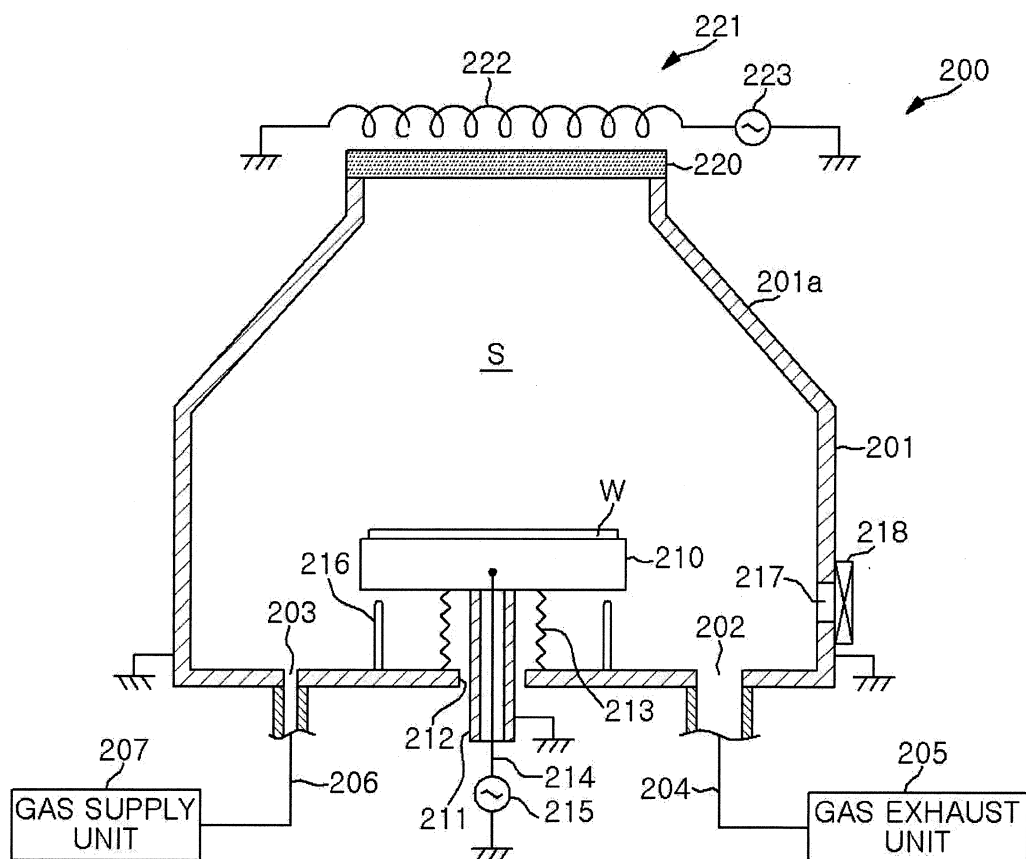
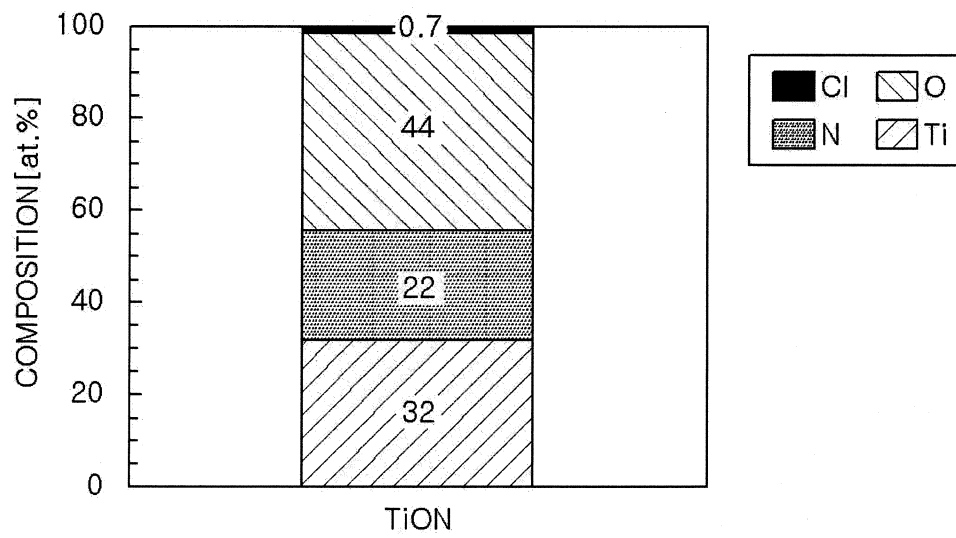
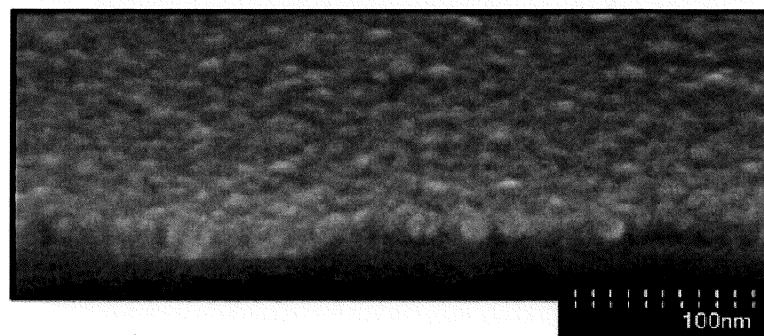


FIG. 13*FIG. 14*

12/20

FIG. 15

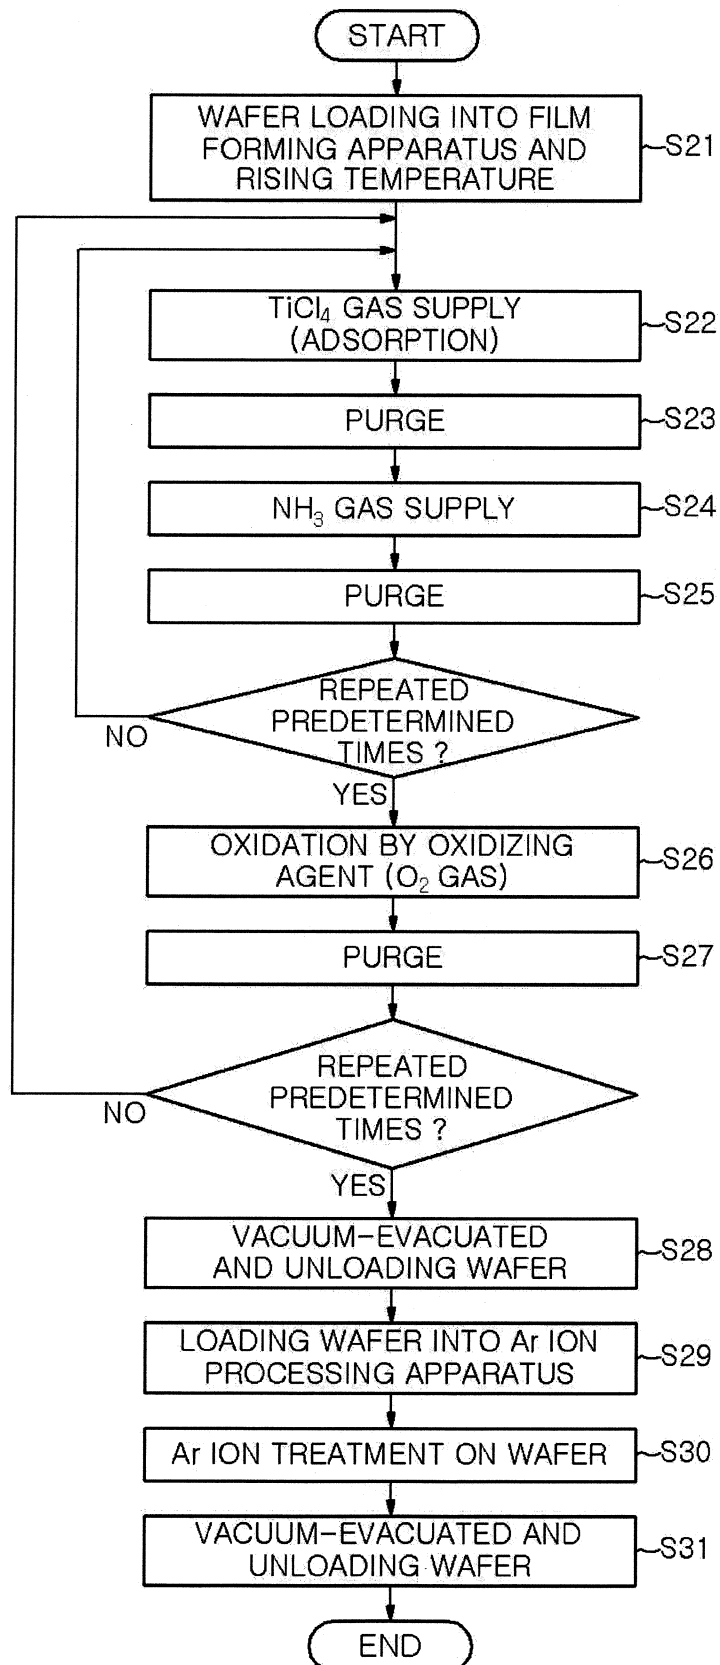


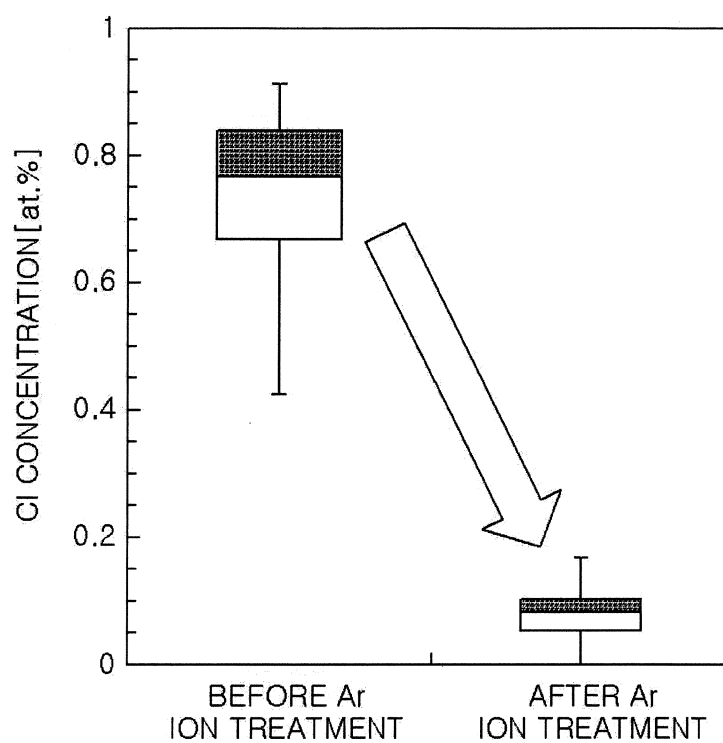
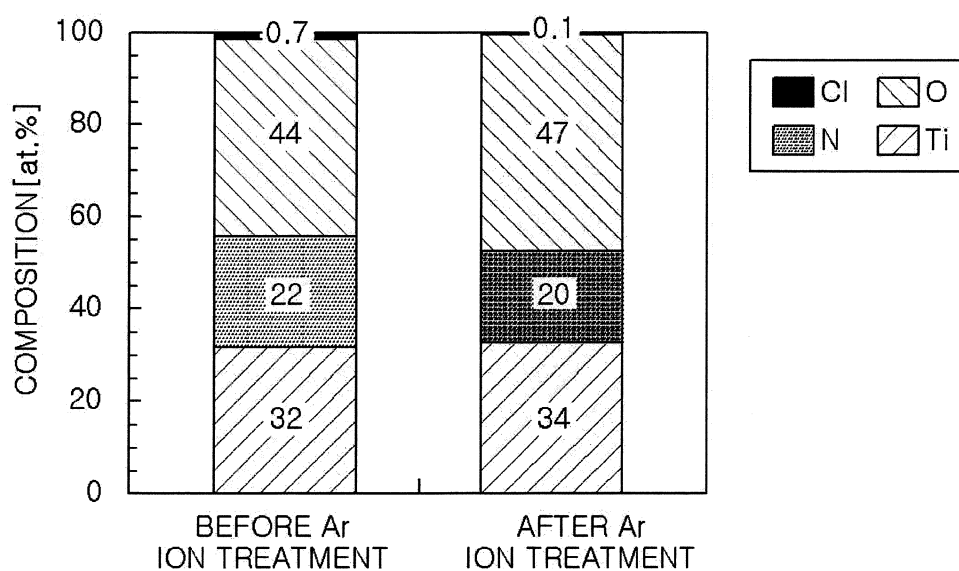
FIG. 16**FIG. 17**

FIG. 18A

BEFORE Ar ION TREATMENT

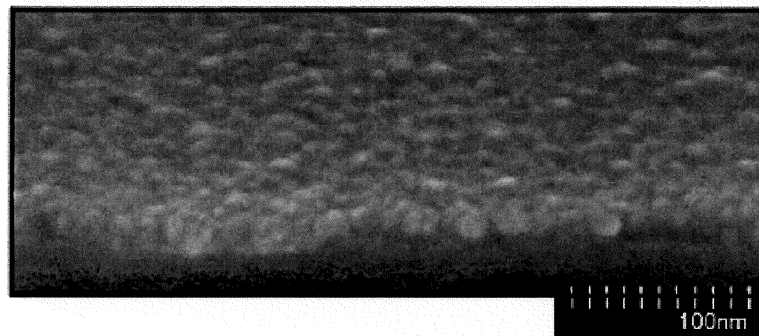


FIG. 18B

AFTER Ar ION TREATMENT



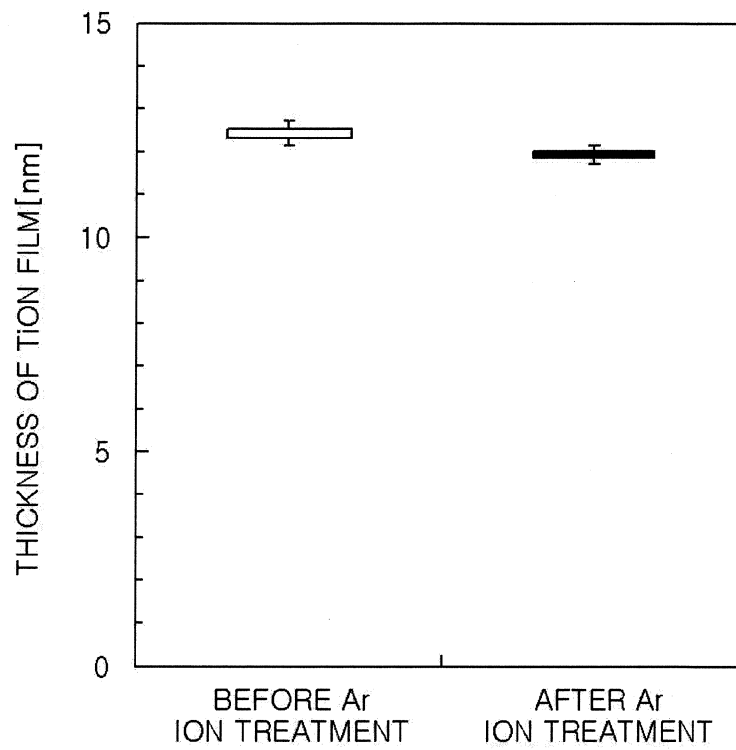
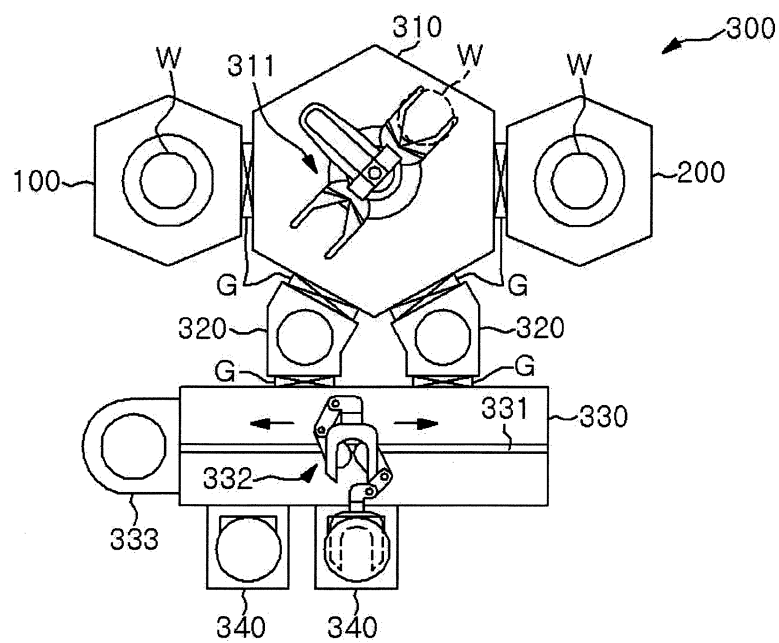
FIG. 19**FIG. 20**

FIG. 21

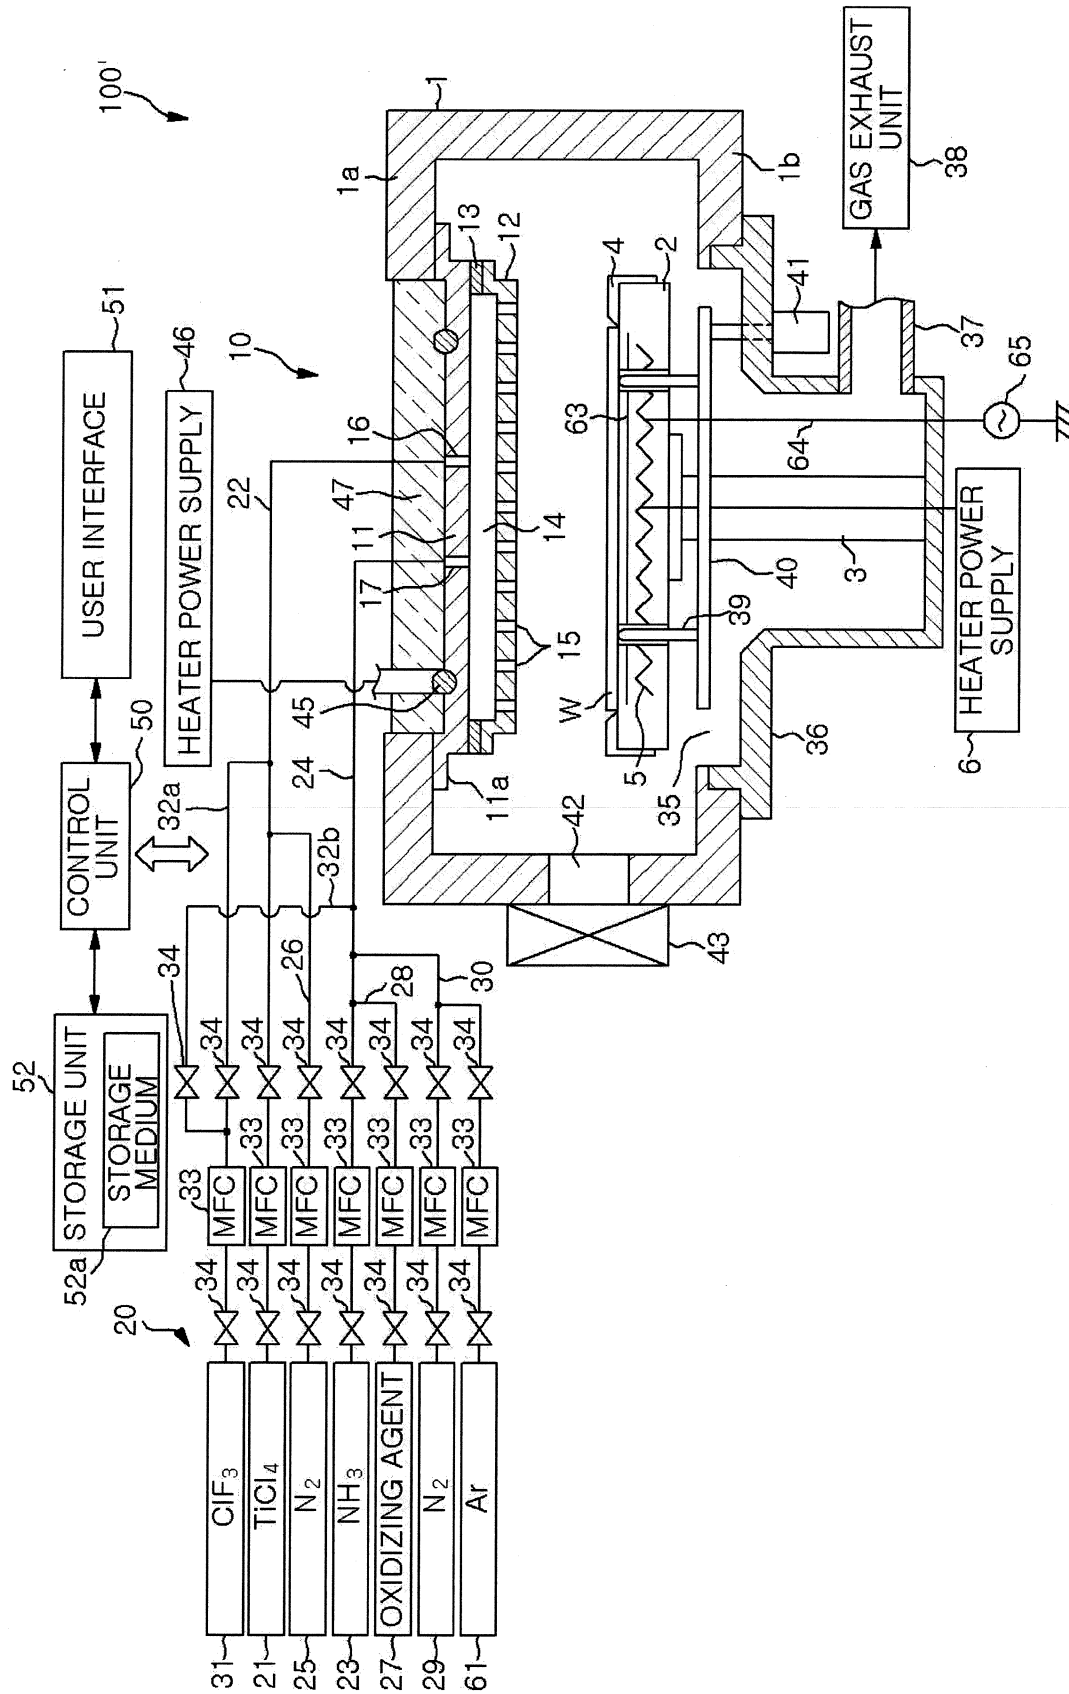


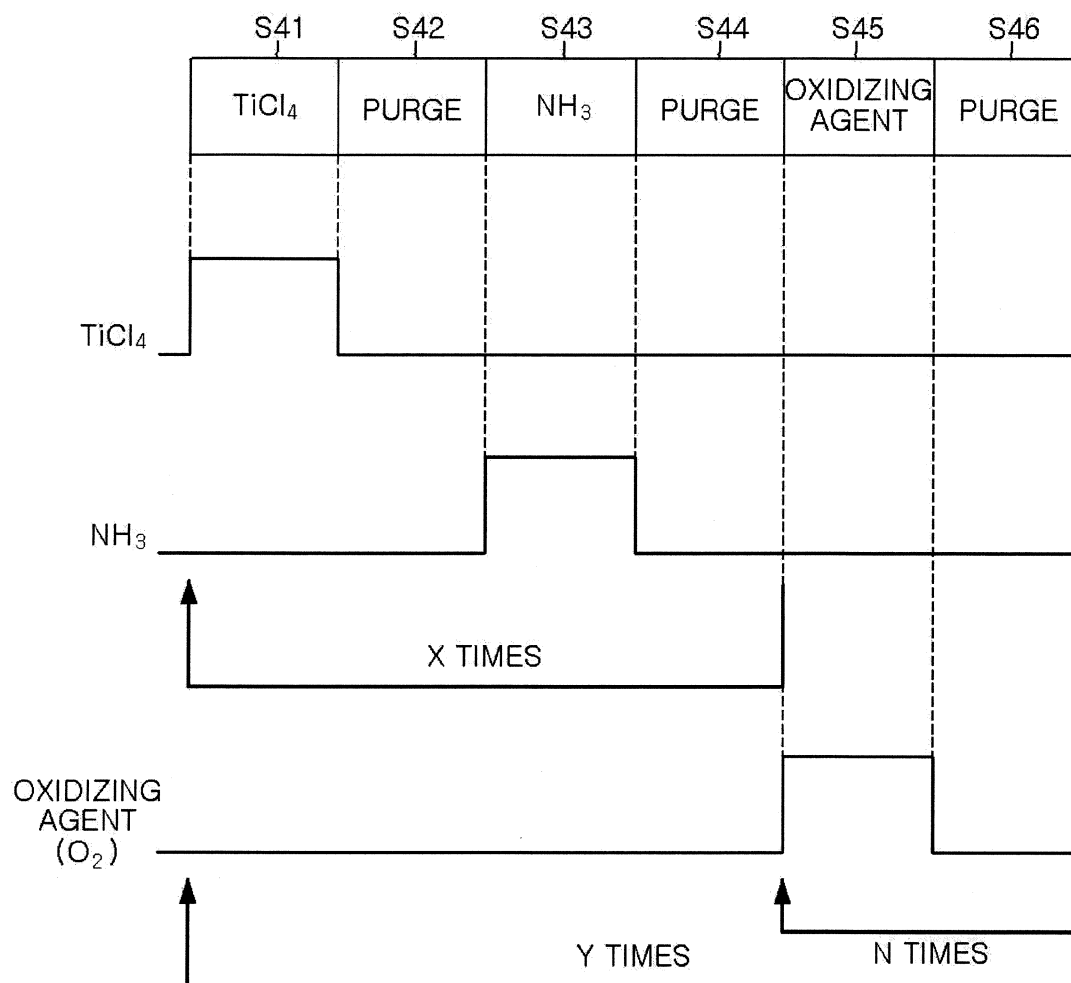
FIG.22

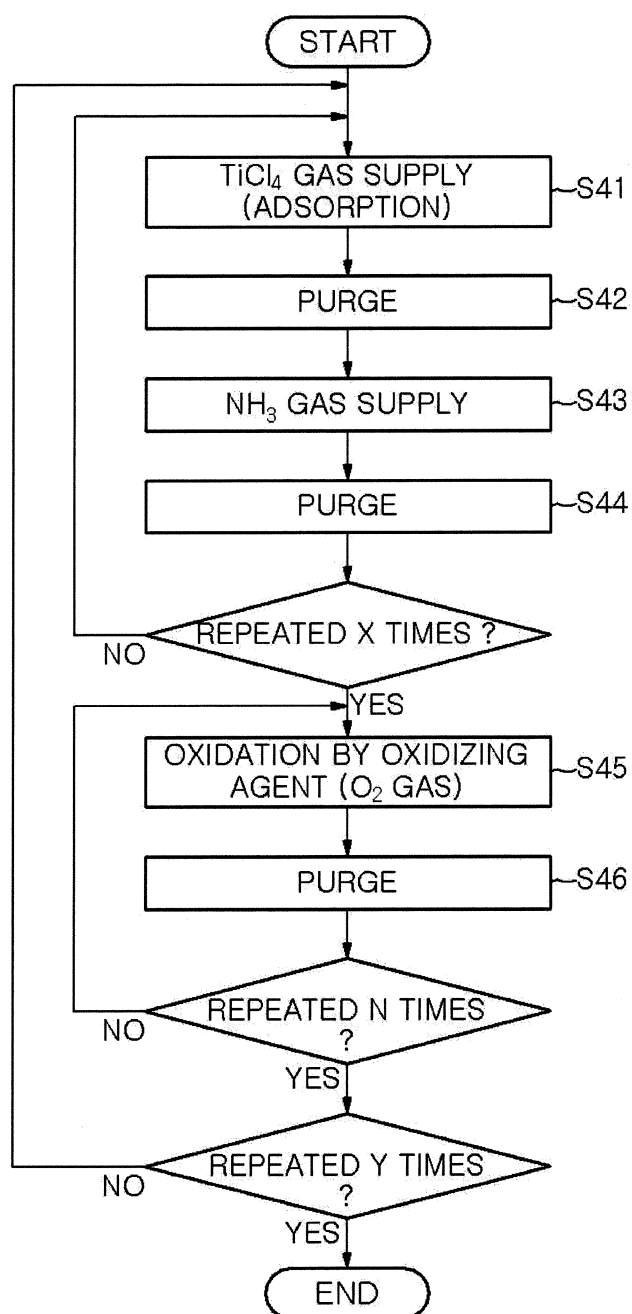
FIG.23

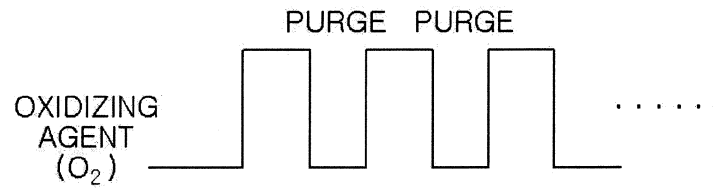
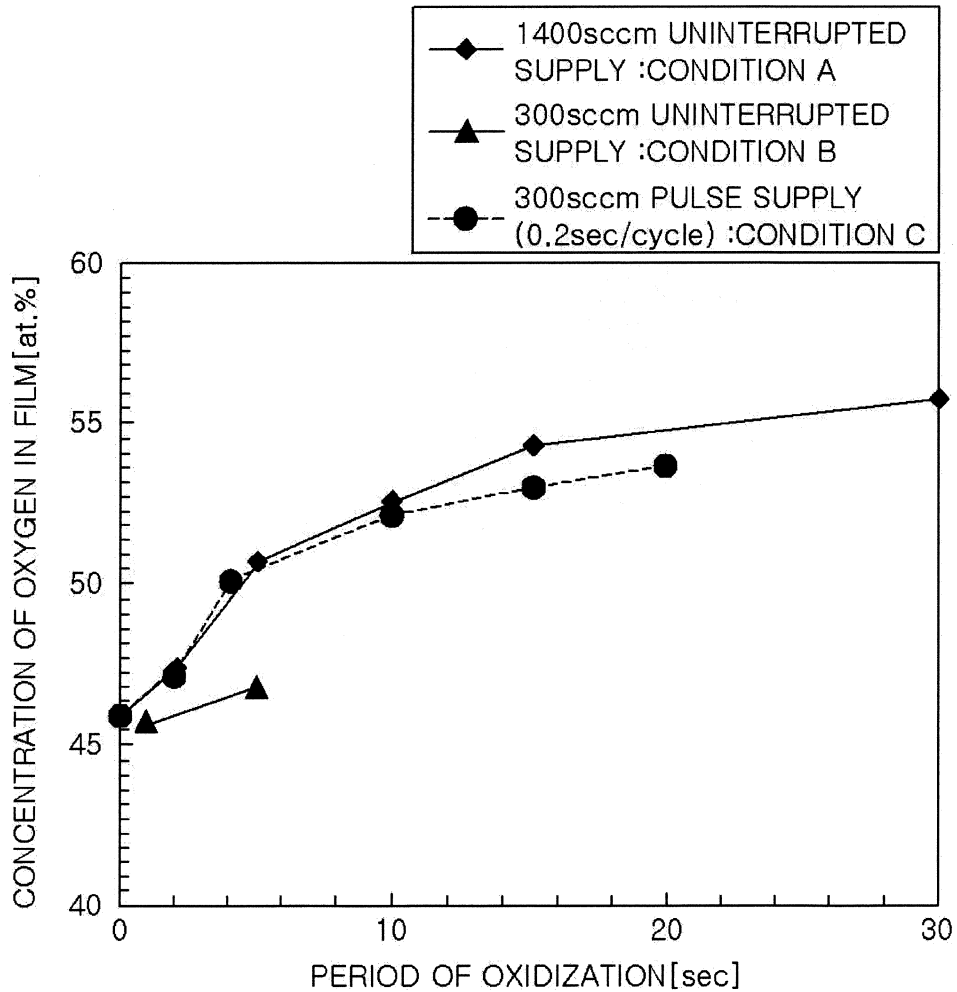
FIG.24**FIG.25**

FIG. 26

