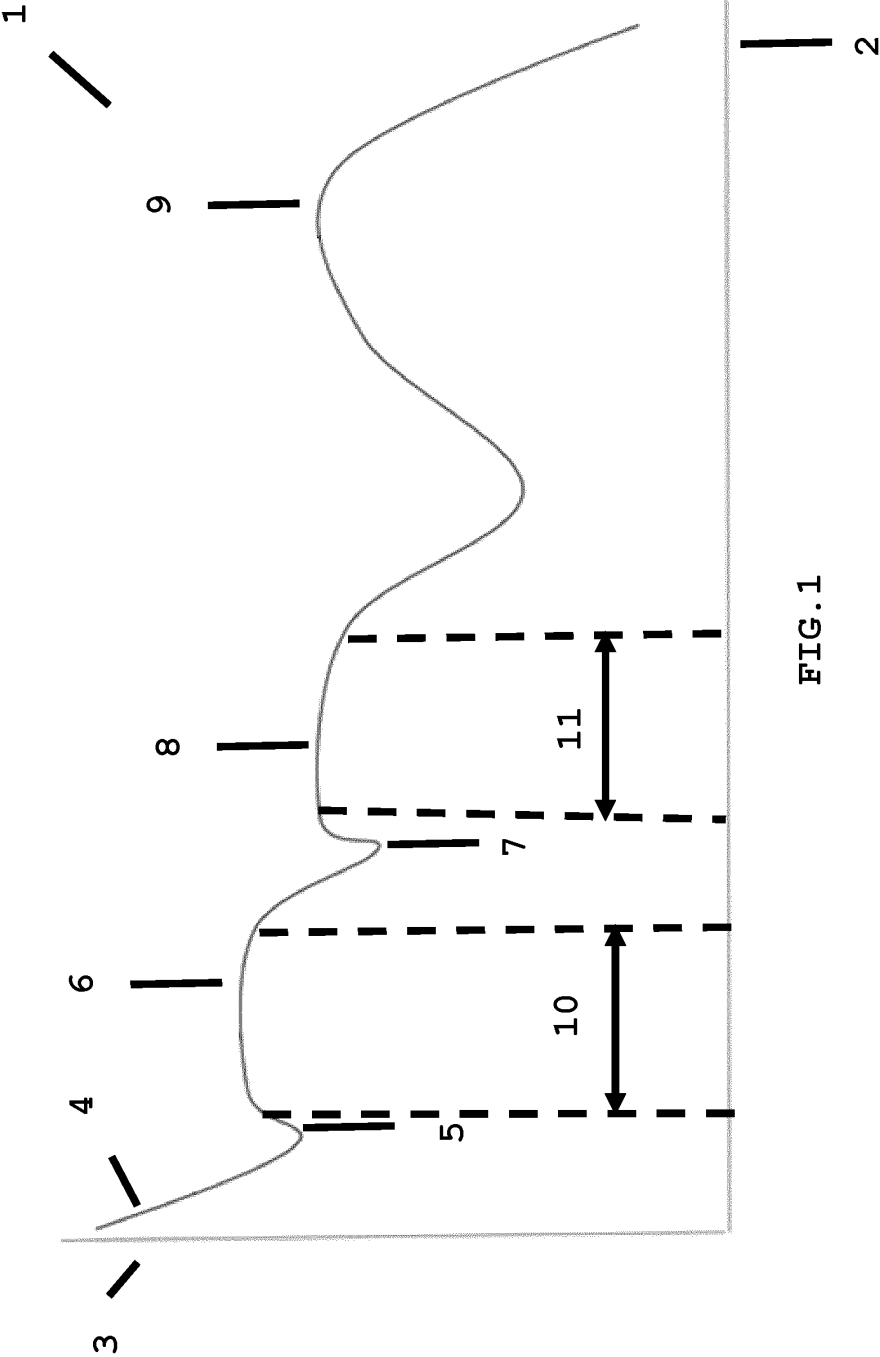




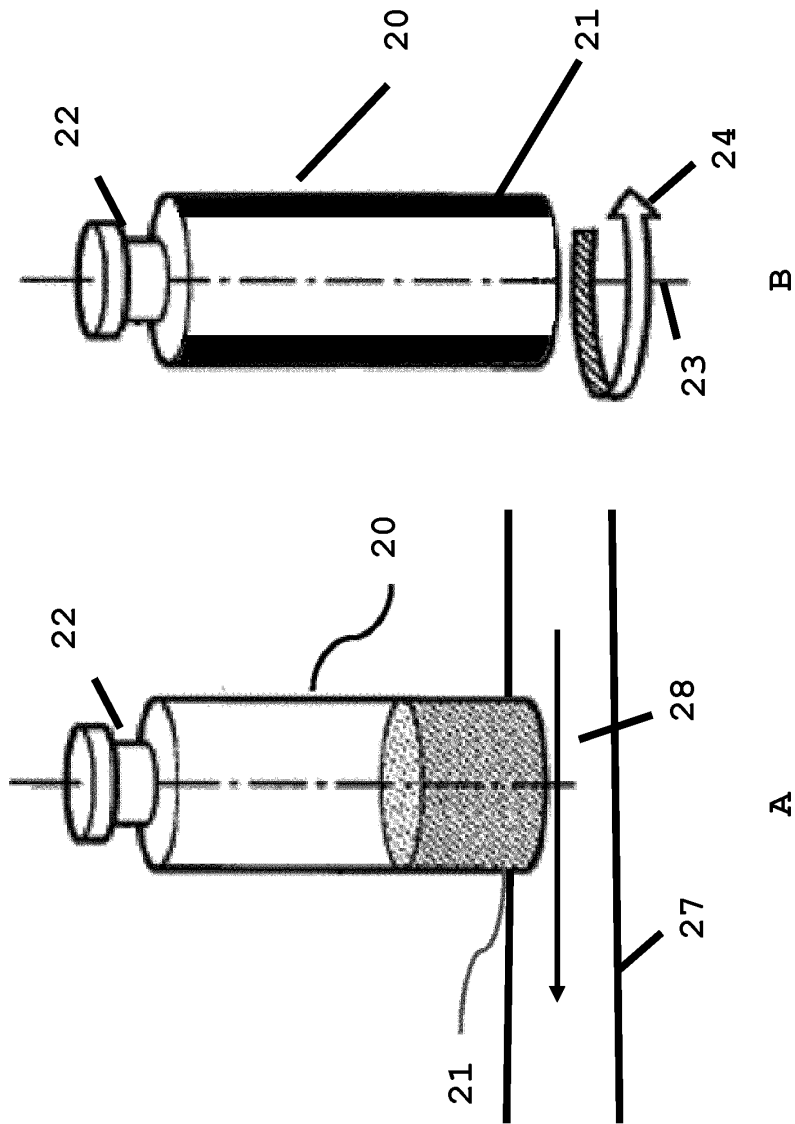


FIG. 2 (PRIOR ART)

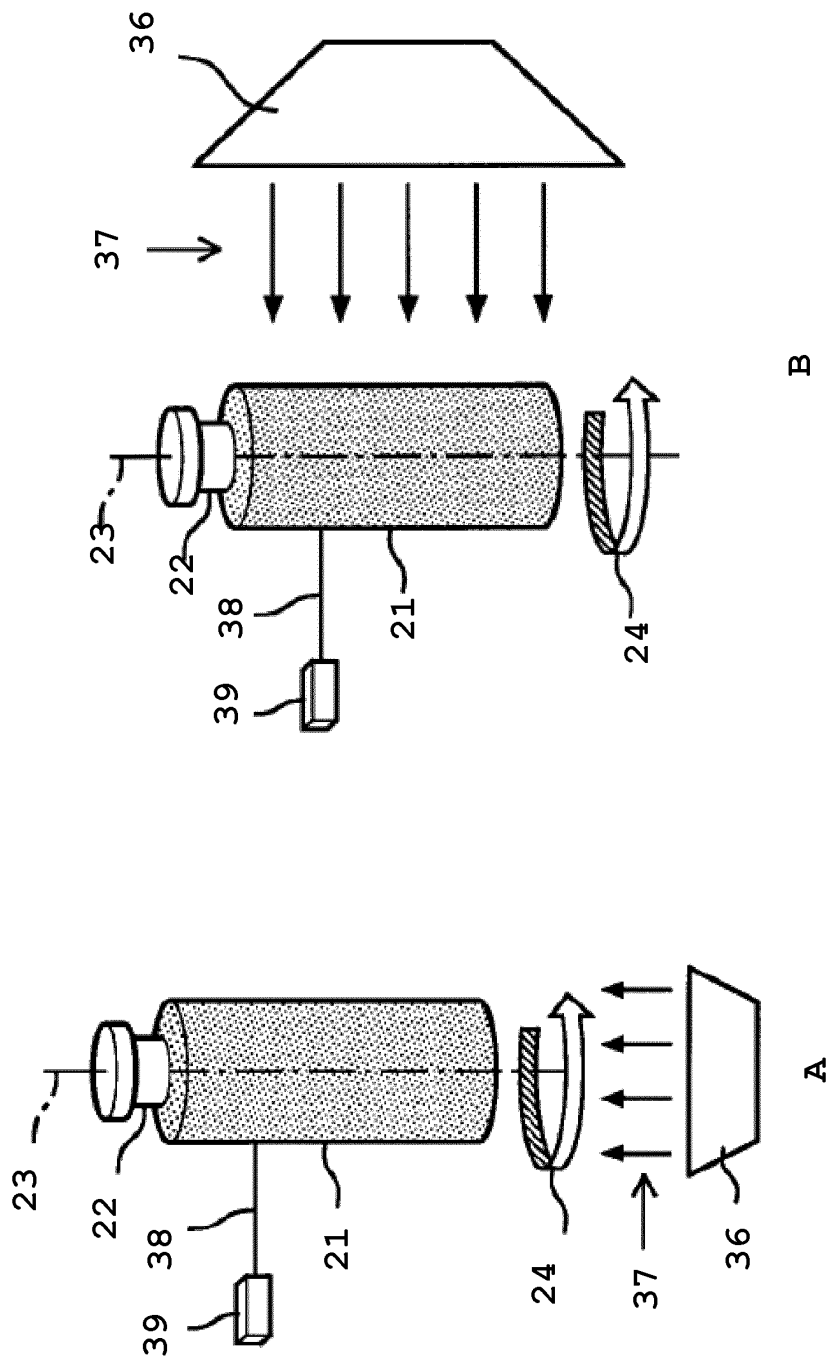


FIG. 3 (PRIOR ART)

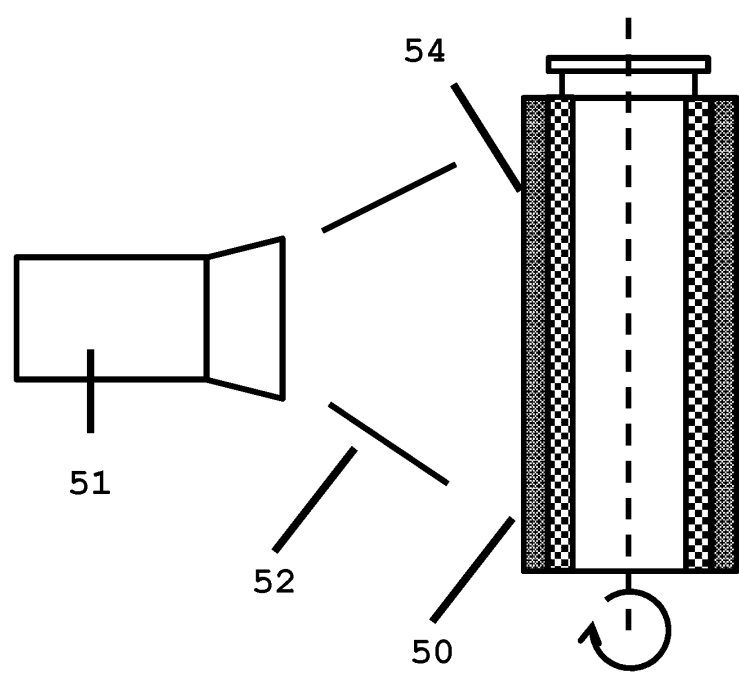


FIG. 4

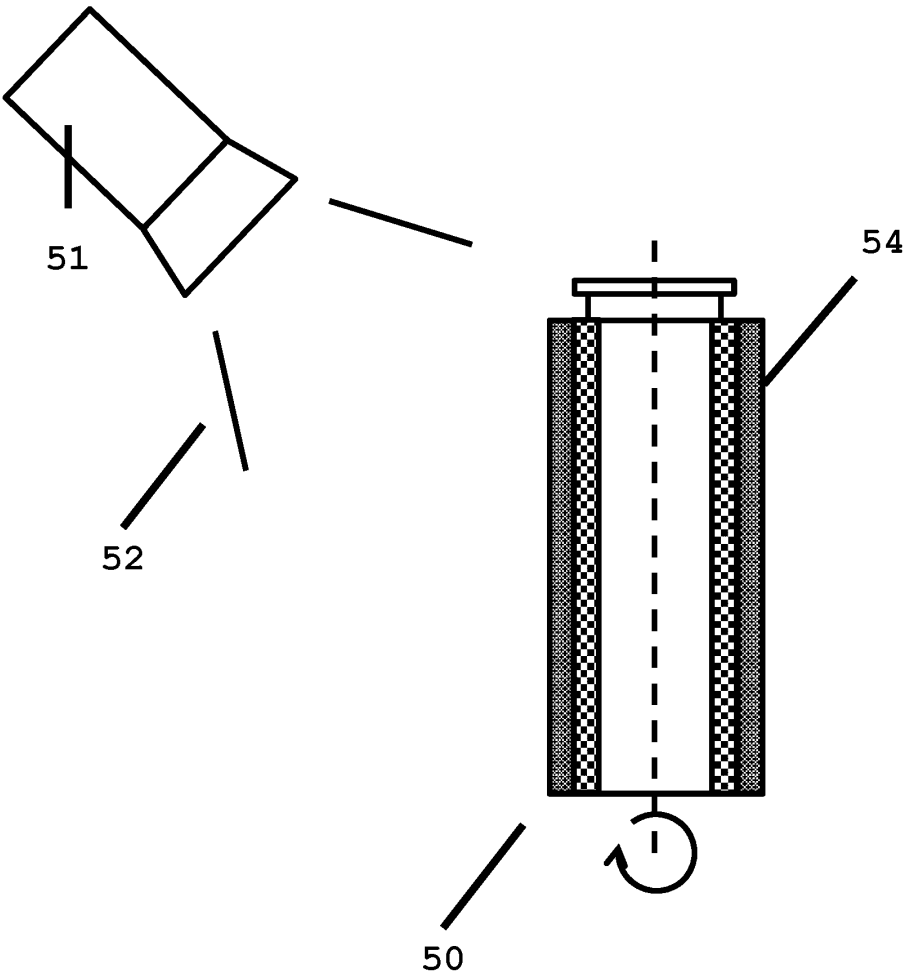


FIG. 5

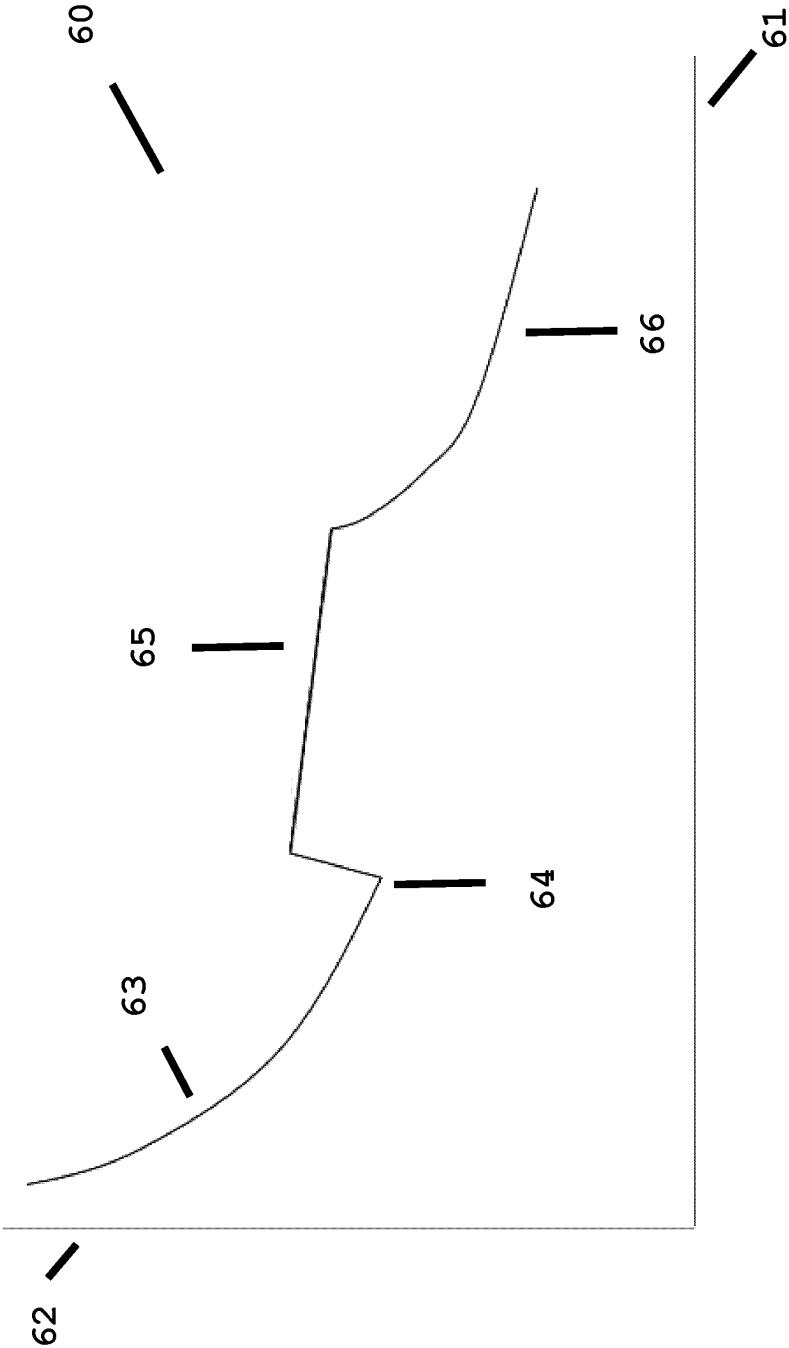


FIG. 6

7/29

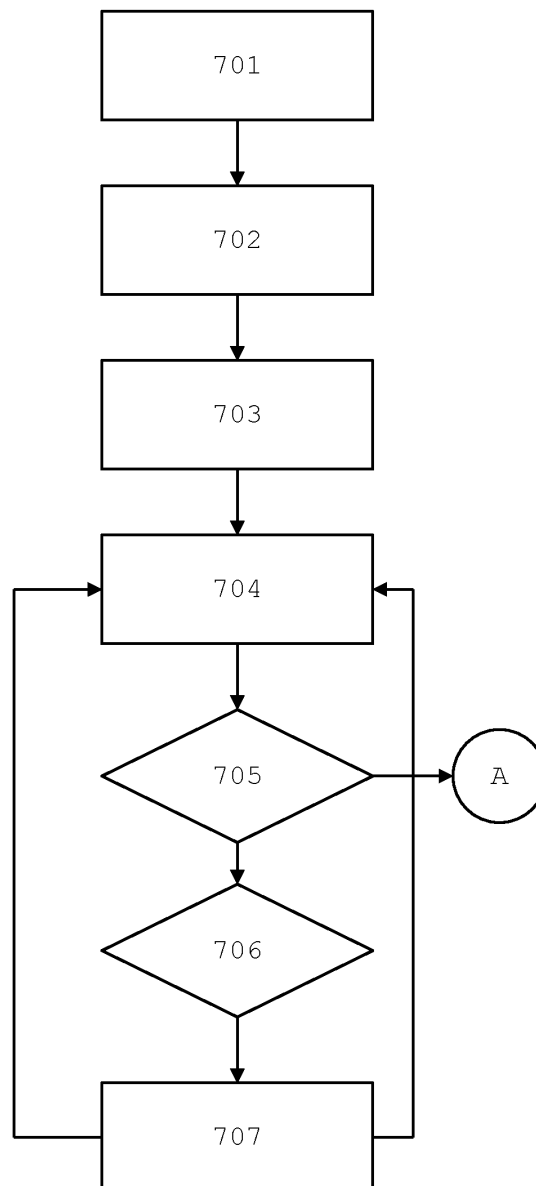


FIG. 7A

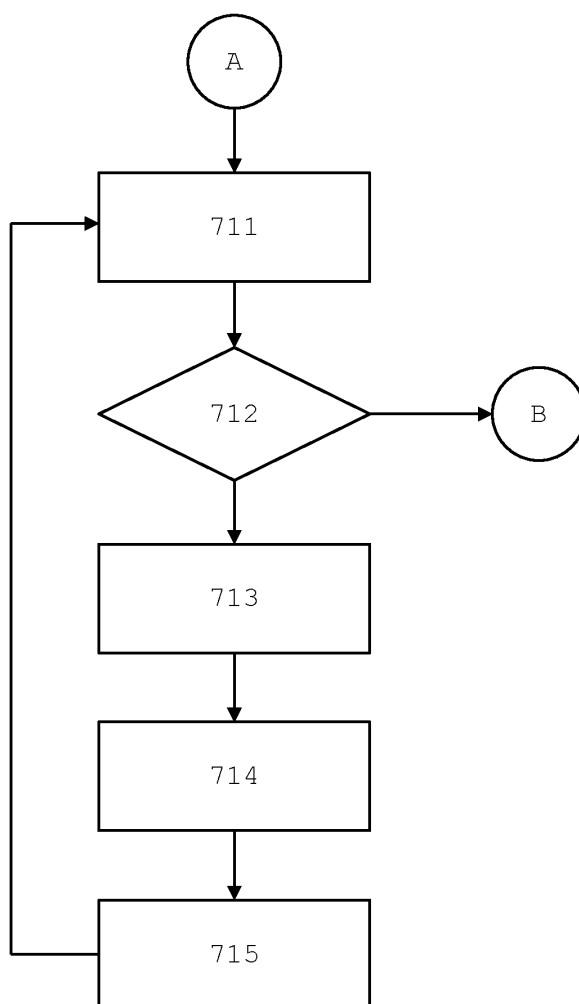
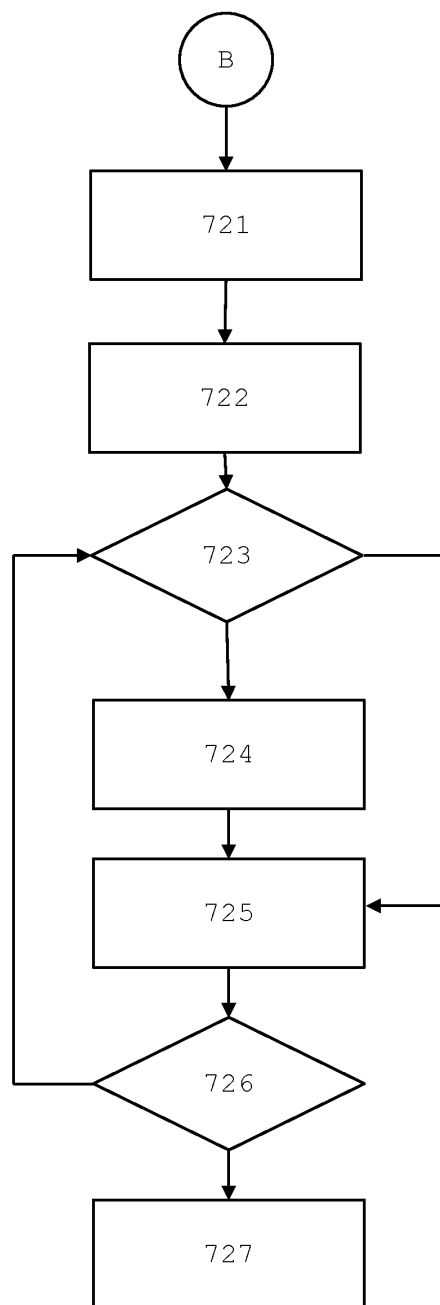


FIG. 7B

9/29

**FIG. 7C**

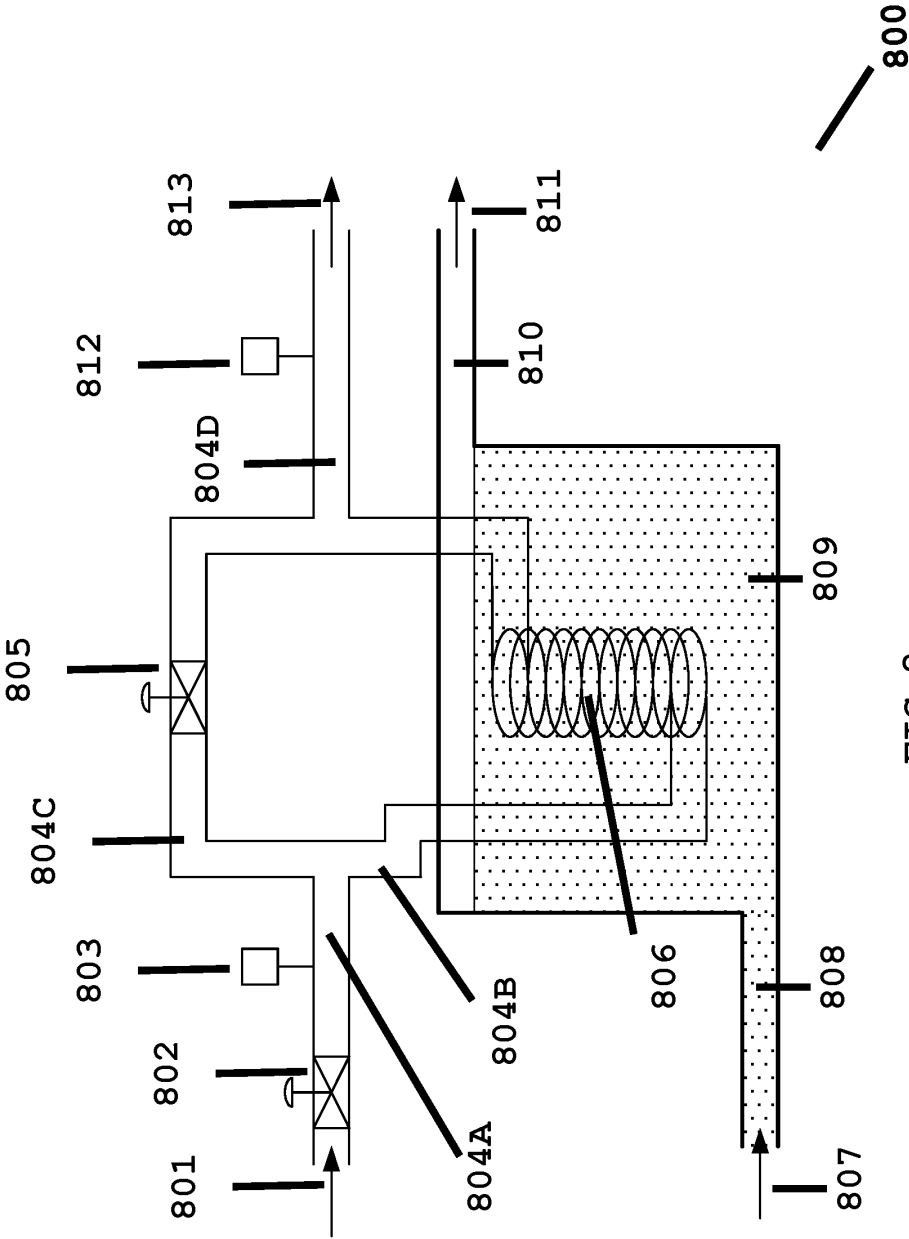


FIG. 8

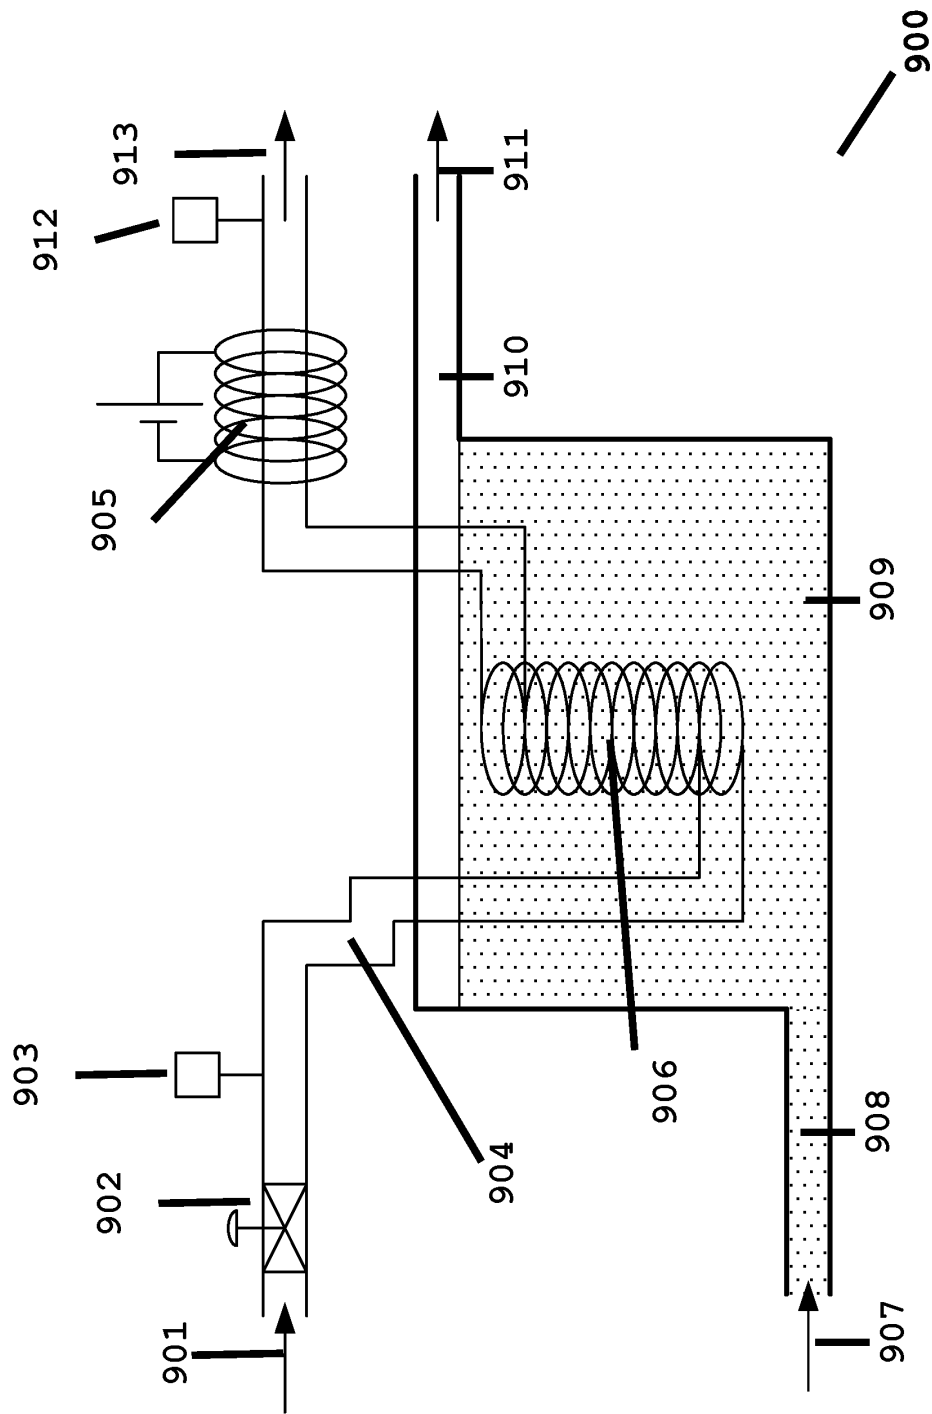


FIG. 9

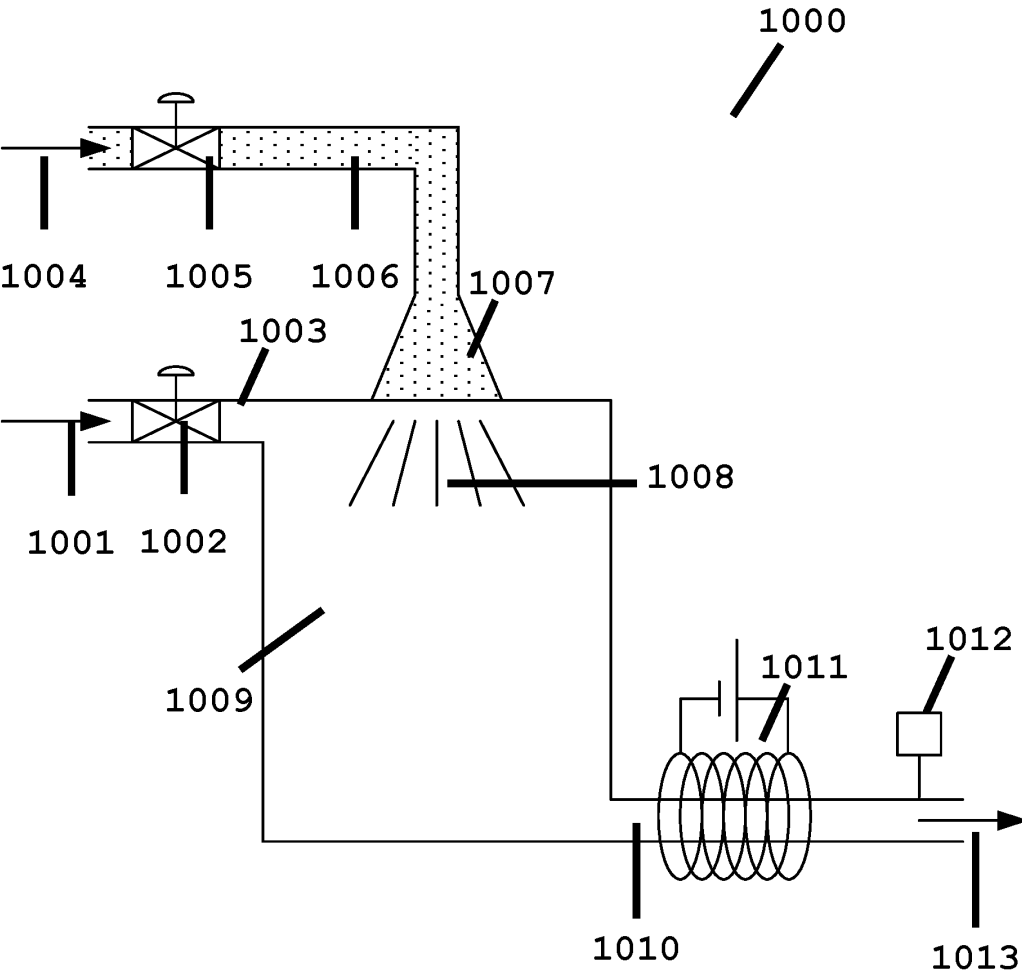


FIG. 10

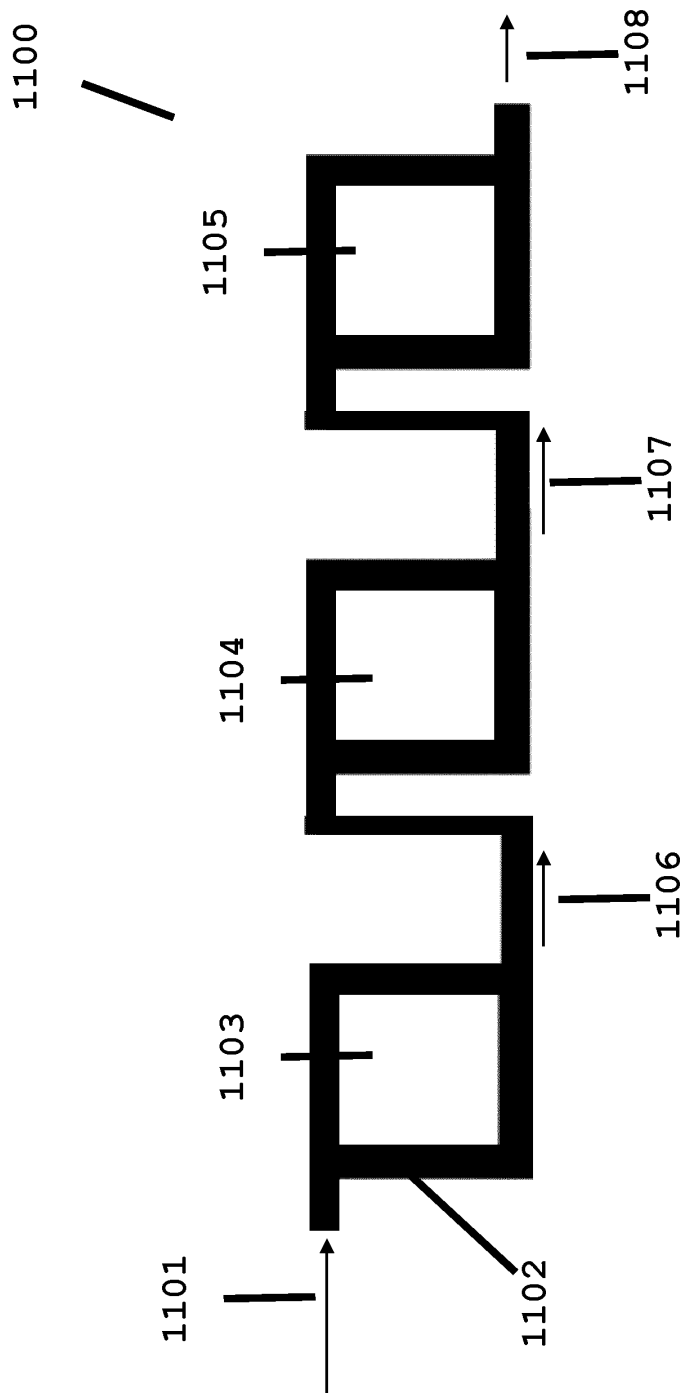


FIG. 11

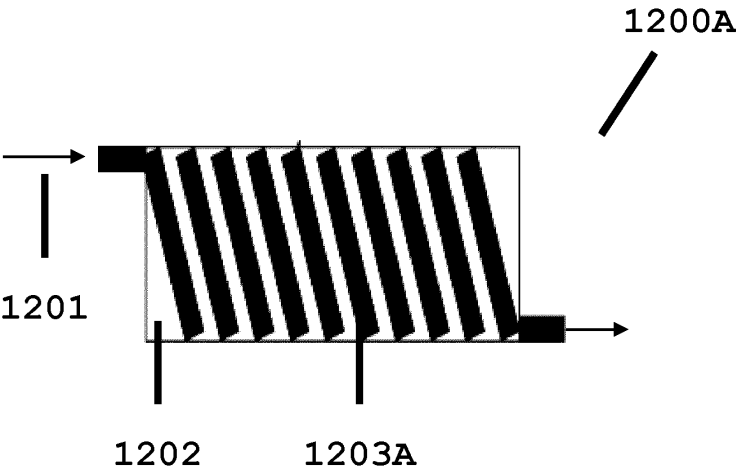


FIG. 12A

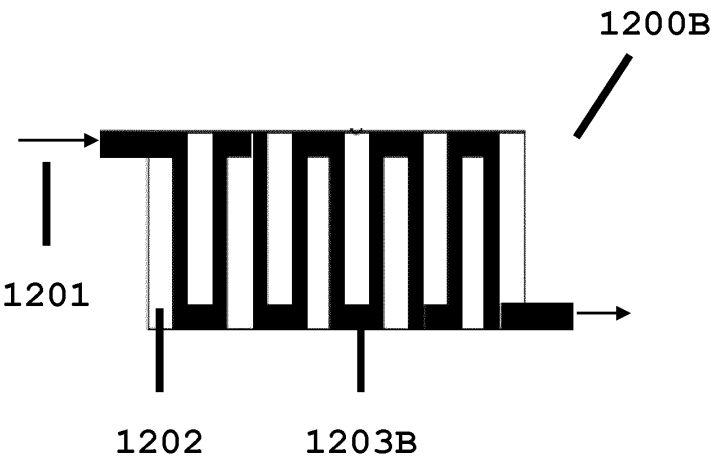


FIG. 12B

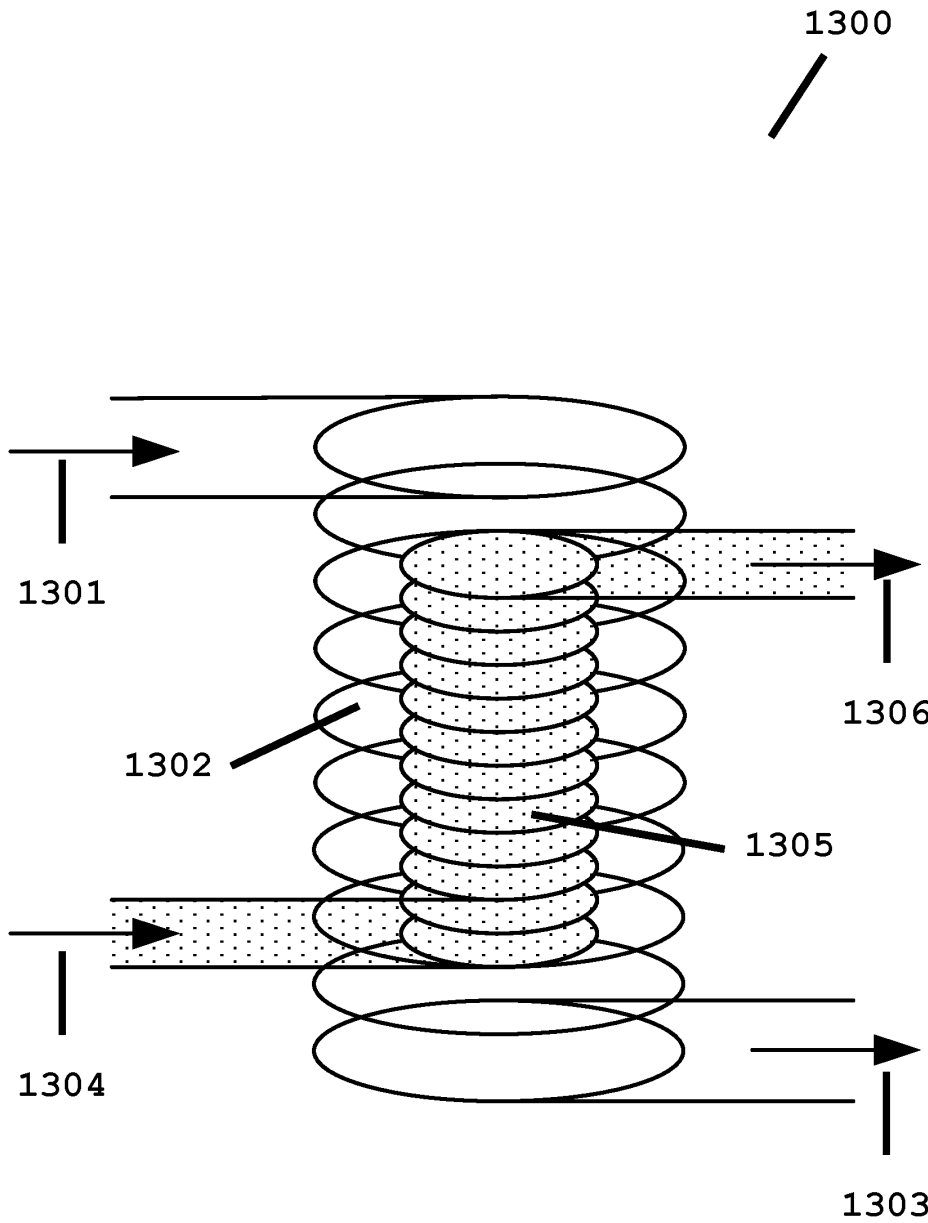


FIG.13

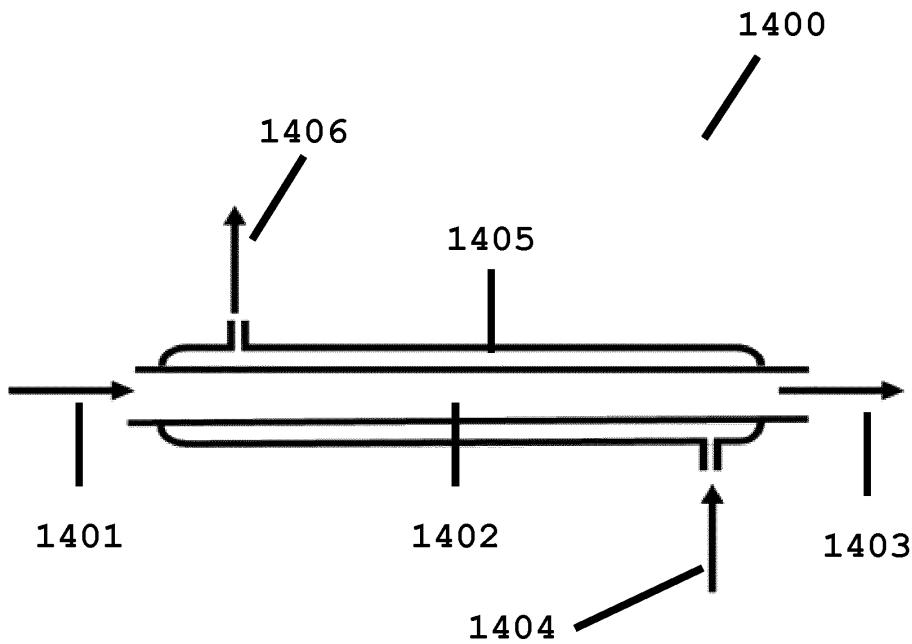


FIG. 14

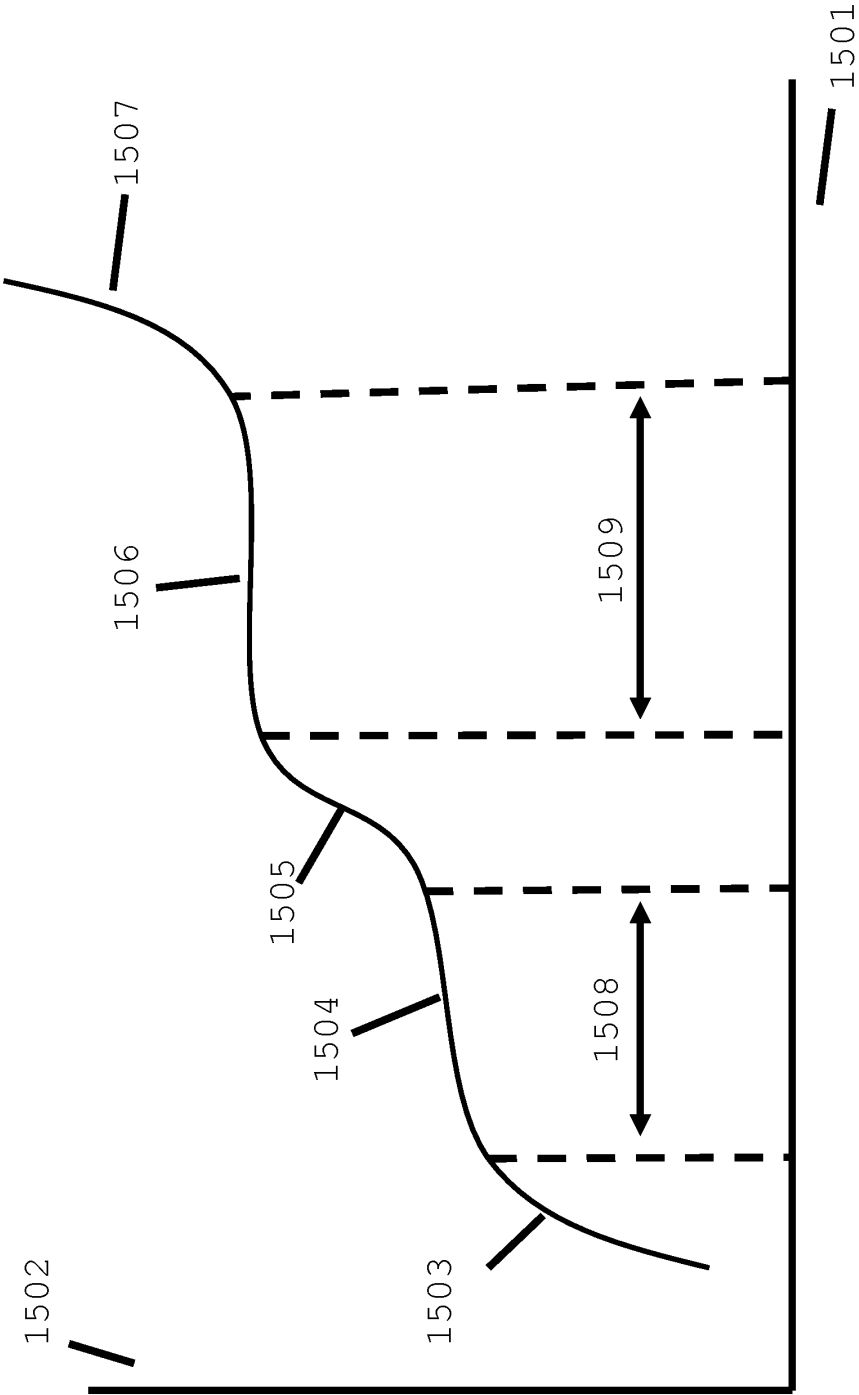


FIG. 15

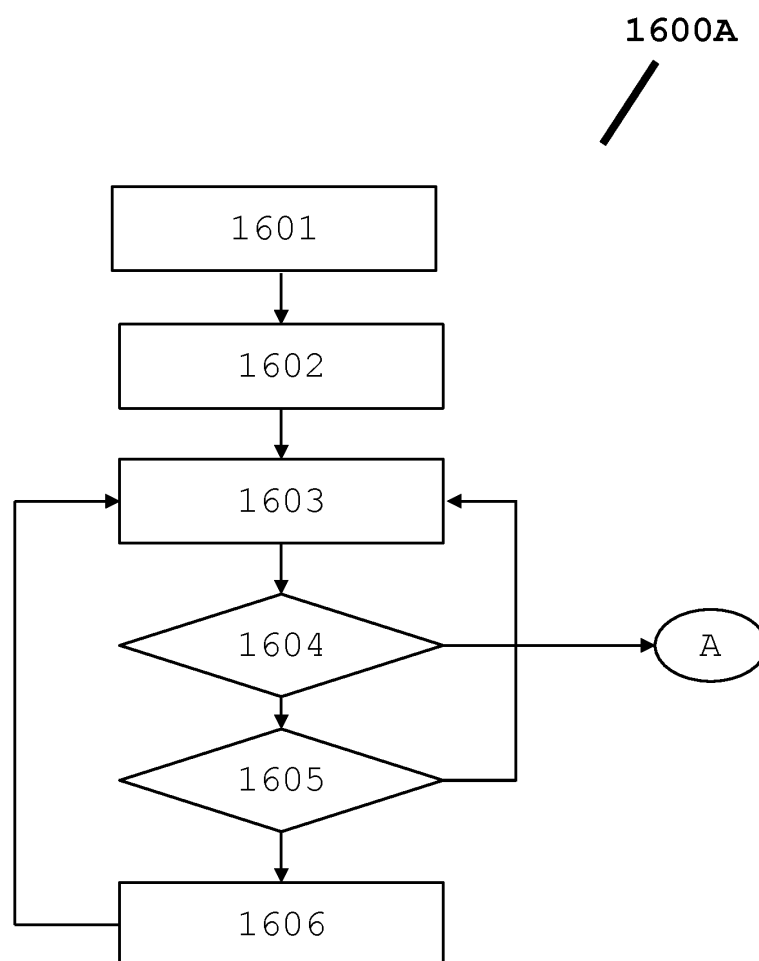


FIG. 16A

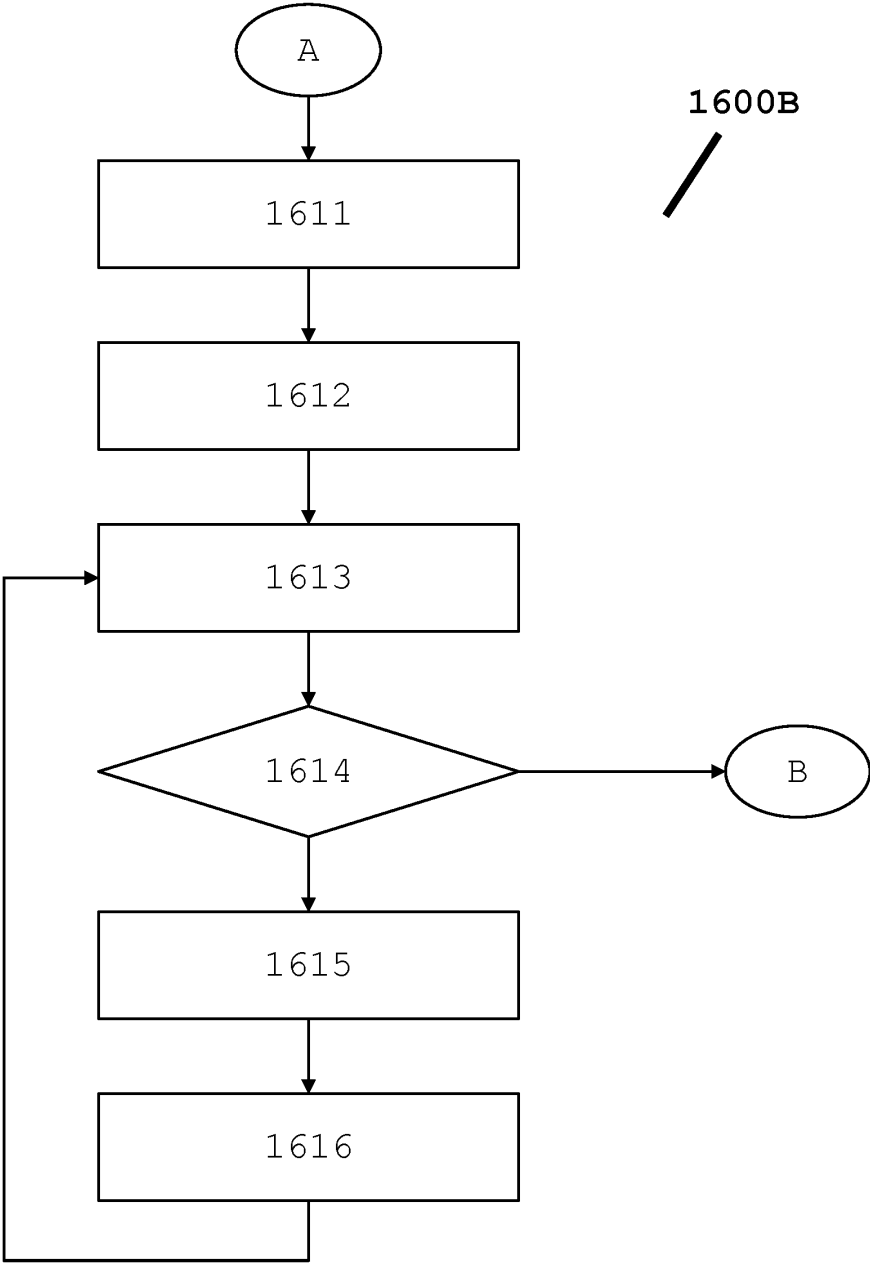


FIG. 16B

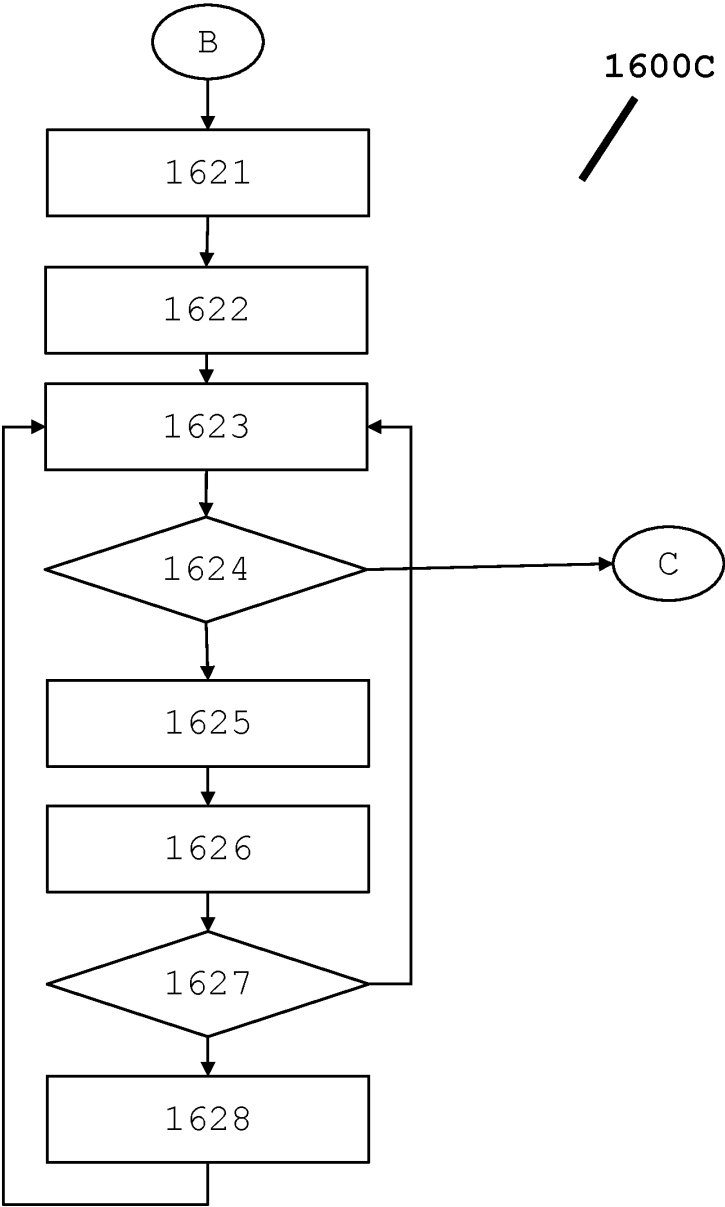


FIG.16C

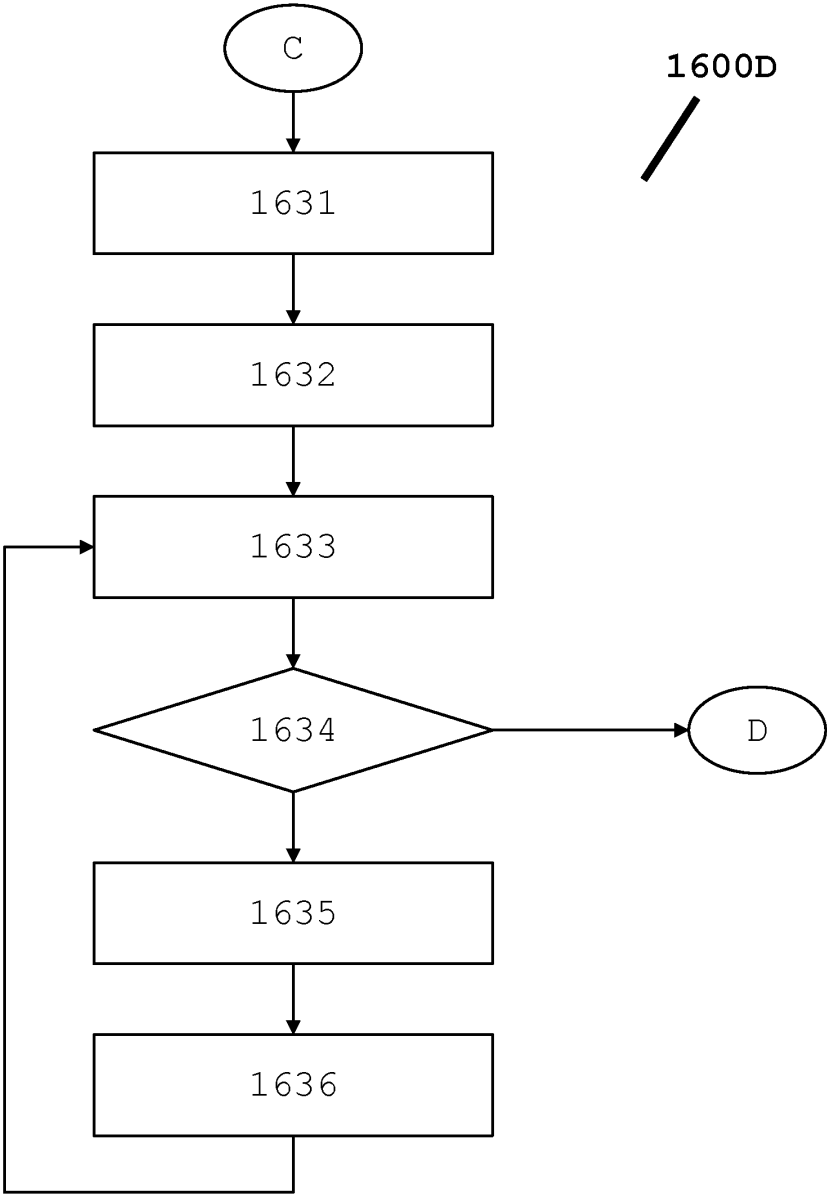


FIG.16D

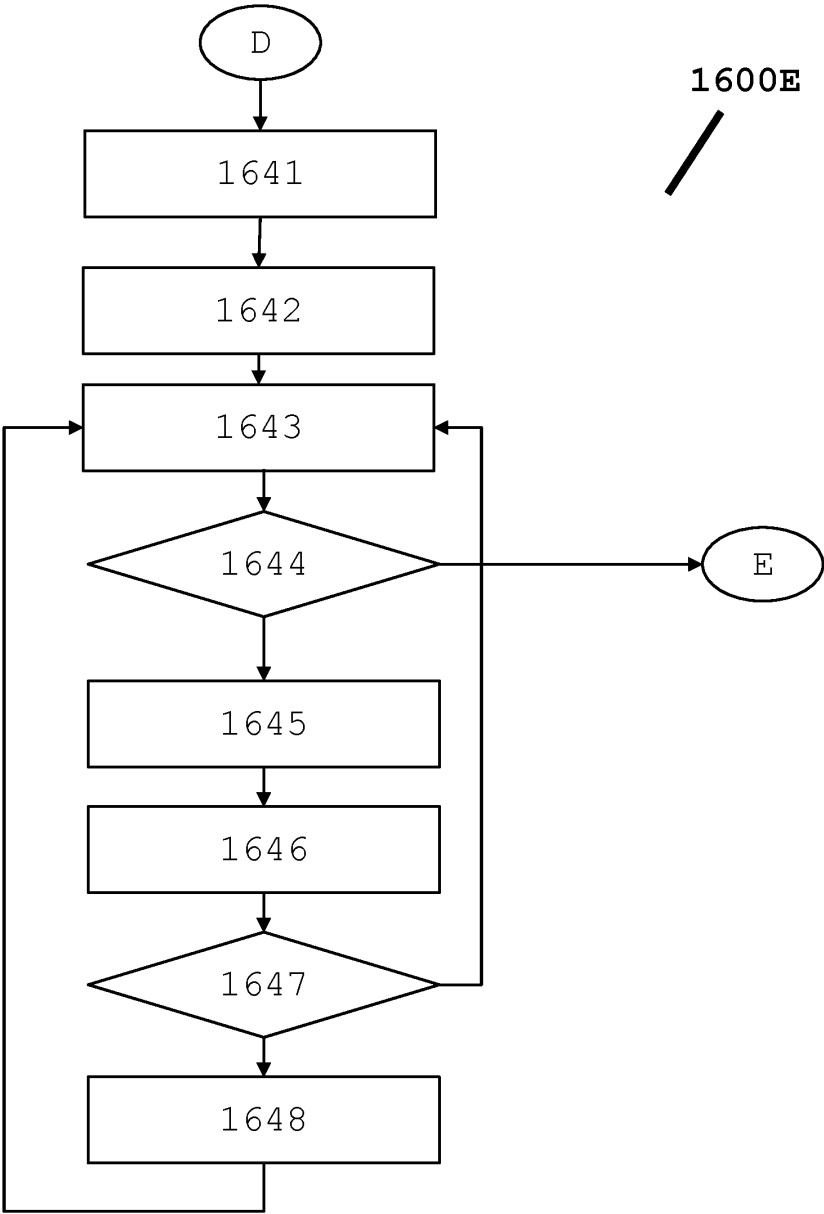


FIG.16E

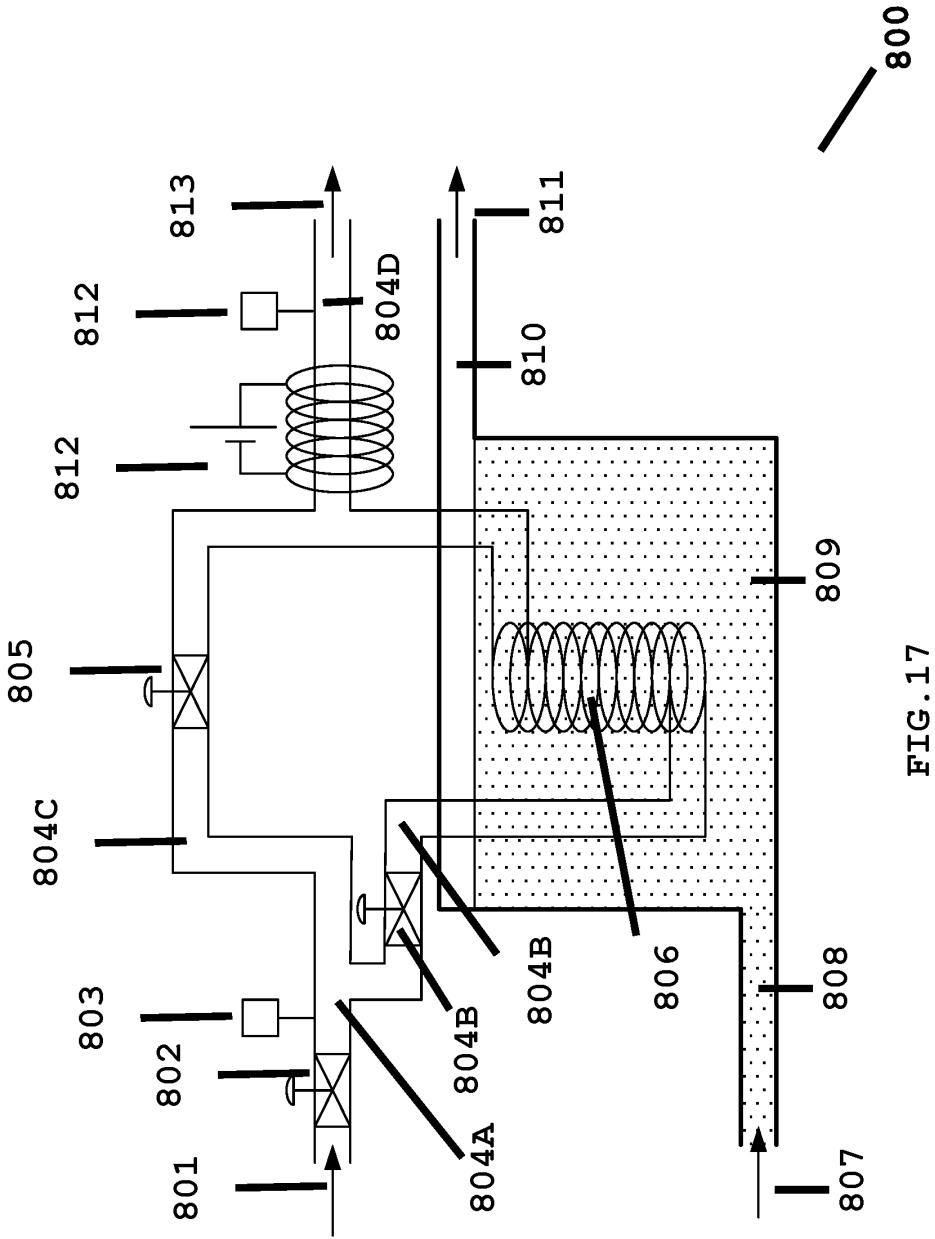


FIG. 17

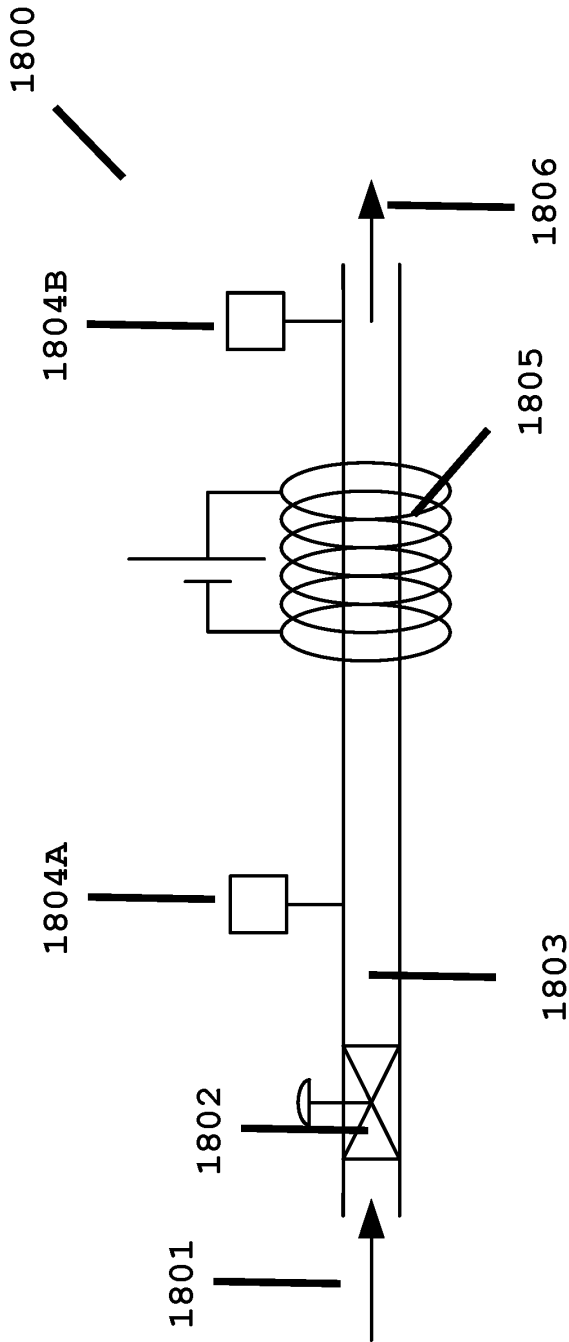


FIG.18

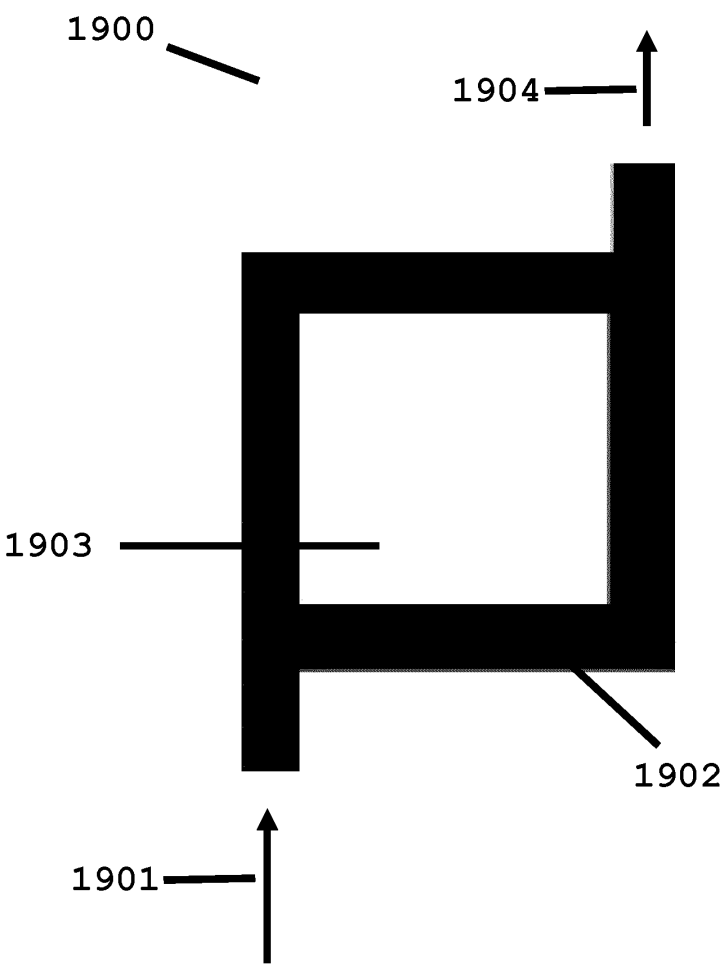


FIG. 19

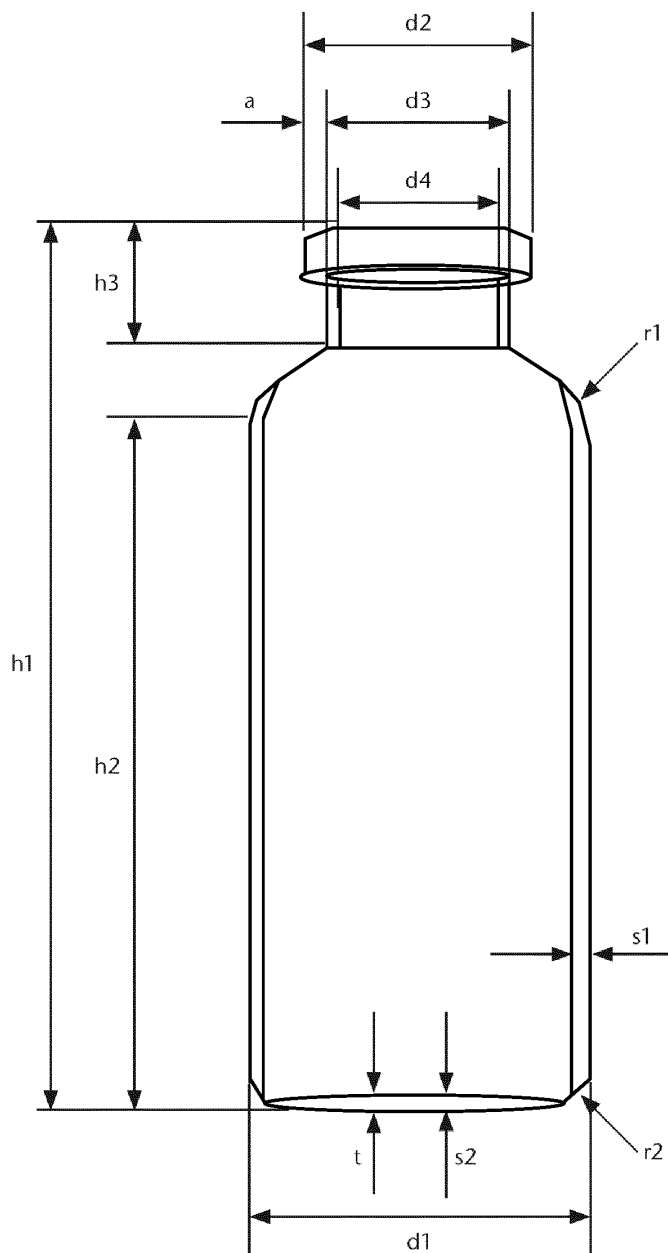


FIG. 20

Size designation of injection vial	Overflow capacity		a	d1		d2	d3	d4	h1		h2	h3	r1		r2	s1		s2	t	Mass
	ml	Tol	mm	mm	Tol	mm	max.	mm	mm	Tol	mm	mm	mm	mm	mm	mm	mm	mm	mm	g
2R	4		1	16	±0.15	13	10.5	7	35		22	8	2.5	1.5				0.6		4.4
4R	6	±0.5							45		32									5.7
6R	10								40	±0.5	26	8.5	3.5		2	1	±0.04		0.7	7.9
8R	11.5			22			16.5		45		31									8.7
10R	13.5	±1	1.2	24	±0.2				45		30	9	4					0.7		9.5
15R	19								60		45									12.0
20R	26					20		12.6	55		35									16.2
25R	32.5	±1.5	1.5	30	±0.25				65	±0.7	45		5.5	2.5		1.2	±0.05	1		18.9
30R	37.5						17.5		75		55	10								21.9
50R	62	±4	2.5	40	±0.4				73	±0.75	49		6	4		1.5	±0.07			34.5
100R	123	±7	3.5	47	±0.5				100		75		6.5			1.7		0.9	1.5	60

FIG.21

28/29

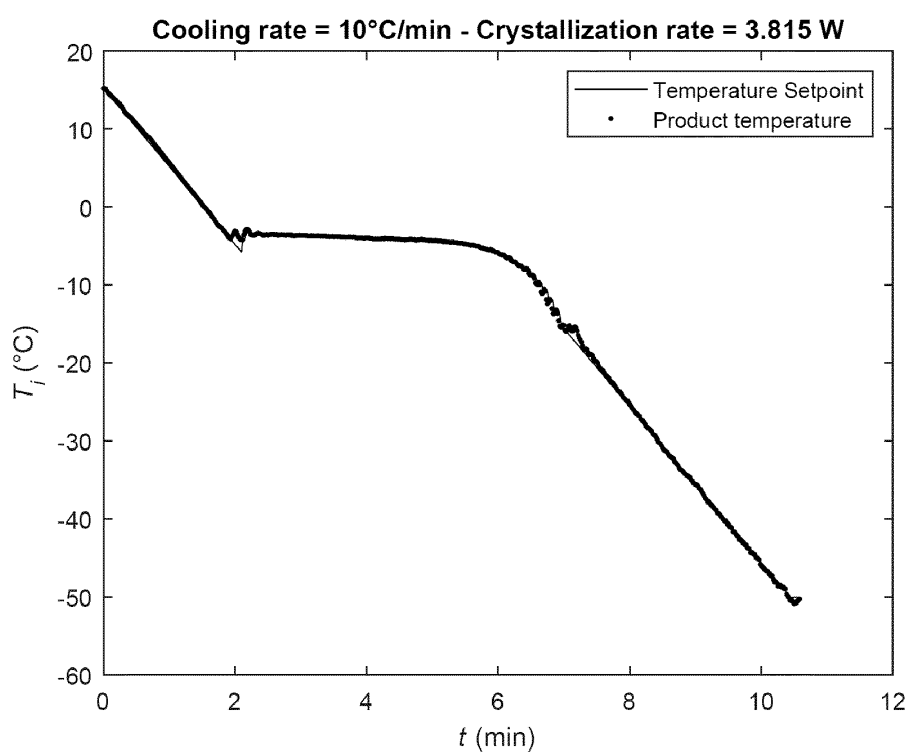


FIG. 22A

29/29

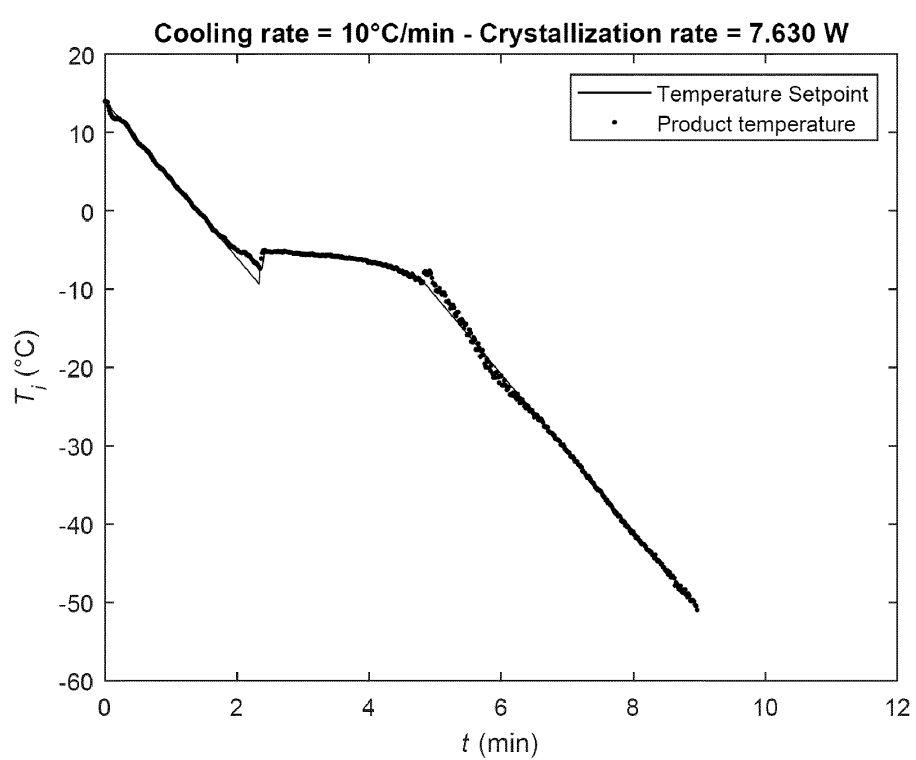


FIG. 22B