

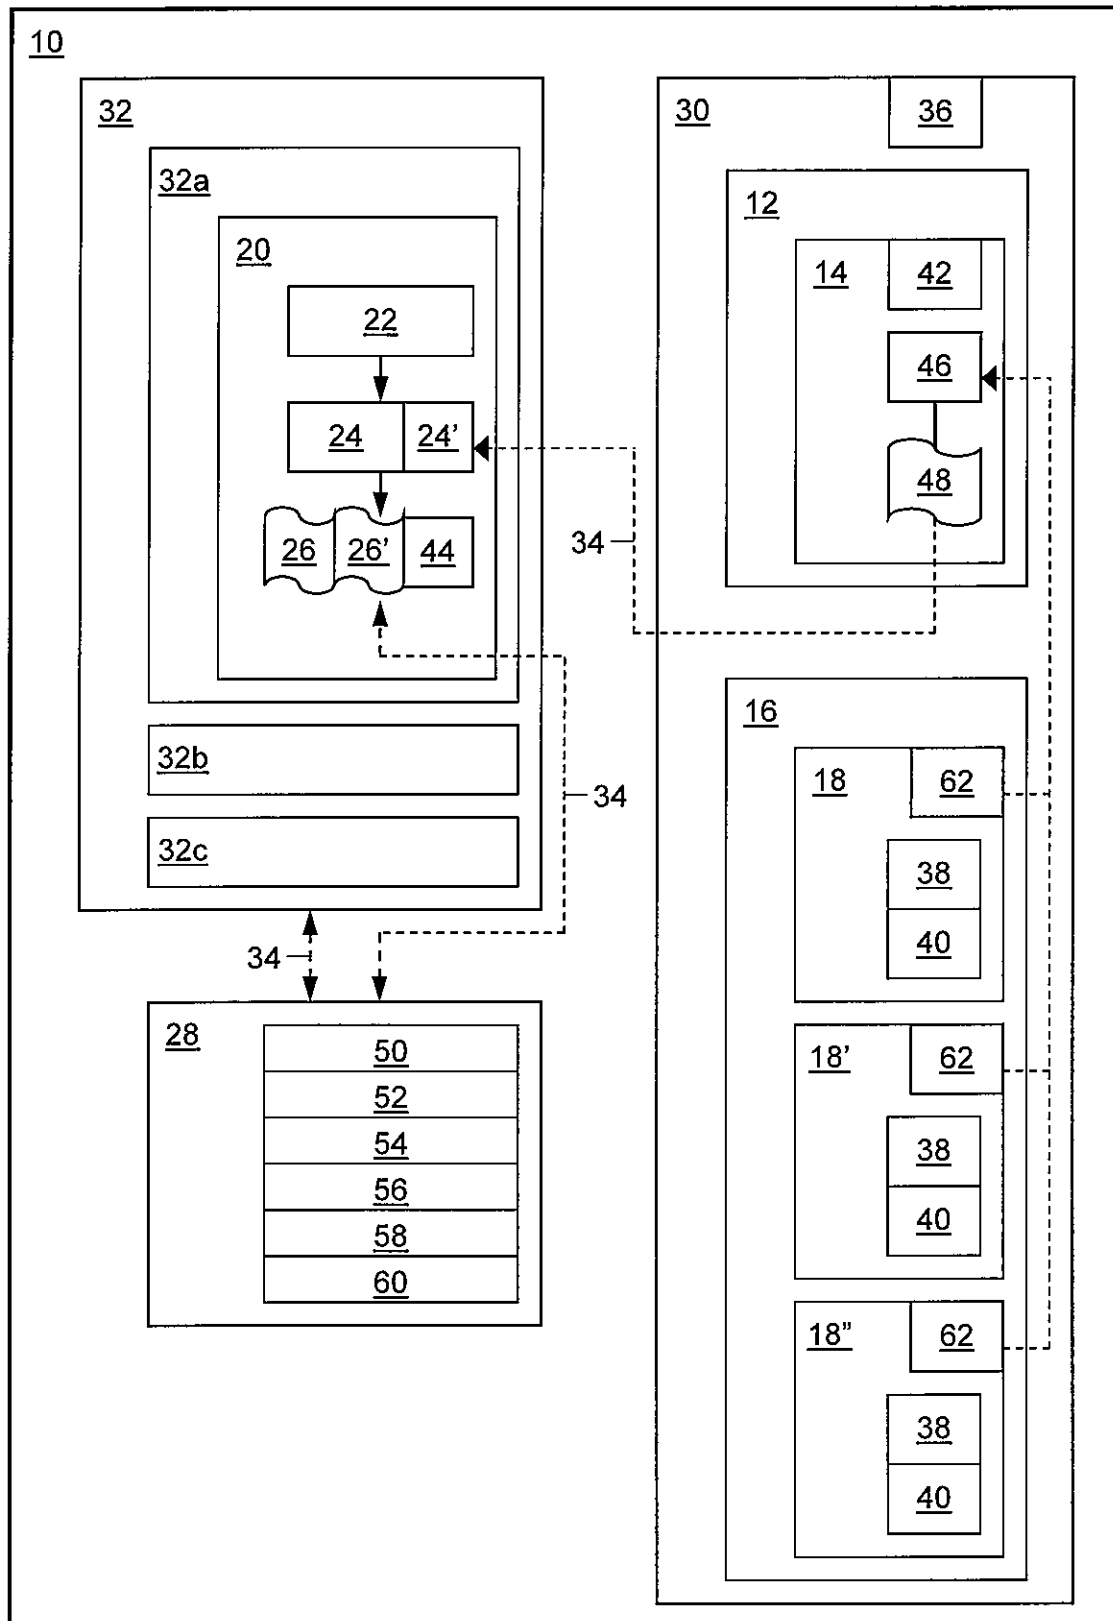


FIG.1

Step 1 : Select Application

Select the chromatography application in which you are using the selected consumable(s)



☒ Gas Chromatography (GC)
Gas Chromatography (GC)



☐ Liquid Chromatography (LC)
Liquid Chromatography (LC)



☐ ICP
ICP

Detector Type:

☒ MS

☐ ECD

☐ ELCD

☐ NPD

☐ FID

Detector Type:

☐ MS

Detector Type:

☐ MS

[Previous](#) [Next](#)

FIG. 2

Step 2 : Application Usage

Please indicate the necessary details to calculate the lifetime of the selected consumable(s)

Gas Chromatography (GC) / MS 		Carrier Gas Helium
		Source Gas Quality (%) 99.9999
Usage: ☒ Daily ☐ Weekly ☐ Monthly	Gas Delivery System ☒ Bottle ☐ Generator	
	Flow 2 L/Min.	
	Pressure 5	☒ Bar ☐ Psi
5 5 Sample(s).	Tubing & Fittings	Material: ☒ Stainless Steel ☐ Brass
Runtime per sample: 30 30 Minutes 25 25 Seconds	Size: ☐ 1/4" ☒ 1/8"	

[Previous](#) [Next](#)

FIG. 3

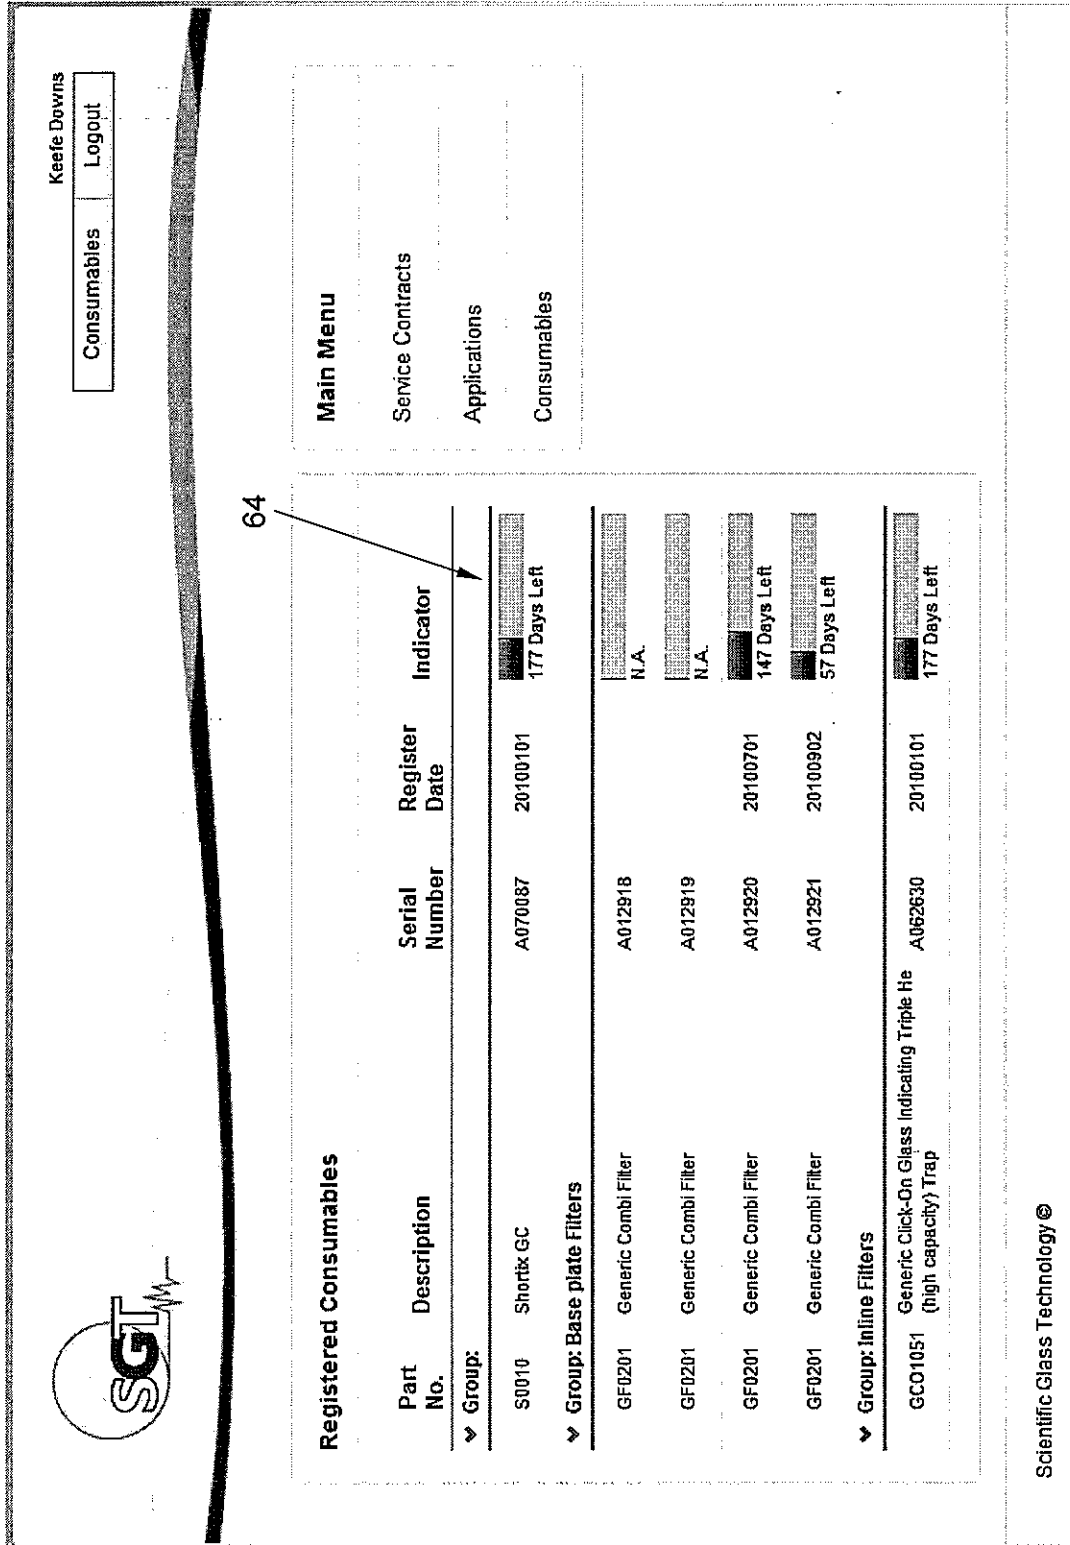


FIG. 4