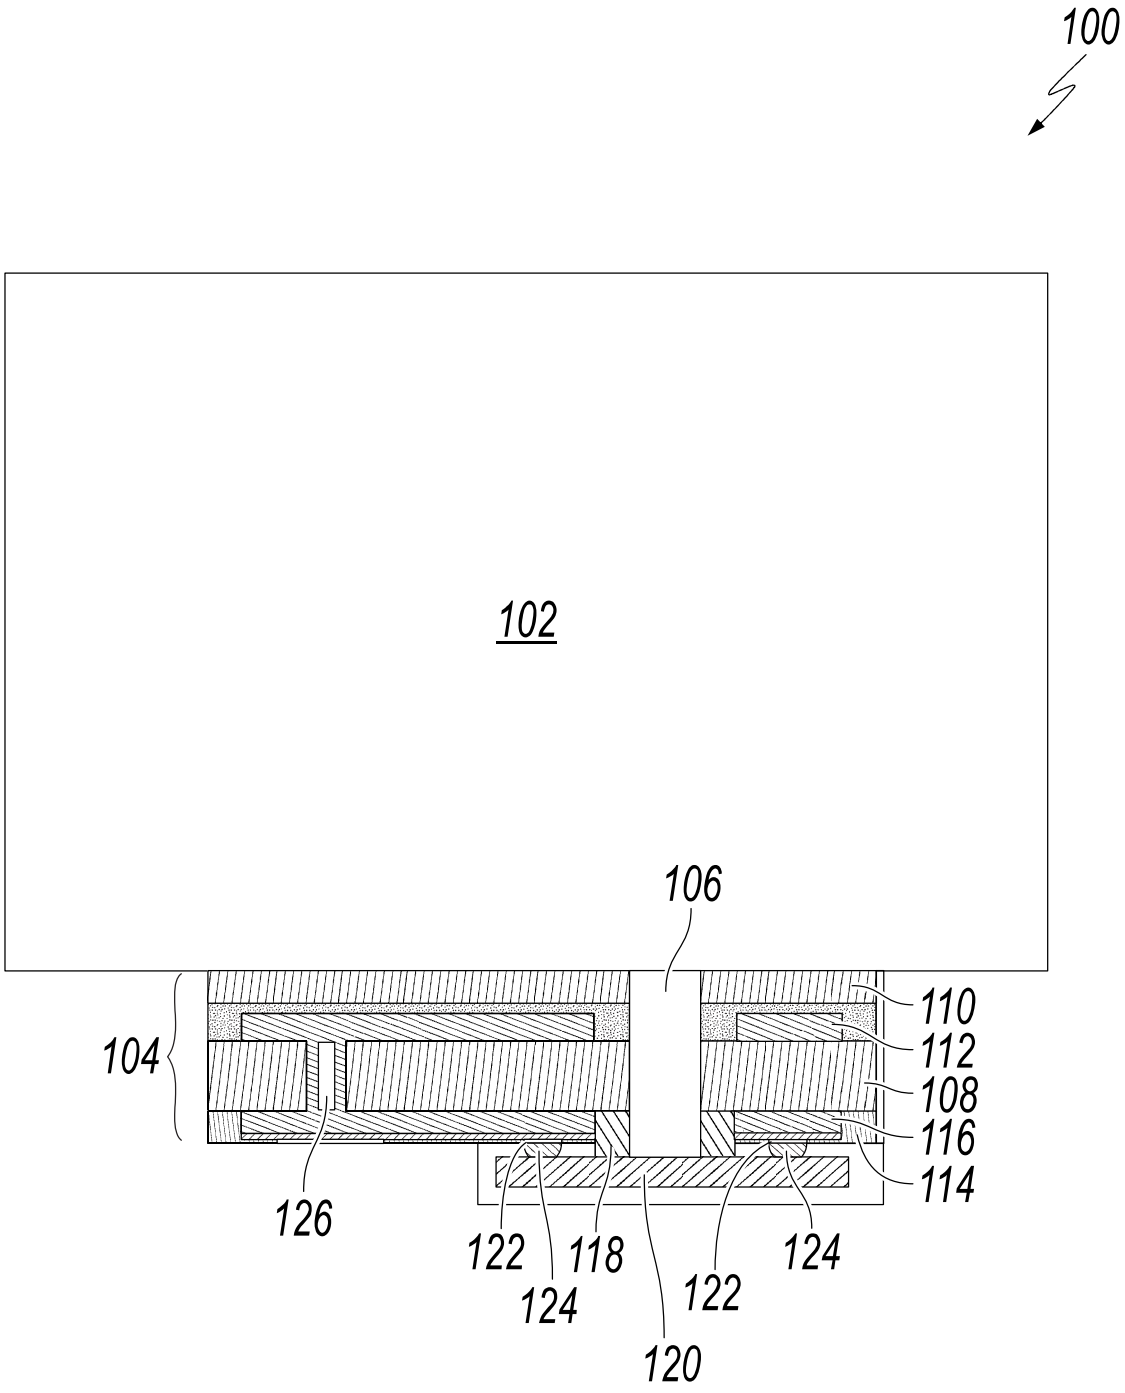


FIG. 1

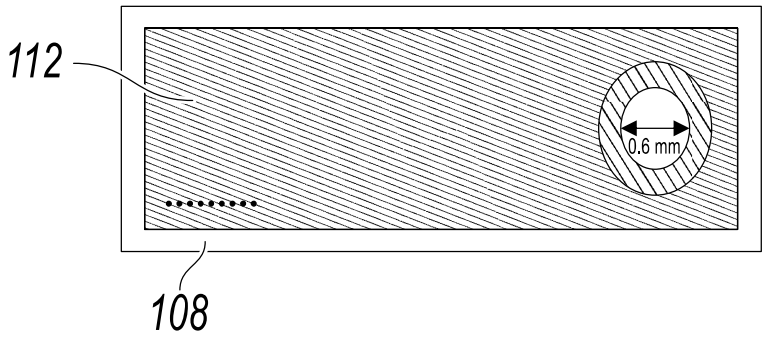


FIG. 2

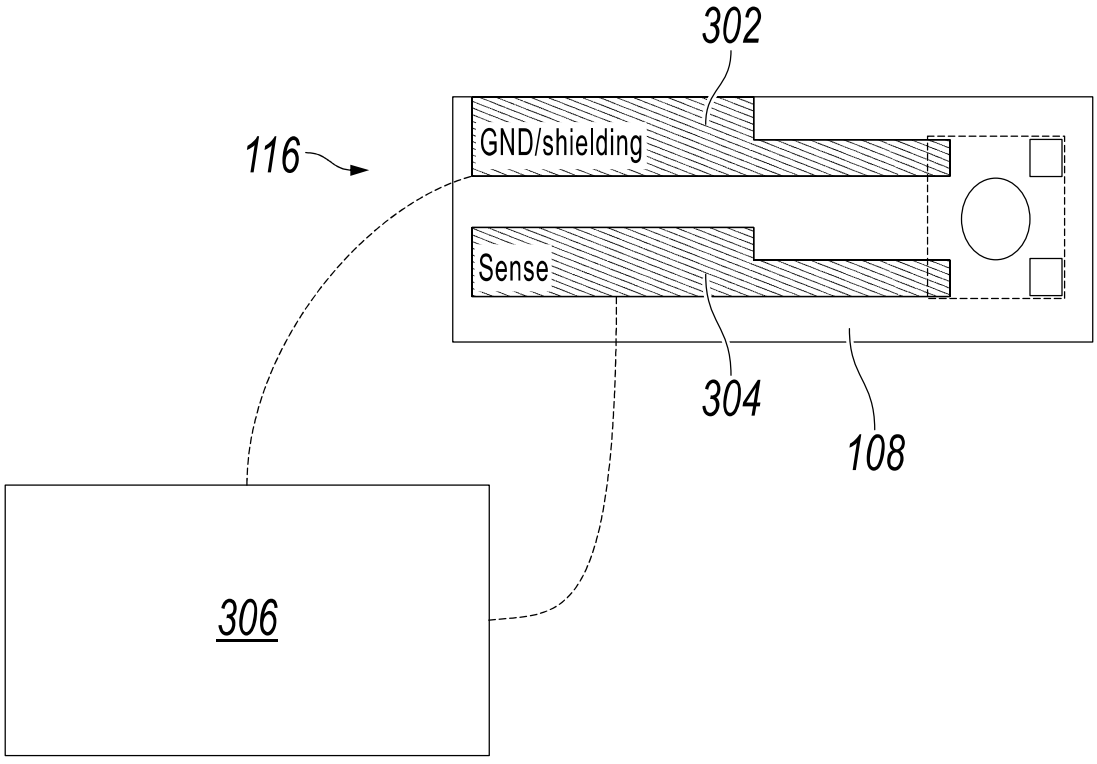


FIG. 3

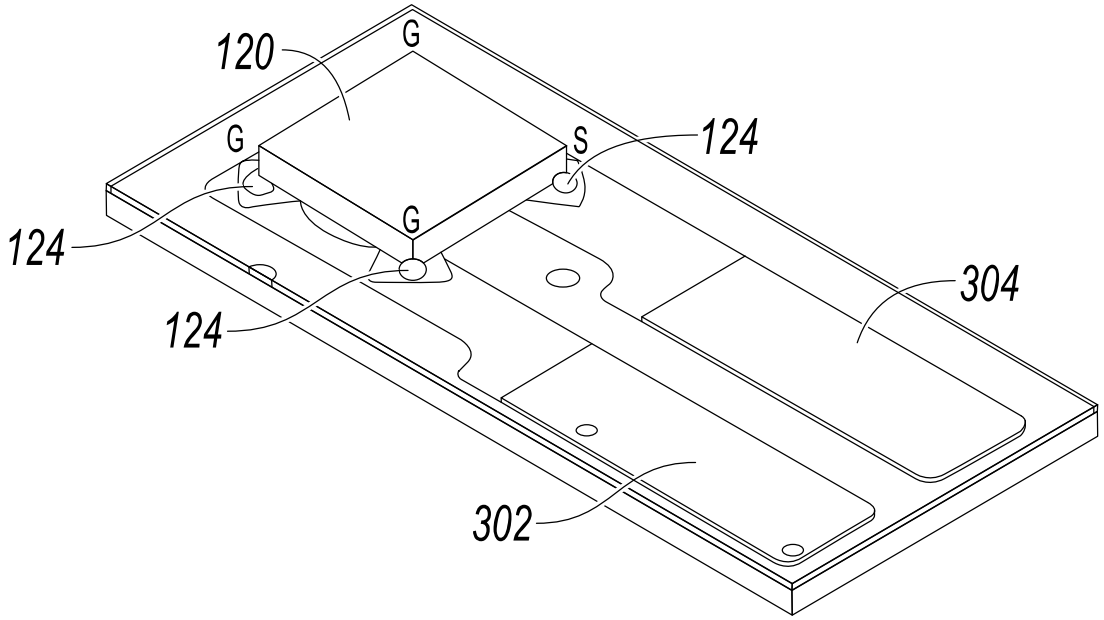


FIG. 4

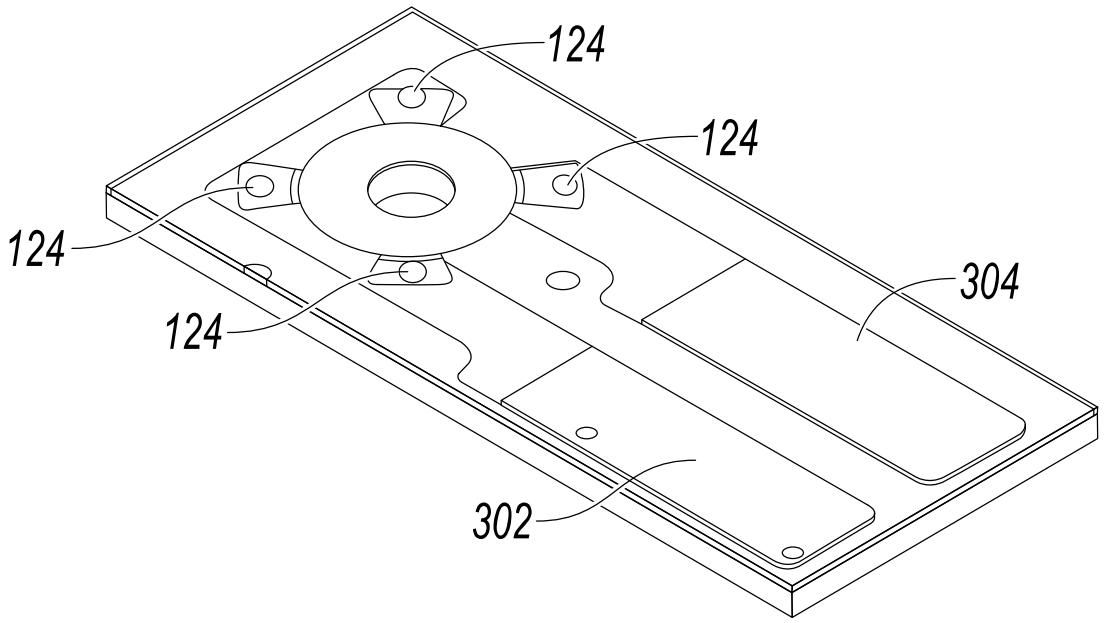


FIG. 5

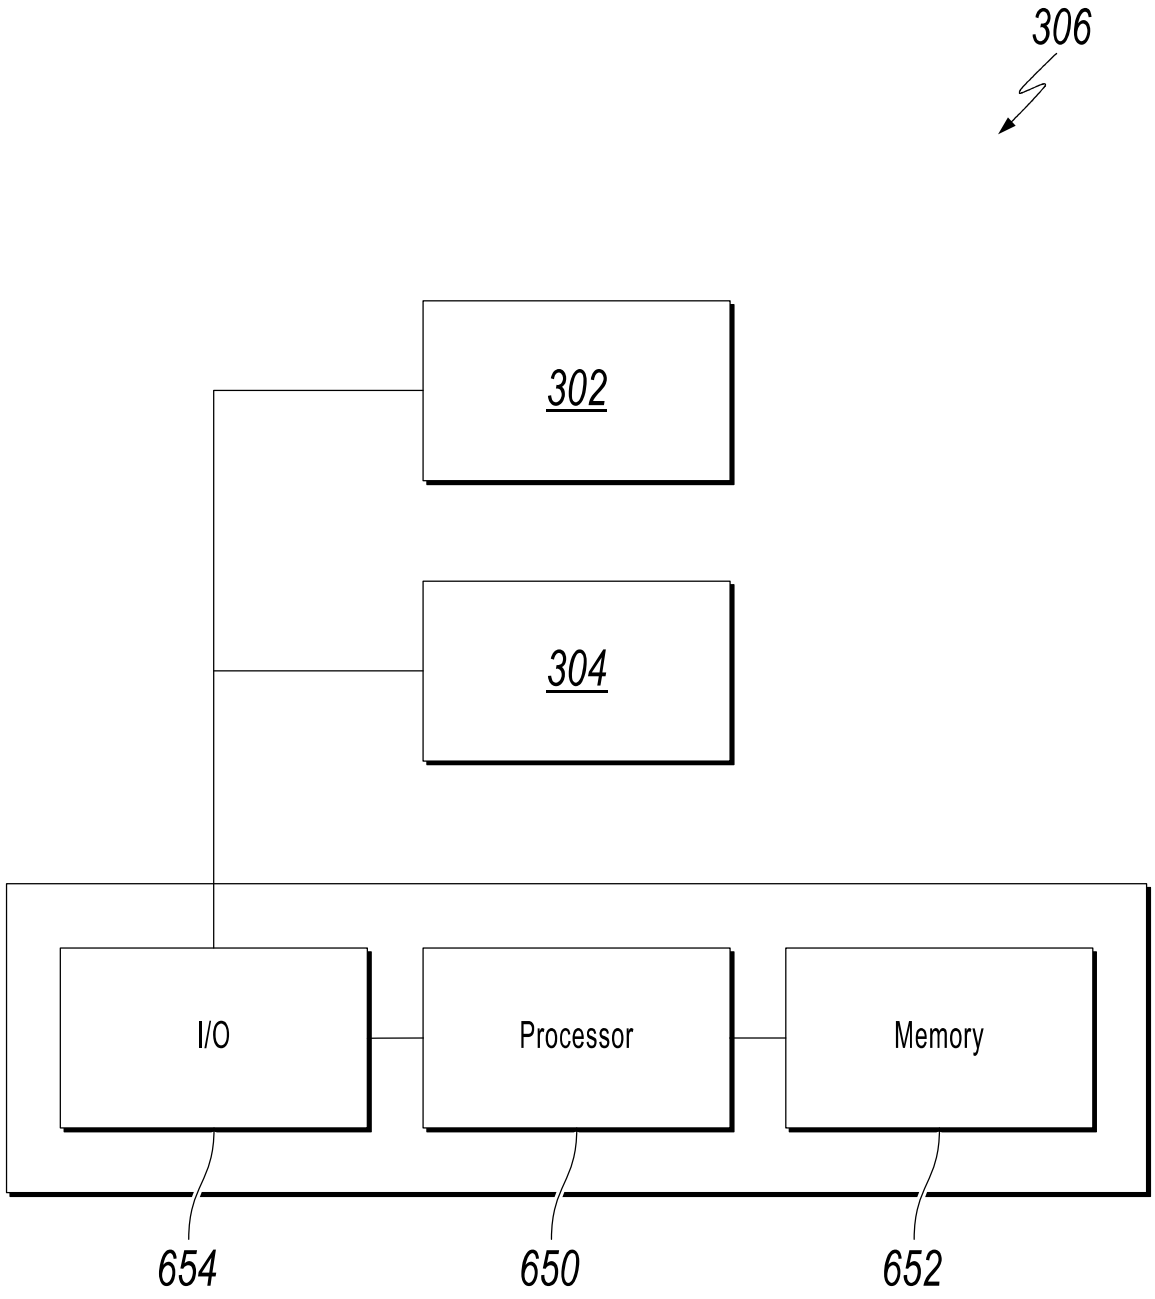


FIG. 6

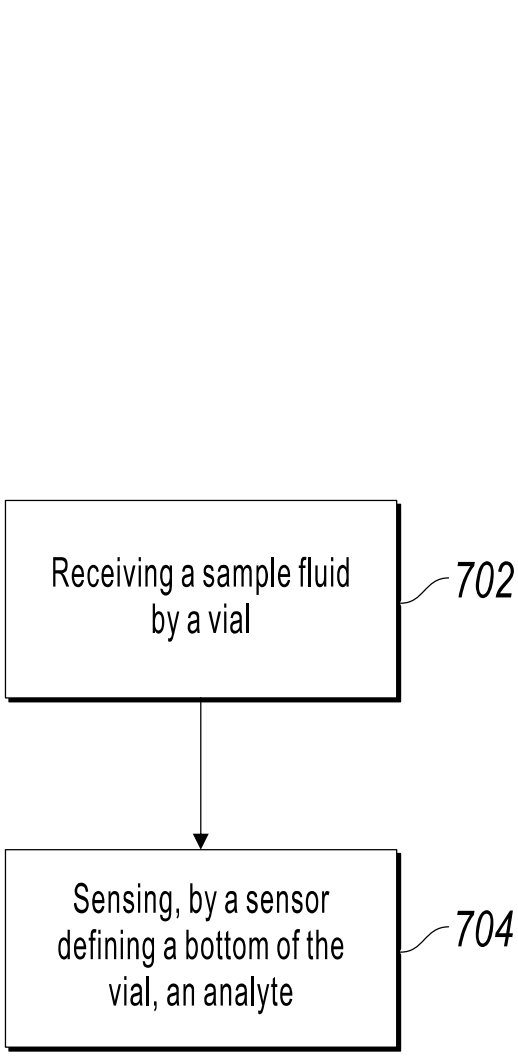

700
Receiving a sample fluid by a vial
702
Sensing, by a sensor defining a bottom of the vial, an analyte
704

FIG. 7