

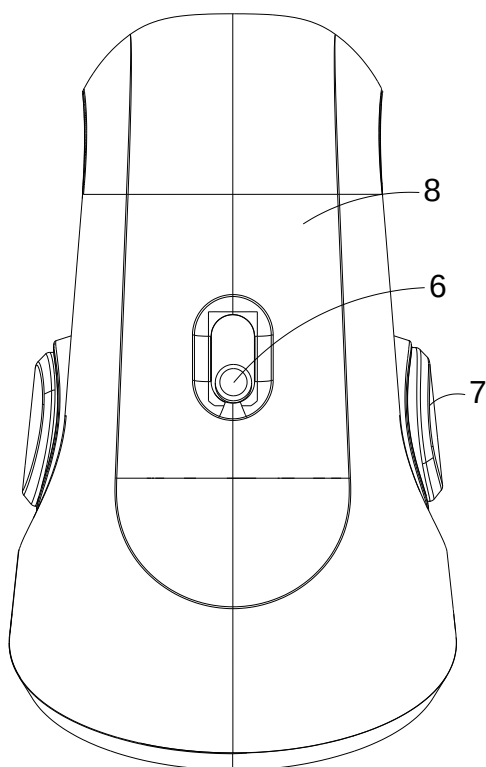


FIG. 1

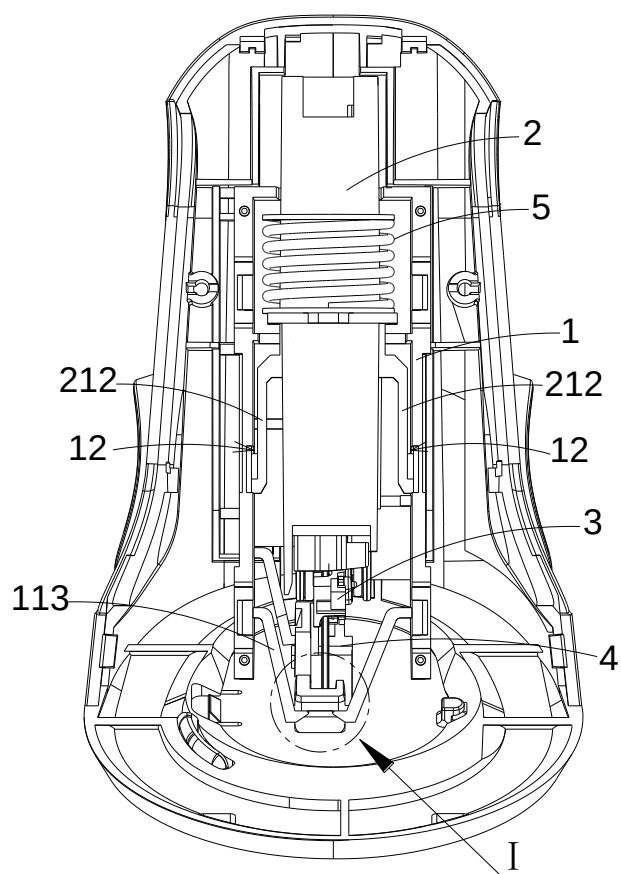


FIG. 2

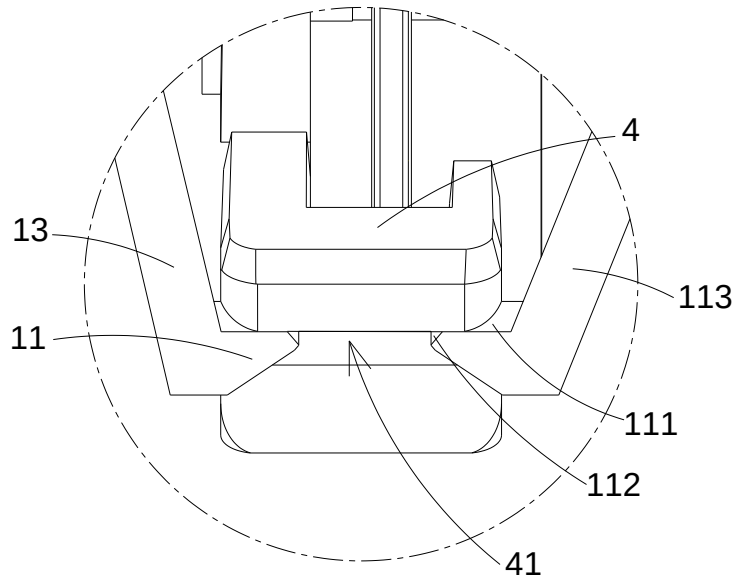


FIG. 3

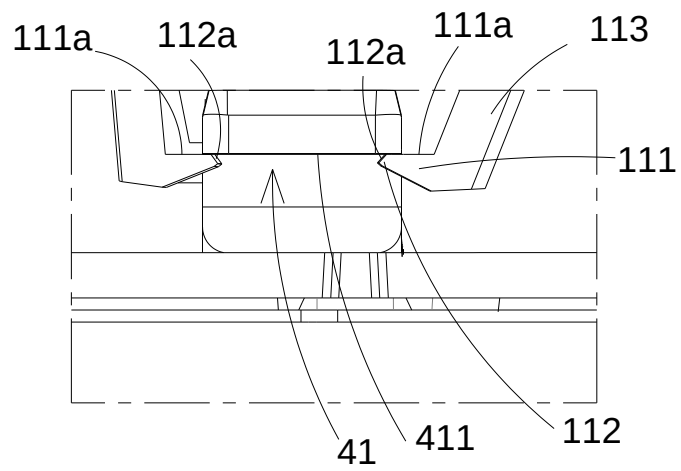


FIG. 4

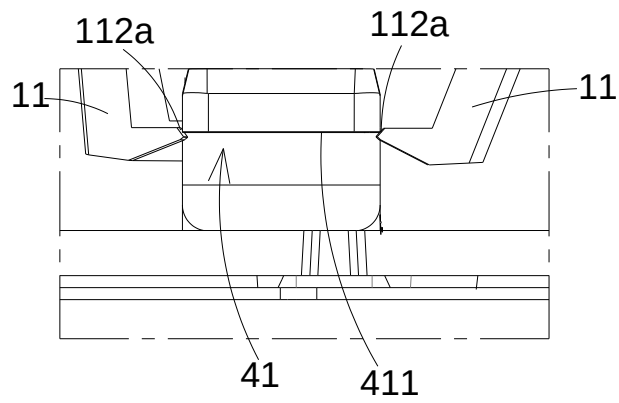


FIG. 5

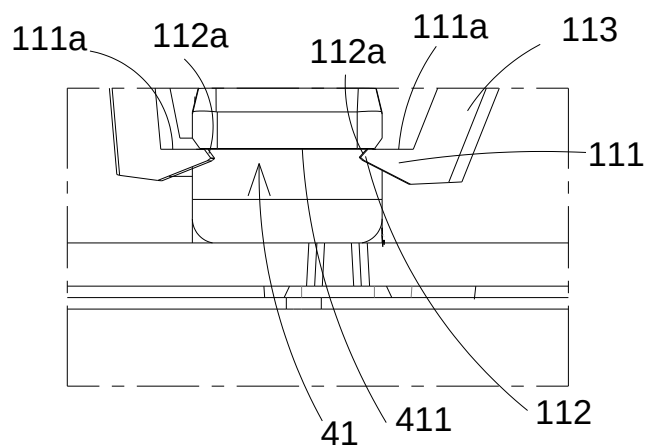


FIG. 6

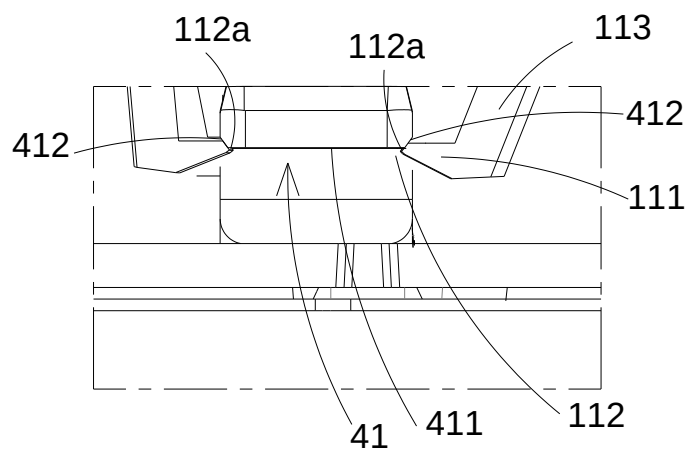


FIG. 7

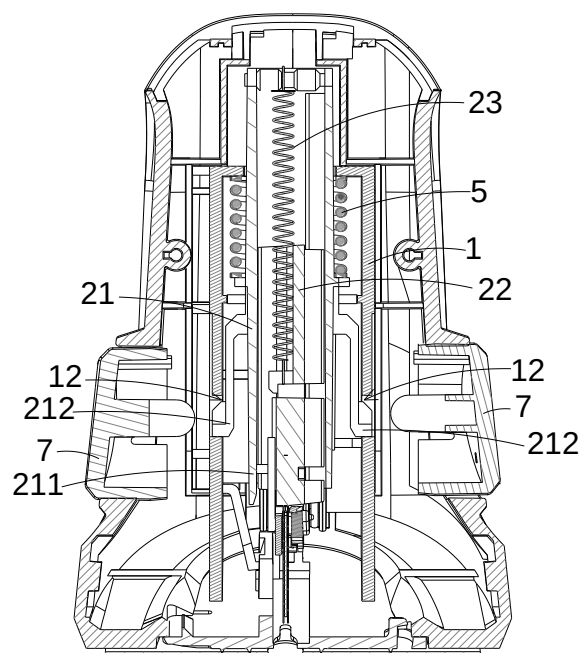


FIG. 8

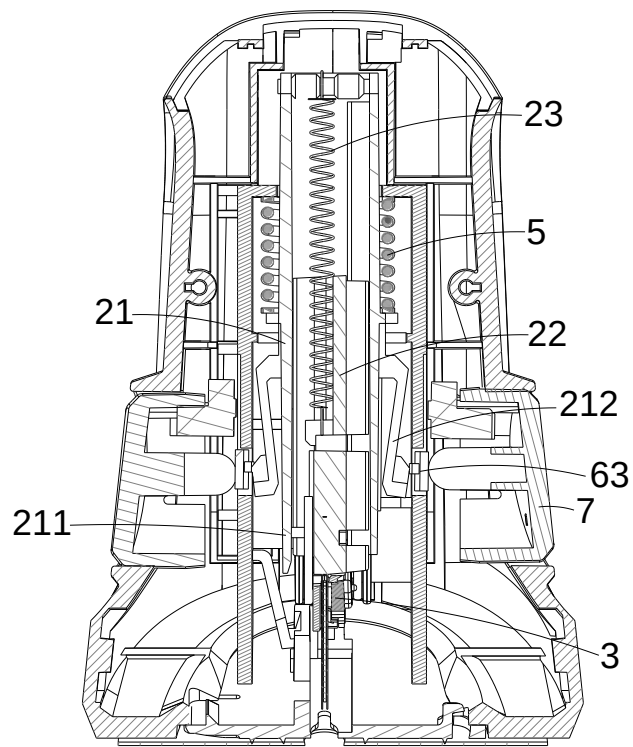


FIG. 9

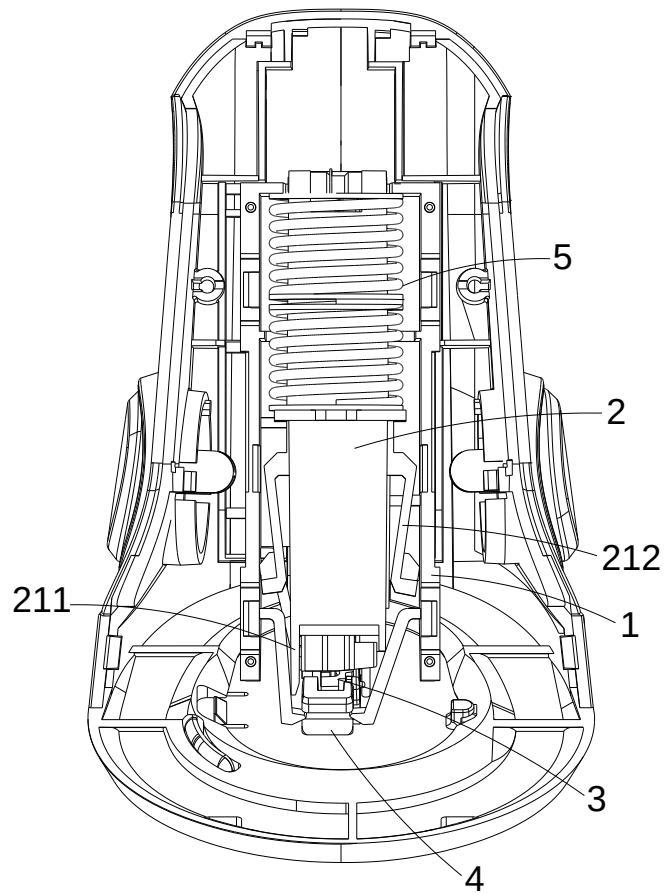


FIG. 10

Figure 1 is a perspective view of a medical device 1 in an open position. The device includes a handle 21, a trigger 22, a spring 23, a base 13, a trigger assembly 213, and a base assembly 3. The trigger assembly 213 is shown in a retracted position, and the base assembly 3 is shown in an extended position.

FIG. 12

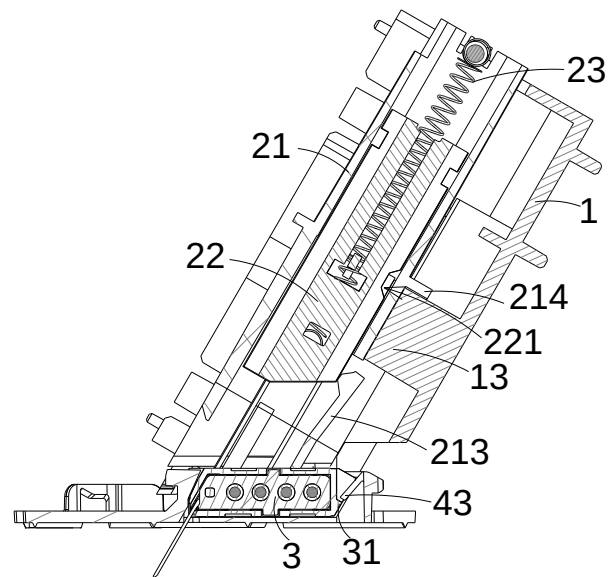


FIG. 13

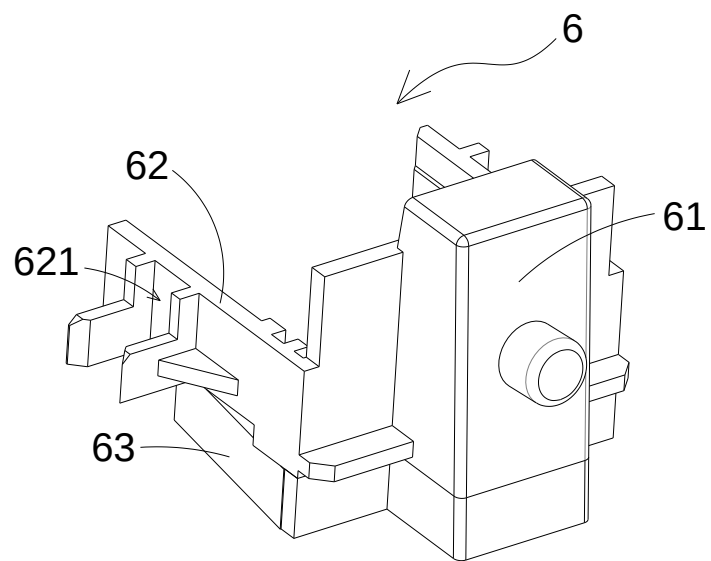


FIG. 14

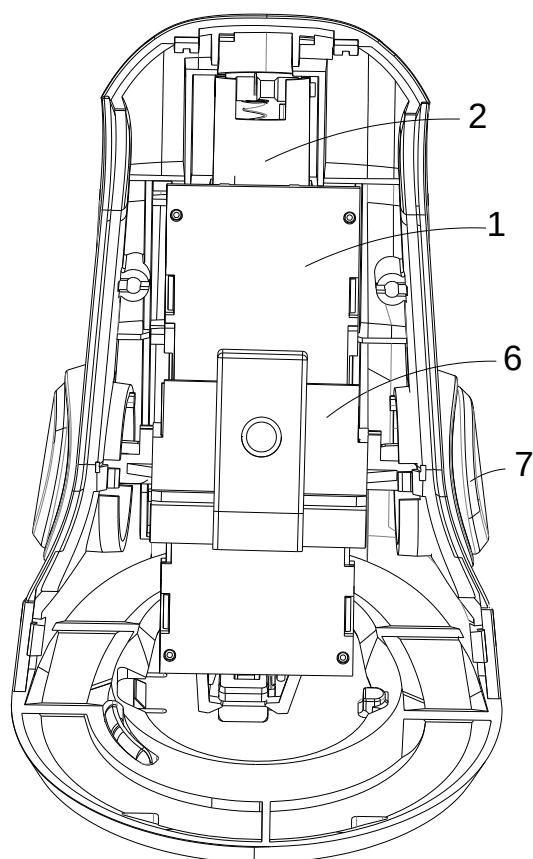


FIG. 15

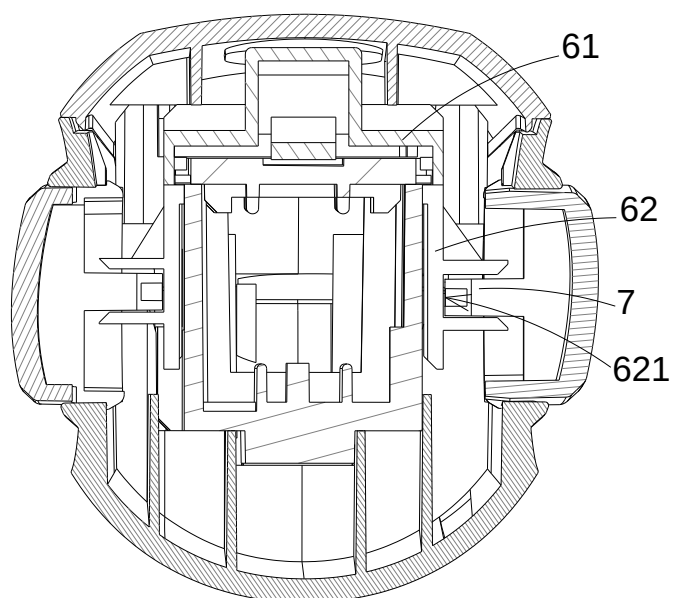


FIG. 16

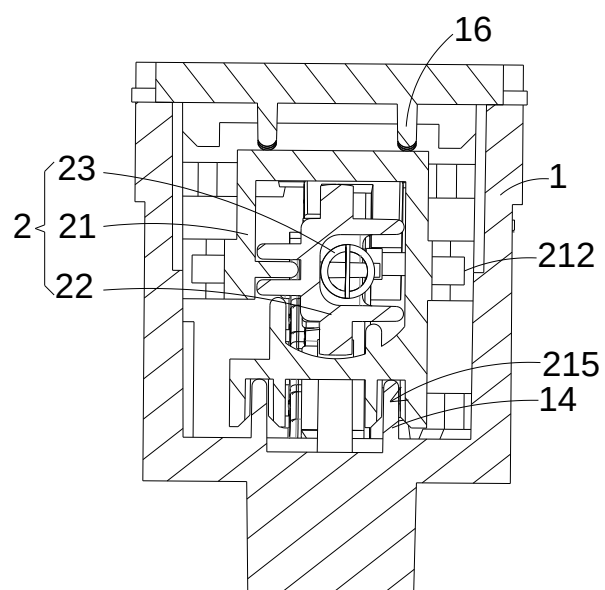


FIG. 17

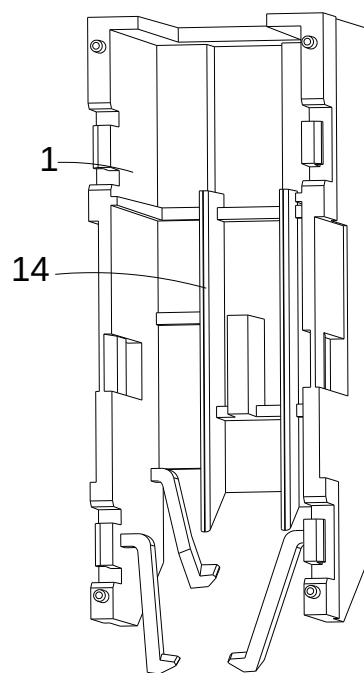


FIG. 18

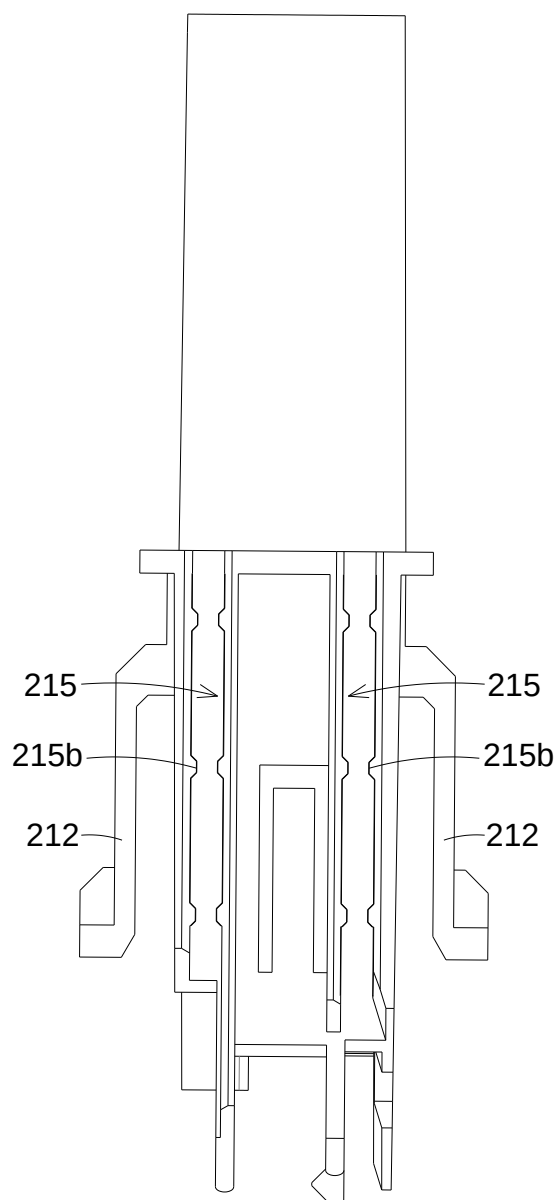


FIG. 19

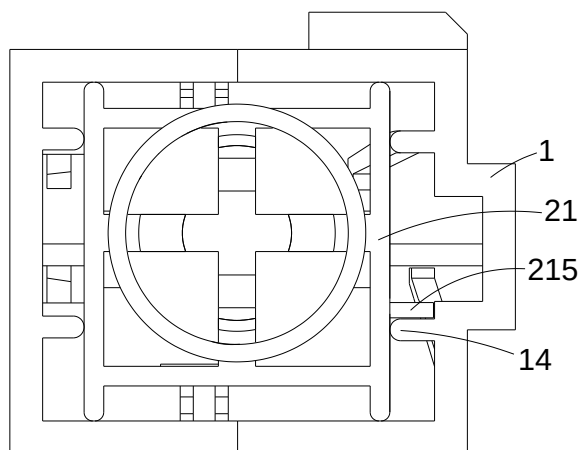


FIG. 20

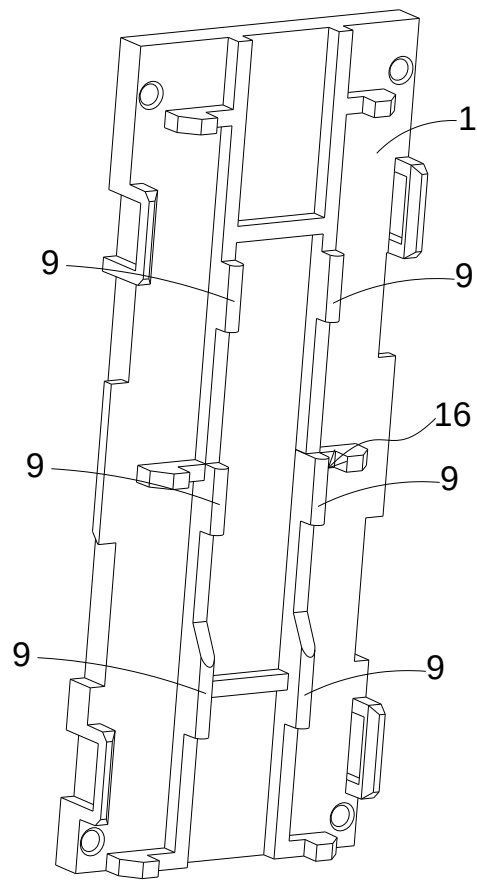


FIG. 21

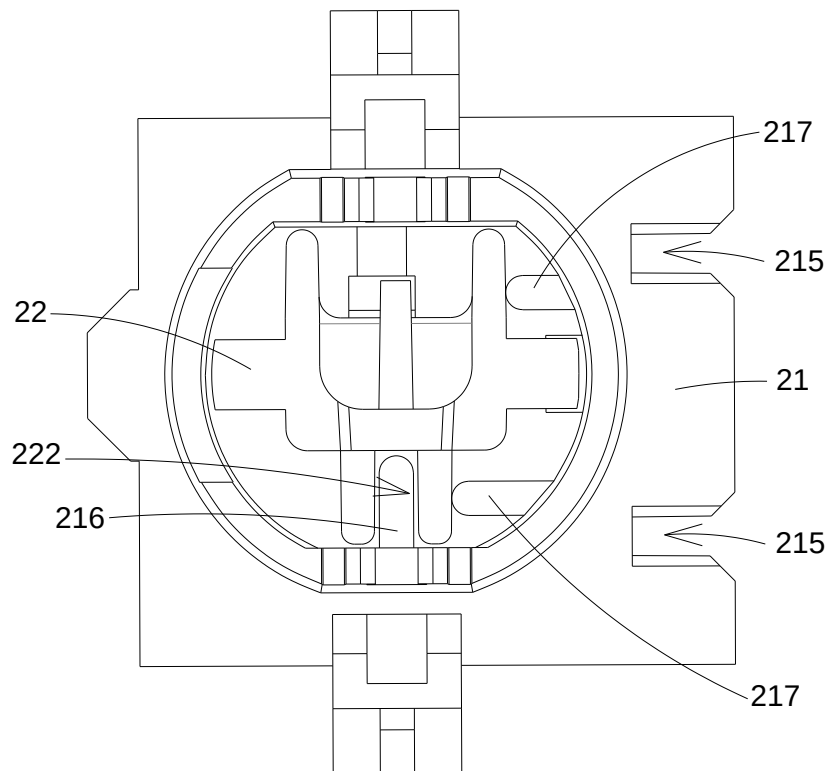


FIG. 22