




[図1]

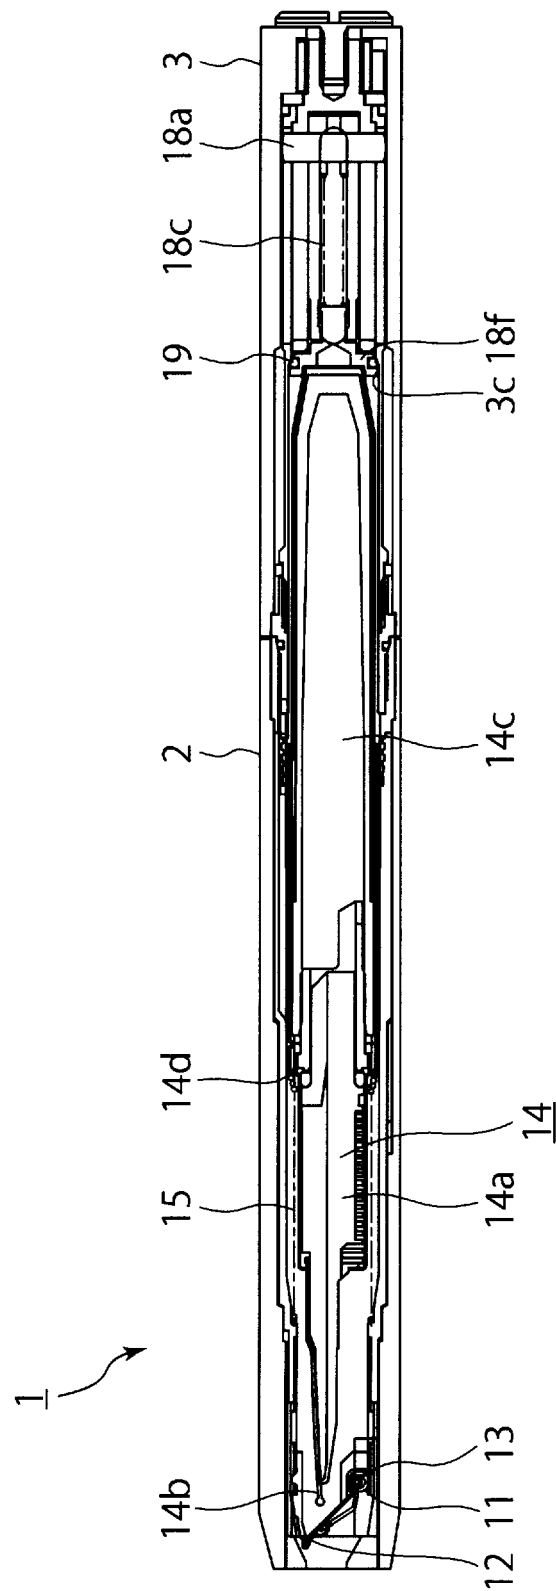


[図2]

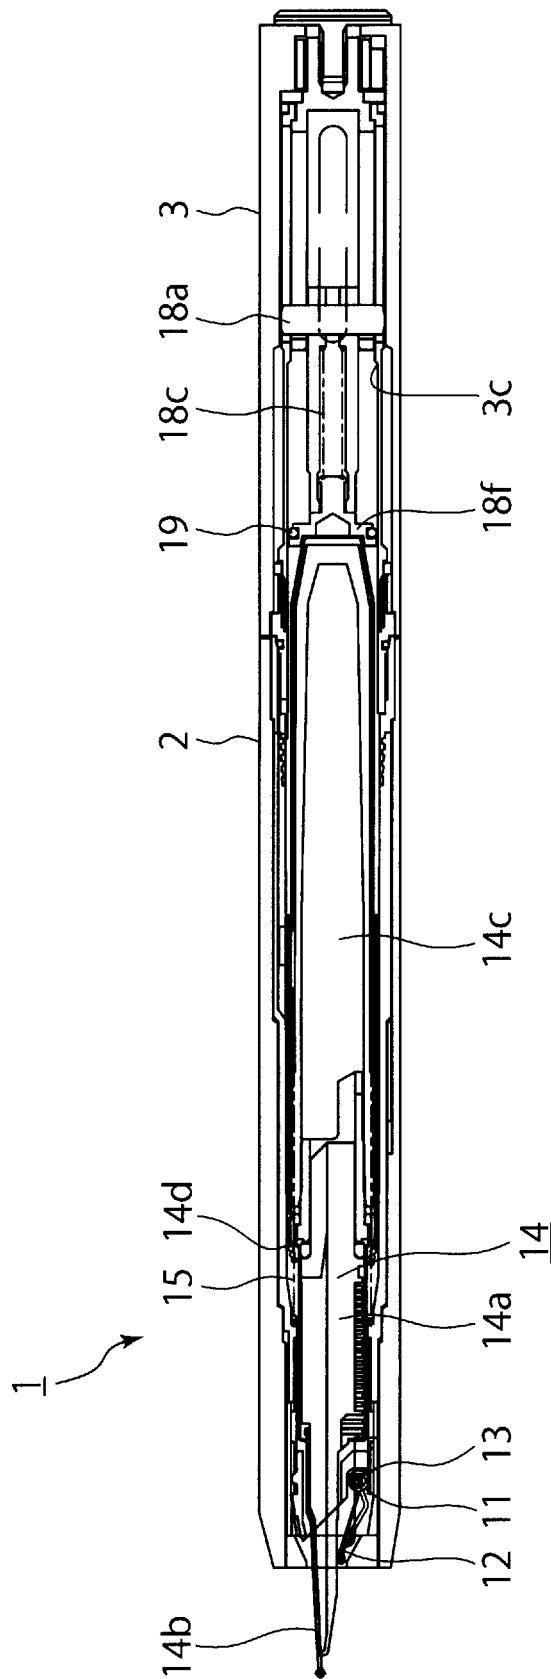


[図3]




[図4]

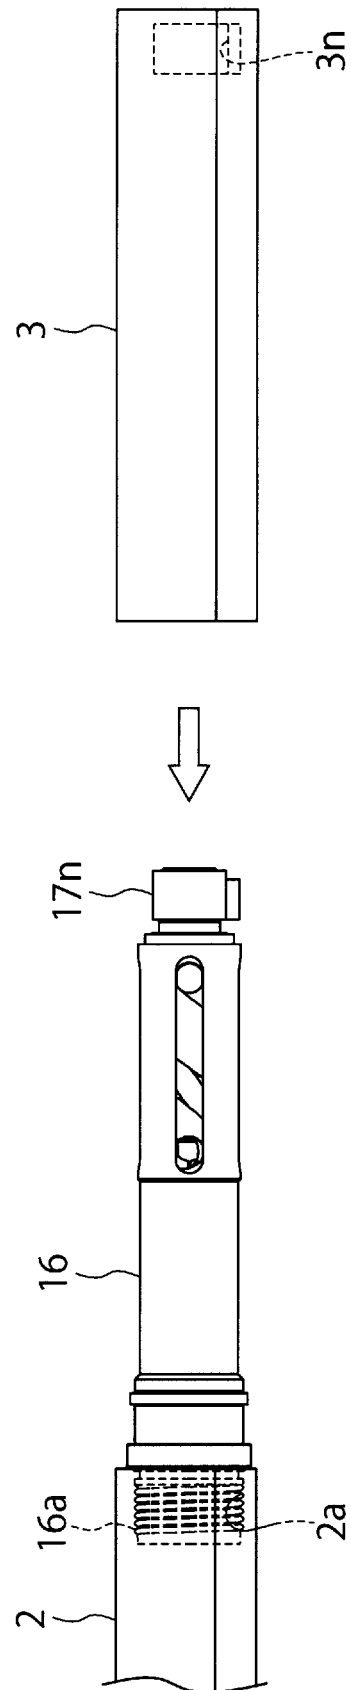


[図5]

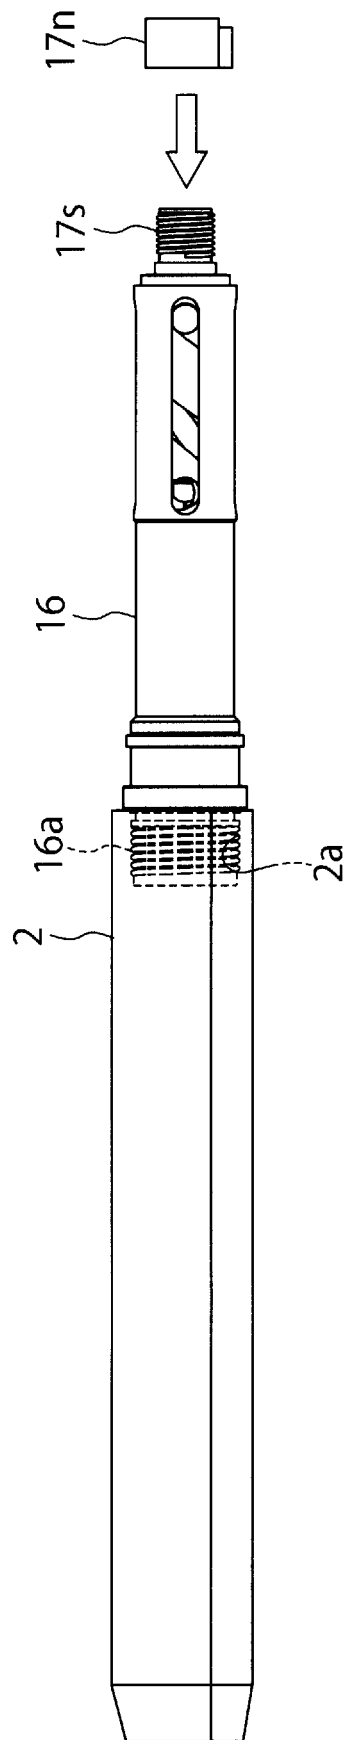

[図6]

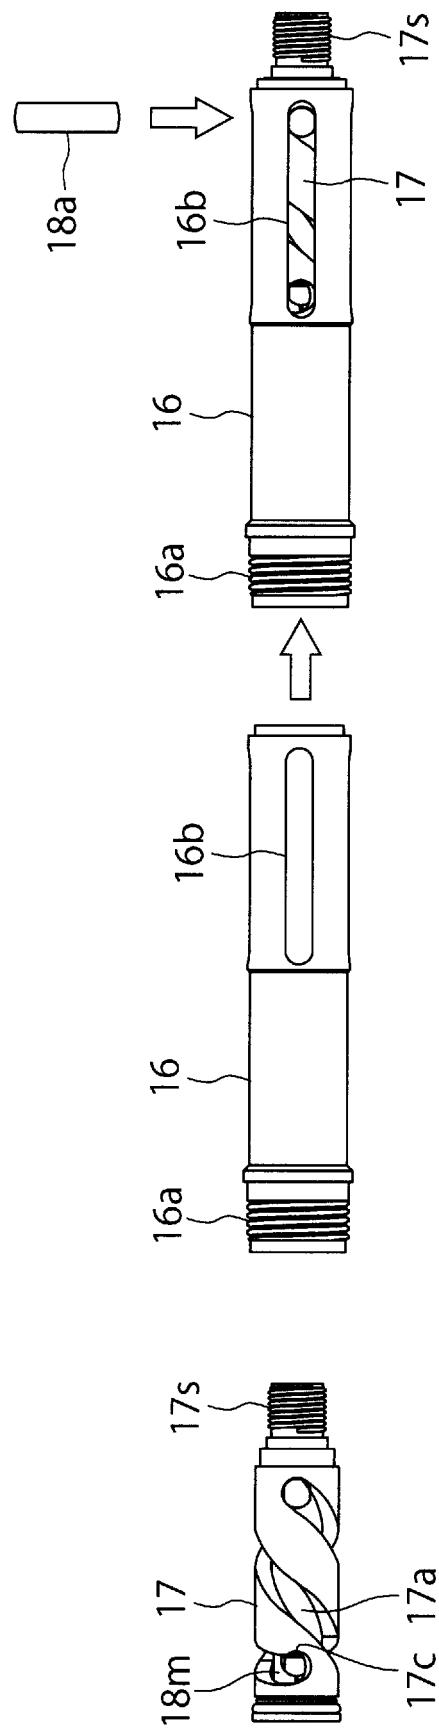

[図7]

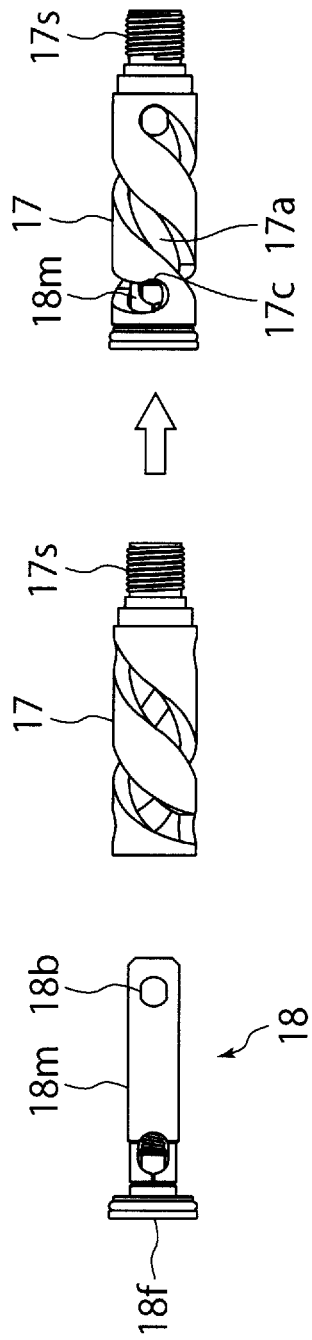

[図8]

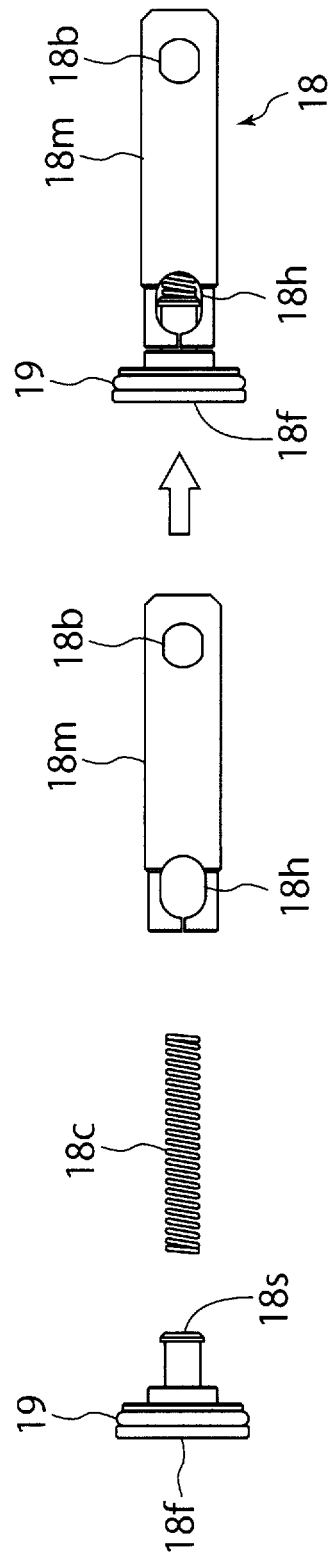




Fig. 1 is a longitudinal cross-sectional view of a medical device 101. The device includes a central shaft 107 with a proximal handle assembly 104 and a distal tip 114b. The handle assembly 104 includes a grip 116, a trigger 117, and a release button 118. The device is shown in a retracted state, with the distal tip 114b at the proximal end. A curved arrow at the bottom indicates the device can rotate.