

(43) International Publication Date
04 January 2024 (04.01.2024)



(10) International Publication Number
WO 2024/006267 A1



(51)	International Patent Classification: <i>G01N 35/00</i> (2006.01)	<i>G01N 35/10</i> (2006.01)
(21)	International Application Number:	PCT/US2023/026330
(22)	International Filing Date:	27 June 2023 (27.06.2023)
(25)	Filing Language:	English
(26)	Publication Language:	English
(30)	Priority Data: 63/355,879	27 June 2022 (27.06.2022) US
(71)	Applicant: ILLUMINA, INC. [US/US]; 5200 Illumina Way, San Diego, CA 92122 (US).	
(72)	Inventor: CRANE, Bryan; c/o Illumina, Inc., 5200 Illumina Way, San Diego, CA 92122 (US).	

(74) **Agent: JORGE, Matthew, M.;** Marshall, Gerstein & Borun LLP, 233 S. Wacker Drive, 6300 Willis Tower, Chicago, IL 60606-6357 (US).

(81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CV, CZ, DE, DJ, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IQ, IR, IS, IT, JM, JO, JP, KE, KG, KH, KN, KP, KR, KW, KZ, LA, LC, LK, LR, LS, LU, LY, MA, MD, MG, MK, MN, MU, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, WS, ZA, ZM, ZW.

(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, CV, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SC, SD, SL, ST, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ,

(54) Title: SUBSTRATES FOR PERFORMING QUANTIFICATION PROCESSES AND RELATED SYSTEMS AND METHODS

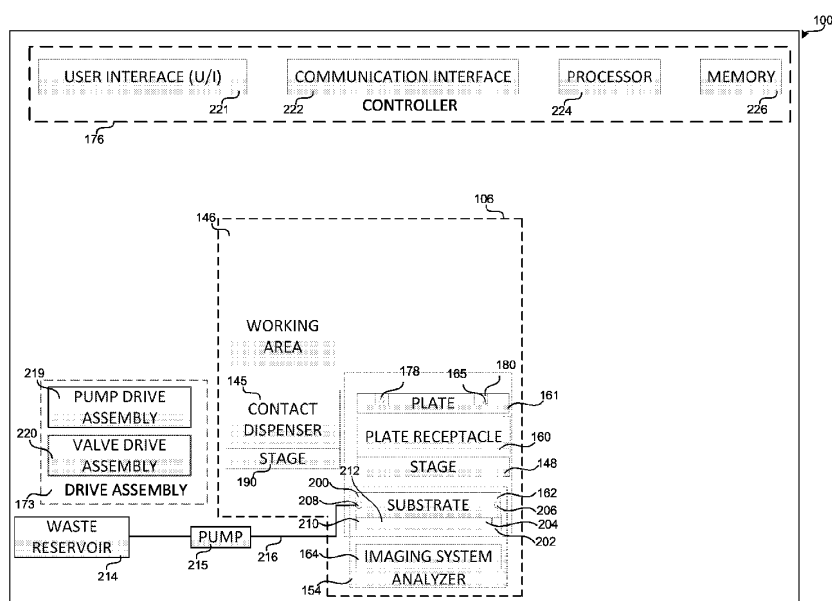


FIG. 1

(57) Abstract: Substrates for performing quantification processes and related systems and methods are disclosed. In an implementation, an apparatus includes a substrate and an imaging system. The substrate includes a pair of plates and a plurality of spacers positioned between the plates to define a gap between the pair of plates. A portion of a sample is to be received within the gap of the substrate and the imaging system is to obtain image data of the portion of the sample. The image data is to be used to determine a concentration of the portion of the sample.

[Continued on next page]

WFO 2024/006267 A1

DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT,
LU, LV, MC, ME, MK, MT, NL, NO, PL, PT, RO, RS, SE,
SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN,
GQ, GW, KM, ML, MR, NE, SN, TD, TG).

Published:

- *with international search report (Art. 21(3))*
- *before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))*