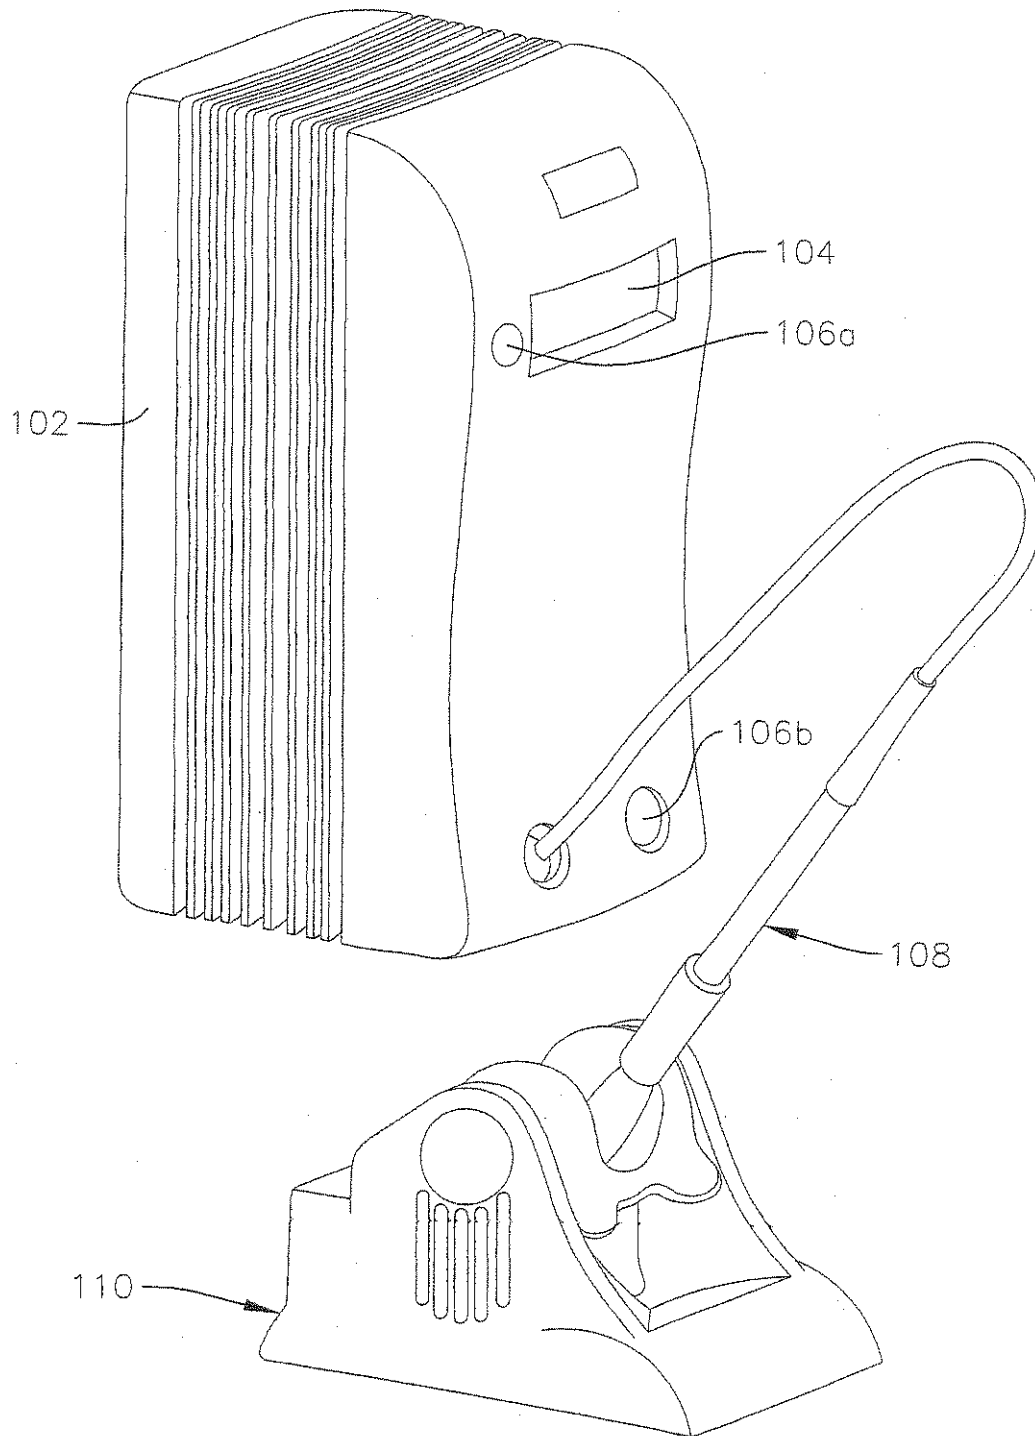


FIG. 1A



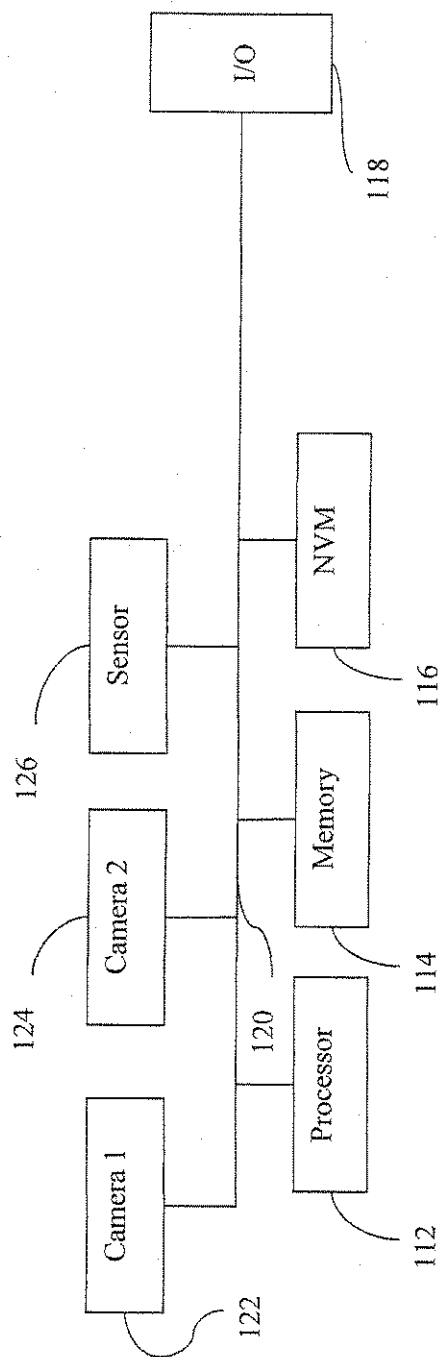


FIG. 1B

FIG. 1C

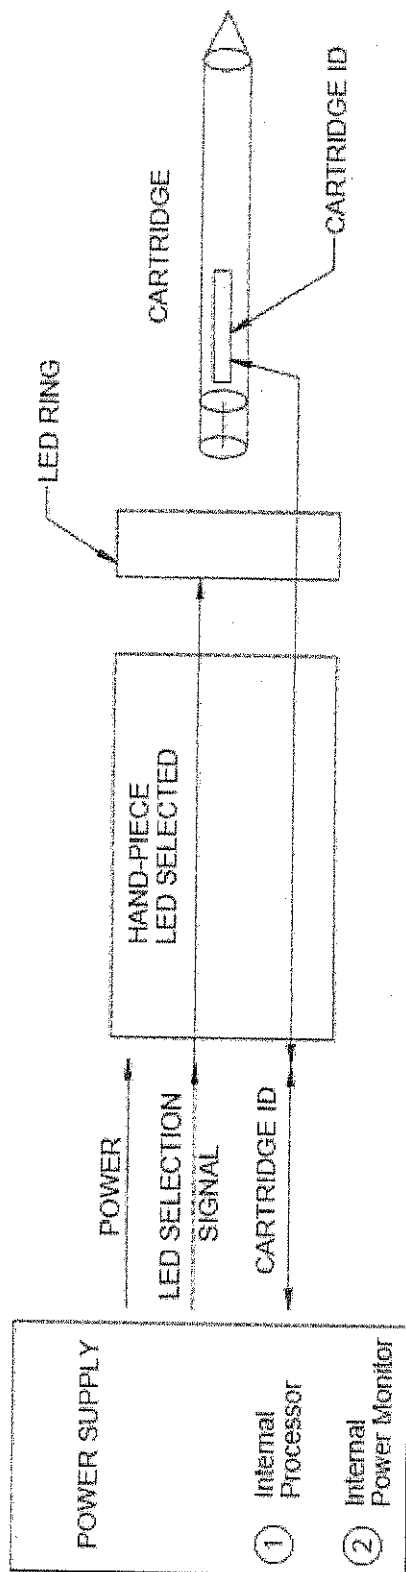


FIG. 1D

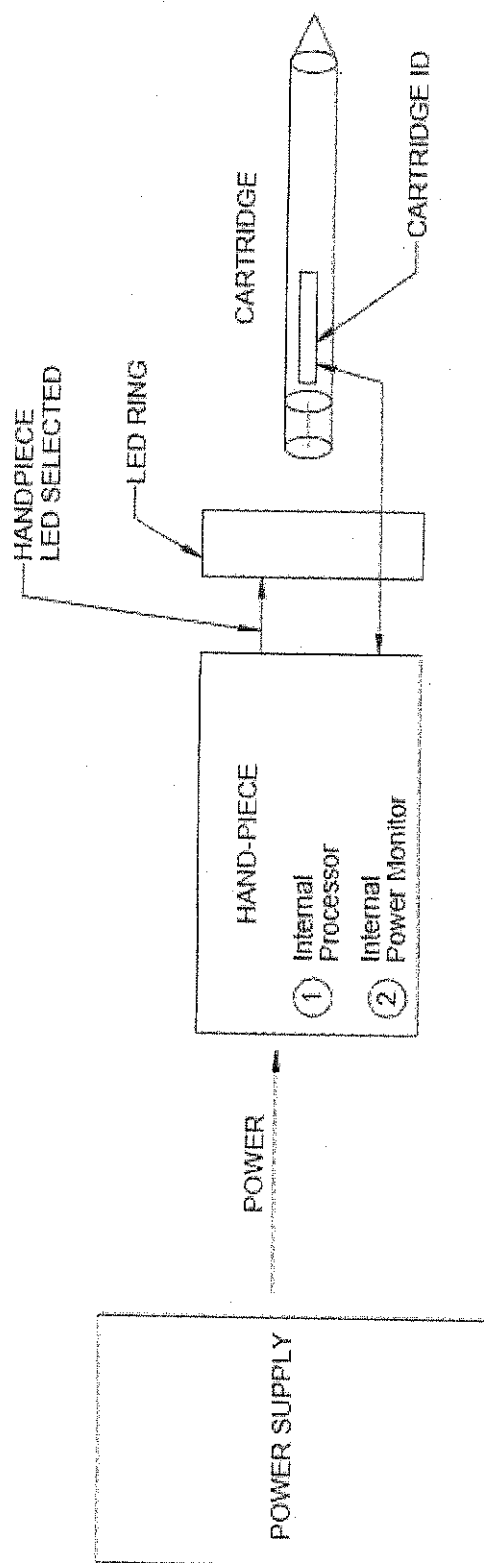


FIG. 1E

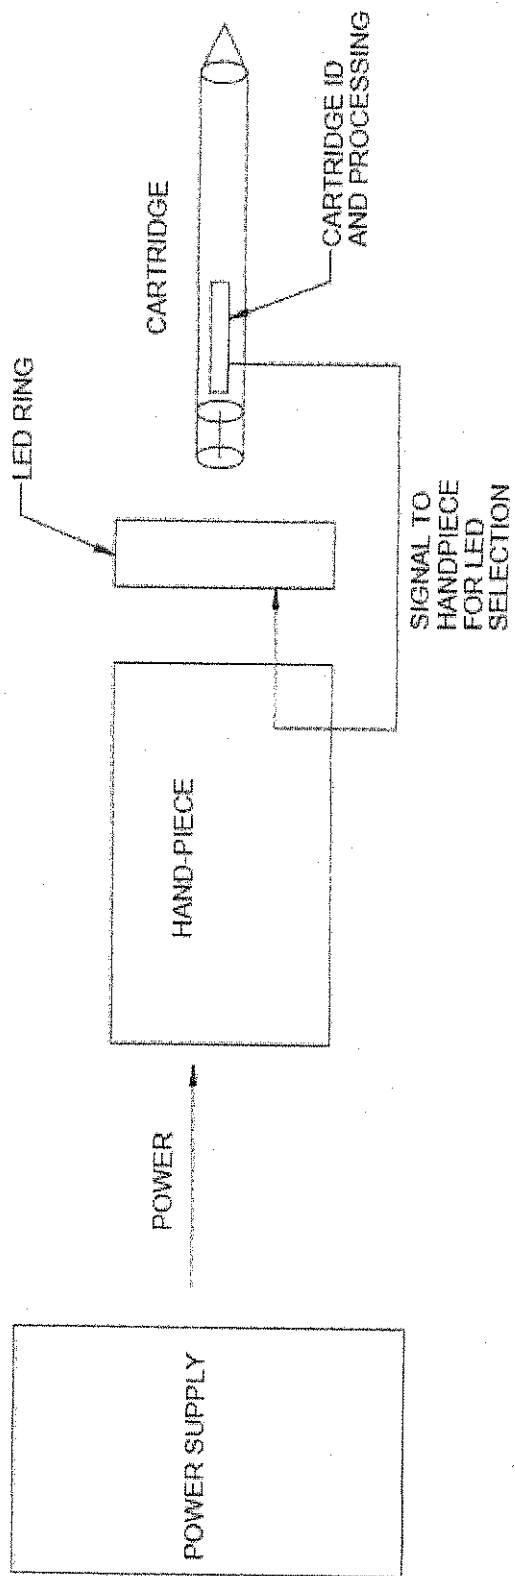


FIG. 1F

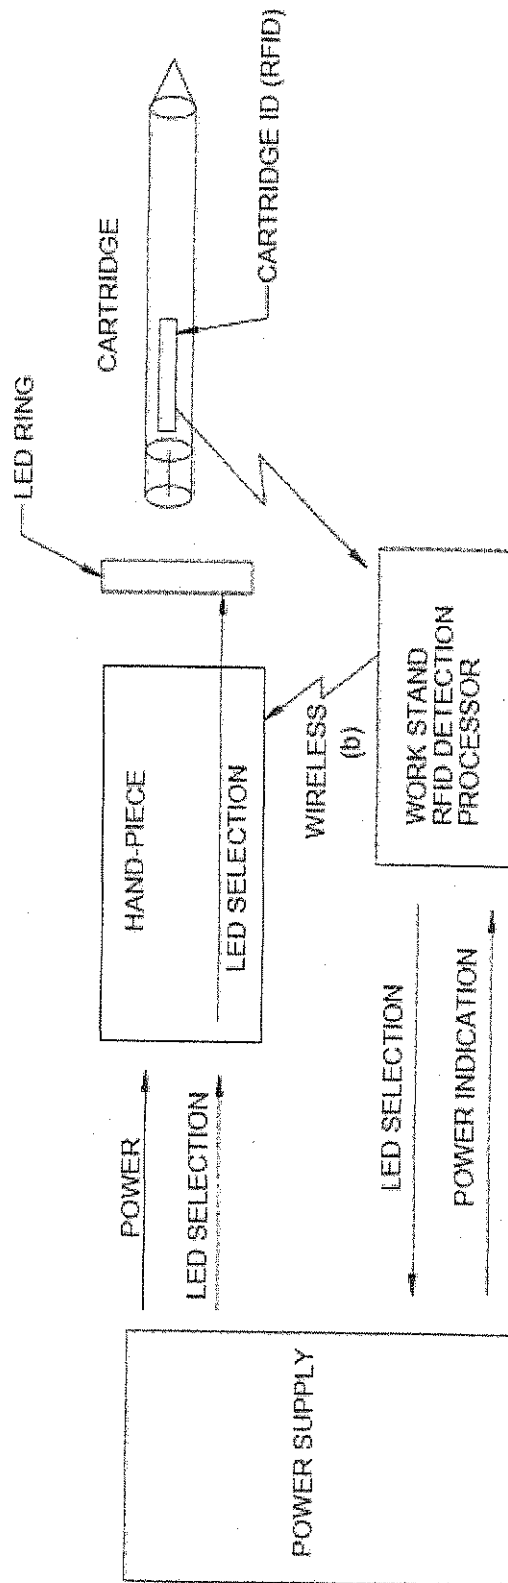


FIG. 1G

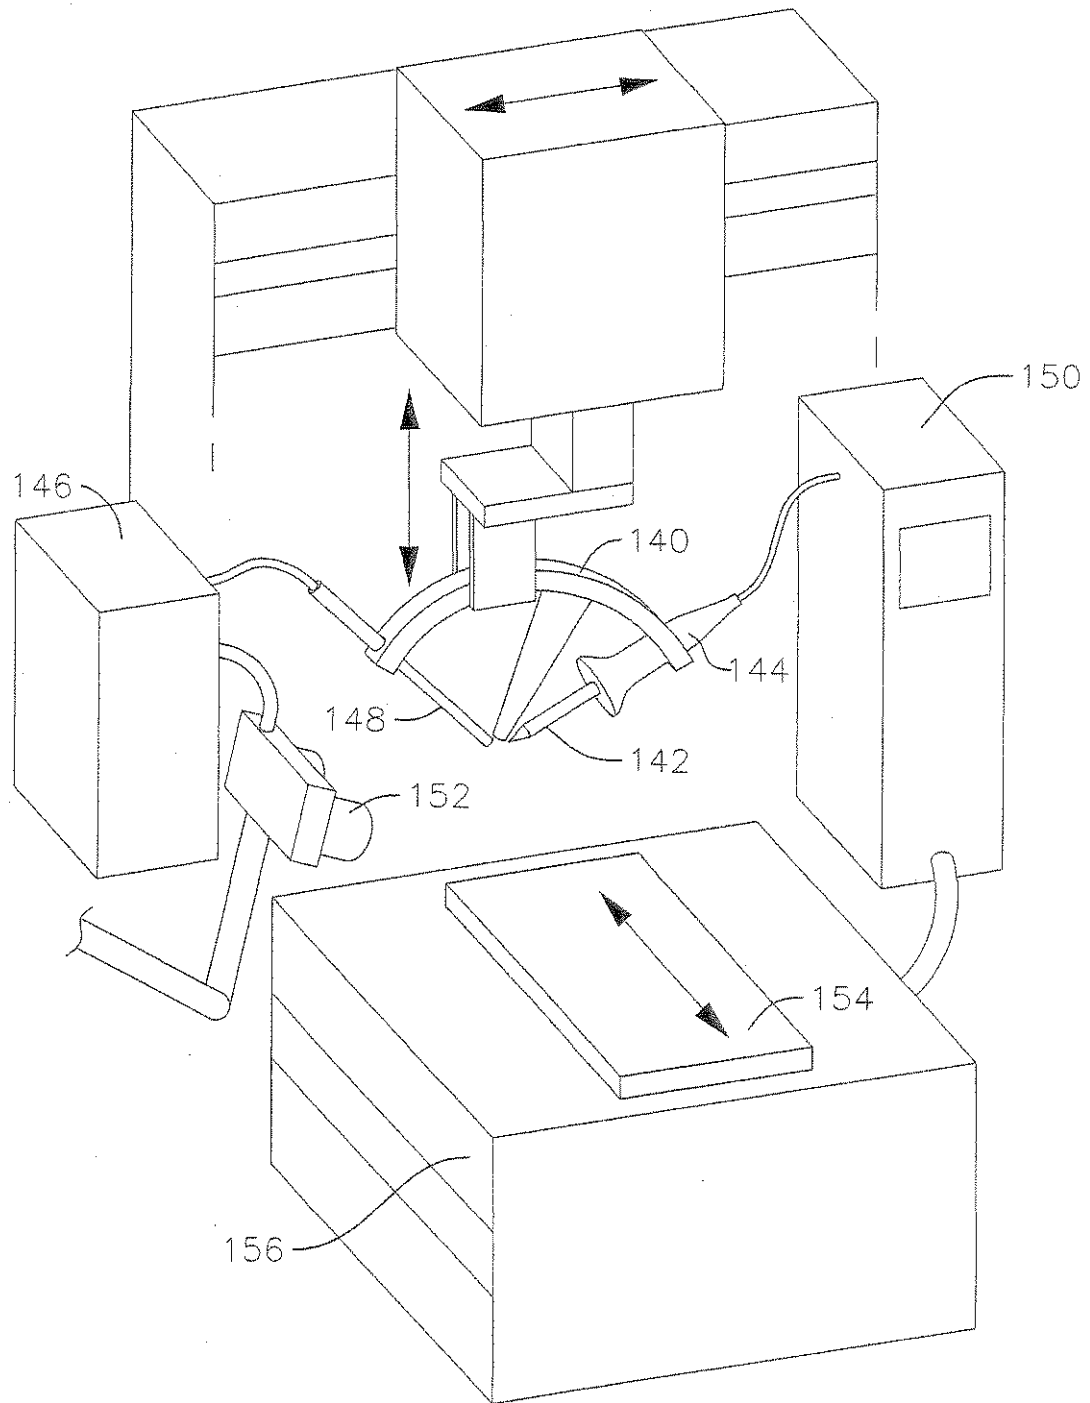


FIG. 2

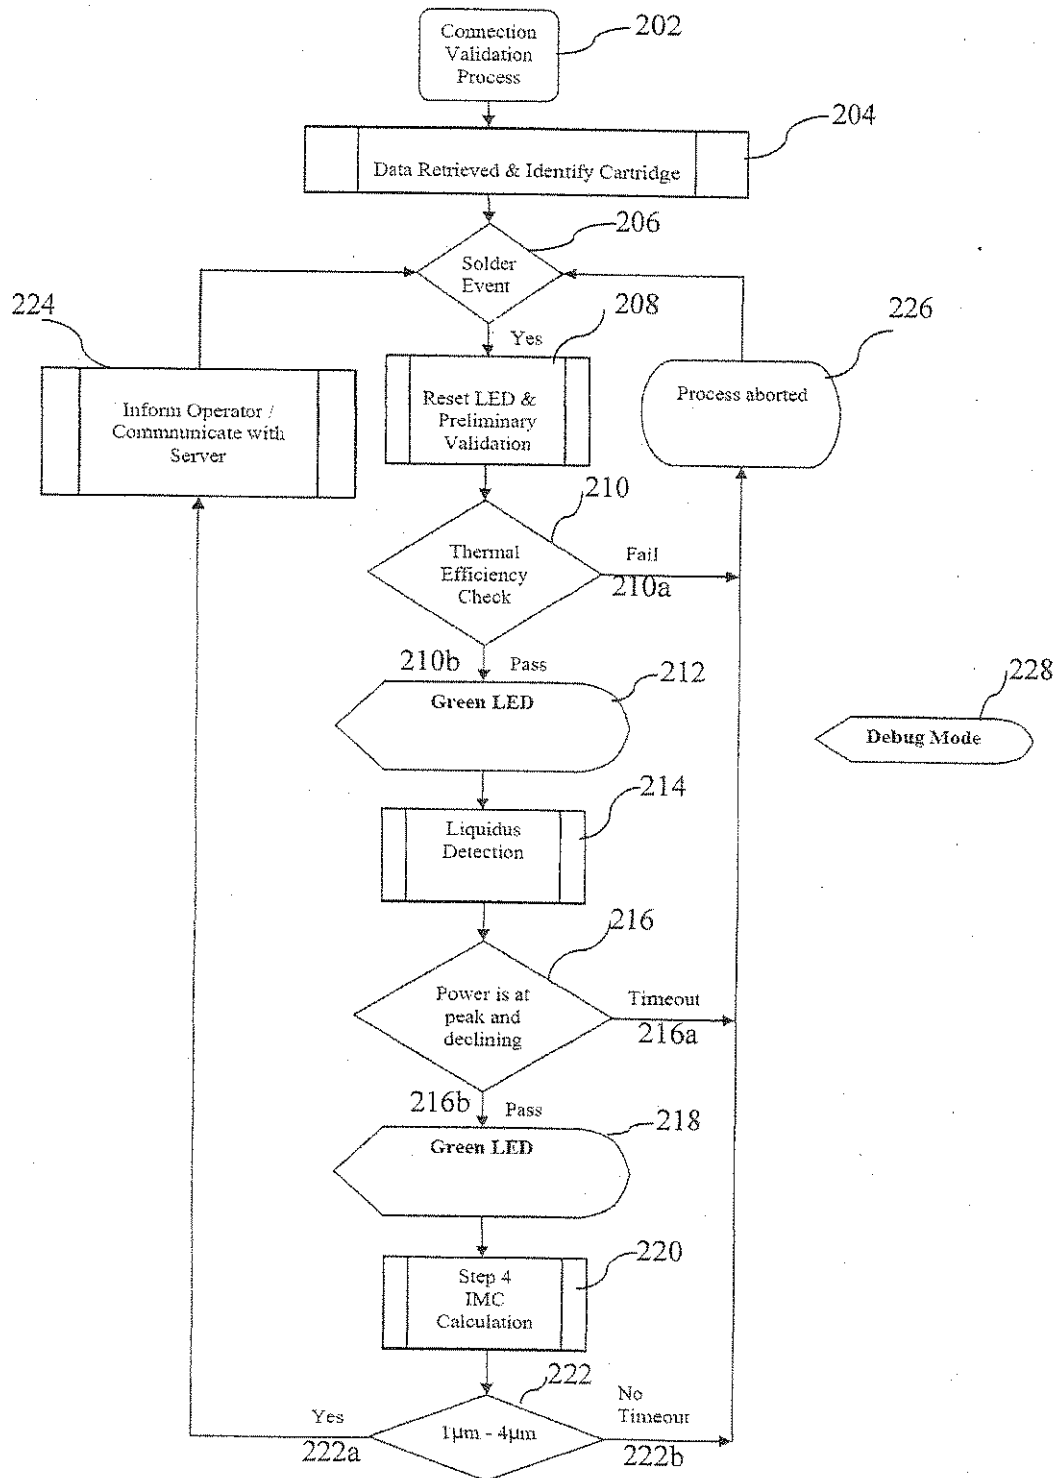


FIG. 3A

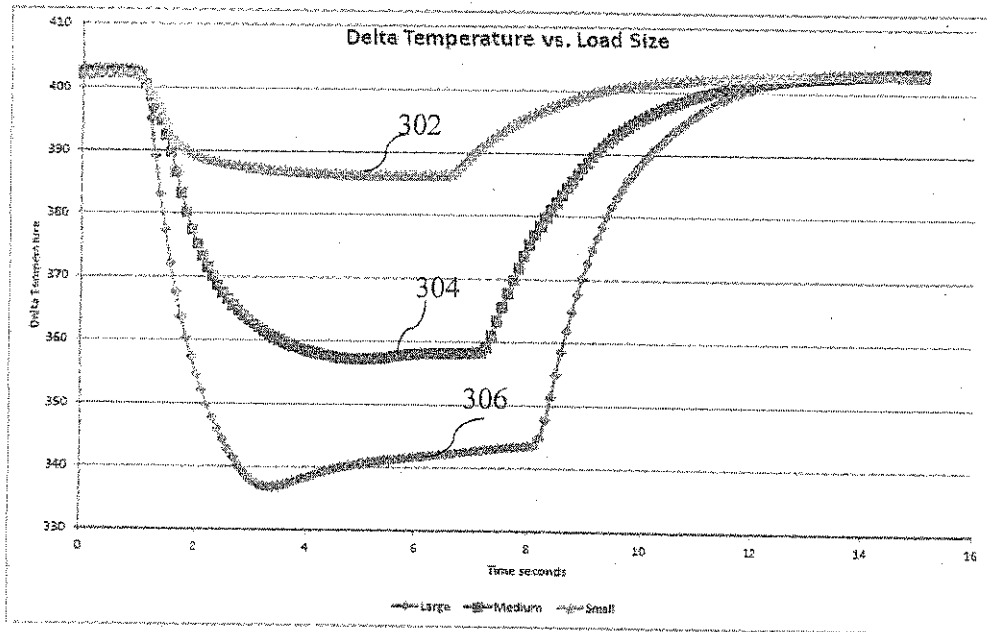


FIG. 3B

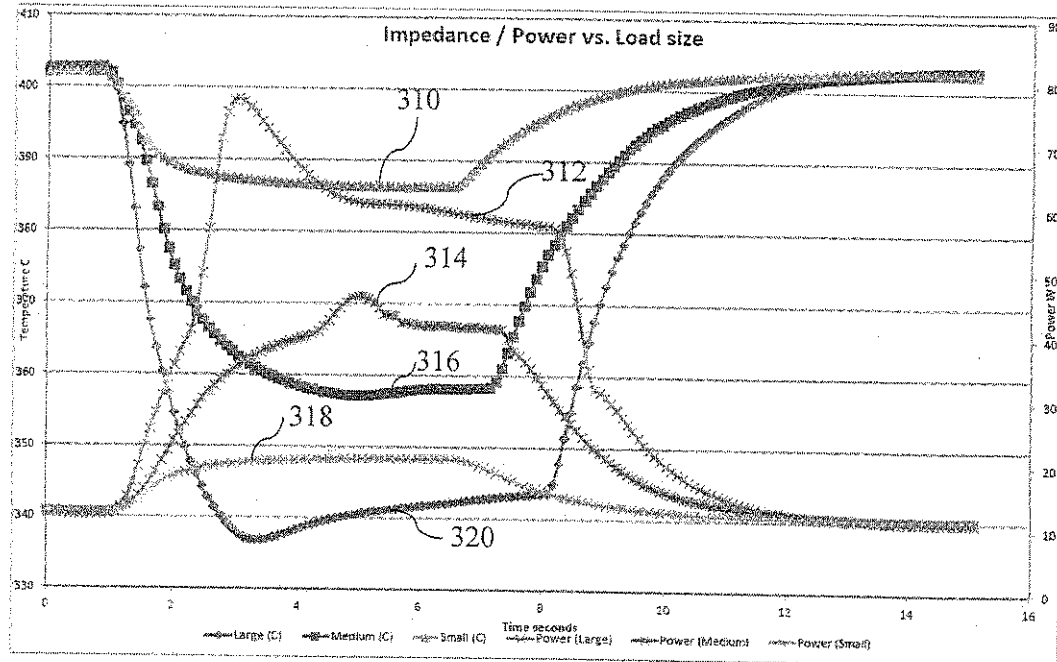


FIG. 4A

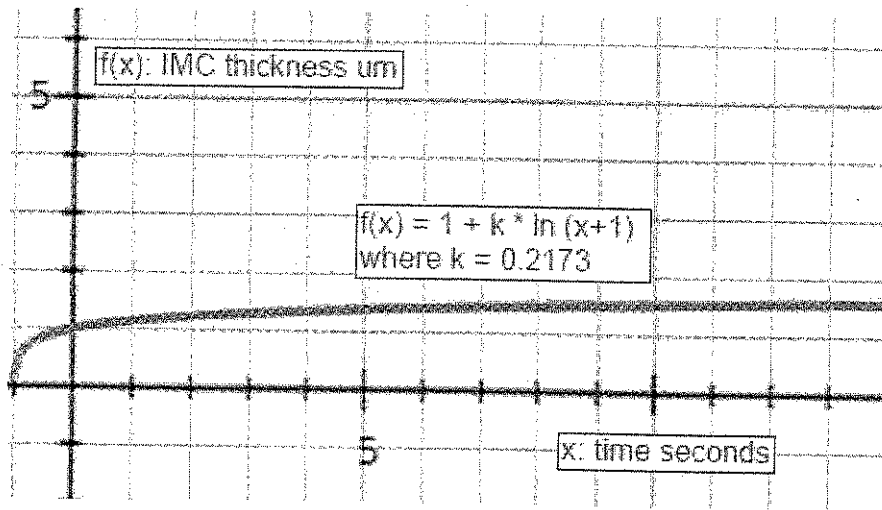


FIG. 4B

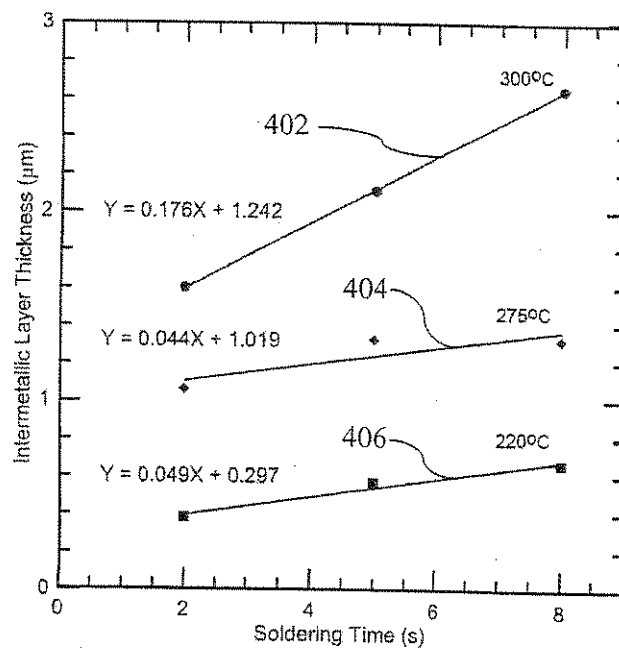


FIG. 4C

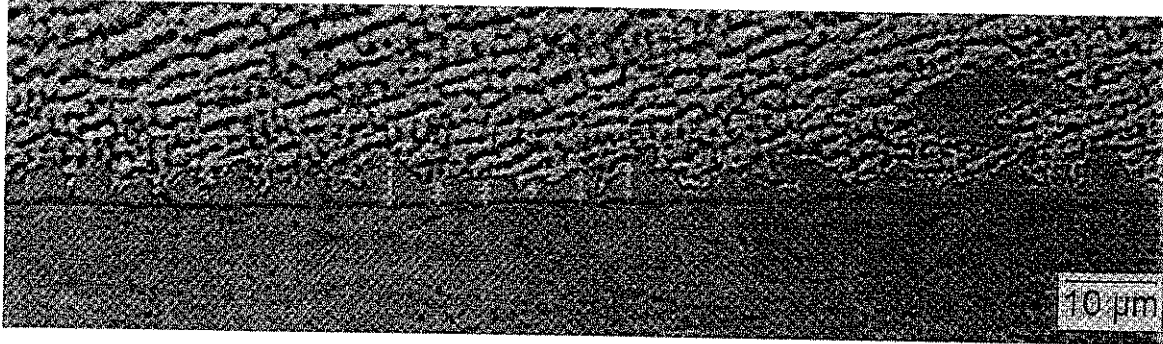


FIG. 5



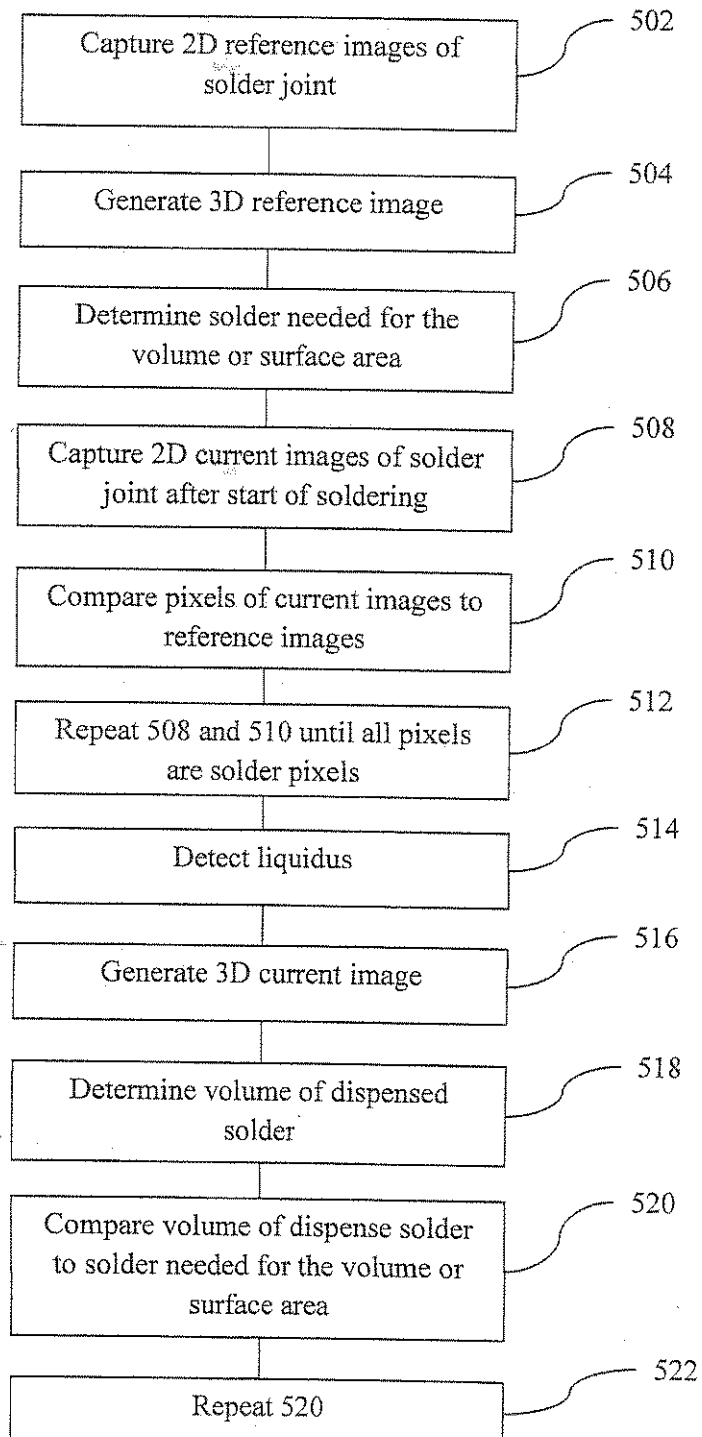


FIG. 6A

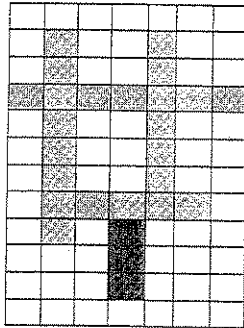


Sample

FIG. 6B

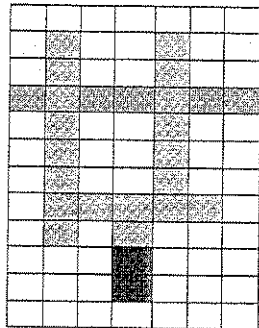


Current

FIG. 6C

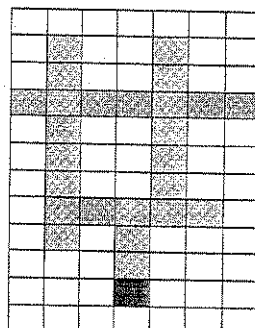

Current

FIG. 6D

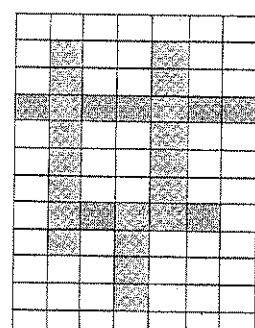

Liquidus detected

FIG. 7A

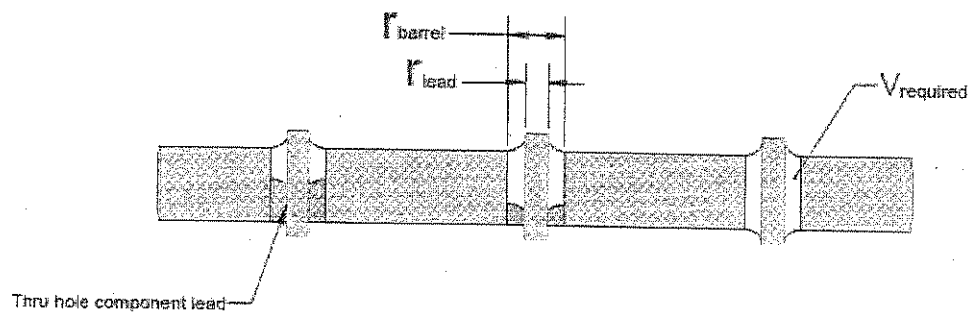


FIG. 7B

