

FIG. 1


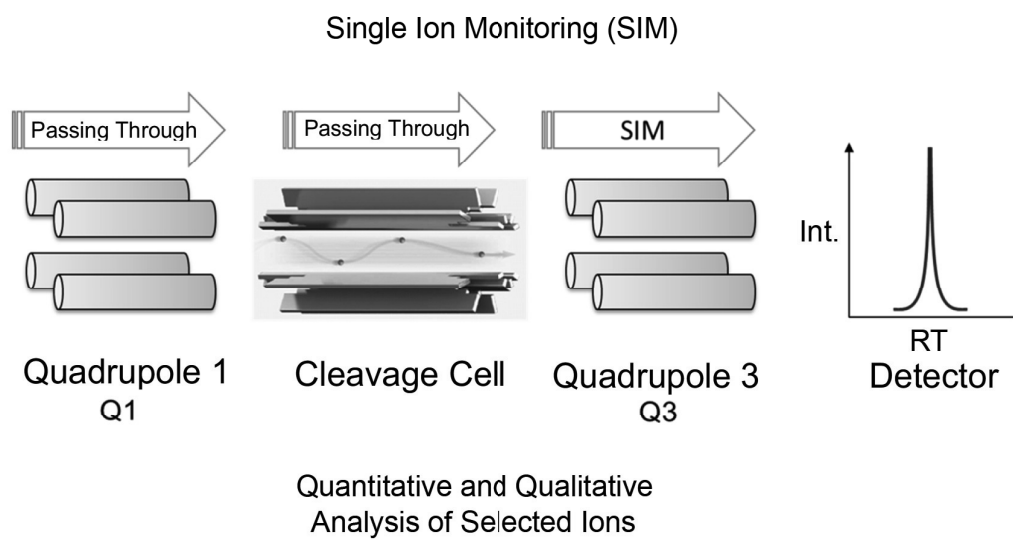


FIG. 2

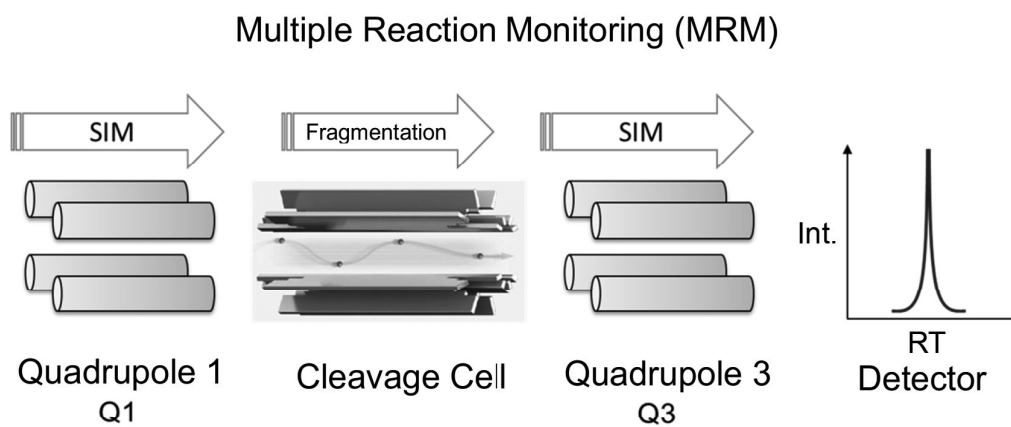

Ultrasensitive Quantitative Analysis of Single Ion

FIG. 3

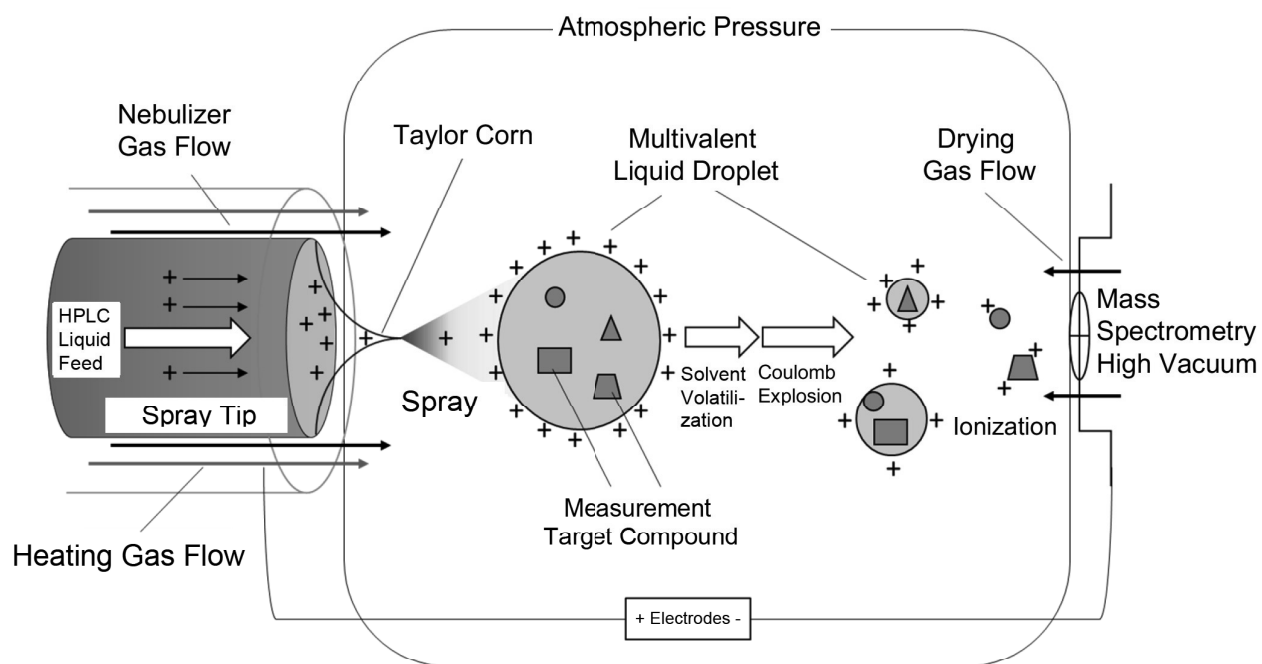


FIG. 4

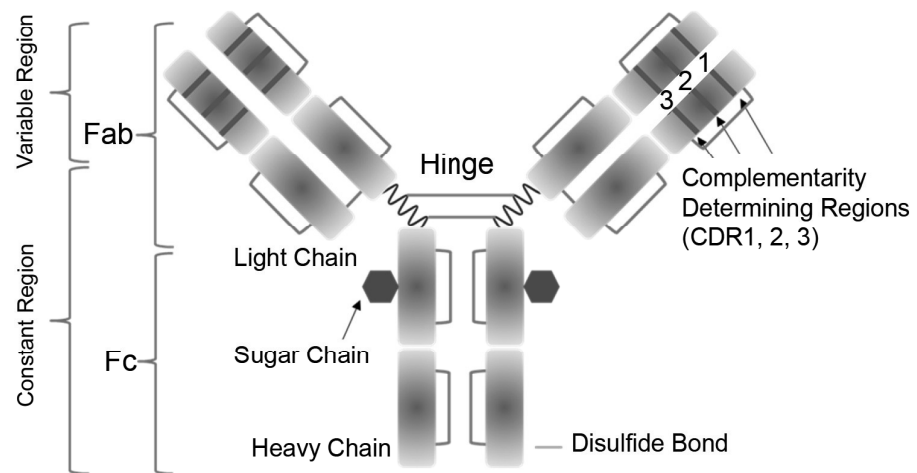


FIG. 5

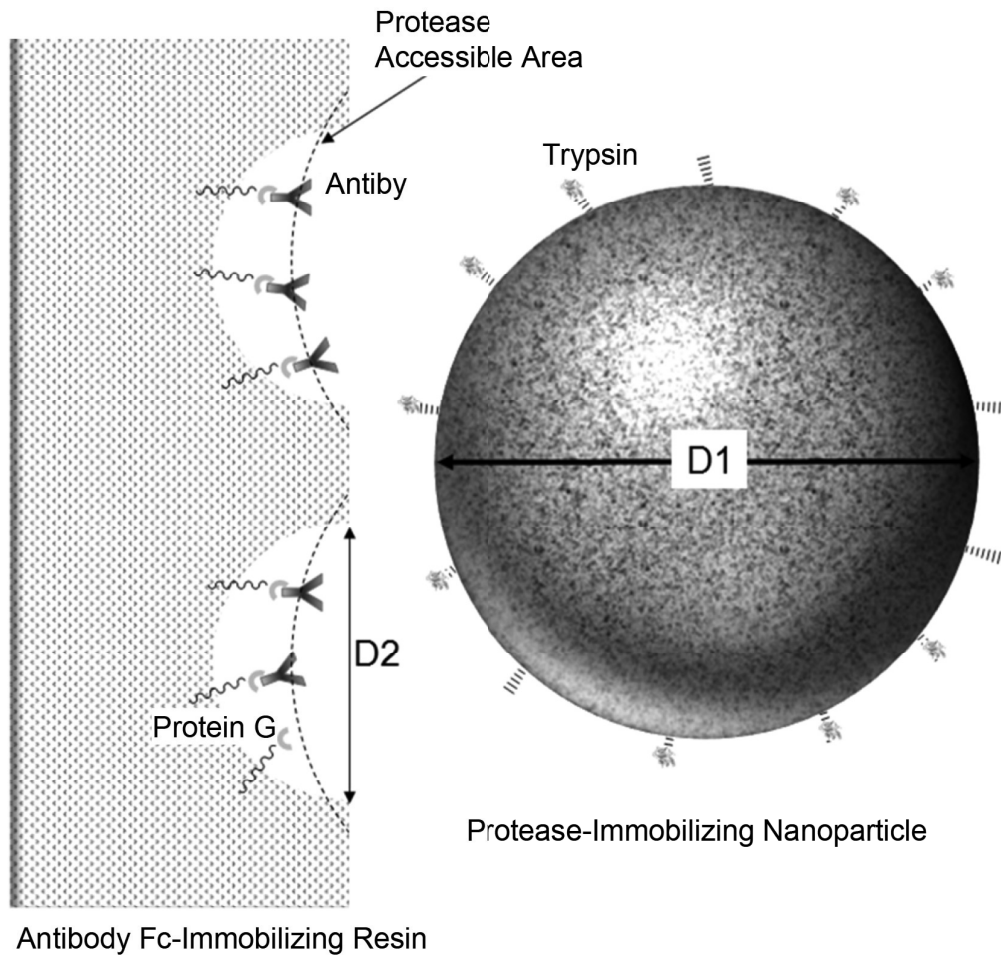


FIG. 6A

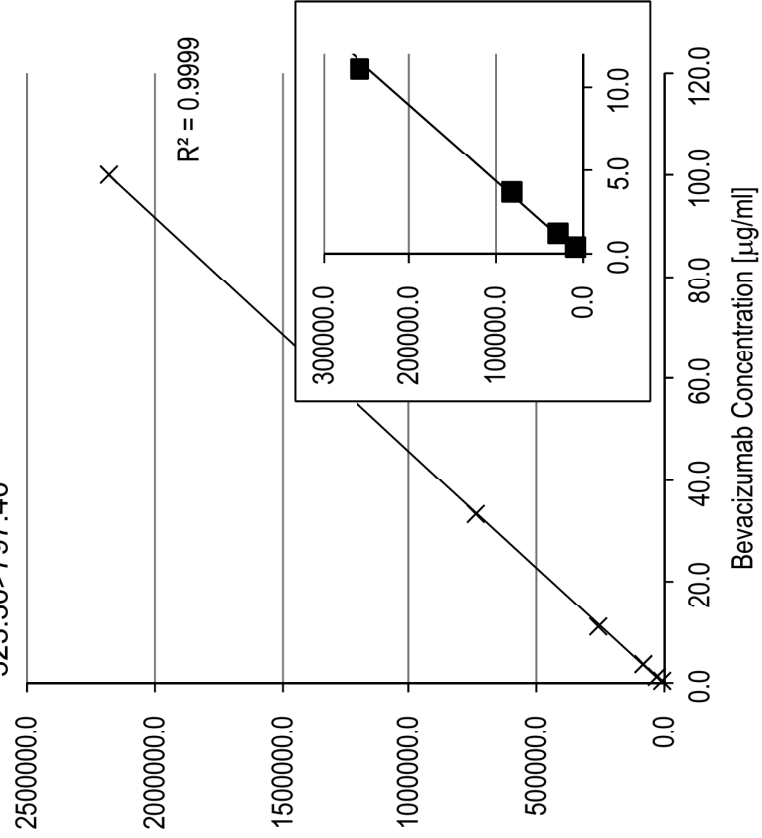
FTFSLDTSK
523.30>797.40

FIG. 6B

VLIYFTSSLHSGVPSR
588.30>775.90