

Fig. 1

1

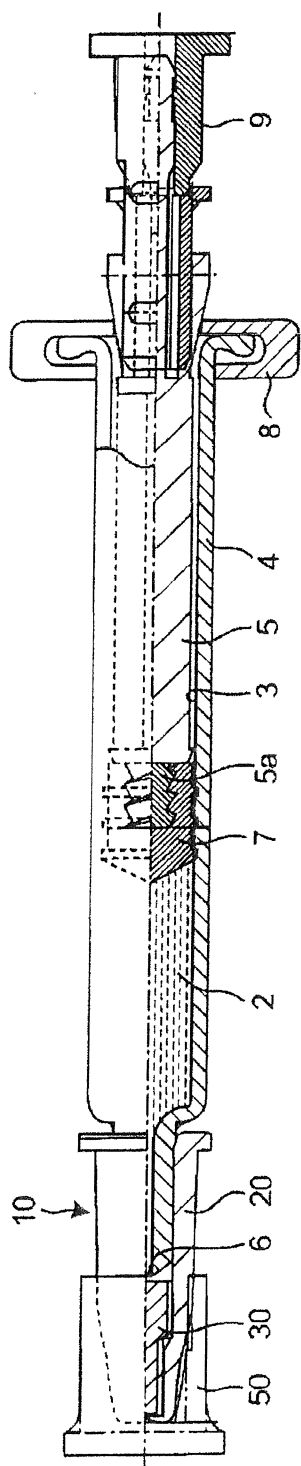


Fig. 2

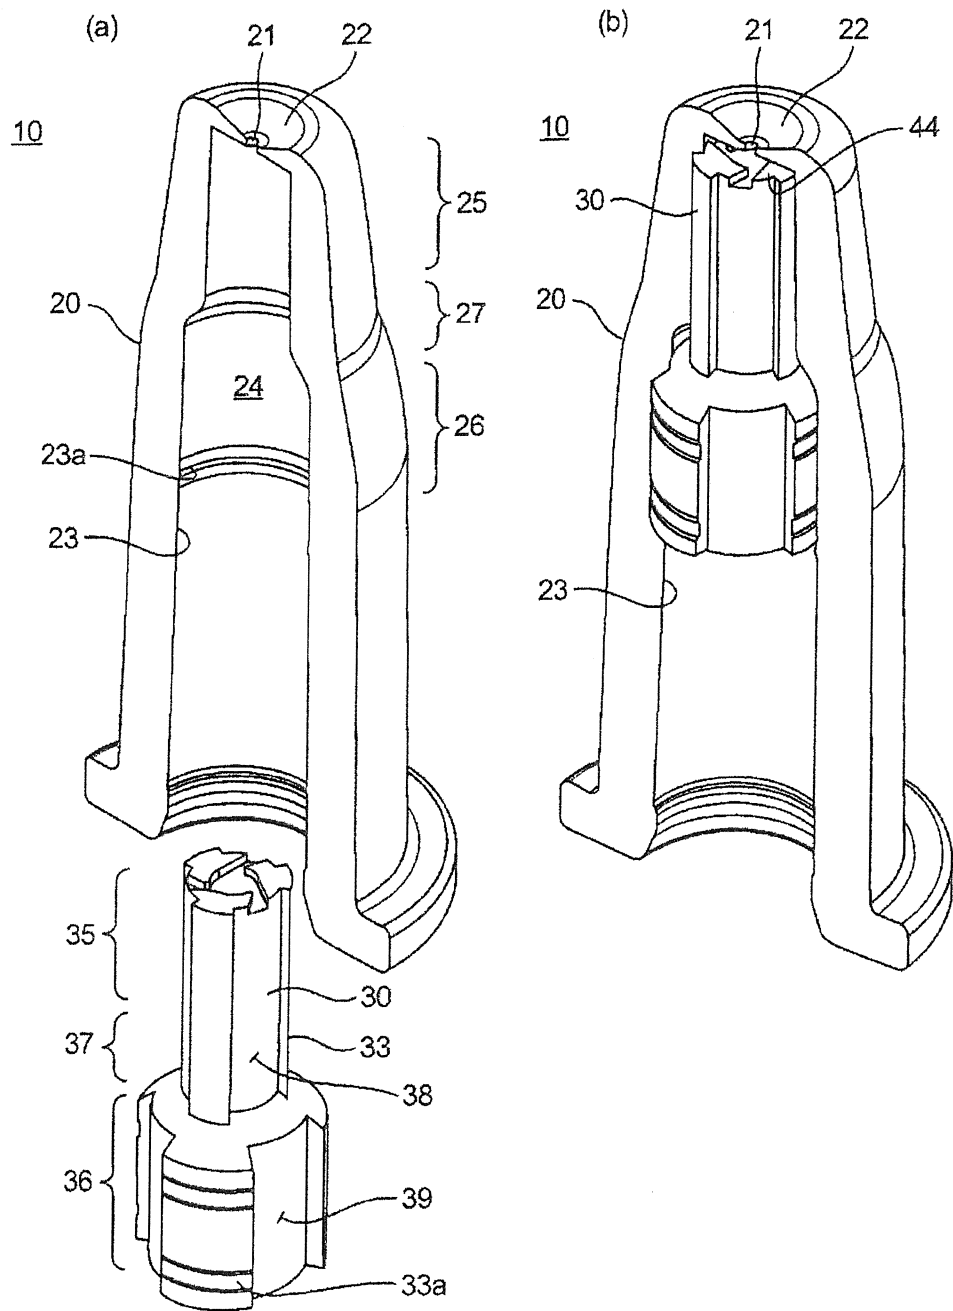


Fig. 3


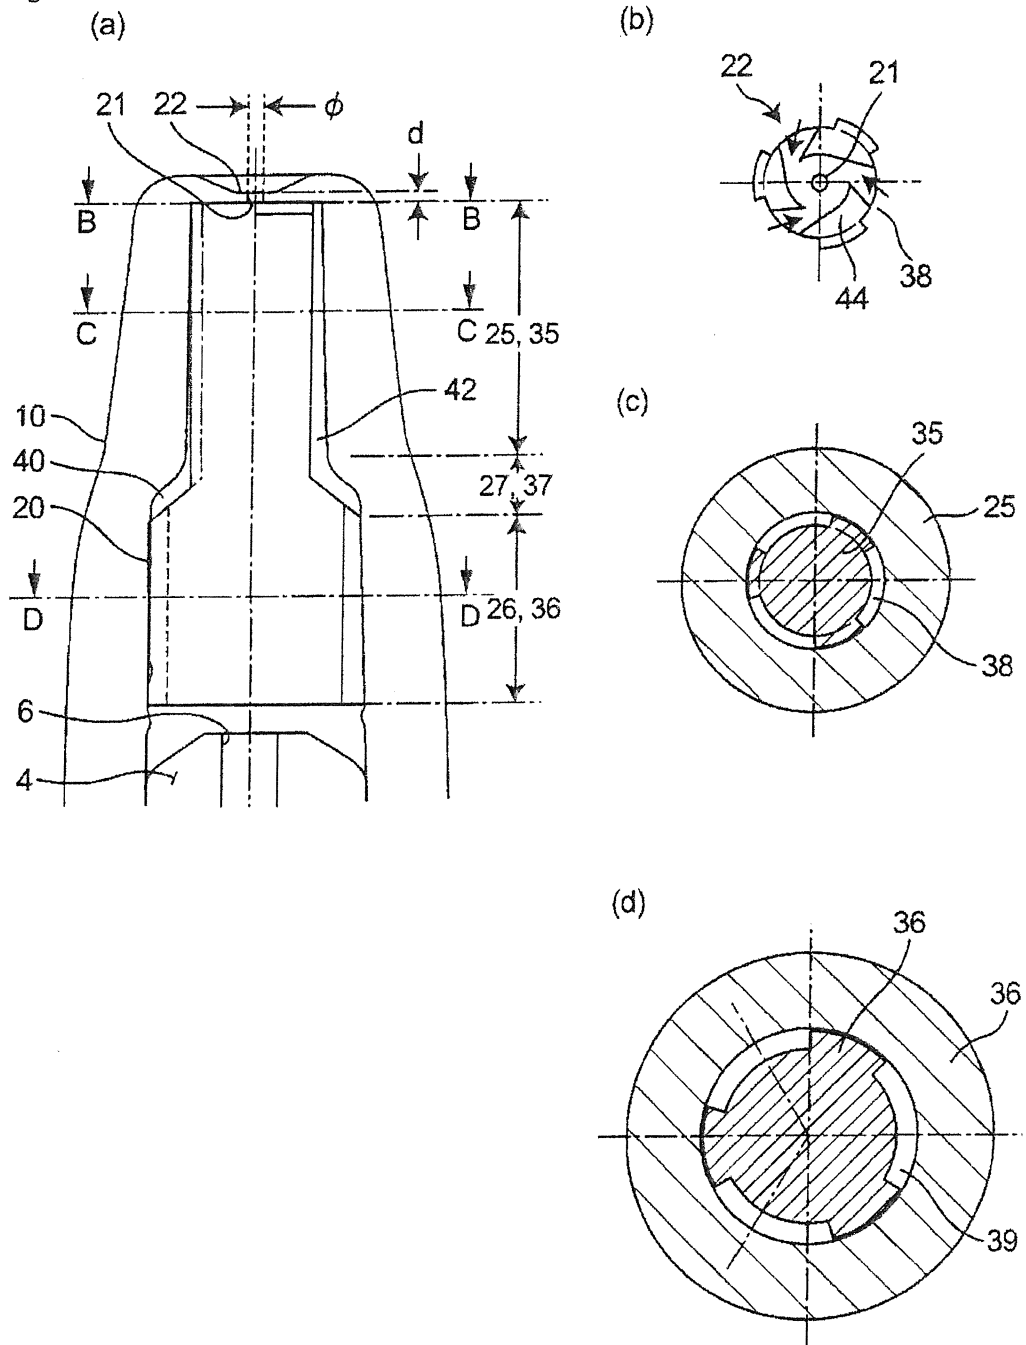


Fig. 4

(a)

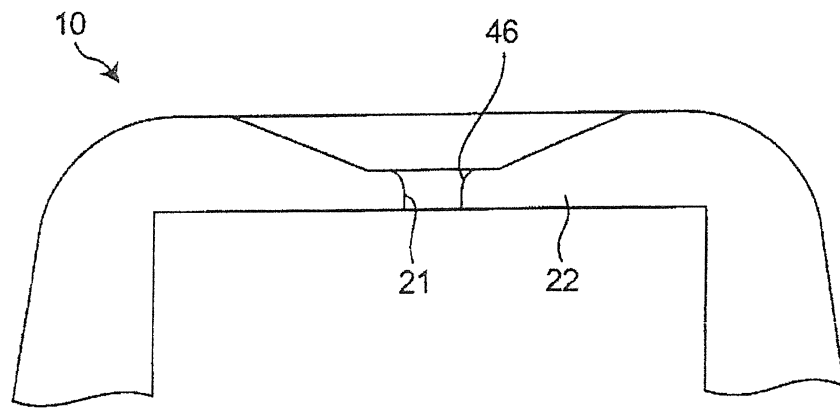

(b)


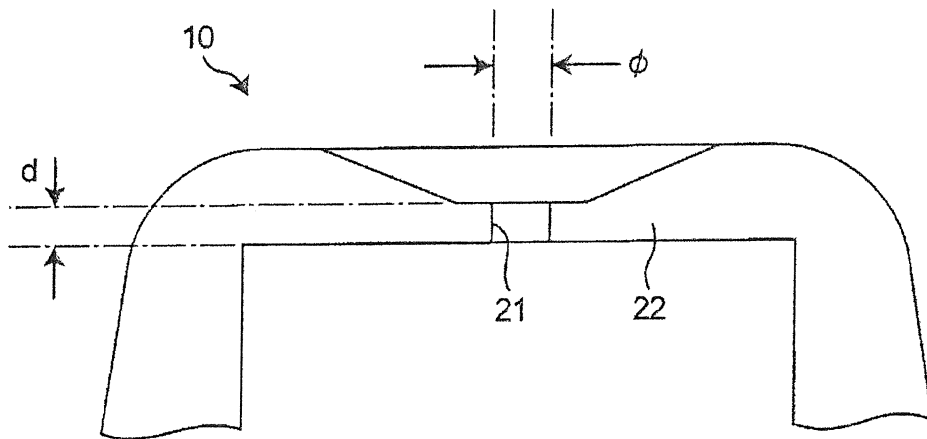


Fig. 5

Standard Values:			Dv(10) = 19.31 (μm)			Span = 2.171		
Trans = 64.0 (%)			Dv(50) = 44.84 (μm)			D[3][2] = 37.23 (μm)		
Cv = 53.5 (PPM)			Dv(90) = 116.6 (μm)			D[4][3] = 59.63 (μm)		
SSA = 0.1612 (m ² /cc)								

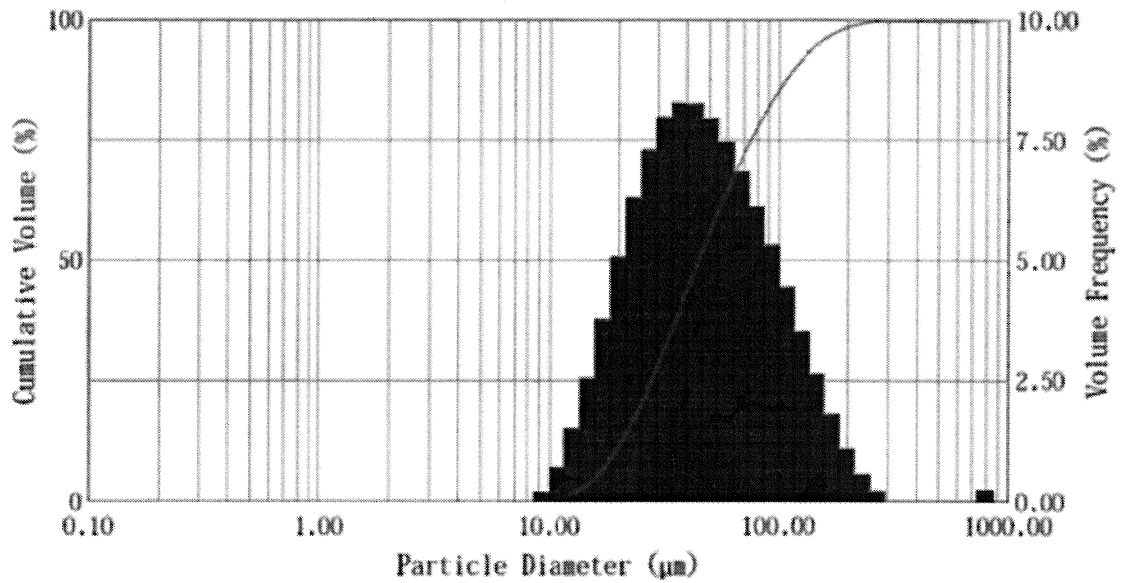

Size (μm)	% V <	% V	Size (μm)	% V <	% V	Size (μm)	% V <	% V
0.117	0.00	0.00	2.51	0.00	0.00	54.12	59.80	7.96
0.136	0.00	0.00	2.93	0.00	0.00	63.10	67.27	7.47
0.158	0.00	0.00	3.41	0.00	0.00	73.56	74.12	6.84
0.185	0.00	0.00	3.98	0.00	0.00	85.77	80.24	6.12
0.215	0.00	0.00	4.64	0.00	0.00	100.00	85.55	5.31
0.251	0.00	0.00	5.41	0.00	0.00	116.59	89.99	4.44
0.293	0.00	0.00	6.31	0.00	0.00	135.94	93.51	3.52
0.341	0.00	0.00	7.36	0.00	0.00	158.49	96.13	2.62
0.398	0.00	0.00	8.58	0.00	0.00	184.79	97.92	1.79
0.464	0.00	0.00	10.00	0.18	0.18	215.44	99.02	1.09
0.541	0.00	0.00	11.66	0.89	0.70	251.19	99.58	0.56
0.631	0.00	0.00	13.59	2.38	1.49	292.87	99.77	0.20
0.736	0.00	0.00	15.85	4.91	2.53	341.46	99.77	0.00
0.858	0.00	0.00	18.48	8.68	3.76	398.11	99.77	0.00
1.00	0.00	0.00	21.54	13.75	5.07	464.16	99.77	0.00
1.17	0.00	0.00	25.12	20.04	6.29	541.17	99.77	0.00
1.36	0.00	0.00	29.29	27.33	7.29	630.96	99.77	0.00
1.58	0.00	0.00	34.15	35.30	7.97	735.64	99.77	0.00
1.85	0.00	0.00	39.81	43.59	8.28	857.70	100.00	0.23
2.15	0.00	0.00	46.42	51.84	8.26	1000.00	100.00	0.00

Fig. 6



Fig. 7

