

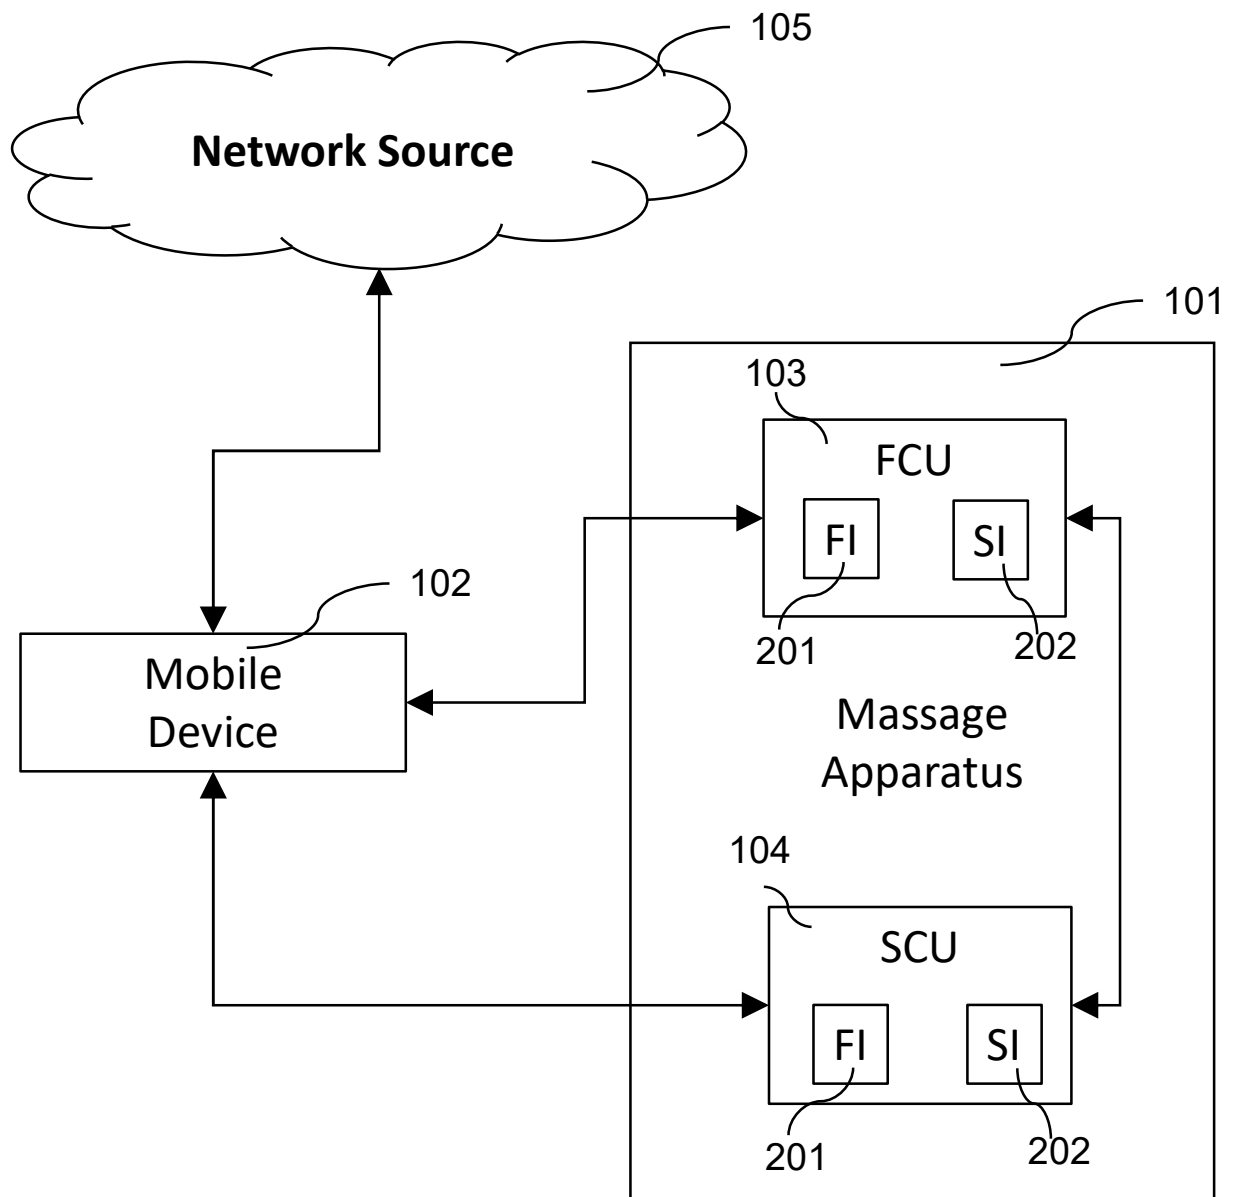


Fig. 1a

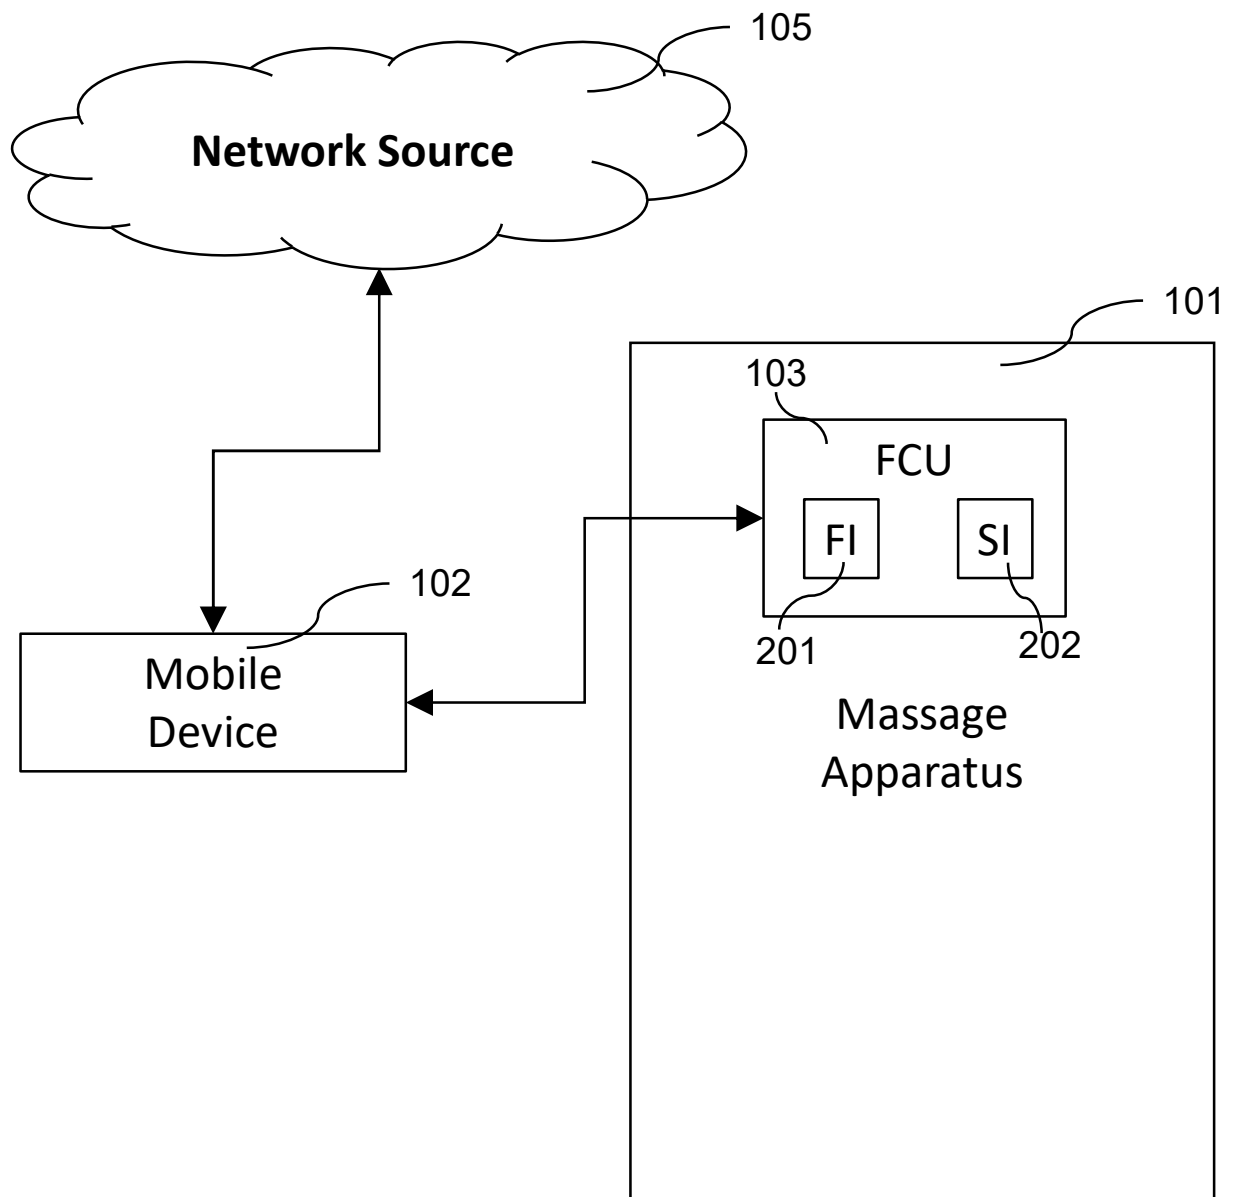


Fig. 1b

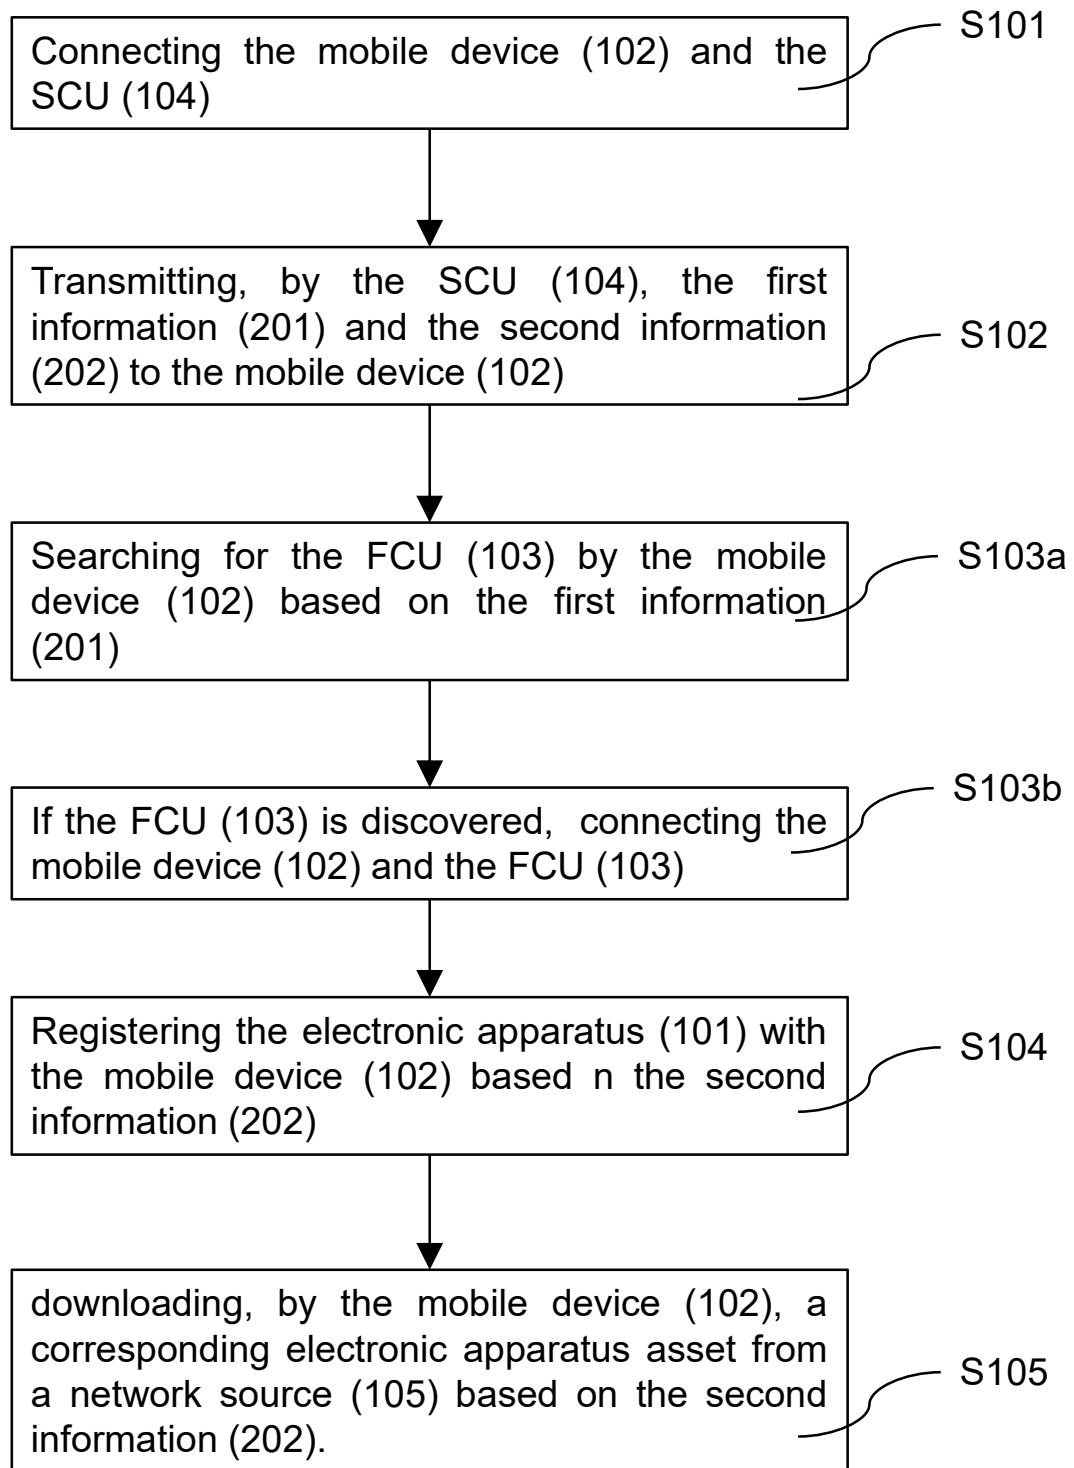


Fig. 2a

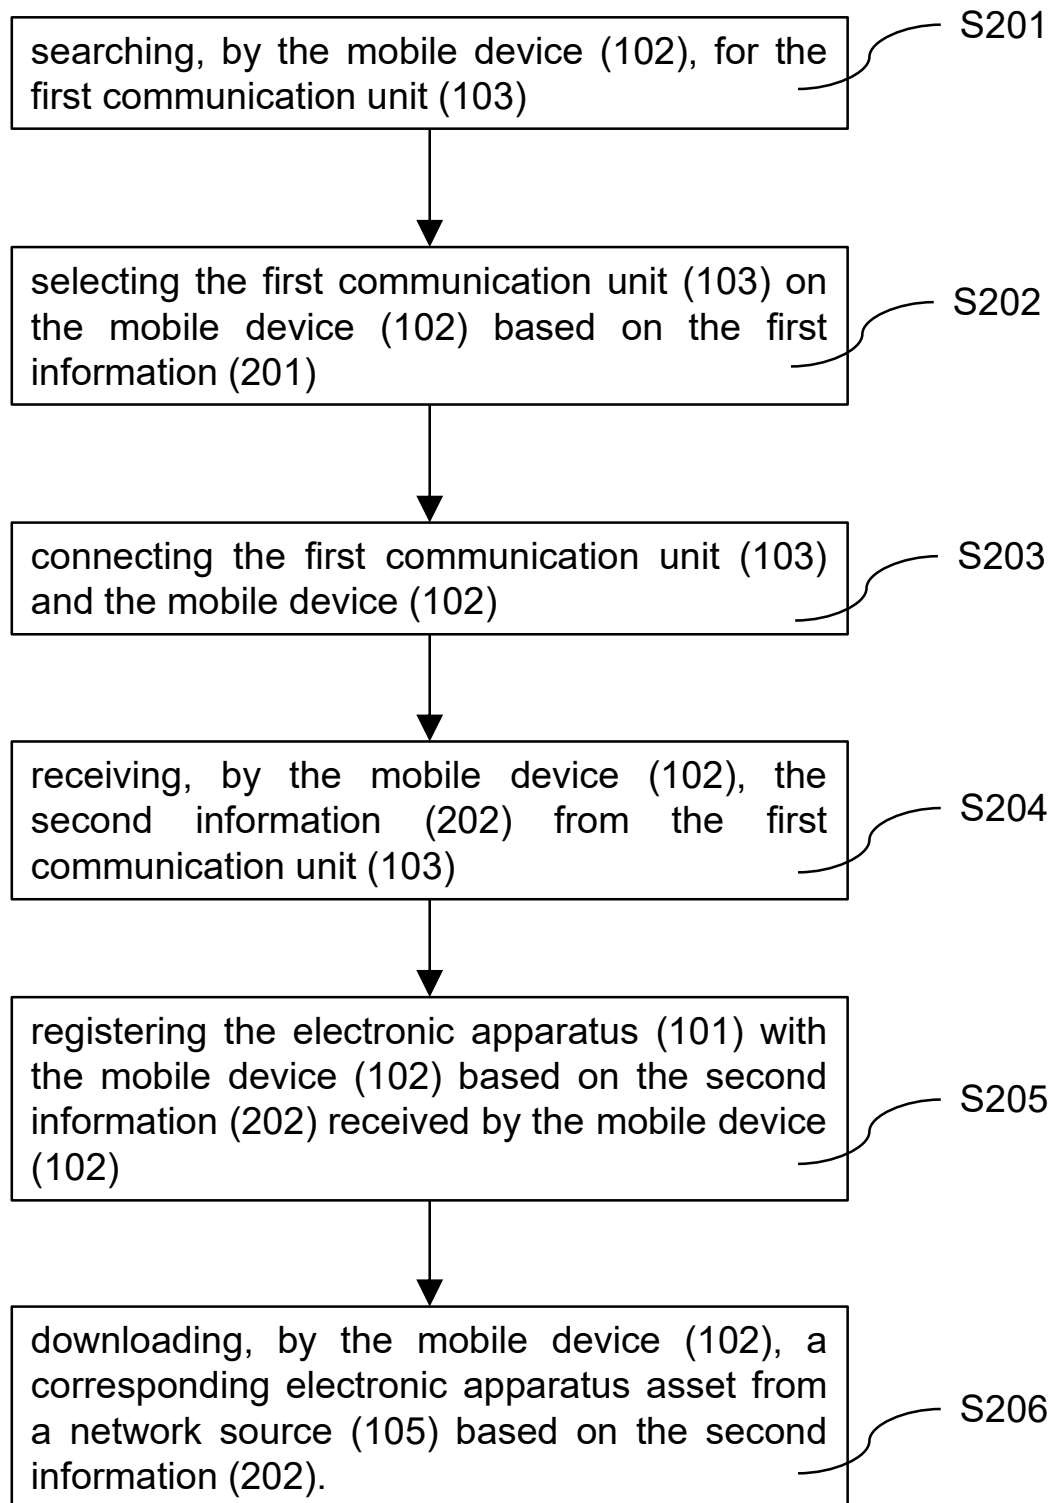


Fig. 2b

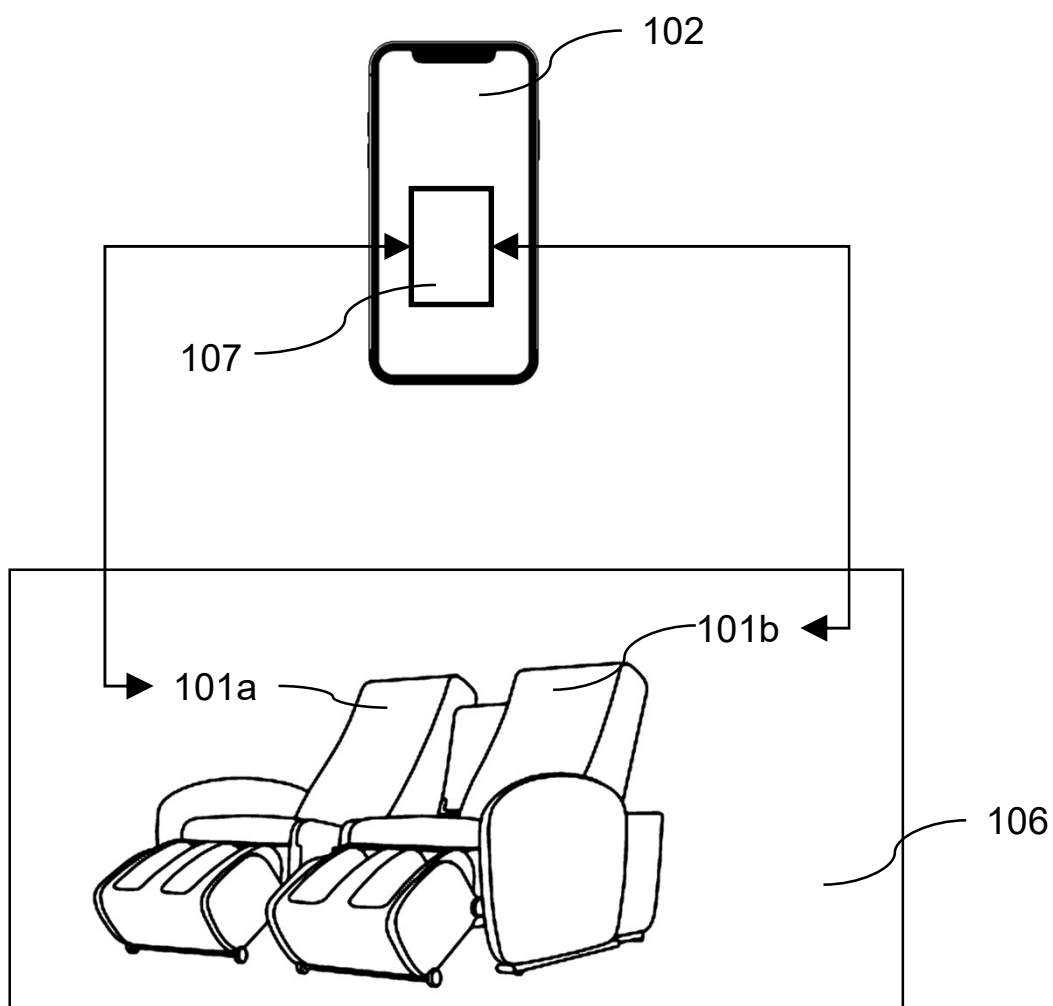


Fig. 3

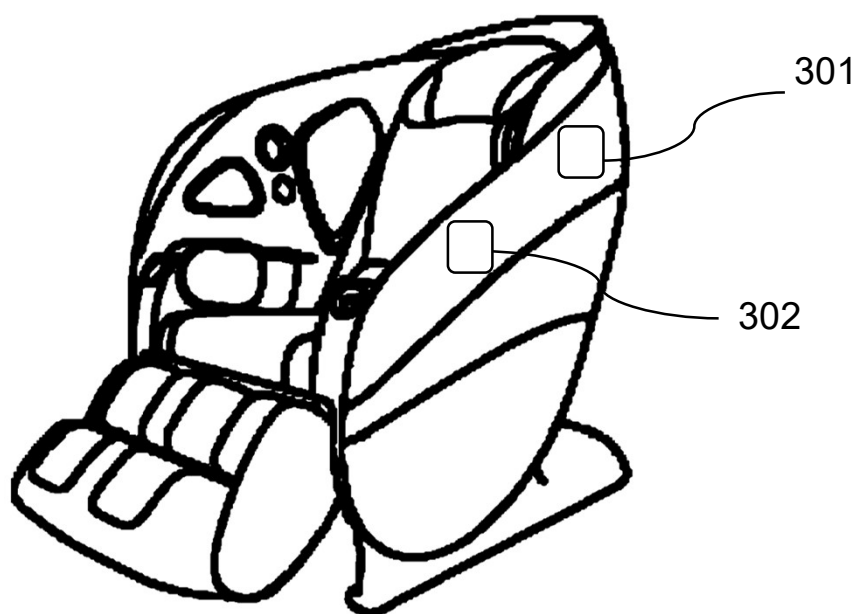


Fig. 4a

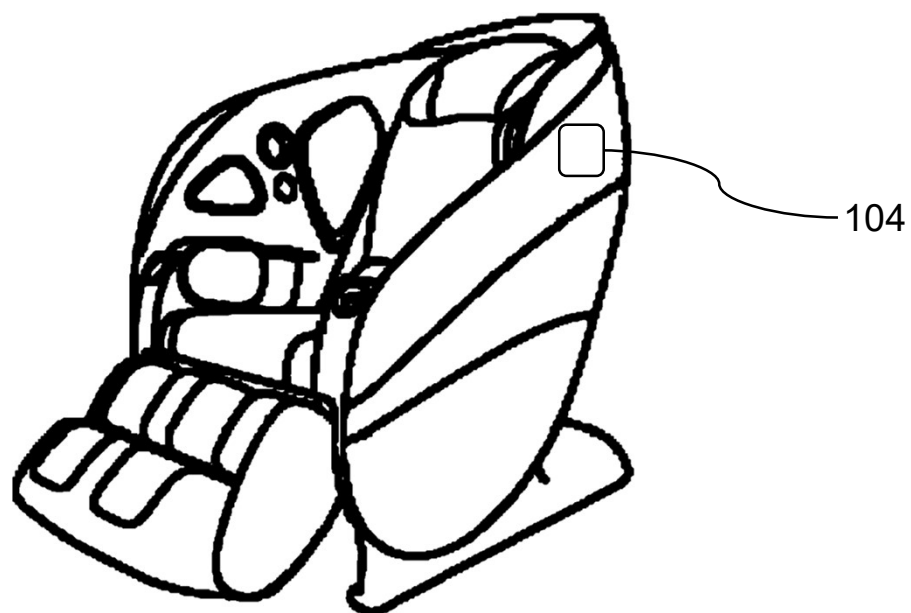


Fig. 4b

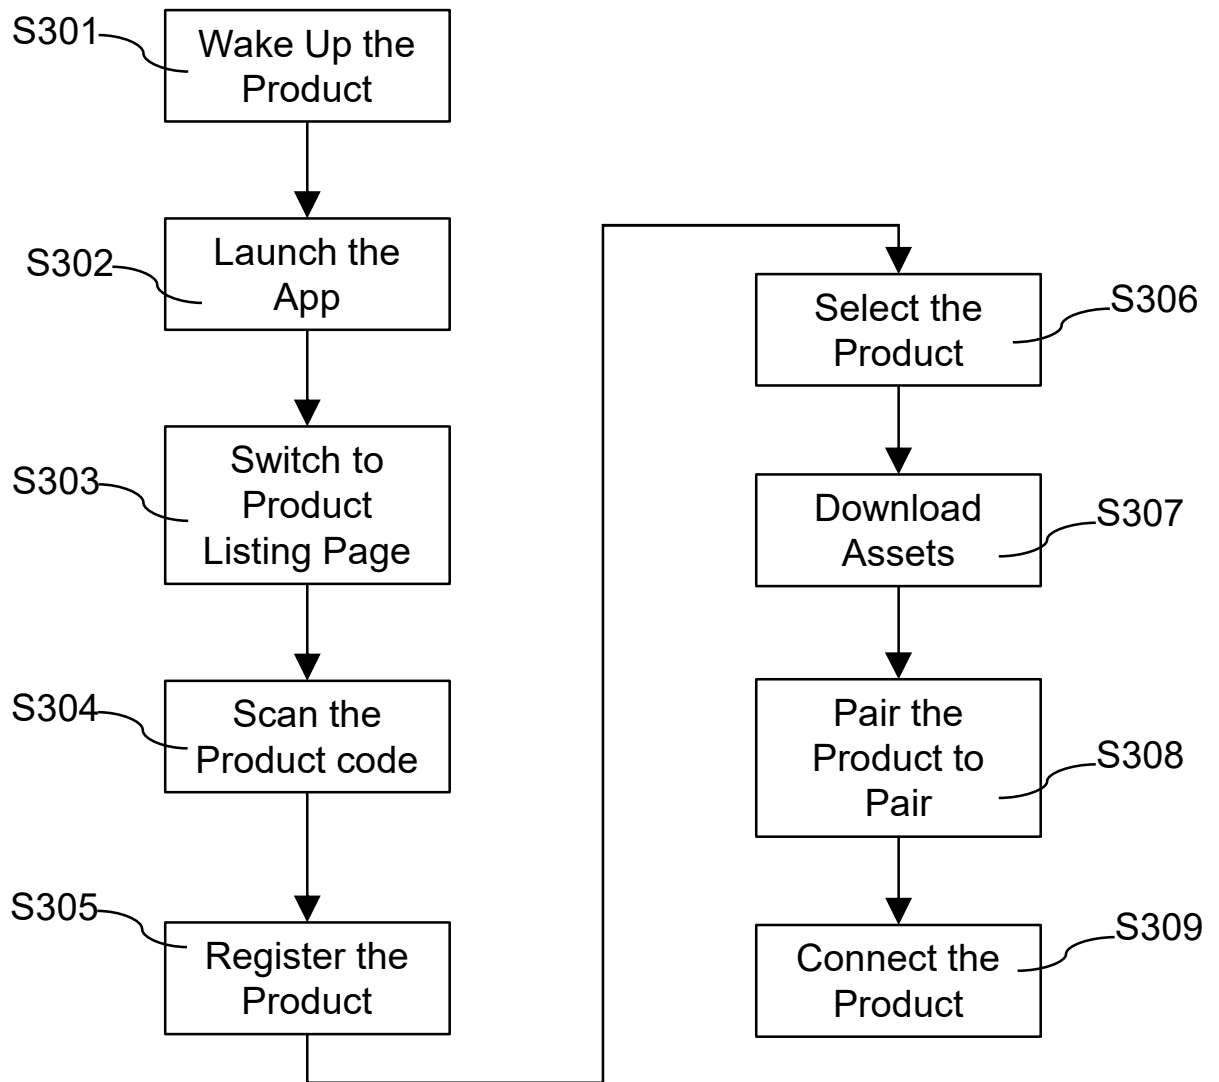


Fig. 5

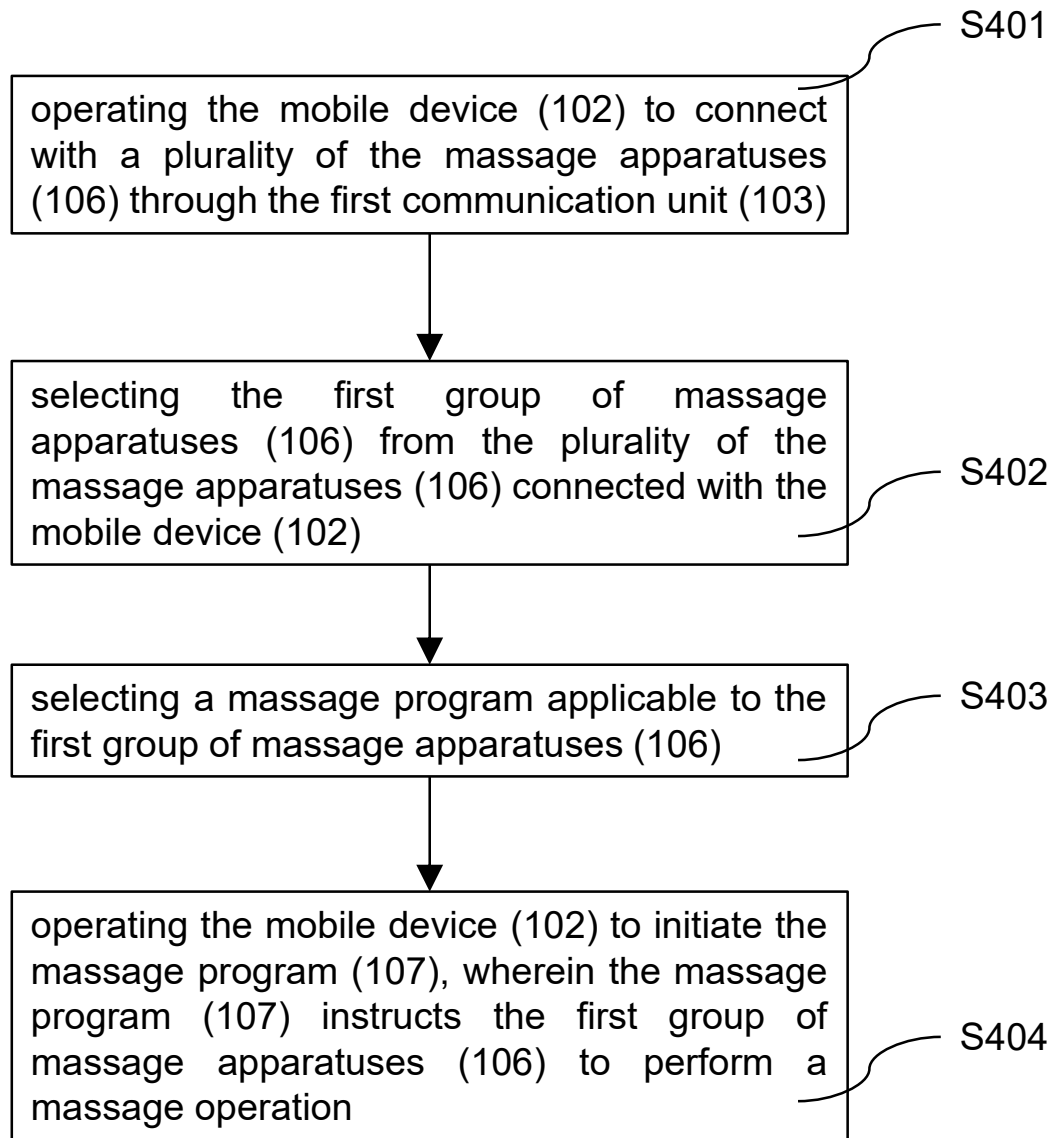


Fig. 6a

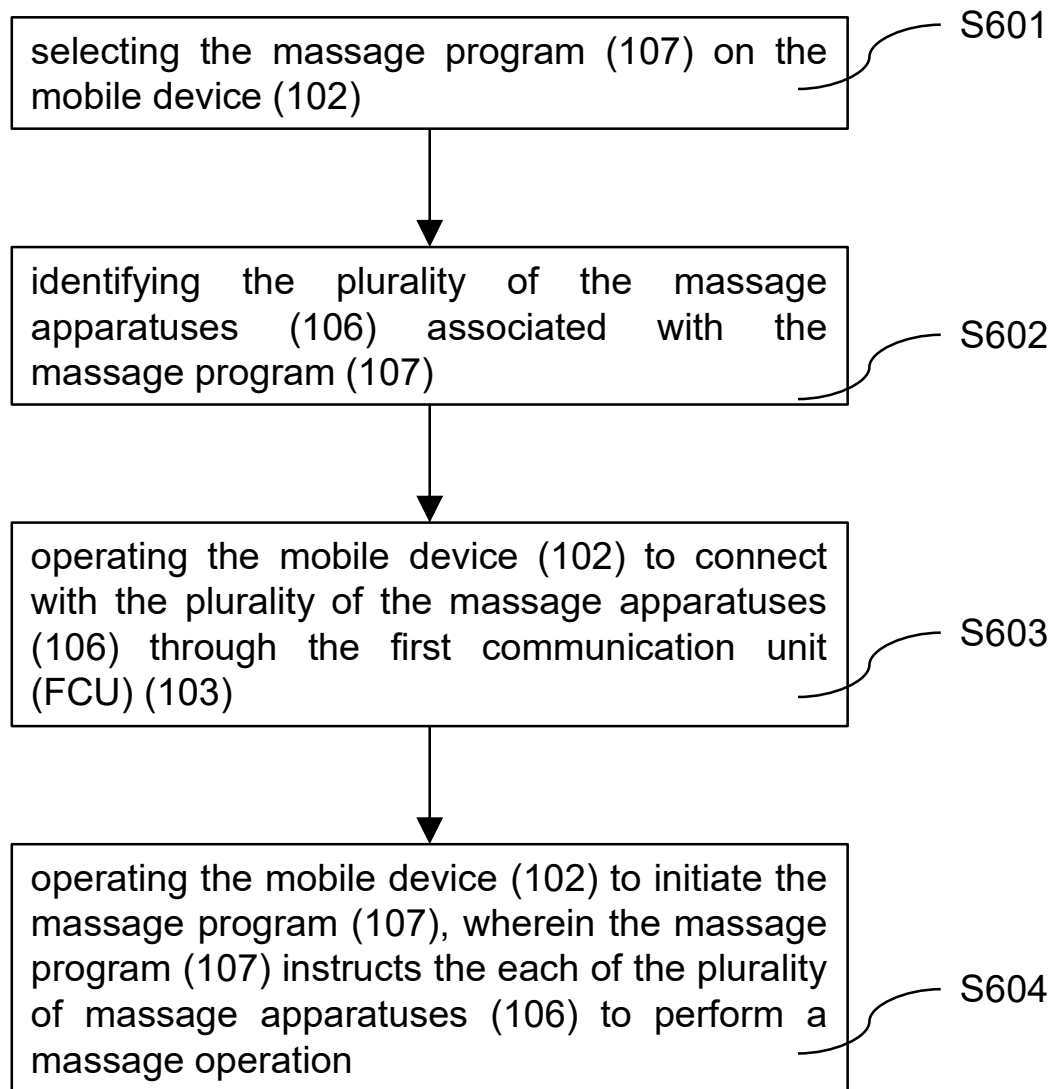


Fig. 6b

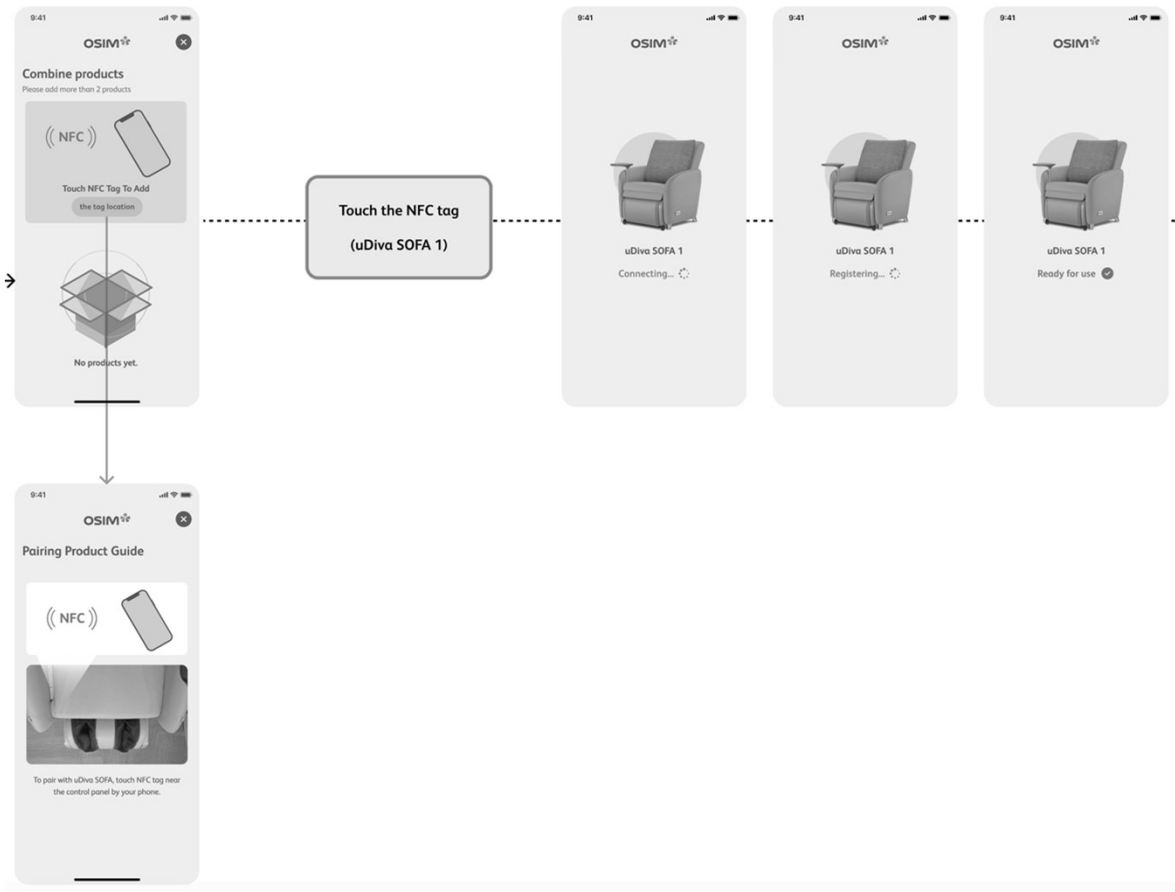


Fig. 7a

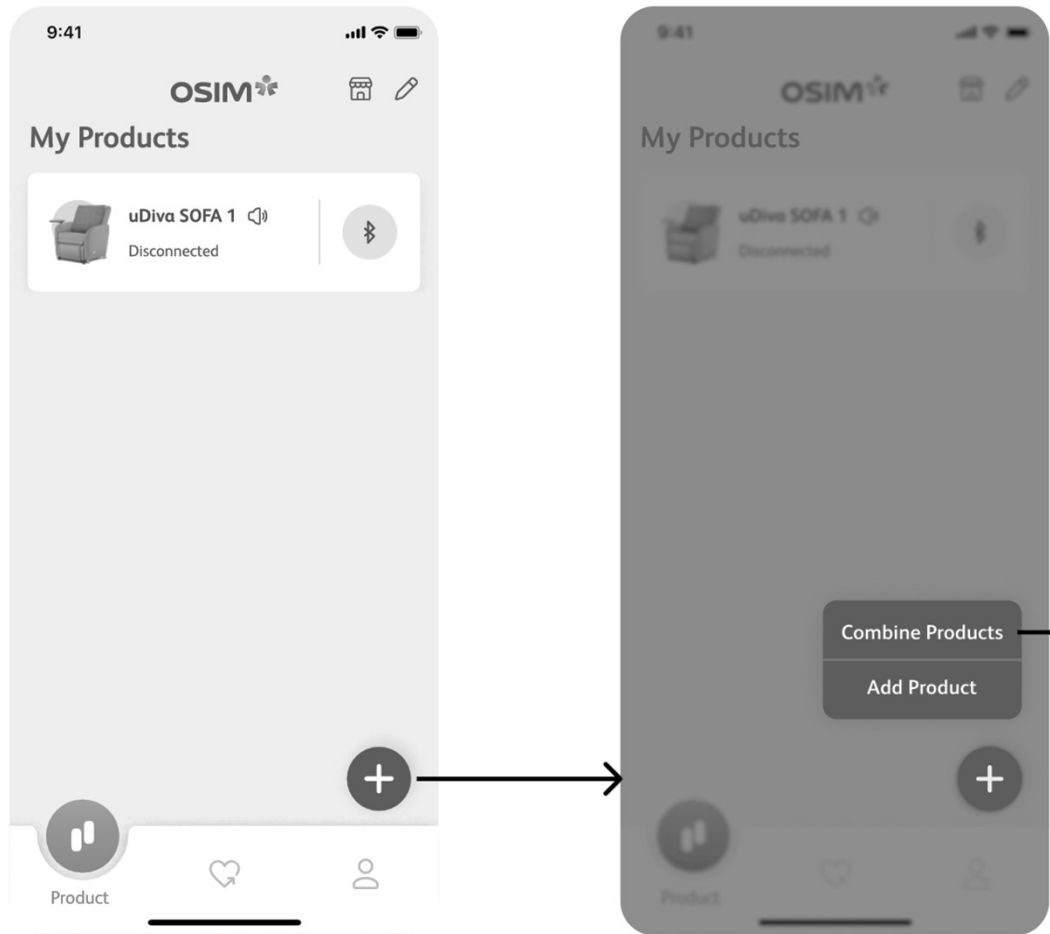


Fig. 7b


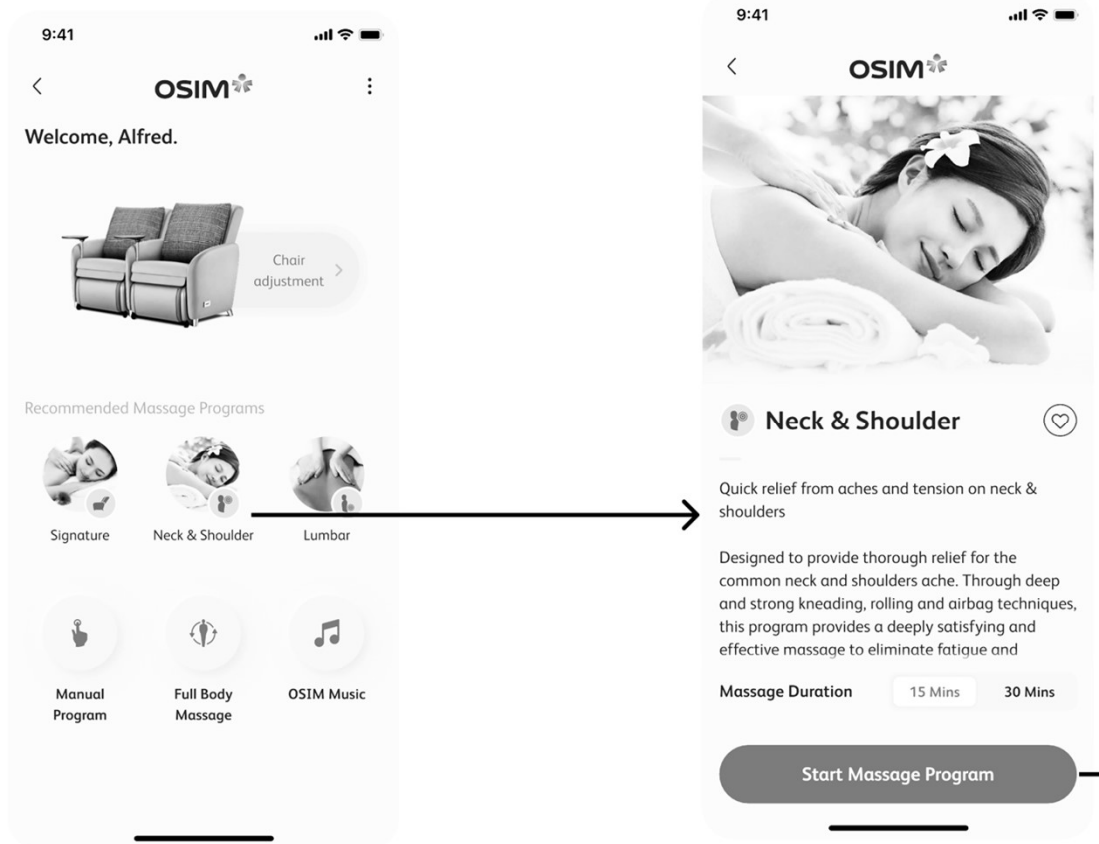


Fig. 8

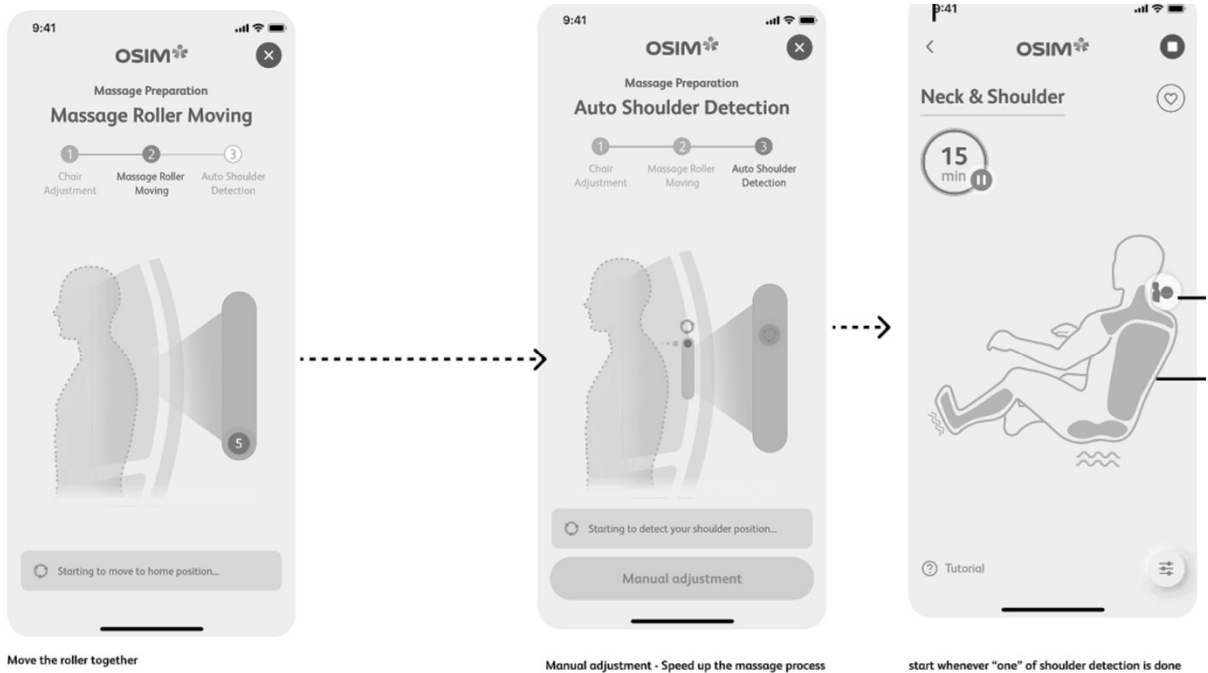

Move the roller together

Manual adjustment - Speed up the massage process

start whenever "one" of shoulder detection is done

Fig. 9

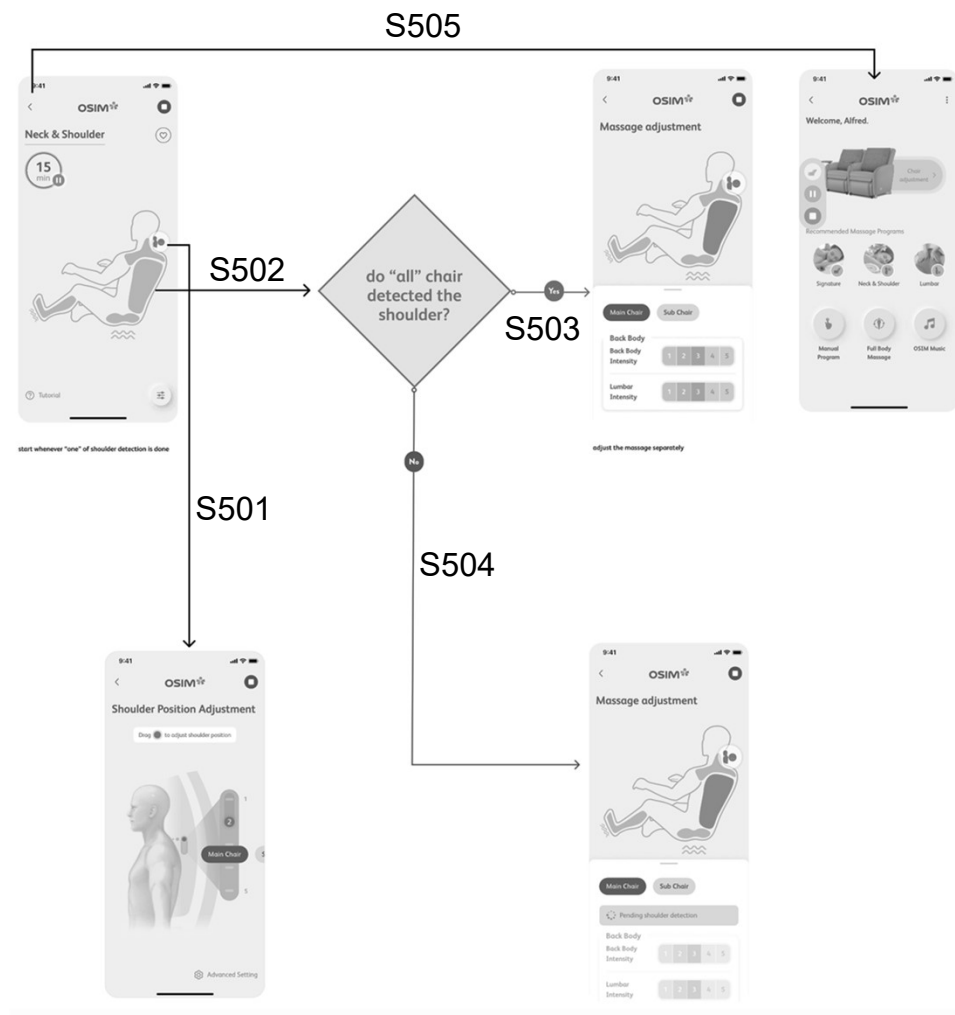


Fig. 10