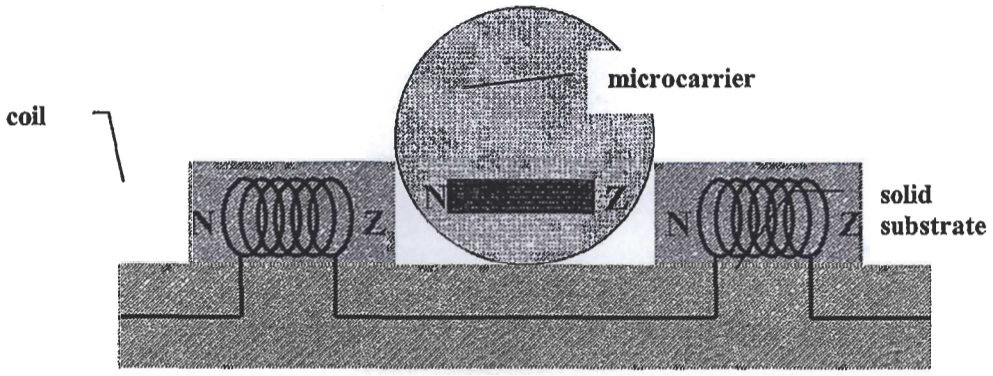


Figure 1

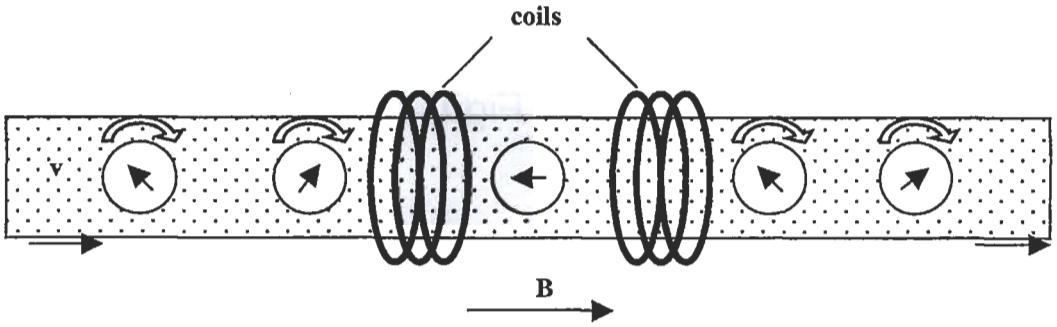


Figure 2

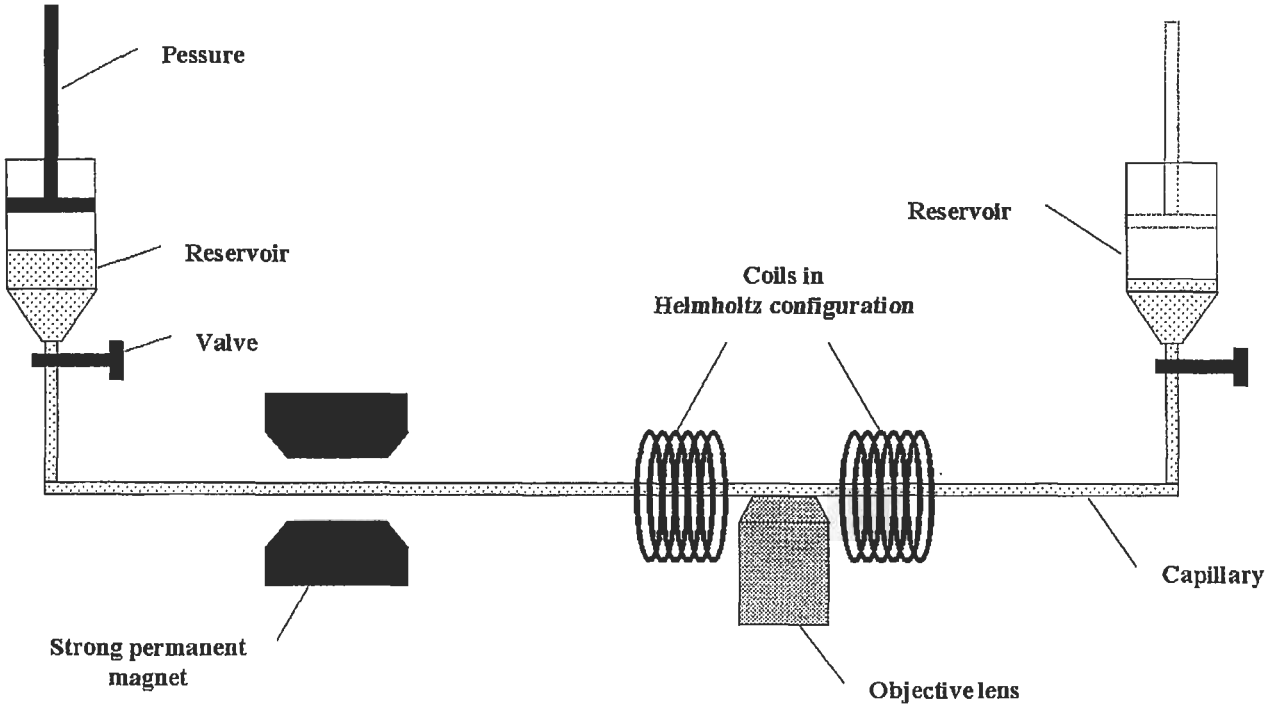

Pessure
Reservoir
Valve
Strong permanent magnet
Coils in Helmholtz configuration
Objective lens
Reservoir
Capillary

Figure 3

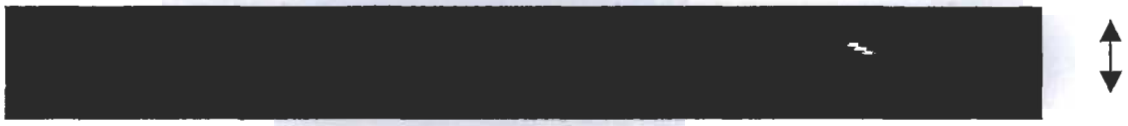


Figure 4

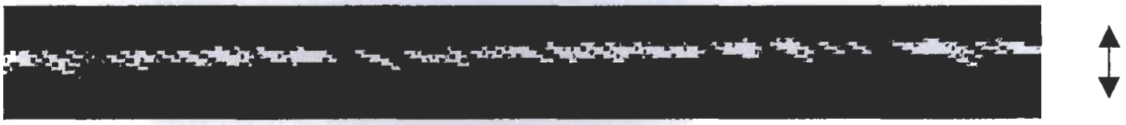


Figure 5



Figure 6



Figure 7

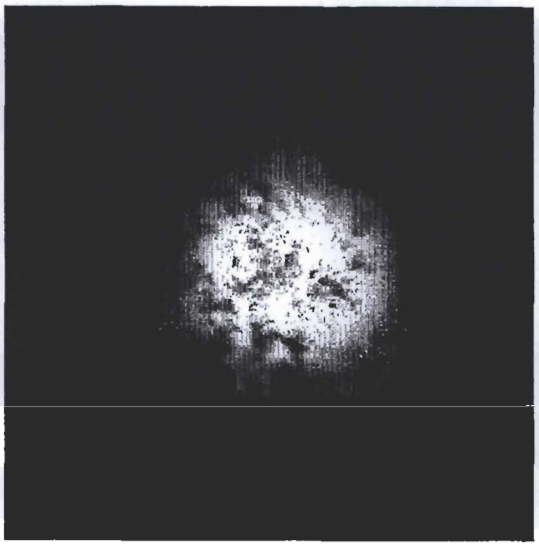


Figure 8

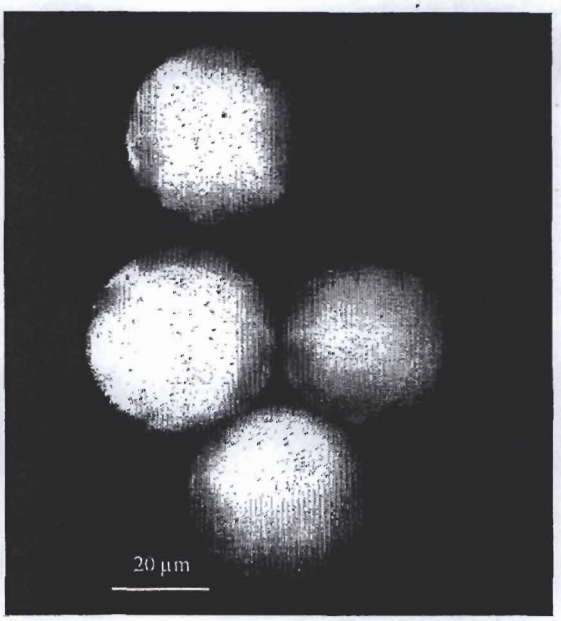


Figure 9

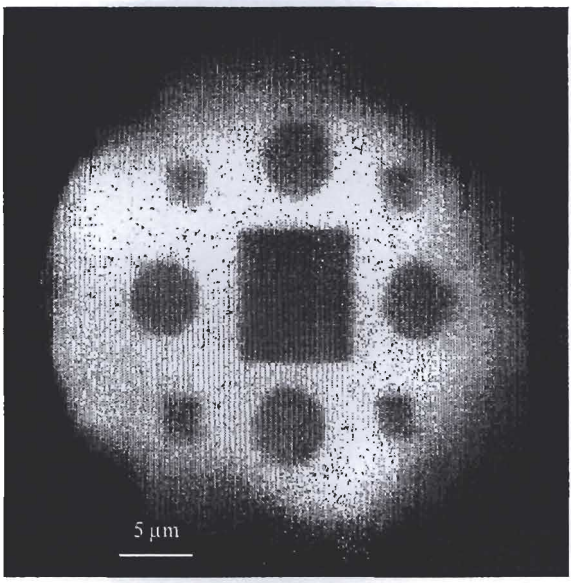


Figure 10

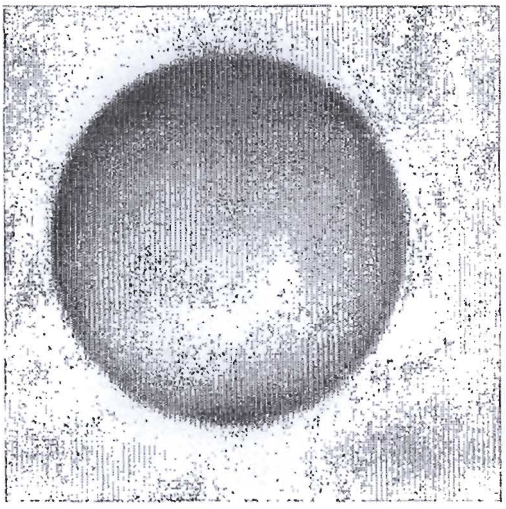


Figure 11

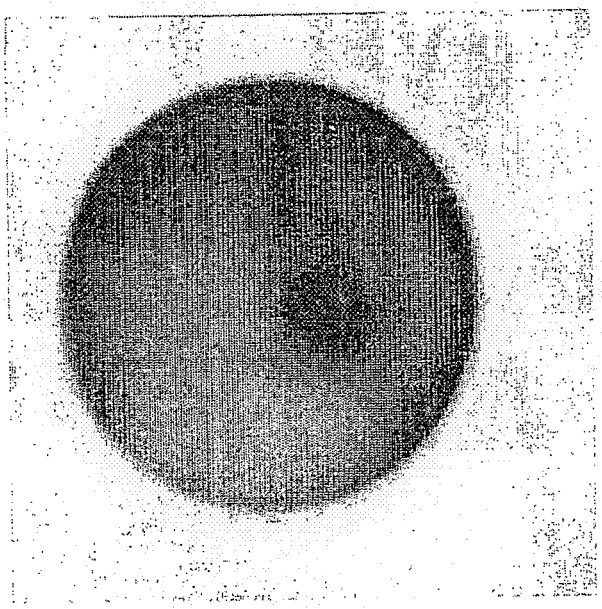


Figure 12

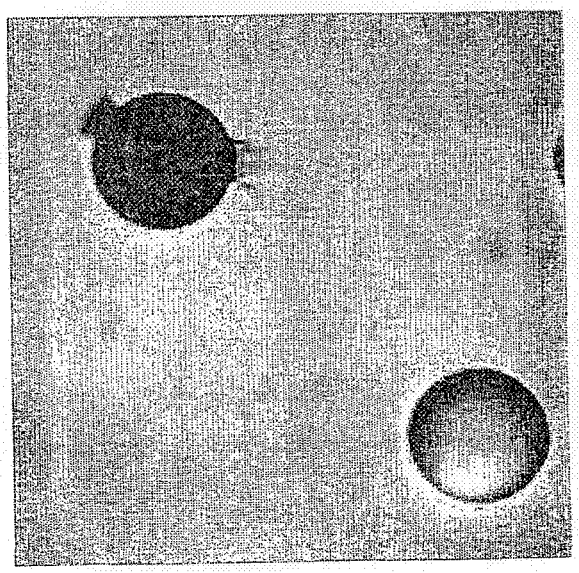


Figure 13

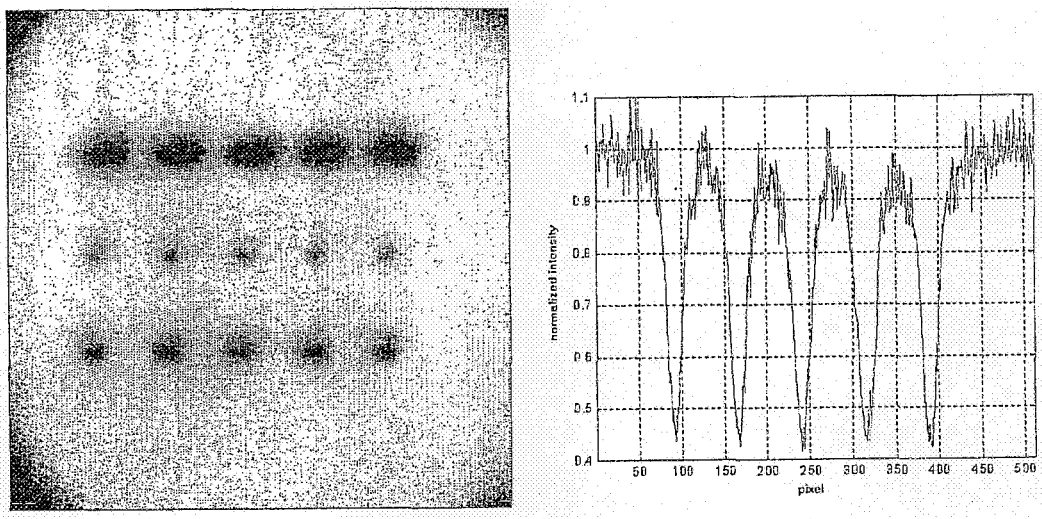


Figure 14

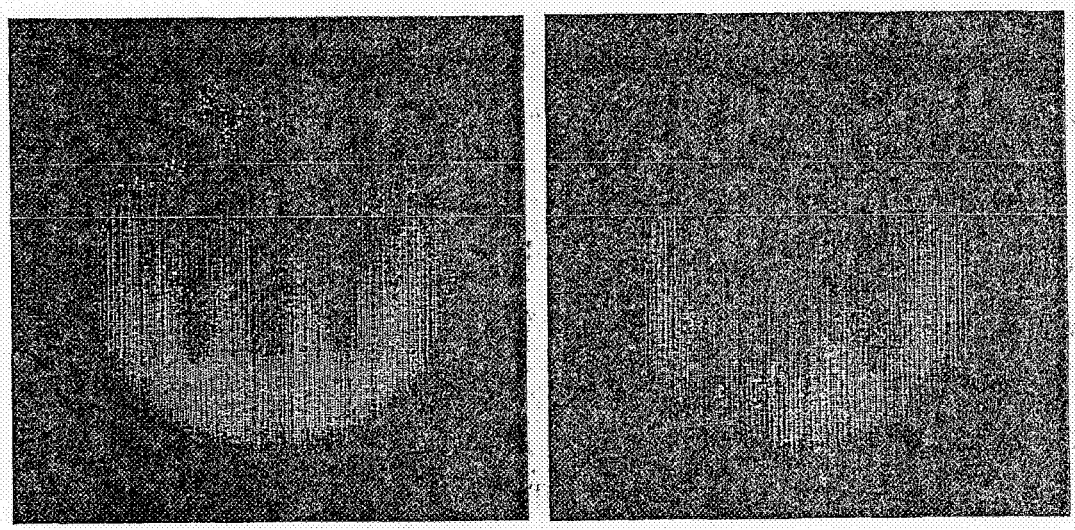


Figure 15

15 APR 2005

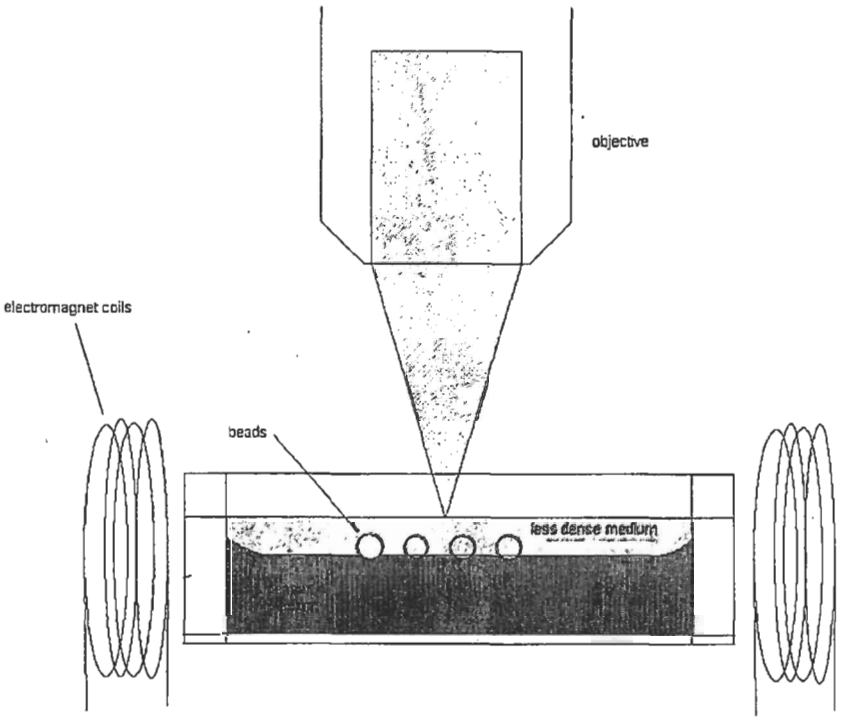


Figure 16

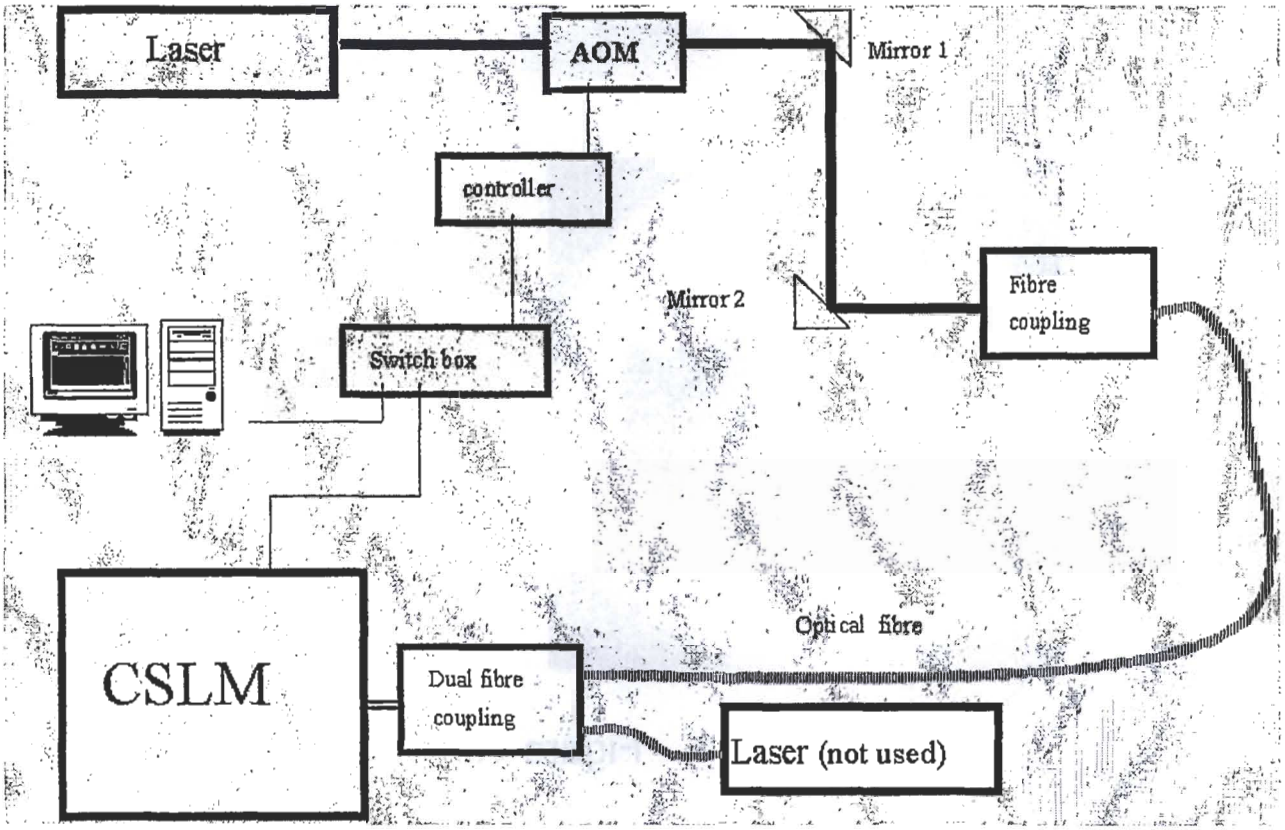


Figure 17

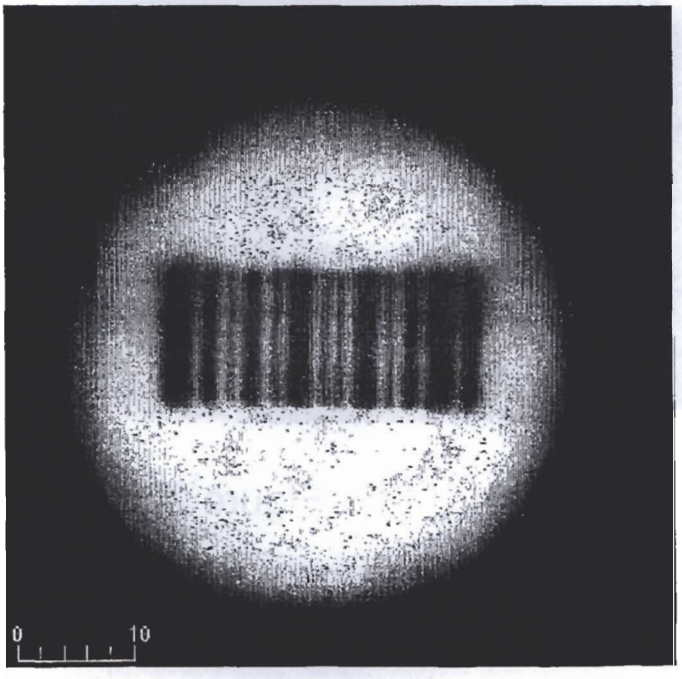


Figure 18

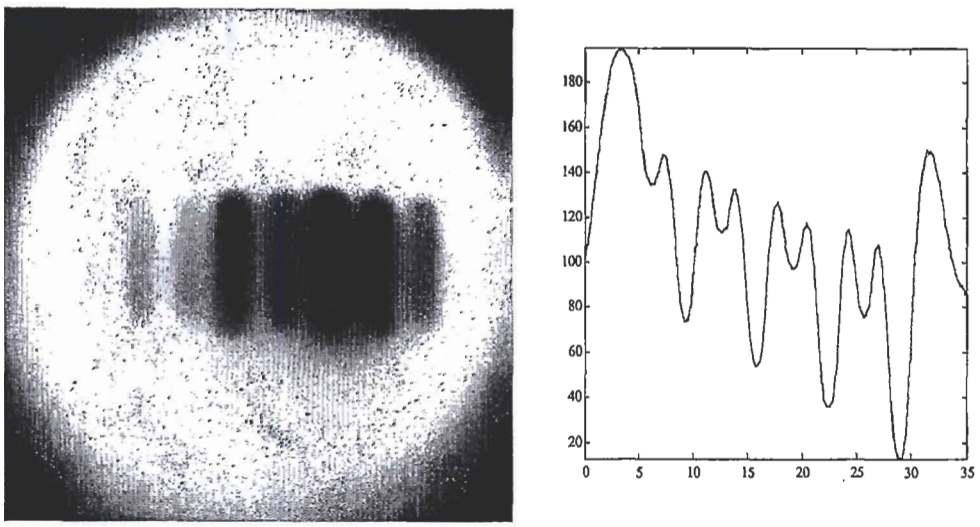


Figure 19

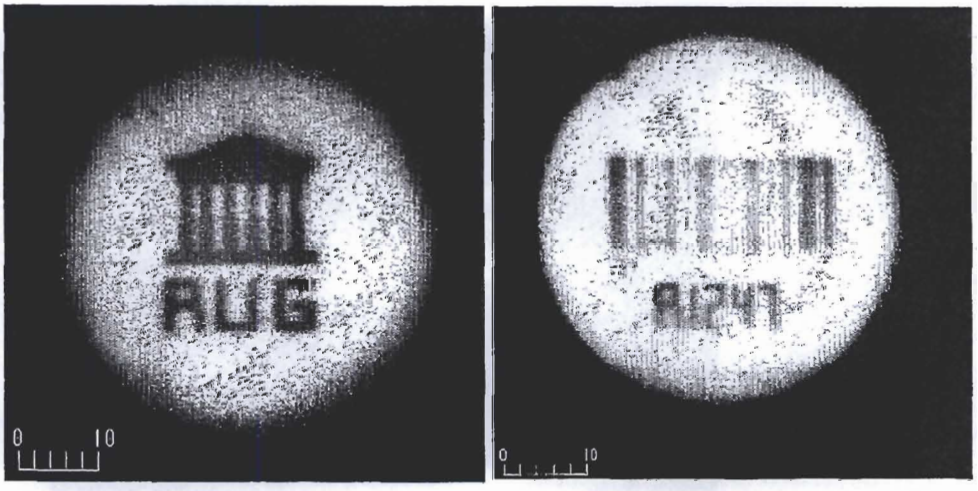


Figure 20

15 APR 2005

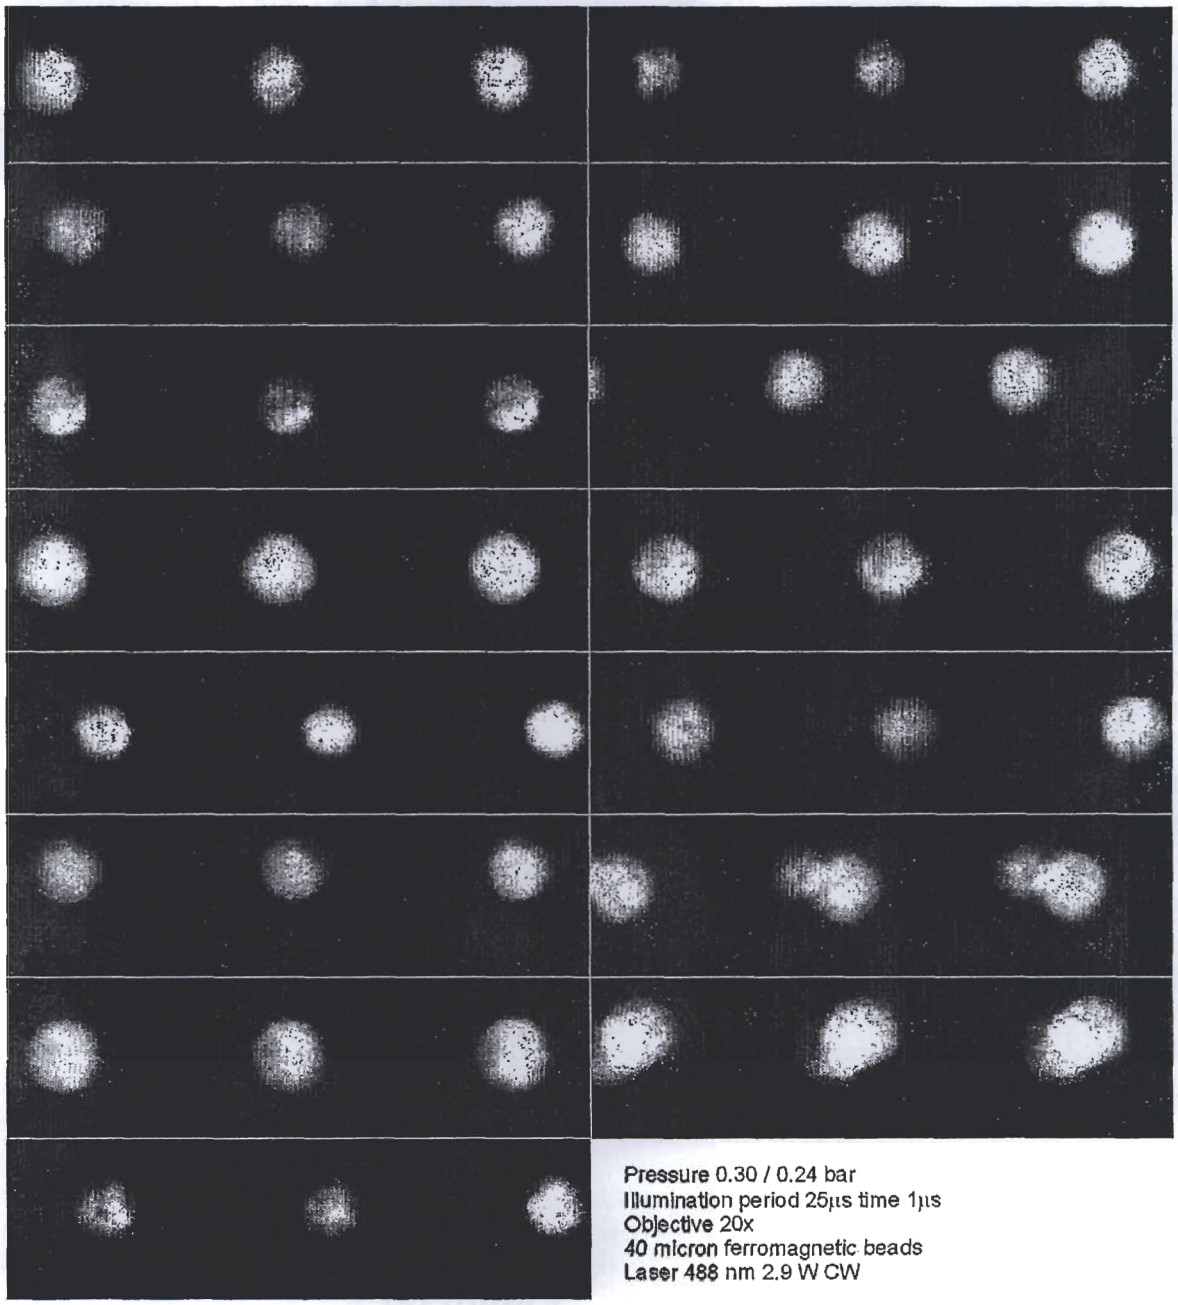


Figure 21

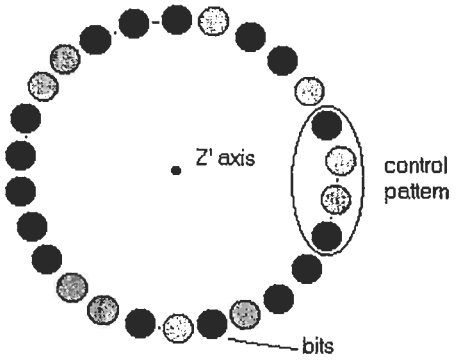


Figure 22

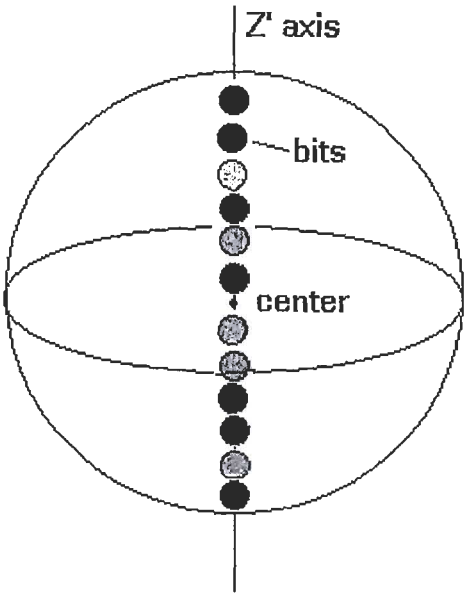


Figure 23

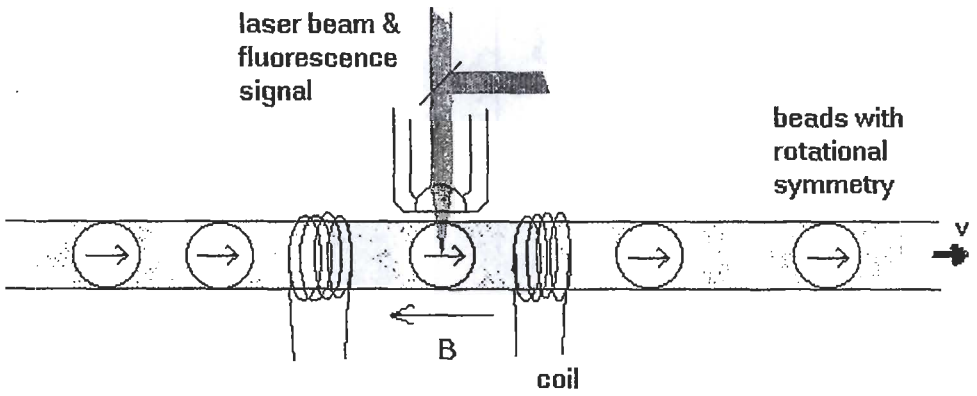


Figure 24

A	0123	L	0303	W	1232
B	0132	M	0232	X	1312
C	0213	N	0323	Y	1313
D	0212	O	1032	Z	1212
E	0312	P	1203	!	1023
F	0313	Q	1202	?	1323
G	0102	R	1302		
H	0103	S	1303		
I	0202	T	1012		
J	0203	U	1013		
K	0302	V	1213		

Figure 25

15 APR 2005

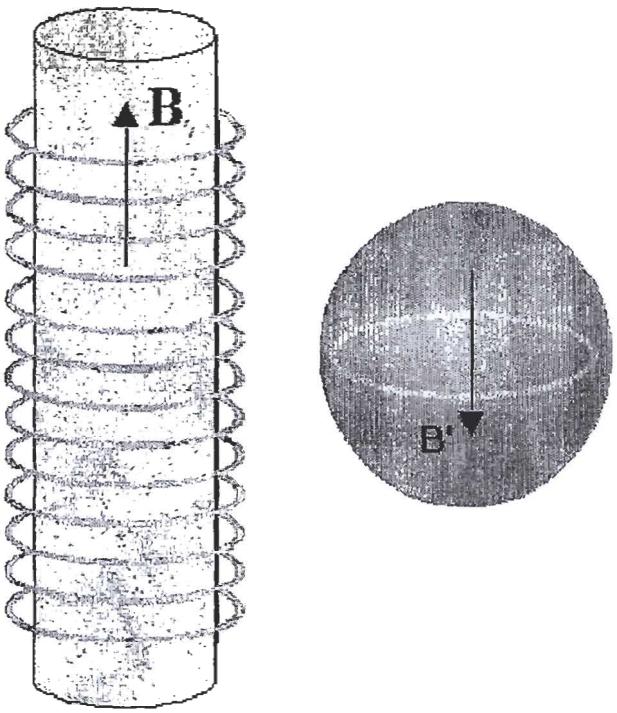


Figure 26

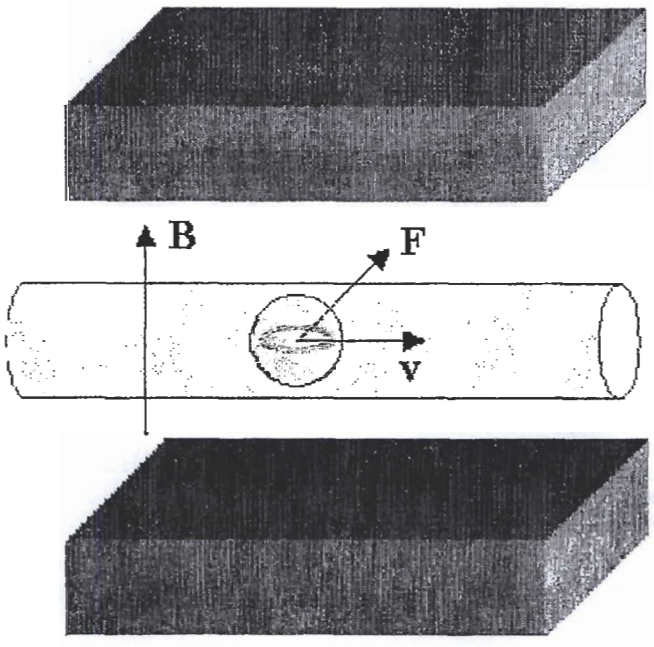


Figure 27

15 APR 2005

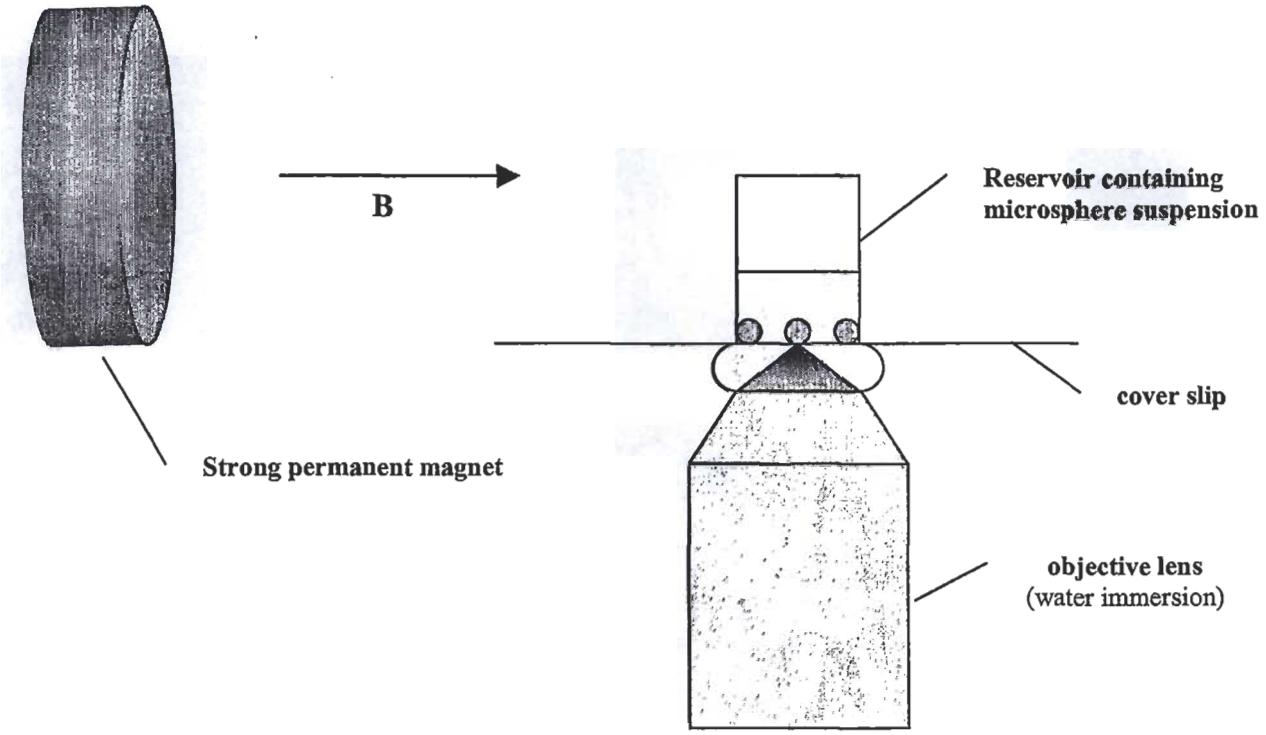


Figure 28

15 APR 2005

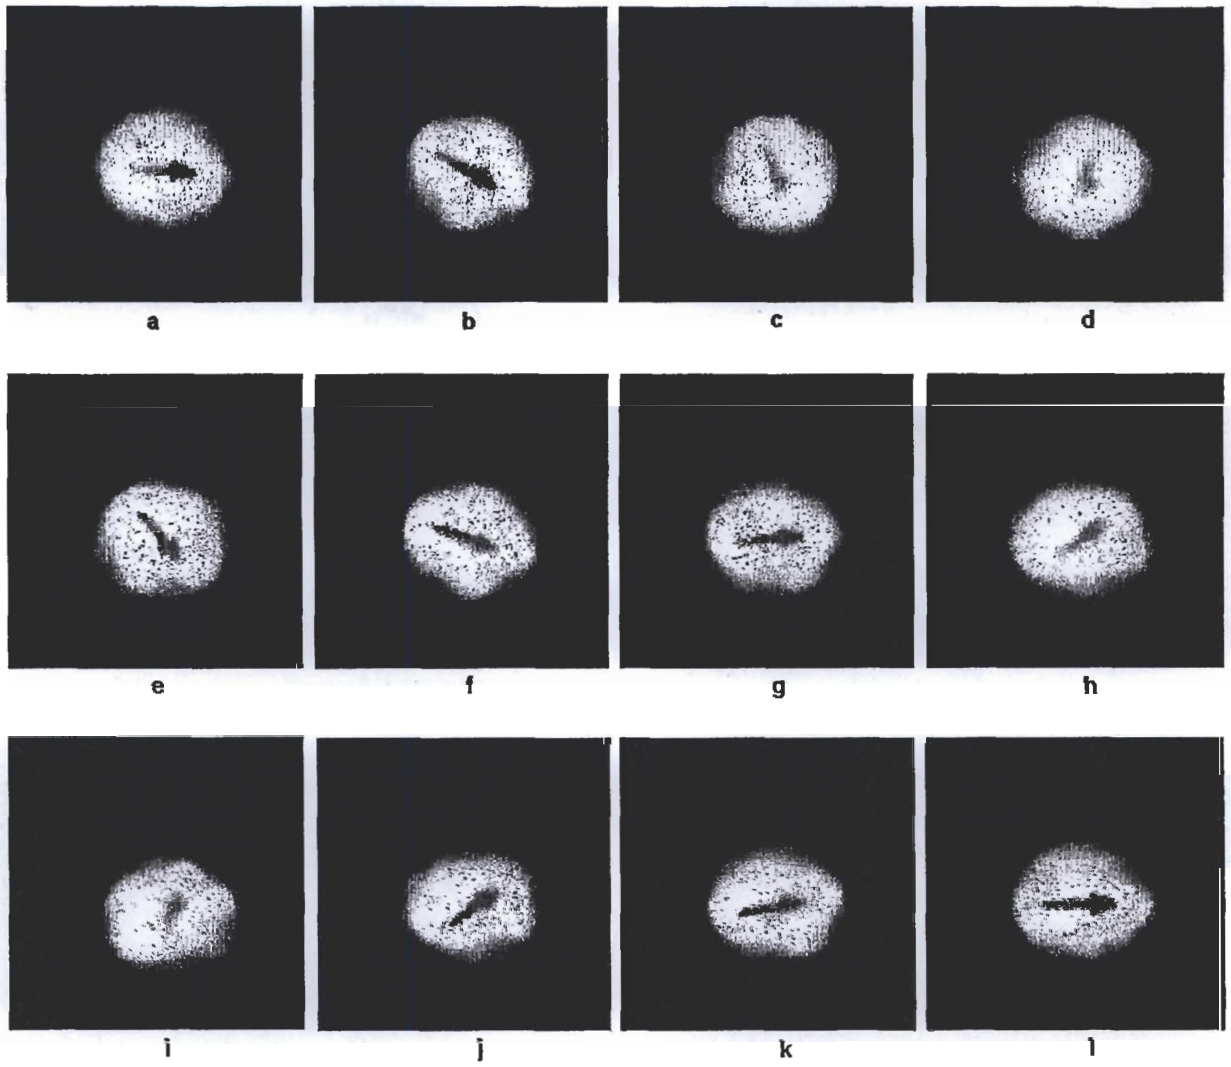


Figure 29

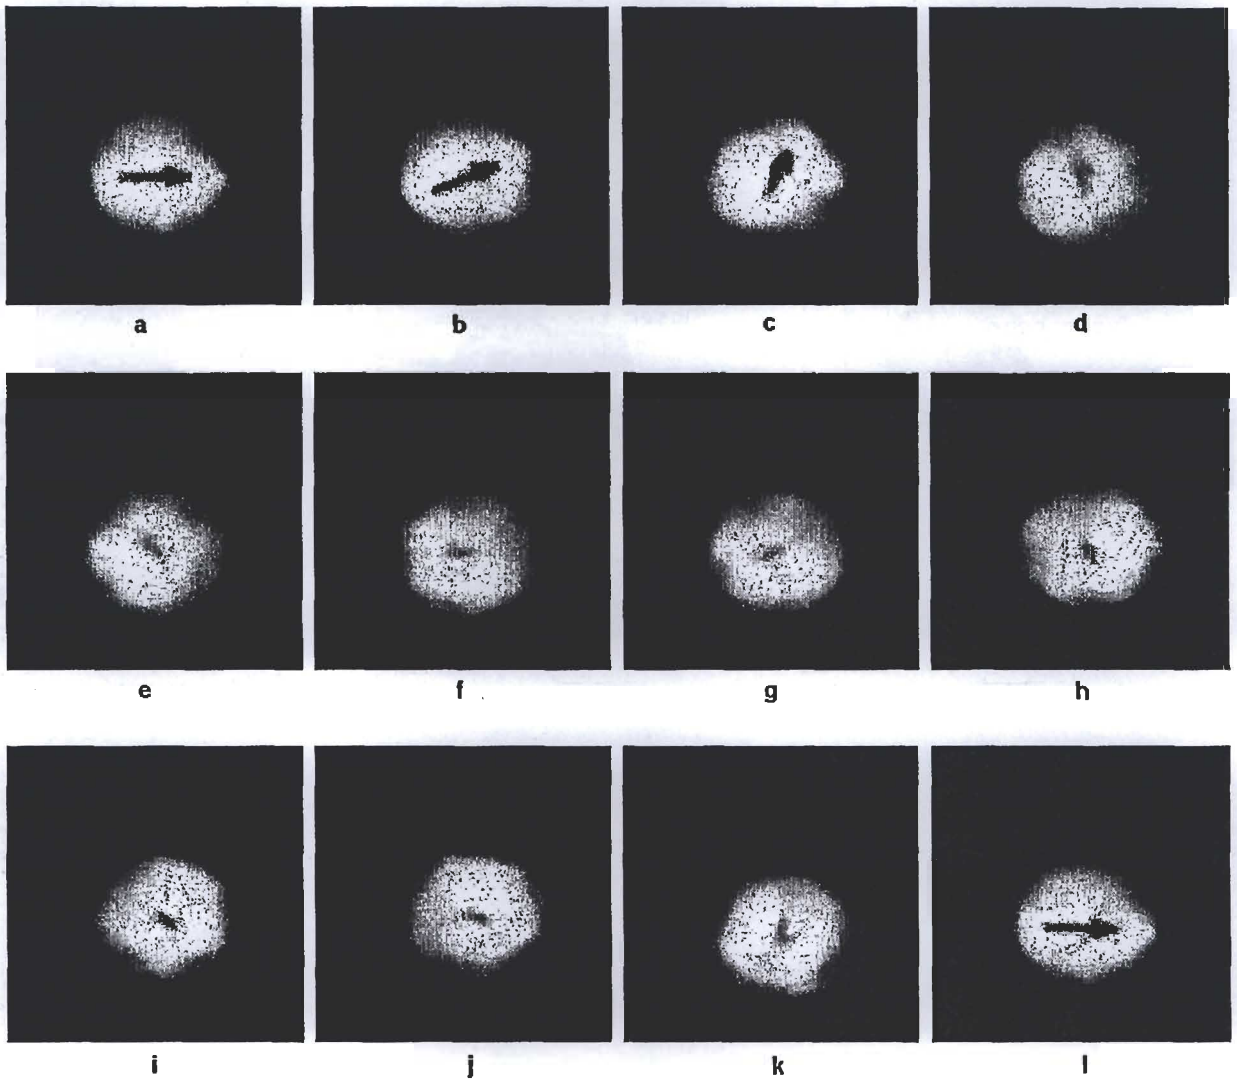


Figure 30

15 APR 2005

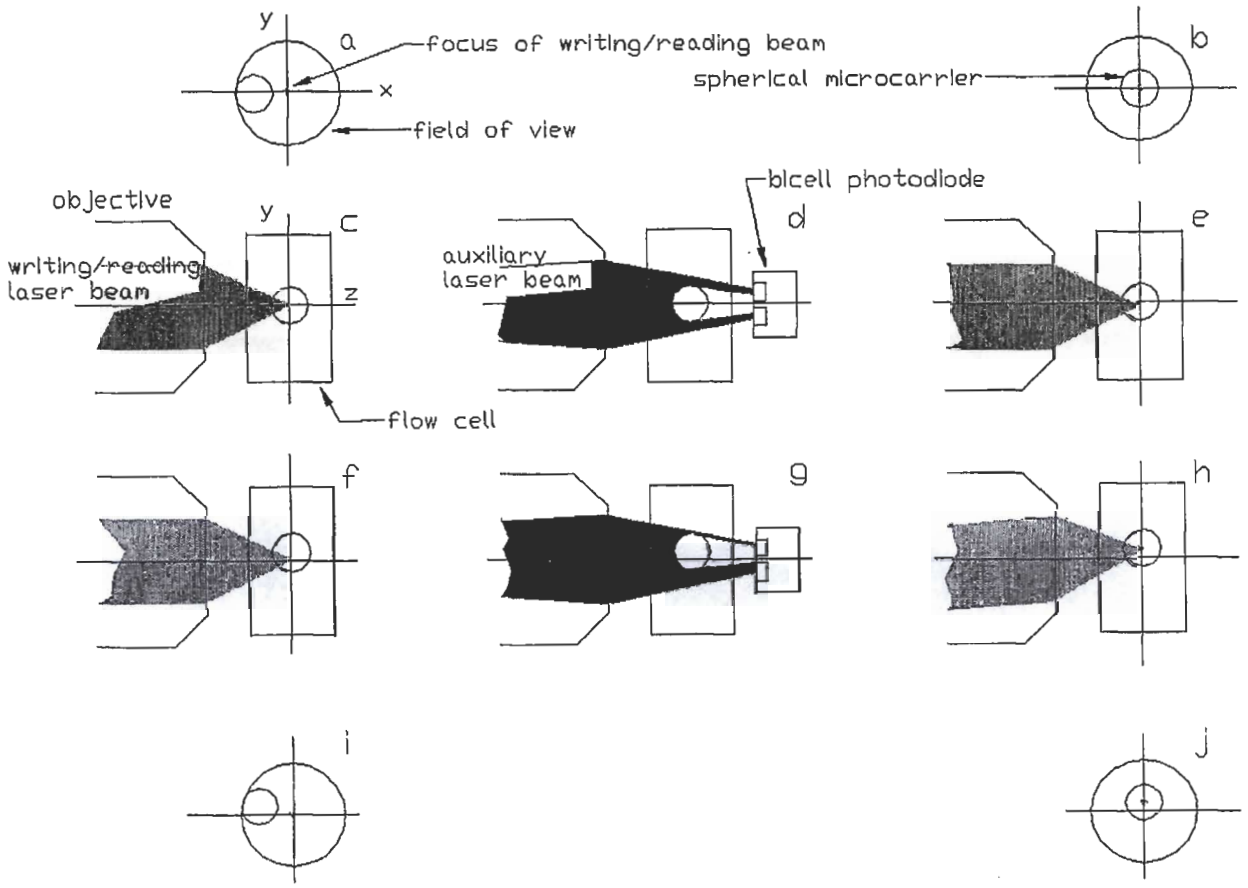


Figure 31