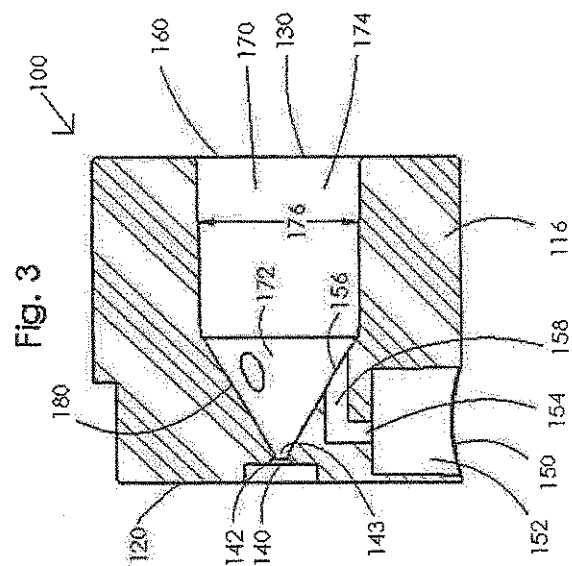
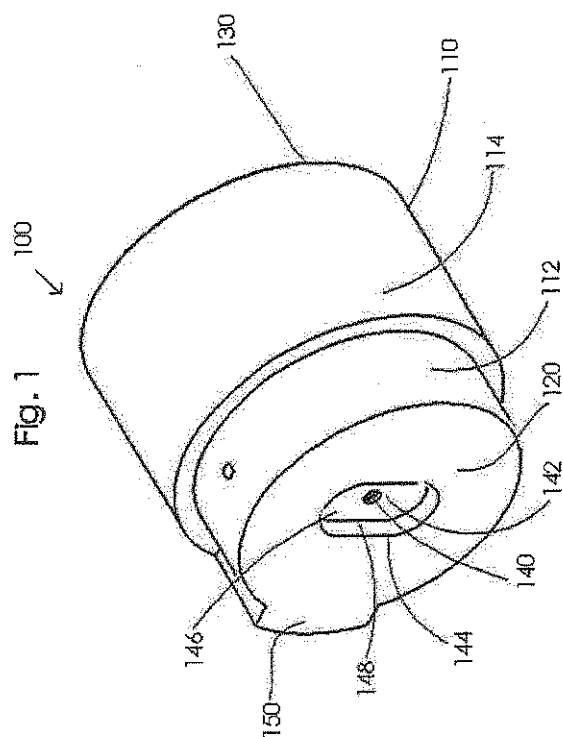
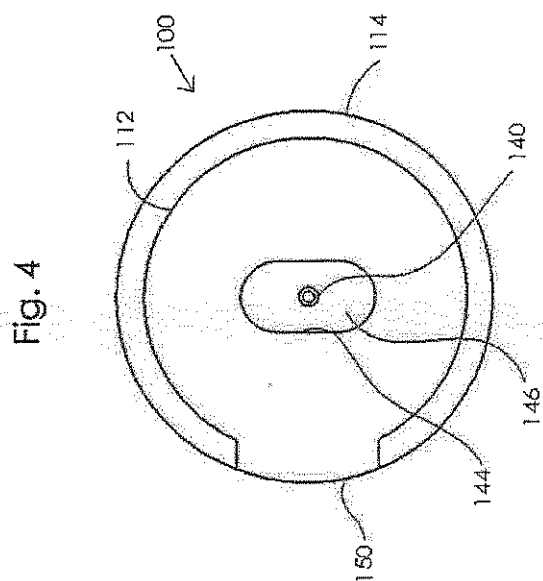
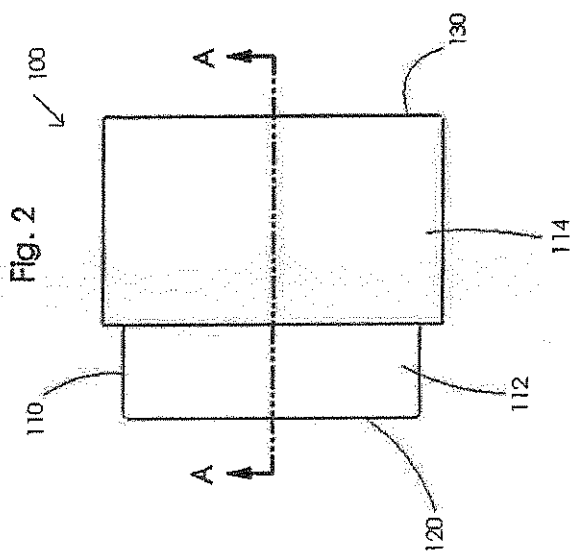




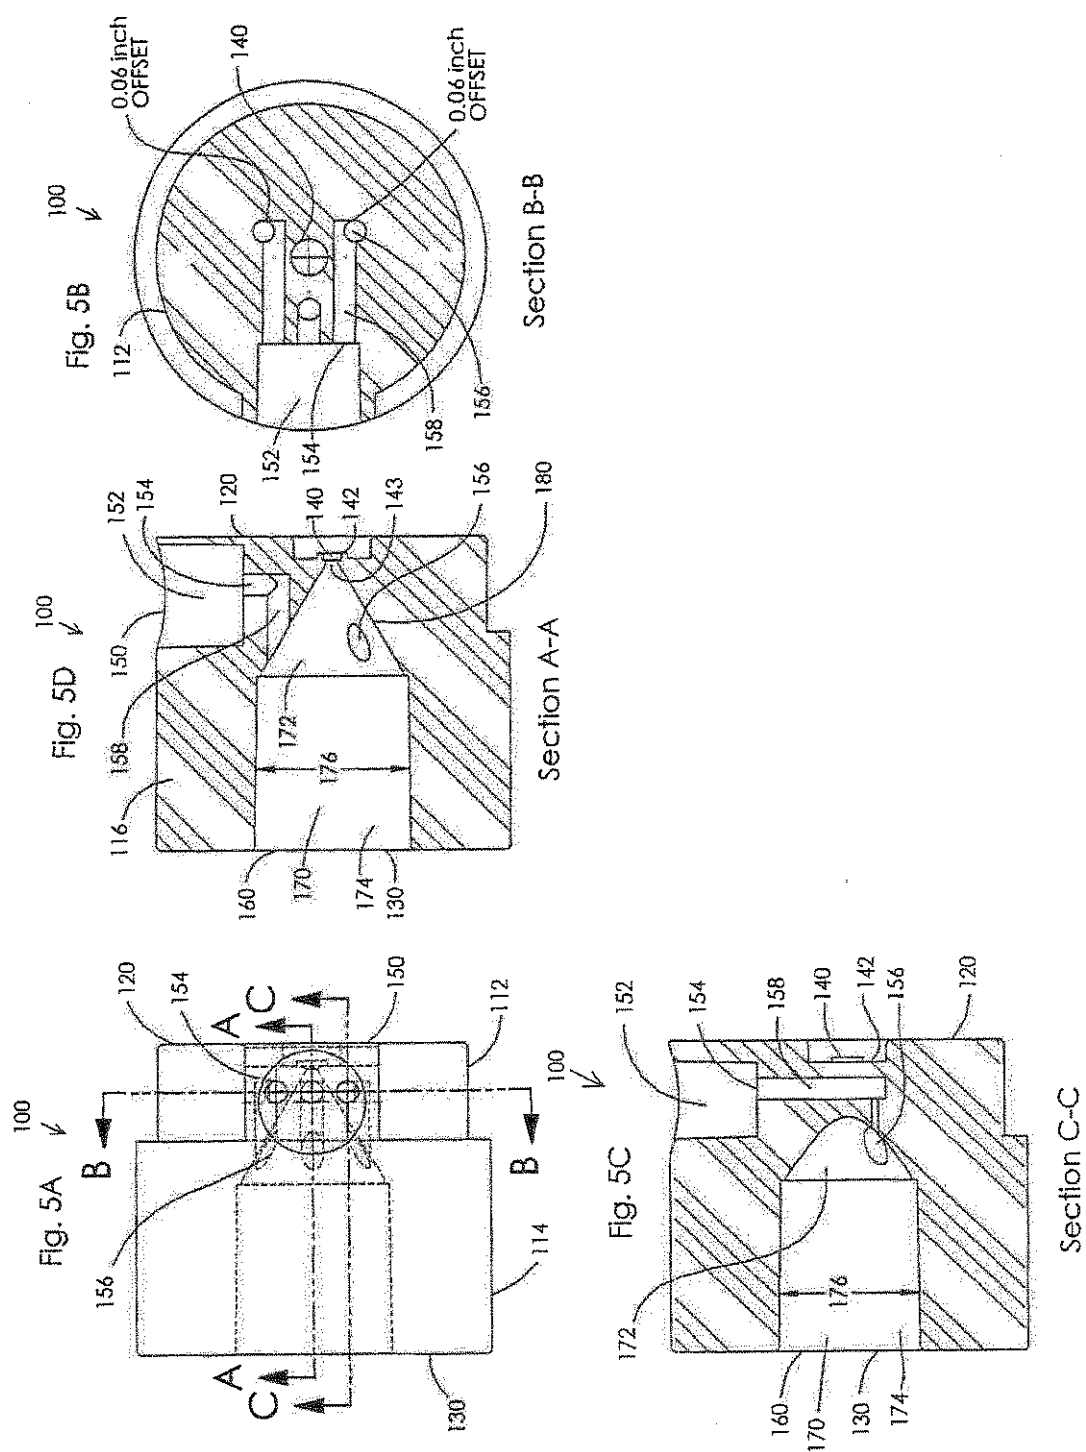


Fig. 6A

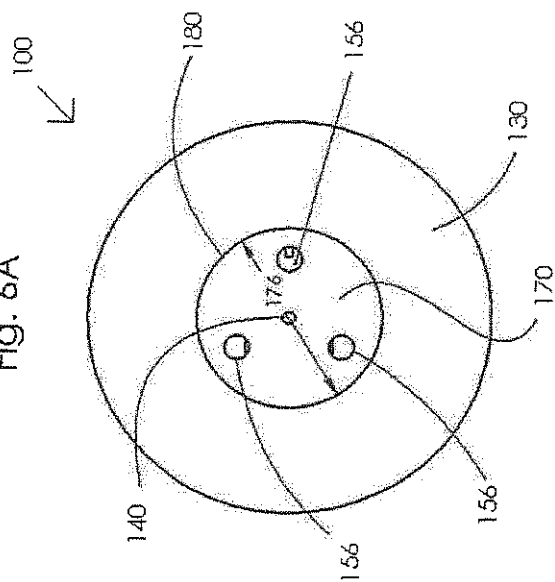


Fig. 6B

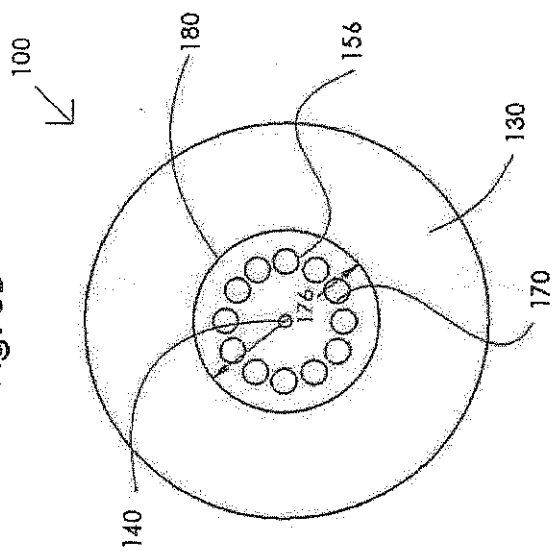


Fig. 6C

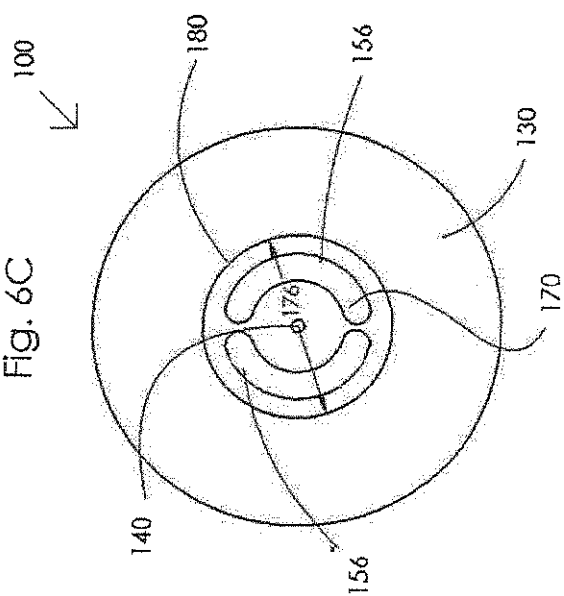


Fig. 7A: Ventilator Aerosol Delivery System

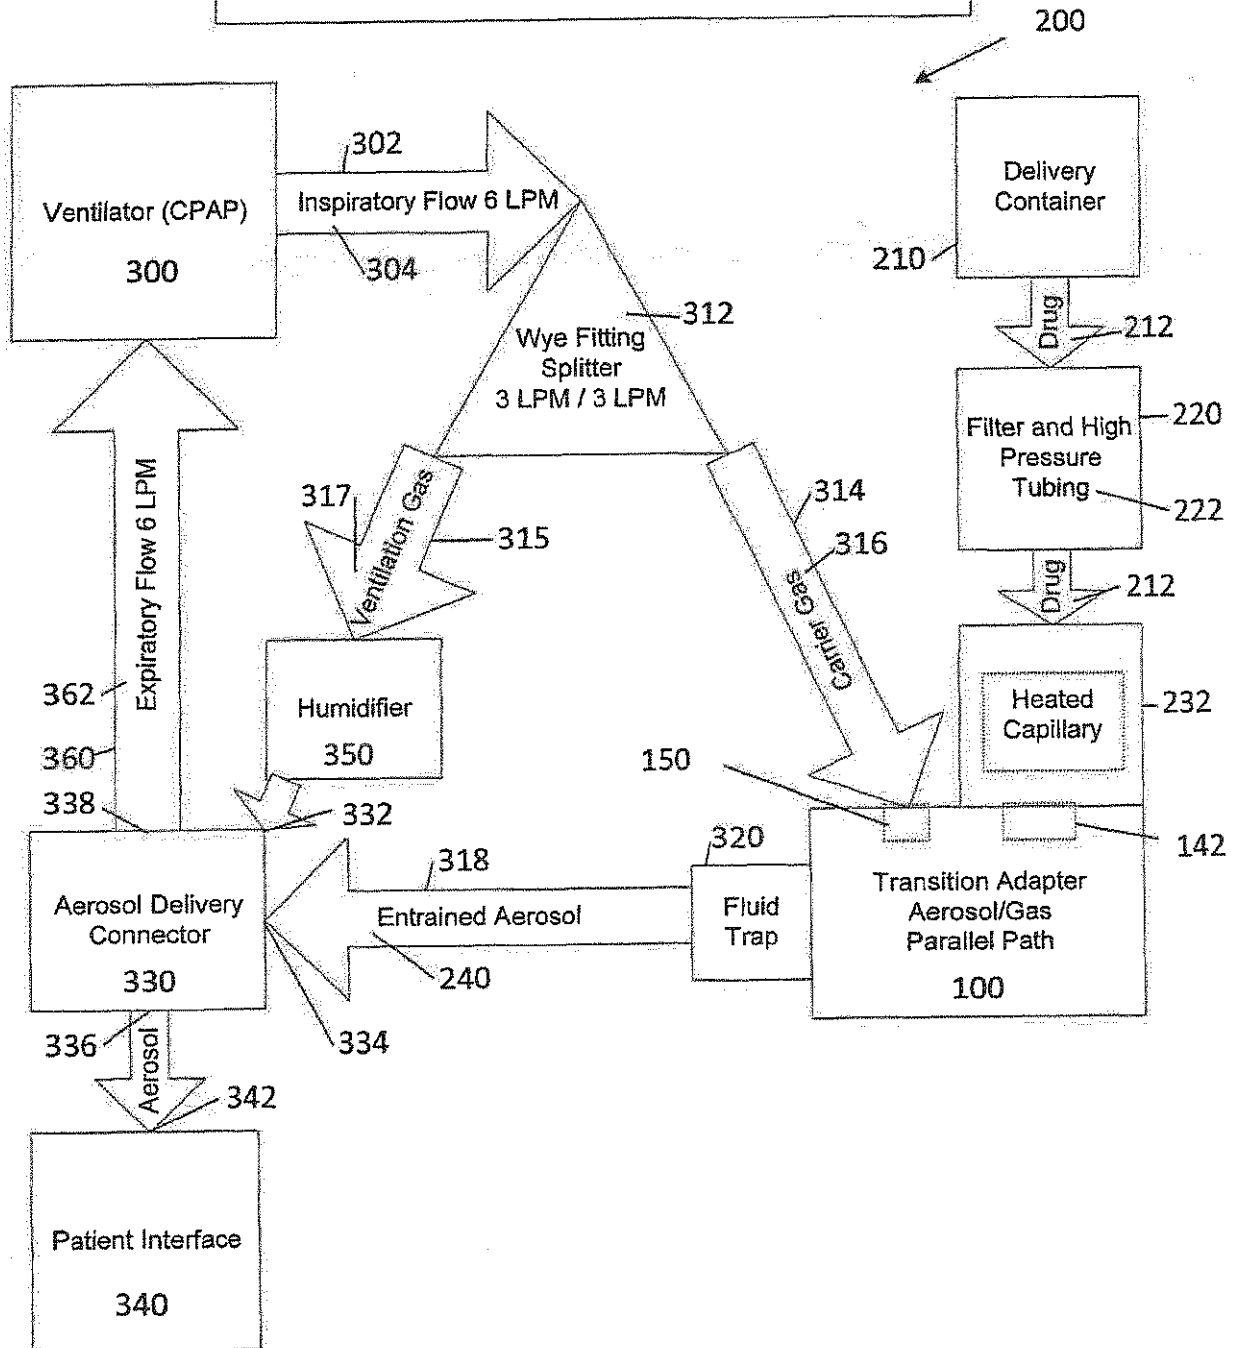


Fig. 7B: Bubble CPAP Ventilator Aerosol Delivery System

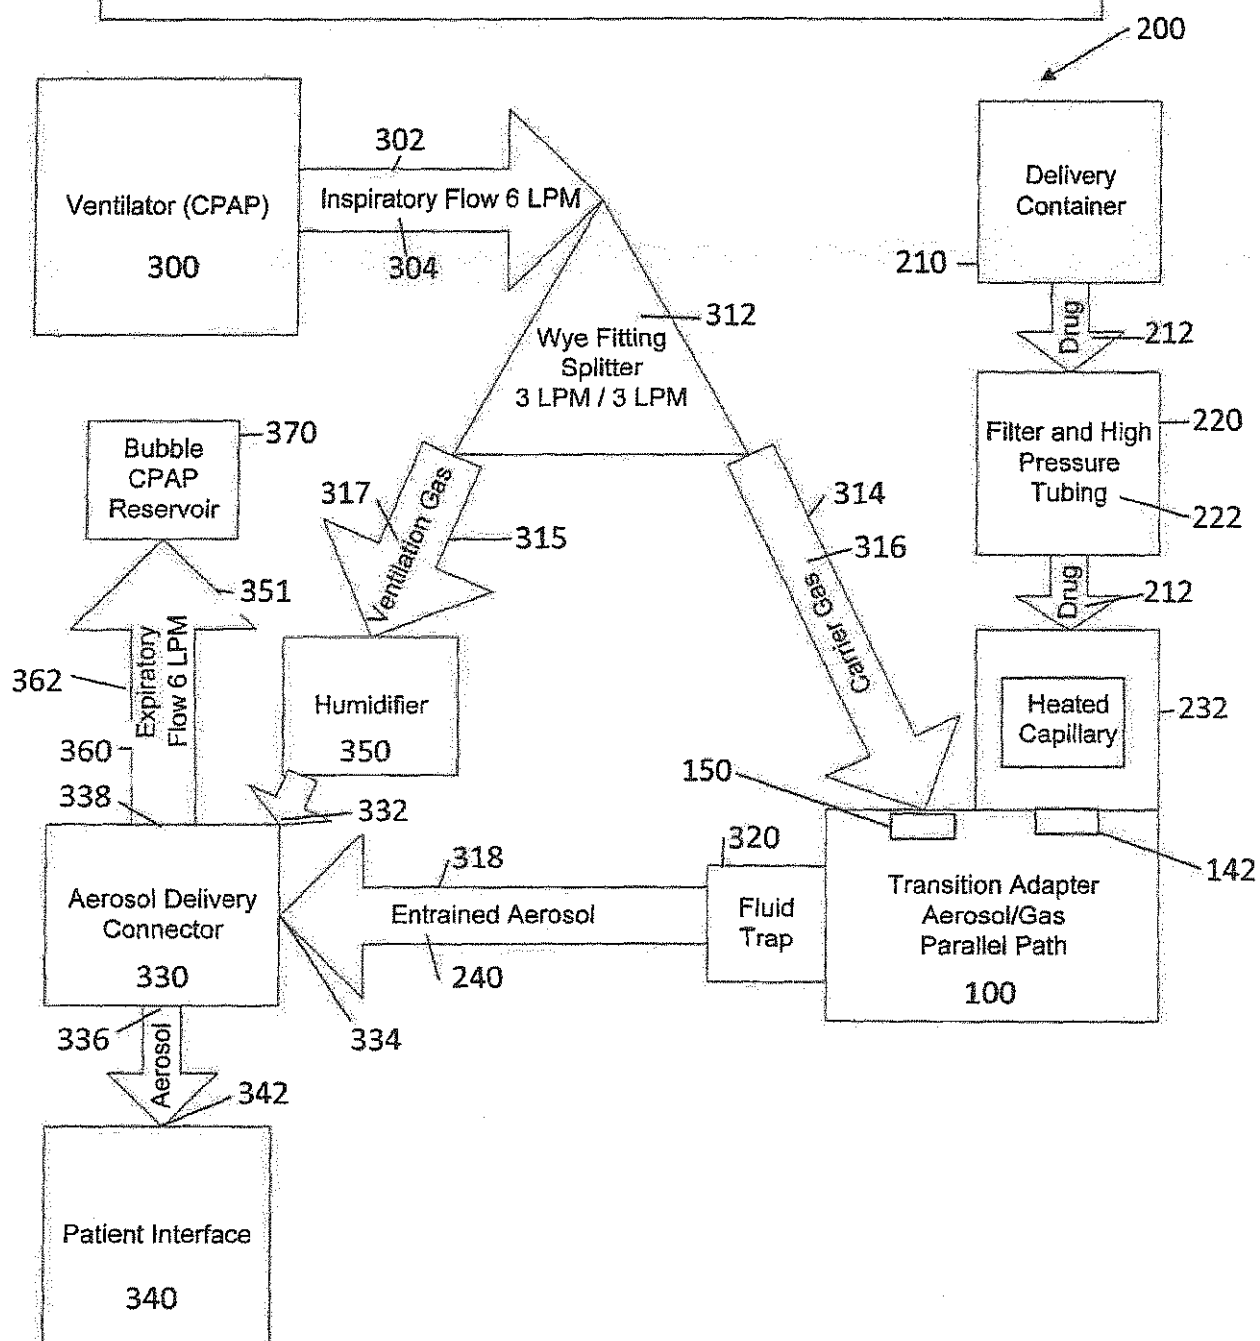


Fig. 7C: Bubble CPAP Ventilator Aerosol Delivery System



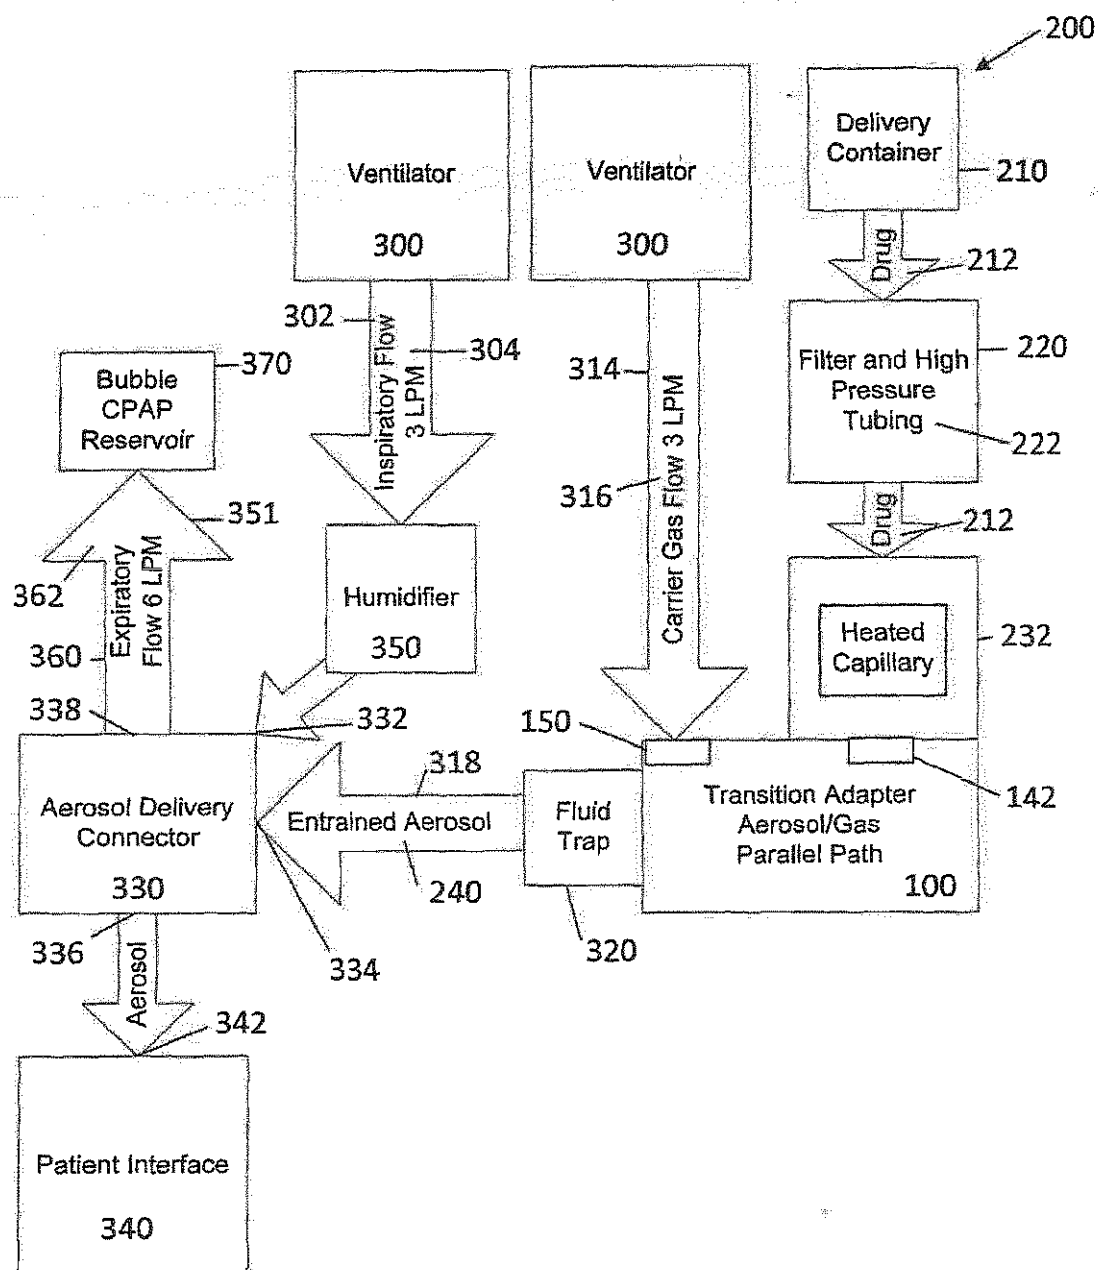


FIG. 8

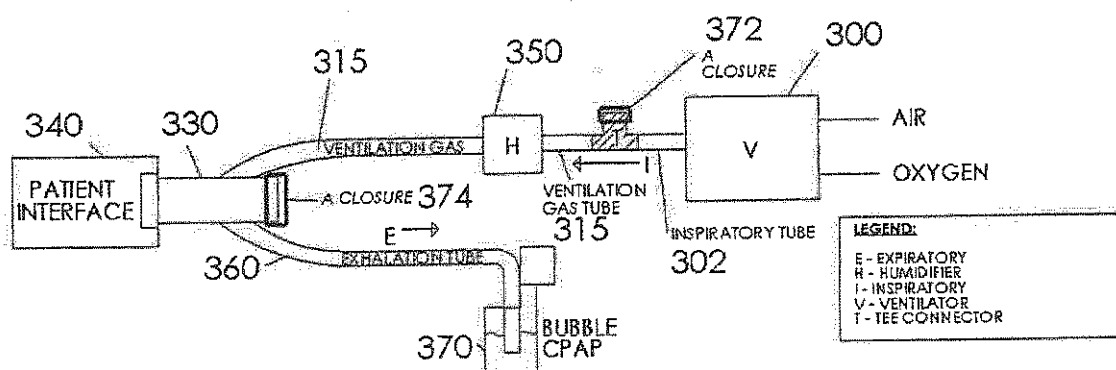

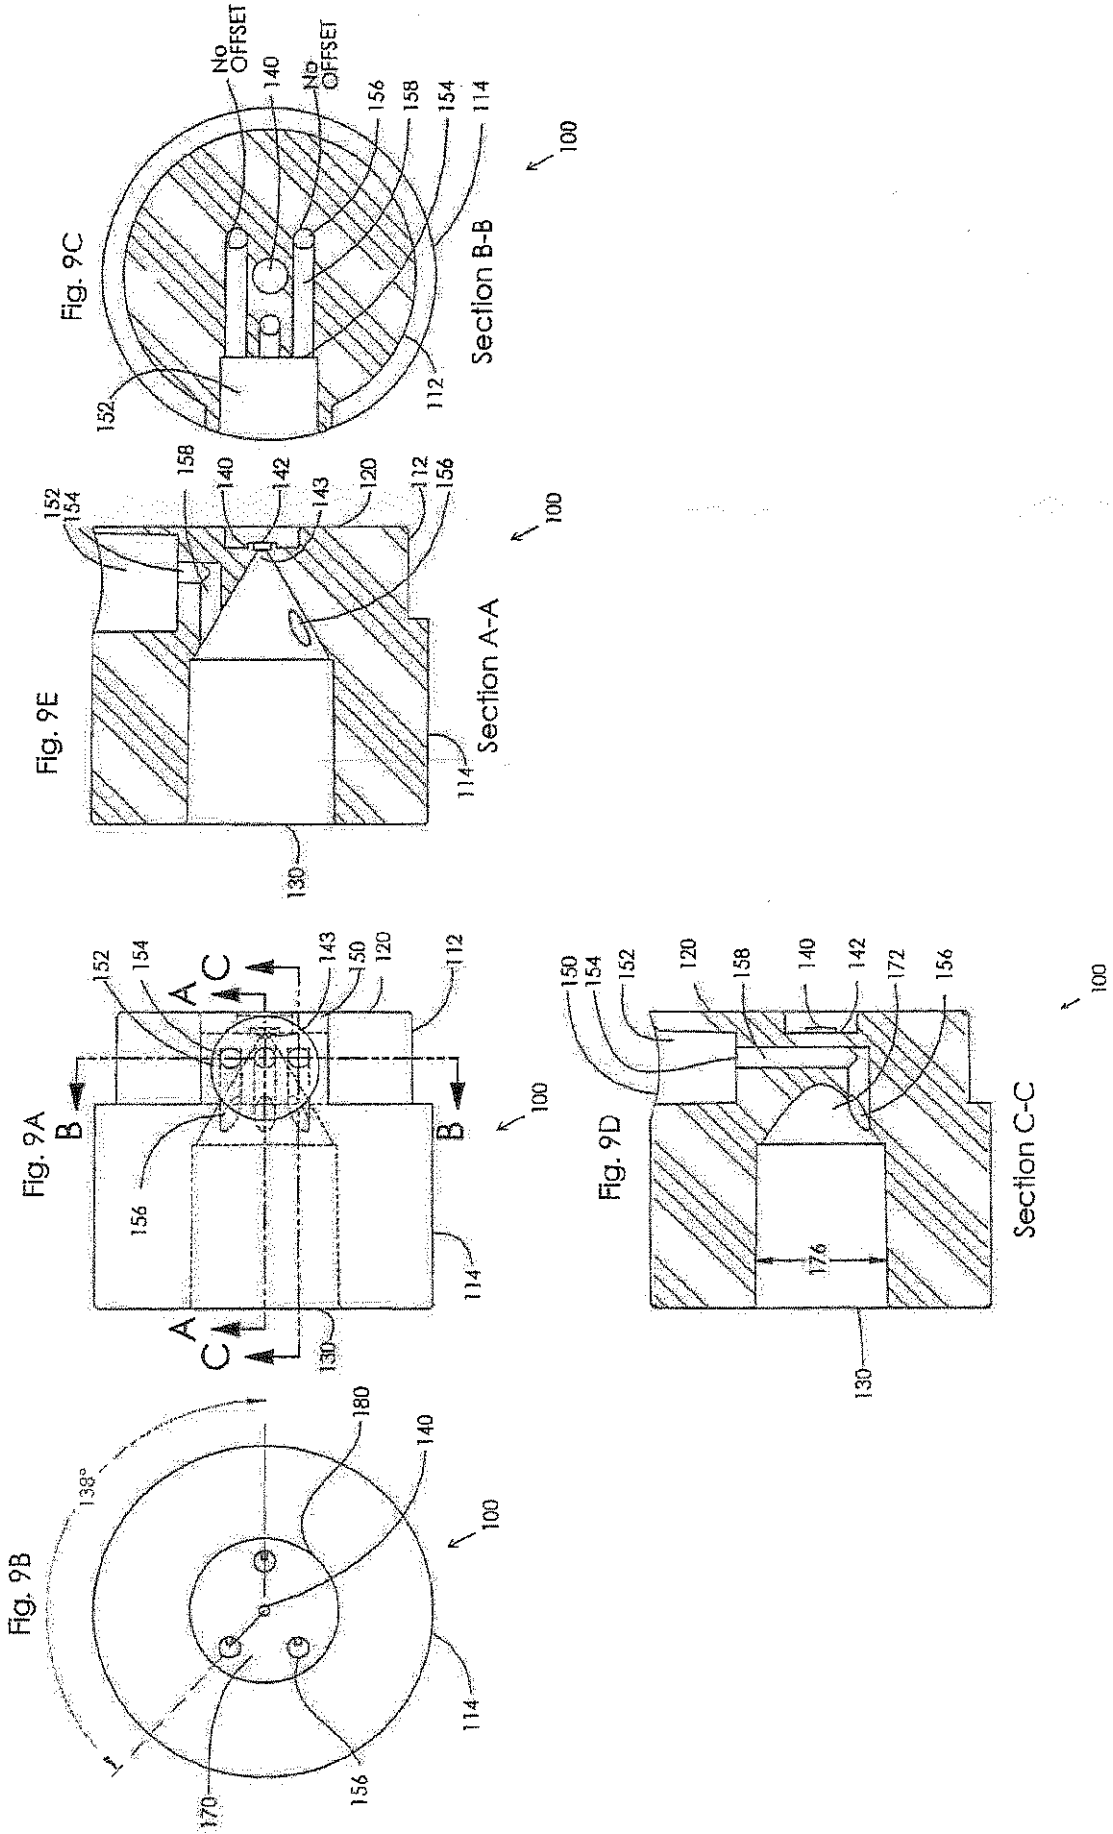

9/13

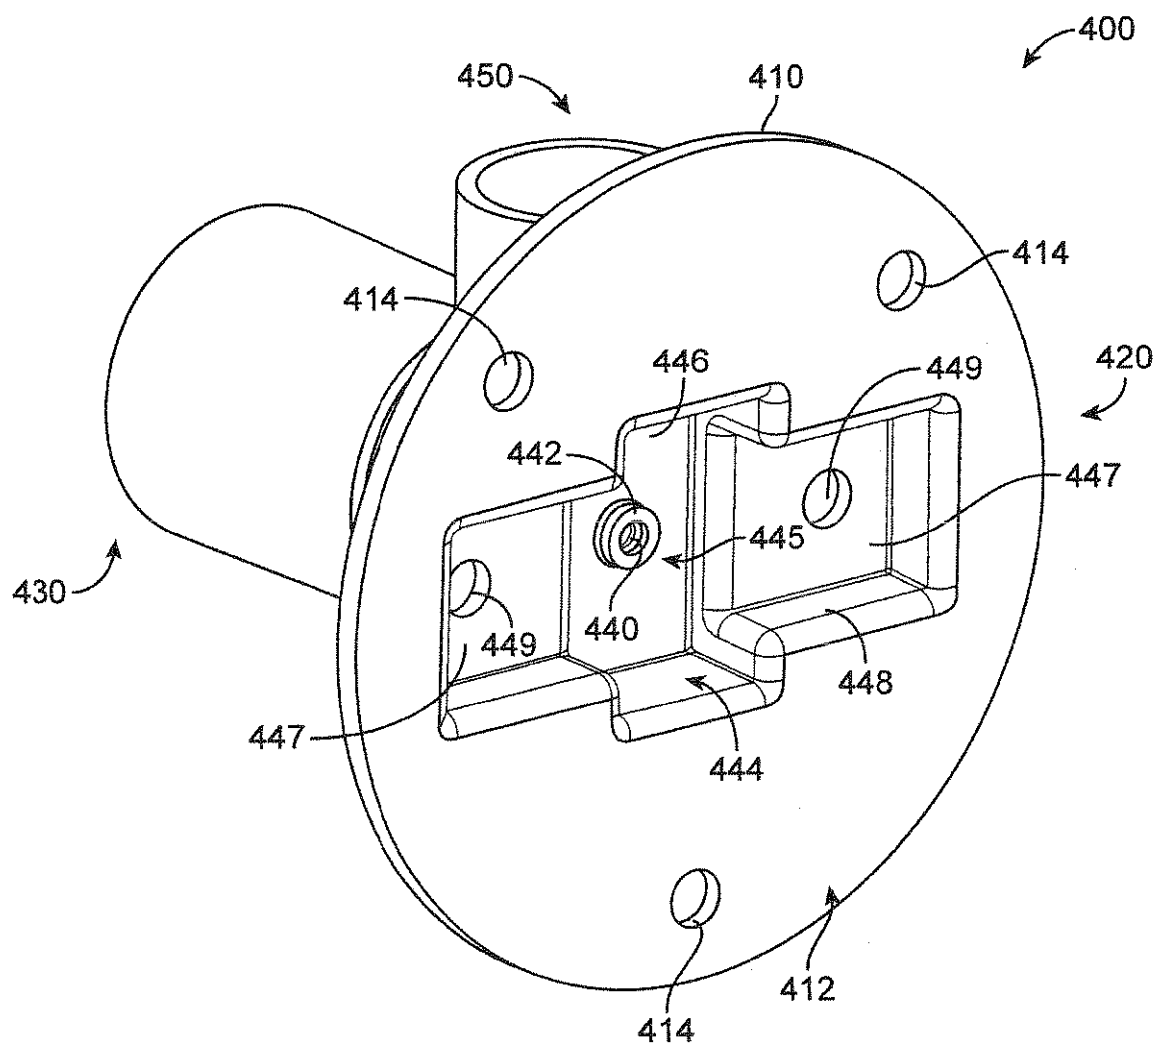


FIG. 10A

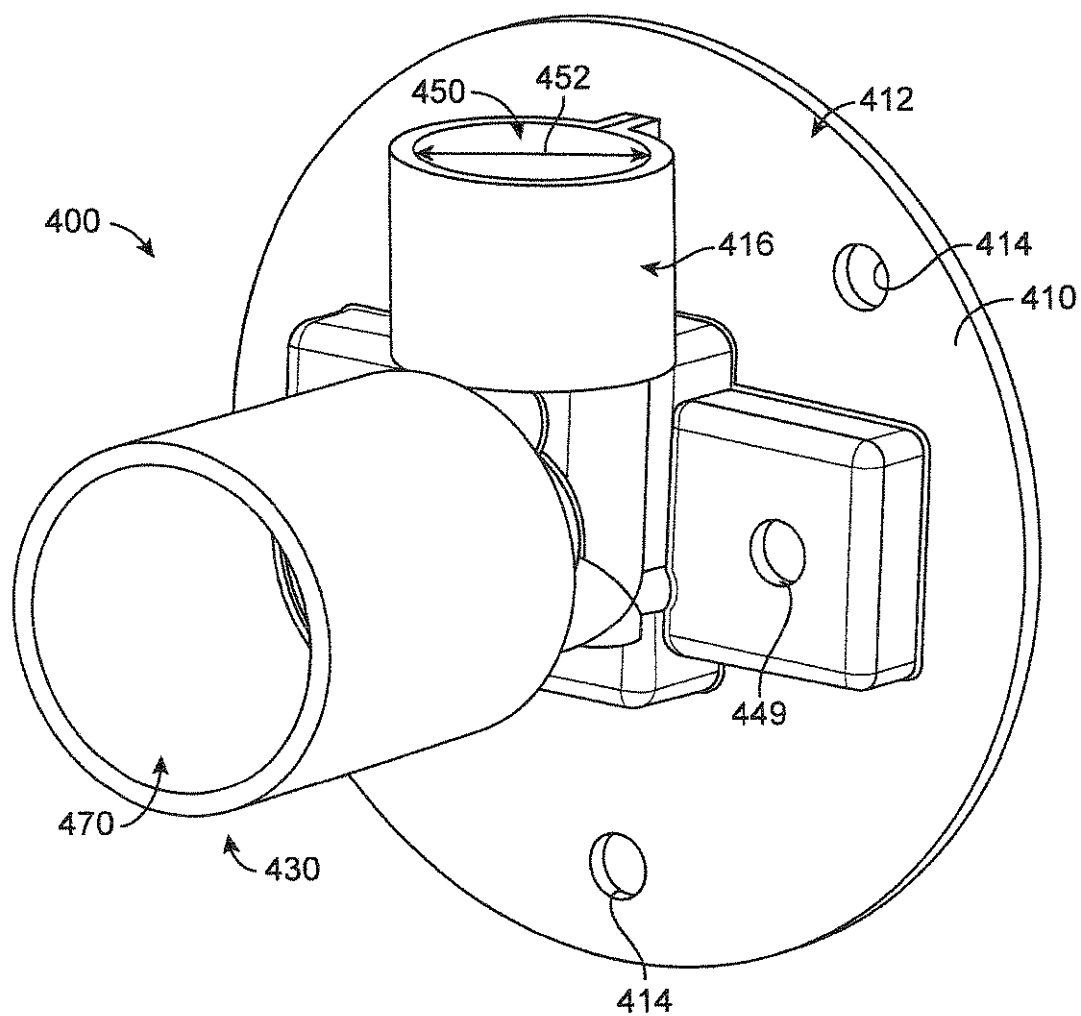


FIG. 10B

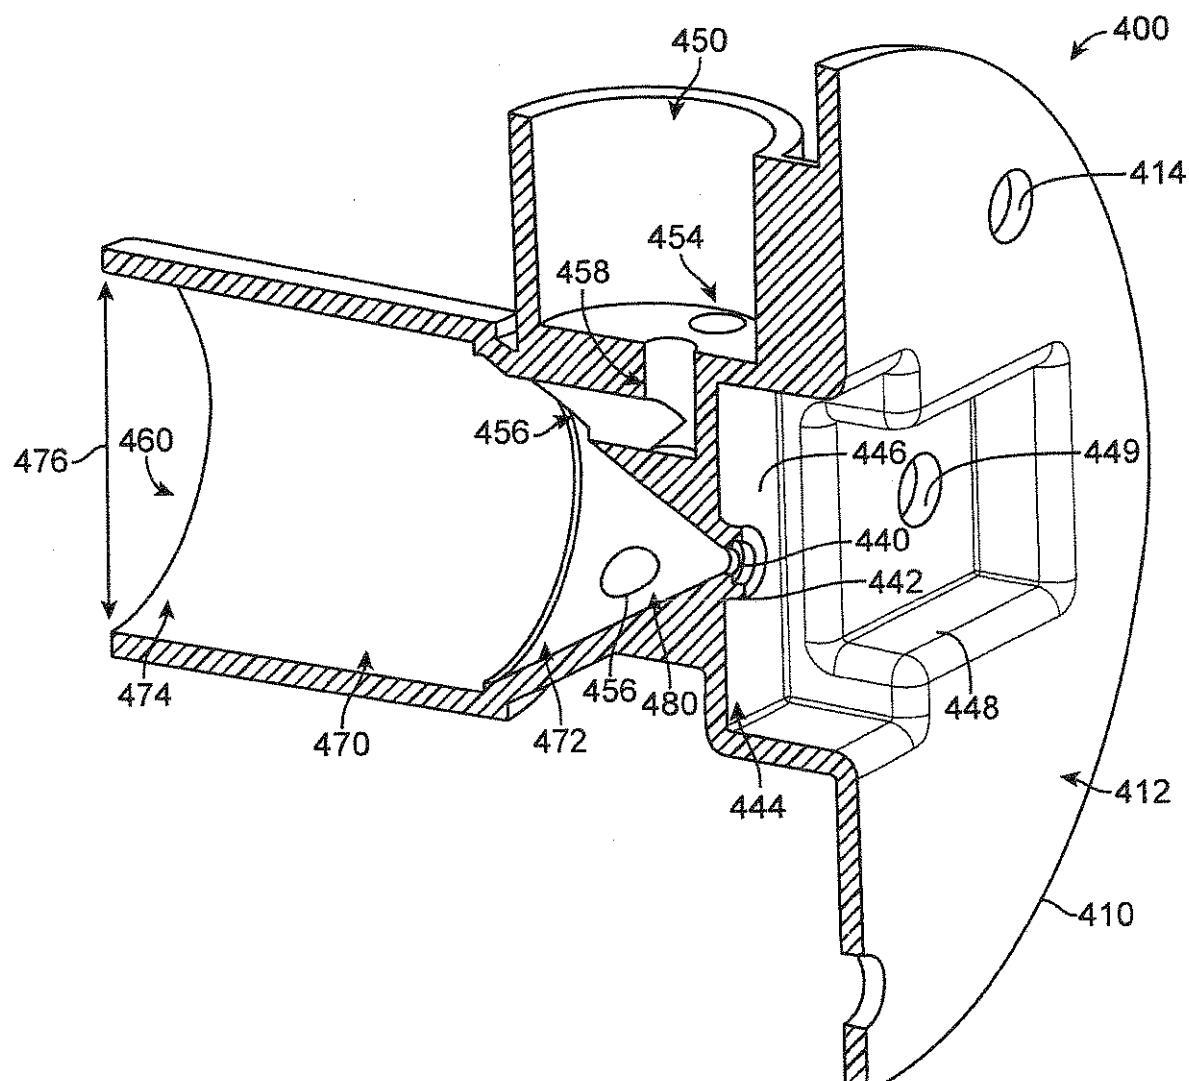


FIG. 10C

12/13

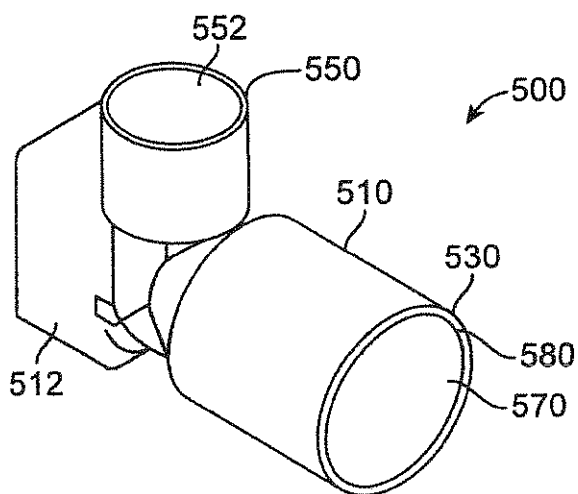


FIG. 11A

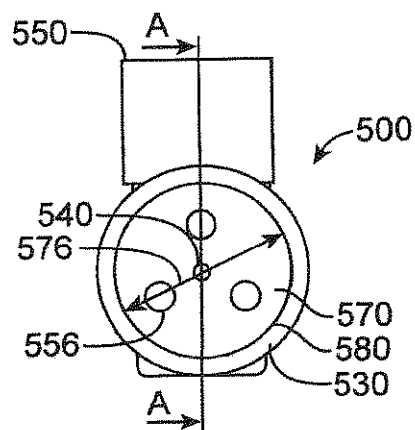


FIG. 11B

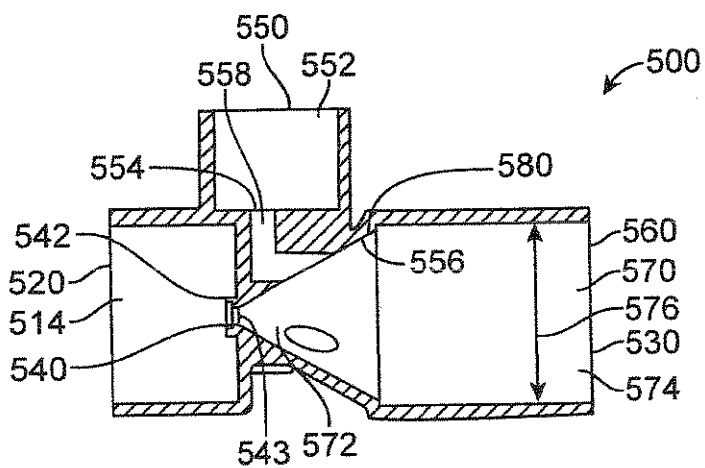


FIG. 11C

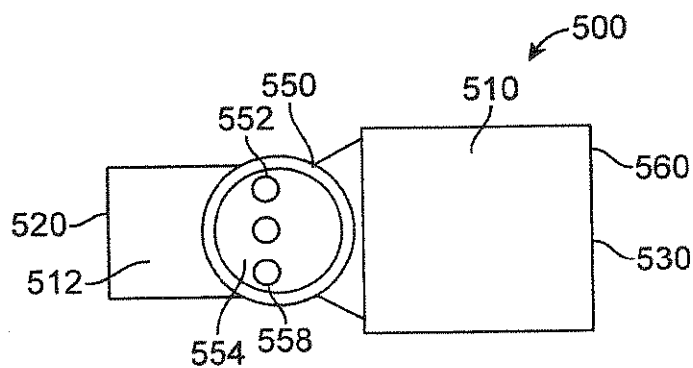


FIG. 11D

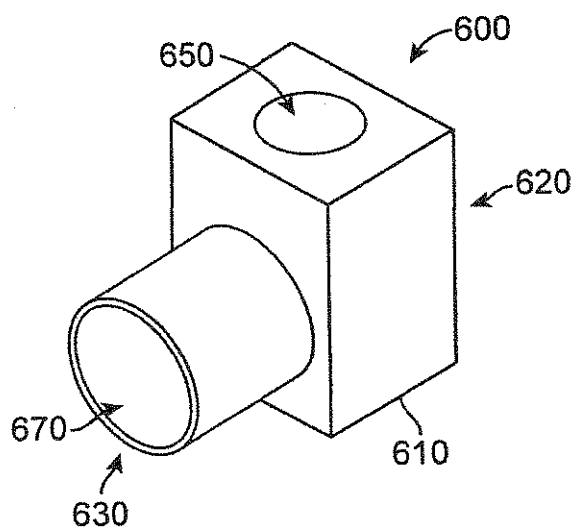


FIG. 12A

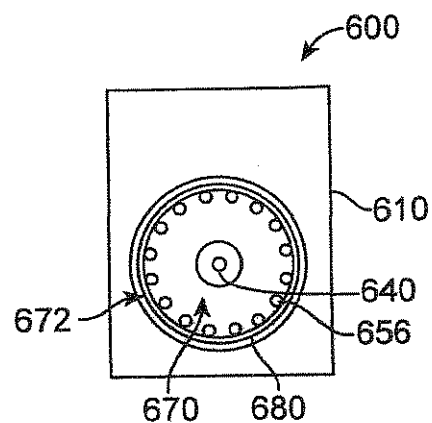


FIG. 12B



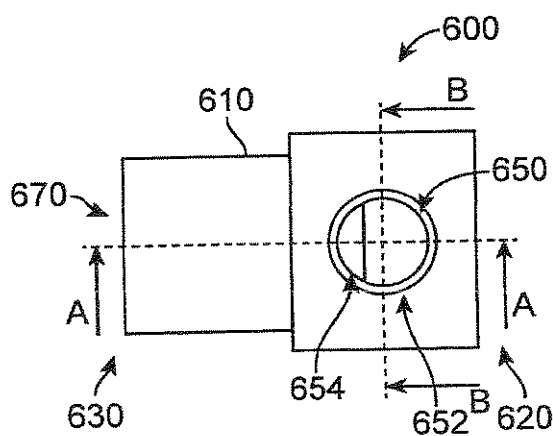


FIG. 12C

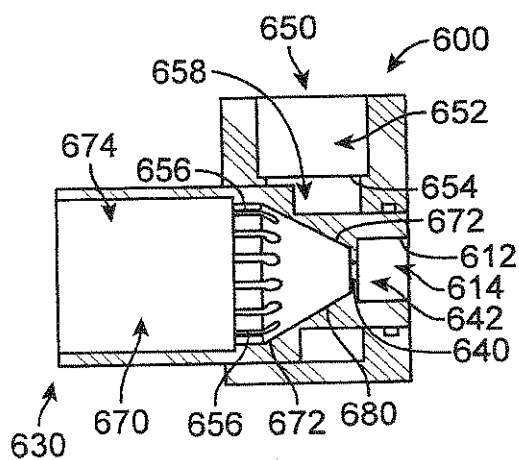

SECTION A-A

FIG. 12D

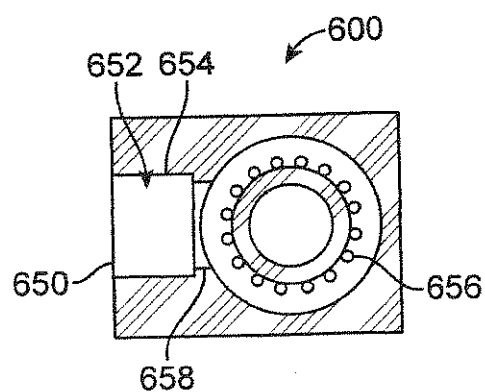

SECTION B-B

FIG. 12E