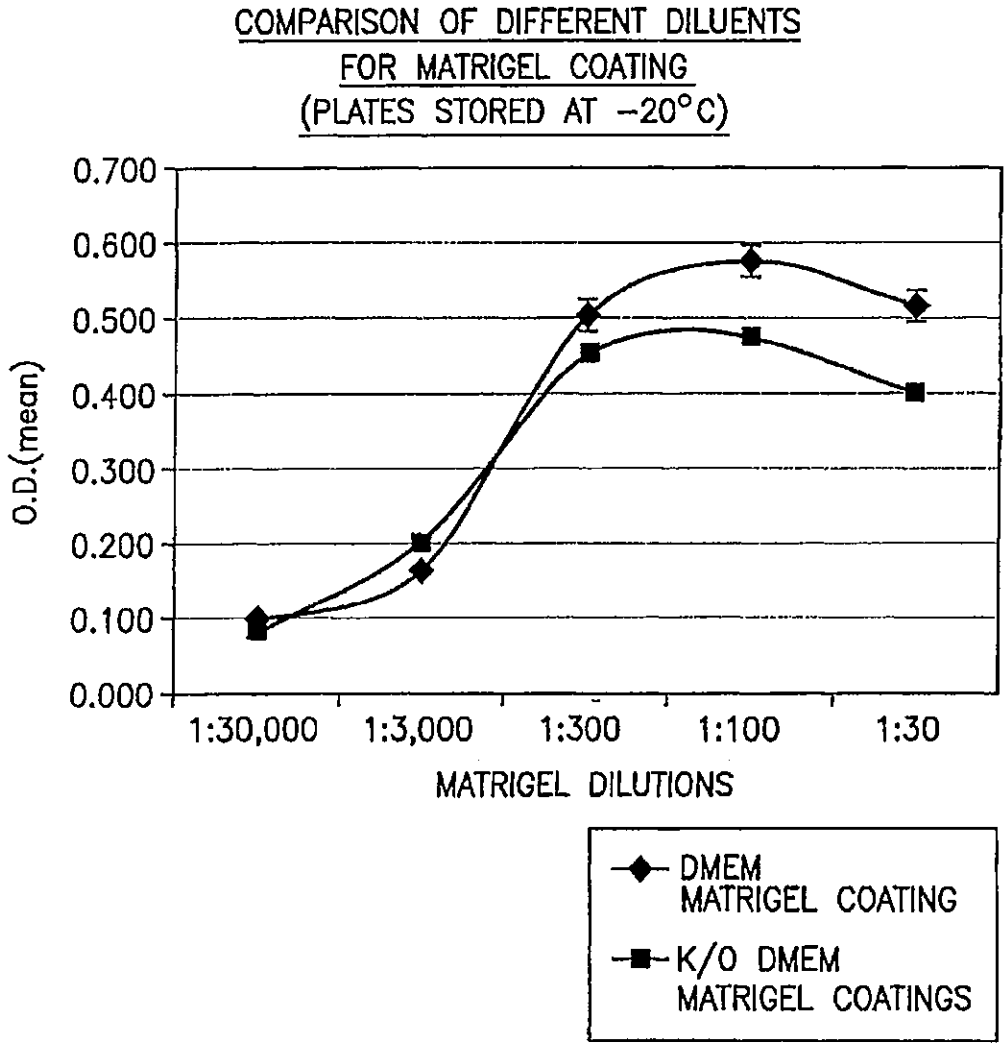

COMPARISON OF DIFFERENT DILUENTS
FOR MATRIGEL COATING
(PLATES STORED AT −20°C)
0.700
0.600
0.500
0.400
0.300
0.200
0.100
0.000
O.D.(mean)
1:30,000
1:3,000
1:300
1:100
1:30
MATRIGEL DILUTIONS
DMEM
MATRIGEL COATING
K/O DMEM
MATRIGEL COATINGS

FIG.1

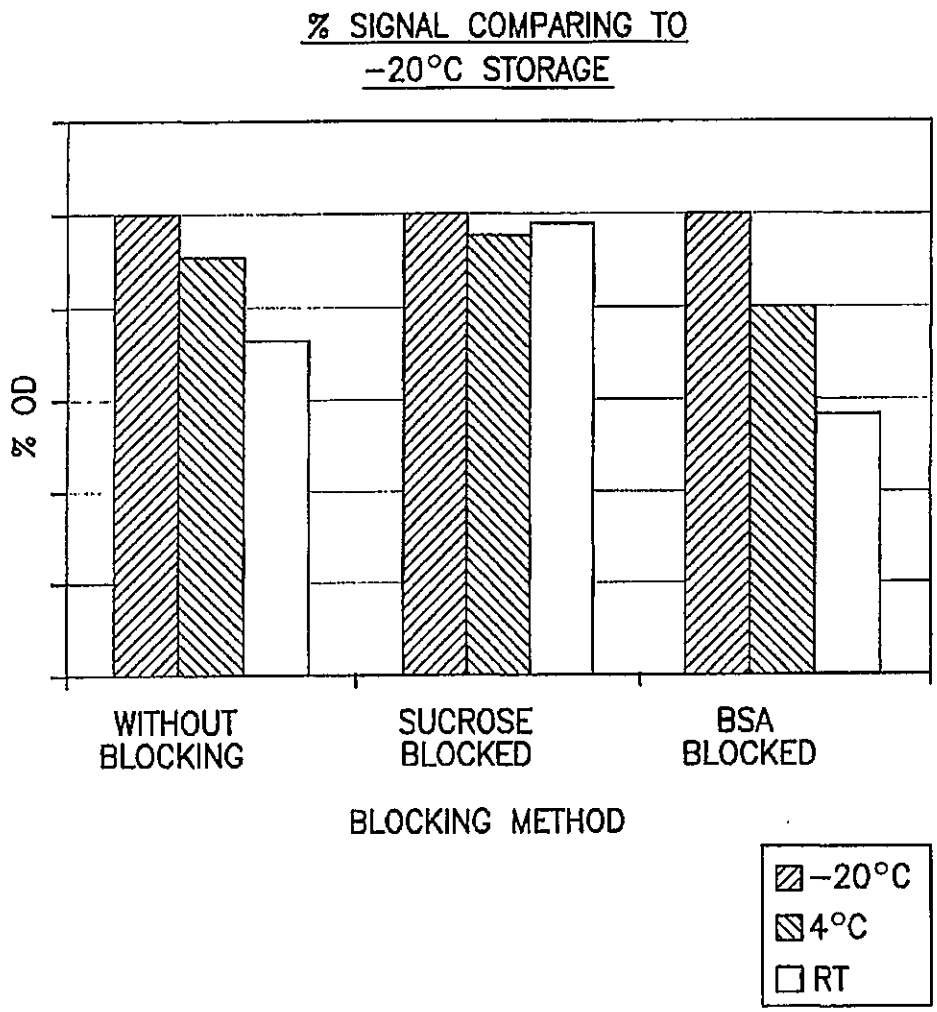

% SIGNAL COMPARING TO
-20°C STORAGE
% OD
WITHOUT BLOCKING
SUCROSE BLOCKED
BSA BLOCKED
BLOCKING METHOD
-20°C
4°C
RT

FIG.2