

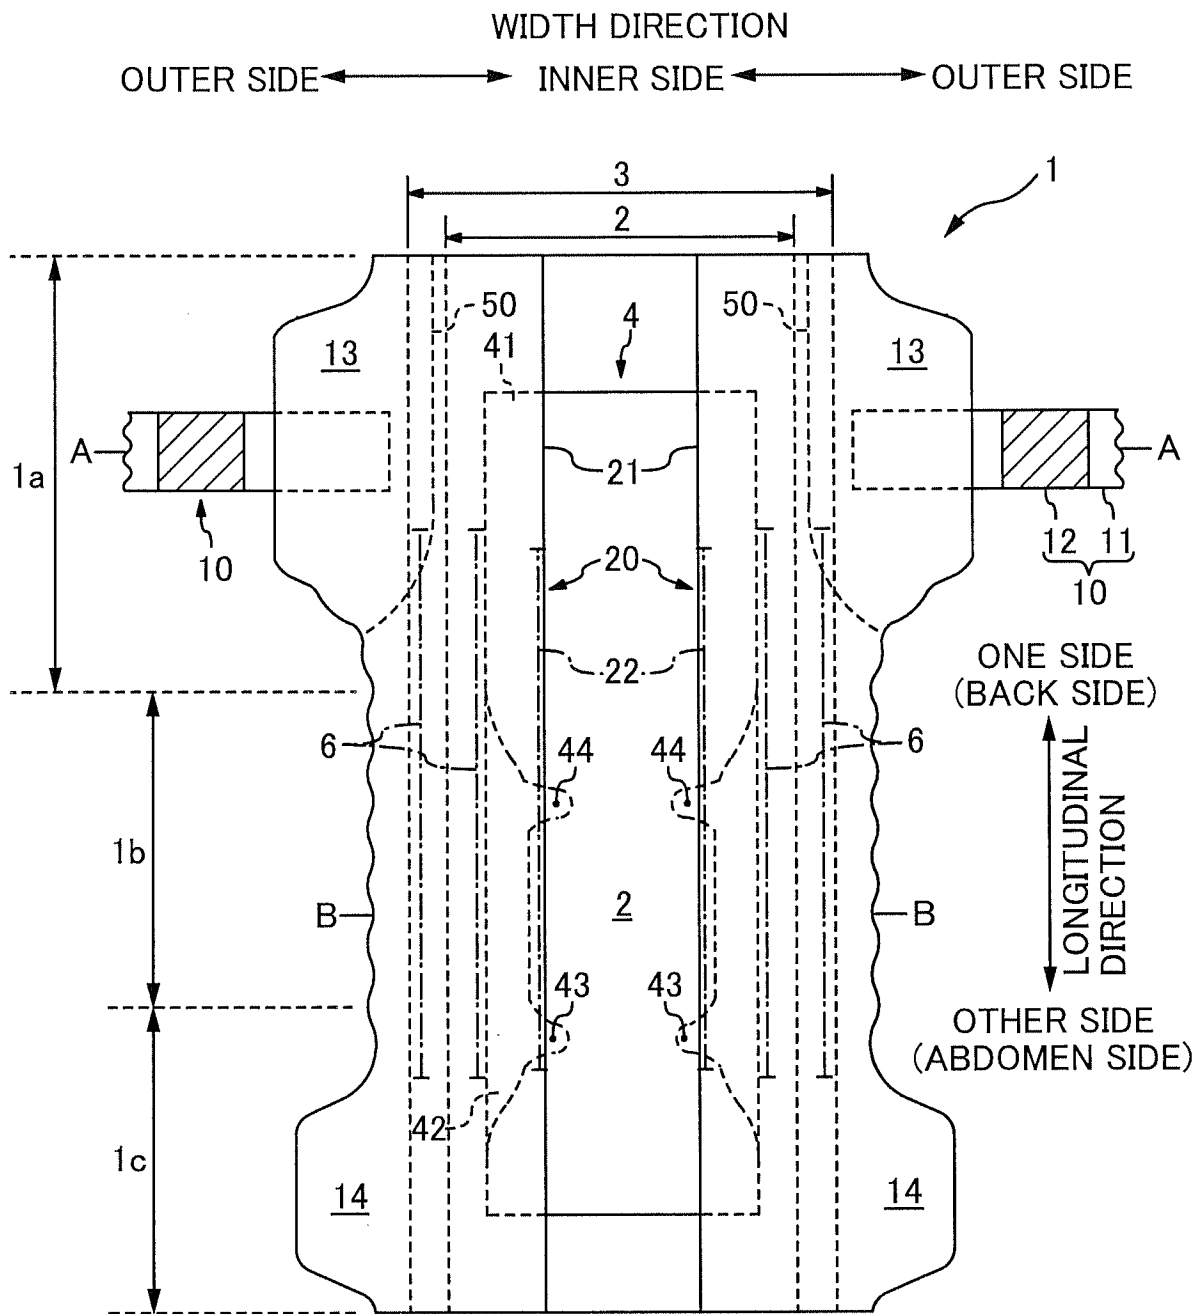


FIG. 1

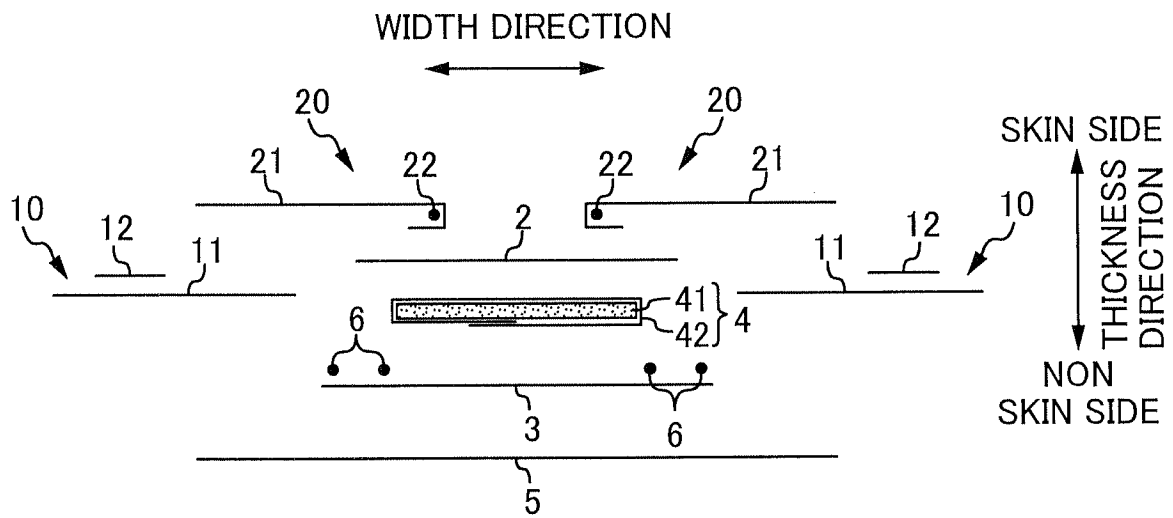


FIG. 2A

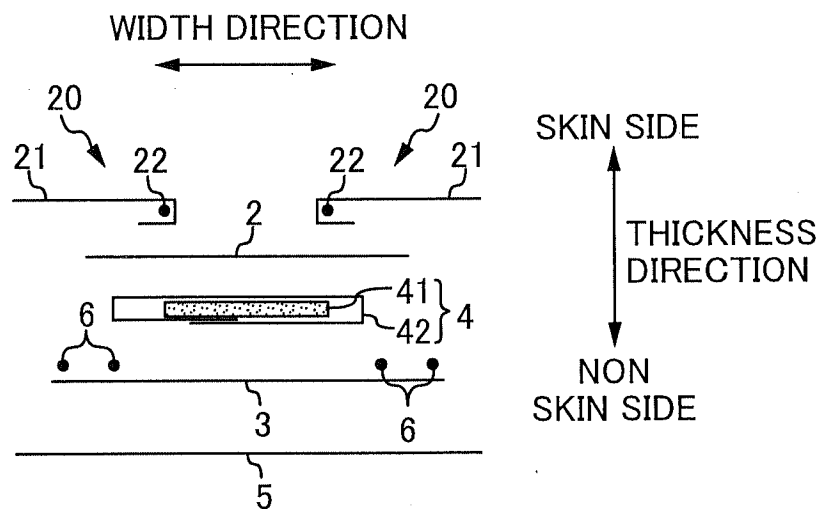


FIG. 2B

FIG. 3A

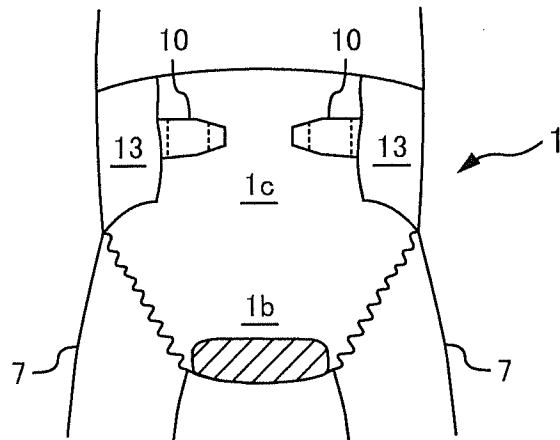


FIG. 3B

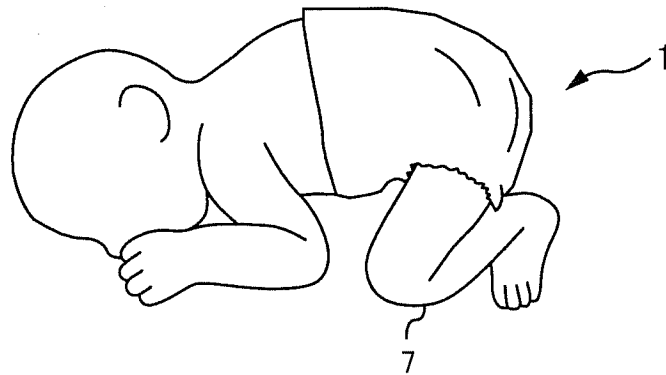
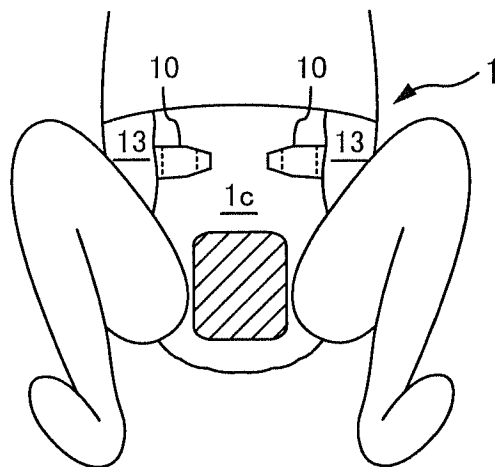


FIG. 3C



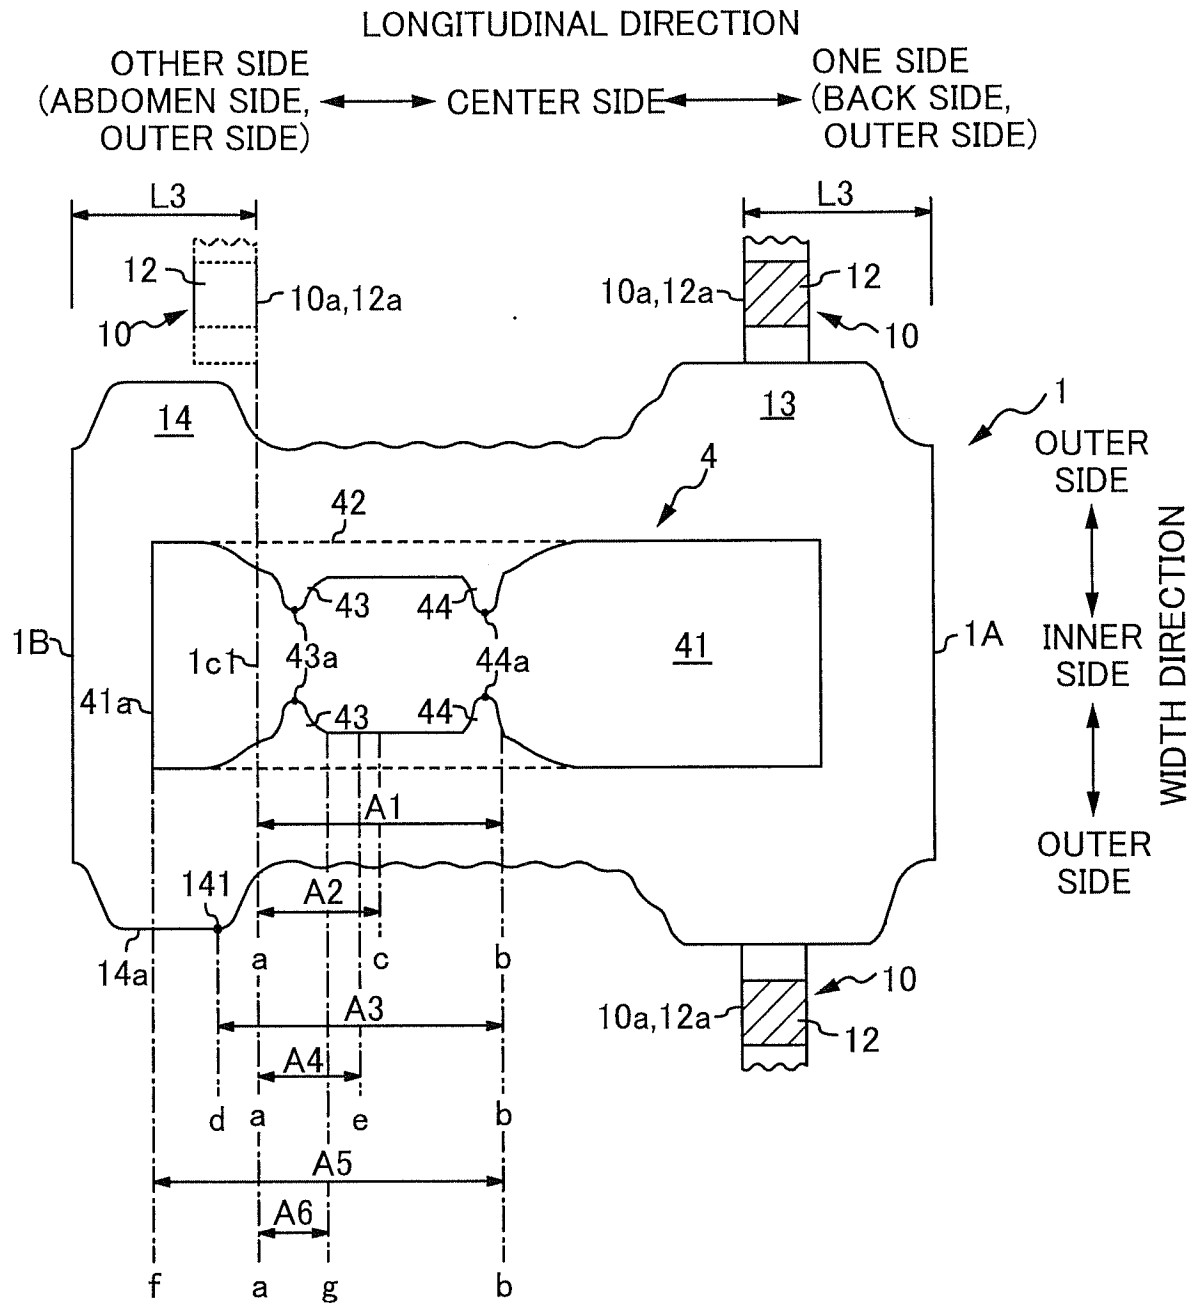


FIG. 4

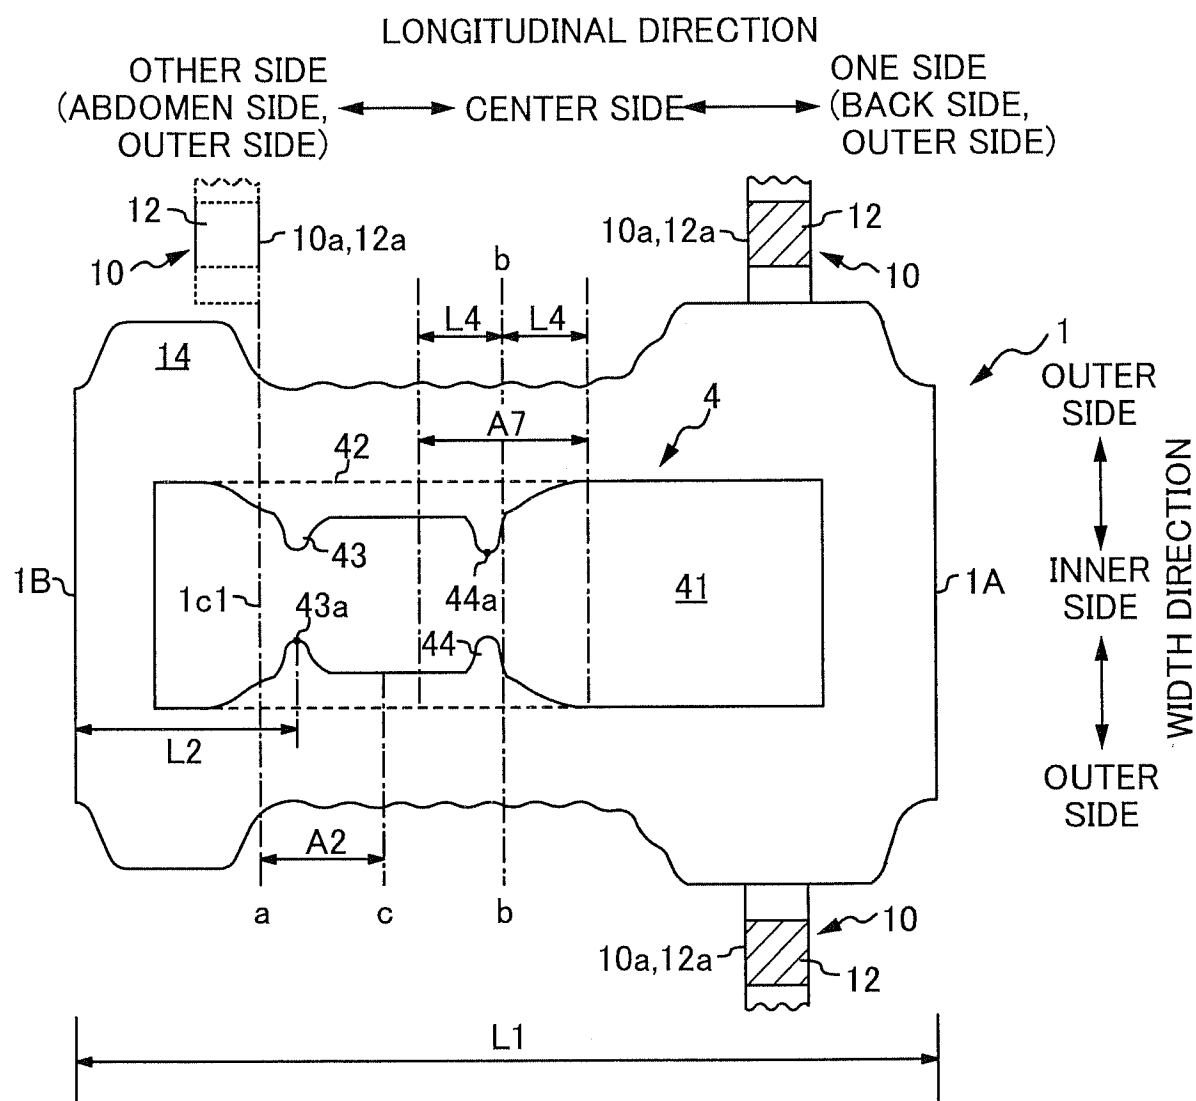


FIG. 5

PRODUCT LENGTH FIRST LENGTH L1 (mm)	OTHER END TO TIP PART OF ABDOMEN SIDE NOTCH		FITTING EVALUATION
	SECOND LENGTH L2(mm)	RATIO L2/L1(%)	
230	45	20	POOR
	55	24	FAIR
	60	26	FAIR
	65	28	POOR
	85	37	POOR
270	40	15	POOR
	50	19	POOR
	60	22	FAIR
	70	26	FAIR
	85	31	POOR
	105	39	POOR

FIG. 6

FIG. 1 is a schematic diagram of a cross-section of a device 10. The diagram shows a central rectangular region 41. On the left side of 41 is a shaded rectangular area 43. On the right side of 41 is a rectangular area 44. The top and bottom edges of 41 are curved. The left side of 43 is labeled 43a. The top and bottom corners of 43 are labeled 43b and 43c respectively. The top and bottom corners of 44 are labeled 44b and 44c respectively. The top and bottom edges of 41 are labeled 431 and 441 respectively. The diagram is labeled "LONGITUDINAL DIRECTION" at the top and "OTHER SIDE (ABDOMEN SIDE, OUTER SIDE)" on the left. The right side is labeled "ONE SIDE (BACK SIDE, OUTER SIDE)". The vertical axis is labeled "INNER SIDE" and "OUTER SIDE" with a double-headed arrow, and "WIDTH DIRECTION".

FIG. 7B

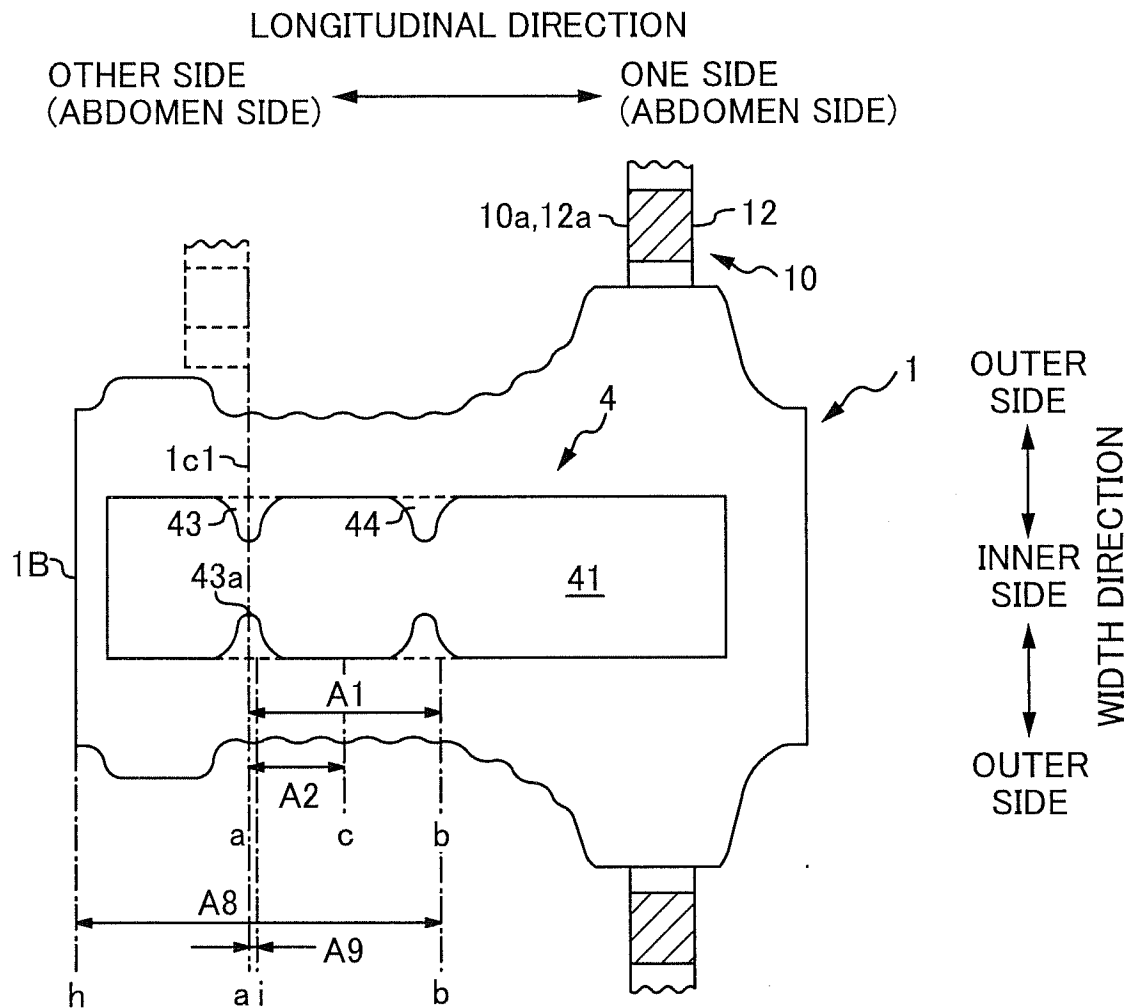


FIG. 8

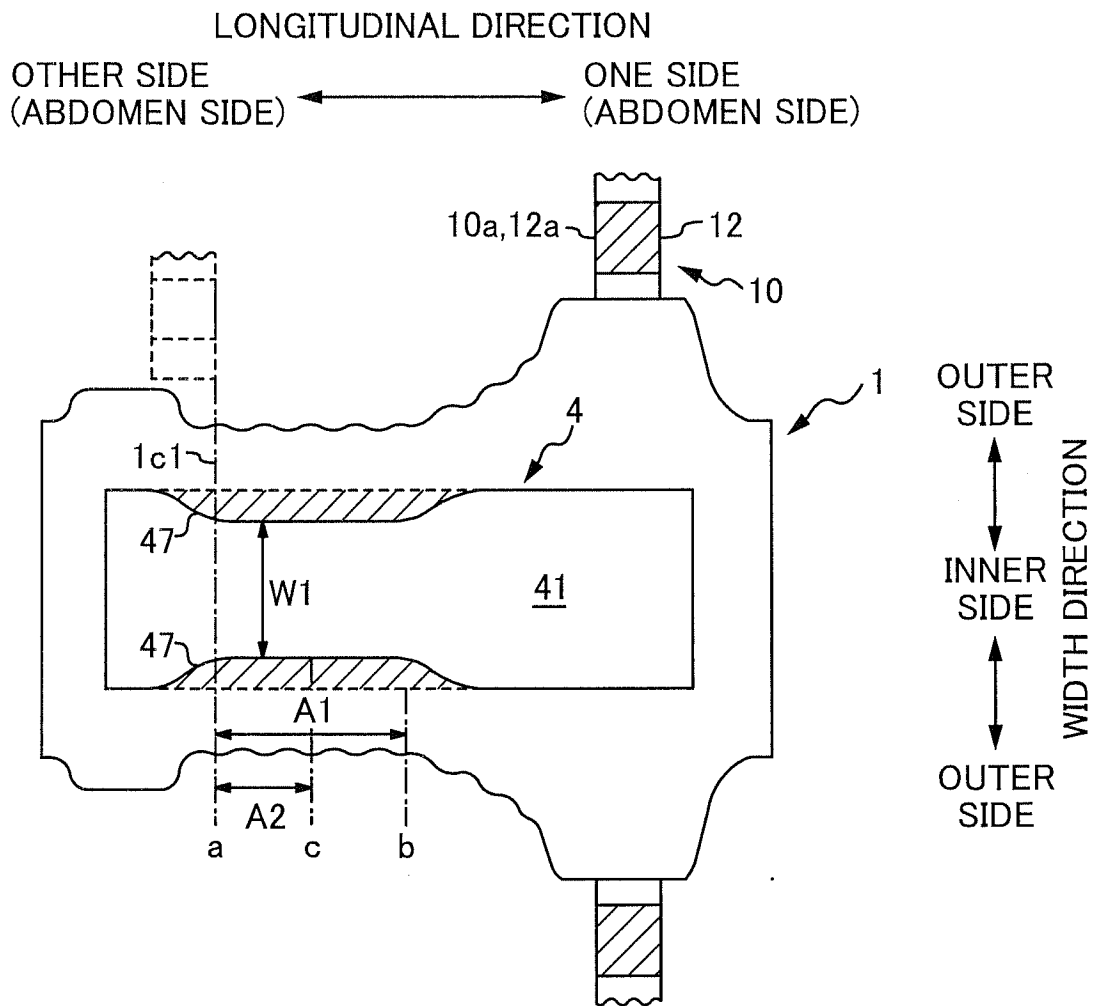


FIG. 9