

1/32

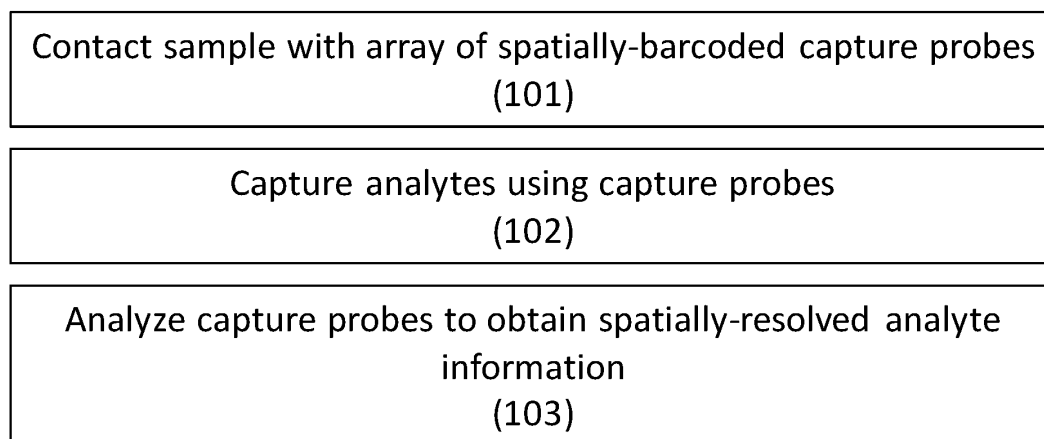


FIG. 1

2/32

Contact sample with array of spatially-barcoded capture probes
(201)

Optionally cleave capture probes from array and capture
analyte on/in sample
(202)

Analyze capture probes to obtain spatially-resolved information
about an analyte
(203)

FIG. 2

3/32

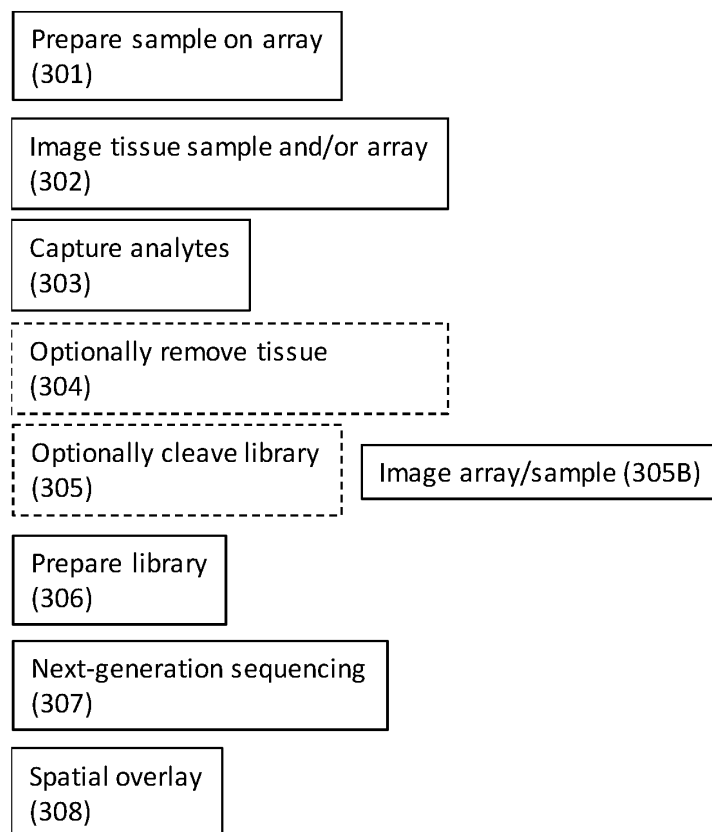


FIG. 3A

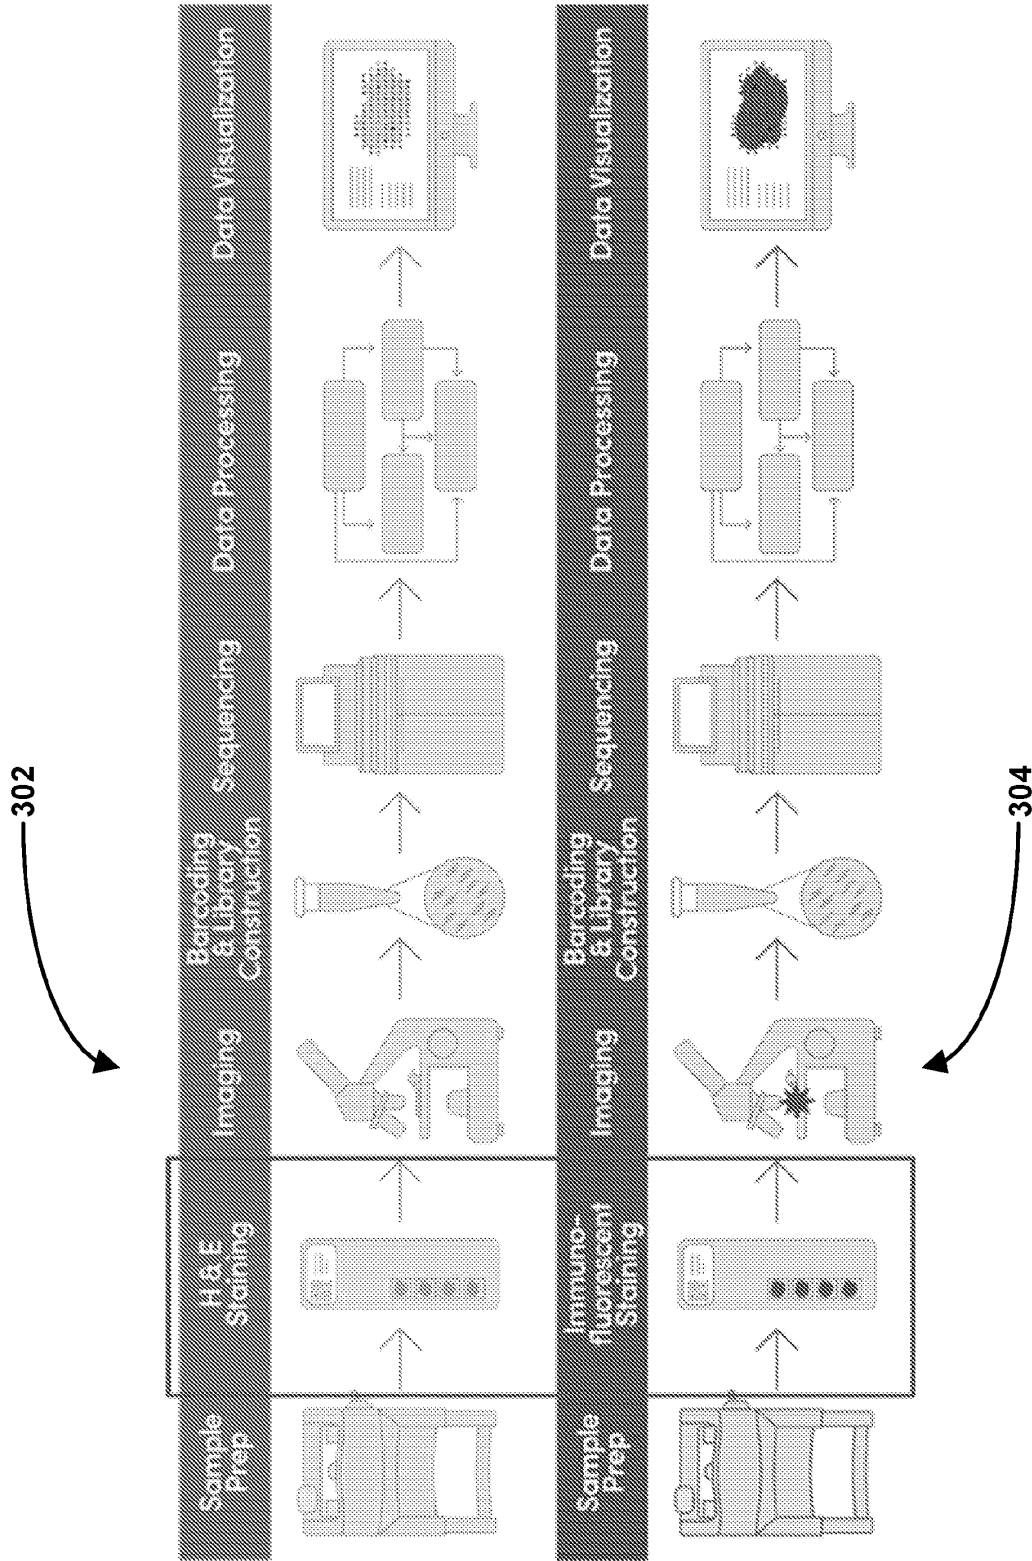


Fig. 3B

5/32

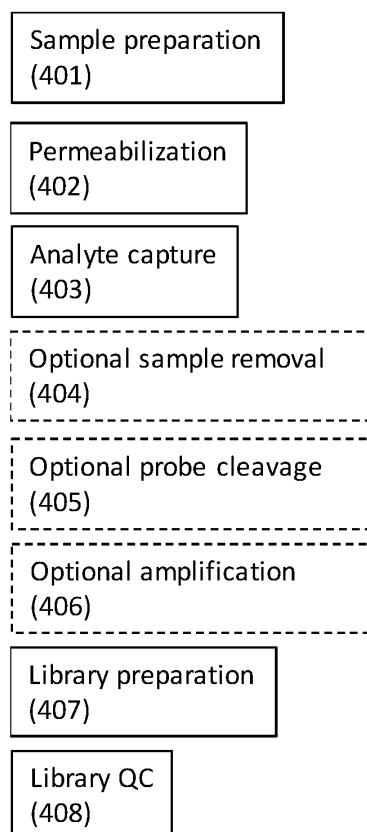


FIG. 4

6/32

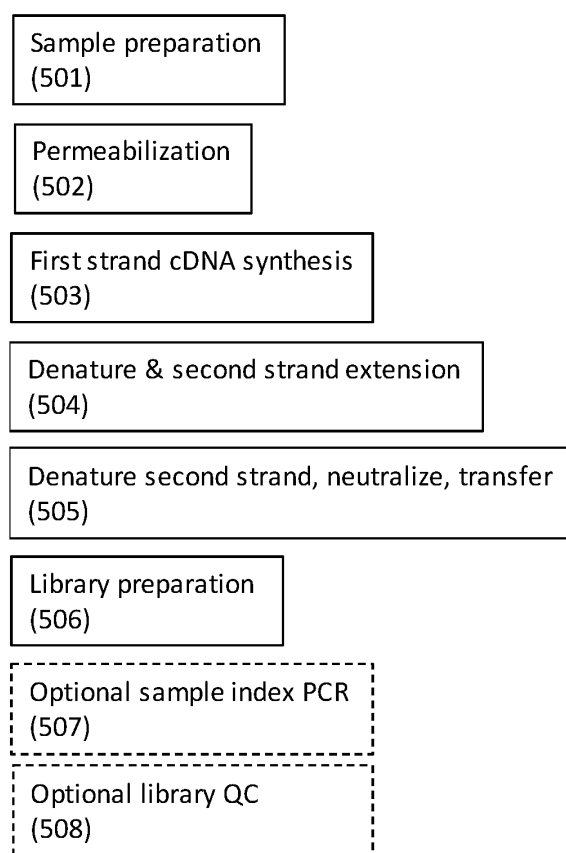


FIG. 5

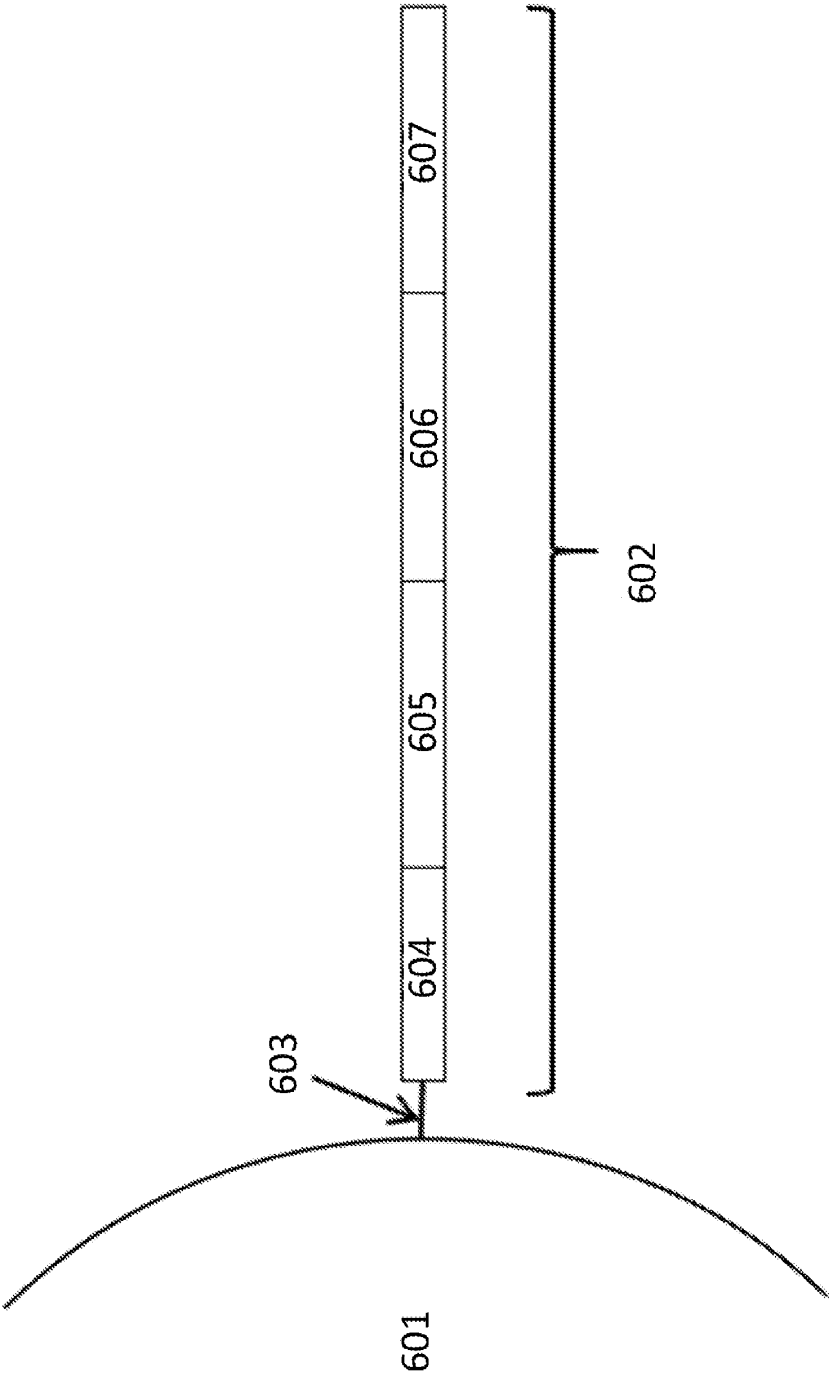


FIG. 6

8/32

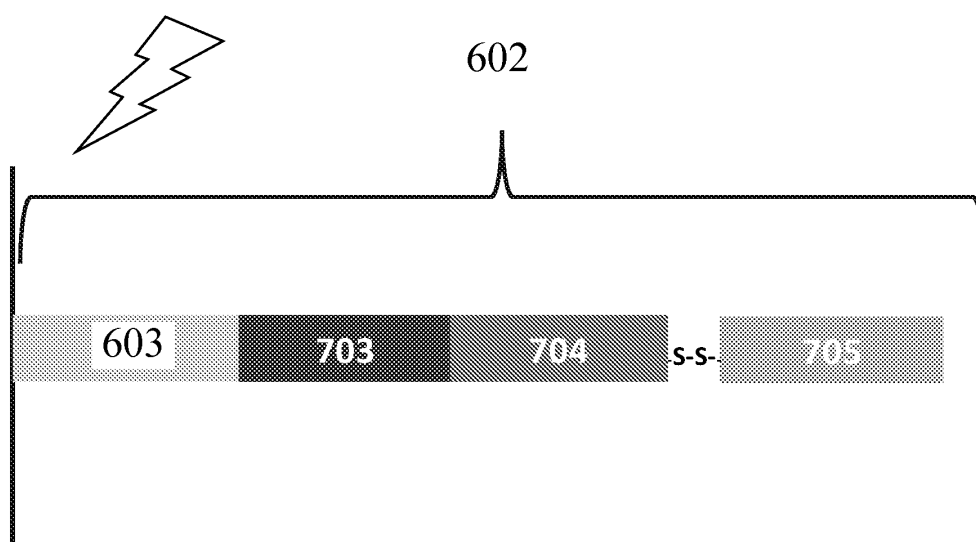


FIG. 7

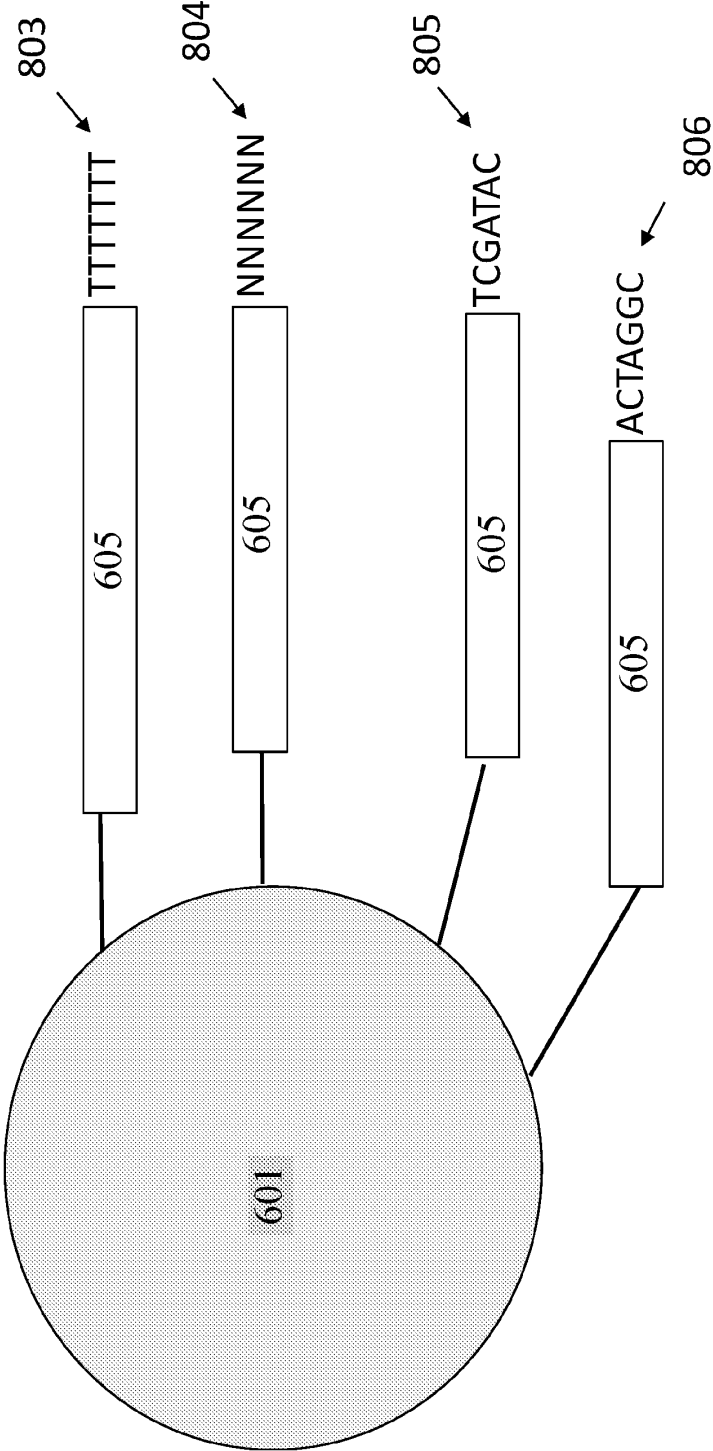


FIG. 8

10/32

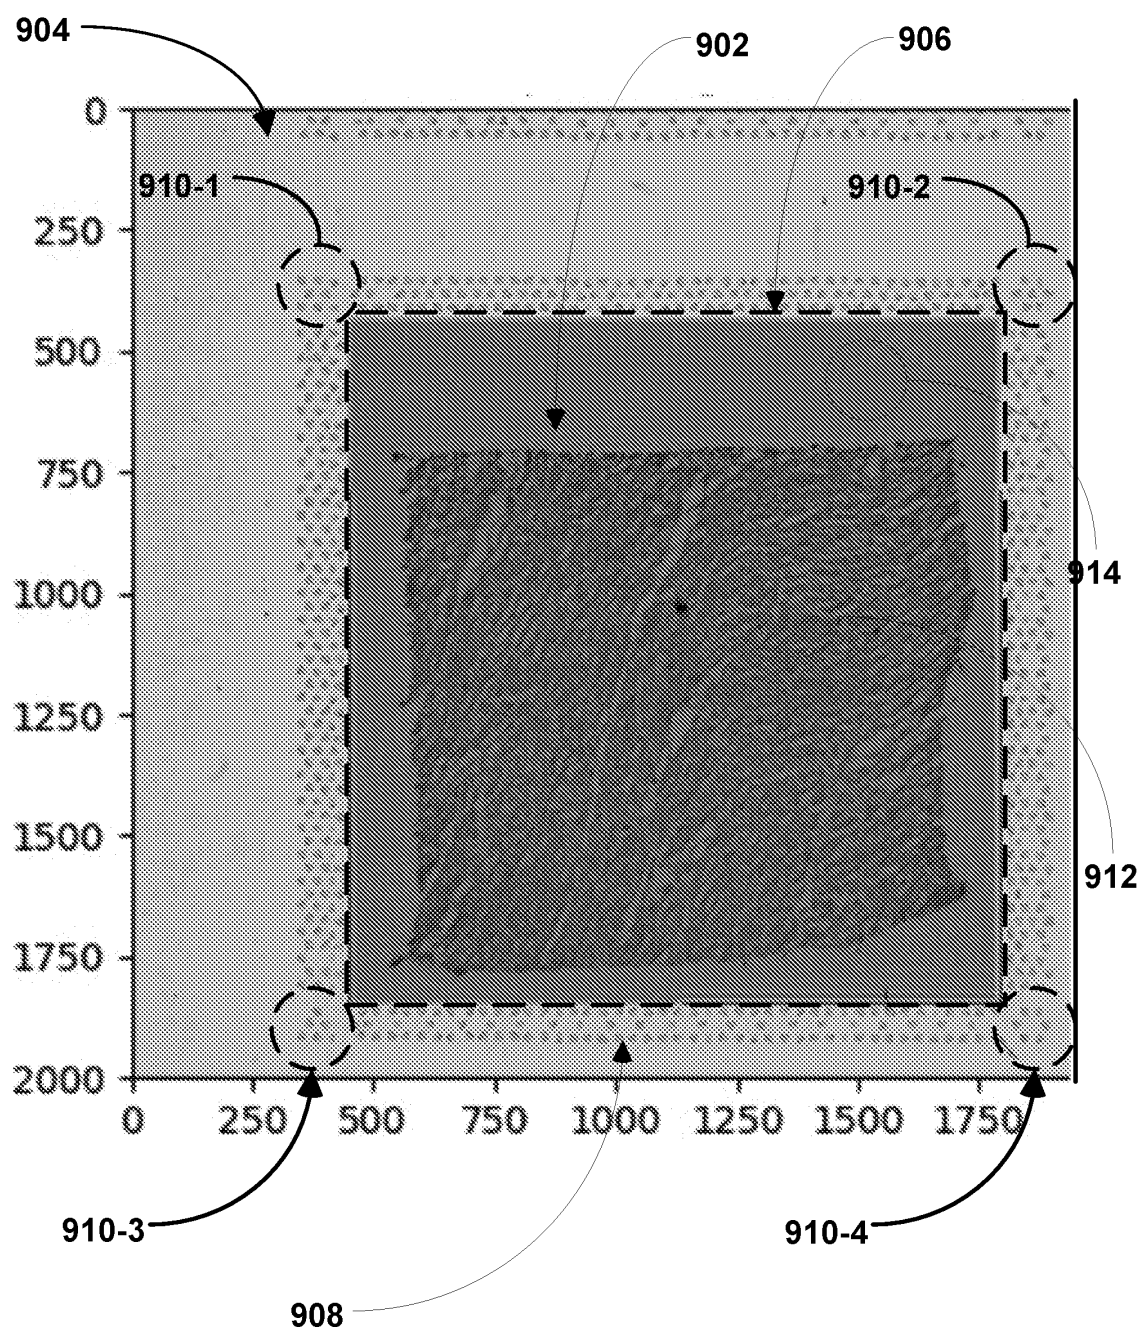


FIG. 9A

11/32

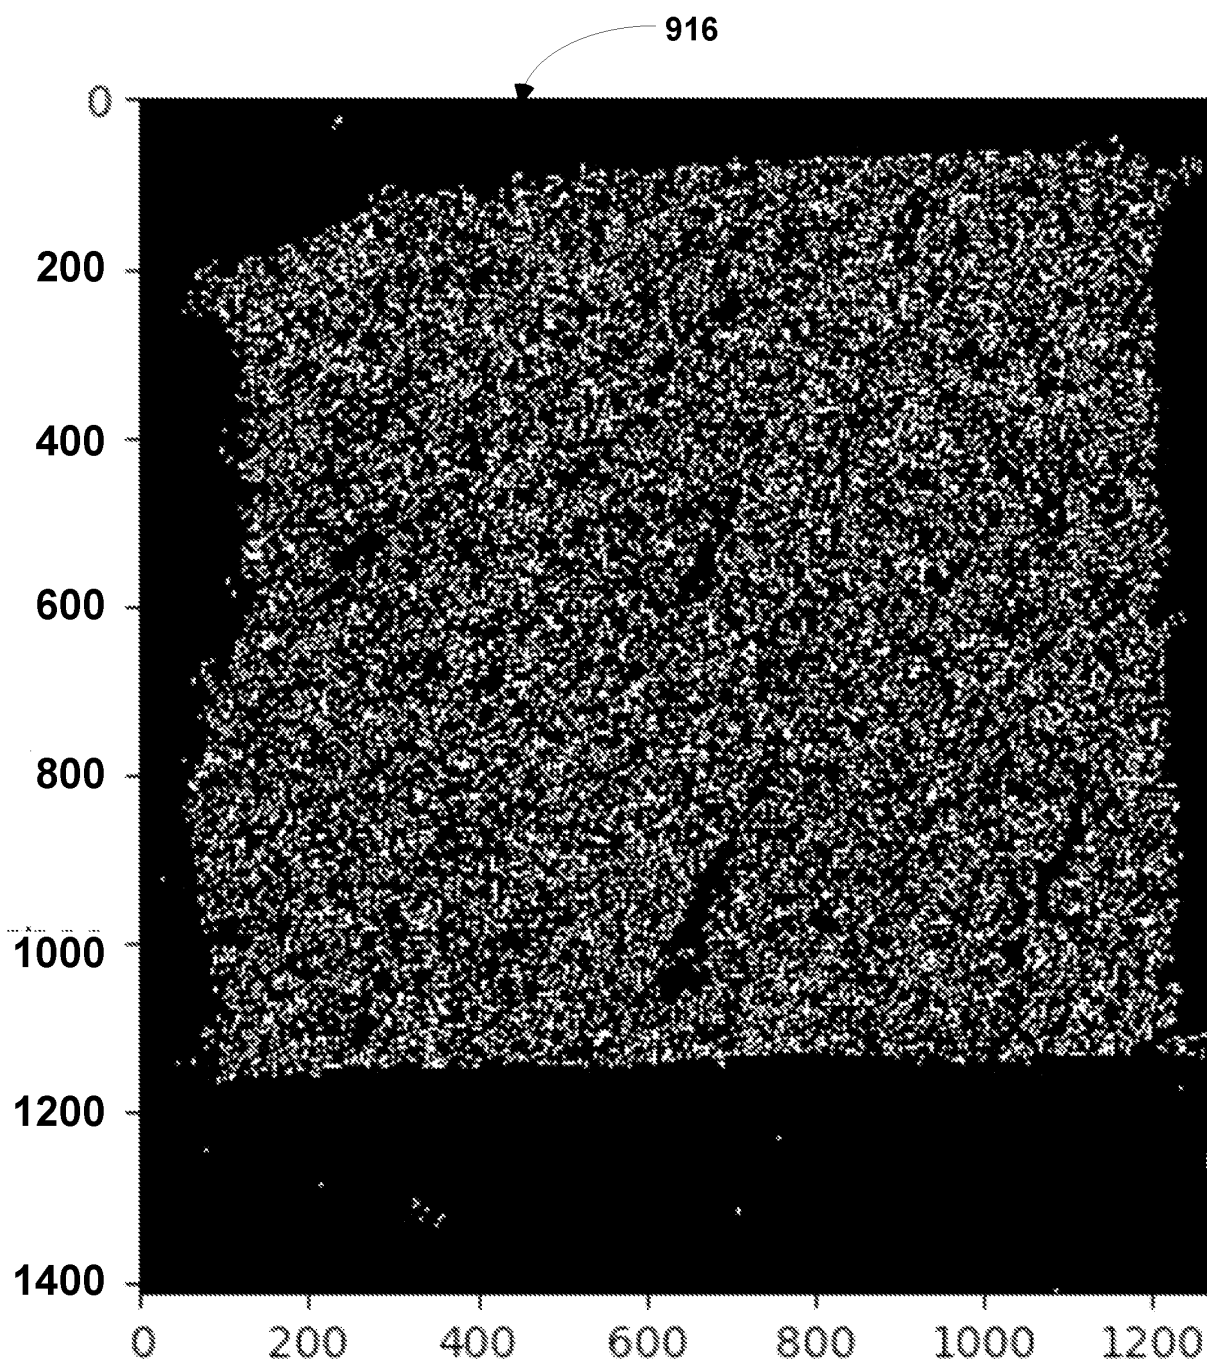


FIG. 9B

12/32

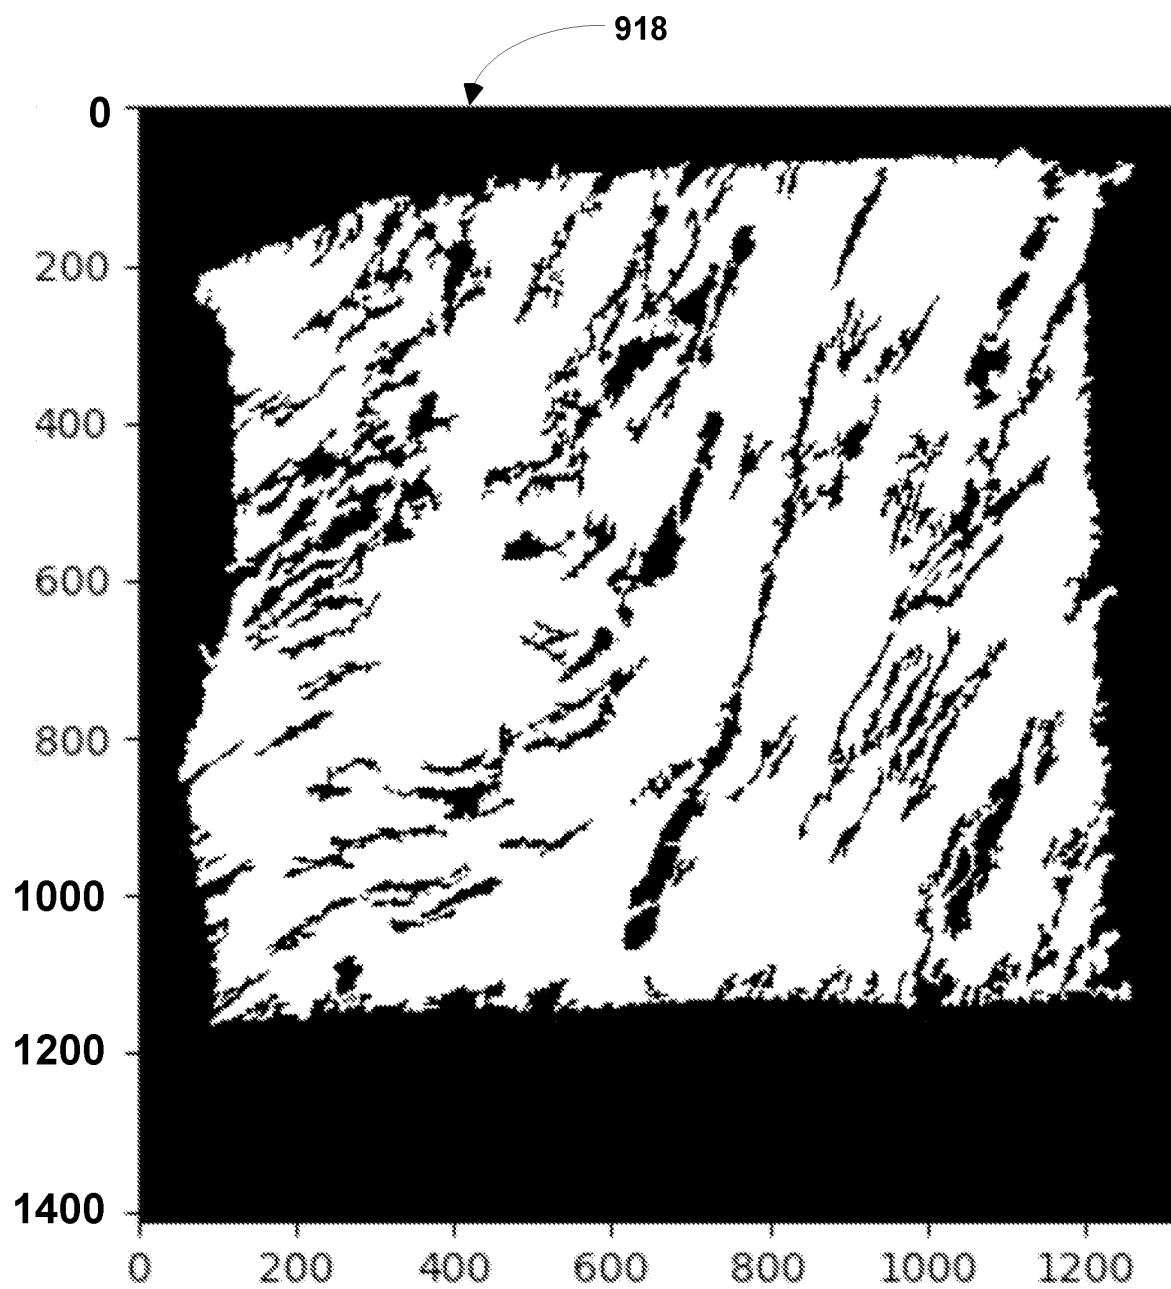


FIG. 9C

13/32

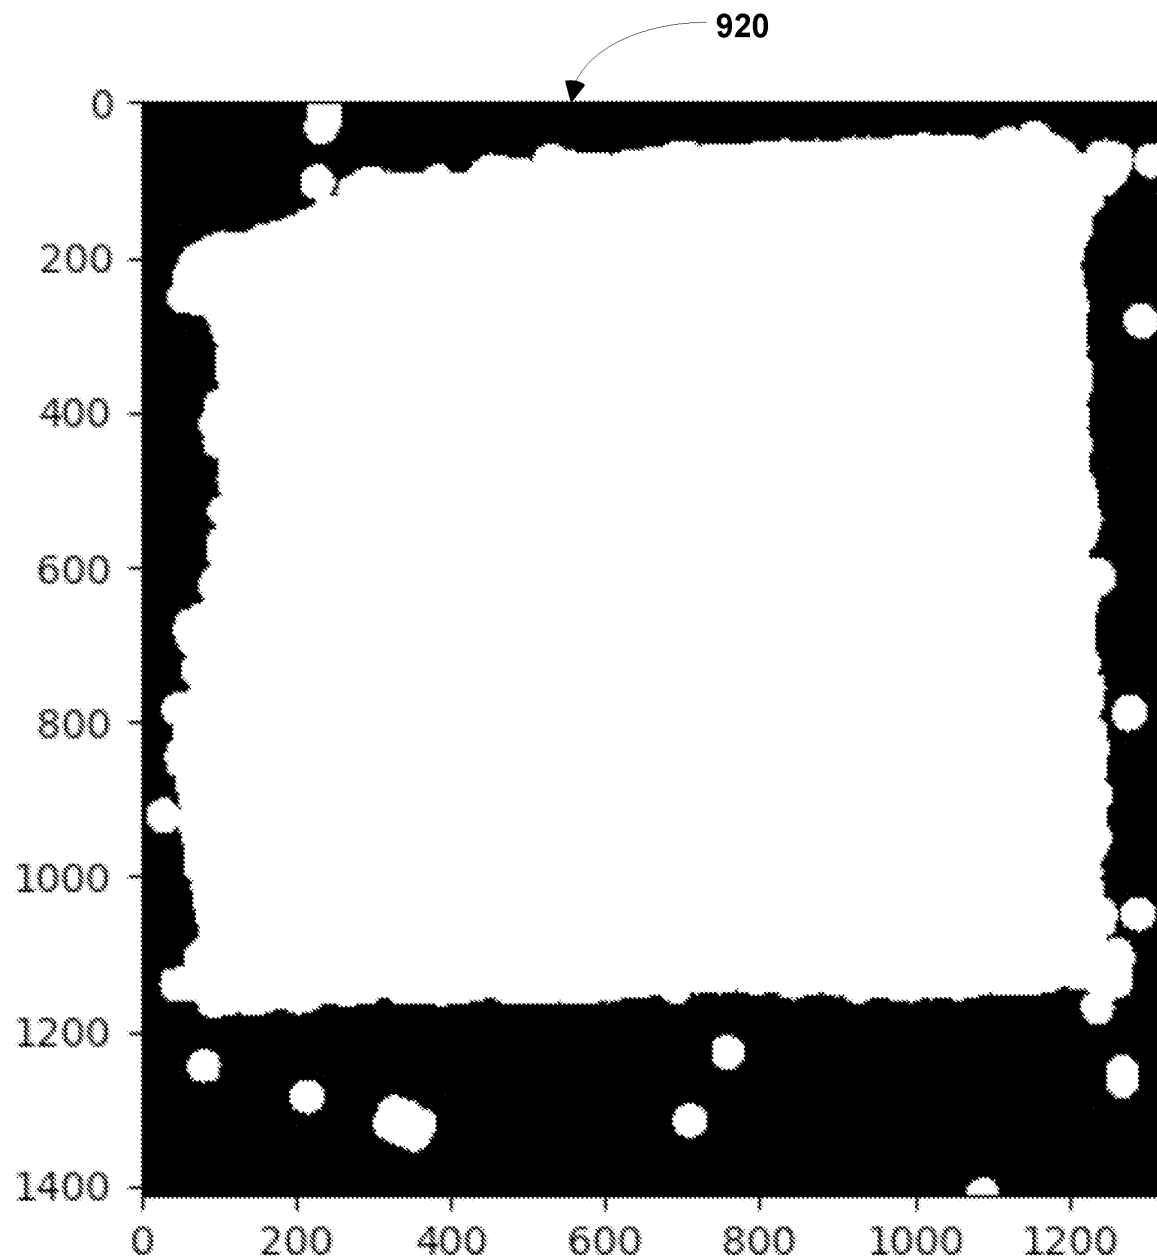


FIG. 9D

14/32

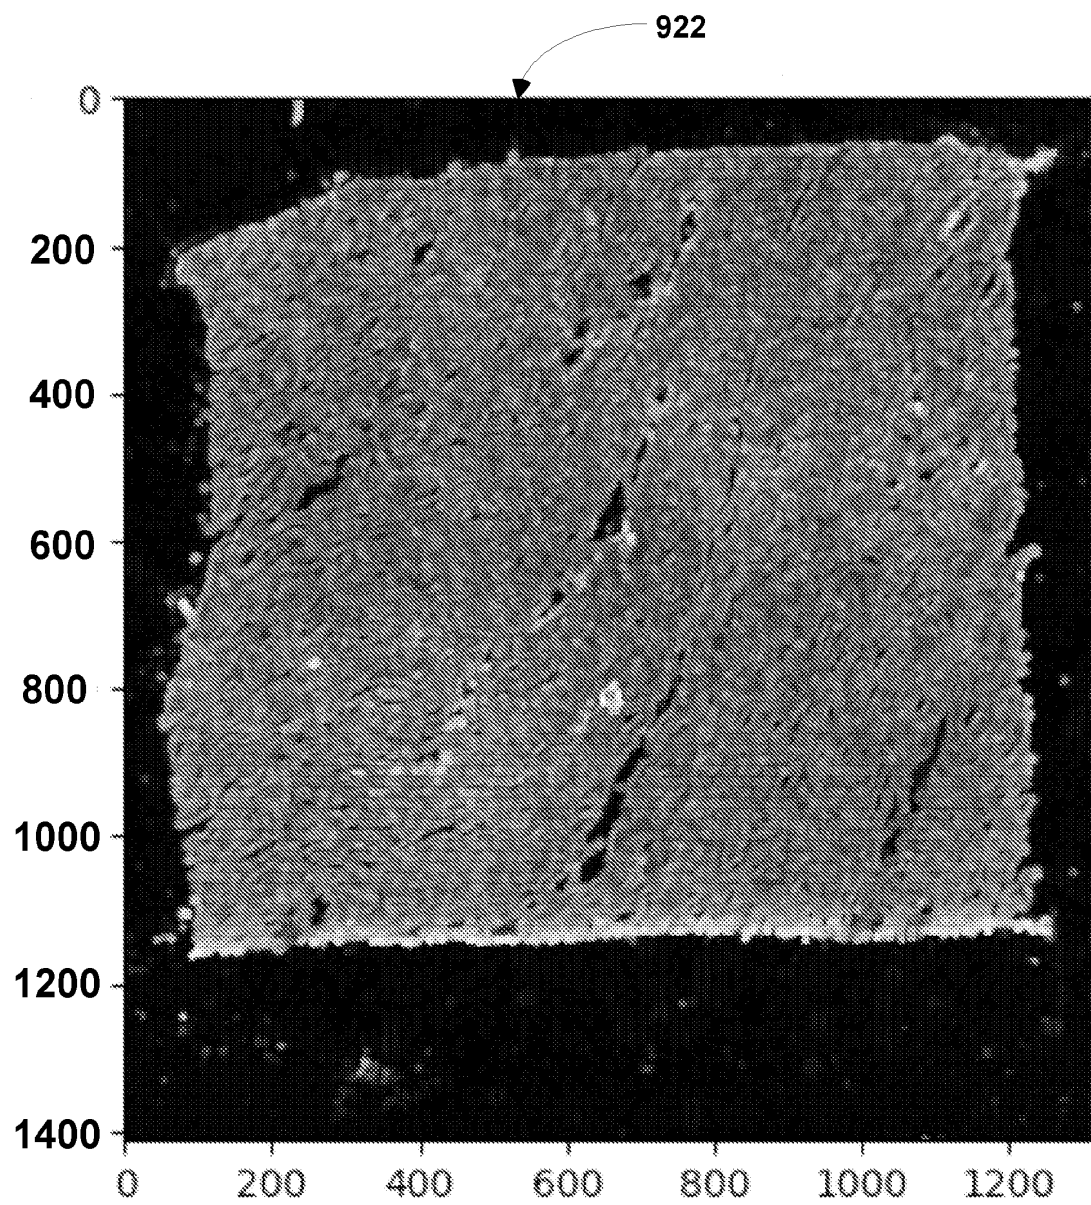


FIG. 9E

15/32

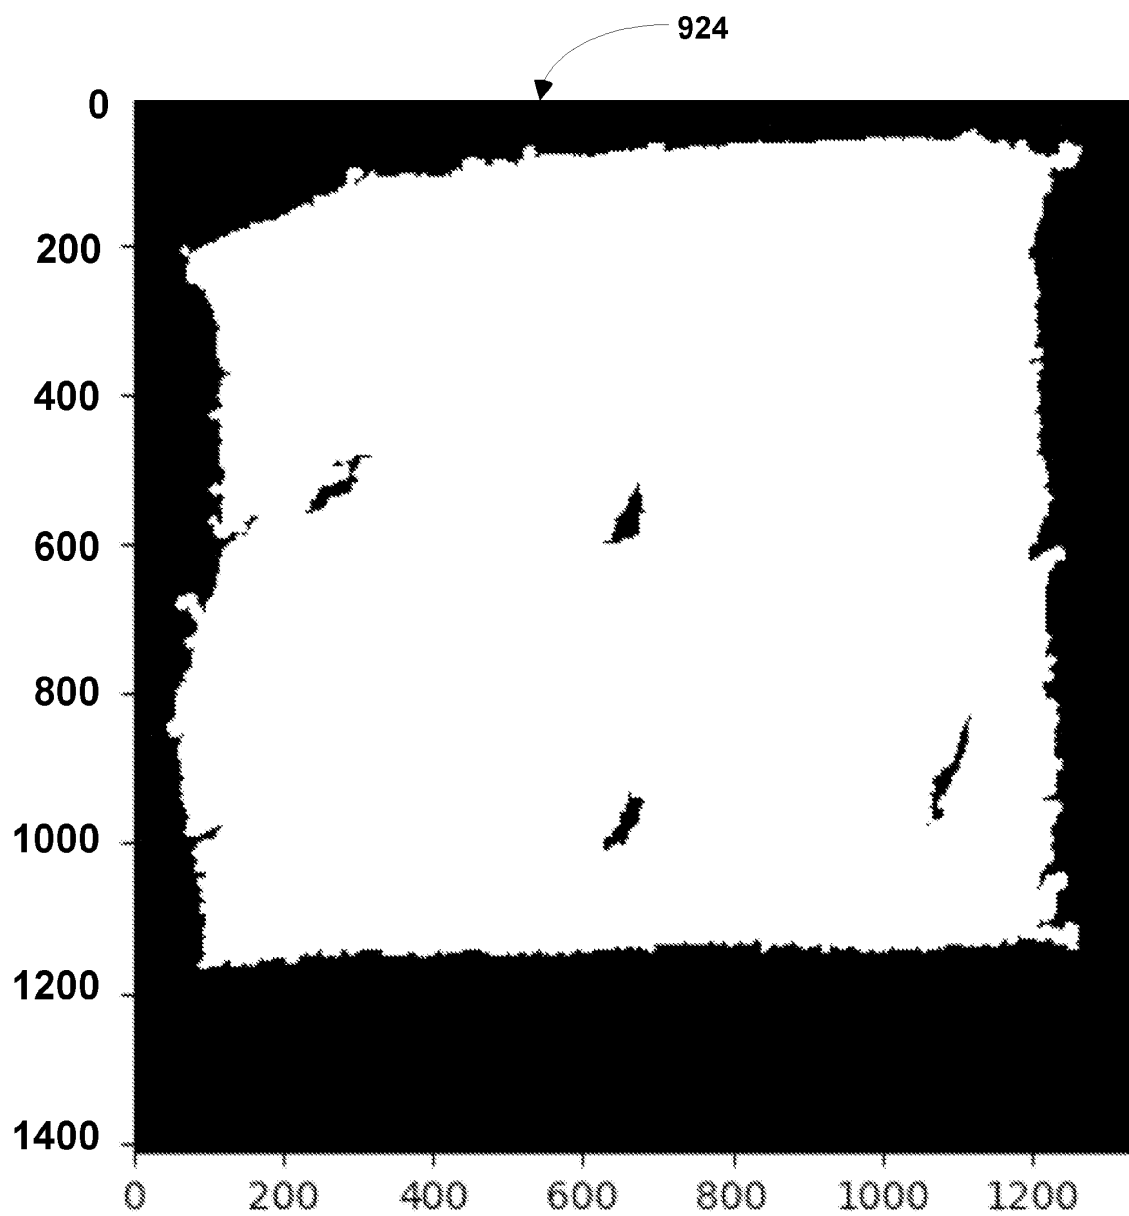


FIG. 9F

16/32

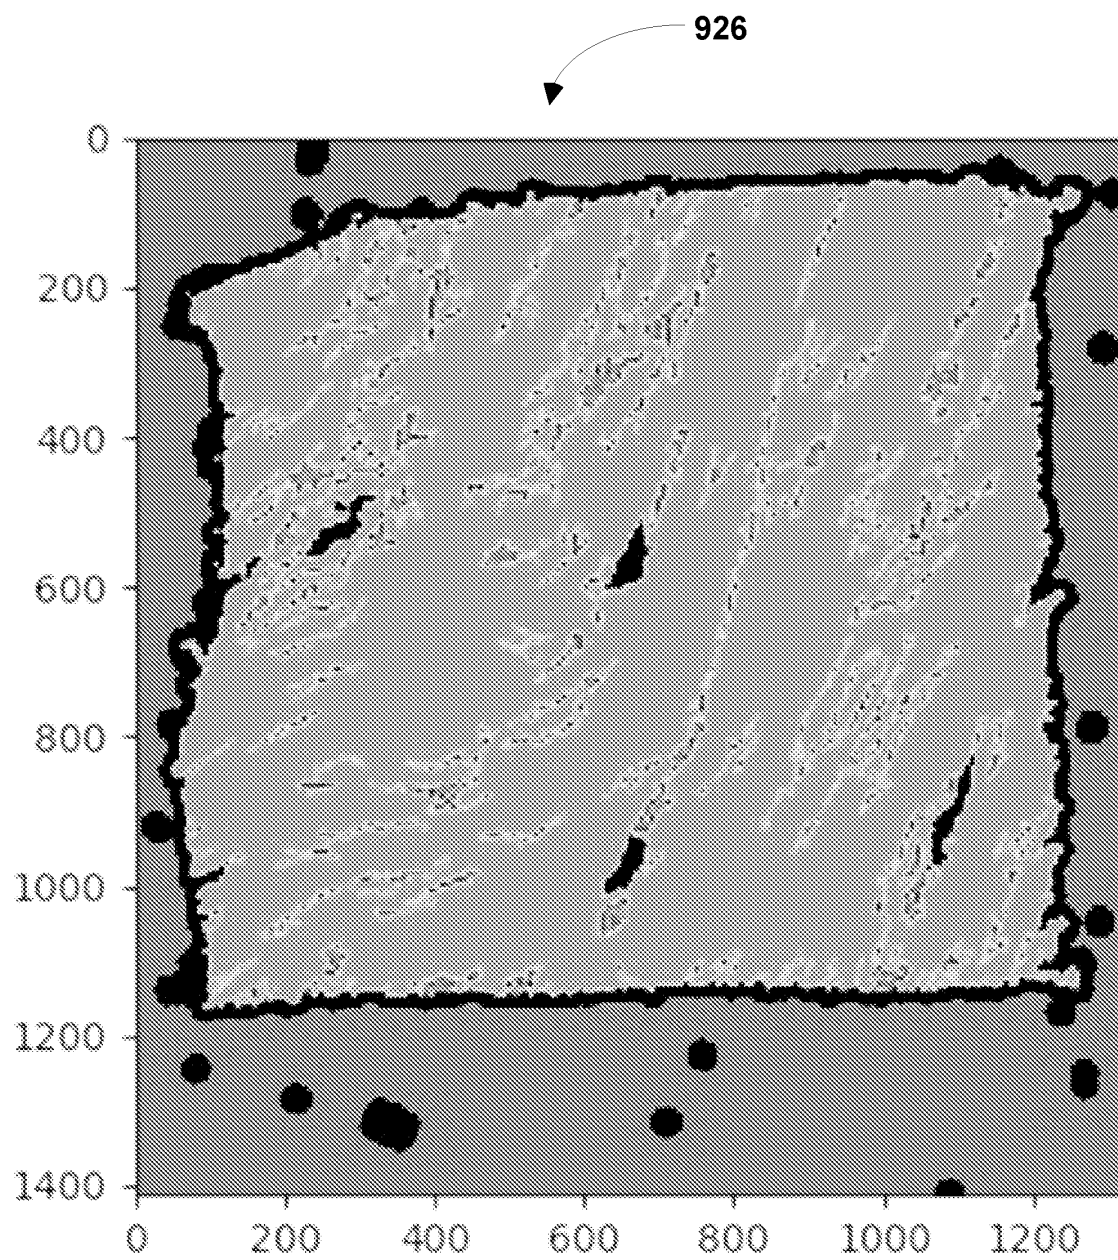


FIG. 9G

17/32

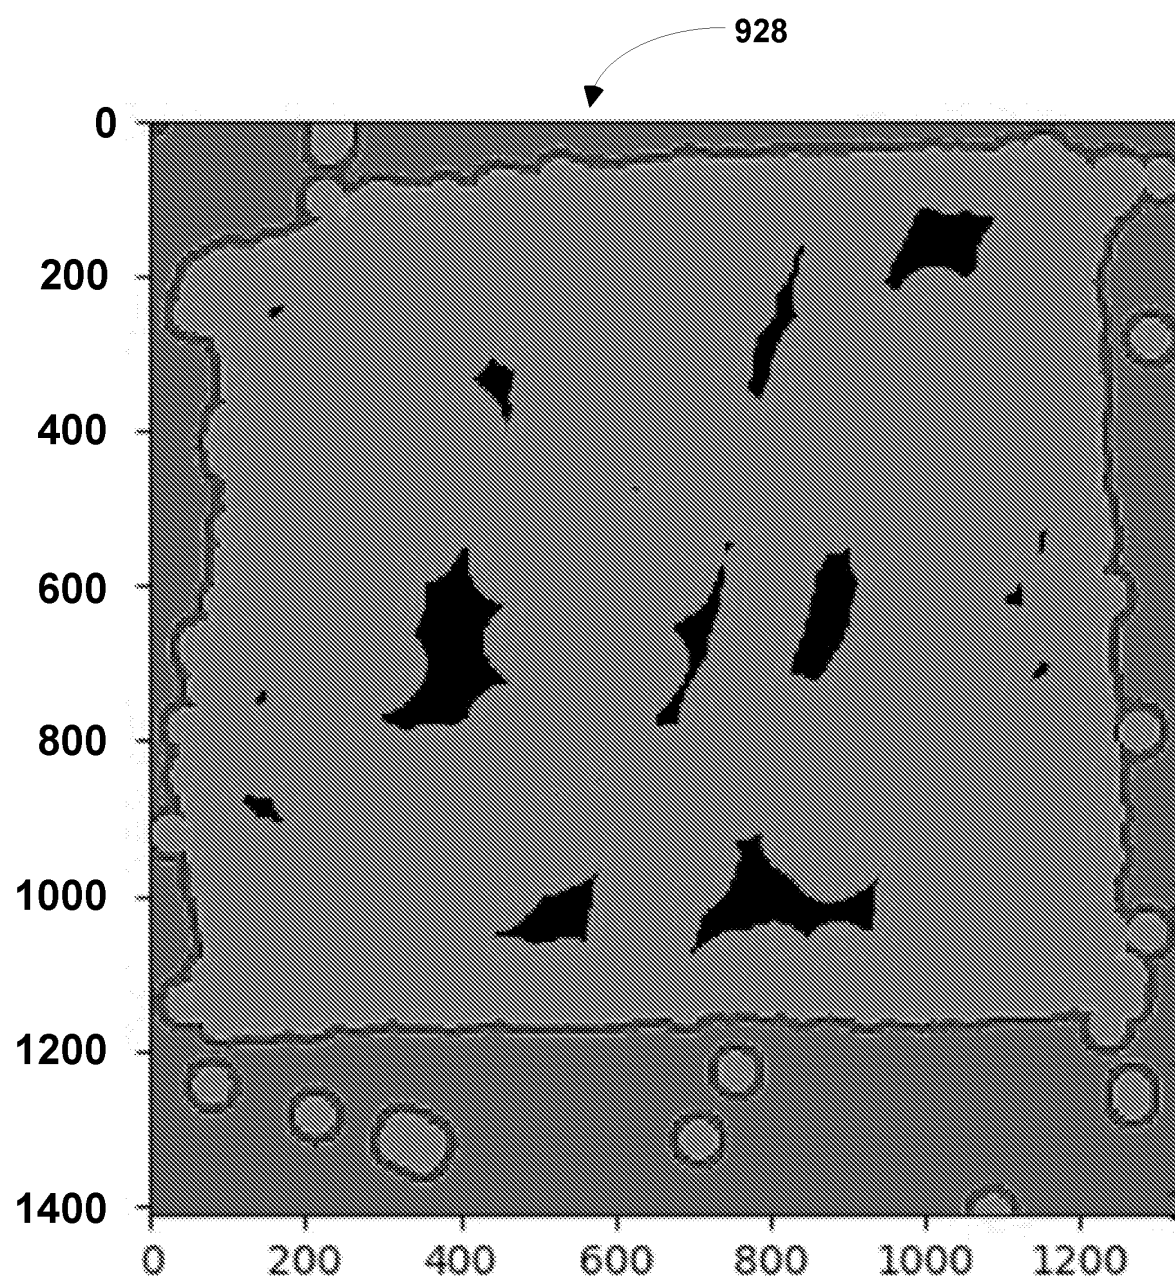


FIG. 9H

18/32

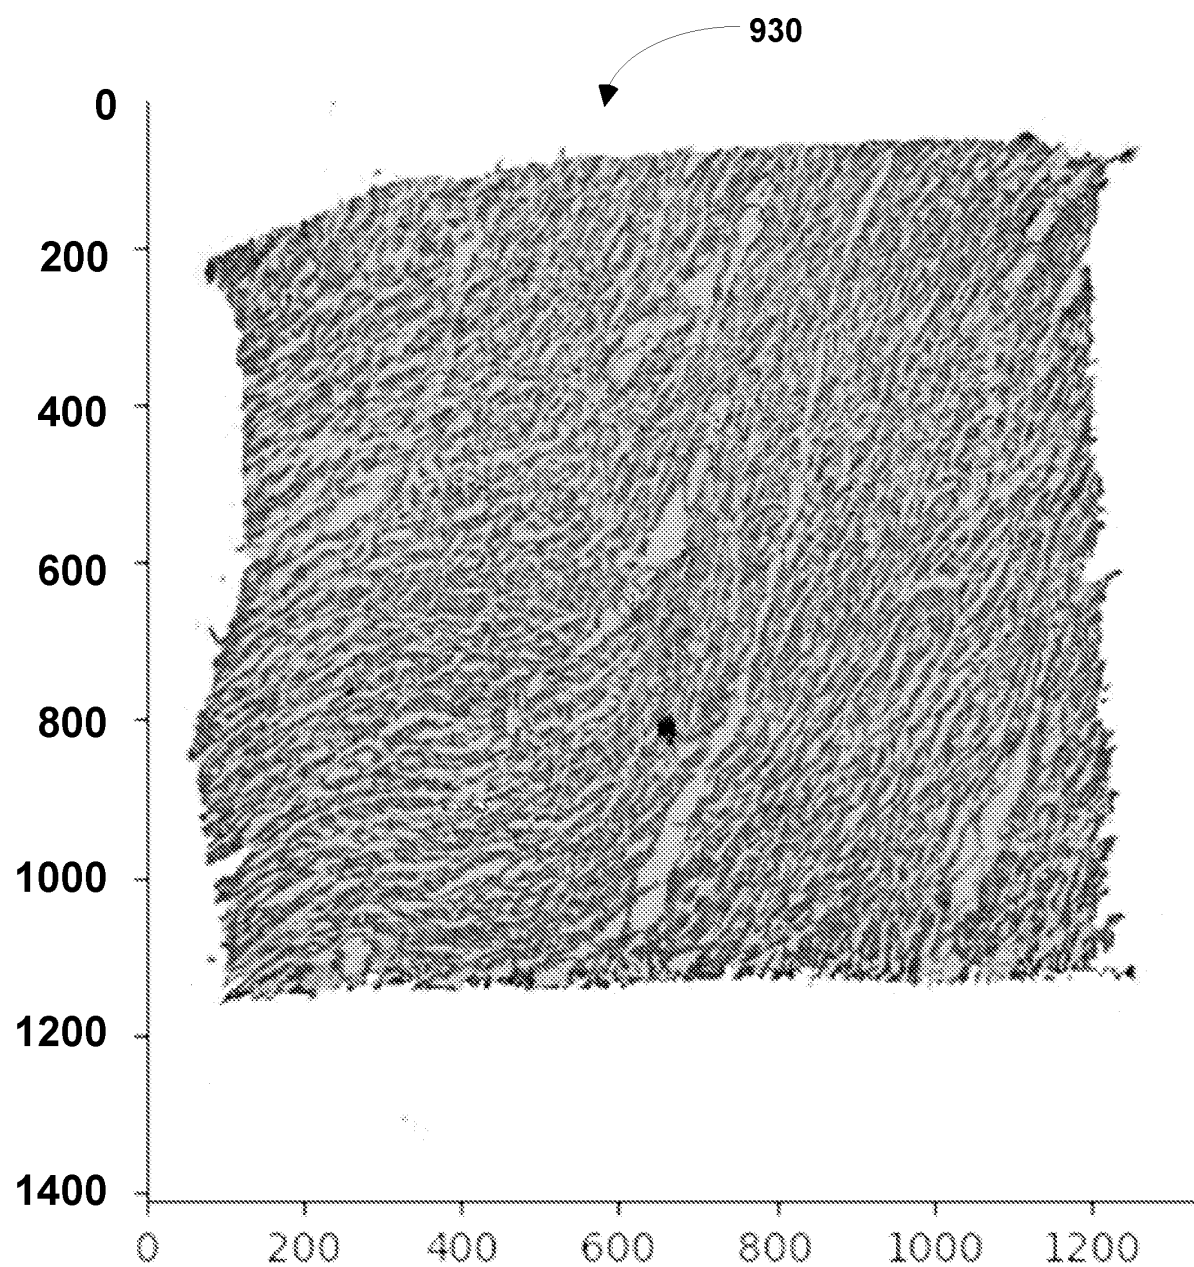


FIG. 9I

19/32

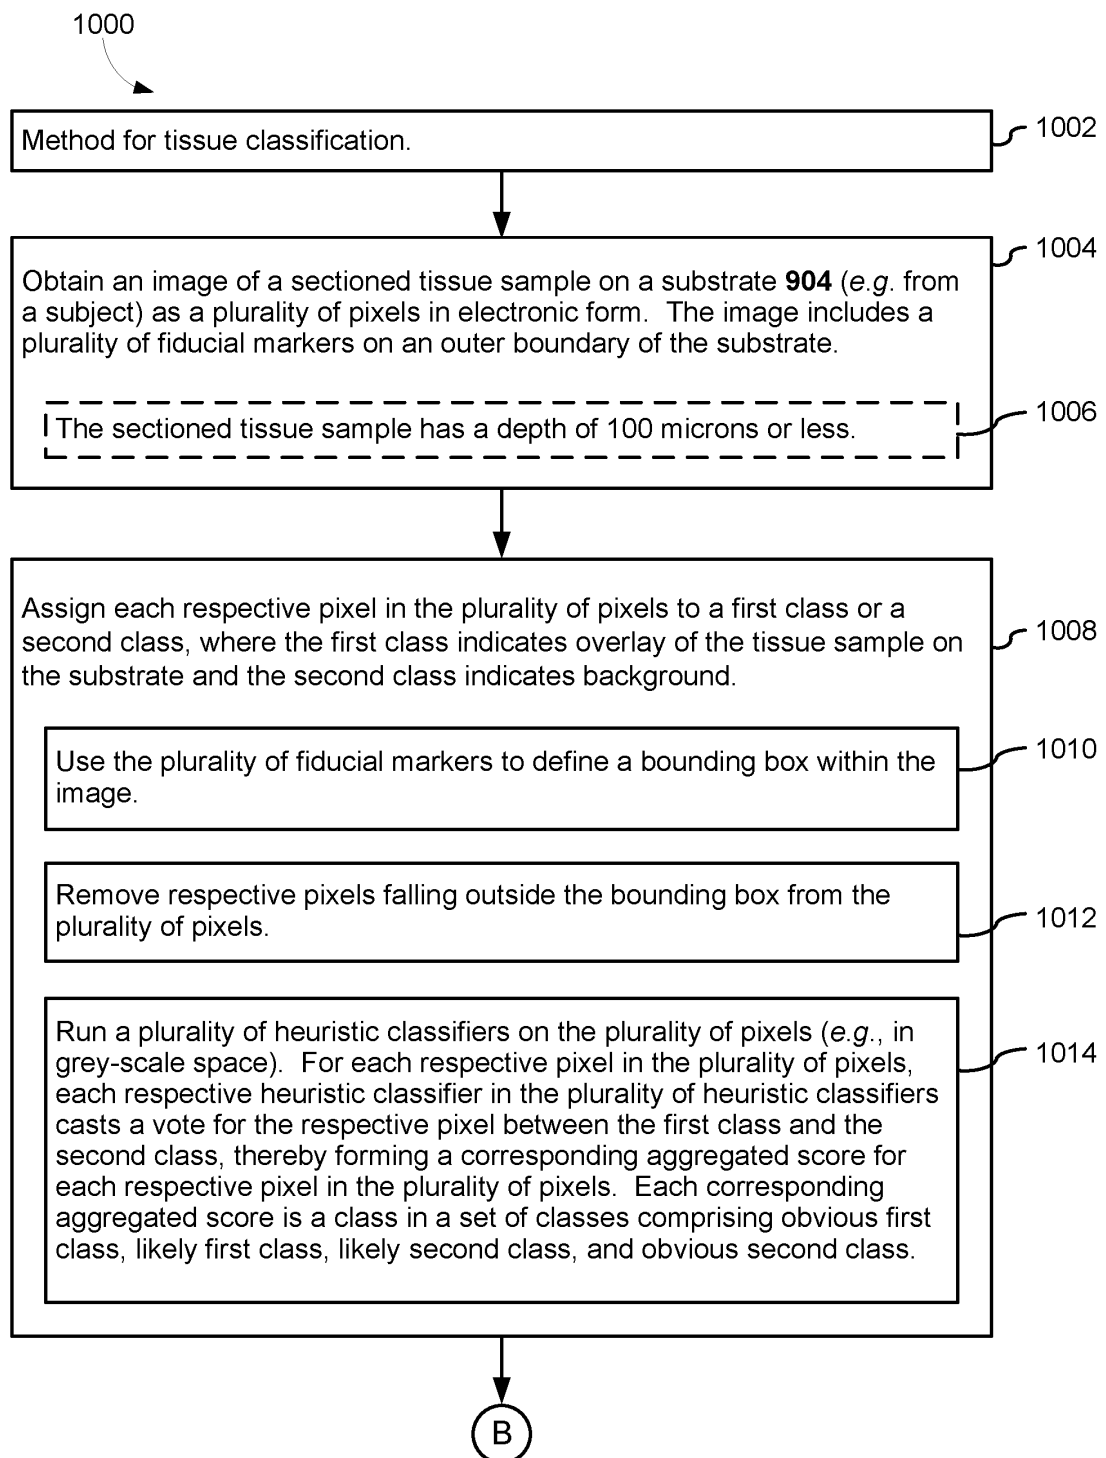


FIG. 10A

20/32

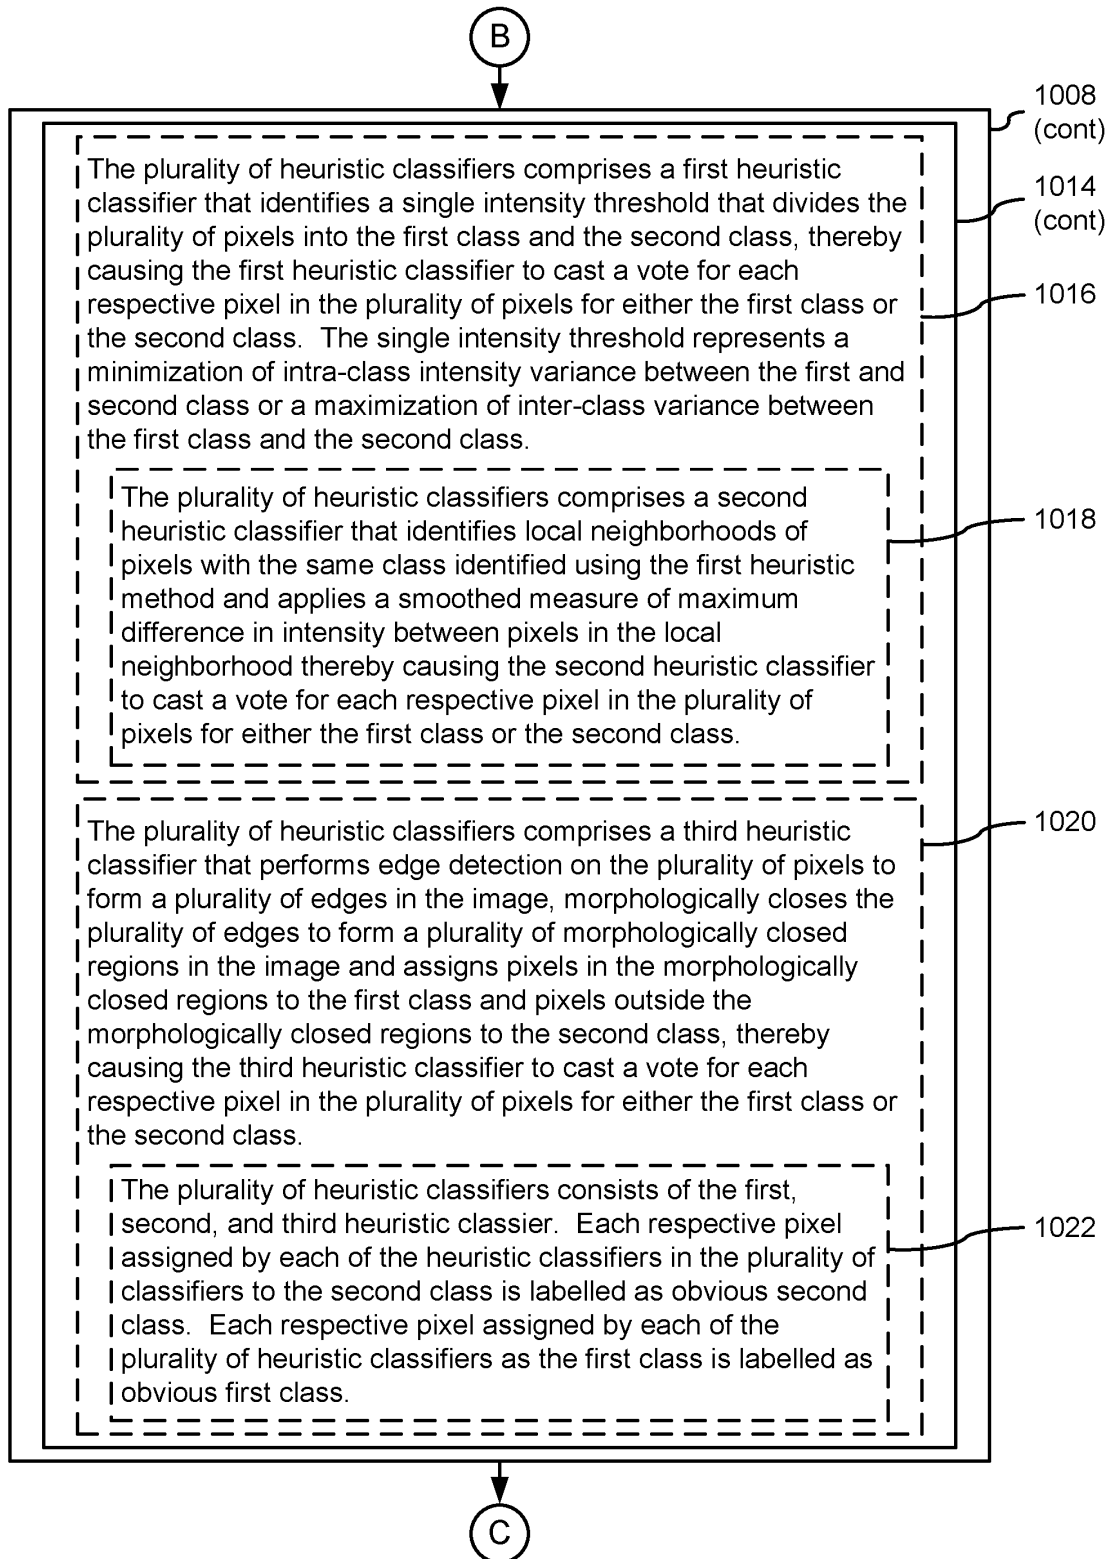


FIG. 10B

21/32

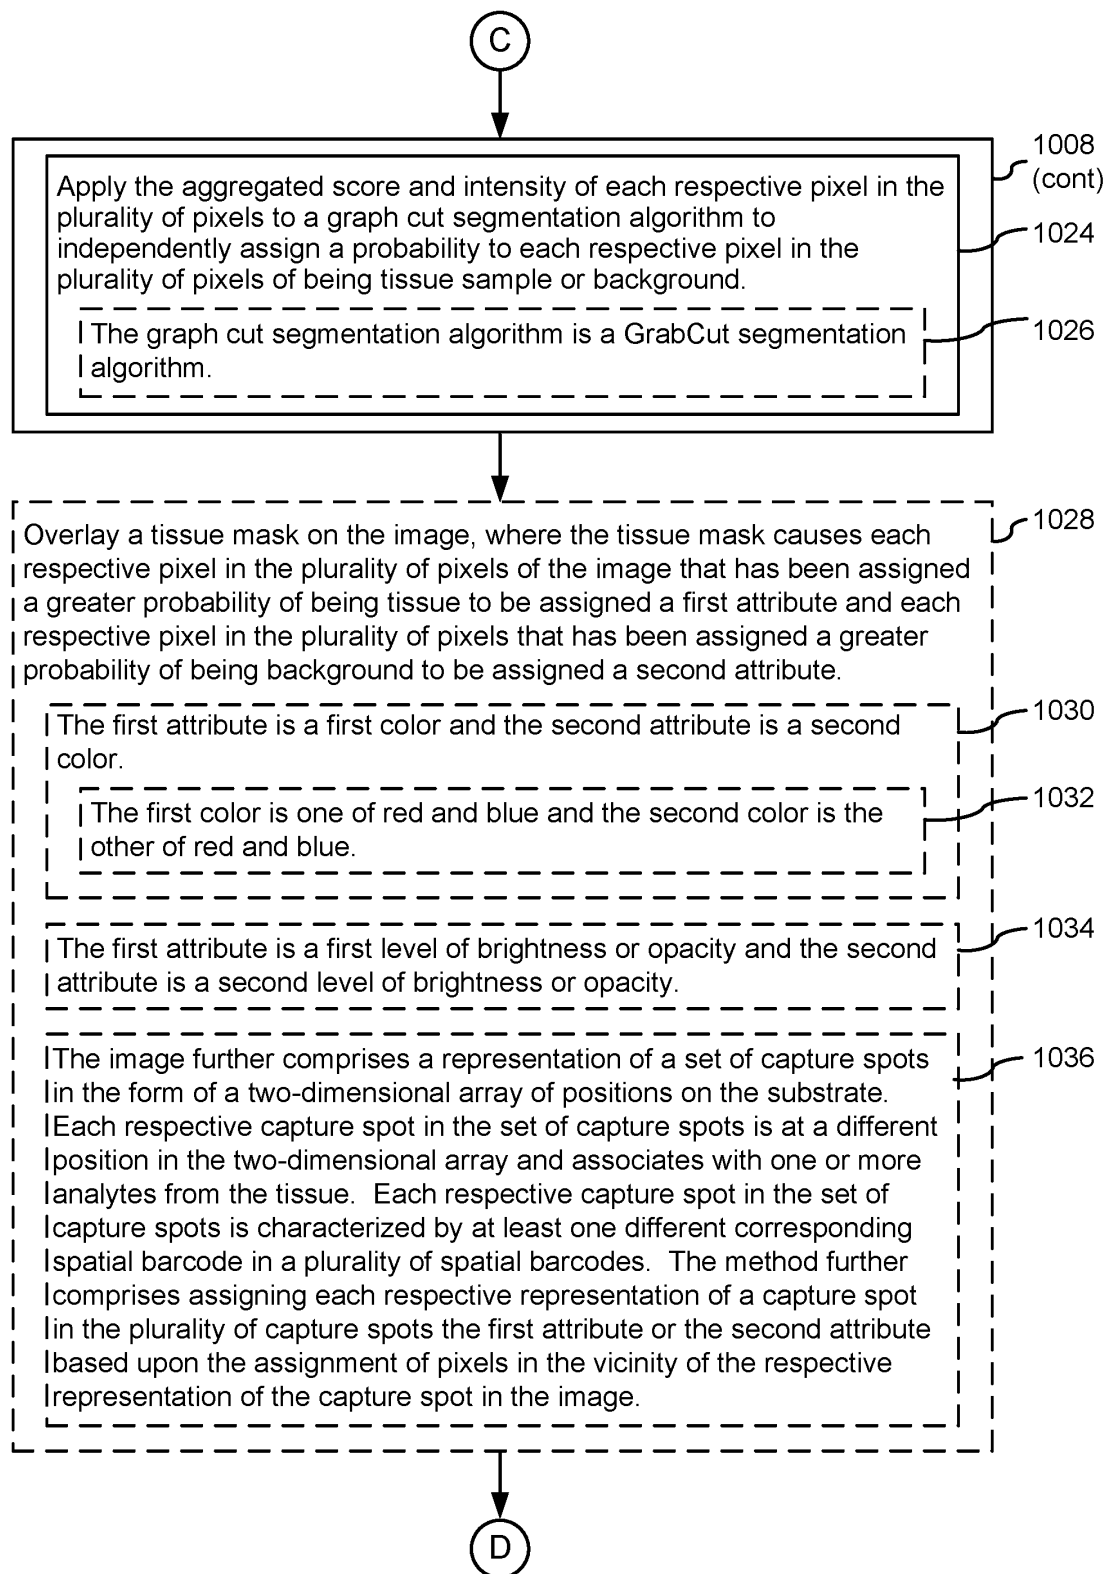


FIG. 10C

22/32

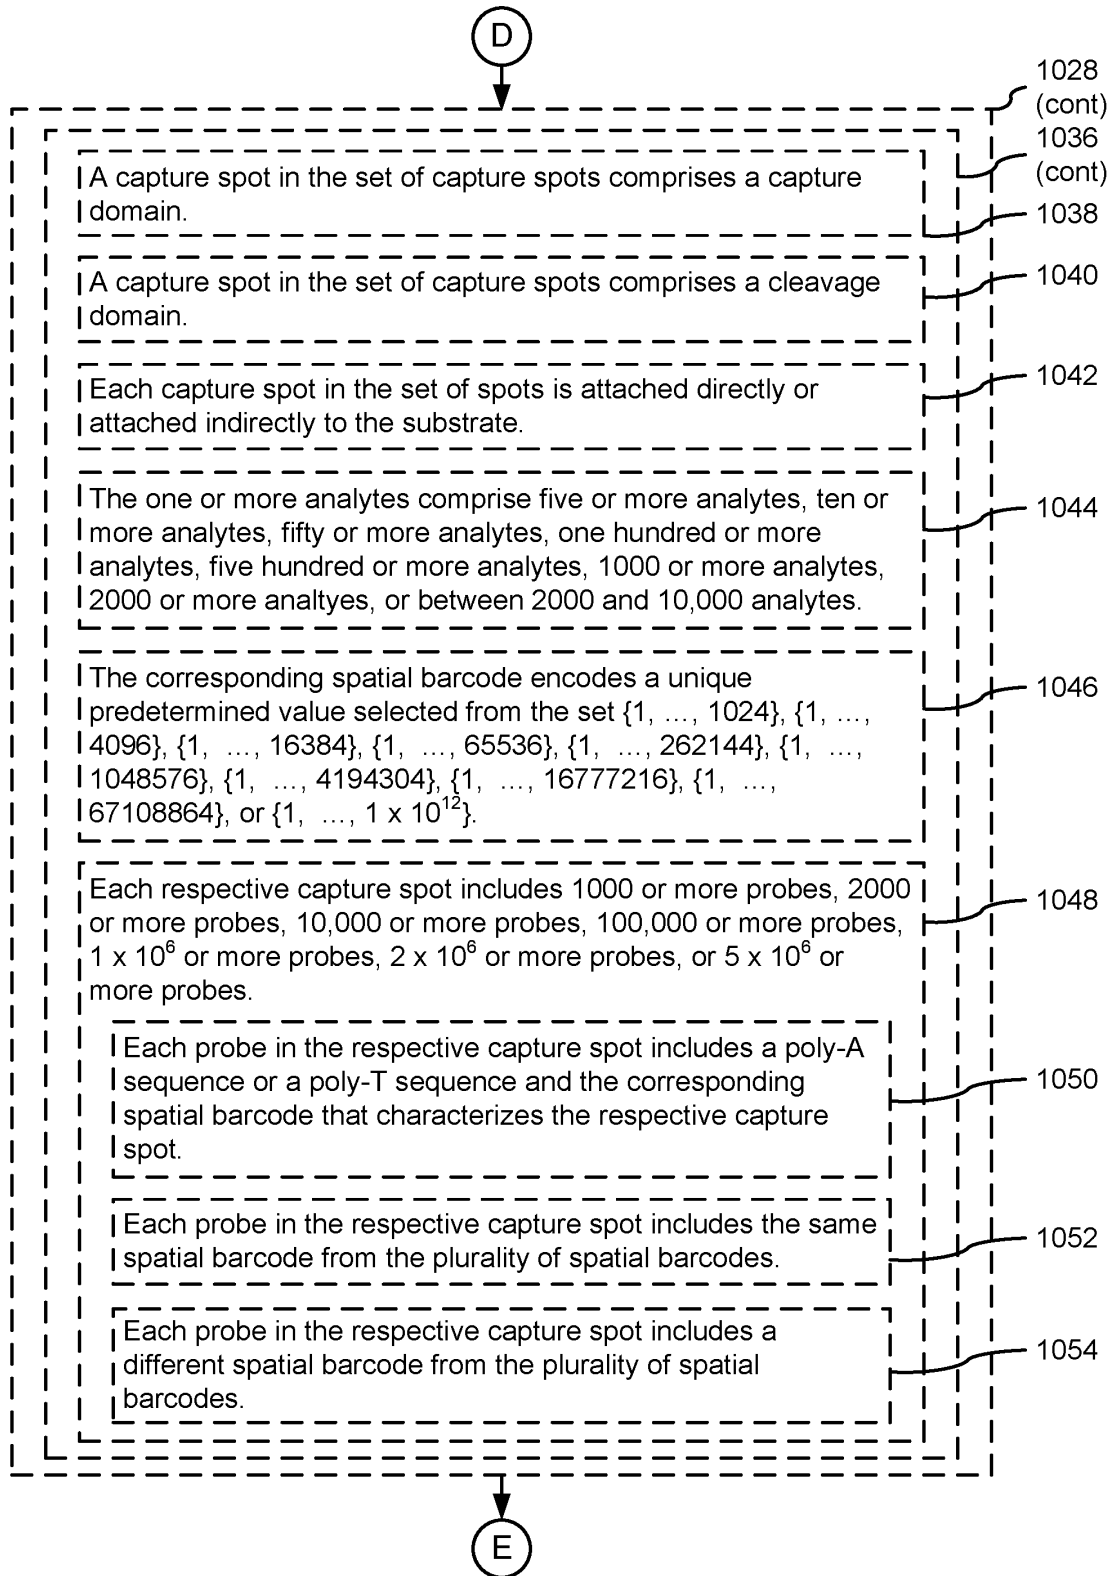


FIG. 10D

23/32

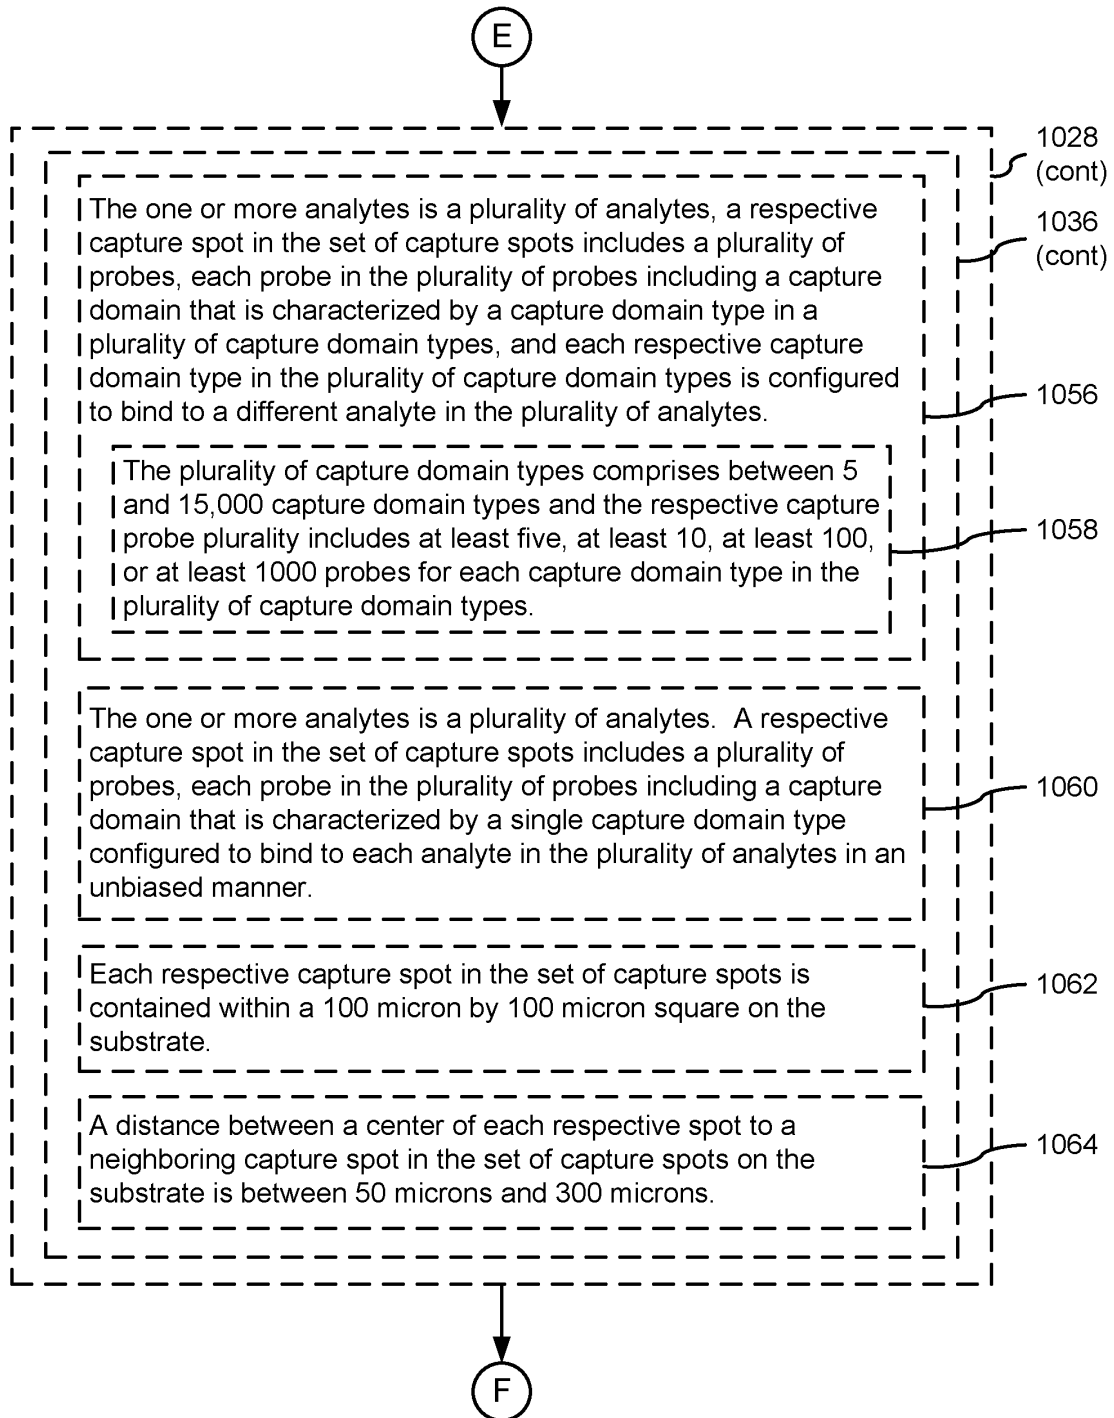


FIG. 10E

24/32

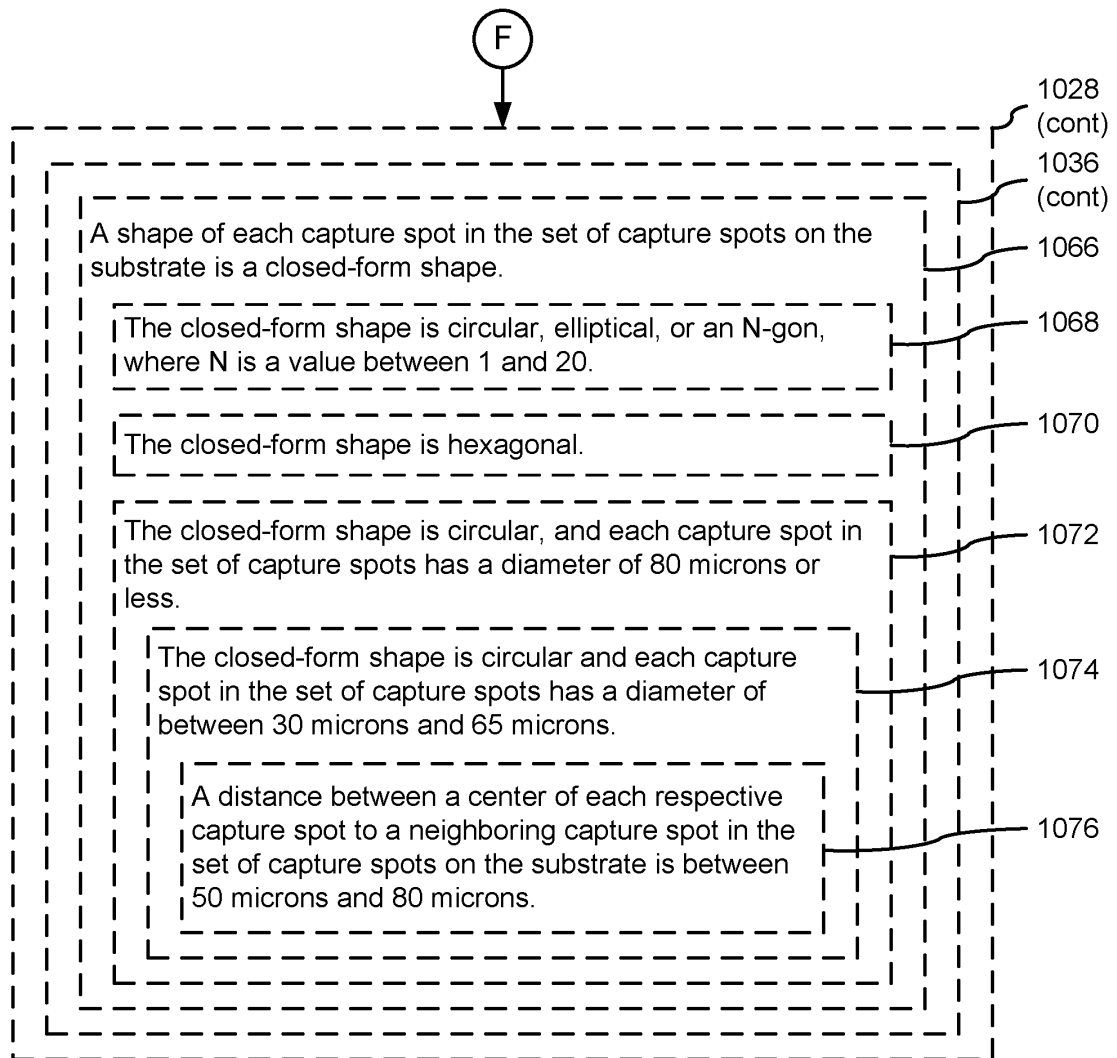


FIG. 10F

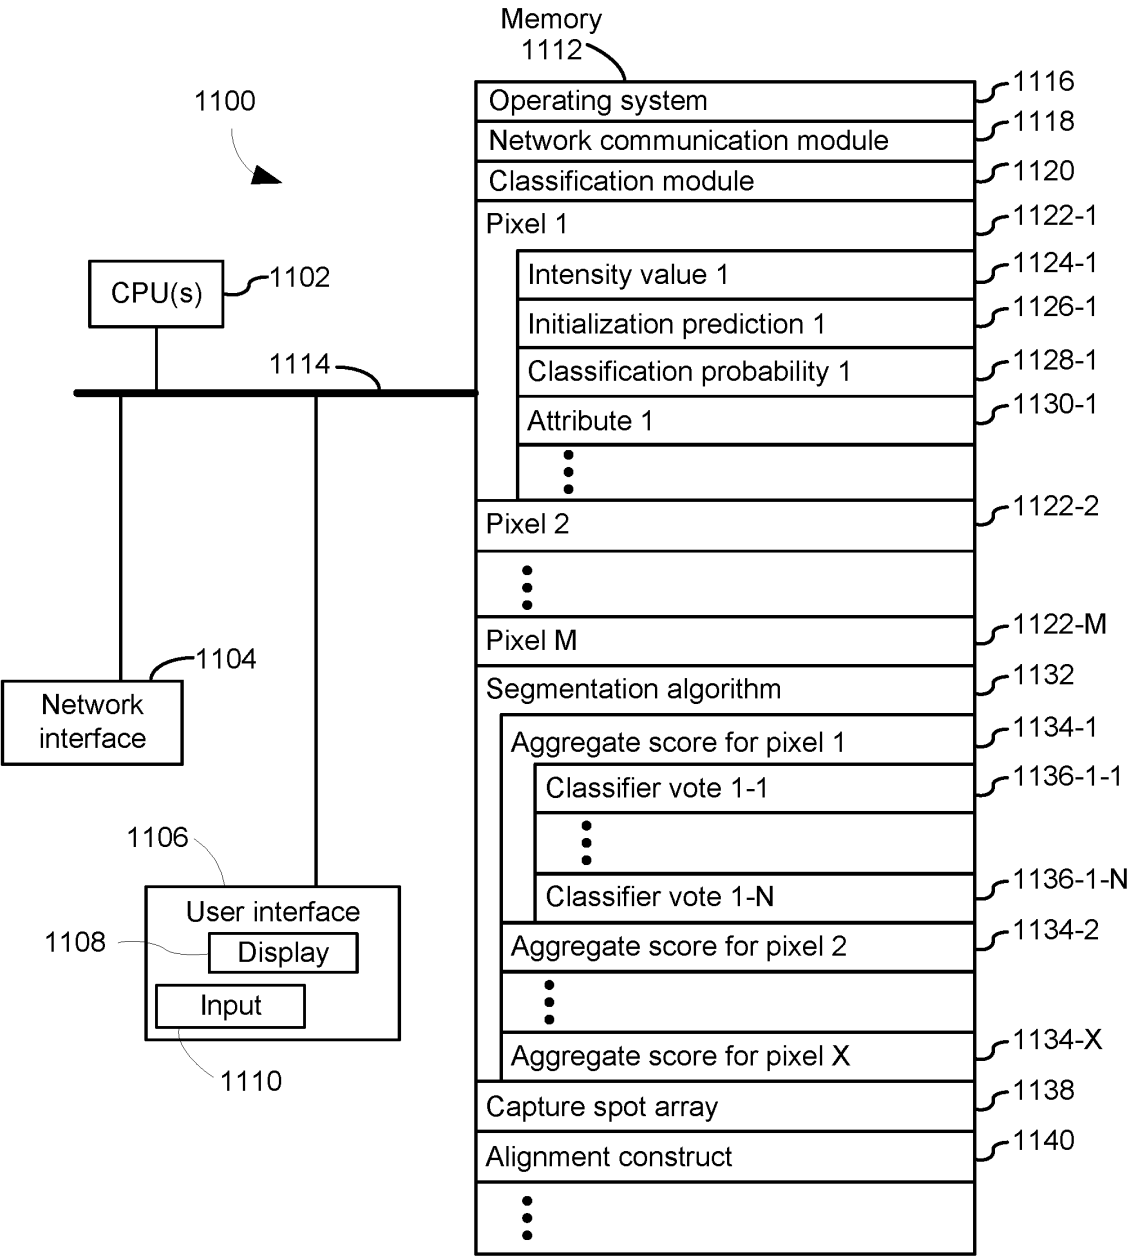


FIG. 11

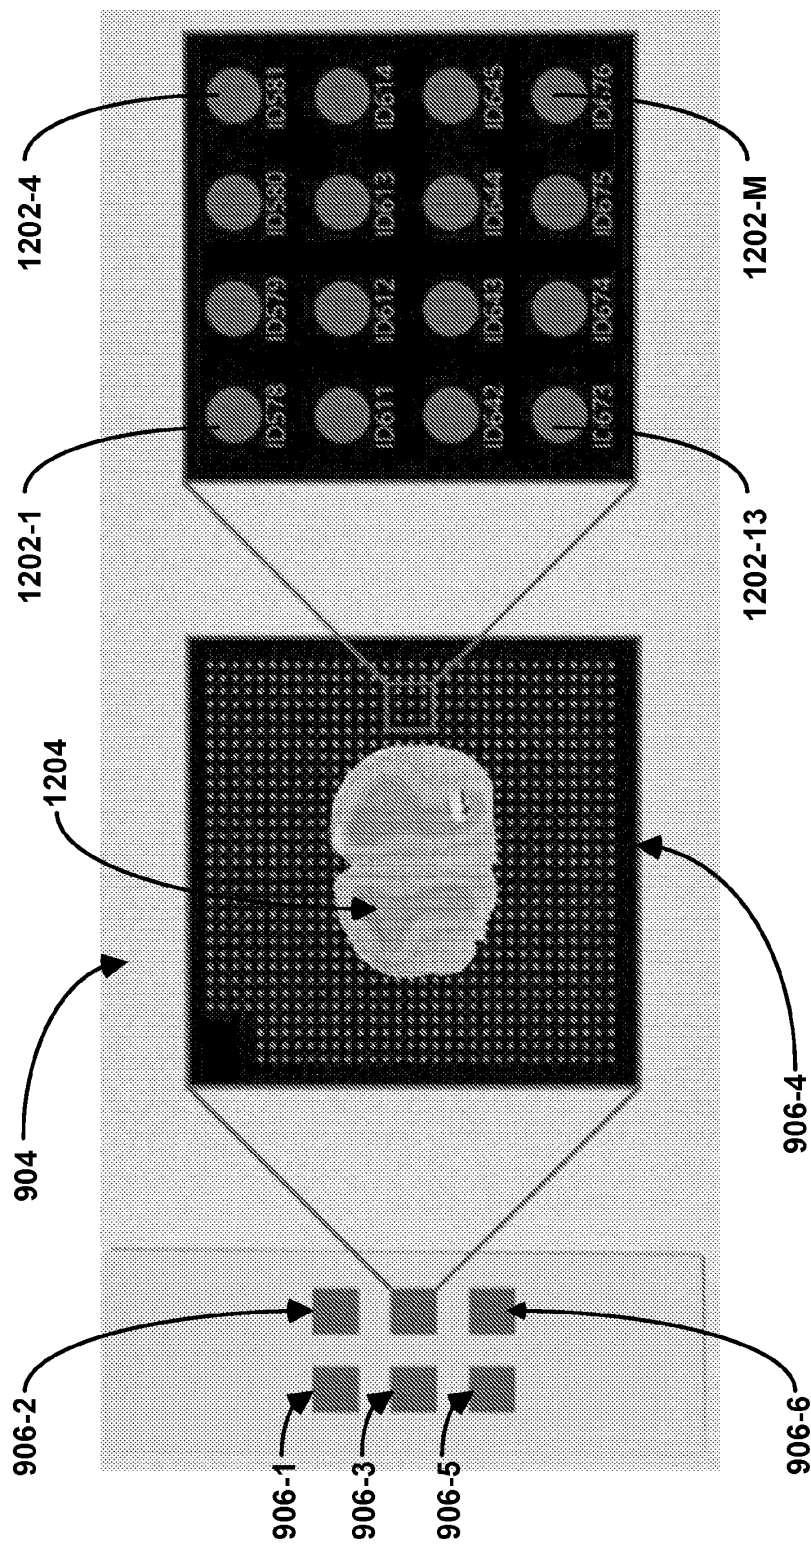


FIG. 12

1202

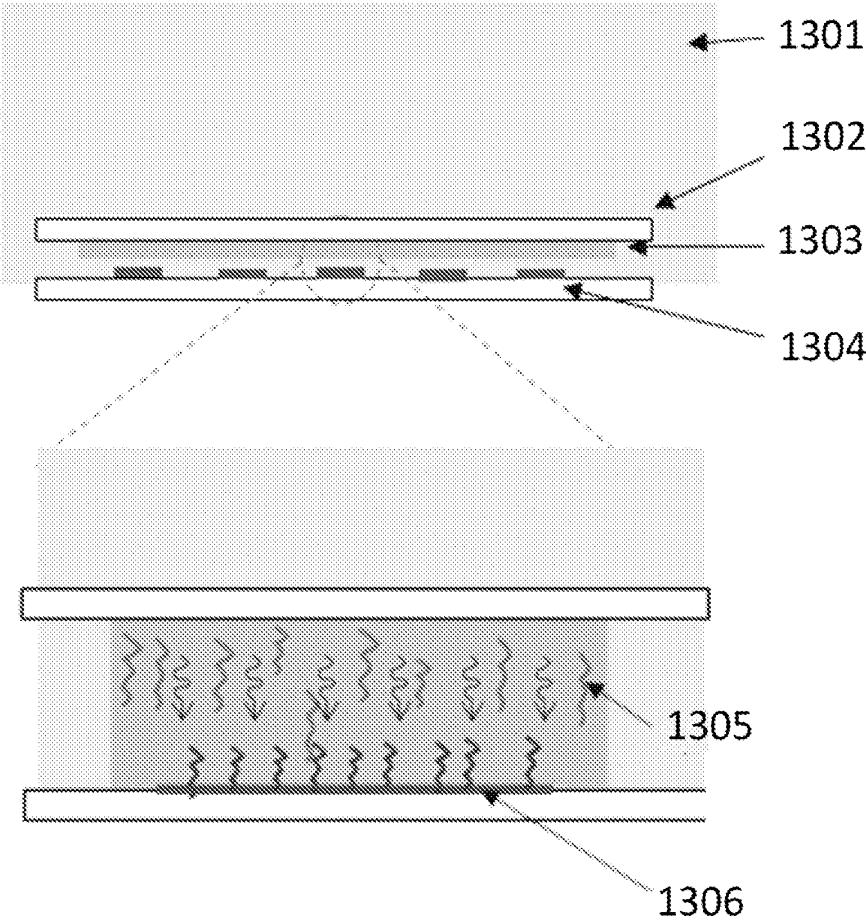


FIG. 13

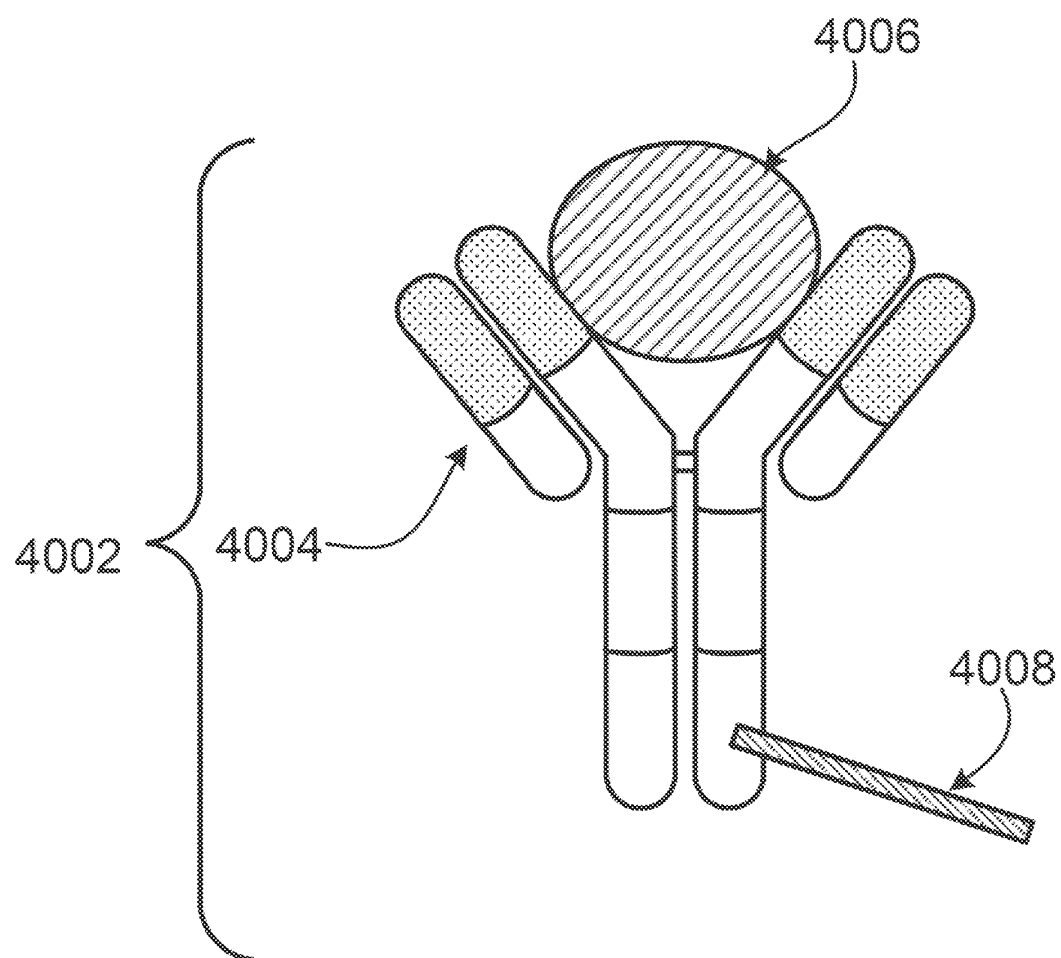


FIG. 14

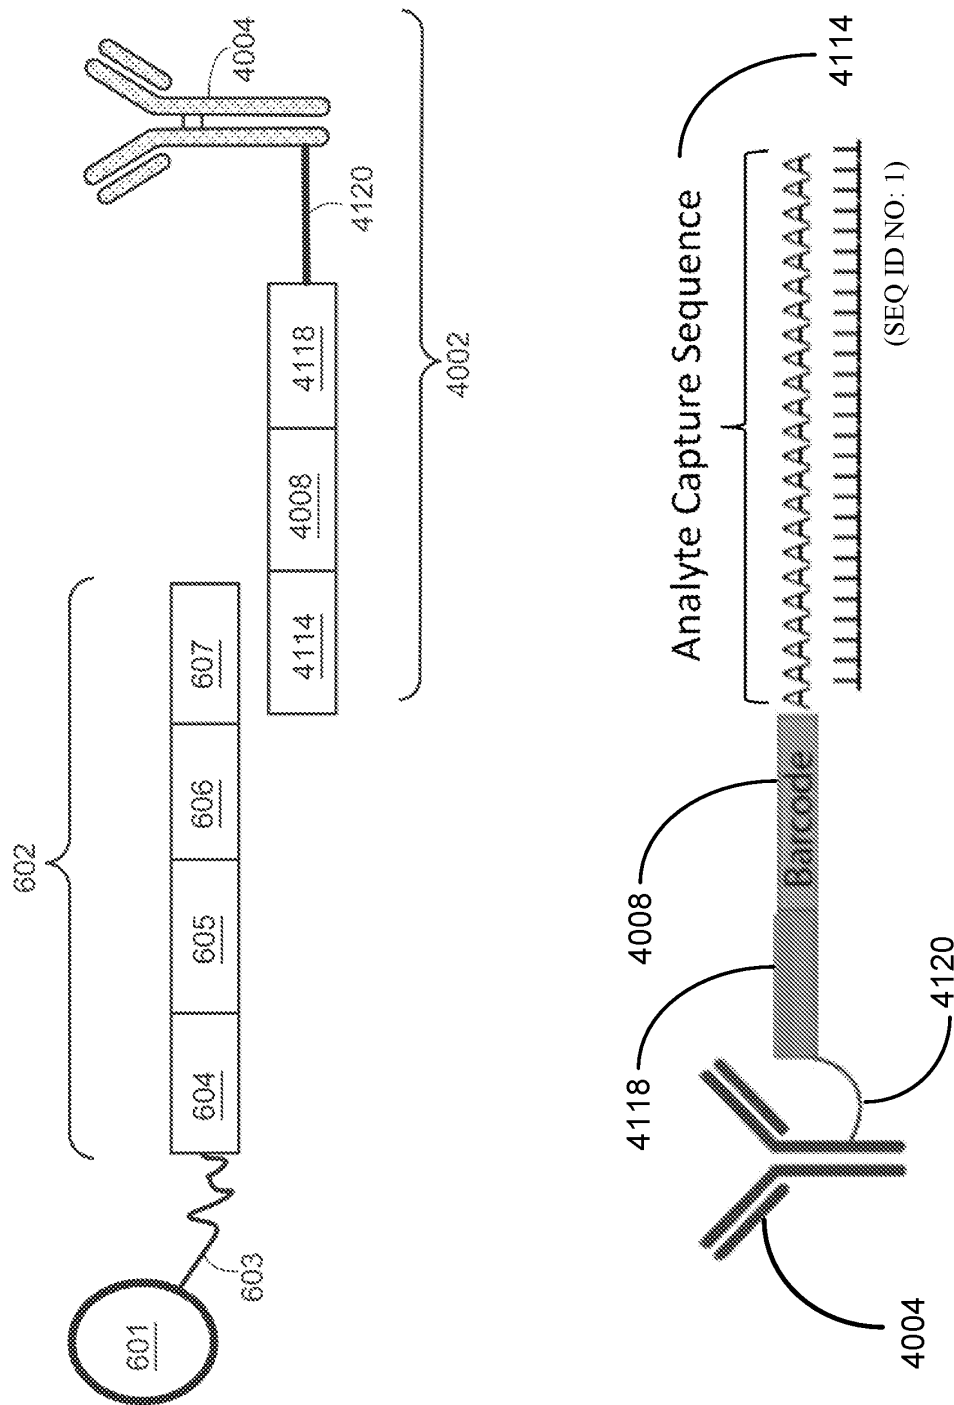


FIG. 15A

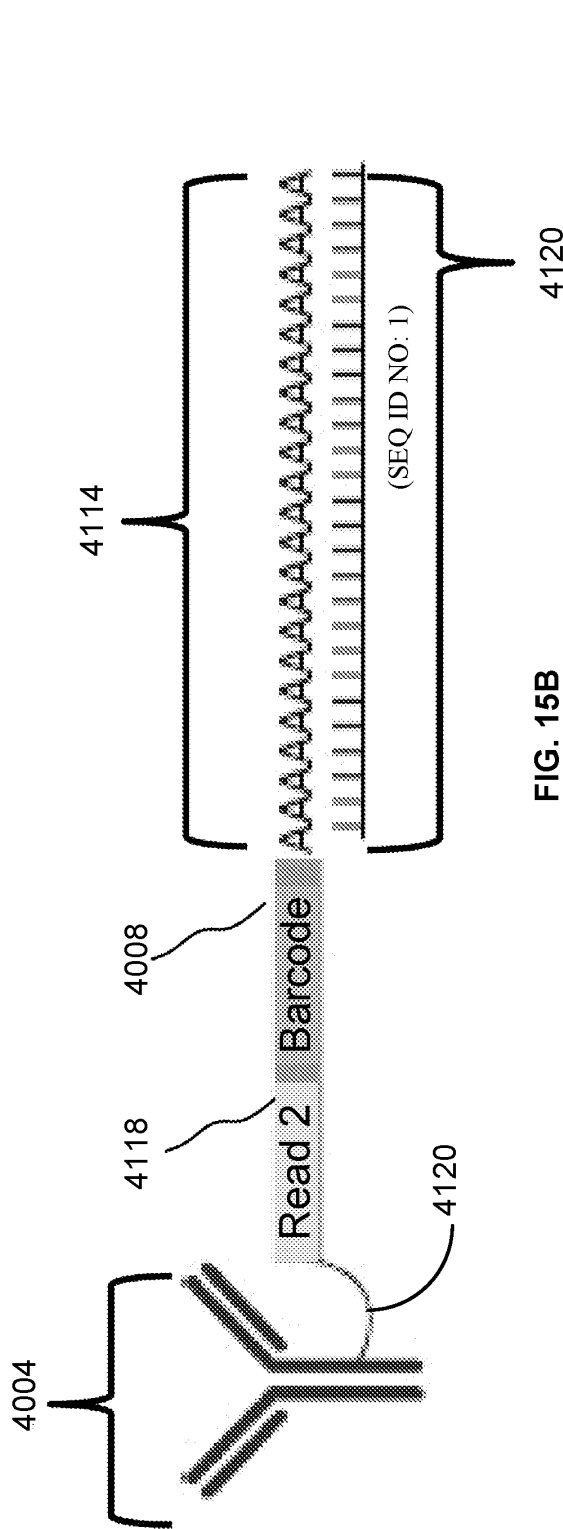


FIG. 15B

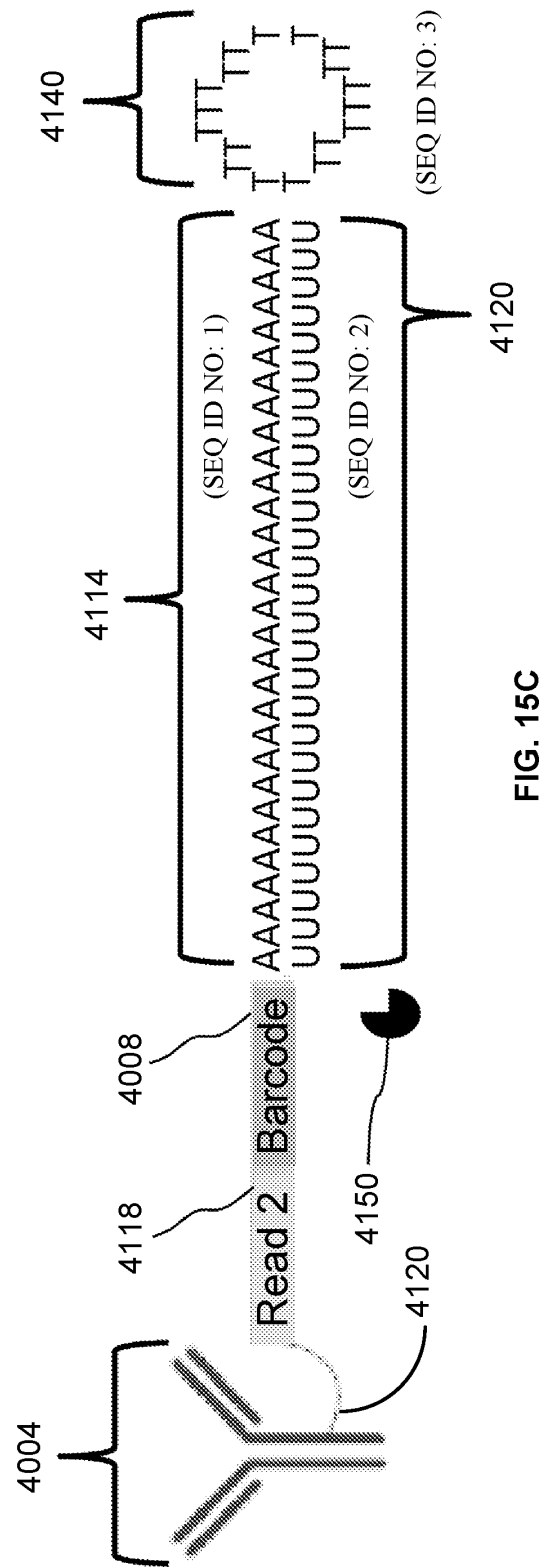


FIG. 15C

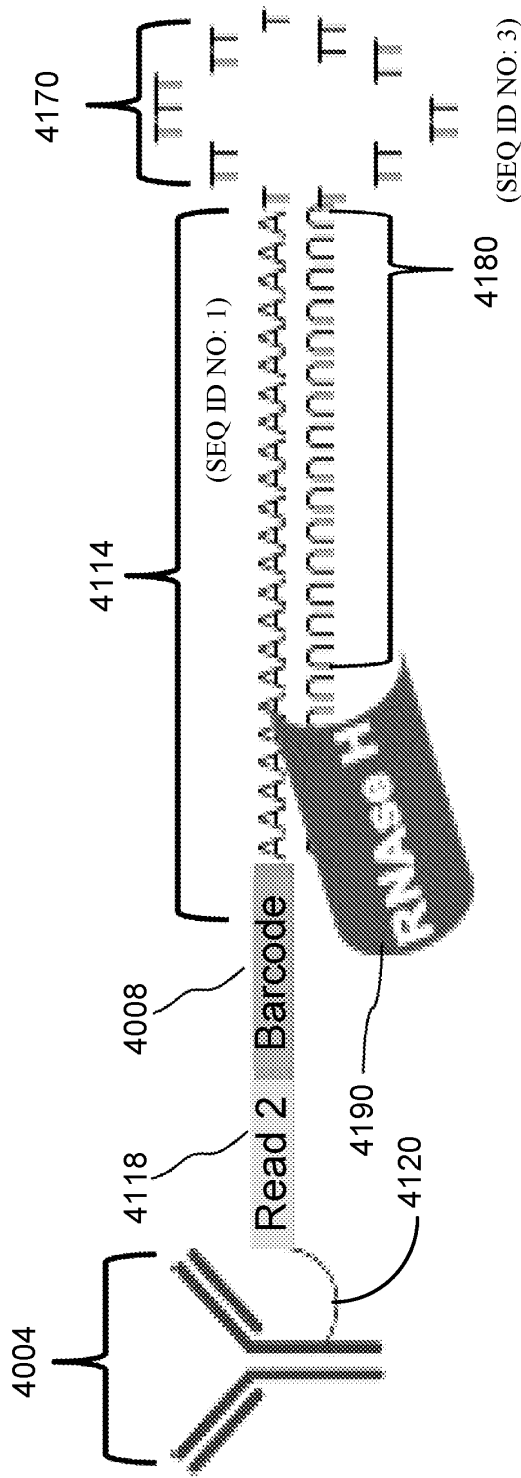


FIG. 15D

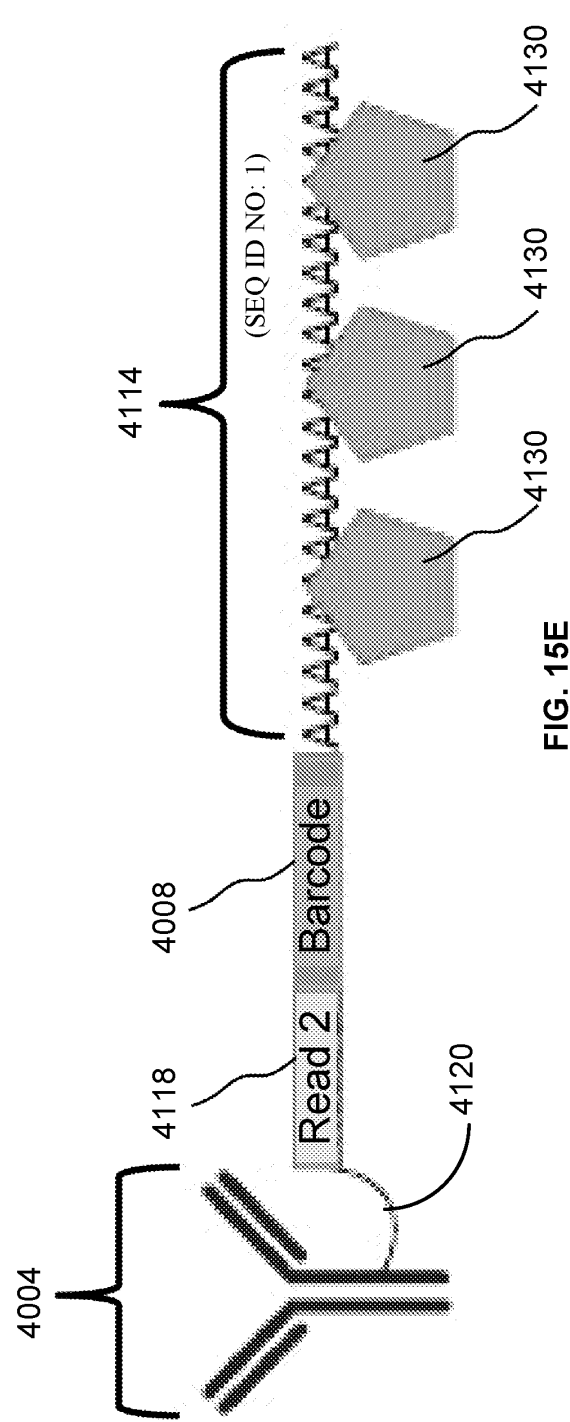


FIG. 15E

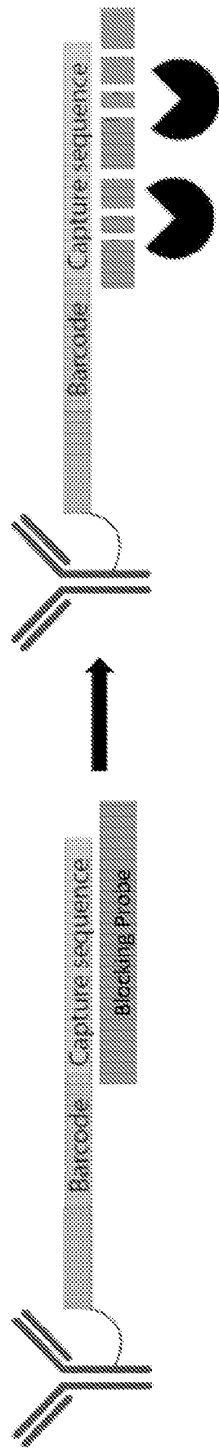


FIG. 16