



1/20

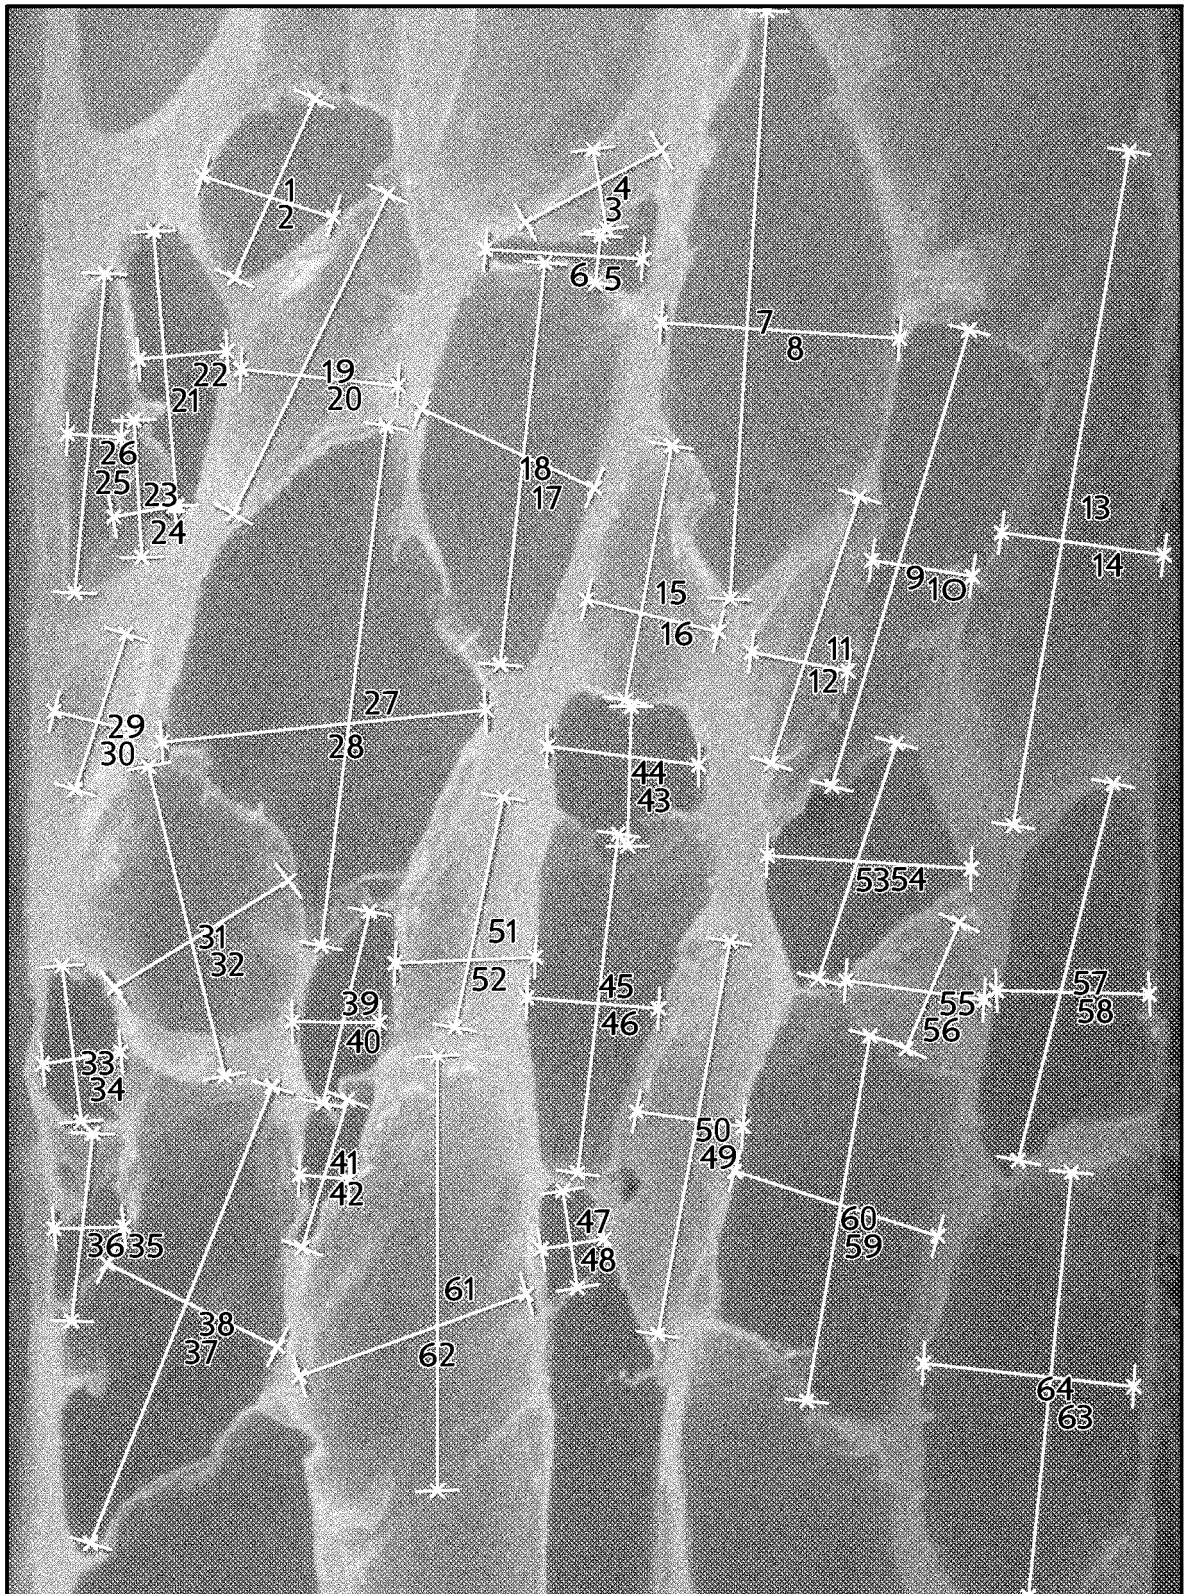


*FIG. 1*

2/20

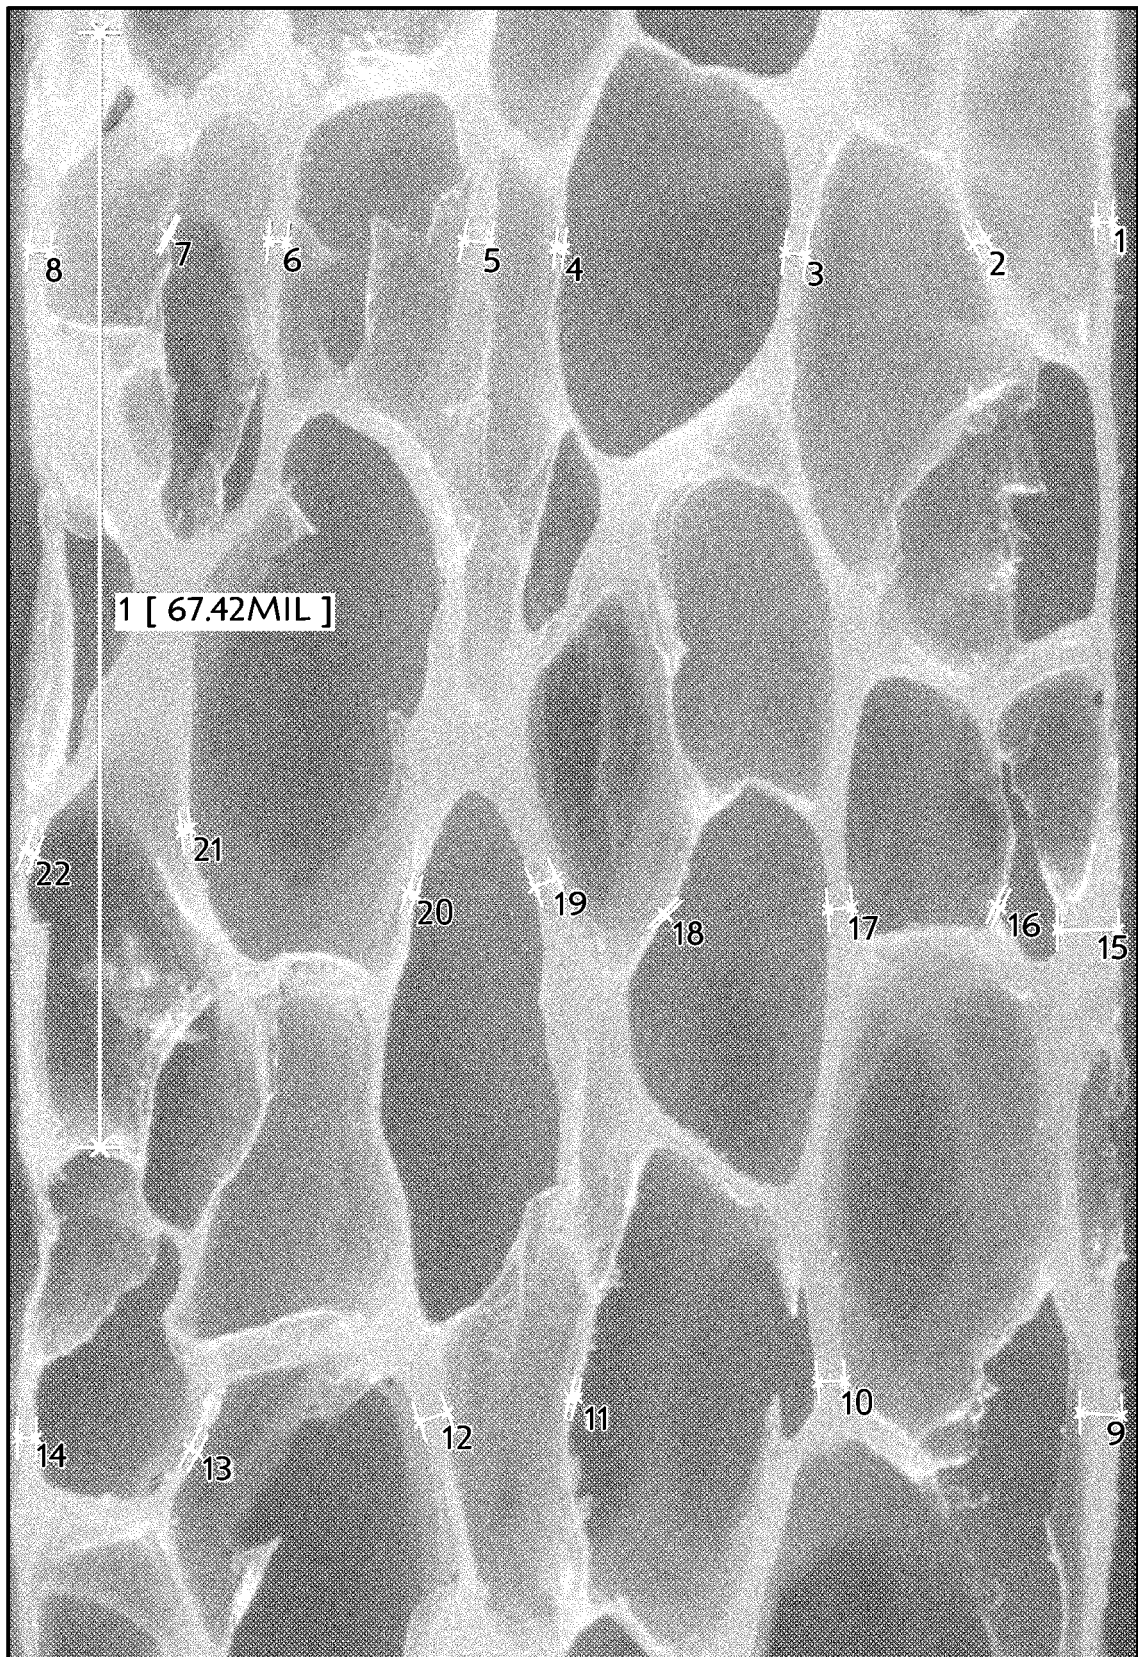


*FIG. 2*

3/20

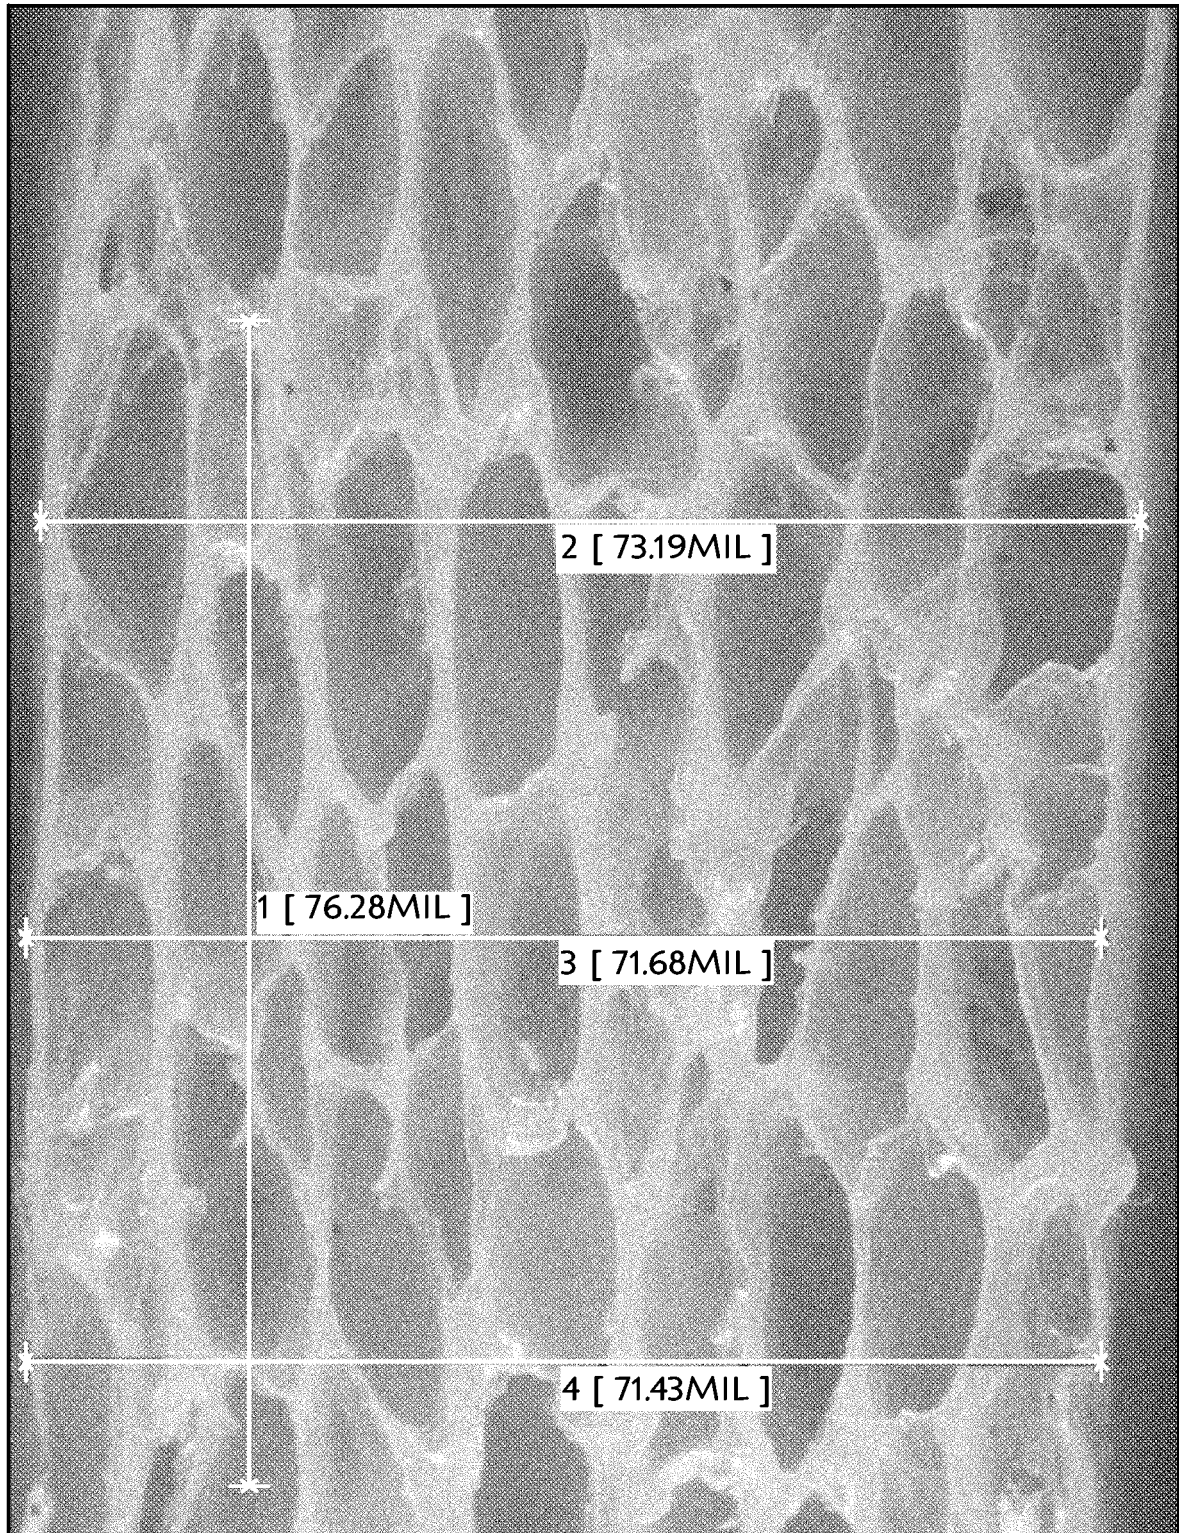


*FIG. 3*

4/20

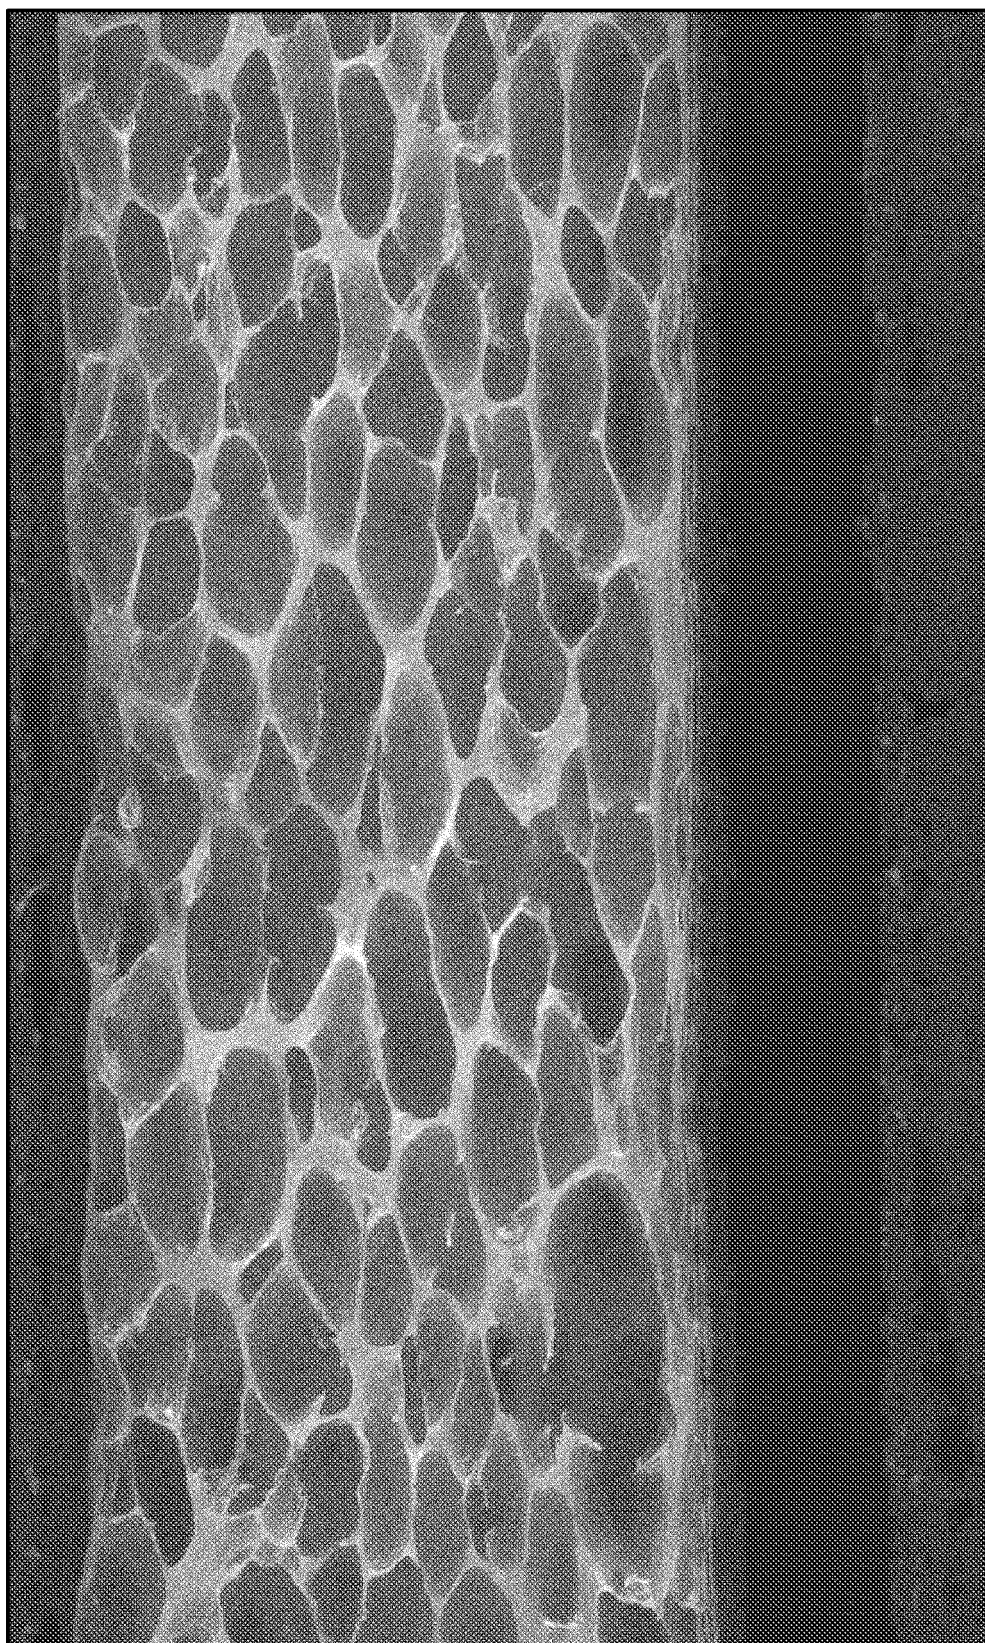


*FIG. 4*

5/20

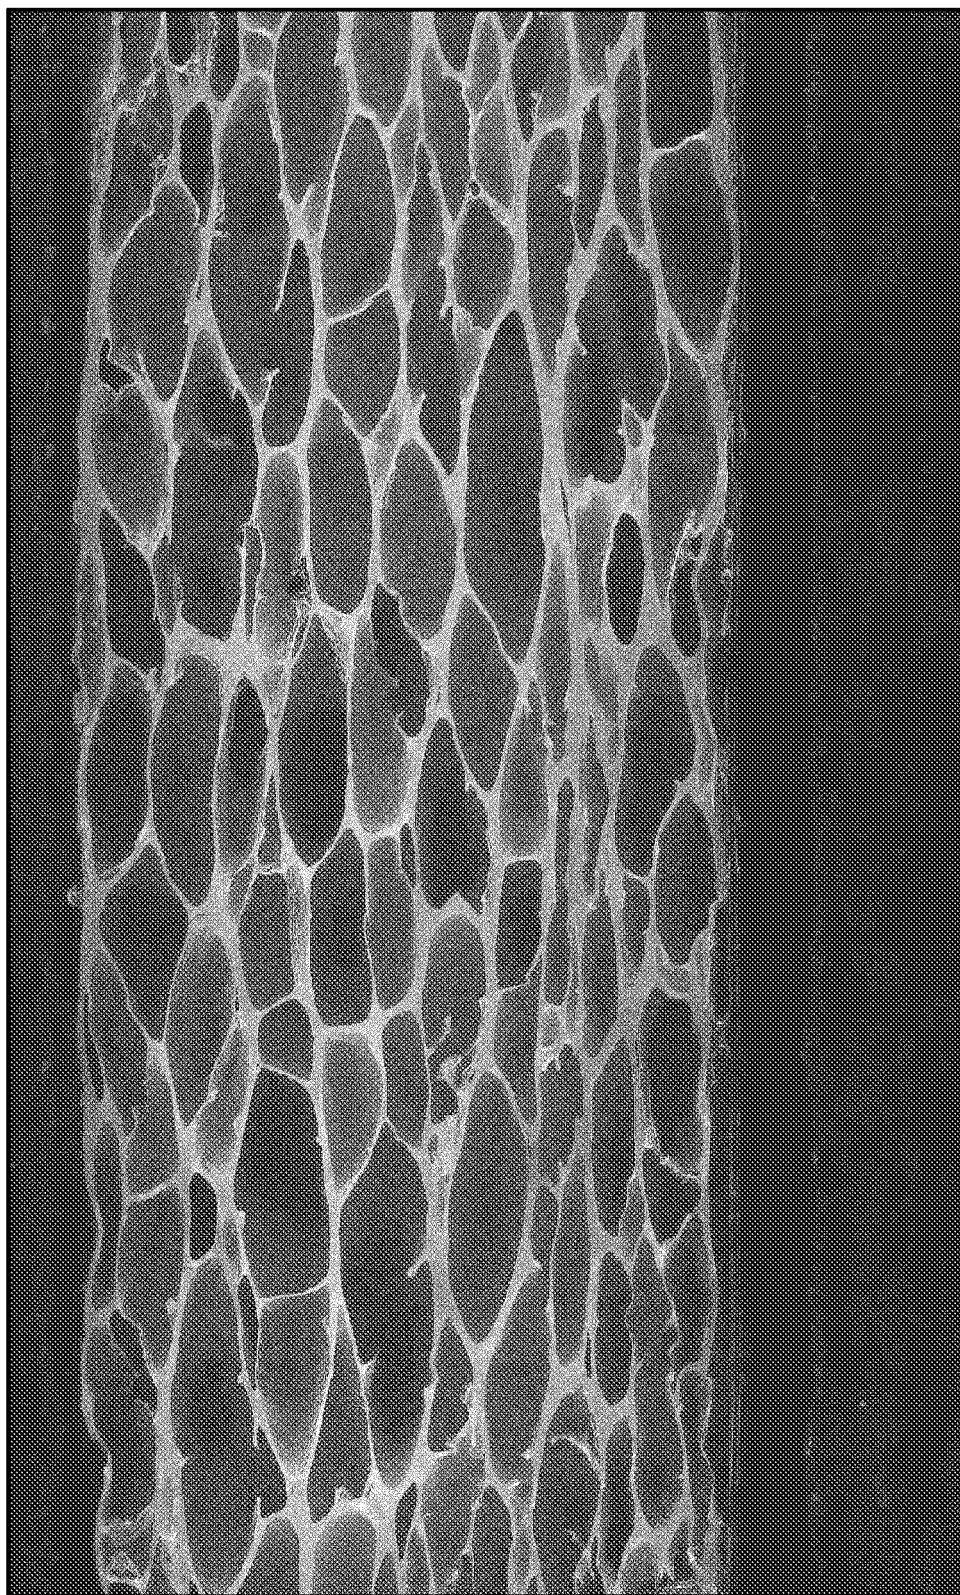


*FIG. 5*

6/20

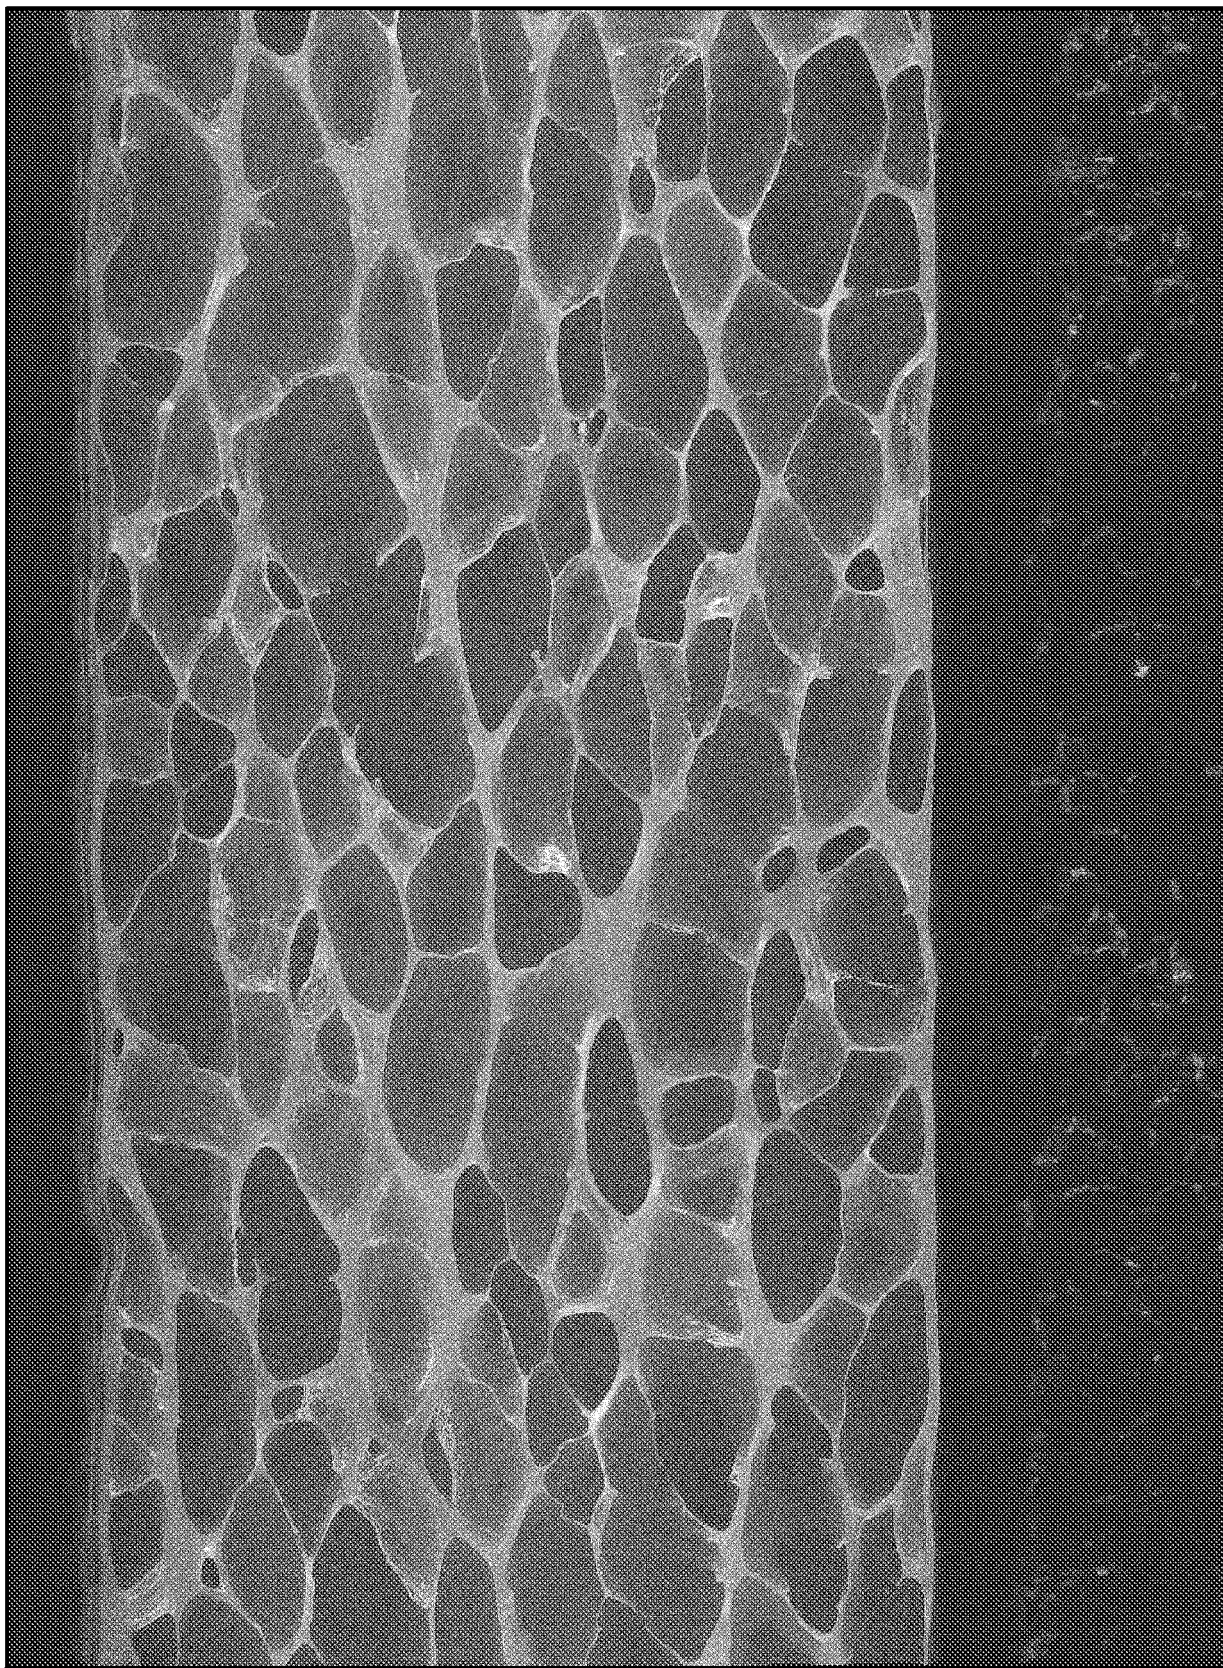

*FIG. 6*

7/20

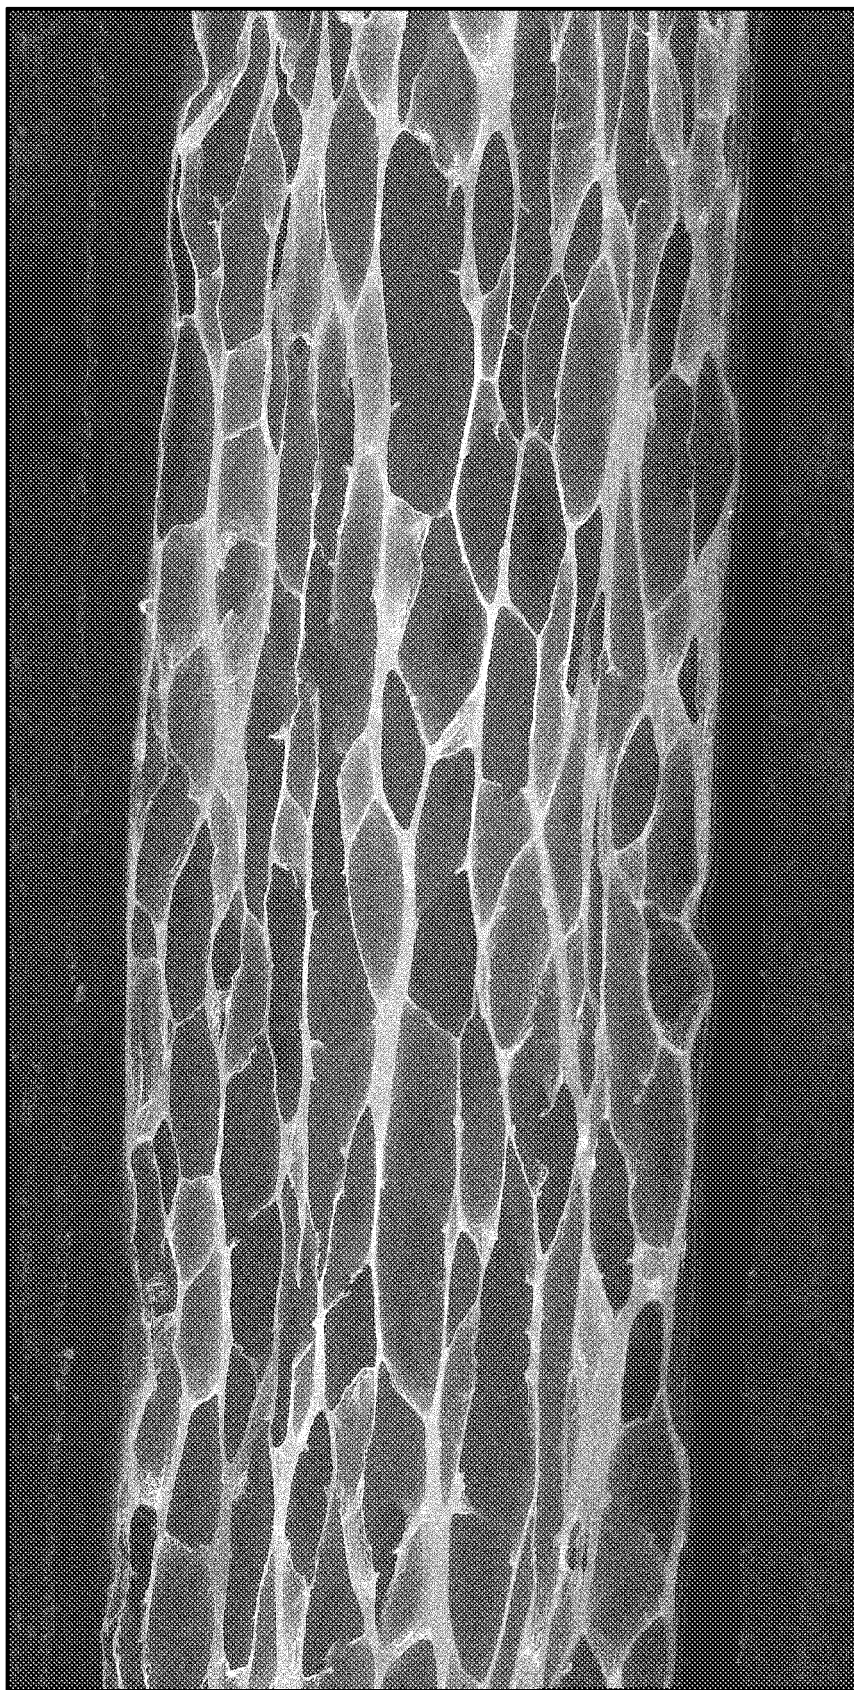

*FIG. 7*

8/20

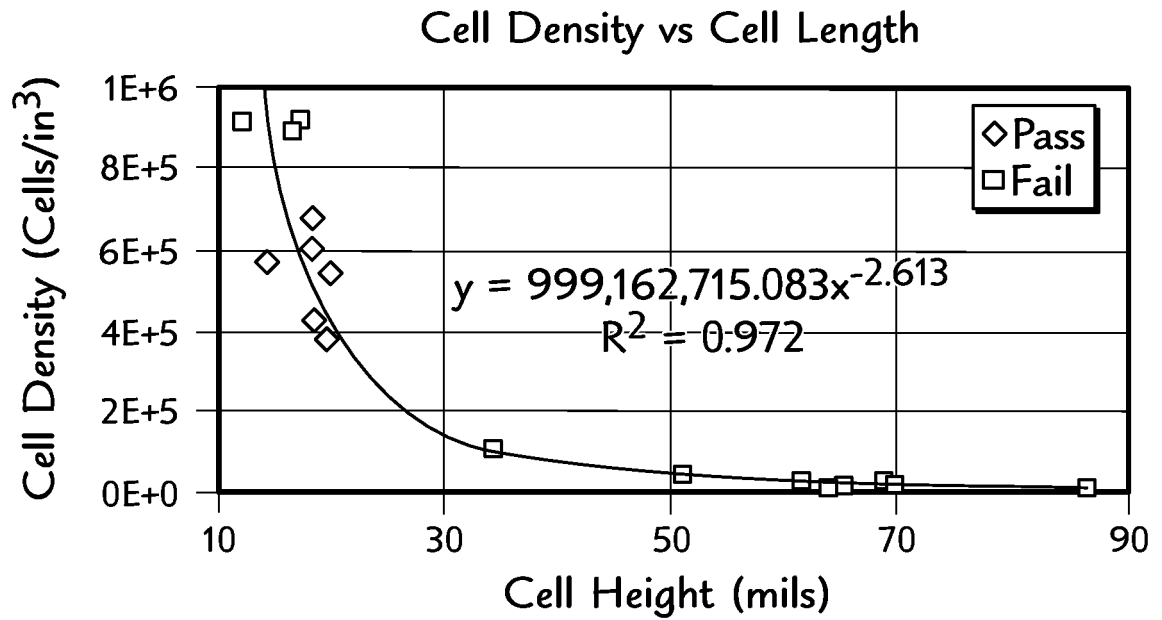


FIG. 8



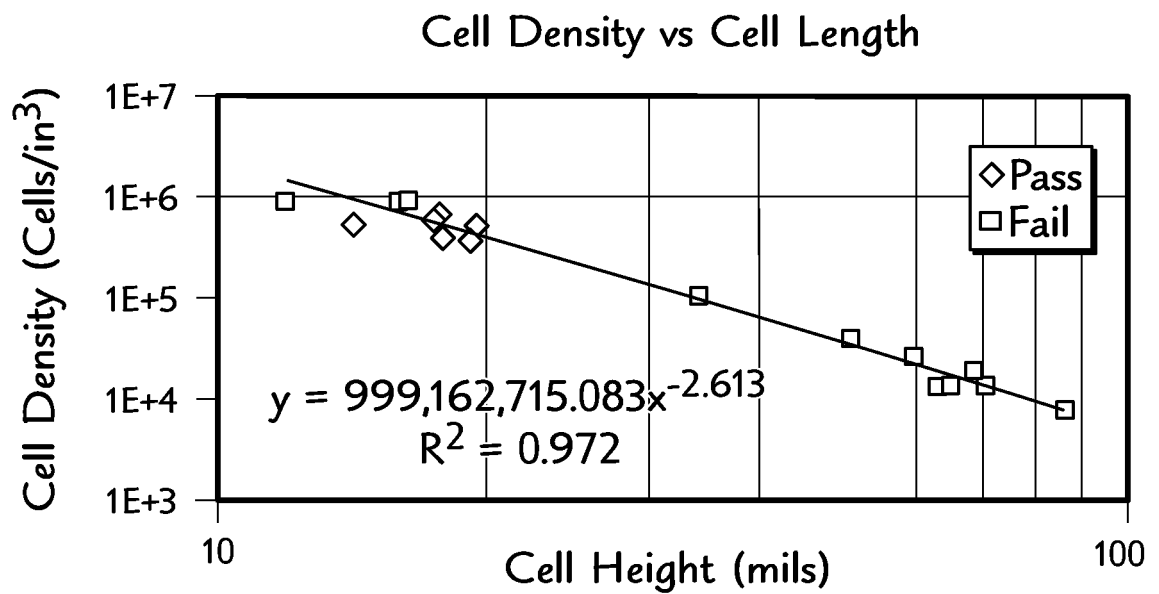


FIG. 9

9/20


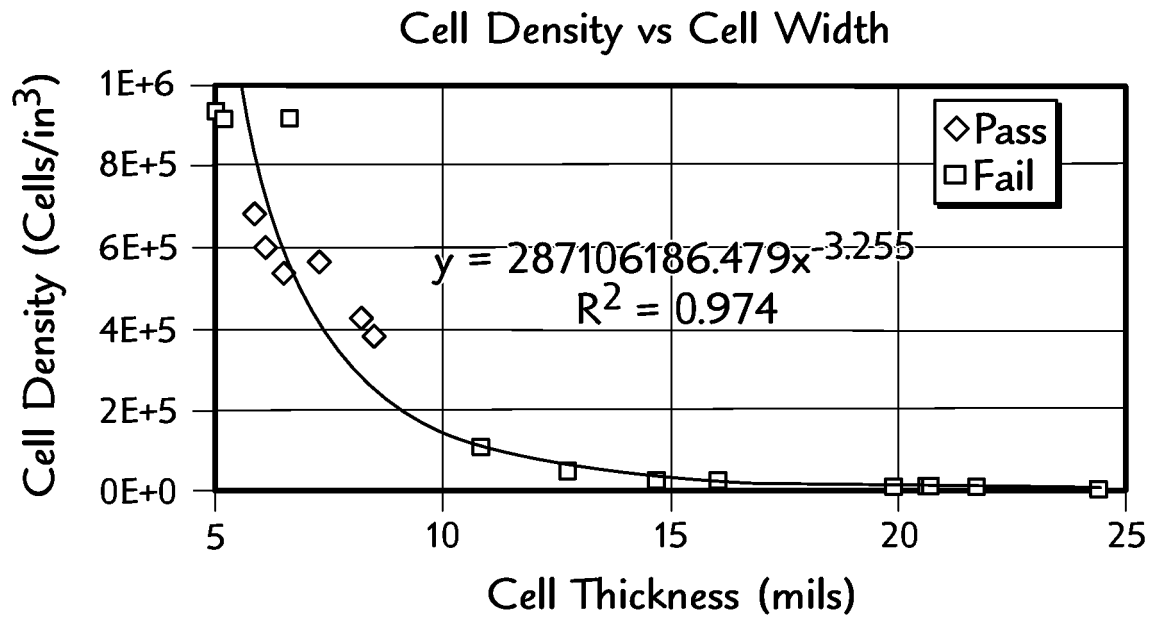


*FIG. 10*


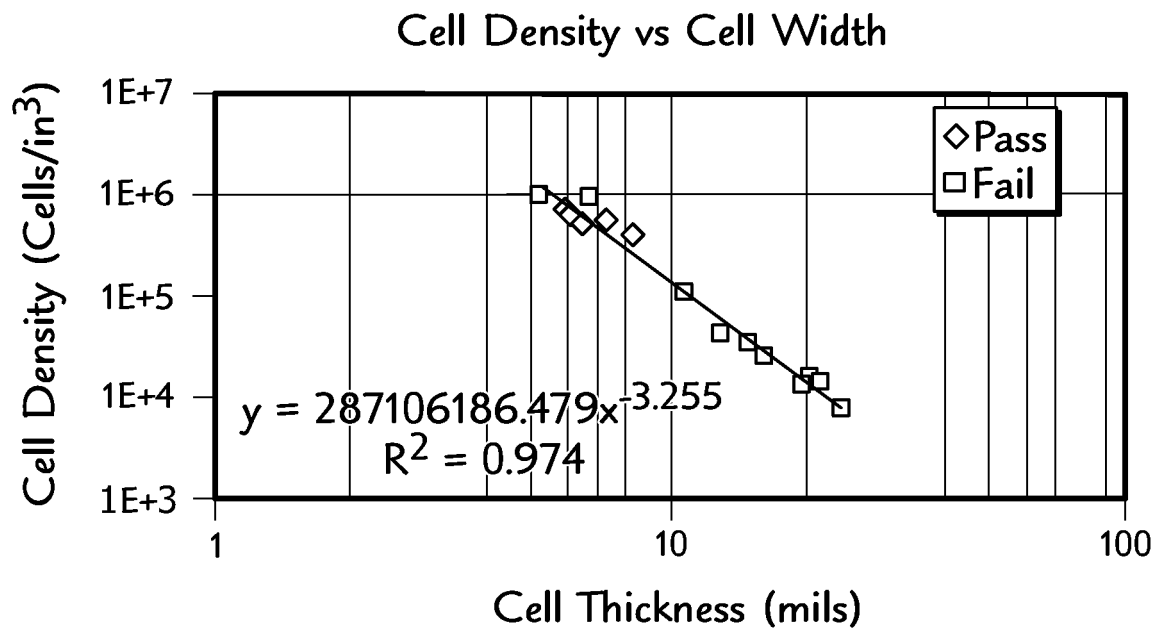


*FIG. 11*

10/20

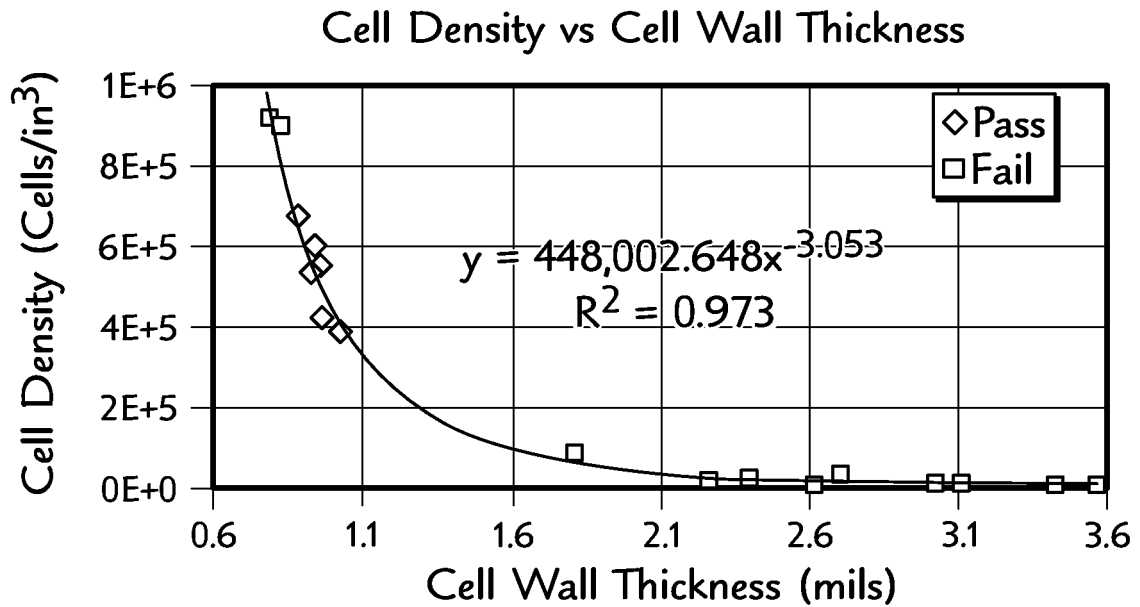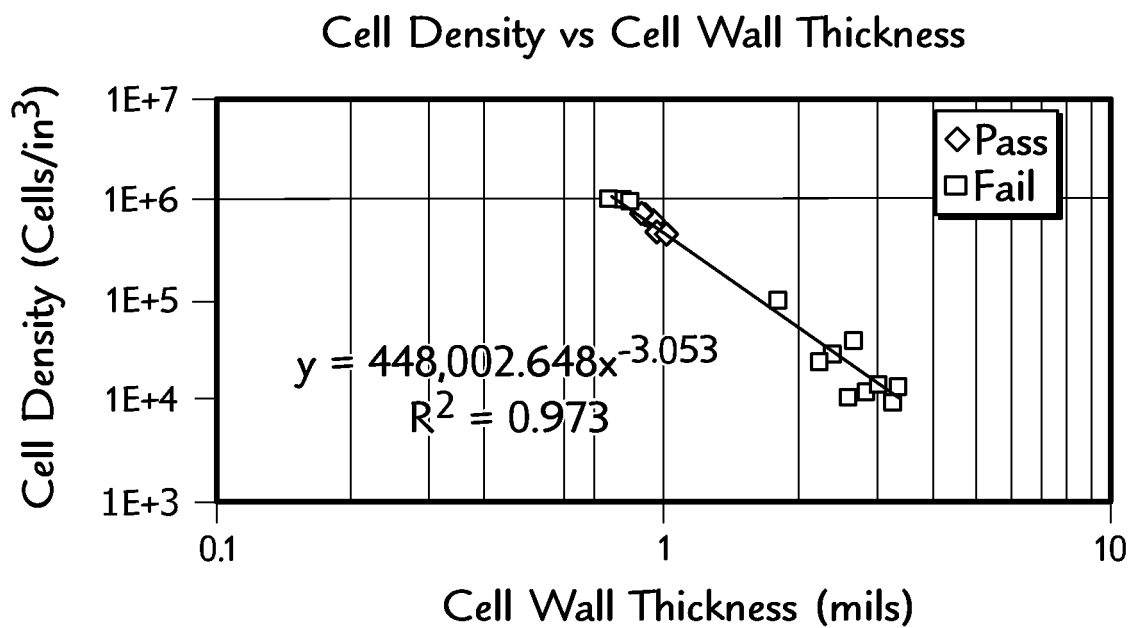*FIG. 12**FIG. 13*

11/20

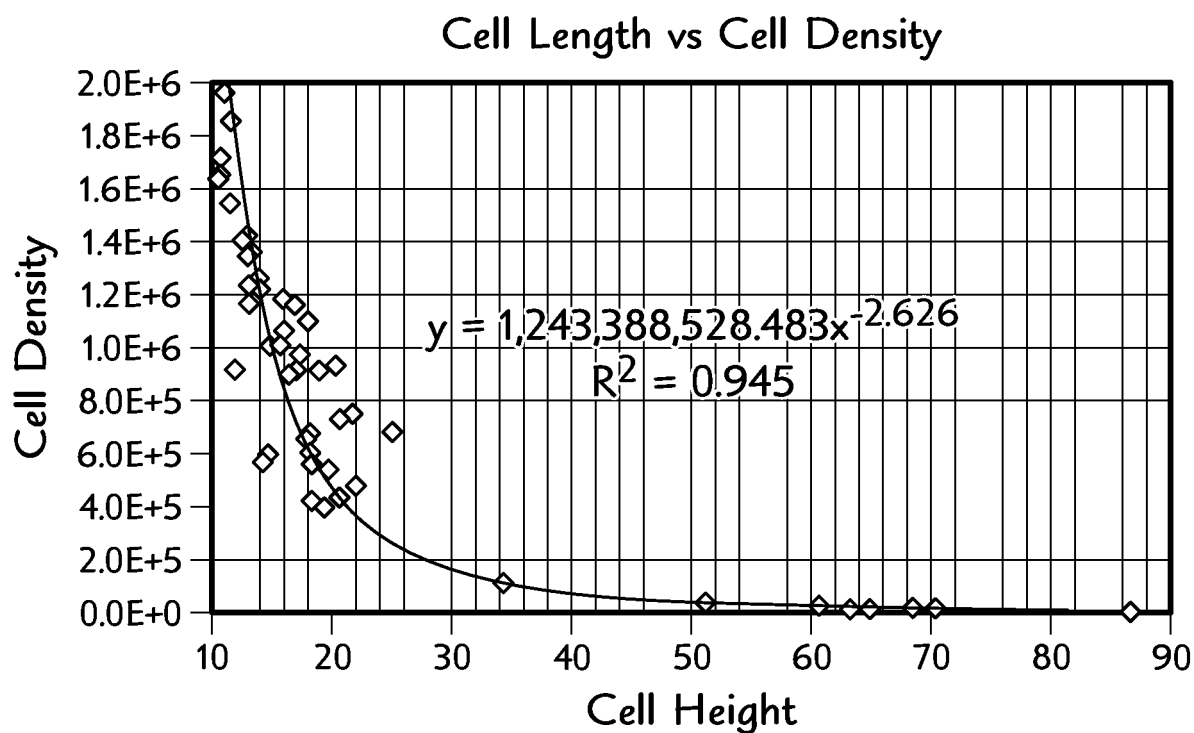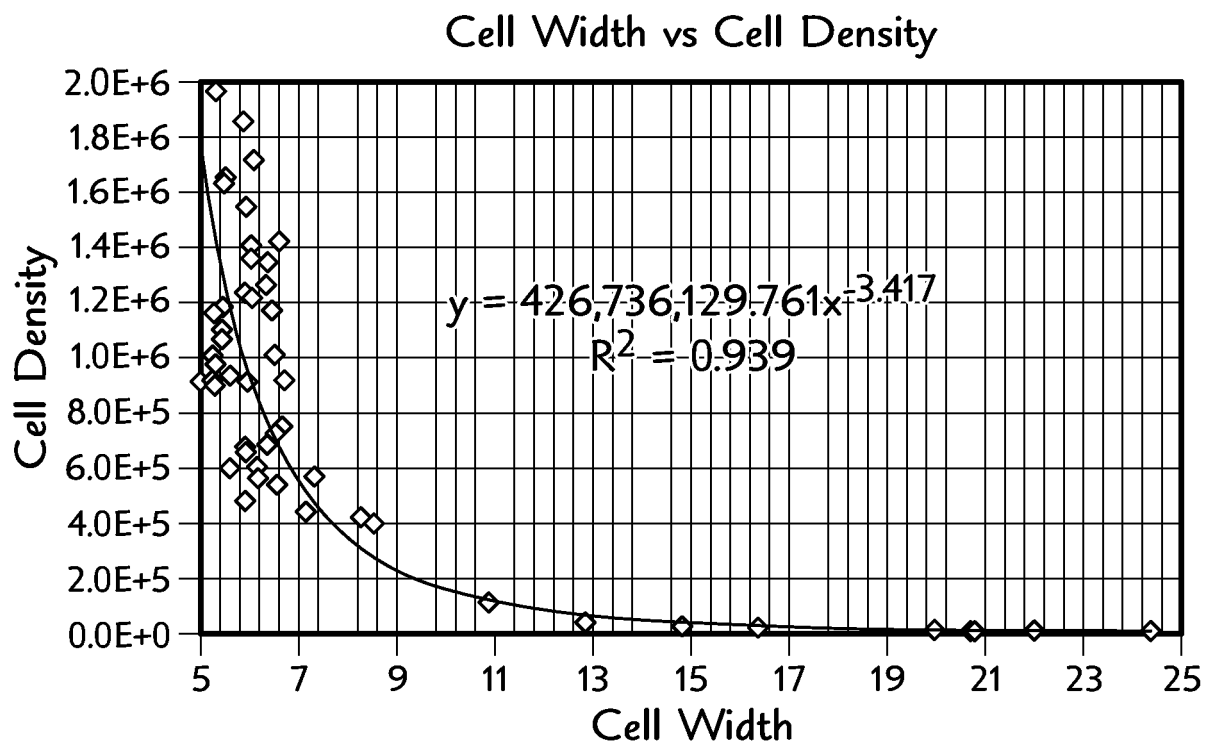*FIG. 14**FIG. 15*

12/20

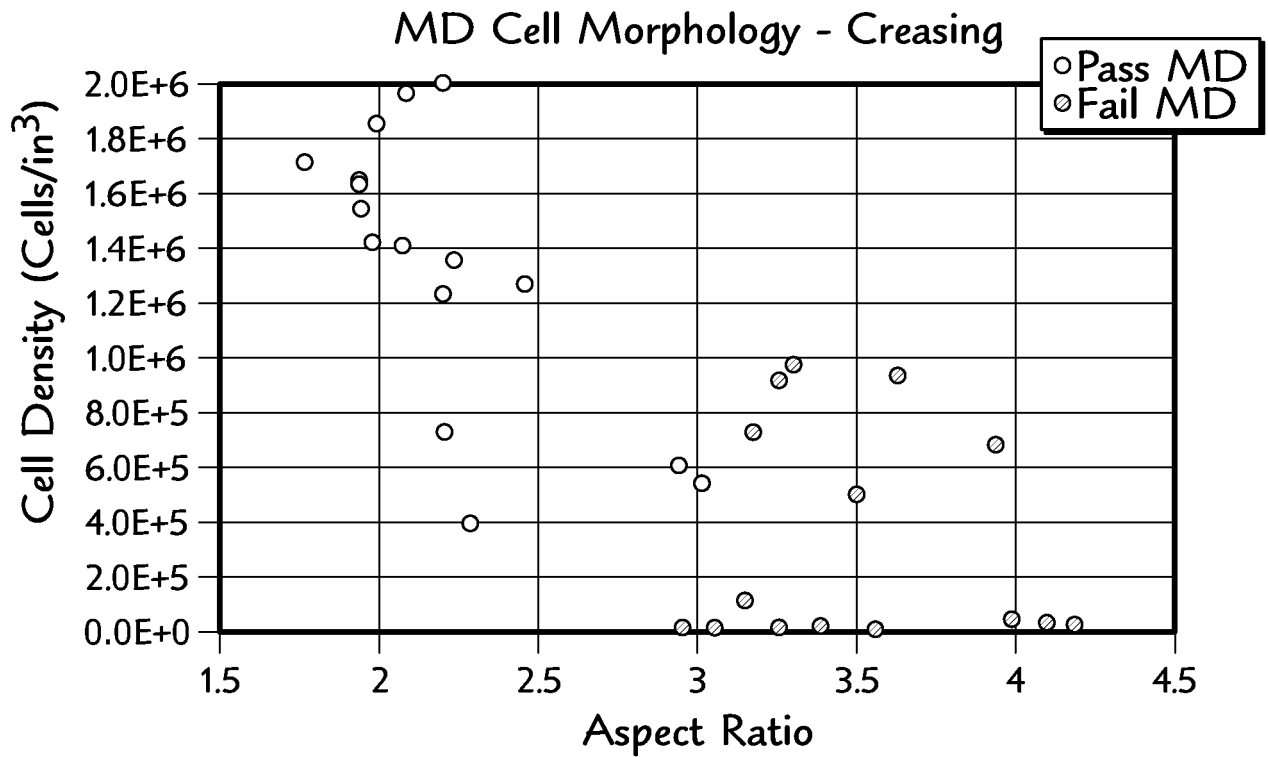


FIG. 16


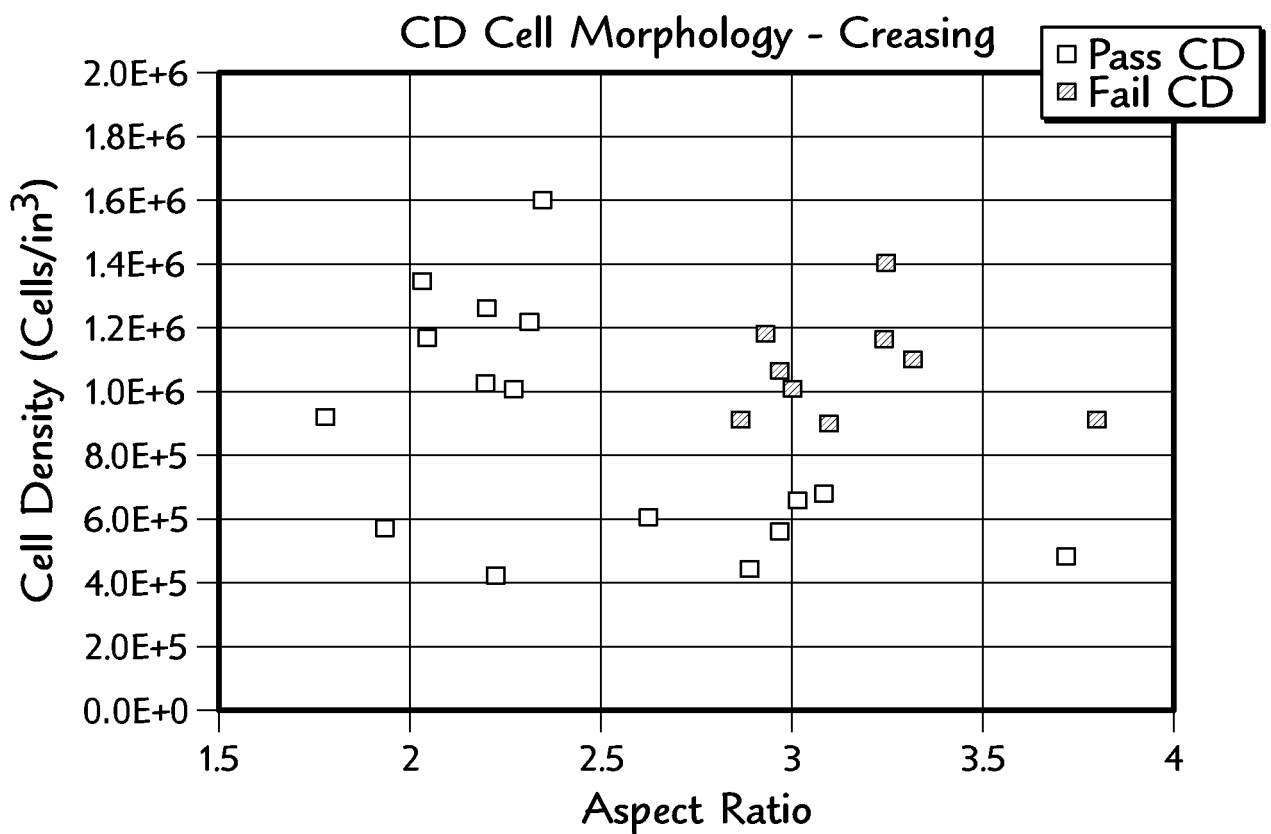


FIG. 17

13/20

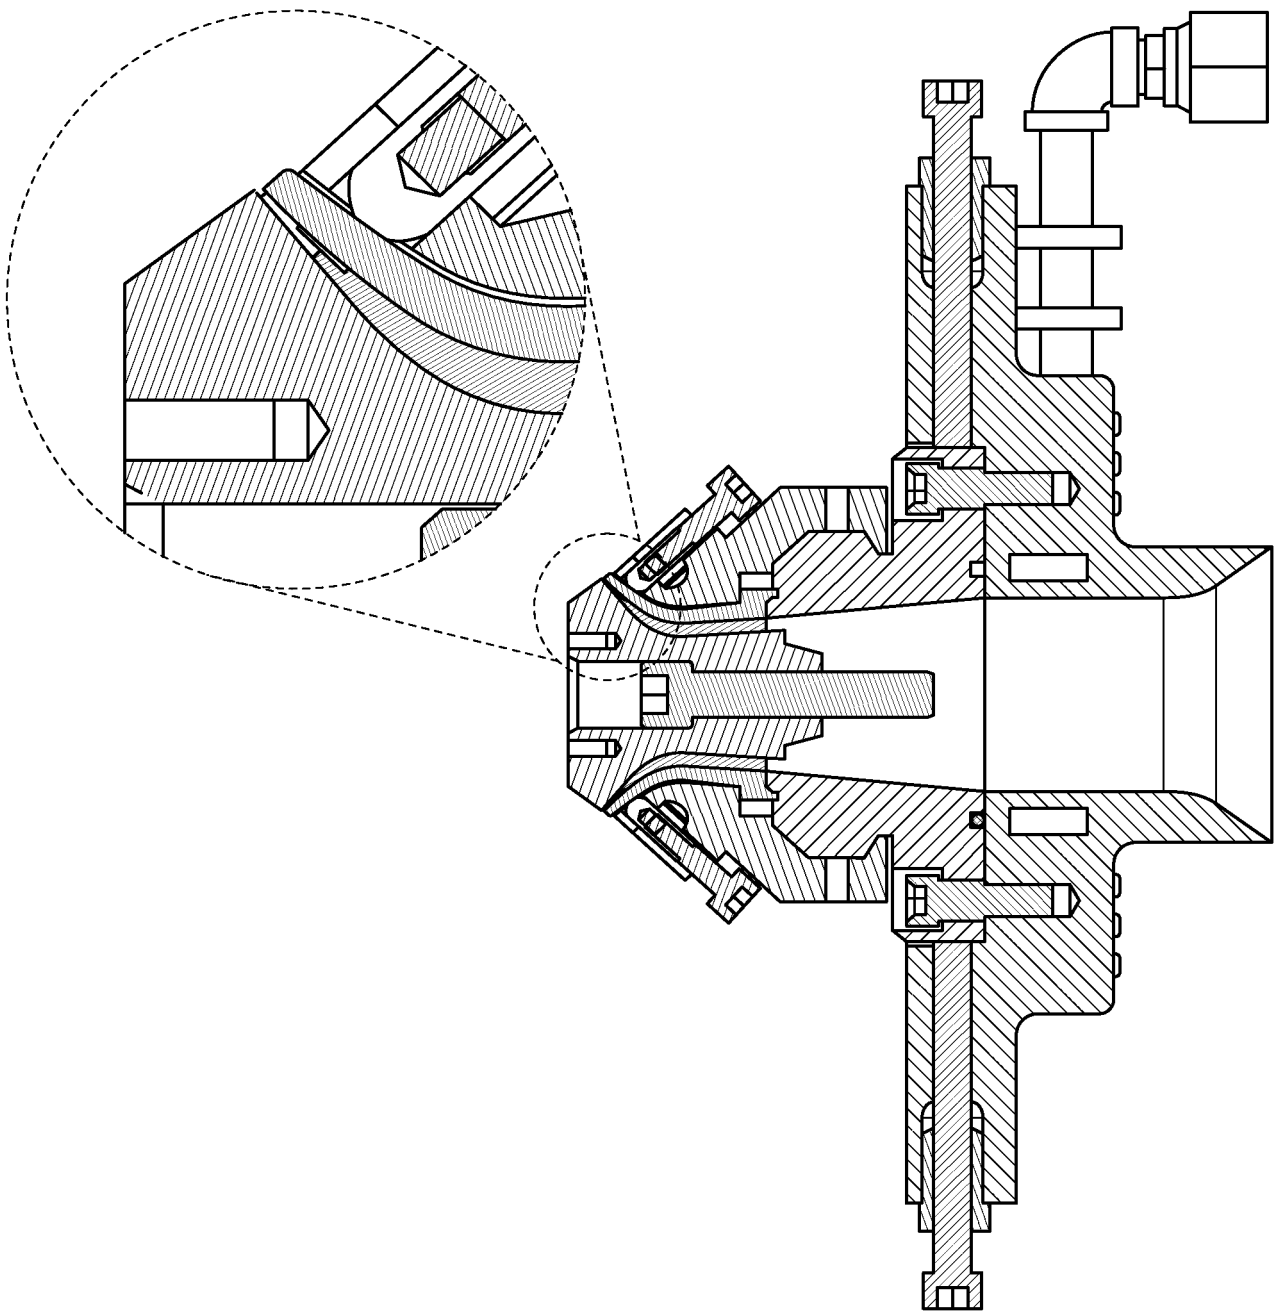

*FIG. 18*


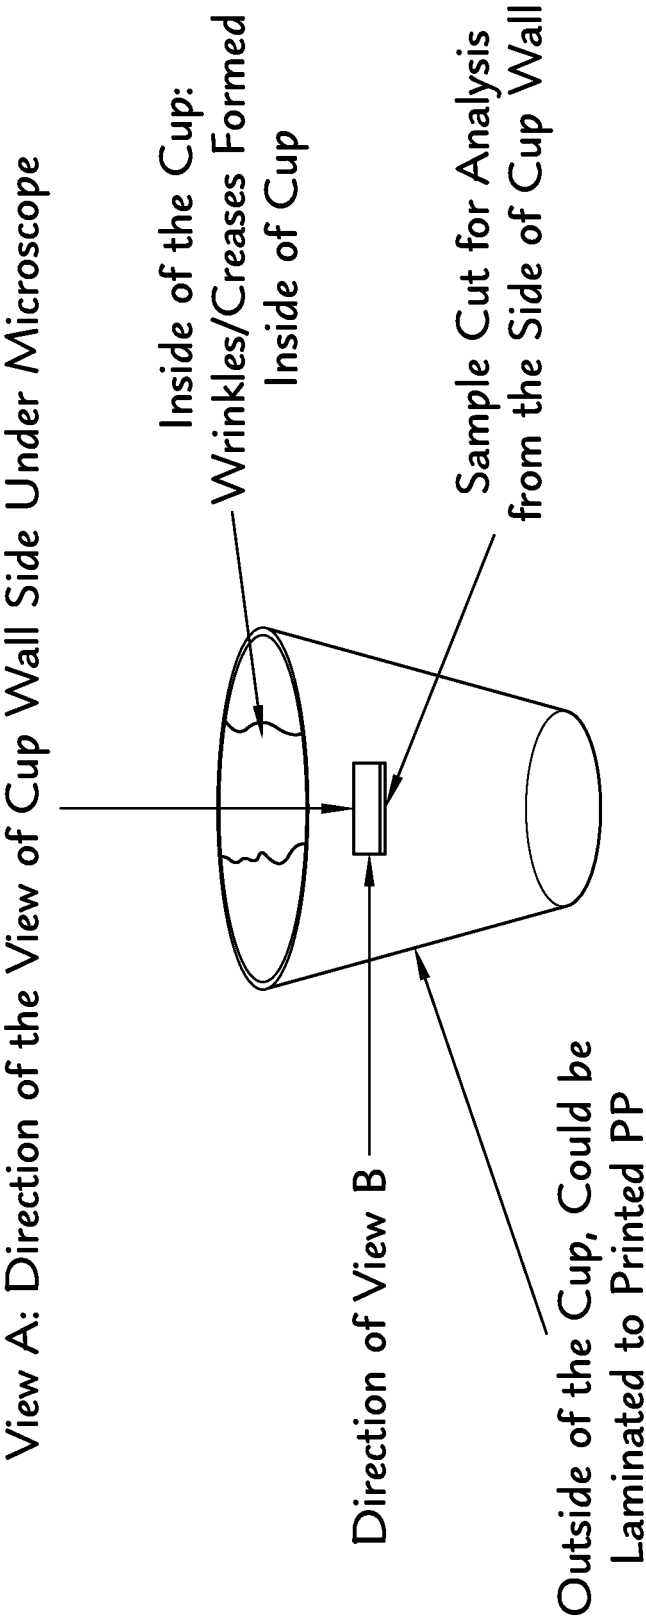


FIG. 19

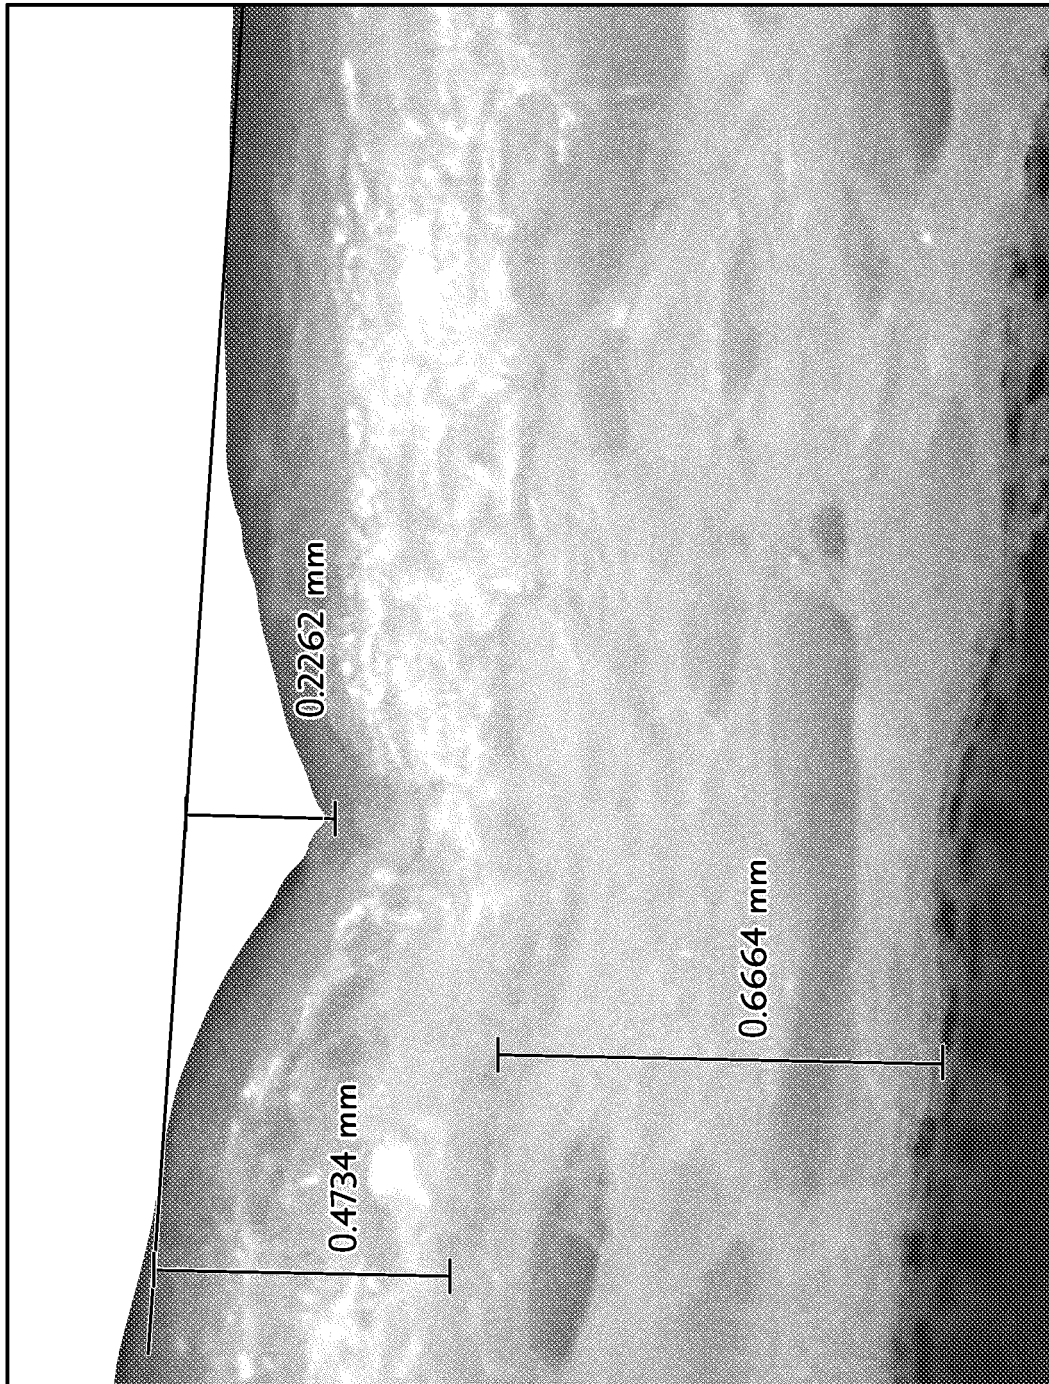

*FIG. 20*

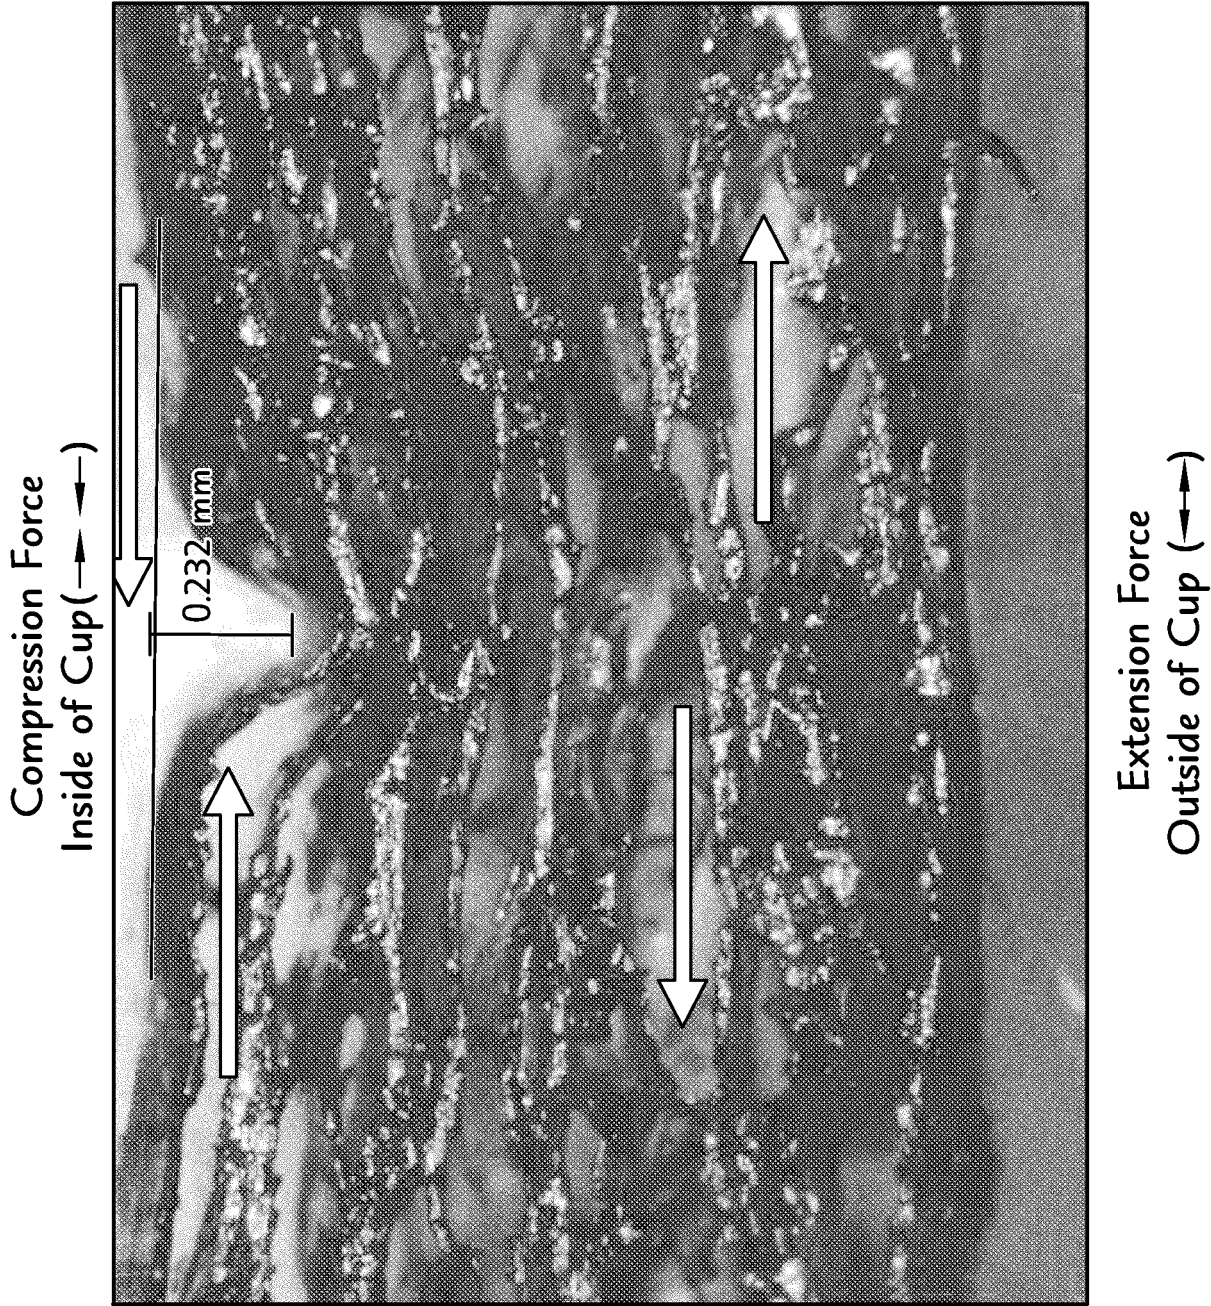
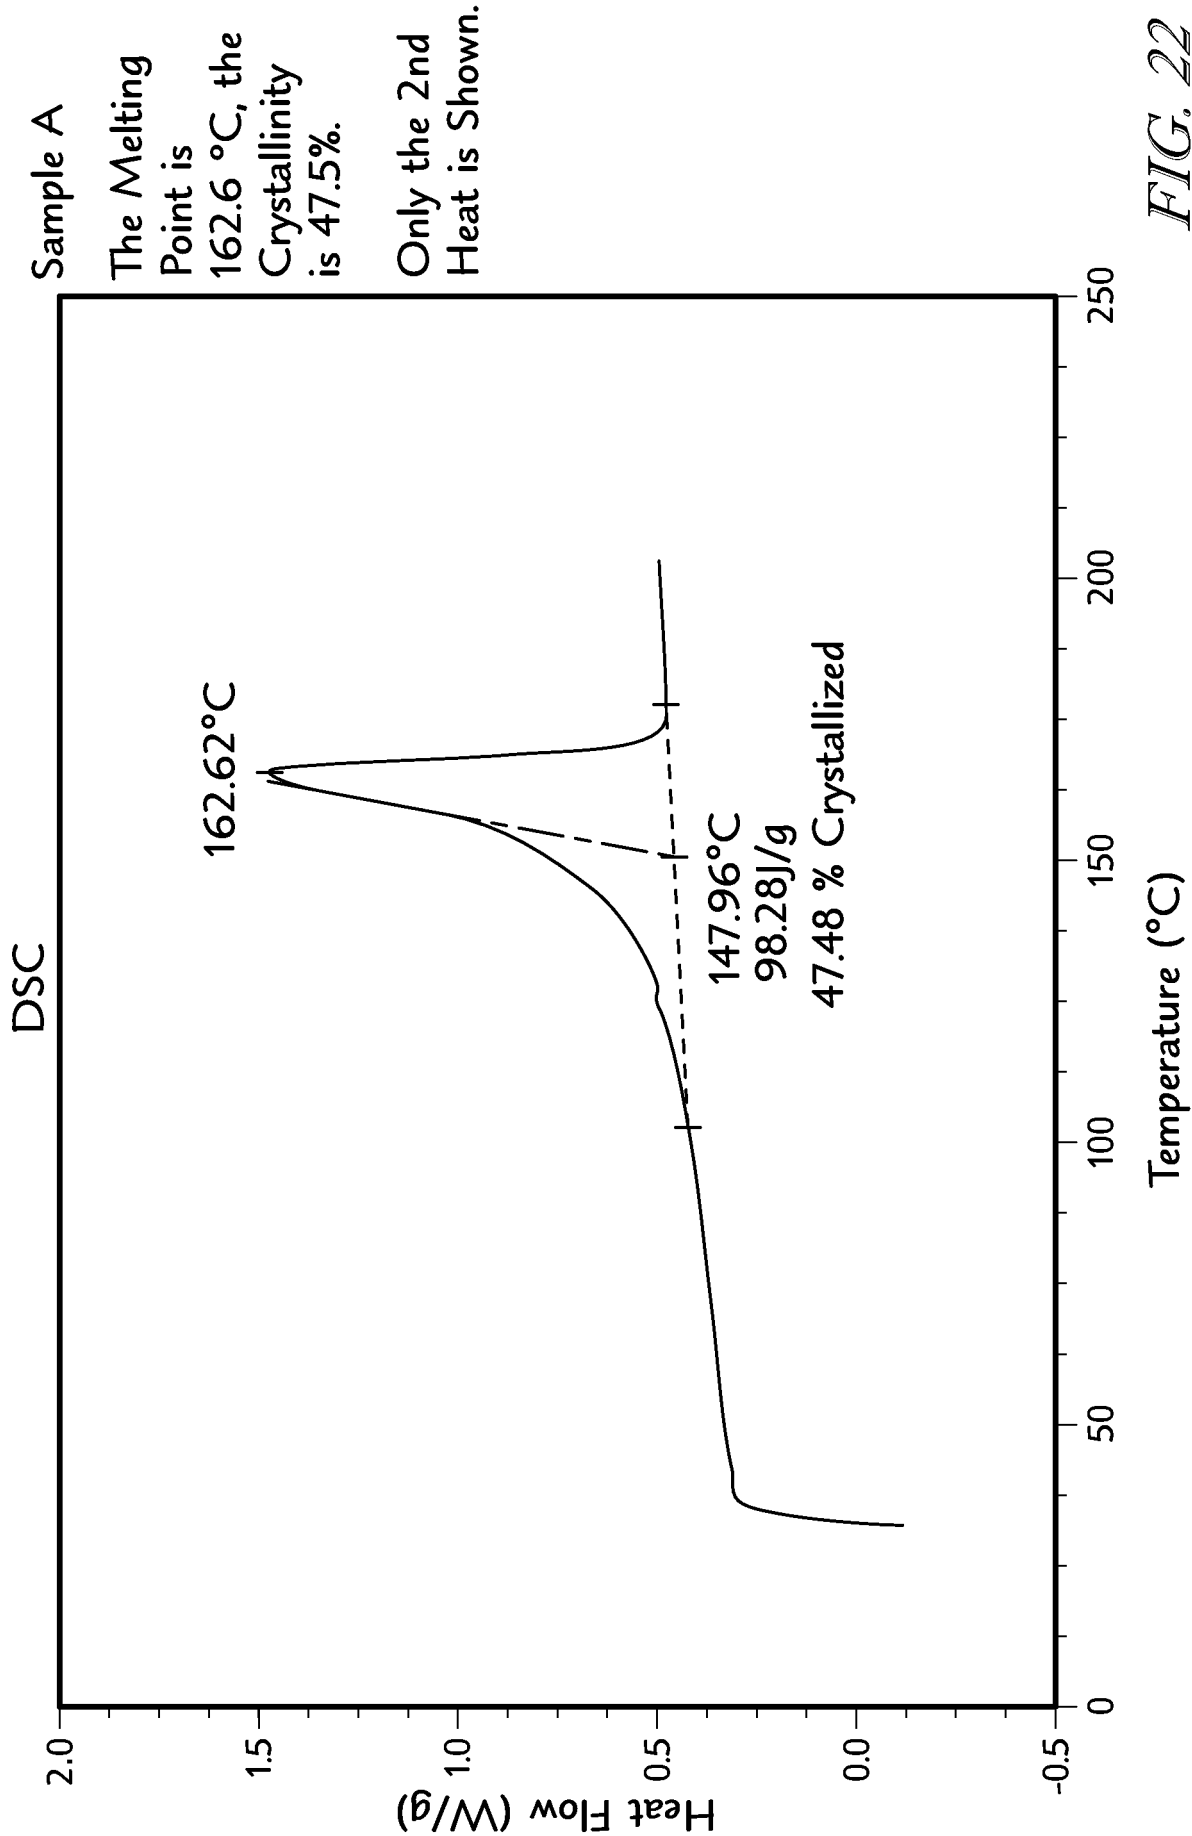


FIG. 21

Sample A DSC Test Result: Laboratory Testing Request 29016



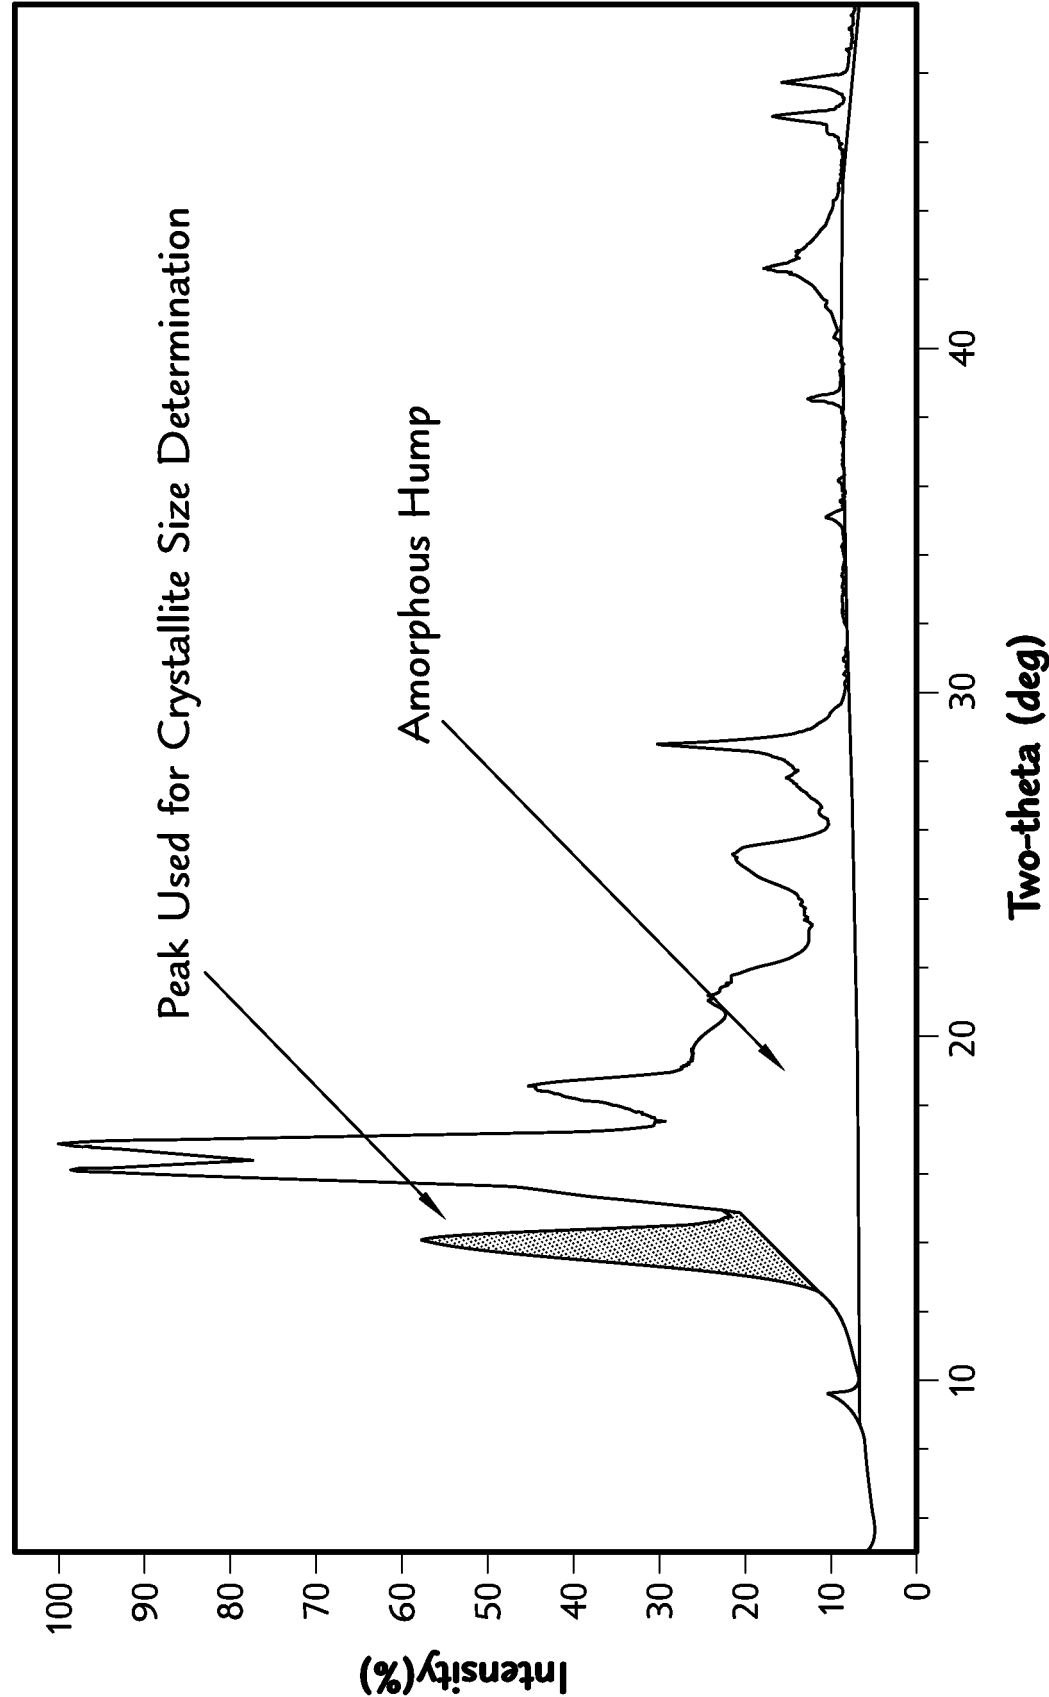


FIG. 23

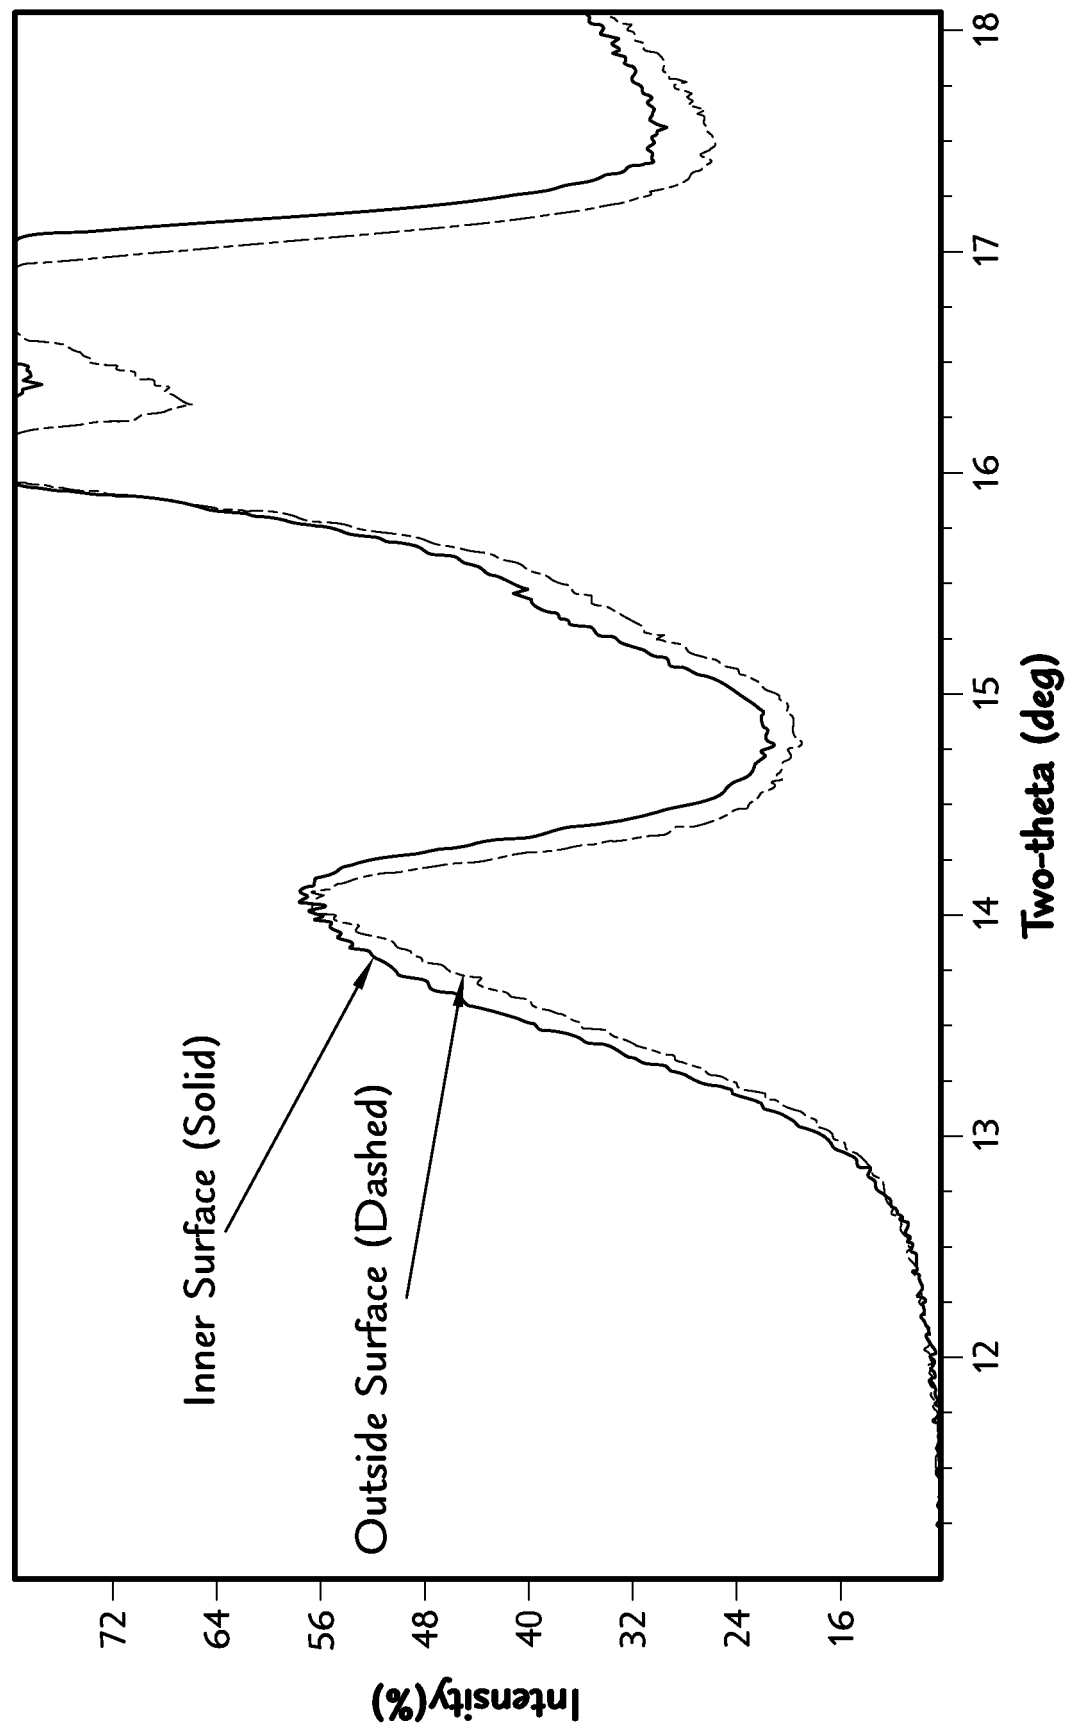


FIG. 24

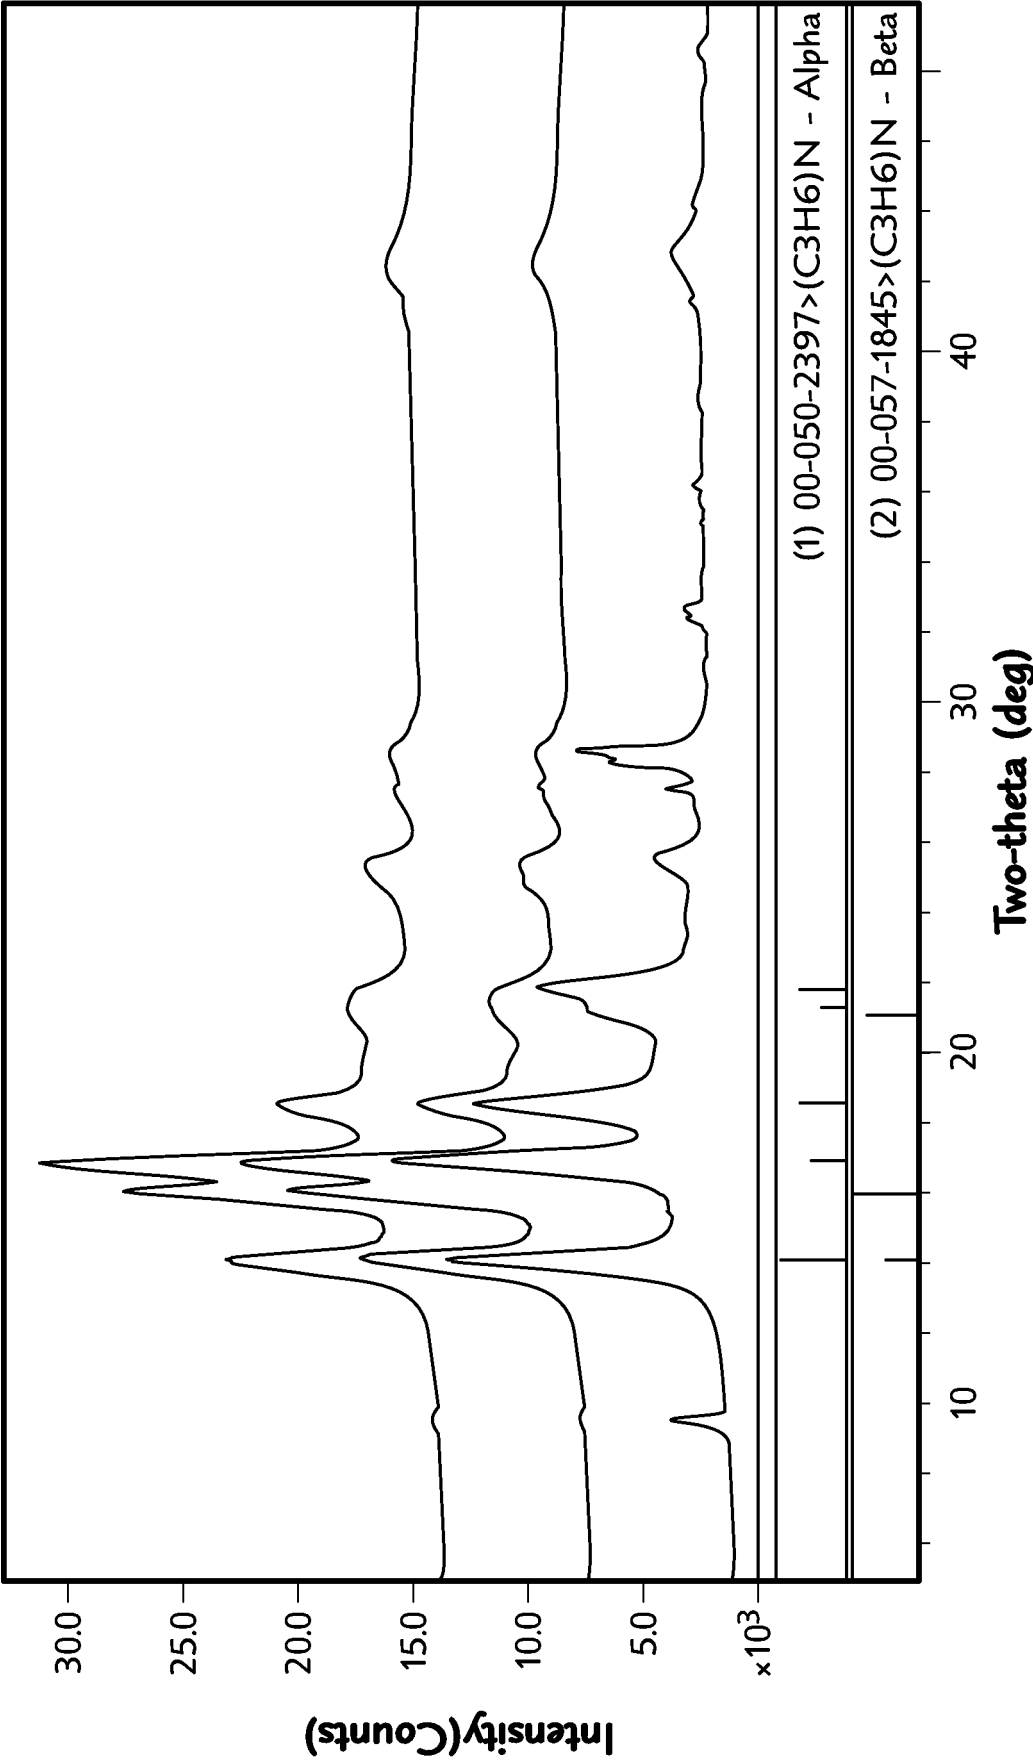


FIG. 25