

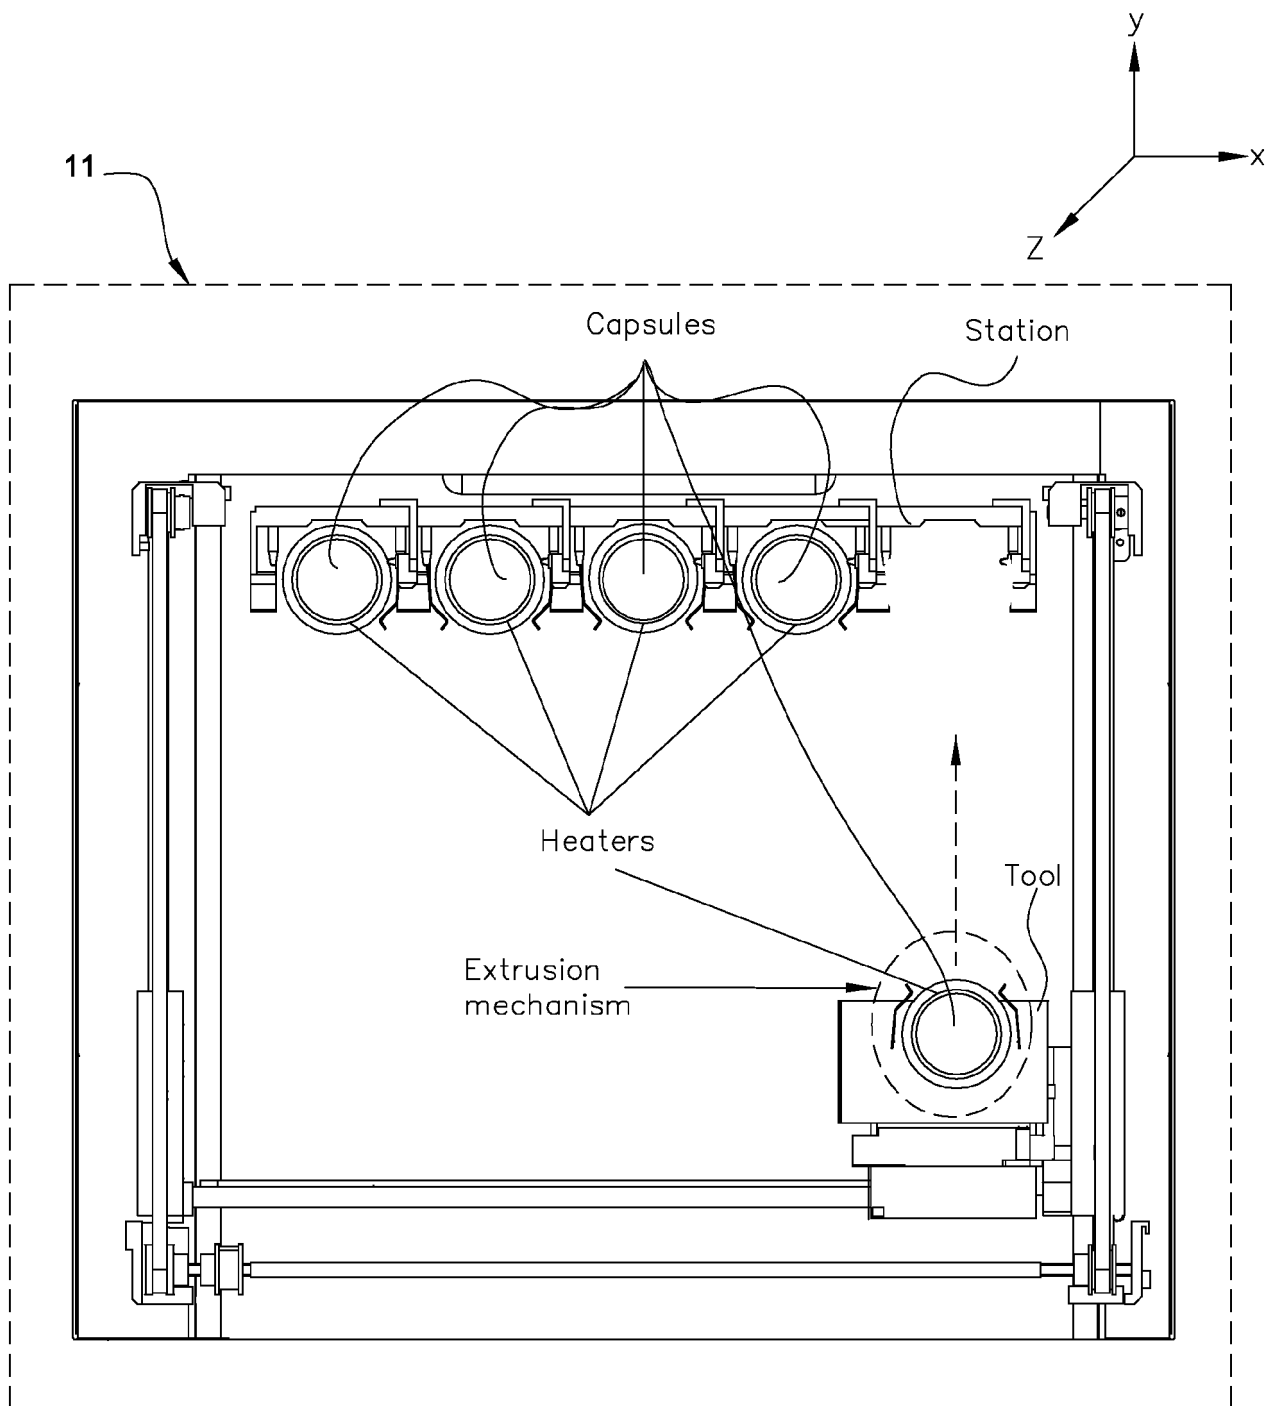


FIG. 1A

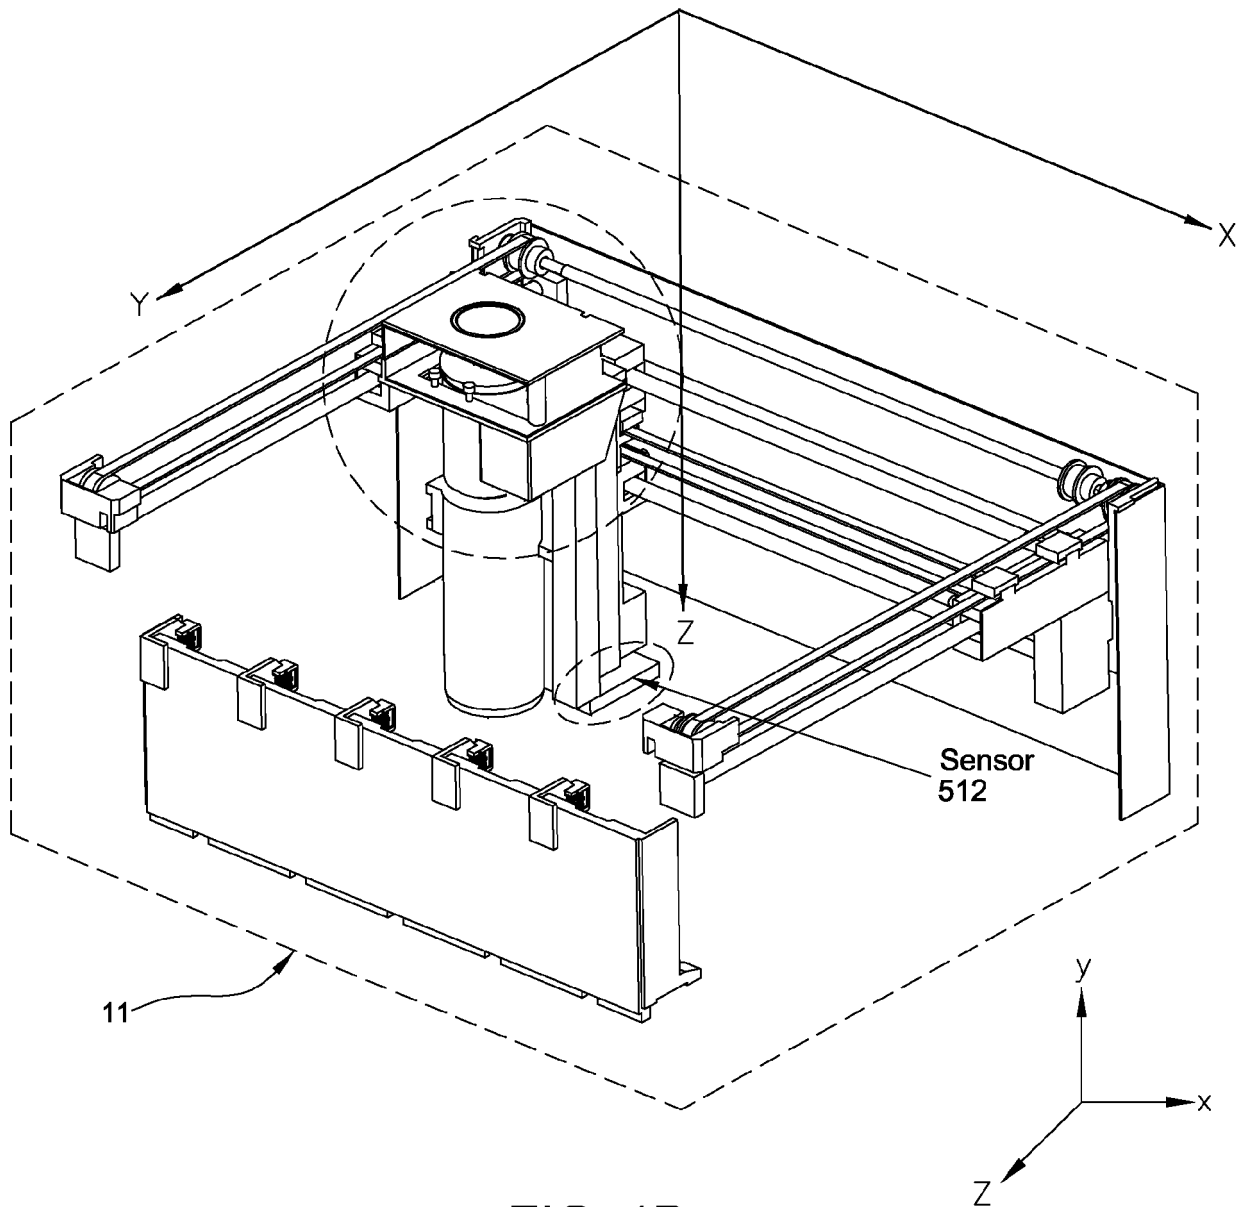


FIG. 1B

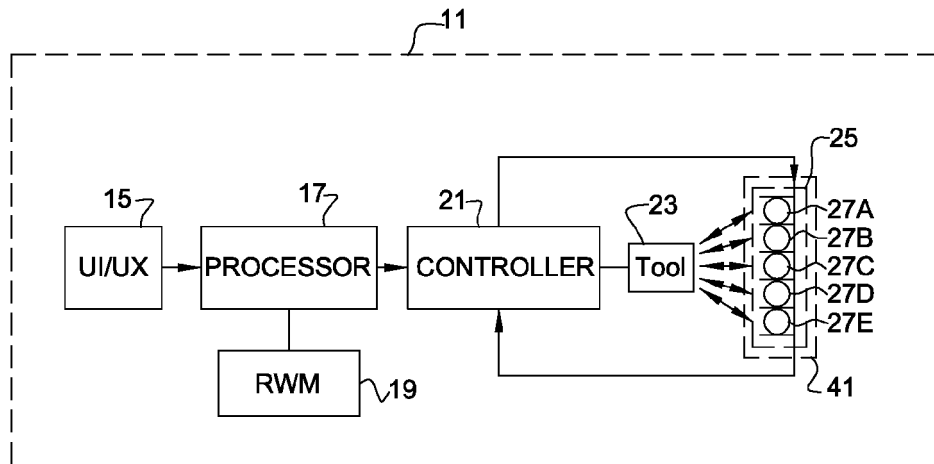


FIG. 2A

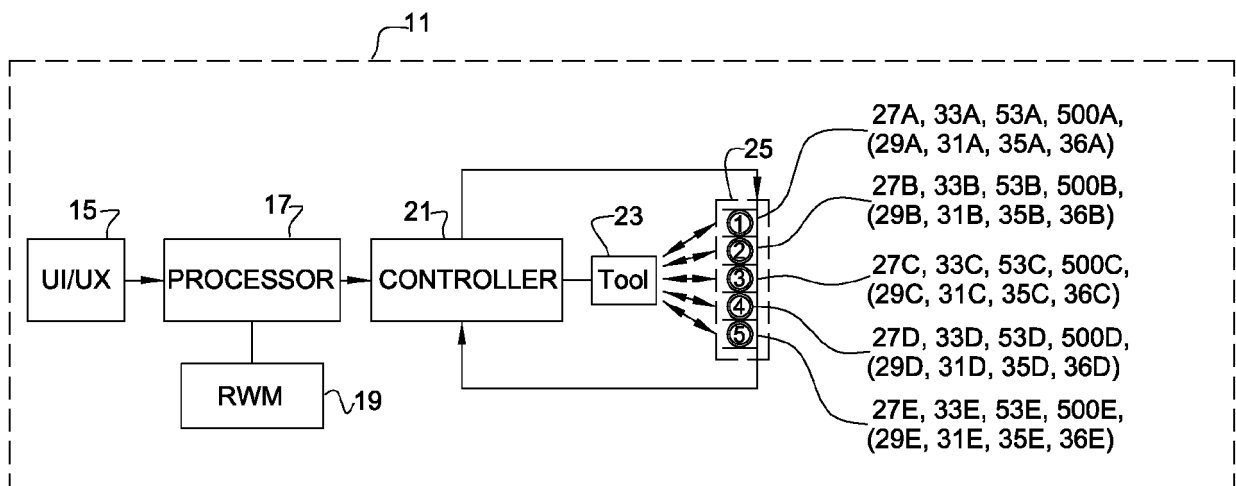


FIG. 2B

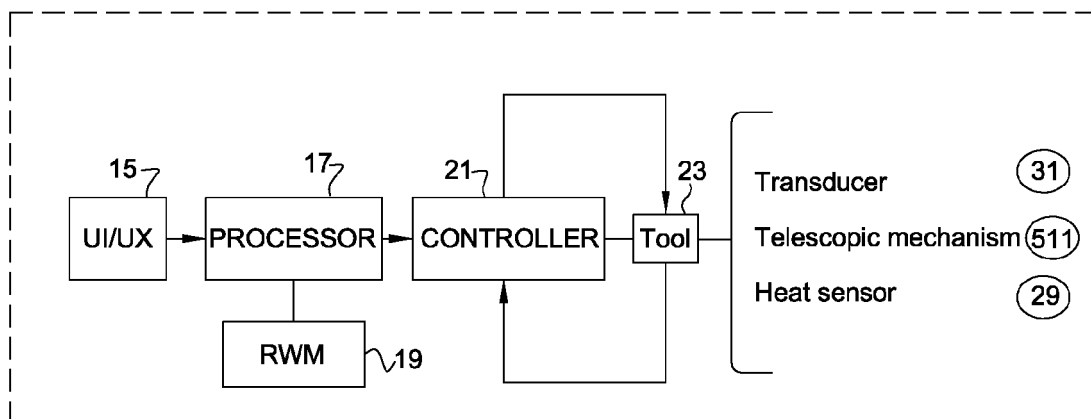
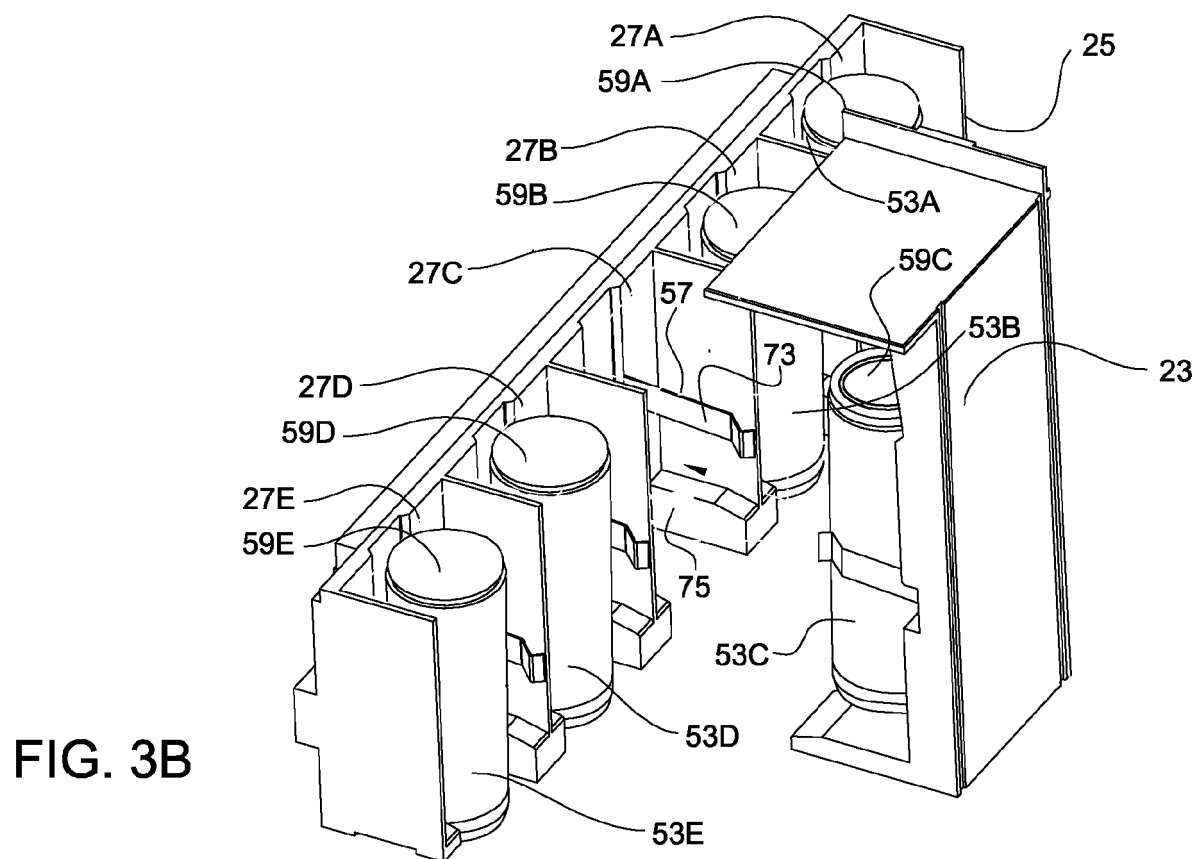
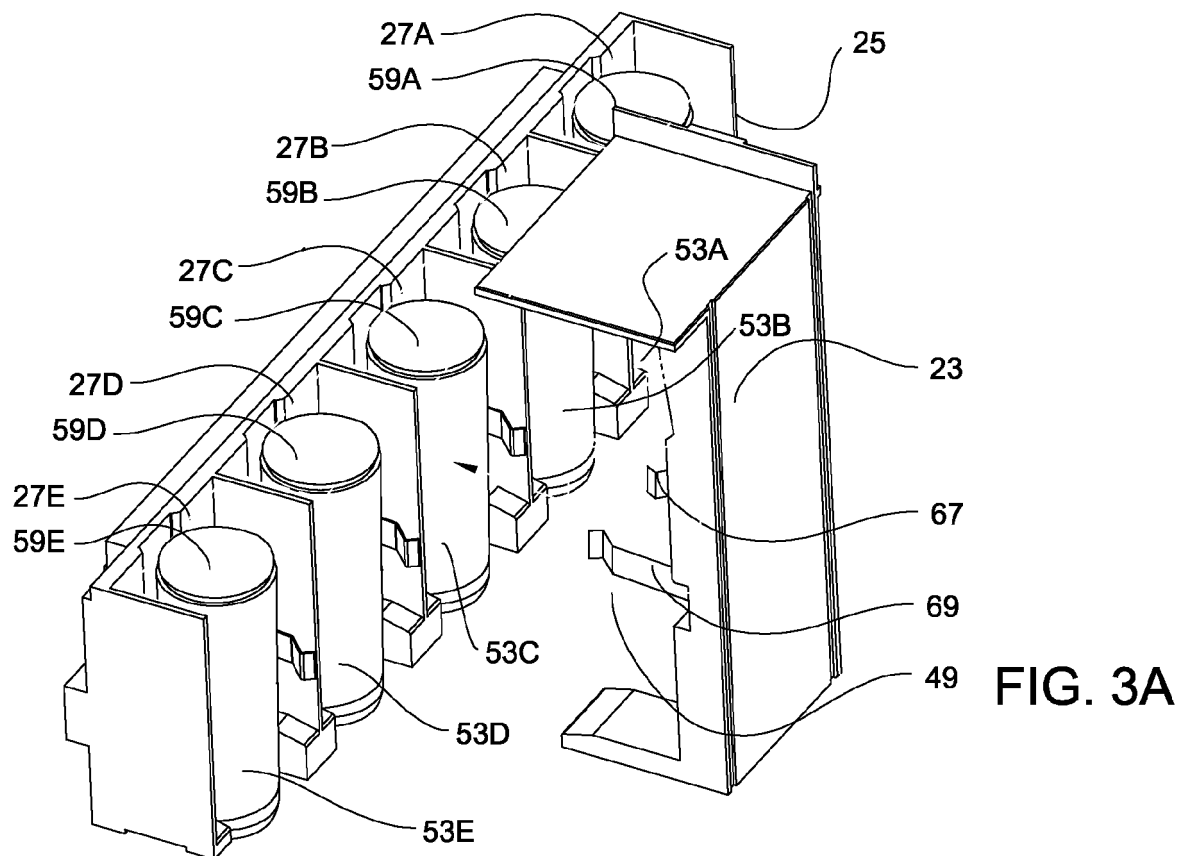


FIG. 2C

4/15



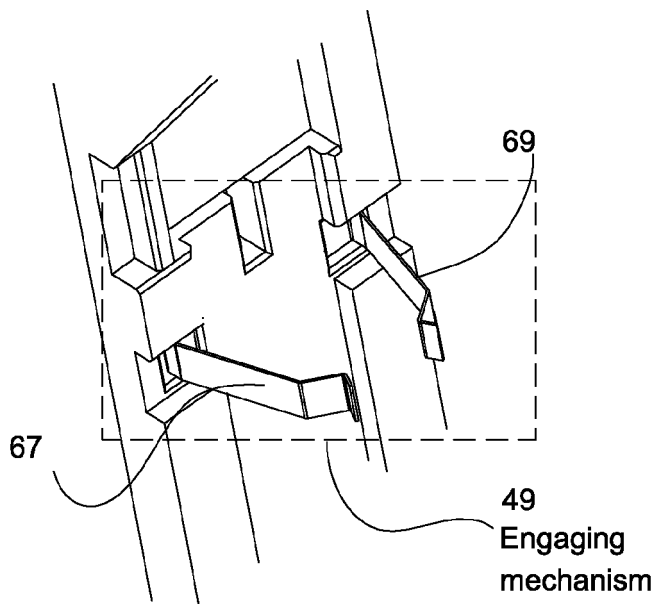


FIG. 4A

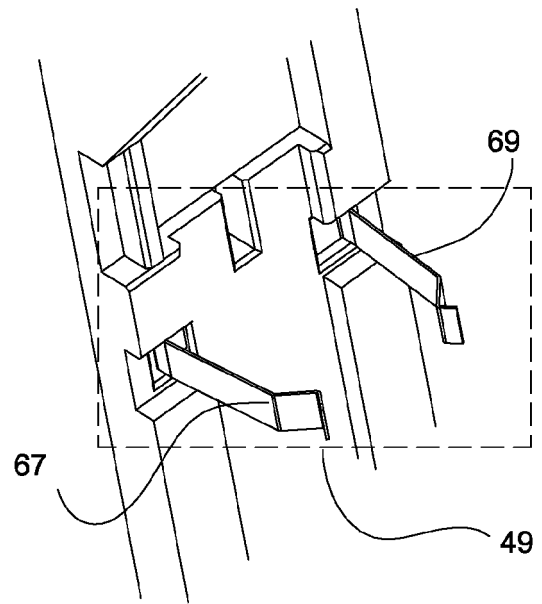


FIG. 4B

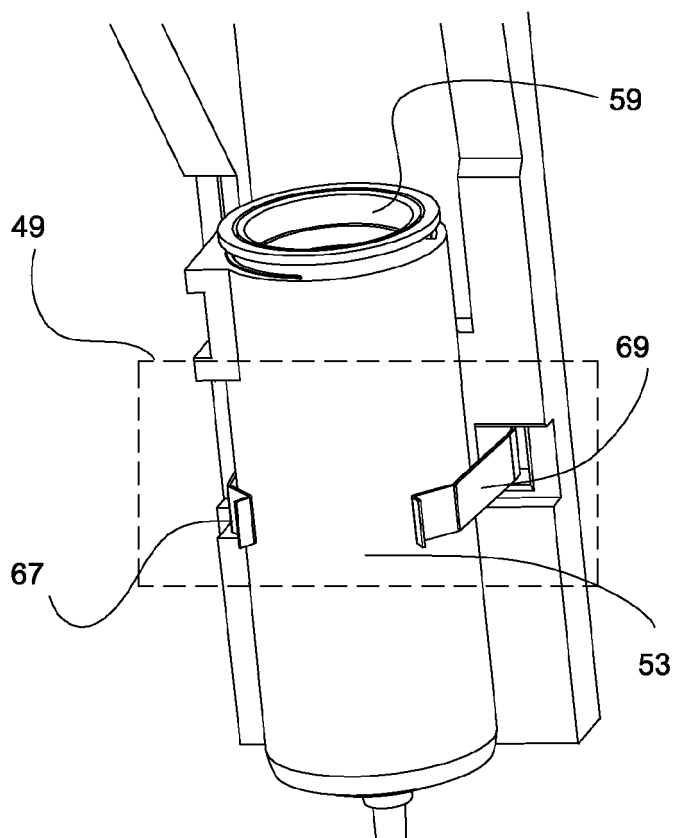


FIG. 4C

6/15

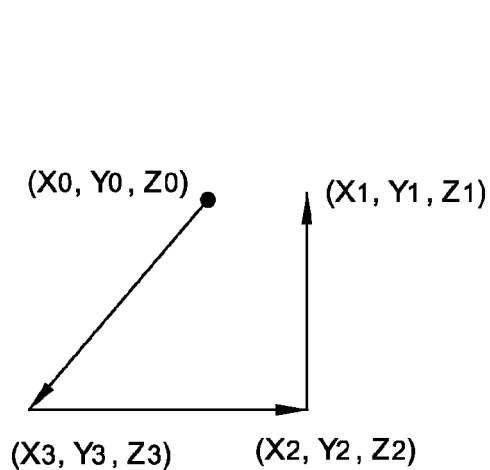


FIG. 5A

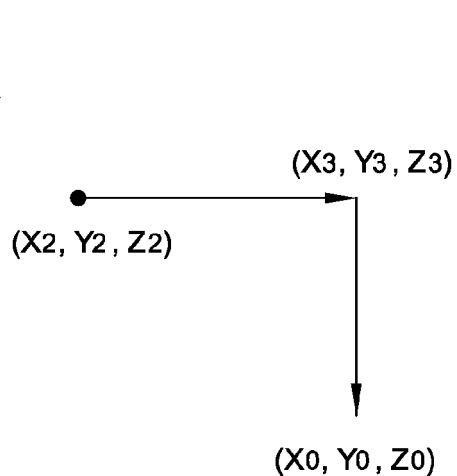


FIG. 5B

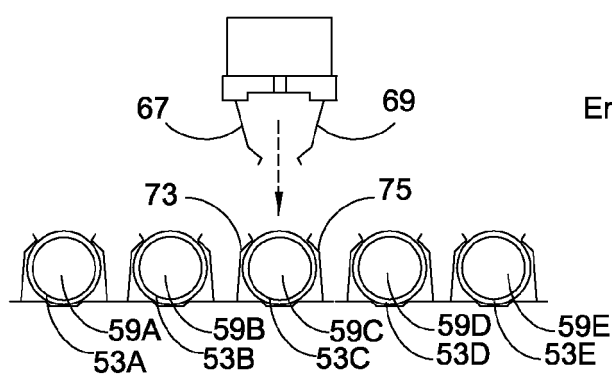


FIG. 6A

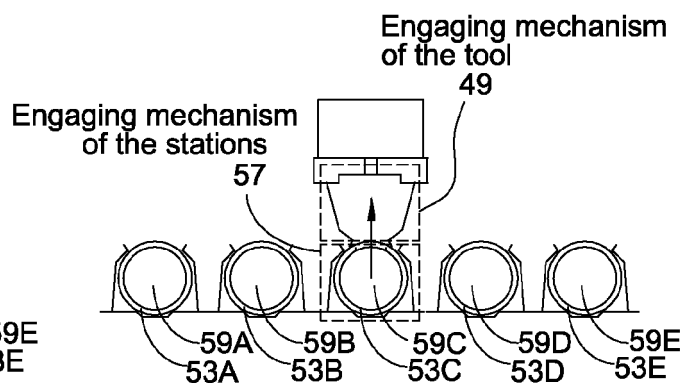


FIG. 6C

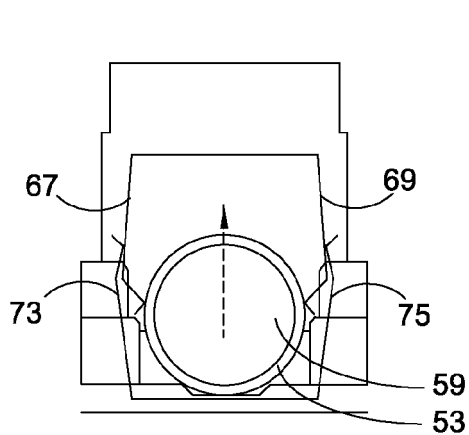


FIG. 6B

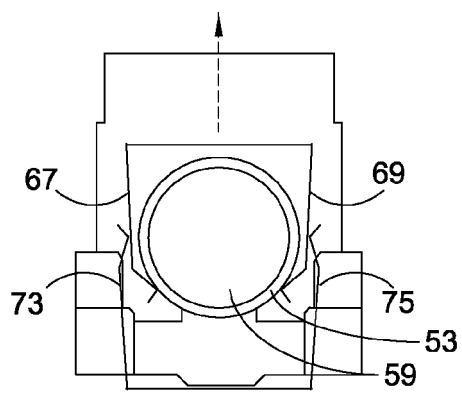


FIG. 6D

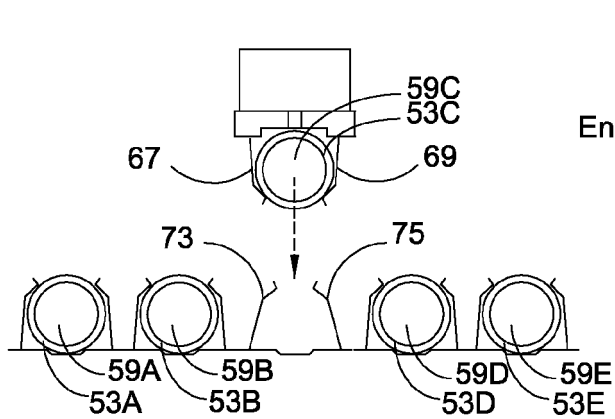


FIG. 7A

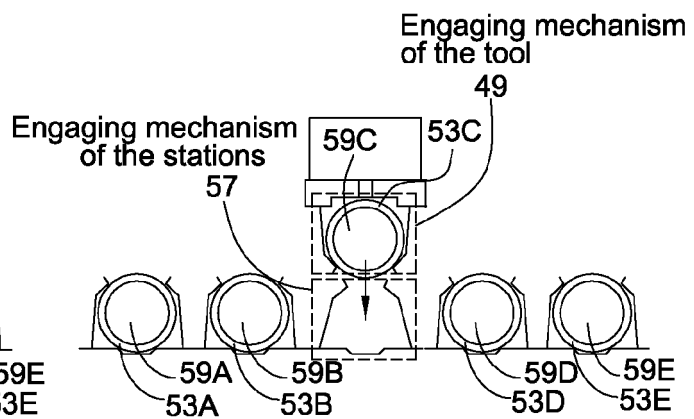


FIG. 7C

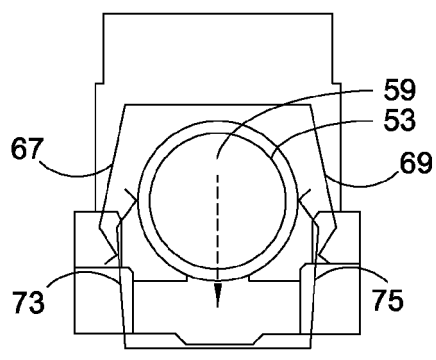


FIG. 7B

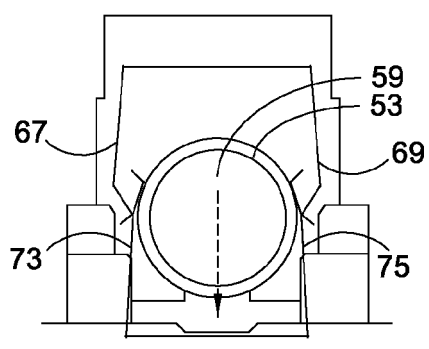


FIG. 7D



FIG. 8

8/15

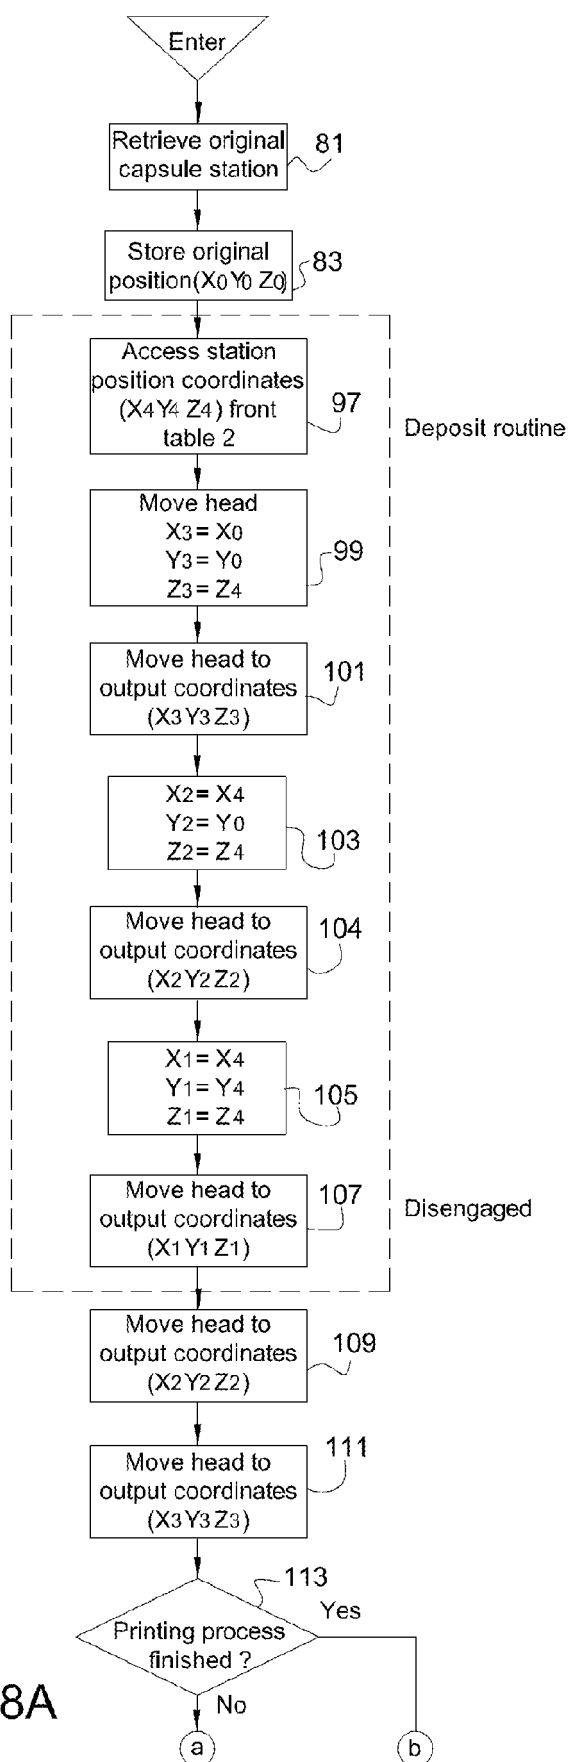


FIG. 8A

9/15

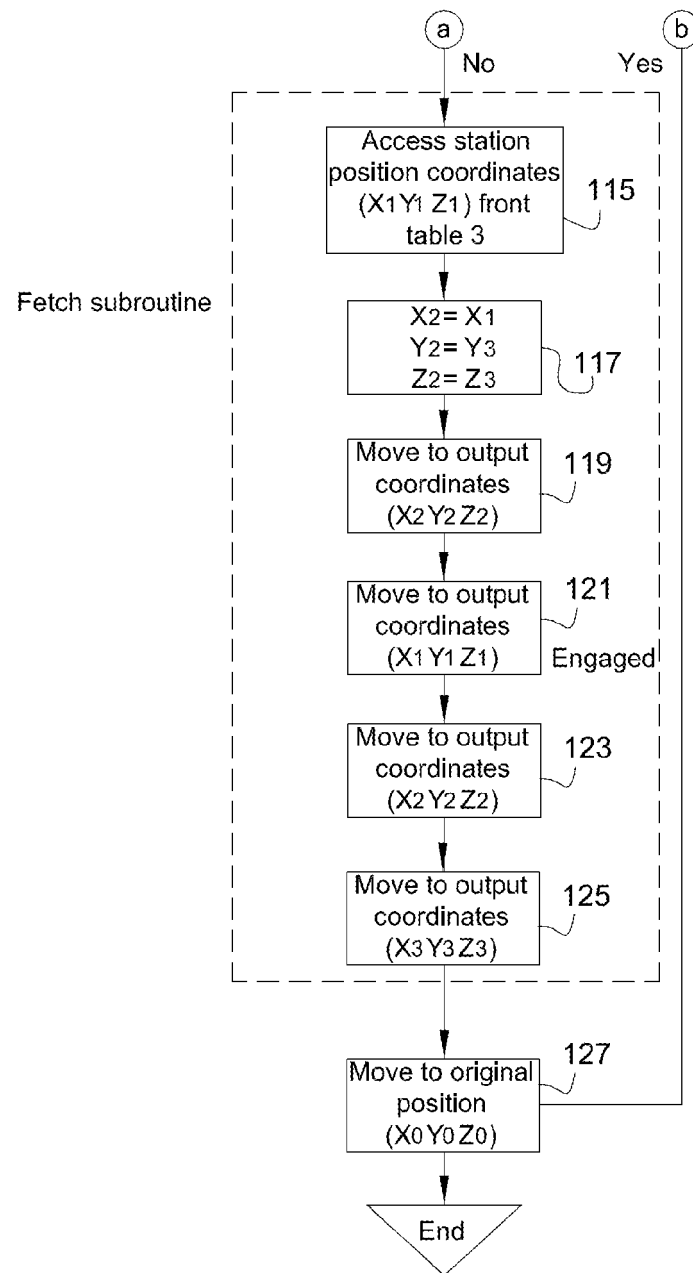


FIG. 8B

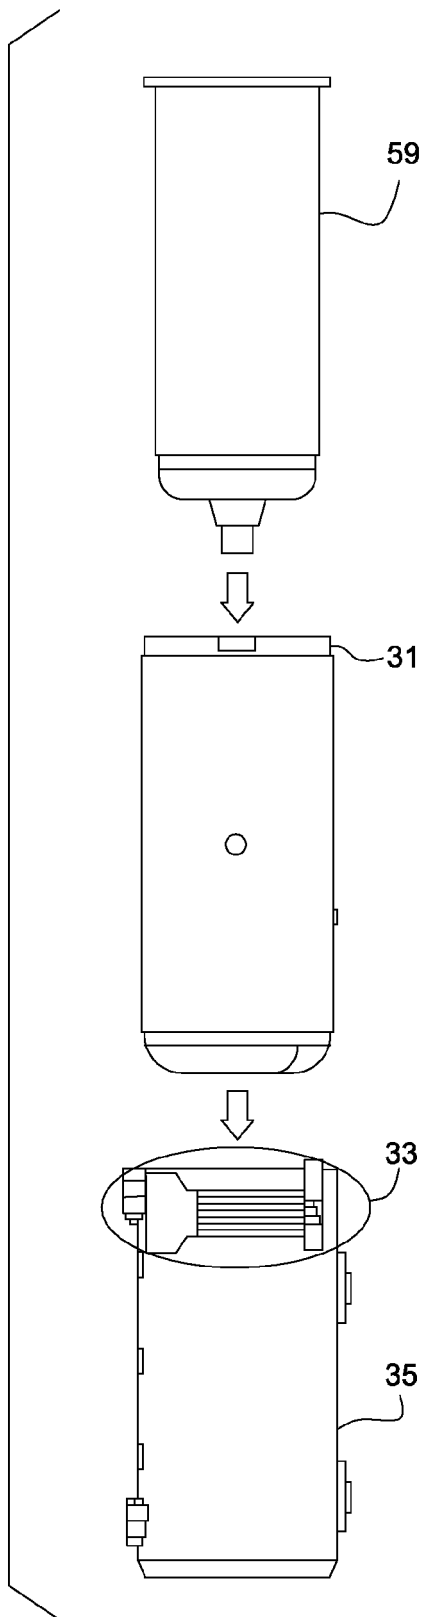


FIG. 9A

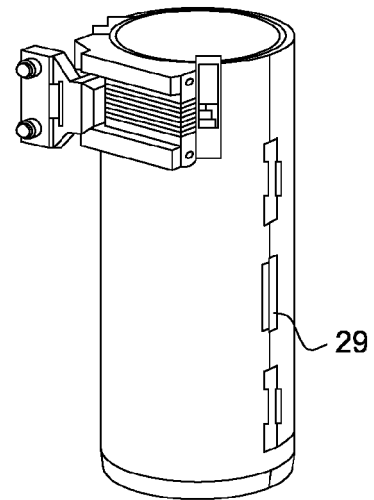


FIG. 9B

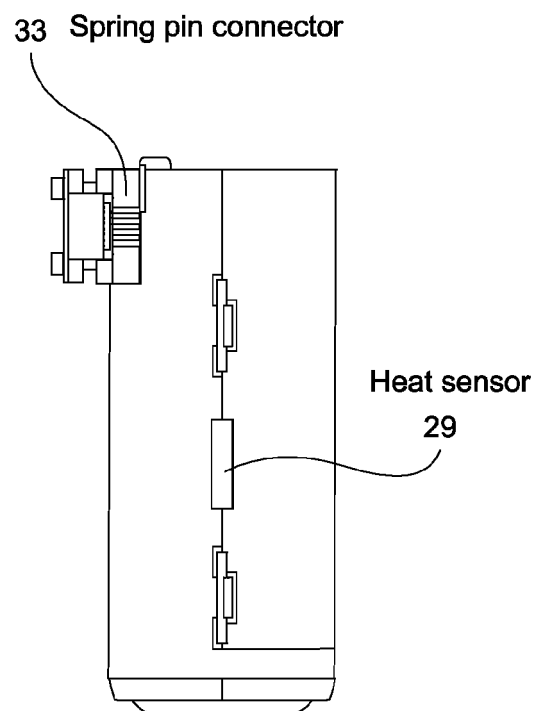


FIG. 9C

11/15

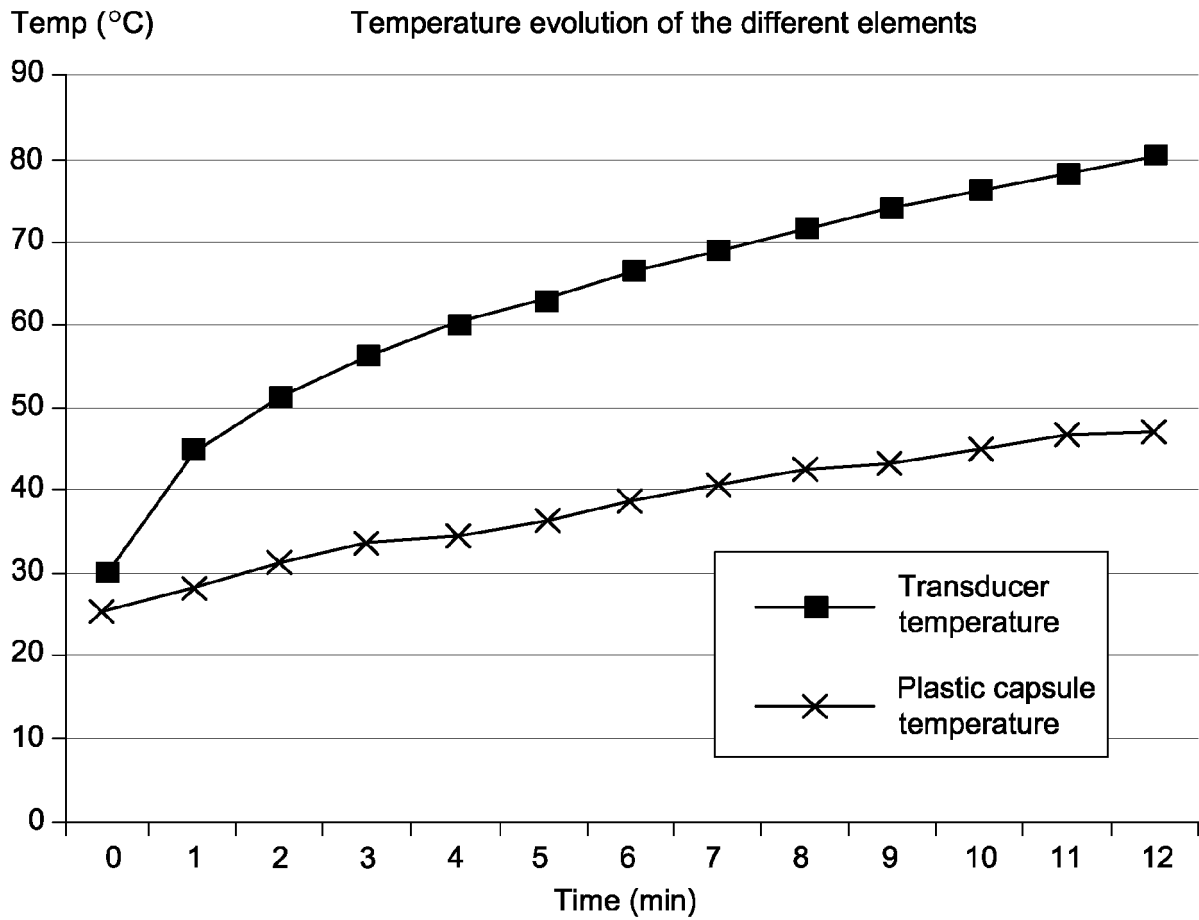


FIG. 10

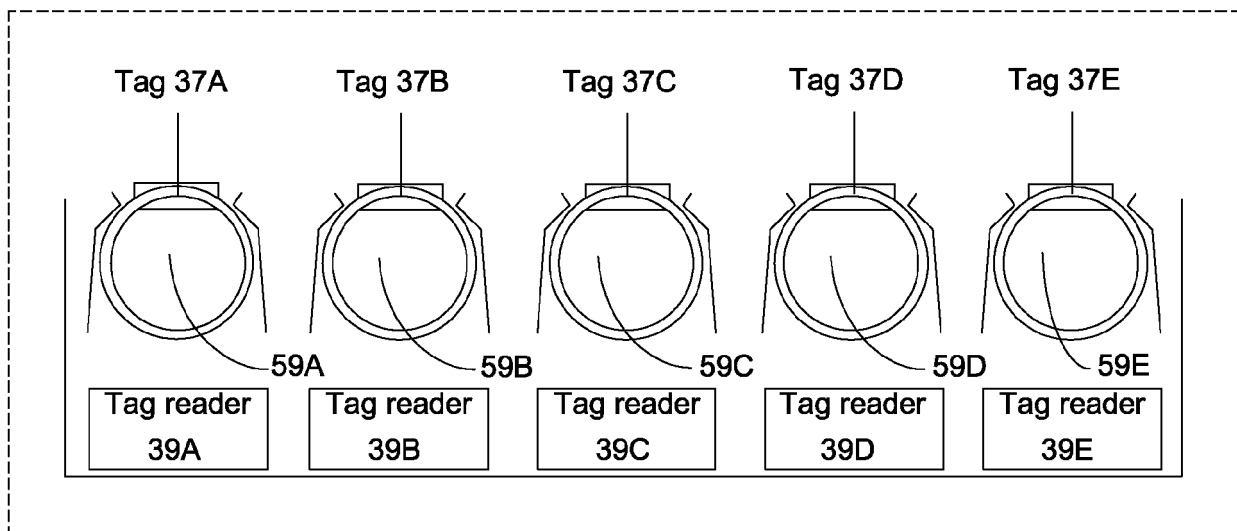


FIG. 14

41
Capsule identification
system

12/15

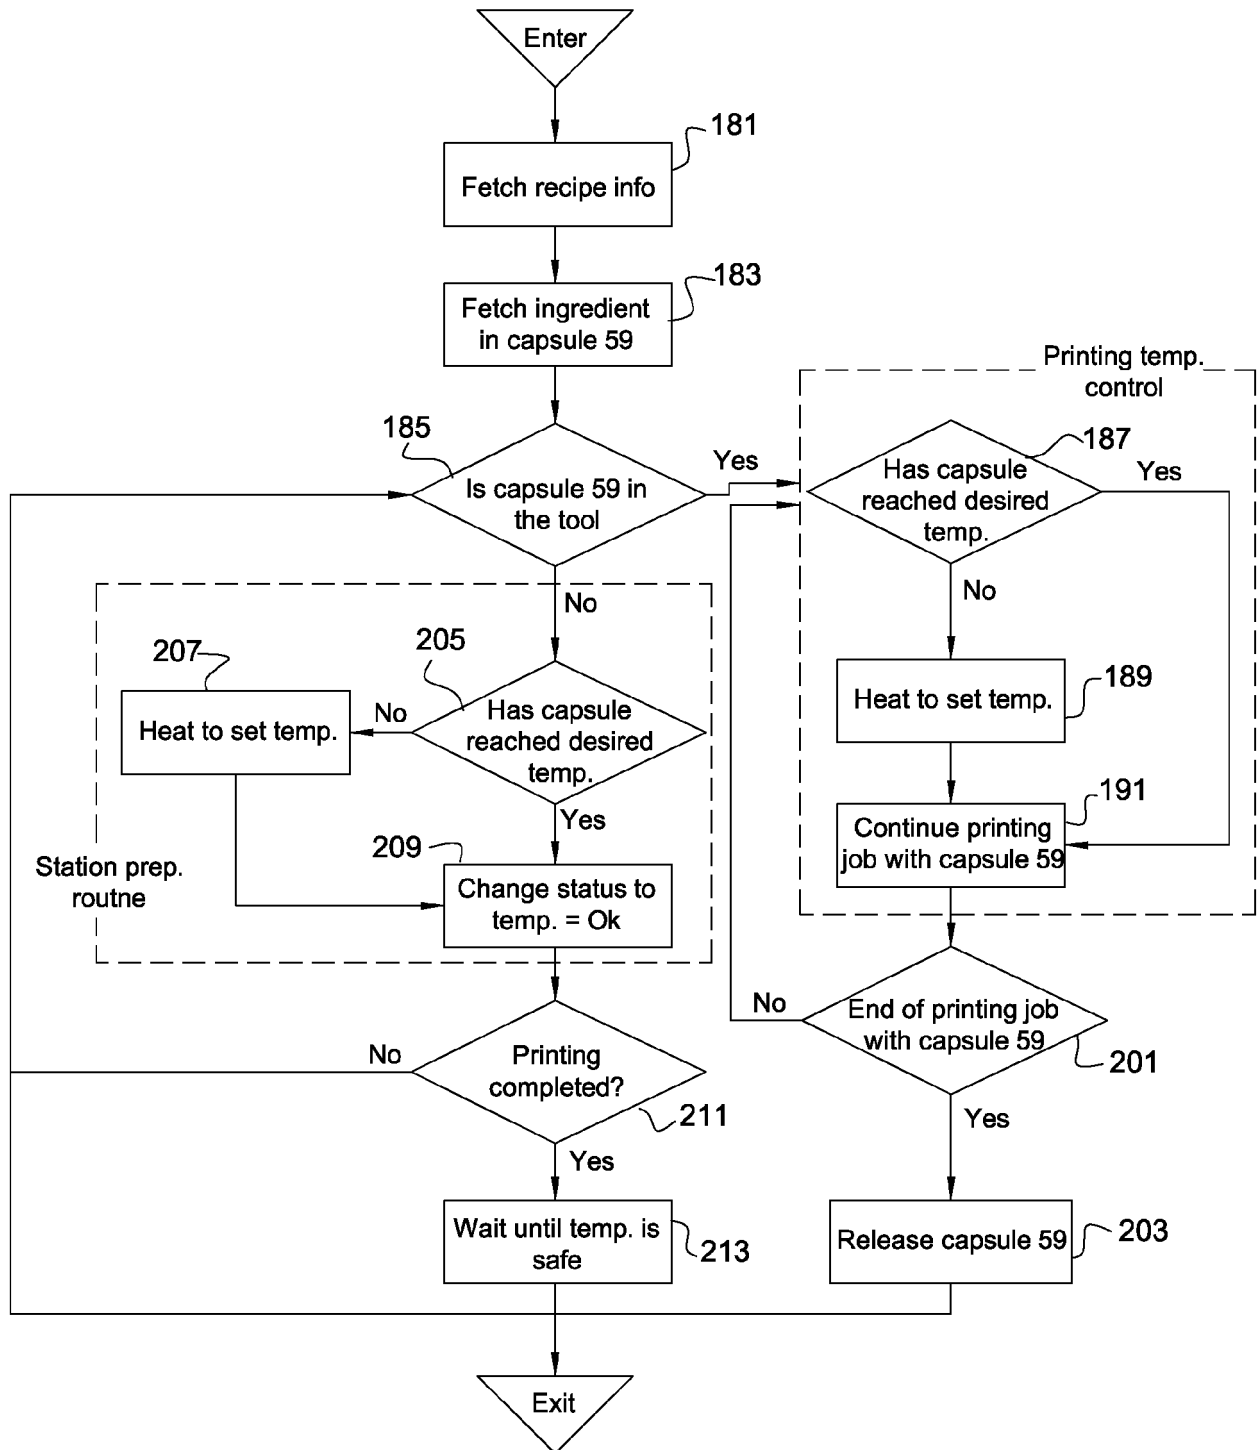


FIG. 11

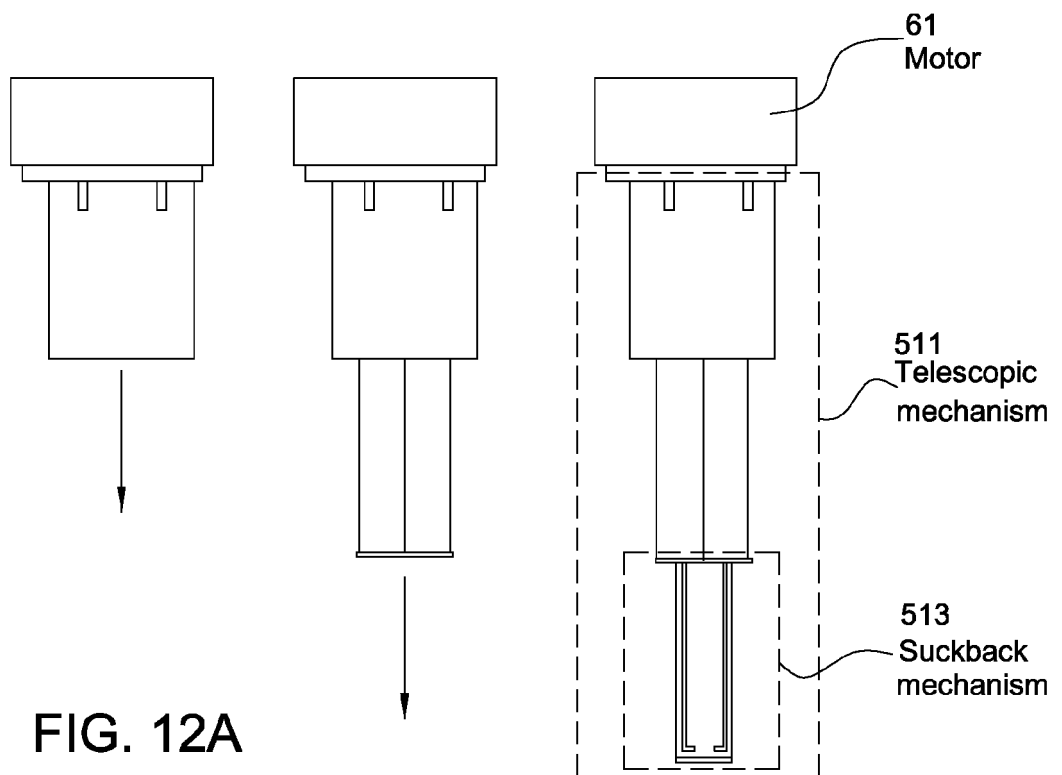


FIG. 12A

FIG. 12B

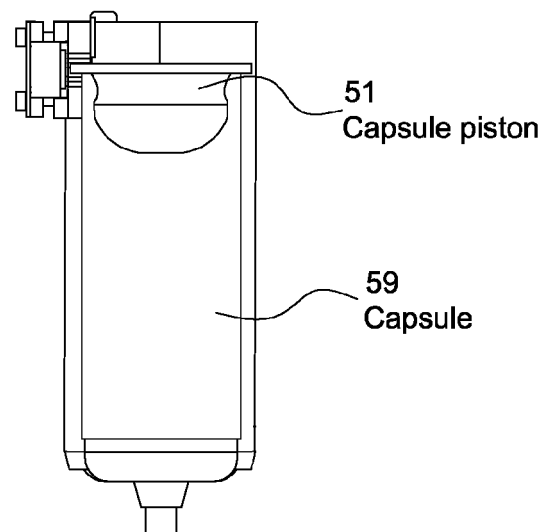


FIG. 12C

14/15

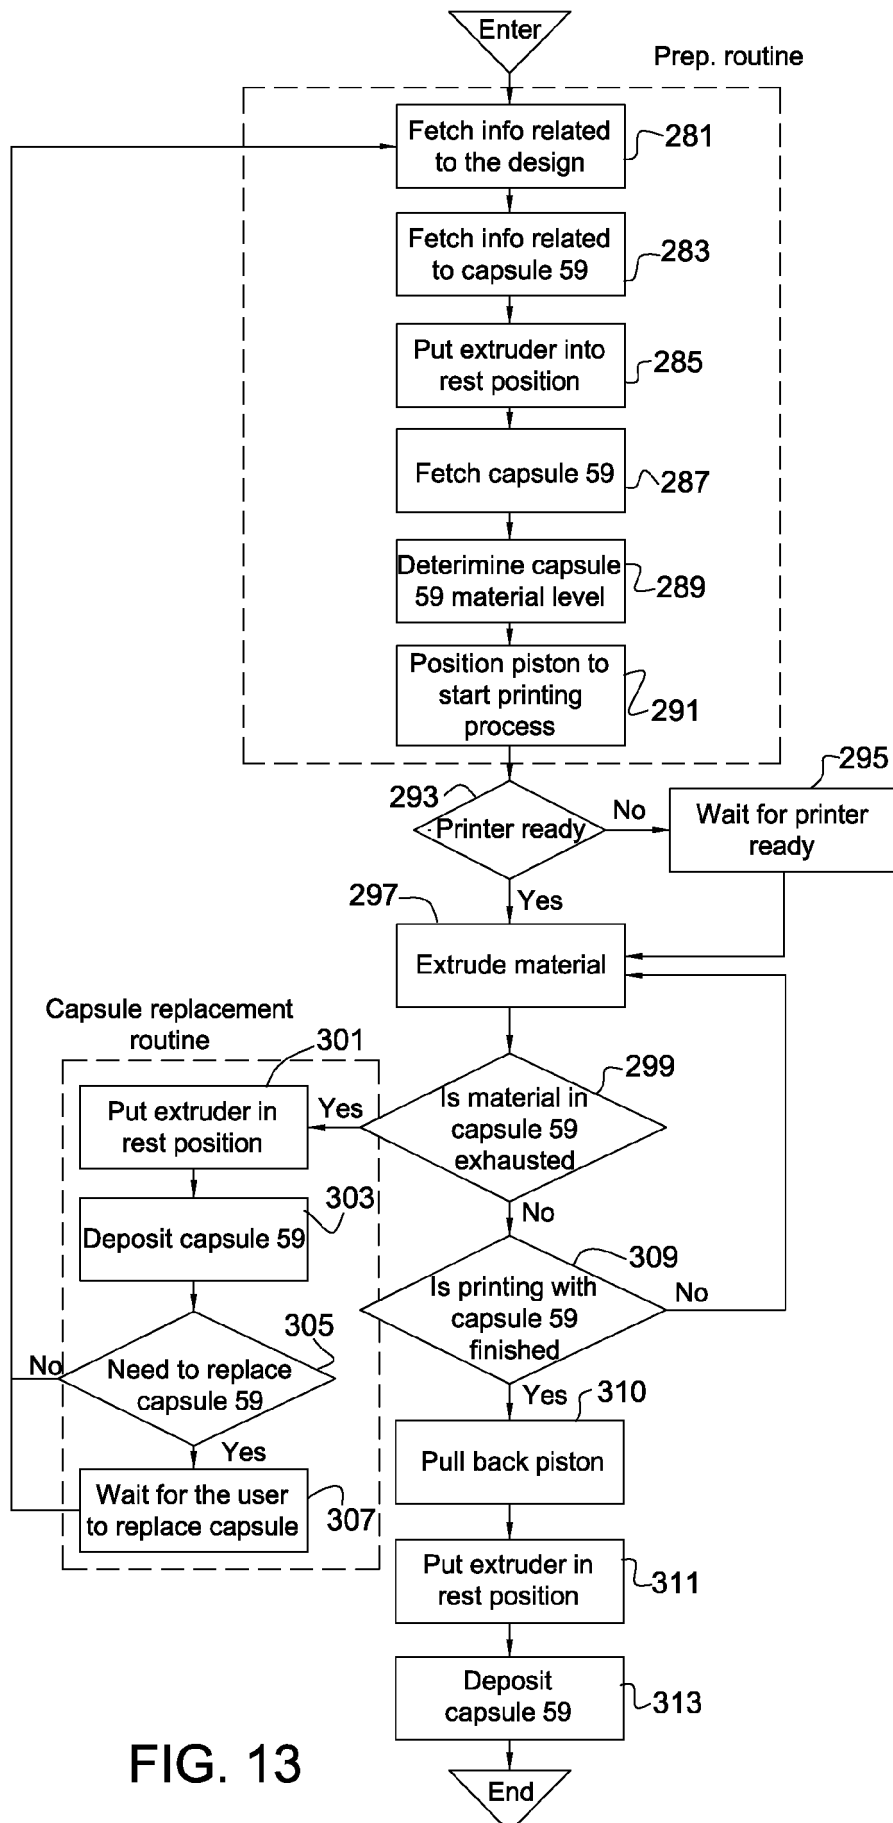


FIG. 13

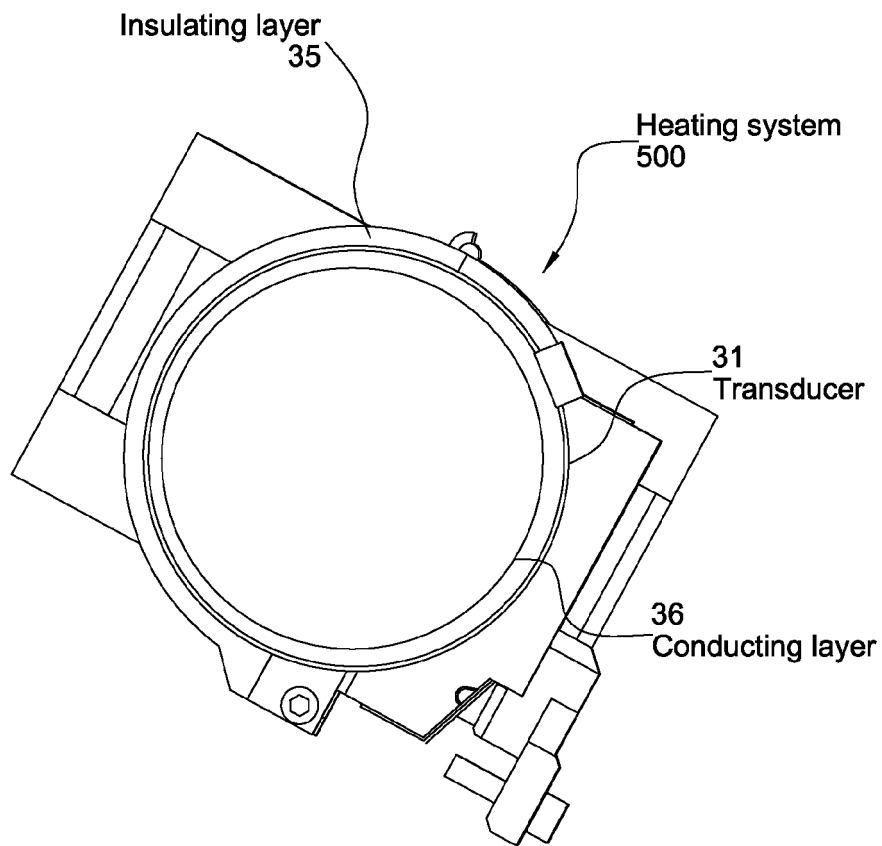


FIG. 15