

1/26

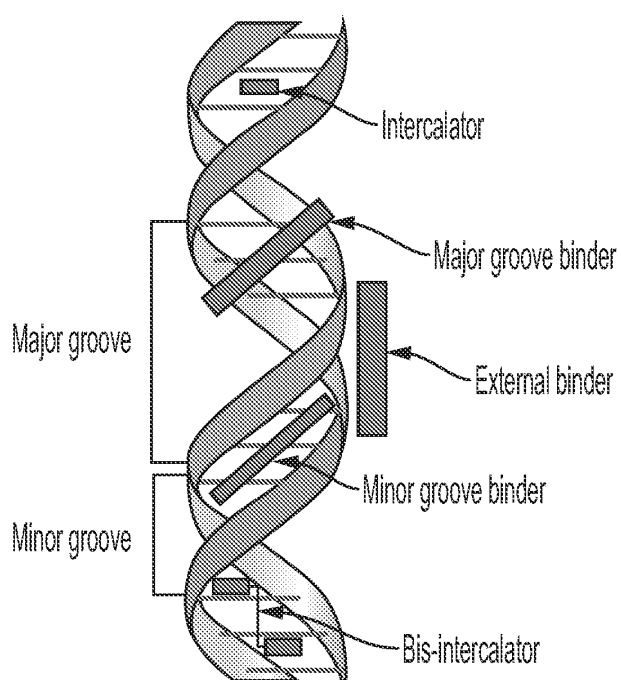


FIG. 1A

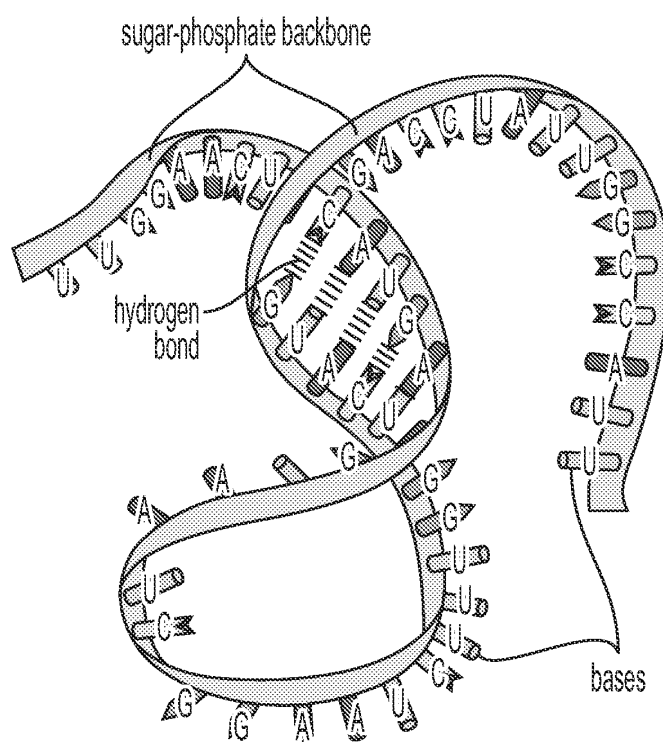


FIG. 1B

2/26

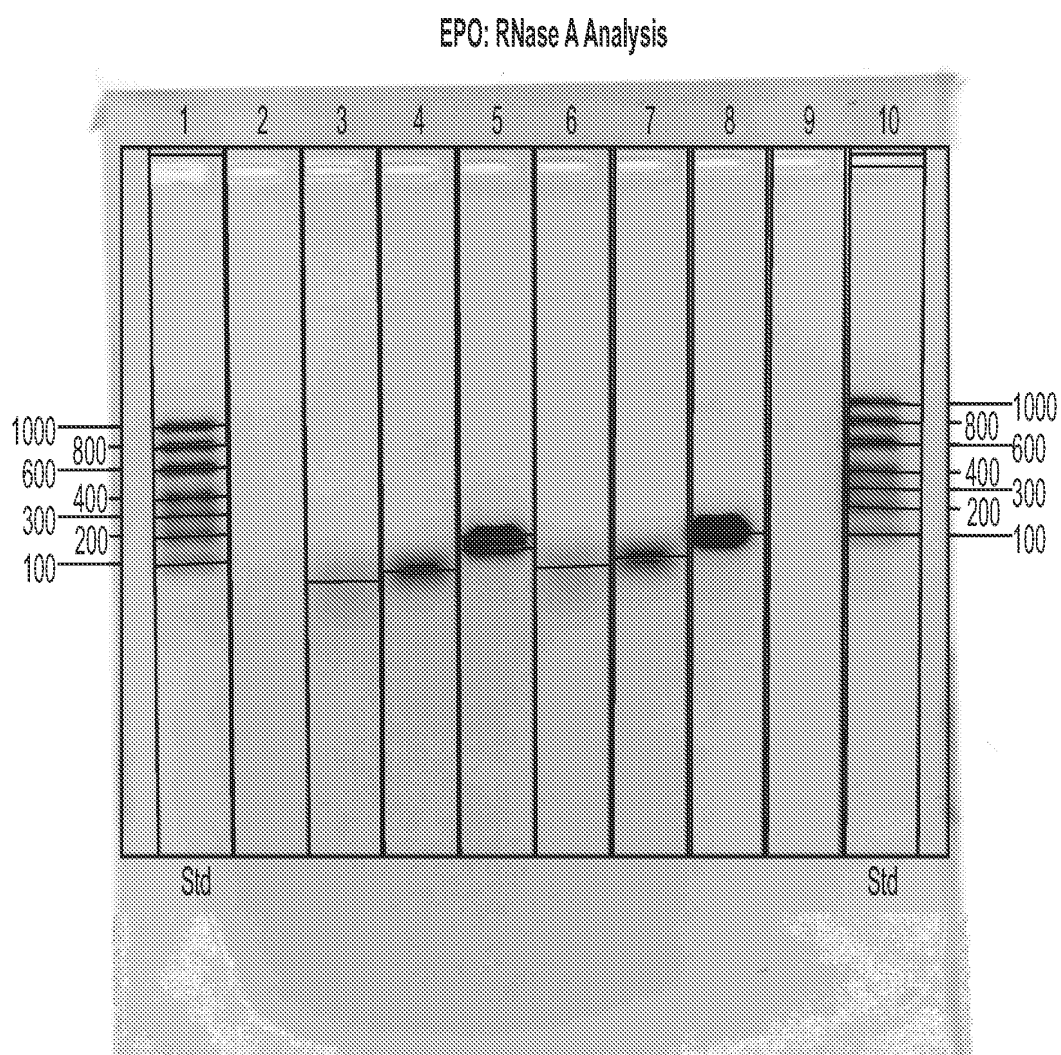


FIG. 2A

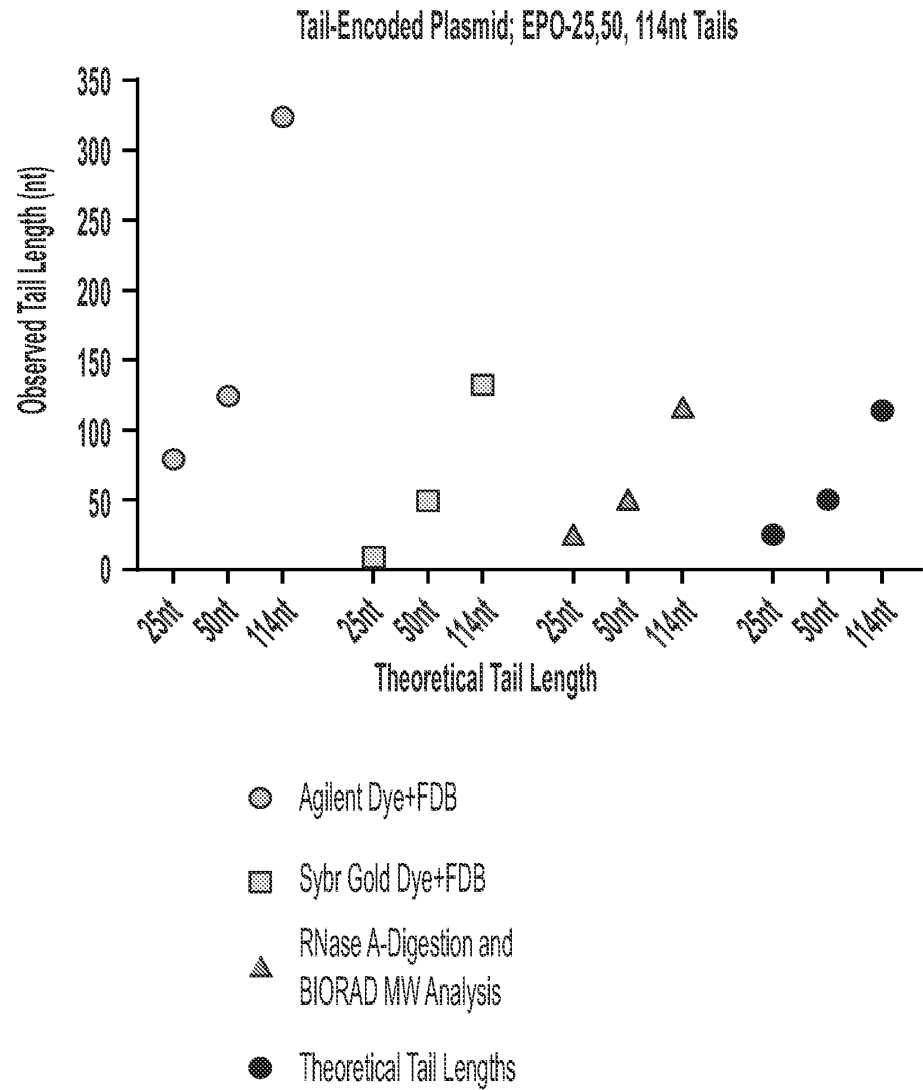


FIG. 2B

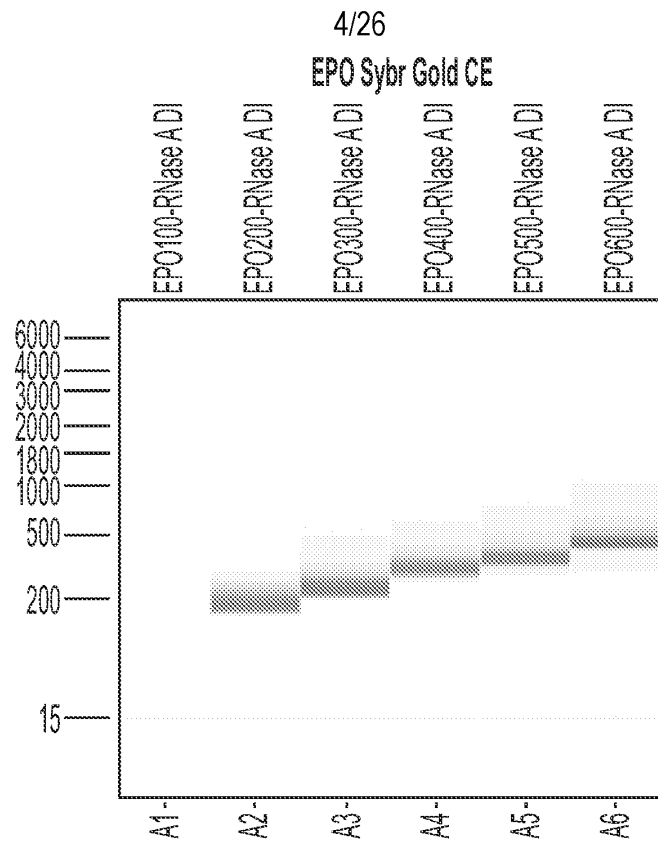


FIG. 3A

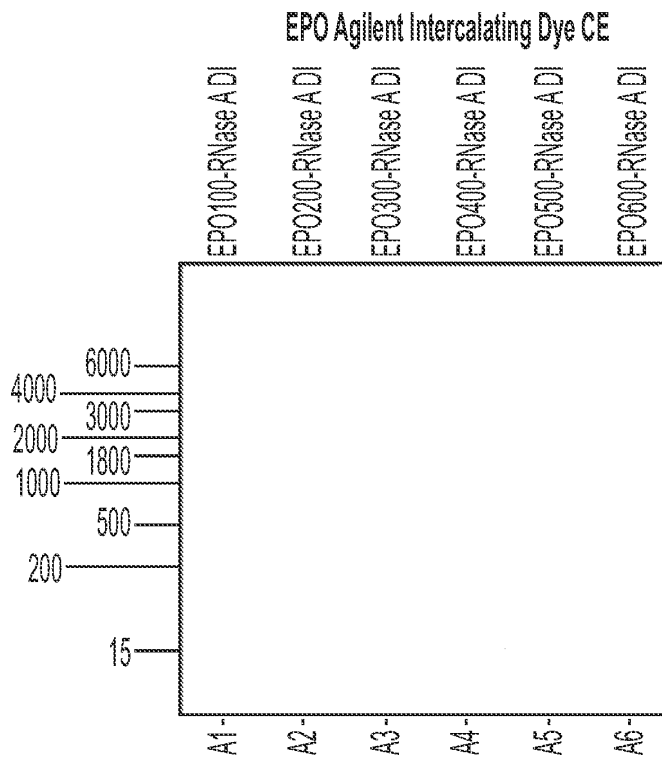


FIG. 3B

5/26

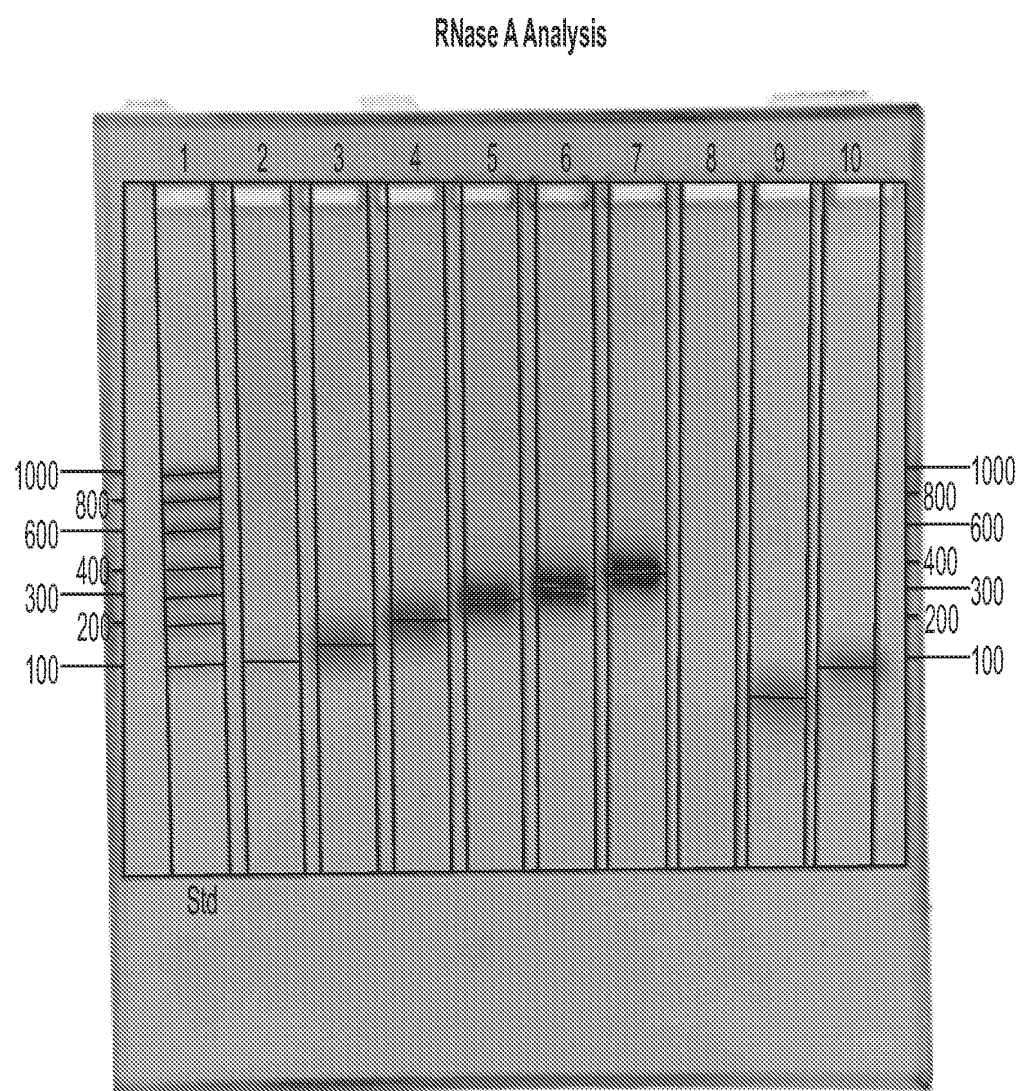


FIG. 4A

6/26


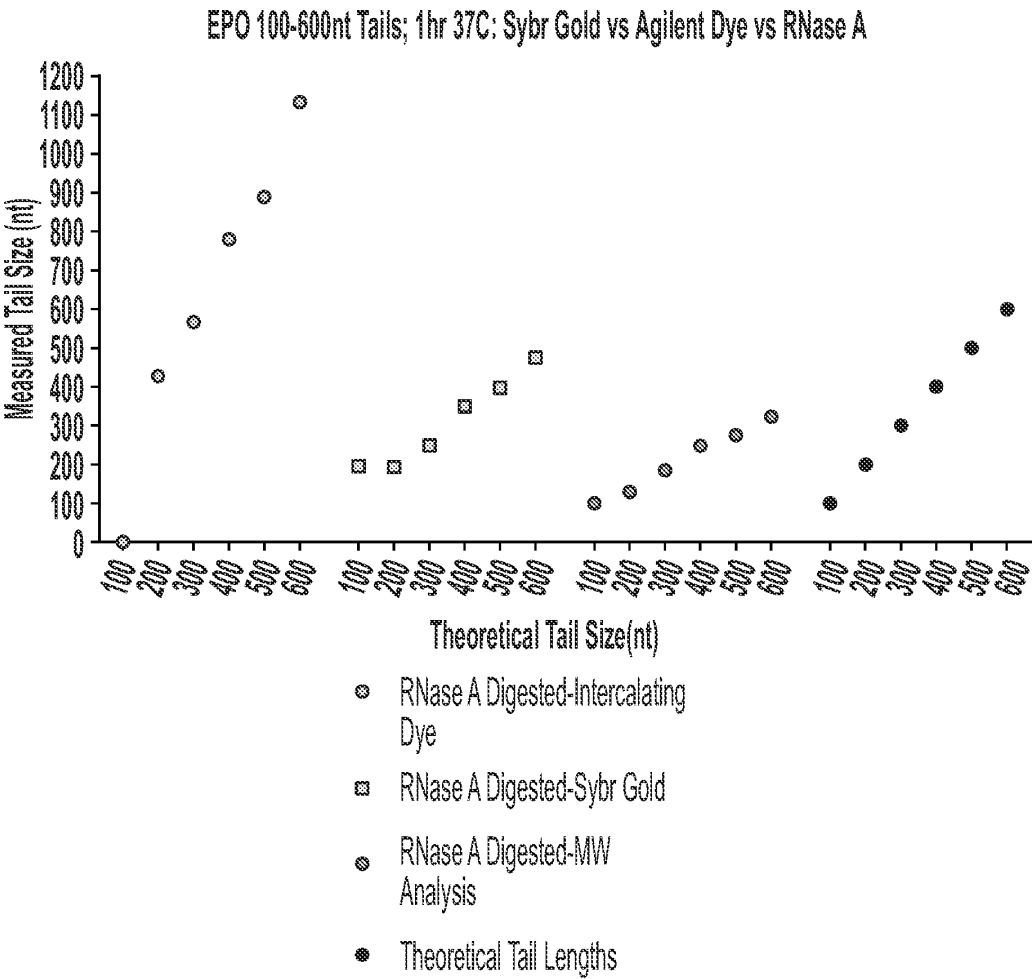


FIG. 4B

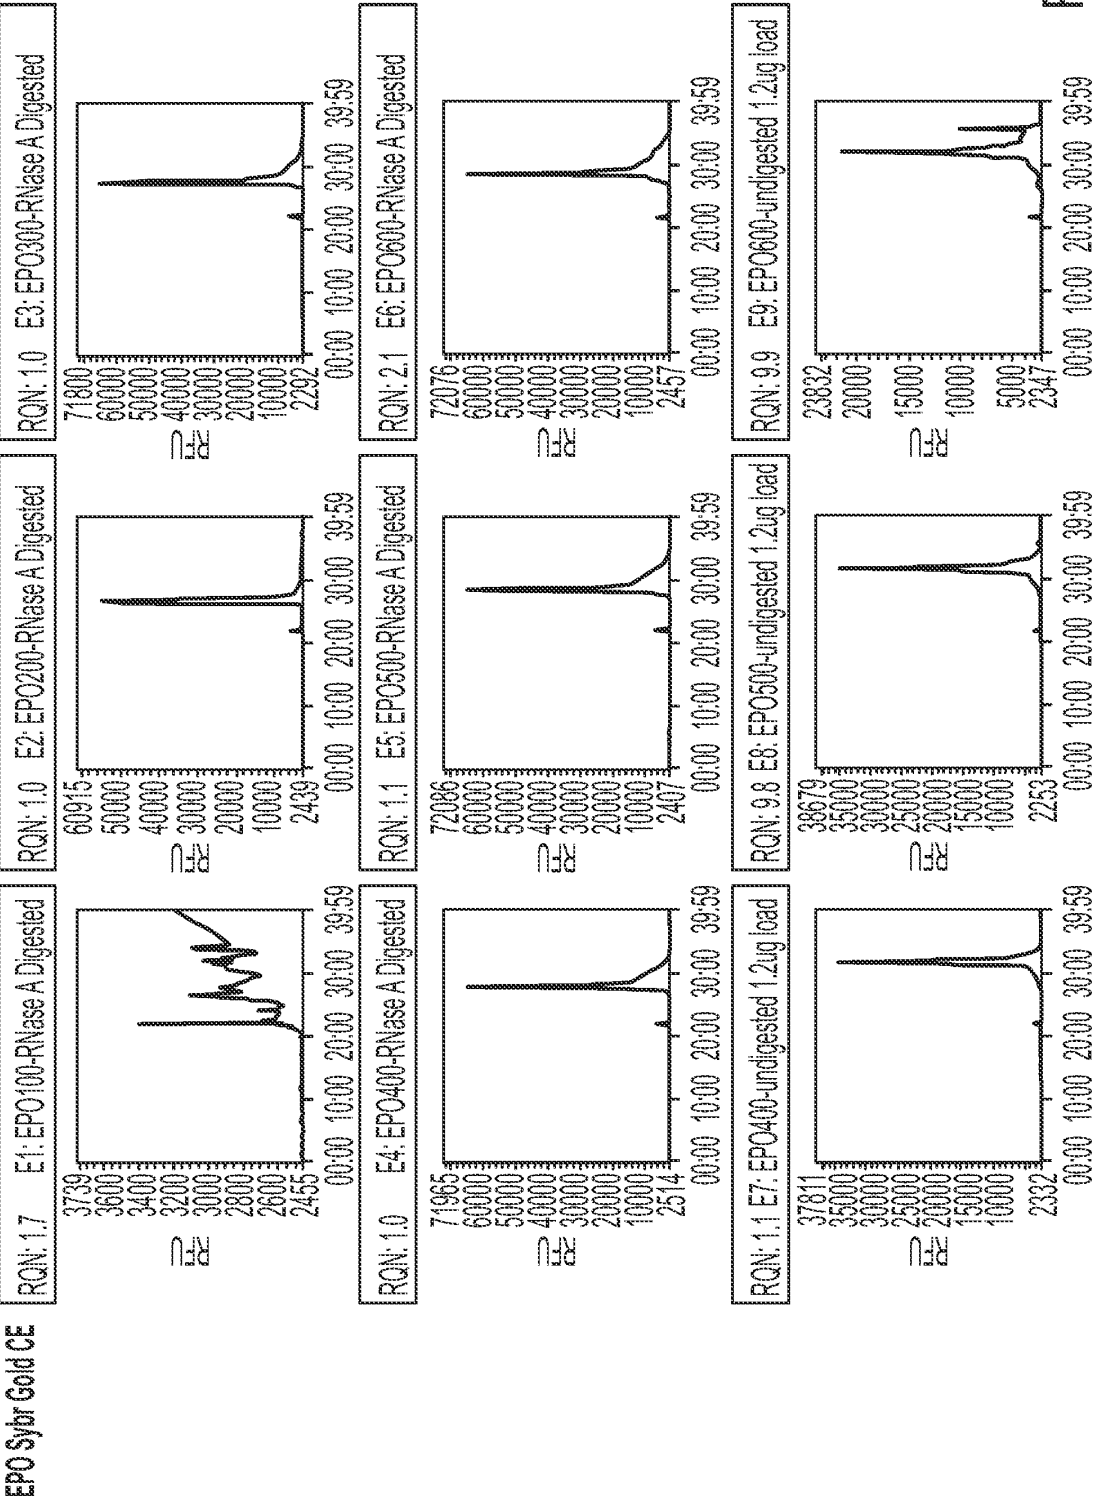

EPO Agilent
Intercalating
Dye CE

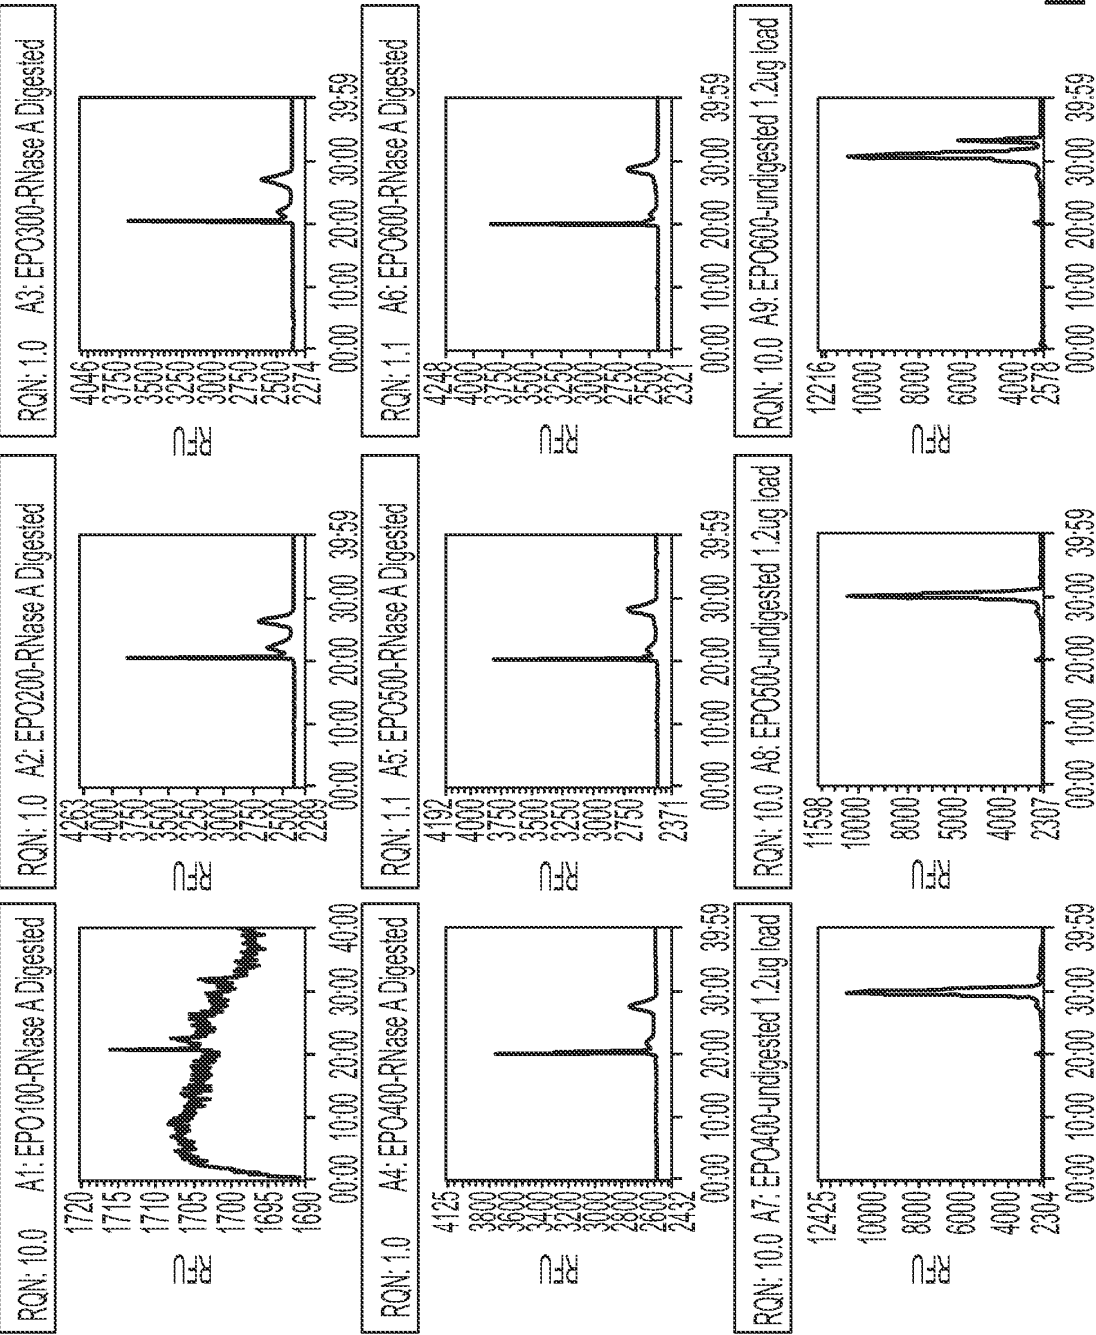


FIG. 5B

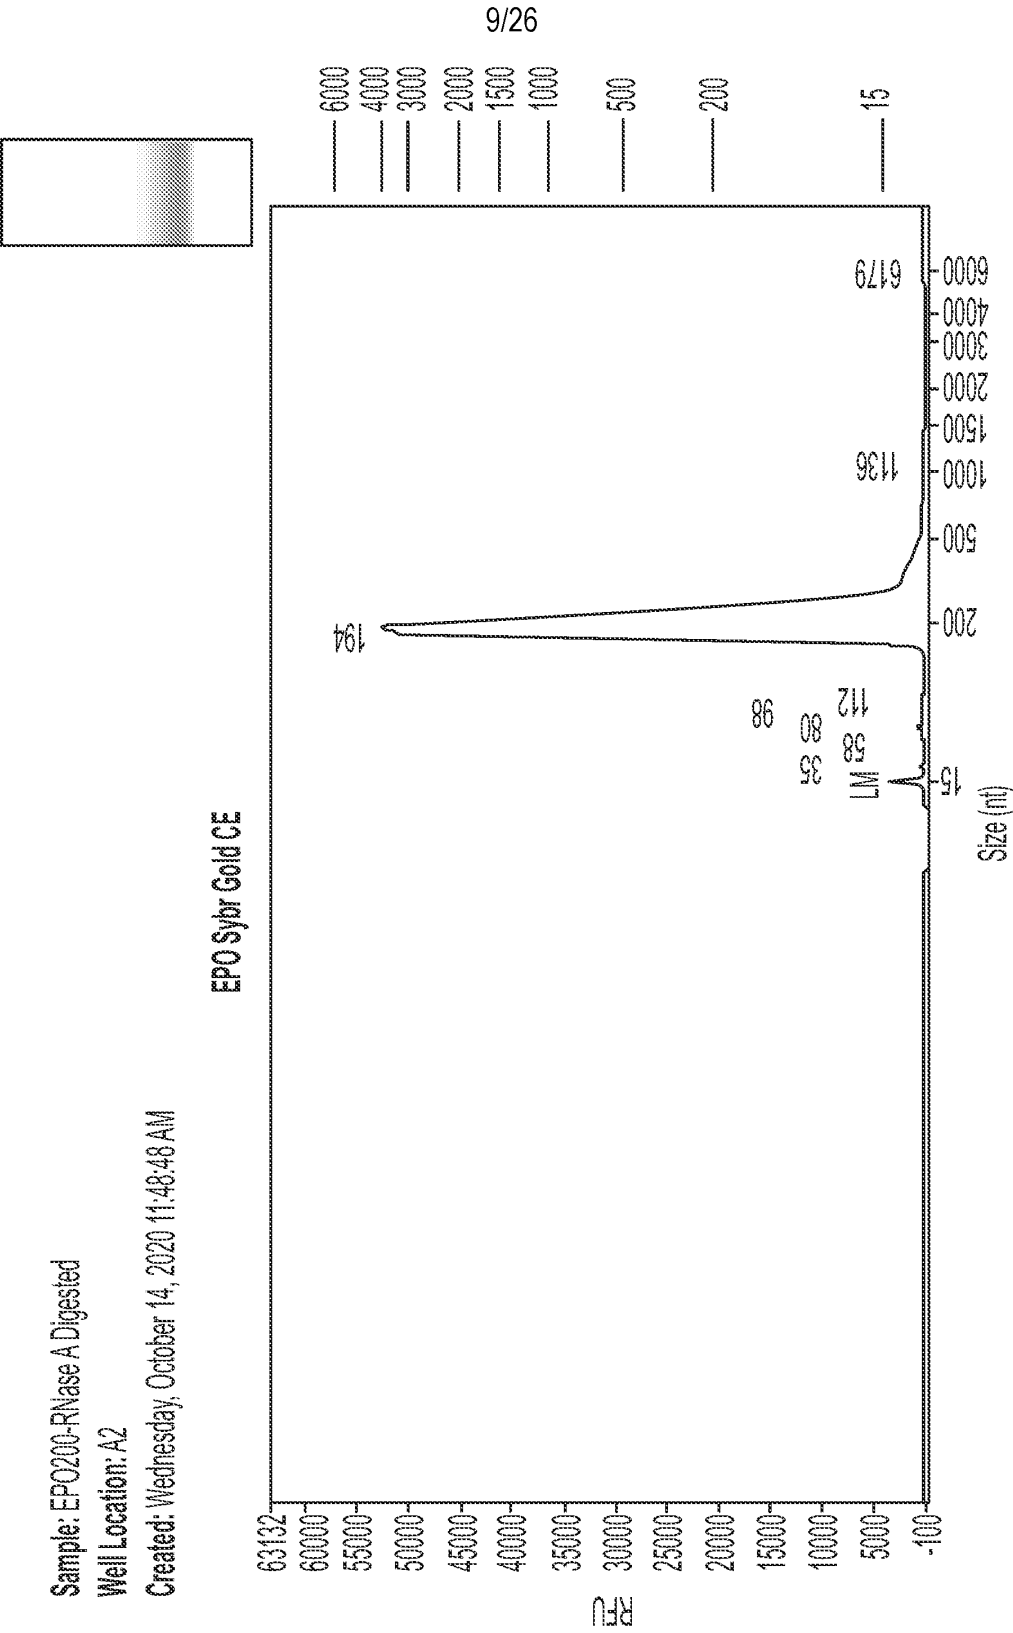


FIG. 6A

Sample: EPO200-RNase A Digested
Well Location: A2
Created: Wednesday, October 14, 2020 11:48:48 AM

Sample: EPO200-RNase A Digested
Well Location: E2
Created: Wednesday, October 14, 2020 7:47:39 PM

EPO Agilent Intercalating Dye CE

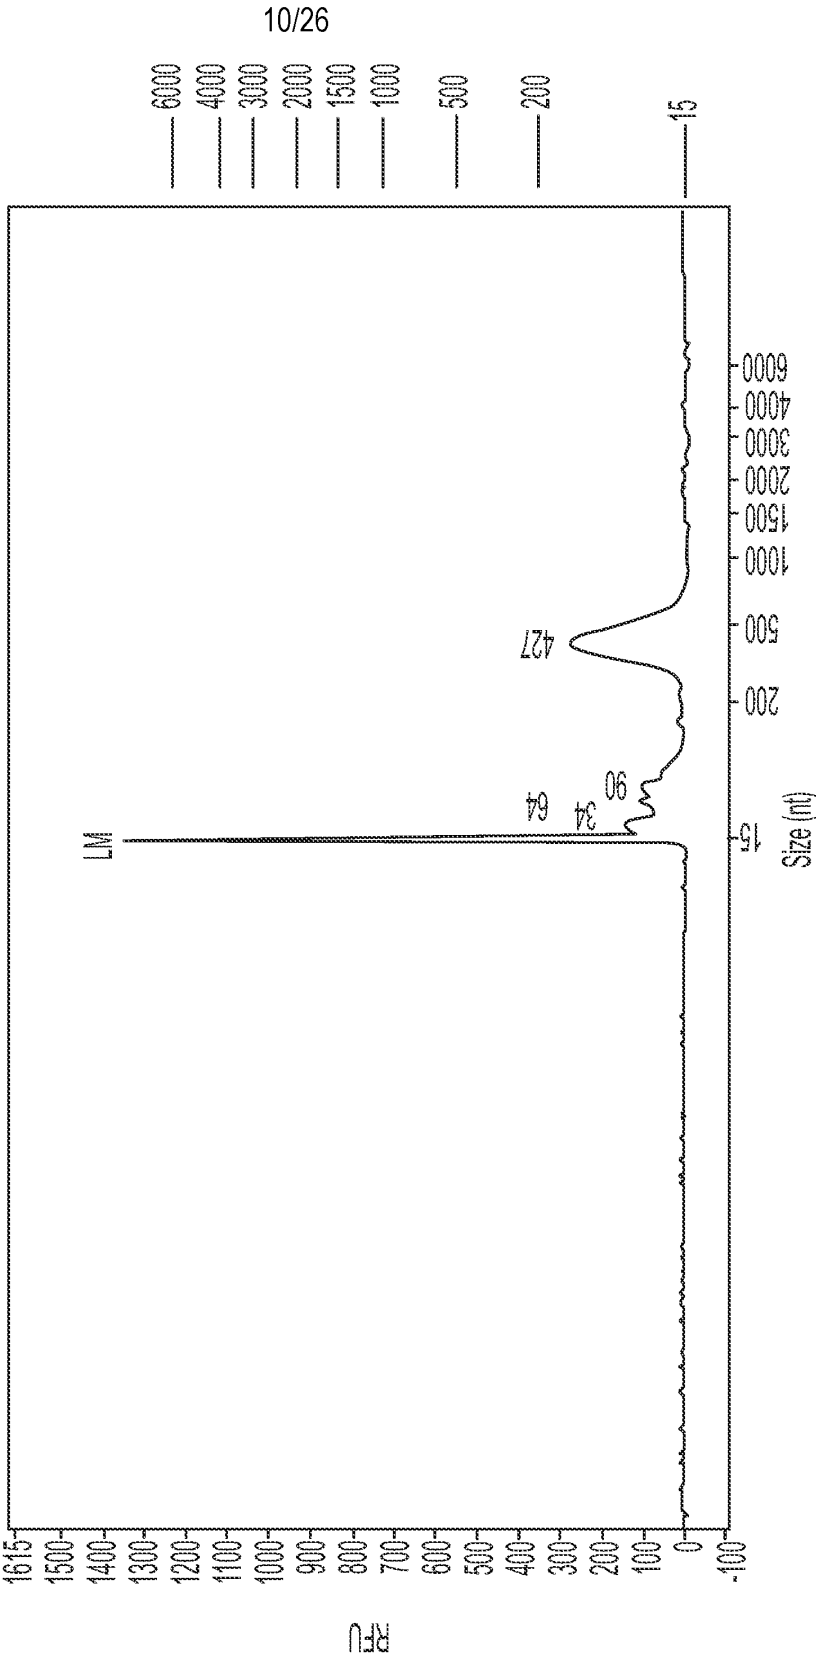


FIG. 6B

11/26

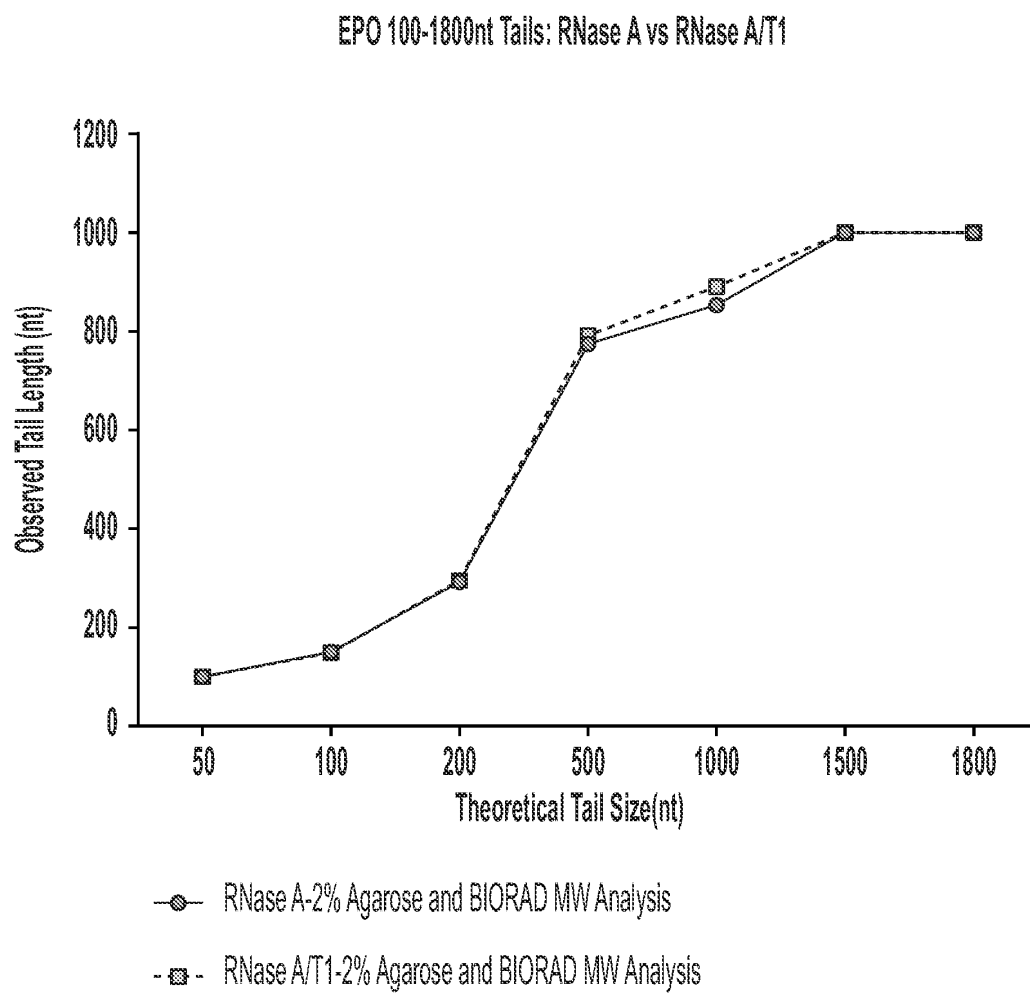
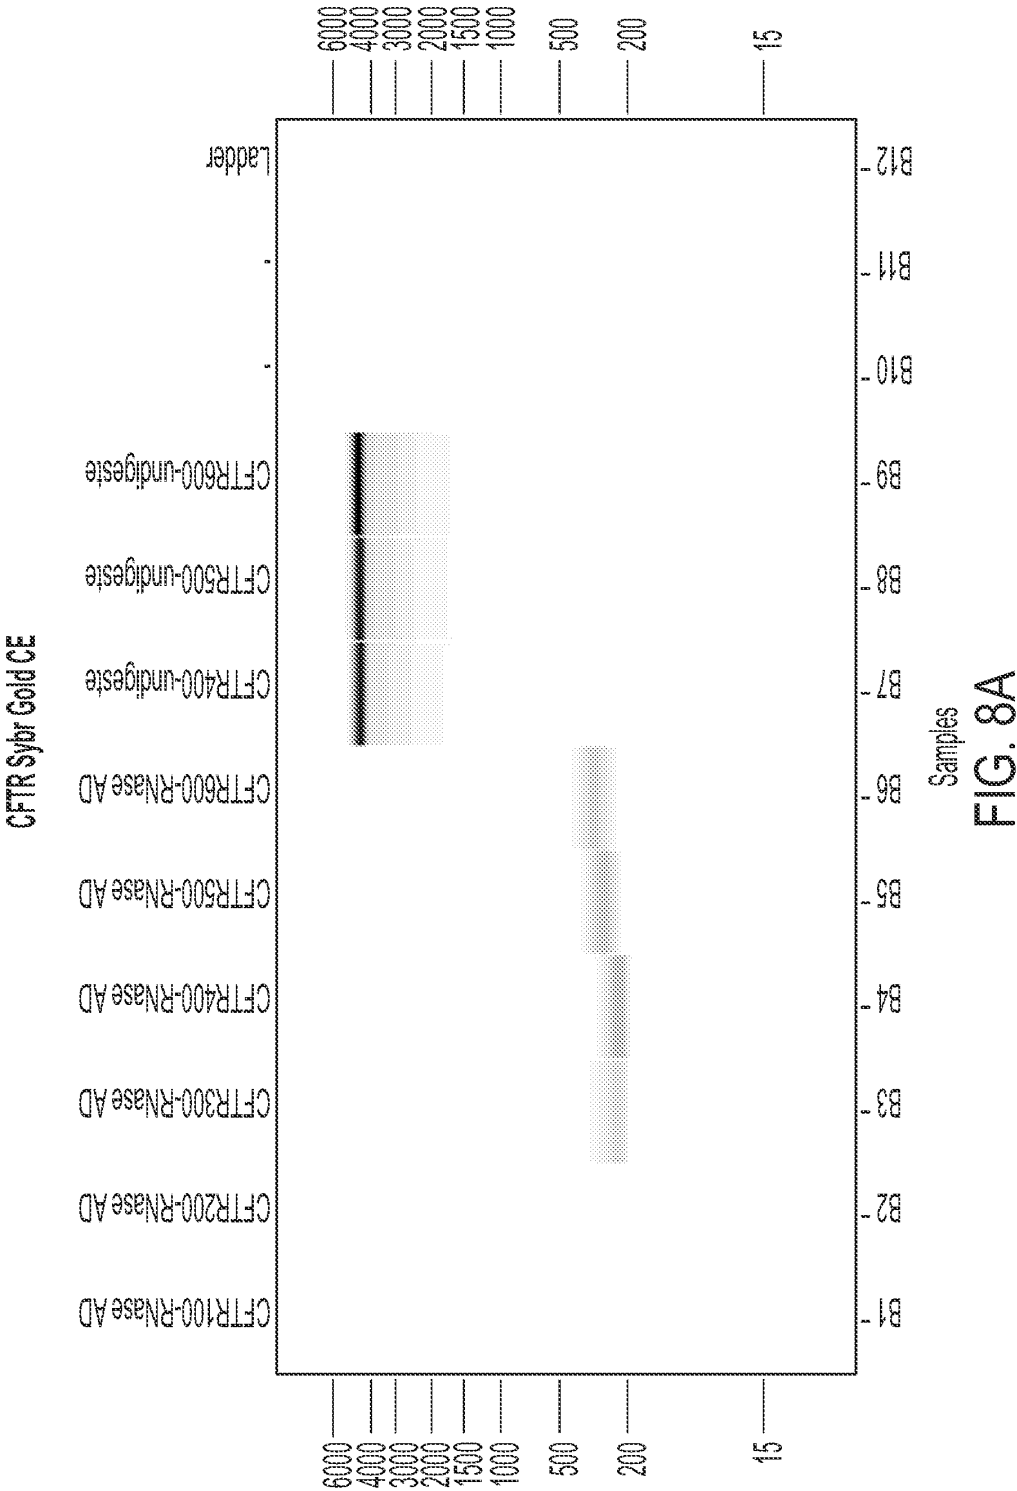
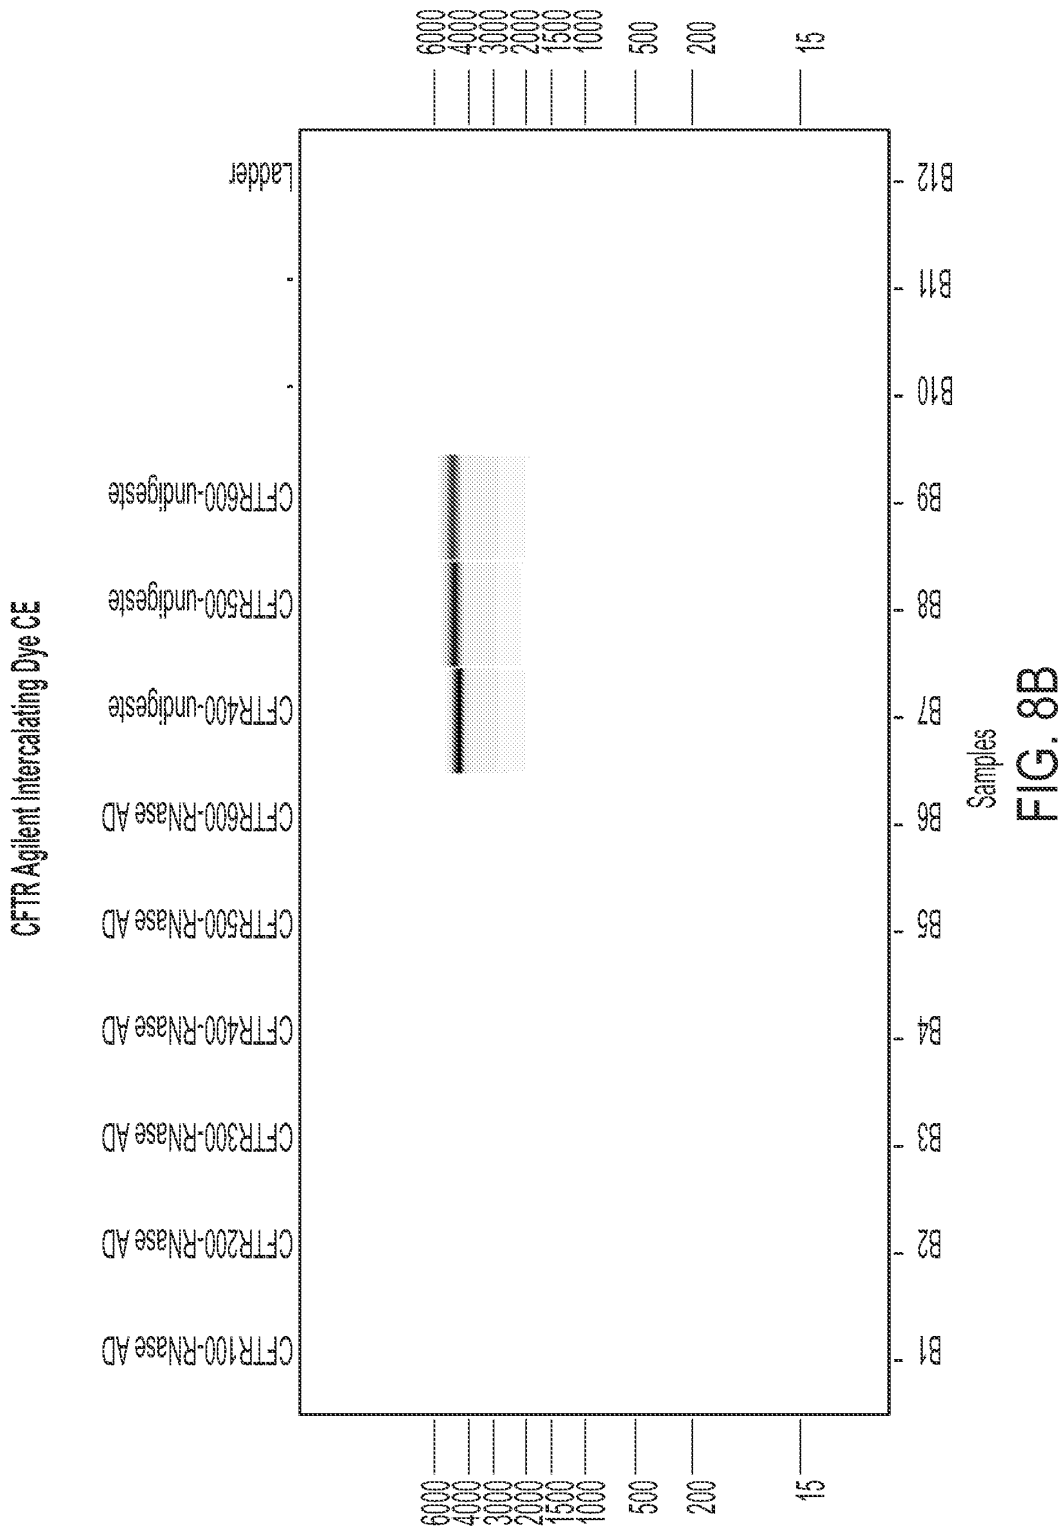
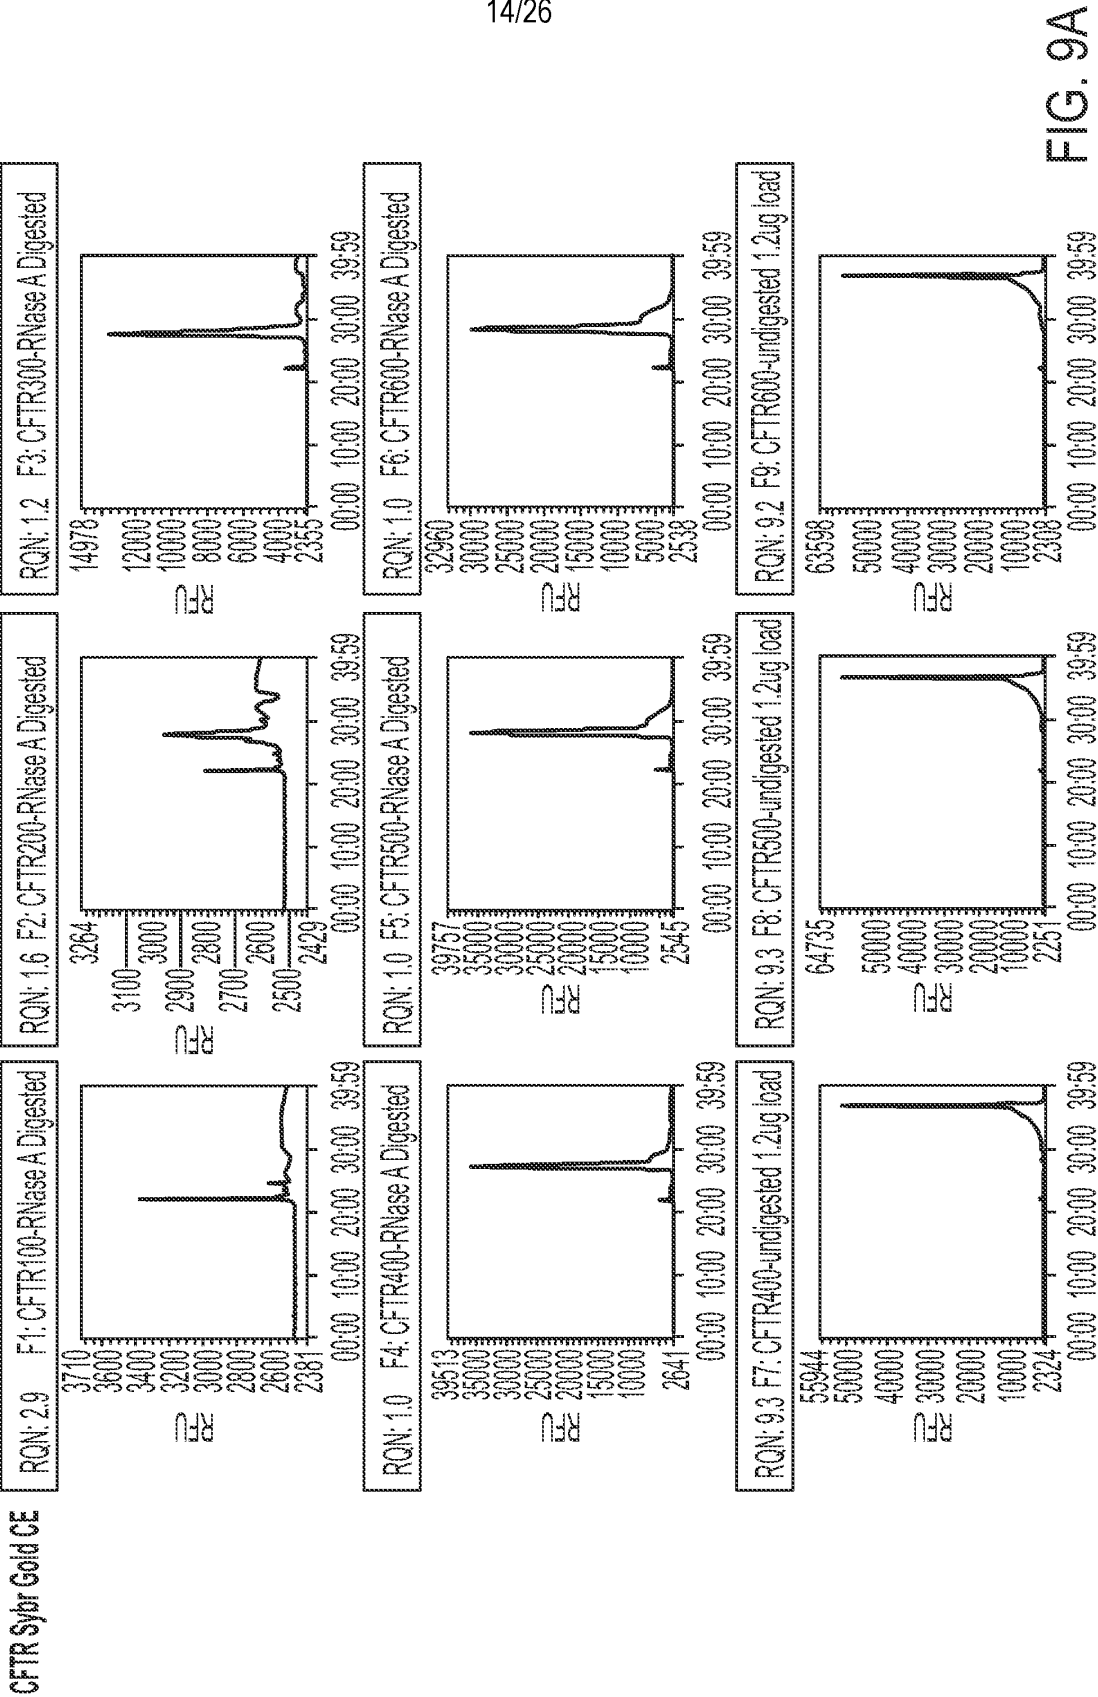


FIG. 7

12/26







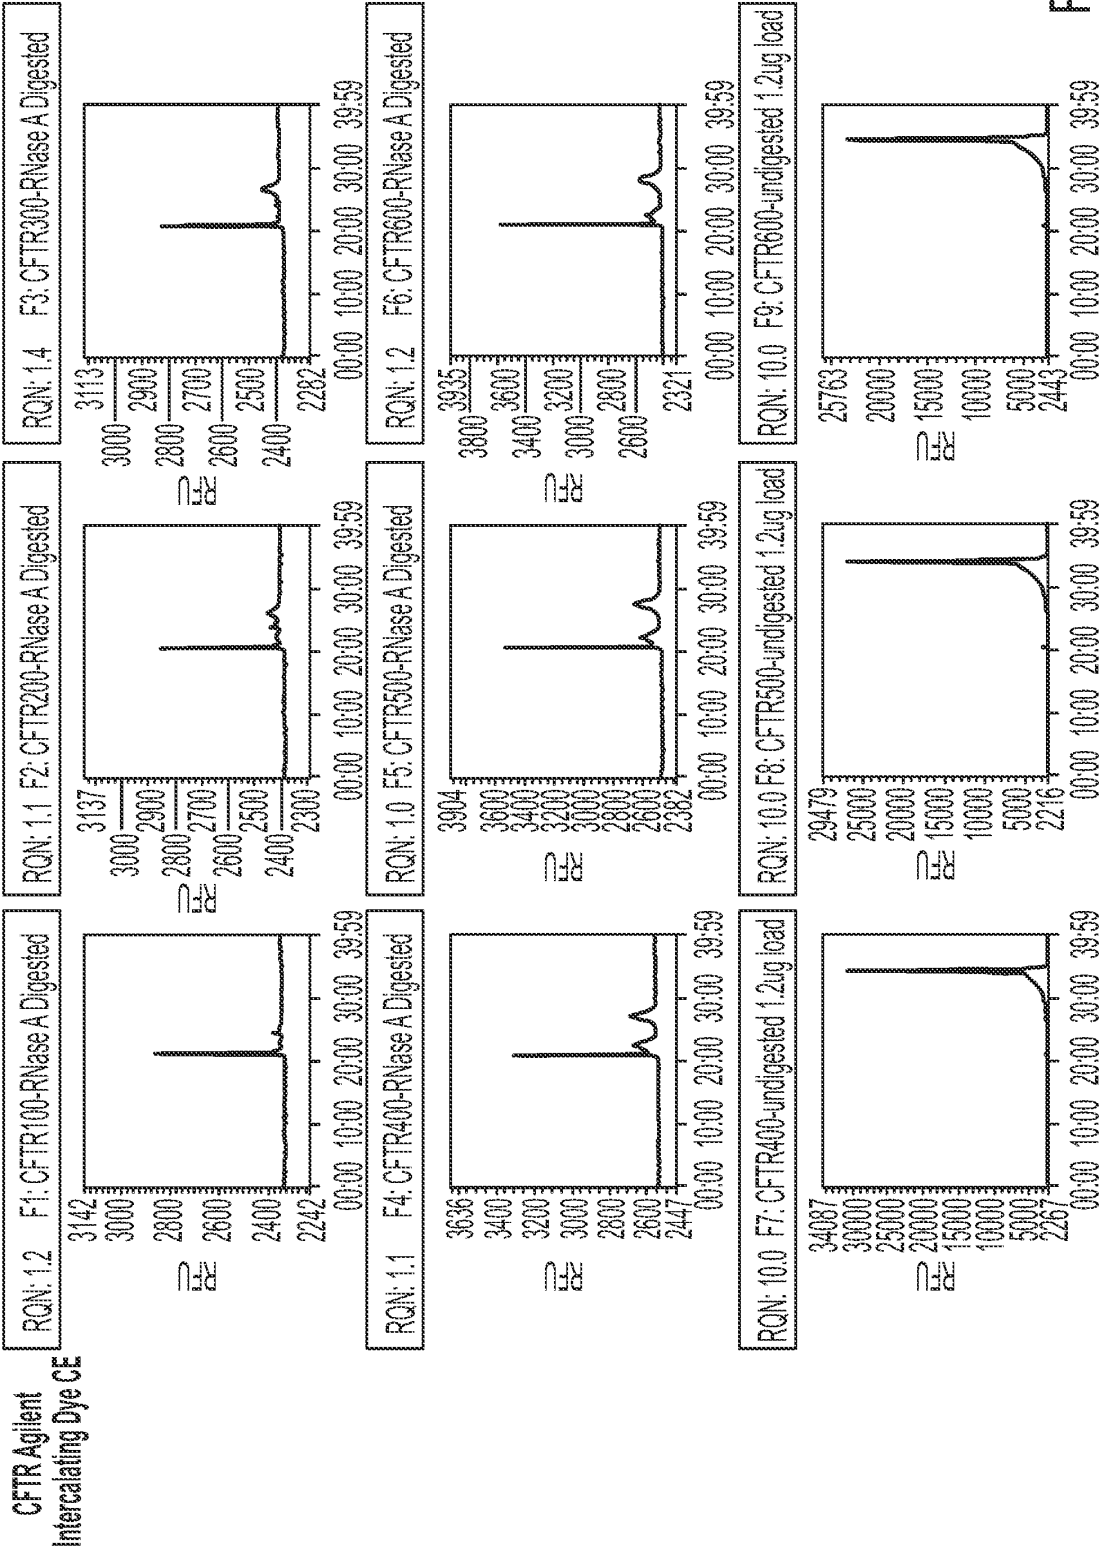


FIG. 9B

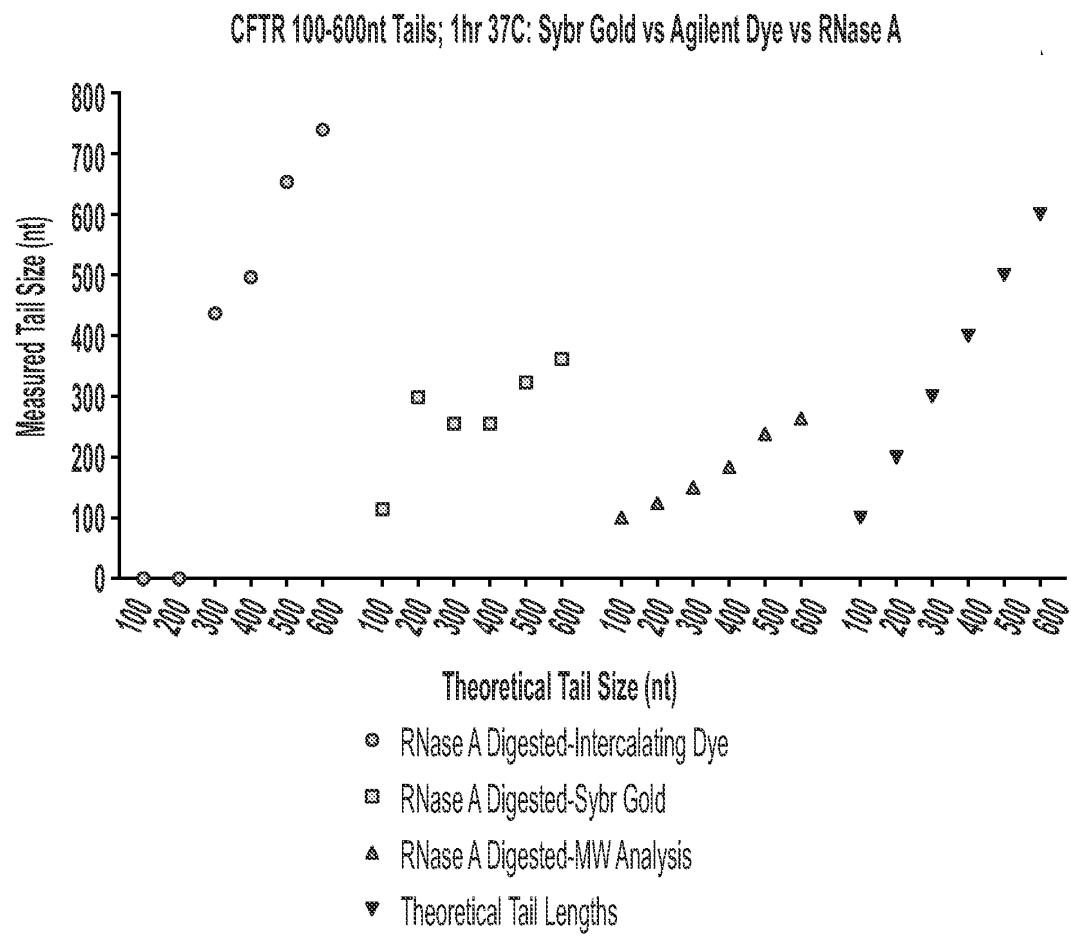


FIG. 10

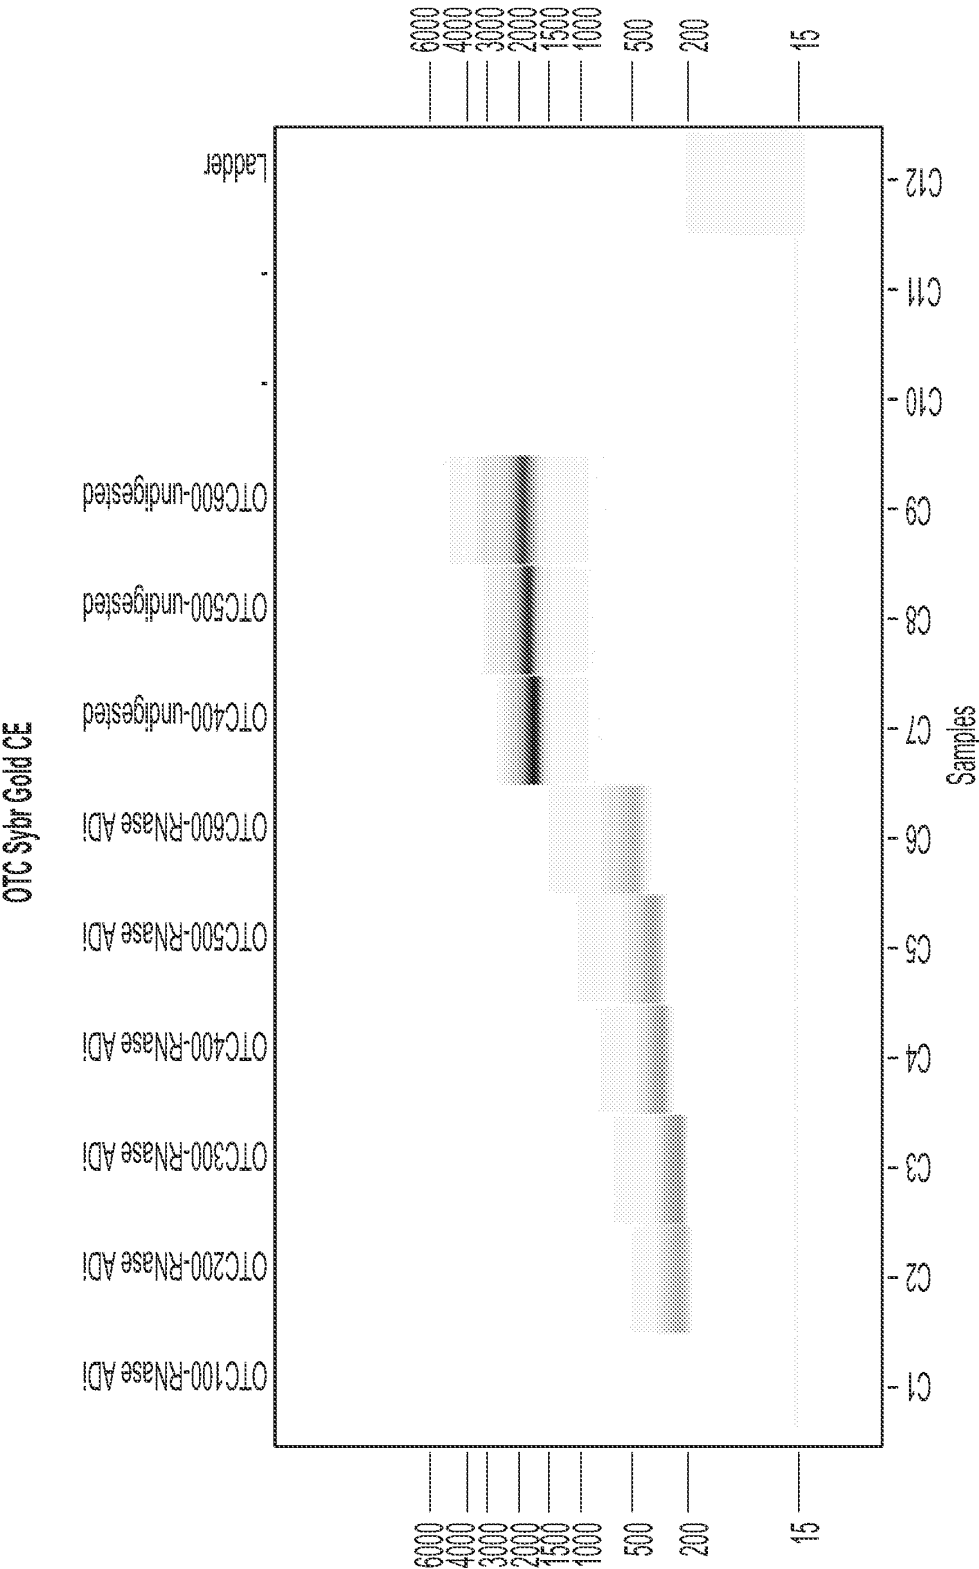


FIG. 11A

18/26

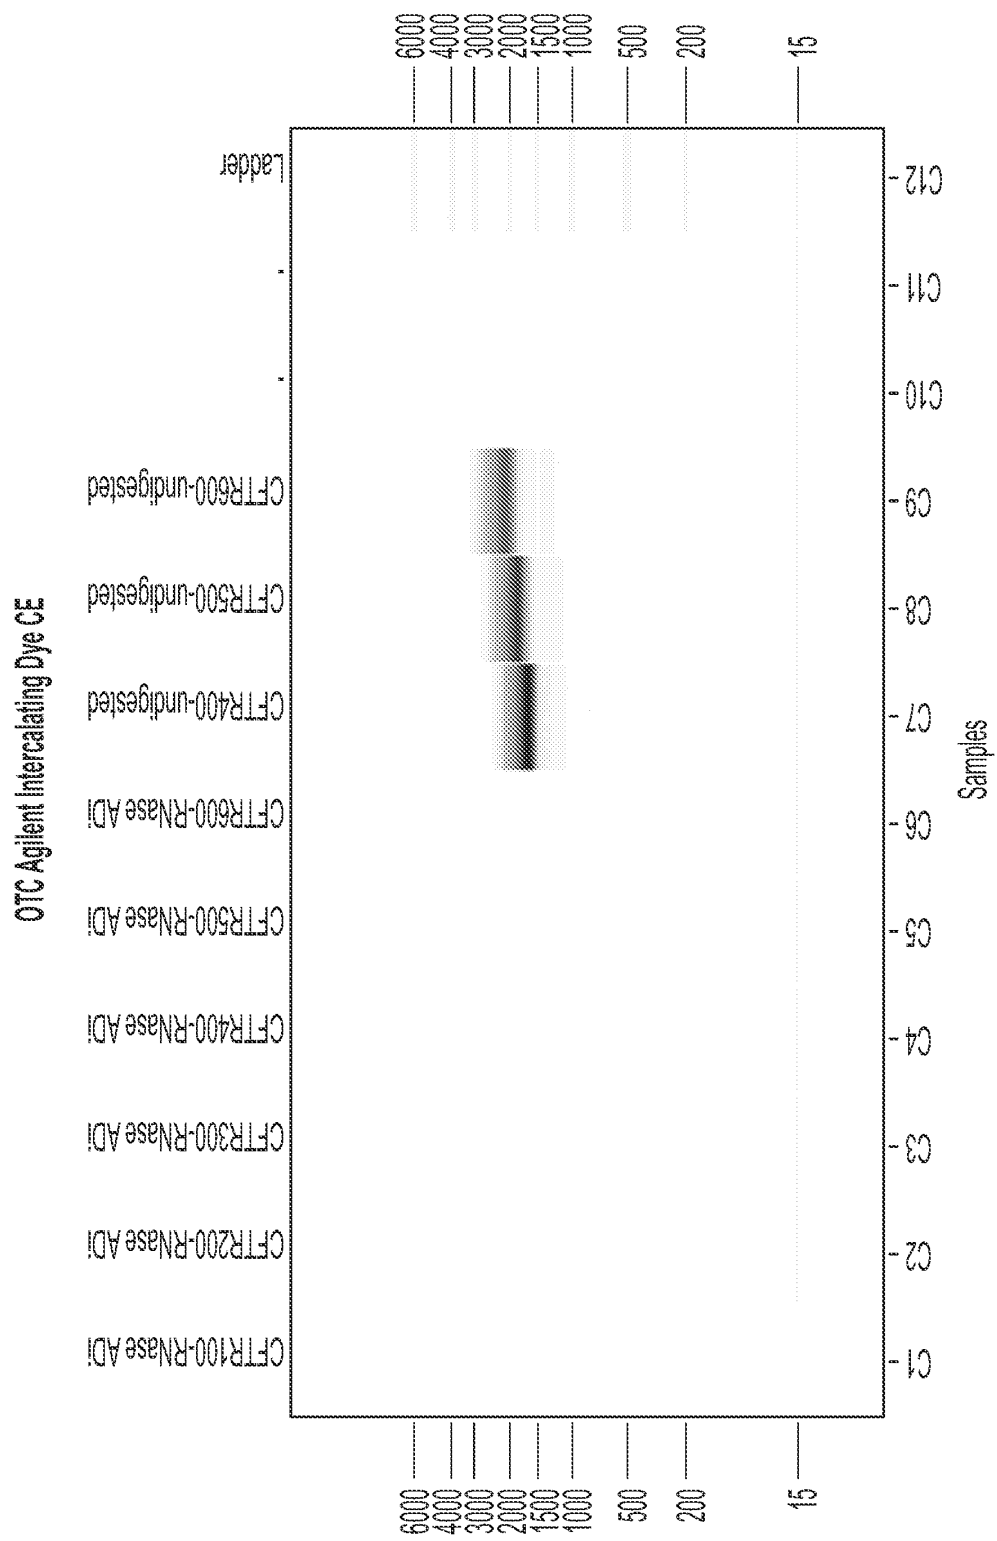


FIG. 11B

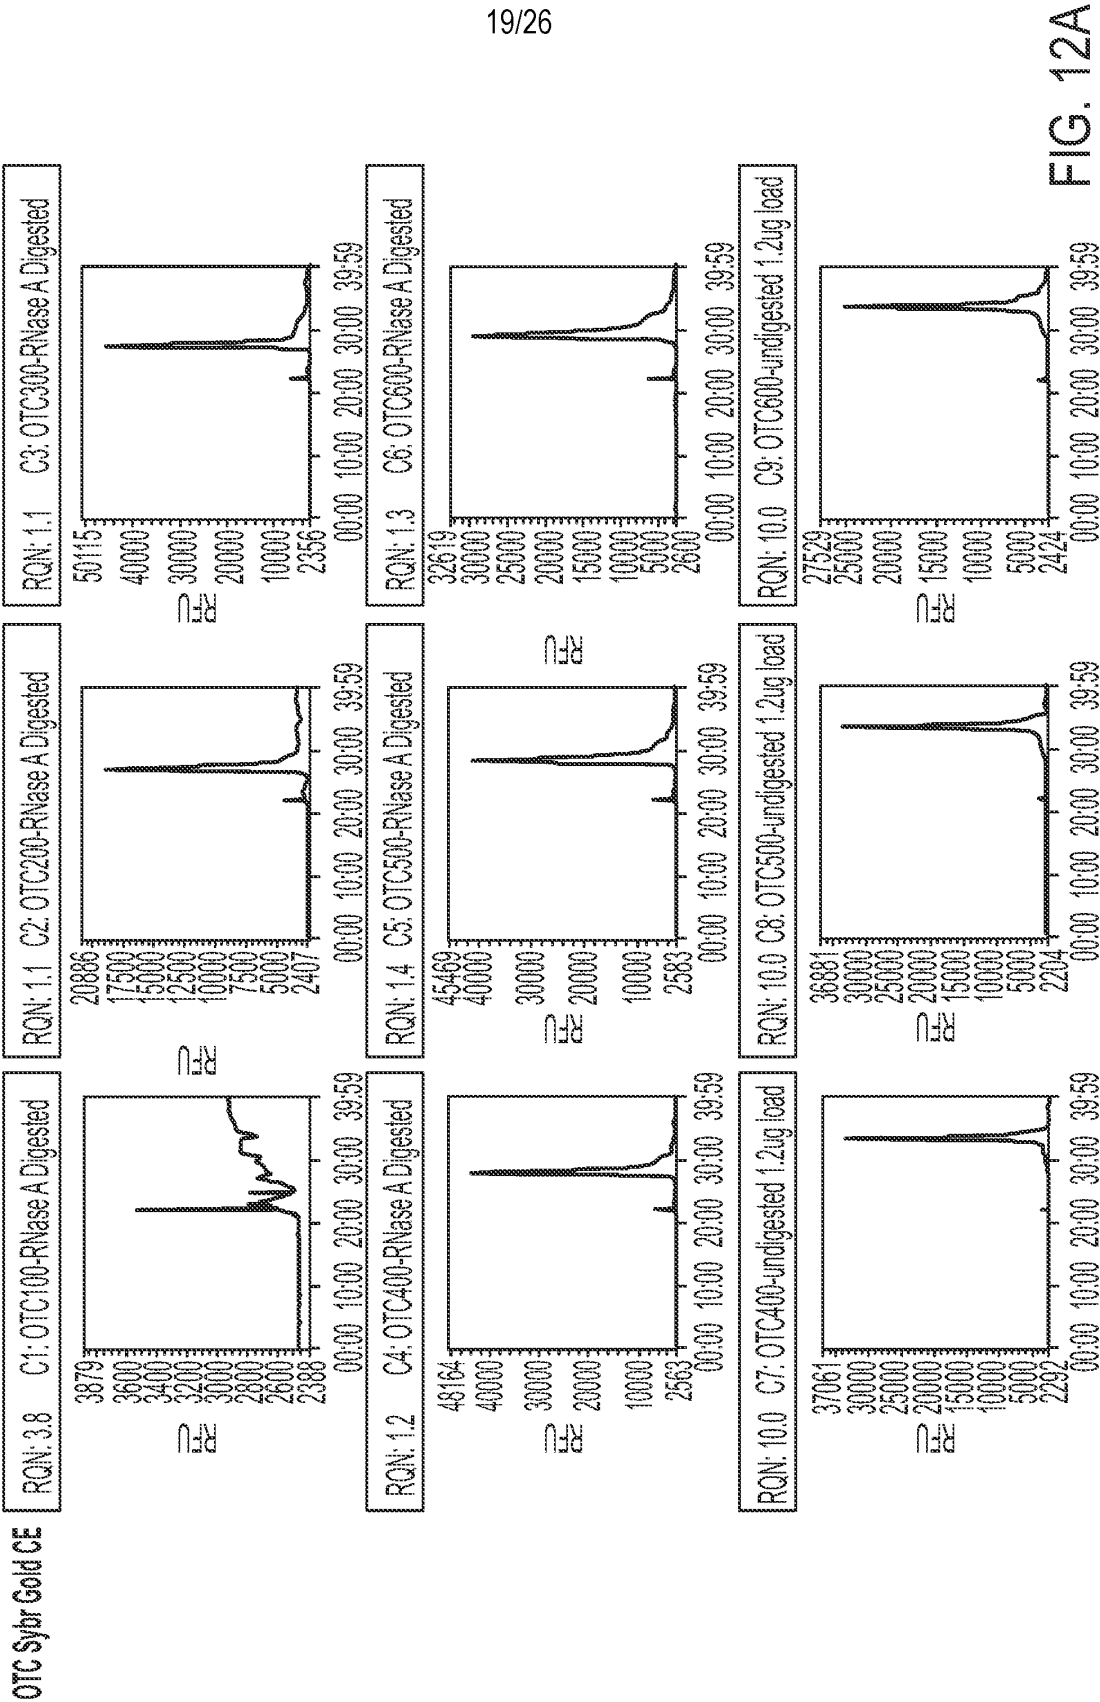
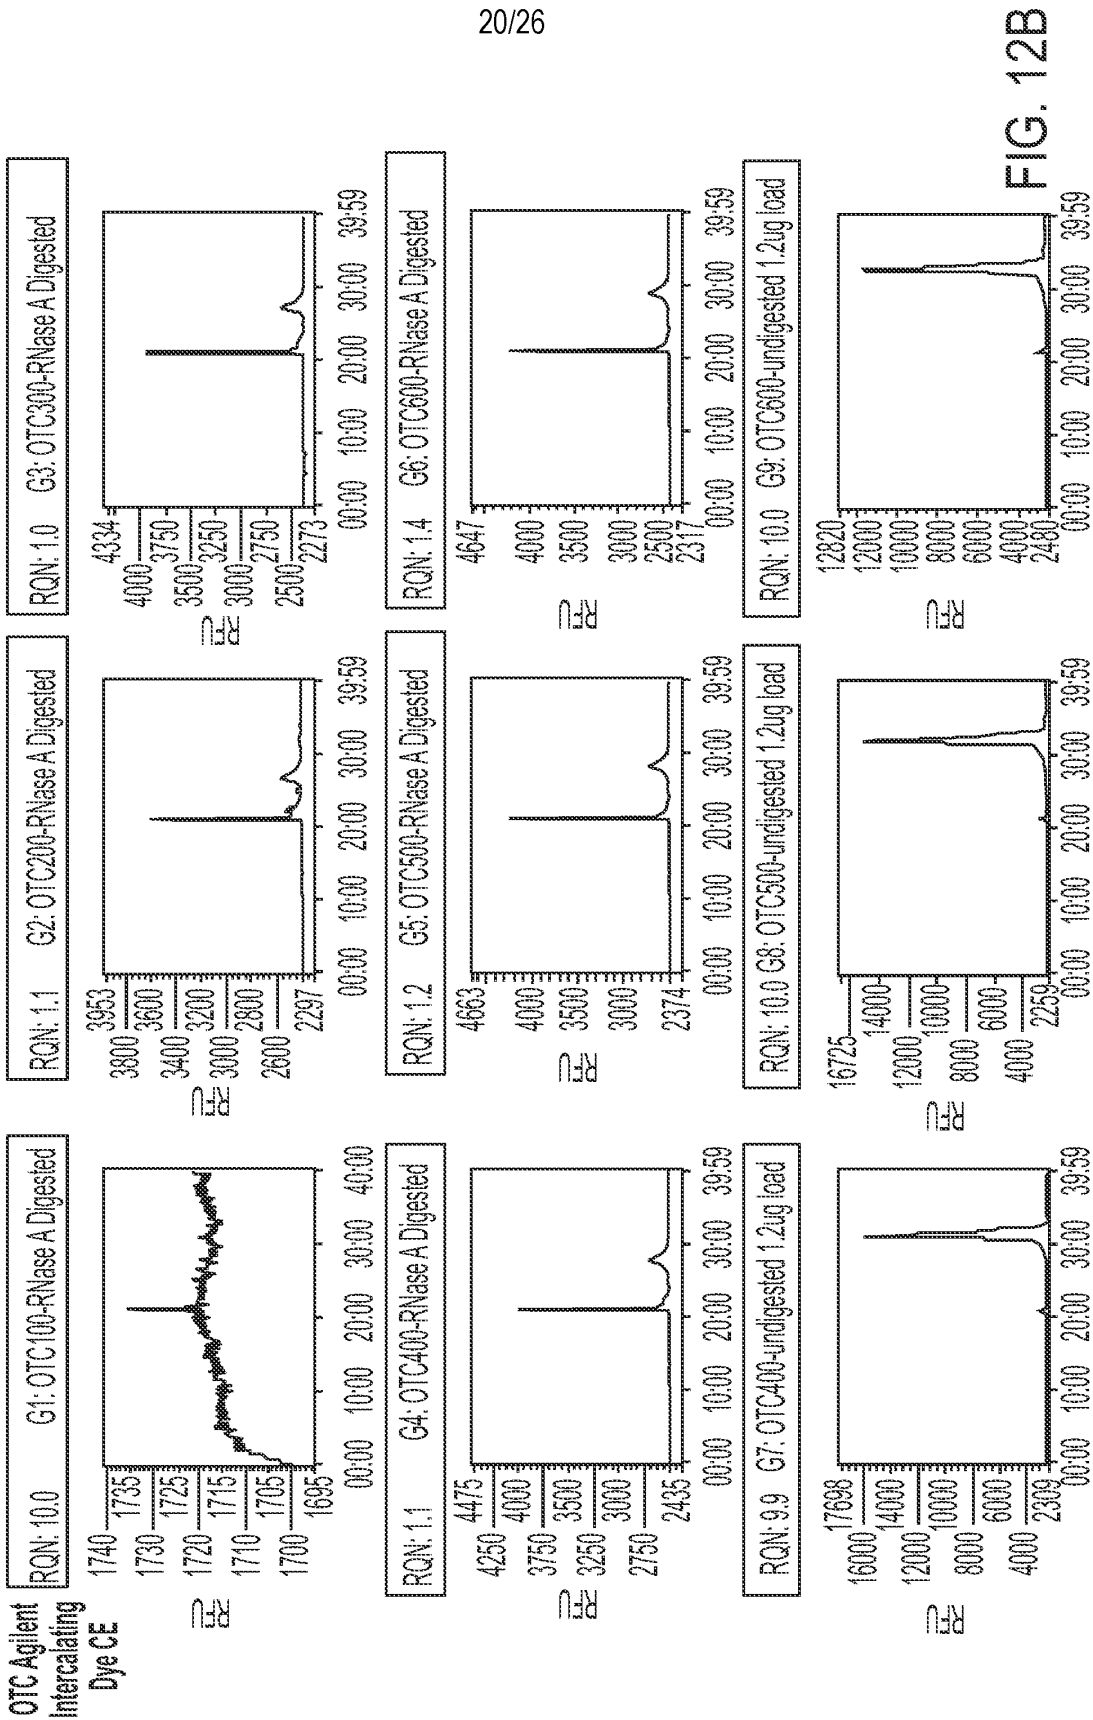


FIG. 12A




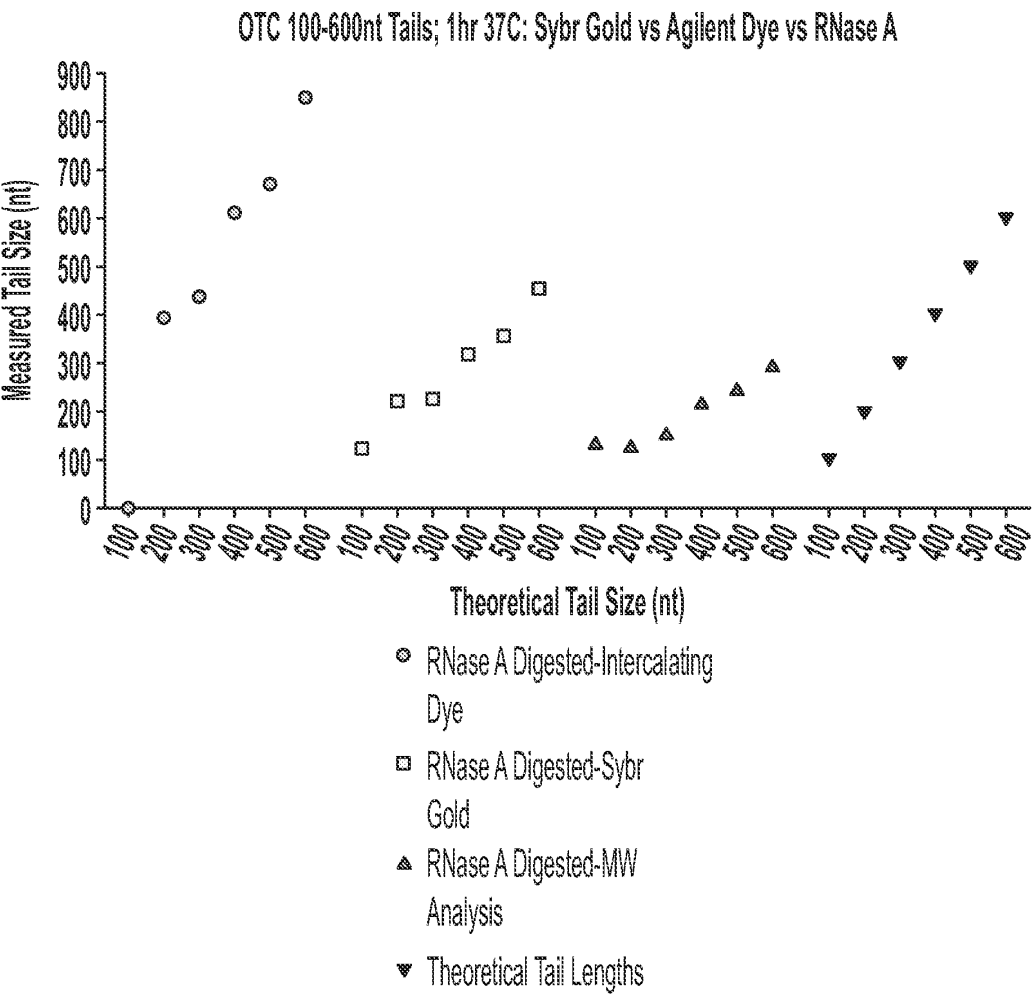


FIG. 13

22/26

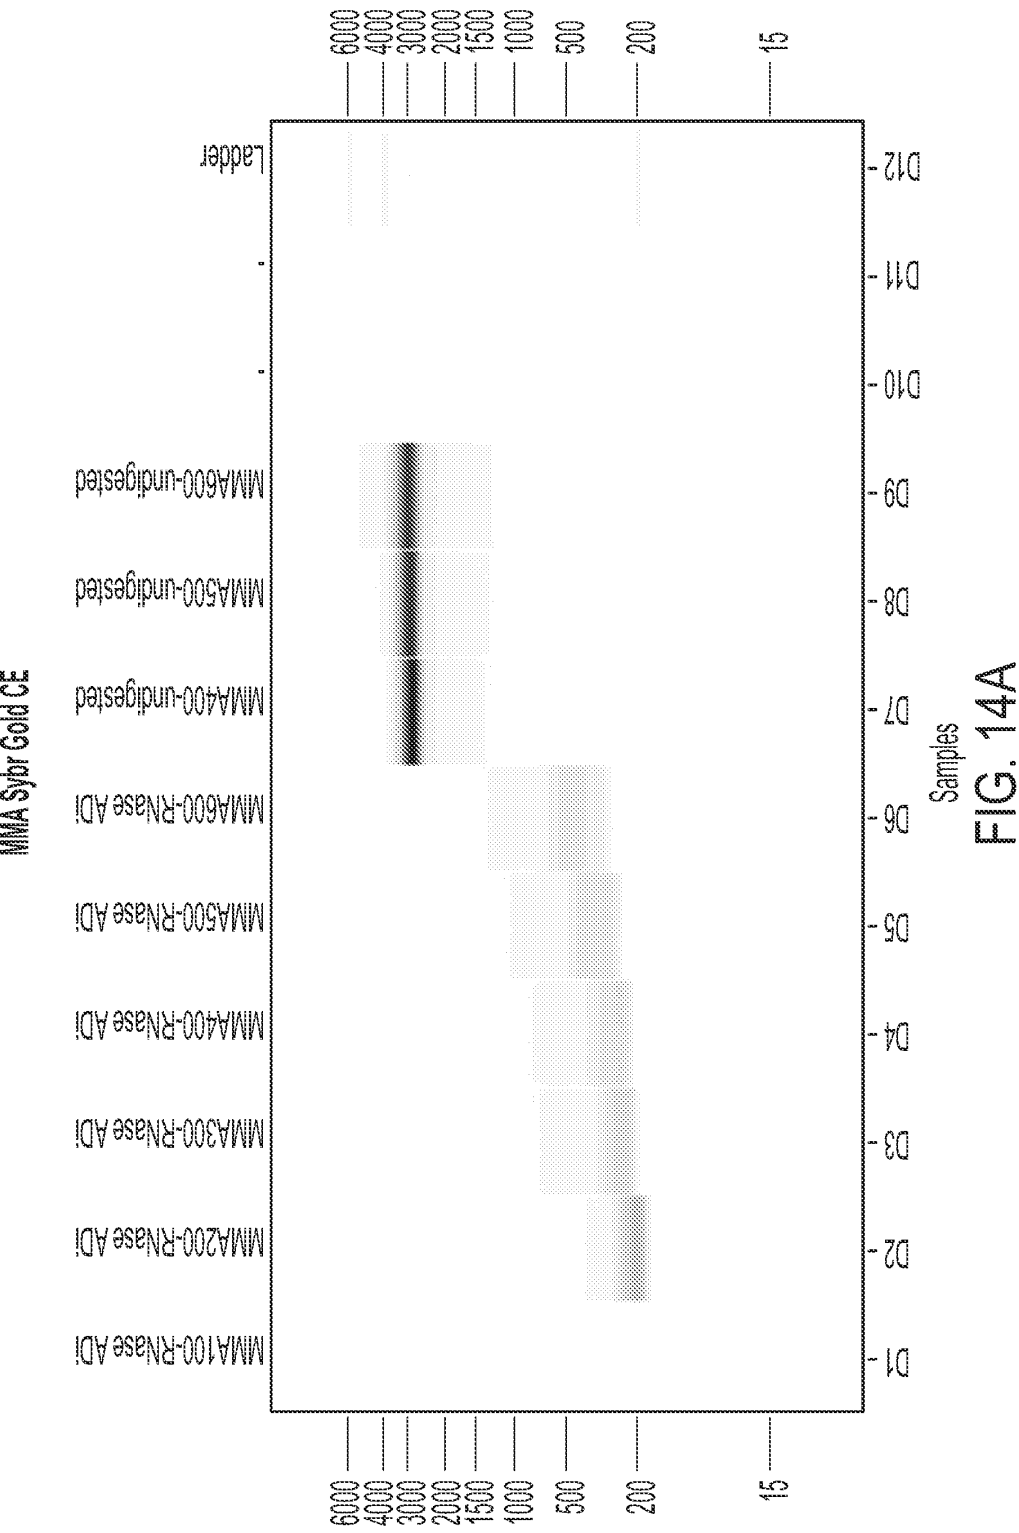

23/26

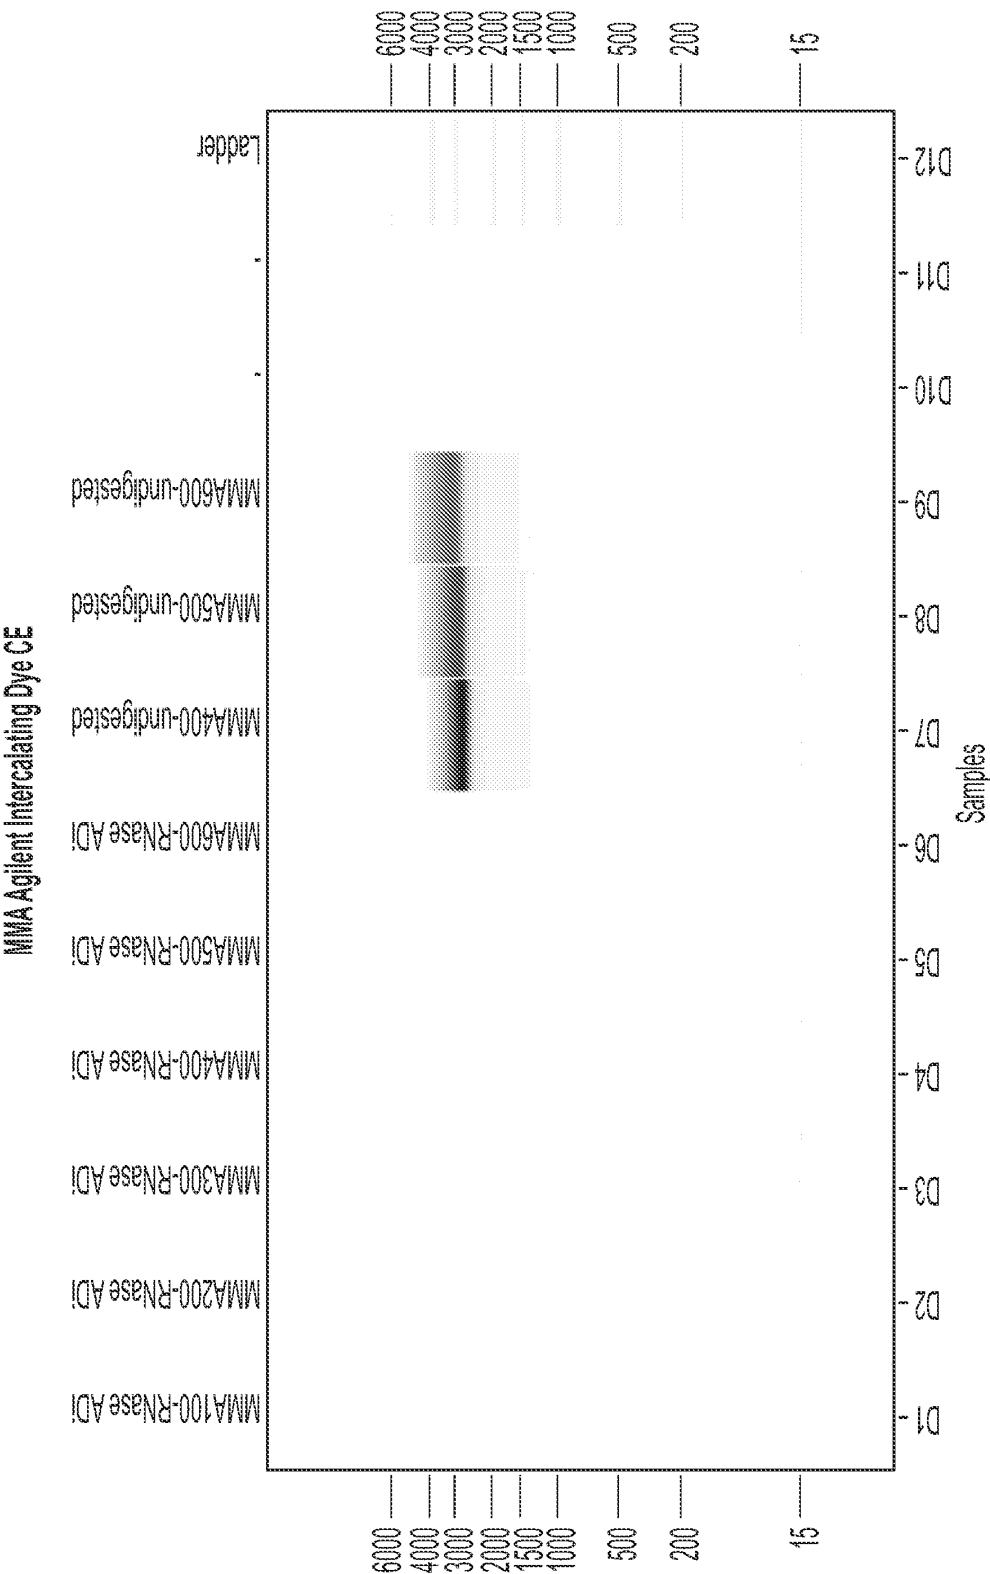


FIG. 14B

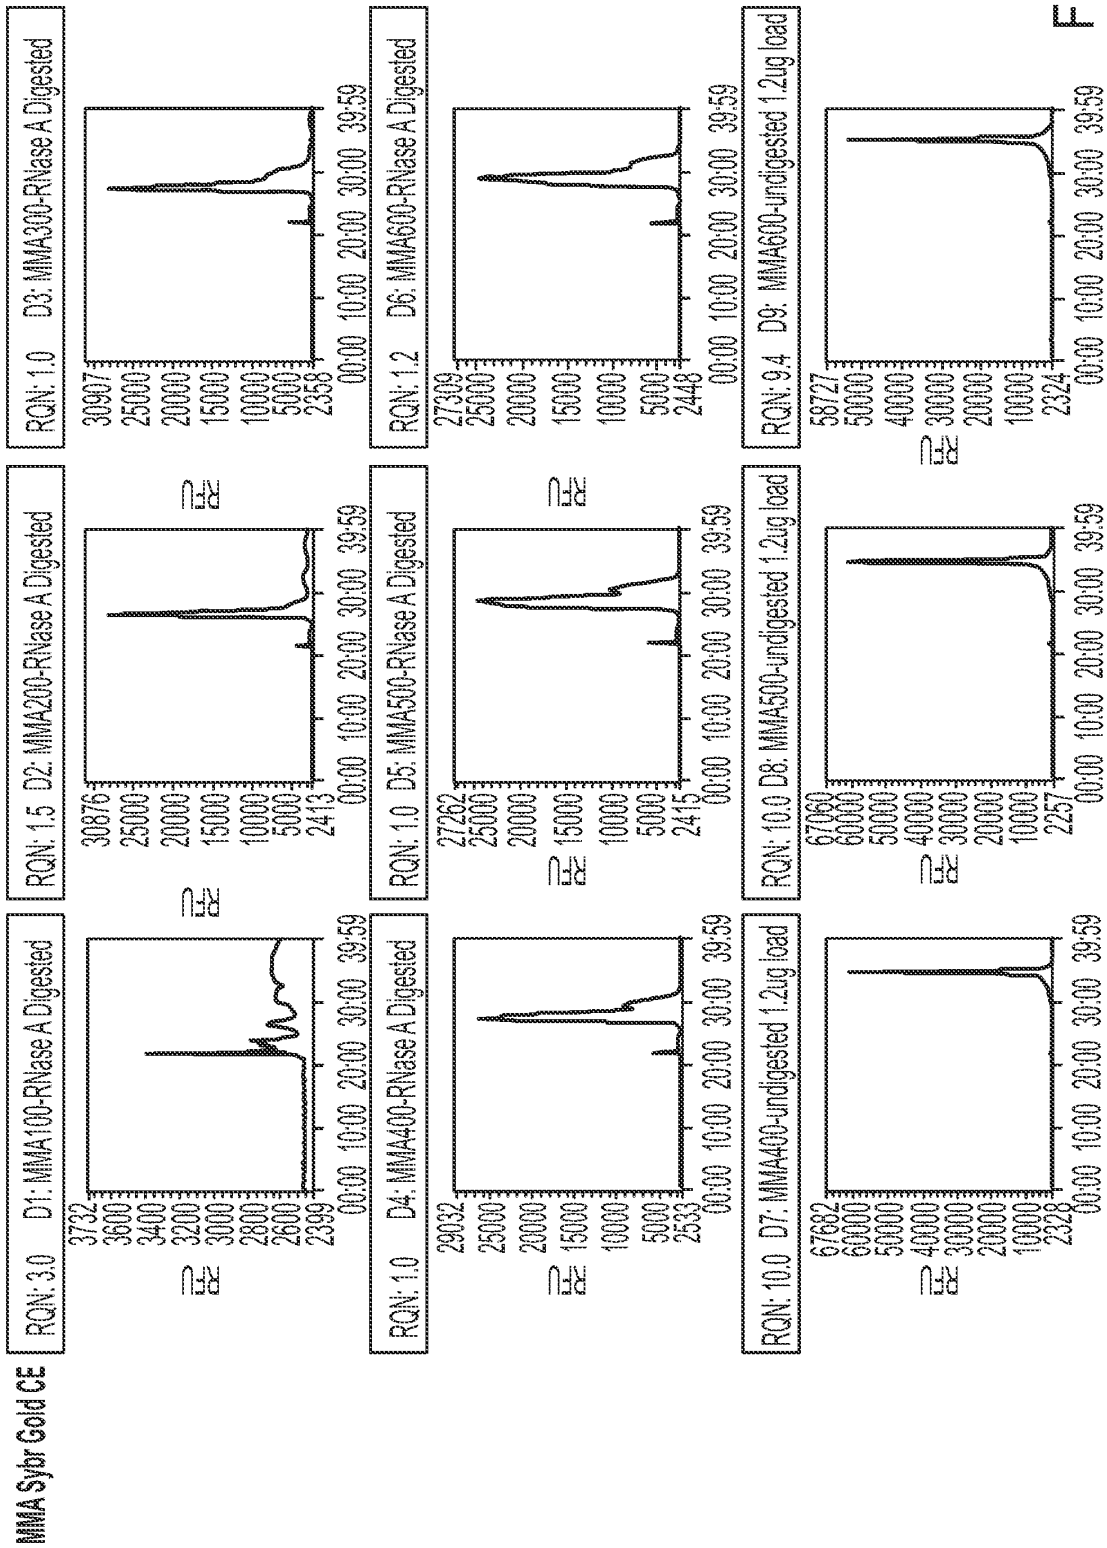
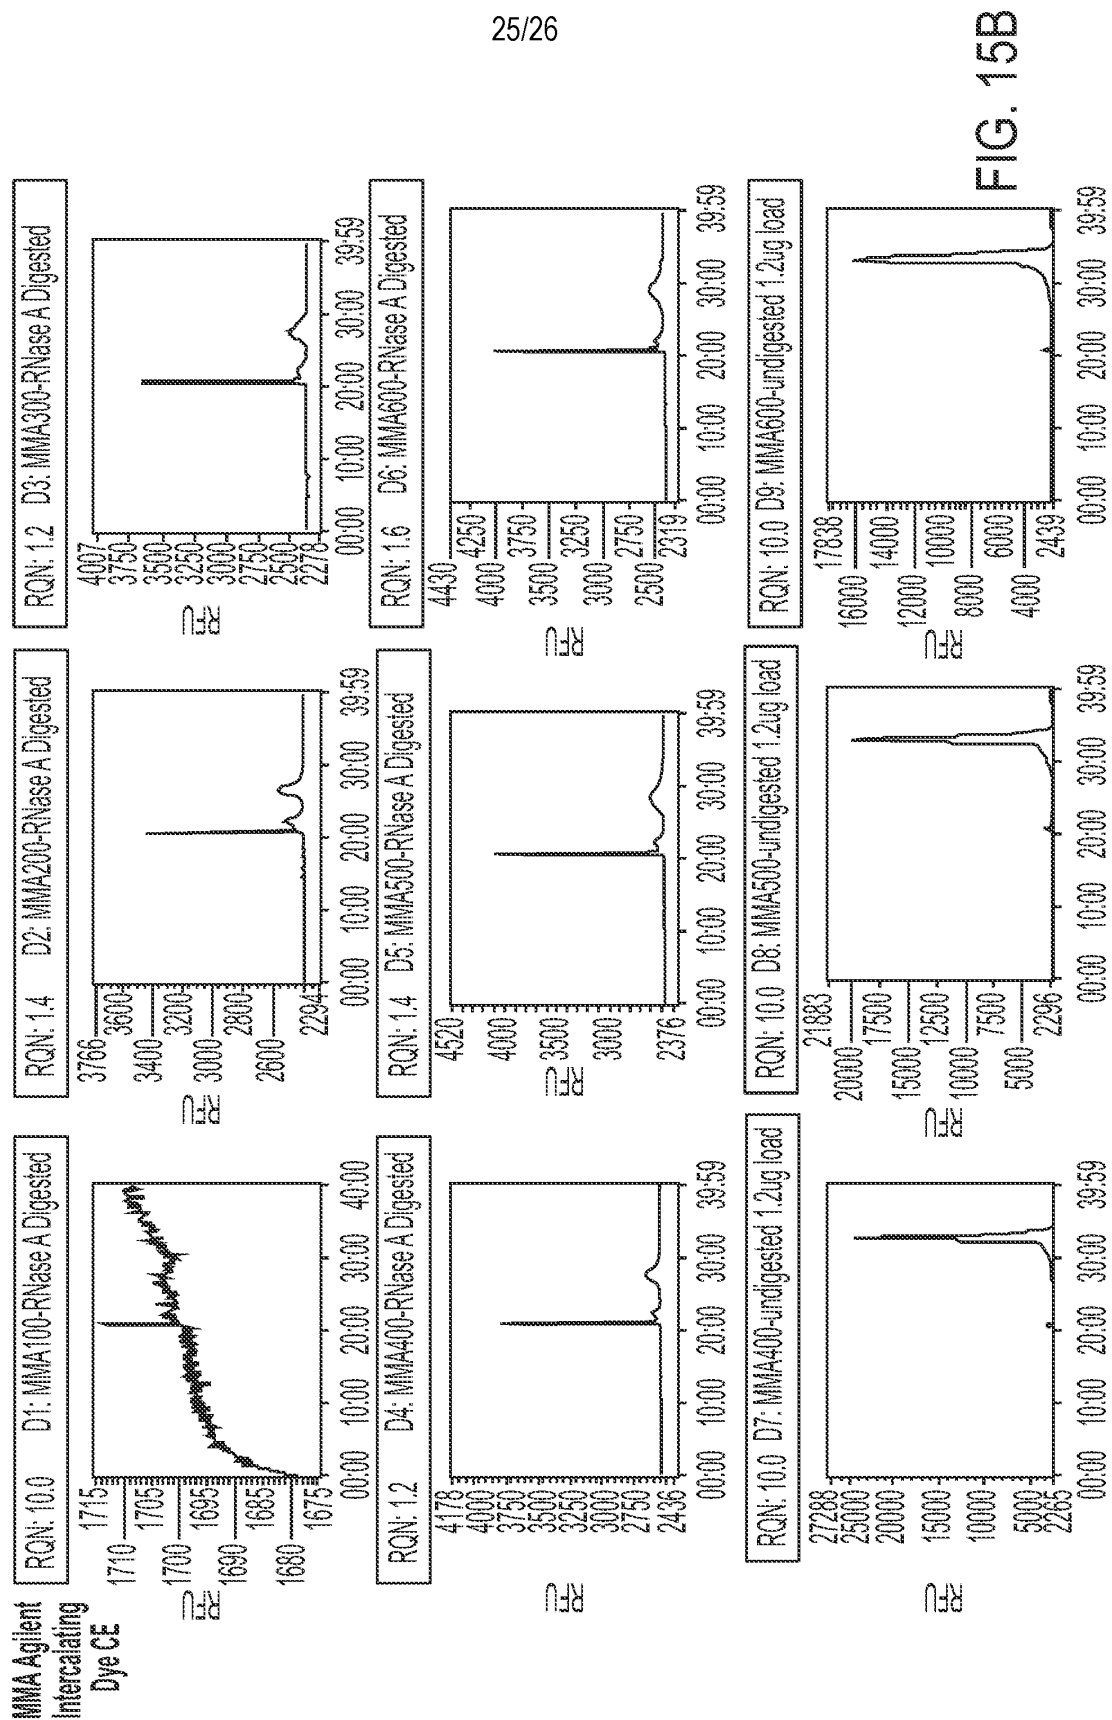


FIG. 15A



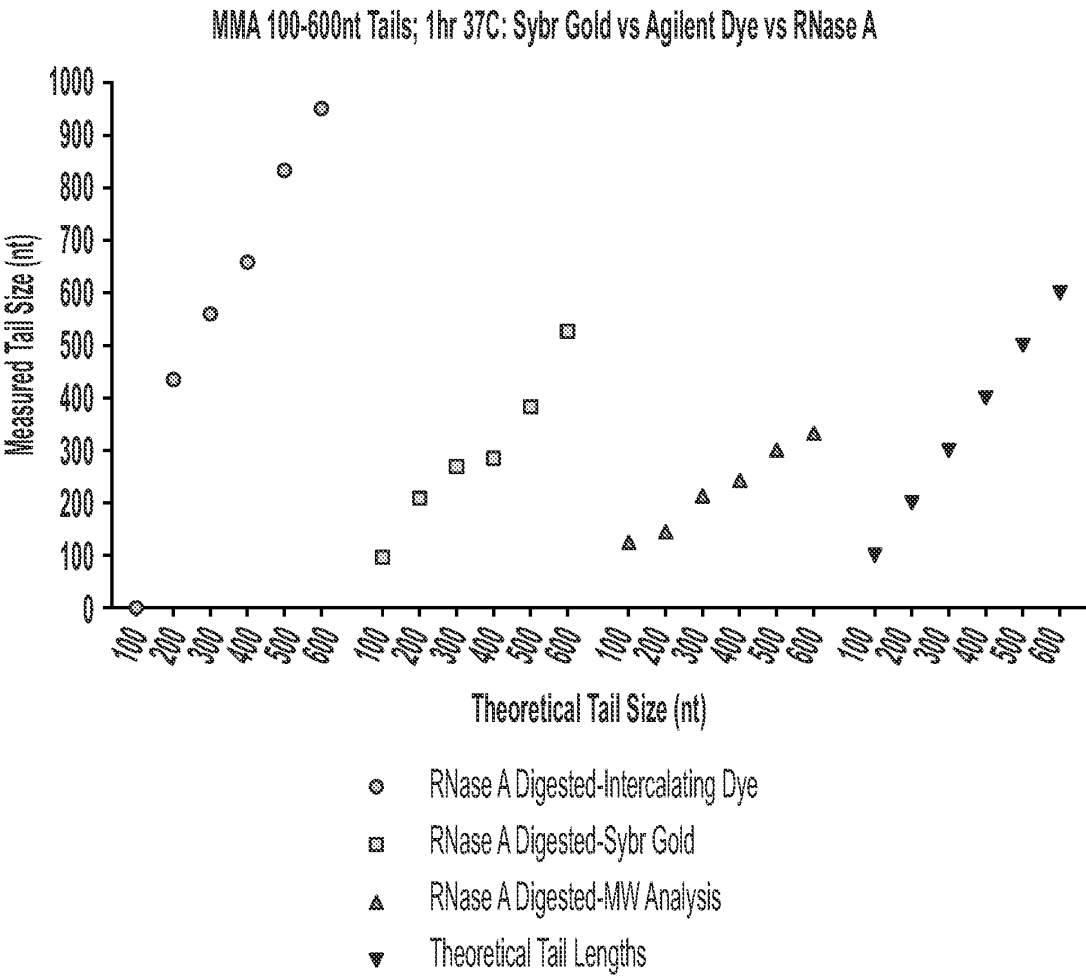


FIG. 16