

FIG. 1
Ion exchange chromatography profile of CAT-8015 reference standard

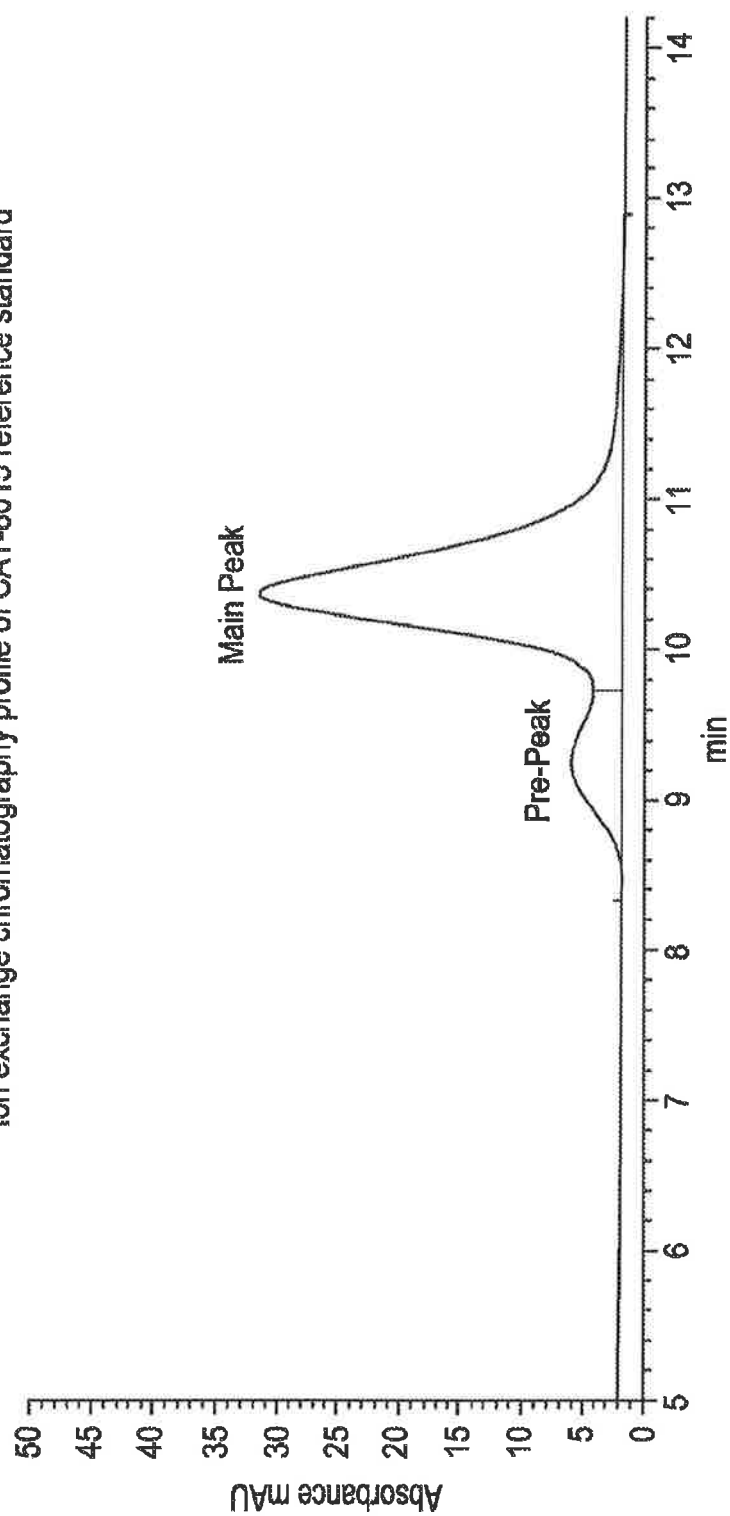


FIG. 2

Correlation between % Relative Potency and % Pre-Peak

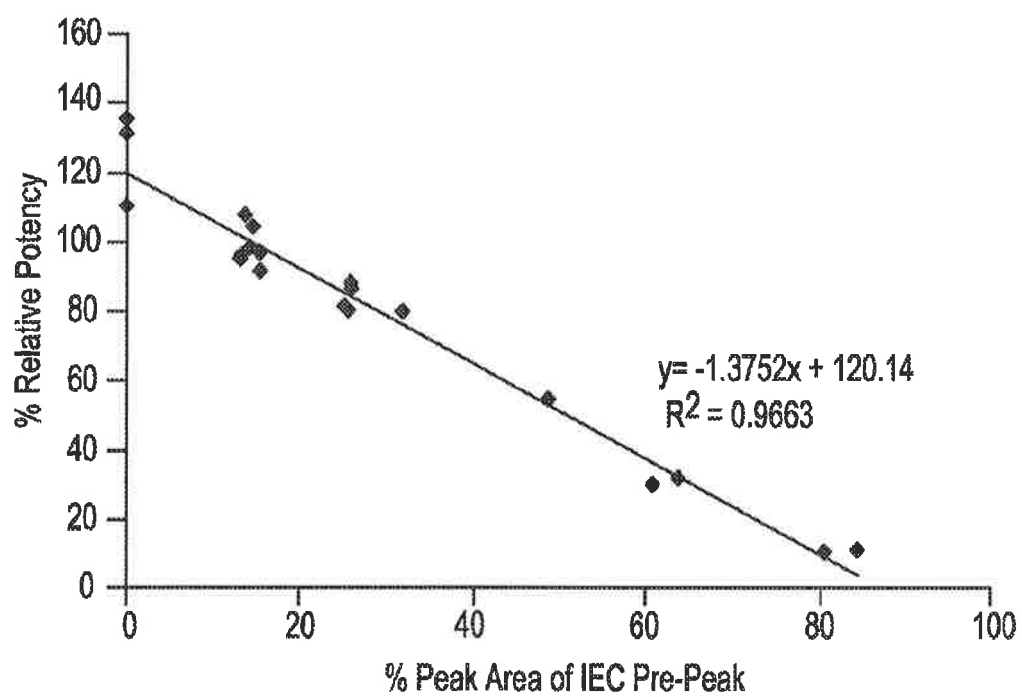


FIG. 3
Purification of CAT-8015 by Q Sepharose HP Chromatography

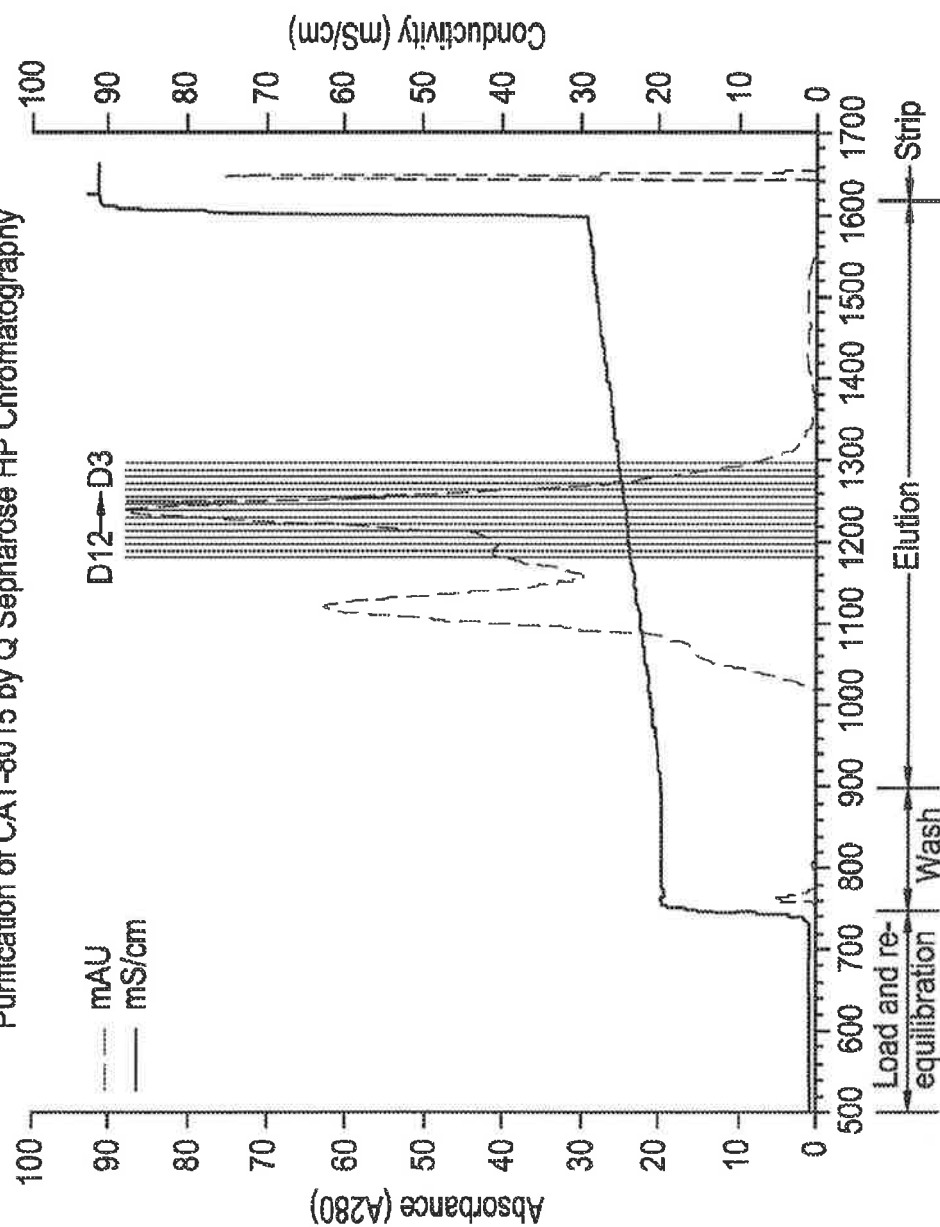


FIG. 4

SDS-PAGE Analysis of QHP
Load and Eluate Pool Samples

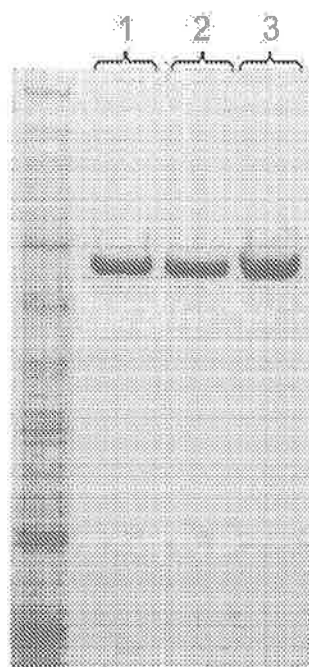


FIG. 5
Large Scale Purification of CAT-8015 on QHP


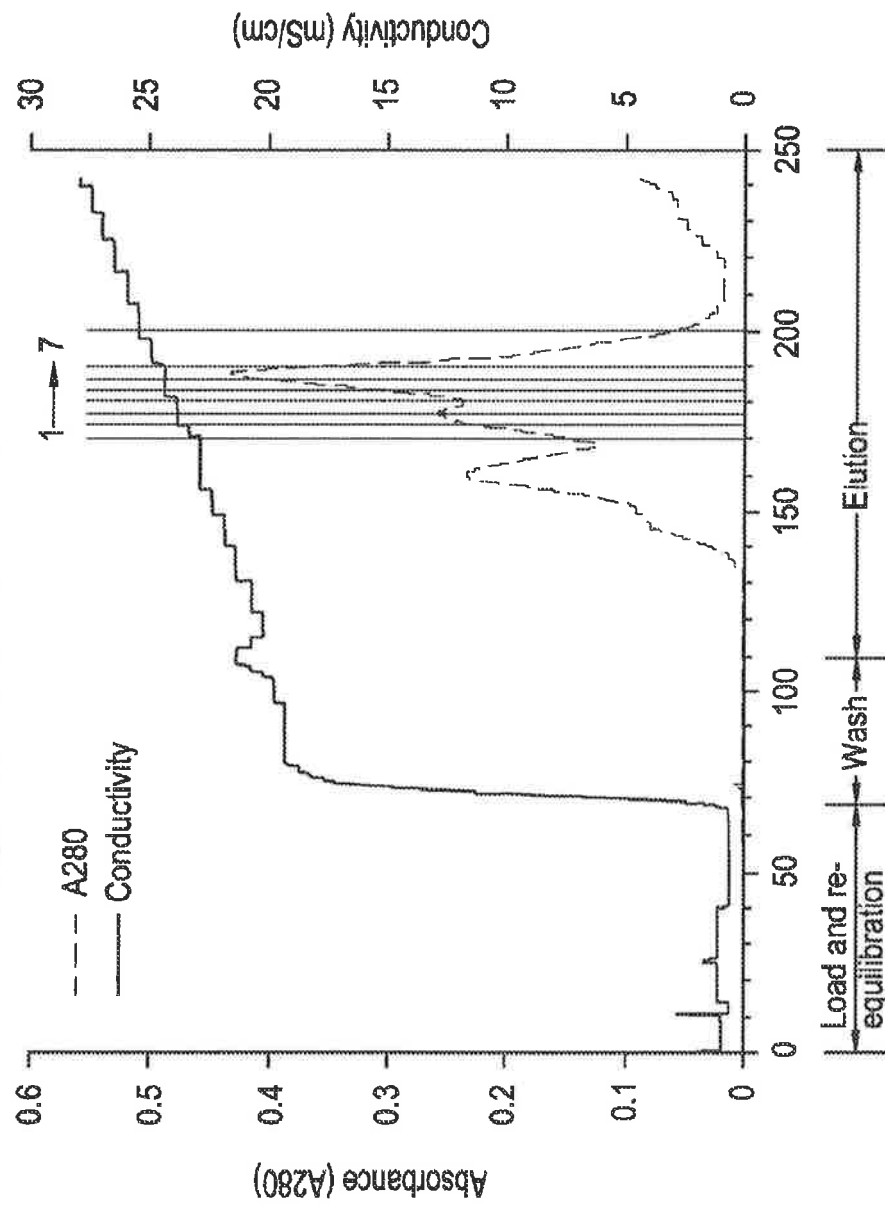


FIG. 6

SDS-PAGE Analysis of QHP Load and Eluate Pool Samples

**FIG. 7**

Percent Pre-Peak in HA Product as a Function of Solubilization pH

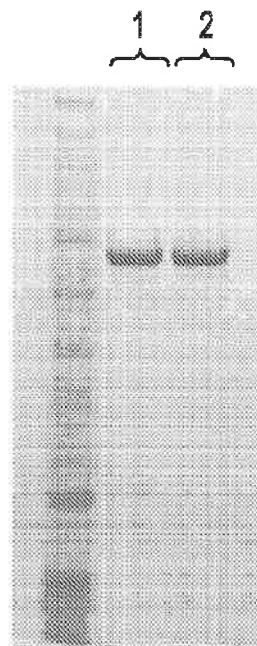