

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
24 July 2003 (24.07.2003)

(10) International Publication Number
WO 03/059235 A2

PCT

(51) International Patent Classification⁷: **A61G**

(21) International Application Number: PCT/US03/01138

(22) International Filing Date: 15 January 2003 (15.01.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/348,999 15 January 2002 (15.01.2002) US

(71) Applicant: STERIS INC. [US/US]; 43425 Business Park Drive, Temecula, CA 92590 (US).

(72) Inventors: RUS, Steven, H.; 112 Woodbridge Lane, Chardon, OH 44024 (US). **DRABINSKI, Terry, A.;** 3096 Northview Drive, Stow, OH 44224 (US). **PETRUCCHI,**


James, A.; 12121 Woodchuck Hollow, Chesterland, OH 44026 (US). **JESURUN, David;** 1196 Dorsh Road, South Euclid, OH 44121 (US). **GRESZLER, Allan, J.;** 10150 East River Road, Elyria, OH 44035 (US). **KESELMAN, Yury;** 24002 East Baintree Road, Beachwood, OH 44122 (US).

(74) Agent: KOCOVSKY, Thomas, E.; Fay, Sharpe, Fagan,
Minnich & McKee, LLP, 7th Floor, 1100 Superior Avenue,
Cleveland, OH 44114 (US).

(81) Designated States (national): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, OM, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, UZ, VC, VN, YU, ZA, ZM, ZW.

[Continued on next page]

(54) Title: SURGICAL LIGHTING CONTROL VIDEO SYSTEM

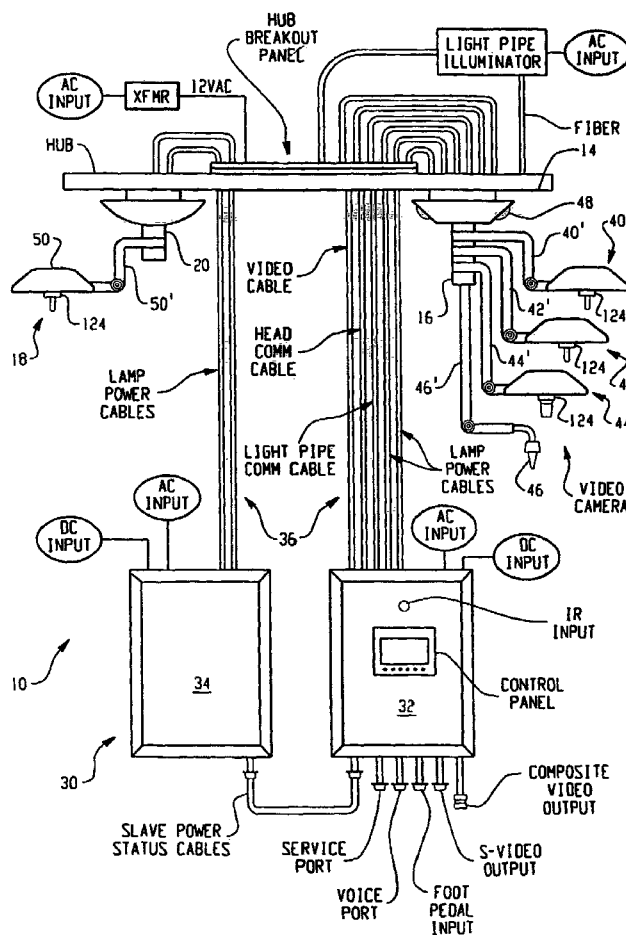

(57) Abstract: A surgical light system (10) includes a lighthead (44) coupled to a suspension arm (41') adapted for mounting to a surface (14) of a surgical room. A bulb (130) is disposed in the lighthead. A processor (120) in the lighthead is operatively coupled with the bulb for controlling an intensity of light of the bulb and is adapted to generate a lighthead status signal representative of a first status of the lighthead. A control apparatus (32, 34) is in operative communication with the processor (120) in the lighthead. The control apparatus receives the lighthead status signal and selects a set of control algorithms from among a group of algorithms based on the lighthead status signal for controlling the lighthead. The lighthead status signal includes information regarding a size of the lighthead, an intensity of light from the bulb, a condition of the bulb, a level of current applied to the bulb, a level of current applied to the bulb, a level of voltage applied to the bulb, an internal temperature of the lighthead, and the presence of one or more of a video camera, a surgical task light, and a controllable ambient light. A human-readable display device (160) is provided for displaying information relating to the lighthead status signal. Several levels of redundancy are provided in the control system to minimize the potential loss of control due to failures. In that regard, the lightheads are operable when the control apparatus (32, 34) fails.



(84) Designated States (regional): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— without international search report and to be republished upon receipt of that report

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.