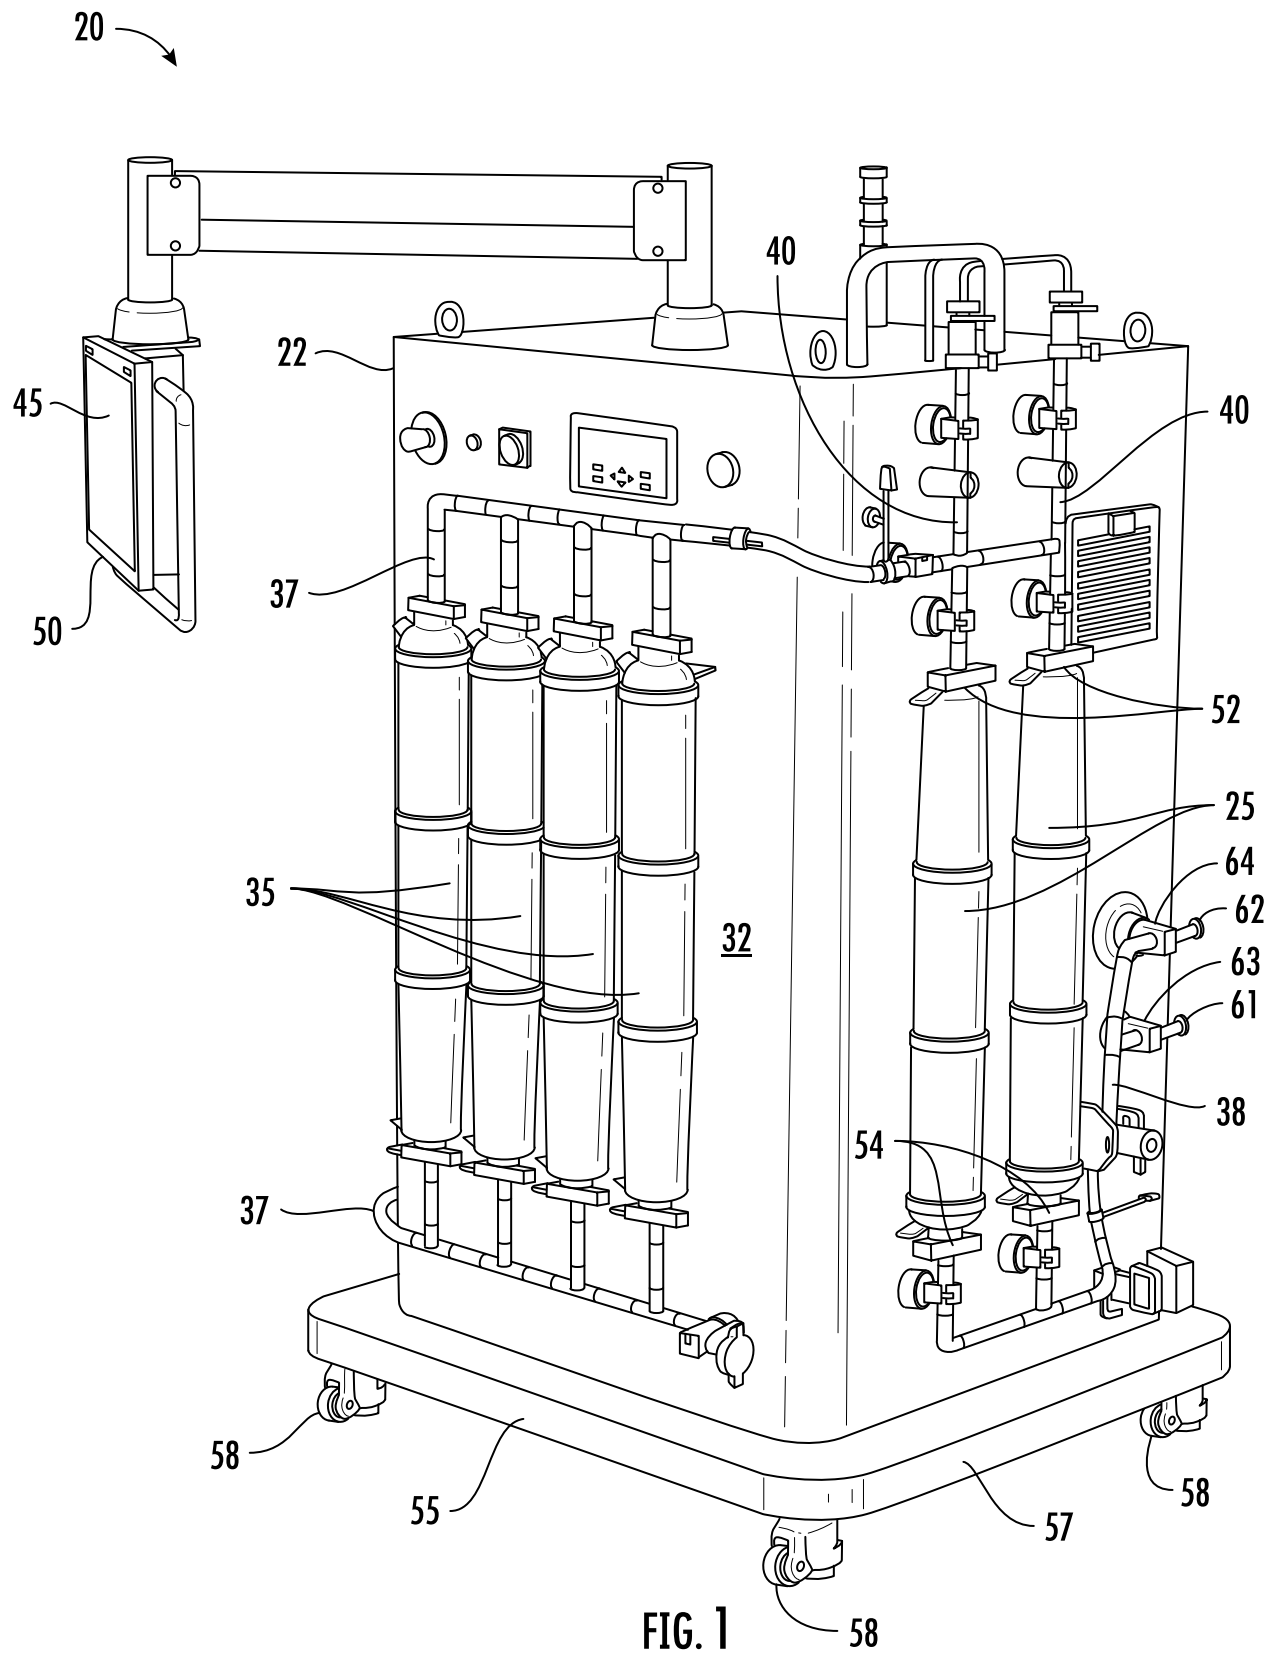




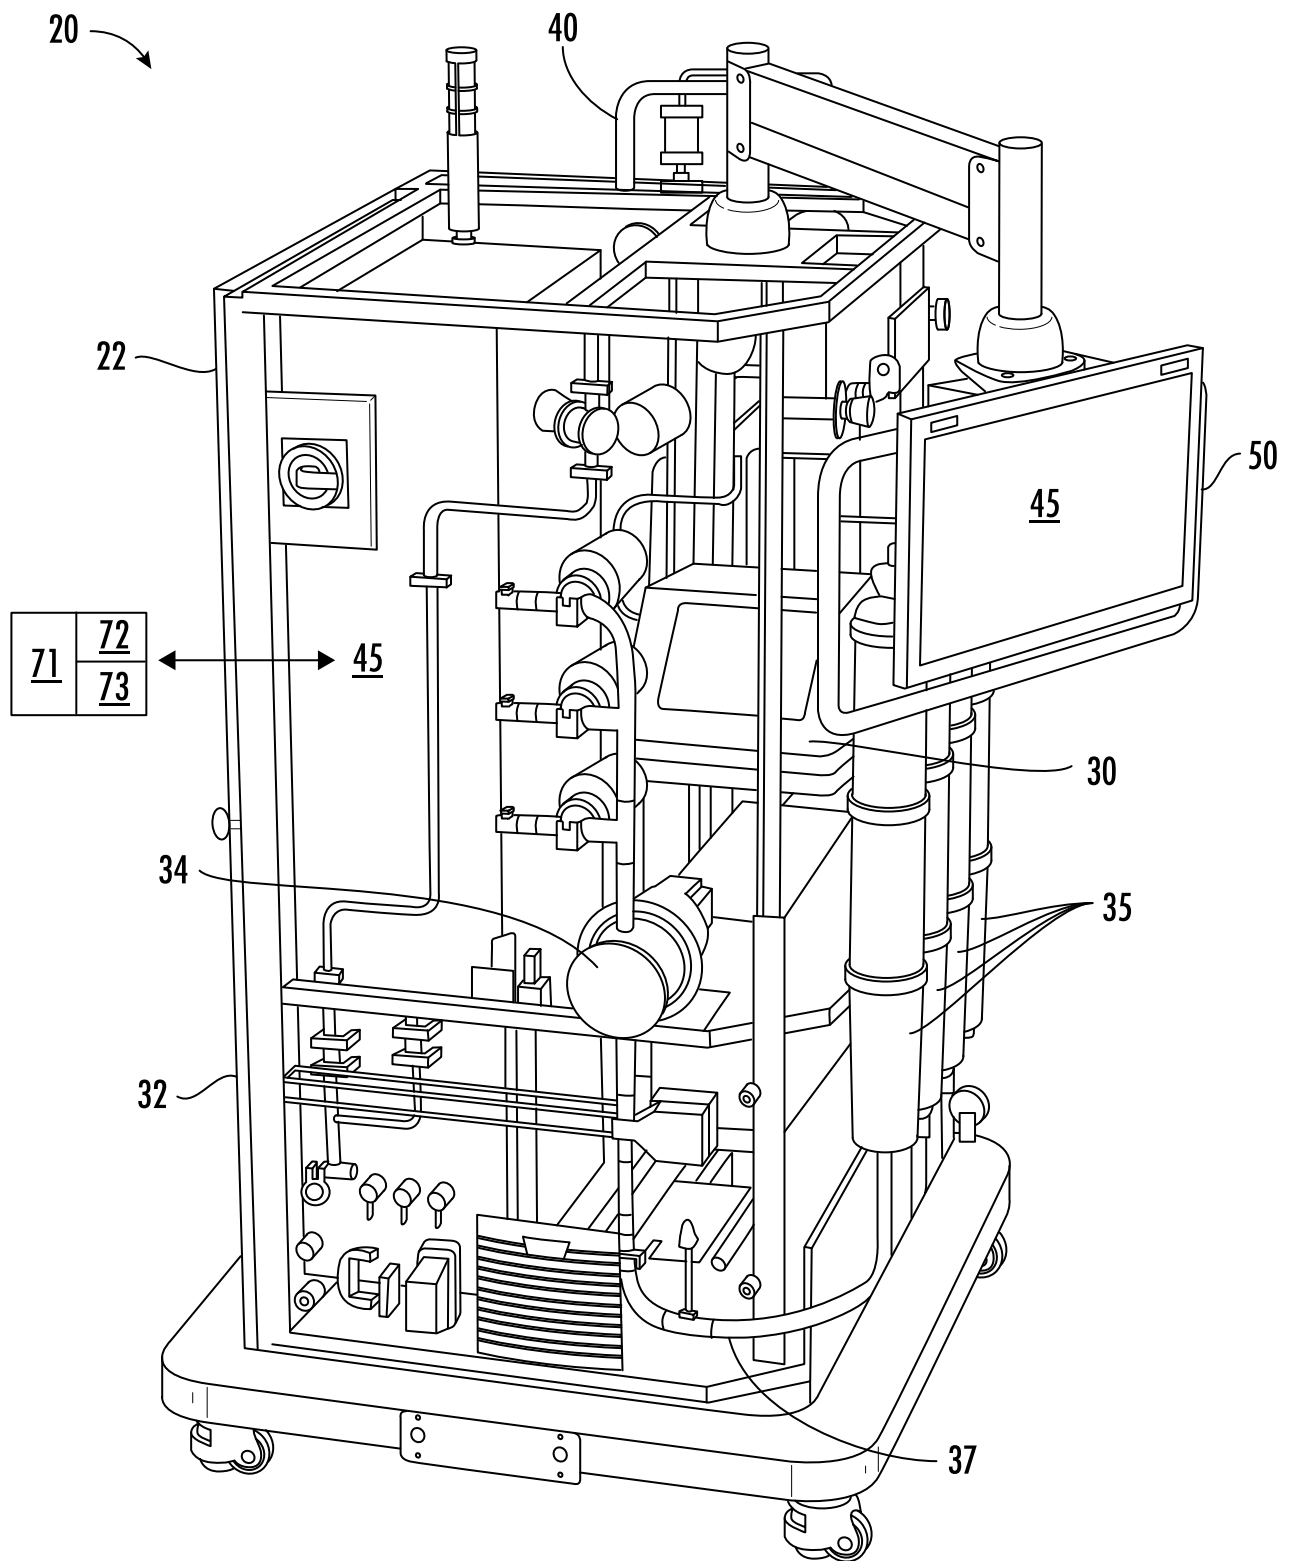


FIG. 2

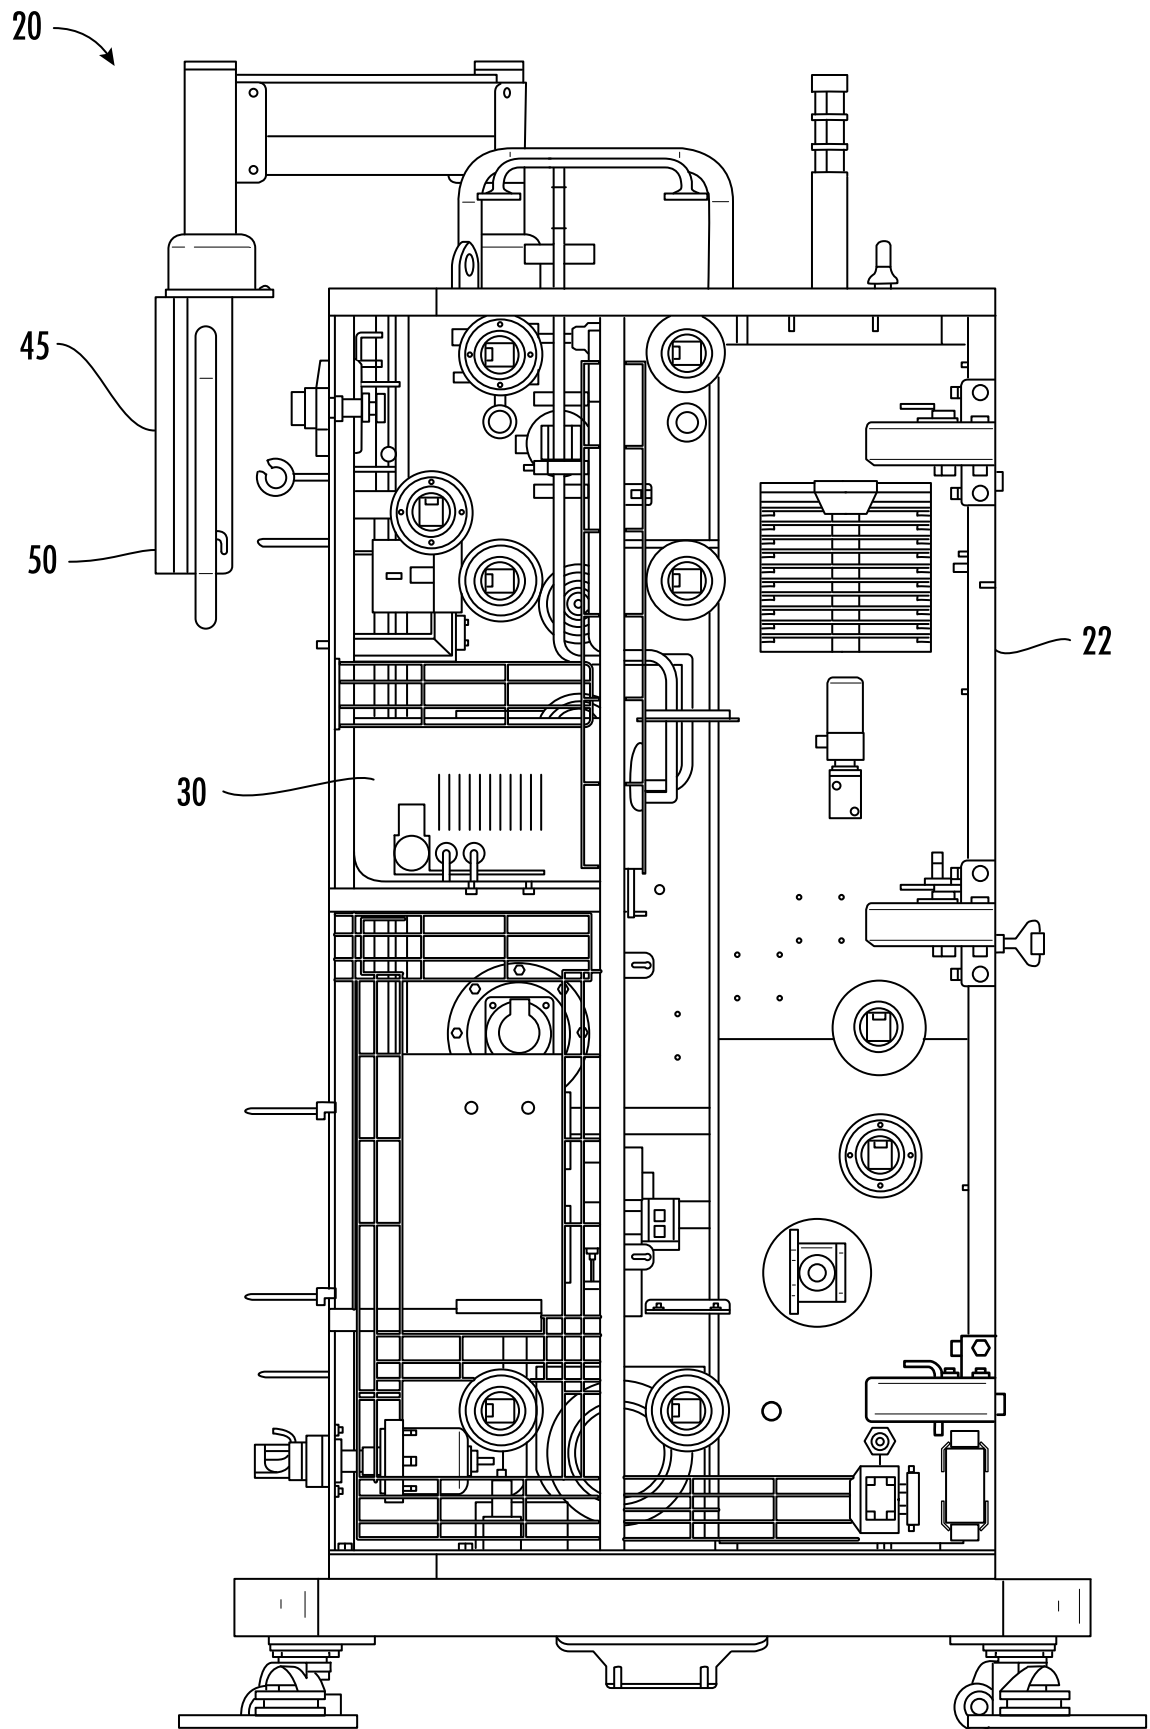
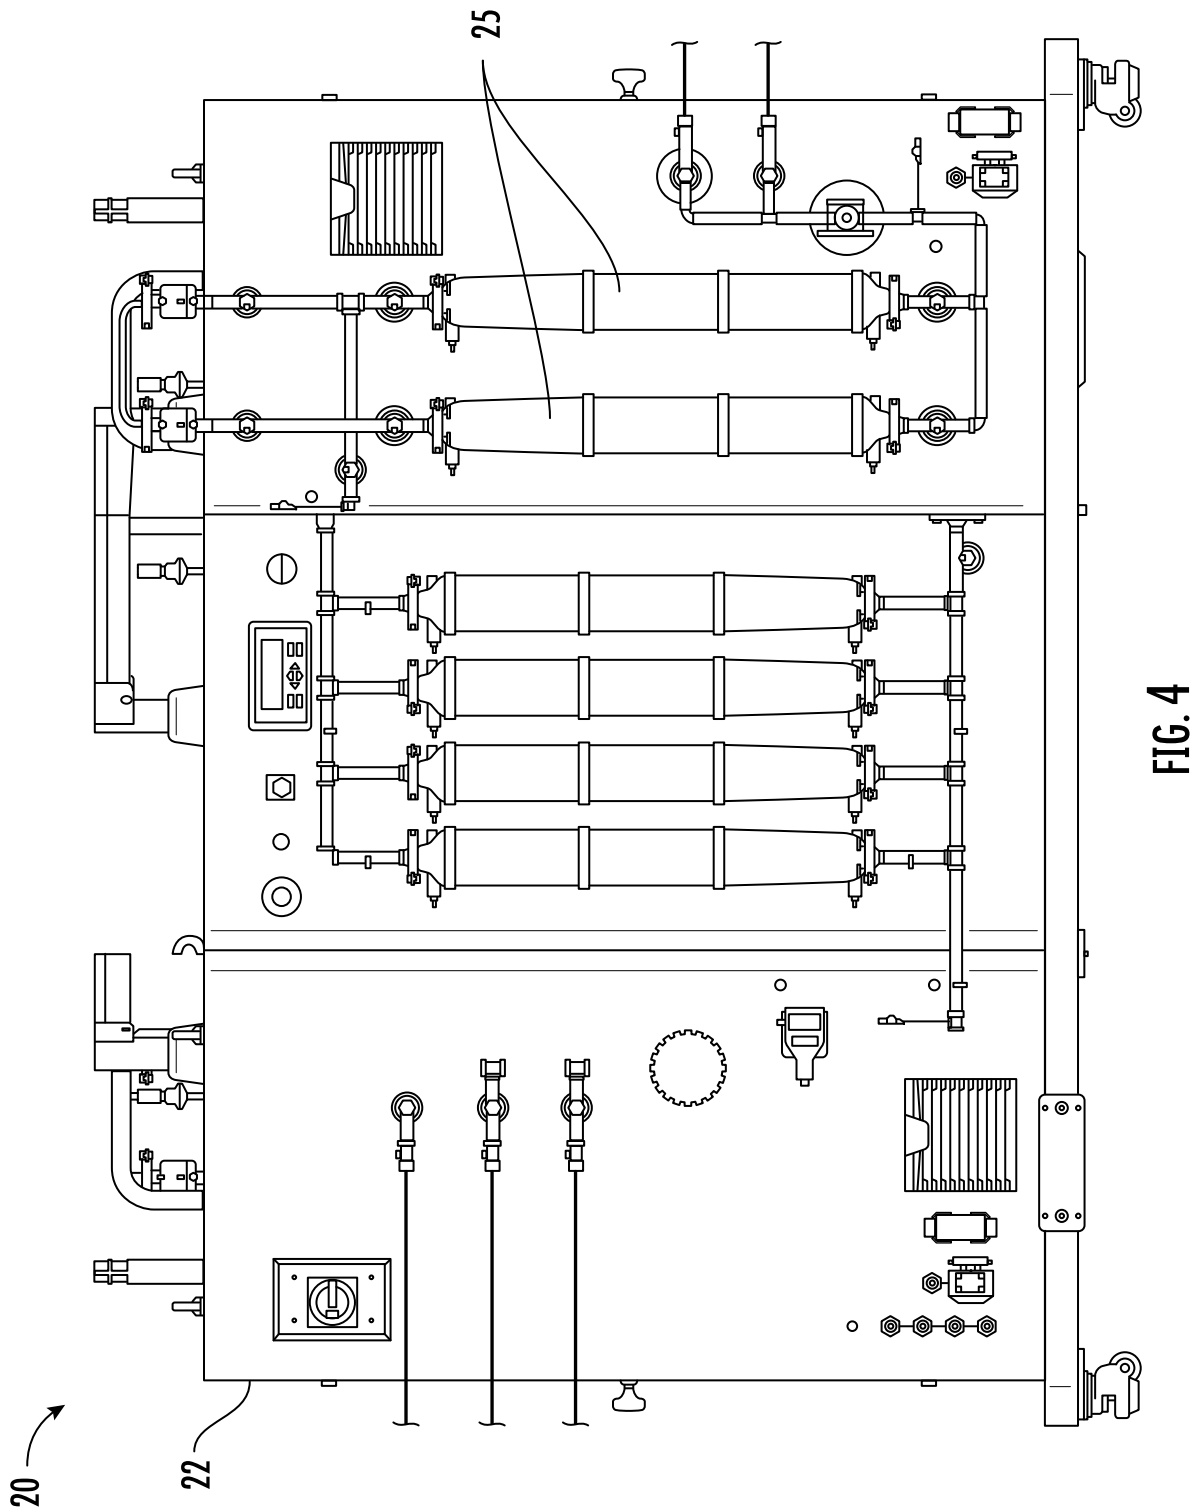
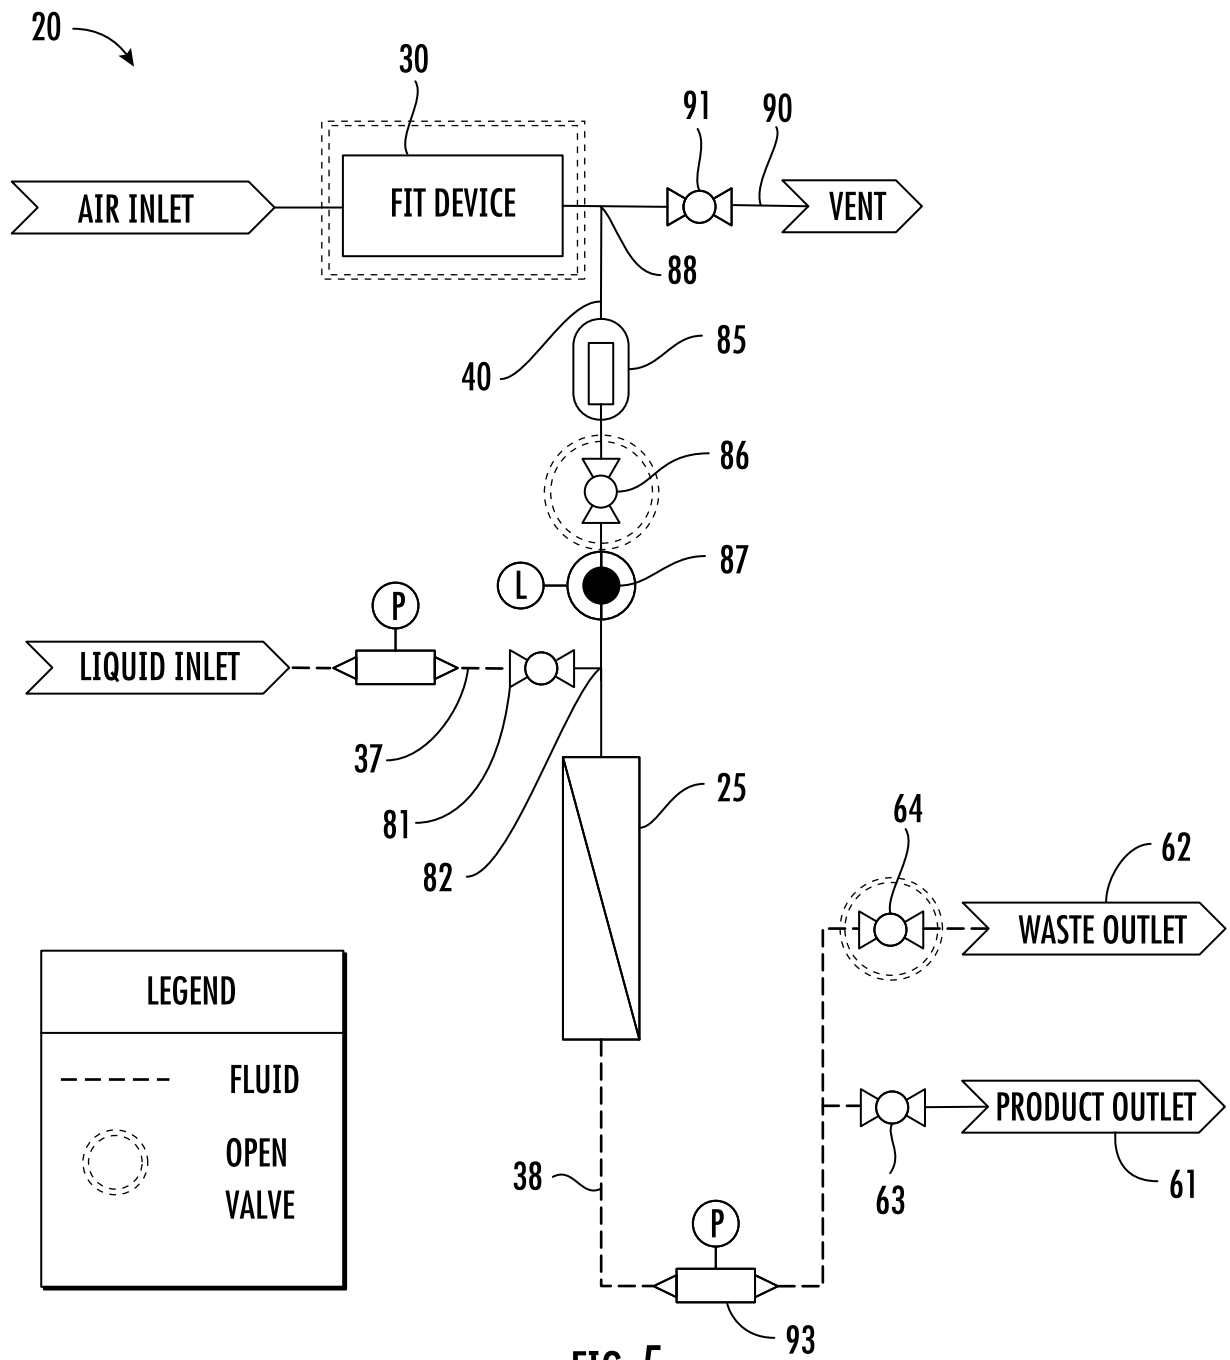


FIG. 3





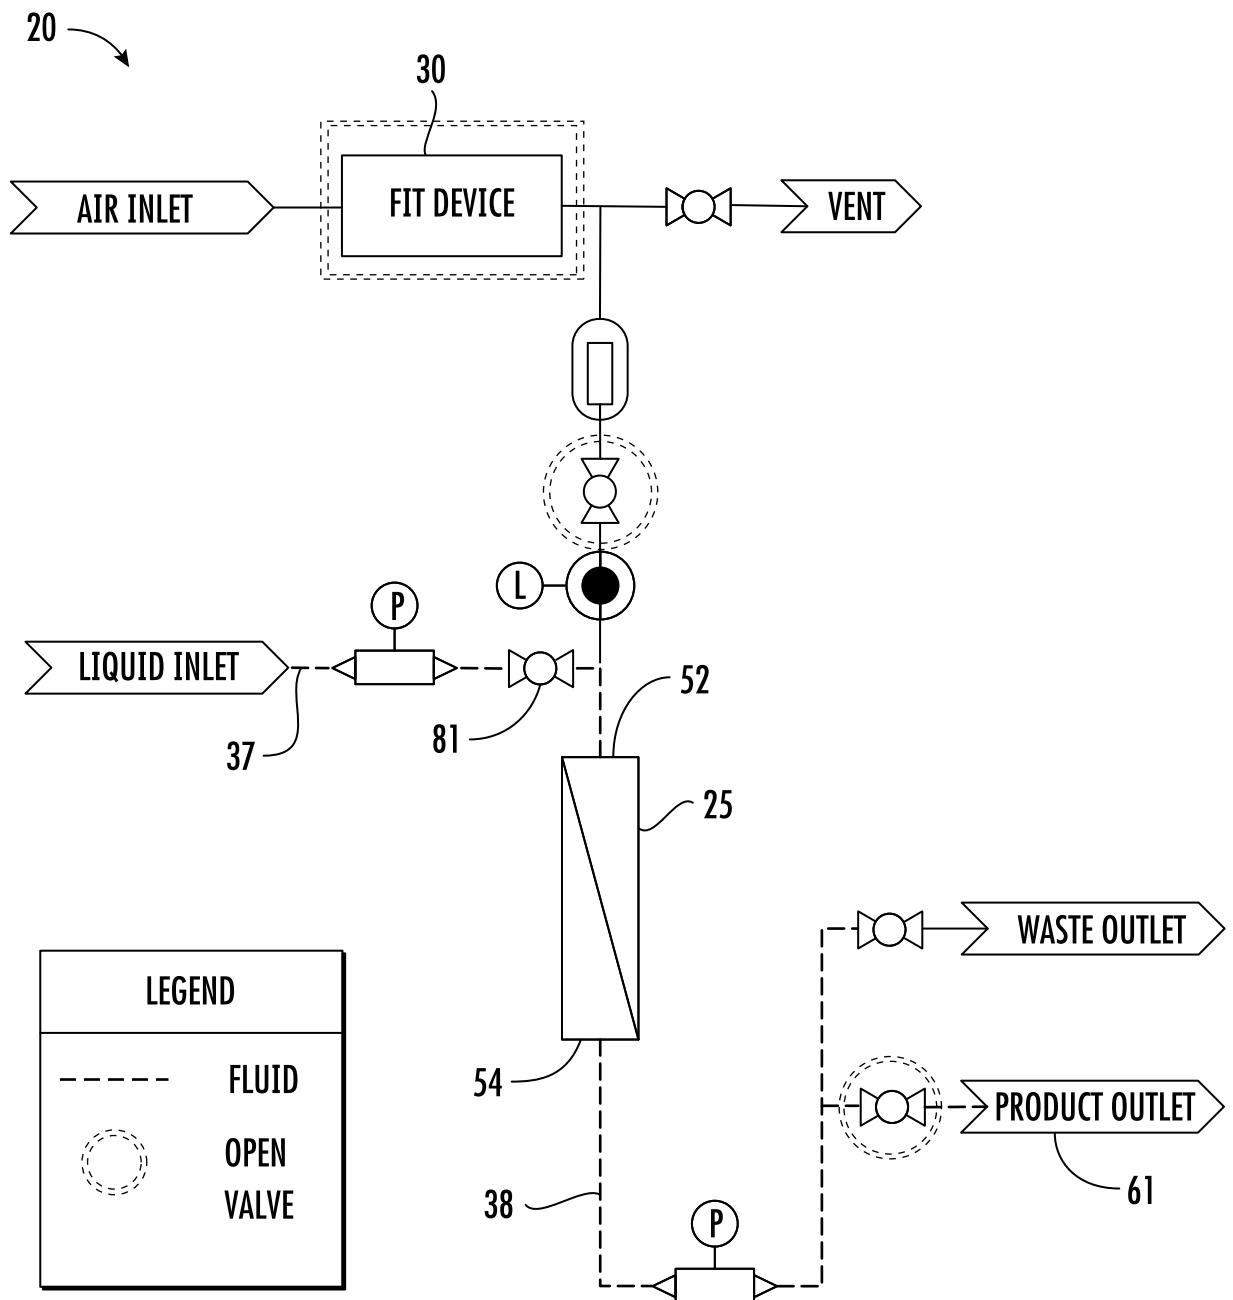


FIG. 6

95 →

BULK FILL
MBF01
23-MAR-2021
07:27:18

BATCH
RECIPE
UNIT OP
OPERATION TESTOP

BATCH 283
TESTFILTERIT
UNITOP

OK

RPHP05FILTERIT - RUN

EEENG

LOG OUT

FORWARD FLOW TEST: F2 (TO FLUSH)

PRESSURIZATION

STABILIZATION

VENTING

RESULTS

☑ PASSED

49.9 ML/MIN

ACCEPTABLE RANGE: 10.0-100.0 ML/MIN

PRE-STABL PRESSURE: 50 MBAR	TEST PRESSURE: 50 MBAR	FILTER HOUSING: N/A	TEST STARTED: 07:24:46 MAR-23
PRE-STABL TIME: 0 S	TEST TIME: 100 S	WETTING LIQUID: WIT	TEST COMPLETE: 07:26:09 MAR-23
	SYSTEM VOLUME: N/A	TEST GAS: 02	

COMMENT:

RE-TEST

CONTINUE

🏠

⚙️

📊

📅

📄

📋

📄

📄

⚙️

PROCESS

ALARMS


TRENDS

EVENT LOG

RECIPES

REPORTS

FIG. 7

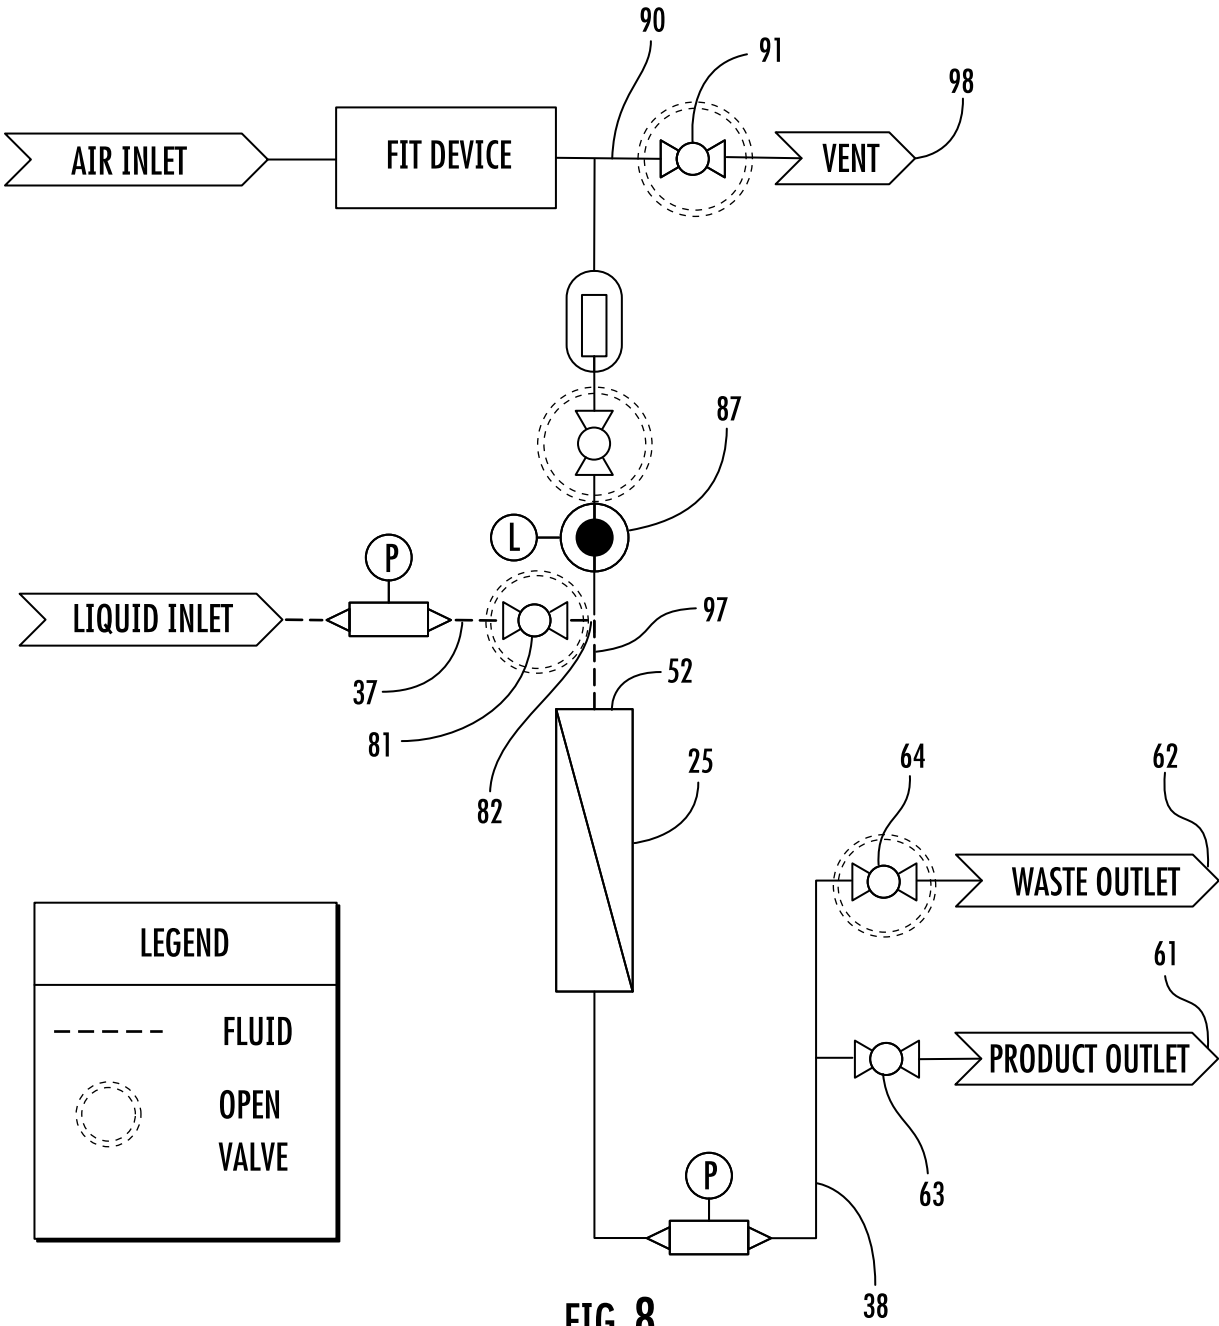

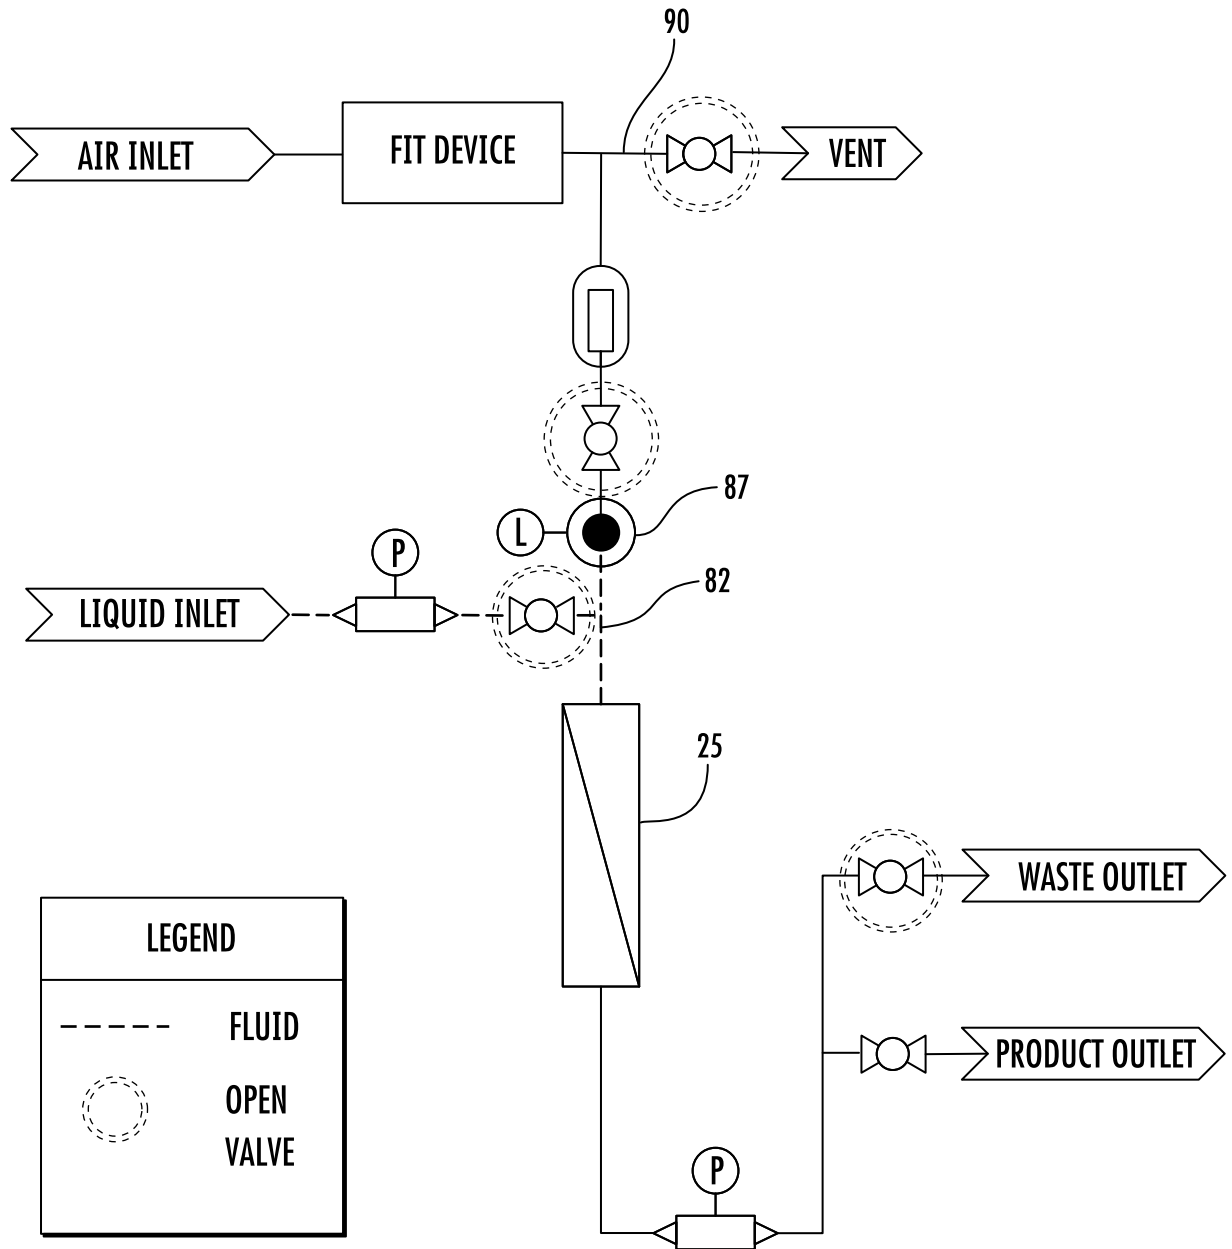
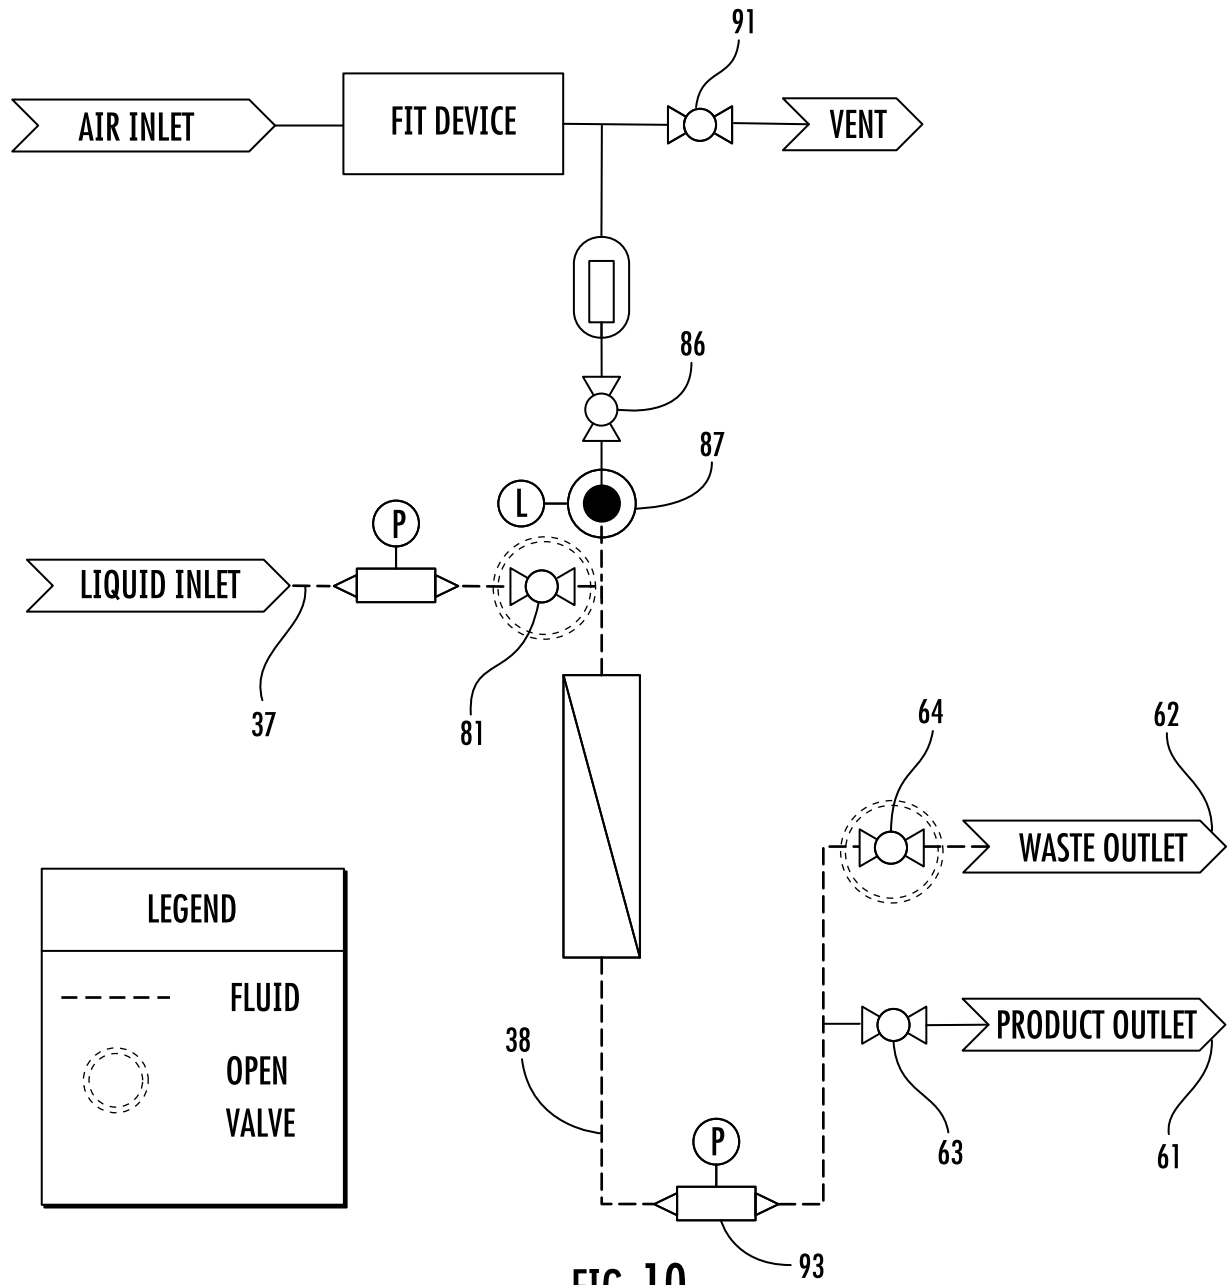
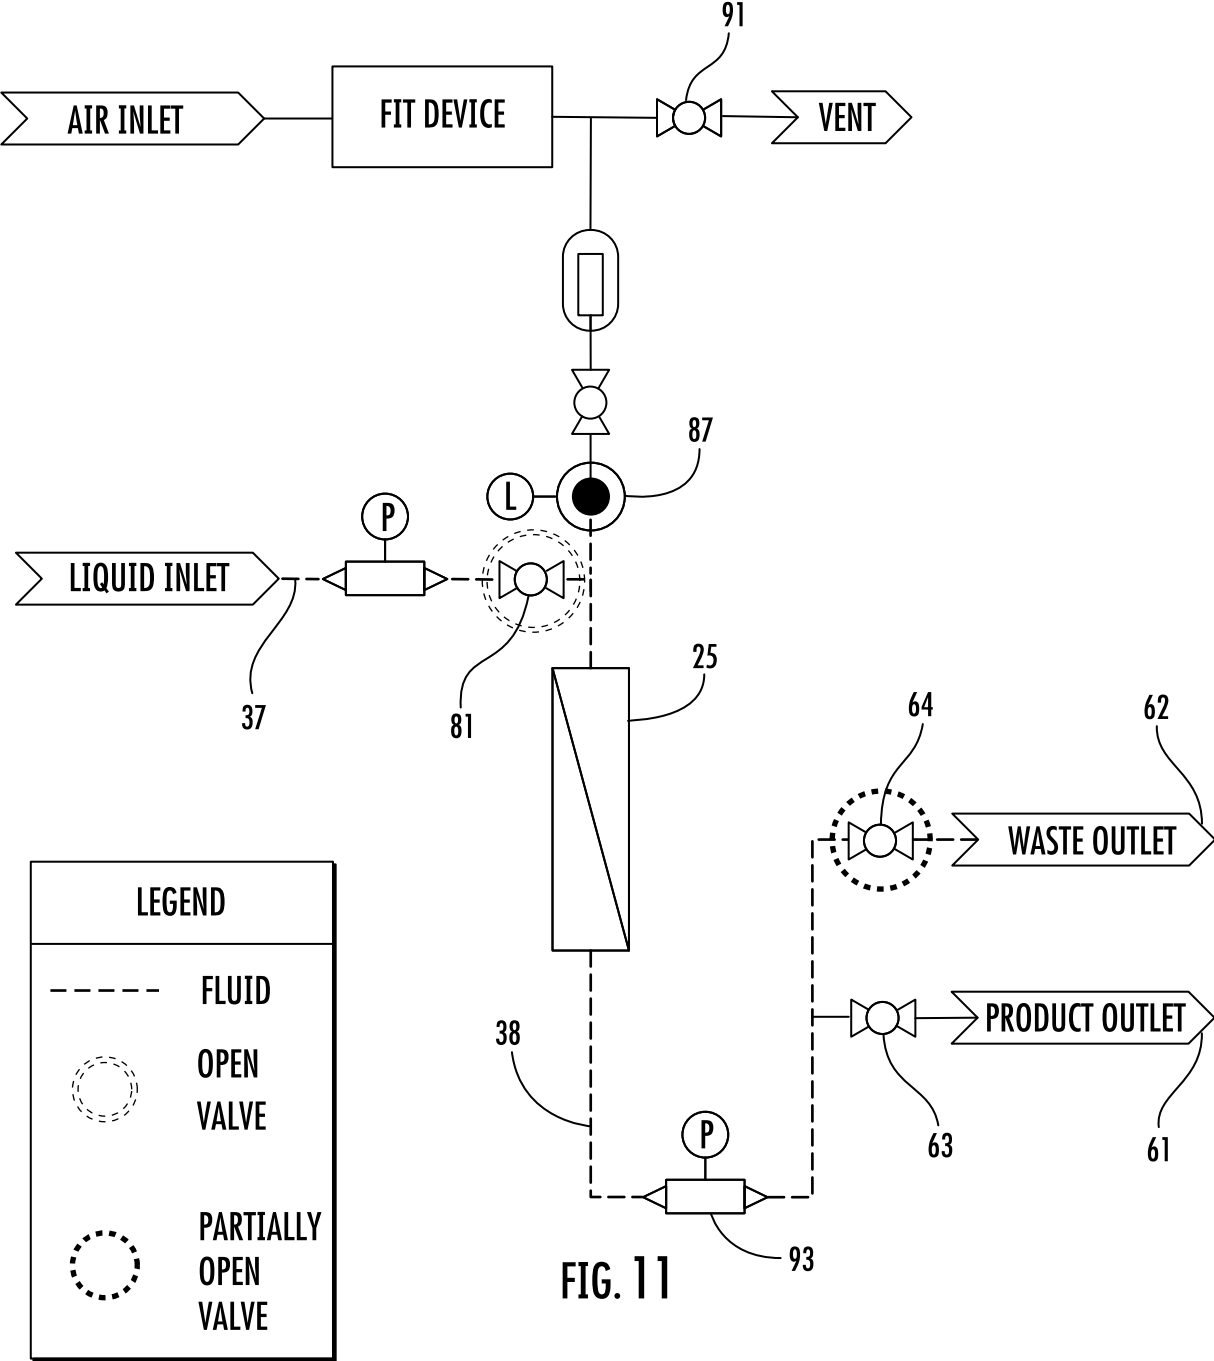


FIG. 9





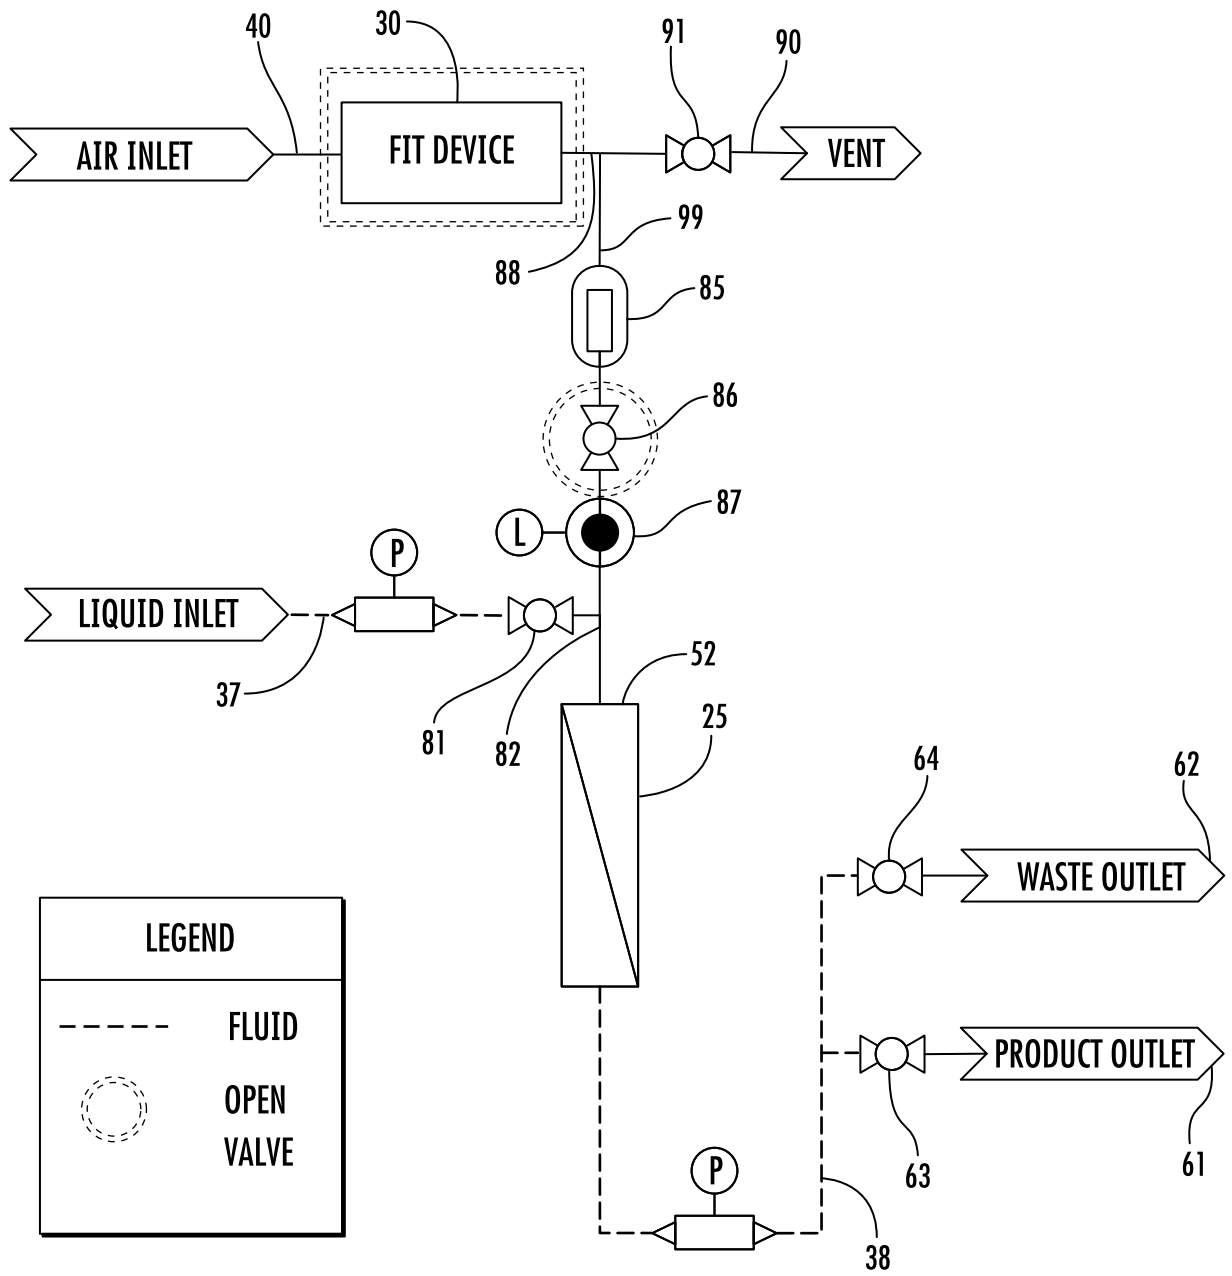


FIG. 12

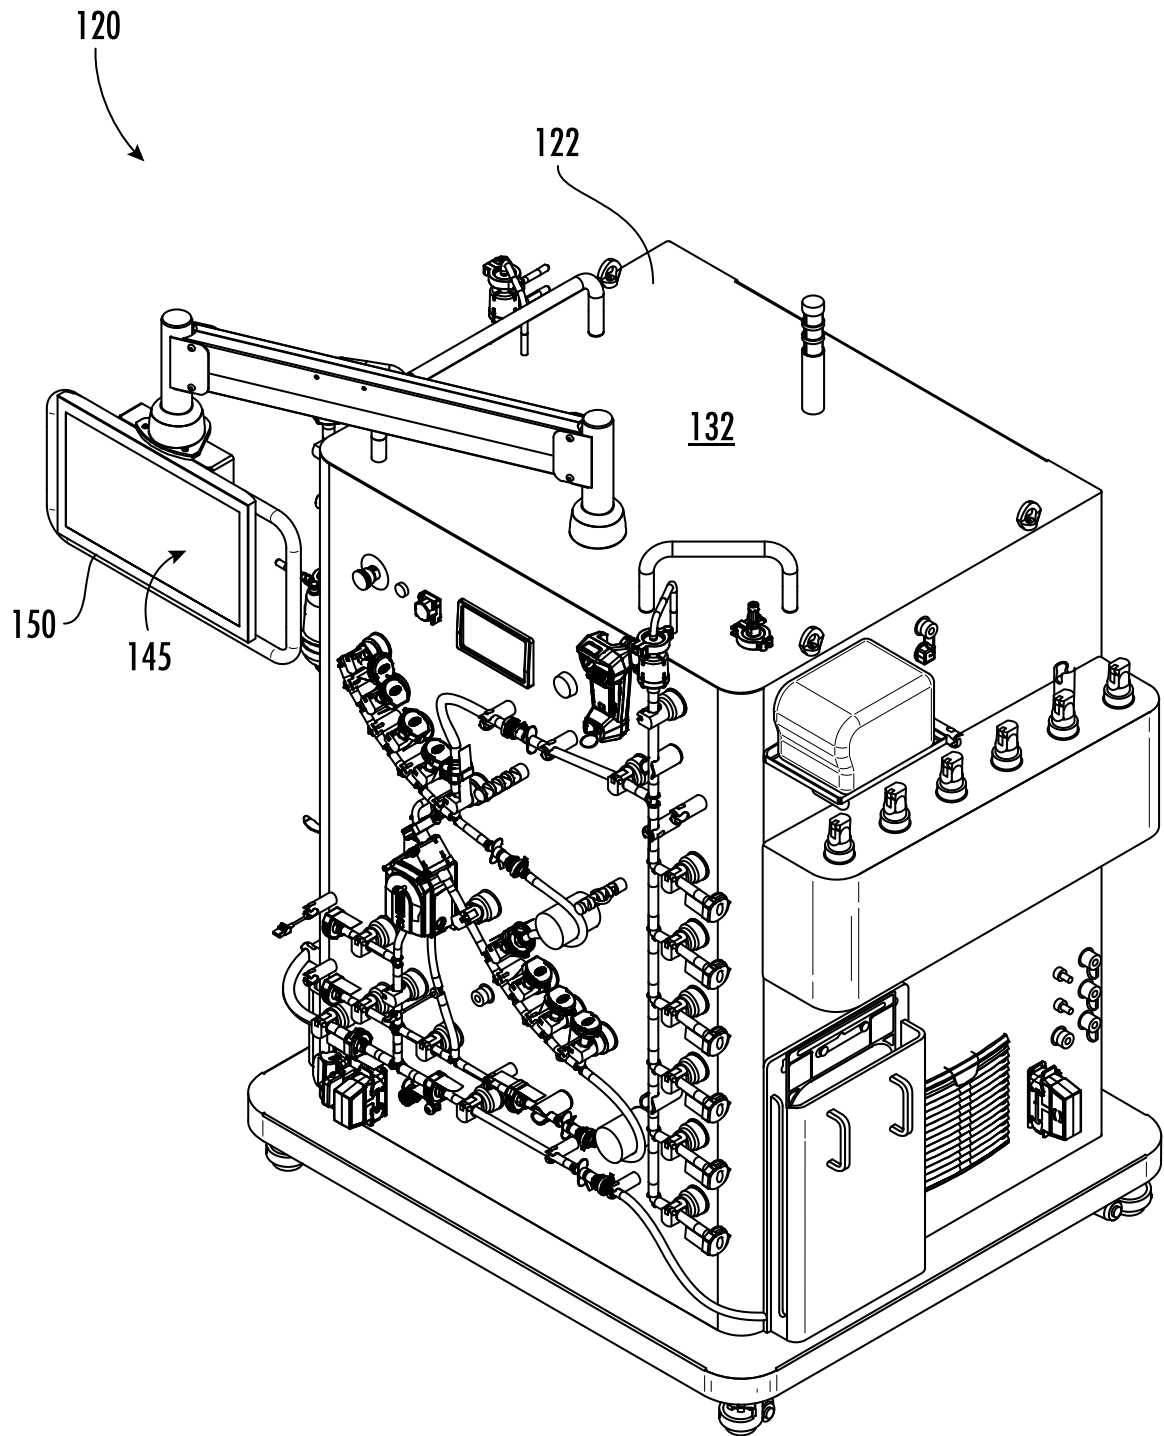


FIG. 13

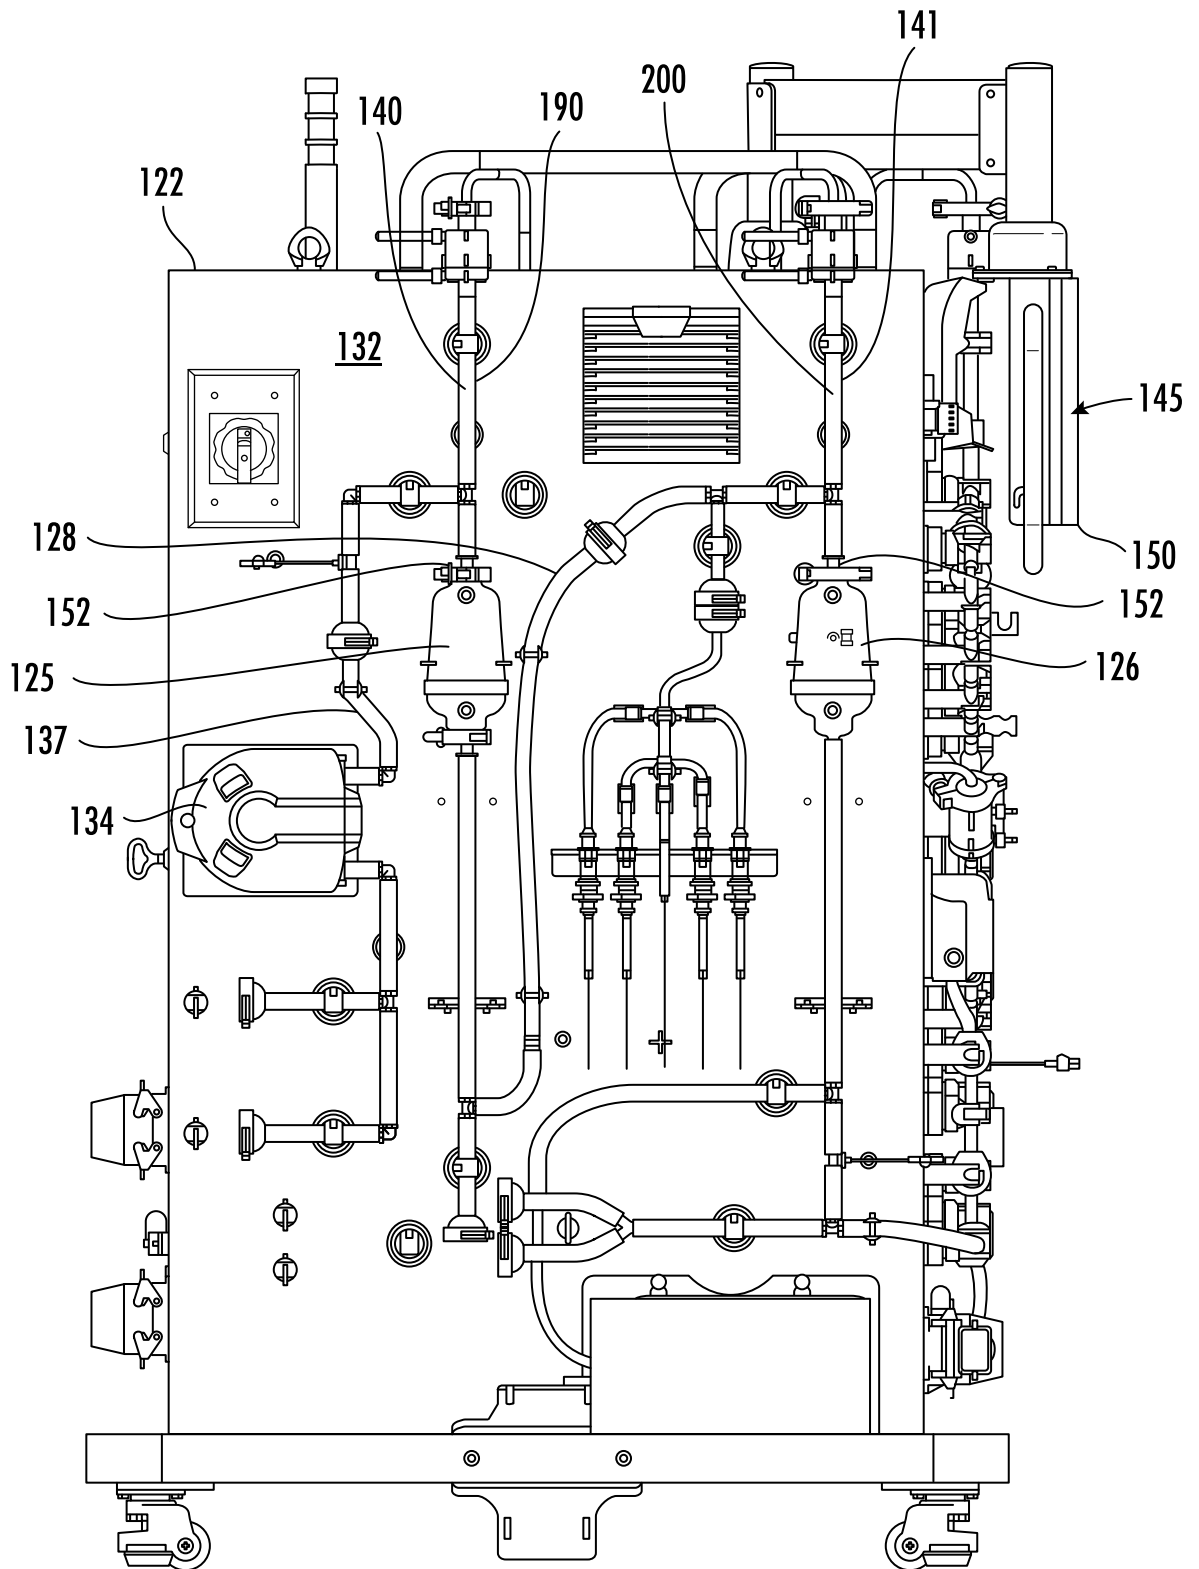


FIG. 14

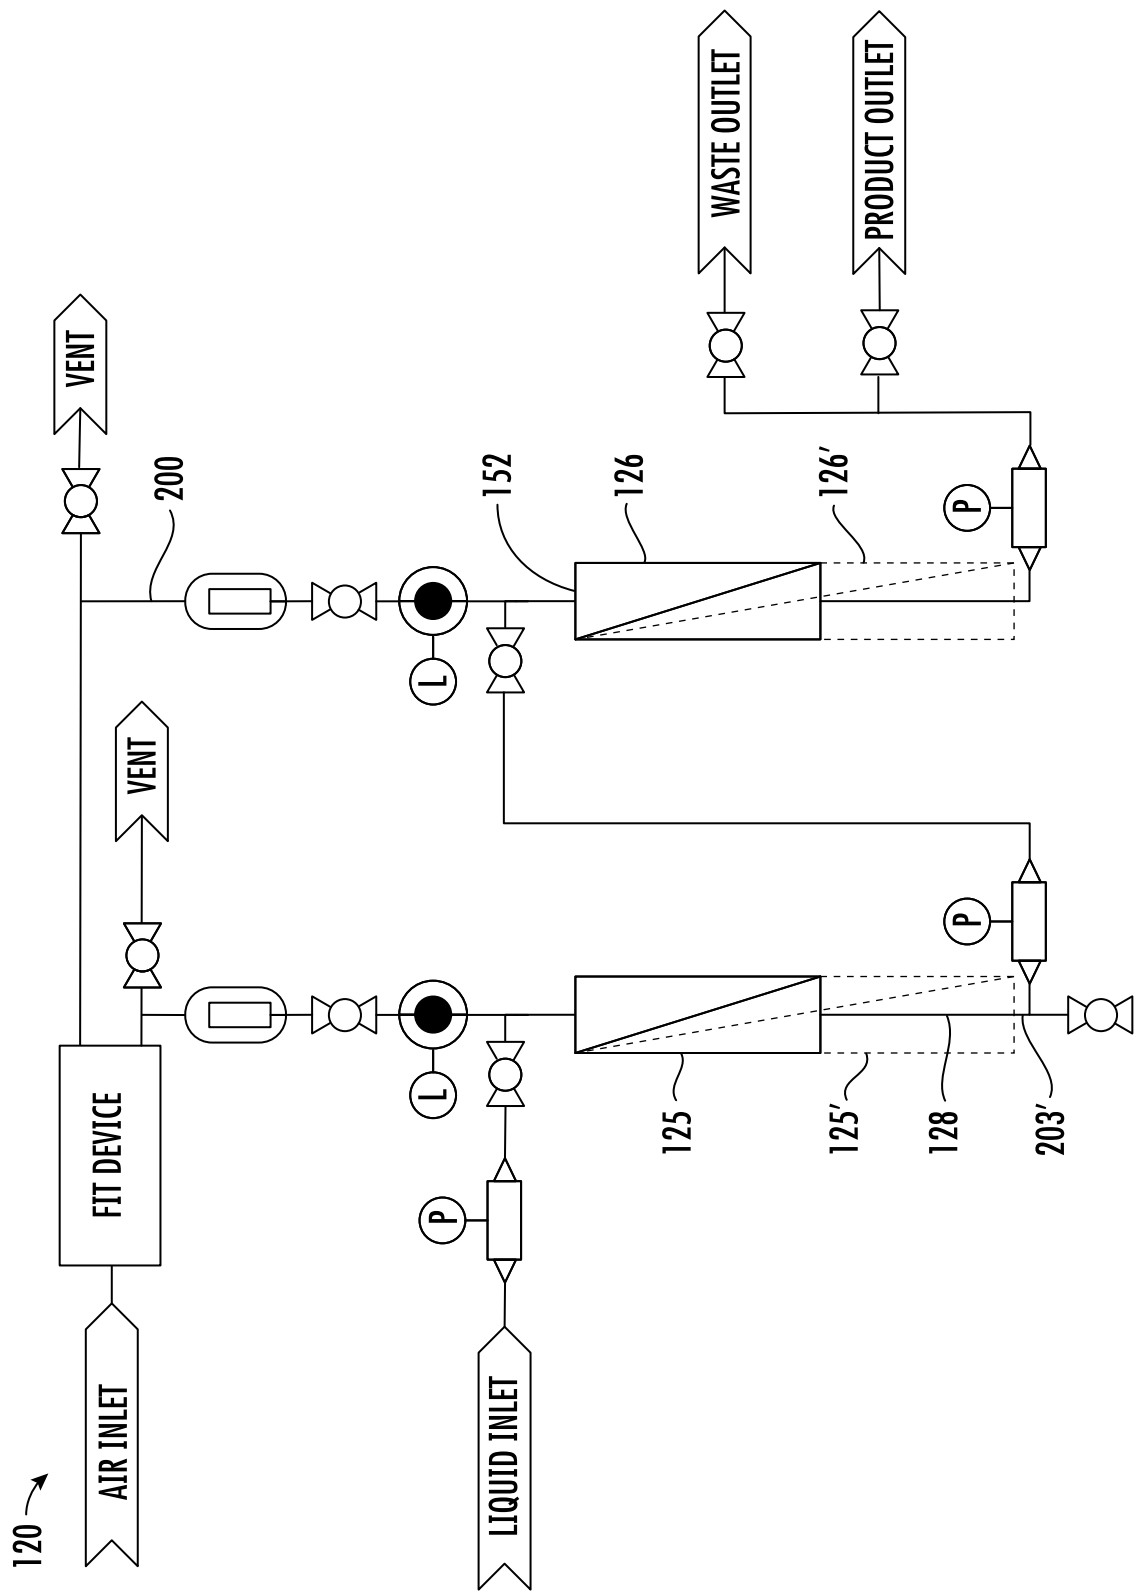


FIG. 15

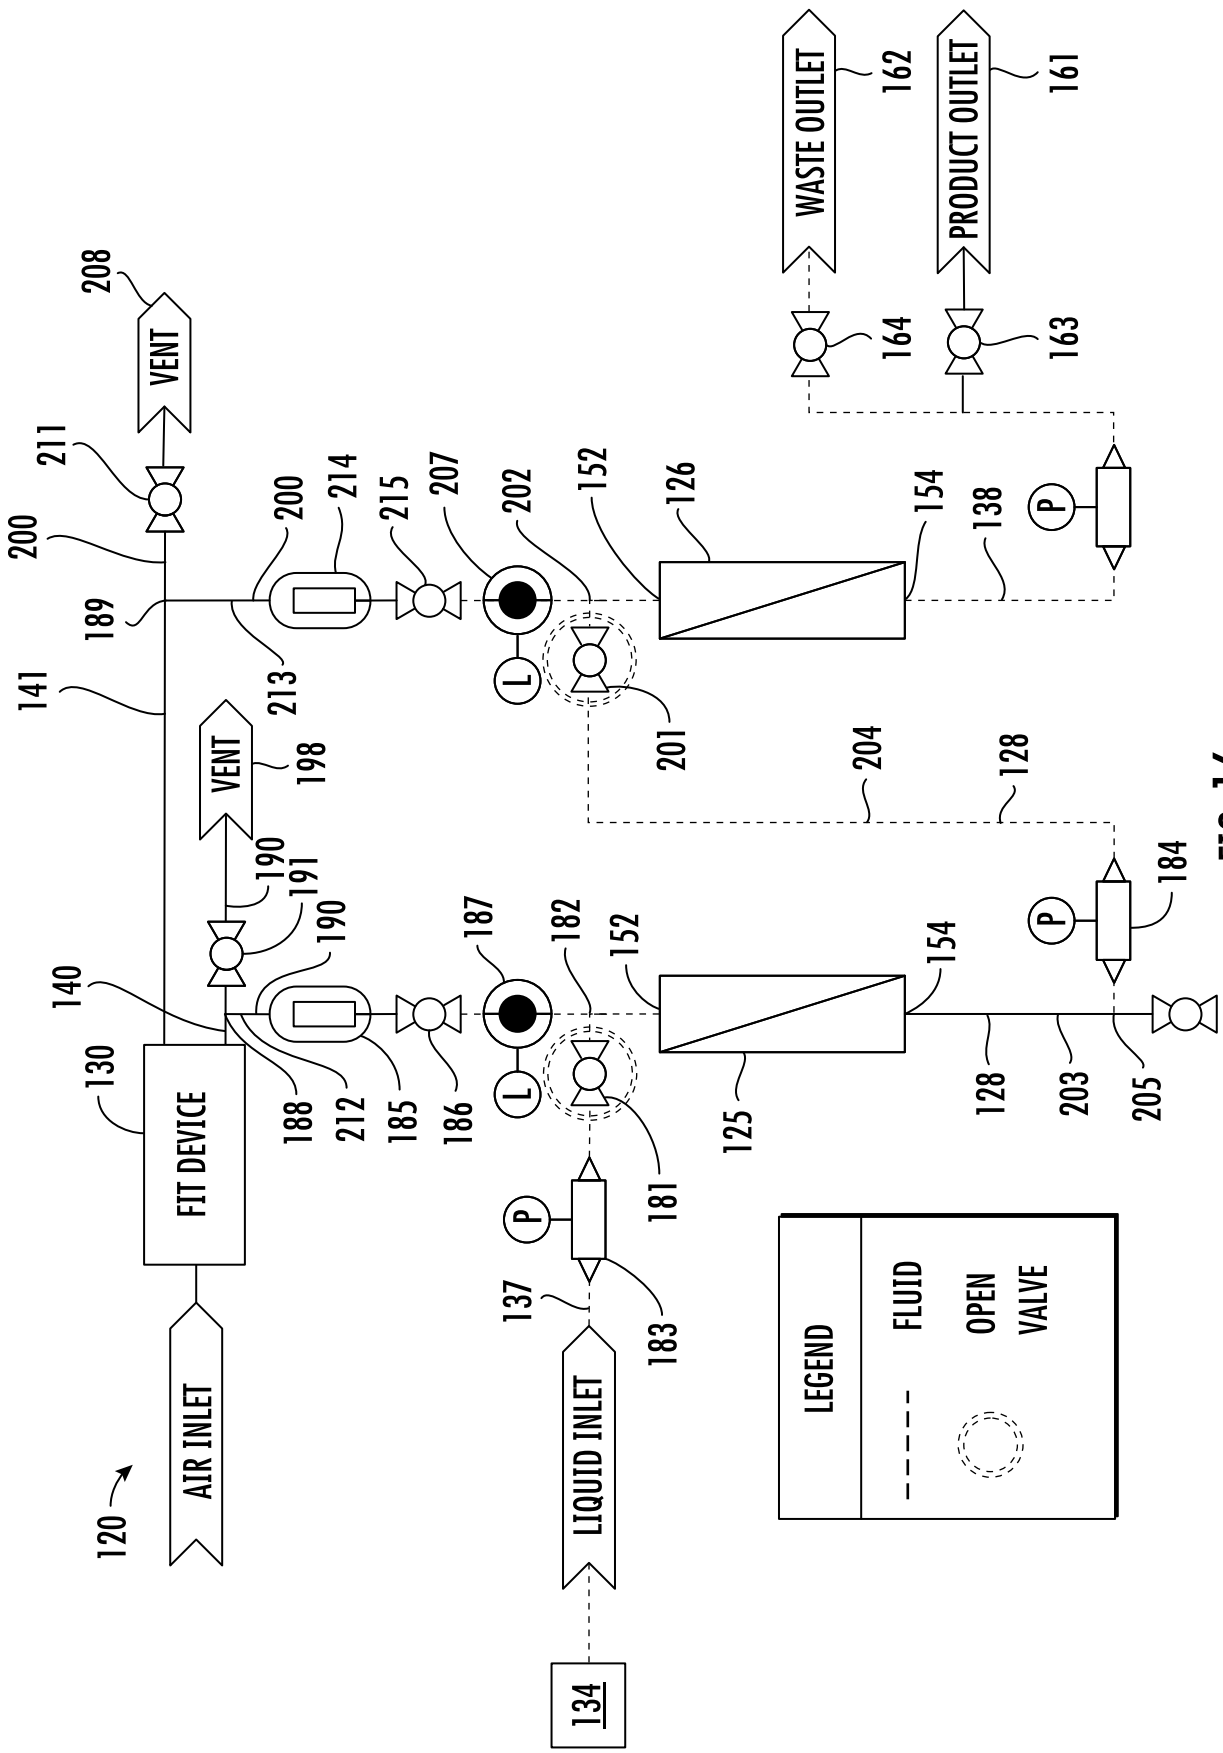


FIG. 16

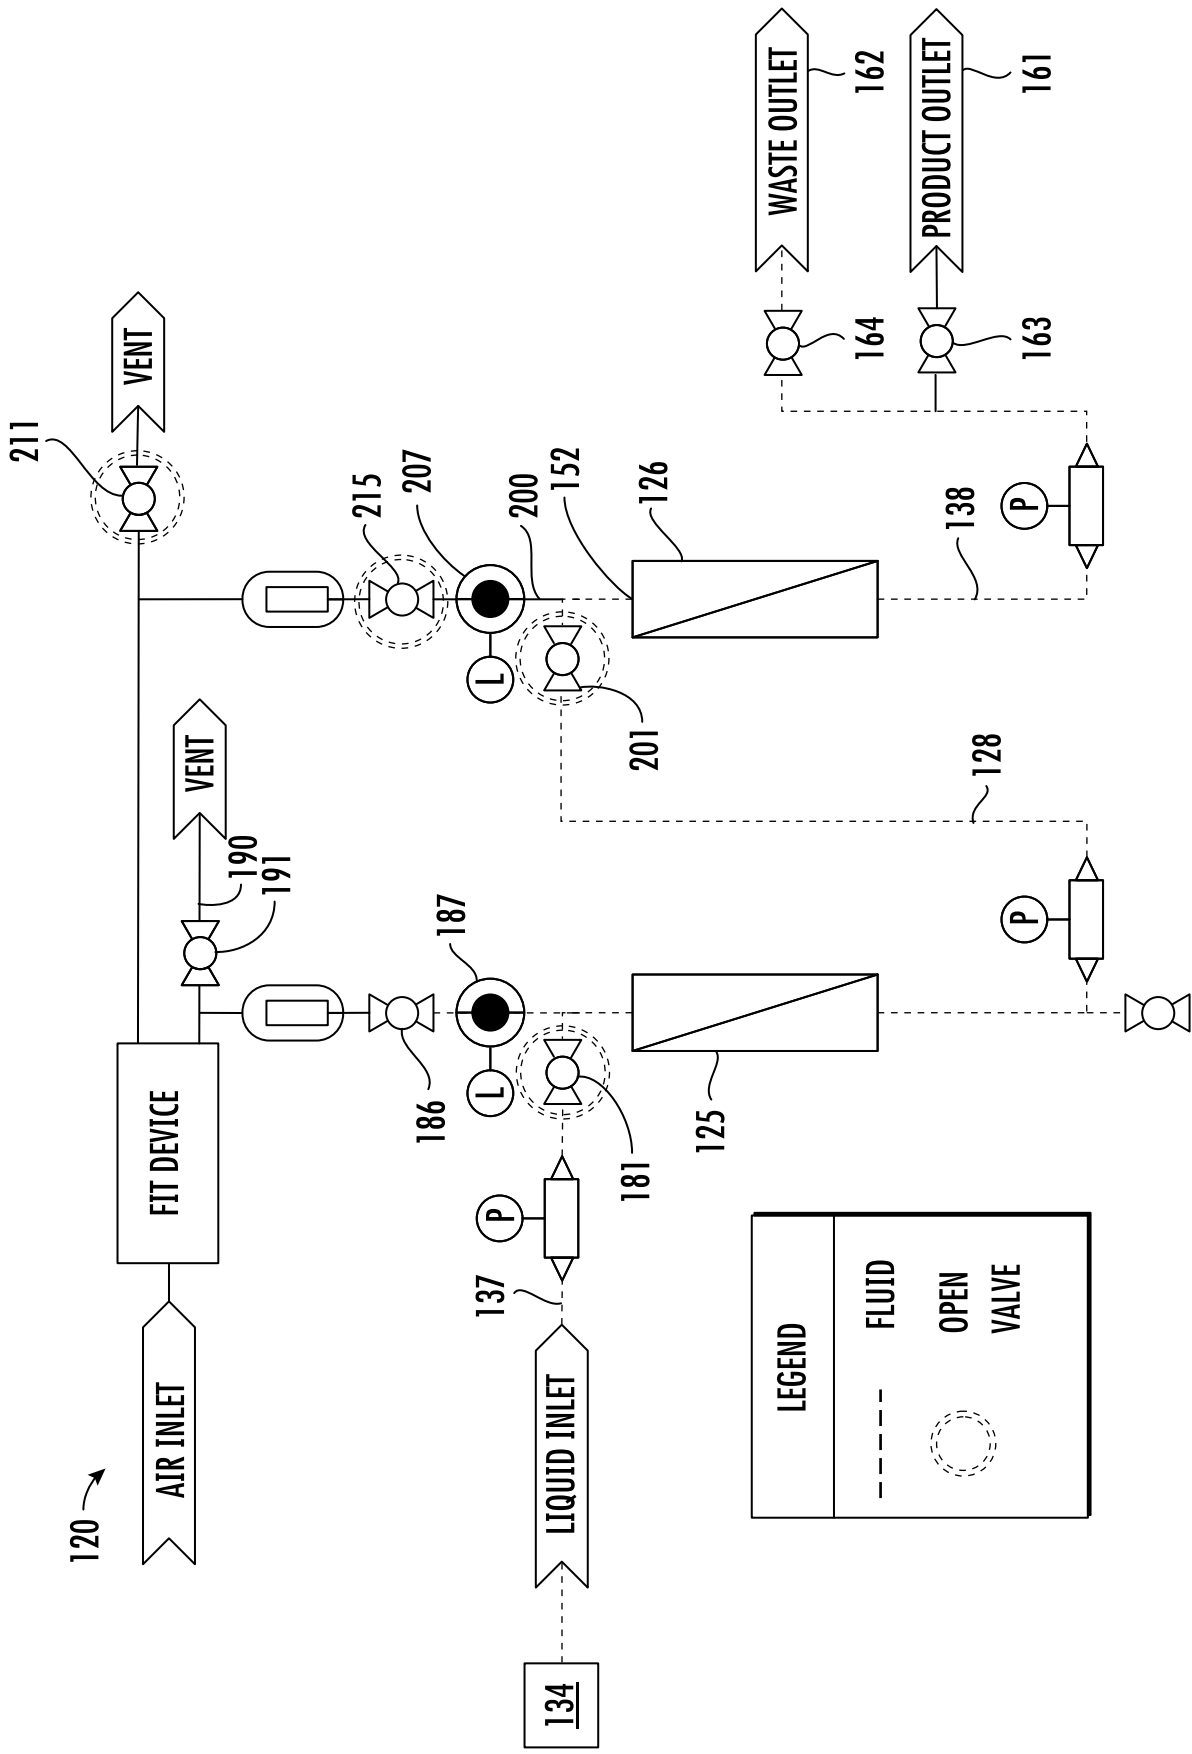


FIG. 17