

1/15
Fig.1

100 INFORMATION PROCESSING DEVICE



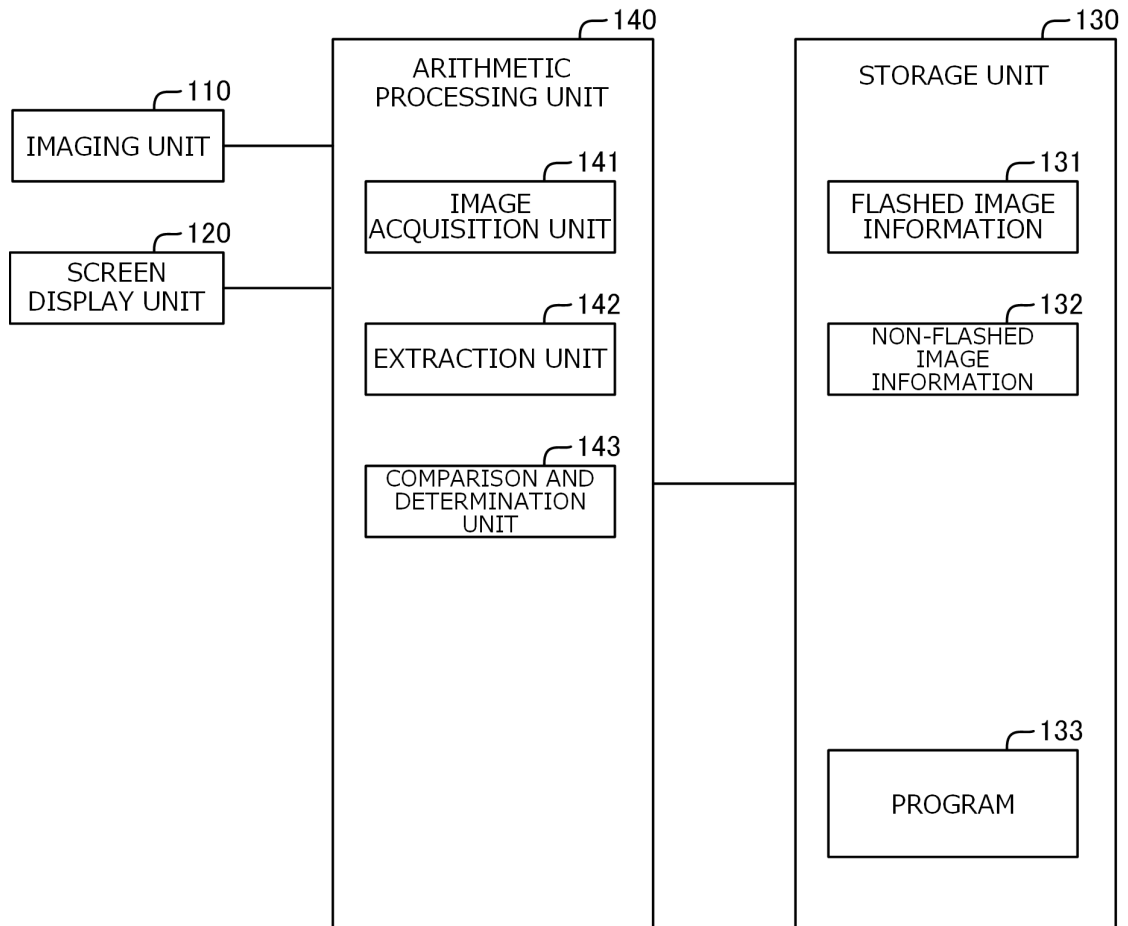


Fig.2

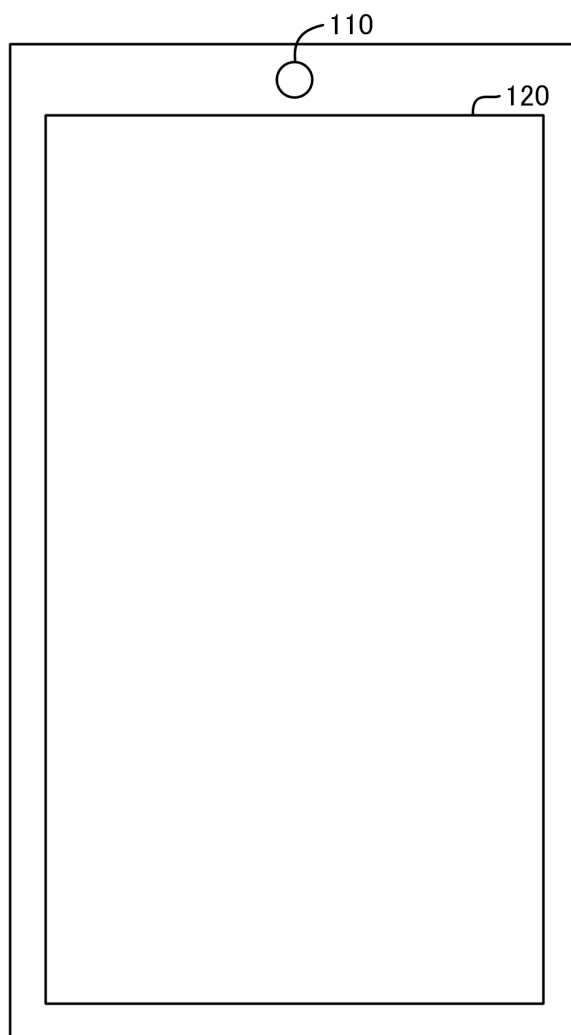

3/15

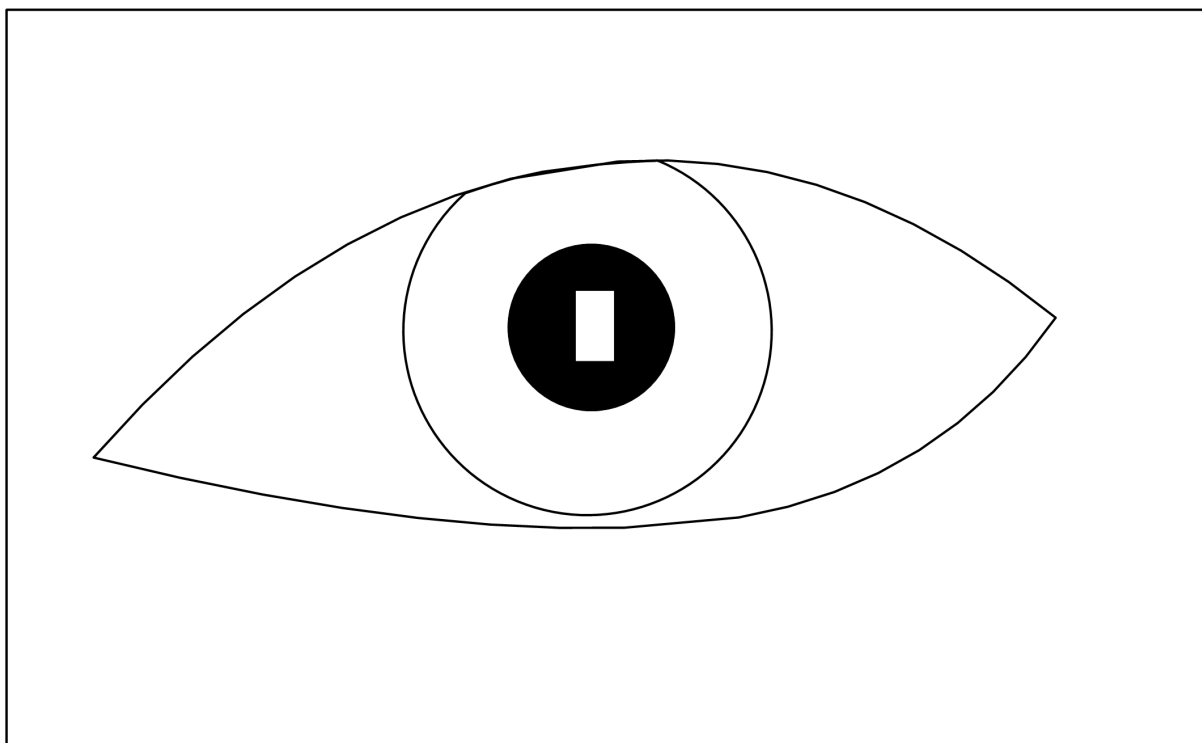Fig.3



4/15

Fig.4

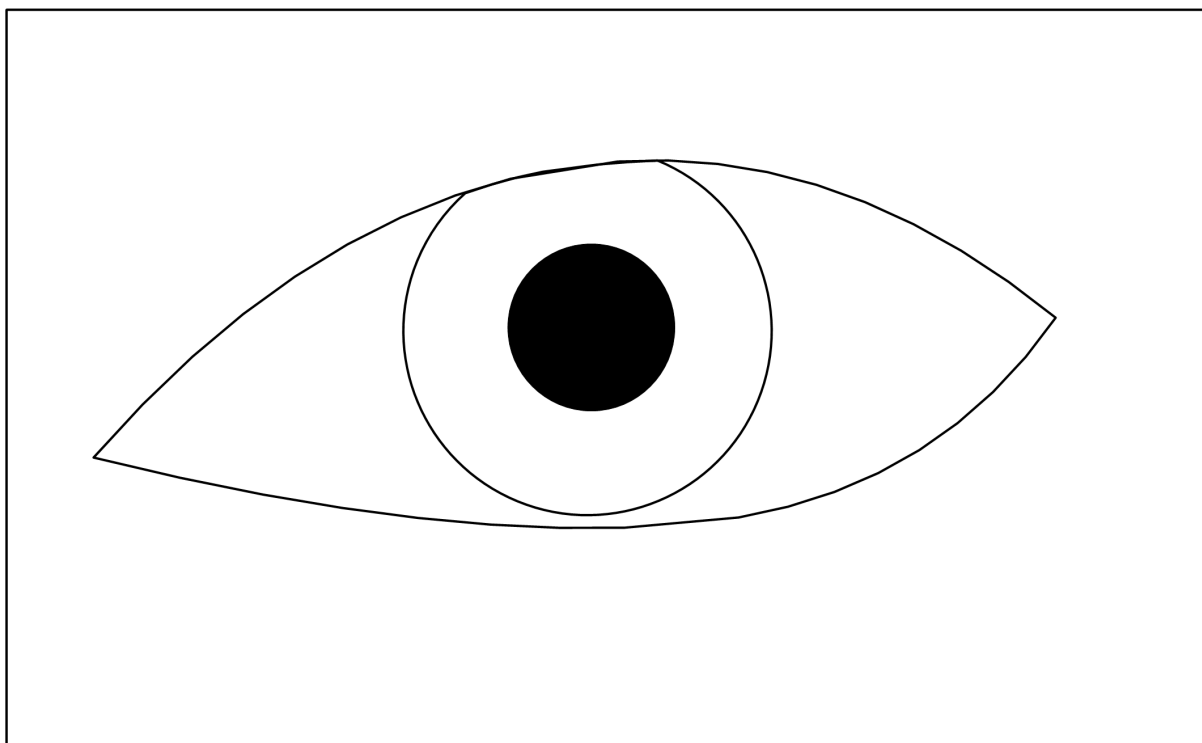


Fig.5








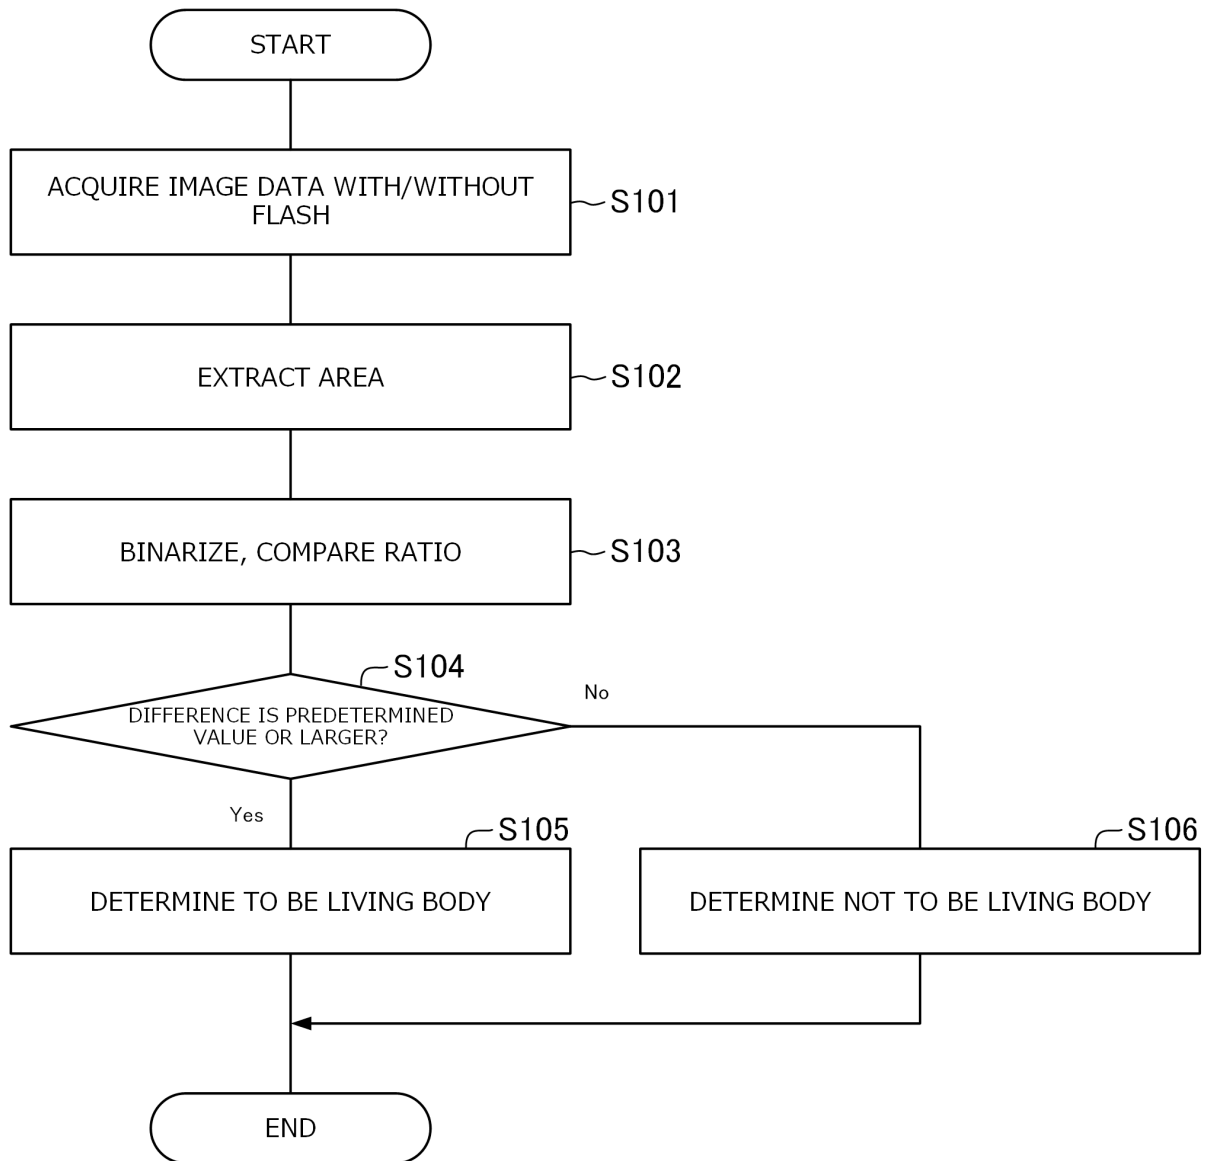
	IMAGE DATA WITH FLASH	IMAGE DATA WITHOUT FLASH
EYE OF LIVING BODY		
PHOTO (WITH FLASH)		
PHOTO (WITHOUT FLASH)		


Fig.6

7/15
Fig.7

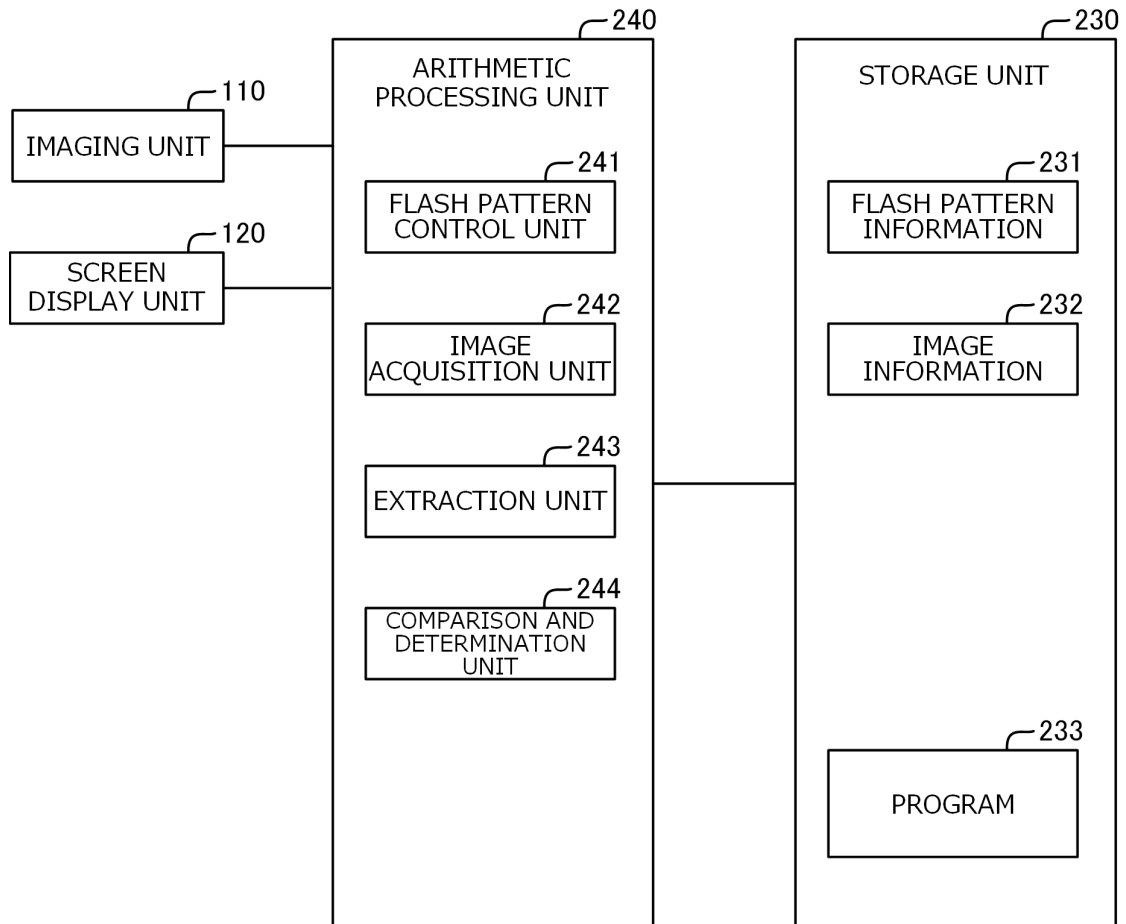200 INFORMATION PROCESSING DEVICE



8/15
Fig.8

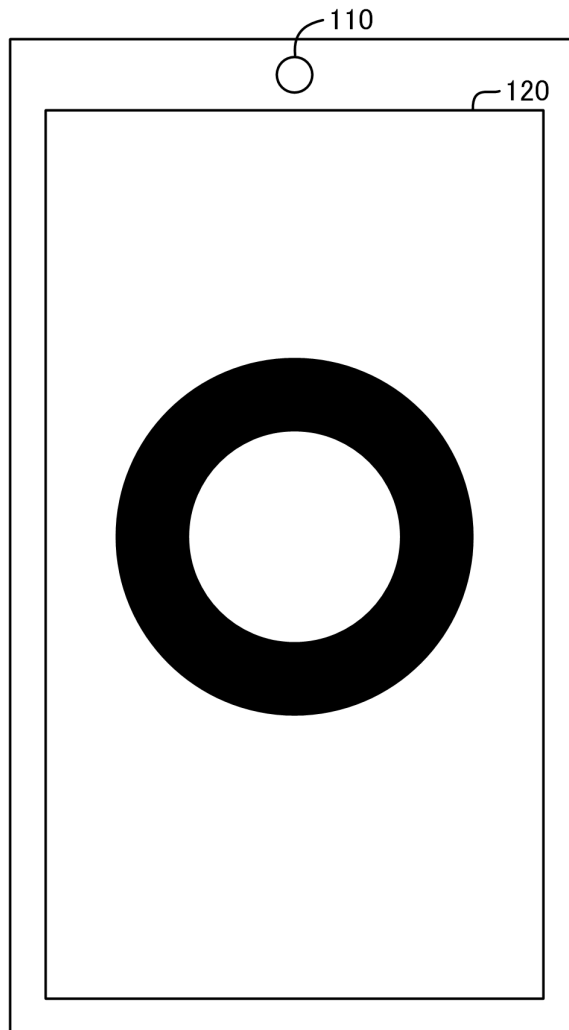

9/15

Fig.9

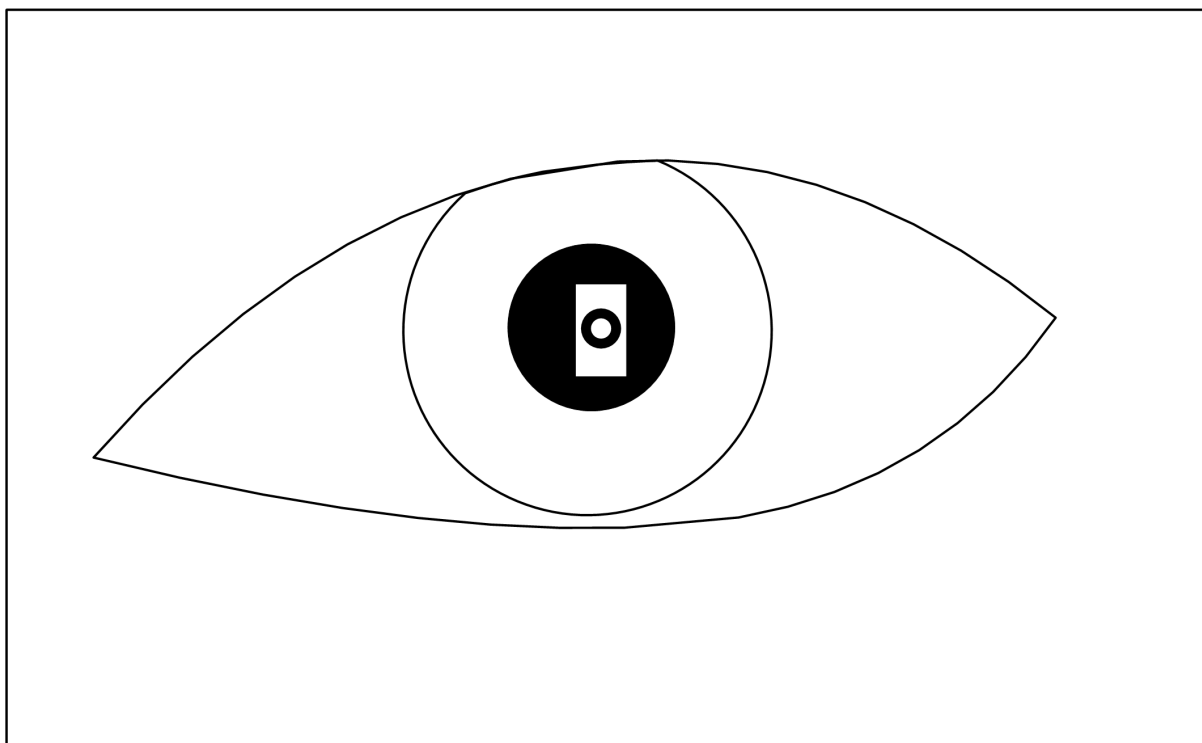



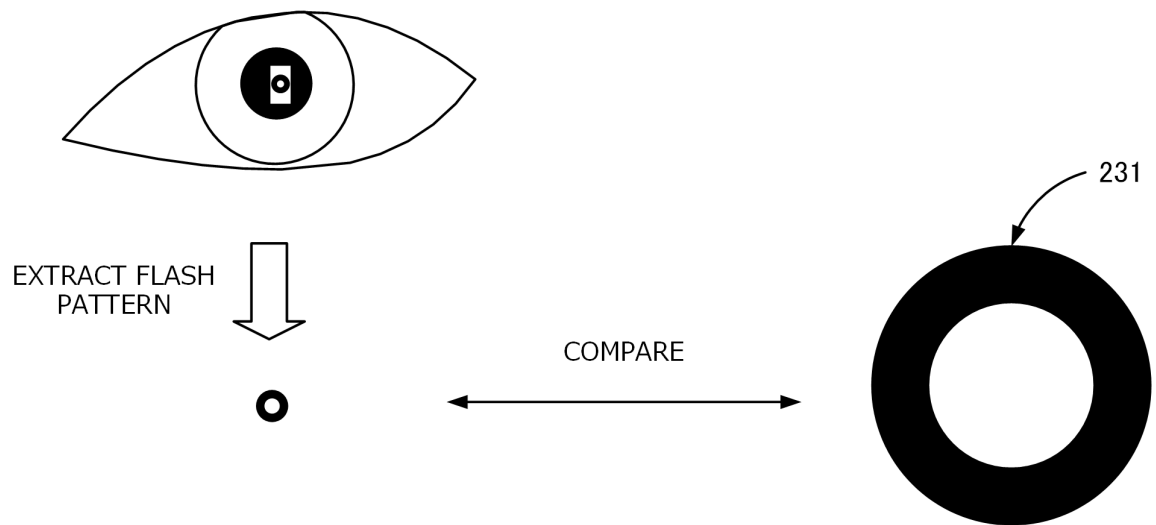
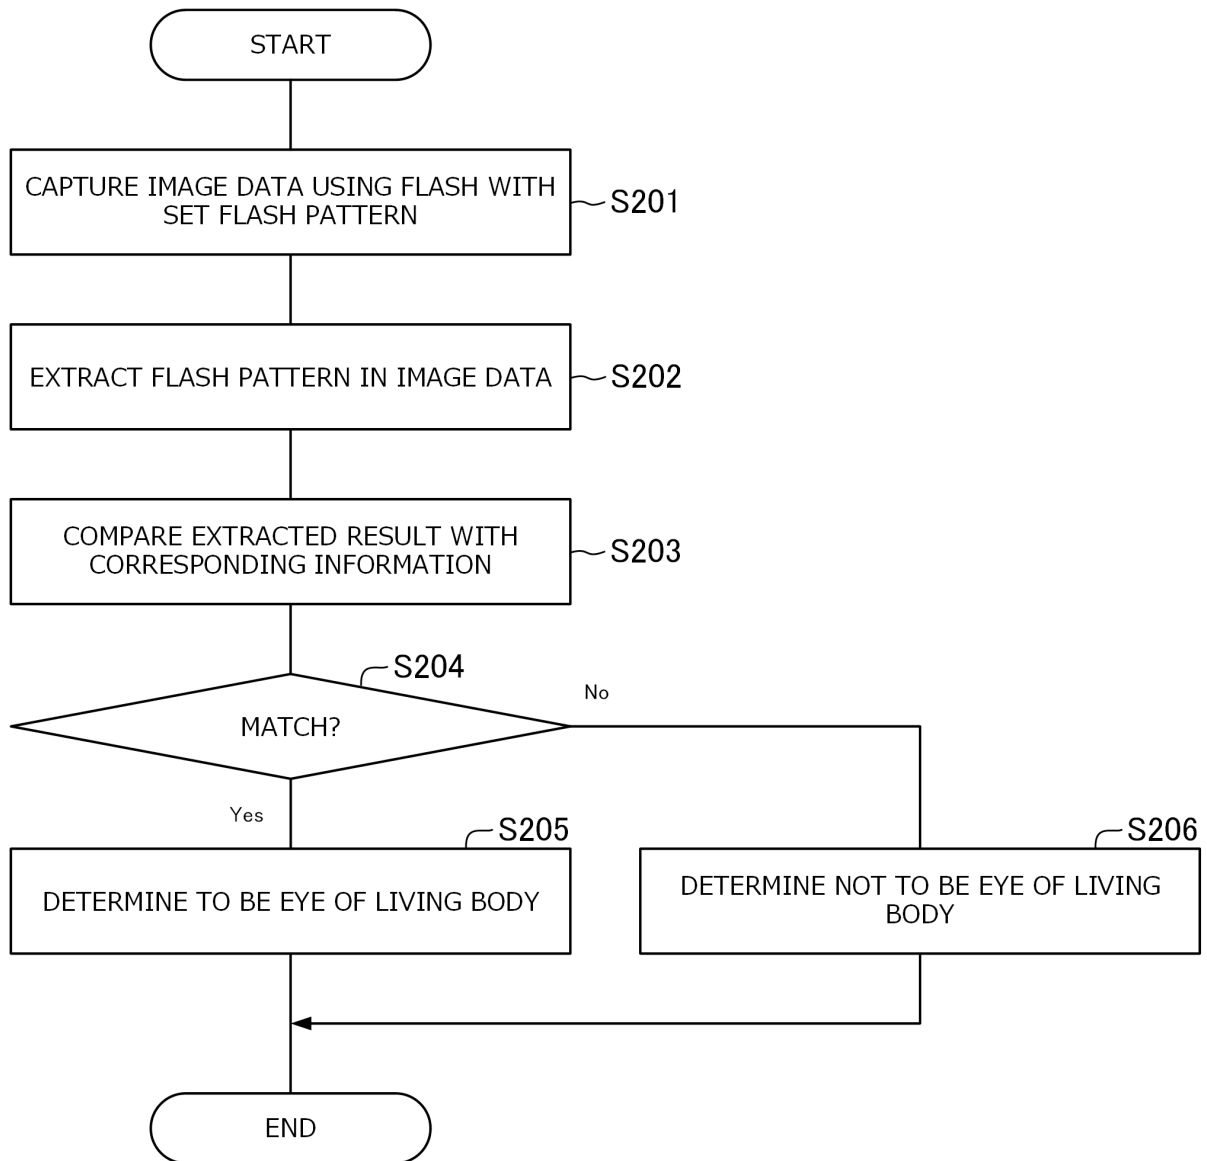
Fig.10

Fig.11

12/15

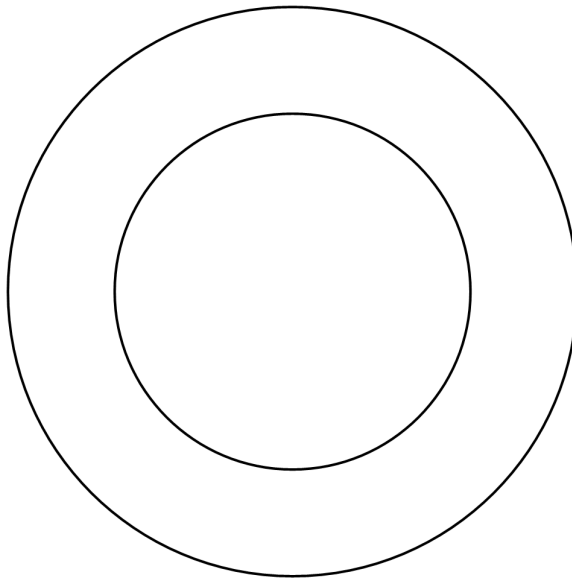Fig.12



13/15
Fig.13

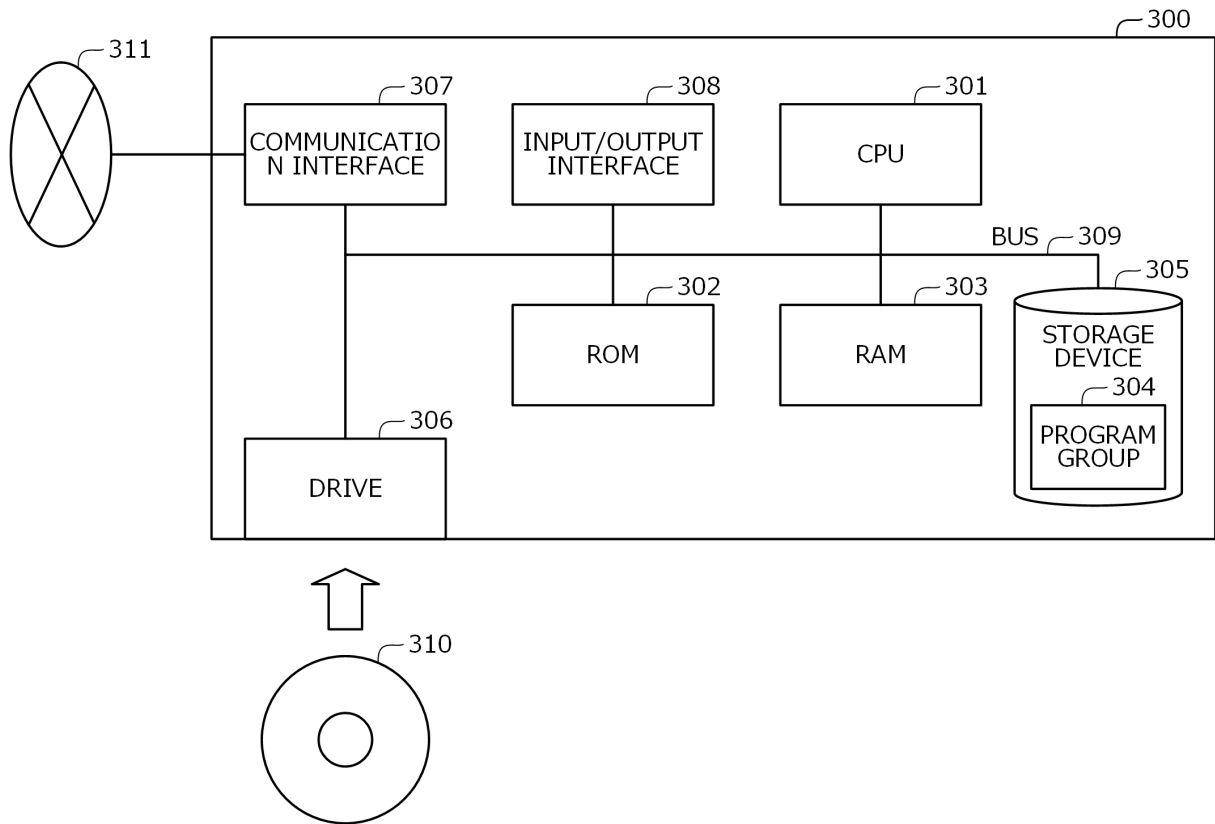


Fig.14

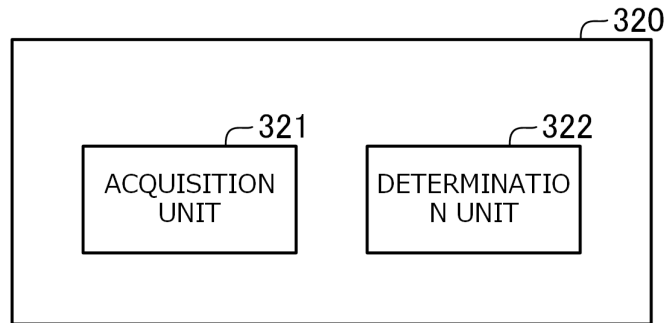


Fig.15

